

US00D380551S

# United States Patent [19]

[11] Patent Number: **Des. 380,551**

Ohnuma et al.

[45] Date of Patent: **\*\*Jul. 1, 1997**

[54] **BIOCHEMICAL ANALYZER**

[75] Inventors: **Mitsuru Ohnuma, Mitaka; Atsushi Katayama, Kokubunji; Isamu Takekoshi, Kodaira; Isao Shindo; Kahei Shiraishi, both of Hitachiota; Hiromichi Sato, Hitachinaka, all of Japan**

[73] Assignee: **Hitachi, Ltd., Tokyo, Japan**

[\*\*] Term: **14 Years**

[21] Appl. No.: **41,933**

[22] Filed: **Jul. 27, 1995**

[30] **Foreign Application Priority Data**

Jun. 12, 1995 [JP] Japan ..... 7-16437

[51] LOC (6) Cl. .... **24-01**

[52] U.S. Cl. .... **D24/186; D10/81; D24/231; D24/232**

[58] Field of Search ..... **D24/231, 232, D24/186, 169; D10/81; 422/102, 100**

[56] **References Cited**

**U.S. PATENT DOCUMENTS**

D. 264,873 6/1982 Olson et al. .... D24/234 X

D. 282,203 1/1986 Leonard et al. .... D24/234 X  
D. 314,049 1/1991 Katayama ..... D24/186  
D. 334,428 3/1993 Horton et al. .... D24/186 X  
D. 339,639 9/1993 Ohnuma et al. .... D24/186 X

*Primary Examiner*—Louis S. Zarfes  
*Assistant Examiner*—I. Simmons  
*Attorney, Agent, or Firm*—Antonelli, Terry, Stout & Kraus, LLP

[57] **CLAIM**

The ornamental design for a biochemical analyzer, as shown.

**DESCRIPTION**

FIG. 1 is a front, top and right side perspective view of a biochemical analyzer showing our new design;  
FIG. 2 is a front elevational view thereof;  
FIG. 3 is a top plan view thereof;  
FIG. 4 is a bottom plan view thereof;  
FIG. 5 is a right side view thereof;  
FIG. 6 is a left side view thereof; and,  
FIG. 7 is a rear elevational view thereof.

**1 Claim, 6 Drawing Sheets**

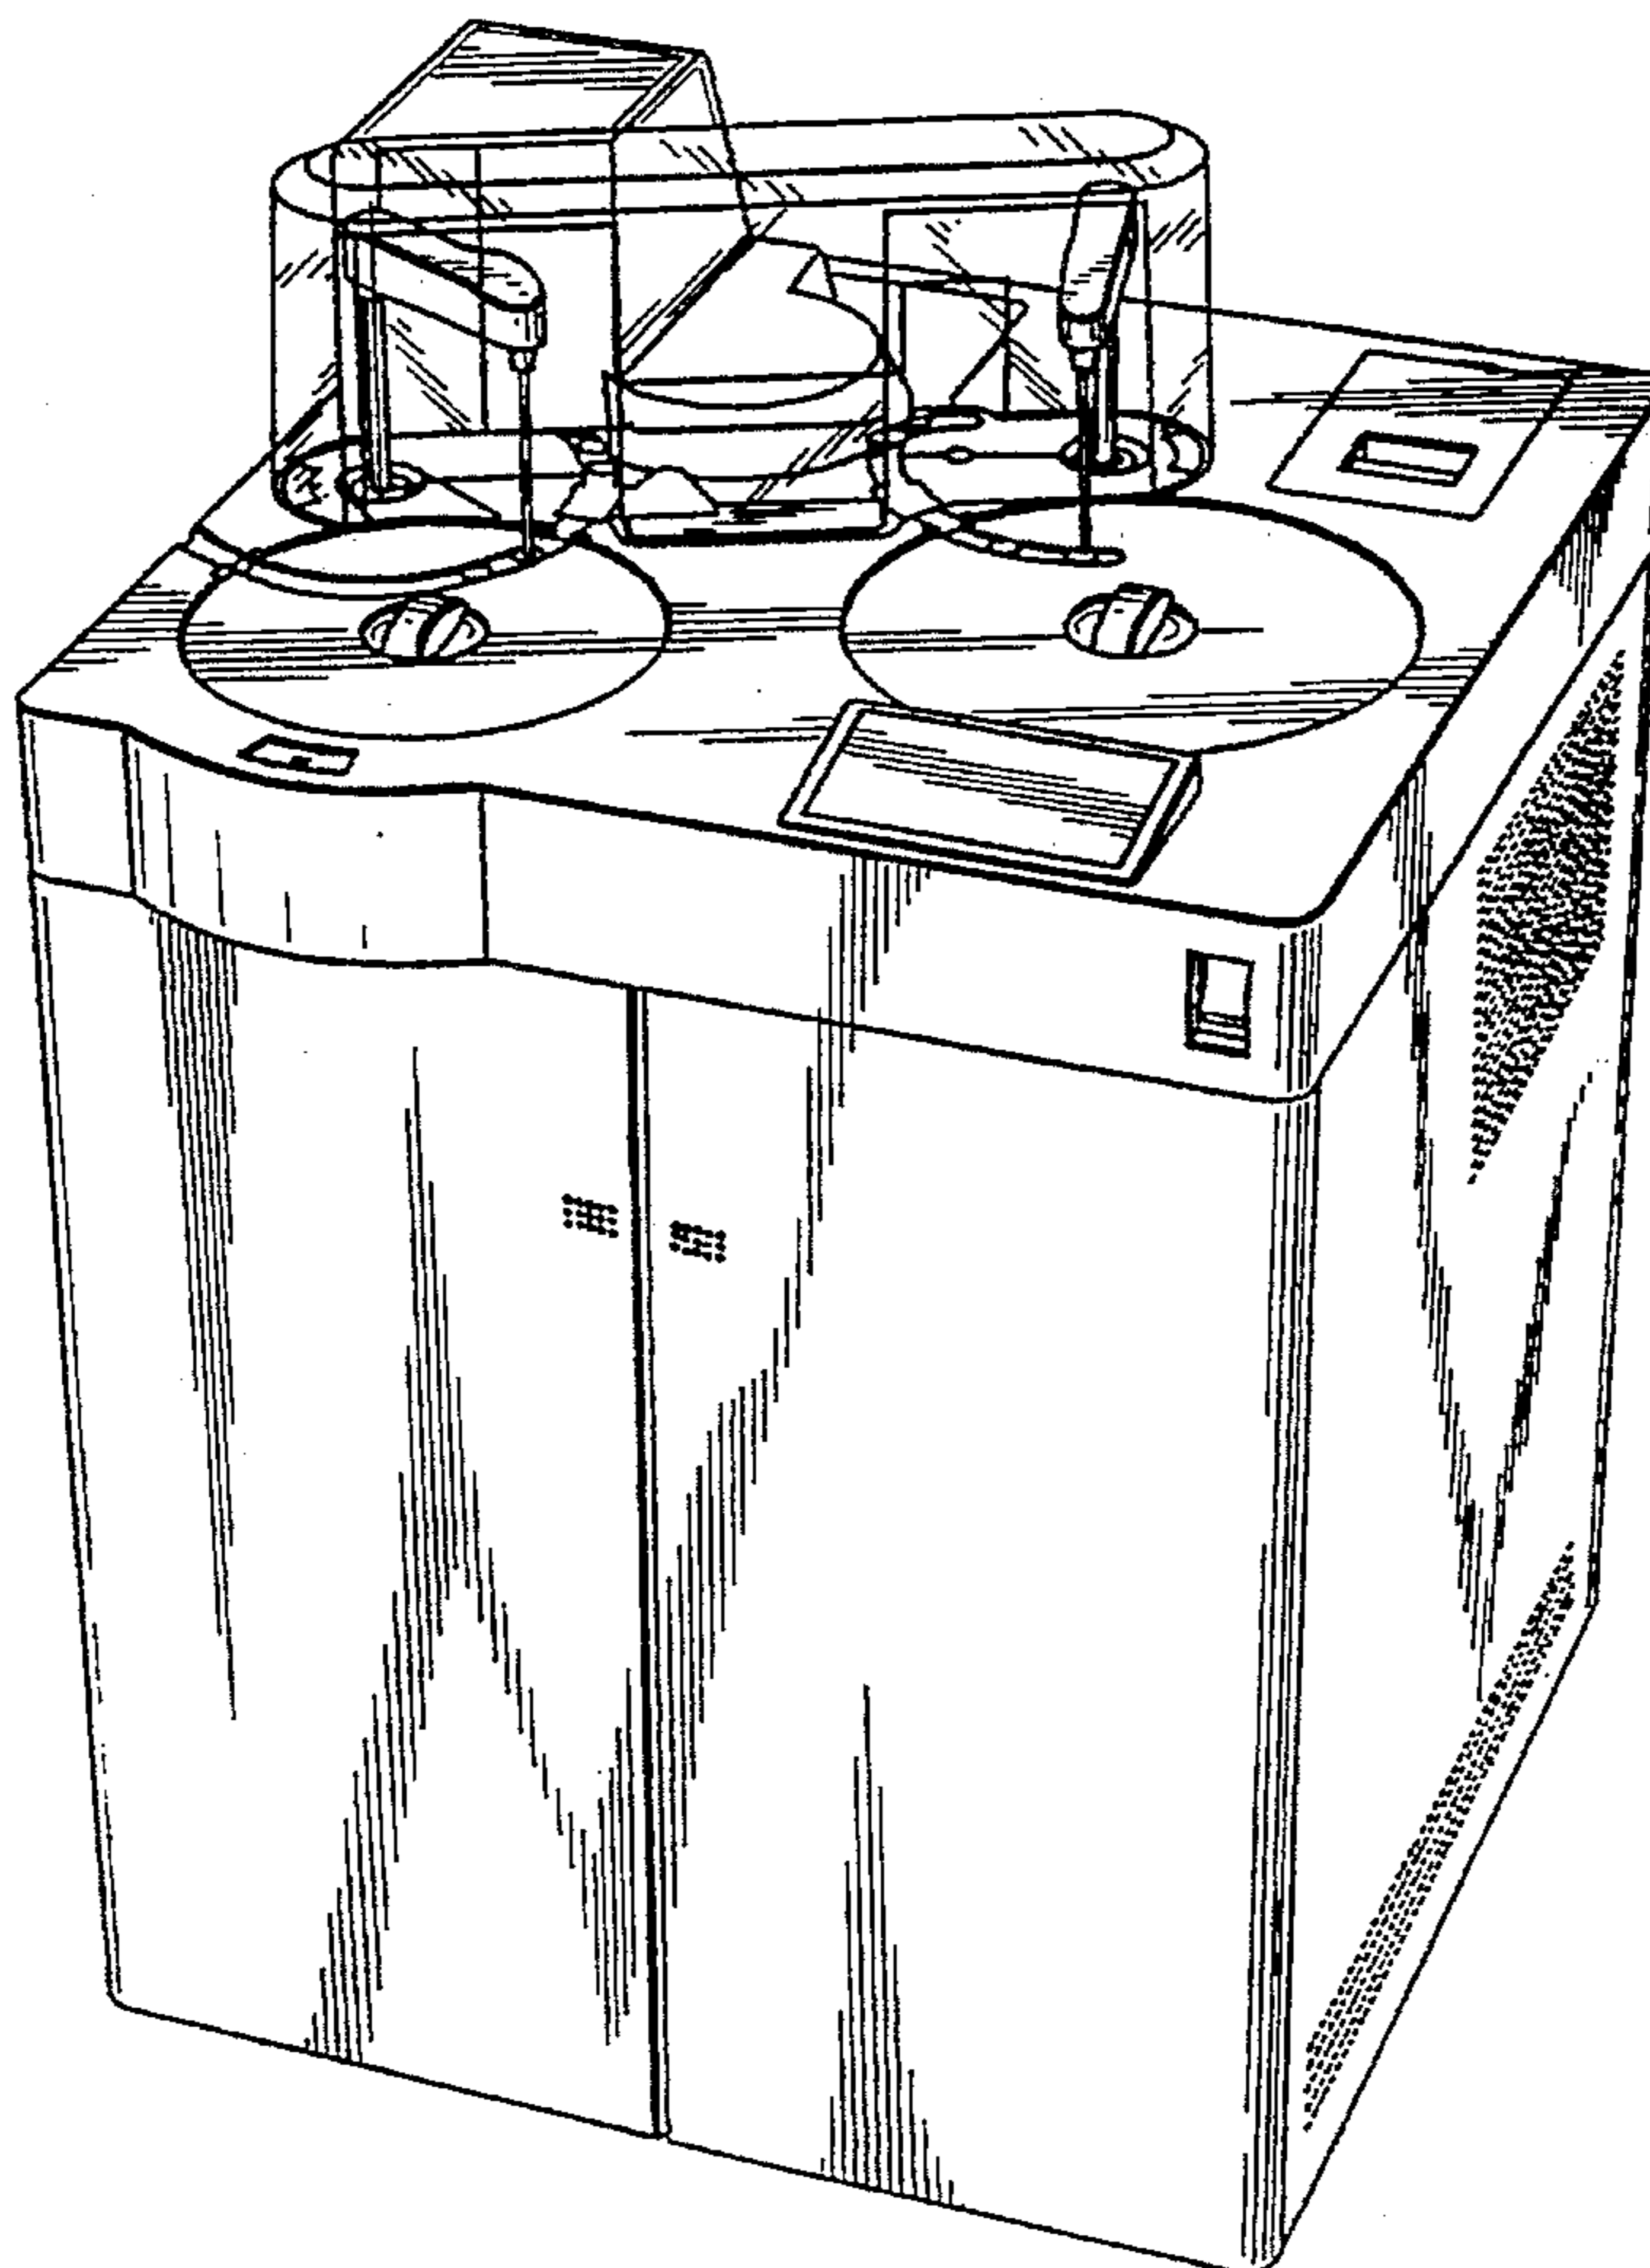


FIG. 1

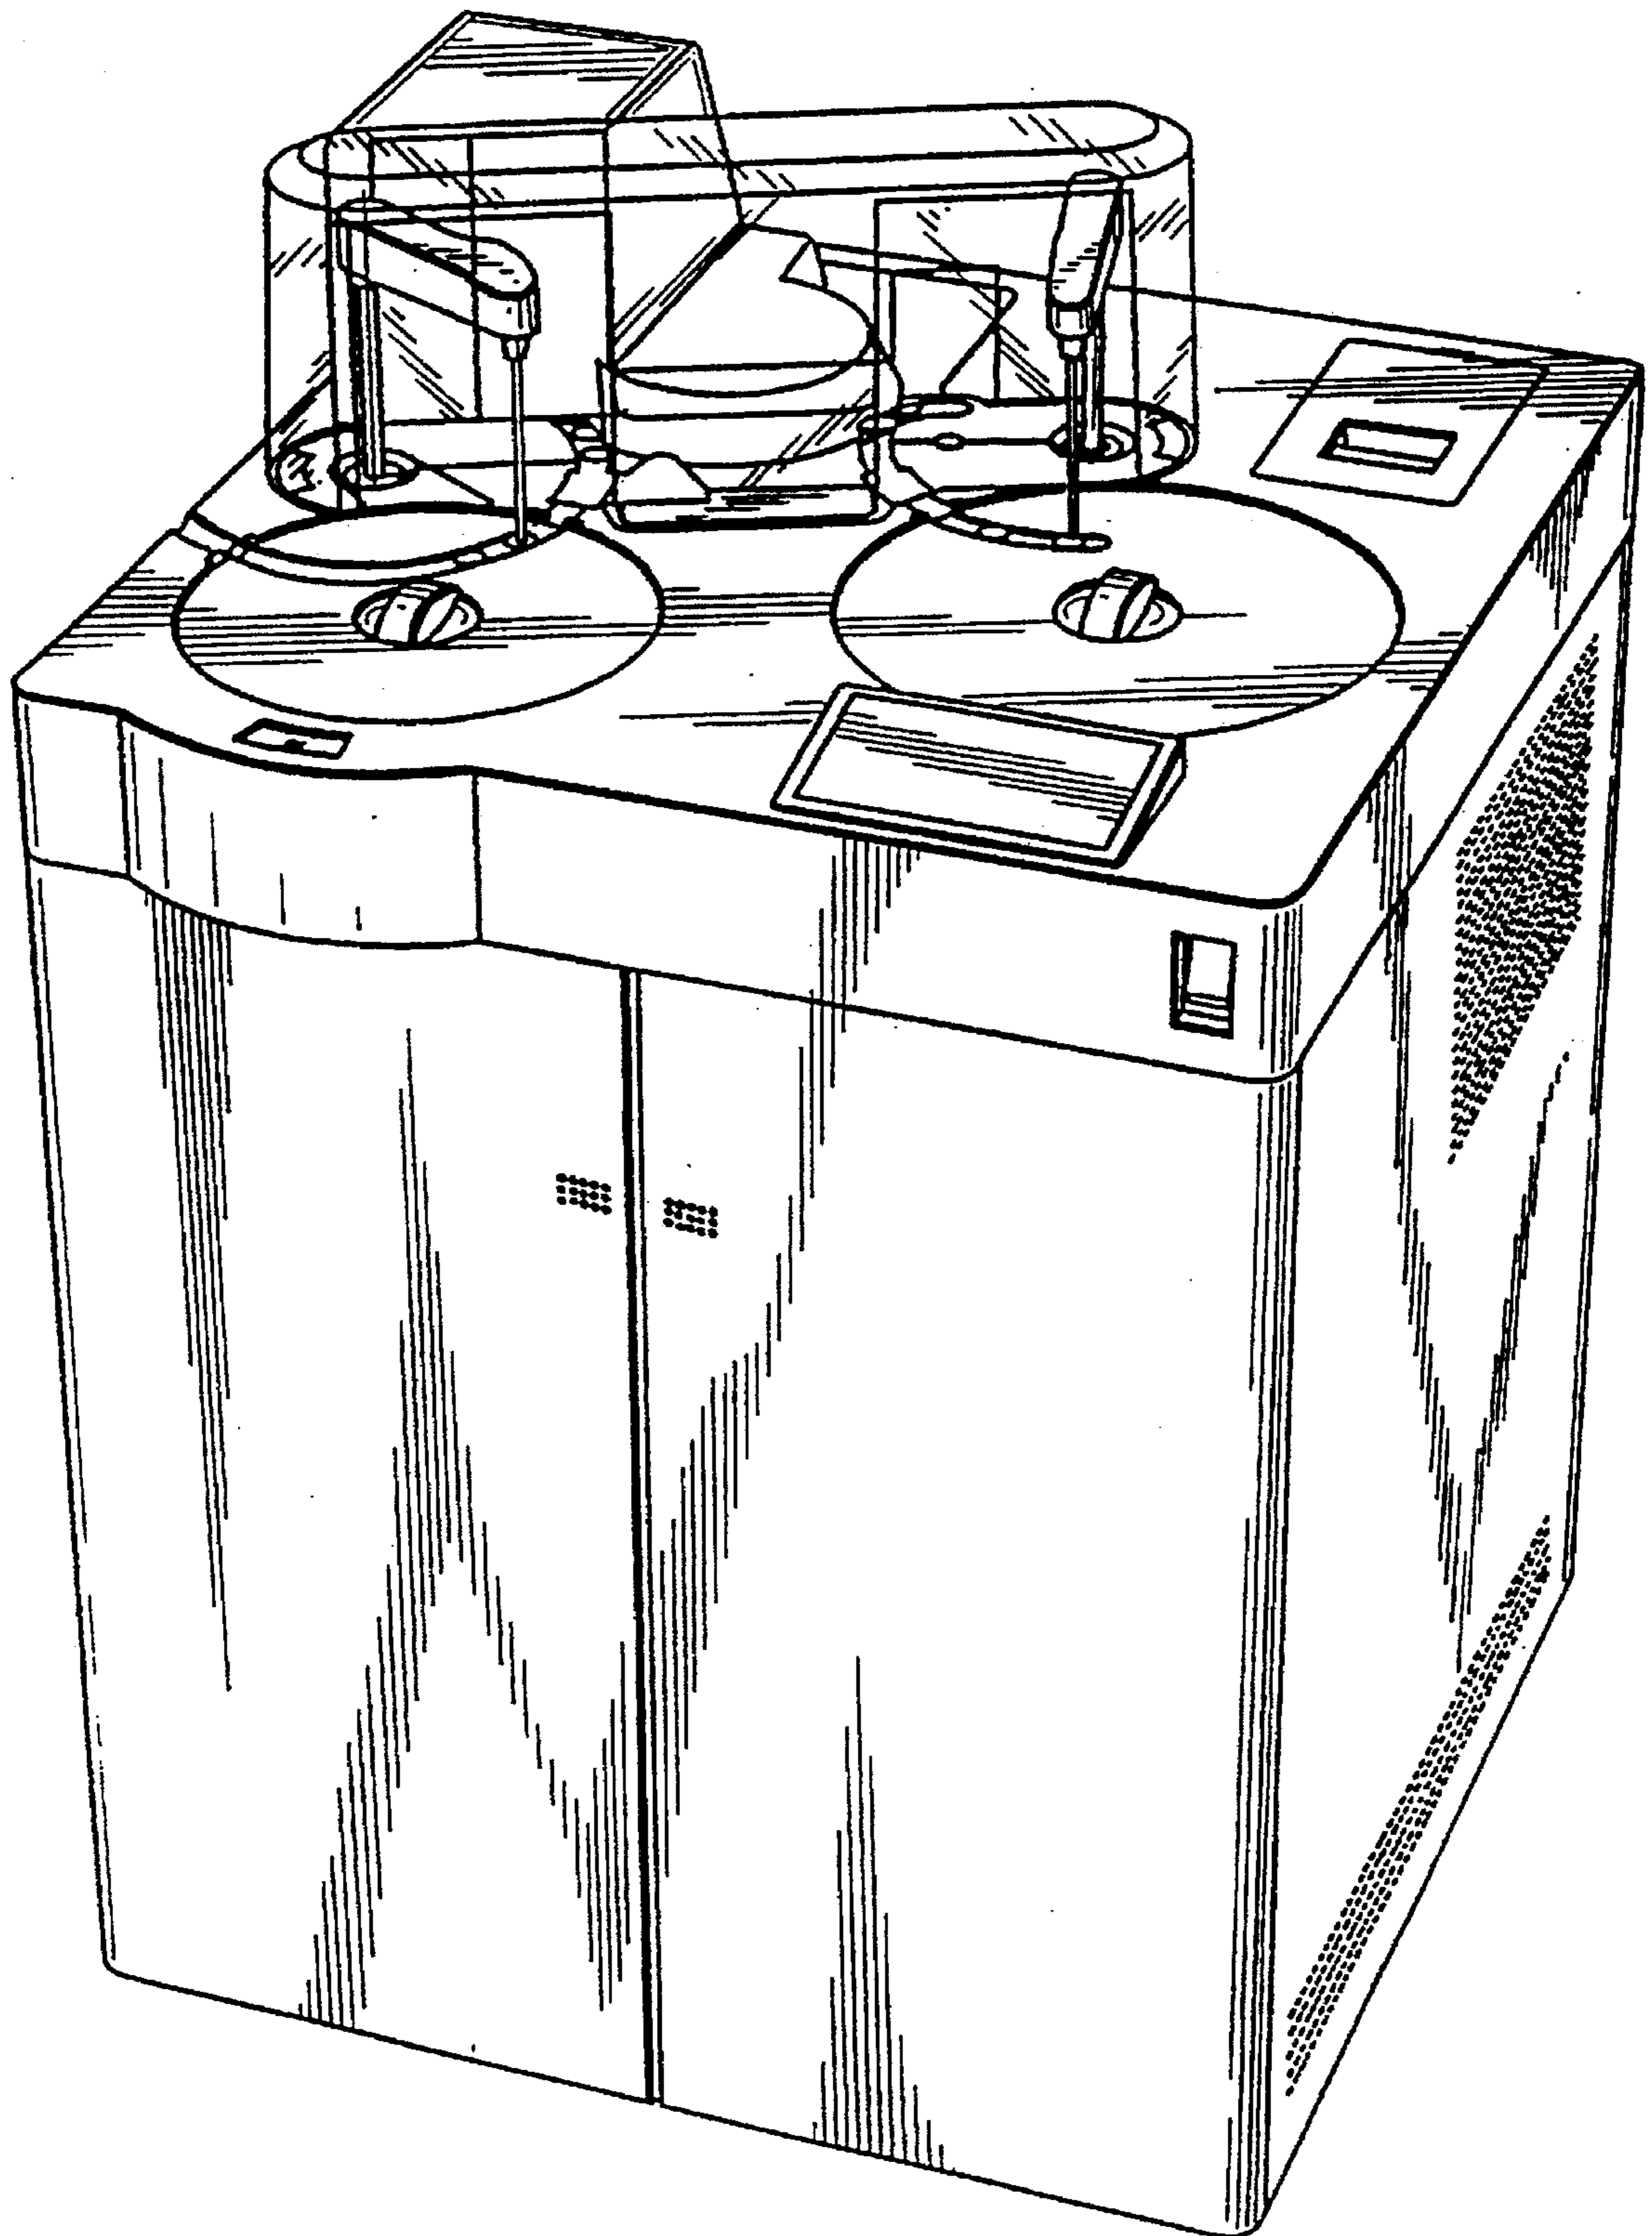


FIG. 2

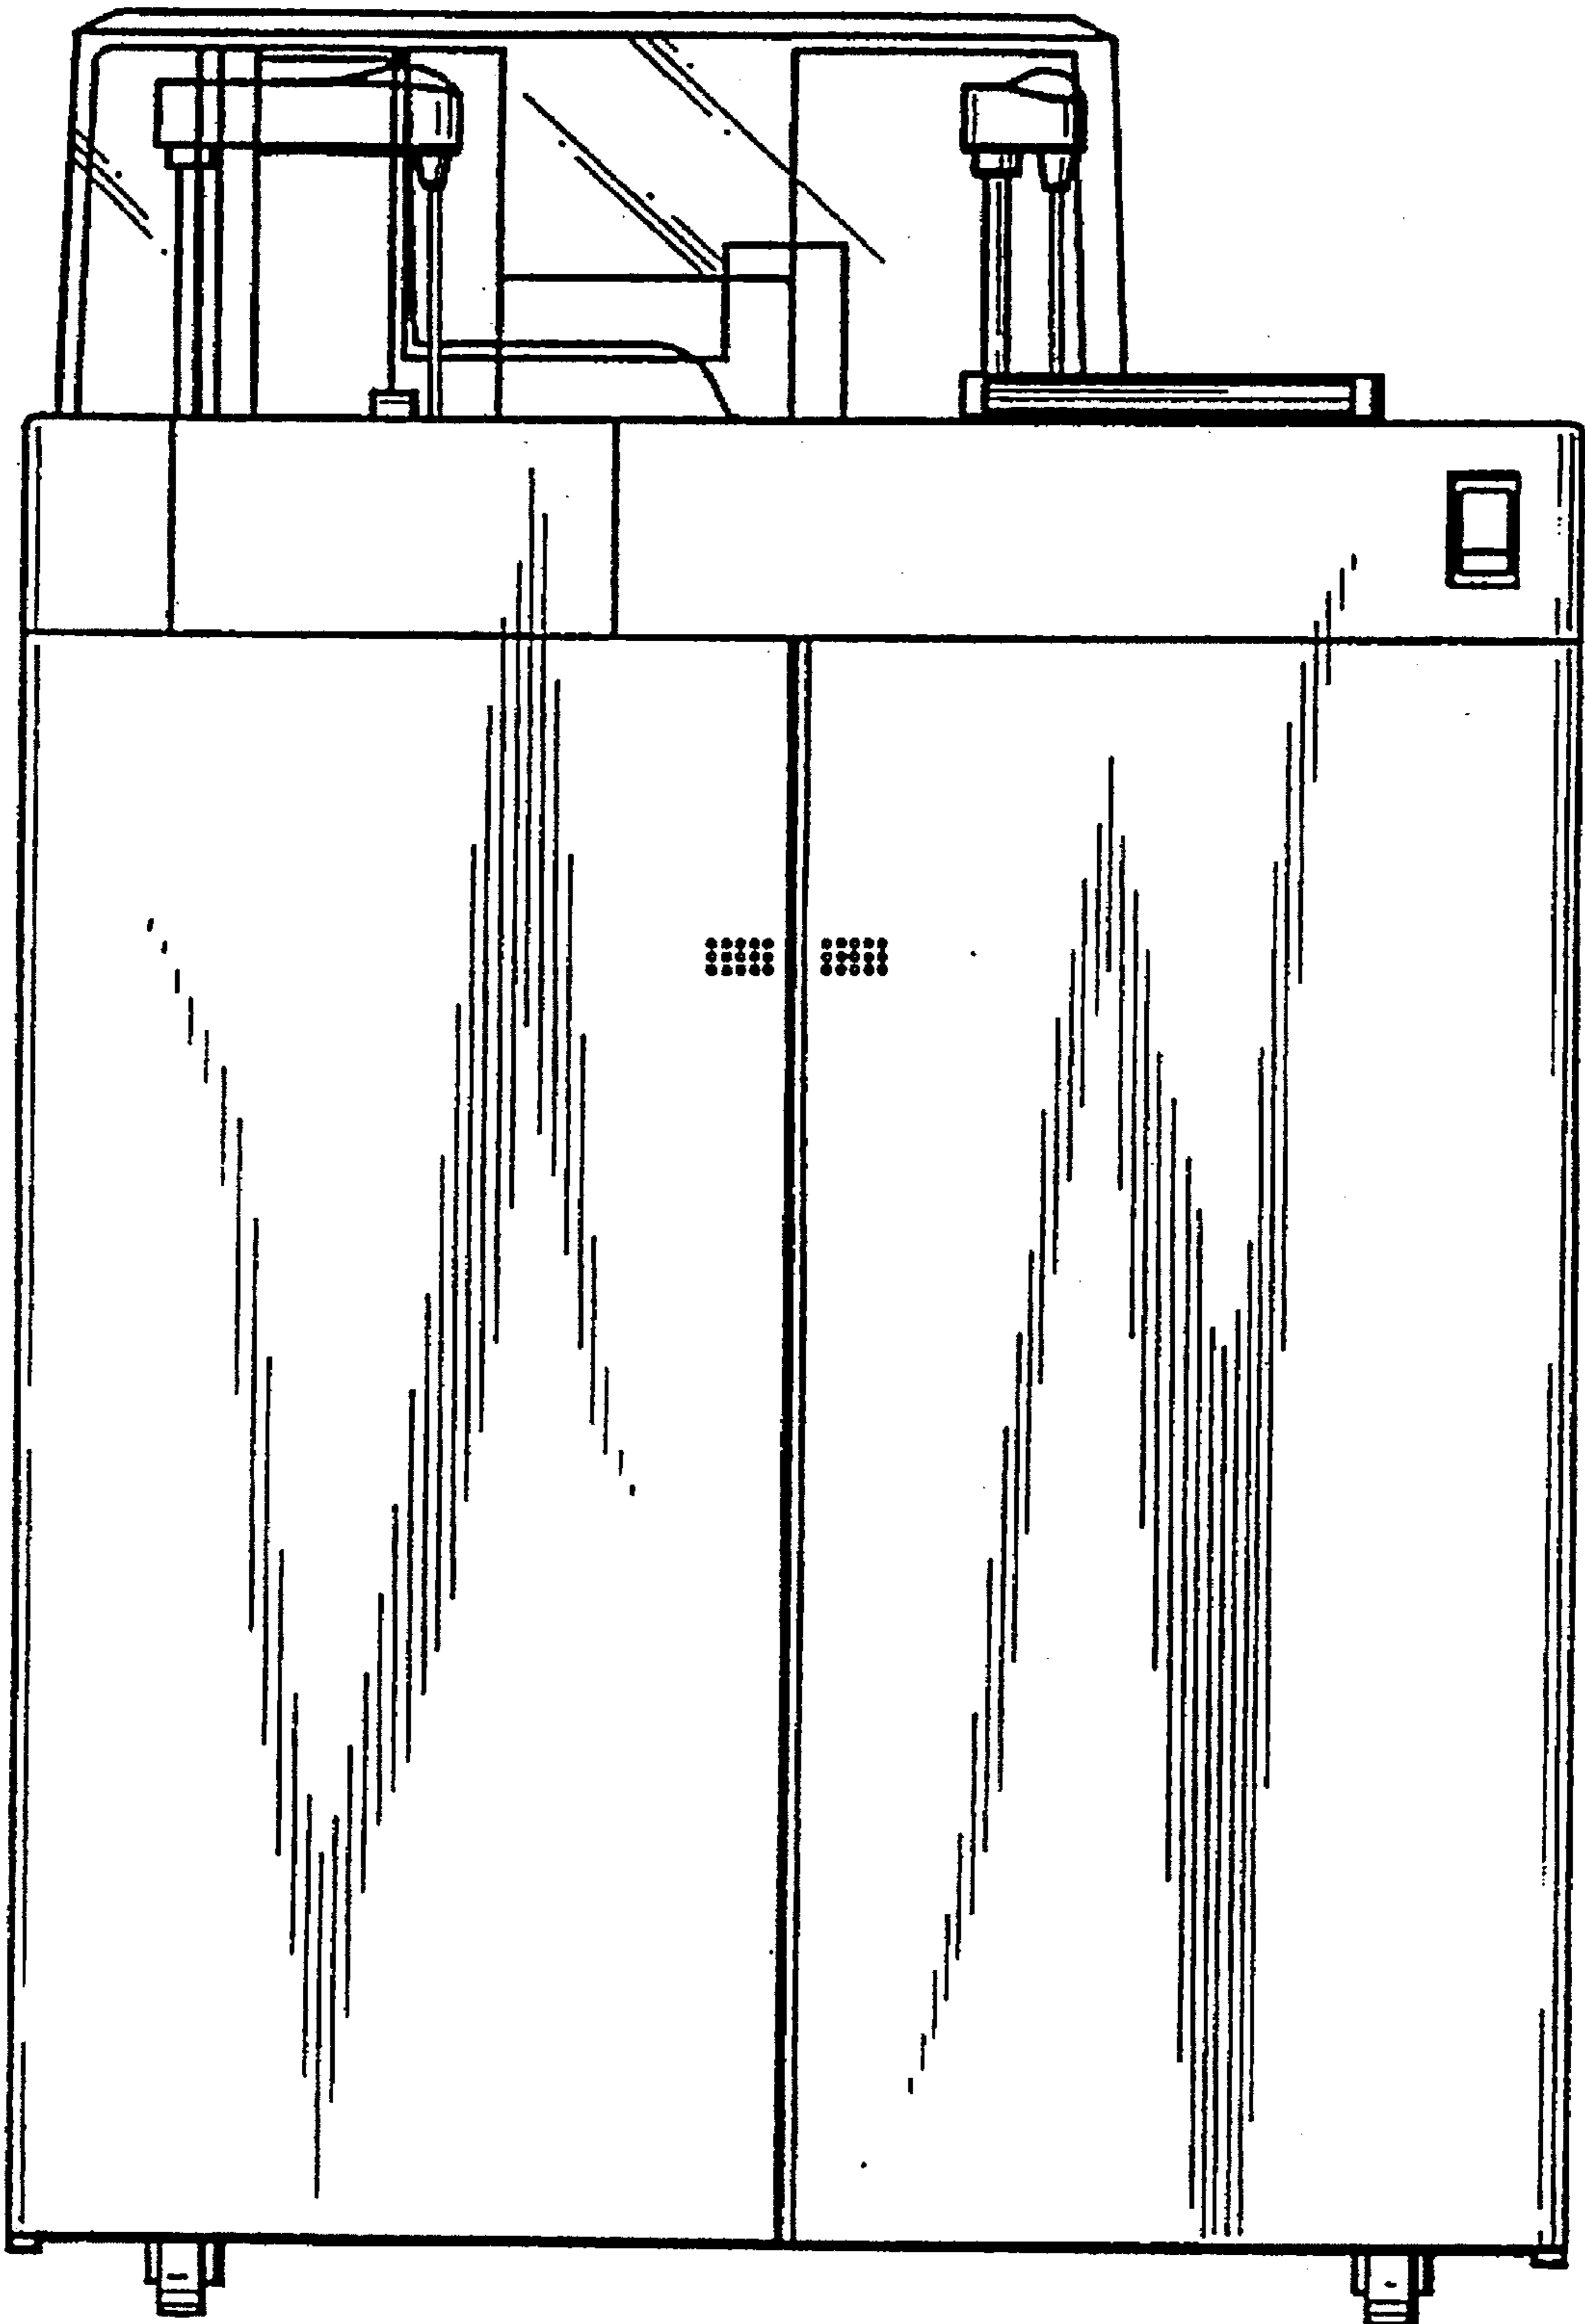




FIG. 3

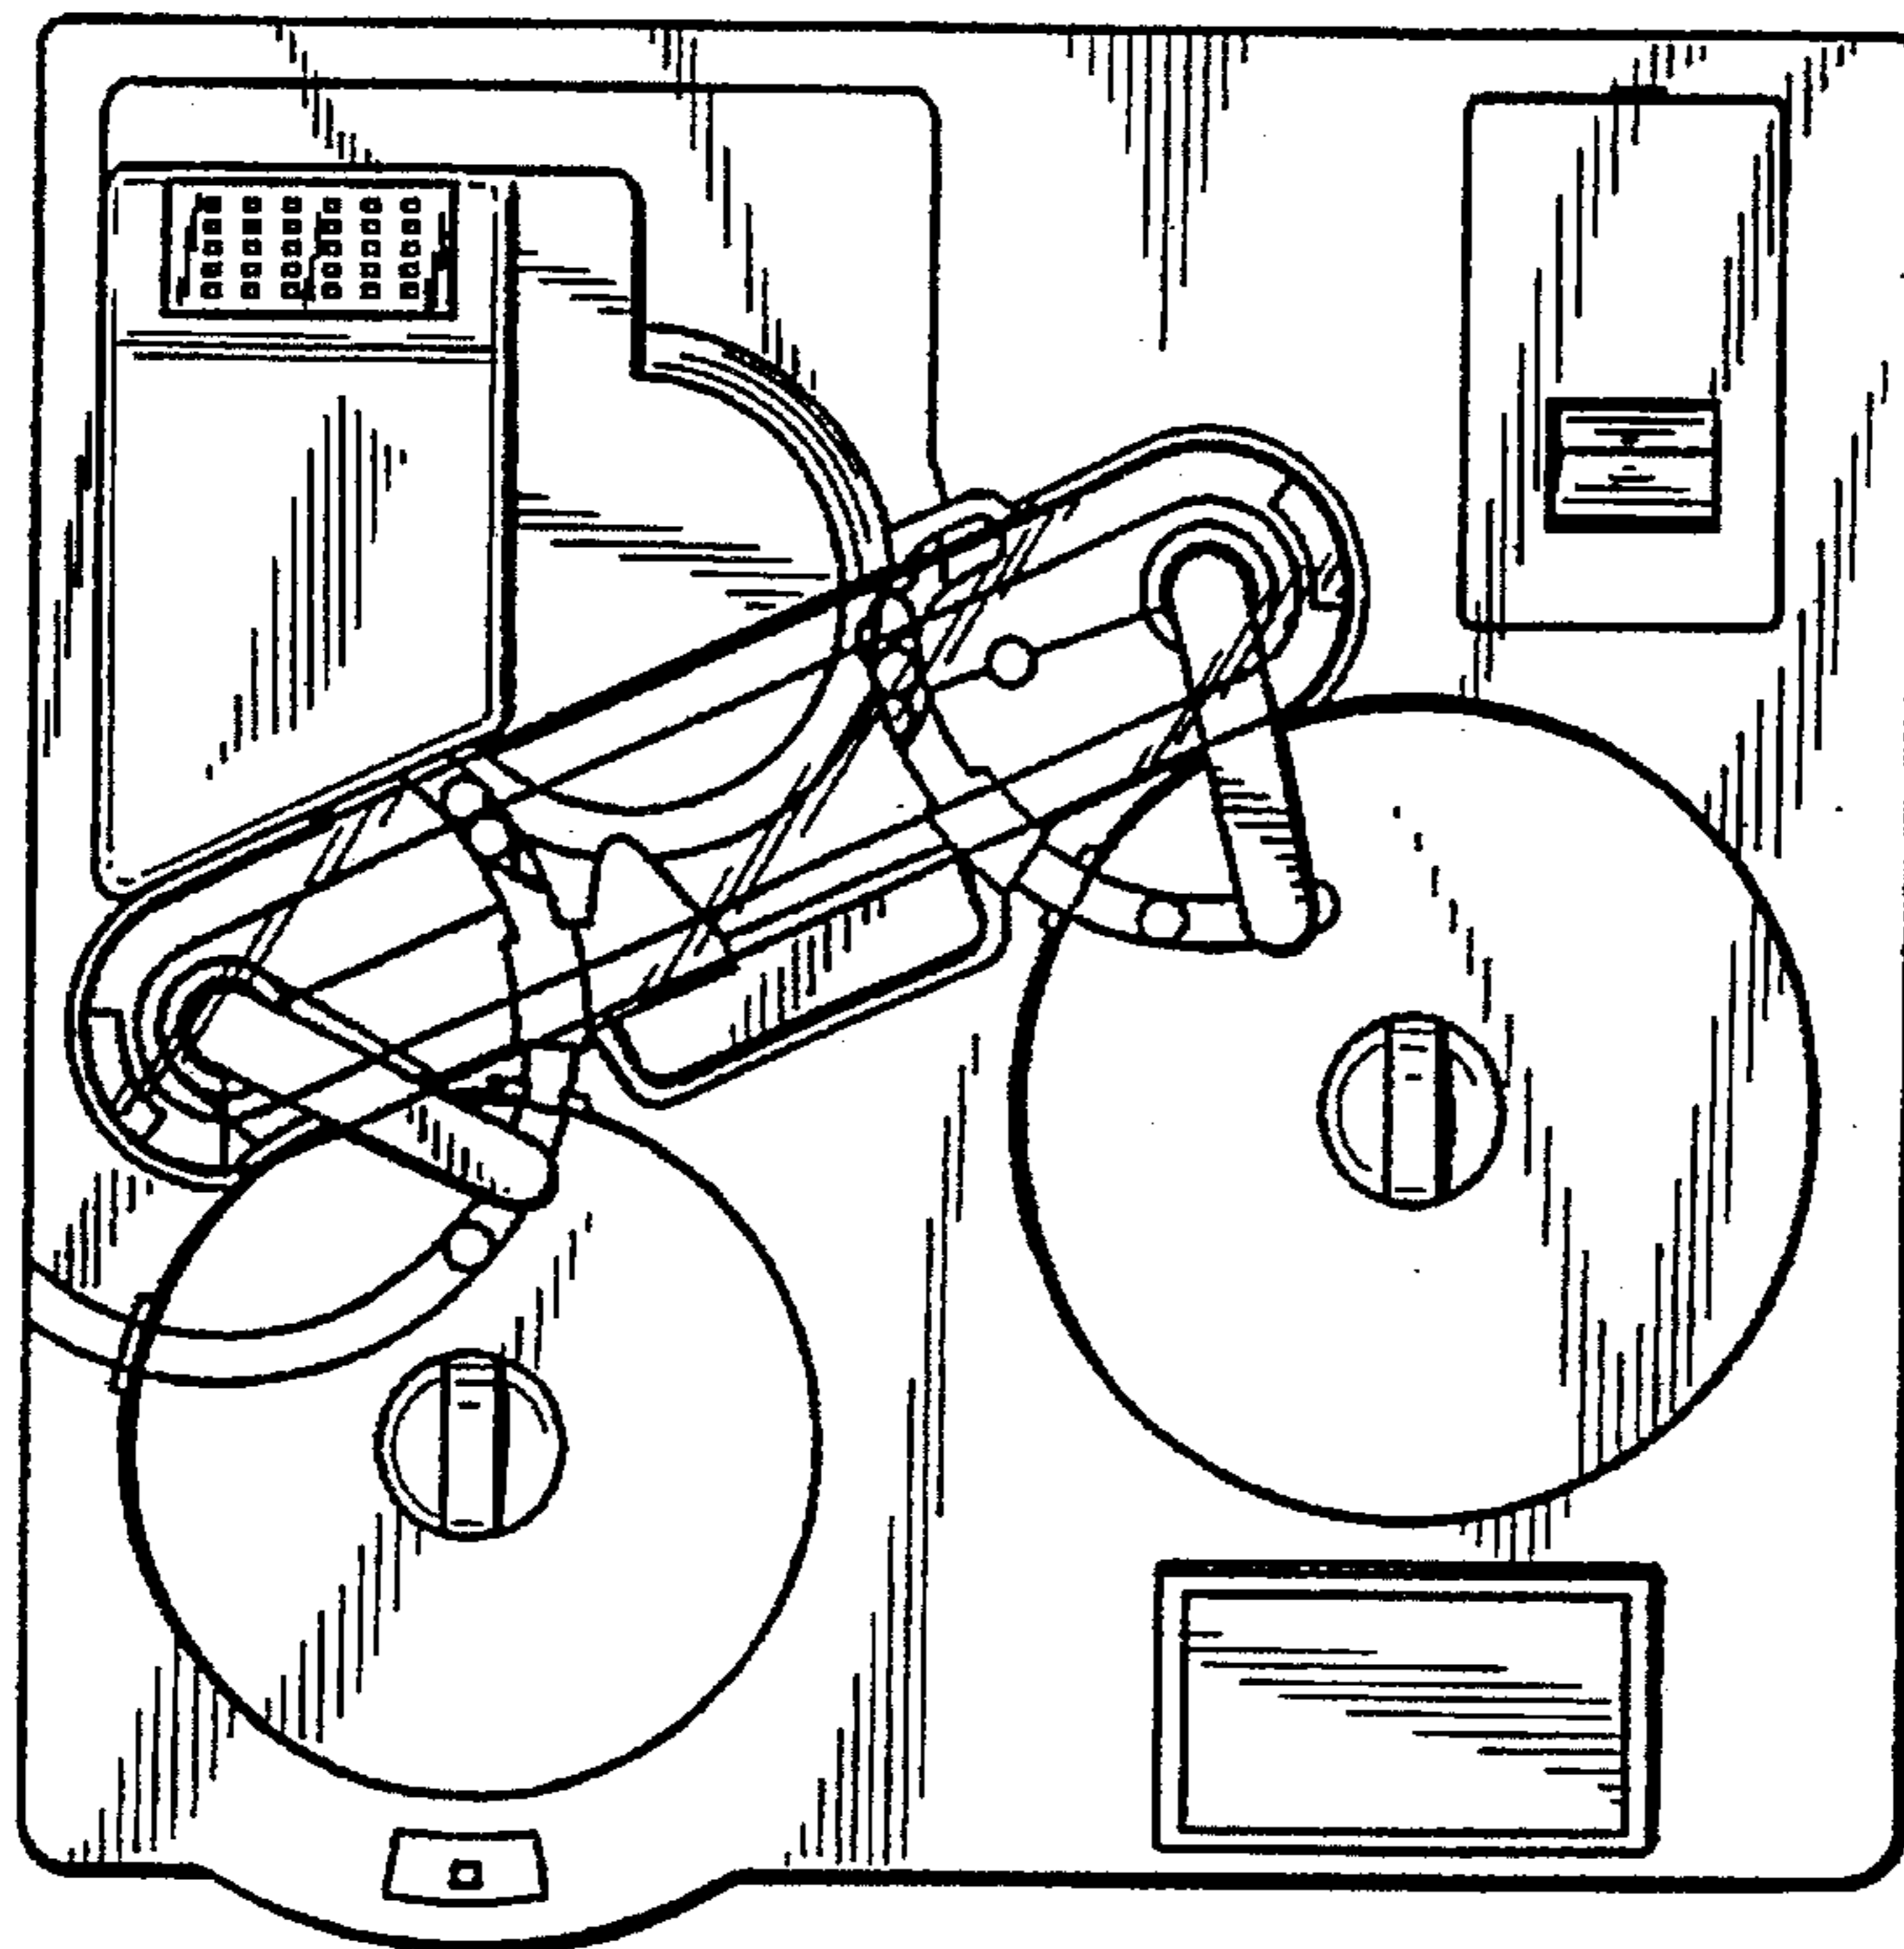
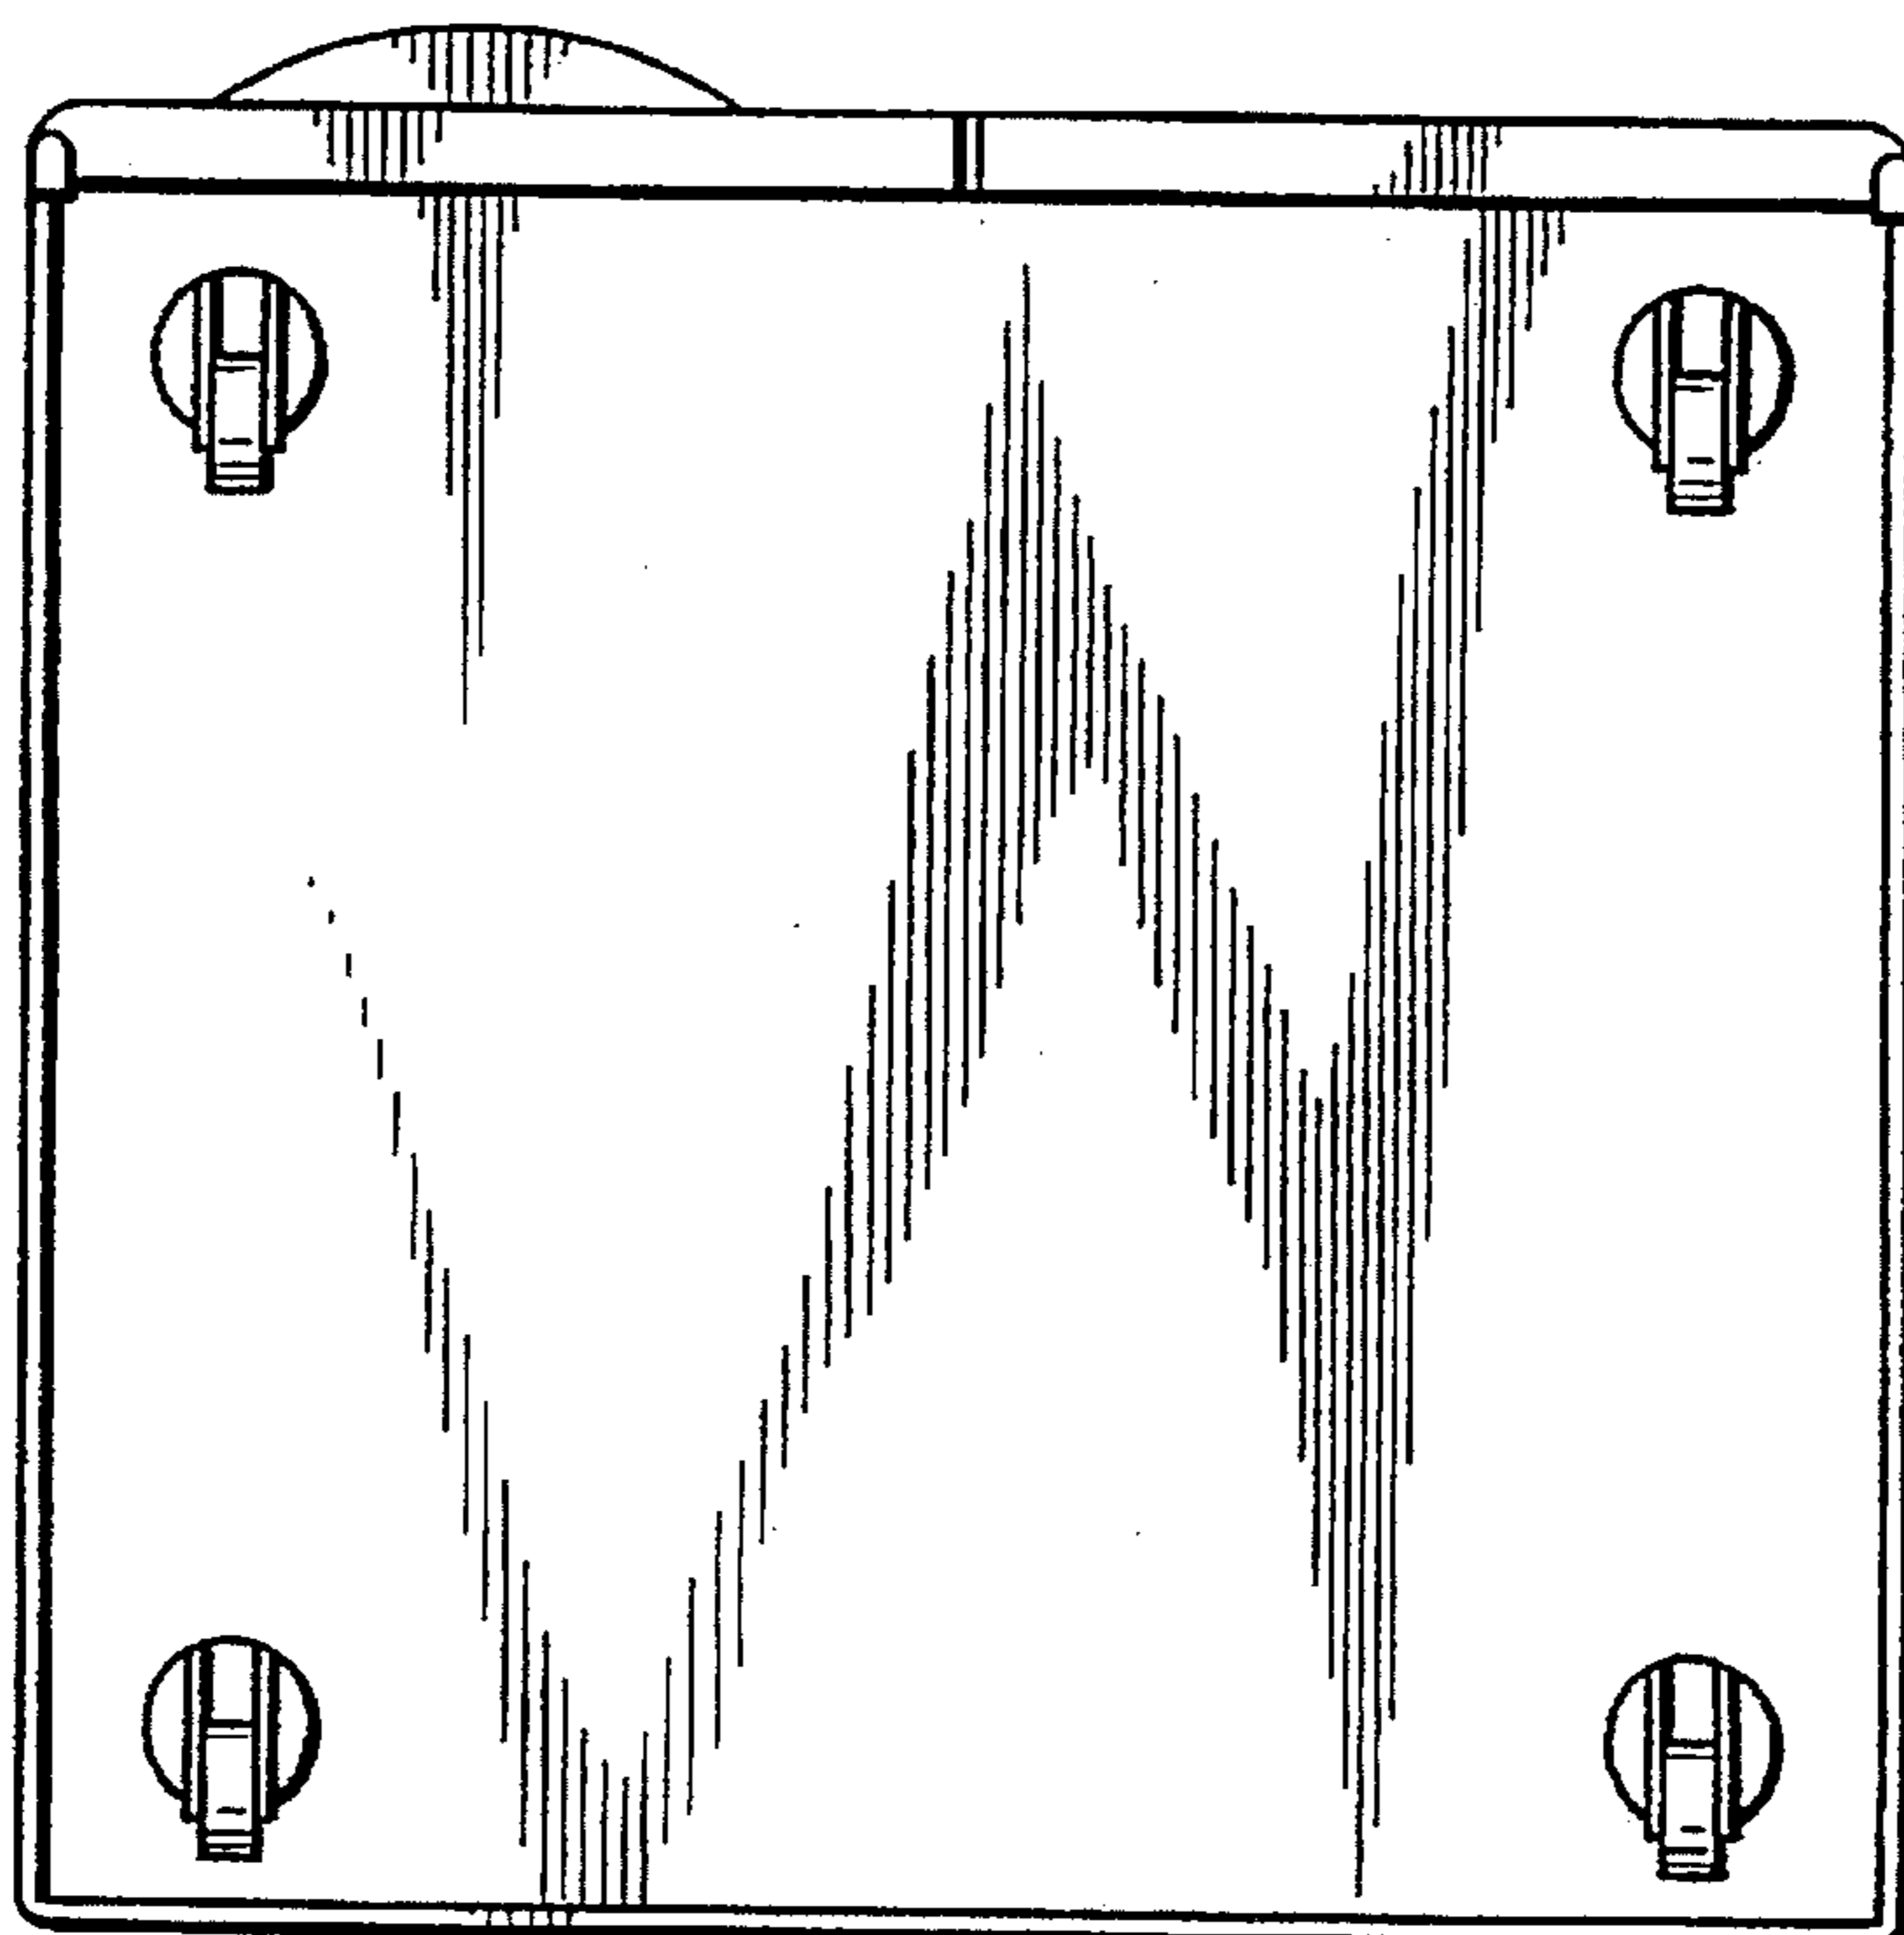


FIG. 4



*FIG. 5*


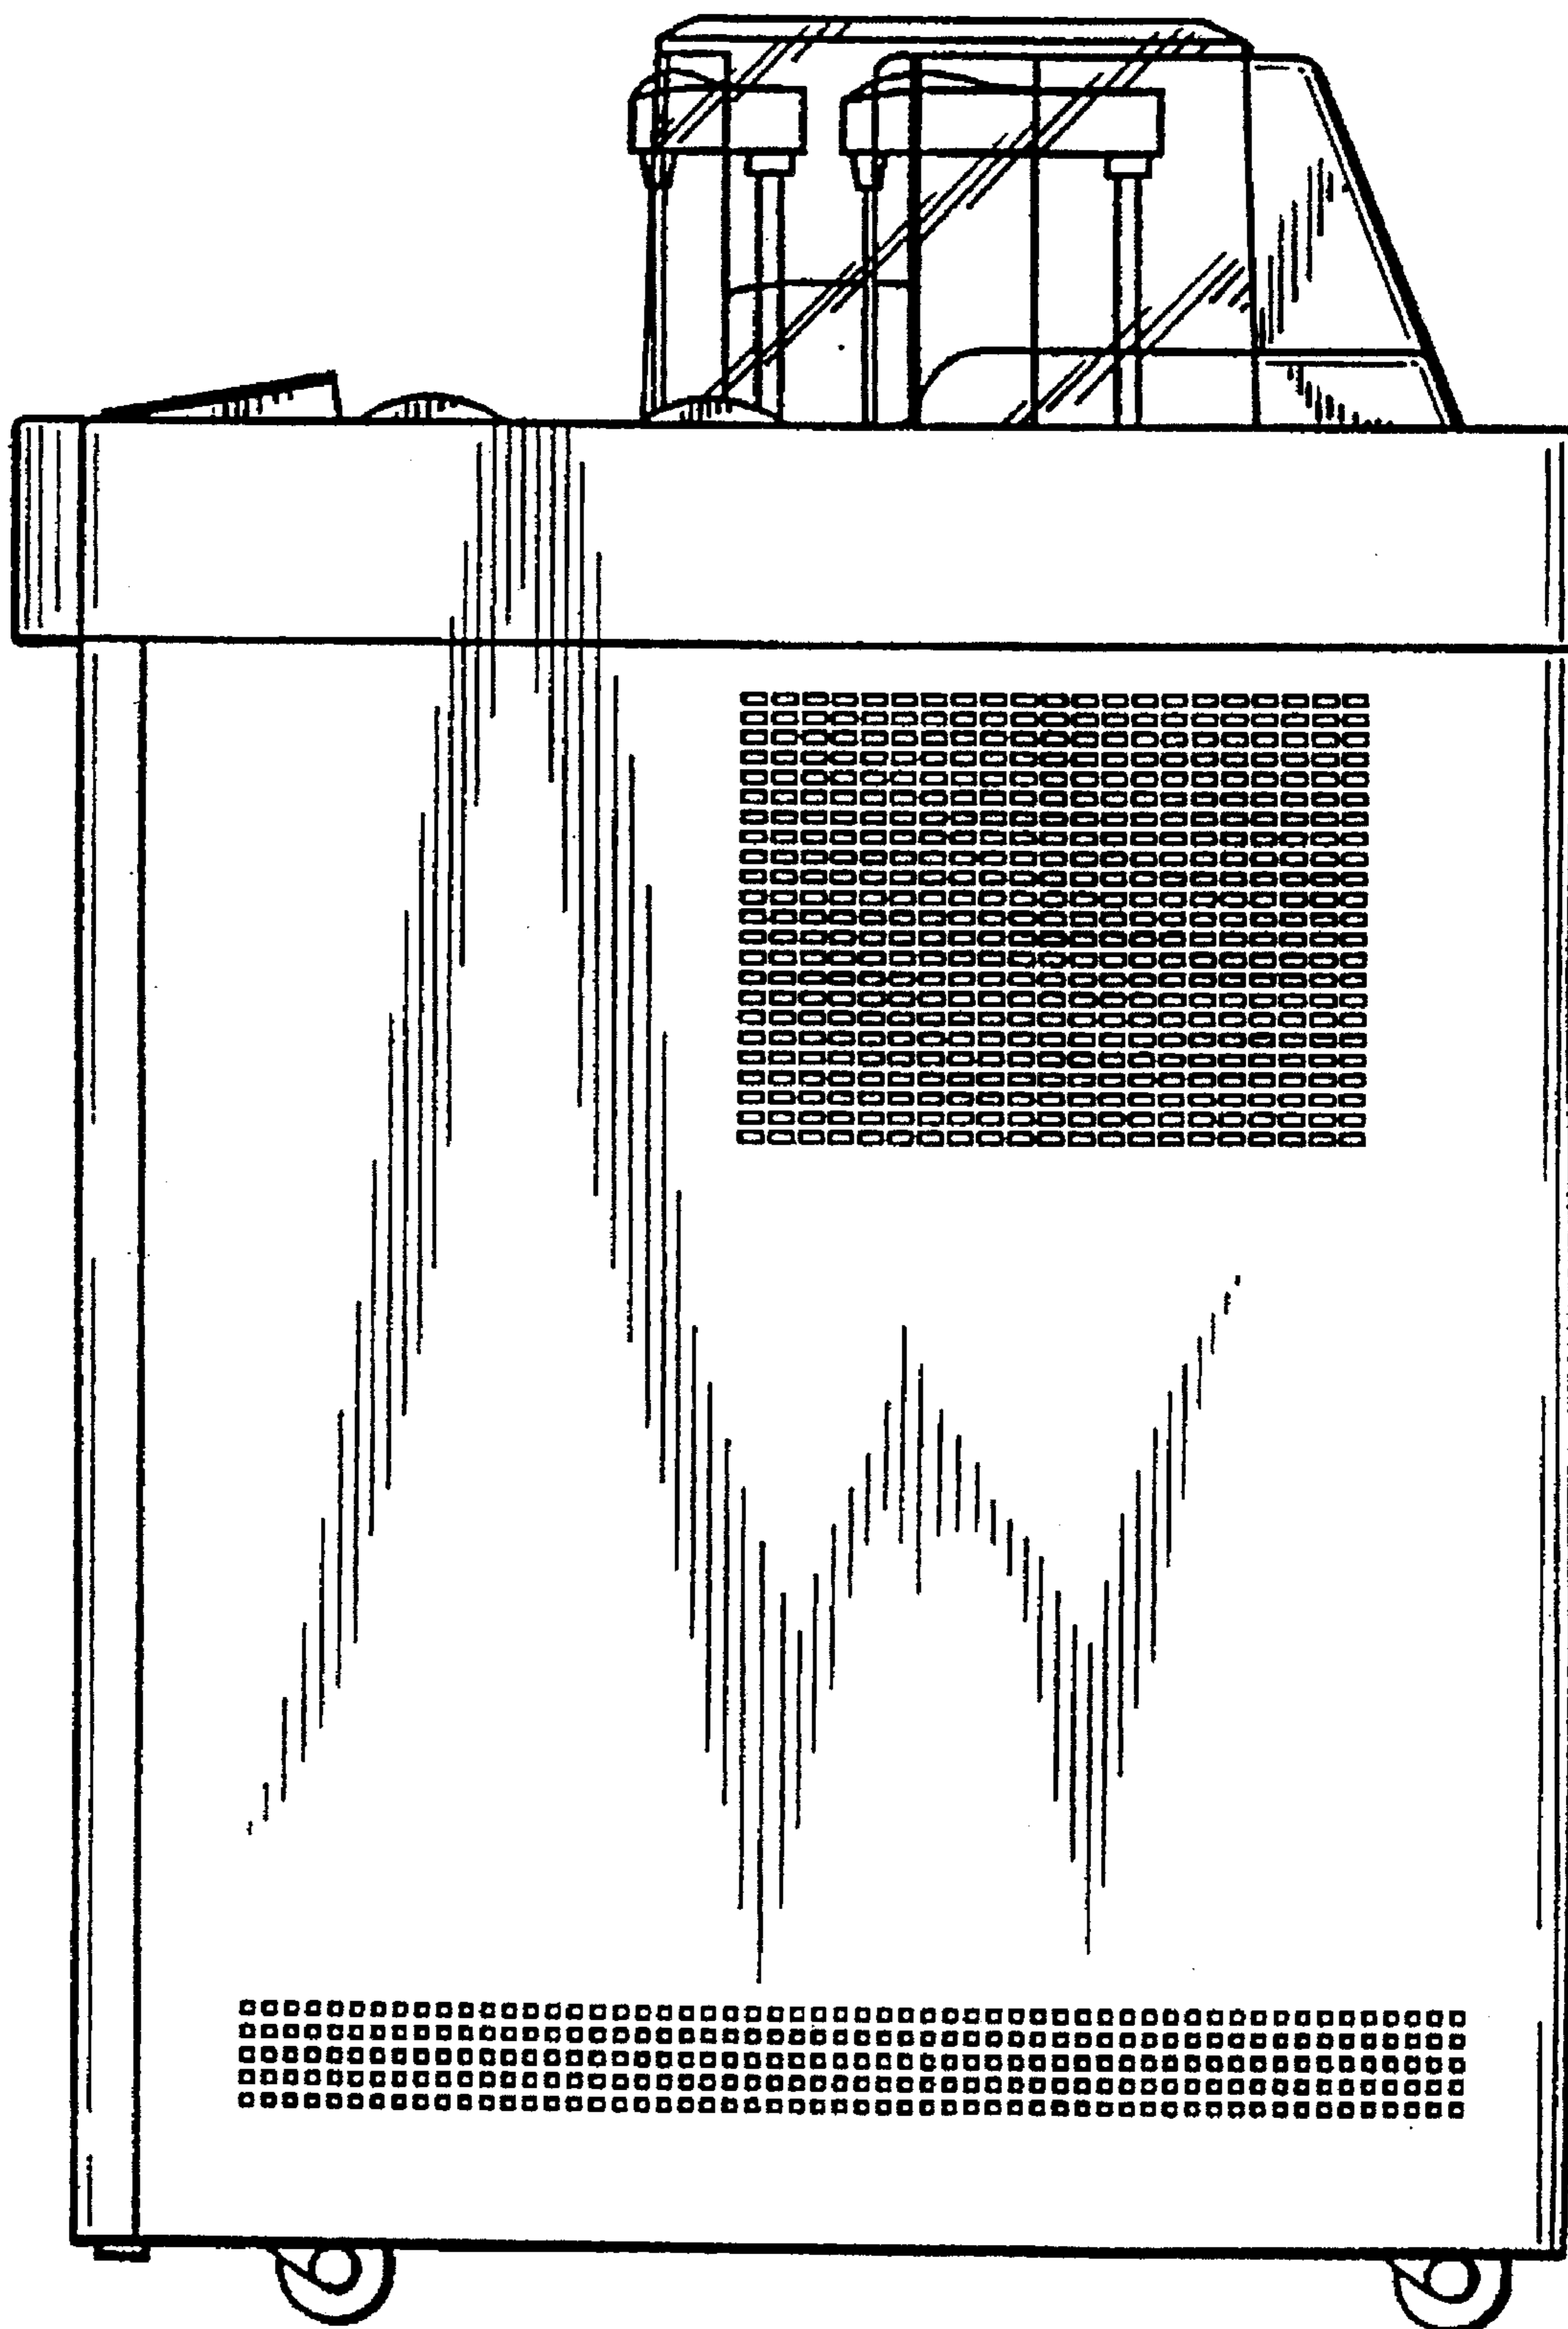


FIG. 6



*FIG. 7*

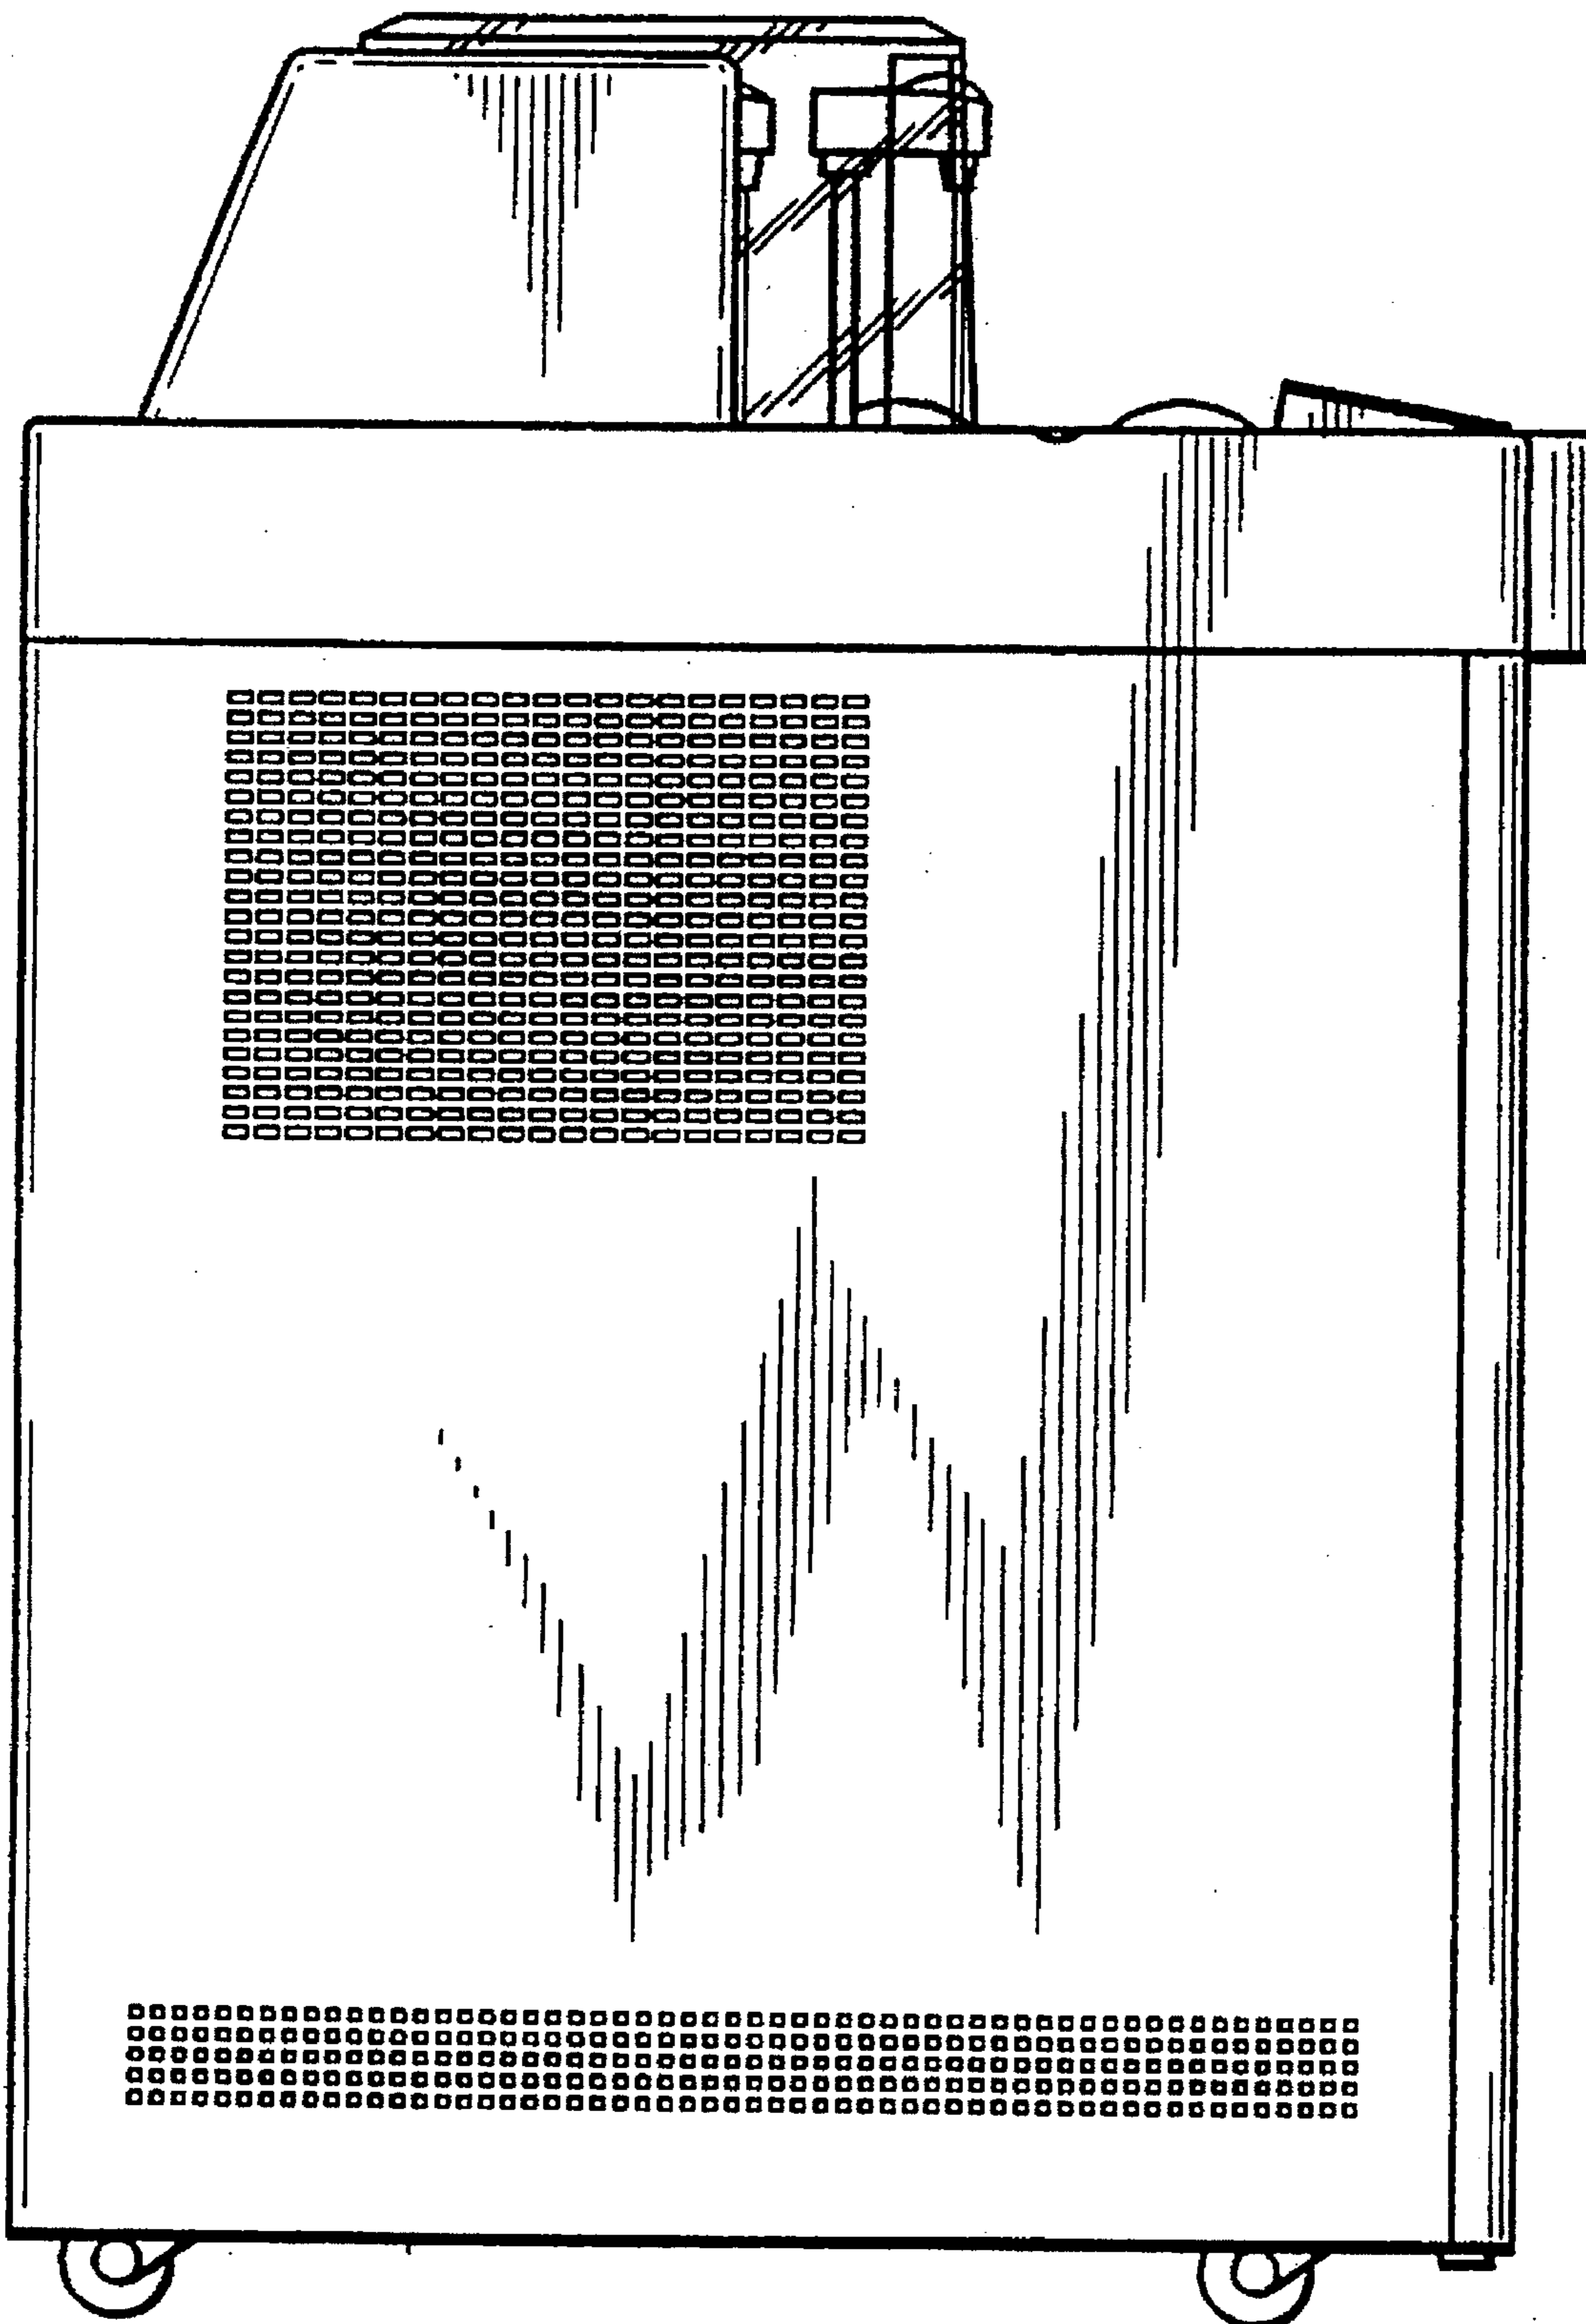