



US00D389587S

# United States Patent [19]

[11] Patent Number: **Des. 389,587**

Orell Porrazzo et al.

[45] Date of Patent: **\*\*Jan. 20, 1998**

[54] **SLIDE DEVICE FOR TESTING AND DISPLAYING FERTILITY DETERMINATIONS**

[57] **CLAIM**

The ornamental design for a slide device for testing and displaying fertility determinations, as shown and described.

[75] Inventors: **Karen P. Orell Porrazzo; Edward M. Porrazzo**, both of Carmichael, Calif.

**DESCRIPTION**

[73] Assignee: **Personal Fertility Technologies, Inc.**, Gold River, Calif.

FIG. 1 is a top plan view of first embodiment the viewing section of a slide device for testing and displaying fertility determinations showing our new design;

[\*\*] Term: **14 Years**

FIG. 2 is a top plan view of a second embodiment of the viewing section of a slide device for testing and displaying fertility determinations showing our new design;

[21] Appl. No.: **49,760**

[22] Filed: **Jan. 30, 1996**

FIG. 3 is a bottom plan view of the embodiments of FIGS. 1 and 2;

[51] LOC (6) Cl. .... **24-01**

[52] U.S. Cl. .... **D24/225; D24/216**

[58] Field of Search ..... **D24/225, 224, D24/223, 216, 217, 226; 128/738; 422/82.05, 61; 435/806; 436/906**

FIG. 4 is a top plan view of the testing section;

FIG. 5 is a bottom plan view of the testing section of FIG. 4;

[56] **References Cited**

**U.S. PATENT DOCUMENTS**

D. 227,942	7/1973	Kelson	.....	D24/217
D. 253,492	11/1979	Augurt	.....	D10/81 X
D. 310,265	8/1990	Mochnal et al.	.....	D24/223
D. 324,426	3/1992	Fan et al.	.....	D24/226
D. 341,663	11/1993	Coulter	.....	D24/225
3,552,929	1/1971	Fields et al.	.....	D24/225 X
4,151,833	5/1979	Polishlik	.....	128/739
4,815,835	3/1989	Ortueta Corona	.....	128/738 X
5,043,888	8/1991	Uriarte	.....	128/738

FIG. 6 is a top plan view of the combined viewing and testing sections rotated 60° from one another;

FIG. 7 is a bottom plan view of the combined viewing and testing sections of FIG. 6;

FIG. 8 is a front elevational view of the combined viewing and testing sections of FIGS. 6 and 7 in congruent orientation, the left and right side views being identical thereto;

FIG. 9 is a front elevational view of the viewing and testing sections of FIGS. 1-5, the left and right side views being identical thereto; and,

FIG. 10 is a rear elevational view of the viewing and testing sections of FIGS. 1-5.


**OTHER PUBLICATIONS**

Abbott Laboratories "Test Pack HCG Urine" Pregnancy Test Kit CLS 1986.

Primary Examiner—Stella Reid

Attorney, Agent, or Firm—Bielen, Peterson & Lampe

**1 Claim, 2 Drawing Sheets**

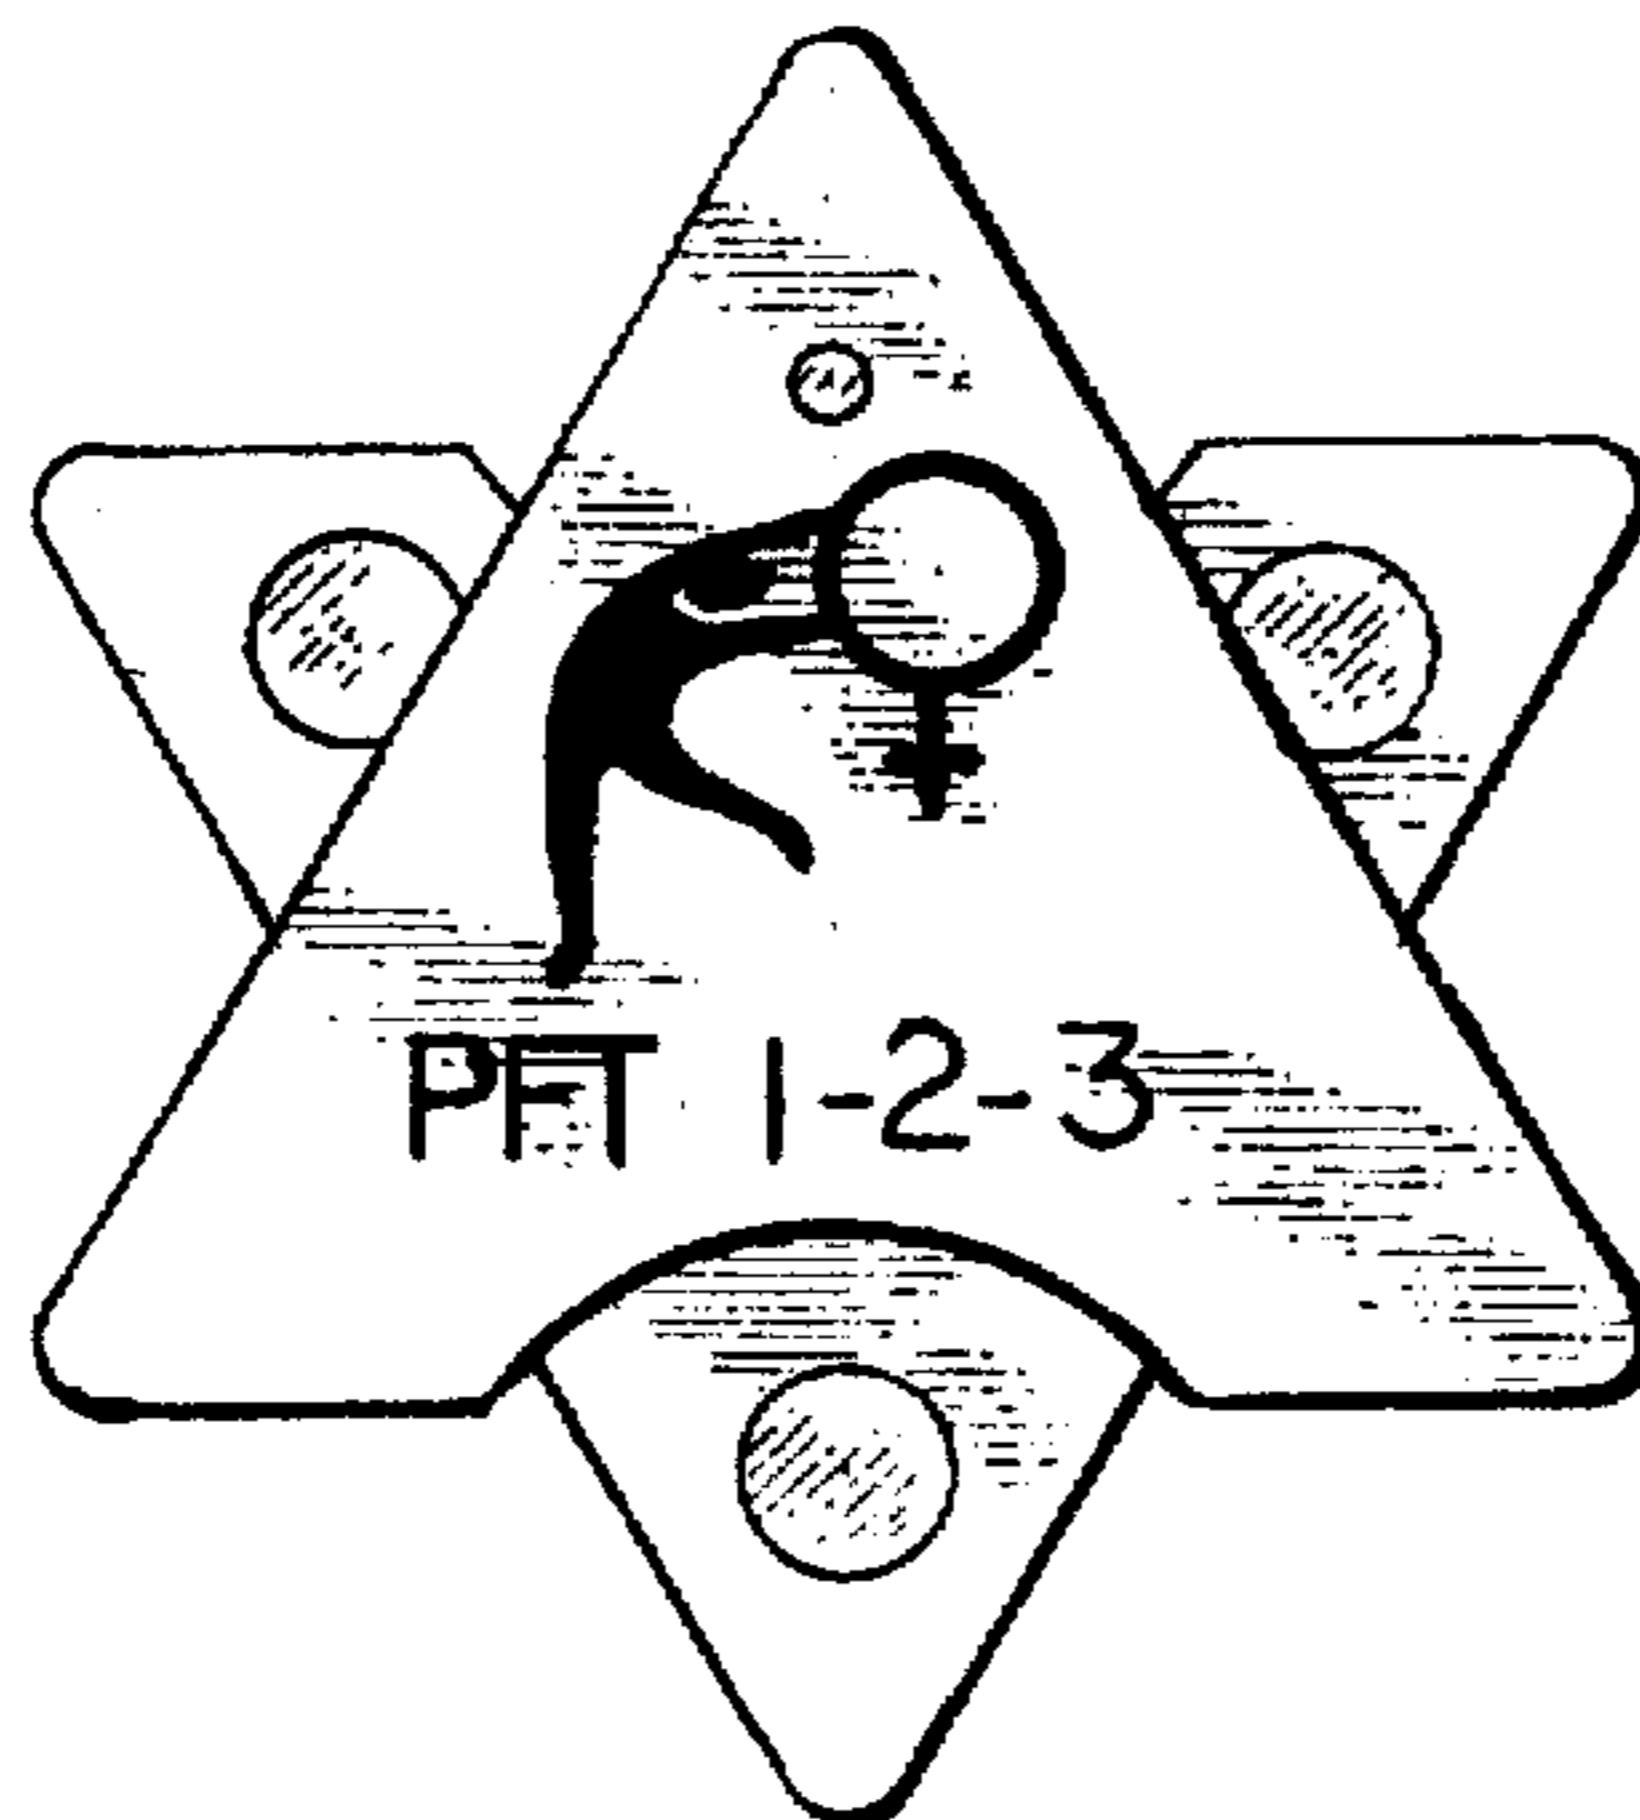

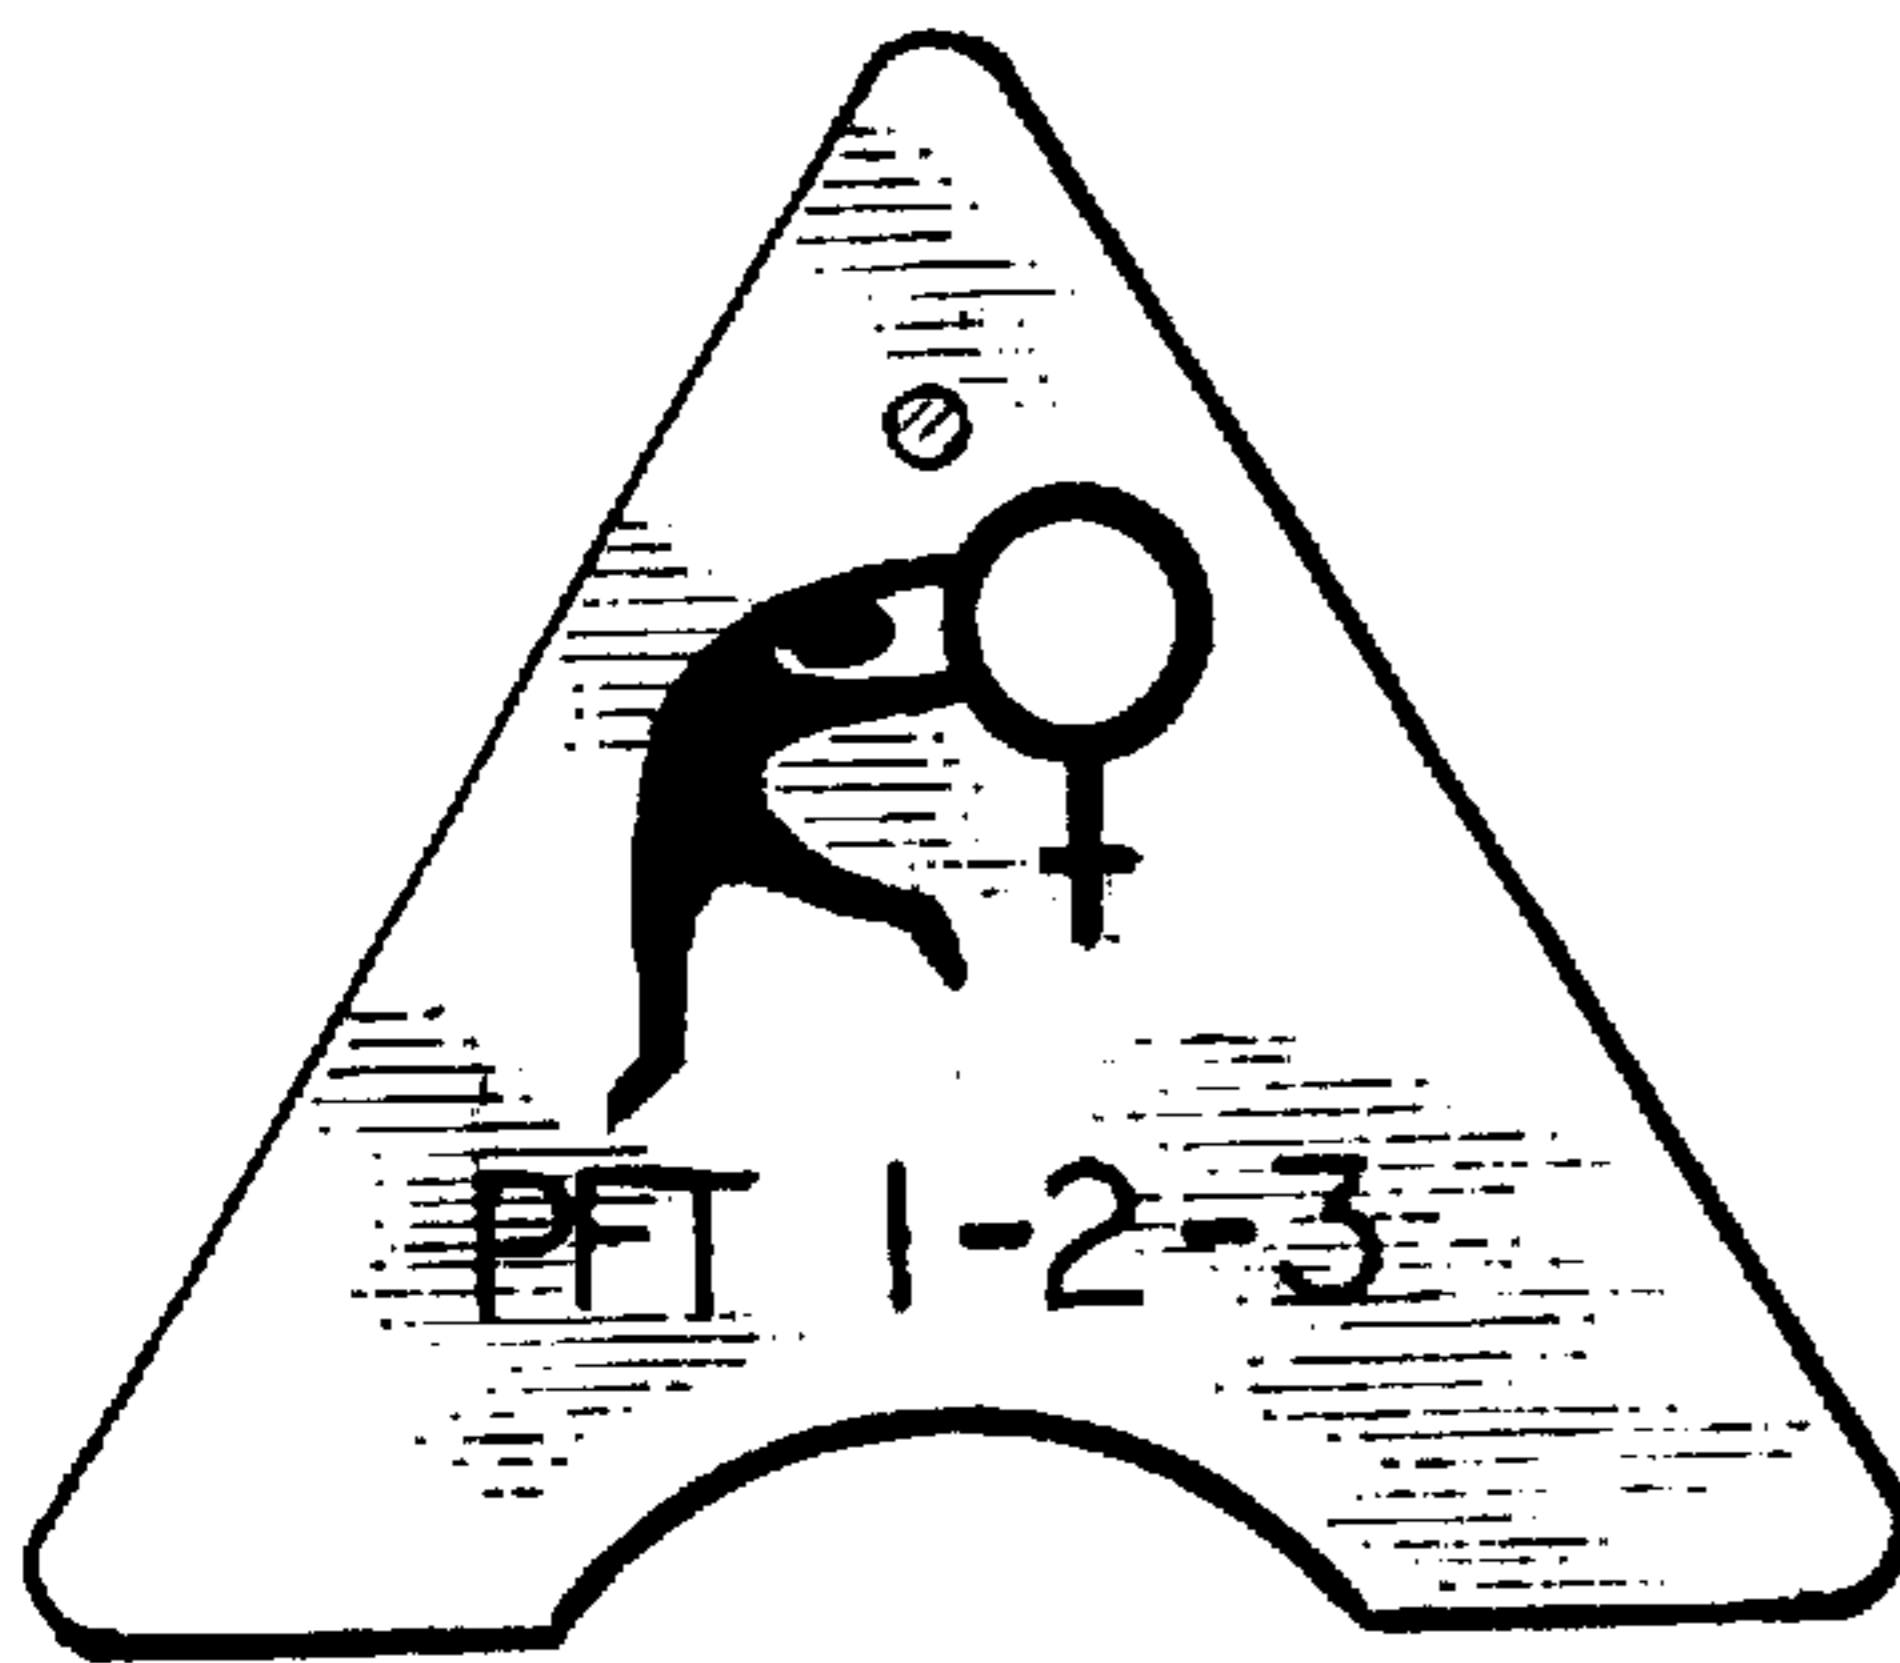


FIG-1

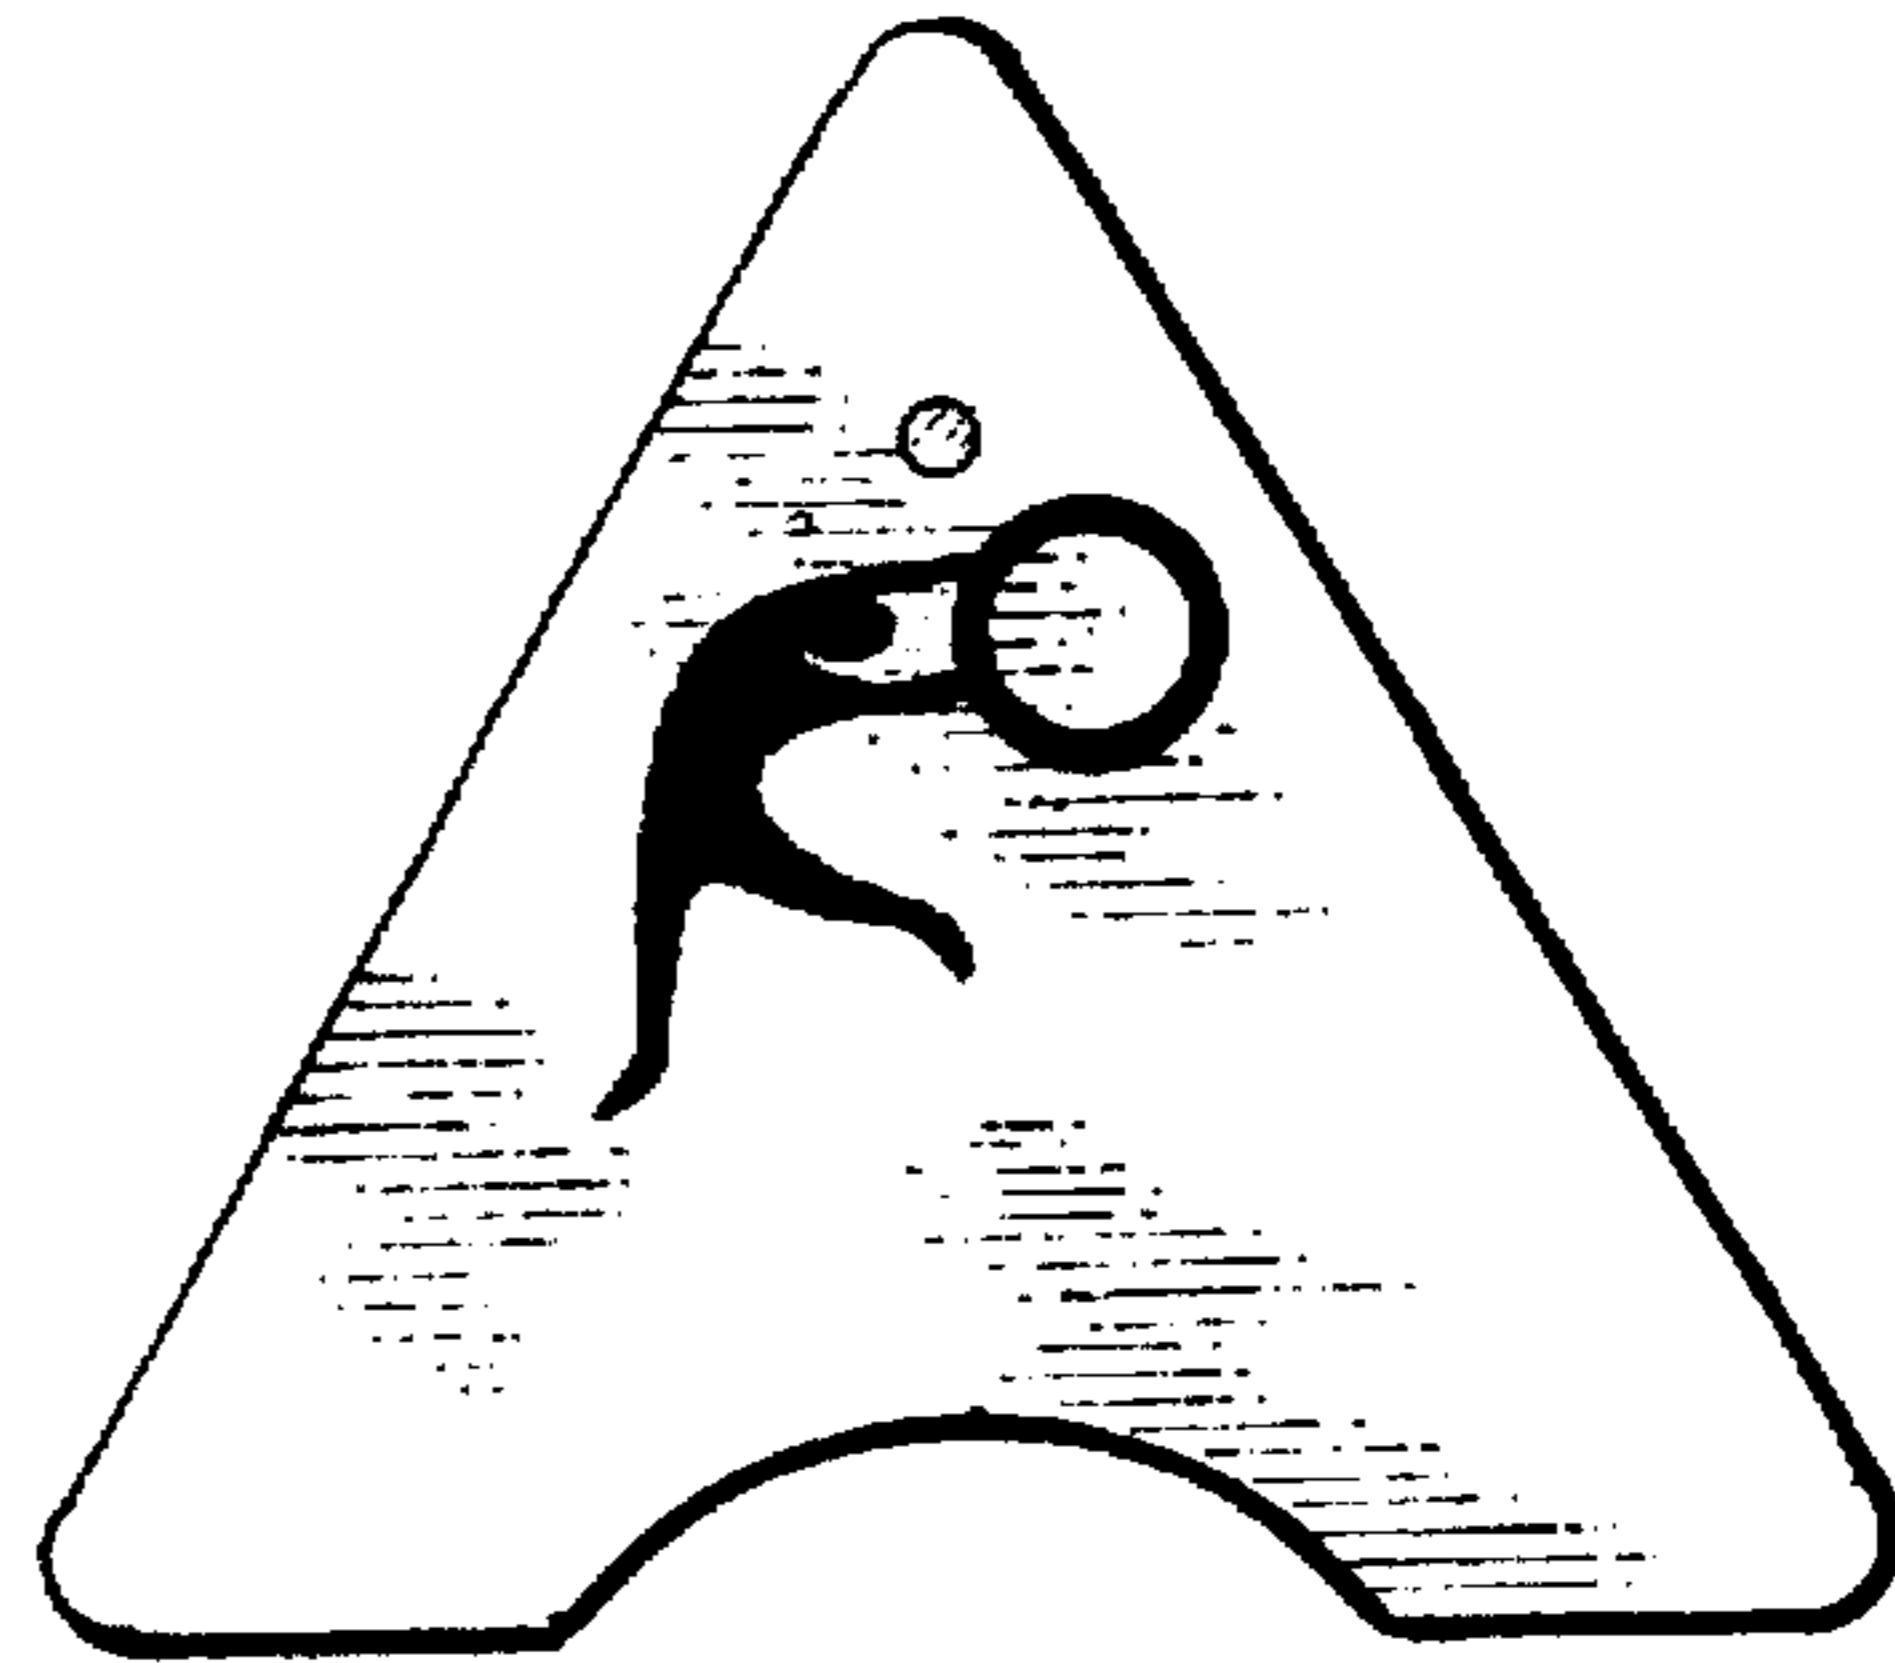


FIG-2

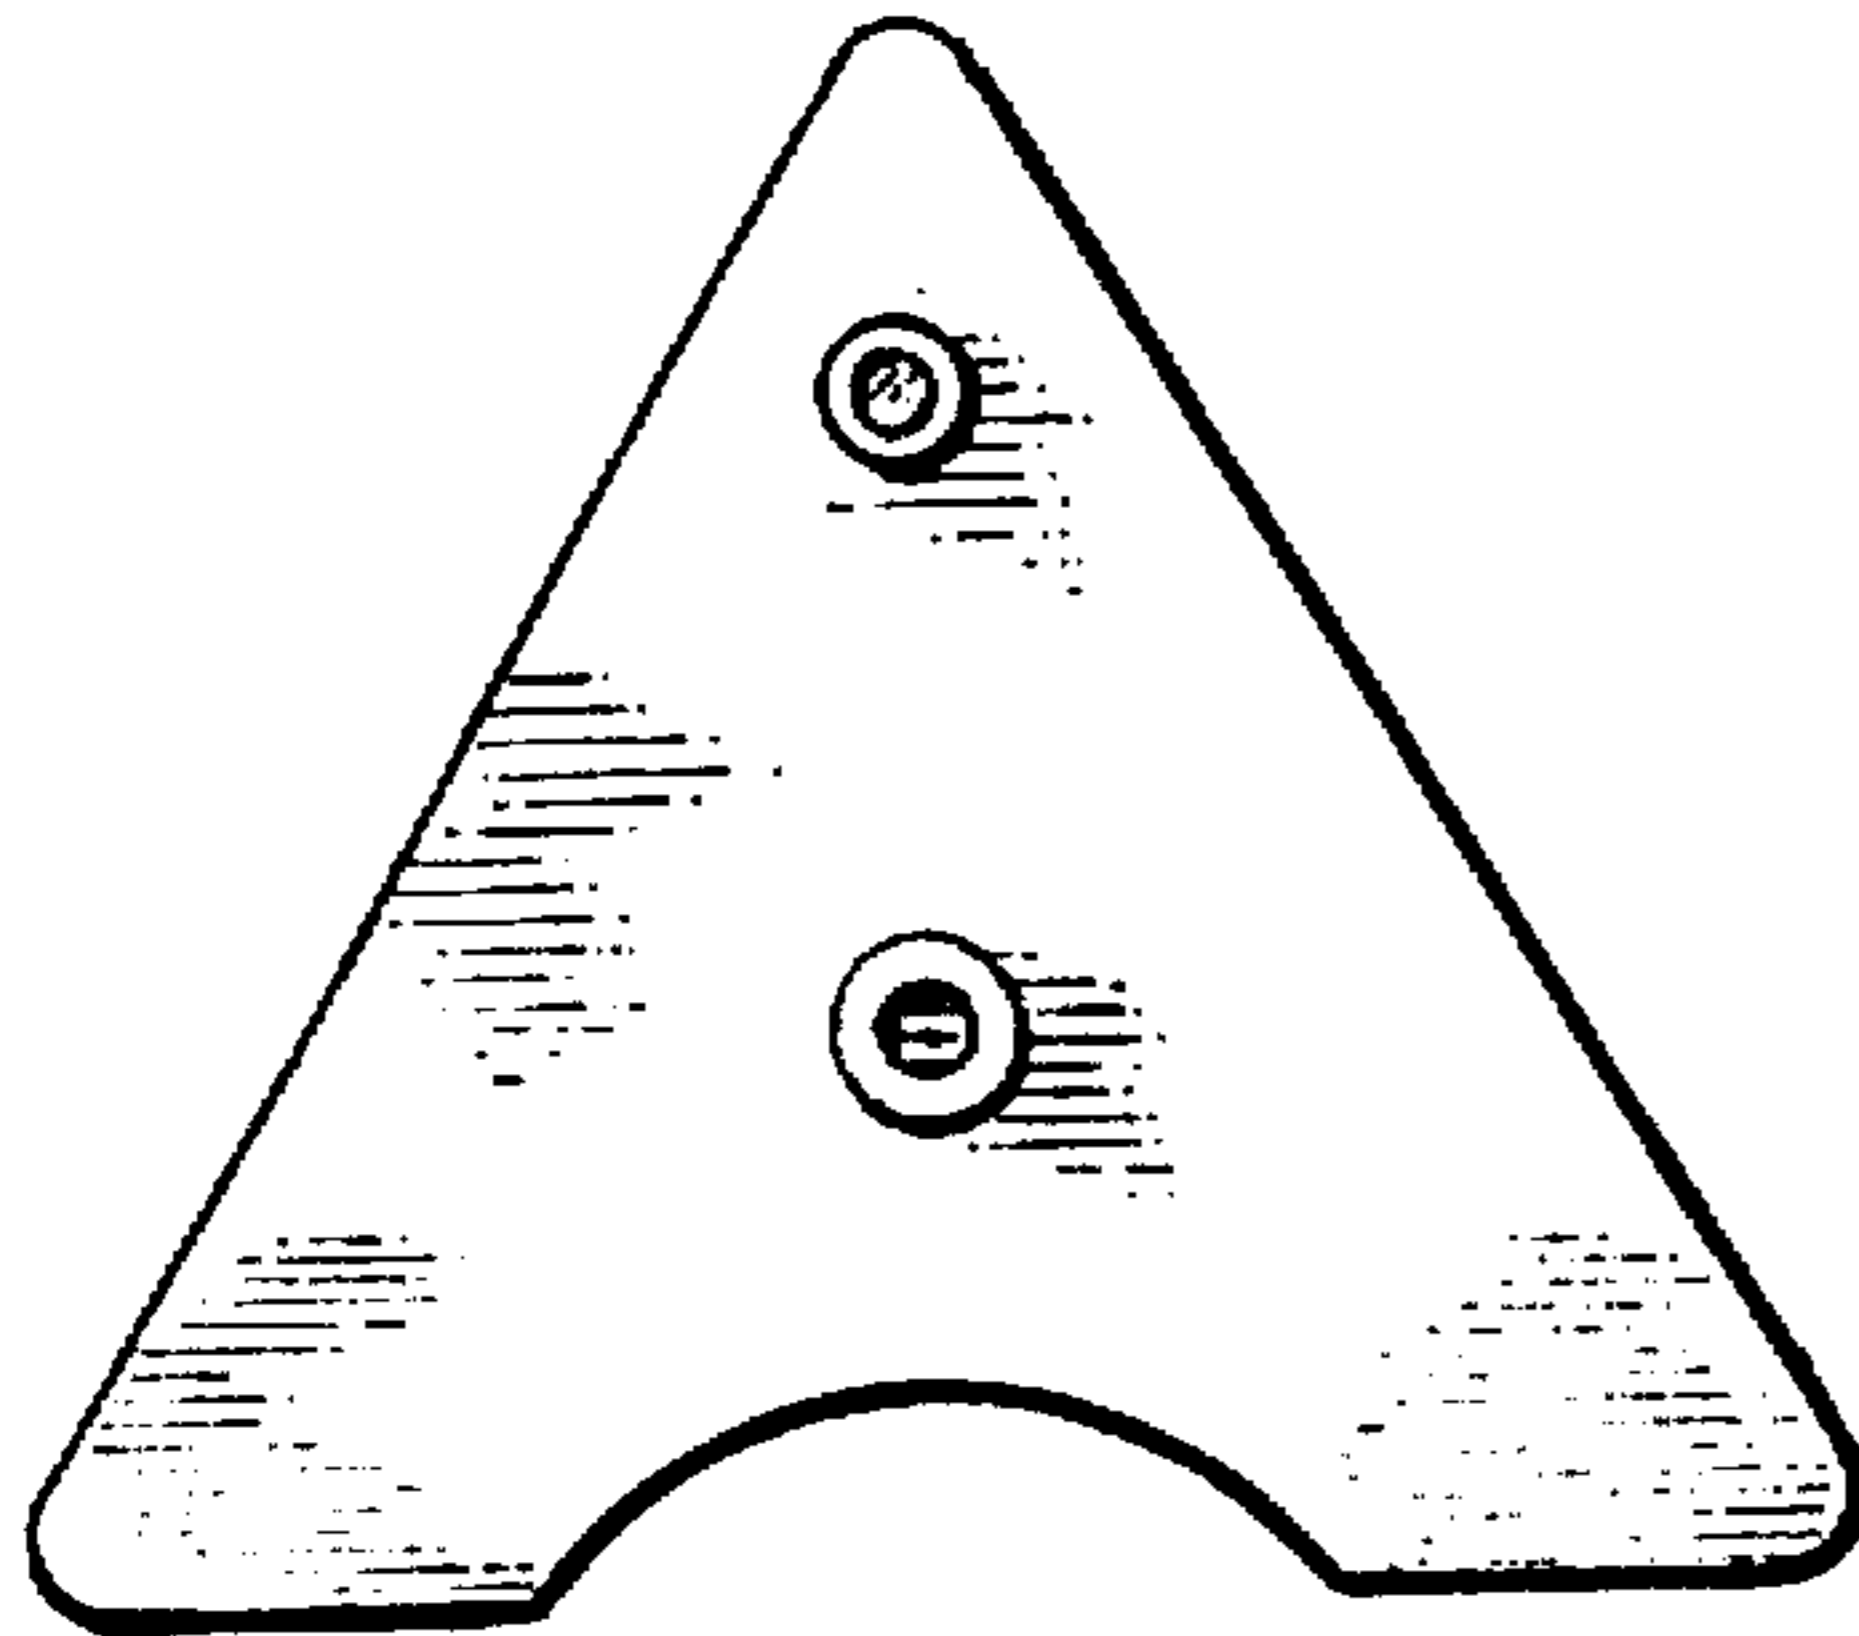


FIG-3

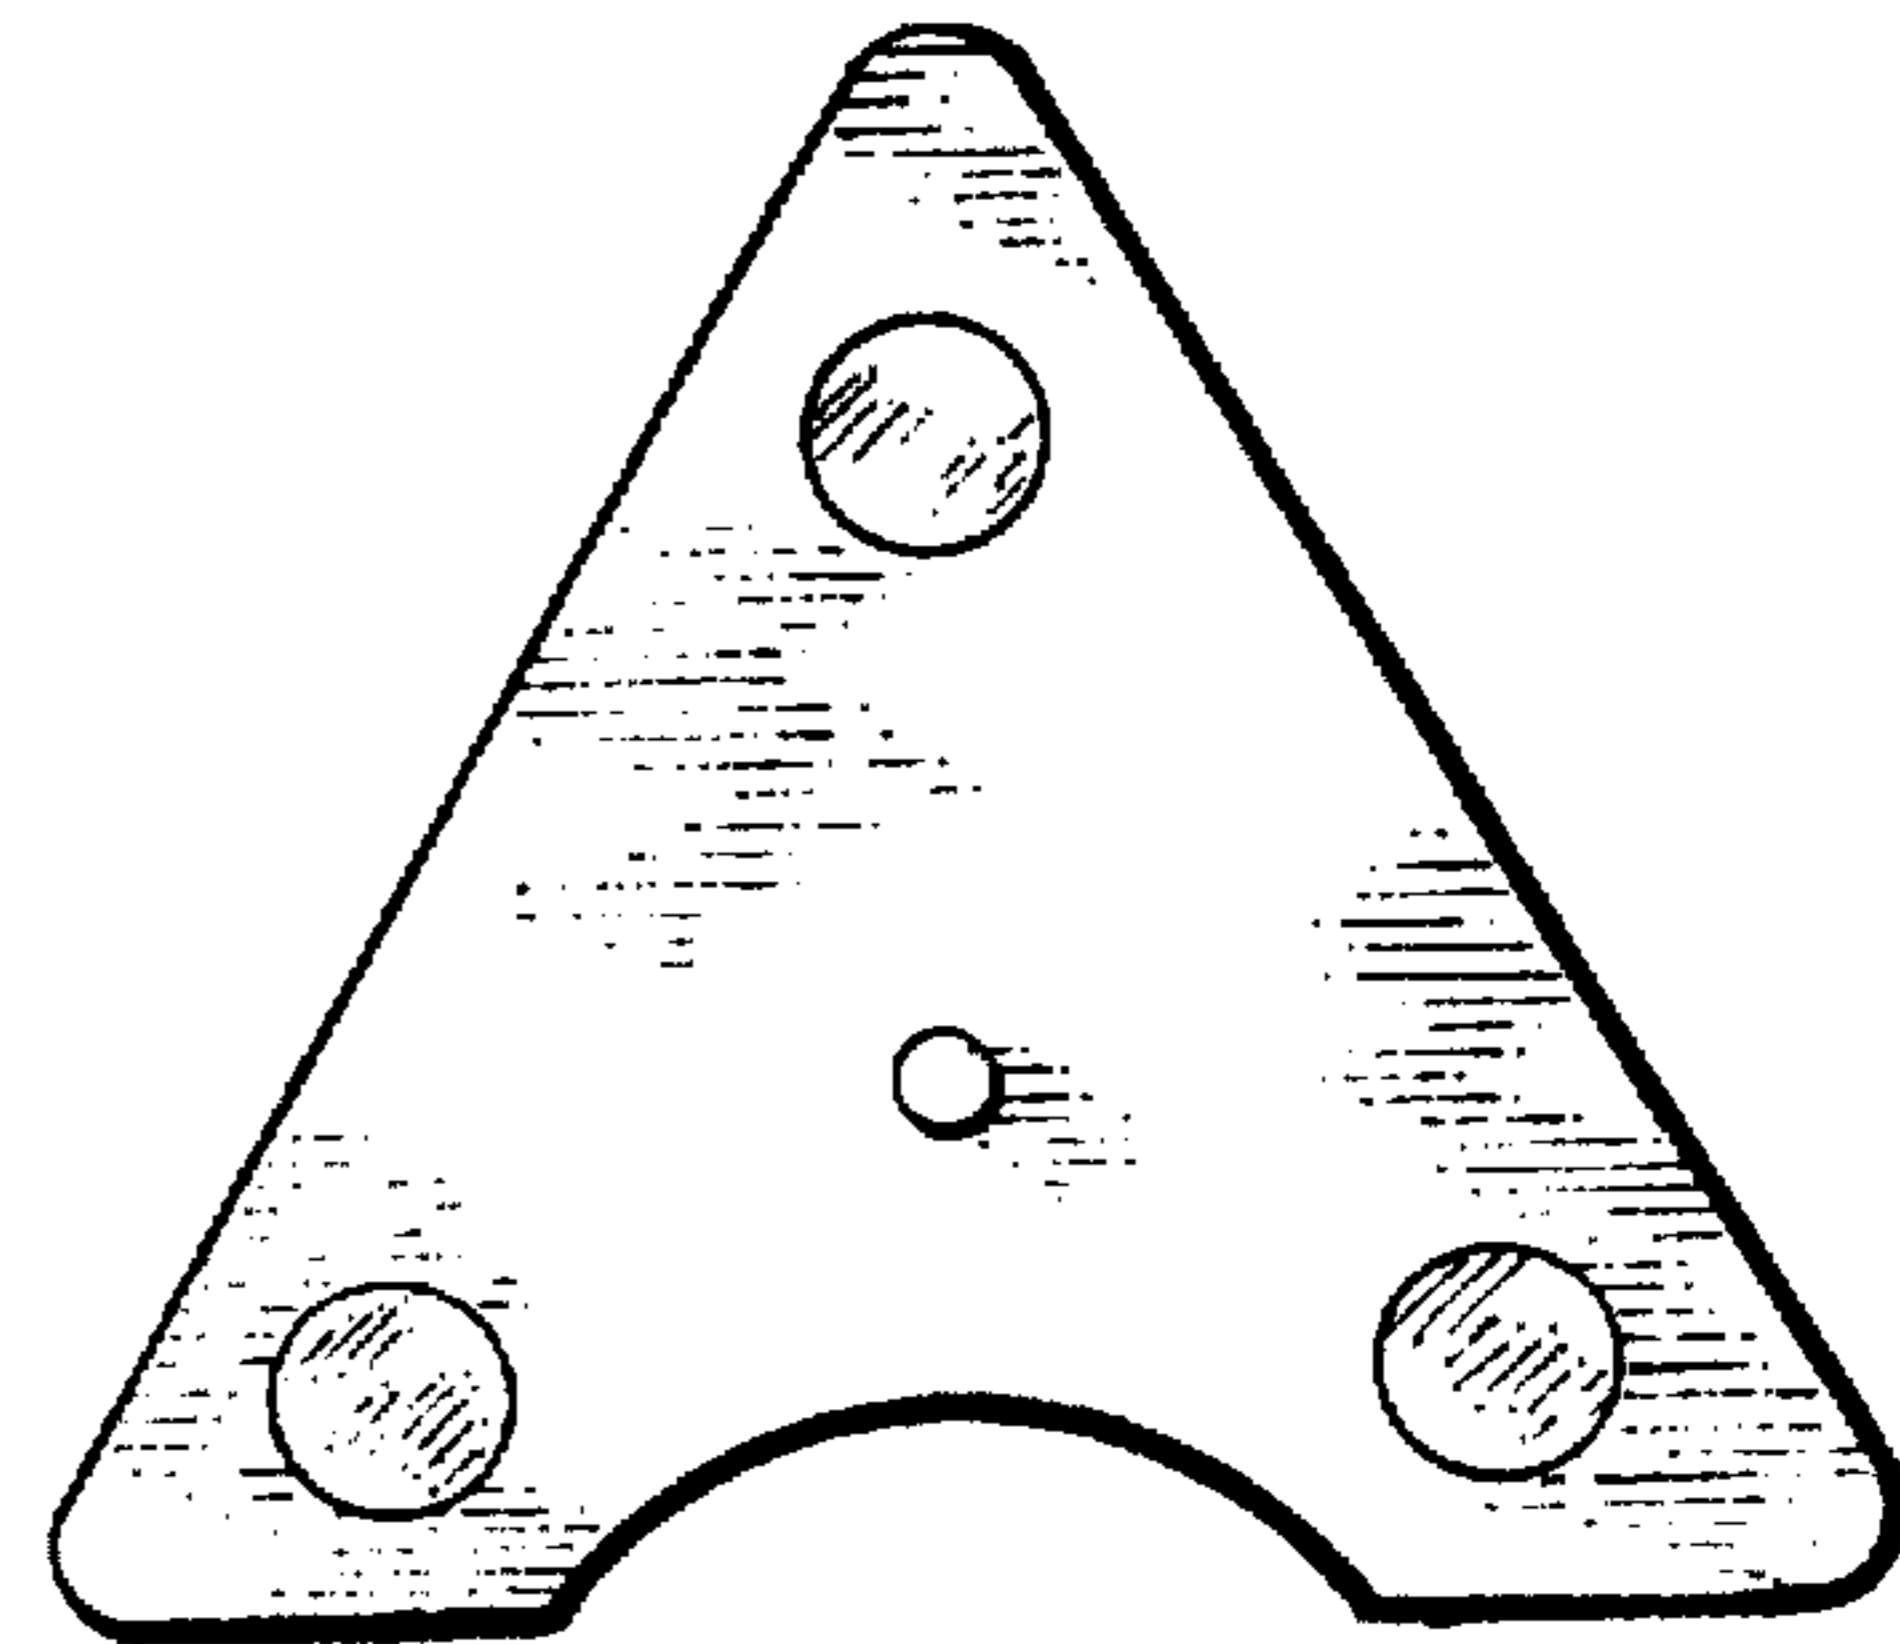


FIG-4

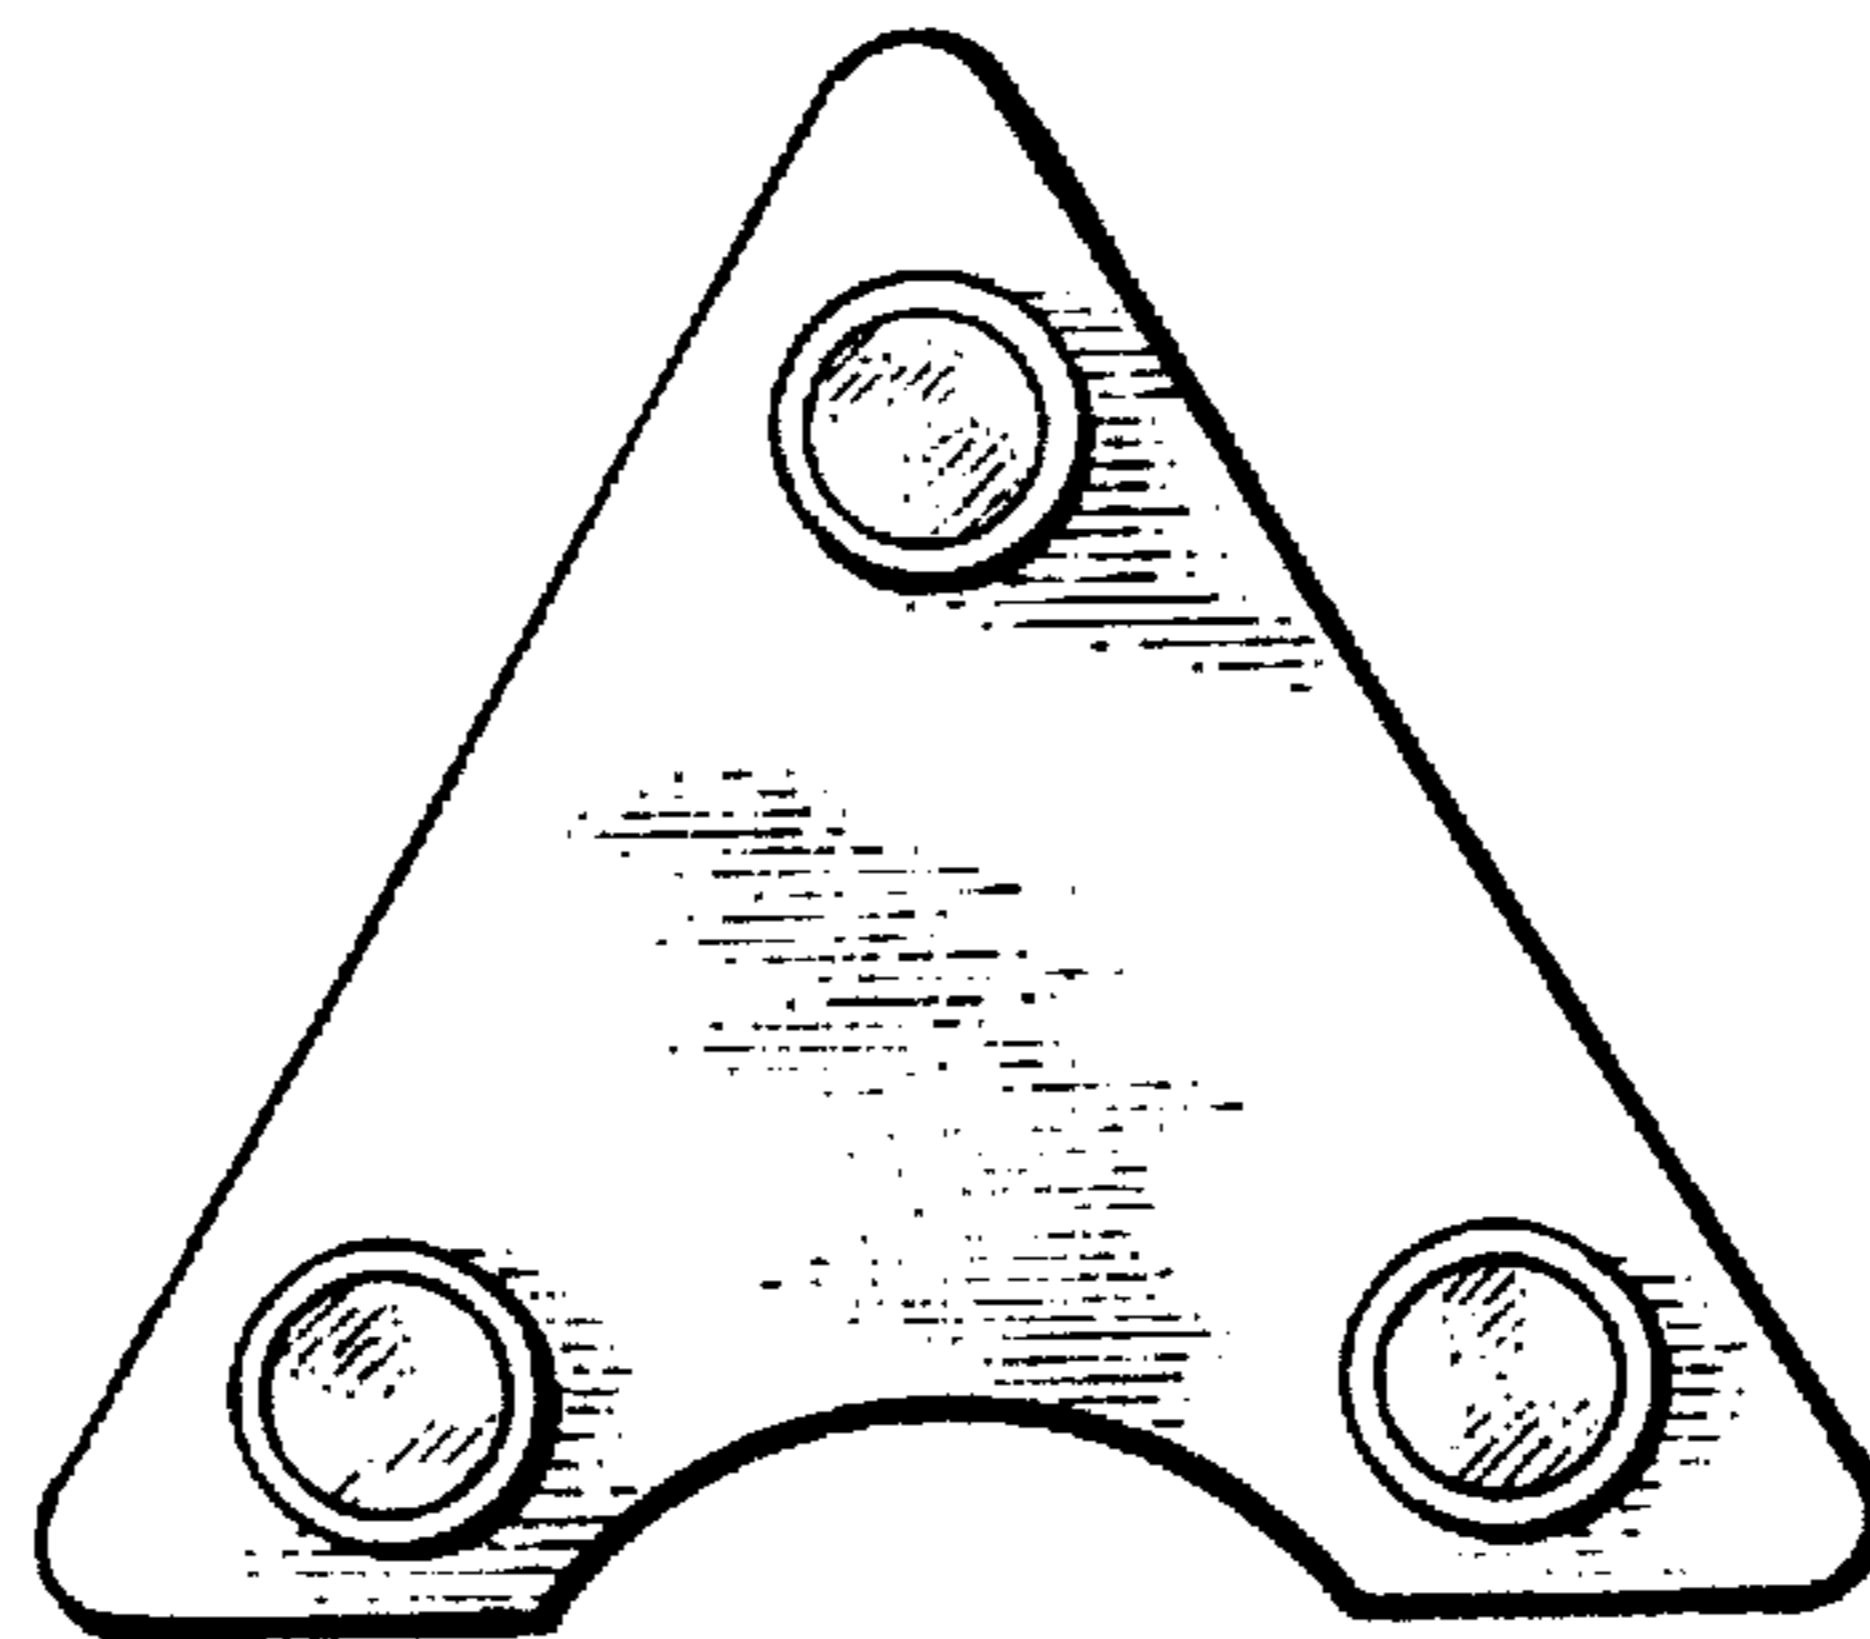


FIG-5

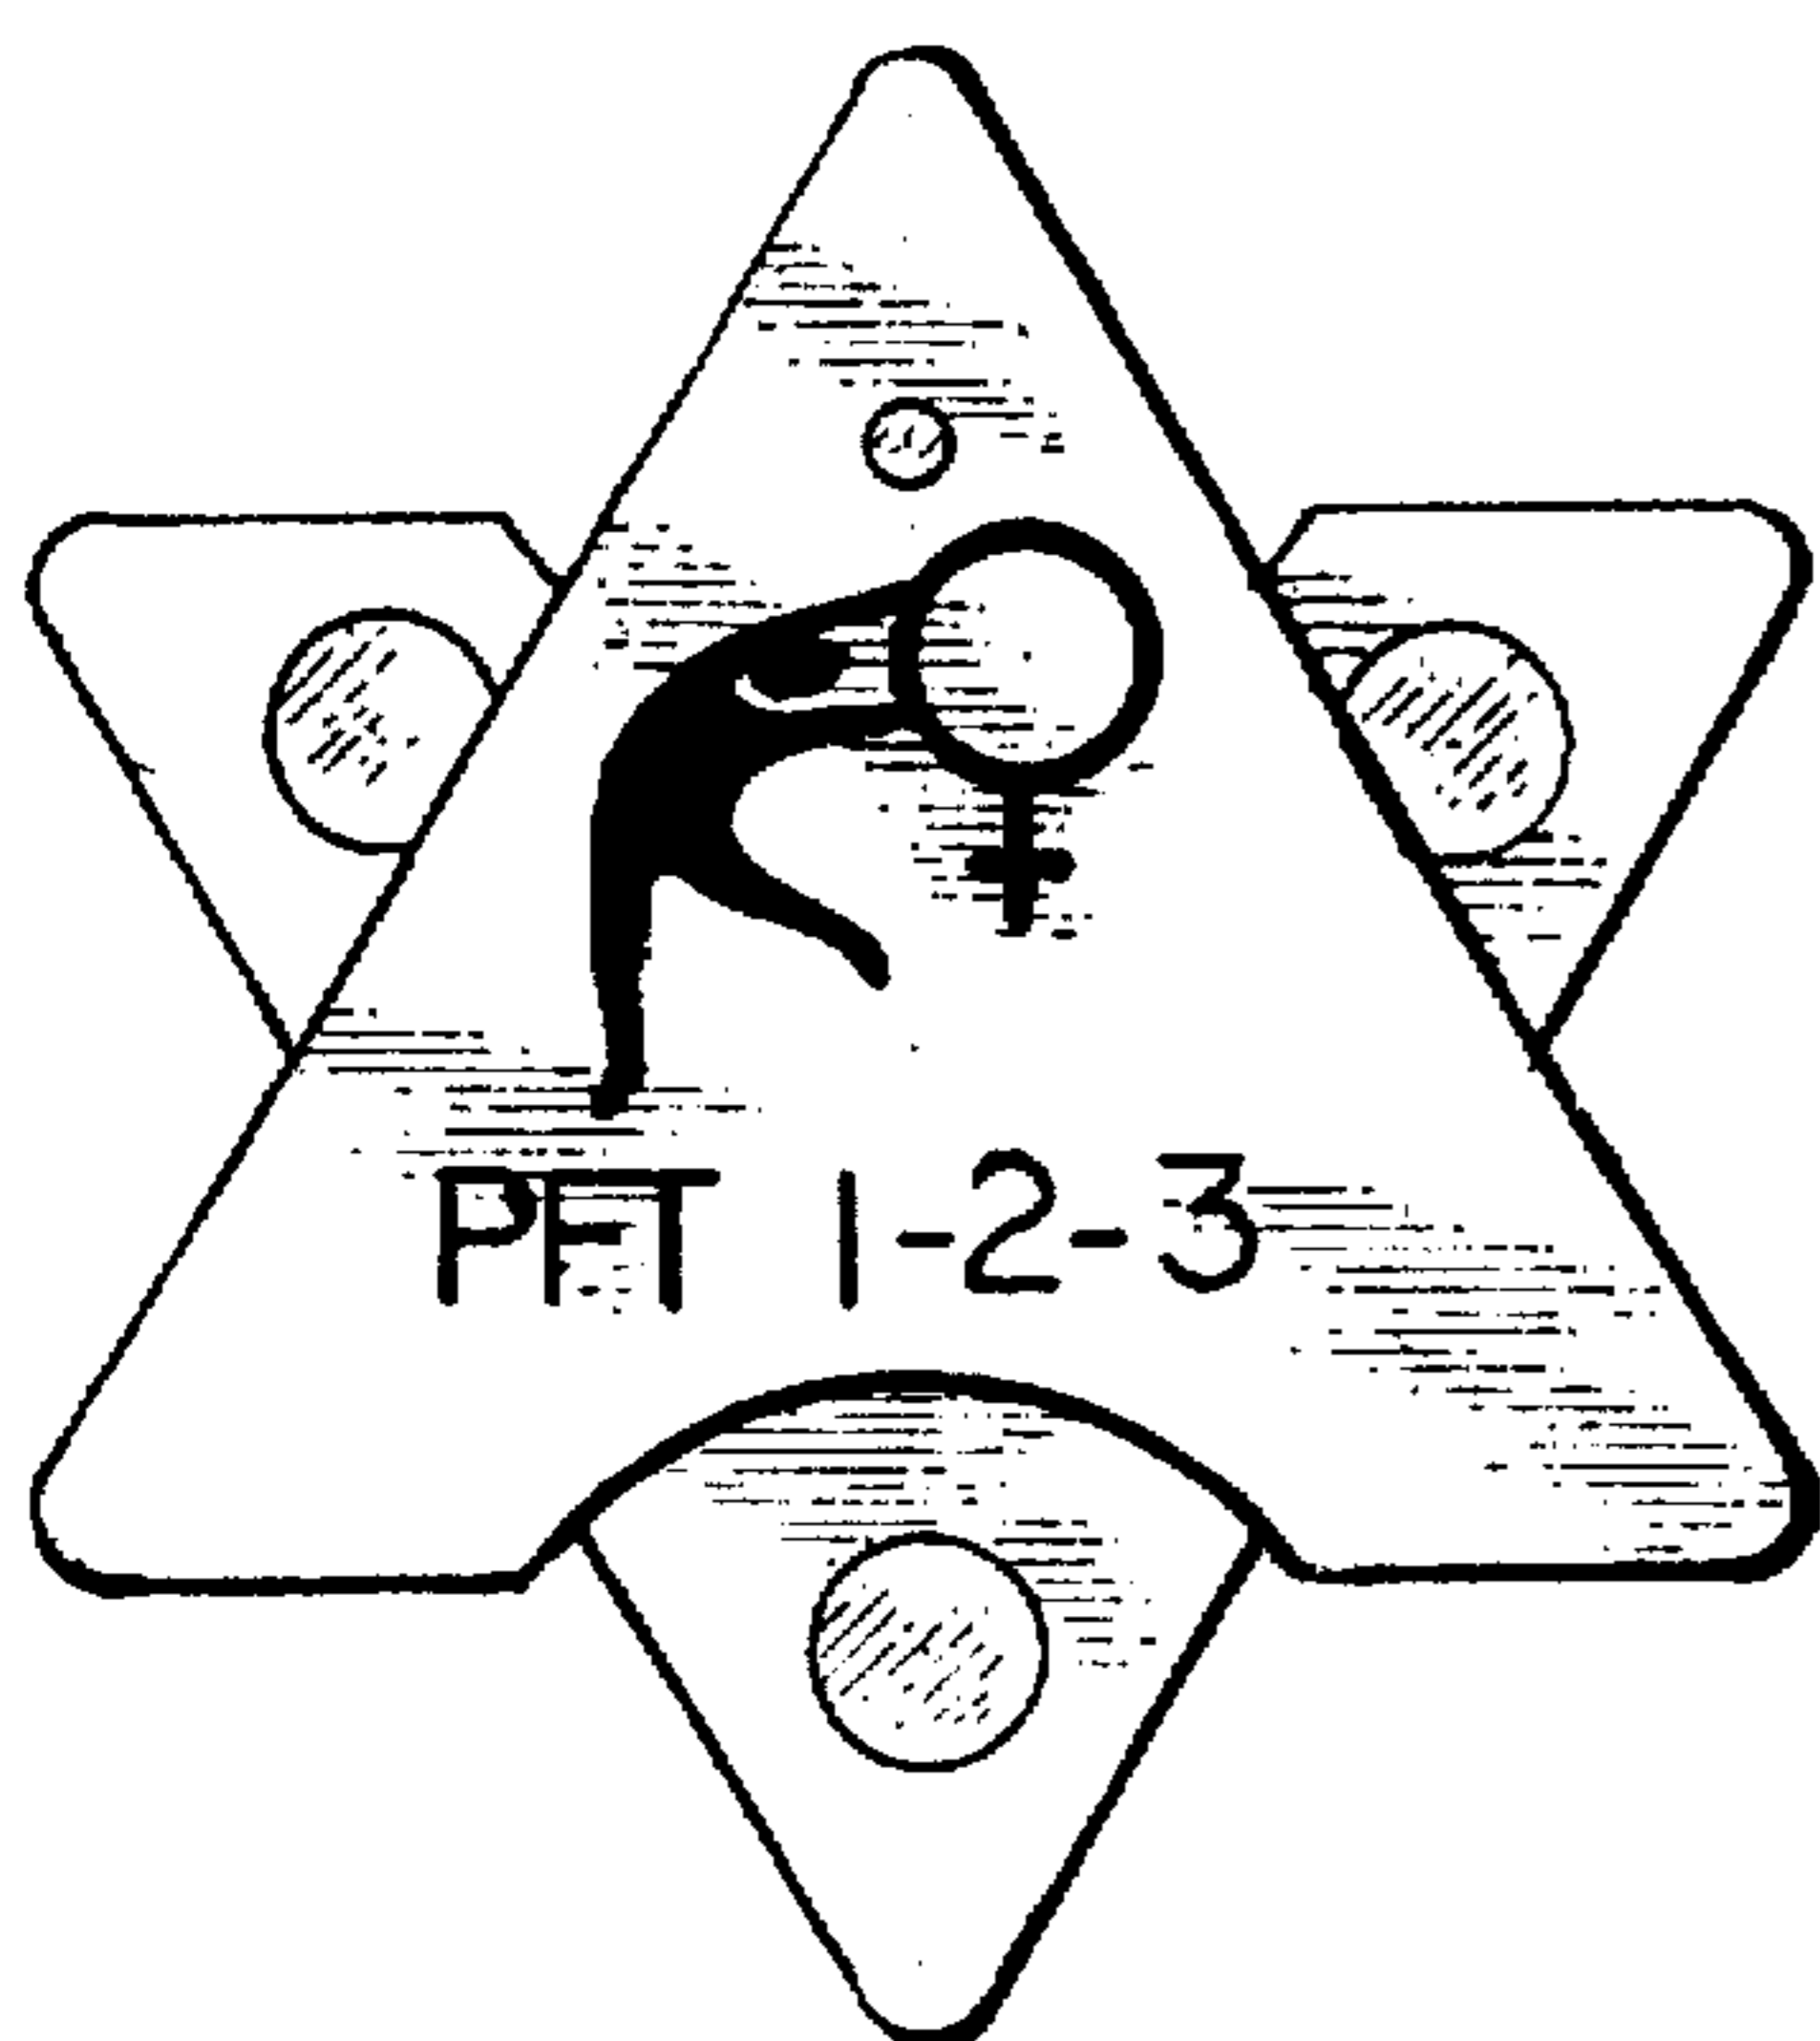


FIG. 6

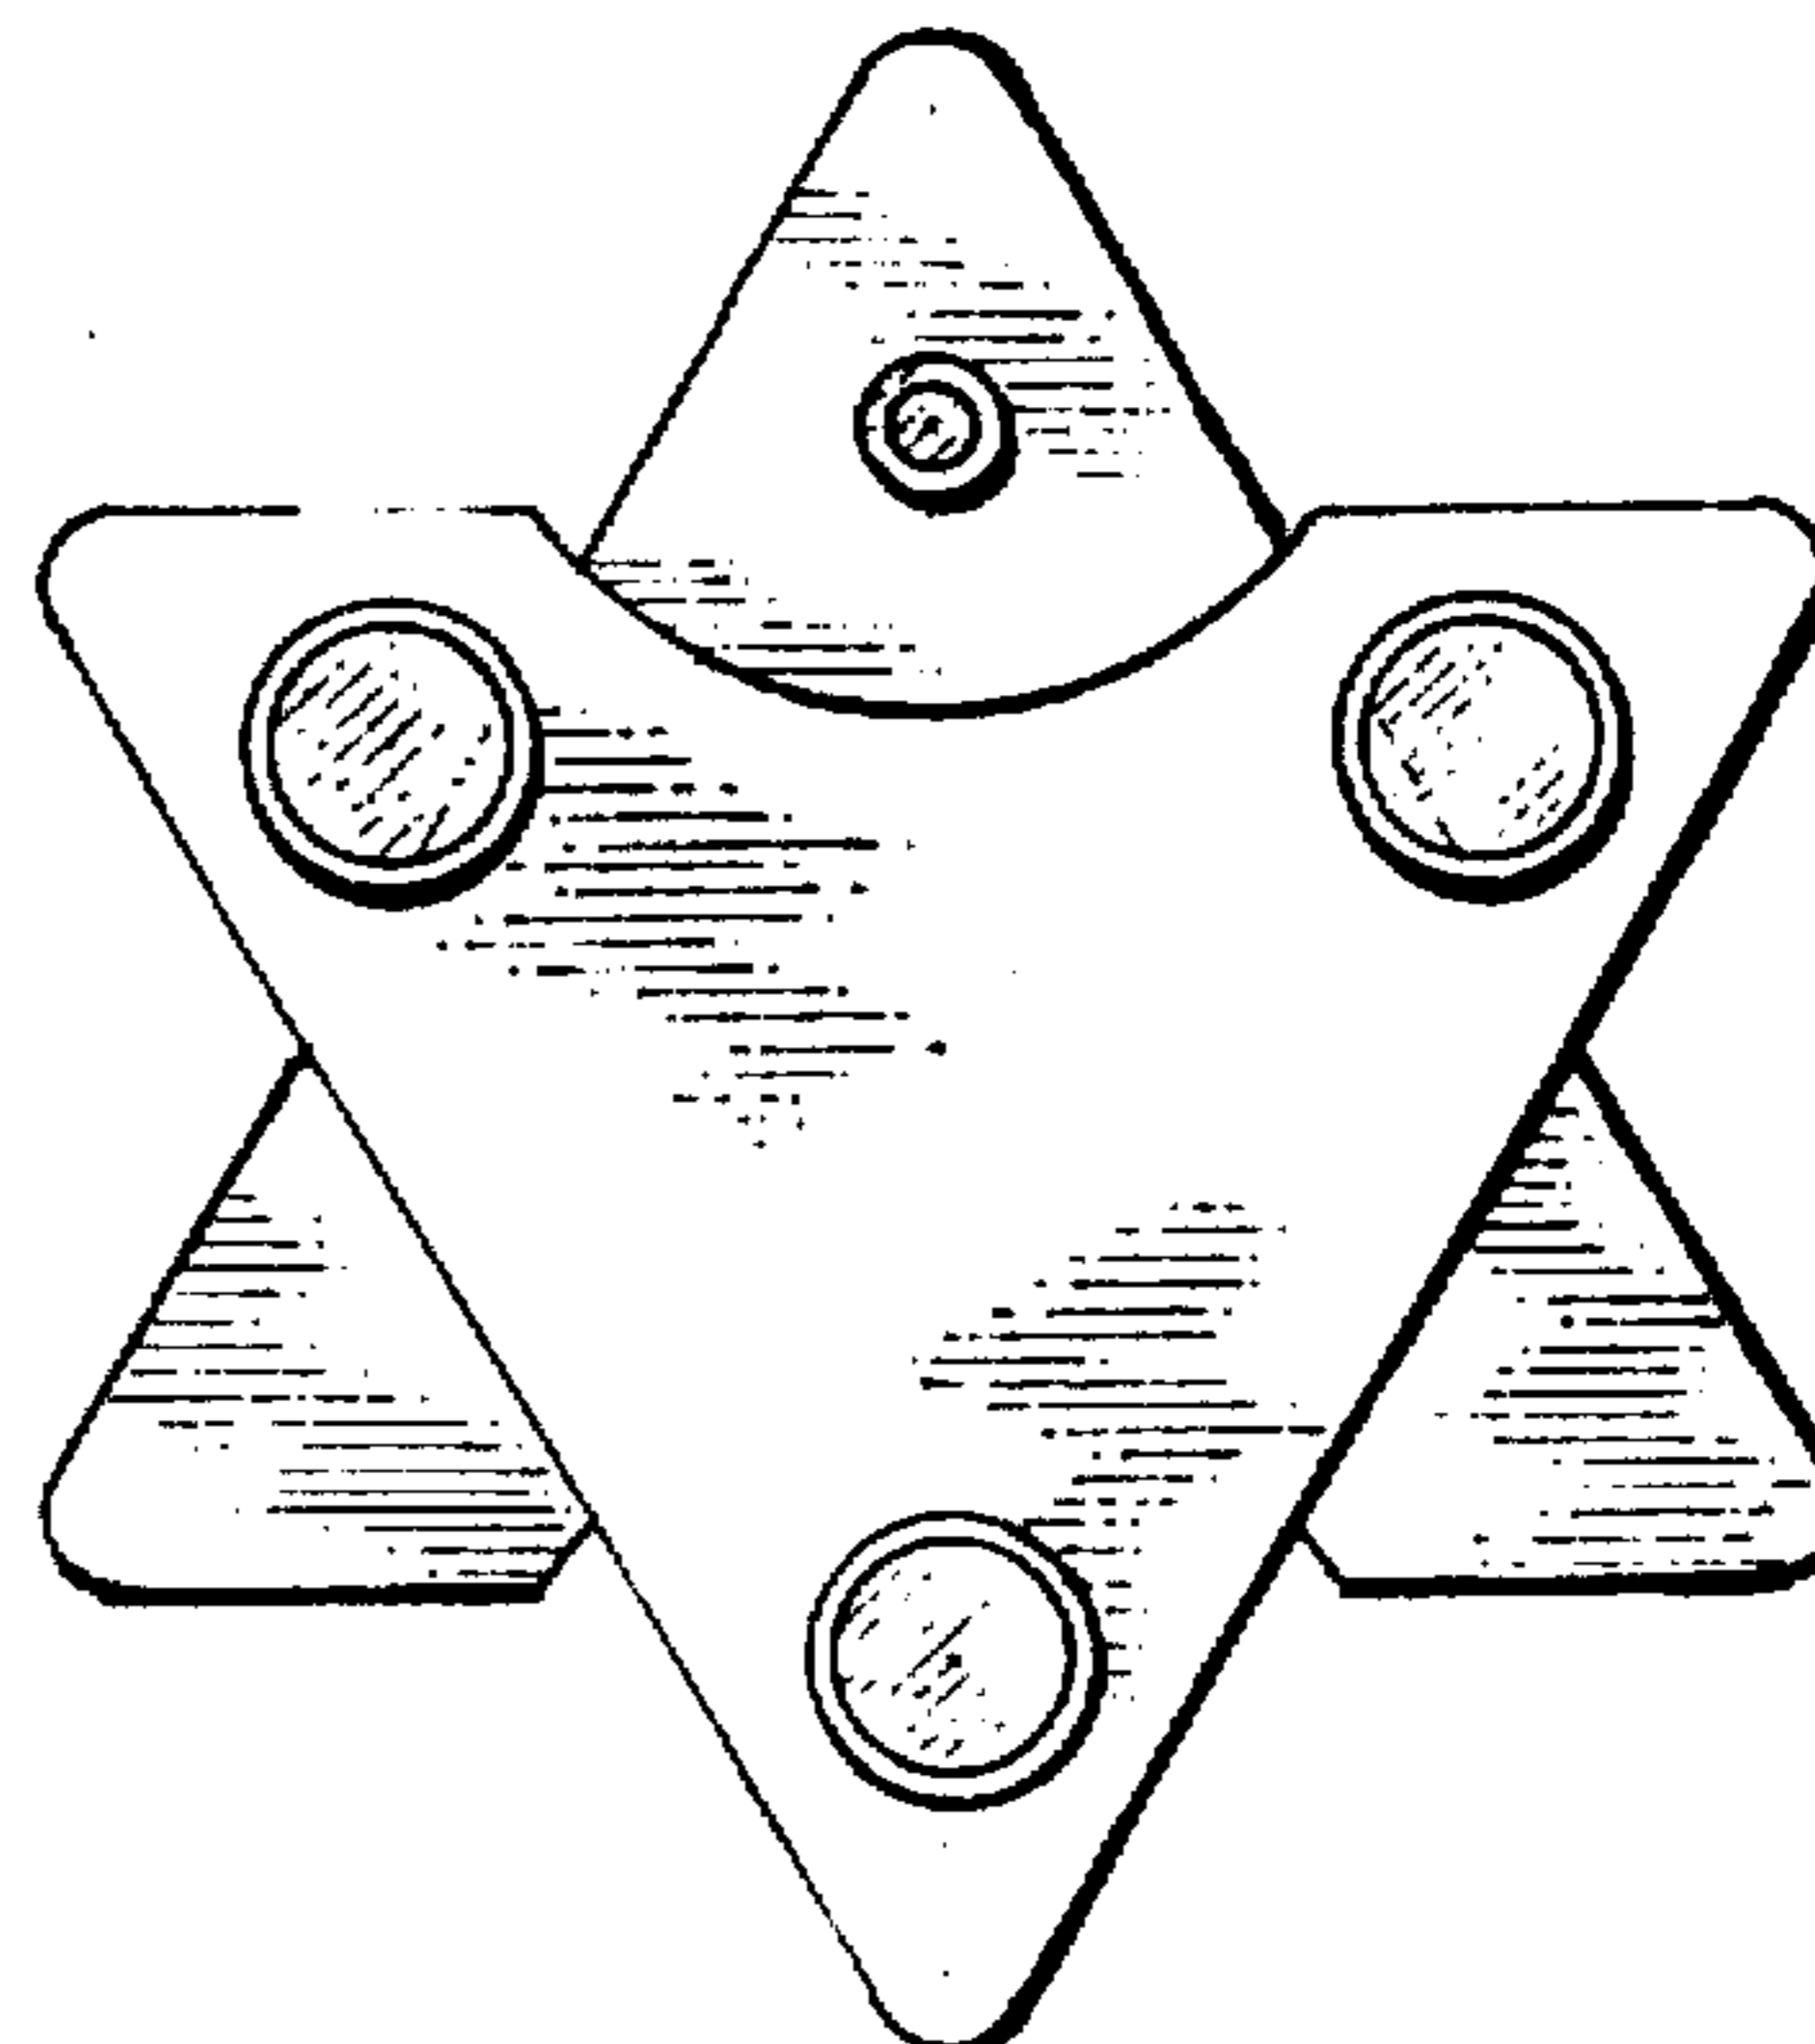


FIG. 7



FIG. 8

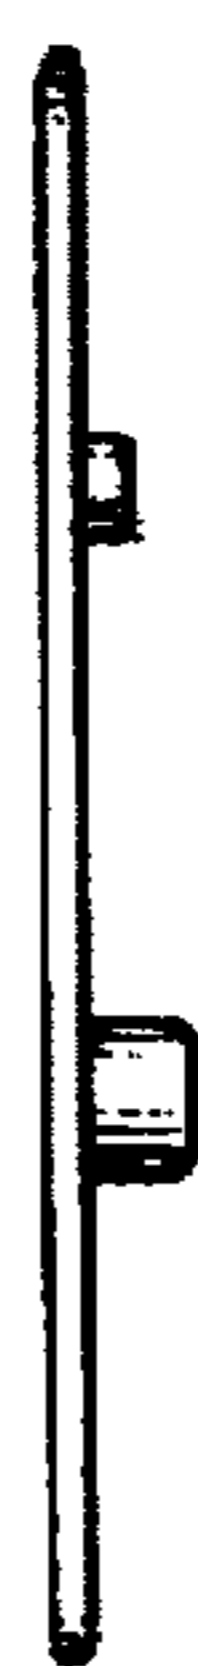


FIG. 9



FIG. 10