



US00D391838S

# United States Patent [19]

Bidwell et al.

[11] Patent Number: **Des. 391,838**

[45] Date of Patent: **\*\*Mar. 10, 1998**

## [54] FITTED ULTRASOUND TRANSDUCER PROBE HOLDER

[75] Inventors: **Dean J. Bidwell; Stephen B. Hooper**, both of Redmond; **Andrew L. Walston**, Seattle; **Peter Wung**, Redmond; **Matthew F. Willkens**, Seattle, all of Wash.

[73] Assignee: **Siemens Medical Systems, Inc.**, Iselin, N.J.

[\*\*] Term: **14 Years**

[21] Appl. No.: **64,487**

[22] Filed: **Jan. 2, 1997**

### Related U.S. Application Data

[63] Continuation of Ser. No. 44,761, Sep. 29, 1995, abandoned.

[51] LOC (6) Cl. .... **08-05**

[52] U.S. Cl. .... **D8/356**

[58] Field of Search ..... **D8/356; 16/2; 248/56; 174/153 G; 600/102**

## [56] References Cited

### U.S. PATENT DOCUMENTS

D. 324,488	3/1992	Fujimoto .....	D8/354
3,788,582	1/1974	Swanquist .....	248/56
4,640,479	2/1987	Shely et al. ....	D8/356 X
4,730,363	3/1988	Asbaghi .....	248/56 X
5,167,047	12/1992	Plumley .....	D8/356 X

*Primary Examiner*—Holly Baynham


## [57] CLAIM

The ornamental design for the fitted ultrasound transducer probe holder, as shown.

## DESCRIPTION

FIG. 1 is a perspective view of a fitted ultrasound transducer probe holder embodiment of this invention; FIG. 2 is an opposite side perspective view; FIG. 3 is a bottom, opposite side perspective view; FIG. 4 is a top view; FIG. 5 is a side view; and, FIG. 6 is a side view turned 90 degrees.

**1 Claim, 2 Drawing Sheets**

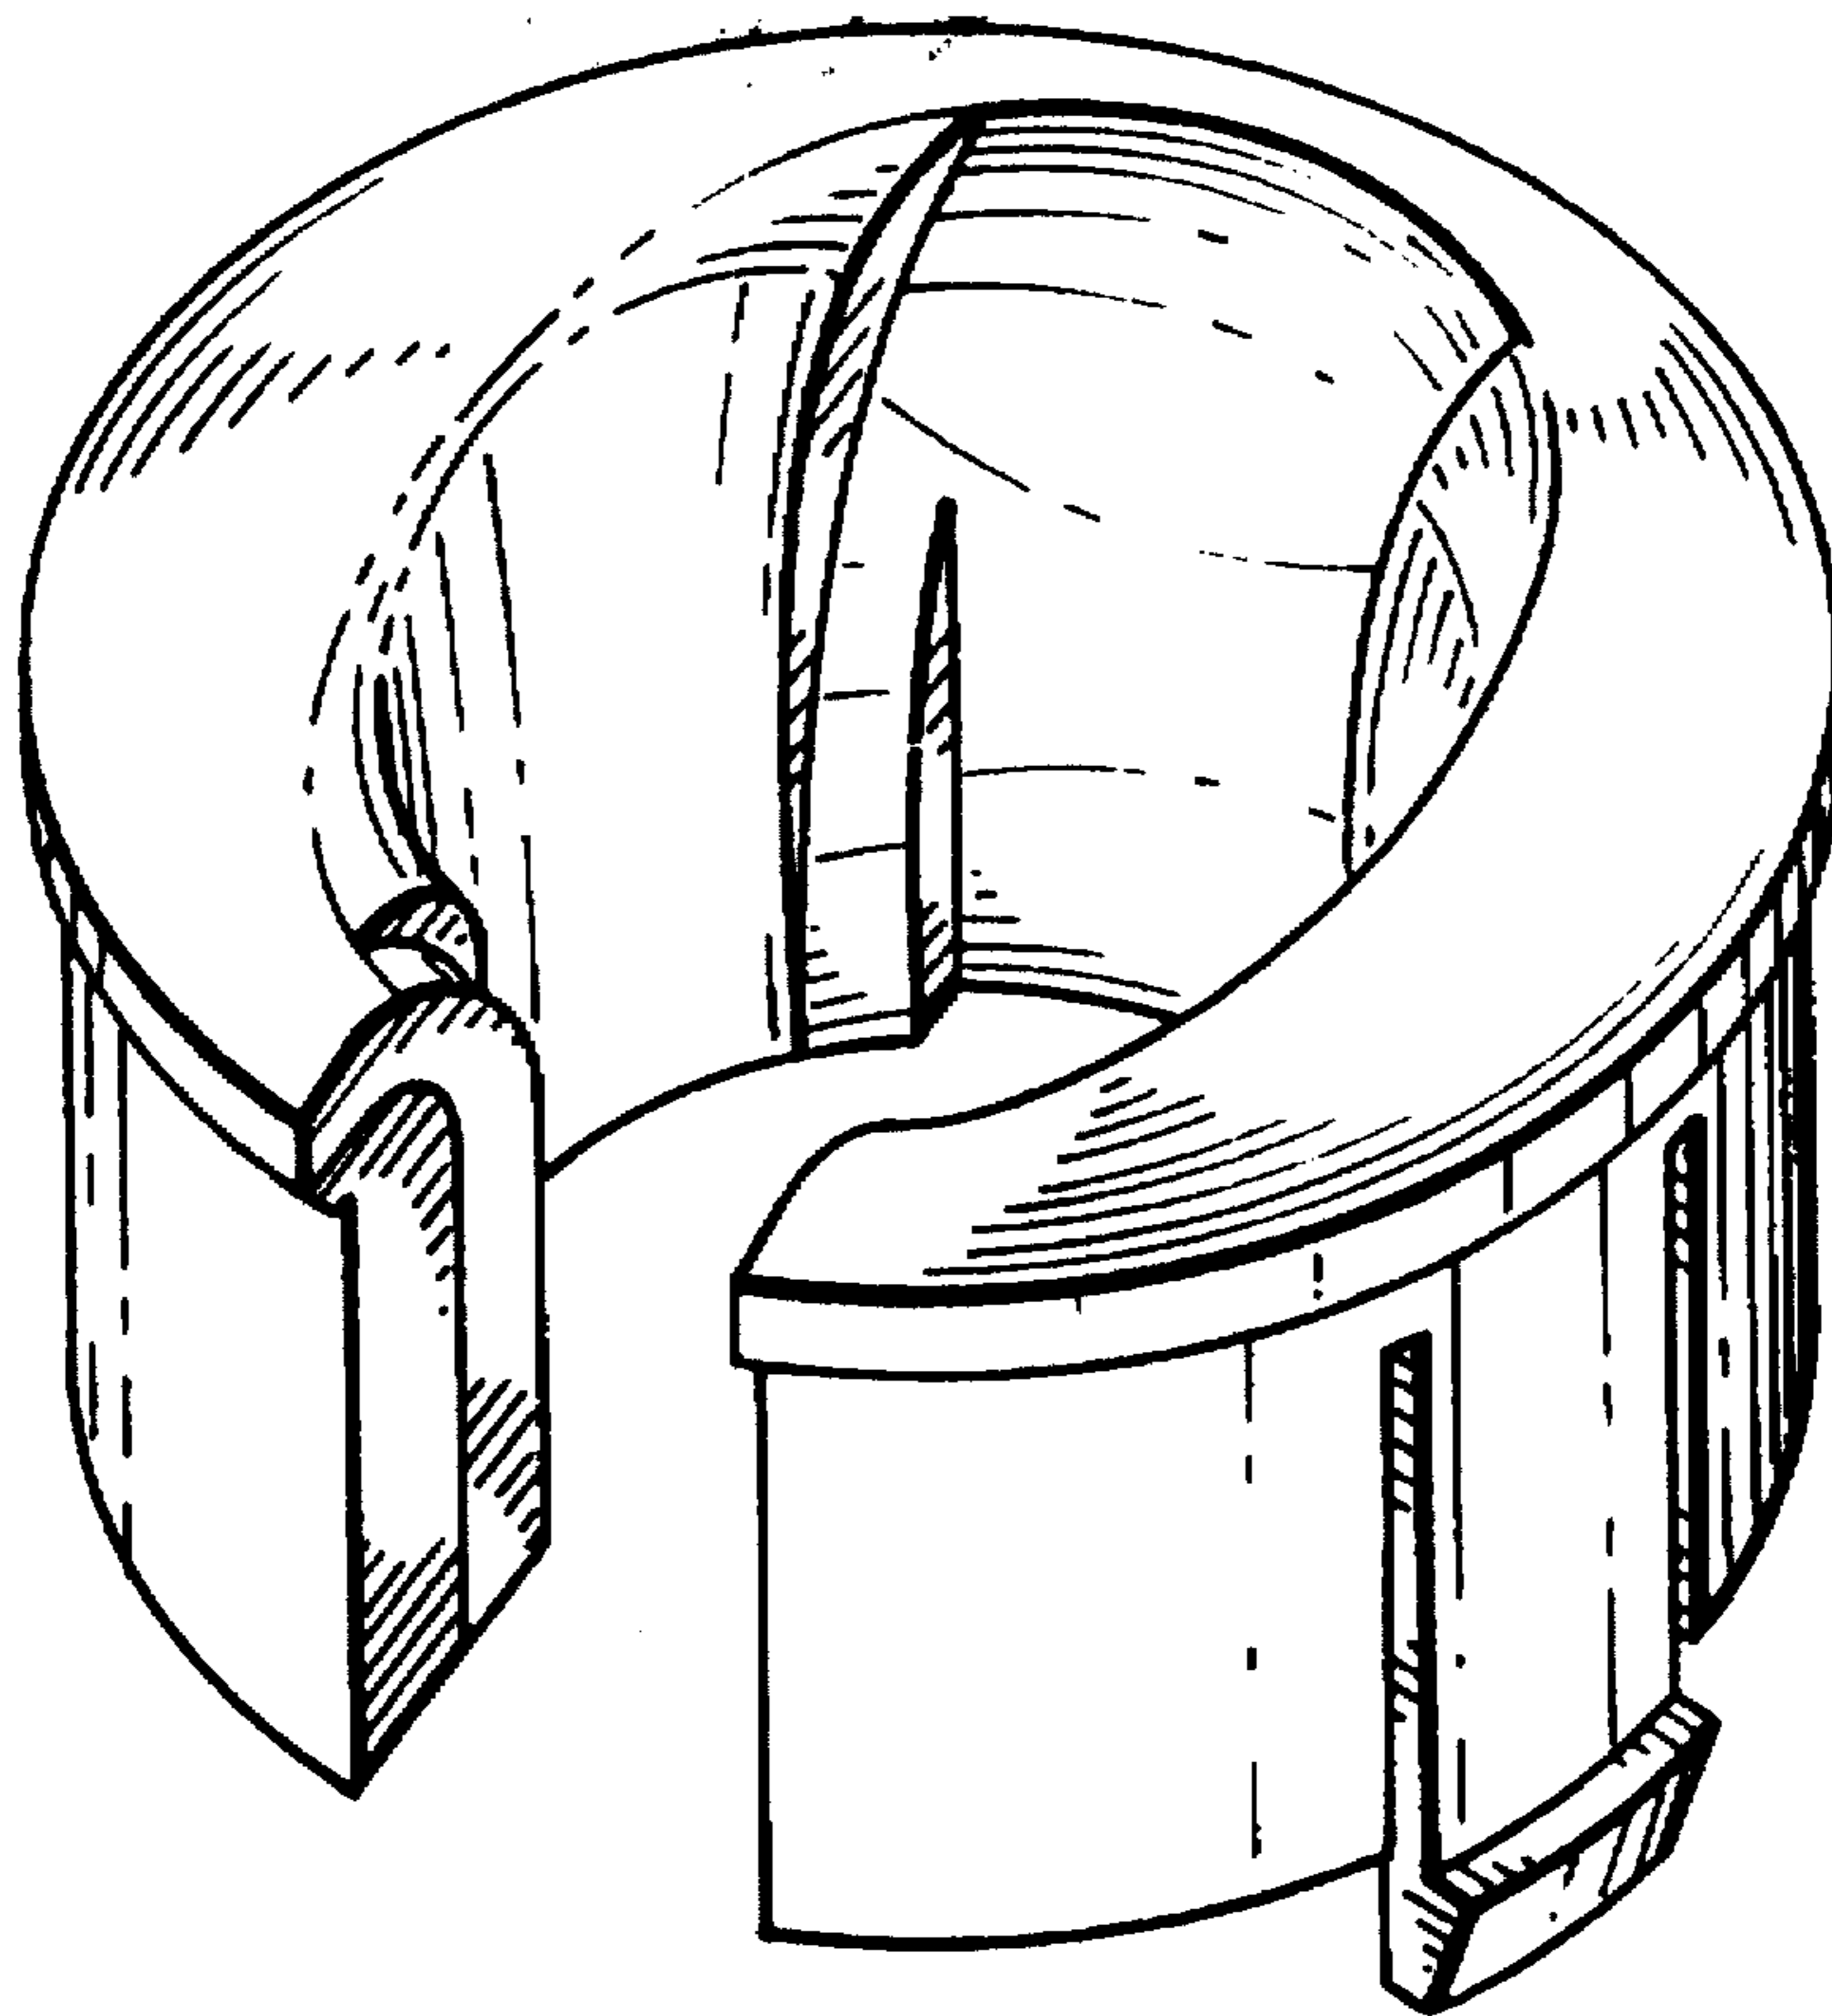

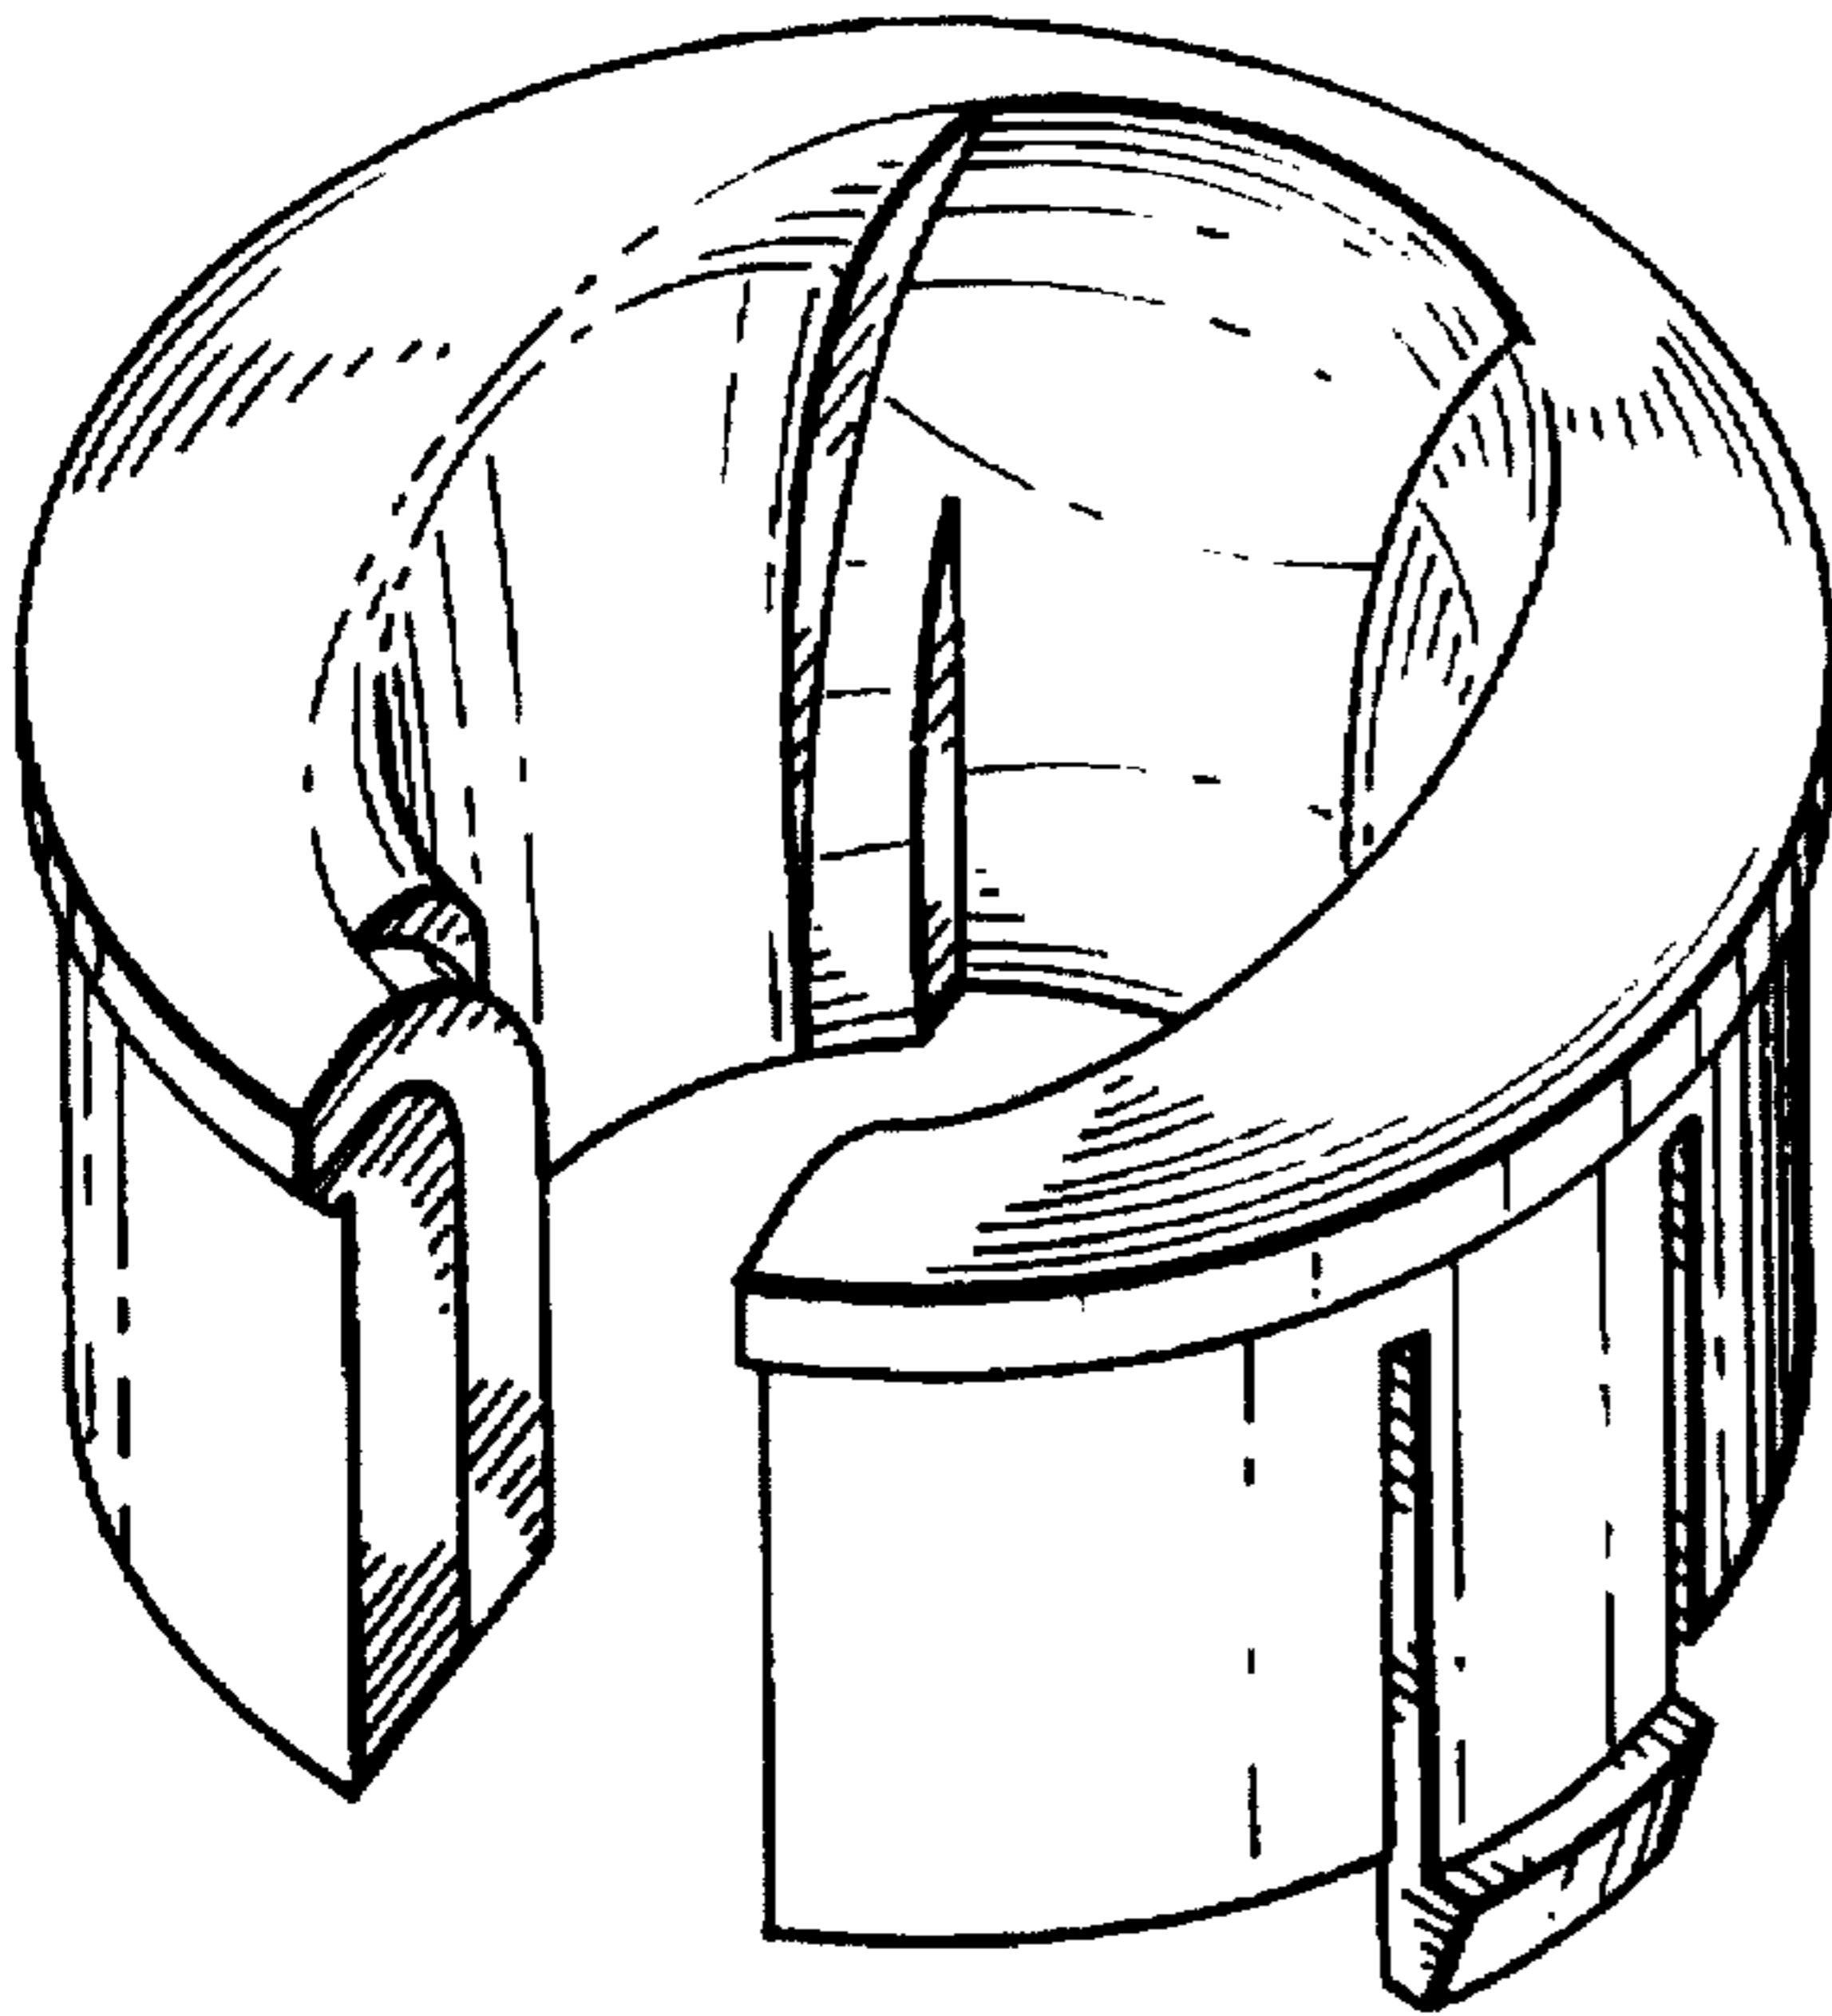


FIG. 1

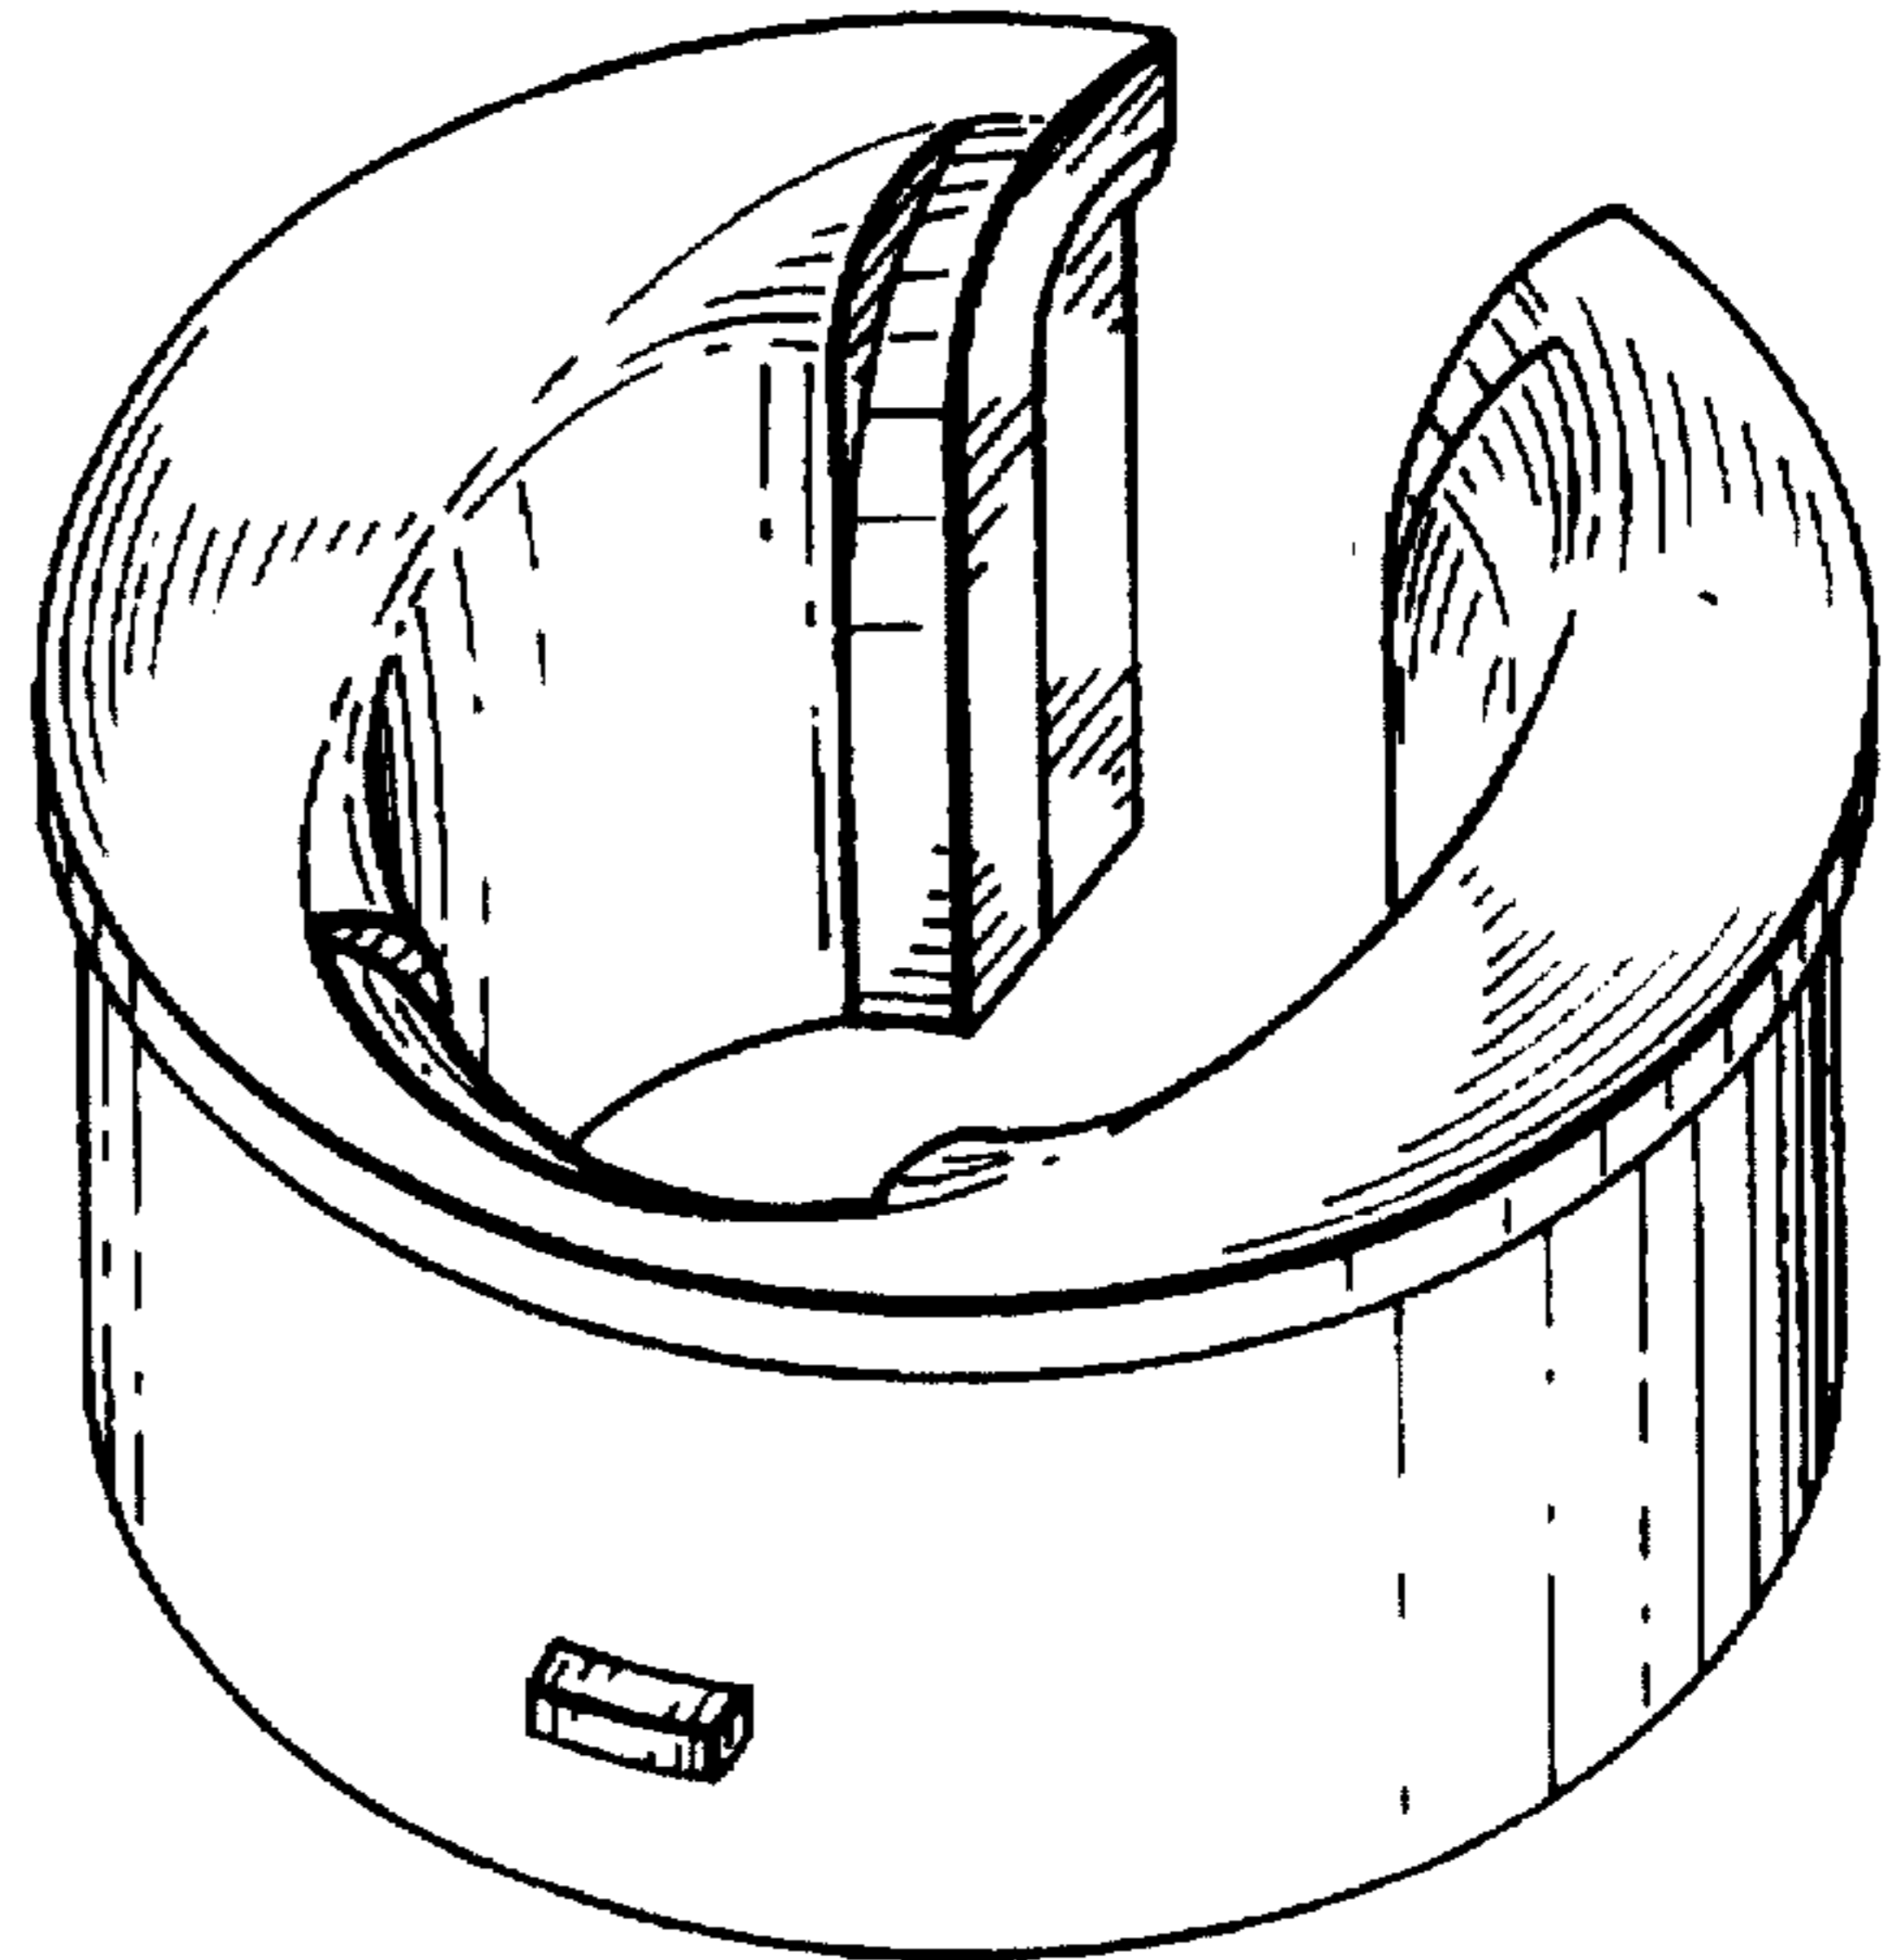


FIG. 2

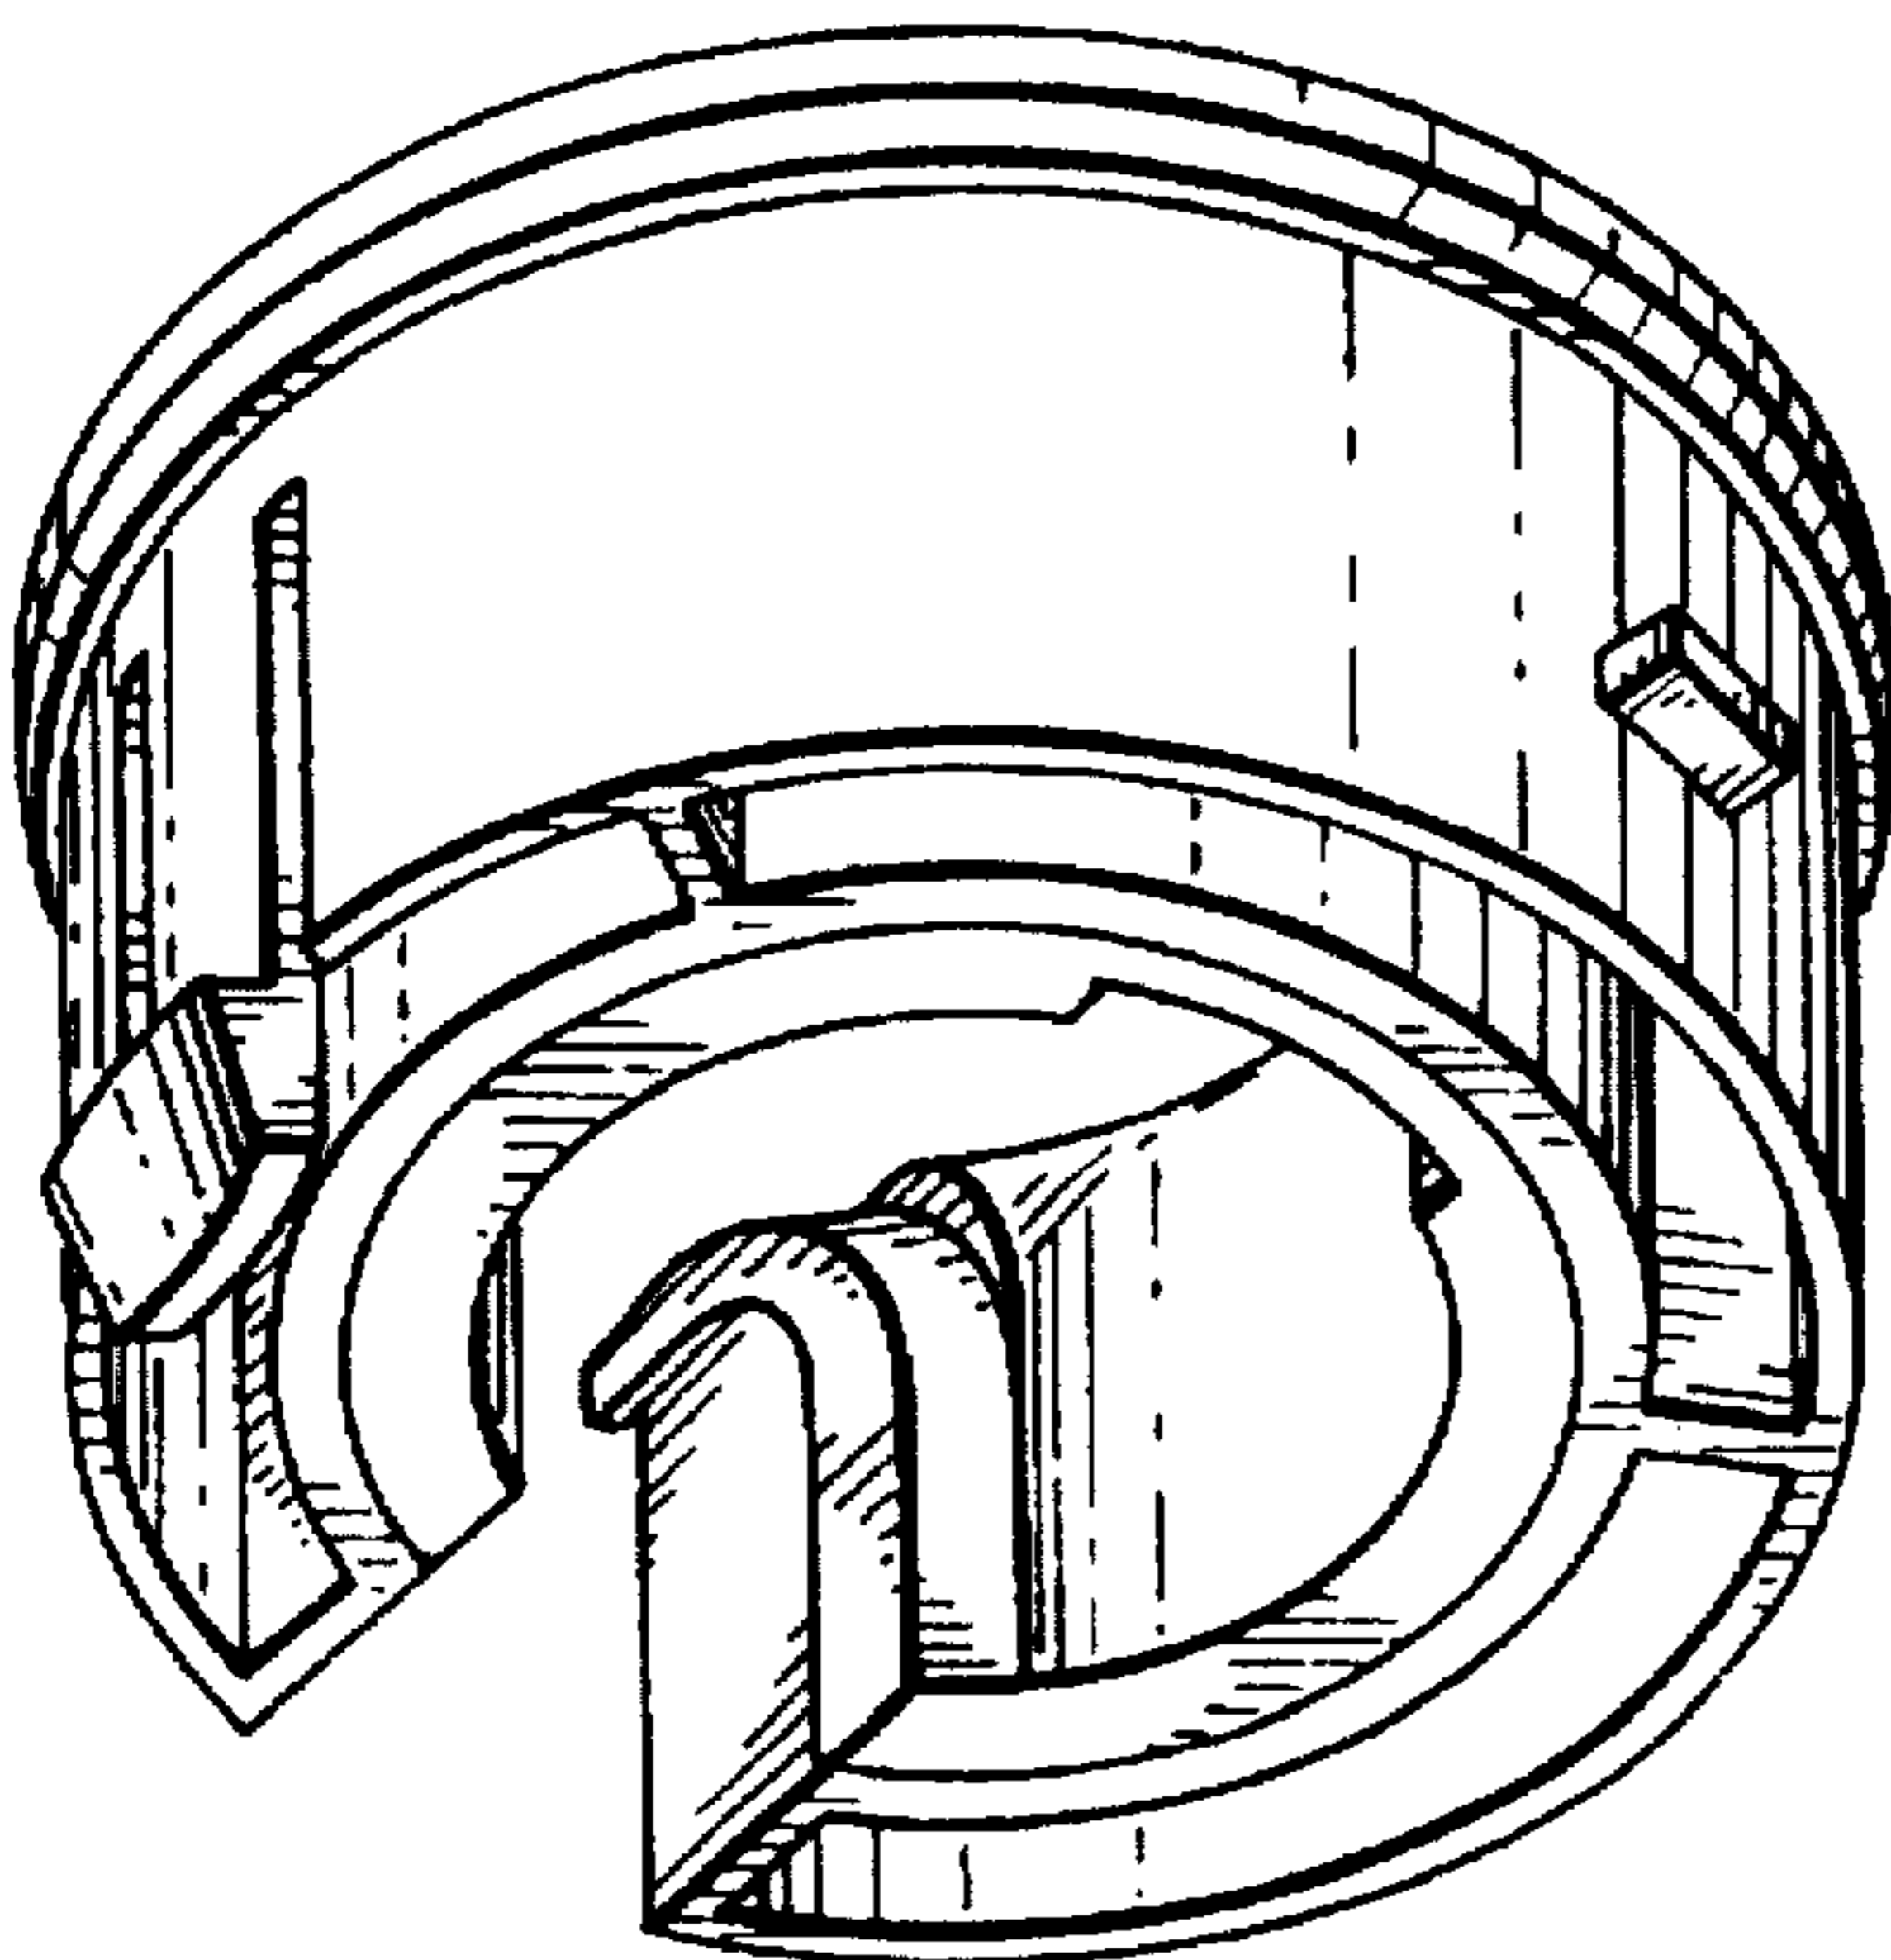


FIG. 3

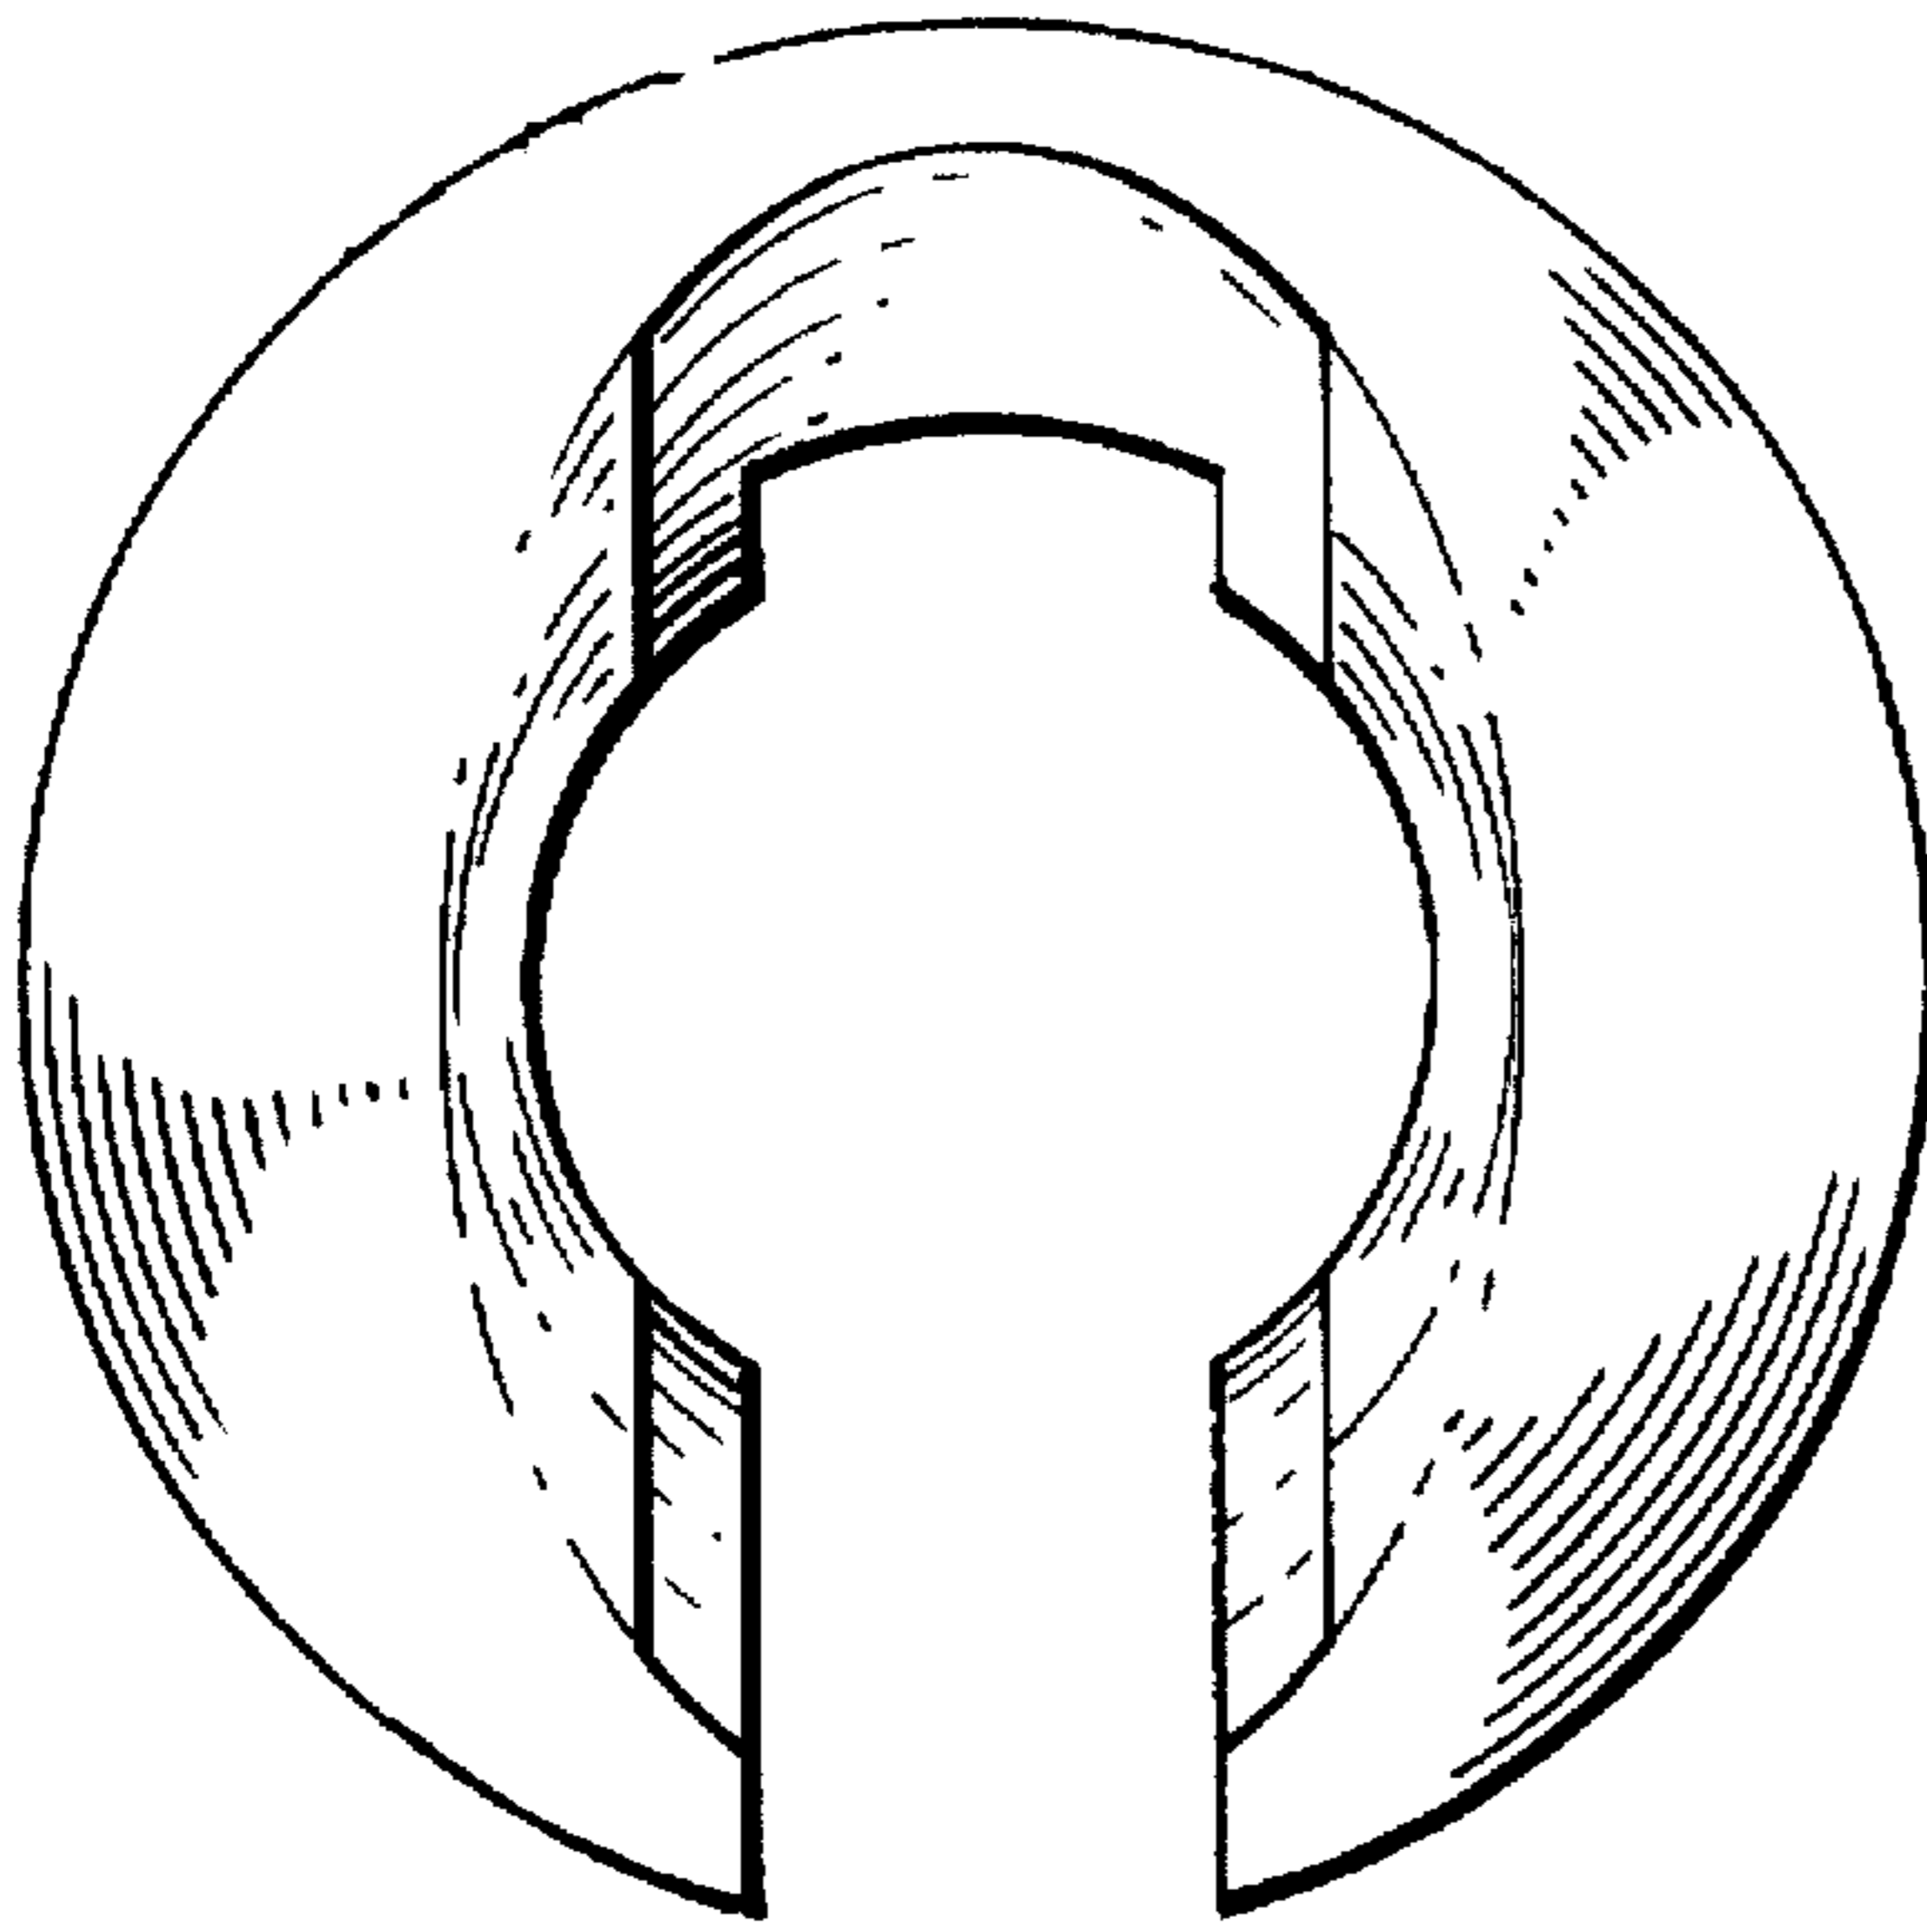


FIG. 4

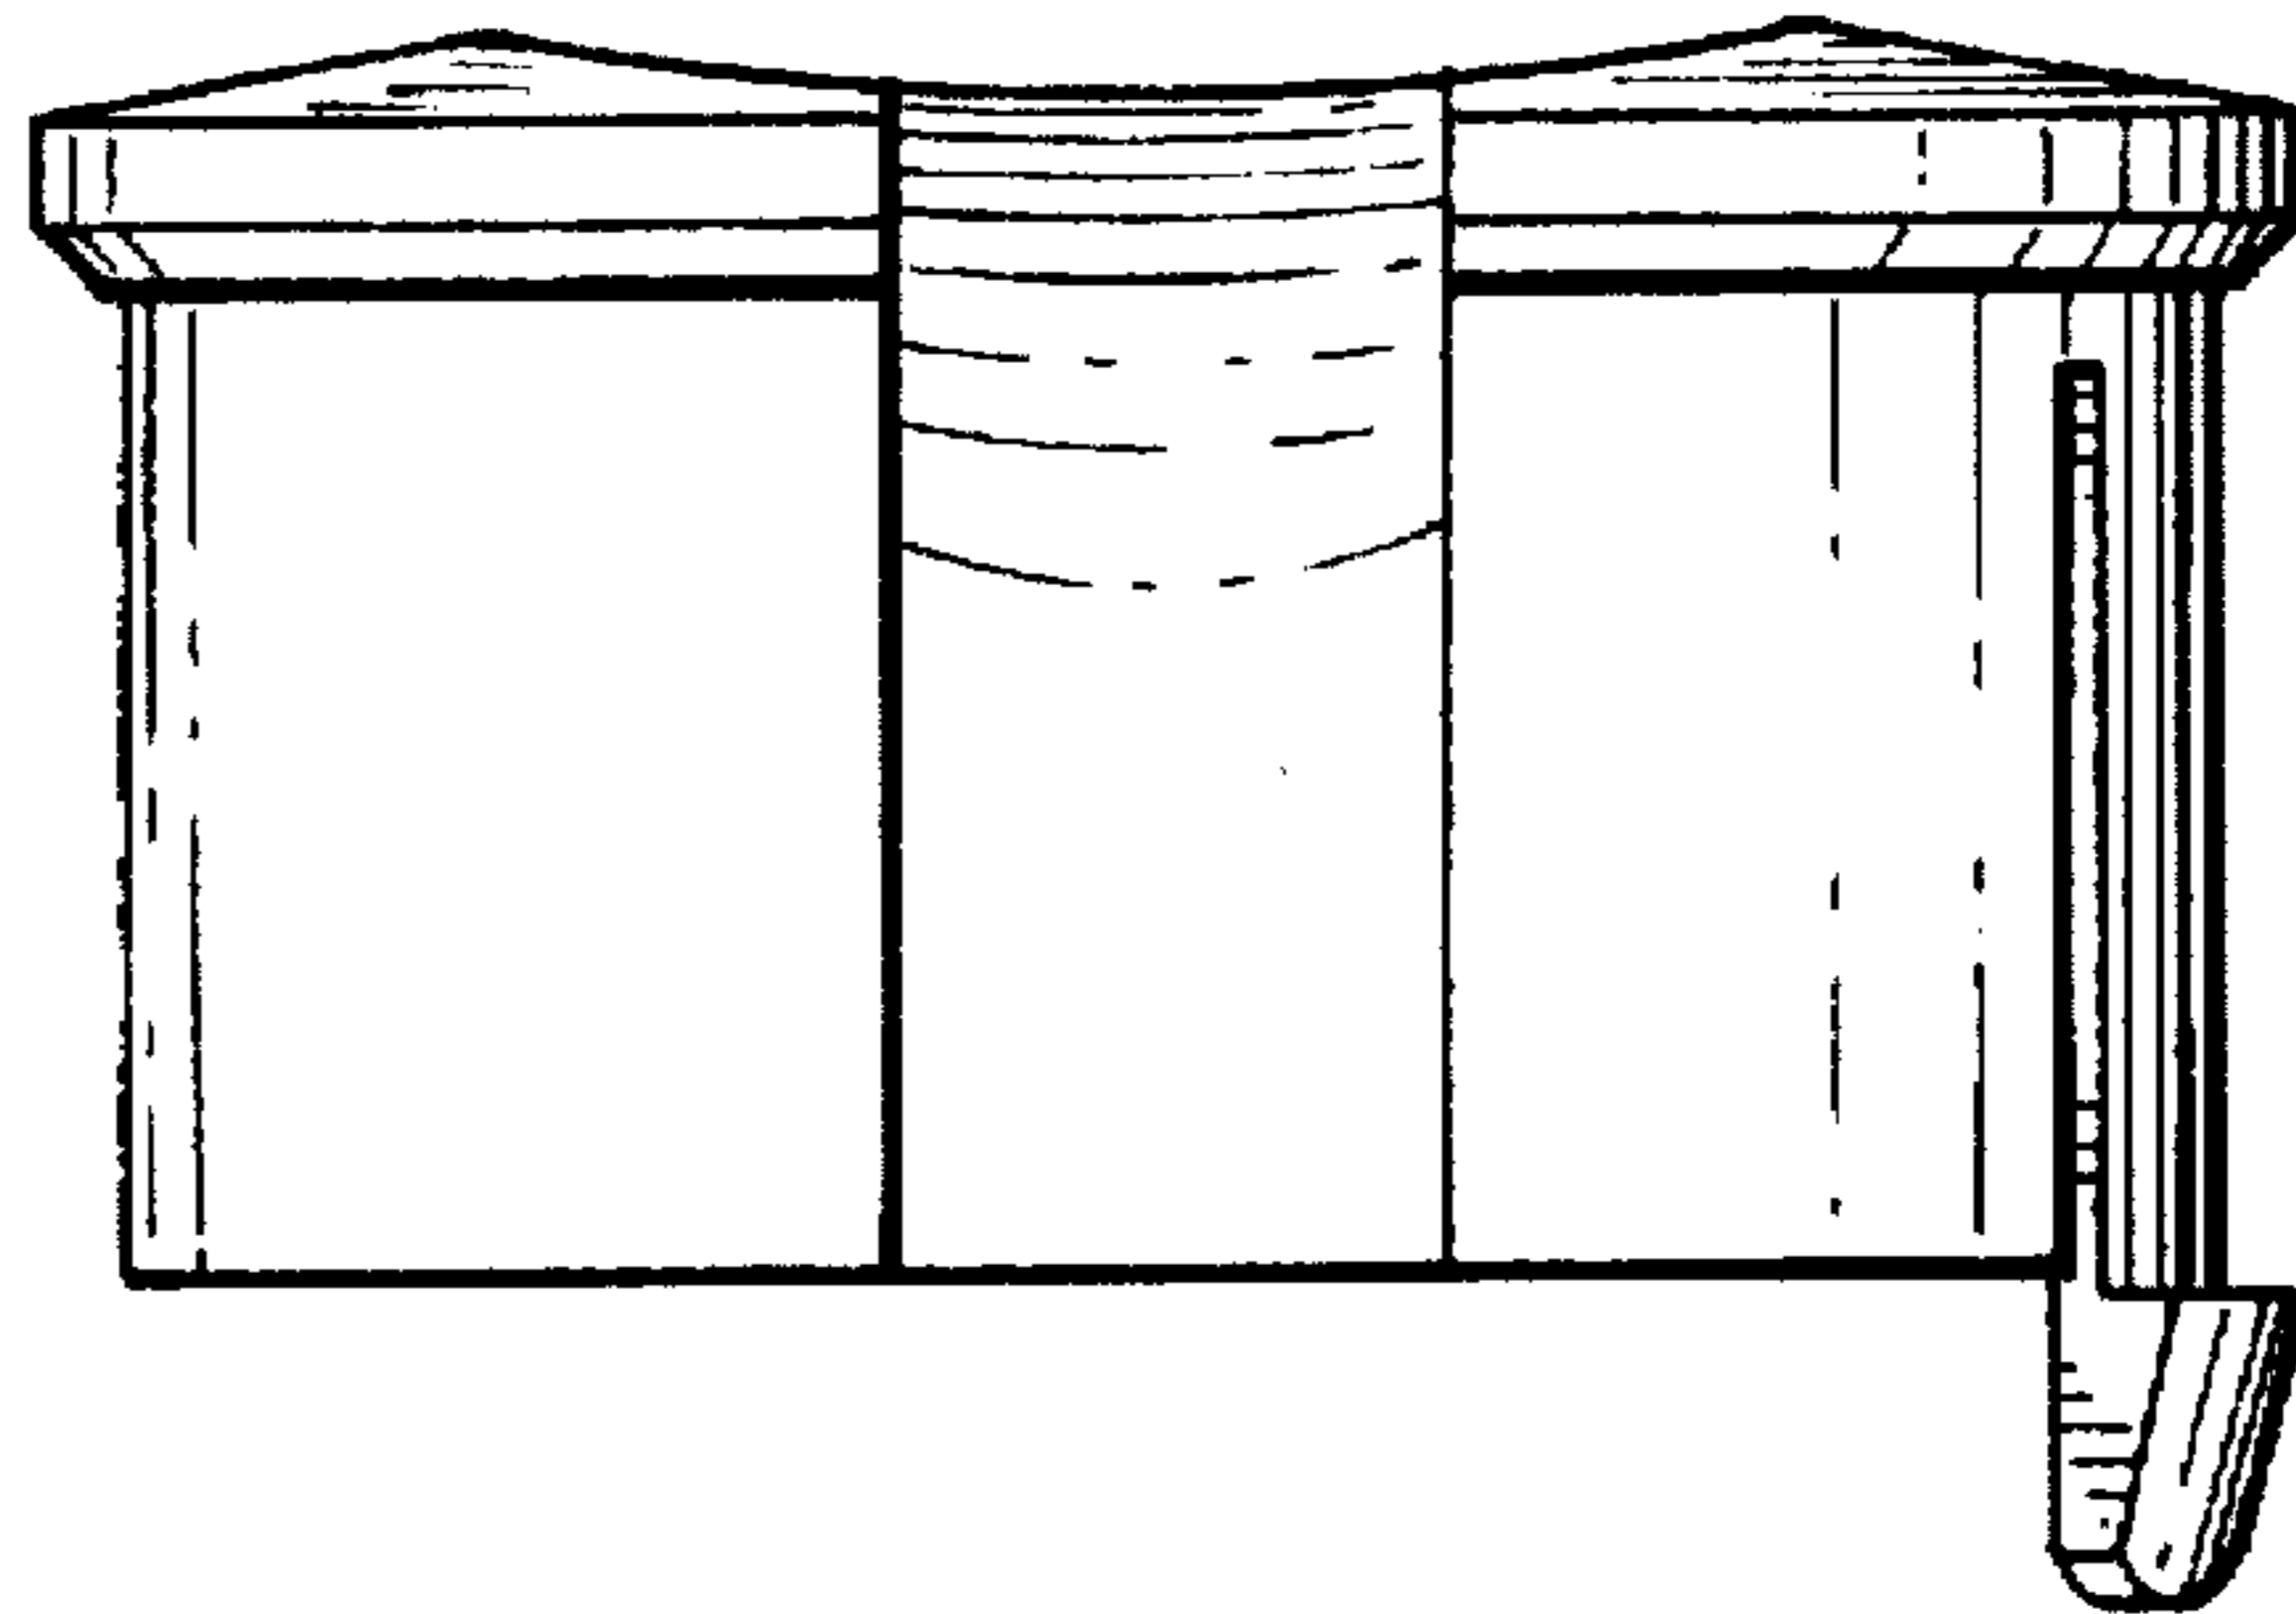


FIG. 5

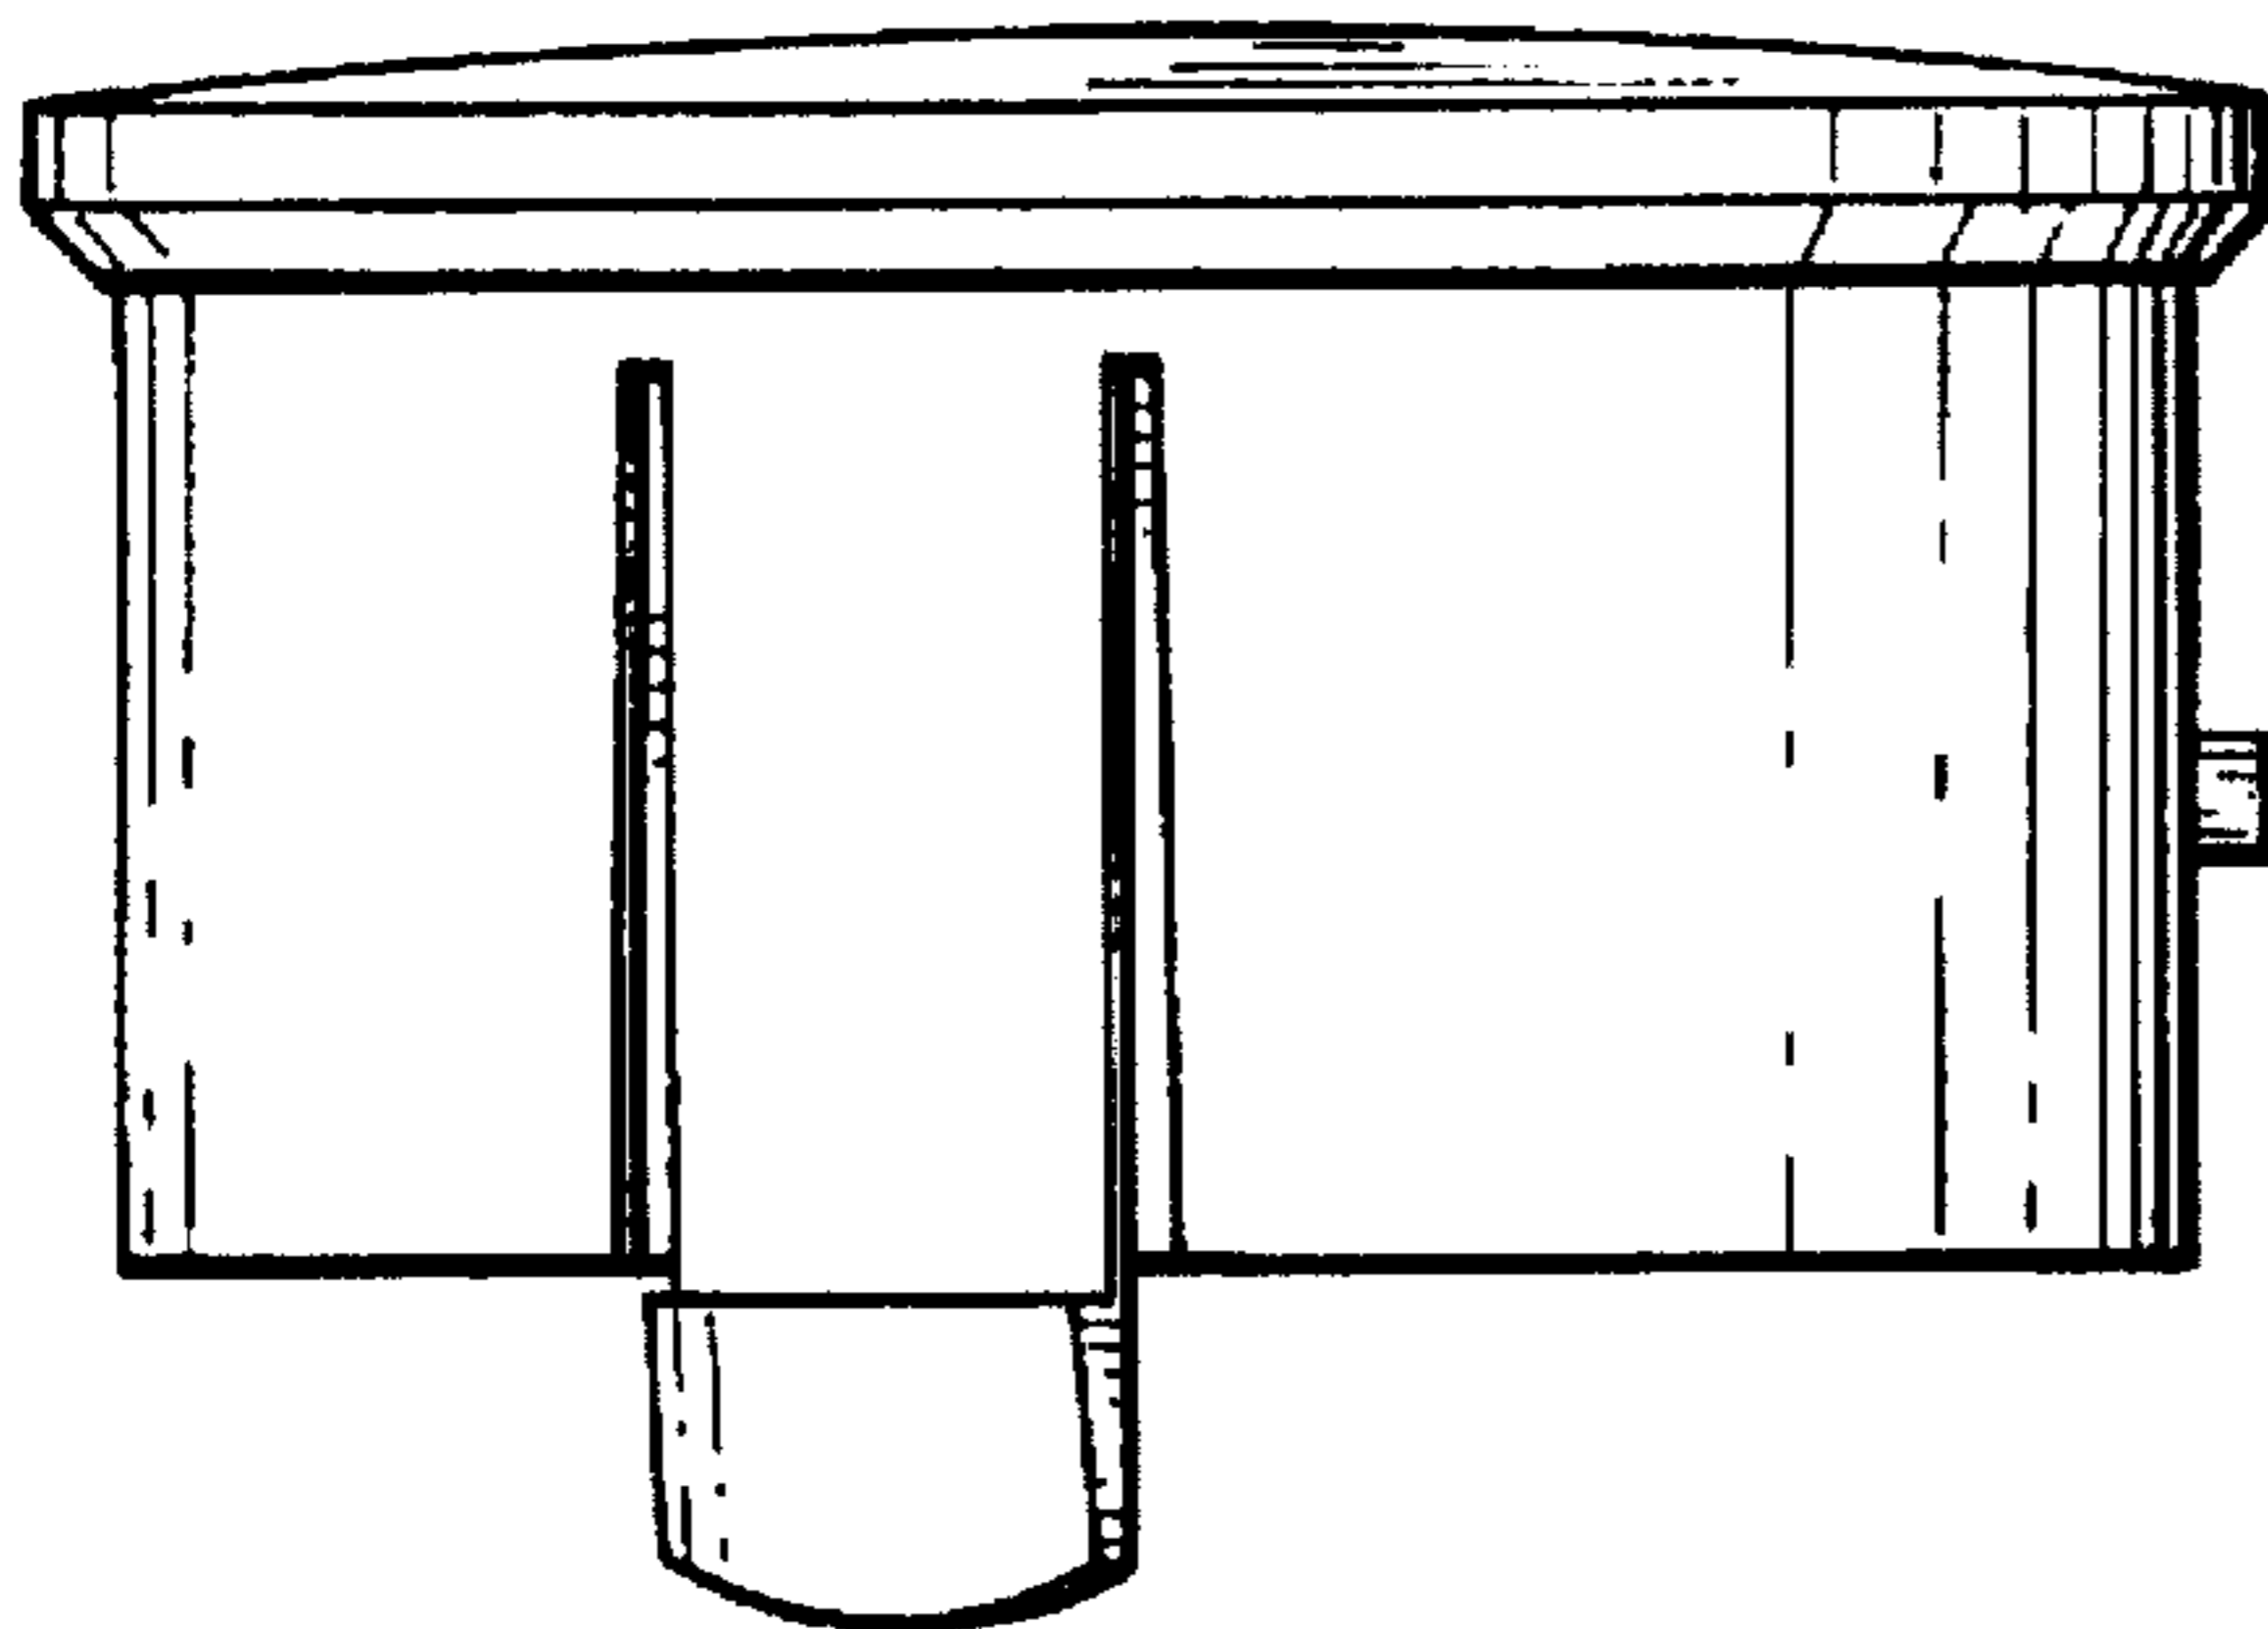


FIG. 6