



US00D397044S

United States Patent [19]

[11] Patent Number: **Des. 397,044**

Lee

[45] Date of Patent: ****Aug. 18, 1998**

[54] **TEMPLATE FOR ENSURING ACCURATE PATIENT POSITIONING FOR UPRIGHT X-RAY EXAMINATIONS**

1,668,396 5/1928 Carroll 33/564

Primary Examiner—Antoine Duval Davis
Attorney, Agent, or Firm—James F. Cottone

[76] Inventor: **Aaron T. Lee**, 25 Castle Dr., Stillwater, N.Y. 12170

[57] **CLAIM**

[**] Term: **14 Years**

The ornamental design for a template for ensuring accurate patient positioning for upright X-ray examinations, as shown and described.

[21] Appl. No.: **78,012**

DESCRIPTION

[22] Filed: **Oct. 15, 1997**

[51] LOC (6) Cl. **10-04**

[52] U.S. Cl. **D10/64**

[58] Field of Search D10/64, 65; 33/511, 33/512, 562, 563, 564, 565


FIG. 1 is a top plan view of my template for ensuring accurate patient positioning for upright X-ray examinations showing my new design, the bottom plan view being a mirror image;
FIG. 2 is an end elevational view thereof, the opposite end elevational view being a mirror image; and,
FIG. 3 is a side elevational view thereof, the opposite end elevational view being a mirror image.

[56] **References Cited**

U.S. PATENT DOCUMENTS

D. 141,691 6/1945 Miller D10/64

1 Claim, 1 Drawing Sheet

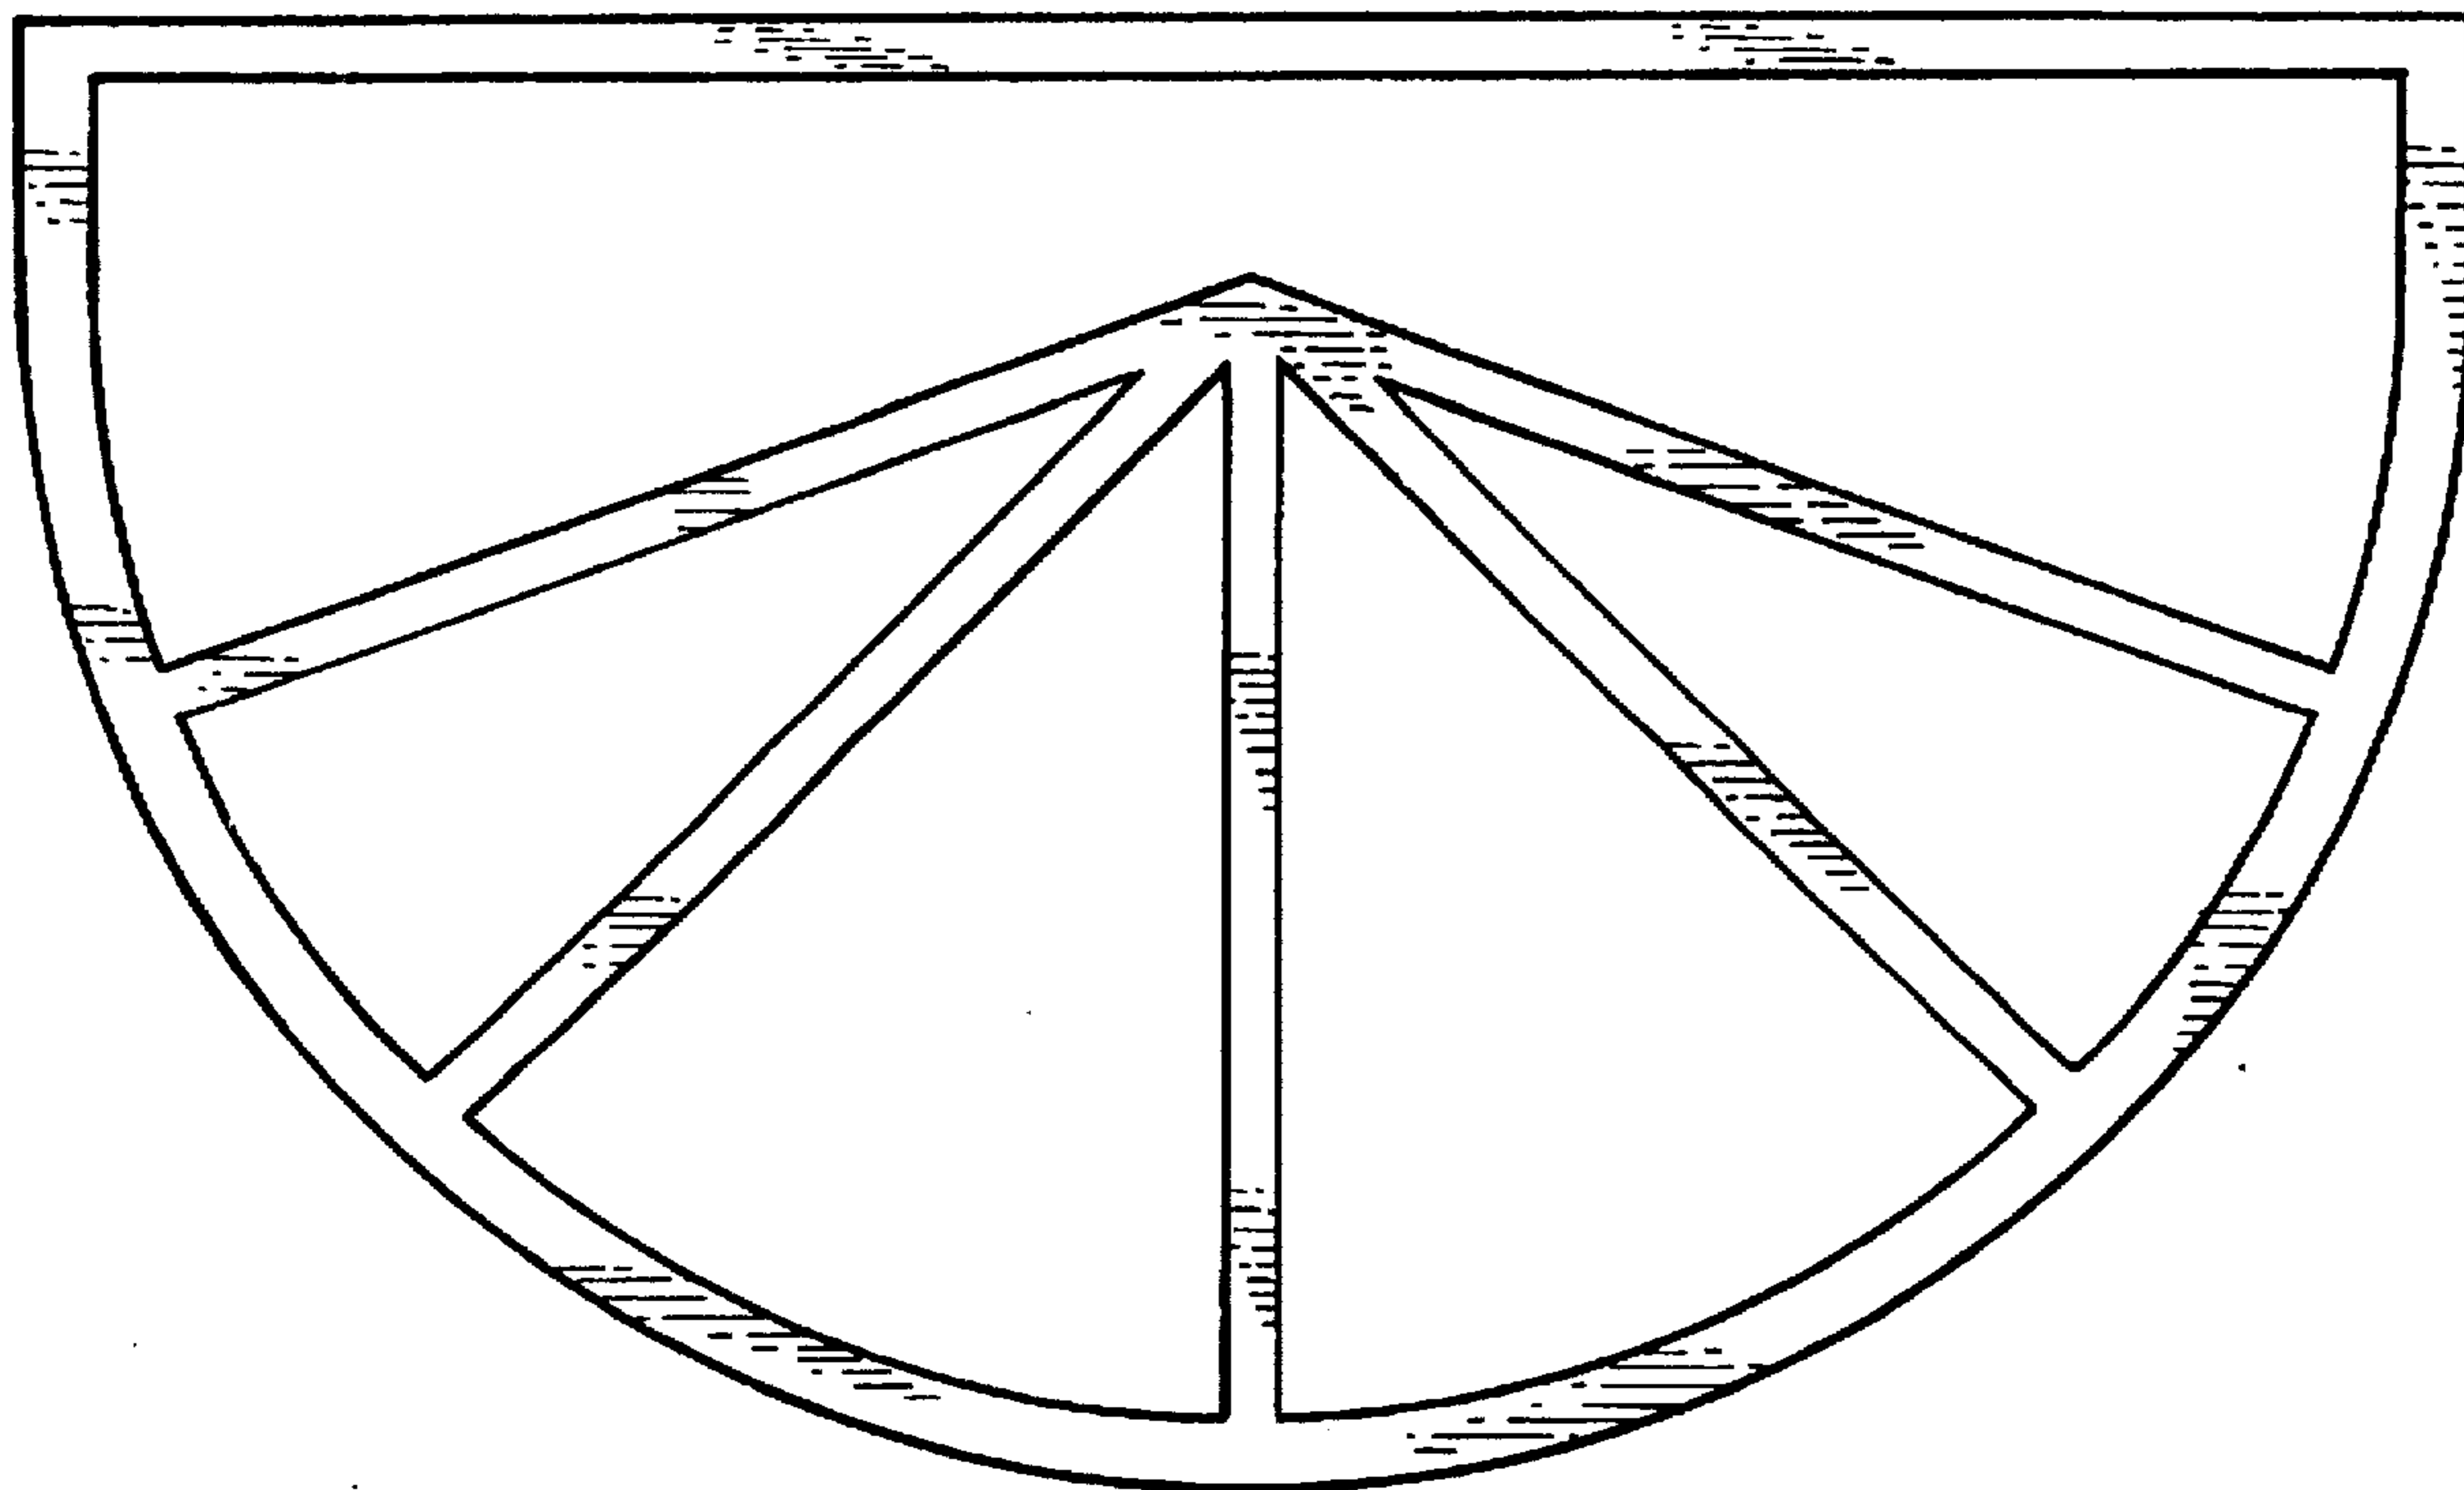

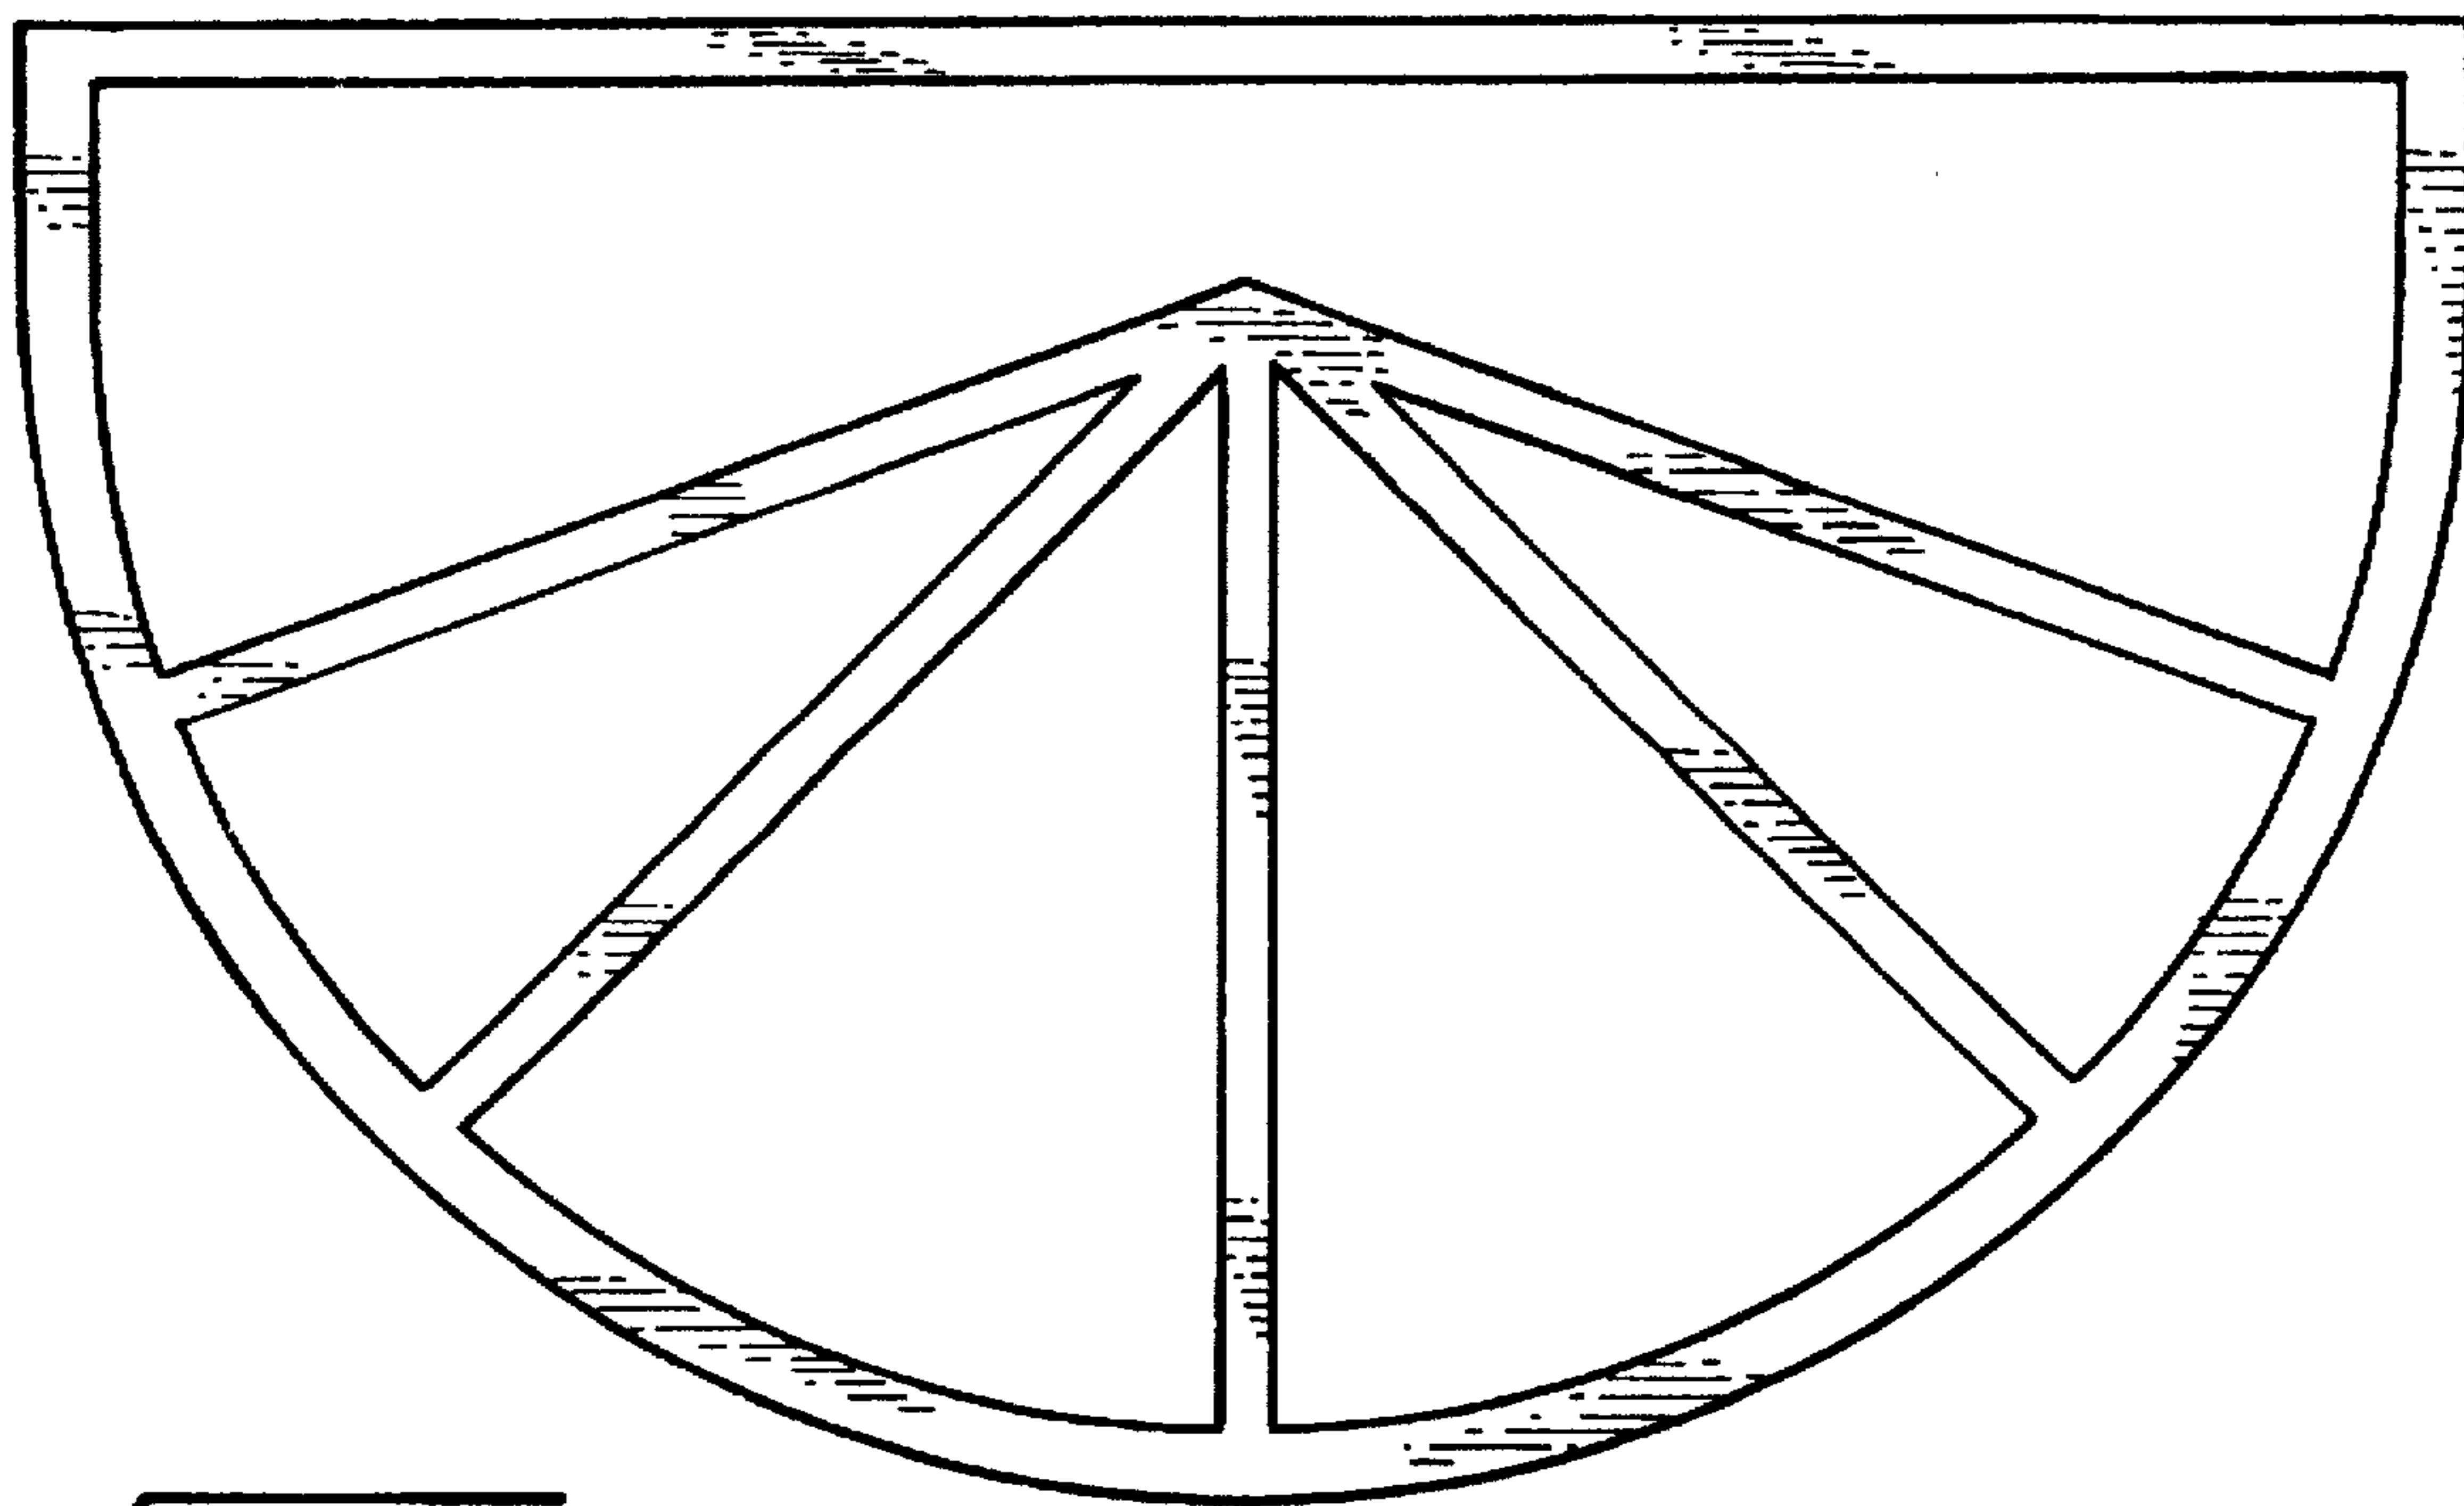


FIG. 1




FIG. 2



FIG. 3