



US00D397440S

United States Patent [19]

Baars

[11] Patent Number: **Des. 397,440**

[45] Date of Patent: ****Aug. 25, 1998**

[54] **SURGICAL X-RAY APPARATUS**

[75] Inventor: **Jan Erik Baars**, Eindhoven, Netherlands

[73] Assignee: **U.S. Philips Corporation**, New York, N.Y.

[**] Term: **14 Years**

[21] Appl. No.: **64,262**

[22] Filed: **Nov. 22, 1996**

[30] **Foreign Application Priority Data**

May 23, 1996 [WO] WIPO DMA/003334

[51] LOC (6) Cl. **24-01**

[52] U.S. Cl. **D24/158**

[58] Field of Search D24/158, 159; 378/198, 197

[56] **References Cited**

U.S. PATENT DOCUMENTS

D. 291,916 9/1987 Davis D24/158

3,070,695	12/1962	Stickney et al. .	
4,887,287	12/1989	Cobben	378/198
5,008,921	4/1991	Kaul et al.	378/198
5,642,395	6/1997	Anderton et al.	378/198

Primary Examiner—Stella Reid
Attorney, Agent, or Firm—Ernestine C. Bartlett


[57] CLAIM

The ornamental design for a surgical X-ray apparatus, as shown.

DESCRIPTION

FIG. 1 is a perspective view showing my new design; FIG. 2 is a front elevational view thereof; FIG. 3 is a rear elevational view thereof; FIG. 4 is a right side elevational view thereof; FIG. 5 is a left side elevational view thereof; FIG. 6 is a top plan view thereof; and, FIG. 7 is a bottom plan view thereof.

1 Claim, 7 Drawing Sheets

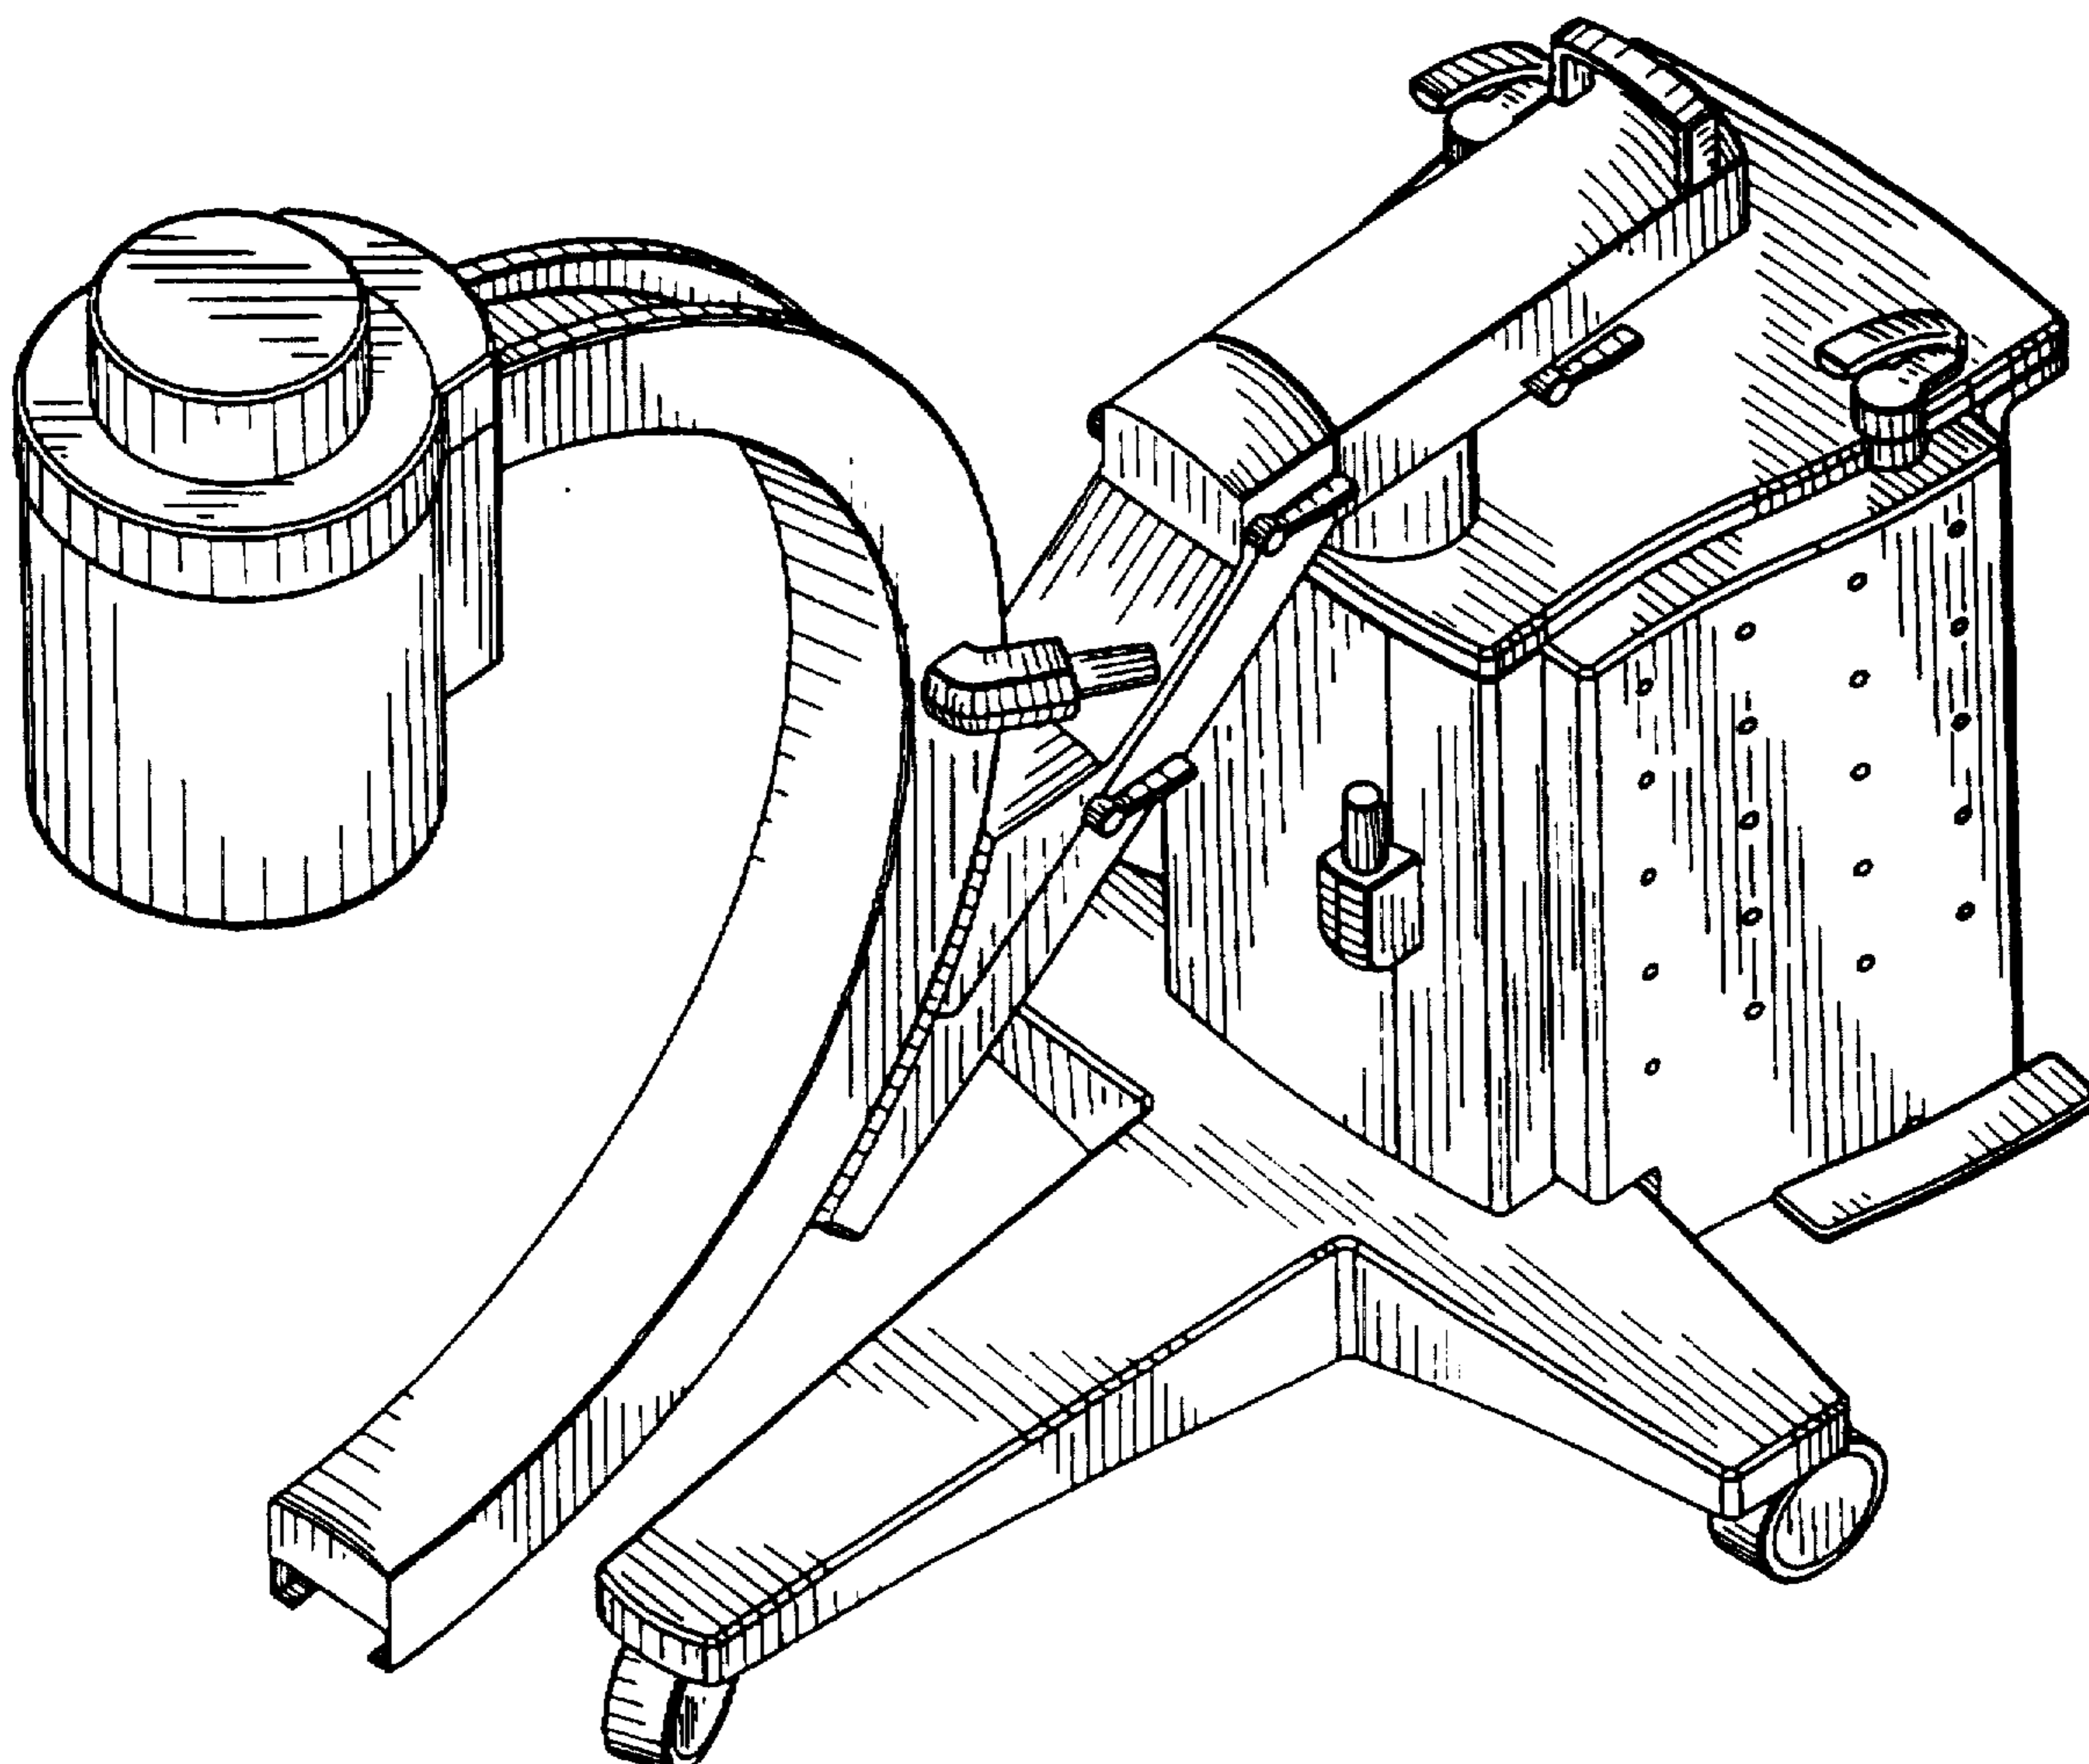

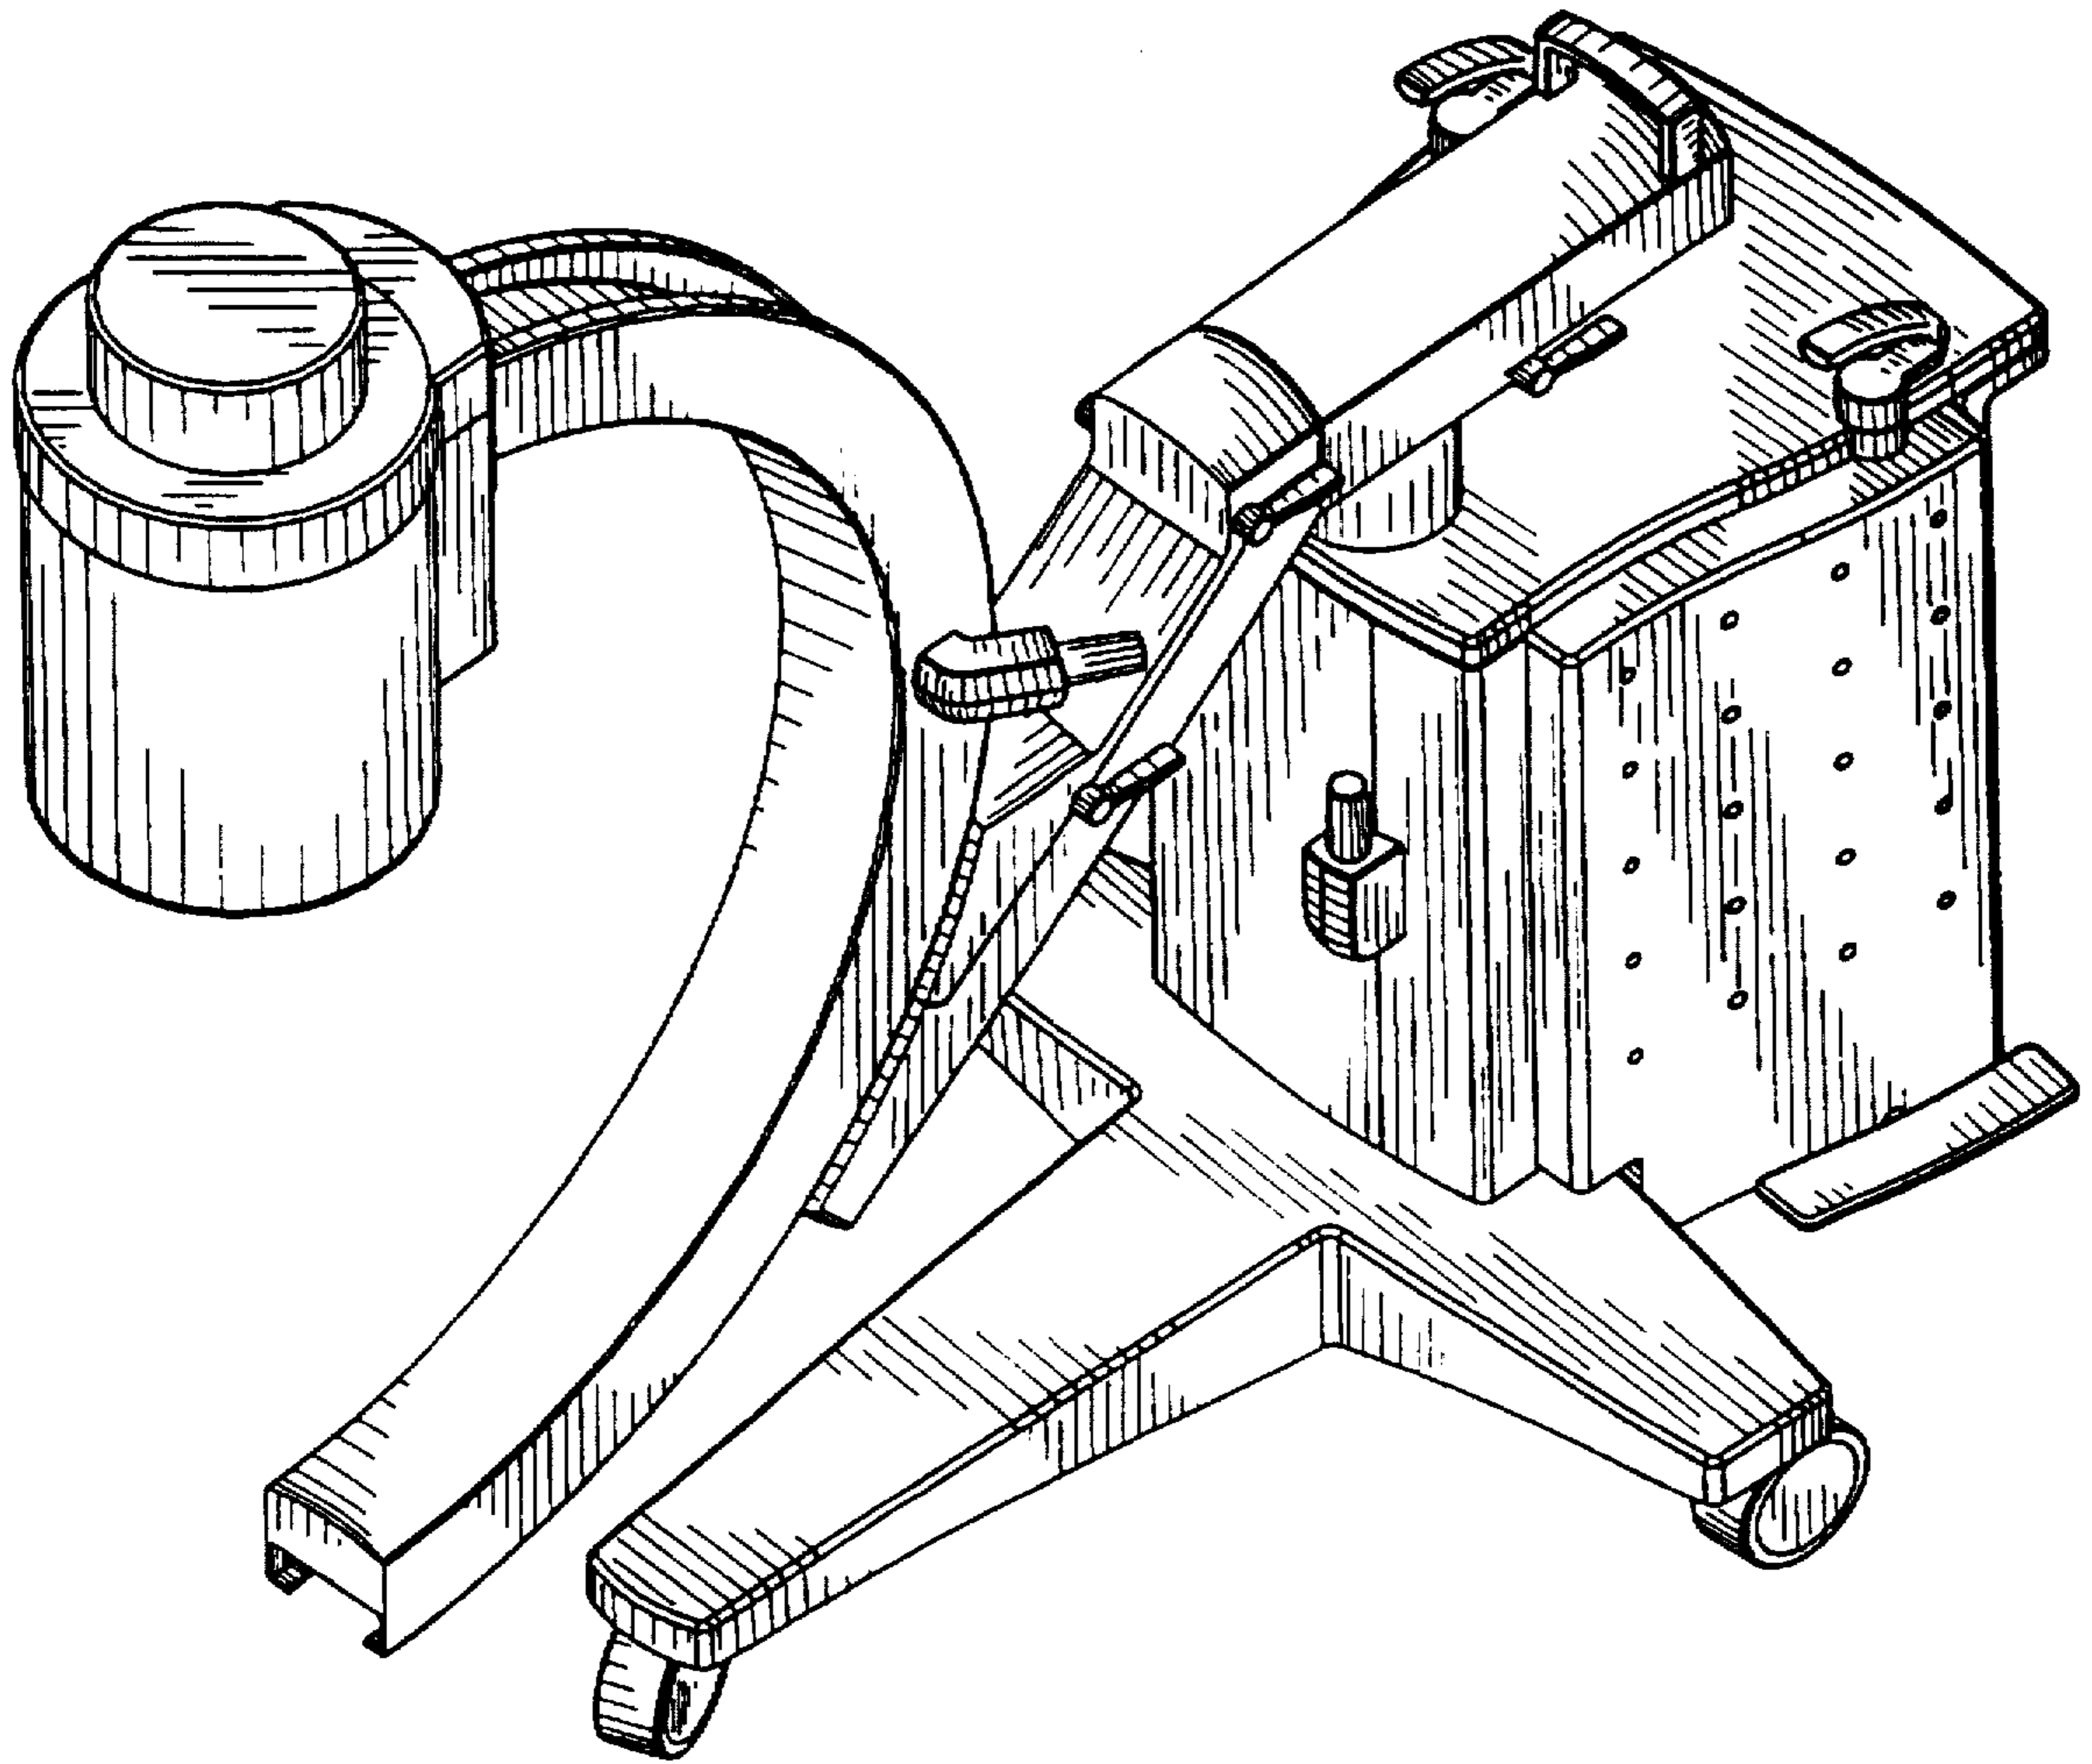


FIG. 1

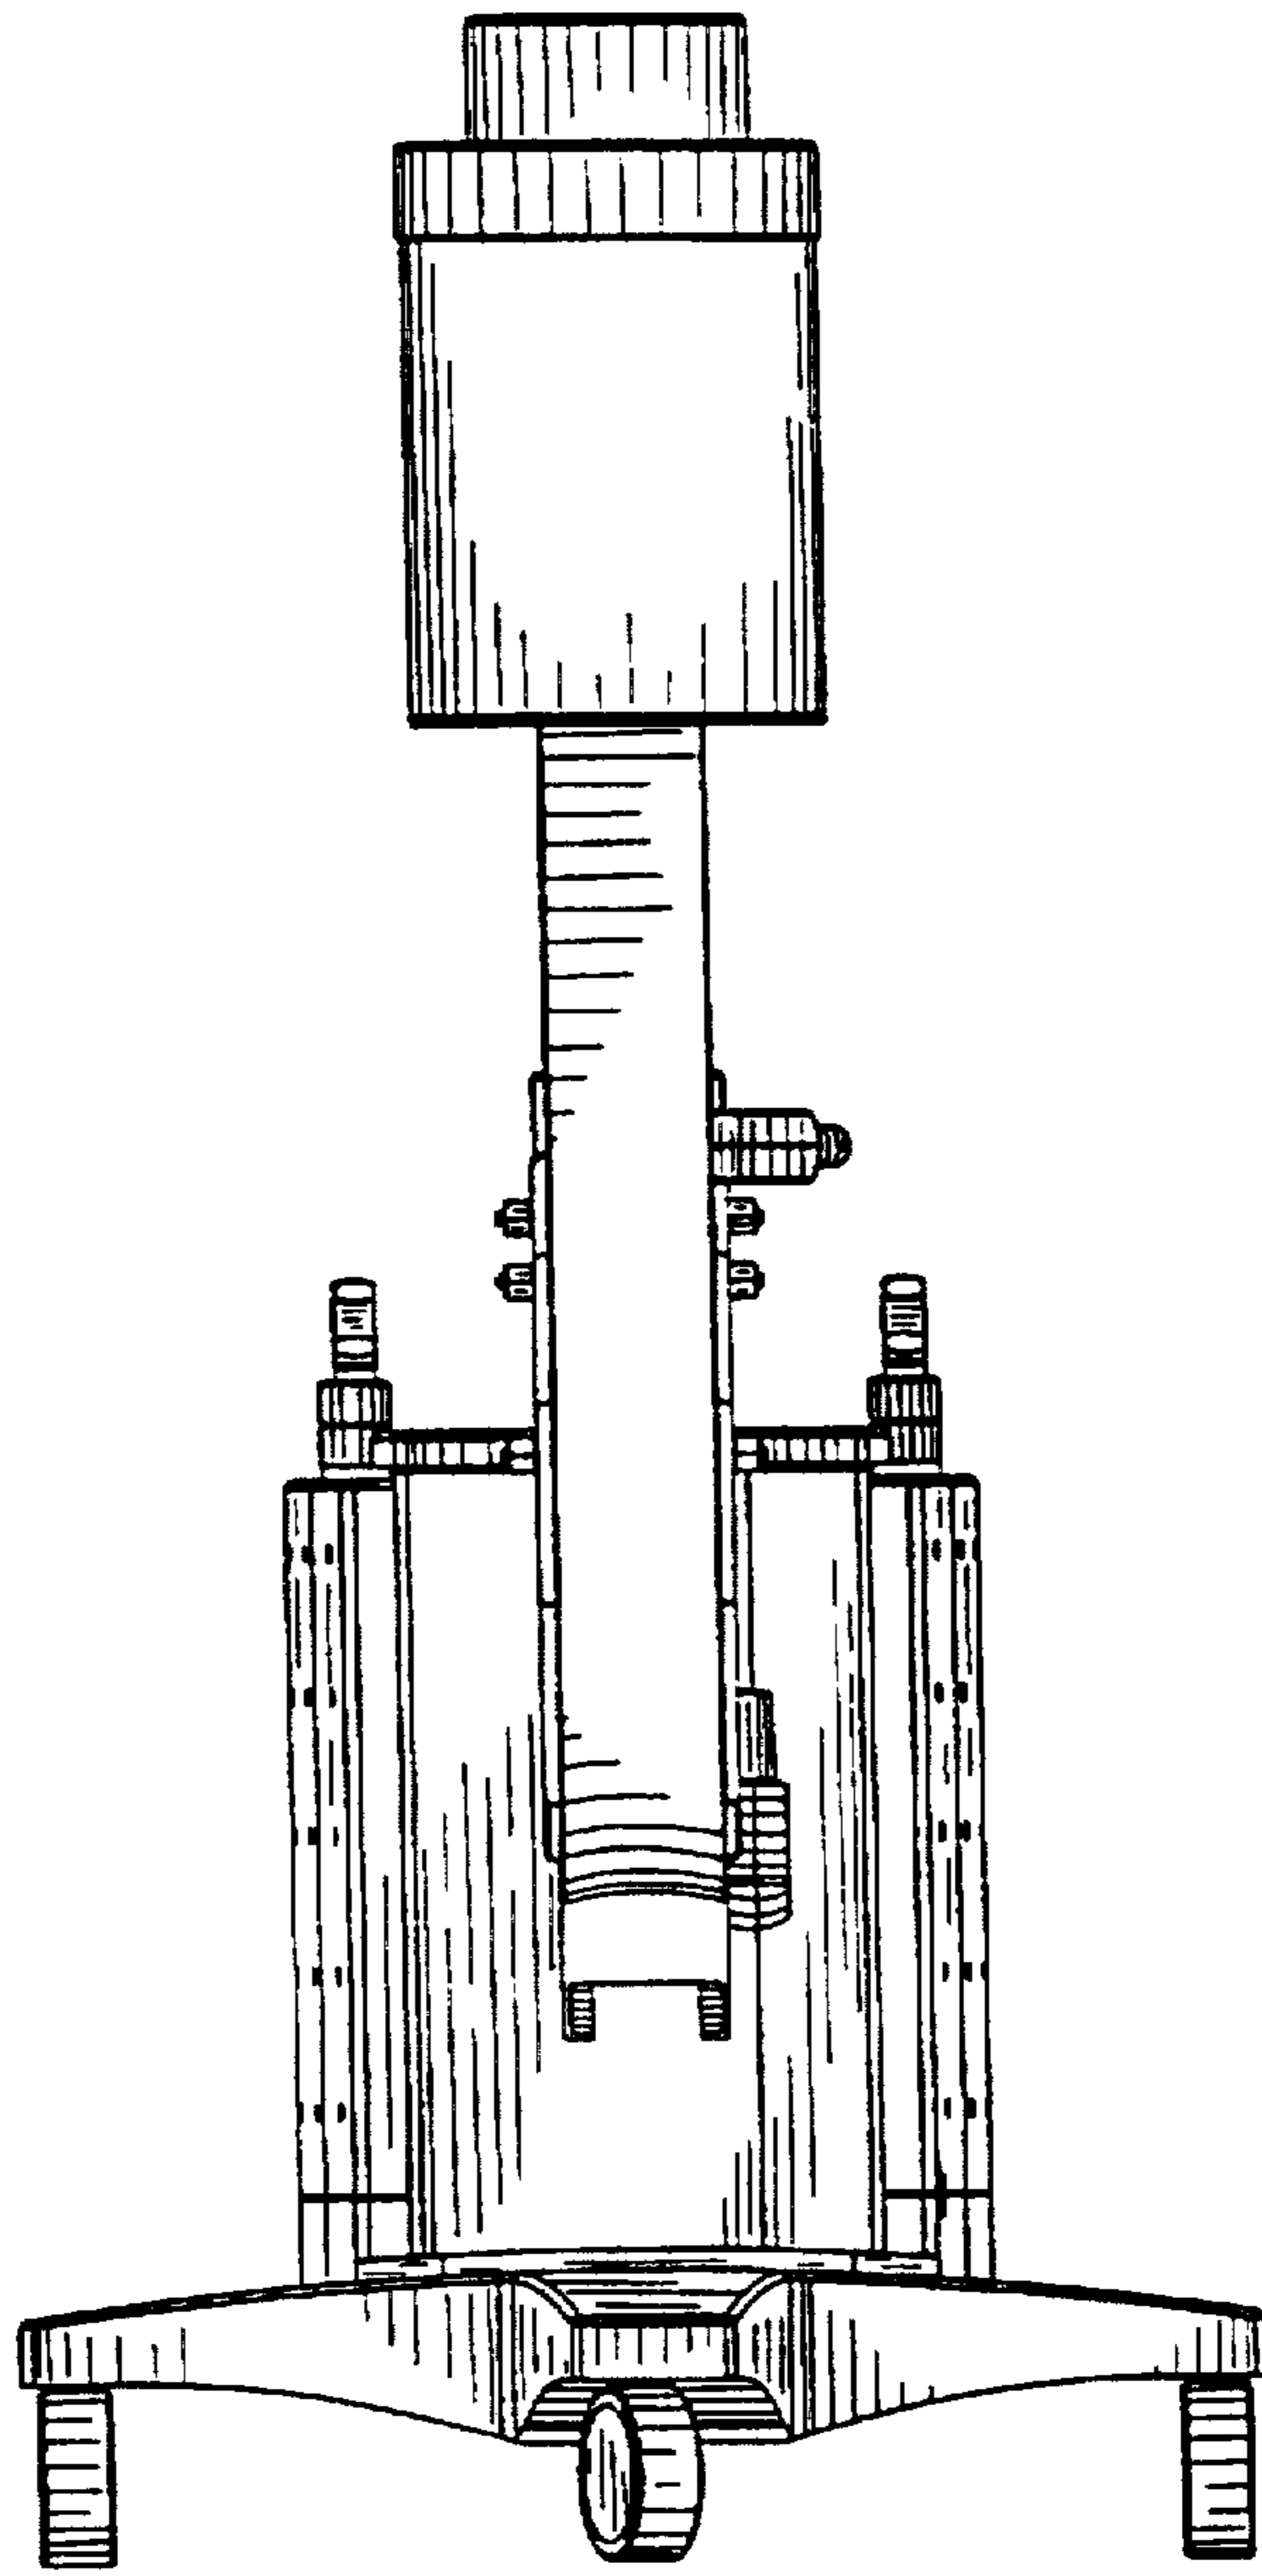


FIG.2

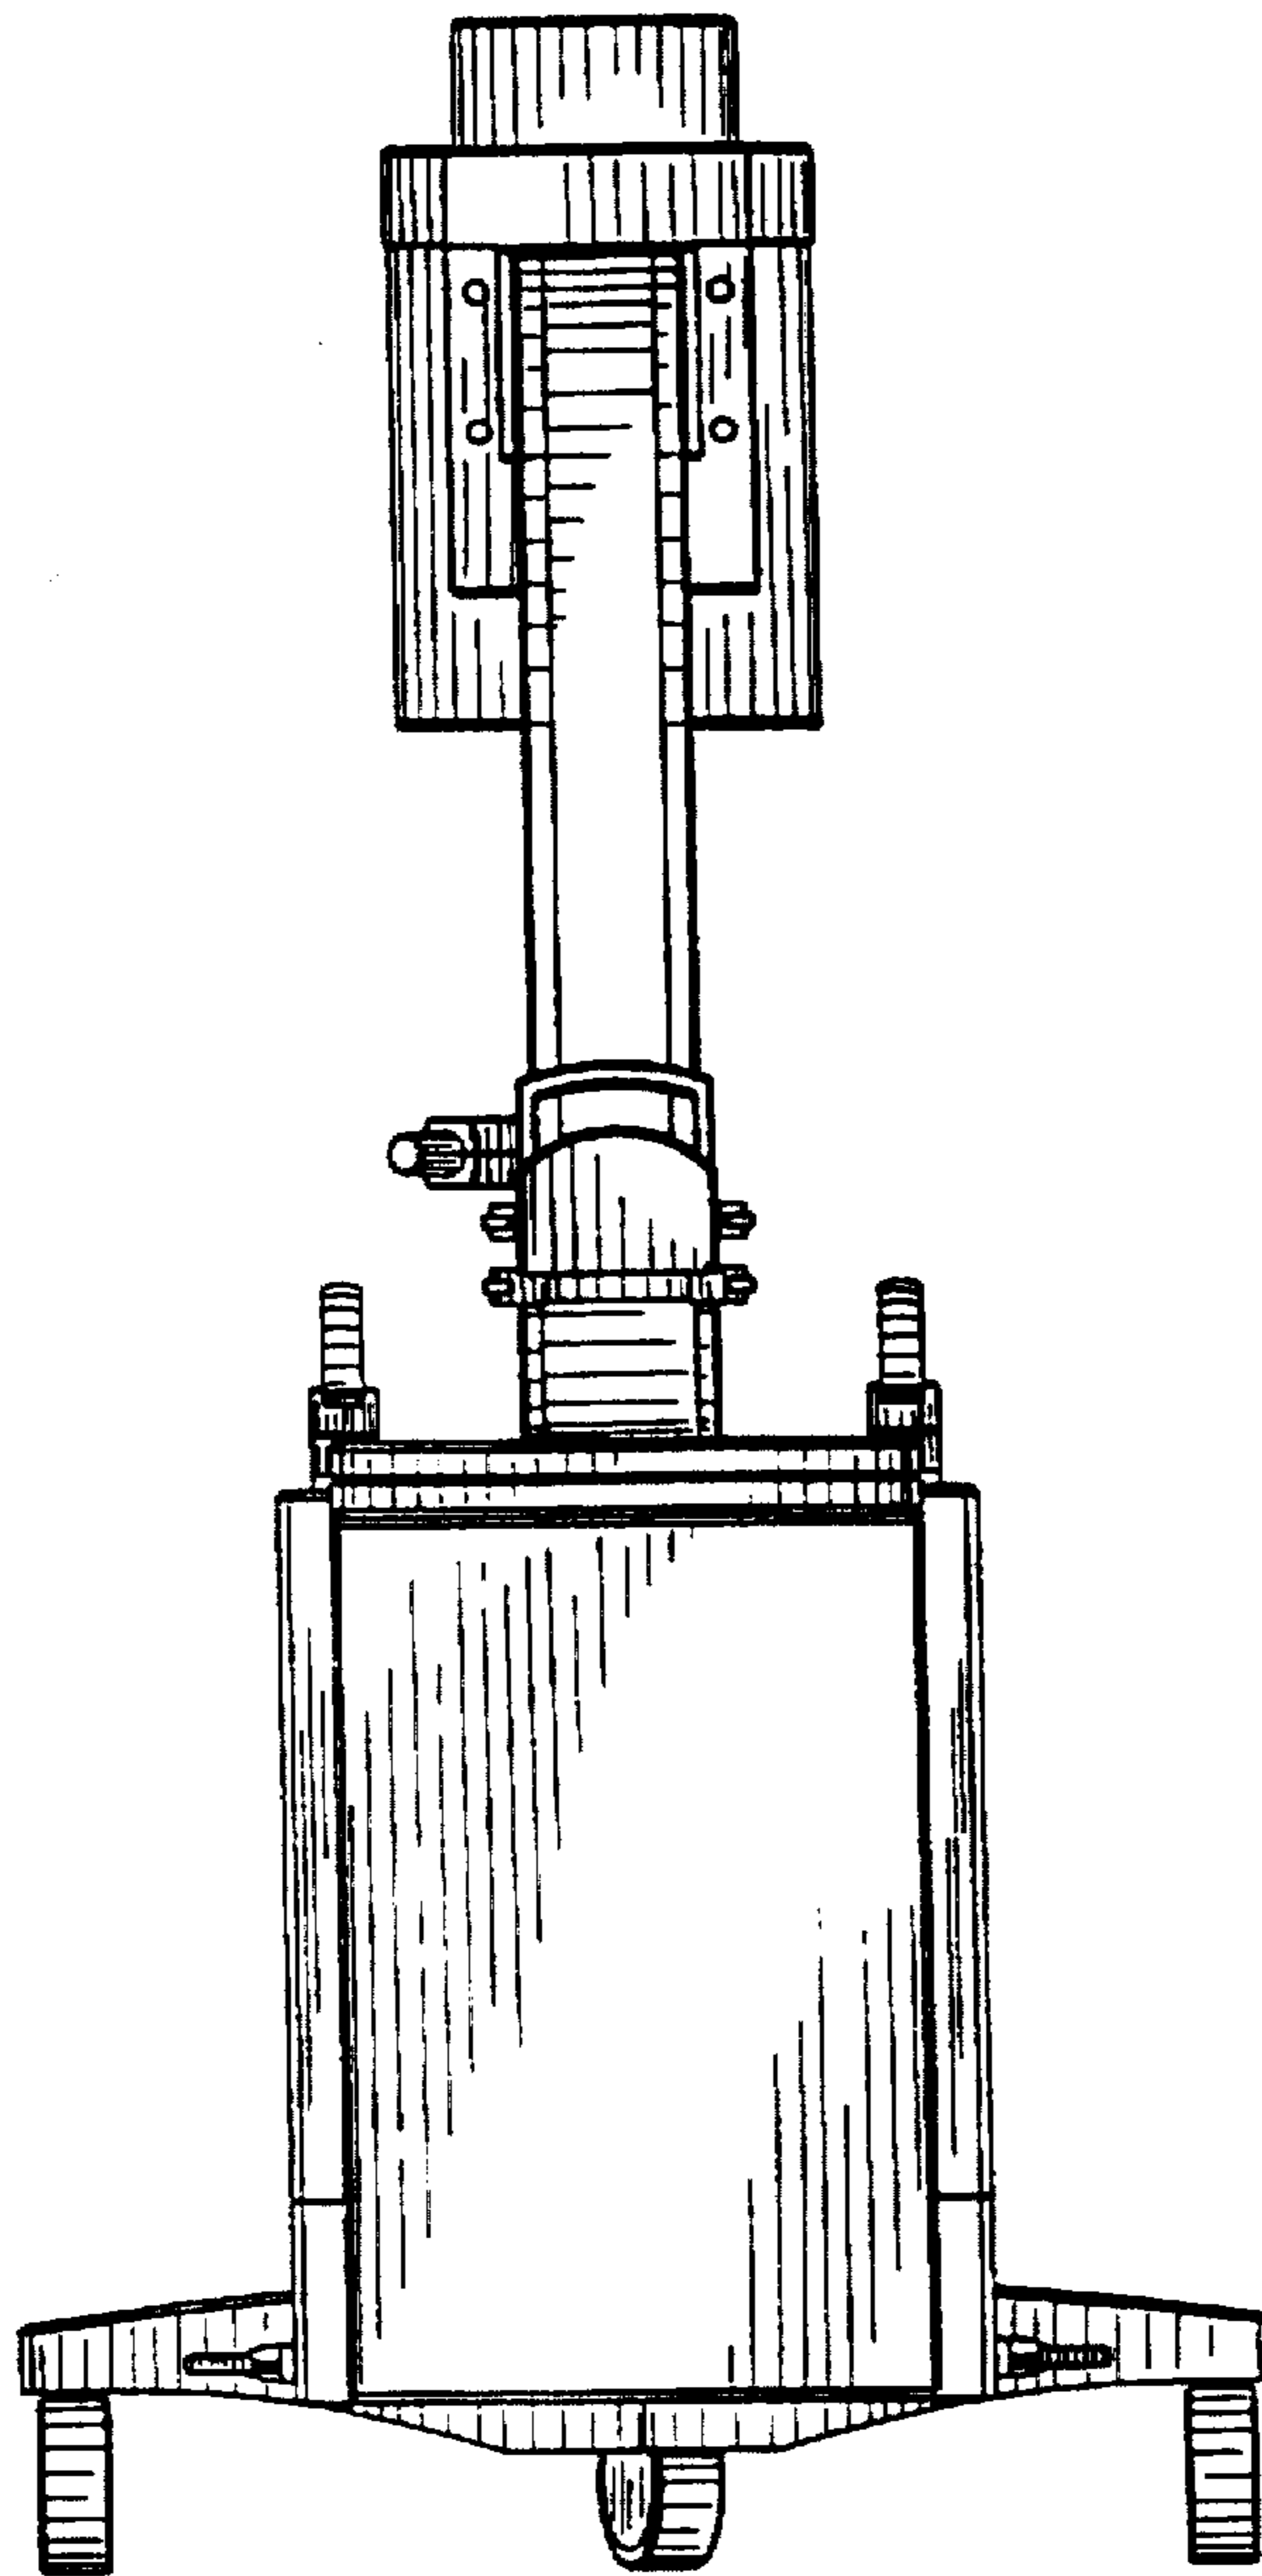


FIG.3

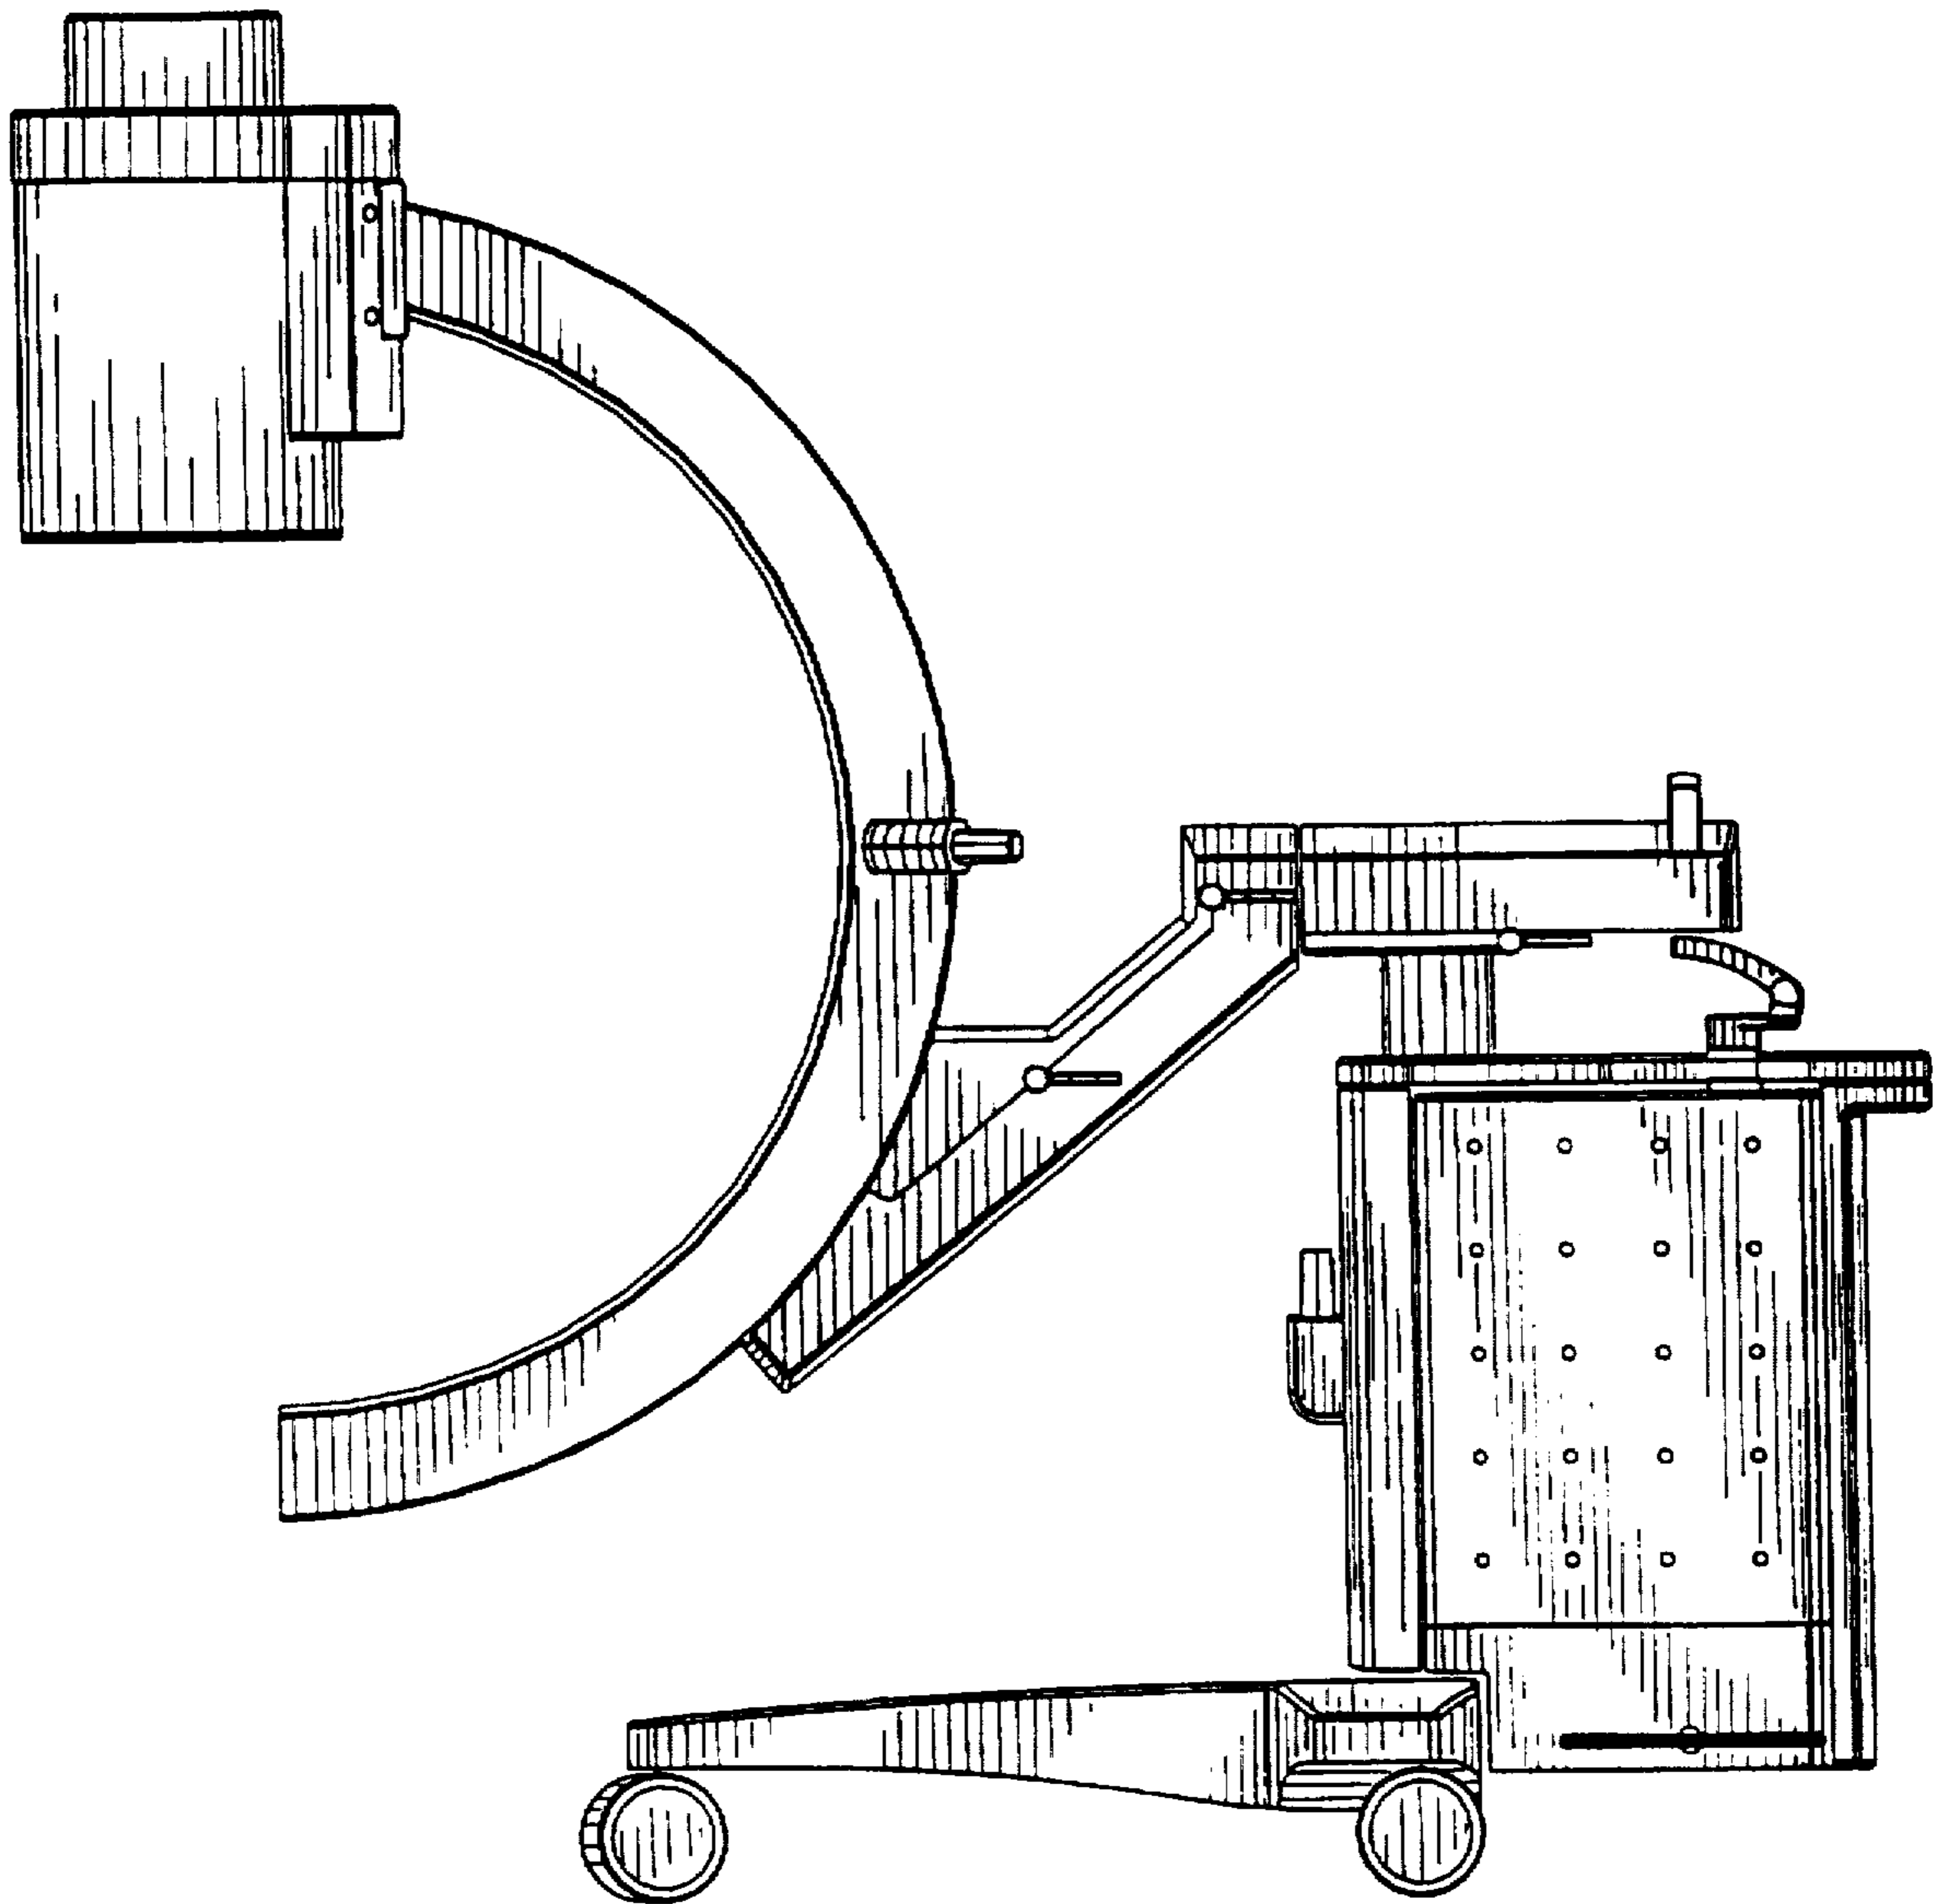


FIG.4

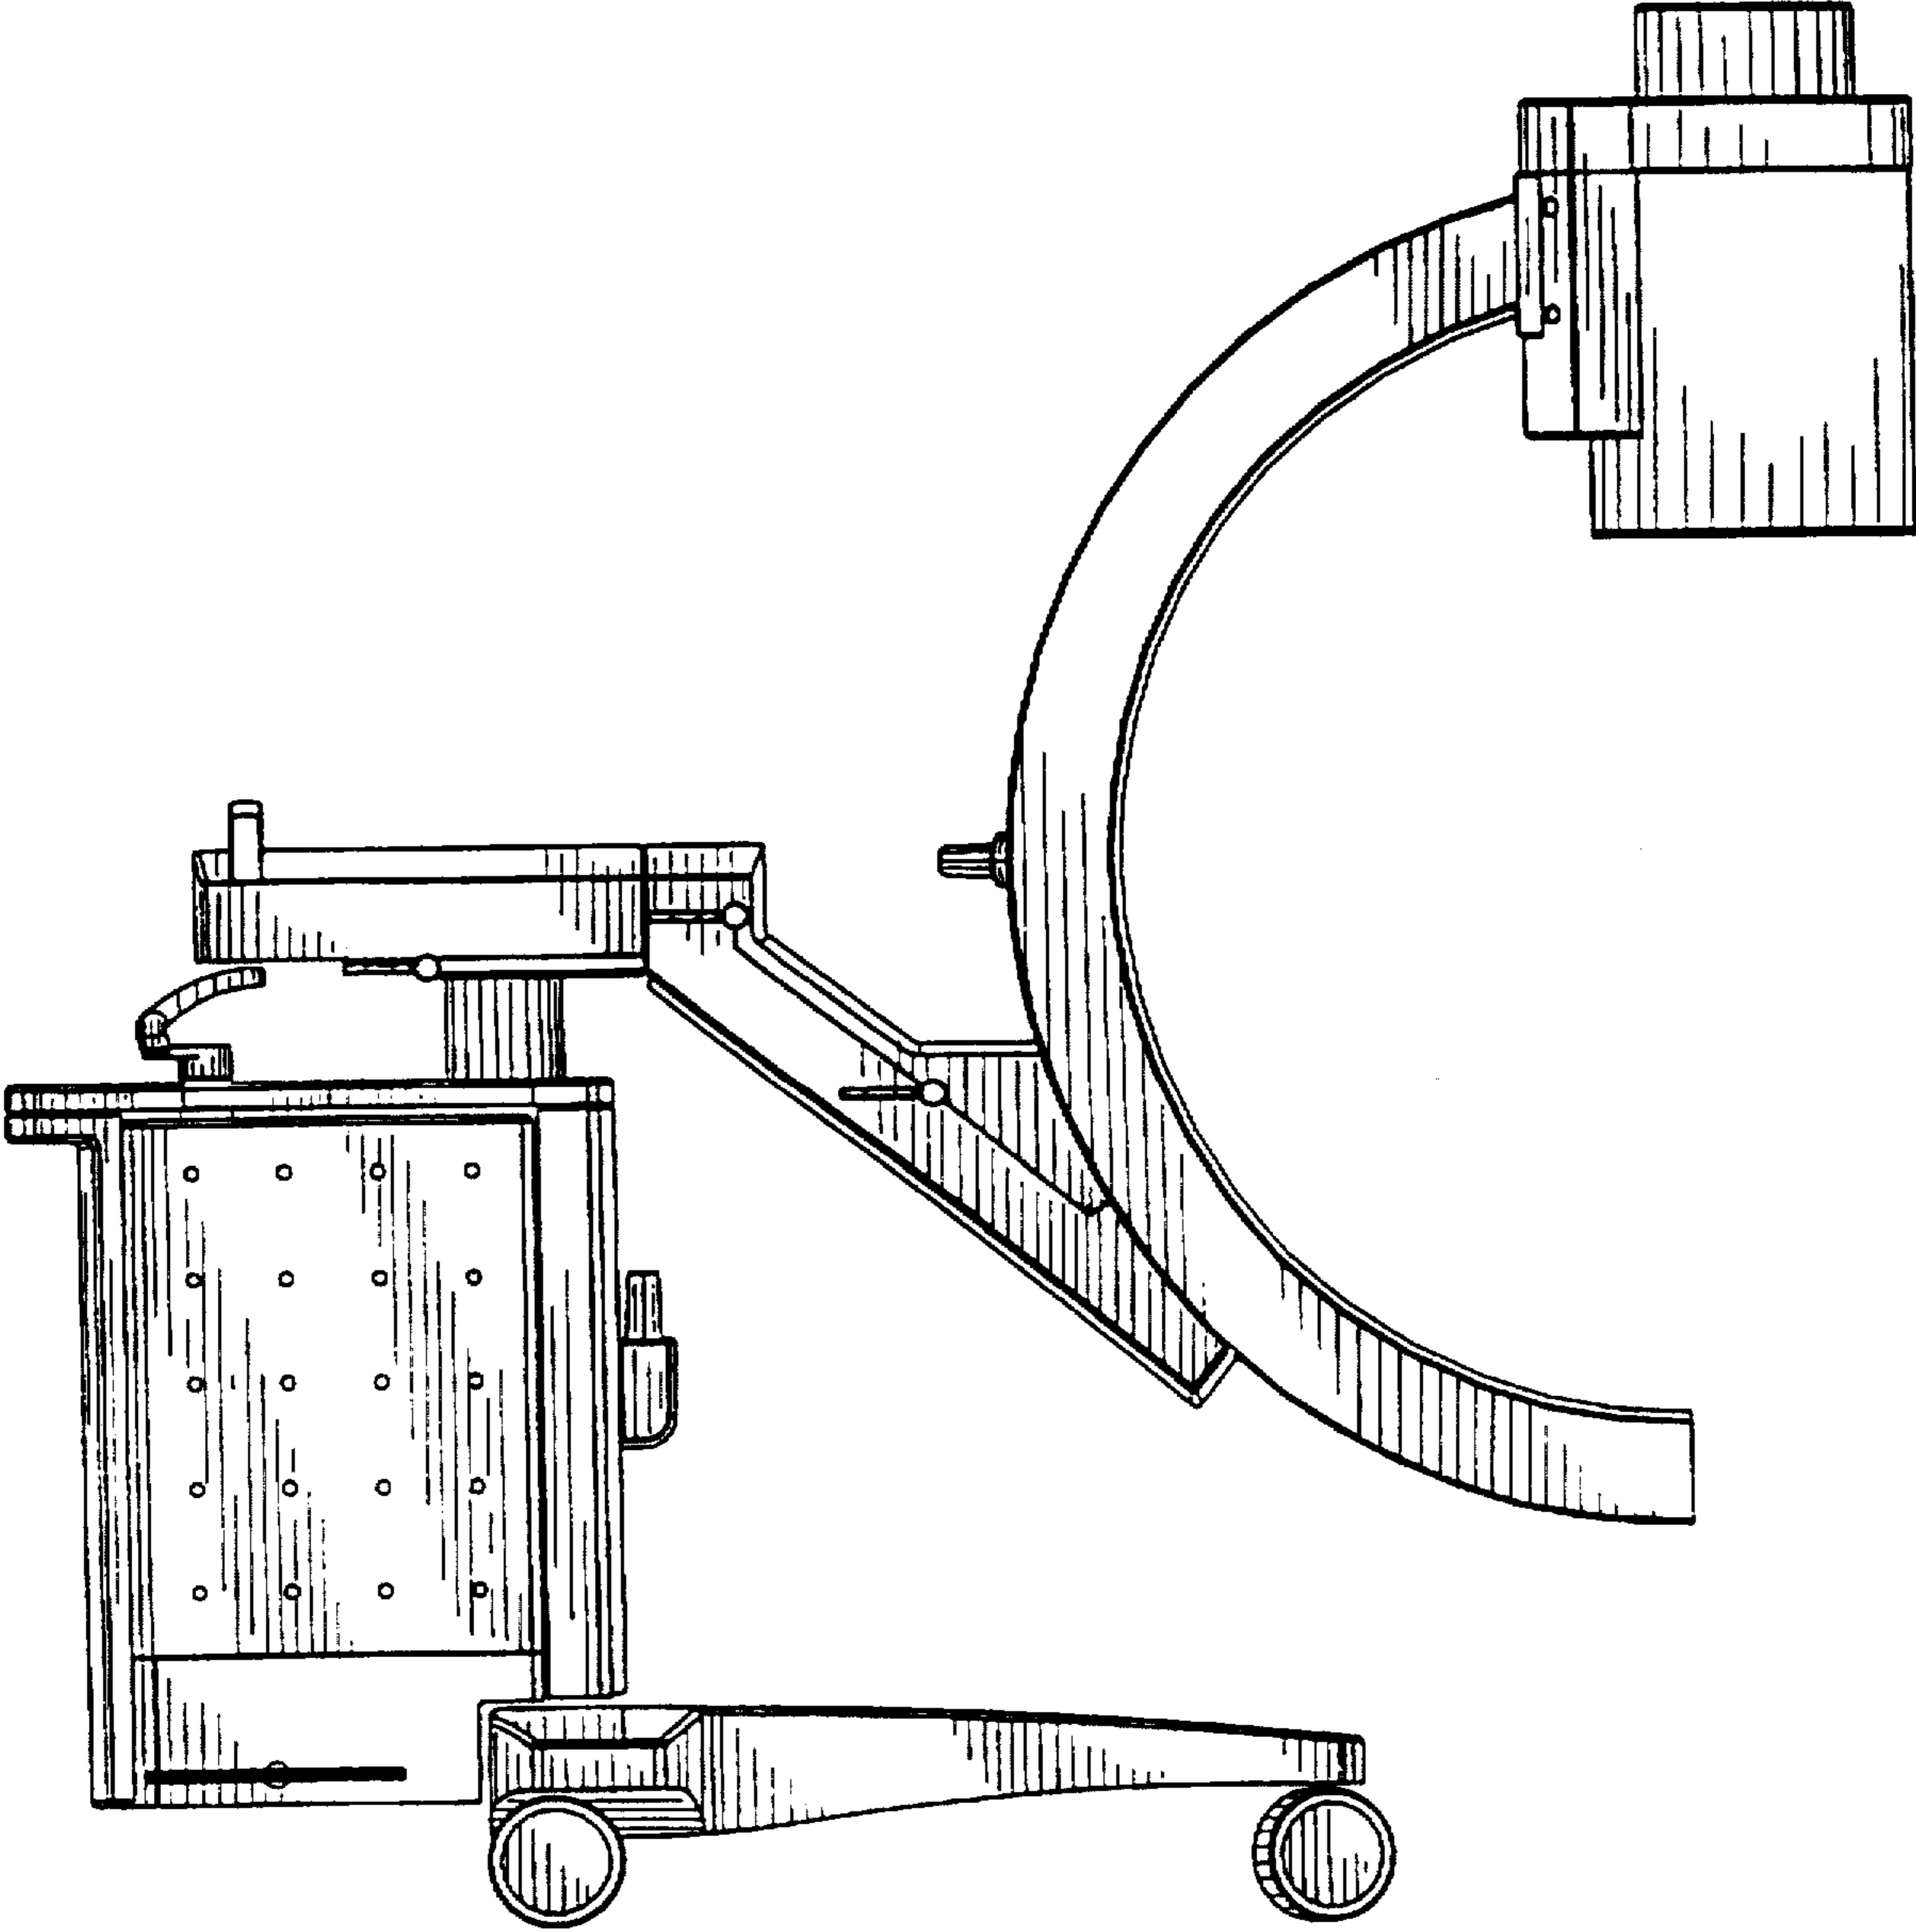


FIG.5

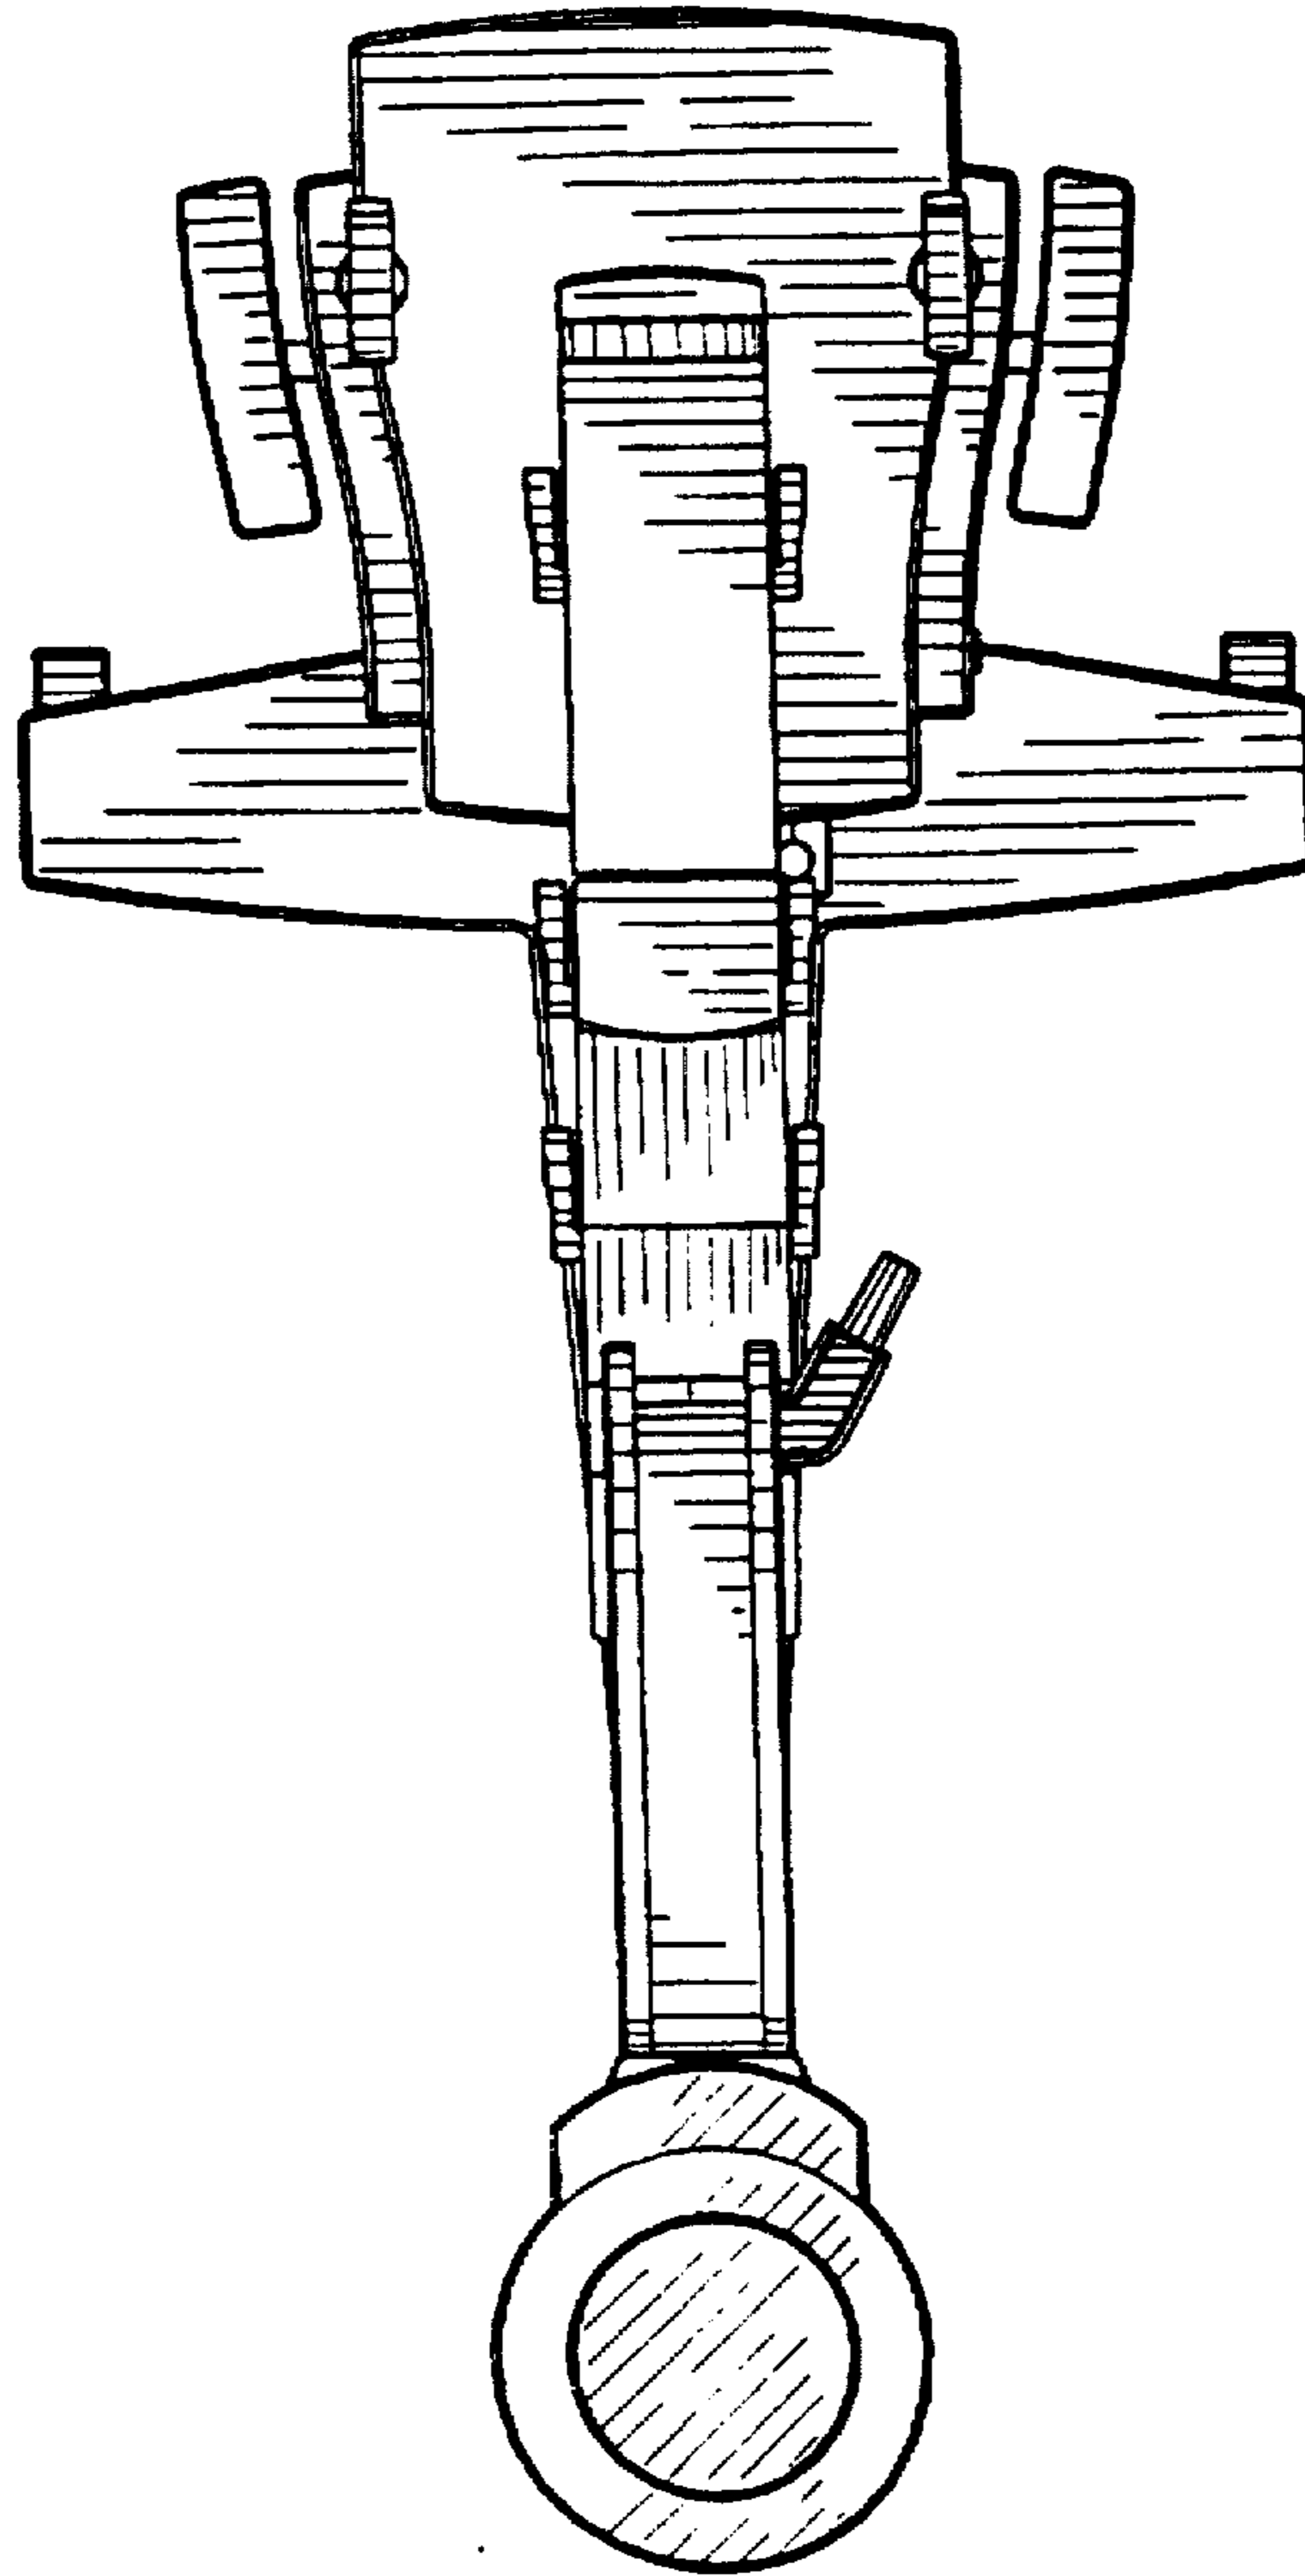


FIG. 6

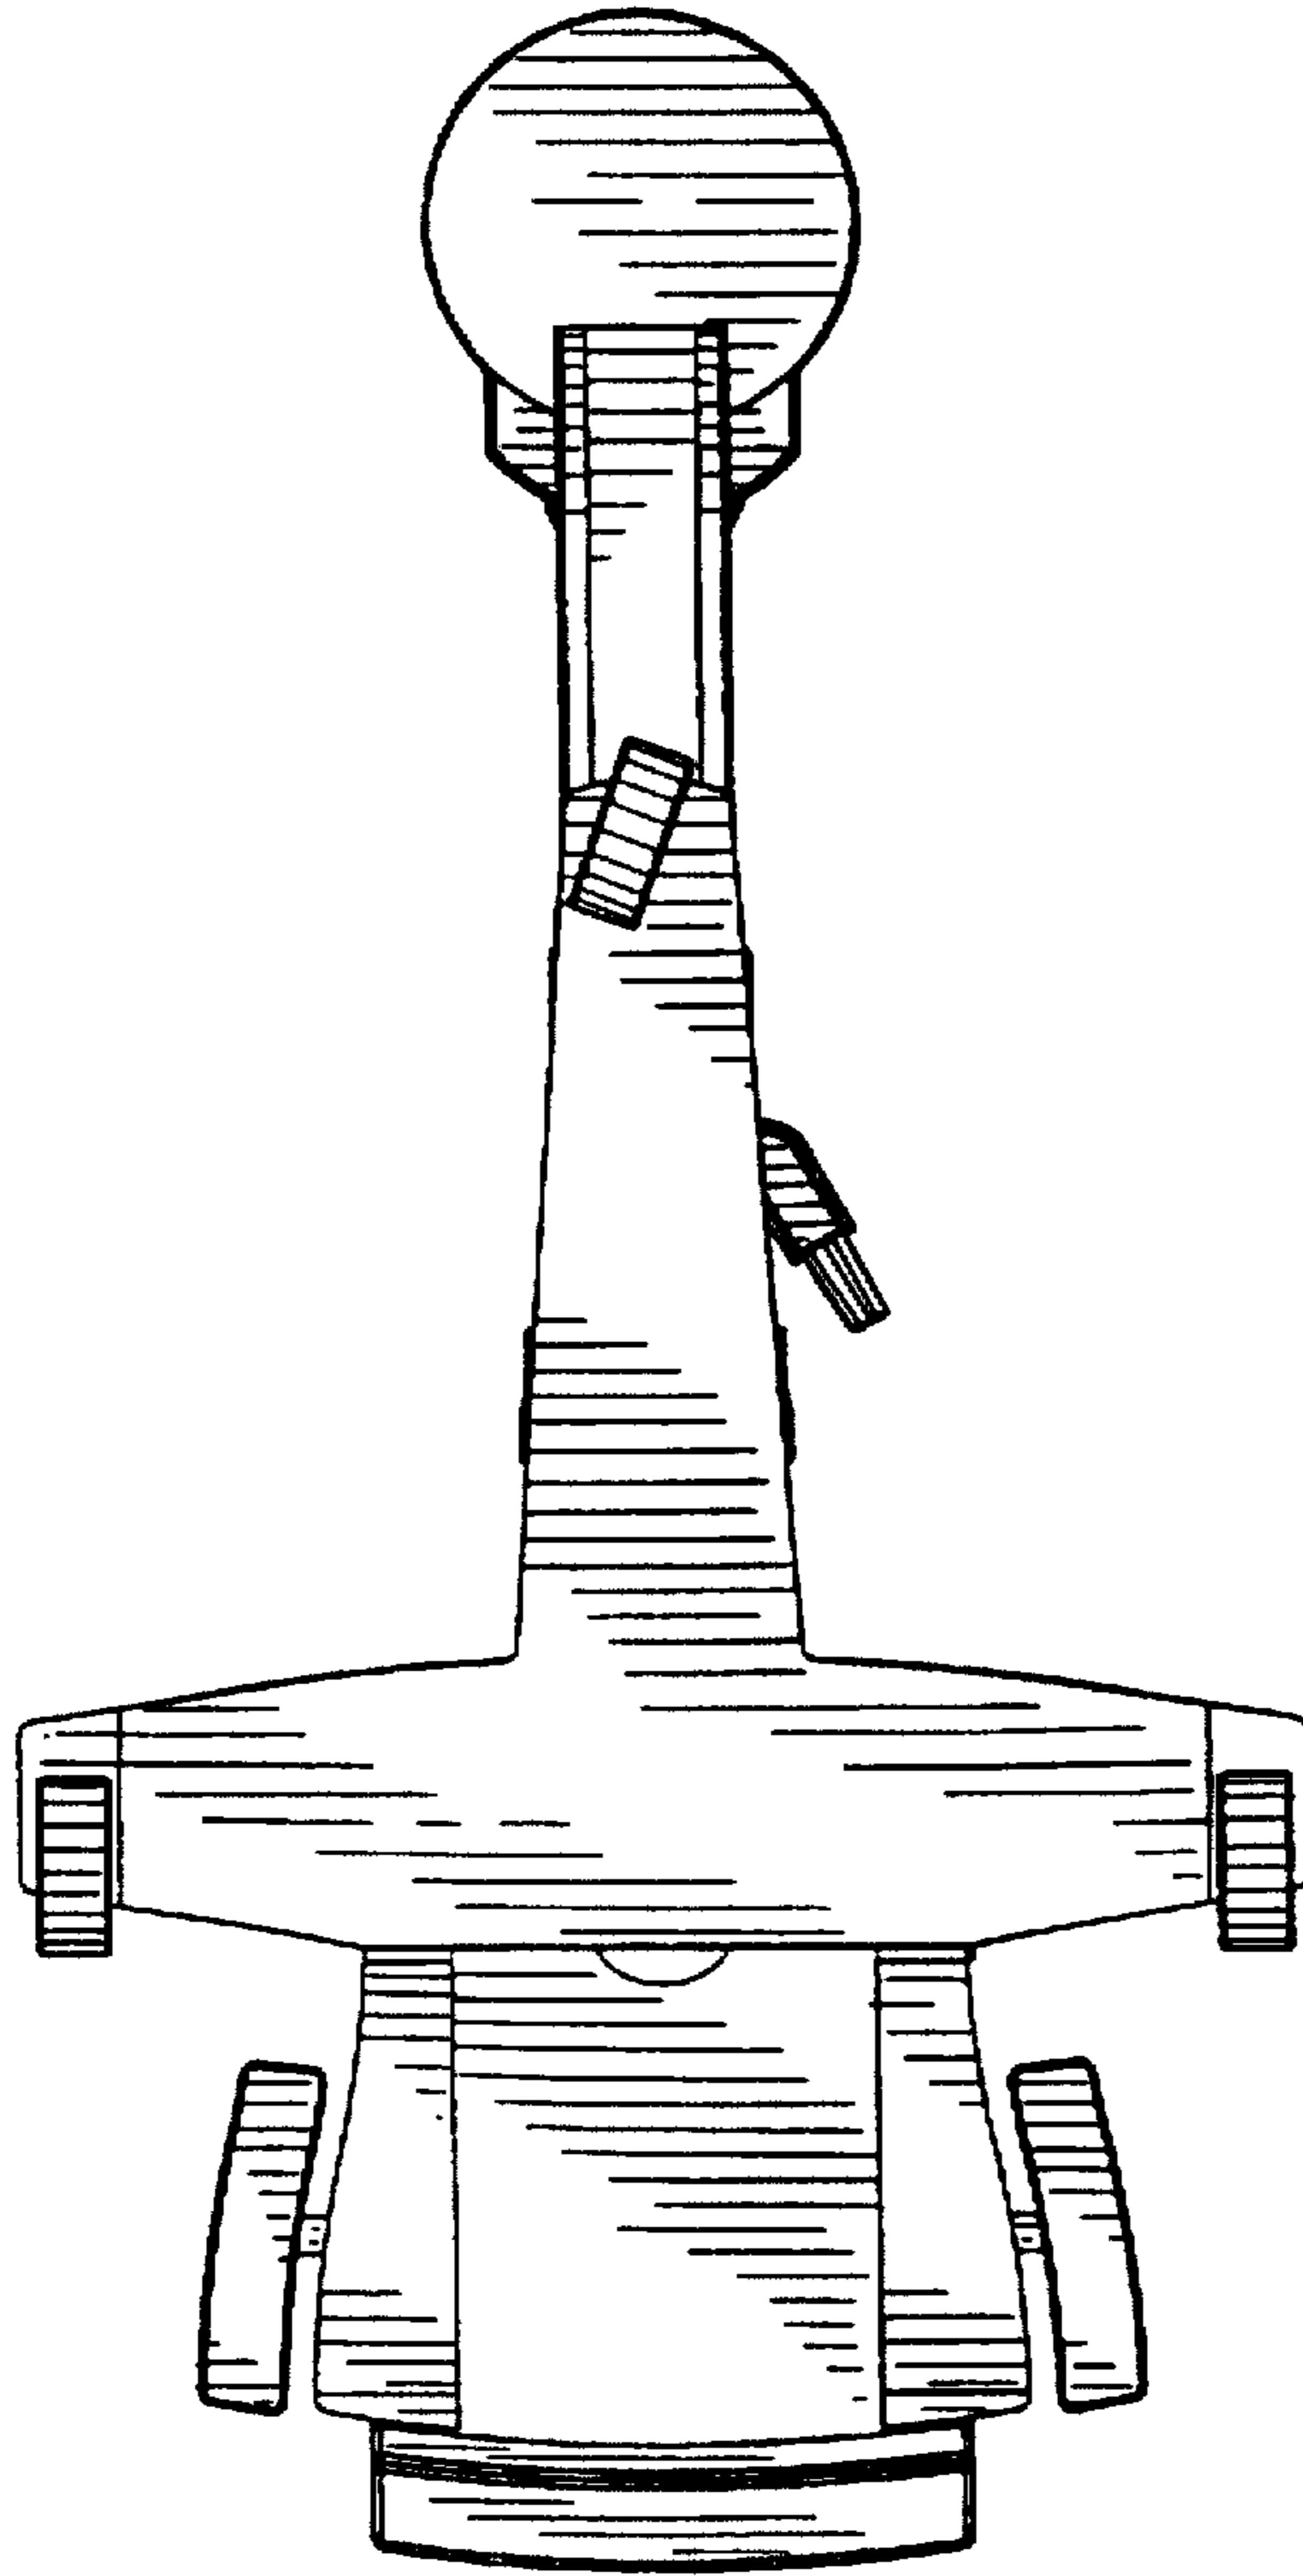


FIG. 7