



US00D399313S

United States Patent [19]
Bydlon et al.

[11] **Patent Number:** **Des. 399,313**
[45] **Date of Patent:** ****Oct. 6, 1998**

[54] **SYRINGE ALIGNMENT DEVICE**

[75] Inventors: **Roland Joseph Bydlon**, Indianapolis;
Javan Eronmy Collins, Fishers;
William Harold Morrison, Jr., Avon;
Bradley Ray Newman, Plainfield, all
of Ind.

[73] Assignee: **Eli Lilly and Company**, Indianapolis,
Ind.

[**] Term: **14 Years**

[21] Appl. No.: **53,856**

[22] Filed: **Mar. 26, 1996**

[51] **LOC (6) Cl.** **24-02**

[52] **U.S. Cl.** **D24/112; D24/133**

[58] **Field of Search** D24/112, 111,
D24/147, 144, 133; 604/35, 27, 902, 118,
119, 264; 606/107; 433/80, 81, 82, 91,
95; D19/51, 56; 24/11 CT

[56] **References Cited**

U.S. PATENT DOCUMENTS

D. 160,670 10/1950 Stern D19/51
D. 277,507 2/1985 Levy D24/112
D. 297,459 8/1988 Heiland et al. D24/112

D. 330,079 10/1992 Dalling et al. D24/112
D. 351,227 10/1994 Patton et al. D24/112
D. 362,683 9/1995 Pitteloud D19/56 X
D. 368,961 4/1996 Himbert et al. D24/114
D. 375,789 11/1996 Bryant et al. D24/112
D. 377,051 12/1996 Takemura D19/51
D. 385,918 11/1997 Katami D19/56 X
5,591,138 1/1997 Vaillancourt 604/263

Primary Examiner—Susan J. Lucas
Assistant Examiner—Cynthia E. Ramirez
Attorney, Agent, or Firm—Michael T. Bates; David E.
Boone


[57] **CLAIM**

The ornamental design for the syringe alignment device, as
shown and described.

DESCRIPTION

FIG. 1 is a perspective view of the syringe alignment device
showing our new design;
FIG. 2 is a top view thereof;
FIG. 3 is a side view thereof; the opposite side being a mirror
image;
FIG. 4 is a bottom view thereof;
FIG. 5 is an end view of the distal end thereof; and,
FIG. 6 is an end view of the proximal end thereof.

1 Claim, 1 Drawing Sheet

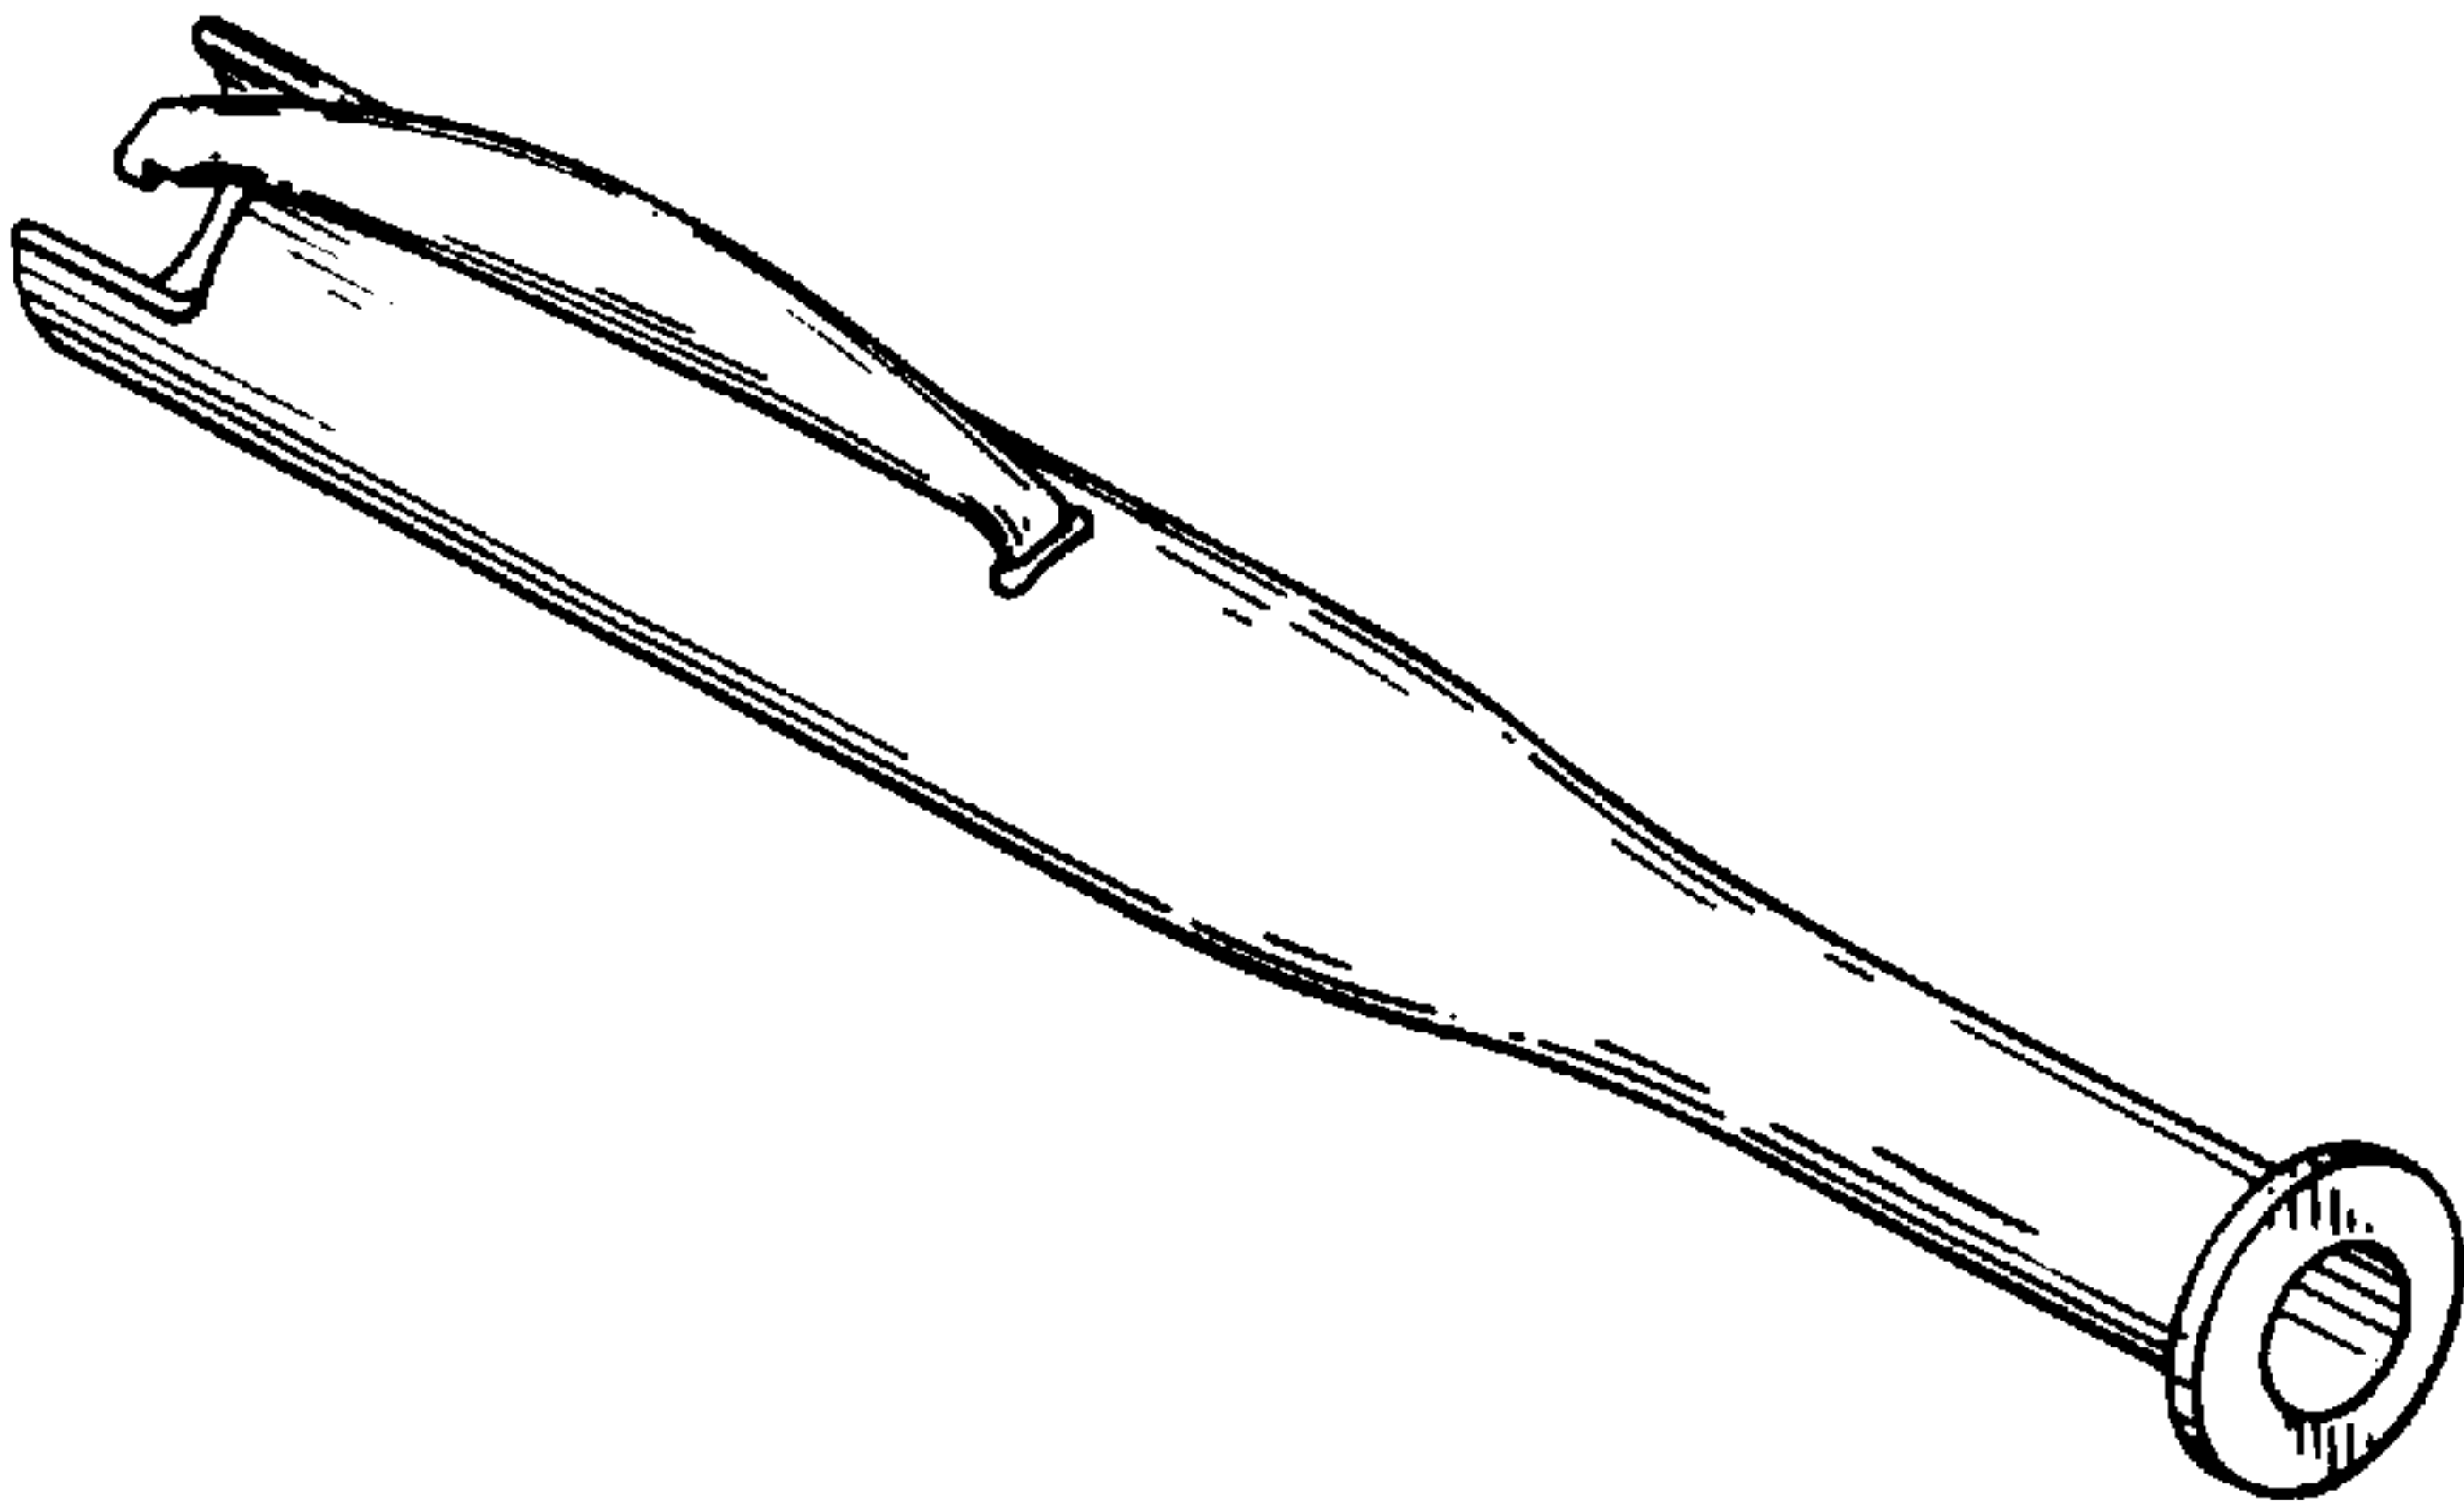

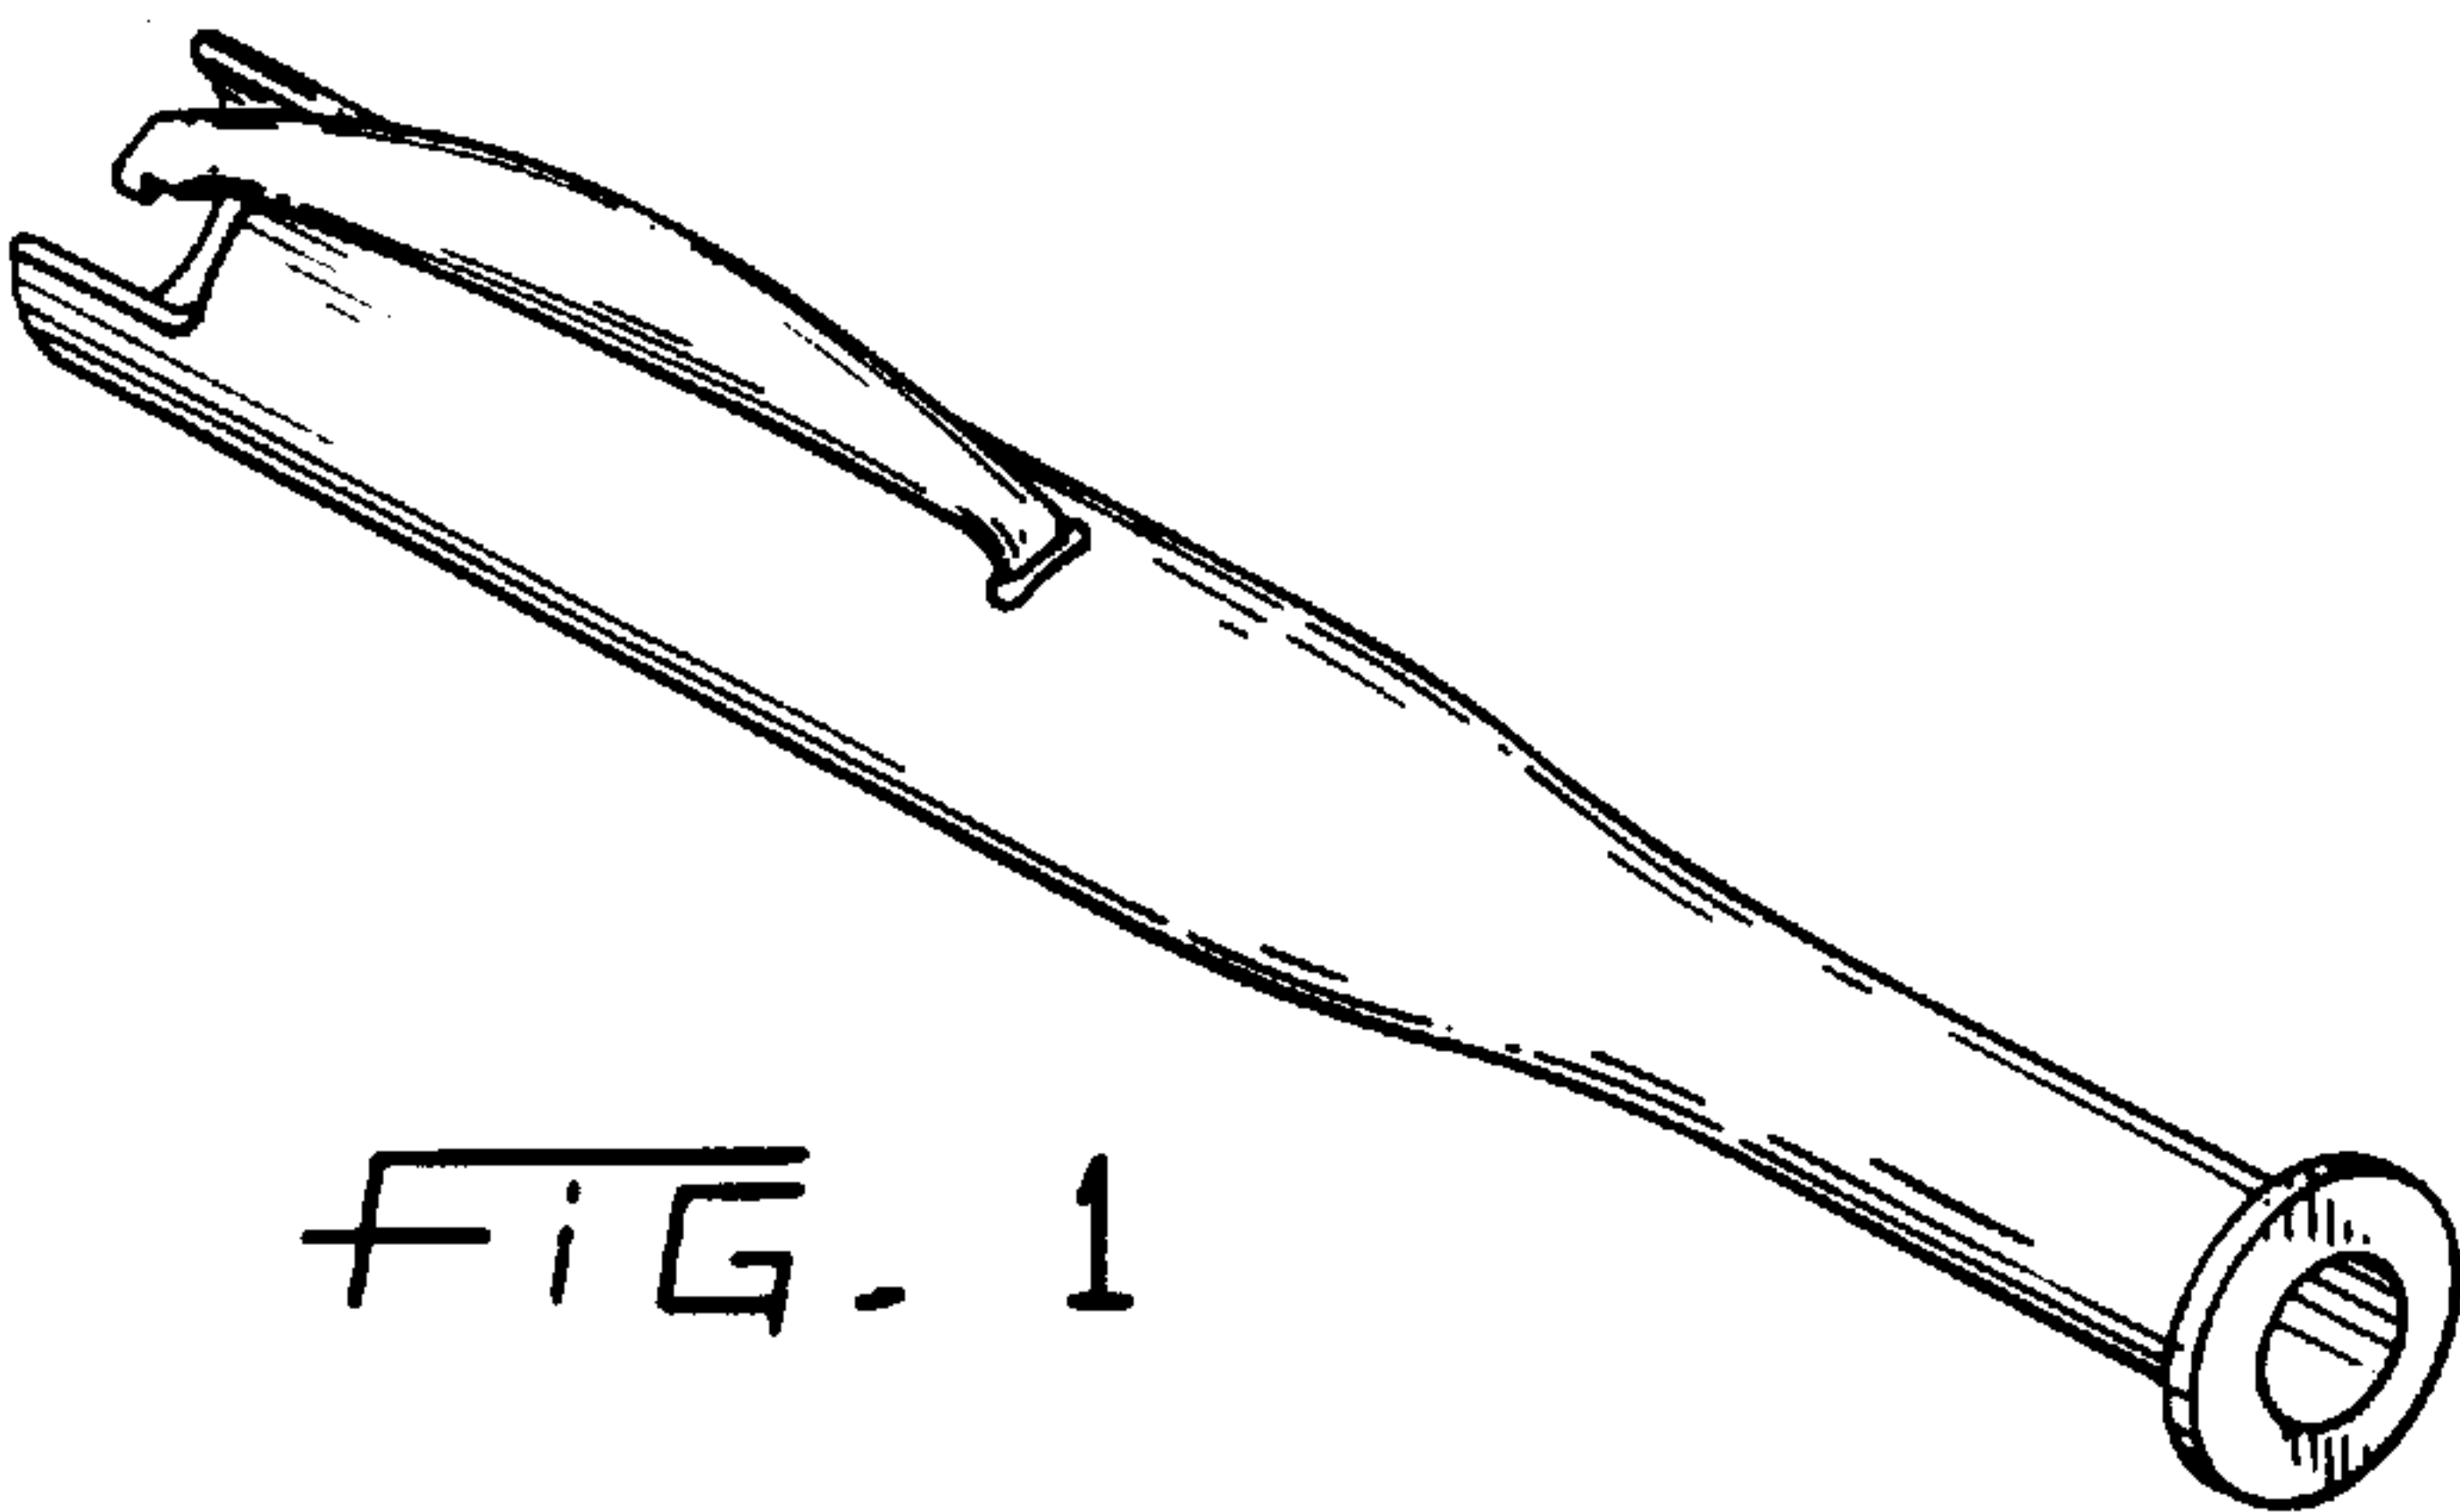


FIG. 1



FIG. 2



FIG. 3

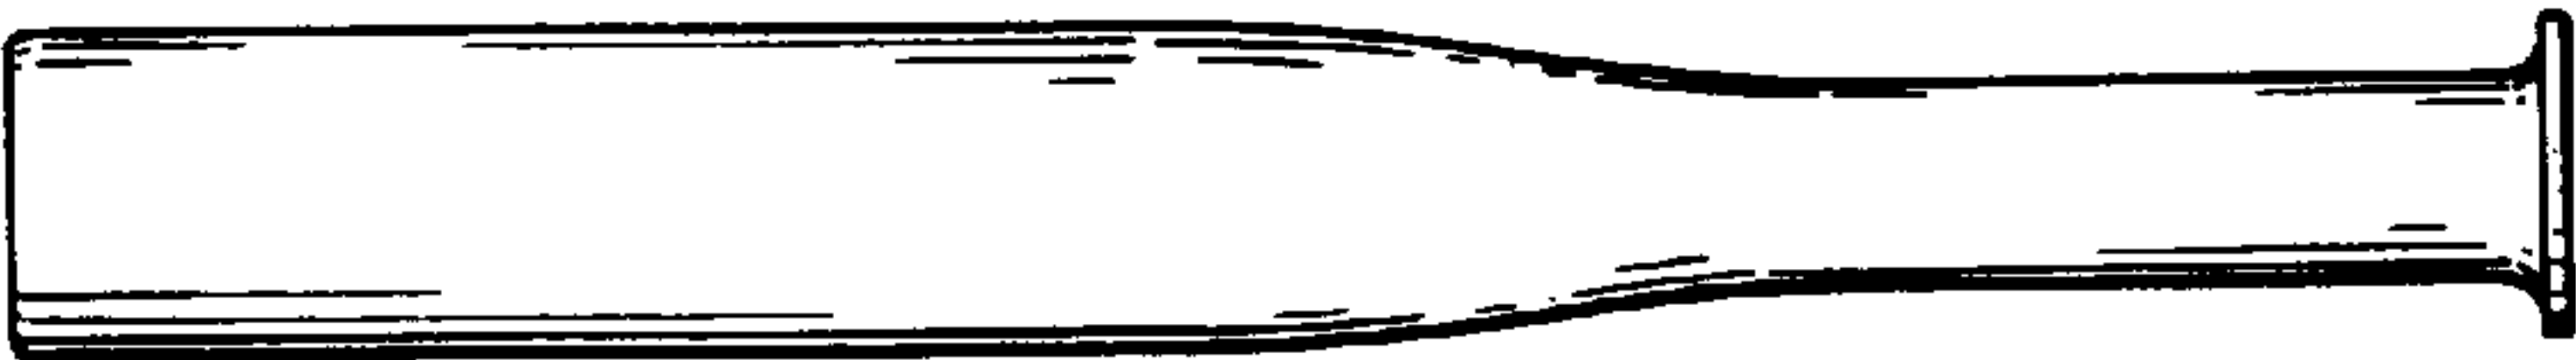


FIG. 4

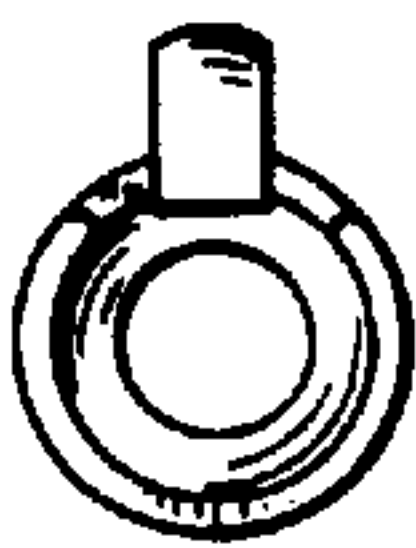


FIG. 5

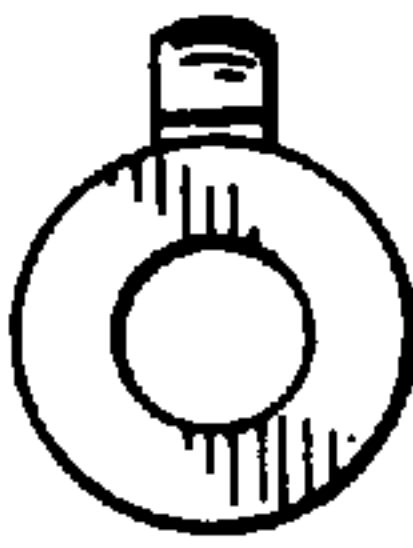


FIG. 6