

US00D401338S

United States Patent [19]
Manzie

[11] Patent Number: Des. 401,338
[45] Date of Patent: **Nov. 17, 1998

[54] TIP OF A RESECTOSCOPE ELECTRODE
ASSEMBLY DESIGN

[75] Inventor: Peter A. Manzie, Berwyn, Ill.

[73] Assignee: Northgate Technologies, Inc., Elgin,
Ill.

[**] Term: 14 Years

[21] Appl. No.: 56,261

[22] Filed: Jun. 18, 1996

[51] LOC (6) Cl. 24-02

[52] U.S. Cl. D24/144

[58] Field of Search D24/155, 176,
D24/144, 146; 606/46, 48, 45, 41, 49, 50,
37, 38, 39, 40

[56] References Cited

U.S. PATENT DOCUMENTS

D. 320,446	10/1991	Gross et al. .	
D. 385,351	10/1997	Manzie et al.	D24/144
4,149,538	4/1979	Mrava et al. .	
4,726,370	2/1988	Karasawa et al. .	
4,917,082	4/1990	Grossi et al. .	
4,955,884	9/1990	Grossi et al. .	
5,007,907	4/1991	Nishigaki et al. .	
5,196,011	3/1993	Korth et al. .	
5,267,994	12/1993	Gentelia et al. .	
5,354,296	10/1994	Turkel	606/41
5,423,813	6/1995	Kaiser et al. .	
5,486,173	1/1996	Vancaillie .	
5,549,605	8/1996	Hahnen .	
5,569,244	10/1996	Hahnen .	
5,582,610	12/1996	Grossi et al. .	

OTHER PUBLICATIONS

“Vapor–Tech,” by Nortech, published prior to 1996.
U.S. Ser. No. 08/568,130 filed Dec. 6, 1995.
U.S. Ser. No. 29/047,522 filed Dec. 6, 1995.

U.S. Ser. No. 08/585,308 filed Jan. 11, 1996.
U.S. Ser. No. 08/640,706 filed May 1, 1996.

Primary Examiner—Doris Clark
Attorney, Agent, or Firm—Brinks, Hofer, Gilson & Lione;
Frank J. Kozak


[57] CLAIM

The ornamental design for a tip of a resectoscope electrode assembly, as shown.

DESCRIPTION

FIG. 1 is a perspective view of a tip of a resectoscope electrode assembly showing my new design;
FIG. 2 is a perspective view of the tip of the resectoscope electrode assembly of FIG. 1;
FIG. 3 is a side view of the tip for a resectoscope electrode assembly shown in FIG. 2;
FIG. 4 is a rear view of the tip of the resectoscope electrode assembly shown in FIG. 2;
FIG. 5 is an front view of the tip for the resectoscope electrode assembly shown in FIG. 2;
FIG. 6 is a bottom view of the tip for the resectoscope electrode assembly shown in FIG. 2;
FIG. 7 is a top view of the tip for the resectoscope electrode assembly shown in FIG. 2;
FIG. 8 is a perspective view of an alternate embodiment of the tip of the resectoscope electrode assembly of FIG. 1;
FIG. 9 is a top view of the embodiment of the tip for the resectoscope electrode assembly shown in FIG. 8;
FIG. 10 is a rear view of the tip of the resectoscope electrode assembly shown in FIG. 8;
FIG. 11 is a side view of the tip for a resectoscope electrode assembly shown in FIG. 8;
FIG. 12 is a front view of the tip for the resectoscope electrode assembly shown in FIG. 8; and,
FIG. 13 is a bottom view of the tip for the resectoscope electrode assembly shown in FIG. 8.

1 Claim, 3 Drawing Sheets

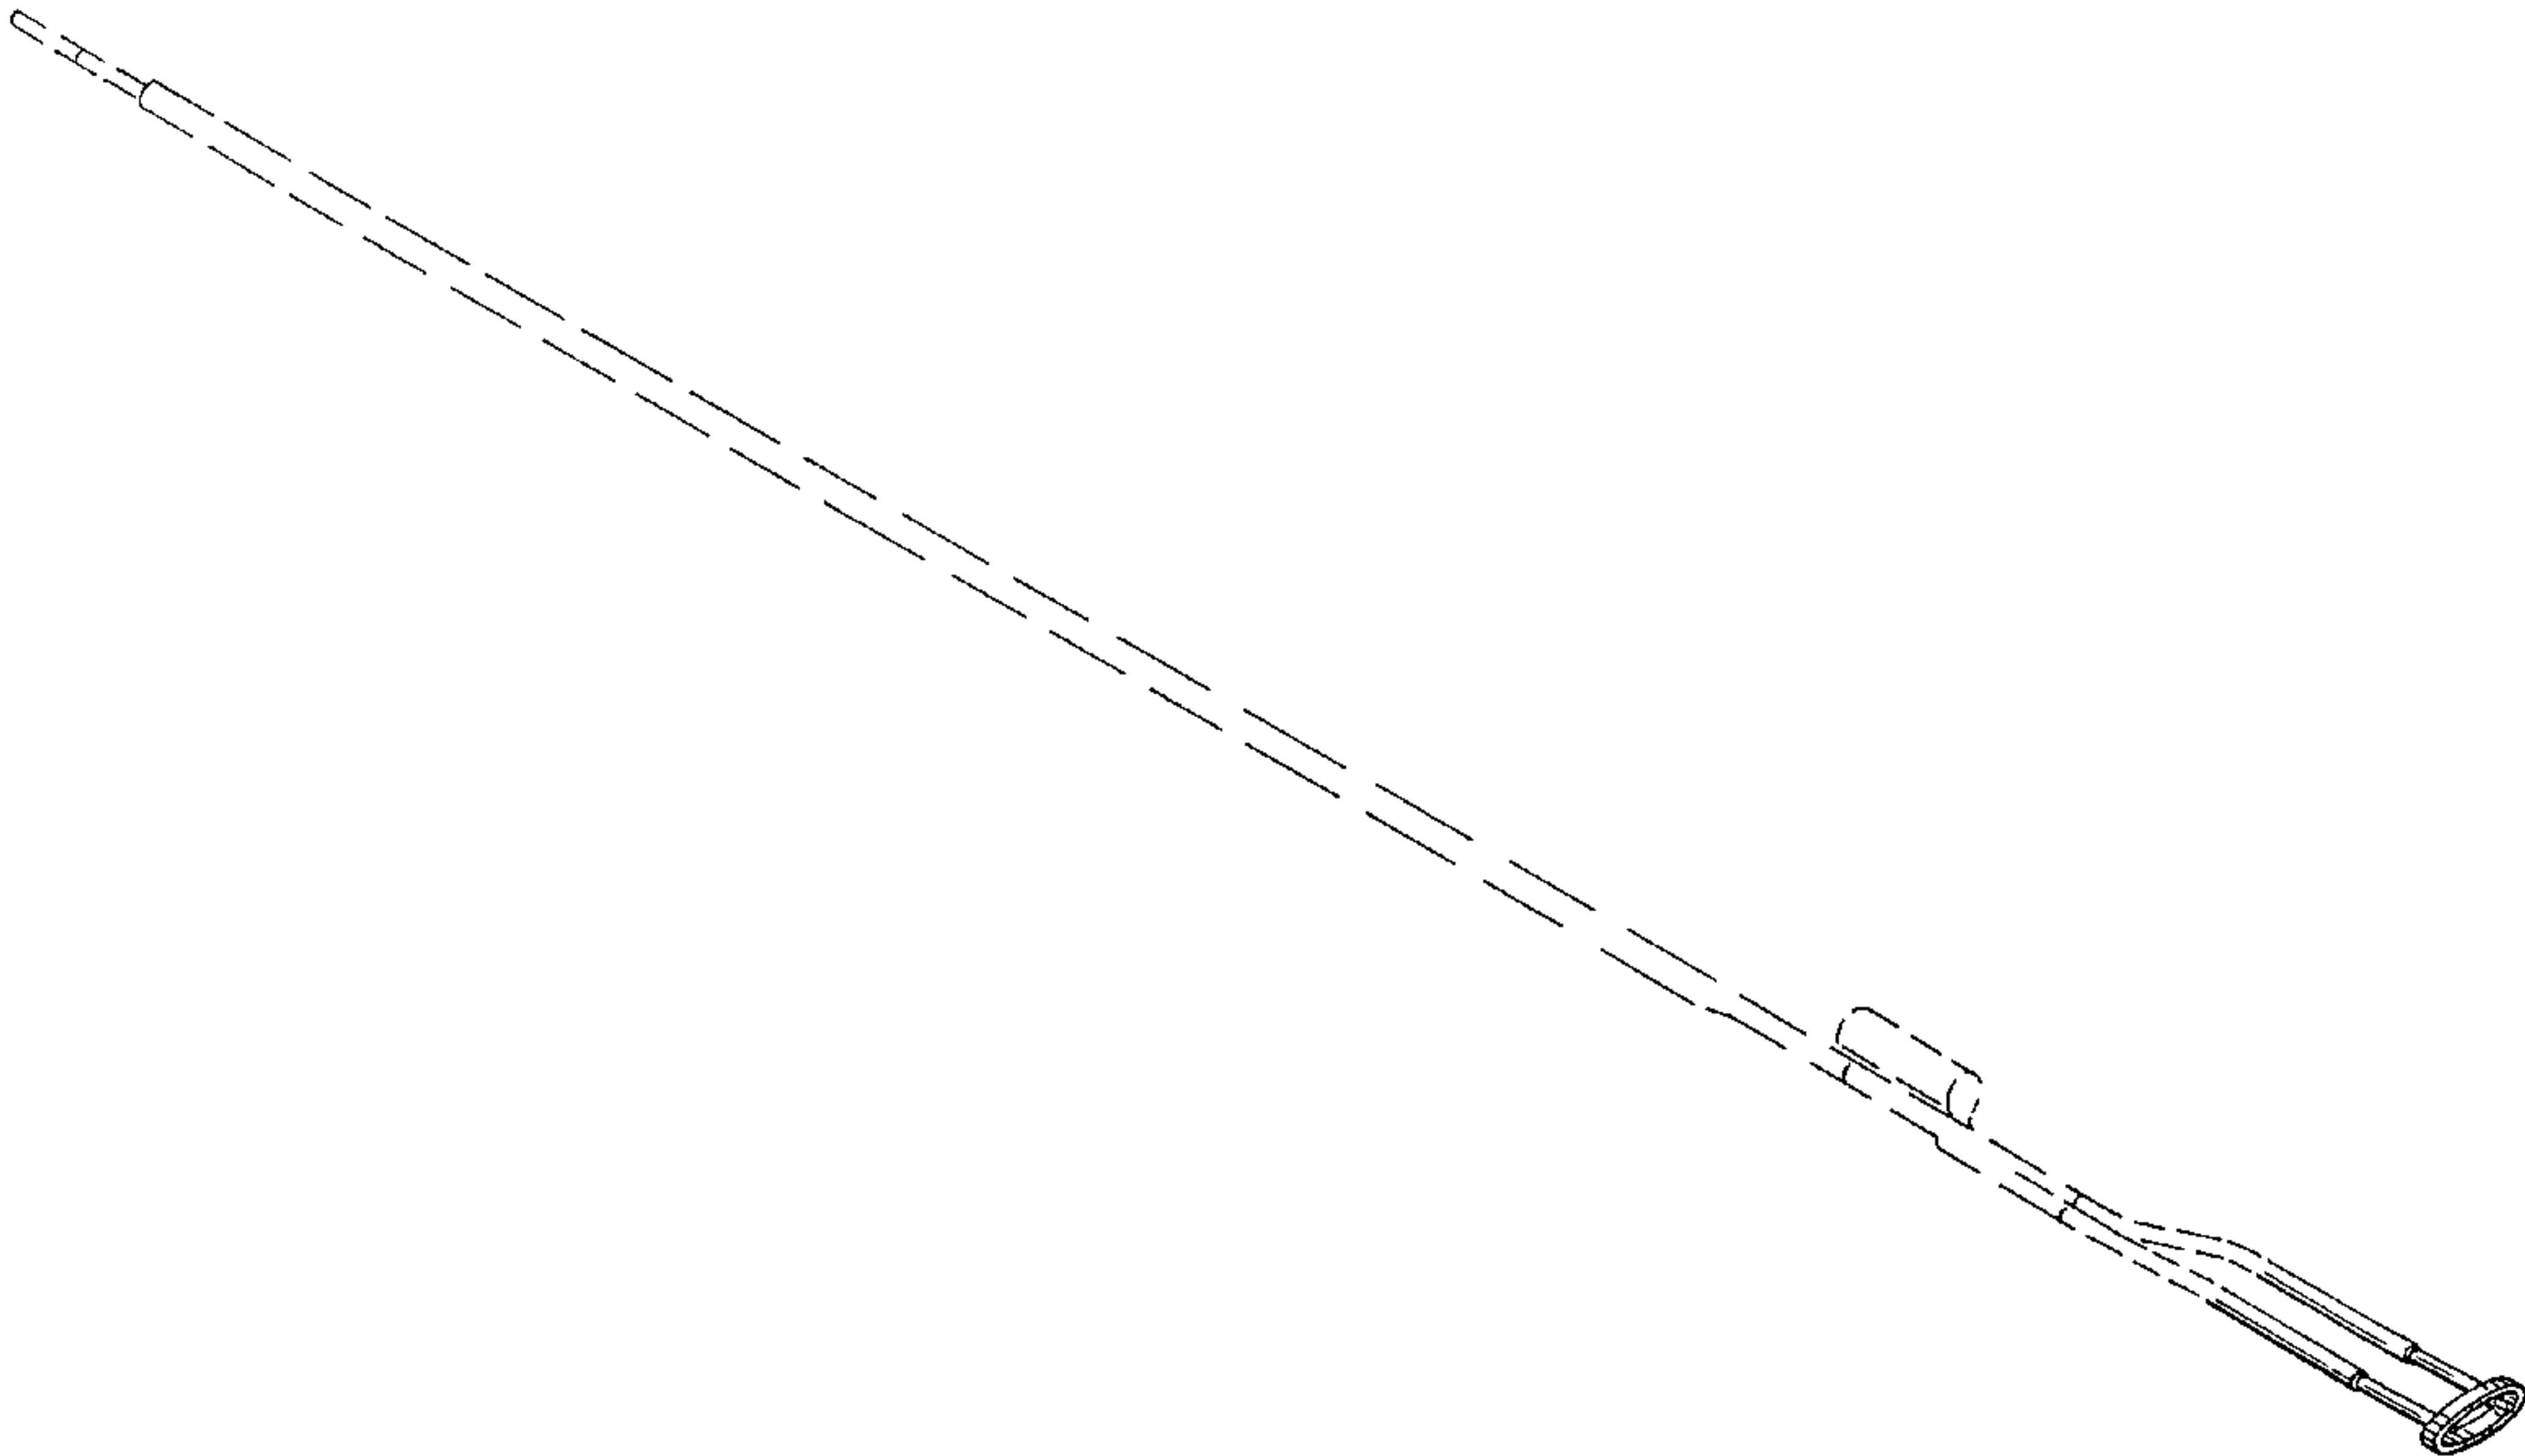

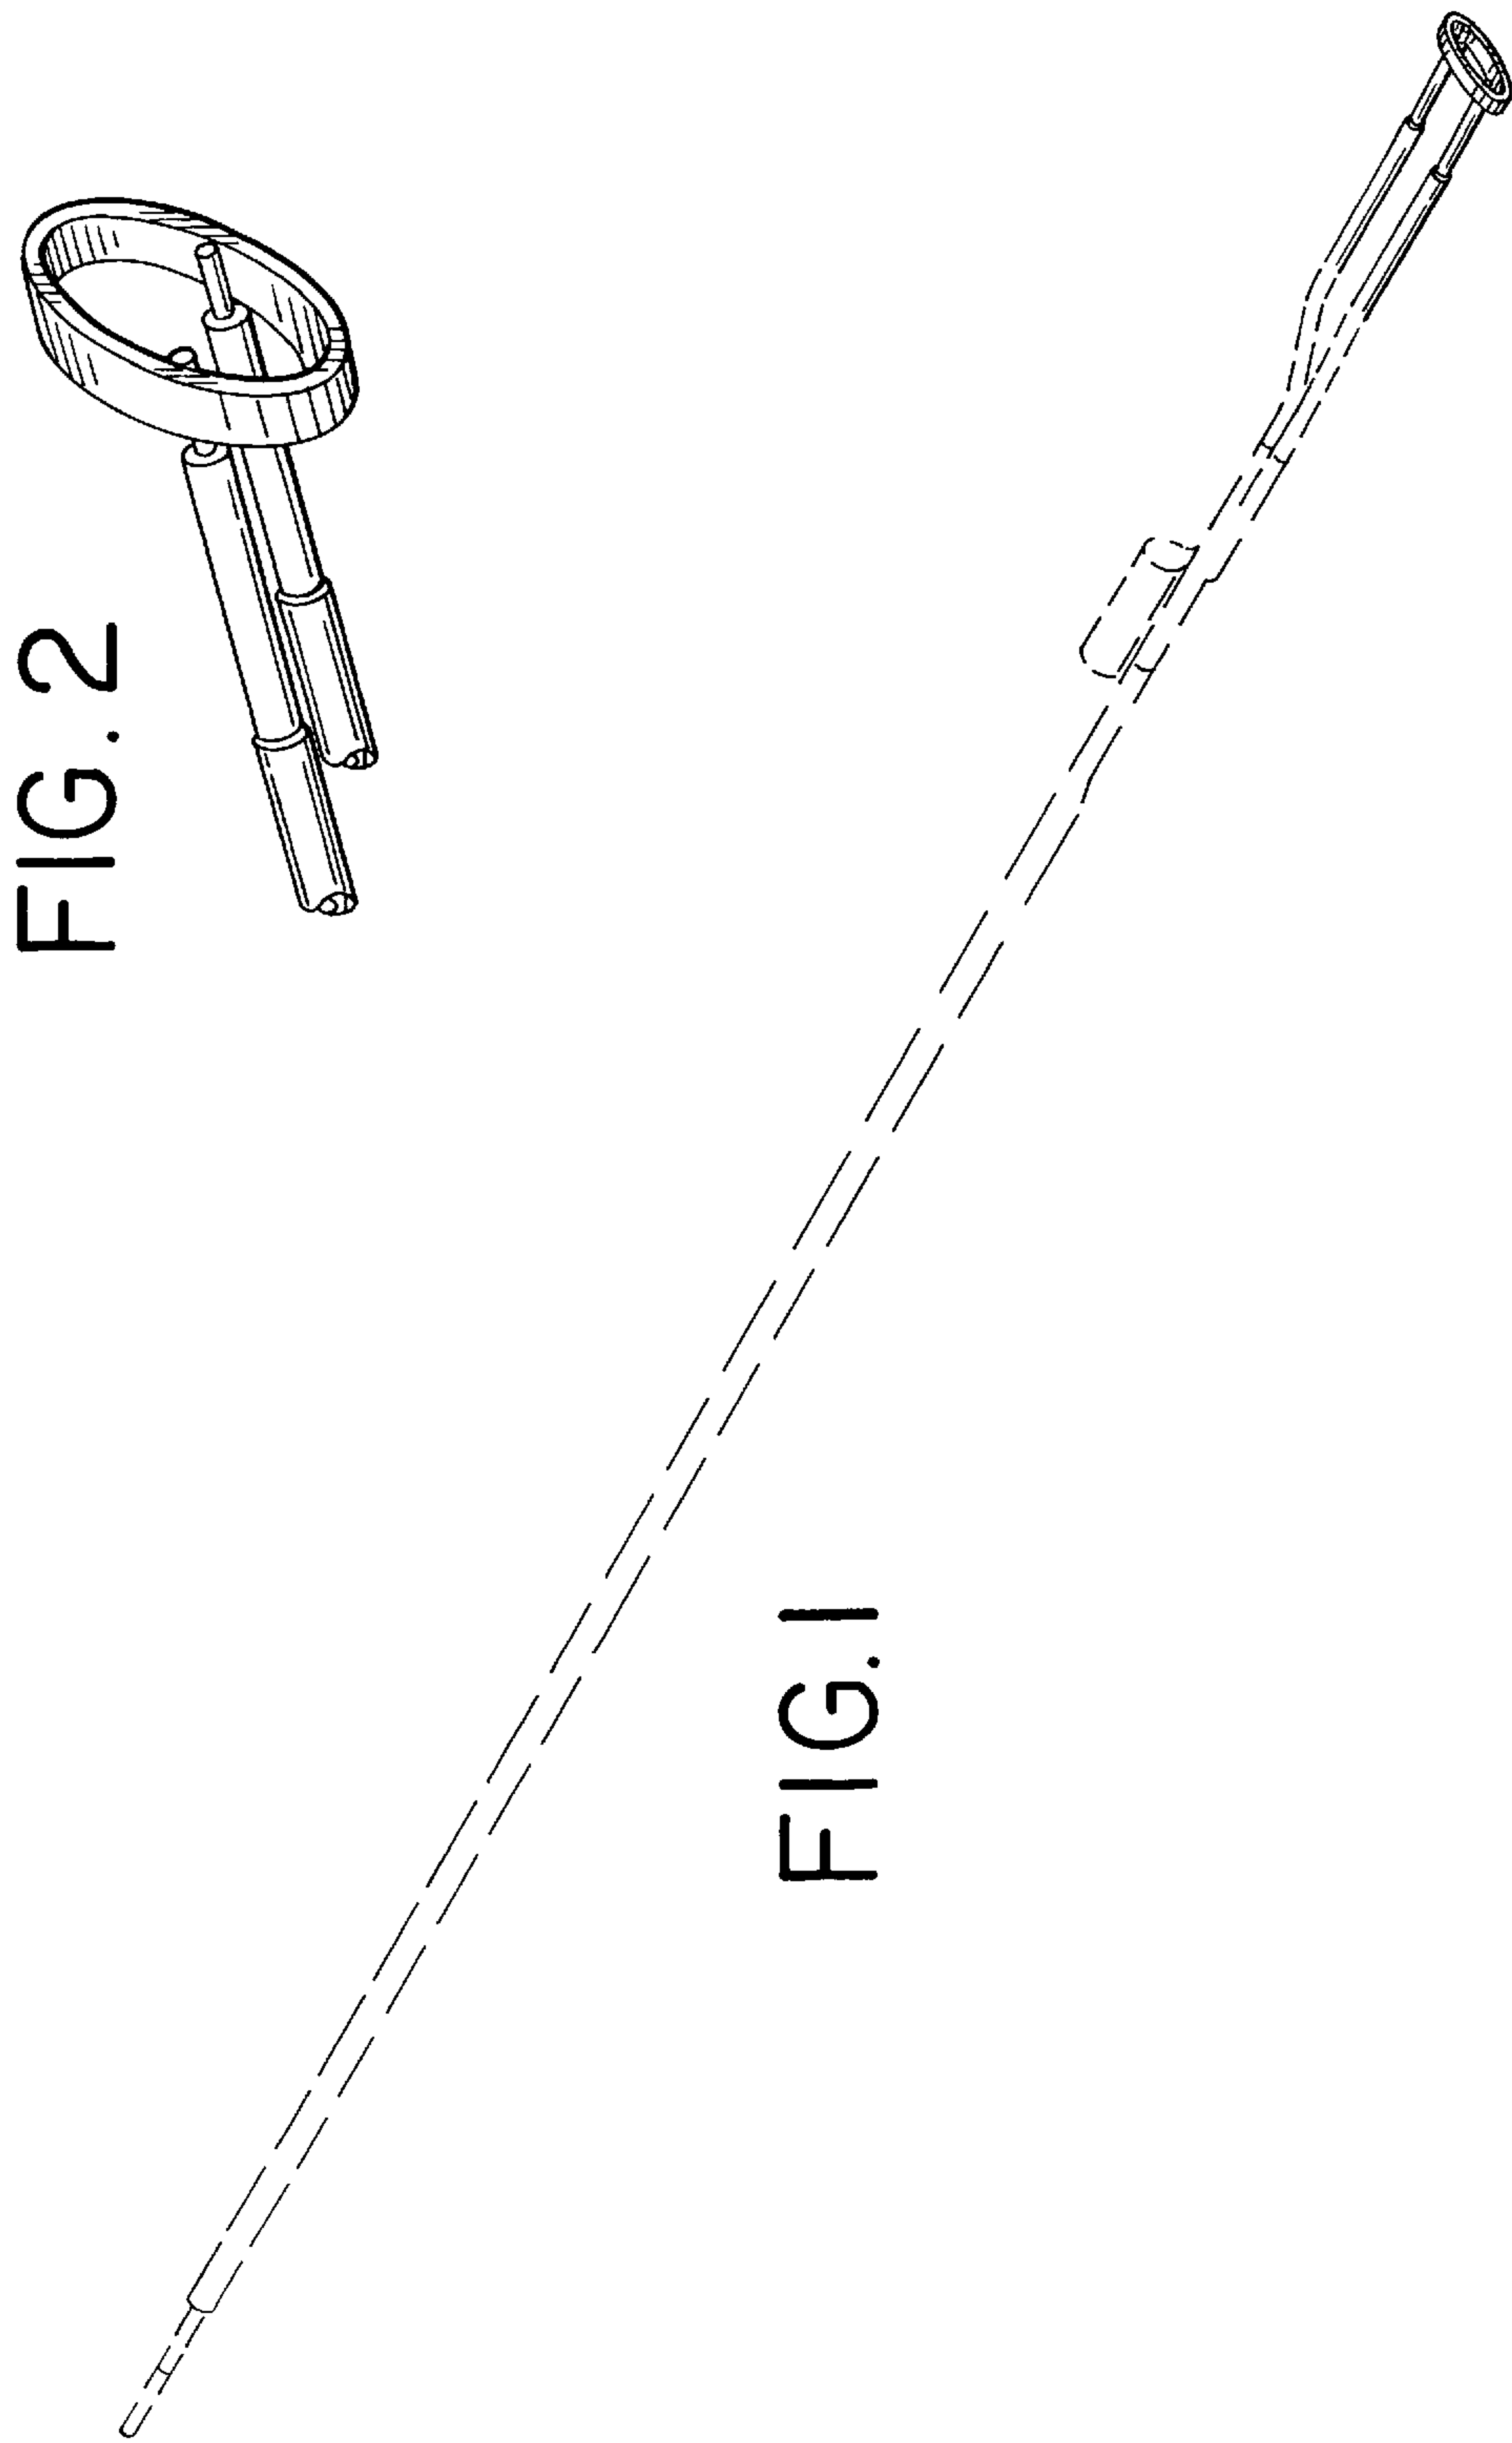


FIG. 7

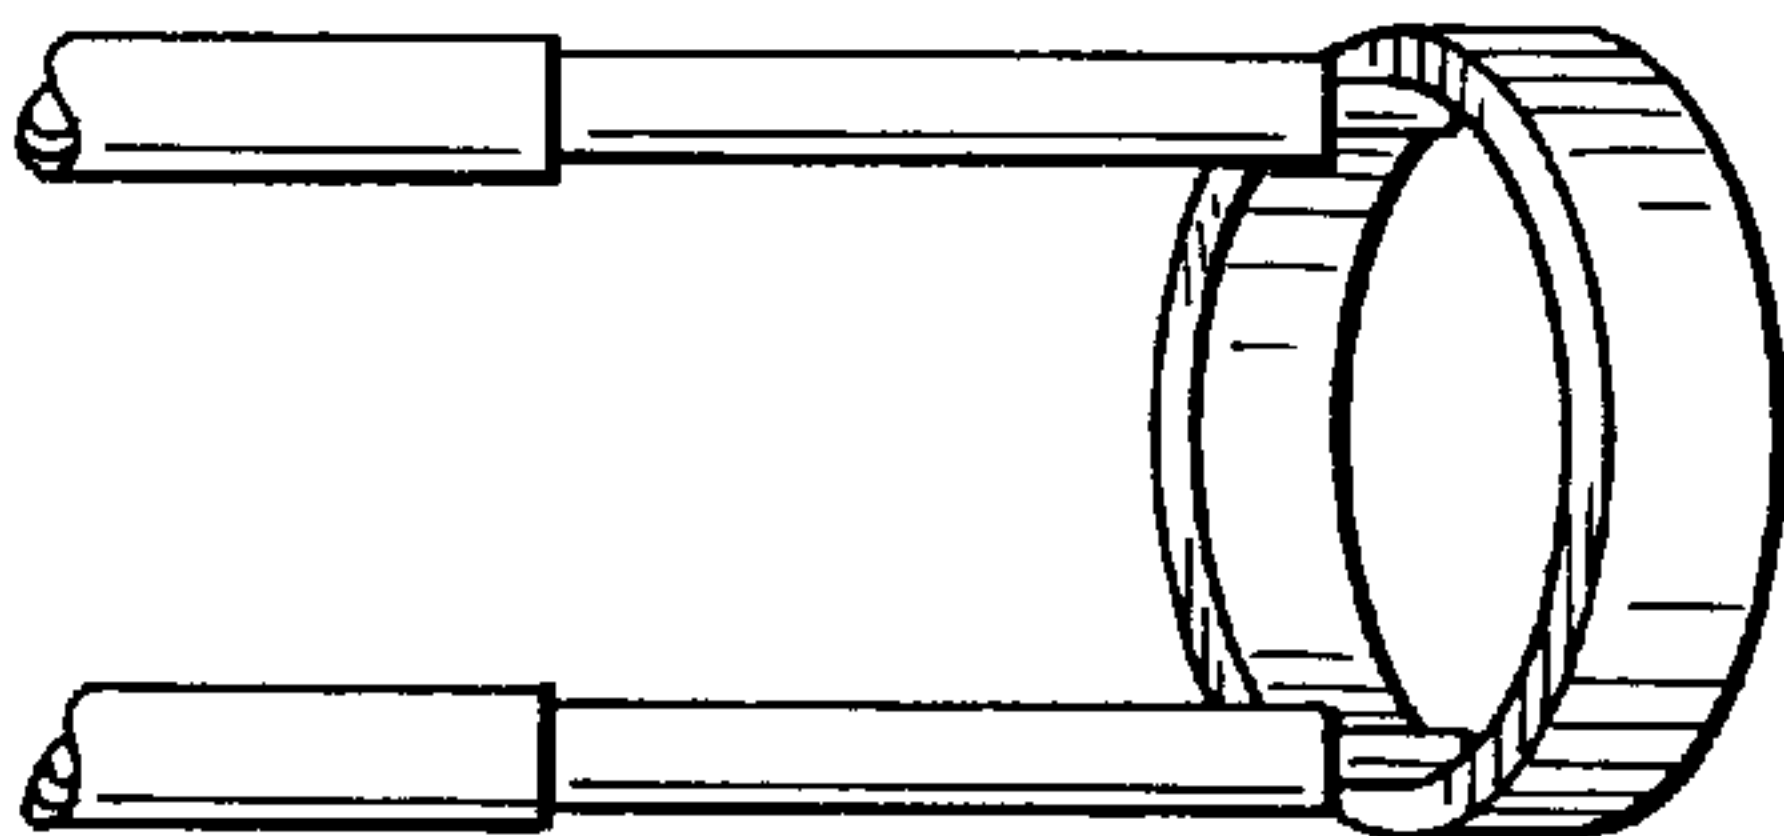


FIG. 4

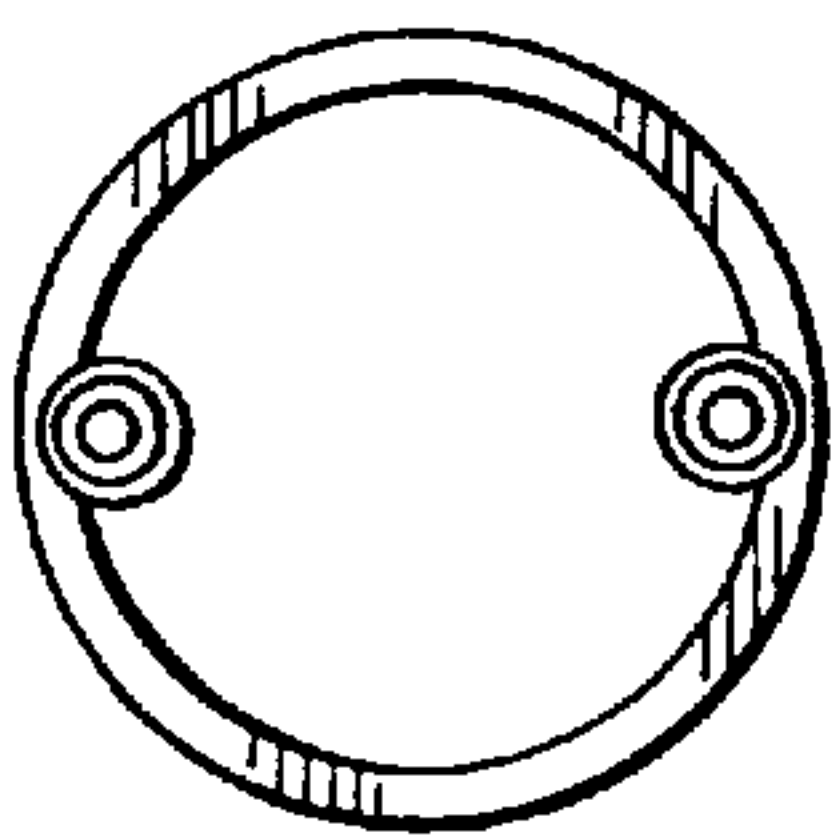


FIG. 3

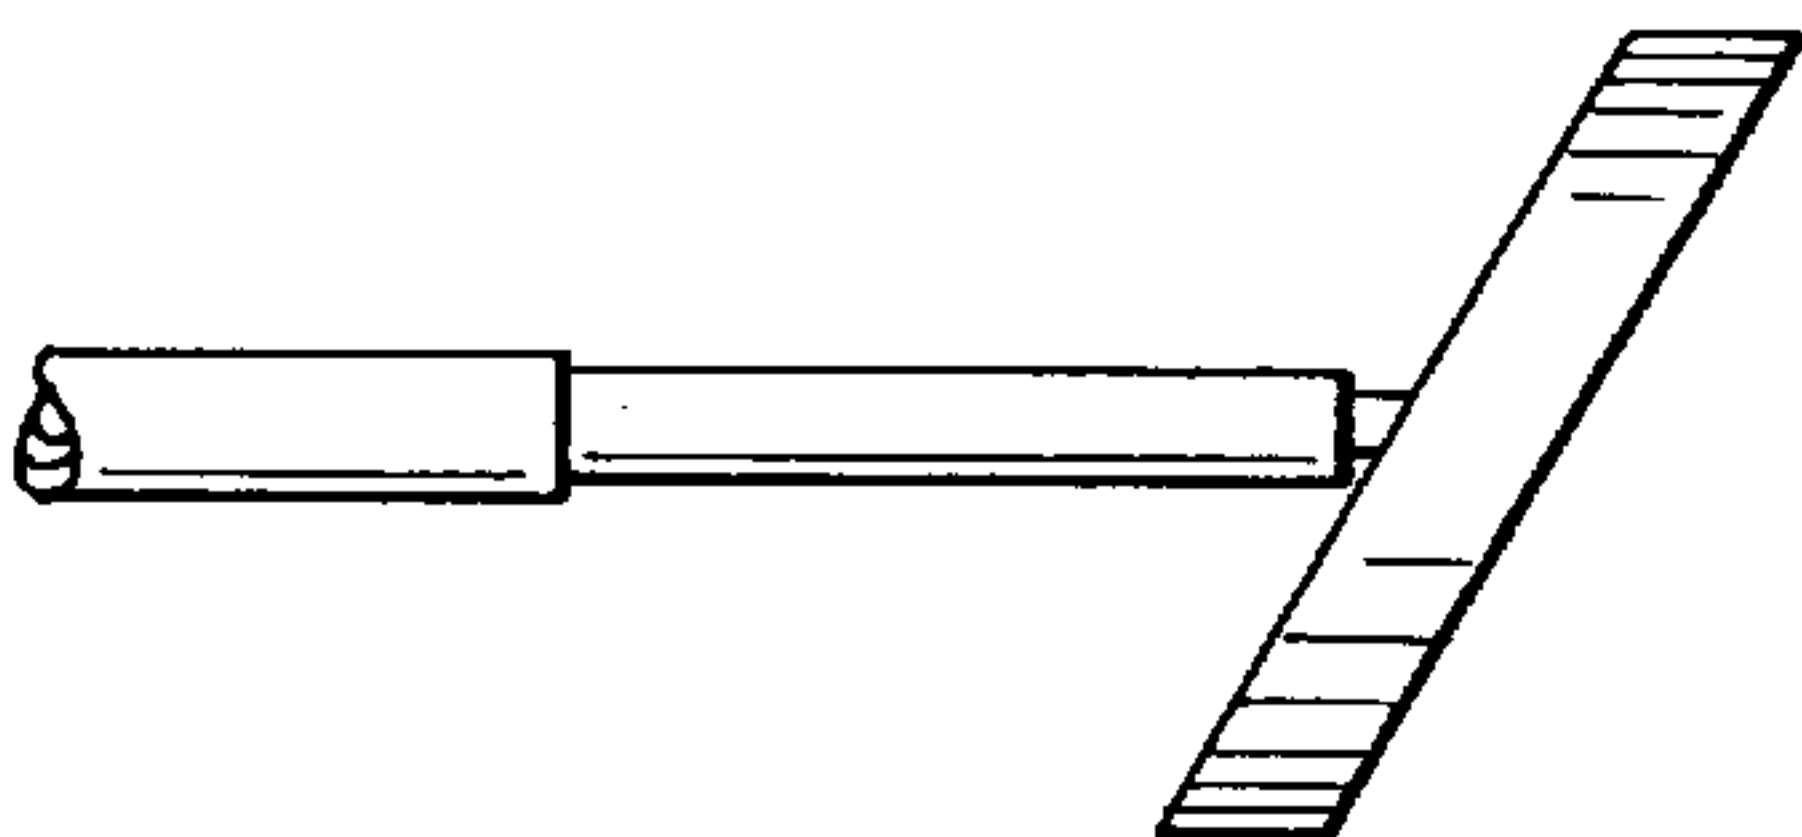


FIG. 5

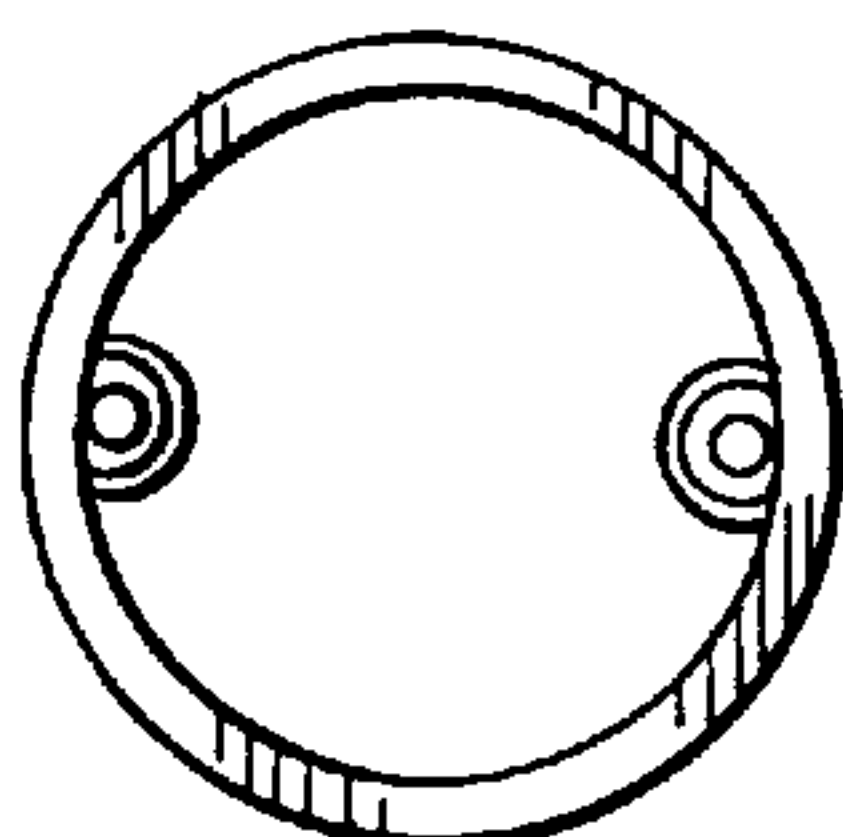


FIG. 6

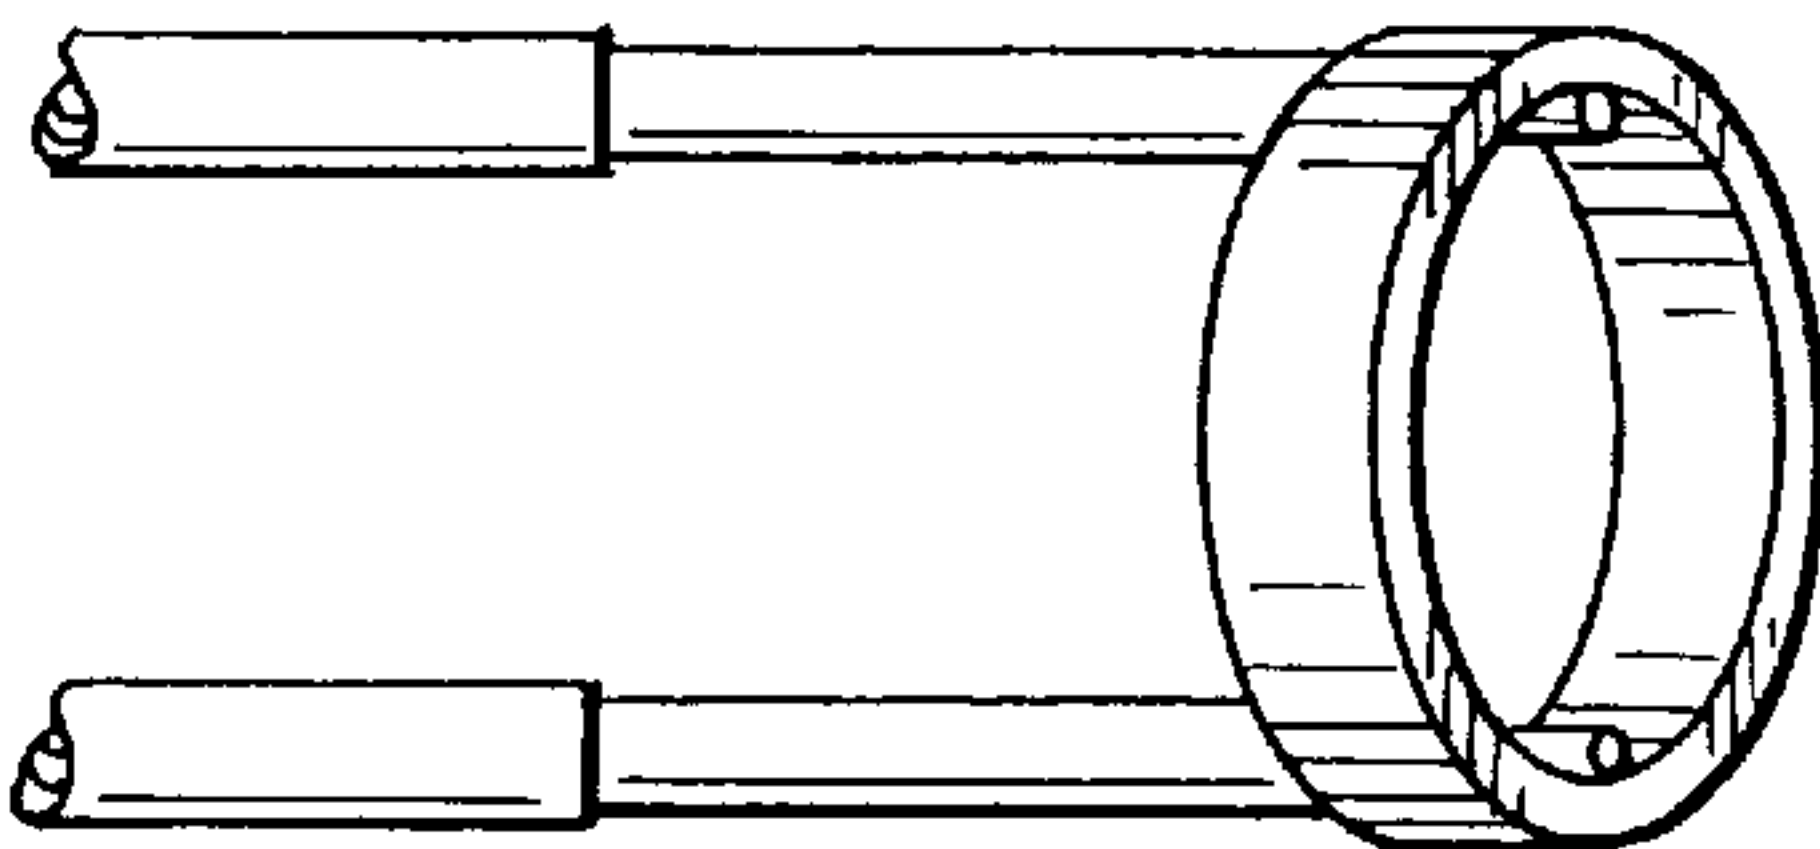


FIG.8

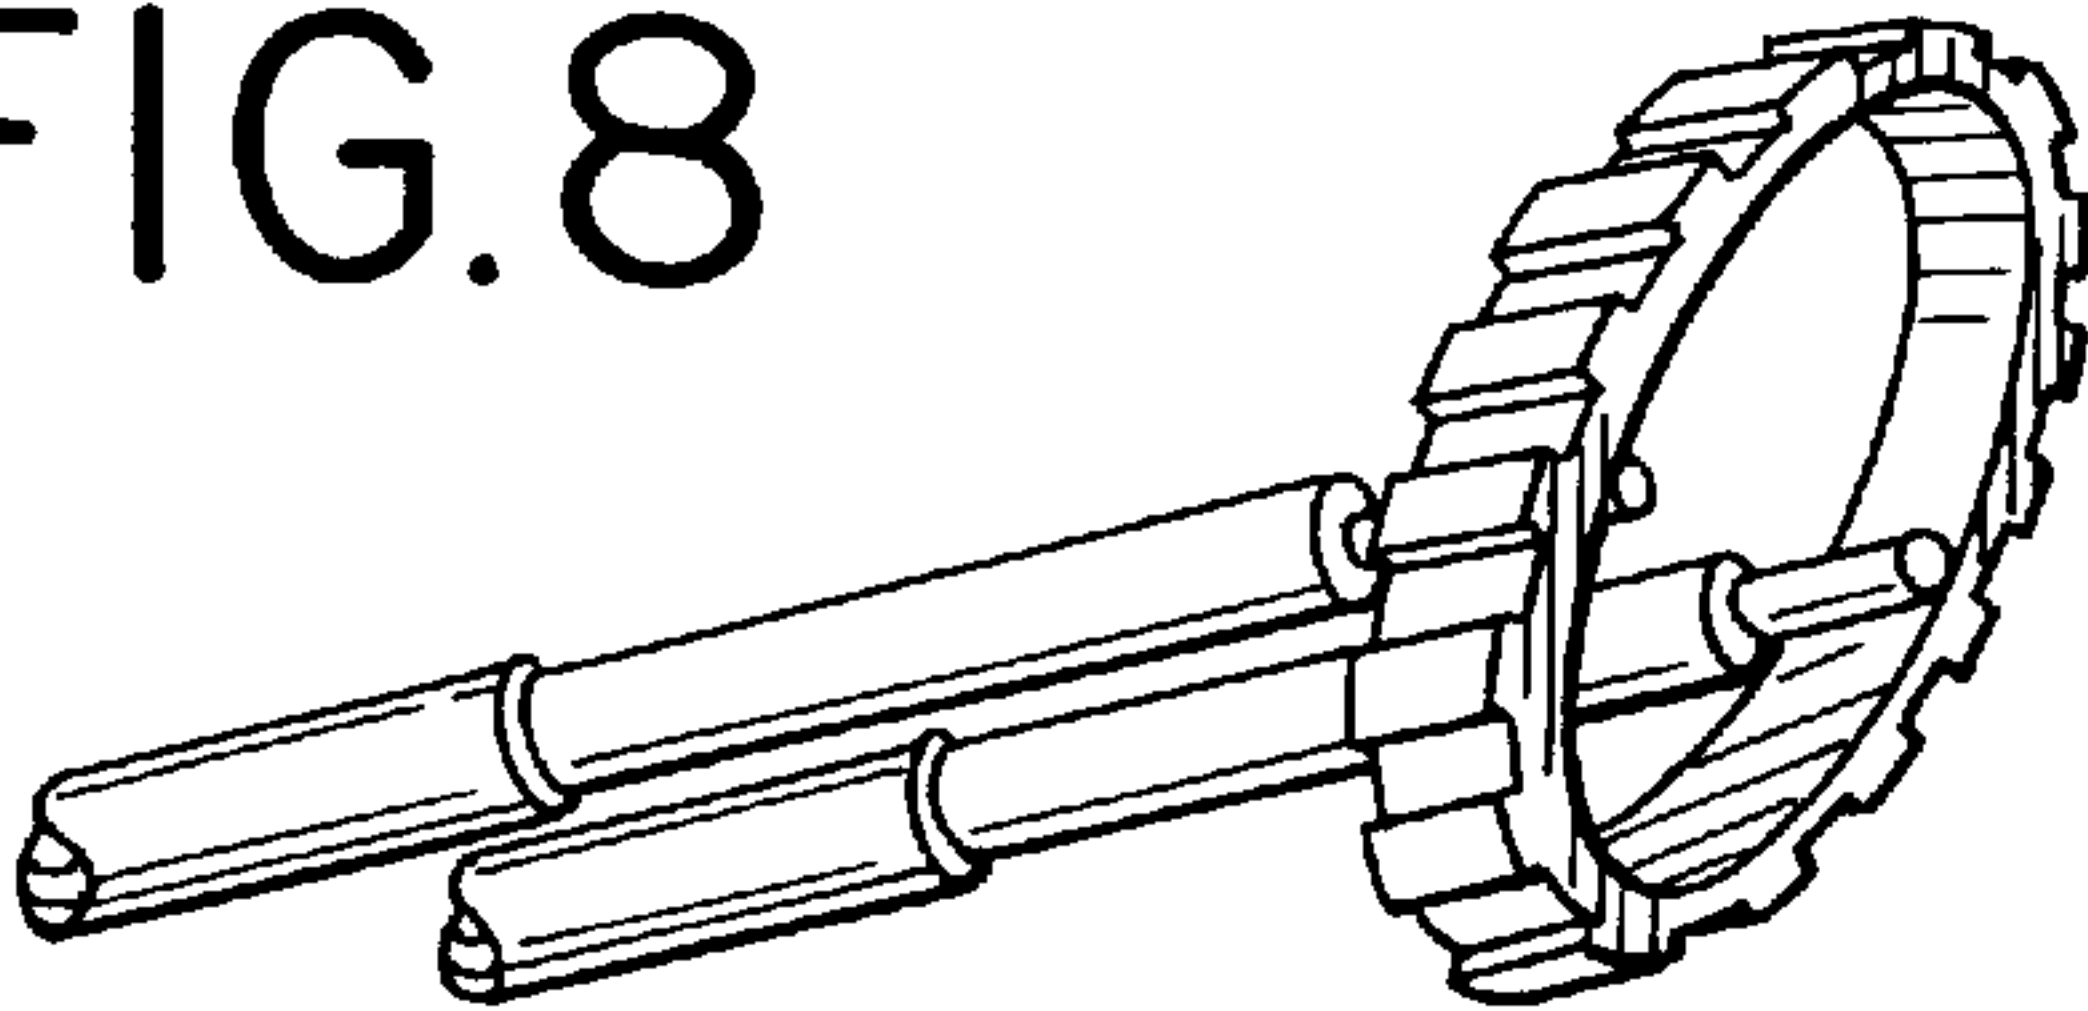


FIG. 9

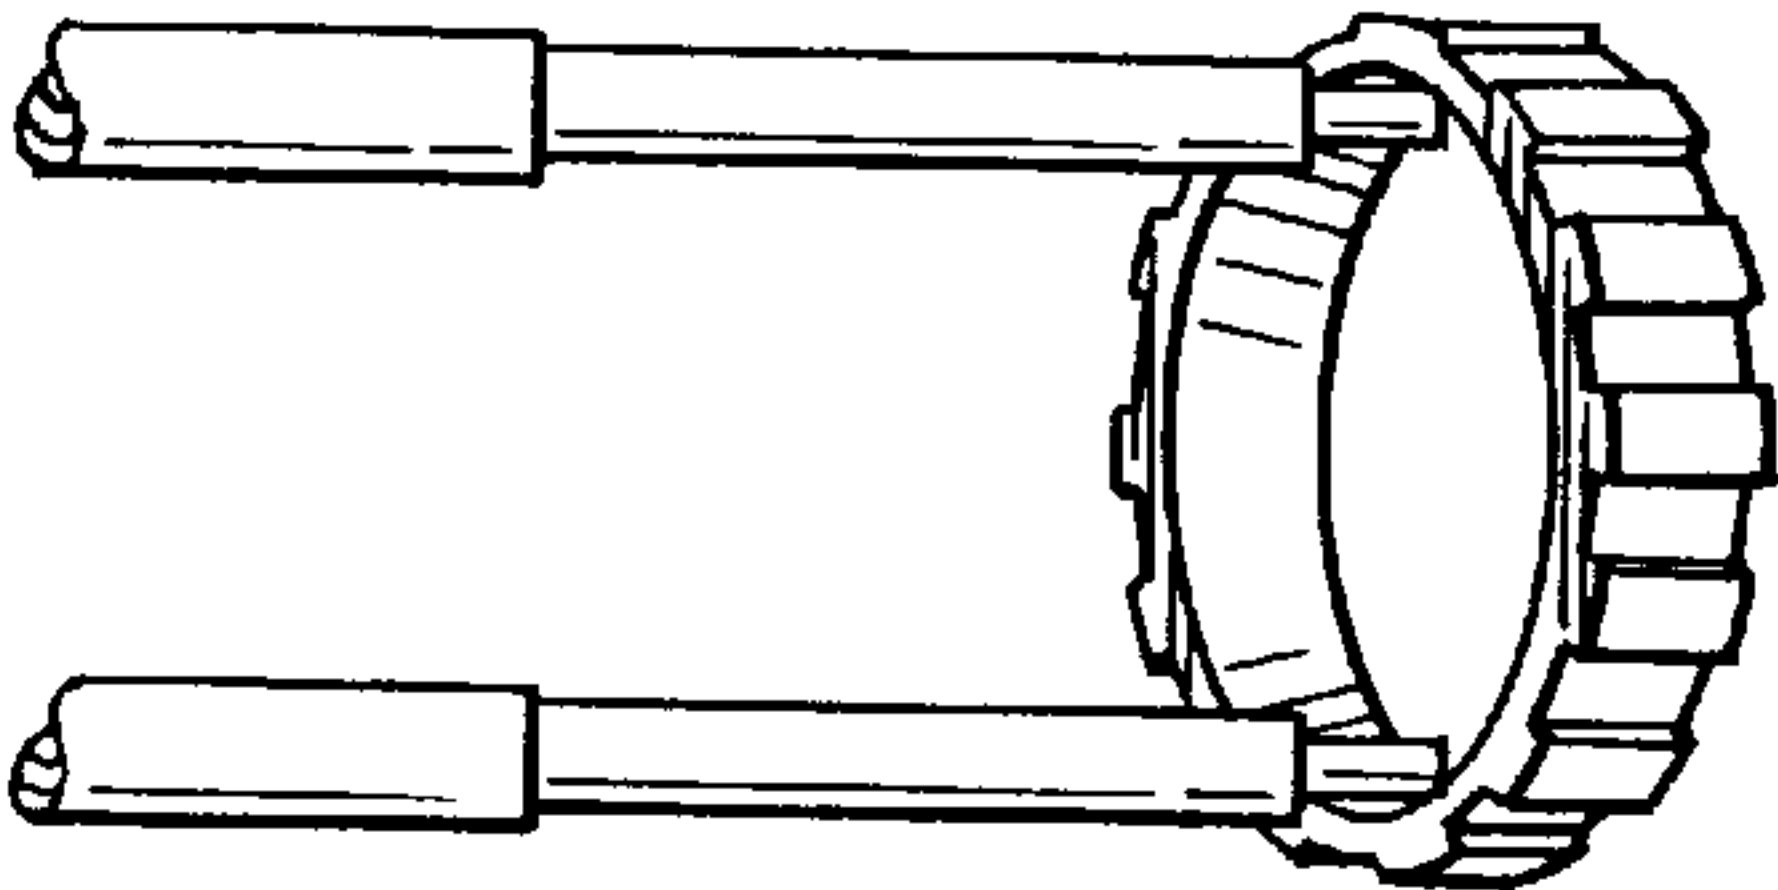


FIG. 10

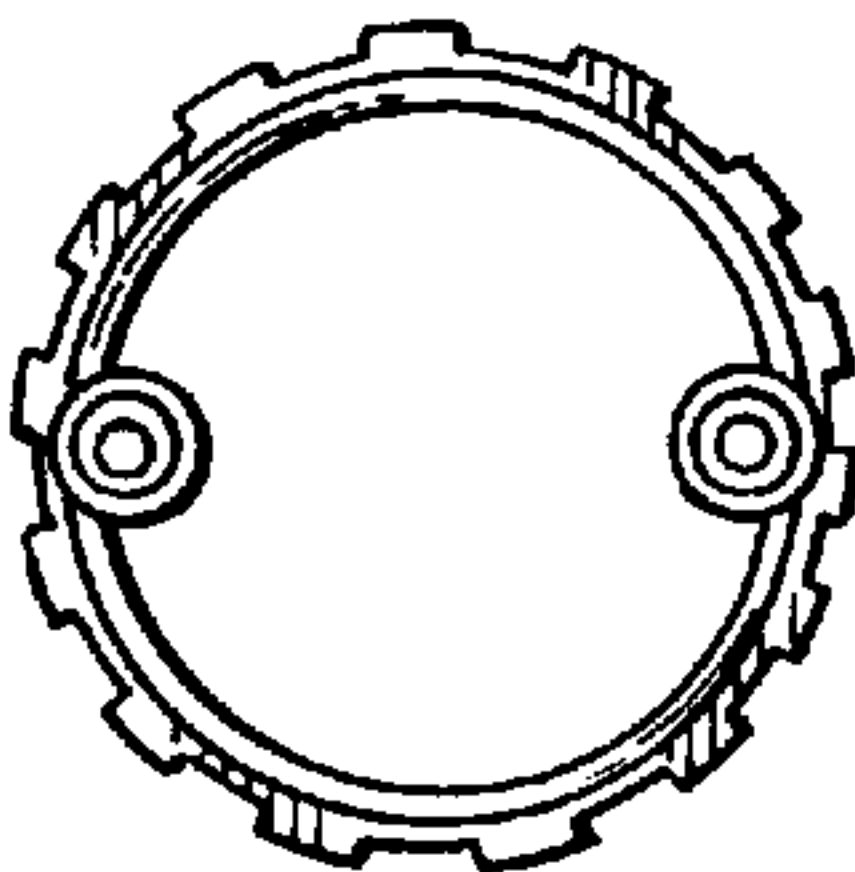


FIG. 11

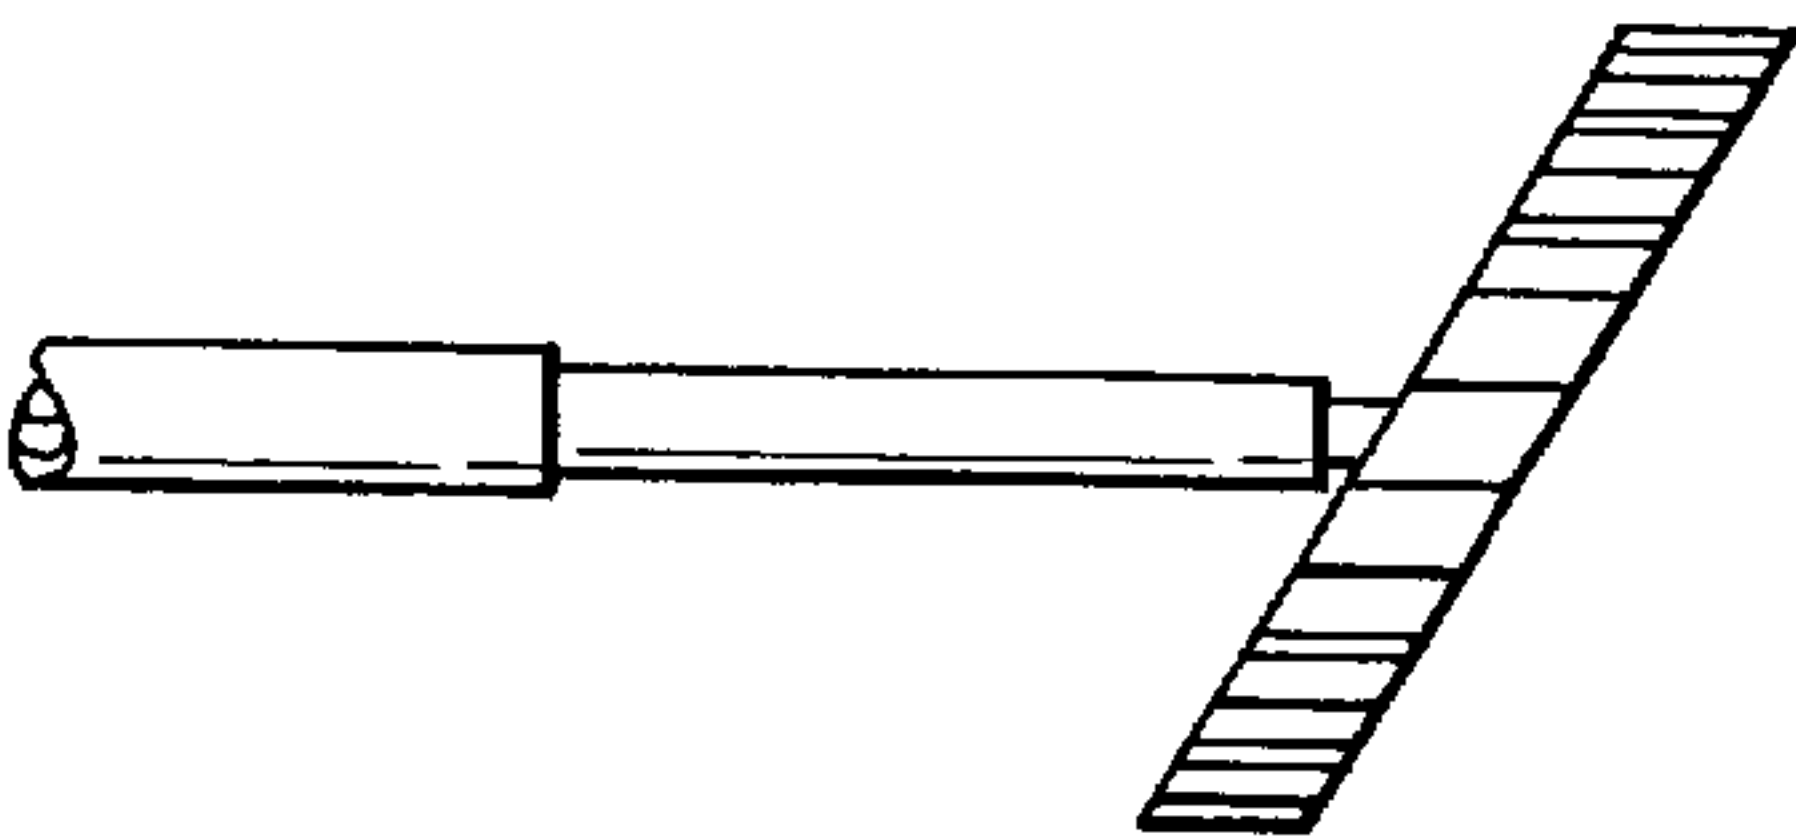


FIG. 12


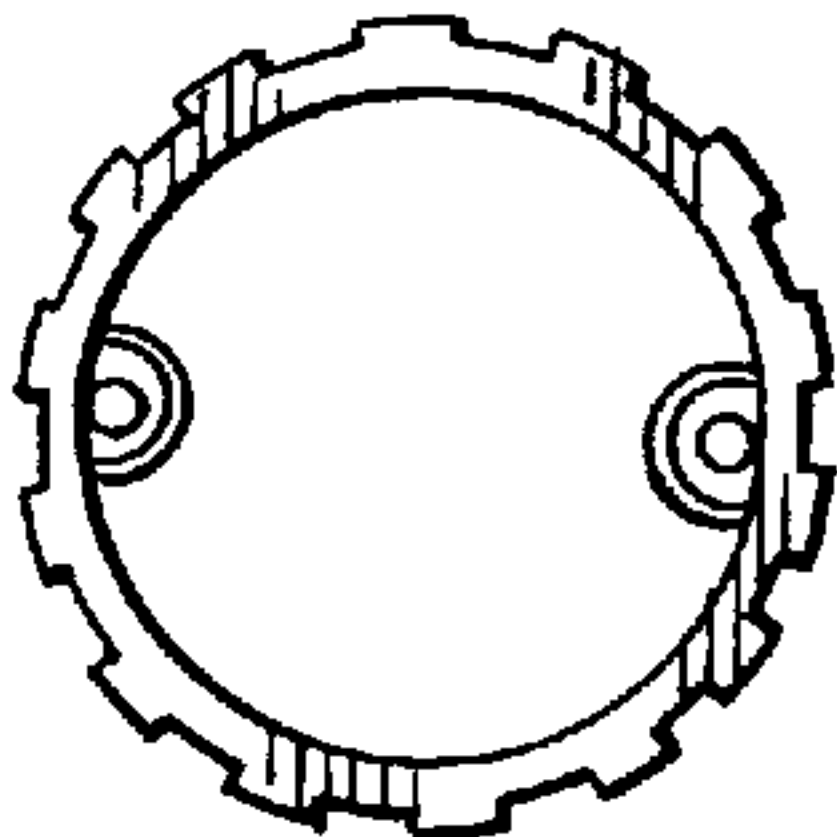


FIG. 13

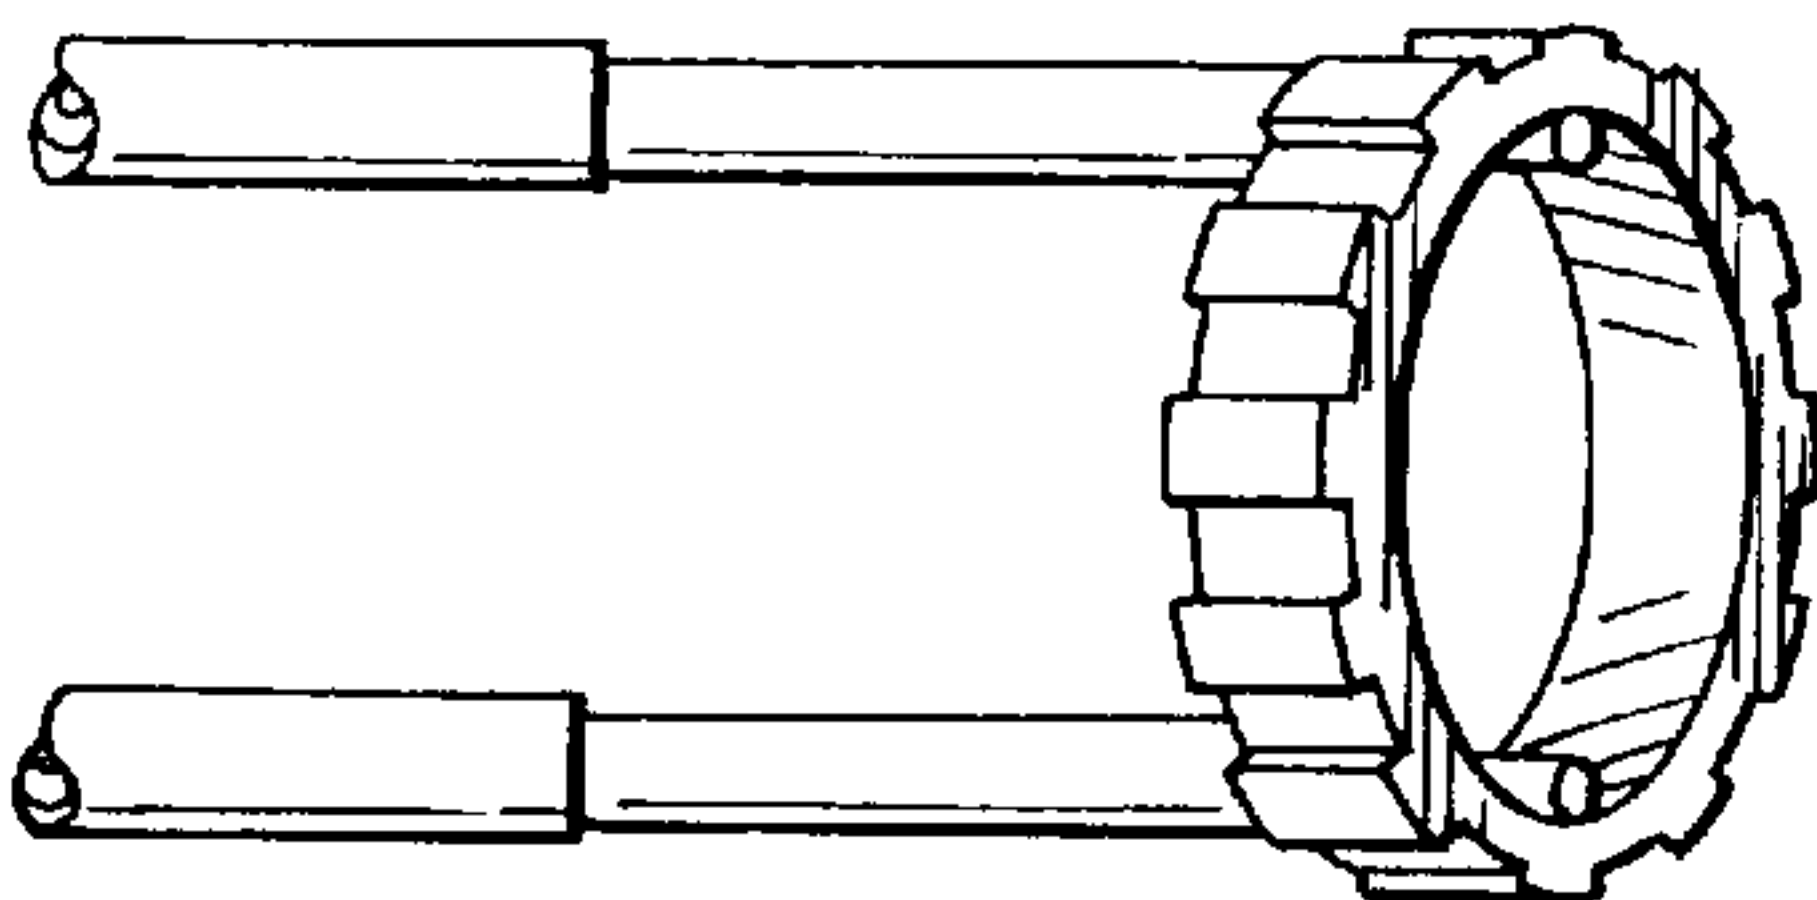

UNITED STATES PATENT AND TRADEMARK OFFICE
CERTIFICATE OF CORRECTION


PATENT NO. : Des. 401,338
DATED : November 17, 1998
INVENTOR(S) : Peter A. Manzie

It is certified that error appears in the above-identified patent and that said Letters Patent is hereby corrected as shown below:

On the Title Page,

In column 2, FIG. 8, line 15, under "**DESCRIPTION**",
please insert --close-up-- after "a".

Signed and Sealed this
Twentieth Day of March, 2001

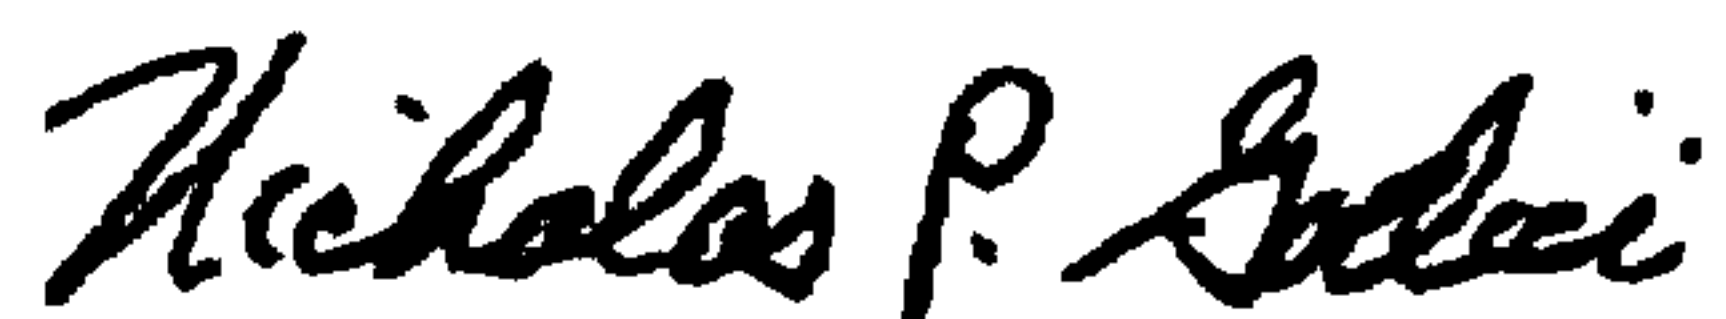

Attest:

NICHOLAS P. GODICI

Attesting Officer

Acting Director of the United States Patent and Trademark Office