



US00D401700S

United States Patent [19]
Gray et al.

[11] **Patent Number: Des. 401,700**
[45] **Date of Patent: **Nov. 24, 1998**

[54] **CONTAINER FOR USE WITH AN
AUTOMATIC ANALYZER**

5,437,841 8/1995 Balmer 422/102
5,571,479 11/1996 Koch 422/102

[75] Inventors: **Robert C. Gray; Linas P. Laurusonis,**
both of Gurnee; **Matthew L. Mittino,**
Evanston; **Jack F. Ramsey,** Grayslake;
Tahua Yang, Darien, all of Ill.

[73] Assignee: **Abbott Laboratories,** Abbott Park, Ill.

[**] Term: **14 Years**

[21] Appl. No.: **71,157**

[22] Filed: **May 22, 1997**

[51] **LOC (6) Cl. 24-02**

[52] **U.S. Cl. D24/224**

[58] **Field of Search D24/224, 216;**
D9/300, 520, 503, 504; 206/526; 402/102,
939, 940; 220/657; 356/246; 606/160; 215/382,
DIG. 3

[56] **References Cited**

U.S. PATENT DOCUMENTS

D. 278,182	3/1985	Aihara et al.	D24/29
D. 283,728	5/1986	Aihara	D24/29
D. 288,845	3/1987	Borer et al.	D24/29
D. 330,428	10/1992	Lewis et al.	D24/224
D. 342,793	12/1993	Balmer	D24/224
D. 344,138	2/1994	Nagata	D24/224
4,229,104	10/1980	Lahme et al.	356/246
4,332,471	6/1982	Gross	356/246
4,560,269	12/1985	Baldszun et al.	356/246
4,634,576	1/1987	Gallee et al.	422/102
4,639,135	1/1987	Borer et al.	356/246
5,098,661	3/1992	Froehlich et al.	422/102
5,104,807	4/1992	Mitsumaki et al.	436/47

FOREIGN PATENT DOCUMENTS

0019870	12/1980	European Pat. Off. .
0100663	2/1984	European Pat. Off. .
0106662	4/1984	European Pat. Off. .
0152964	8/1985	European Pat. Off. .
0209490	7/1986	European Pat. Off. .
0502638A2	9/1992	European Pat. Off. .
0502638A3	9/1992	European Pat. Off. .
0512368	11/1992	European Pat. Off. .
0512368A2	11/1992	European Pat. Off. .
0512368A3	11/1992	European Pat. Off. .
2523320	3/1983	France .
1322728	11/1973	United Kingdom .
9005903	5/1990	WIPO .
9205448	4/1992	WIPO .

Primary Examiner—Louis S. Zarfes
Assistant Examiner—G. Andoll
Attorney, Agent, or Firm—Mark C. Bach

[57] **CLAIM**

We claim the ornamental design for container for use with an automatic analyzer, as shown and as described.

DESCRIPTION

FIG. 1 is a perspective view of the container for use with an automatic analyzer;
FIG. 2 is a side view thereof, at a scale slightly larger than that of FIG. 1, the opposite side being identical;
FIG. 3 is a top view thereof;
FIG. 4 is a bottom view thereof; and,
FIG. 5 is a side view rotated 90 degrees with respect to FIG. 2, the opposite side being identical.

1 Claim, 2 Drawing Sheets

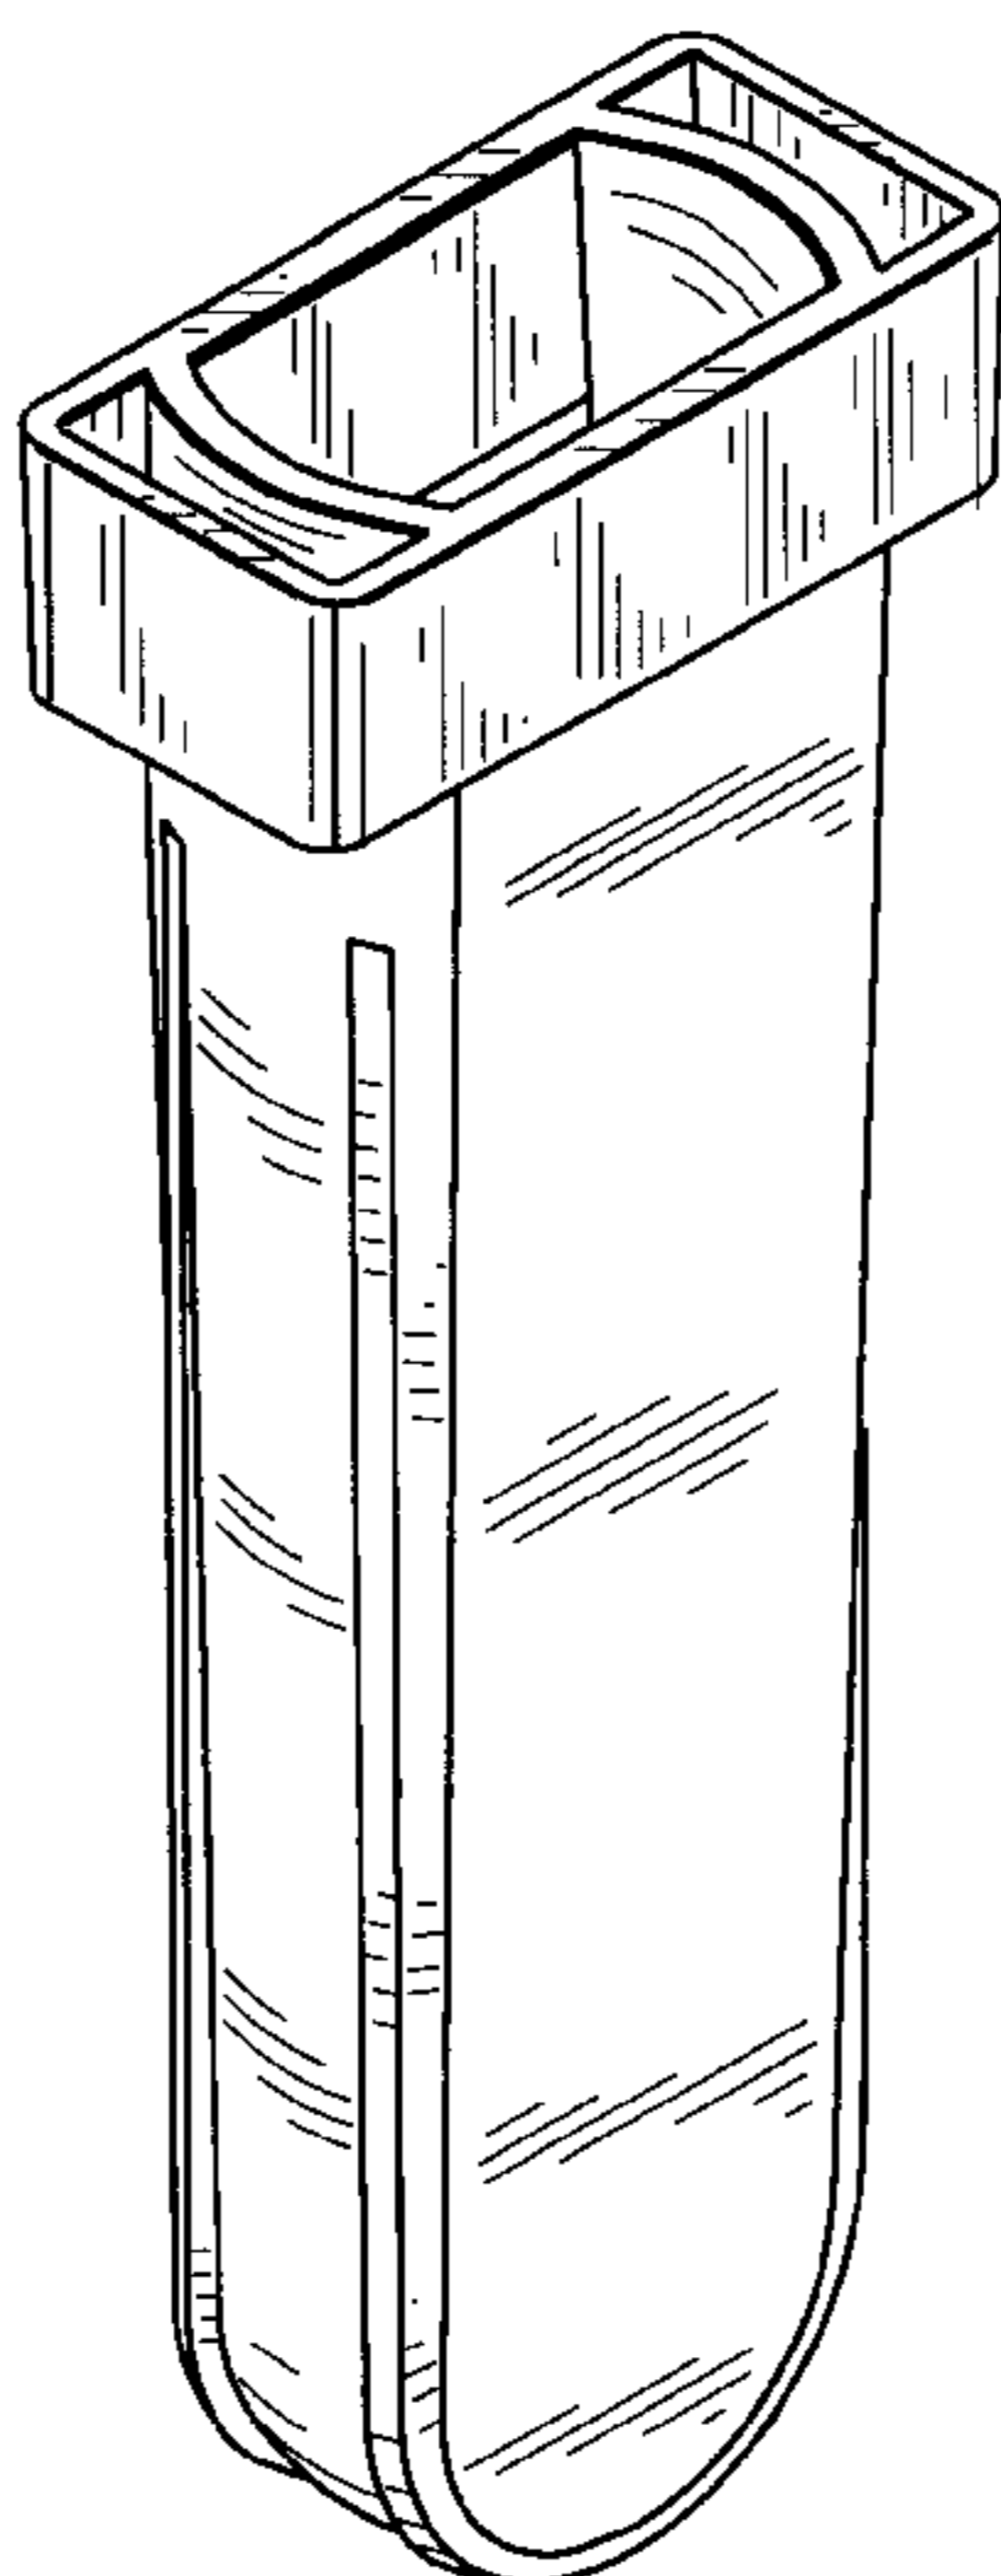


FIG. 1

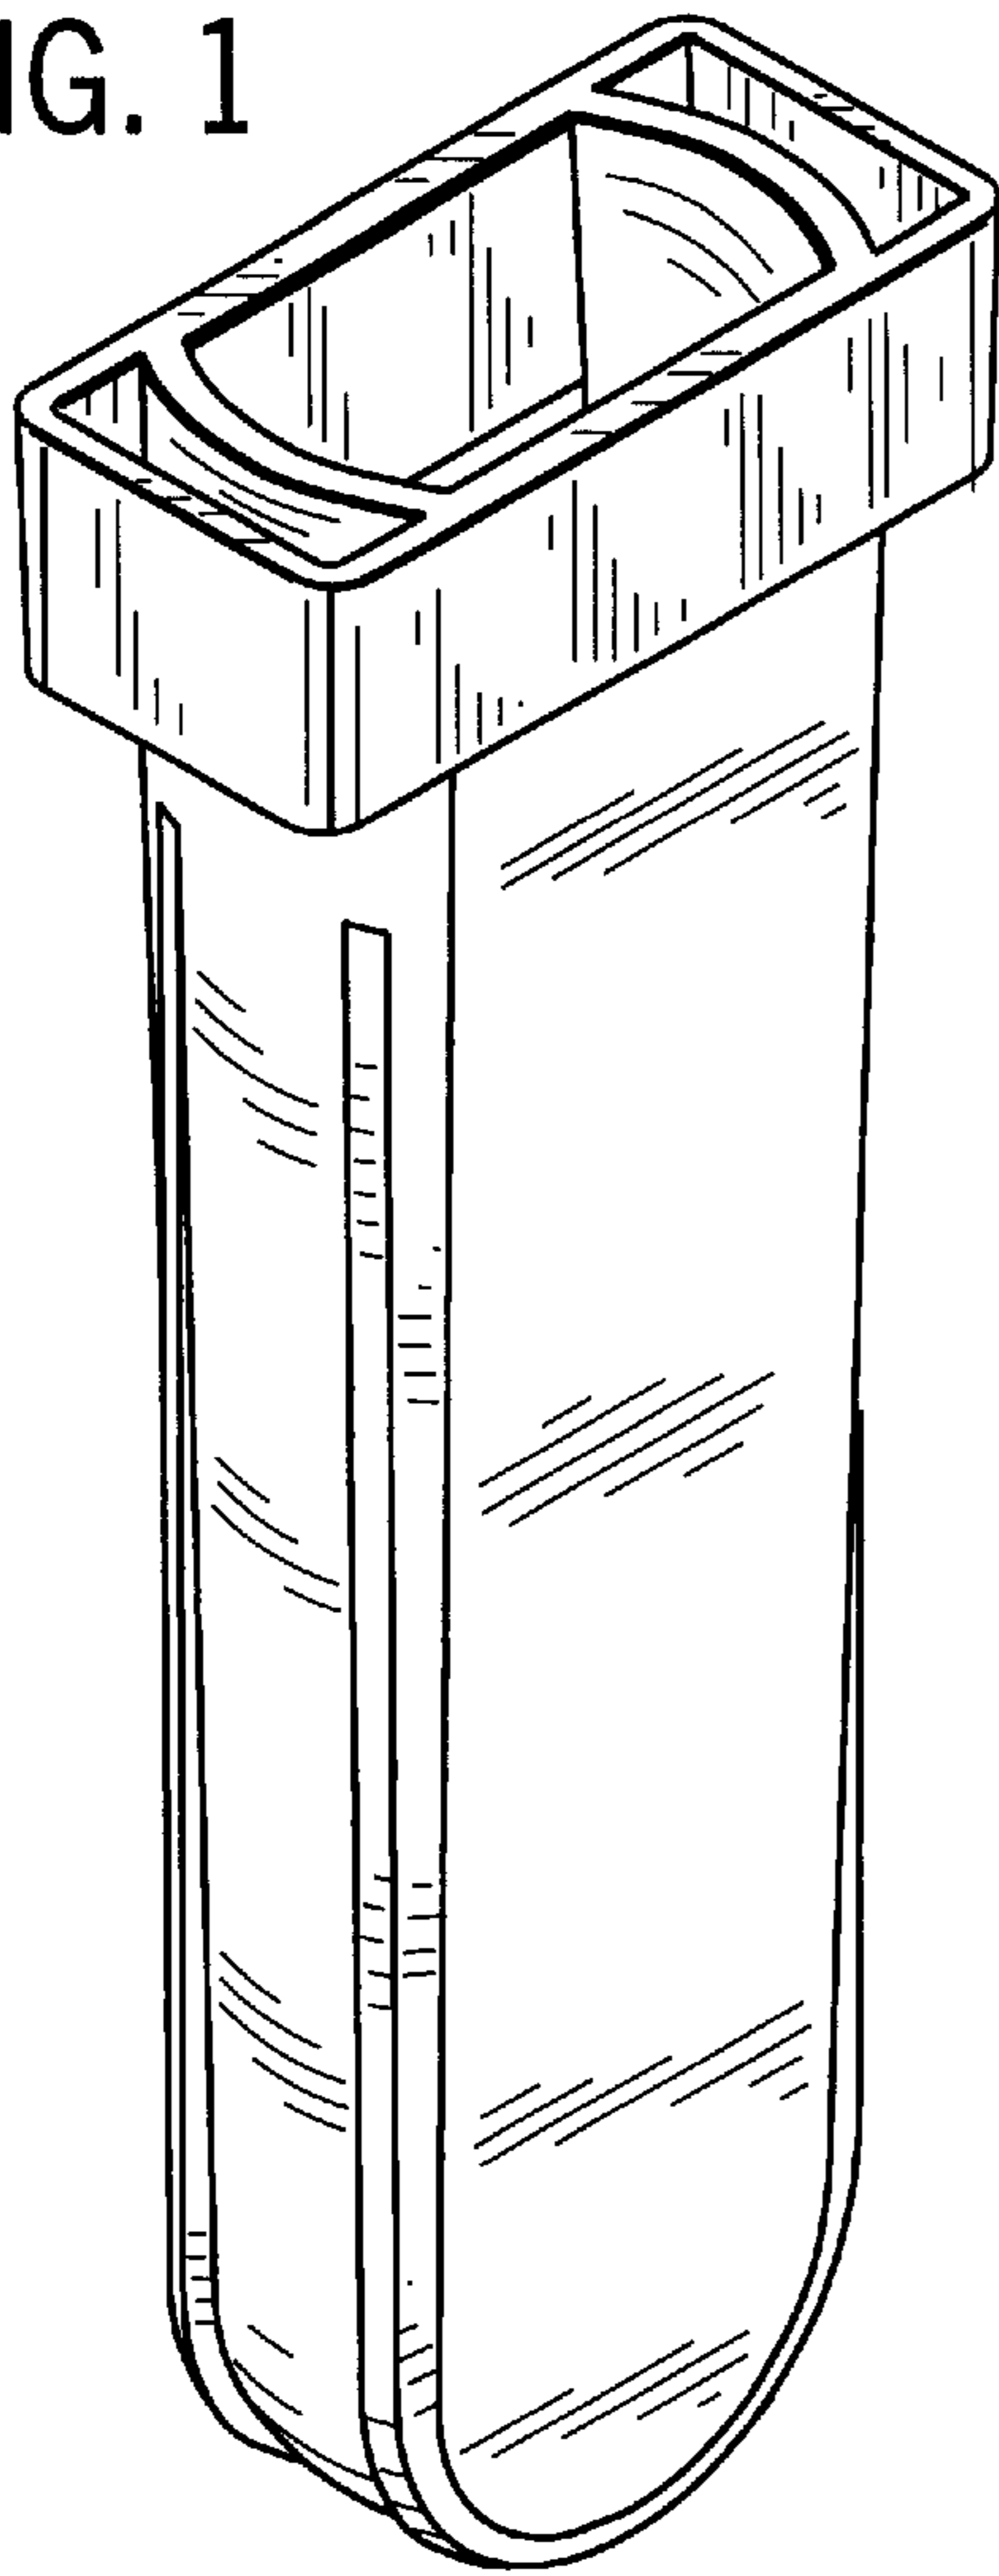


FIG. 2

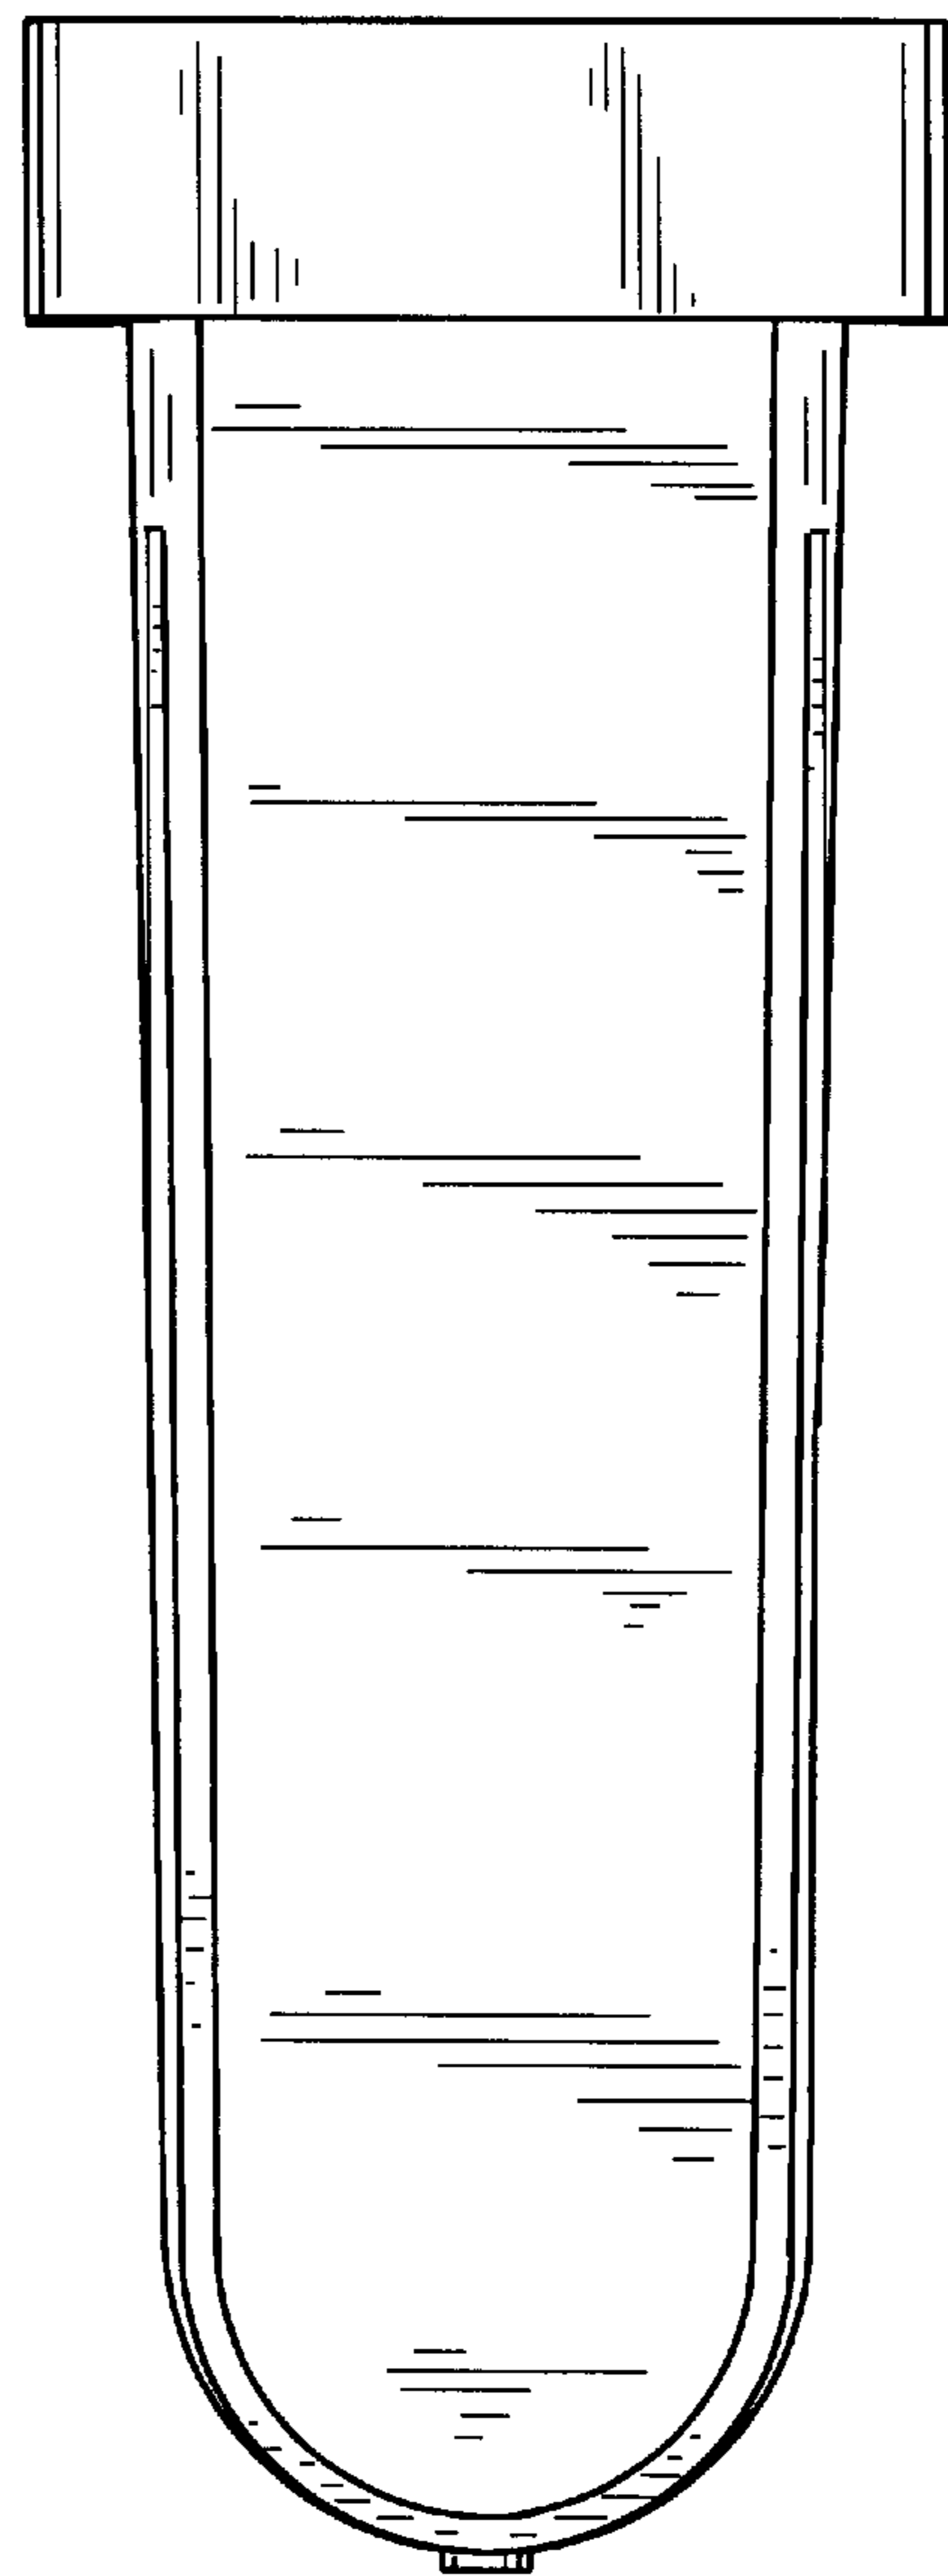


FIG. 3

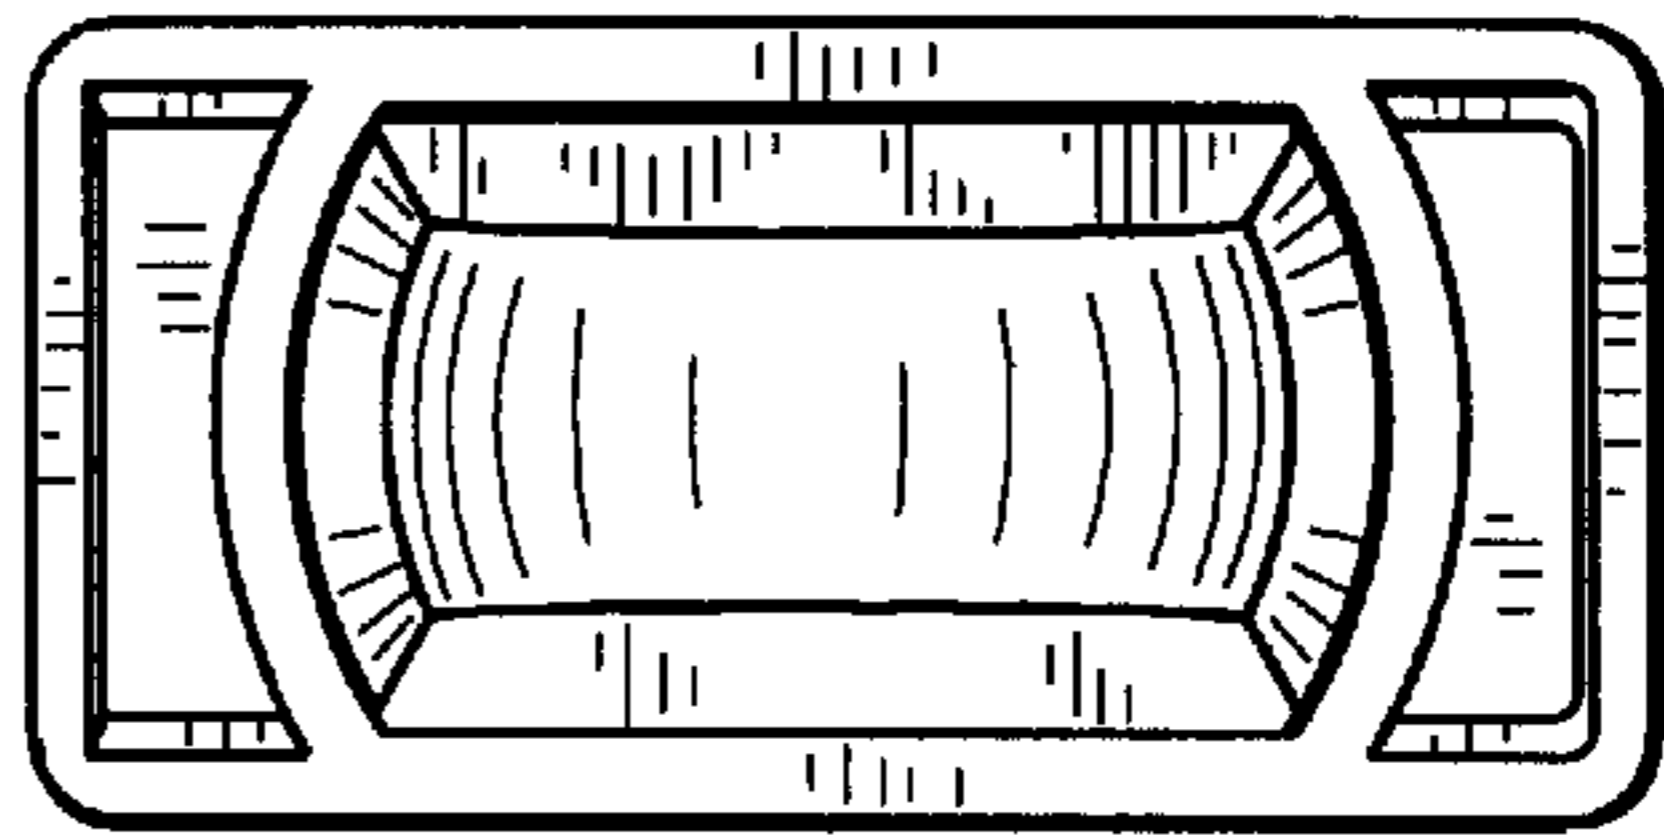


FIG. 4

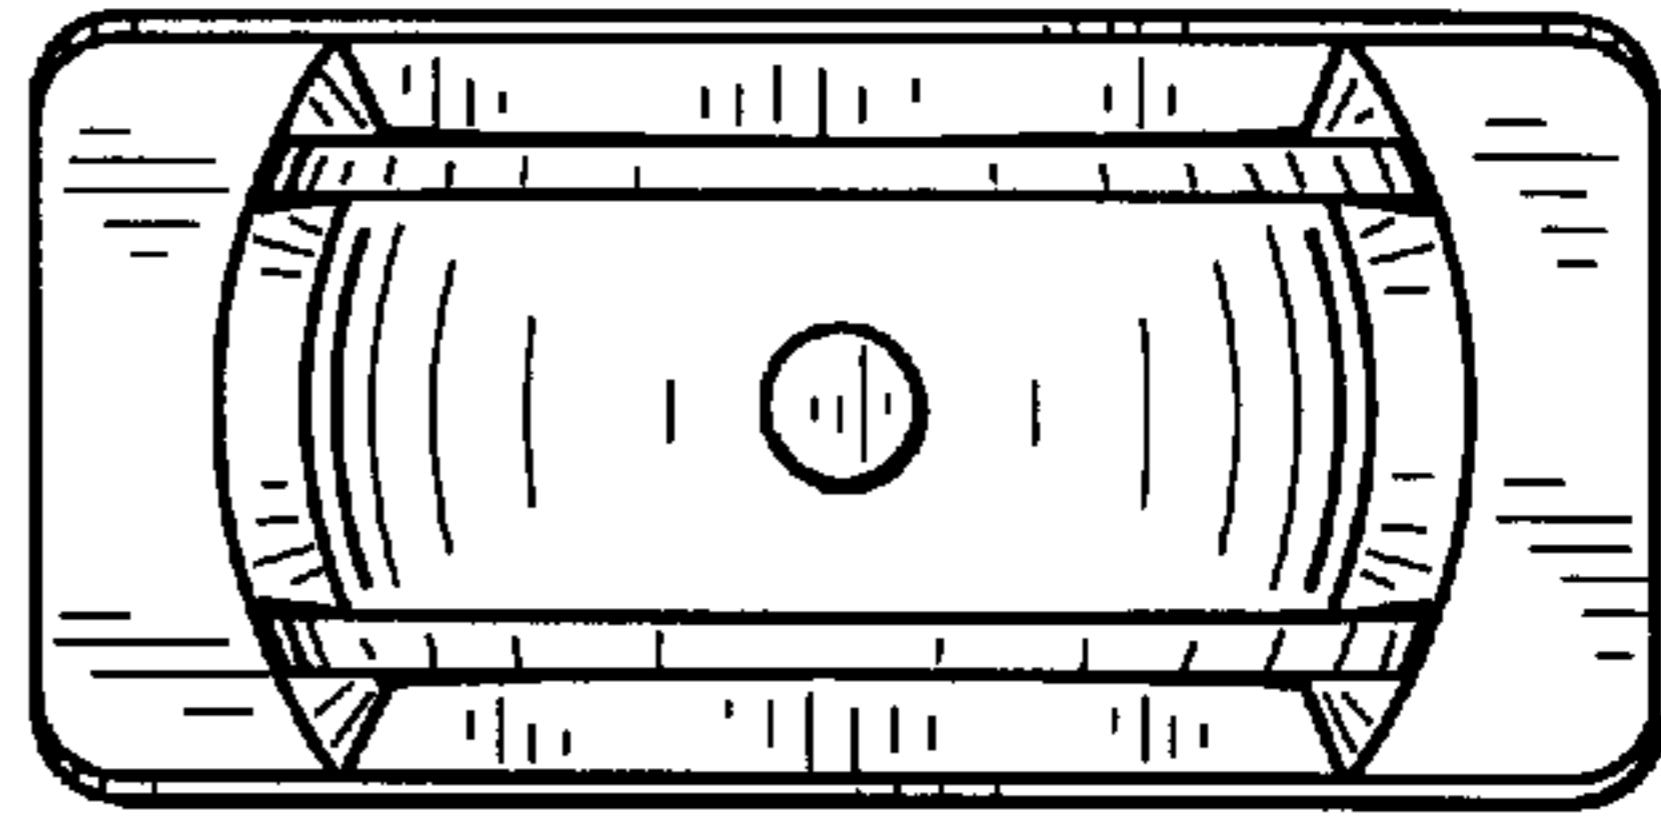


FIG. 5

