



US00D407986S

**United States Patent** [19]

[11] **Patent Number: Des. 407,986**

**Timbel**

[45] **Date of Patent: \*\*Apr. 13, 1999**

[54] **MEDICAL ALARM DEVICE**

5,434,558 7/1995 Zeder ..... 340/687

[75] **Inventor: Ned R. Timbel, Englewood, Colo.**

**OTHER PUBLICATIONS**

[73] **Assignee: Advanced Monitoring Devices, Inc., Littleton, Colo.**

Product Brochure, Climate Sentry 2000™ by Advanced Monitoring Devices, Inc., undated.

[\*\*] **Term: 14 Years**

*Primary Examiner*—Pamela Burgess  
*Attorney, Agent, or Firm*—Townsend and Townsend and Crew

[21] **Appl. No.: 29/086,865**

[57] **CLAIM**

[22] **Filed: Apr. 21, 1998**

The ornamental design for a medical alarm device, as shown and described.

[51] **LOC (6) Cl. .... 10-05**

[52] **U.S. Cl. .... D10/106; D24/107**

[58] **Field of Search** ..... D24/186, 107, D24/232; D10/106, 116, 104, 31; 128/630, 700; 340/540, 628-634, 571-573, 689, 687; D20/18; 364/413.01, 413.02, 413.03, 413.04, 130, 184, 480, 481, 482, 483, 550, 224.5, 224.6

**DESCRIPTION**

FIG. 1 is a perspective view of a medical alarm device showing my new design;  
FIG. 2 is a top plan view thereof;  
FIG. 3 is a front elevational view thereof;  
FIG. 4 is a rear elevational view thereof;  
FIG. 5 is a left side elevational view thereof;  
FIG. 6 is a right side elevational view thereof; and,  
FIG. 7 is a bottom plan view thereof.


It is understood that the cable projecting from the left side of the claimed article herein is of indiscriminate length.

[56] **References Cited**

**U.S. PATENT DOCUMENTS**

D. 321,330	11/1991	Gagnon et al. ....	D10/106
D. 336,053	6/1993	Hayes et al. ....	D10/106
D. 373,964	9/1996	Alexander ....	D10/106
D. 385,503	10/1997	Velazquez ....	D10/106

**1 Claim, 5 Drawing Sheets**

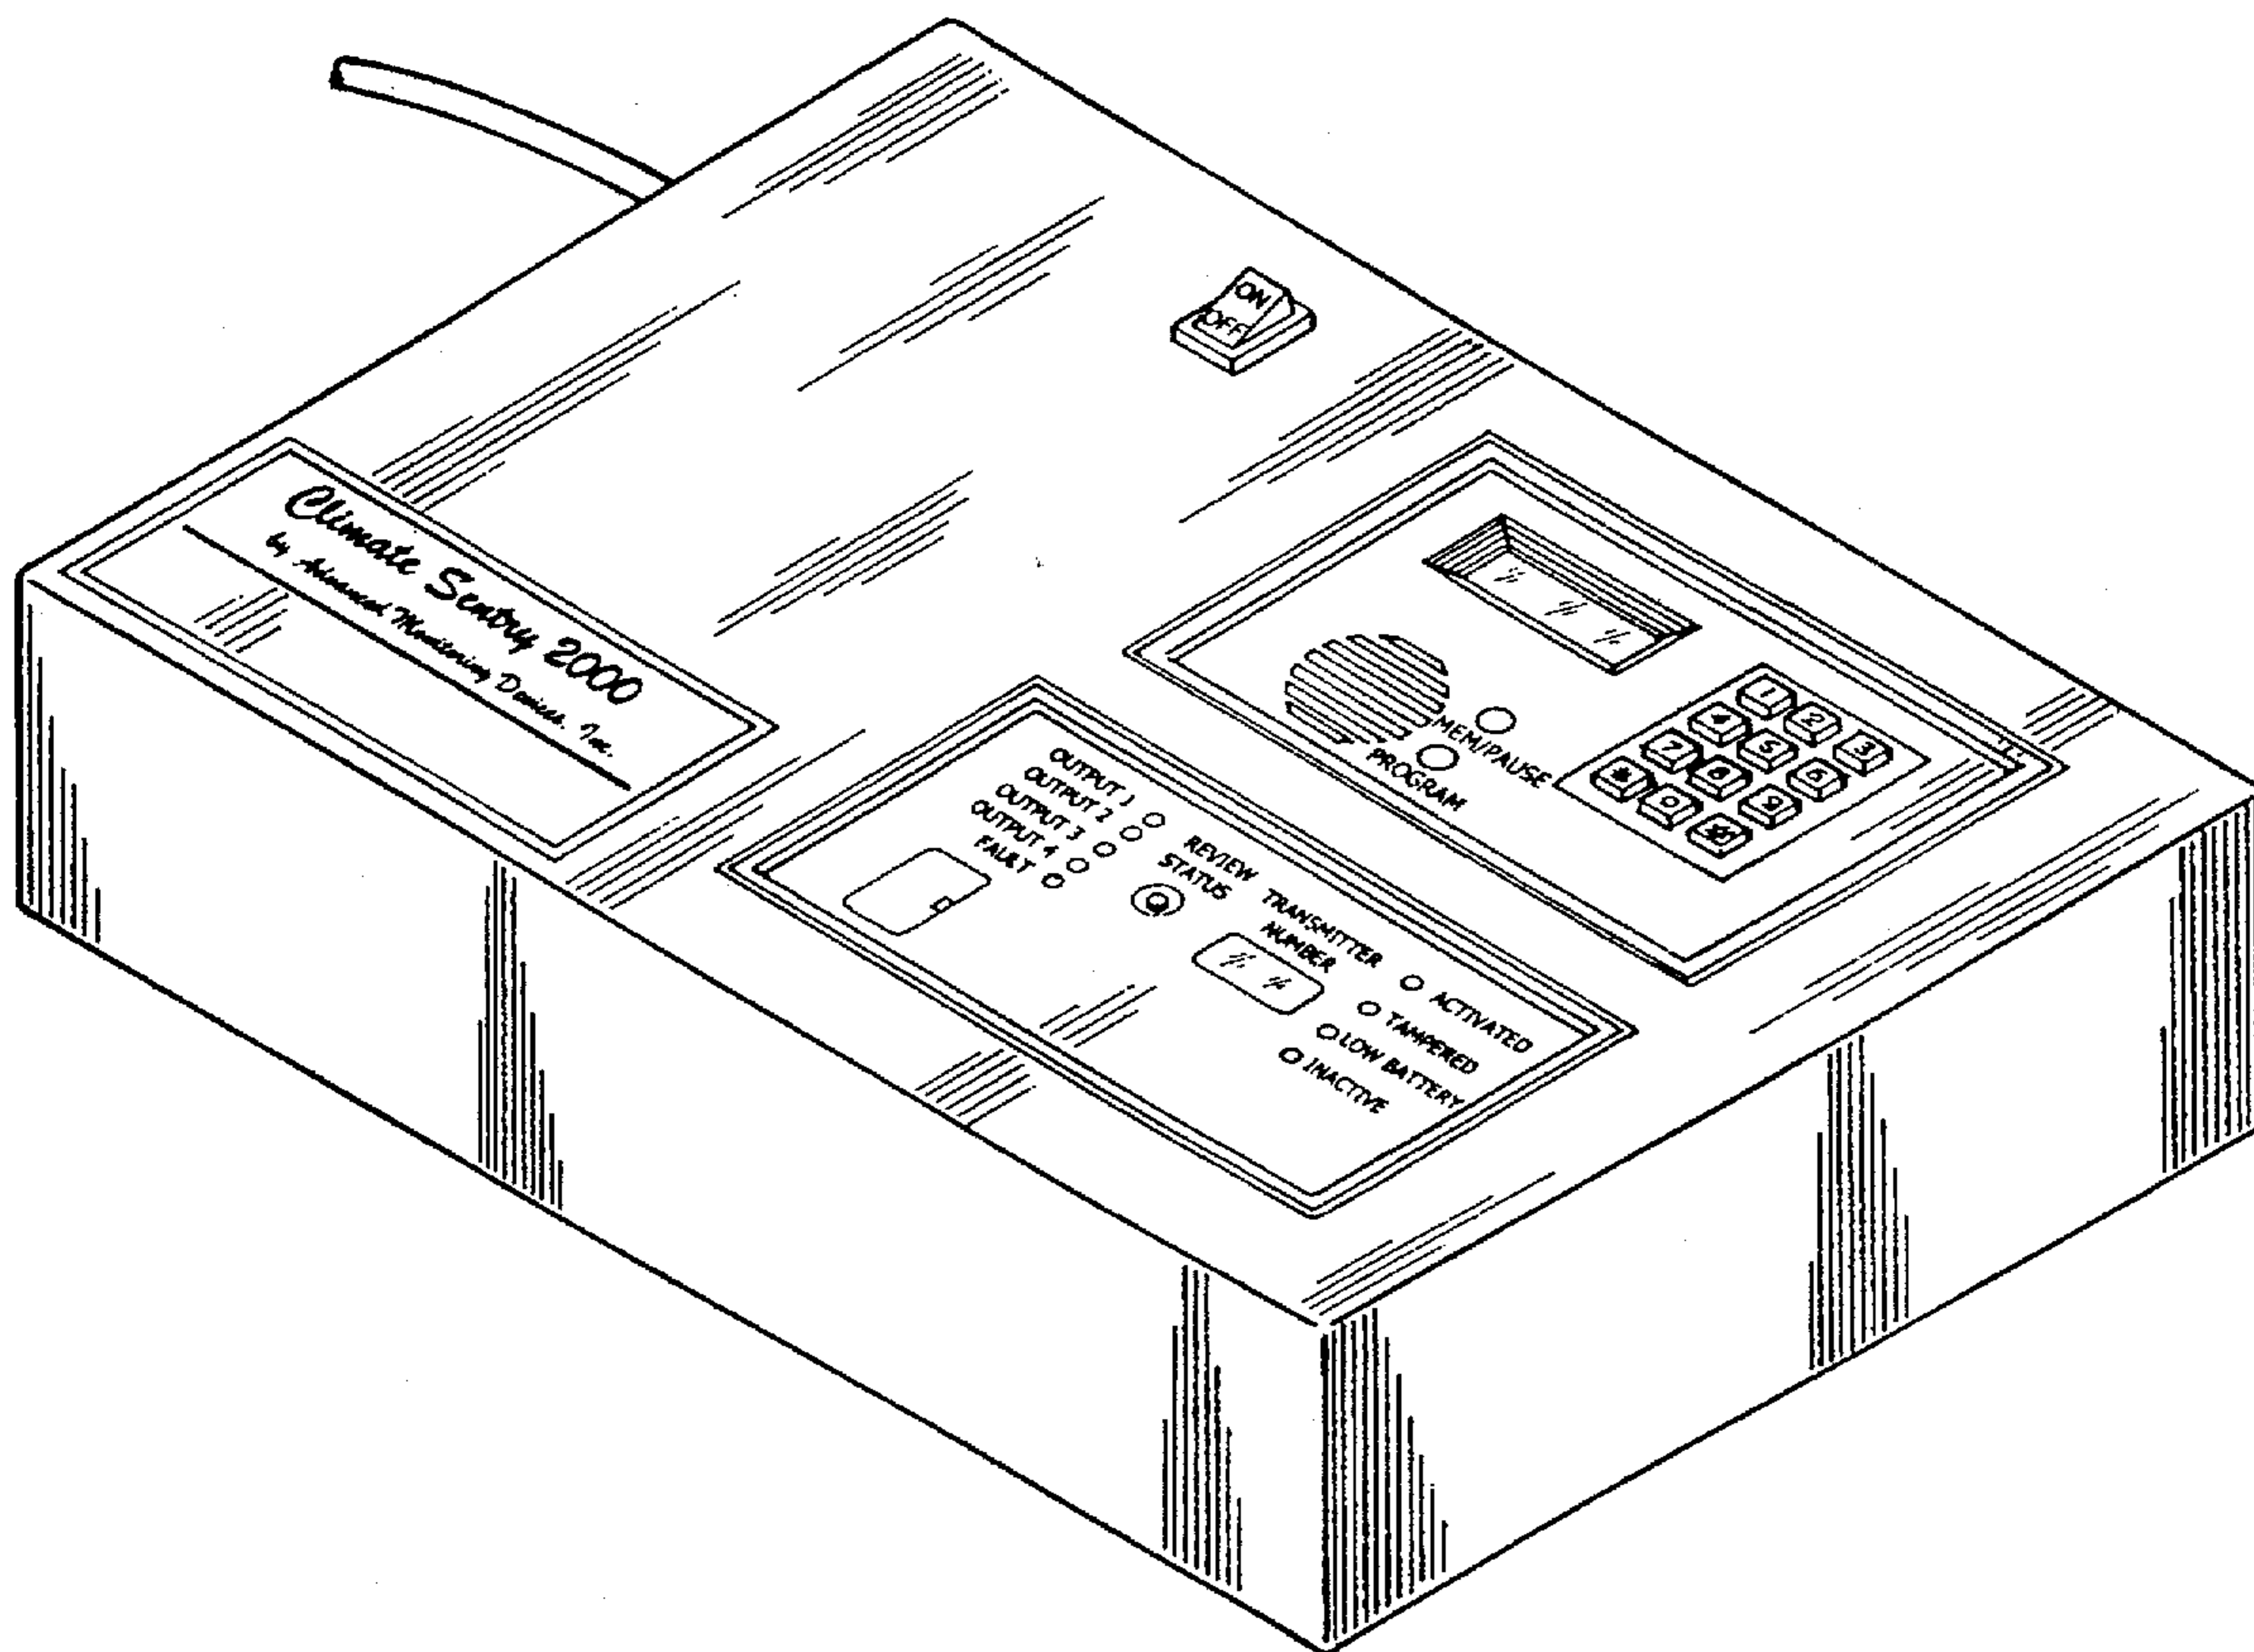

**Fig. 1**




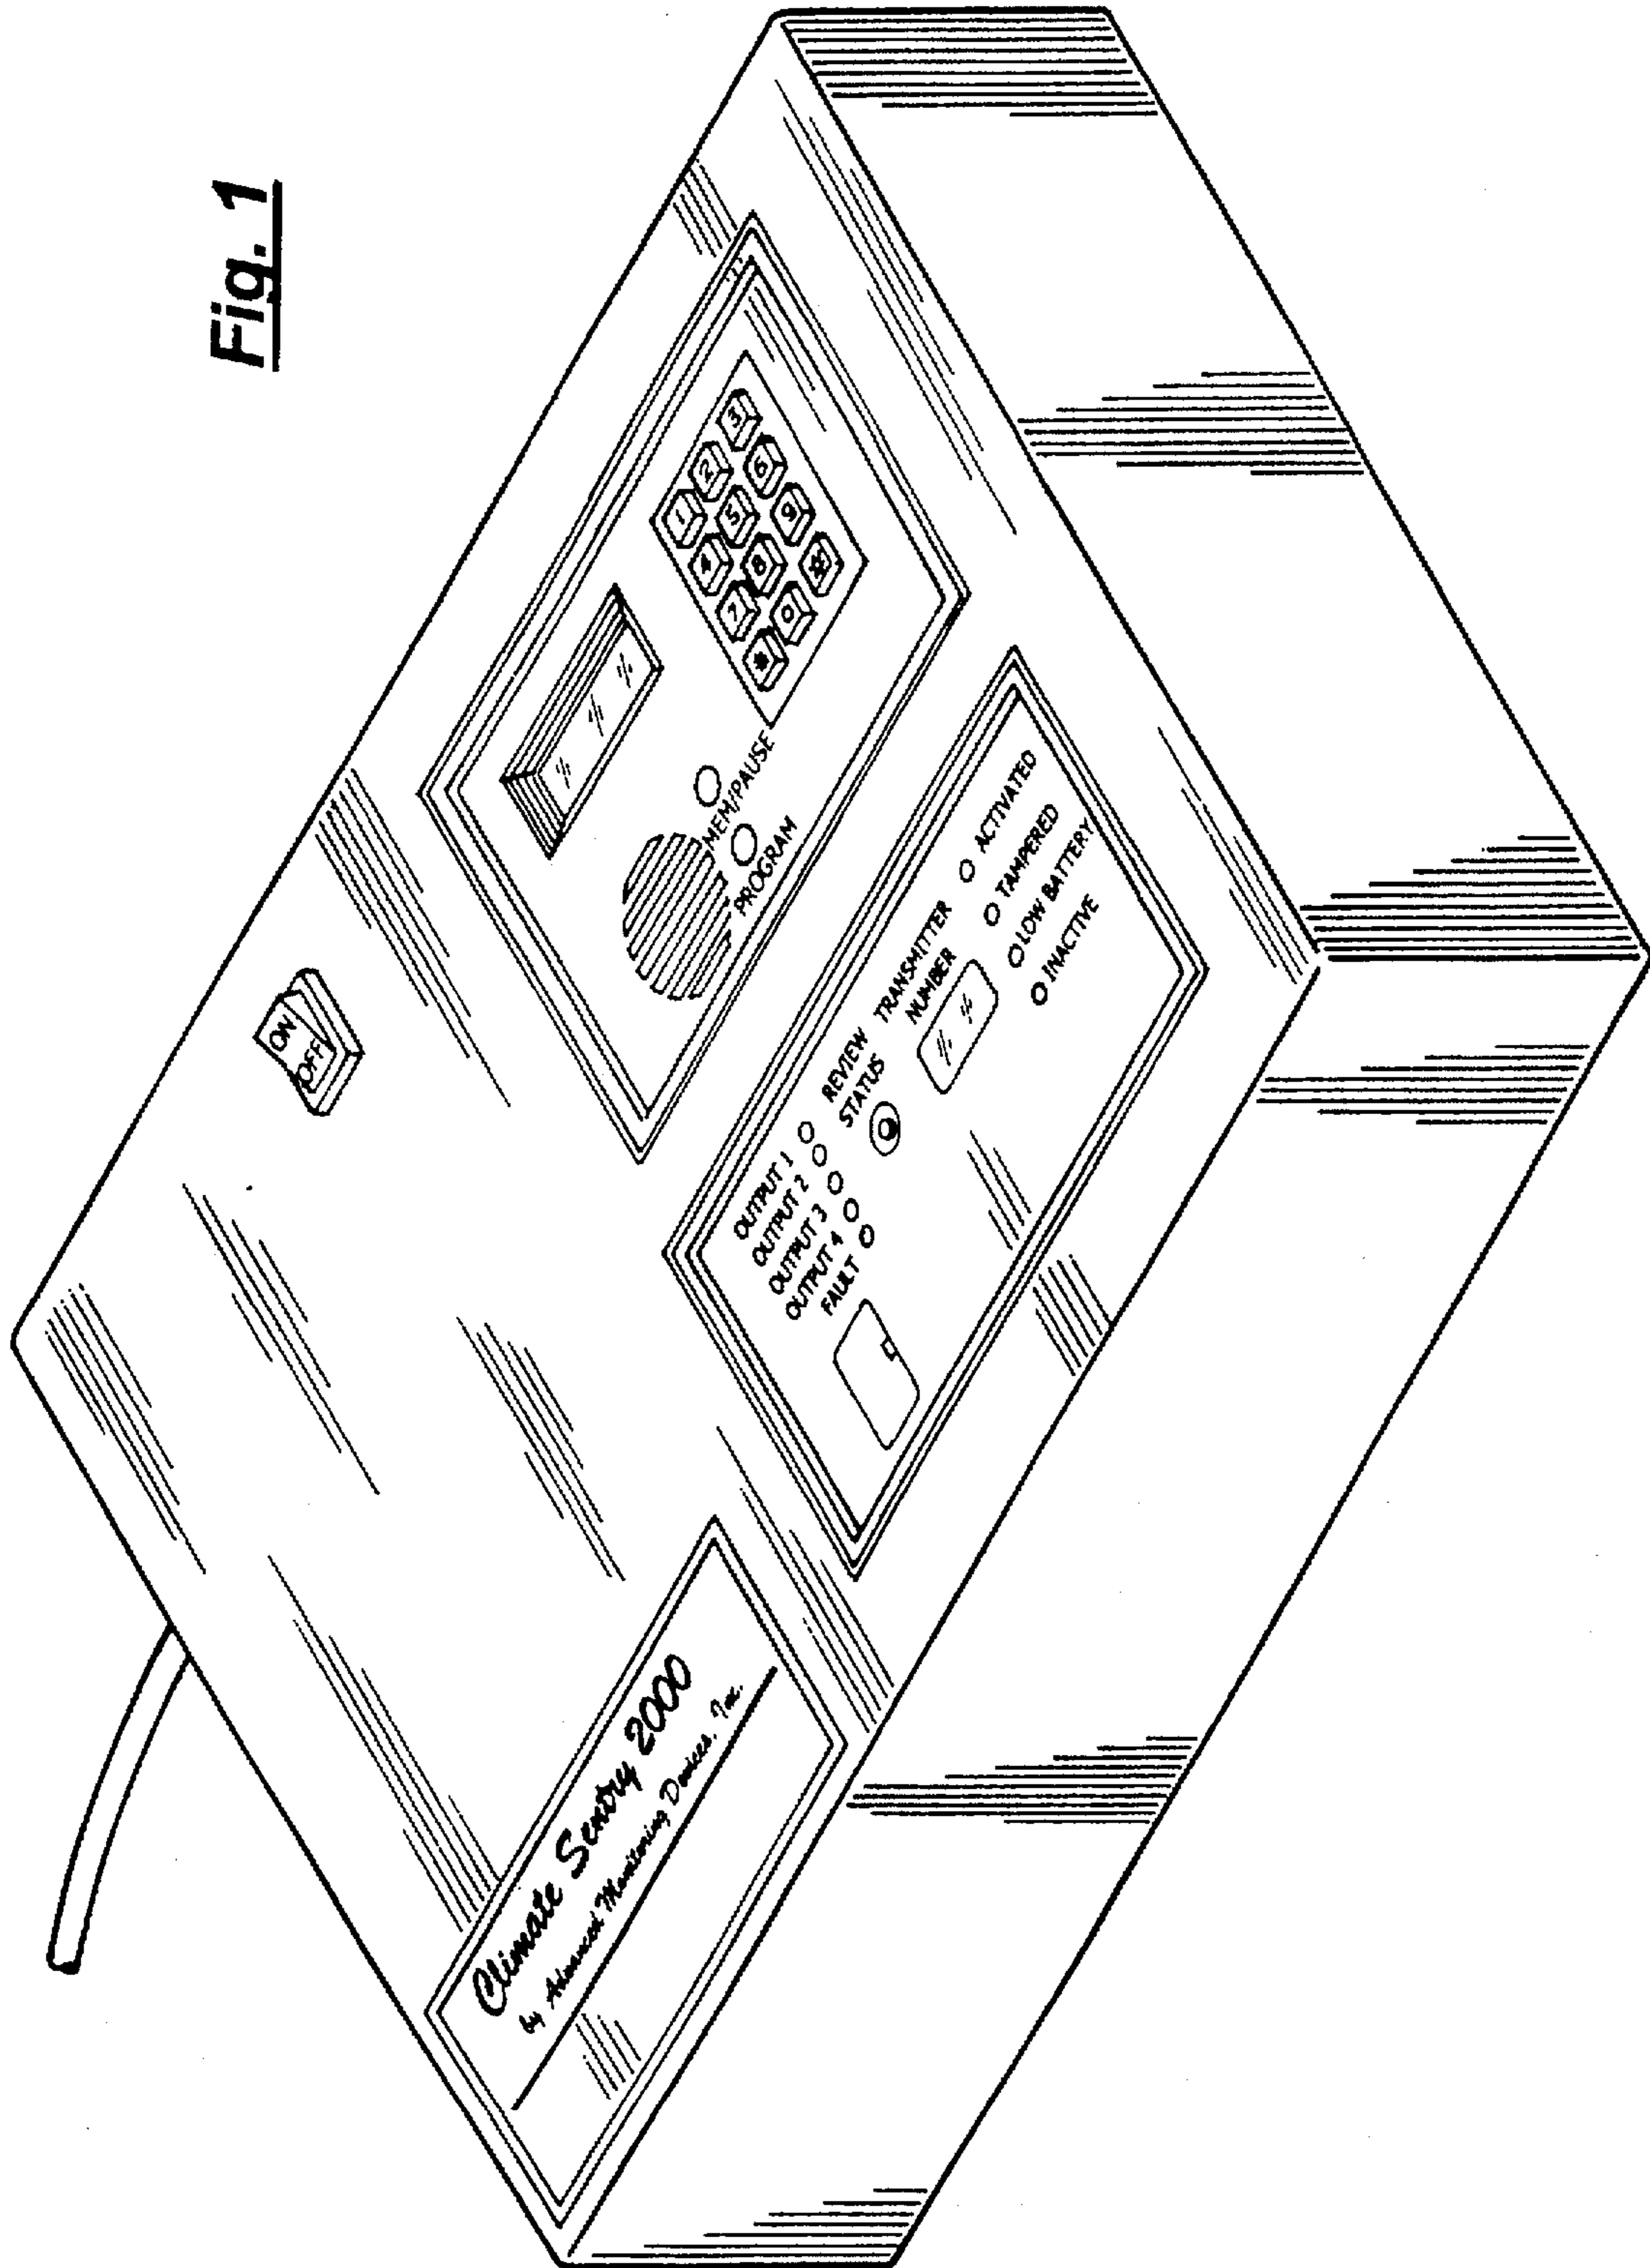


Fig. 2

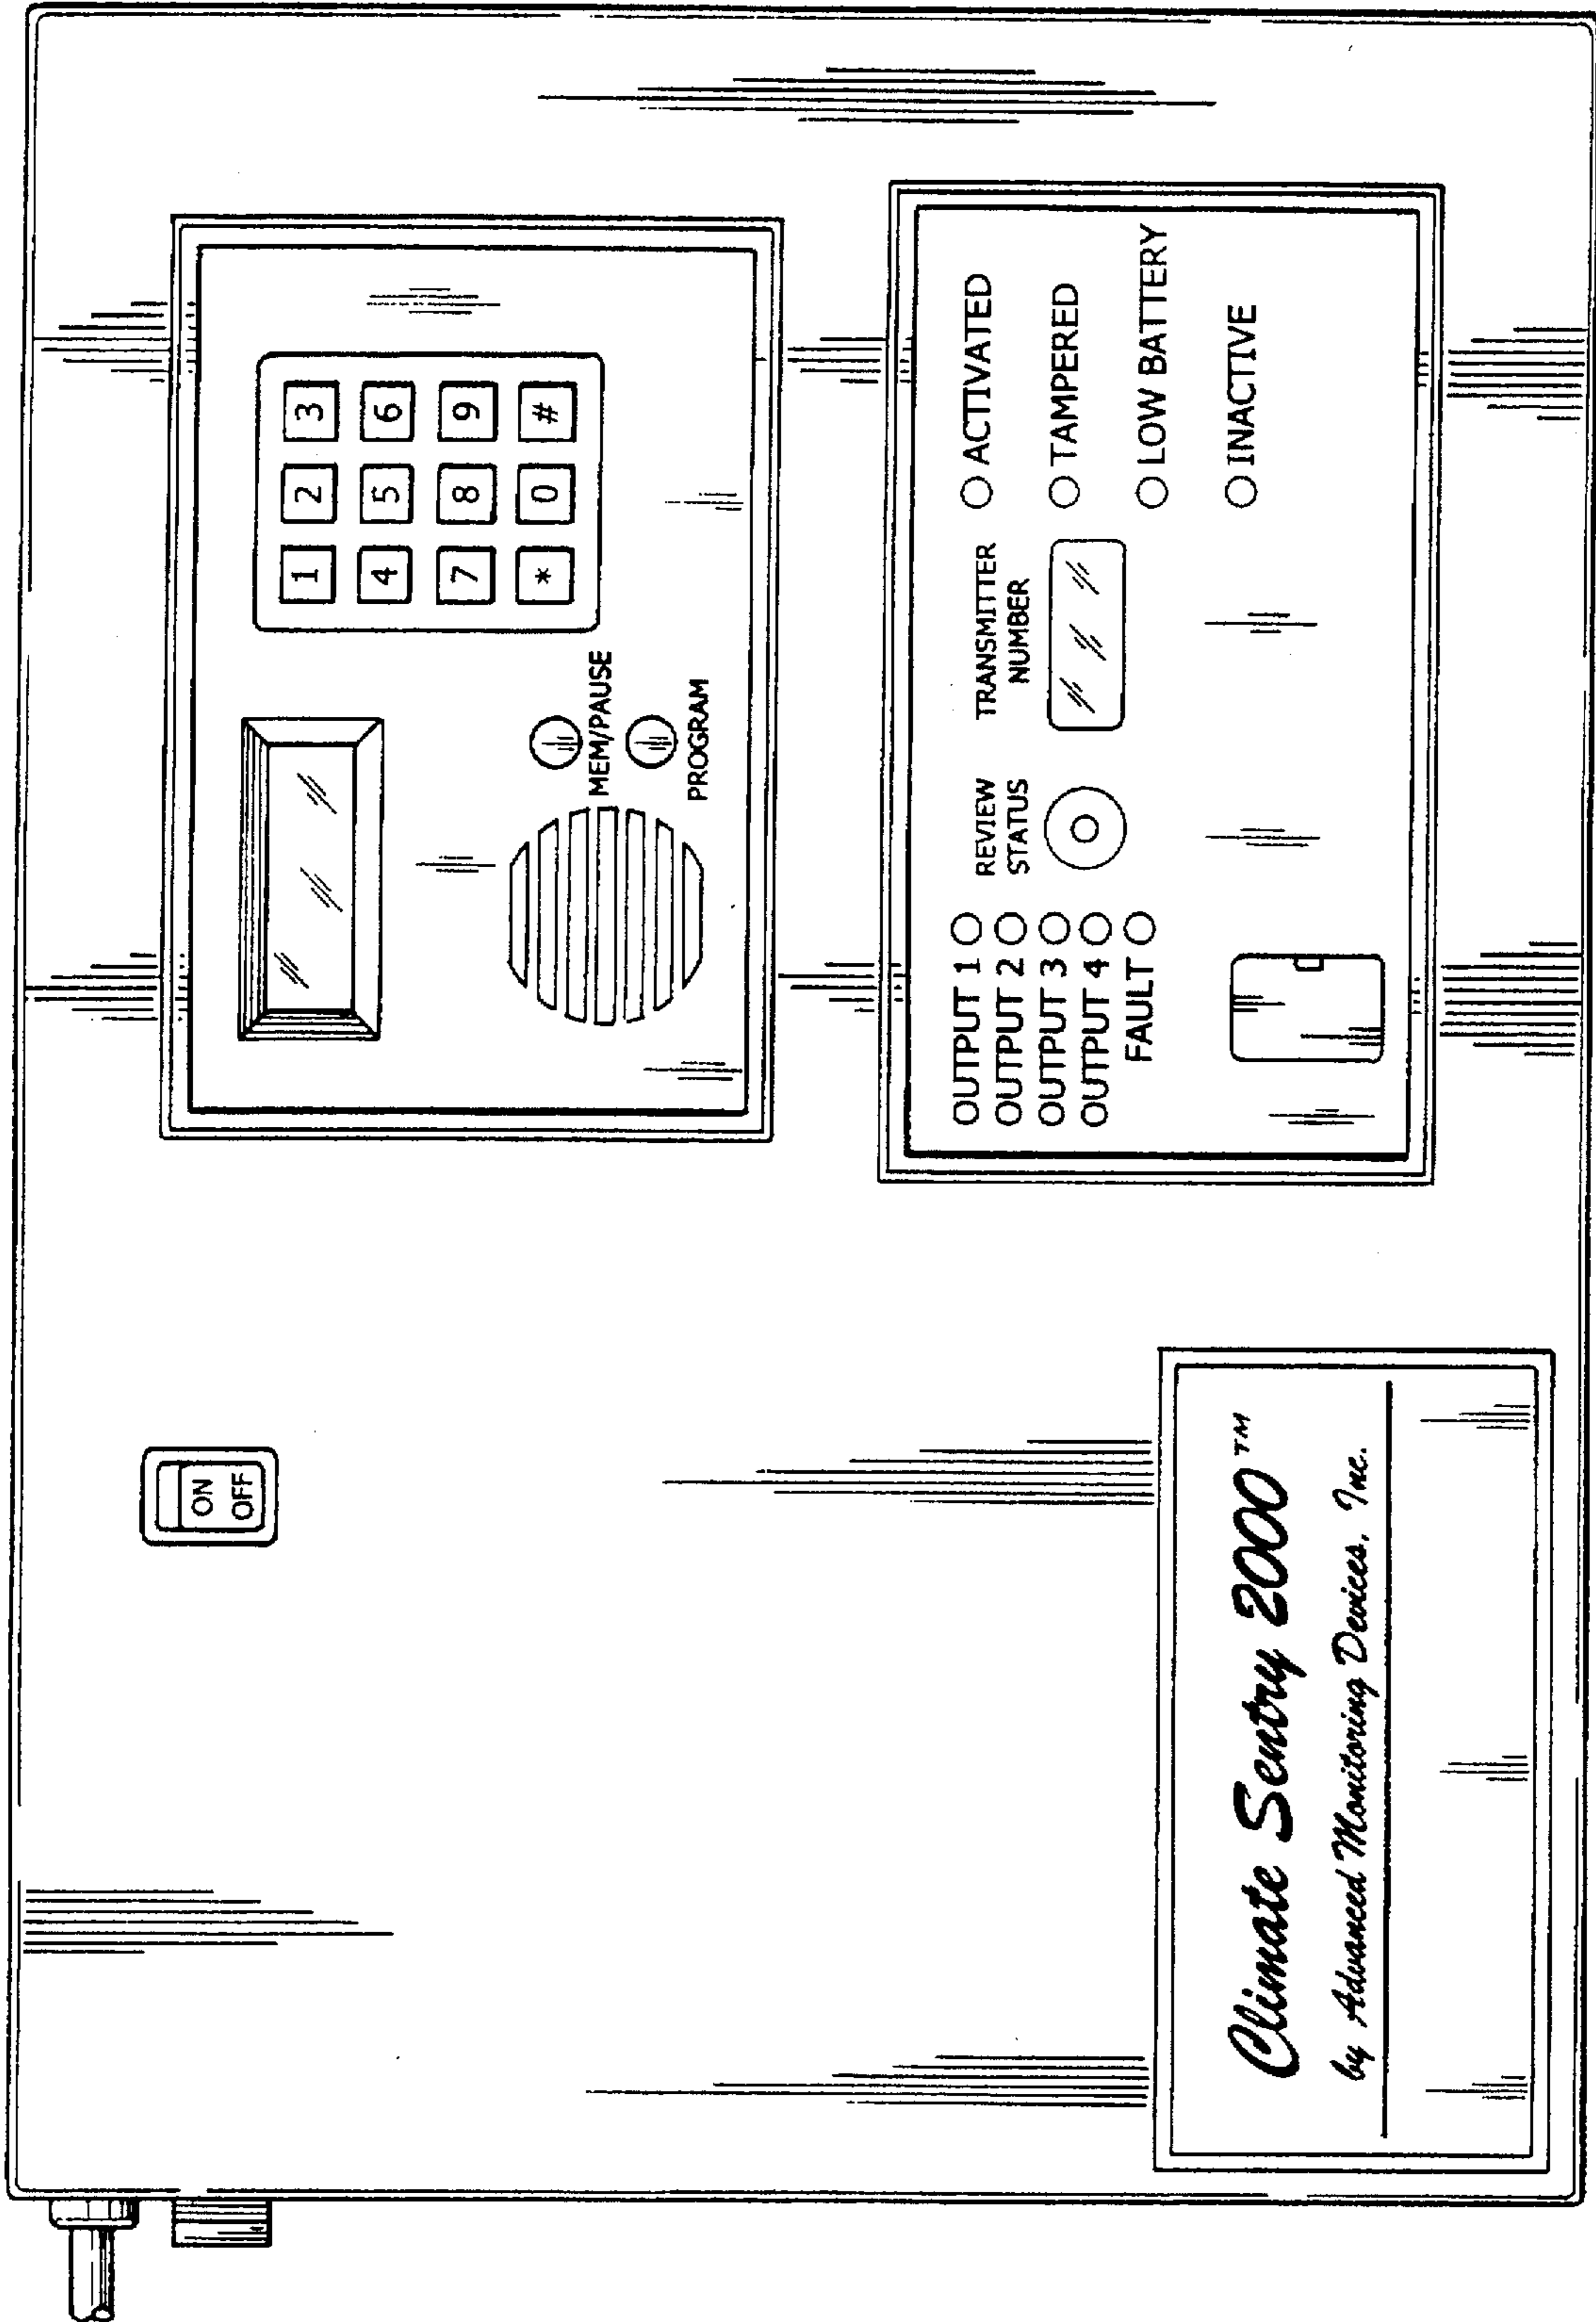

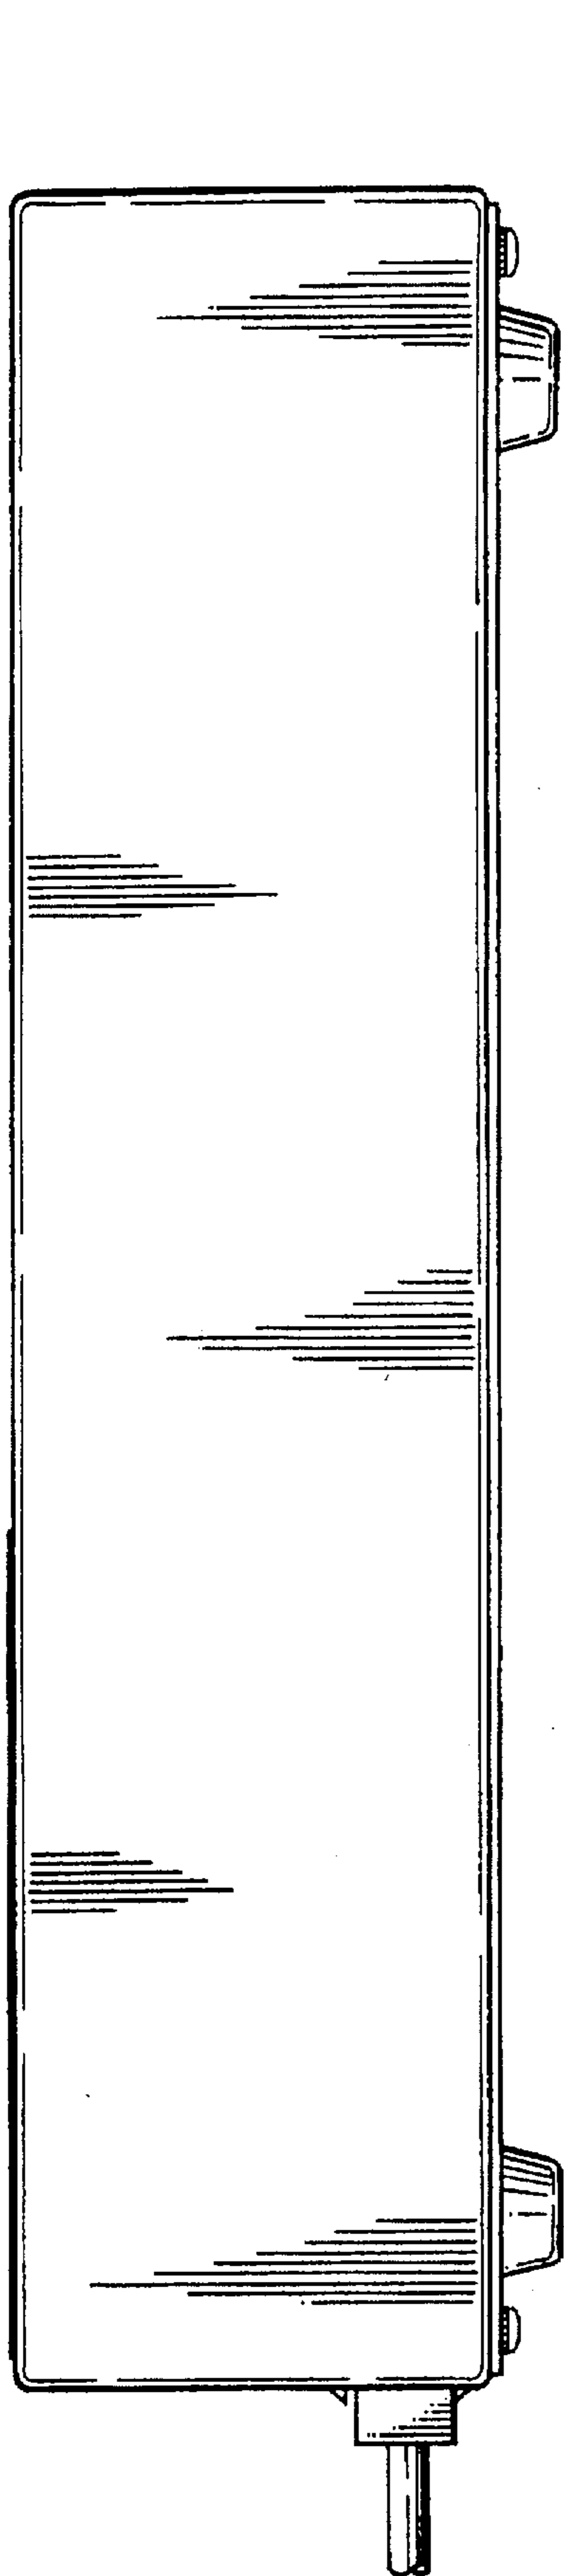

**Fig. 3**

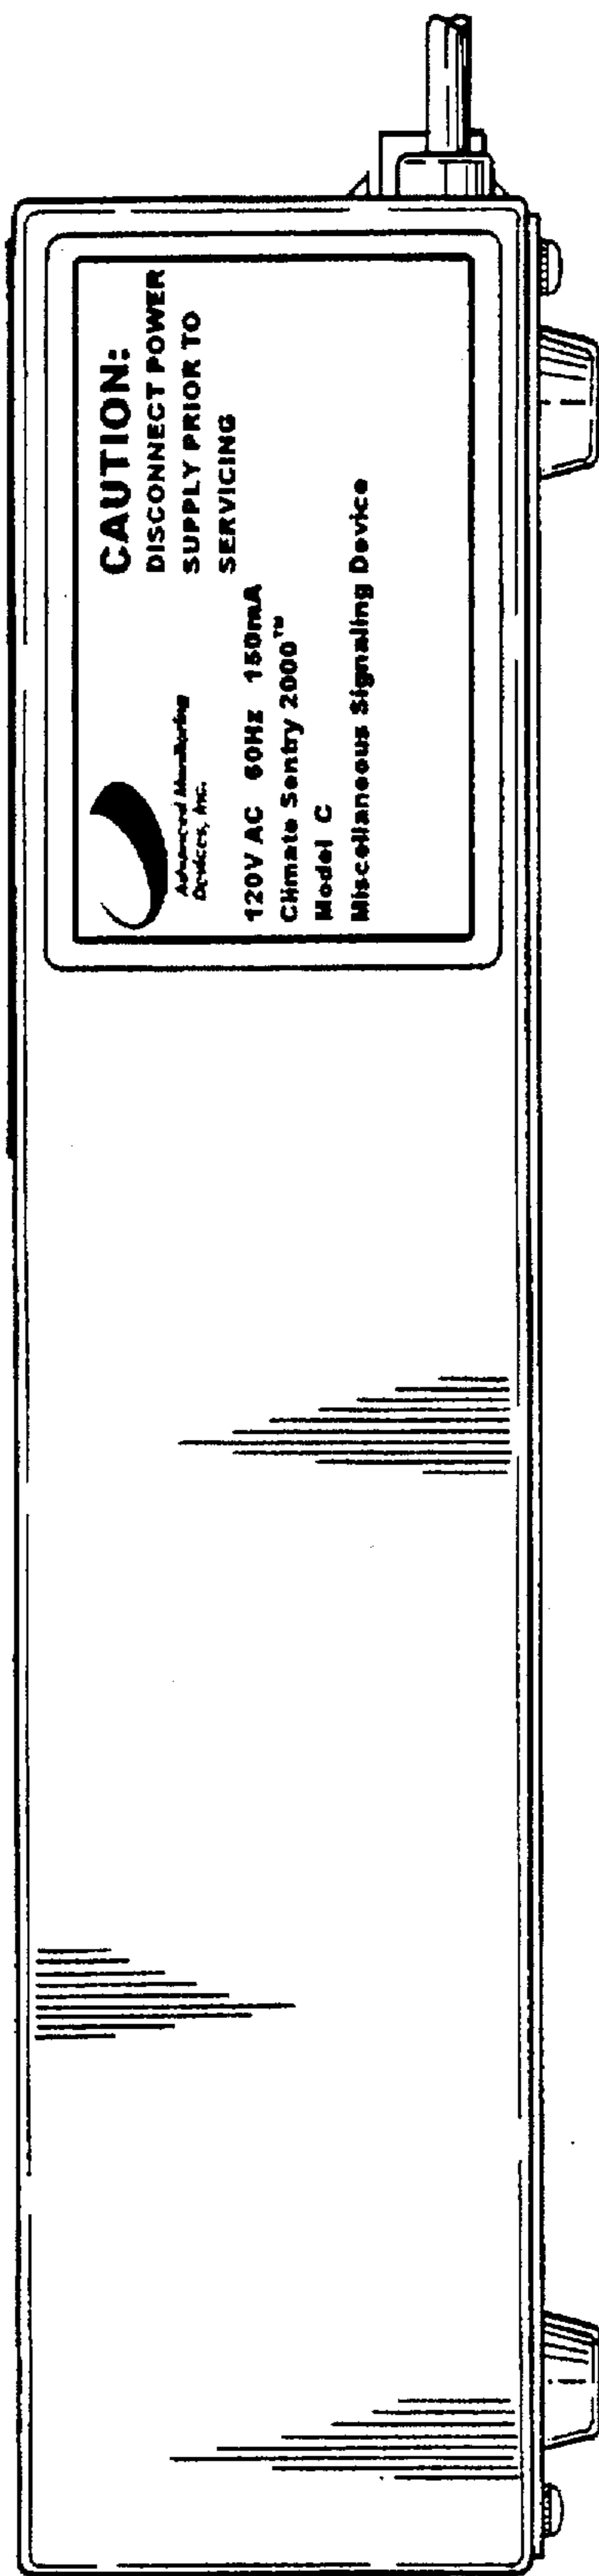

**Fig. 4**

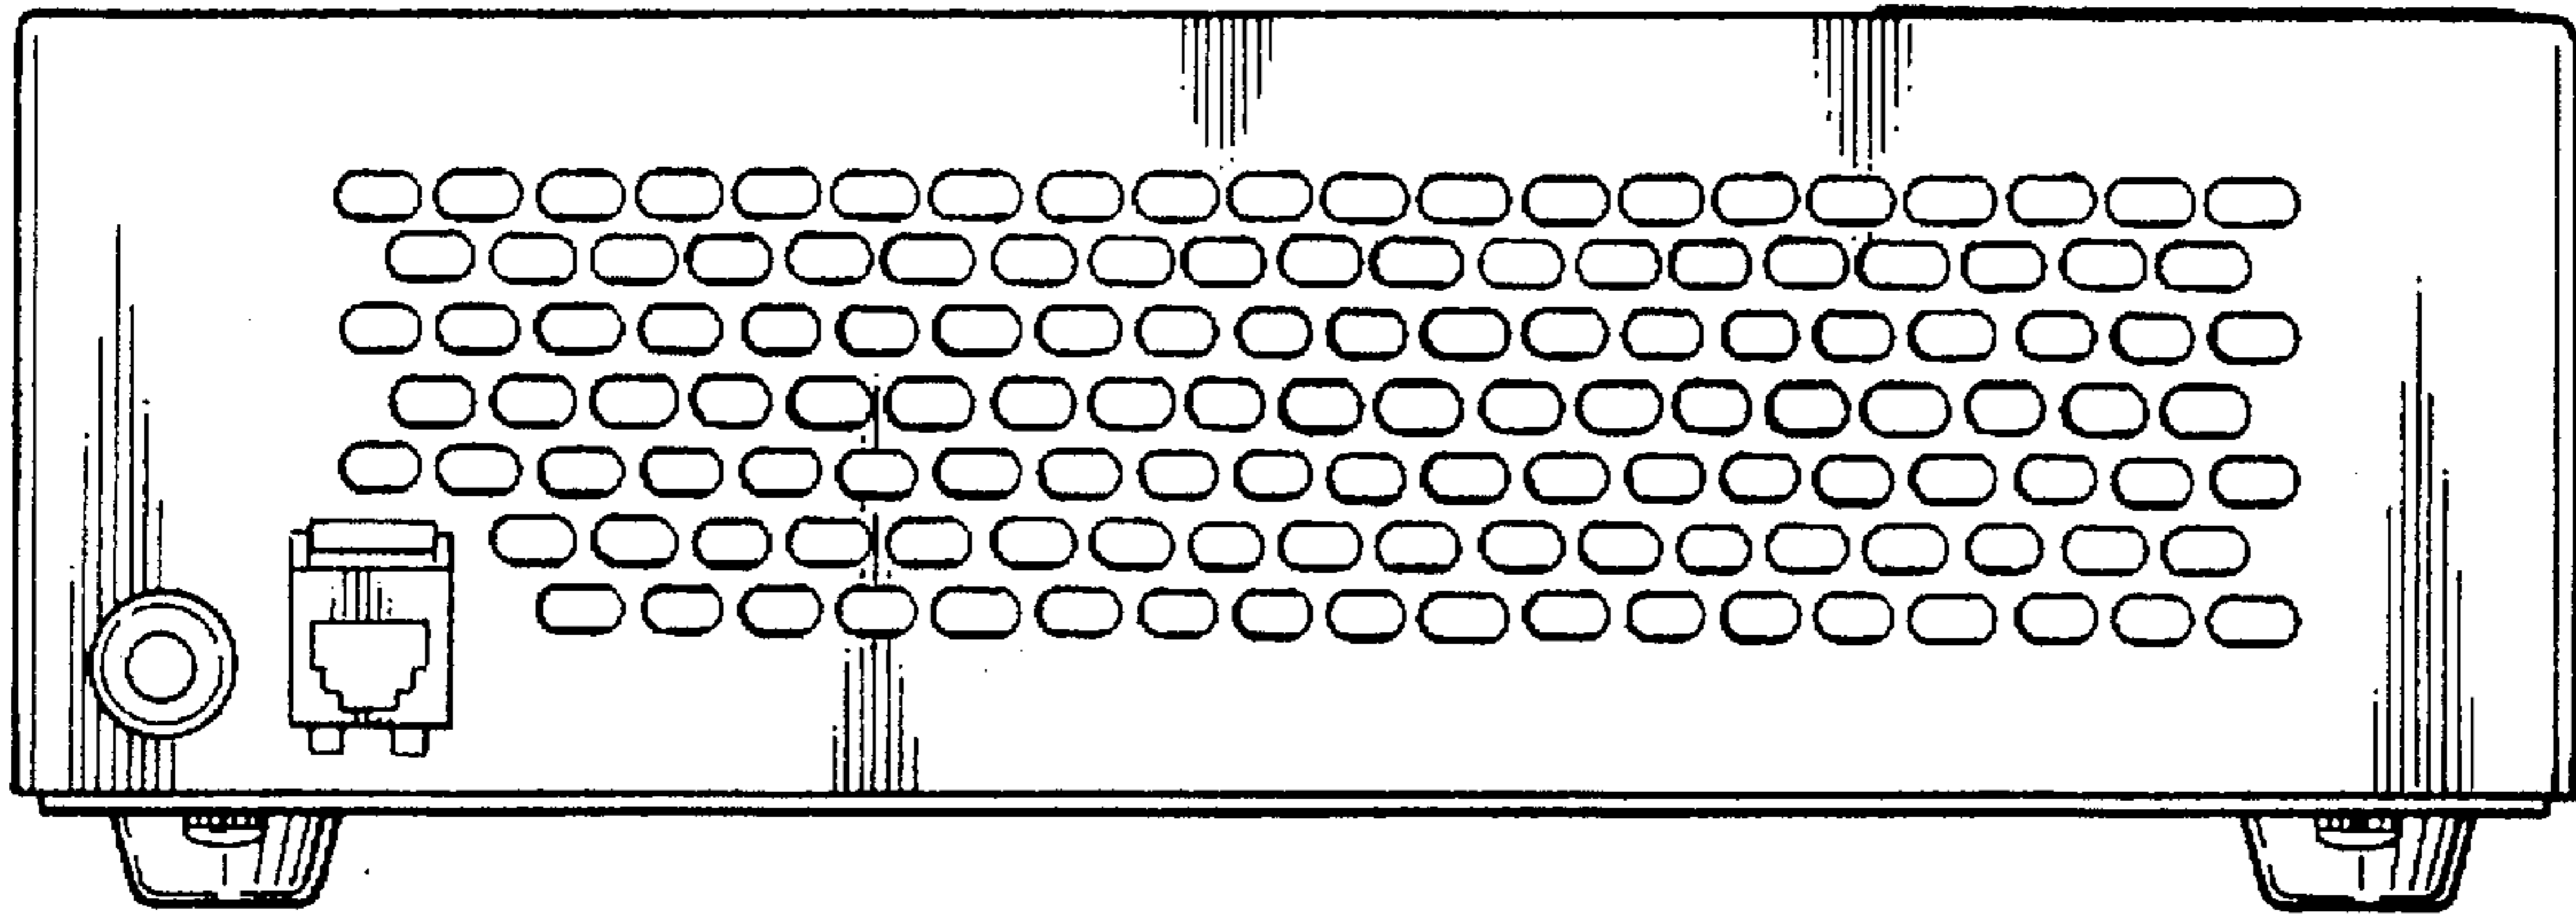


Fig. 5

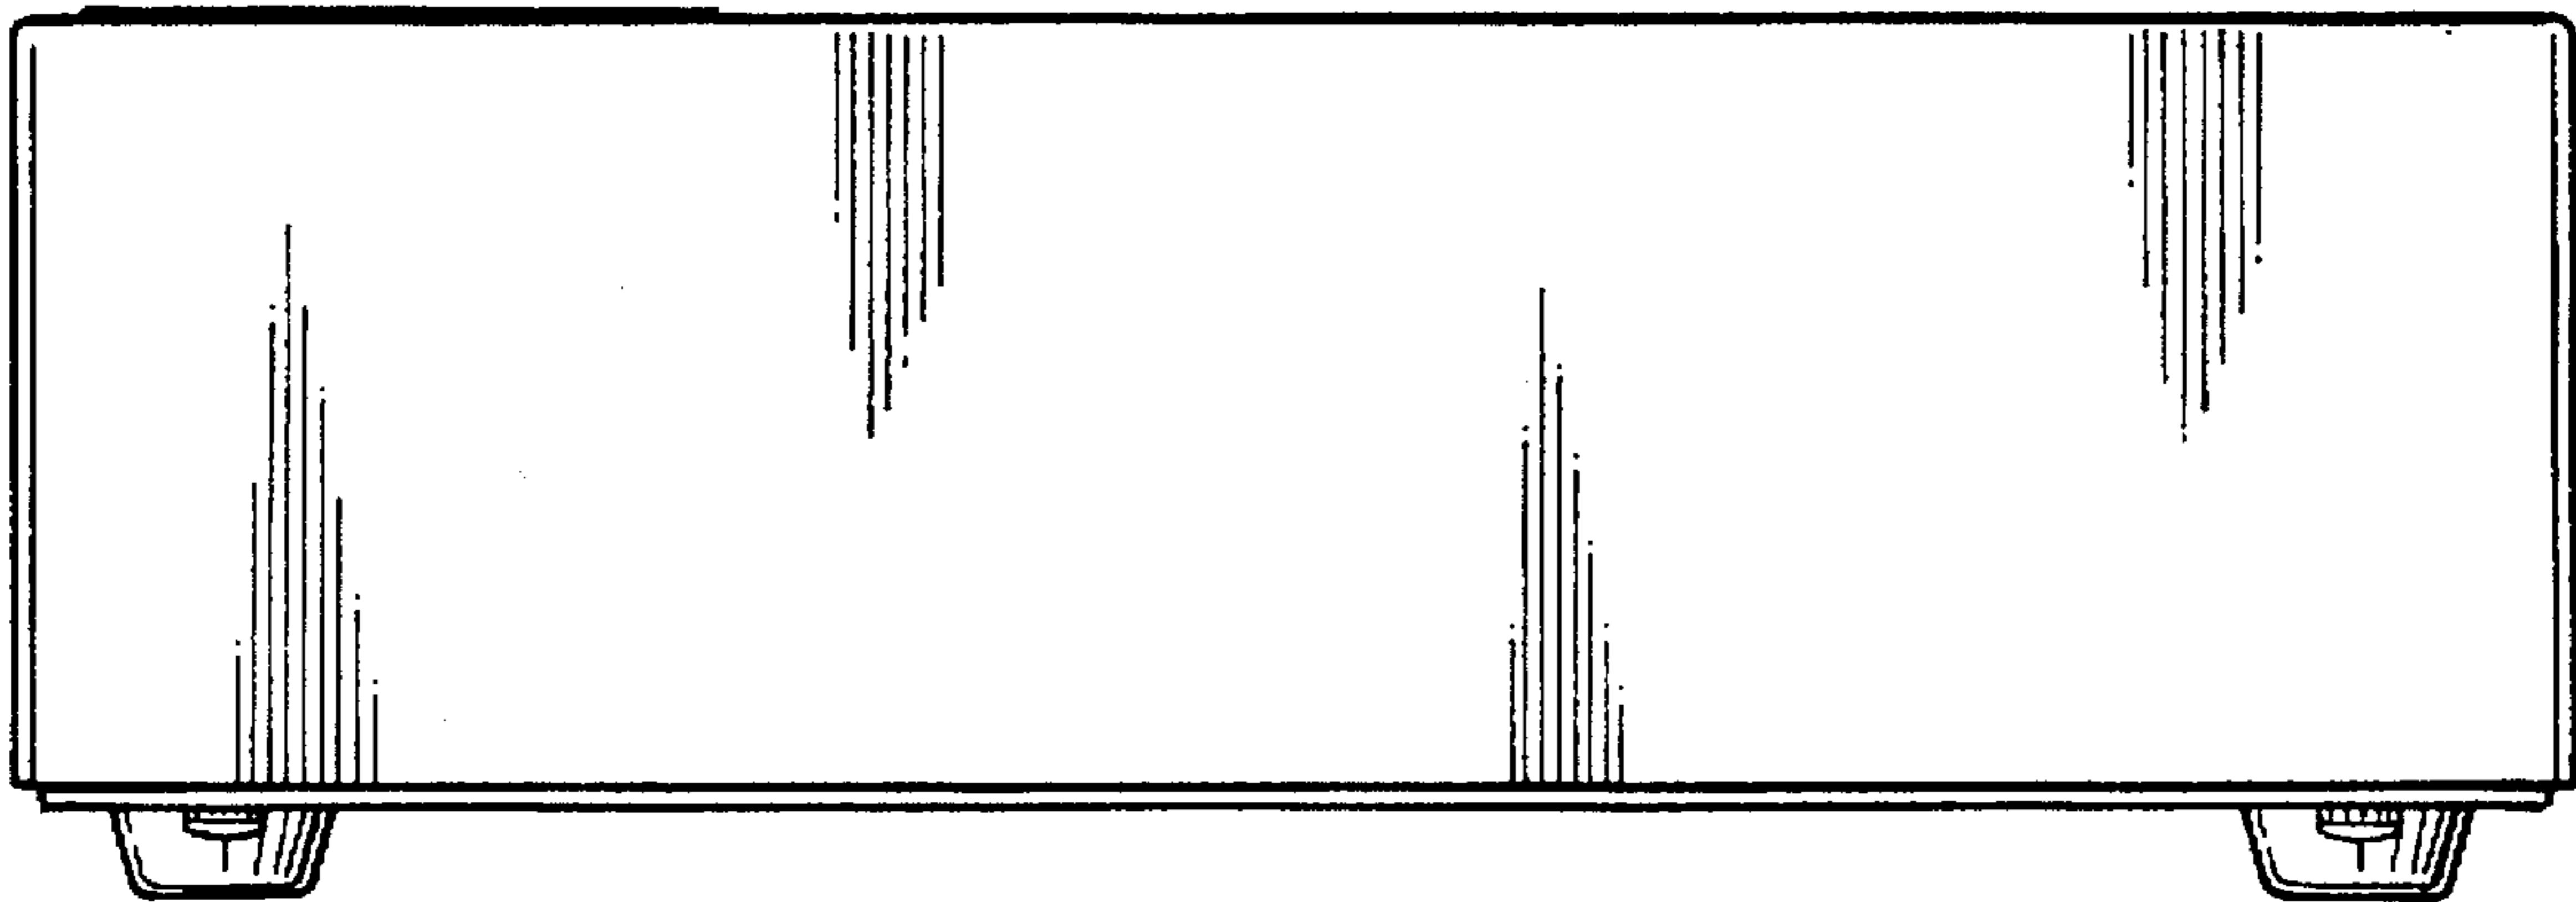


Fig. 6

Fig. 7

