

US00D409307S

United States Patent [19]

Phleps et al.

[11] **Patent Number: Des. 409,307**

[45] **Date of Patent: ** May 4, 1999**

[54] **SENSOR OF RADIOLOGIC APPARATUS FOR USE IN THE MOUTH**

D. 361,619	8/1995	Phelps et al.	D24/158
D. 387,163	12/1997	Osthues et al.	D24/158
4,150,296	4/1979	Edeland et al.	378/170

[75] Inventors: **Tilman Phleps; Michael Döbert**, both of Lorsch; **Uwe Zeller**, Neu-Anspach, all of Germany

Primary Examiner—Stella Reid
Attorney, Agent, or Firm—Watson Cole Grindle Watson, P.L.L.C.

[73] Assignee: **Sirona Dental Systems GmbH & Co. KG**, Bensheim, Germany

[**] Term: **14 Years**

[21] Appl. No.: **29/085,855**

[22] Filed: **Mar. 31, 1998**

[30] **Foreign Application Priority Data**

Oct. 1, 1997 [WO] WIPO WO-GB/FMPP 010

[51] **LOC (6) Cl.** **24-01**

[52] **U.S. Cl.** **D24/158**

[58] **Field of Search** D24/158; 378/167, 378/168, 180, 184, 197, 170

[57] **CLAIM**

The ornamental design for a sensor of radiologic apparatus for use in the mouth, as shown and described.

DESCRIPTION

FIG. 1 is a front elevational view of a sensor of radiologic apparatus for use in the mouth showing our new design;

FIG. 2 is a top view thereof;

FIG. 3 is a rear elevational view thereof;

FIG. 4 is a left side elevational view thereof, the right side being a mirror image; and,

FIG. 5 is a bottom plan view thereof.

[56] **References Cited**

U.S. PATENT DOCUMENTS

D. 355,964 2/1995 Nelvig D24/158

1 Claim, 1 Drawing Sheet

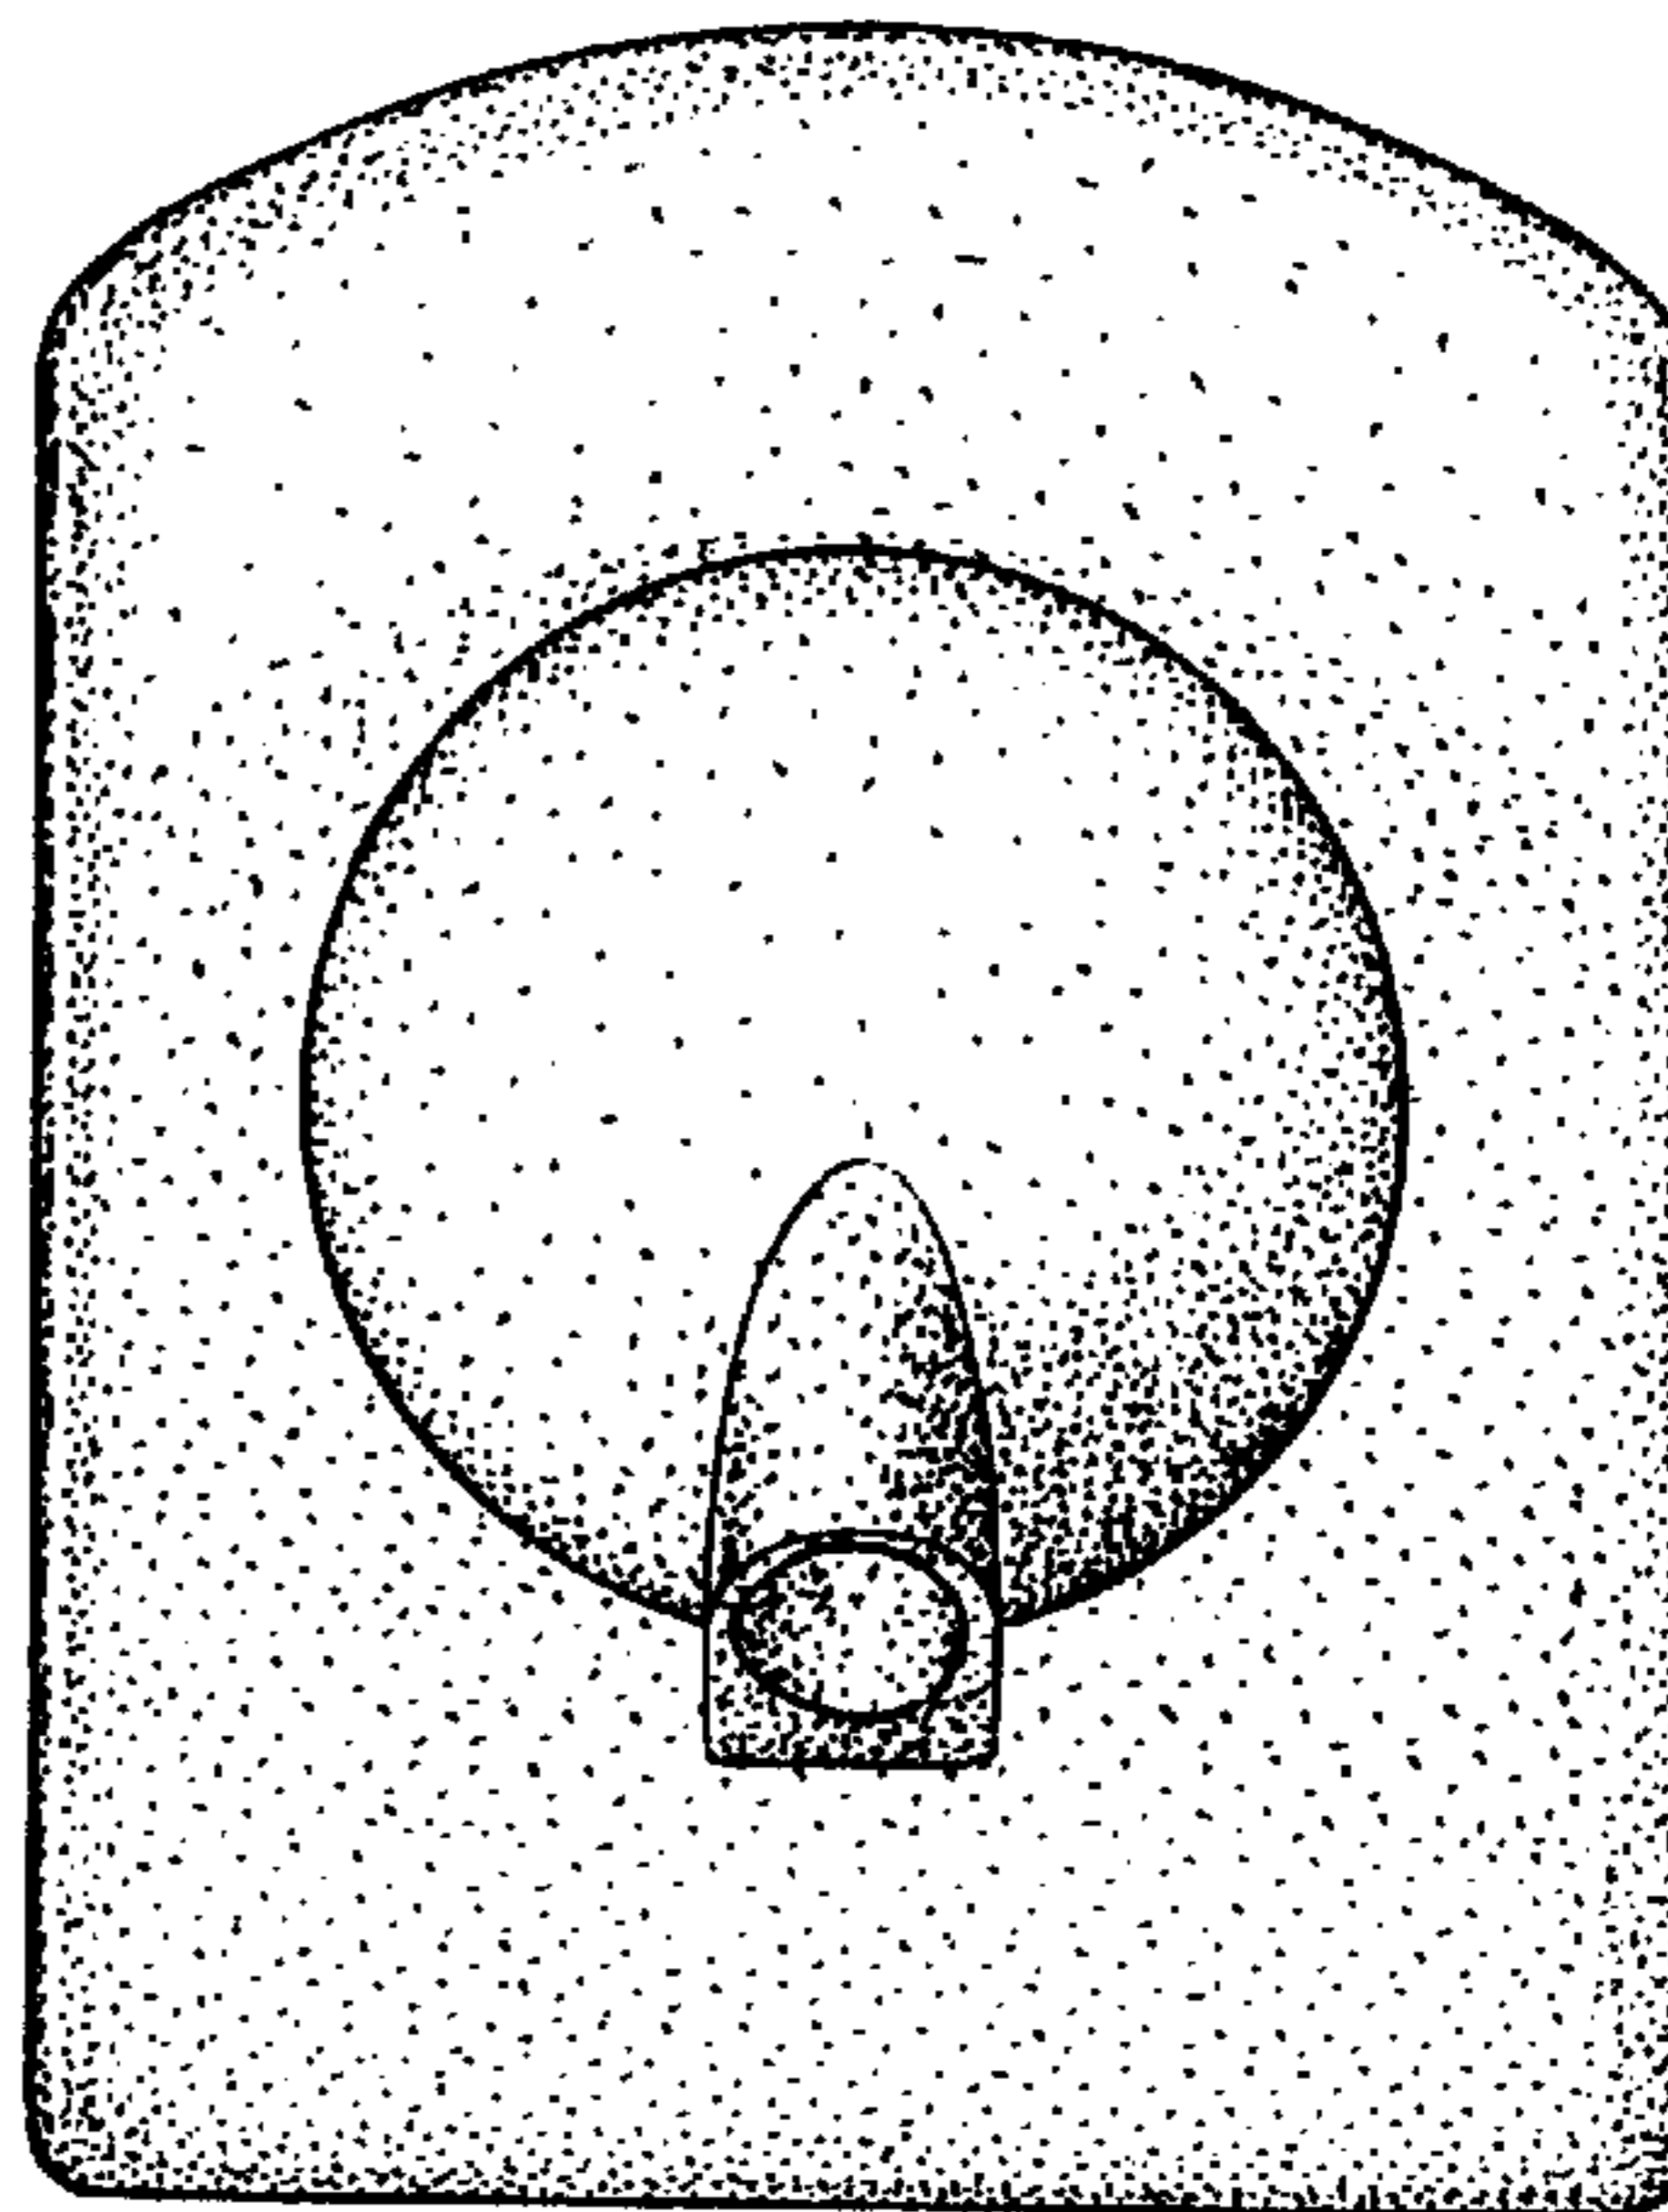
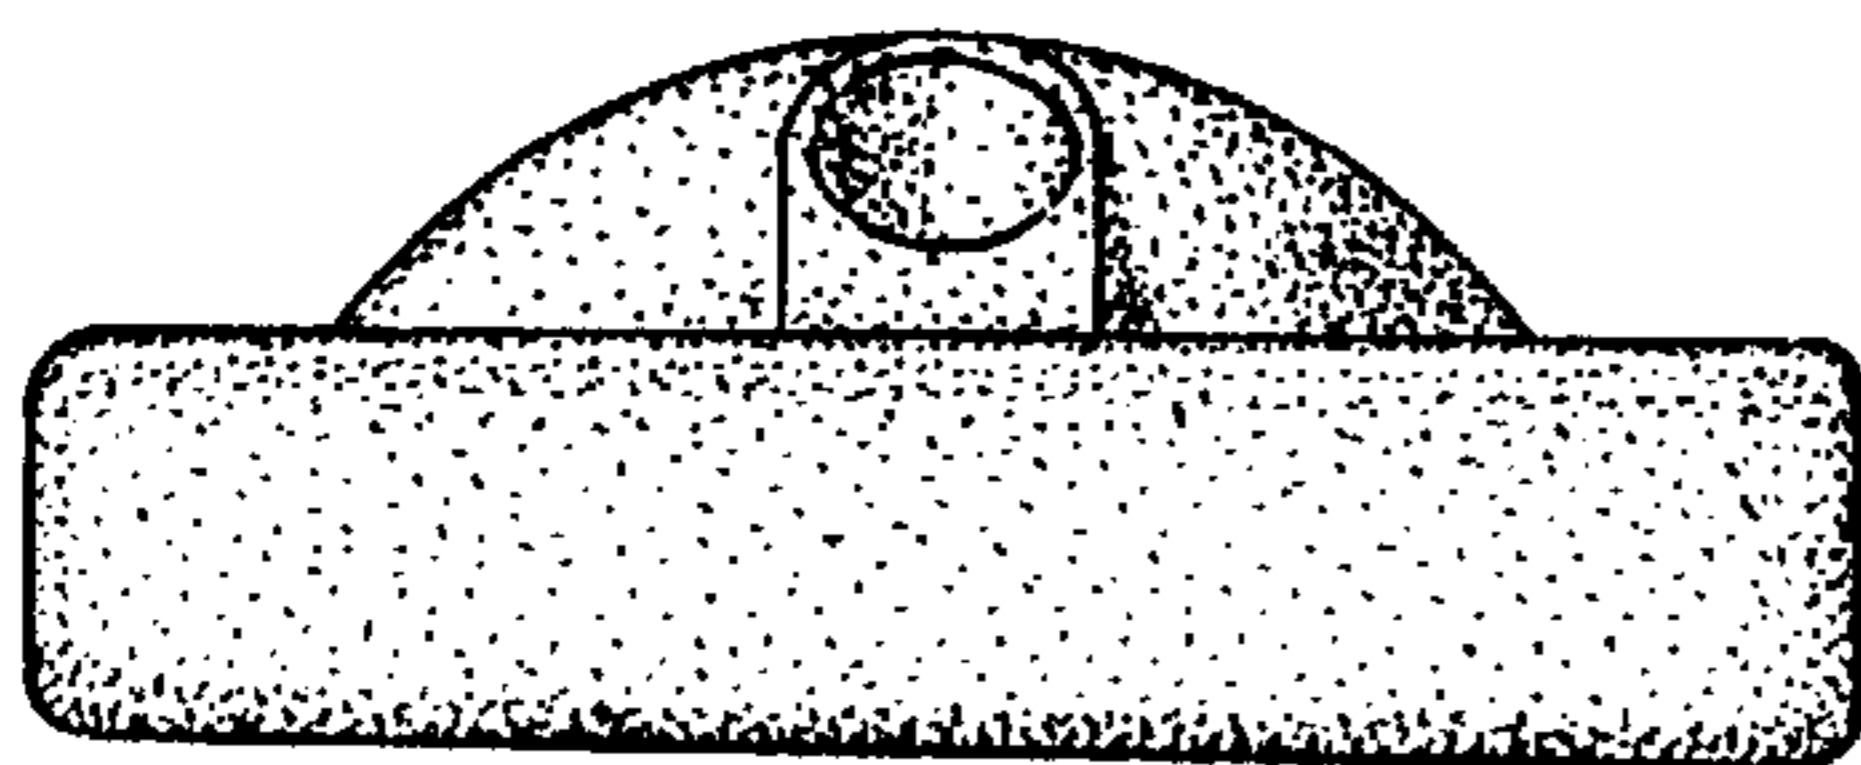


FIG. 1

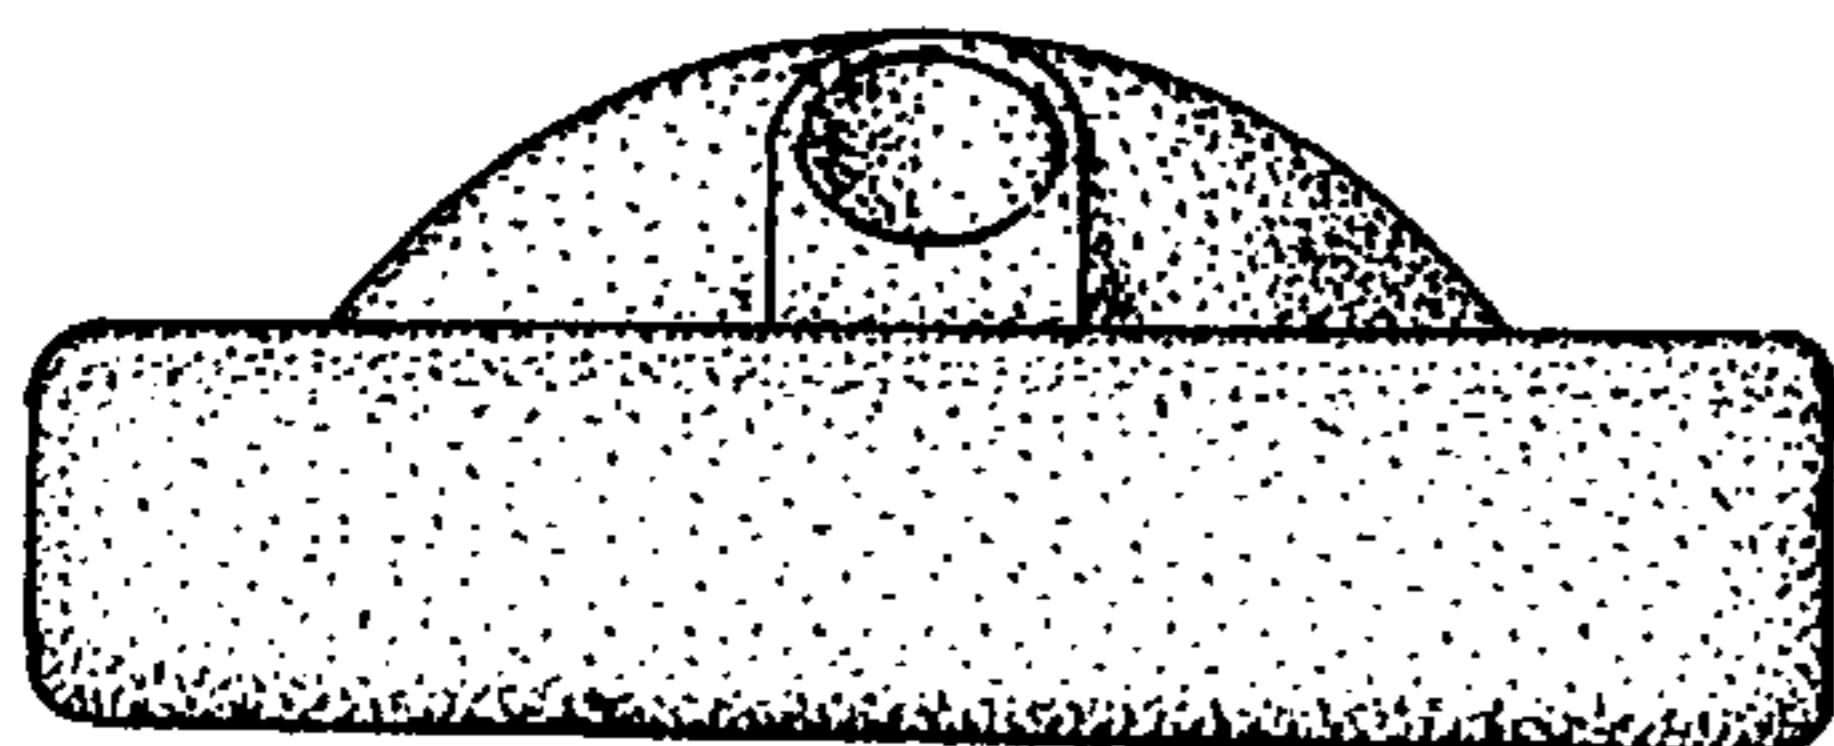


FIG. 2

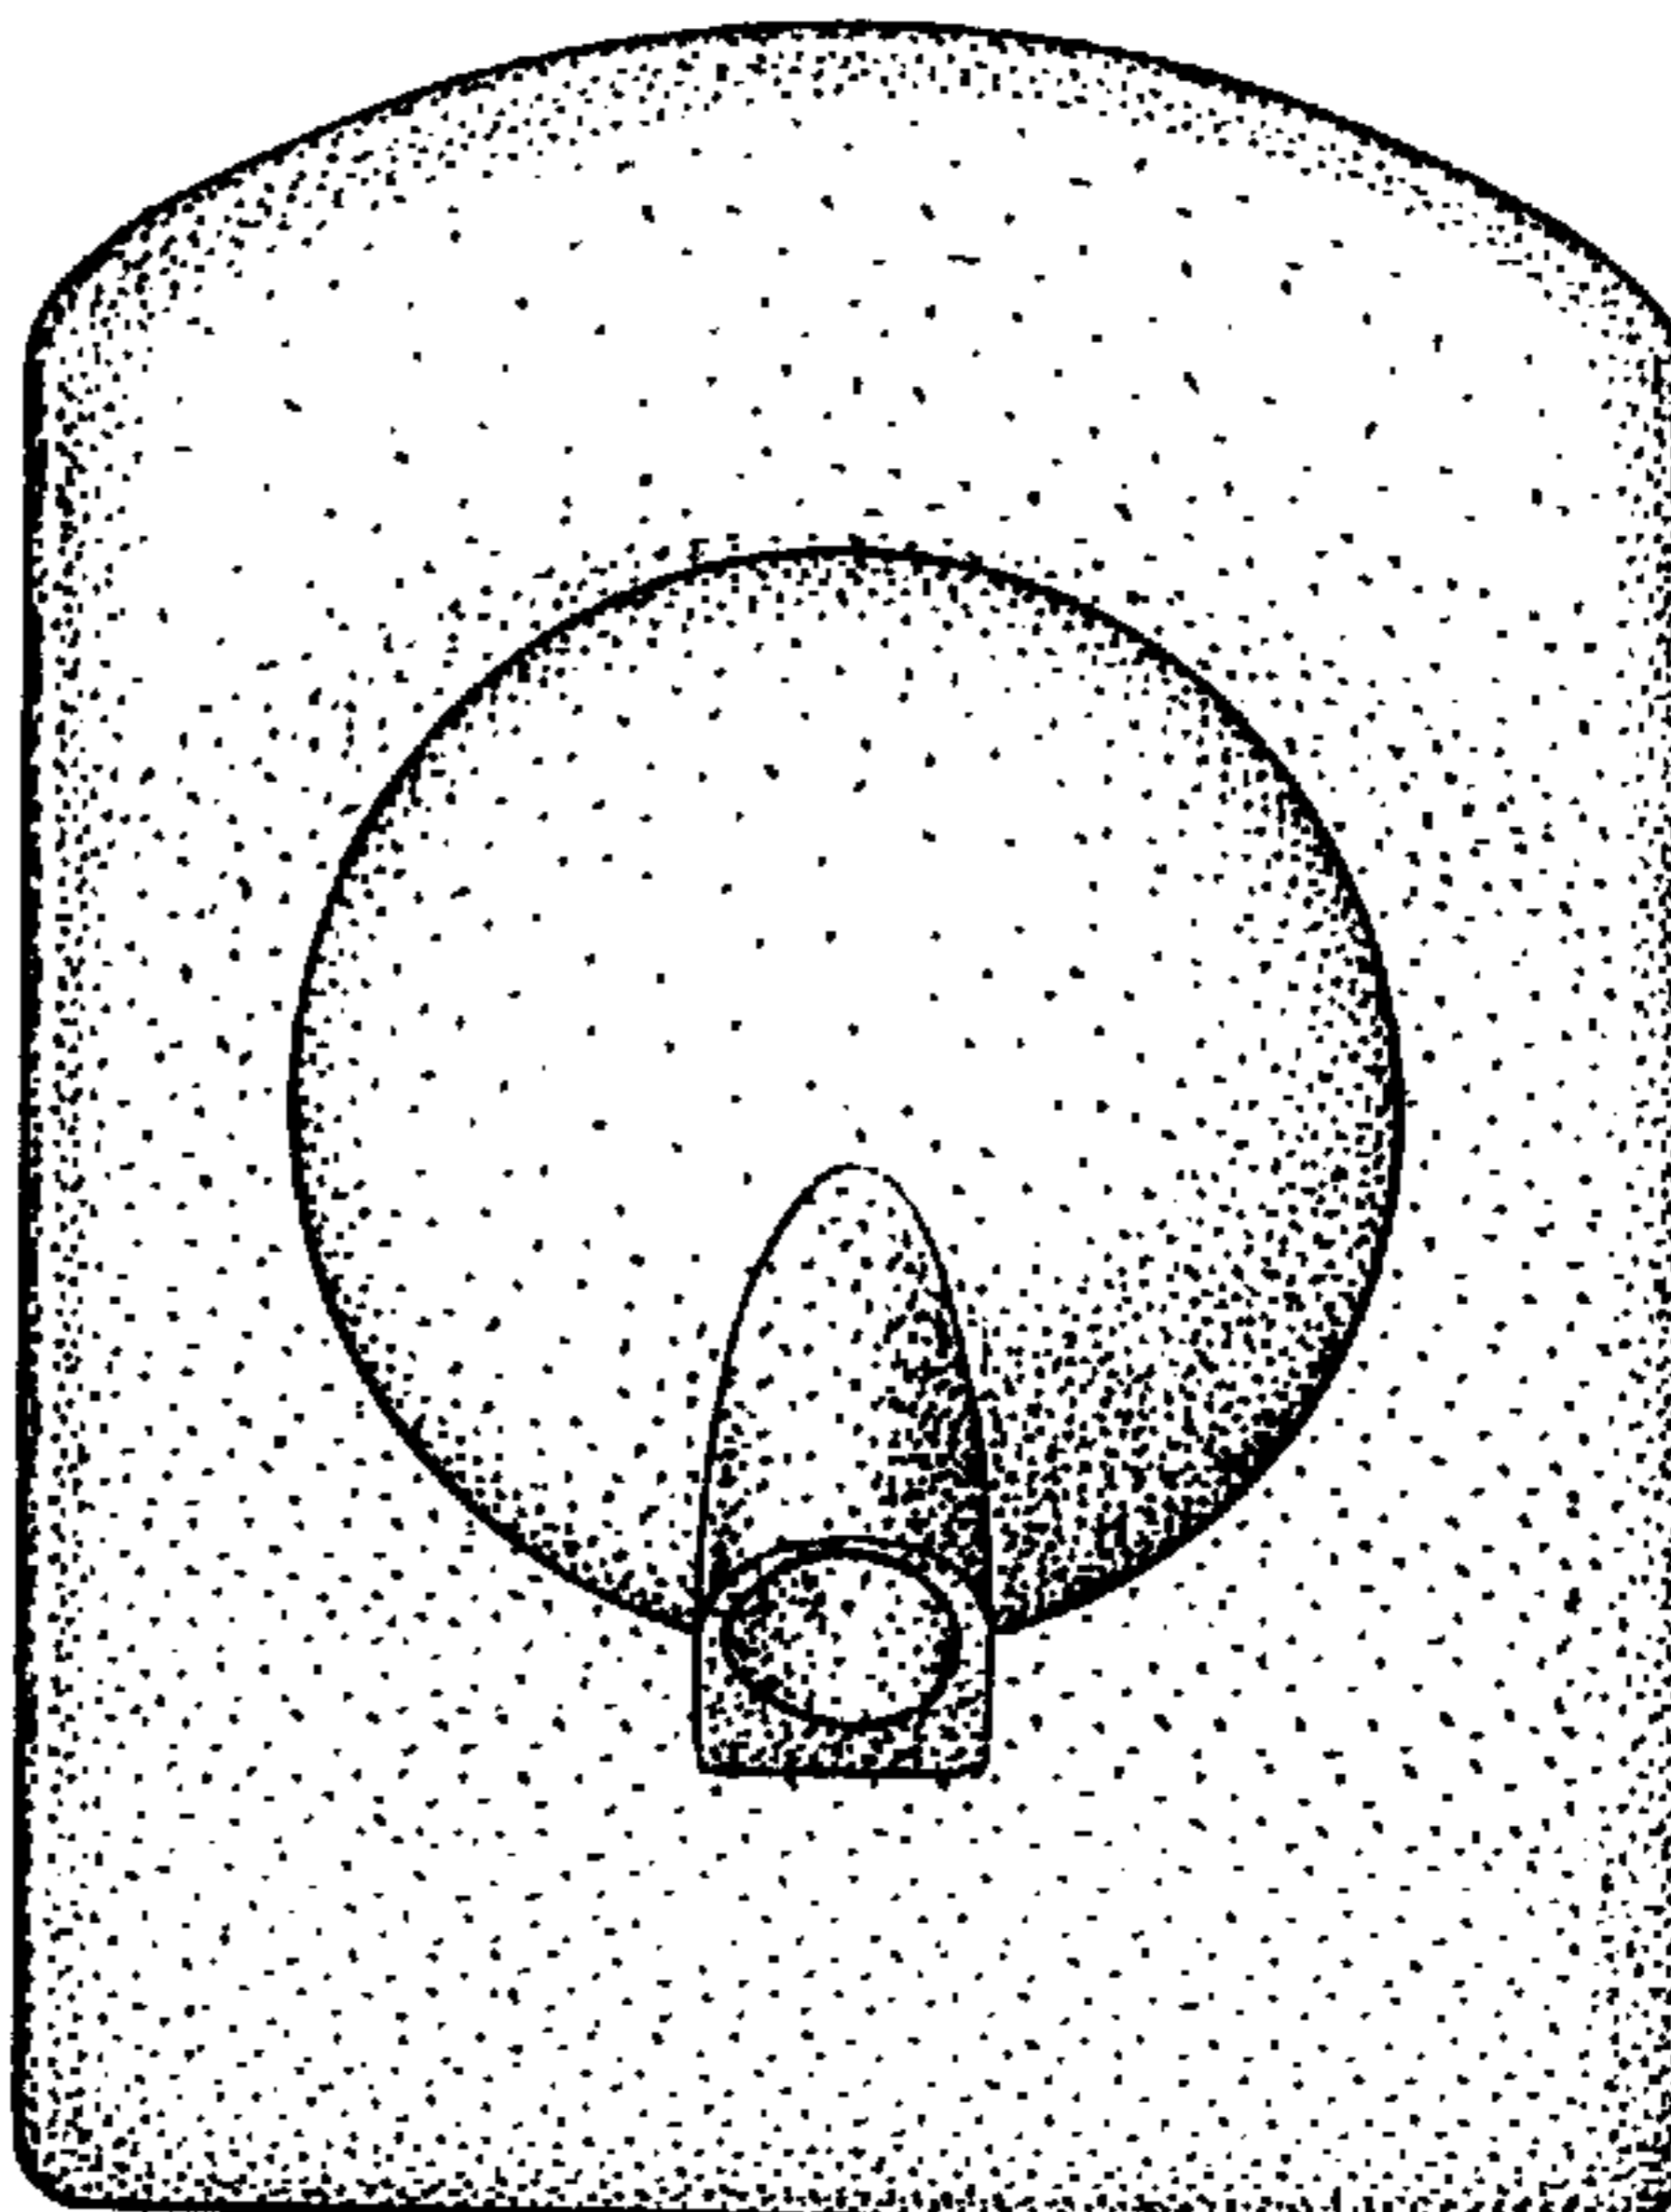


FIG. 3

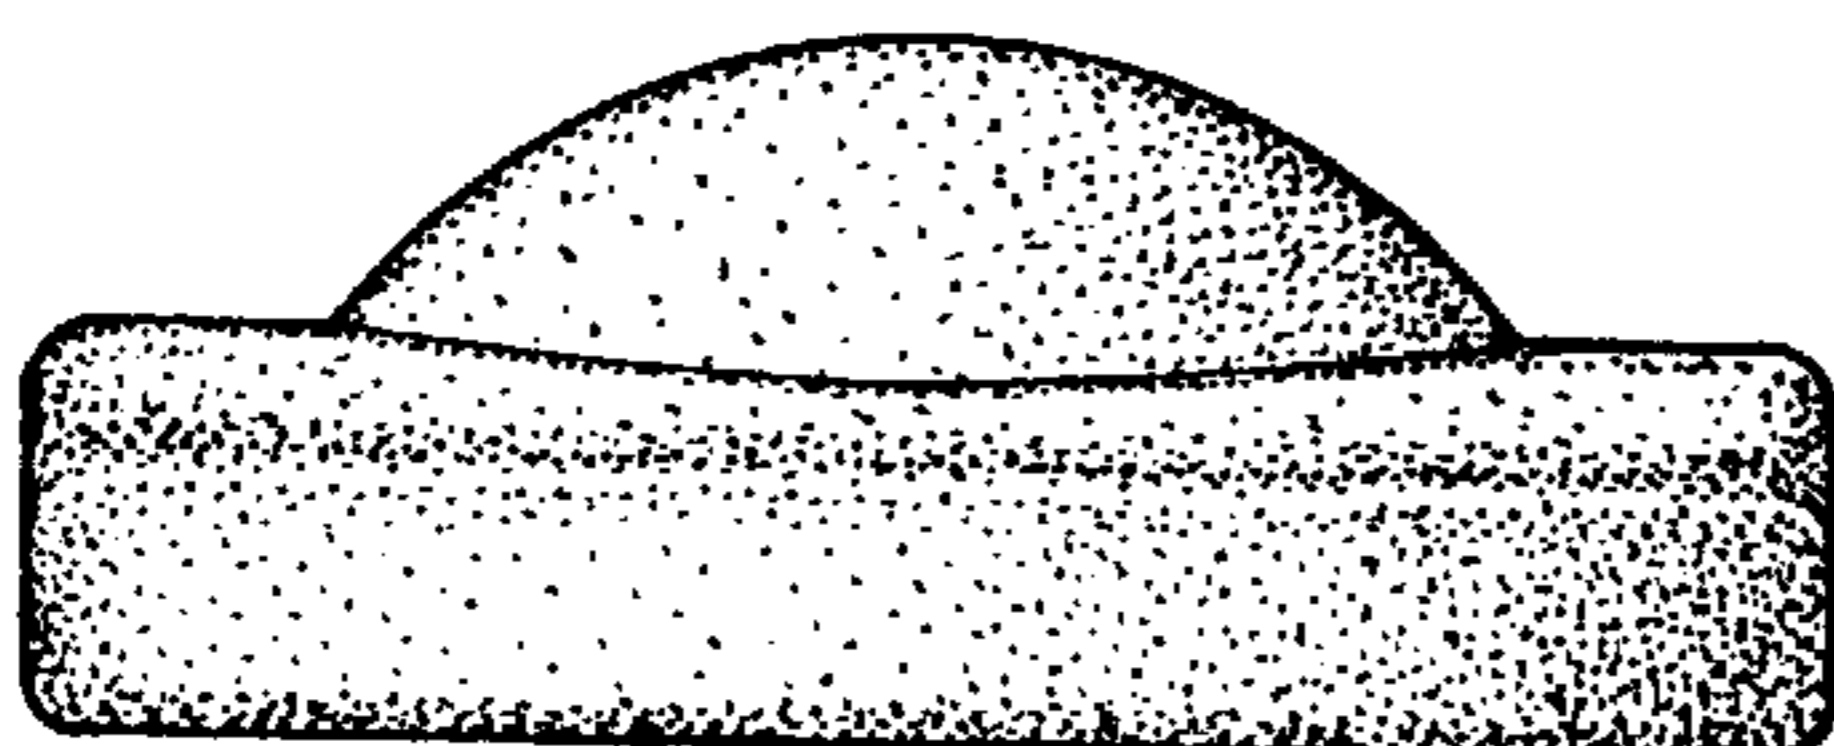


FIG. 4

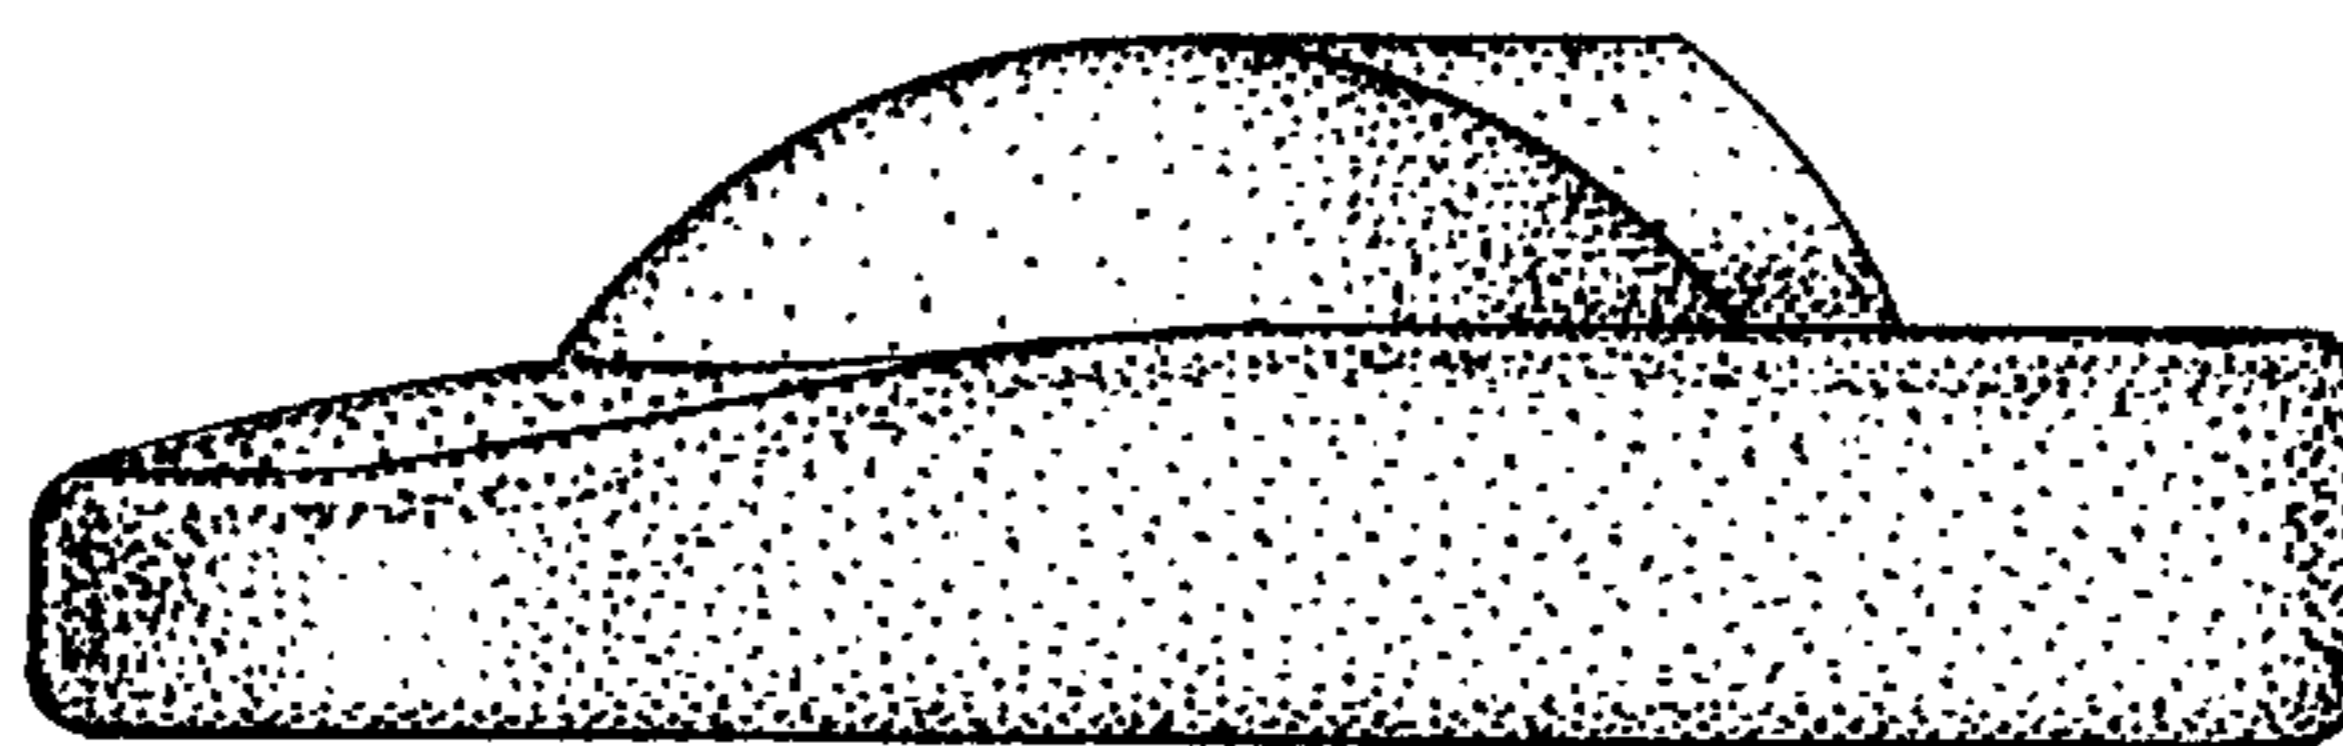


FIG. 5

