



US00D411008S

United States Patent [19]
Gaba et al.

[11] **Patent Number: Des. 411,008**
[45] **Date of Patent: ** Jun. 15, 1999**

[54] **CABINET FOR HOUSING A MEDICAL WASTE CONTAINER**

[75] Inventors: **Rodolfo Gaba**, Simi Valley; **Michael Griffin**, Agua Dulce, both of Calif.; **Ignaty Gusakov**, East Aurora, N.Y.; **Ruane S. Jeter**, Los Angeles; **Gordon H. Marsh**, West Hills, both of Calif.

[73] Assignee: **Graphic Controls Corporation**, Buffalo, N.Y.

[**] Term: **14 Years**

[21] Appl. No.: **29/079,532**

[22] Filed: **Nov. 7, 1997**

[51] **LOC (6) Cl.** **24-01**

[52] **U.S. Cl.** **D24/131**

[58] **Field of Search** D24/131; D34/7, D34/8; 206/363-366, 370

“Infection Control Illustrating Herculite of Devon Industries, Inc.,” Hospital Purchasing News (1996).

“Bemis Delivers Exceptional Quality In The Sharps Disposal Units You Depend On,” Bemis Manufacturing Company (1996).

“Encore Sharps Collection Unit,” Devon Industries, Inc. (Jul., 1996).

“In-Room Sharps Disposal System,” Sage Products, Inc. (1993).

“VHA+Plus Sharps Disposal Containers,” VHA Supply Co. (1991).

“How To Use The In-Room Wall Enclosure System,” Sage Products, Inc. (1993).

Primary Examiner—Louis S. Zarfes

Assistant Examiner—G. Andoll

Attorney, Agent, or Firm—Ratner & Prestia

[57] **CLAIM**

The ornamental design for a cabinet for housing a medical waste container, as shown and described.

[56] **References Cited**

U.S. PATENT DOCUMENTS

- Re. 33,413 10/1990 Hanifl .
- D. 304,493 11/1989 Bemis D24/131
- D. 307,841 5/1990 Hanifl et al. .
- D. 332,680 1/1993 Ramirez .

(List continued on next page.)

FOREIGN PATENT DOCUMENTS

- 85 03 511 6/1985 Germany .

OTHER PUBLICATIONS

European Search Report Dated Feb. 19, 1998.

“Sharps—A—Gator, Sharps Collection and Disposal System, Point—Of—Use Sharps Containers,” CA—4833—1, Devon Industries, Inc. (1992).

“VHA+Plus Sharps Container,” Sales Manual, VHA Supply Co. (1989).

“Sharps Container System Product Profile,” Sherwood Medical (1989).

“Stop—Don’t Get Stuck With an Obsolete Sharps Disposal System,” Premium Plastics, Inc. (1988).

DESCRIPTION

FIG. 1 is a perspective view illustrating the front, right side, and top of a cabinet for housing a medical waste container, showing our new design;

FIG. 2 is a perspective view illustrating the rear, left side, and bottom of the cabinet for housing a medical waste container shown in FIG. 1;

FIG. 3 is a front view of the cabinet for housing a medical waste container shown in FIGS. 1 and 2;

FIG. 4 is a right side view of the cabinet for housing a medical waste container shown in FIGS. 1 and 2;

FIG. 5 is a rear view of the cabinet for housing a medical waste container shown in FIGS. 1 and 2;


FIG. 6 is a left side view of the cabinet for housing a medical waste container shown in FIGS. 1 and 2;

FIG. 7 is a top view of the cabinet for housing a medical waste container shown in FIGS. 1 and 2; and,

FIG. 8 is a bottom view of the cabinet for housing a medical waste container shown in FIGS. 1 and 2.

The broken lines in the Figures is for illustrative purposes only and forms no part of the claimed design.

1 Claim, 4 Drawing Sheets

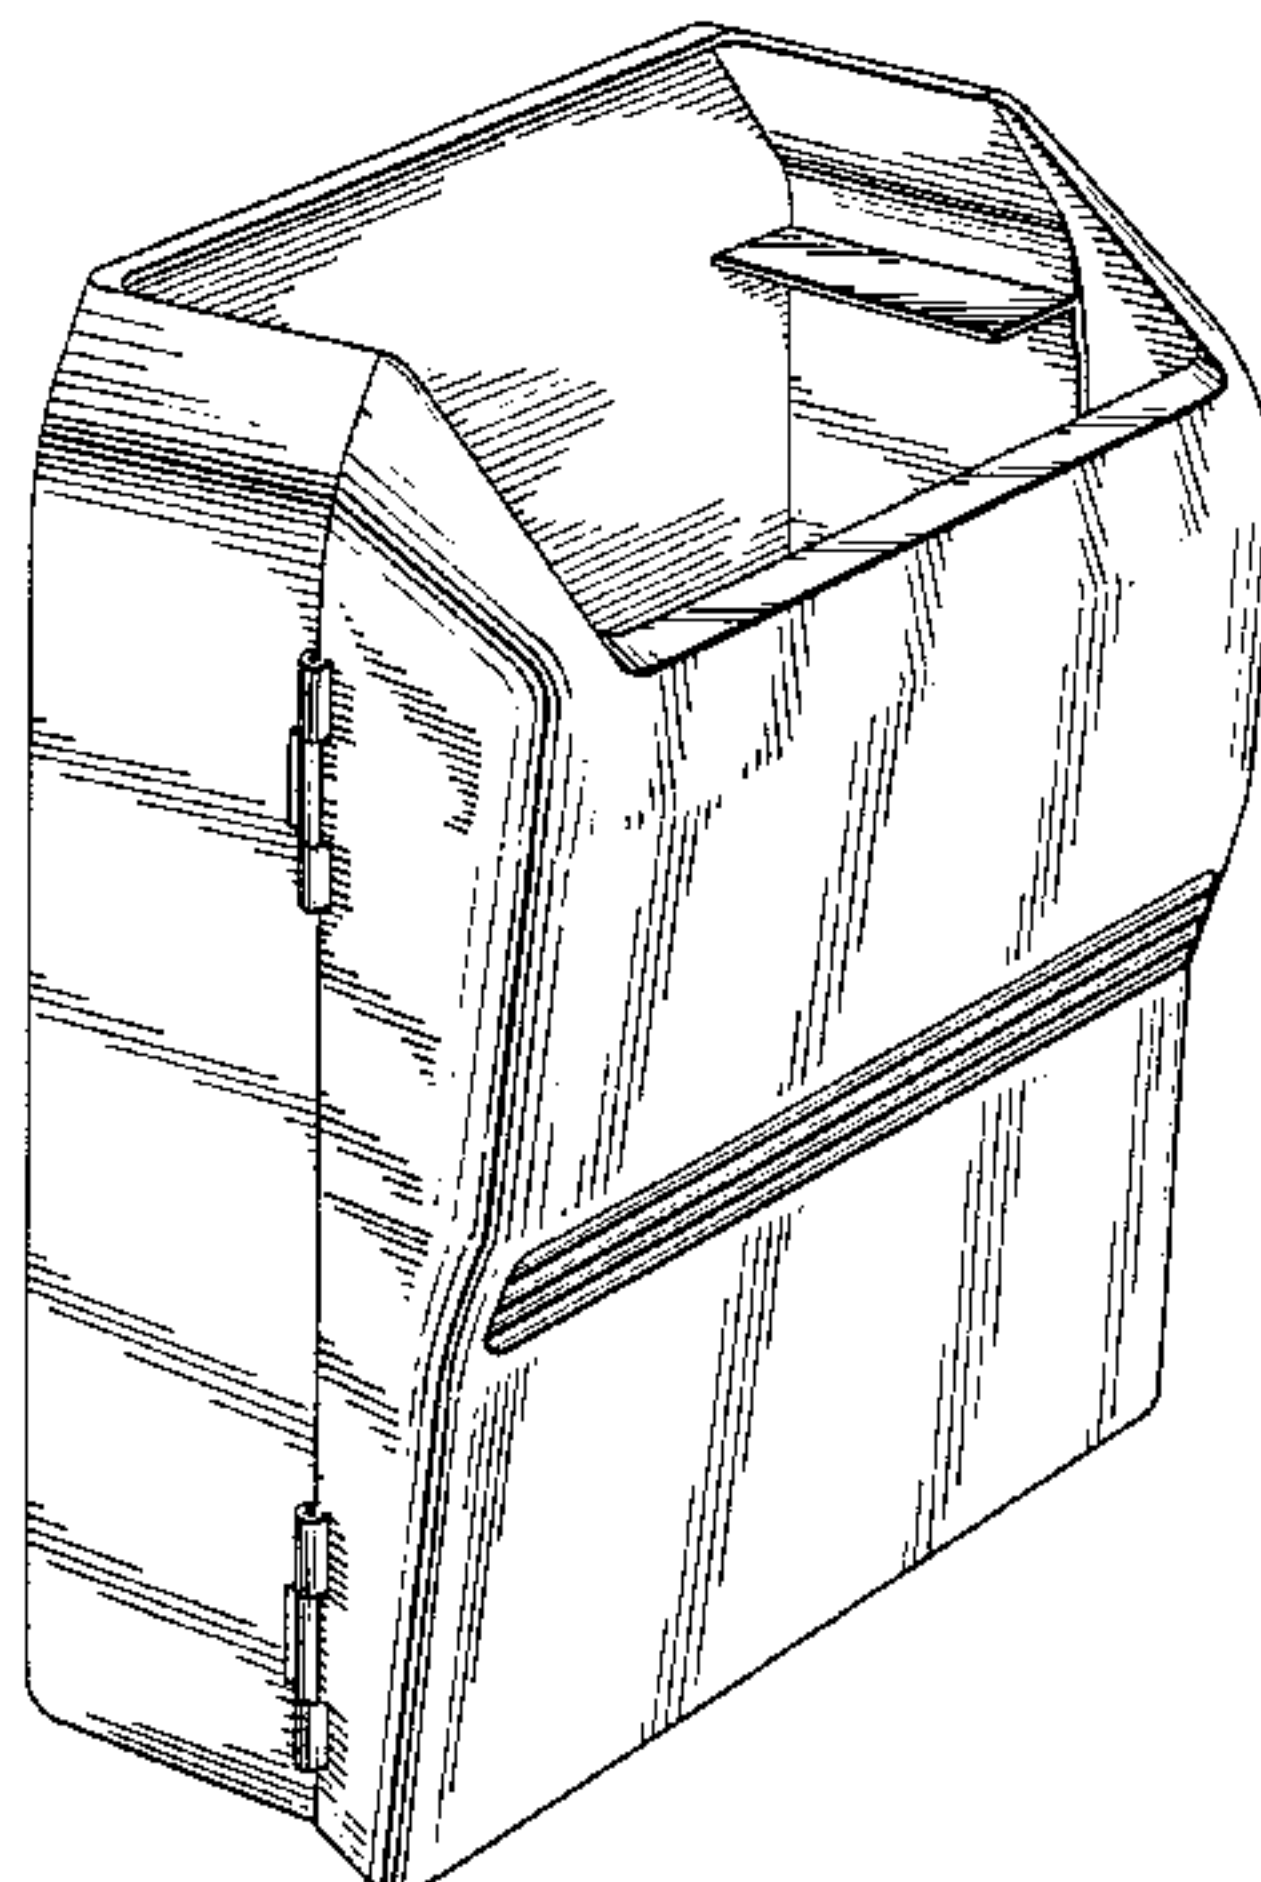

Des. 411,008

Page 2

U.S. PATENT DOCUMENTS					
			4,903,832	2/1990	Stewart .
			4,927,076	5/1990	Simpson .
			4,955,477	9/1990	Bruno .
D. 335,373	5/1993	Mosior .	5,076,429	12/1991	Patrick et al. .
D. 385,349	10/1997	Mosior et al. D24/131	5,080,251	1/1992	Noack .
449,149	3/1891	Whelan .	5,178,322	1/1993	Shillington .
457,918	8/1891	Stevenson et al. .	5,211,303	5/1993	Mosior .
697,655	4/1902	O'Leary .	5,323,994	6/1994	Shillington et al. .
1,333,051	3/1920	Young .	5,387,735	2/1995	Ponsi et al. .
4,580,688	4/1986	Harris et al. .	5,413,243	5/1995	Bemis et al. .
4,714,168	12/1987	Johnson et al. .	5,423,450	6/1995	Shillington et al. .
4,715,498	12/1987	Hanifl .	5,465,841	11/1995	Wilson et al. .
4,779,728	10/1988	Hanifl et al. .	5,494,186	2/1996	Marsh .
4,809,850	3/1989	Laible et al. 206/366	5,603,404	2/1997	Nazare et al. .
4,828,107	5/1989	Spencer .	5,605,245	2/1997	Bemis et al. .
4,863,057	9/1989	Hanifl et al. .			

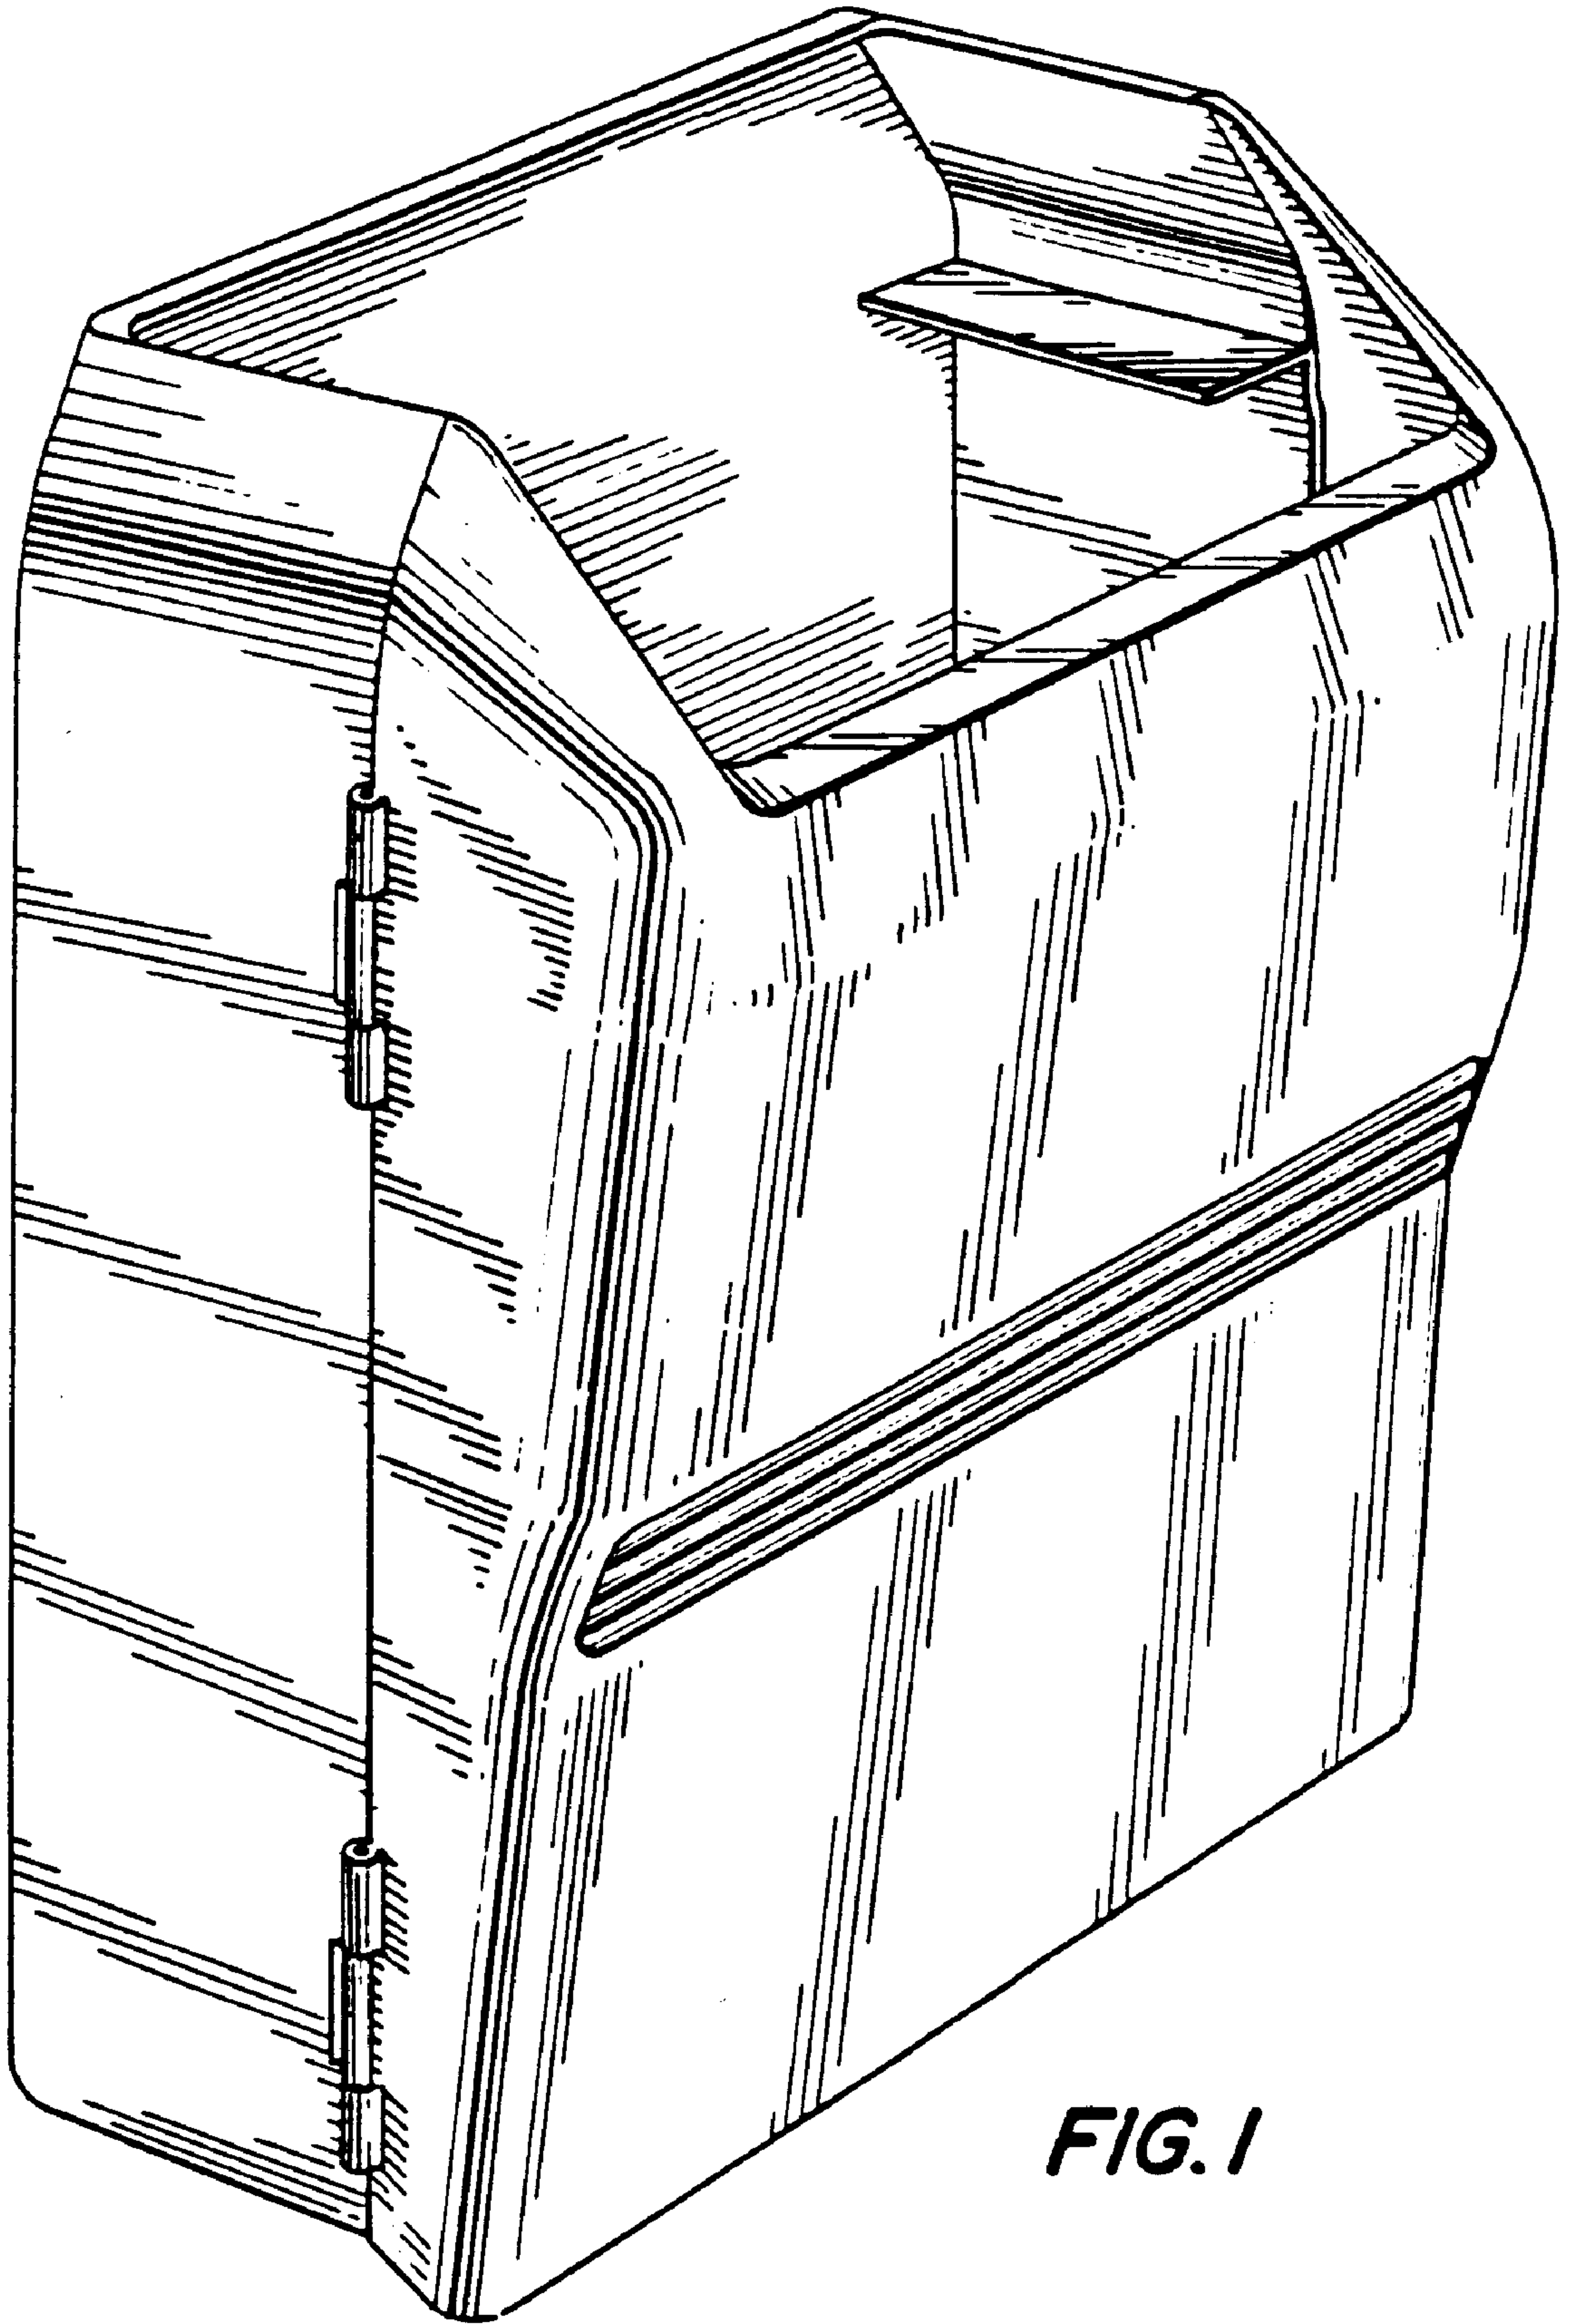


FIG. 1

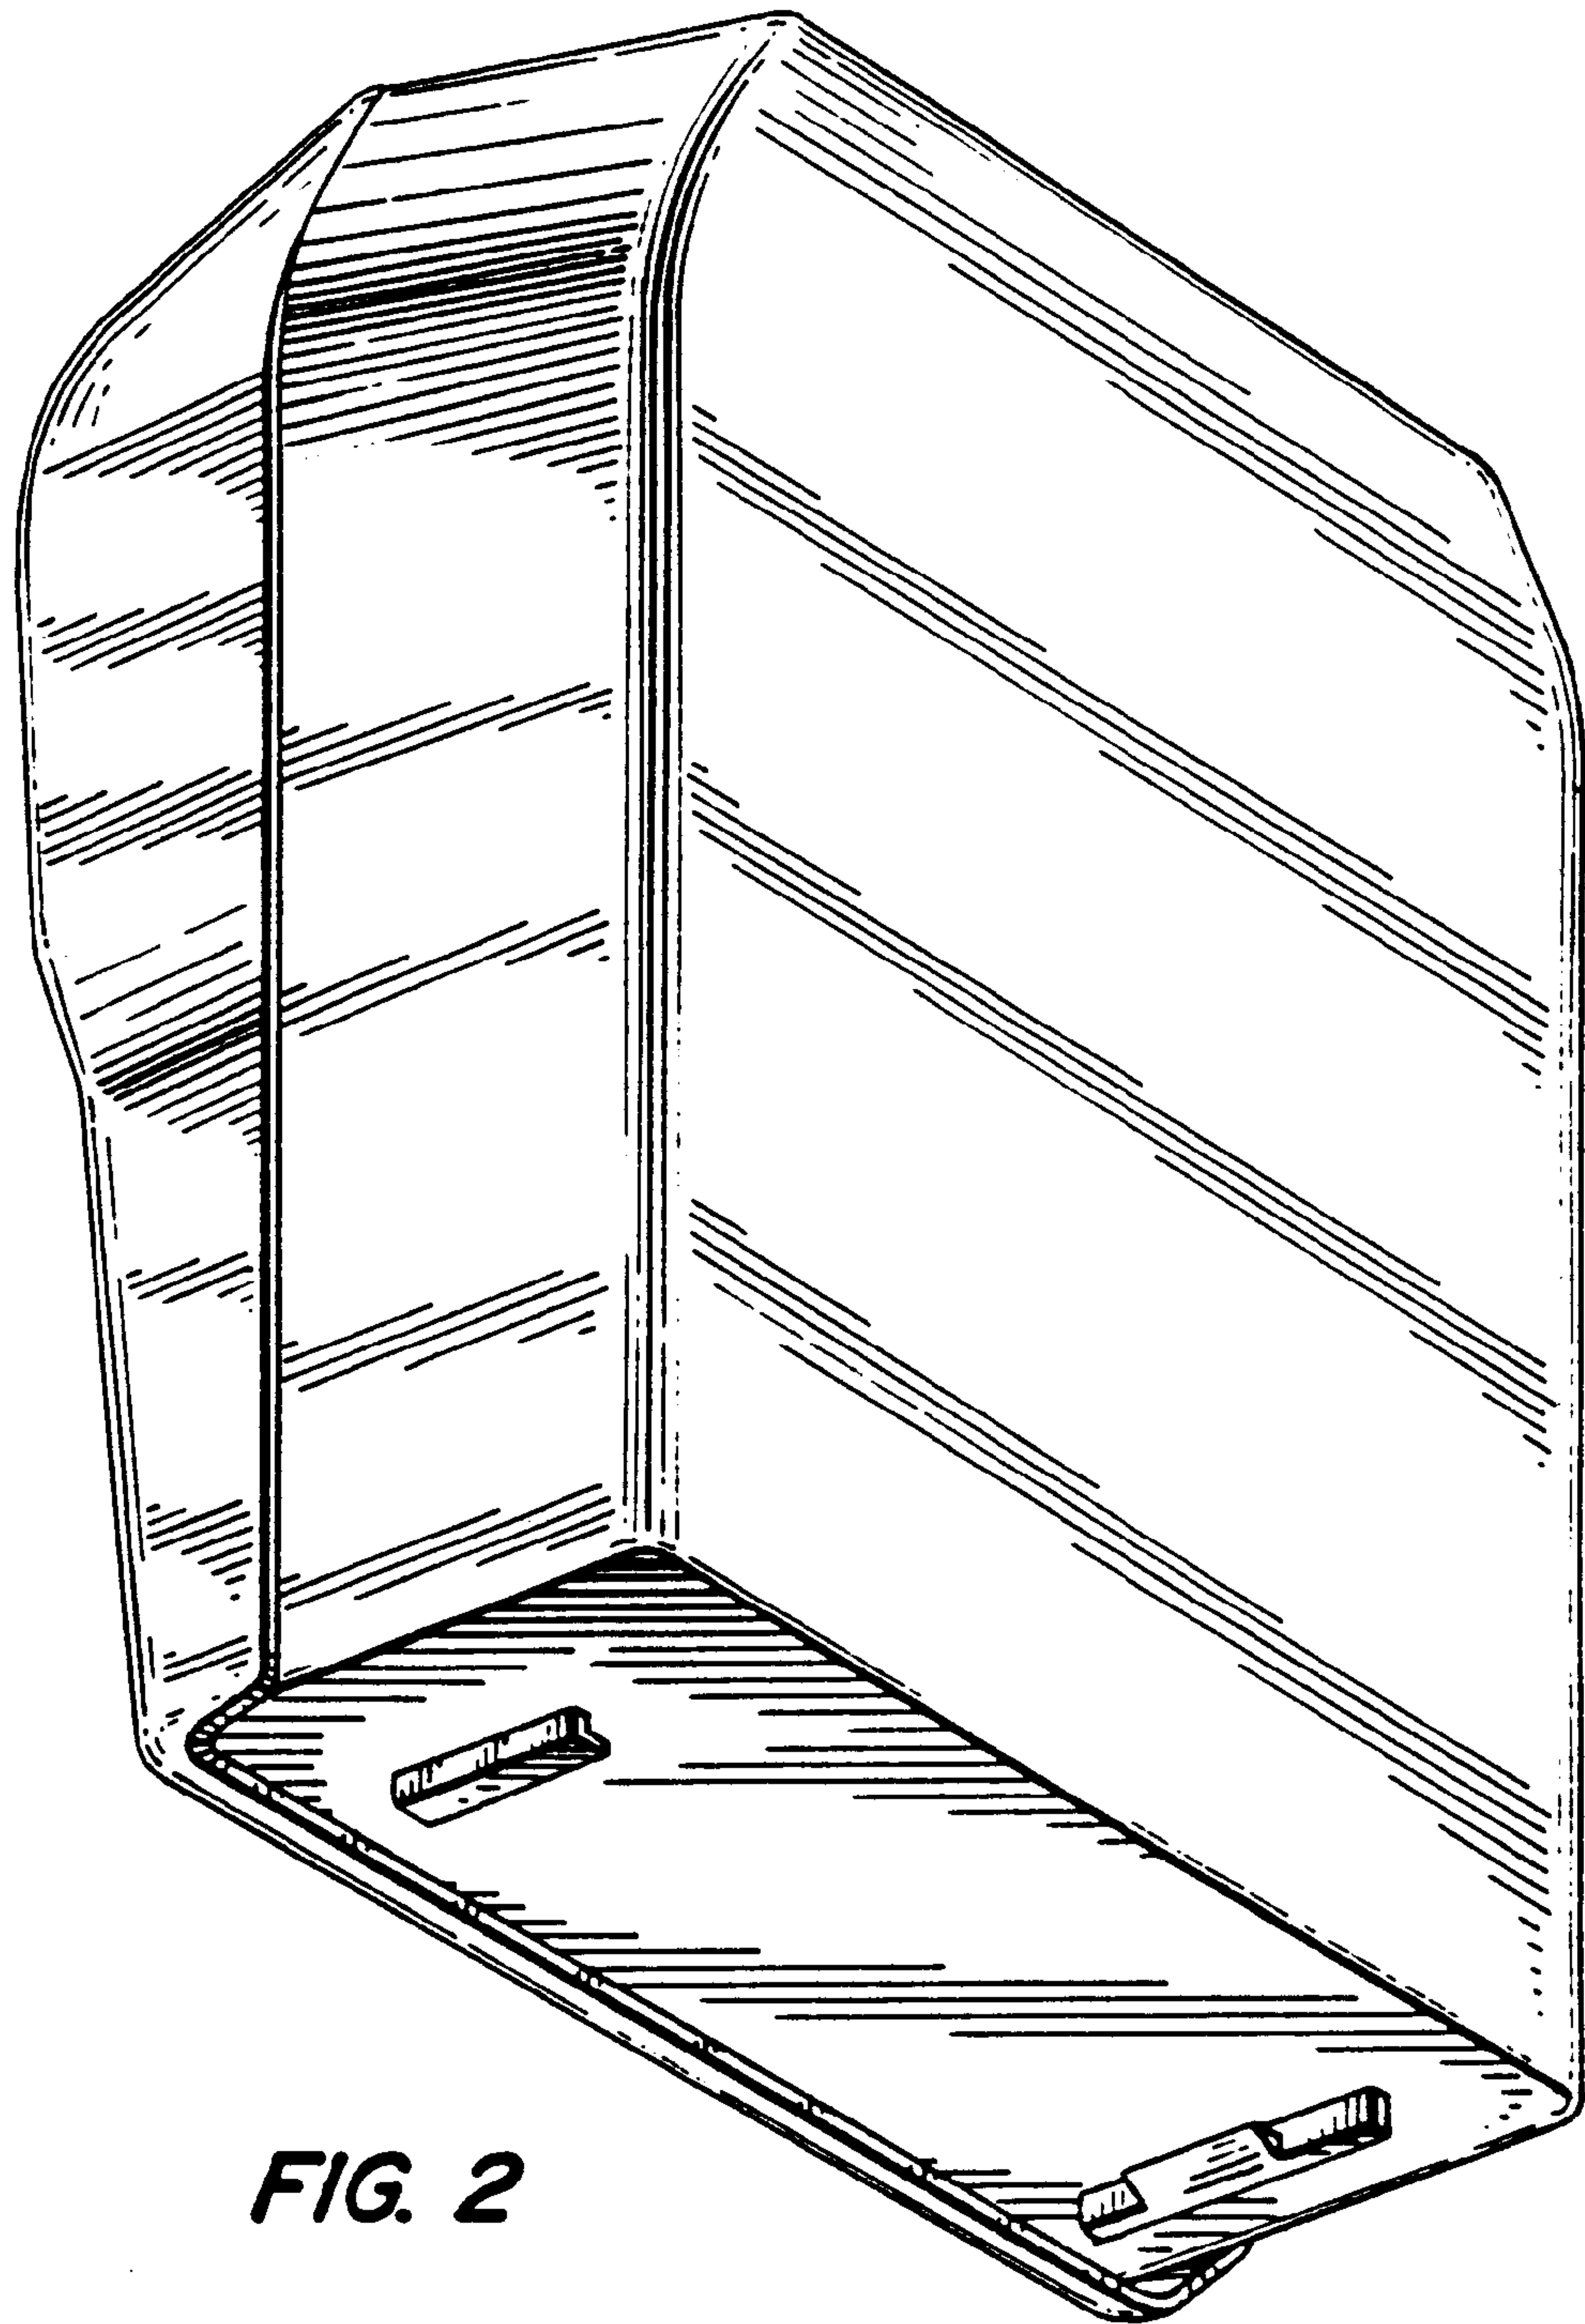


FIG. 2

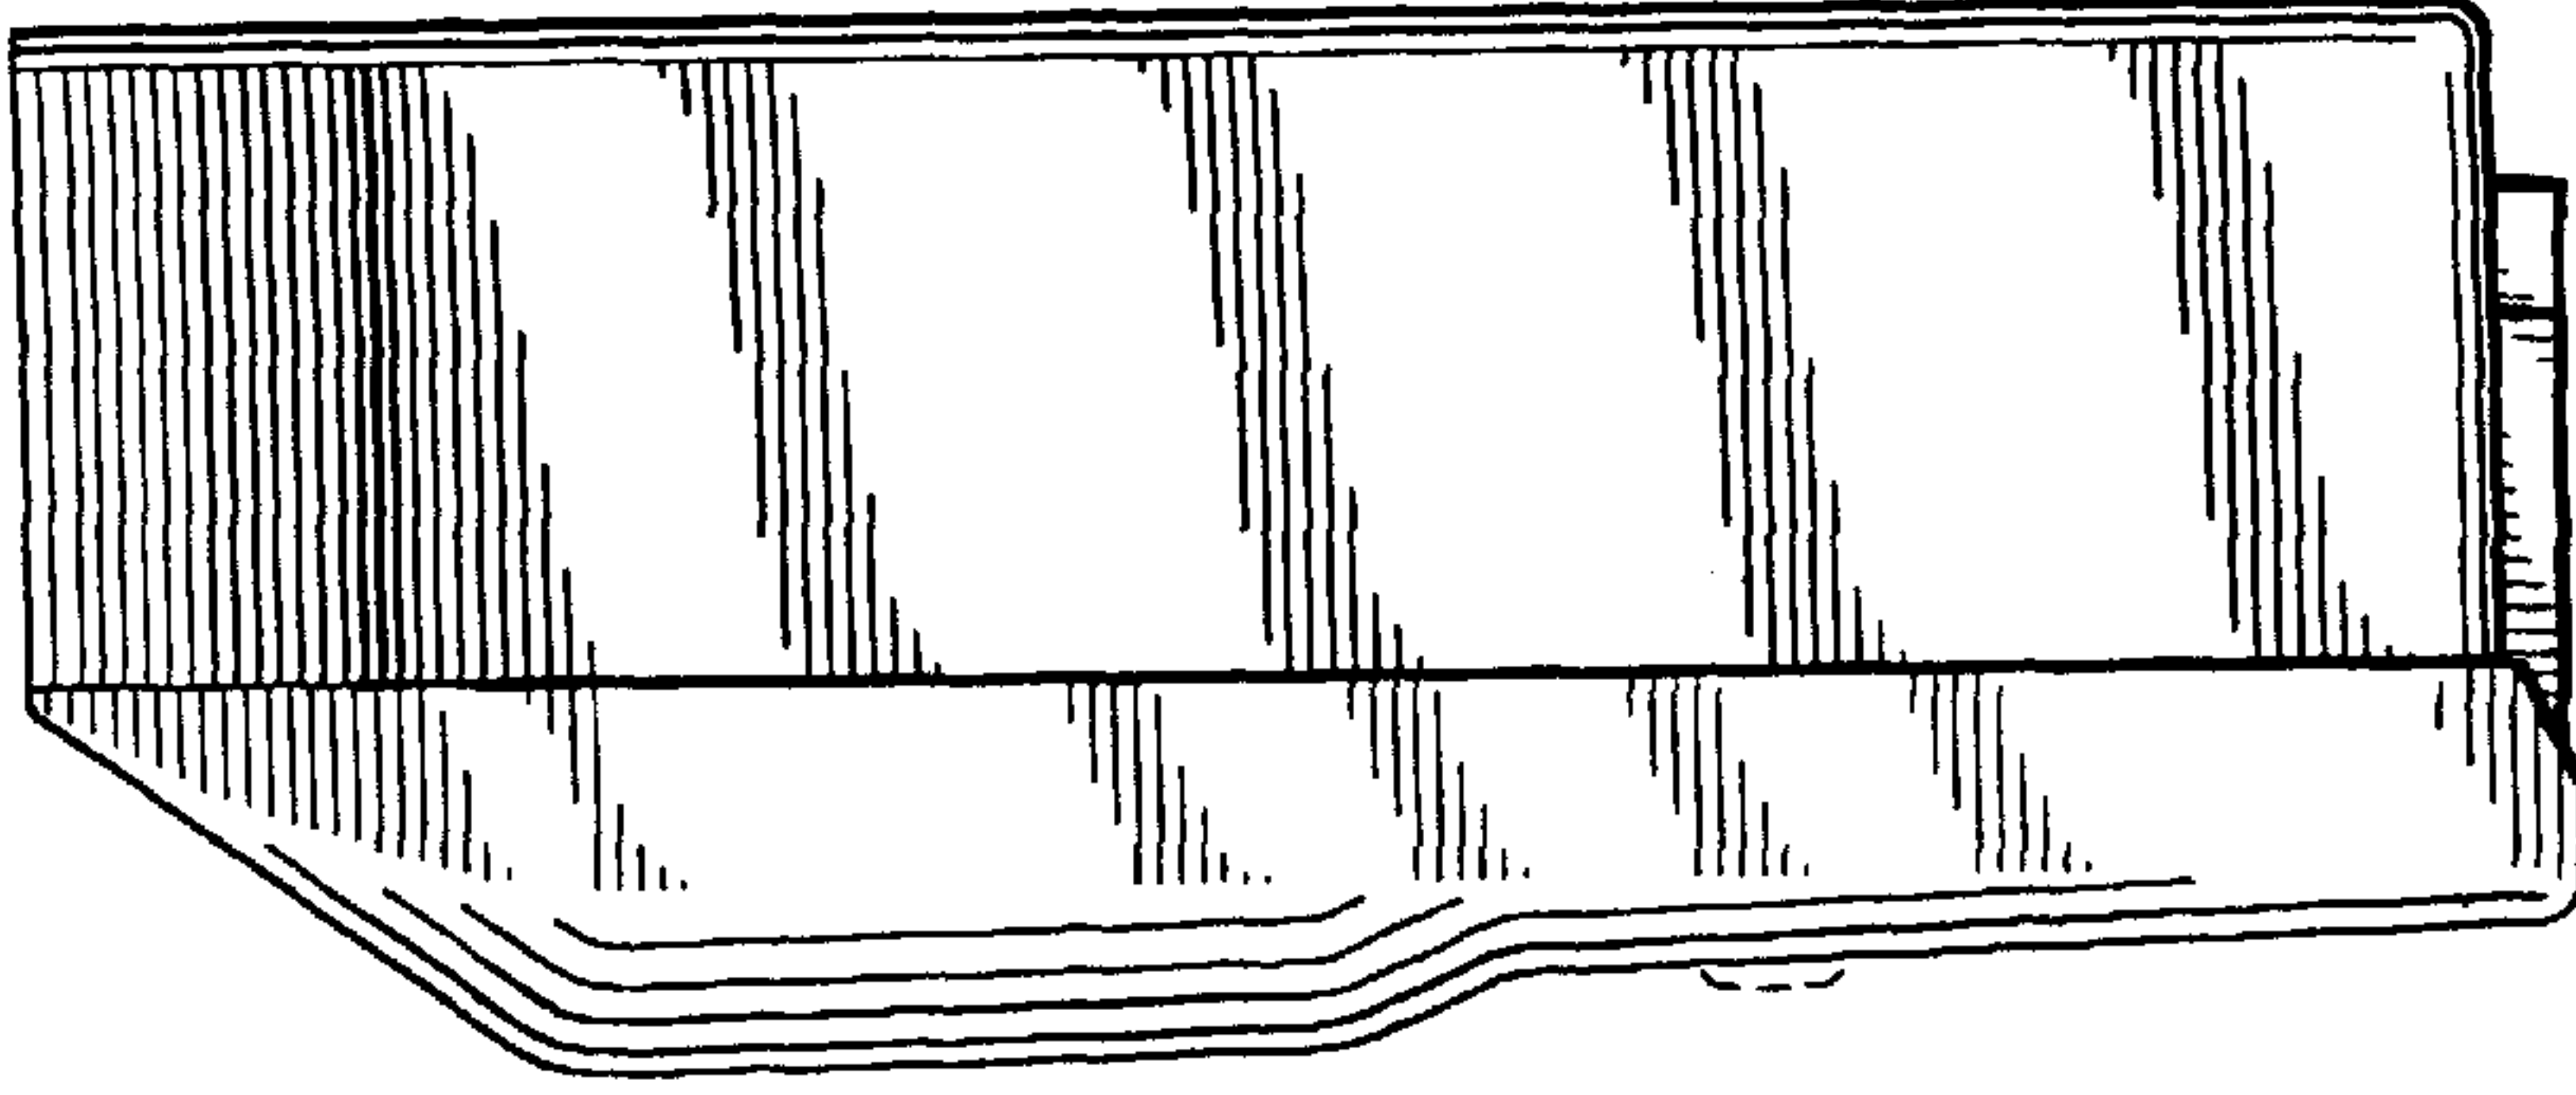


Fig. 6

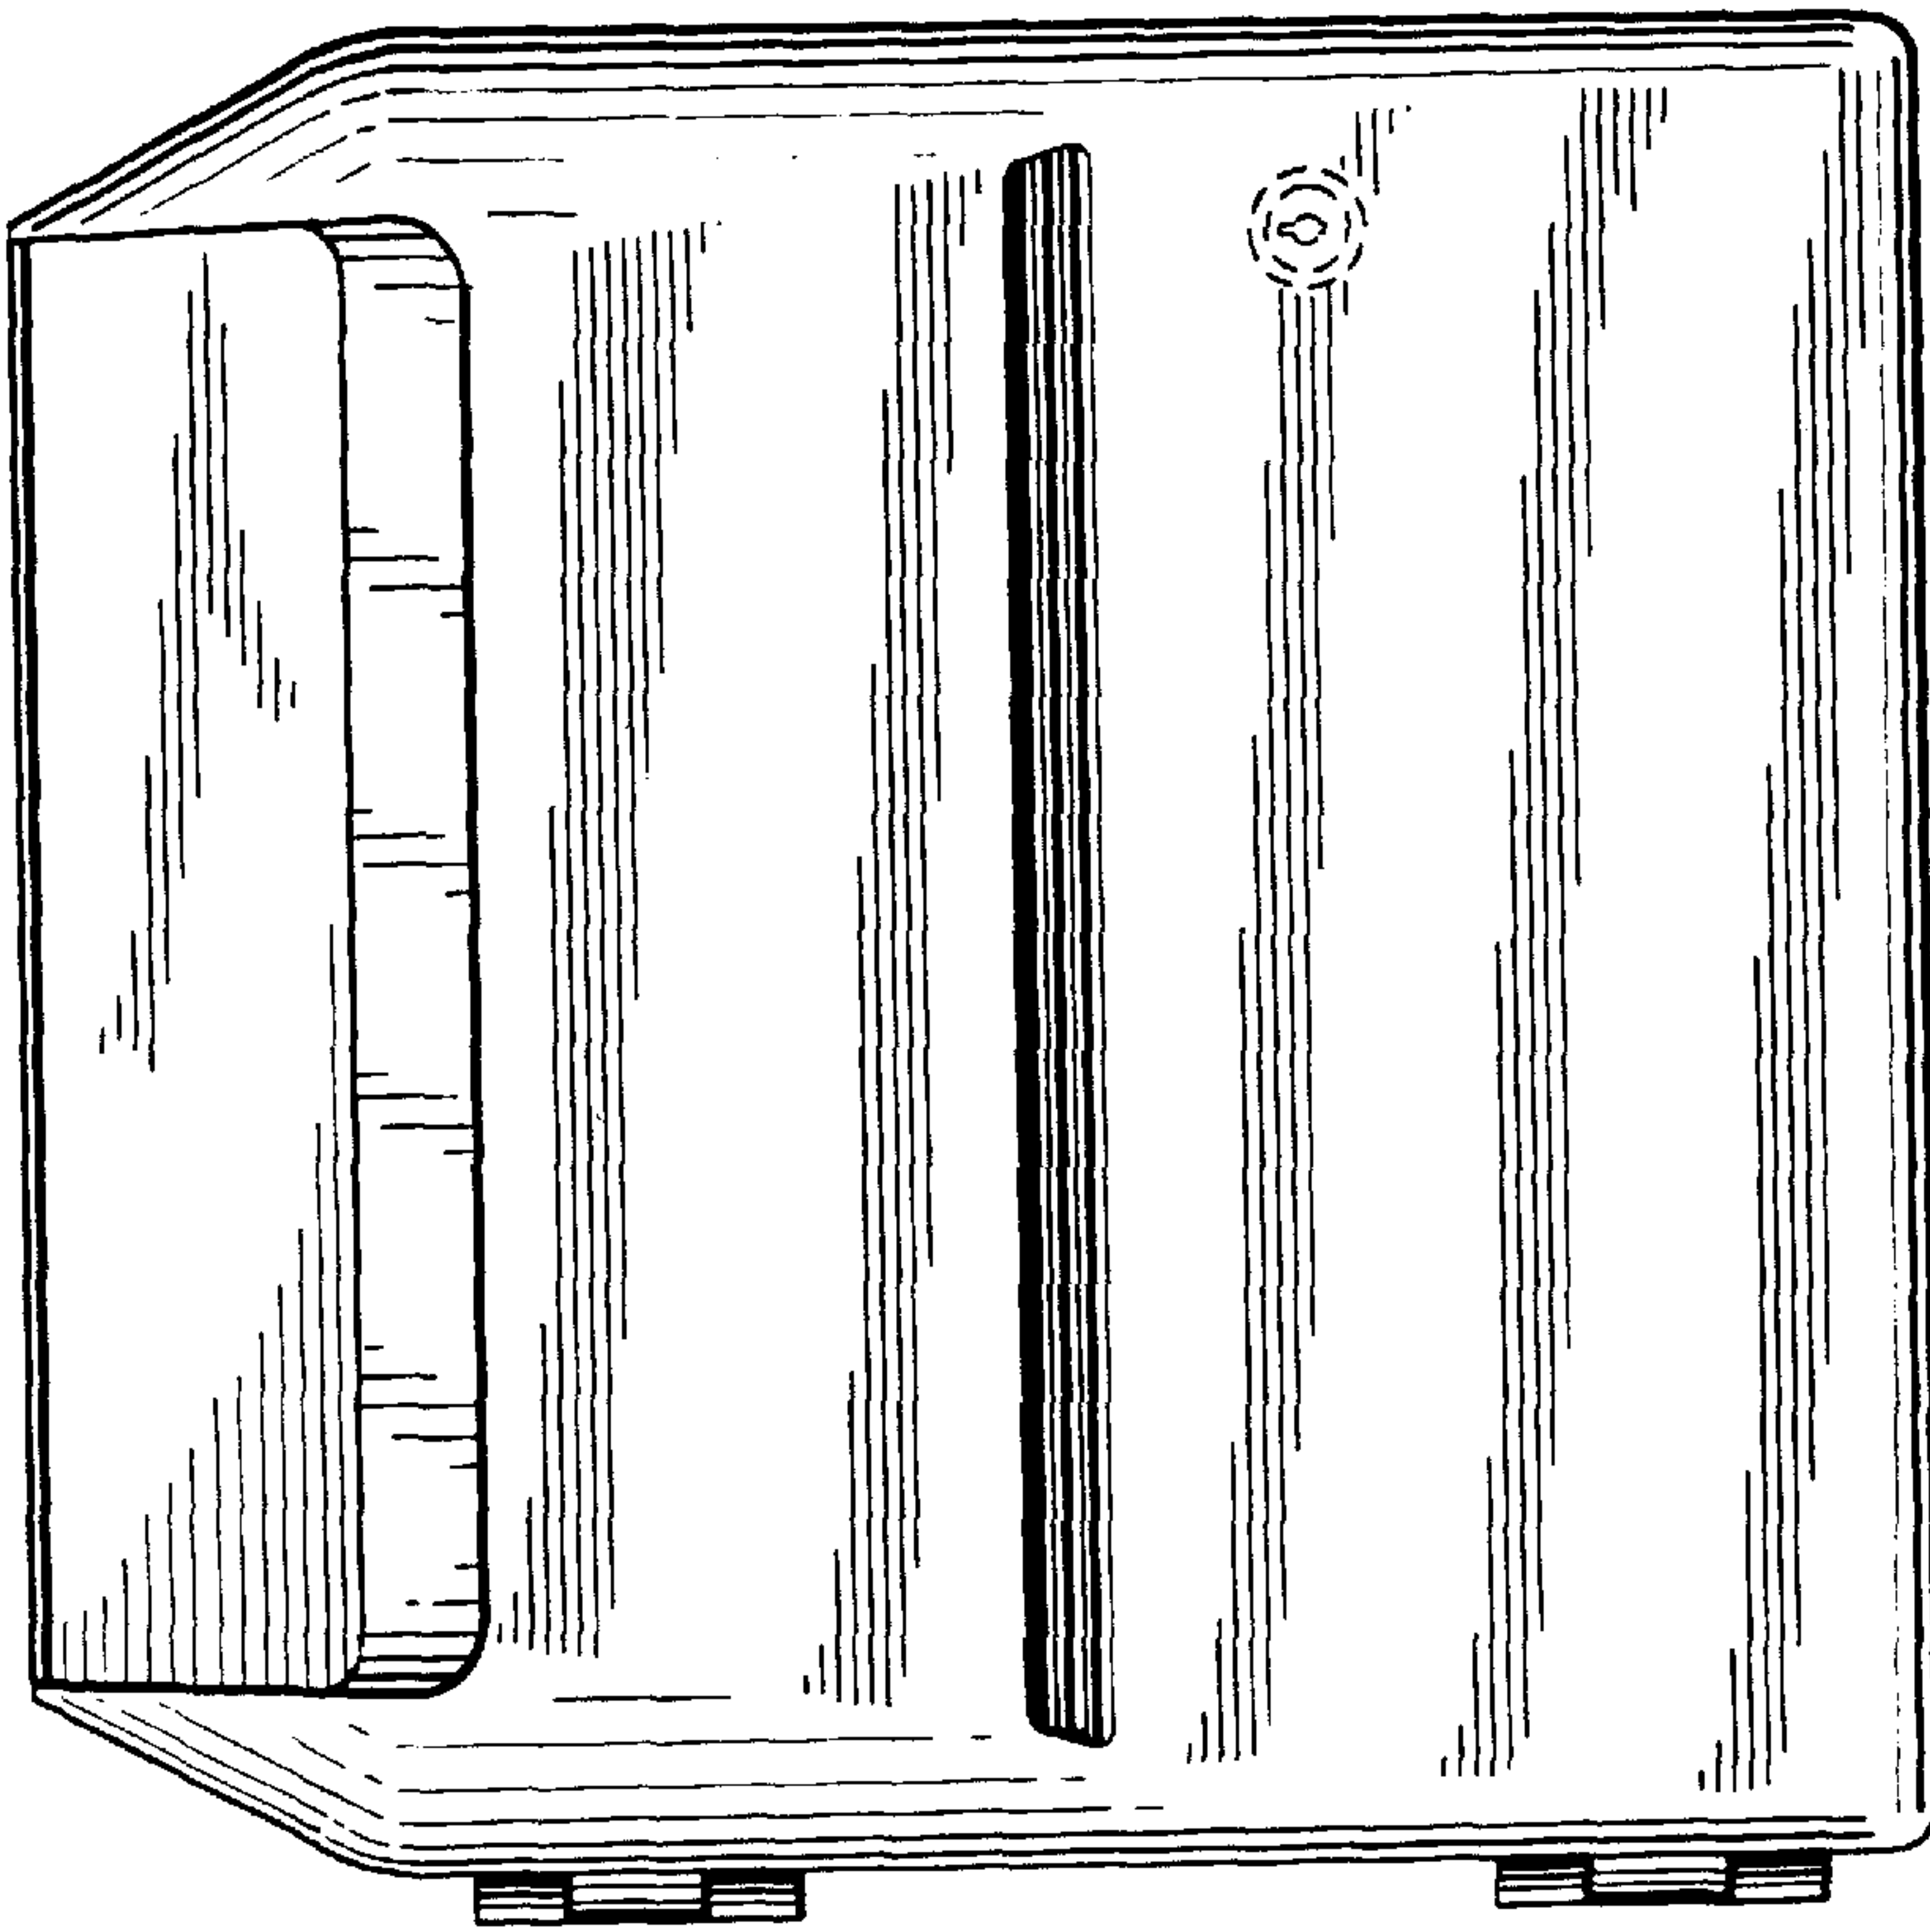


Fig. 3

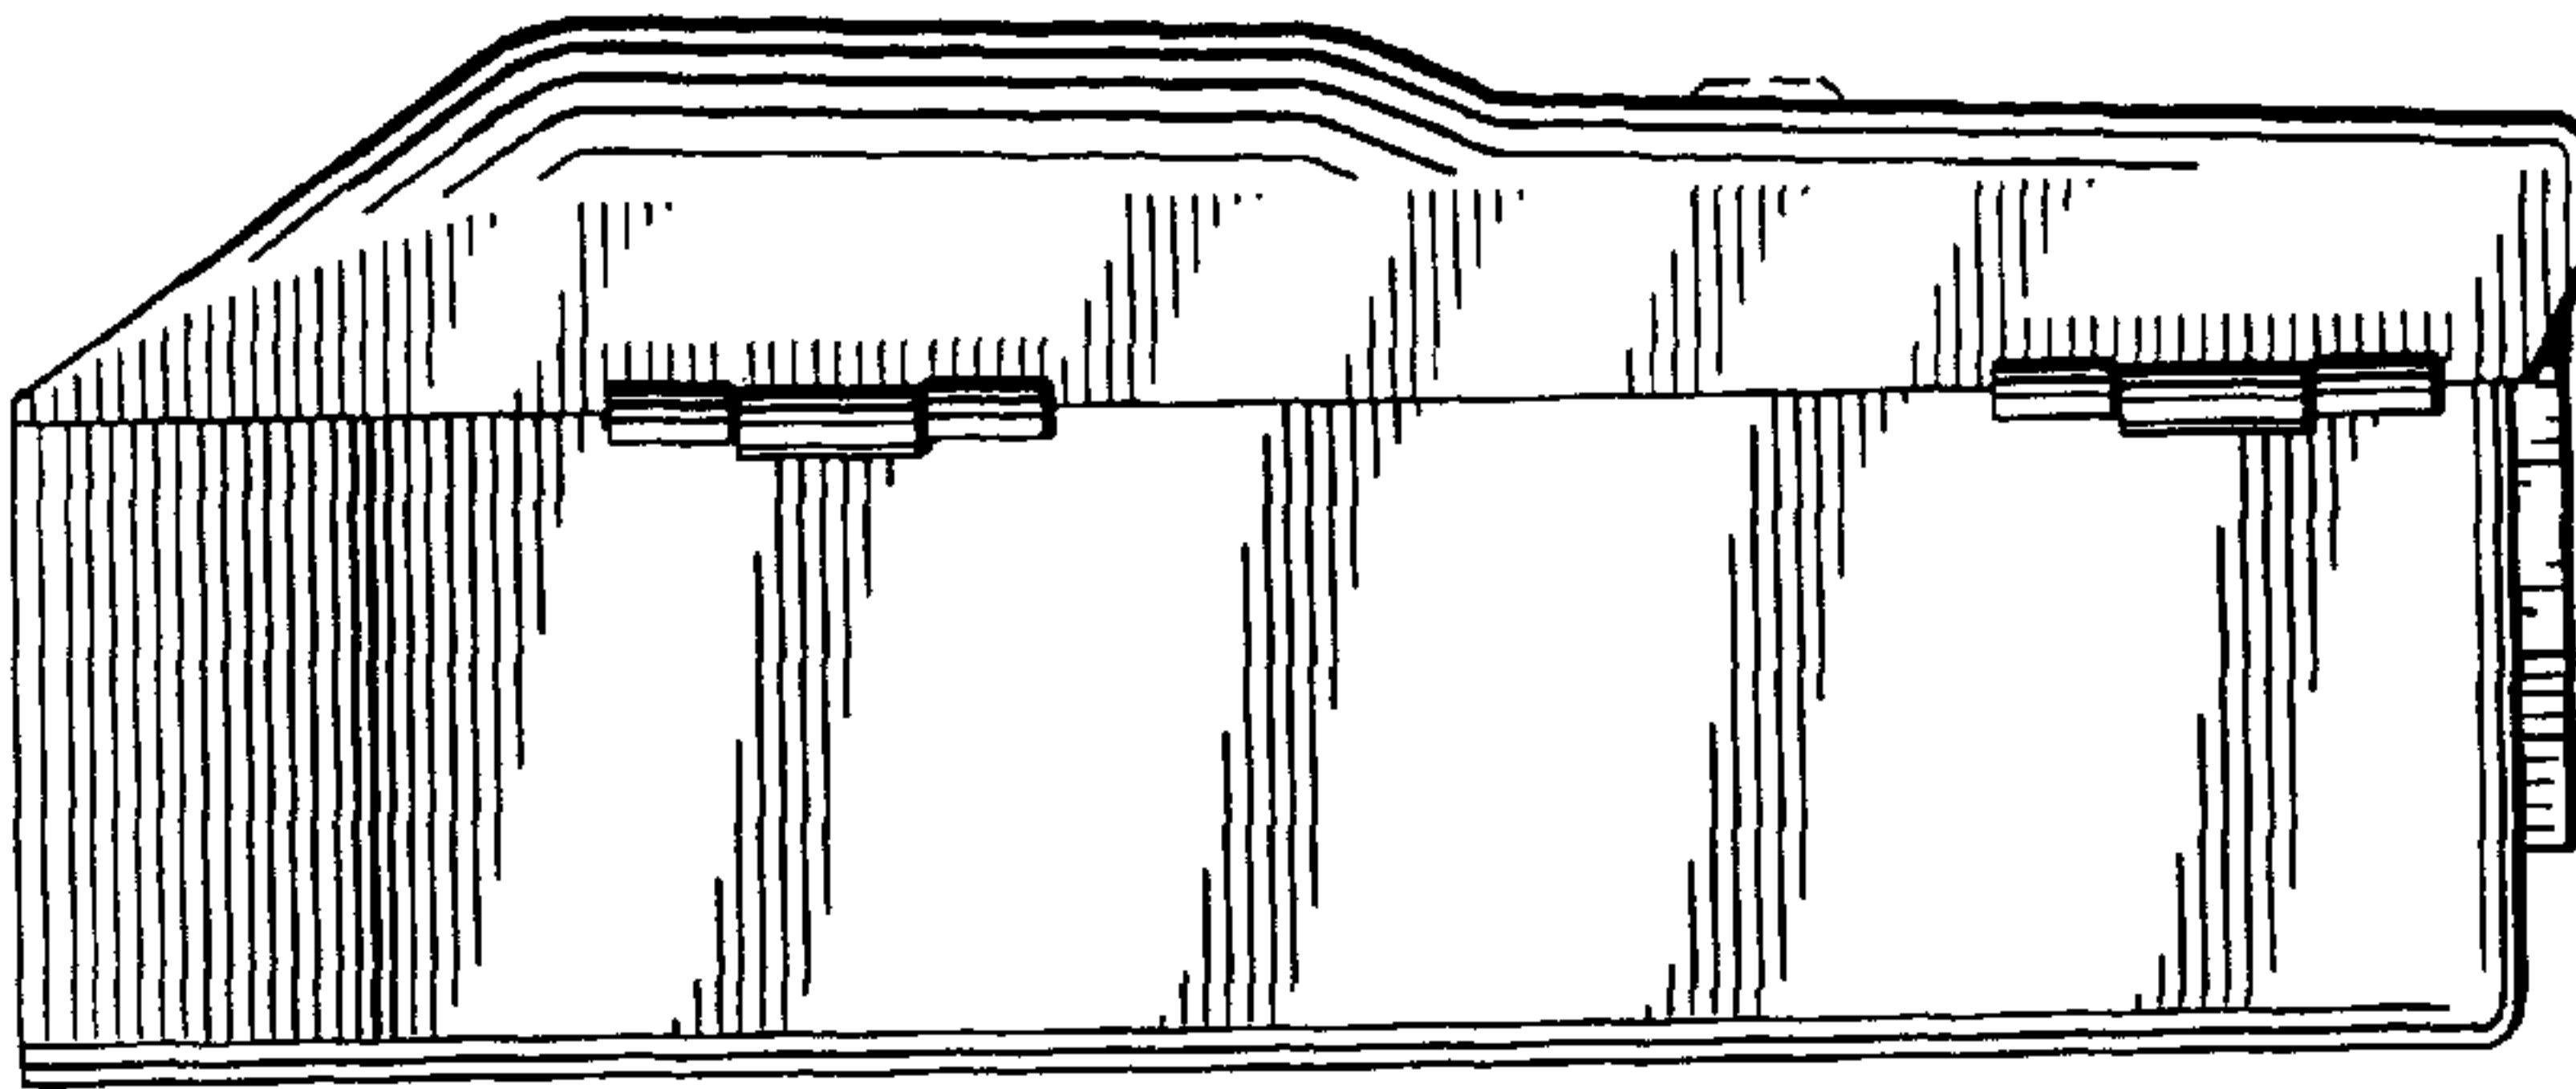


Fig. 4

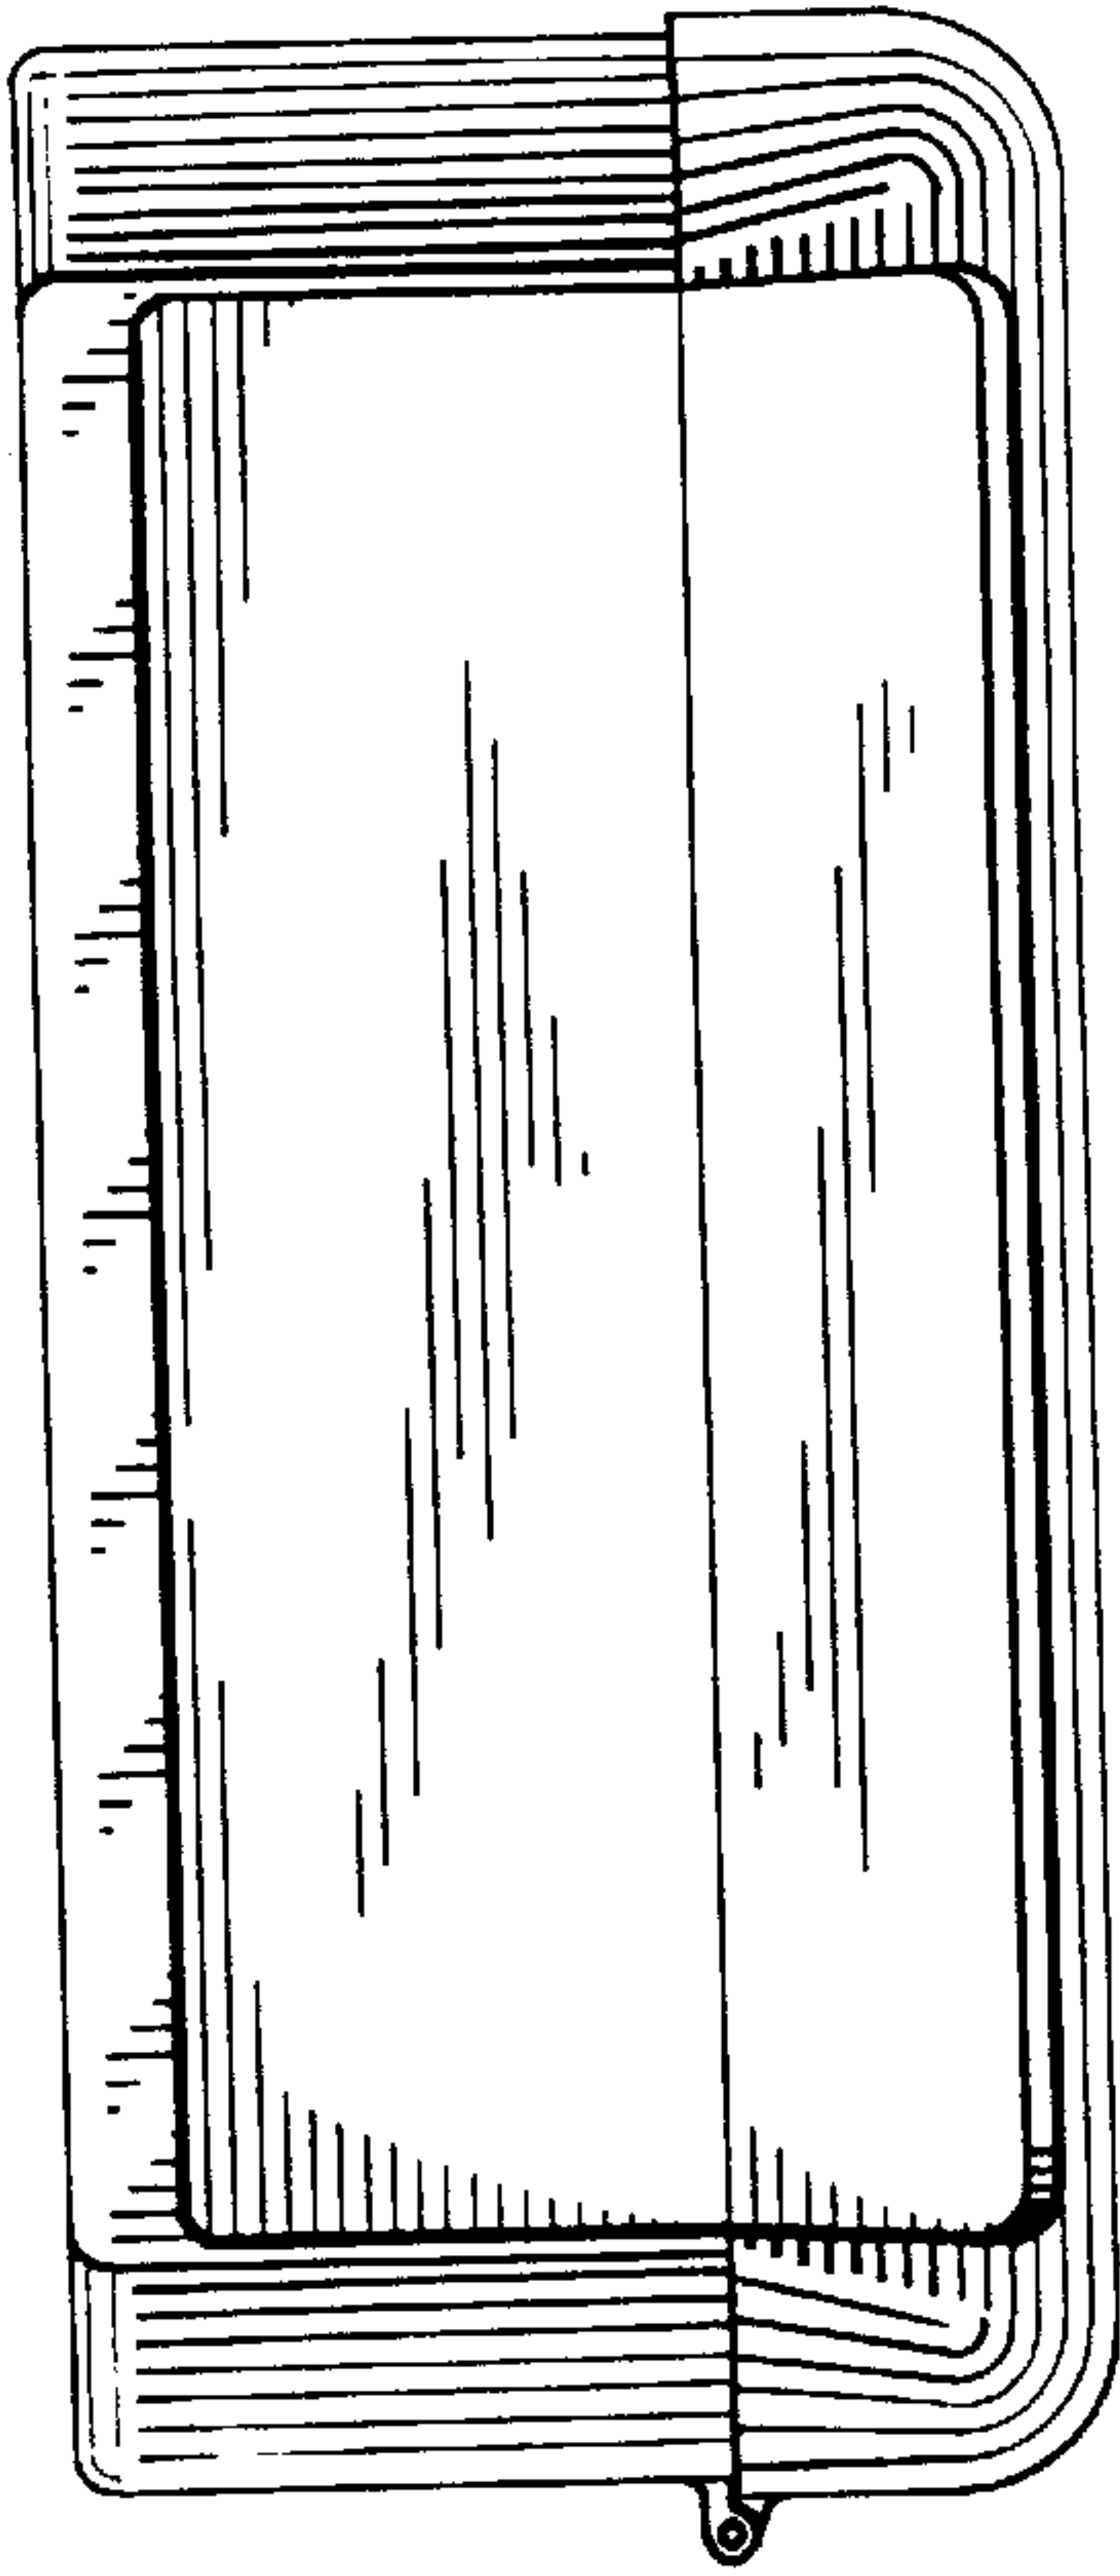


Fig. 7

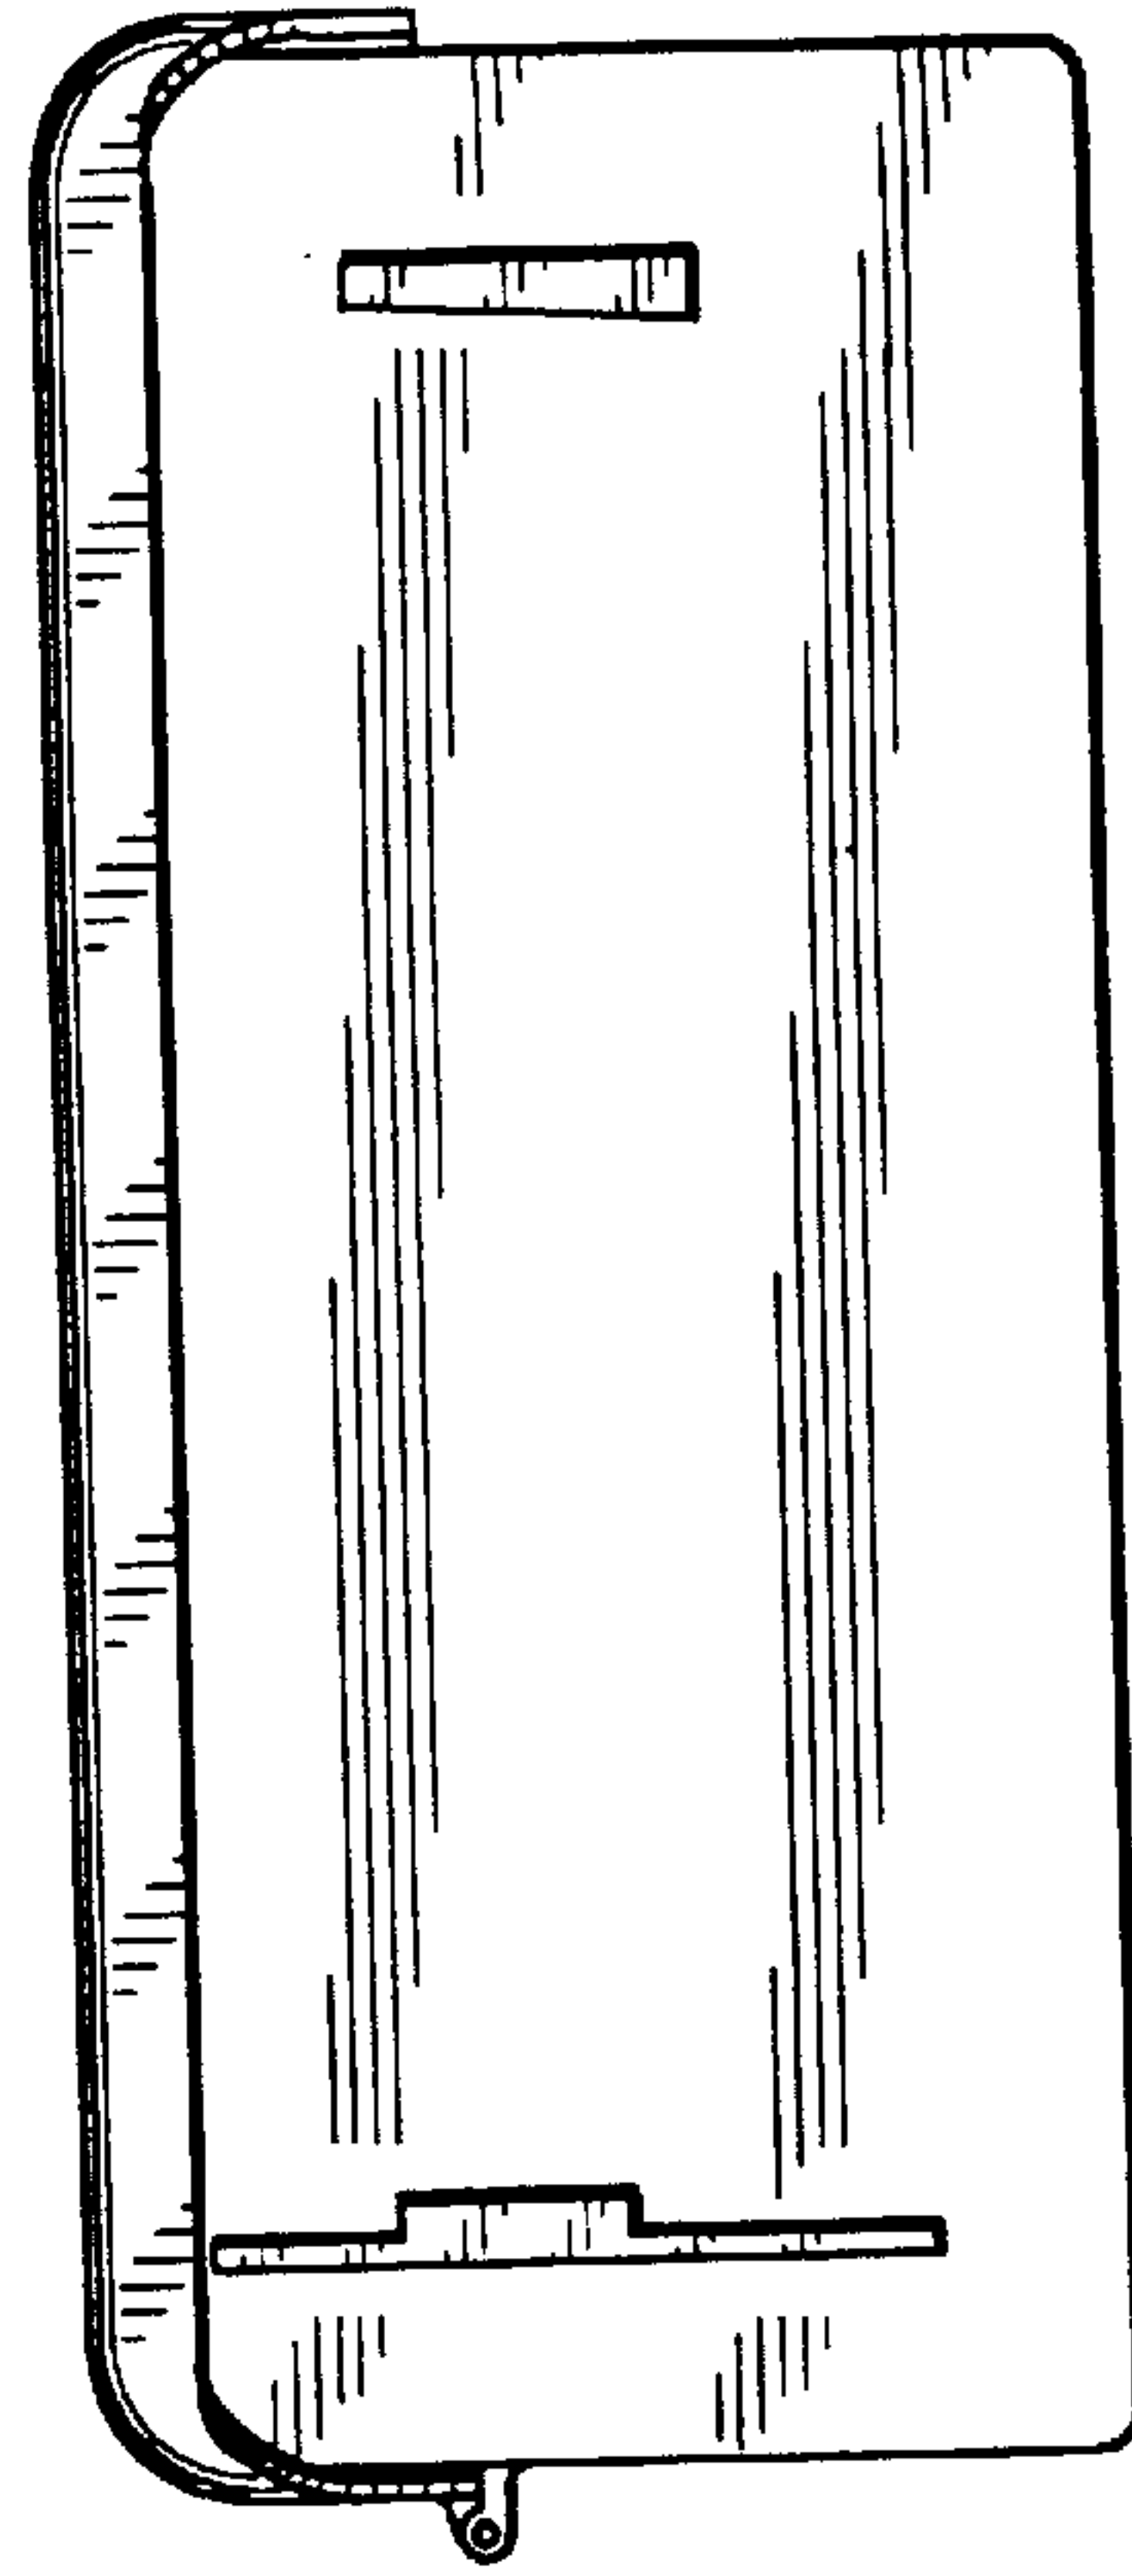


Fig. 8

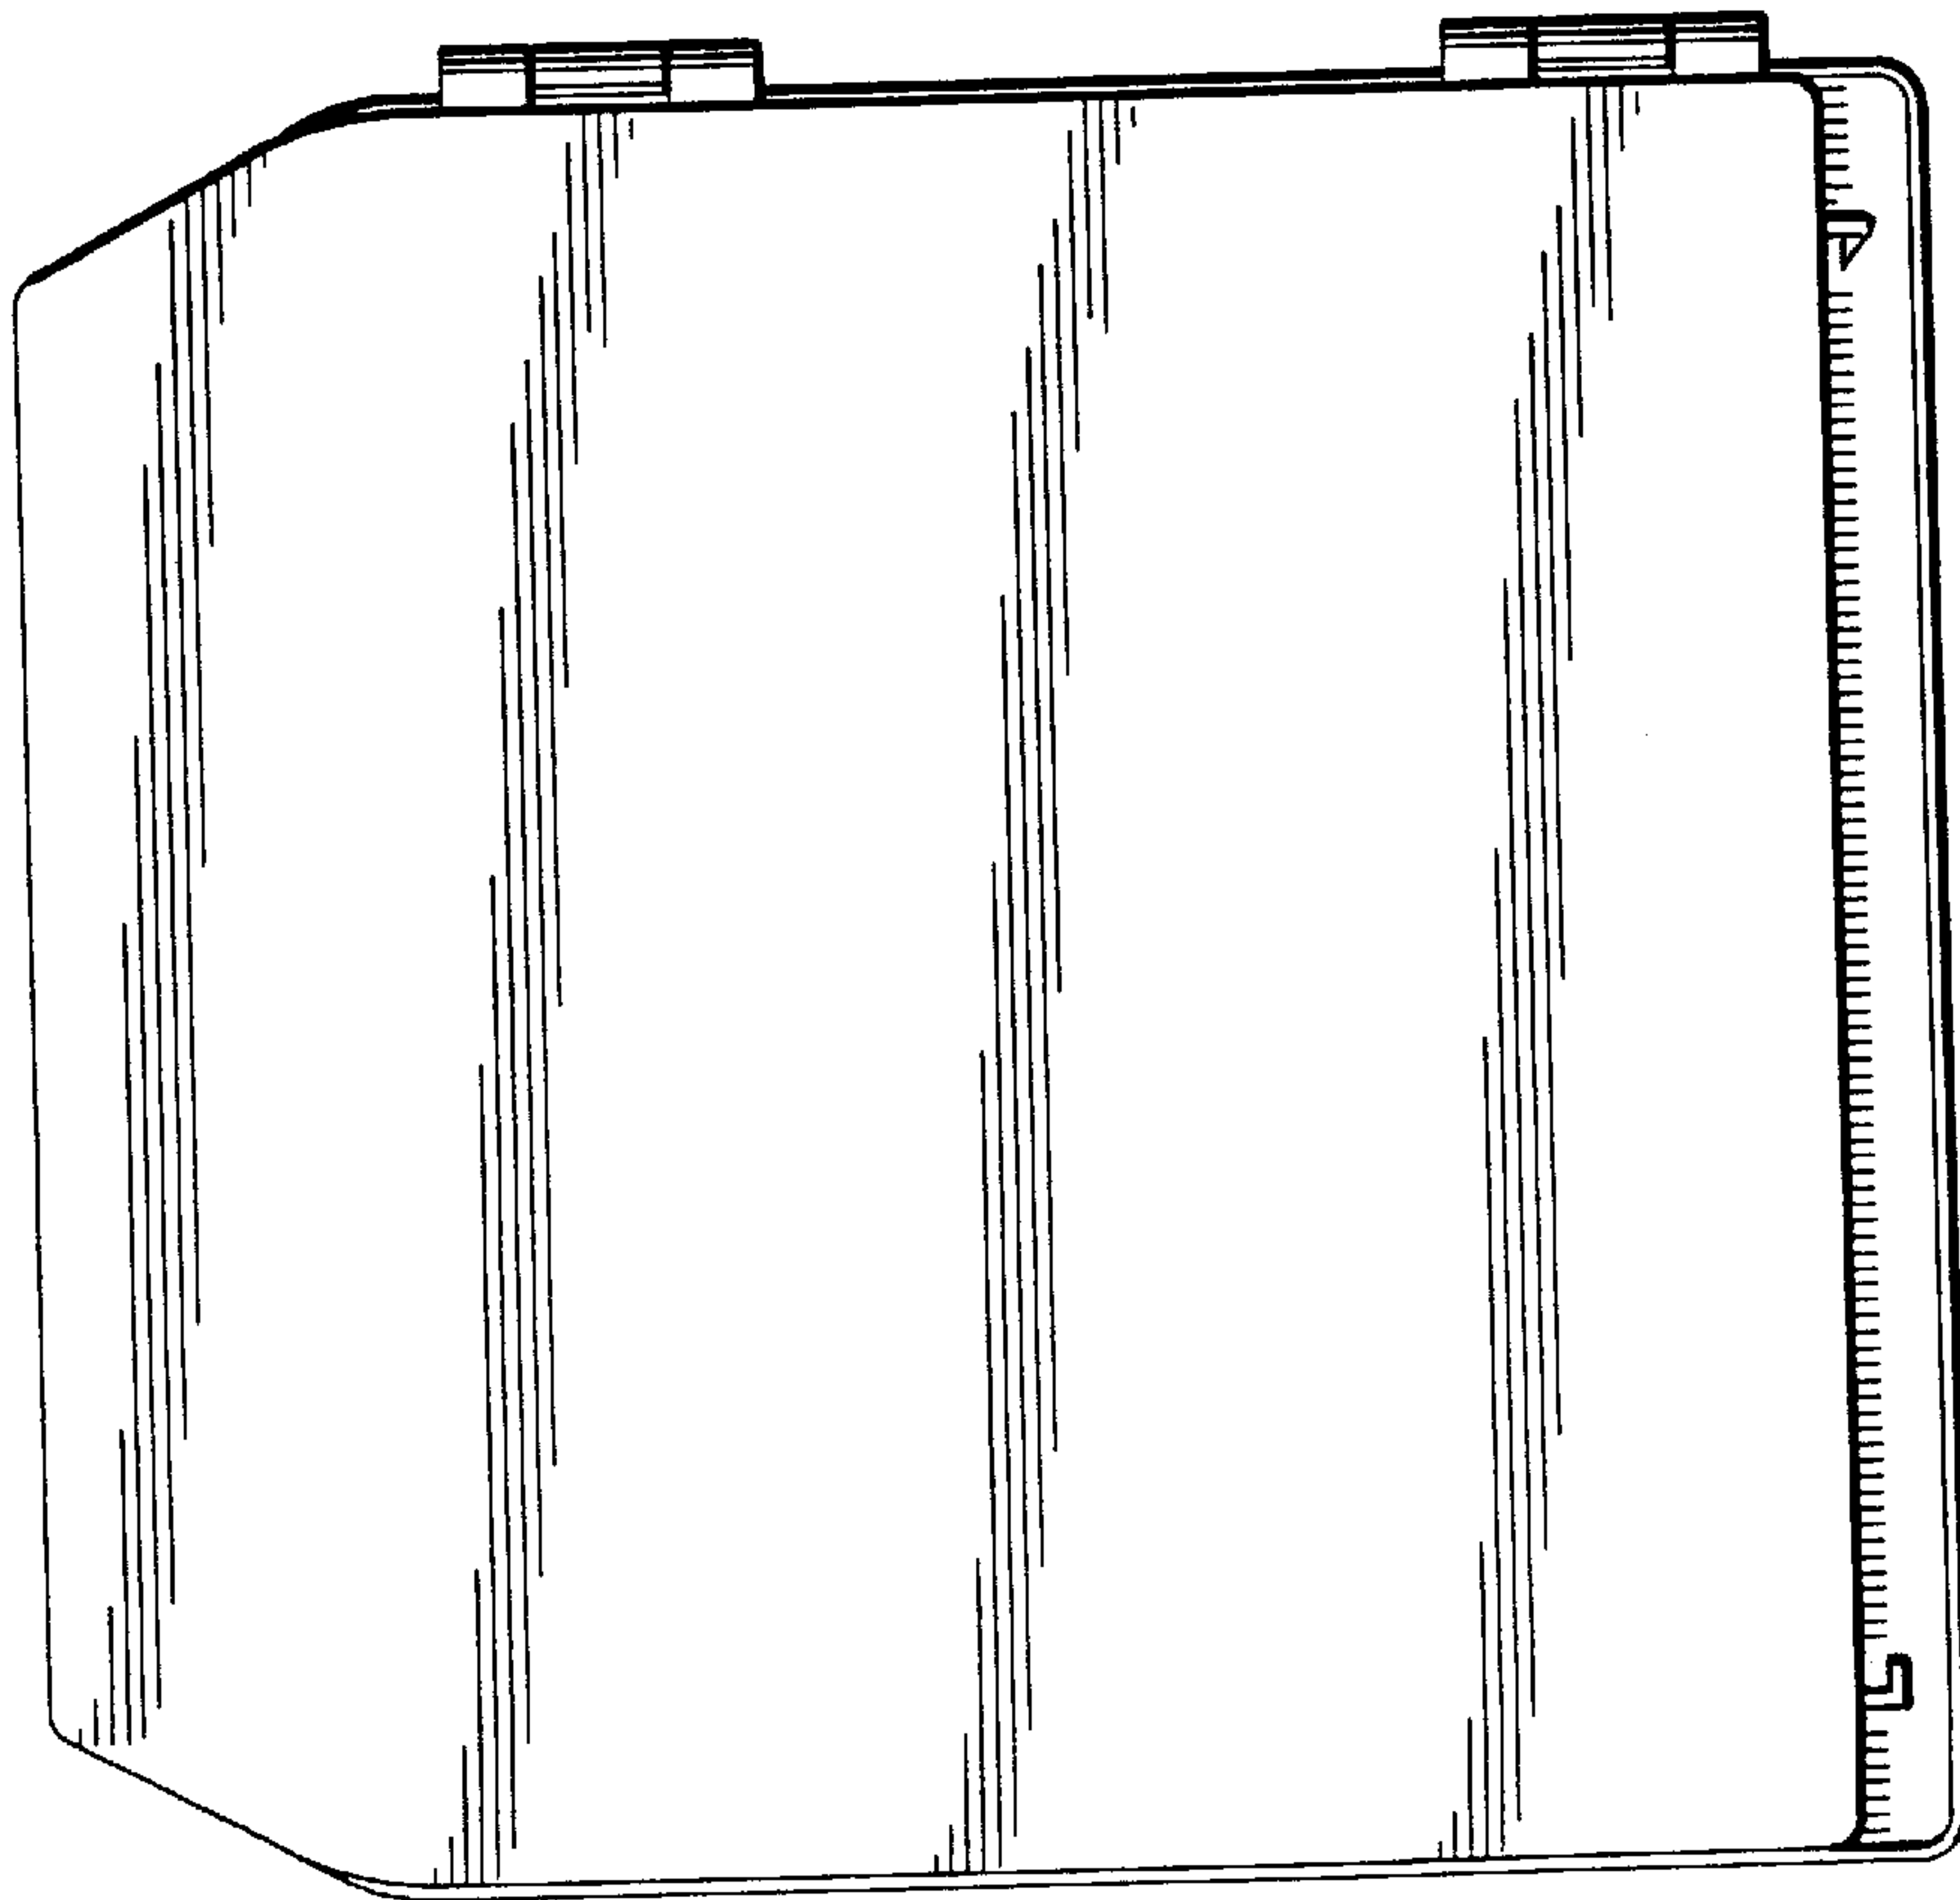


Fig. 5