



US00D413825S

# United States Patent [19]

Storsved

[11] Patent Number: **Des. 413,825**

[45] Date of Patent: **\*\* Sep. 14, 1999**

[54] **RESPIRATORY AIR FLOW MEASURING DEVICE**

[75] Inventor: **Mark S. Storsved**, Menomonee Falls, Wis.

[73] Assignee: **CardioPulmonary Technologies, Inc.**, Pewaukee, Wis.

[\*\*] Term: **14 Years**

[21] Appl. No.: **29/093,533**

[22] Filed: **Sep. 14, 1998**

[51] **LOC (6) Cl.** ..... **10-04**

[52] **U.S. Cl.** ..... **D10/96; D24/129**

[58] **Field of Search** ..... **D10/96; D24/129; 73/861.52, 861.53, 861.65, 207; 600/532; 128/716, 205.53, 725**

[56] **References Cited**

**U.S. PATENT DOCUMENTS**

D. 342,135	12/1993	Goldberger et al. ....	D24/129
D. 348,616	7/1994	Apigian et al. ....	D10/96
4,083,245	4/1978	Osborn .....	73/207
4,852,583	8/1989	Walker .....	128/716
4,989,456	2/1991	Stupecky .....	73/863.53
4,993,269	2/1991	Guillaume et al. ....	73/861.53
5,033,312	7/1991	Stupecky .....	73/861.53
5,038,621	8/1991	Stupecky .....	73/861.53
5,067,492	11/1991	Yelderman et al. ....	128/719
5,088,332	2/1992	Meriläinen et al. ....	73/861.65
5,197,895	3/1993	Stupecky .....	439/194
5,213,109	5/1993	Susi .....	128/719

5,287,851	2/1994	Beran et al. ....	128/204.23
5,357,972	10/1994	Norlien .....	128/725
5,379,650	1/1995	Kofoed et al. ....	73/861.52
5,443,075	8/1995	Holscher .....	128/725
5,565,630	10/1996	Shene .....	73/861.53 X
5,598,839	2/1997	Niles et al. ....	128/205.23
5,620,004	4/1997	Johansen .....	128/716

**OTHER PUBLICATIONS**

U.S. application No. 09/172,486, Storsved, filed Oct. 14, 1998.

*Primary Examiner*—Antoine Duval Davis  
*Attorney, Agent, or Firm*—Nilles & Nilles, S.C.

[57] **CLAIM**

The ornamental design for a respiratory air flow measuring device, as shown and described.

**DESCRIPTION**

FIG. 1 is a top view of a respiratory air flow measuring device showing my new design.

FIG. 2 is a front view of the respiratory air flow measuring device of my new design, said front showing the internal geometry of the device.


FIG. 3 is a side view of the respiratory air flow measuring device.

FIG. 4 is a rear view of the respiratory air flow measuring device.

FIG. 5 is a bottom view (opposite FIG. 1) of the respiratory air flow measuring device; and,

FIG. 6 is a side view (opposite FIG. 3) of the respiratory air flow measuring device.

**1 Claim, 1 Drawing Sheet**

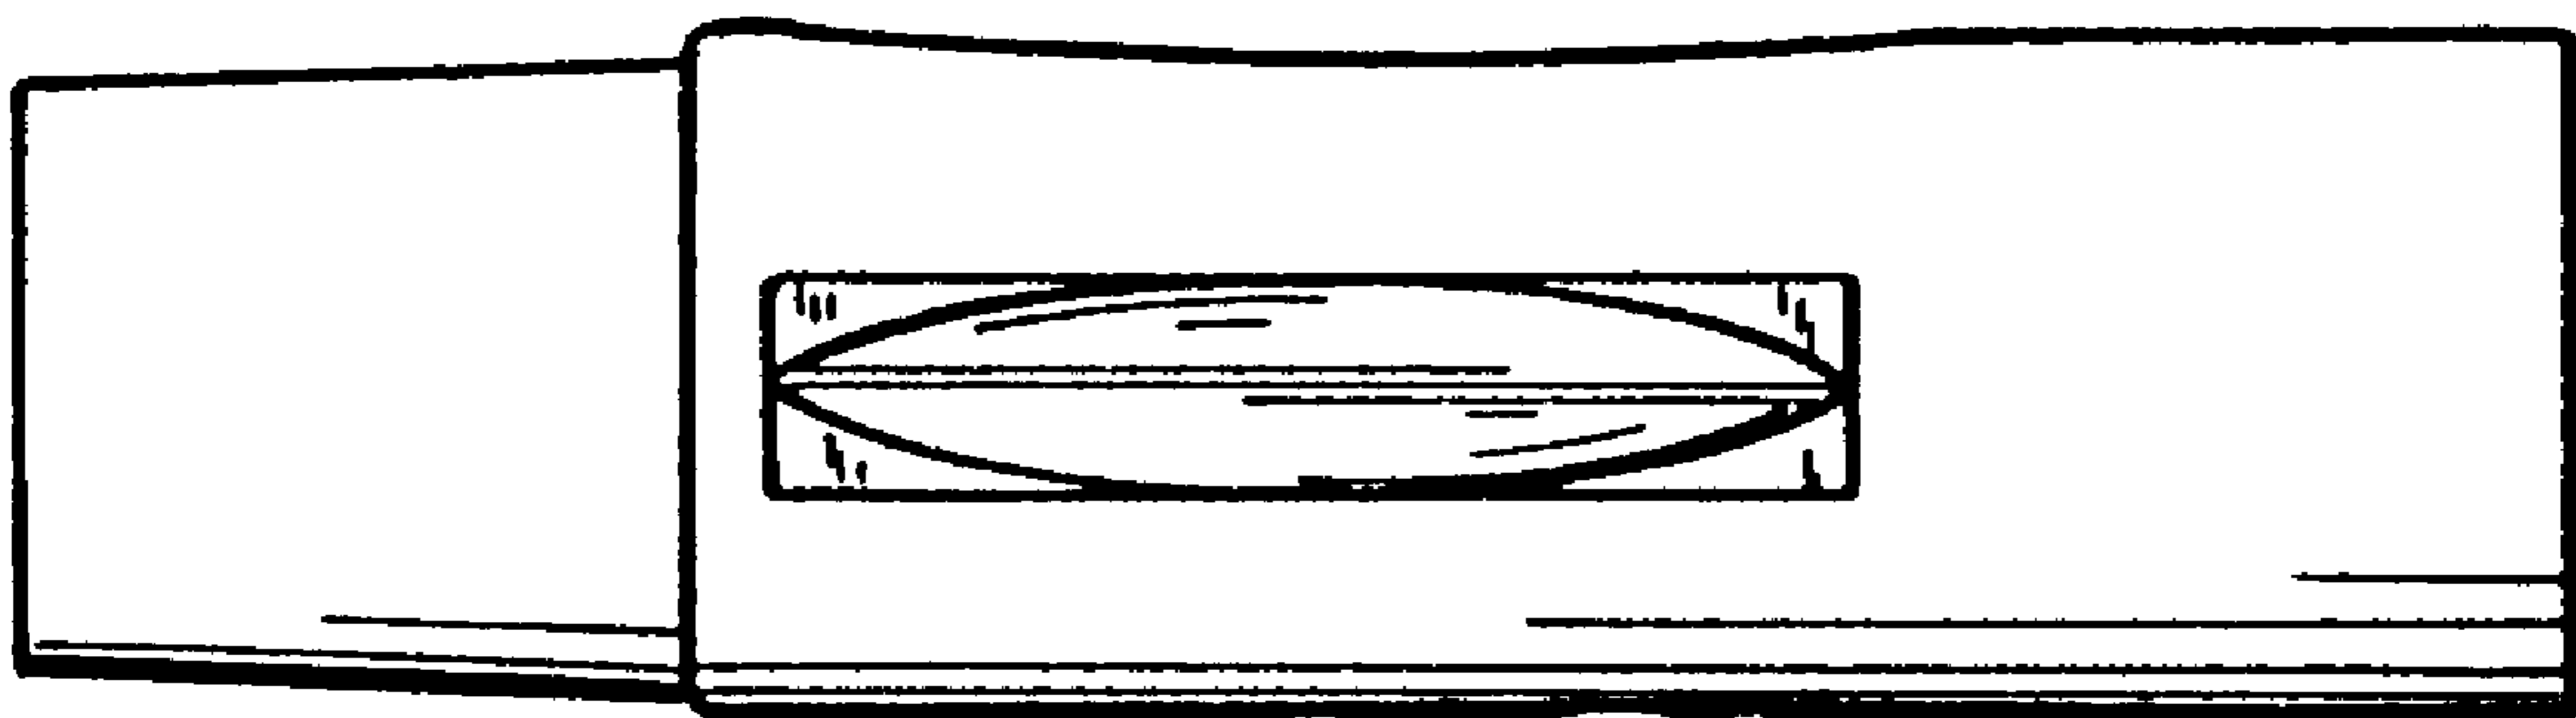

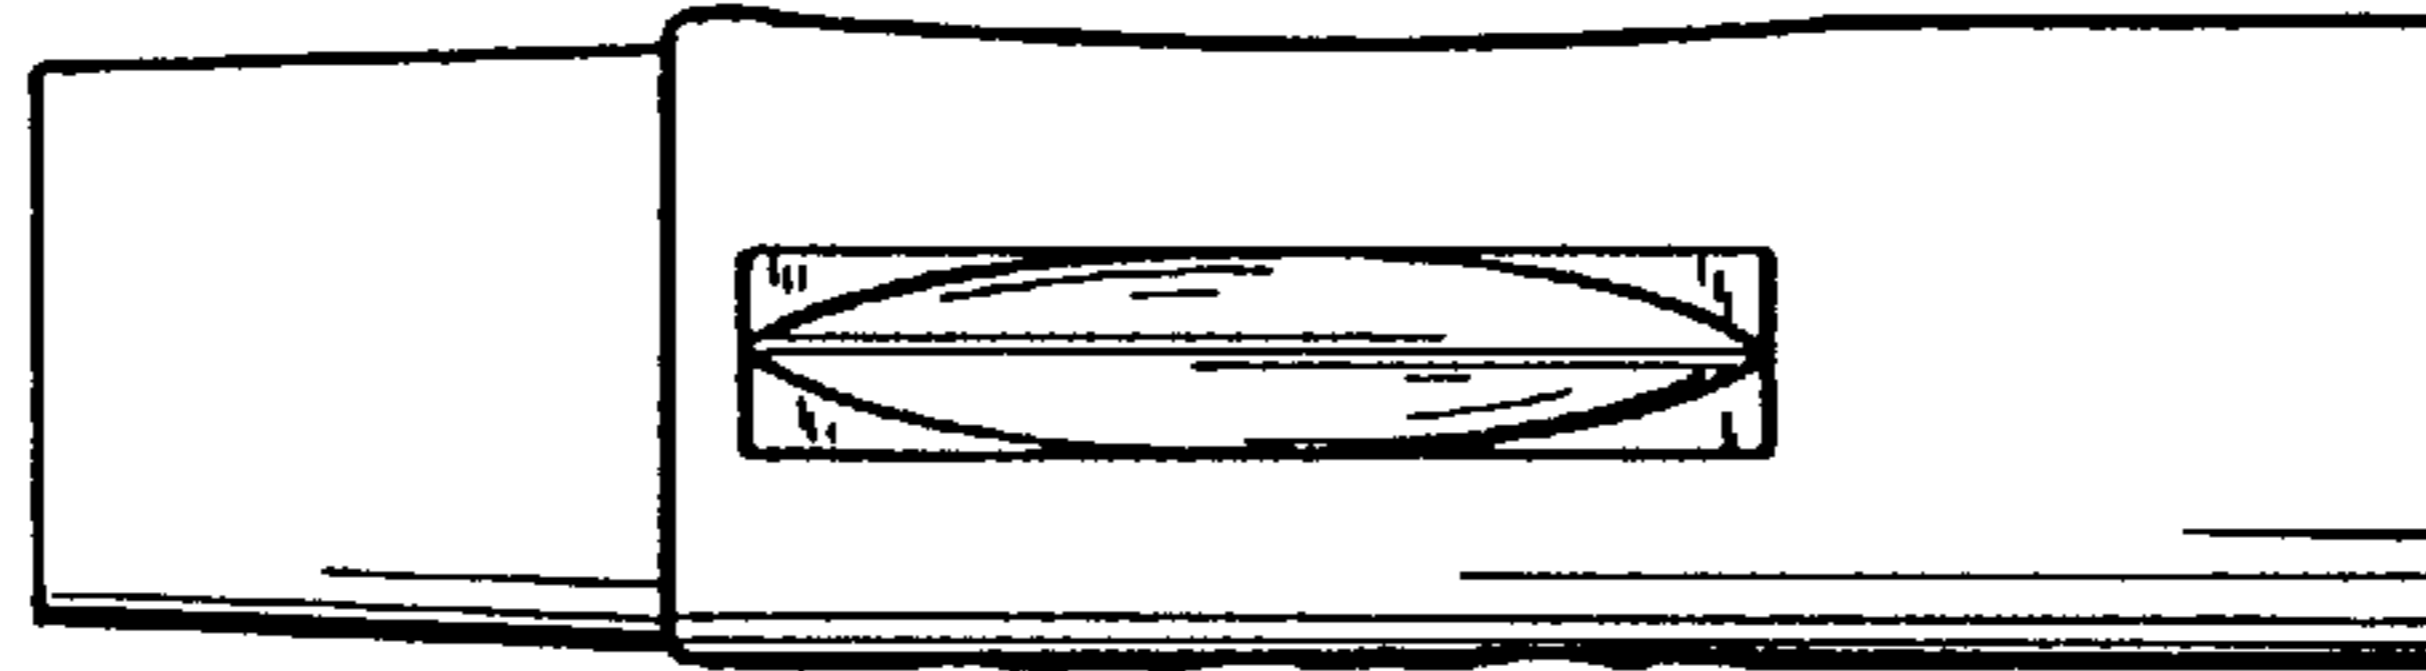


FIG. 1

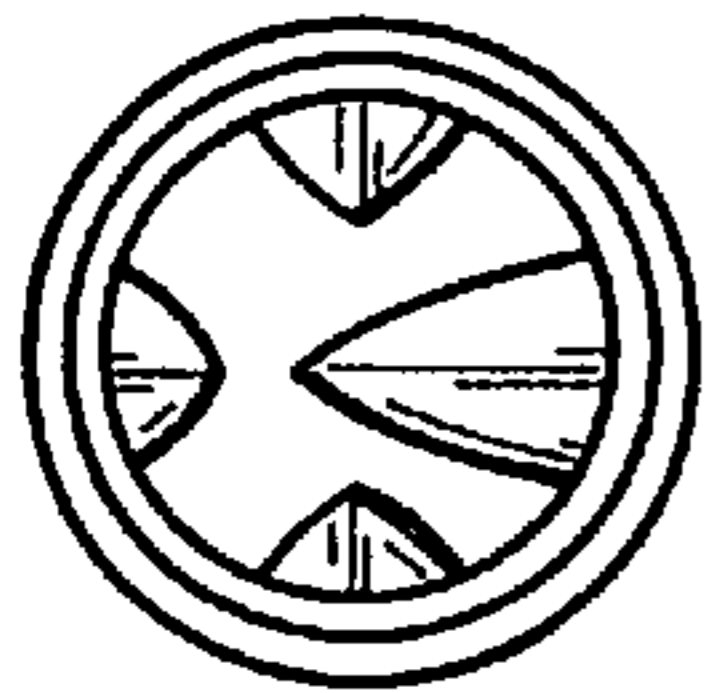


FIG. 2

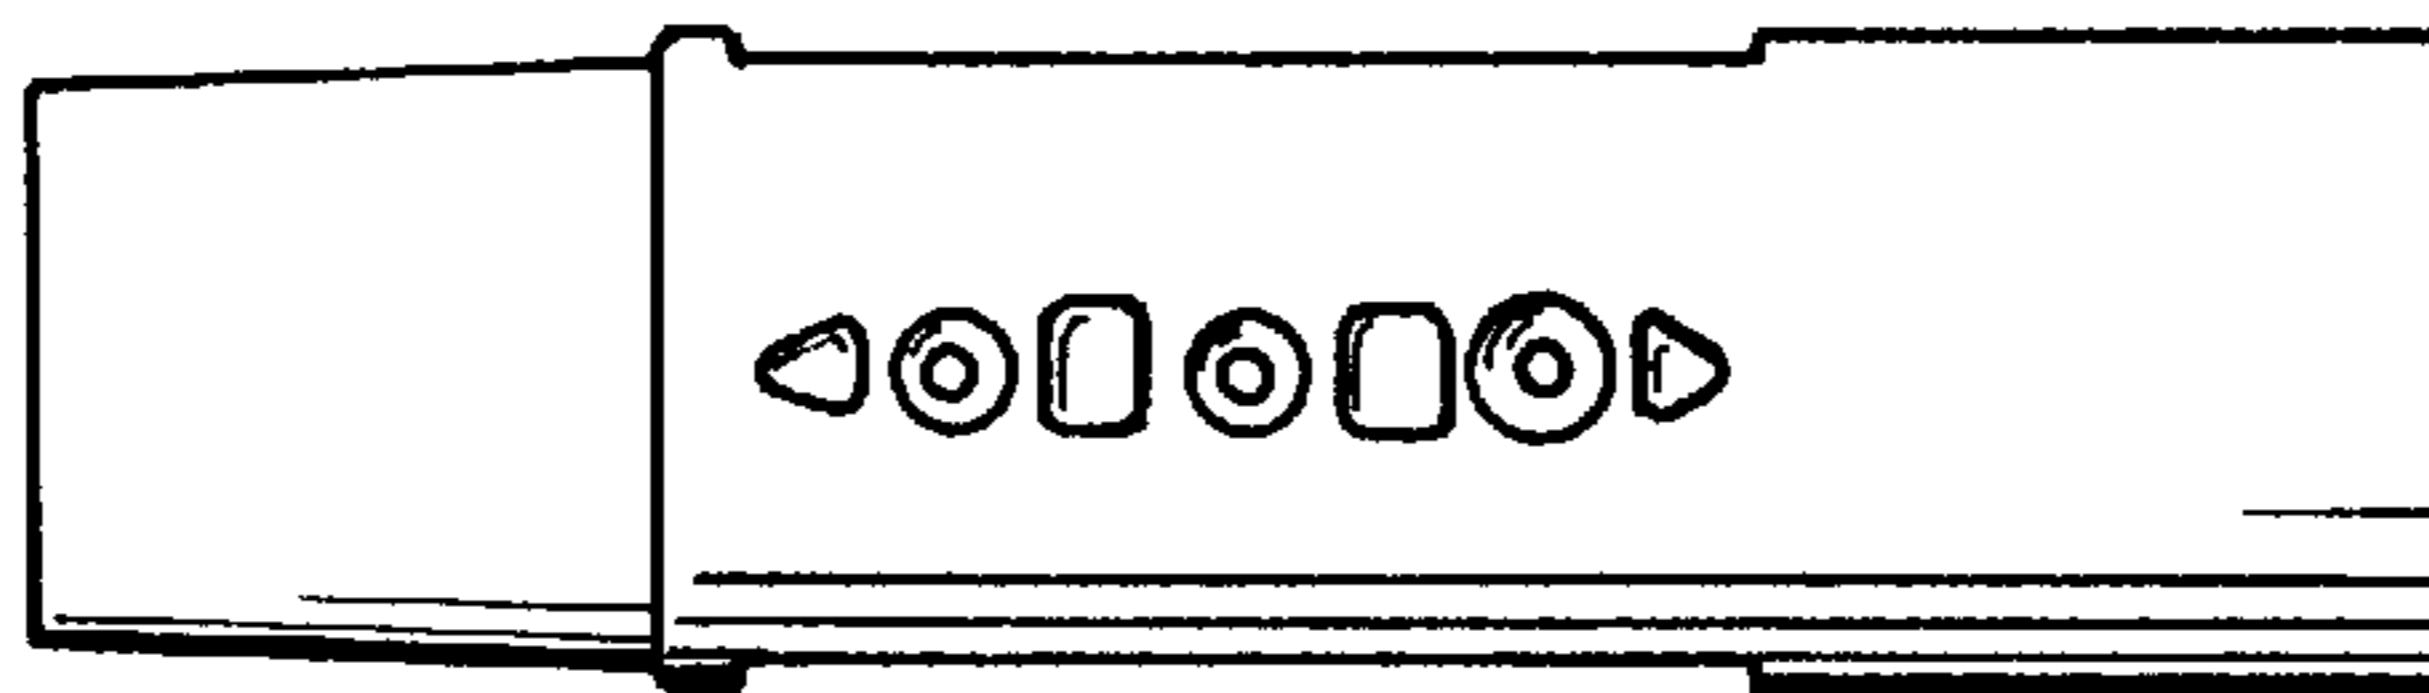


FIG. 3

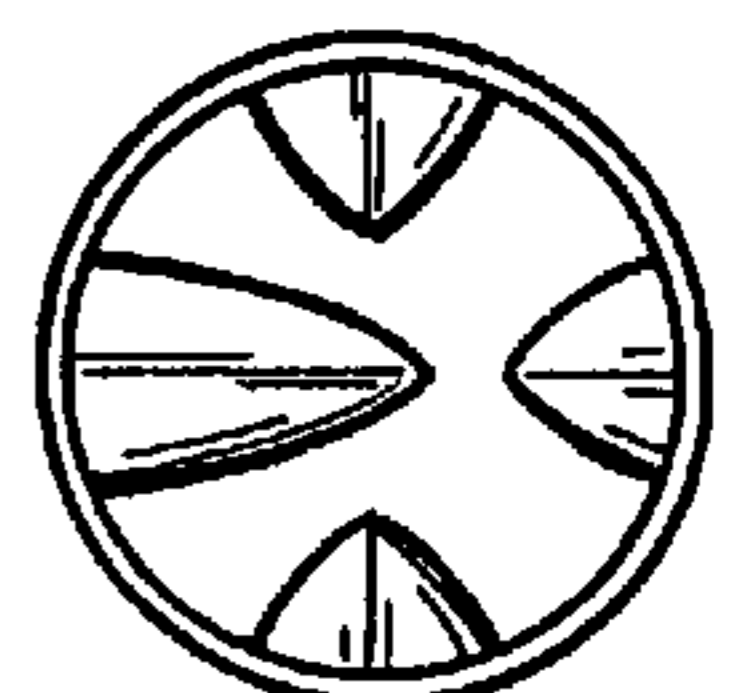


FIG. 4

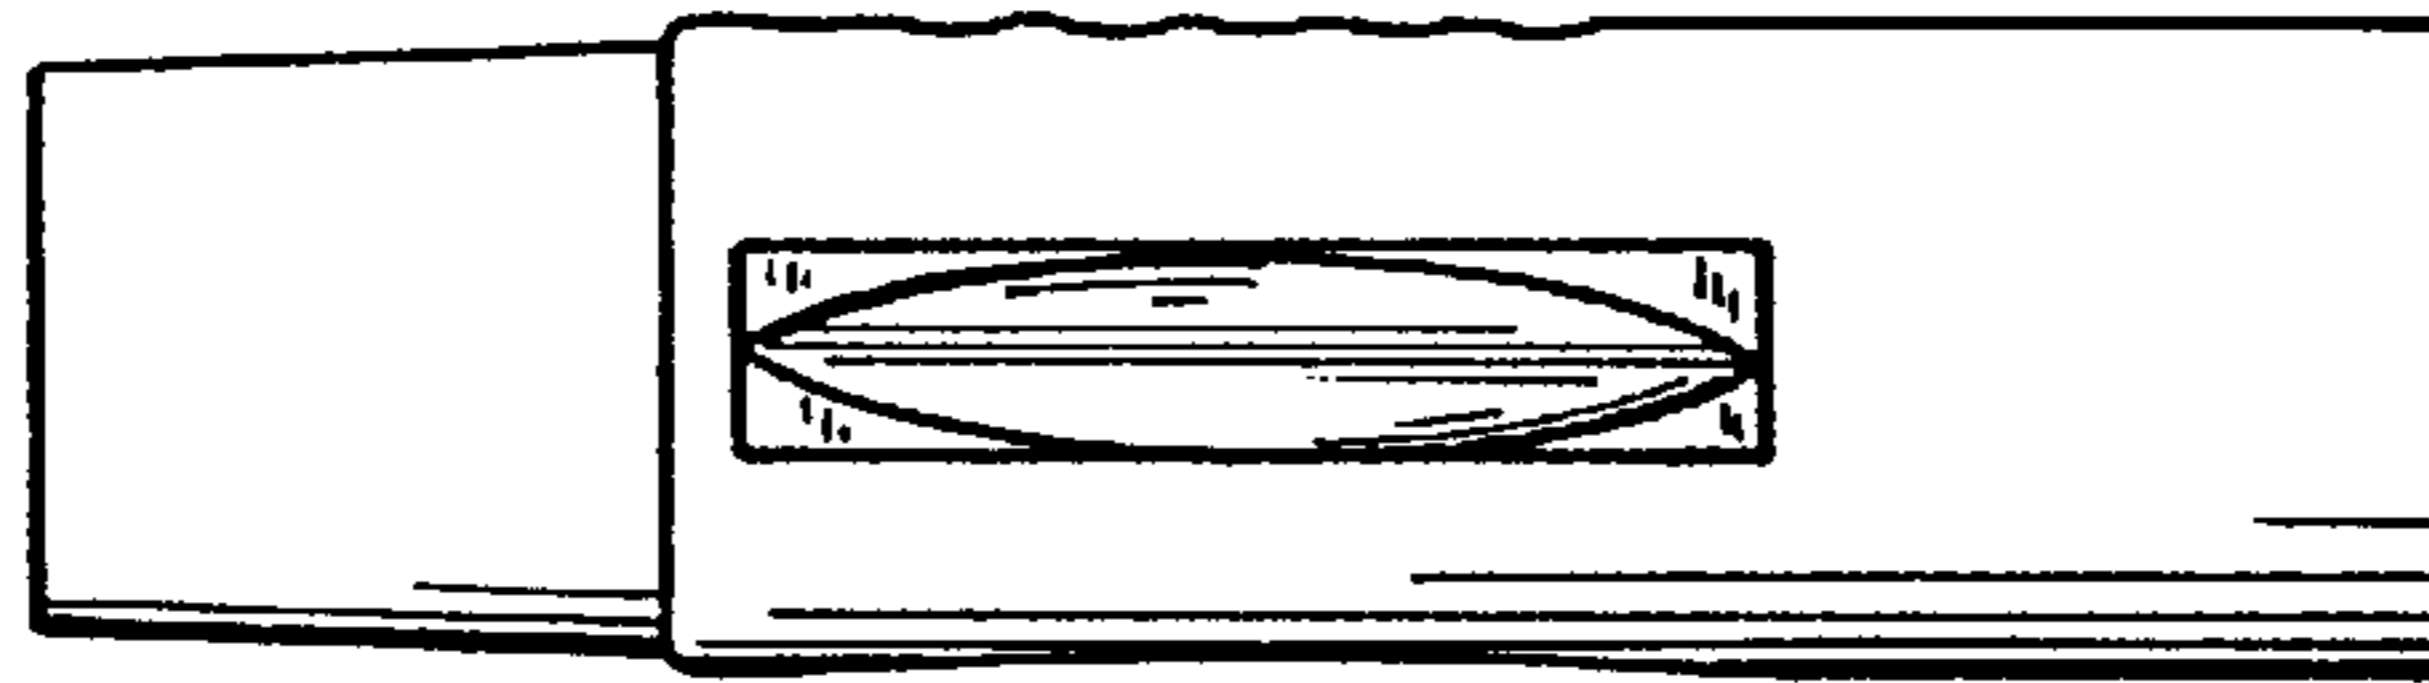


FIG. 5

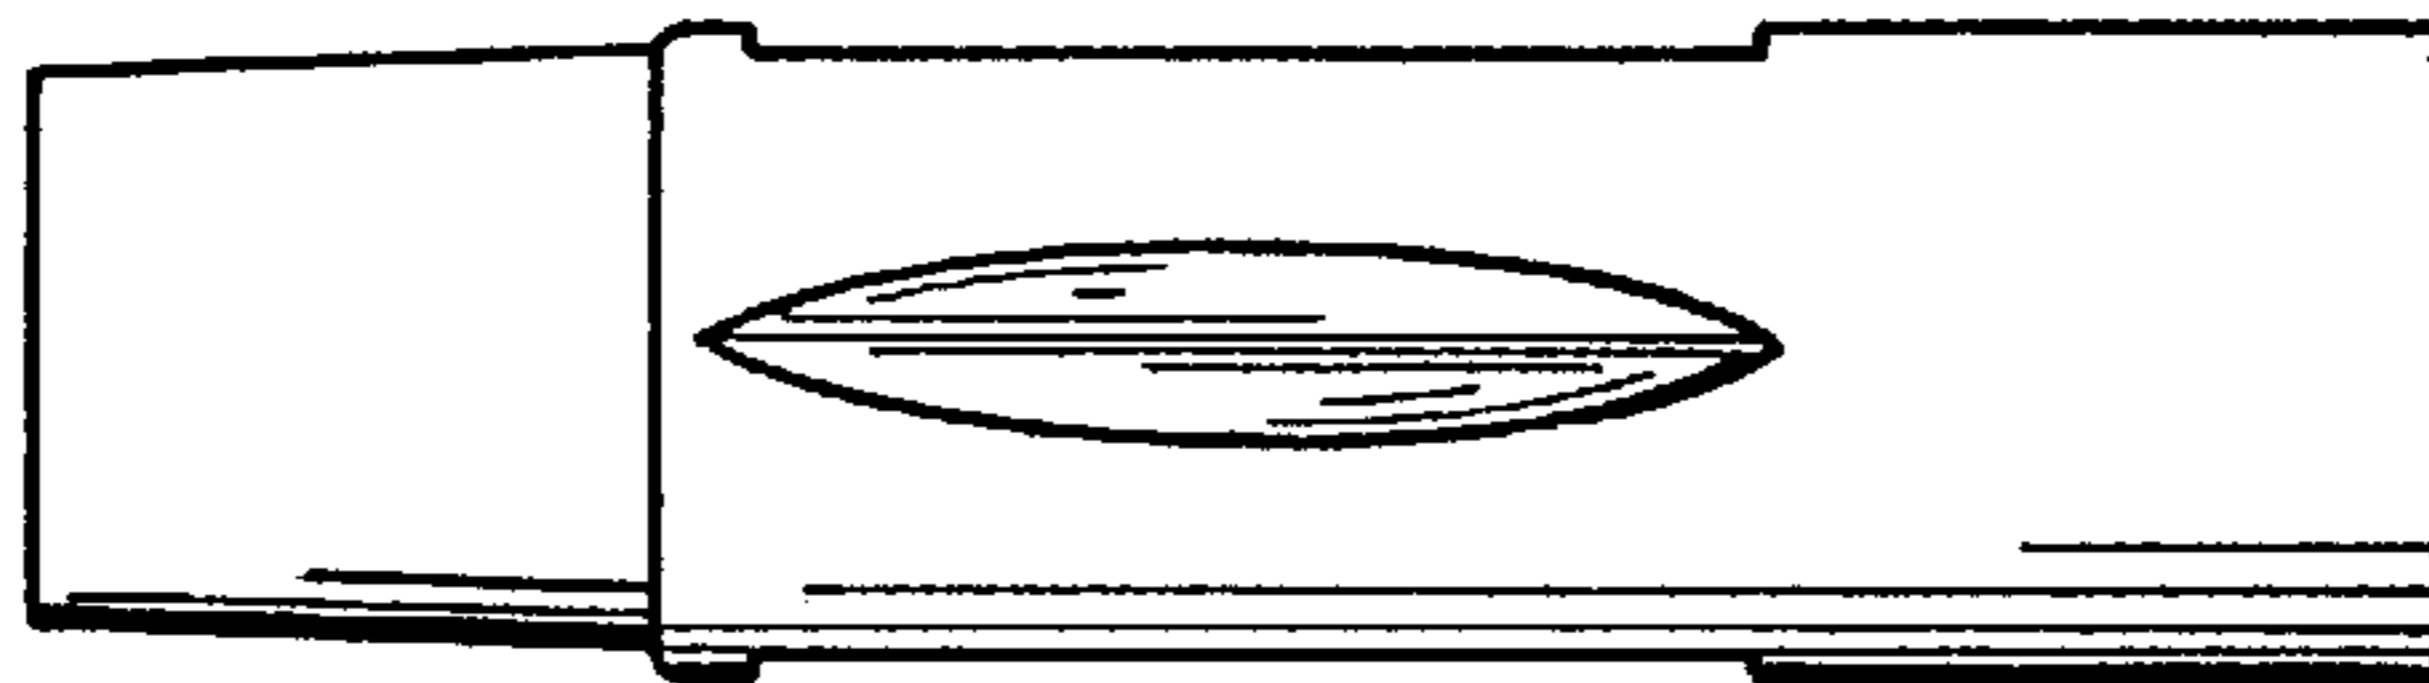


FIG. 6