



US00D418220S

United States Patent [19]
Picha et al.

[11] Patent Number: Des. 418,220
[45] Date of Patent: ** Dec. 28, 1999

[54] **LOW PROFILE BALLOON FEEDING
DEVICE**
[75] Inventors: **George J. Picha**, Independence;
Anthony J. Szpak, Parma, both of
Ohio
[73] Assignee: **Applied Medical Technology, Inc.**,
Cleveland, Ohio
[**] Term: **14 Years**
[21] Appl. No.: **29/085,585**
[22] Filed: **Mar. 26, 1998**
[51] **LOC (6) Cl.** **24-02**
[52] **U.S. Cl.** **D24/112; D24/129**
[58] **Field of Search** D24/112, 129;
604/247, 246, 96, 174, 250, 175

[56] **References Cited**

U.S. PATENT DOCUMENTS			
D. 350,343	9/1994	Potter	D24/110
D. 360,030	7/1995	Michels et al.	D24/112
3,831,629	8/1974	Mackal et al.	137/525
4,344,434	8/1982	Robertson	128/283
4,381,765	5/1983	Burton	128/1 R
4,393,873	7/1983	Nawash et al.	604/151
4,610,663	9/1986	Rosenberg	604/99
4,666,433	5/1987	Parks	604/178
4,685,901	8/1987	Parks	604/96
4,701,163	10/1987	Parks	604/178
4,776,347	10/1988	Matthews	128/774
4,776,848	10/1988	Solazzo	604/247
4,798,592	1/1989	Parks	601/49
4,850,953	7/1989	Haber et al.	600/32
4,863,438	9/1989	Gauderer et al.	604/247
4,944,732	7/1990	Russo	604/247
5,064,434	11/1991	Haber	623/11
5,071,405	12/1991	Piontek et al.	604/96
5,073,166	12/1991	Parks et al.	609/93
5,084,014	1/1992	Picha et al.	604/54
5,085,636	2/1992	Burns	604/99
5,100,384	3/1992	McBrien et al.	604/99
5,125,897	6/1992	Quinn et al.	604/99
5,224,933	7/1993	Bromander	604/99
5,234,417	8/1993	Parks et al.	604/283

5,248,302	9/1993	Patrick et al.	604/178
5,250,040	10/1993	Parks et al.	604/283
5,261,896	11/1993	Conway et al.	604/265
5,308,325	5/1994	Quinn et al.	604/96
5,336,203	8/1994	Goldhardt et al.	604/247

(List continued on next page.)


OTHER PUBLICATIONS
Bard Interventional Products Division, “Announcing The Gauderer Genie System”, Brochure @95.
Medical Innovations Corp., A Division of Ballard Medical Products, MIC-KEY Skin Level Gastrostomy Kit.
Medical Innovations Corp., MIC-KEY Skin Level Gastrostomy Feeding Kit @94.
Biosearch Medical Products, Inc., The Medical Innovator Presents: Pee Wee A Low Profile Gastrostomy Feeding Kit.
Bard Interventional Products Division, C.R. Bard, Inc., It’s More Than An Illusion @95.
Easyfit Button, Medicina, Ridgefield House, 14 John Dalton Street, Manchester M2 6JR.

Primary Examiner—Stella Reid
Assistant Examiner—I Simmons
Attorney, Agent, or Firm—Pearne, Gordon, McCoy & Granger LLP

[57] **CLAIM**
The ornamental design for a low profile balloon feeding device, as shown and described.


DESCRIPTION
FIG. 1 is a perspective view of a low profile balloon feeding device, showing our new design.
FIG. 2 is a front elevational view thereof.
FIG. 3 is a right side elevational view thereof.
FIG. 4 is a top plan view thereof.
FIG. 5 is a left side elevational view thereof; and,
FIG. 6 is a bottom plan view thereof.
The broken line showing of a retention balloon in FIGS. 1–6 is for illustrative purposes only and forms no part of the claimed design. The broken line showing of an air control valve in FIGS. 1, 2, 4, and 6 is for illustrative purposes only and forms no part of the claimed design.

1 Claim, 3 Drawing Sheets

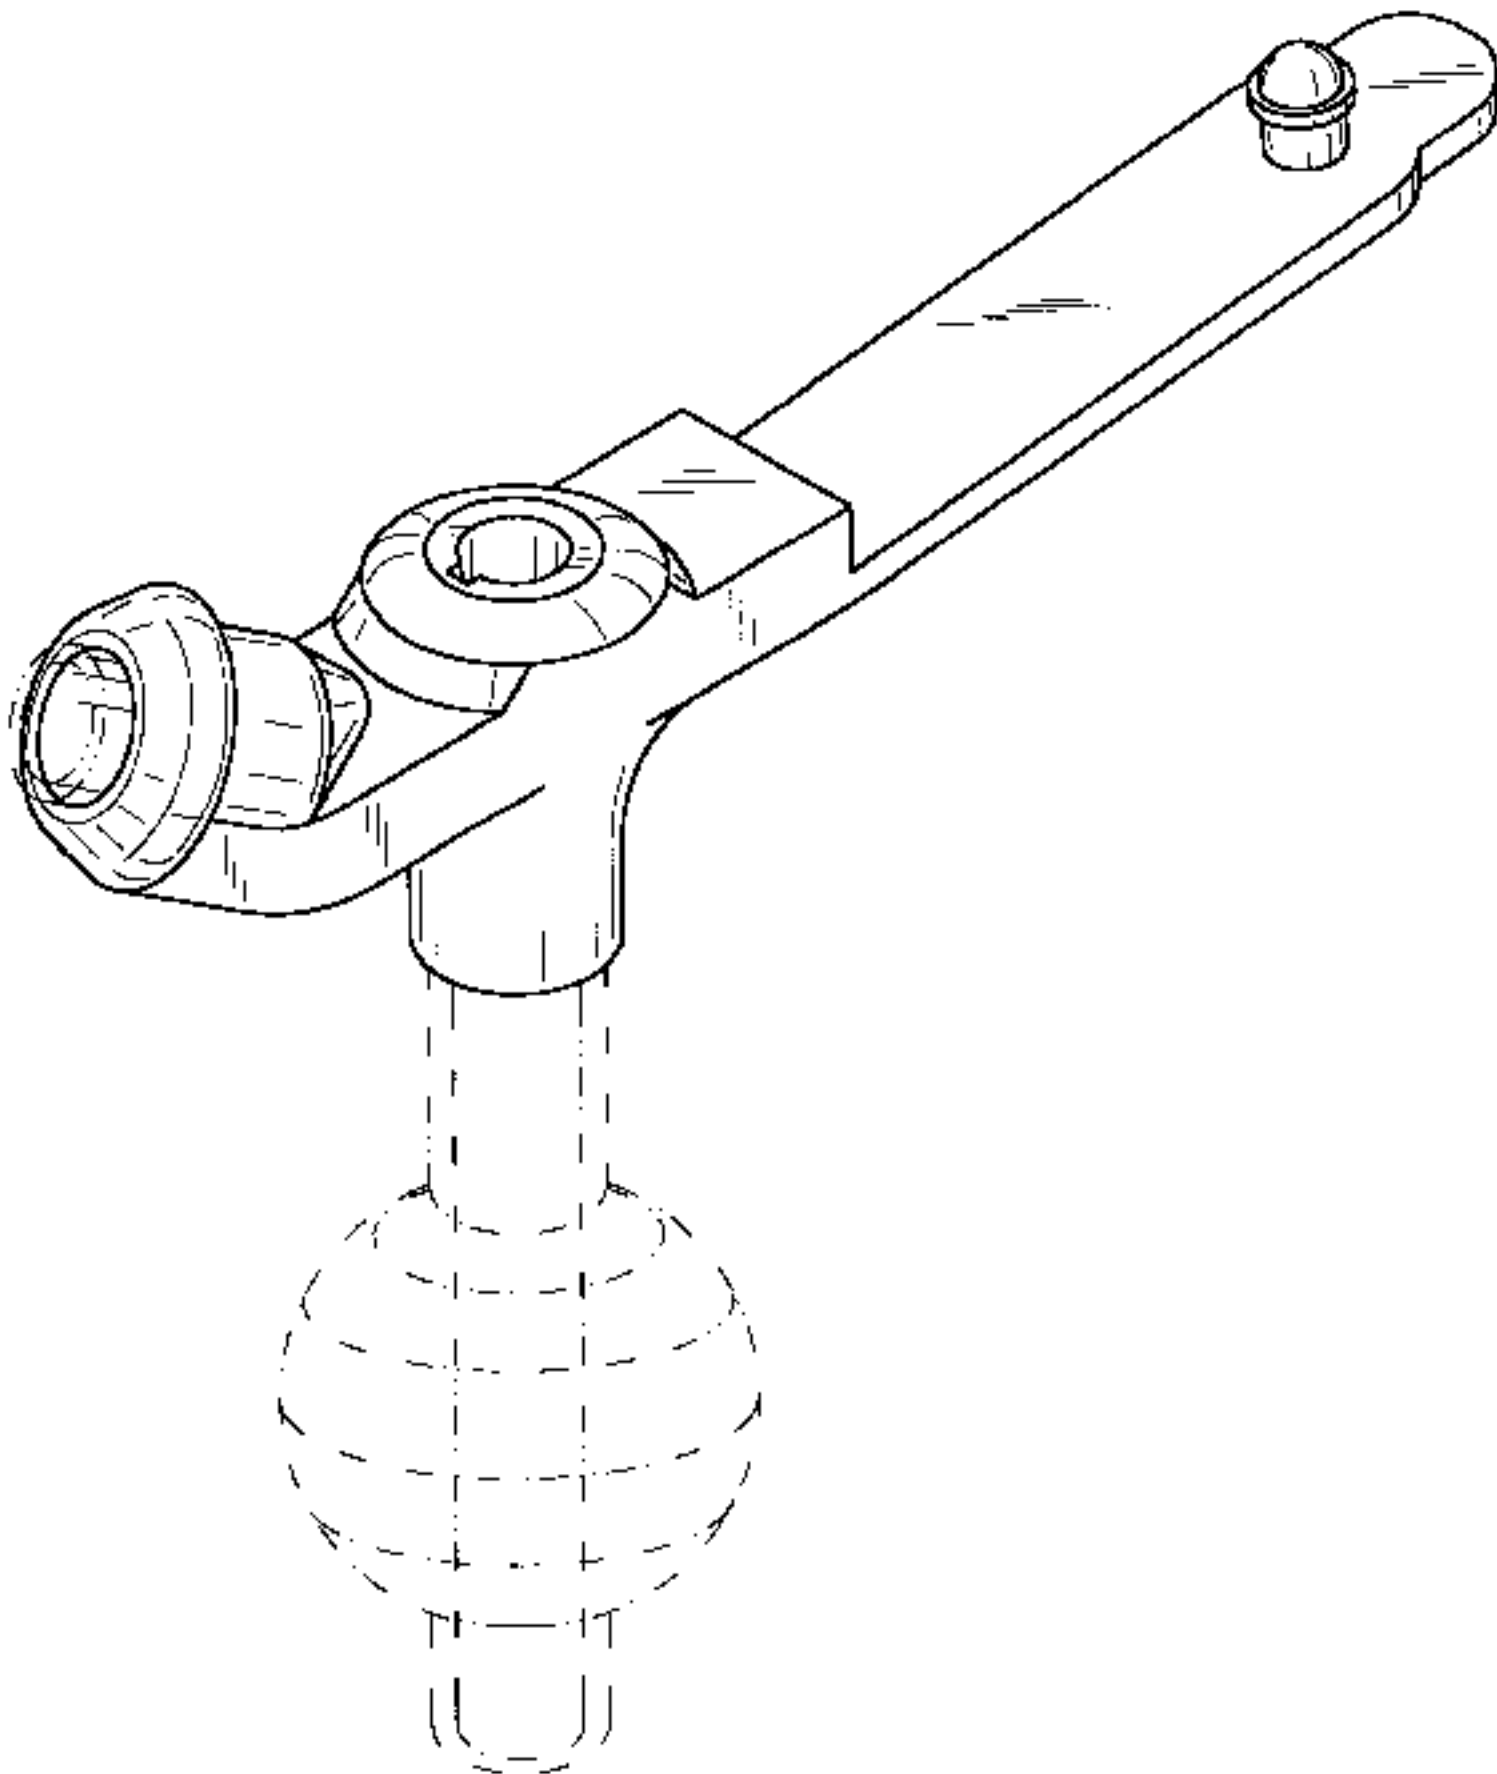

U.S. PATENT DOCUMENTS							
				5,411,491	5/1995	Goldhardt et al.	604/247
				5,413,565	5/1995	Michels et al.	604/247
				5,445,615	8/1995	Yoon	604/96
				5,458,583	10/1995	McNeely et al.	604/96
				5,556,385	9/1996	Anderson	604/174
				5,836,924	11/1998	Kelliher et al.	604/248
5,342,303	8/1994	Ghaerzadeh	604/96				
5,342,321	8/1994	Potter	604/174				
5,356,391	10/1994	Stewart	604/175				
5,358,488	10/1994	Suriyapa	604/96				
5,399,173	3/1995	Parks et al.	604/282				

Fig.1

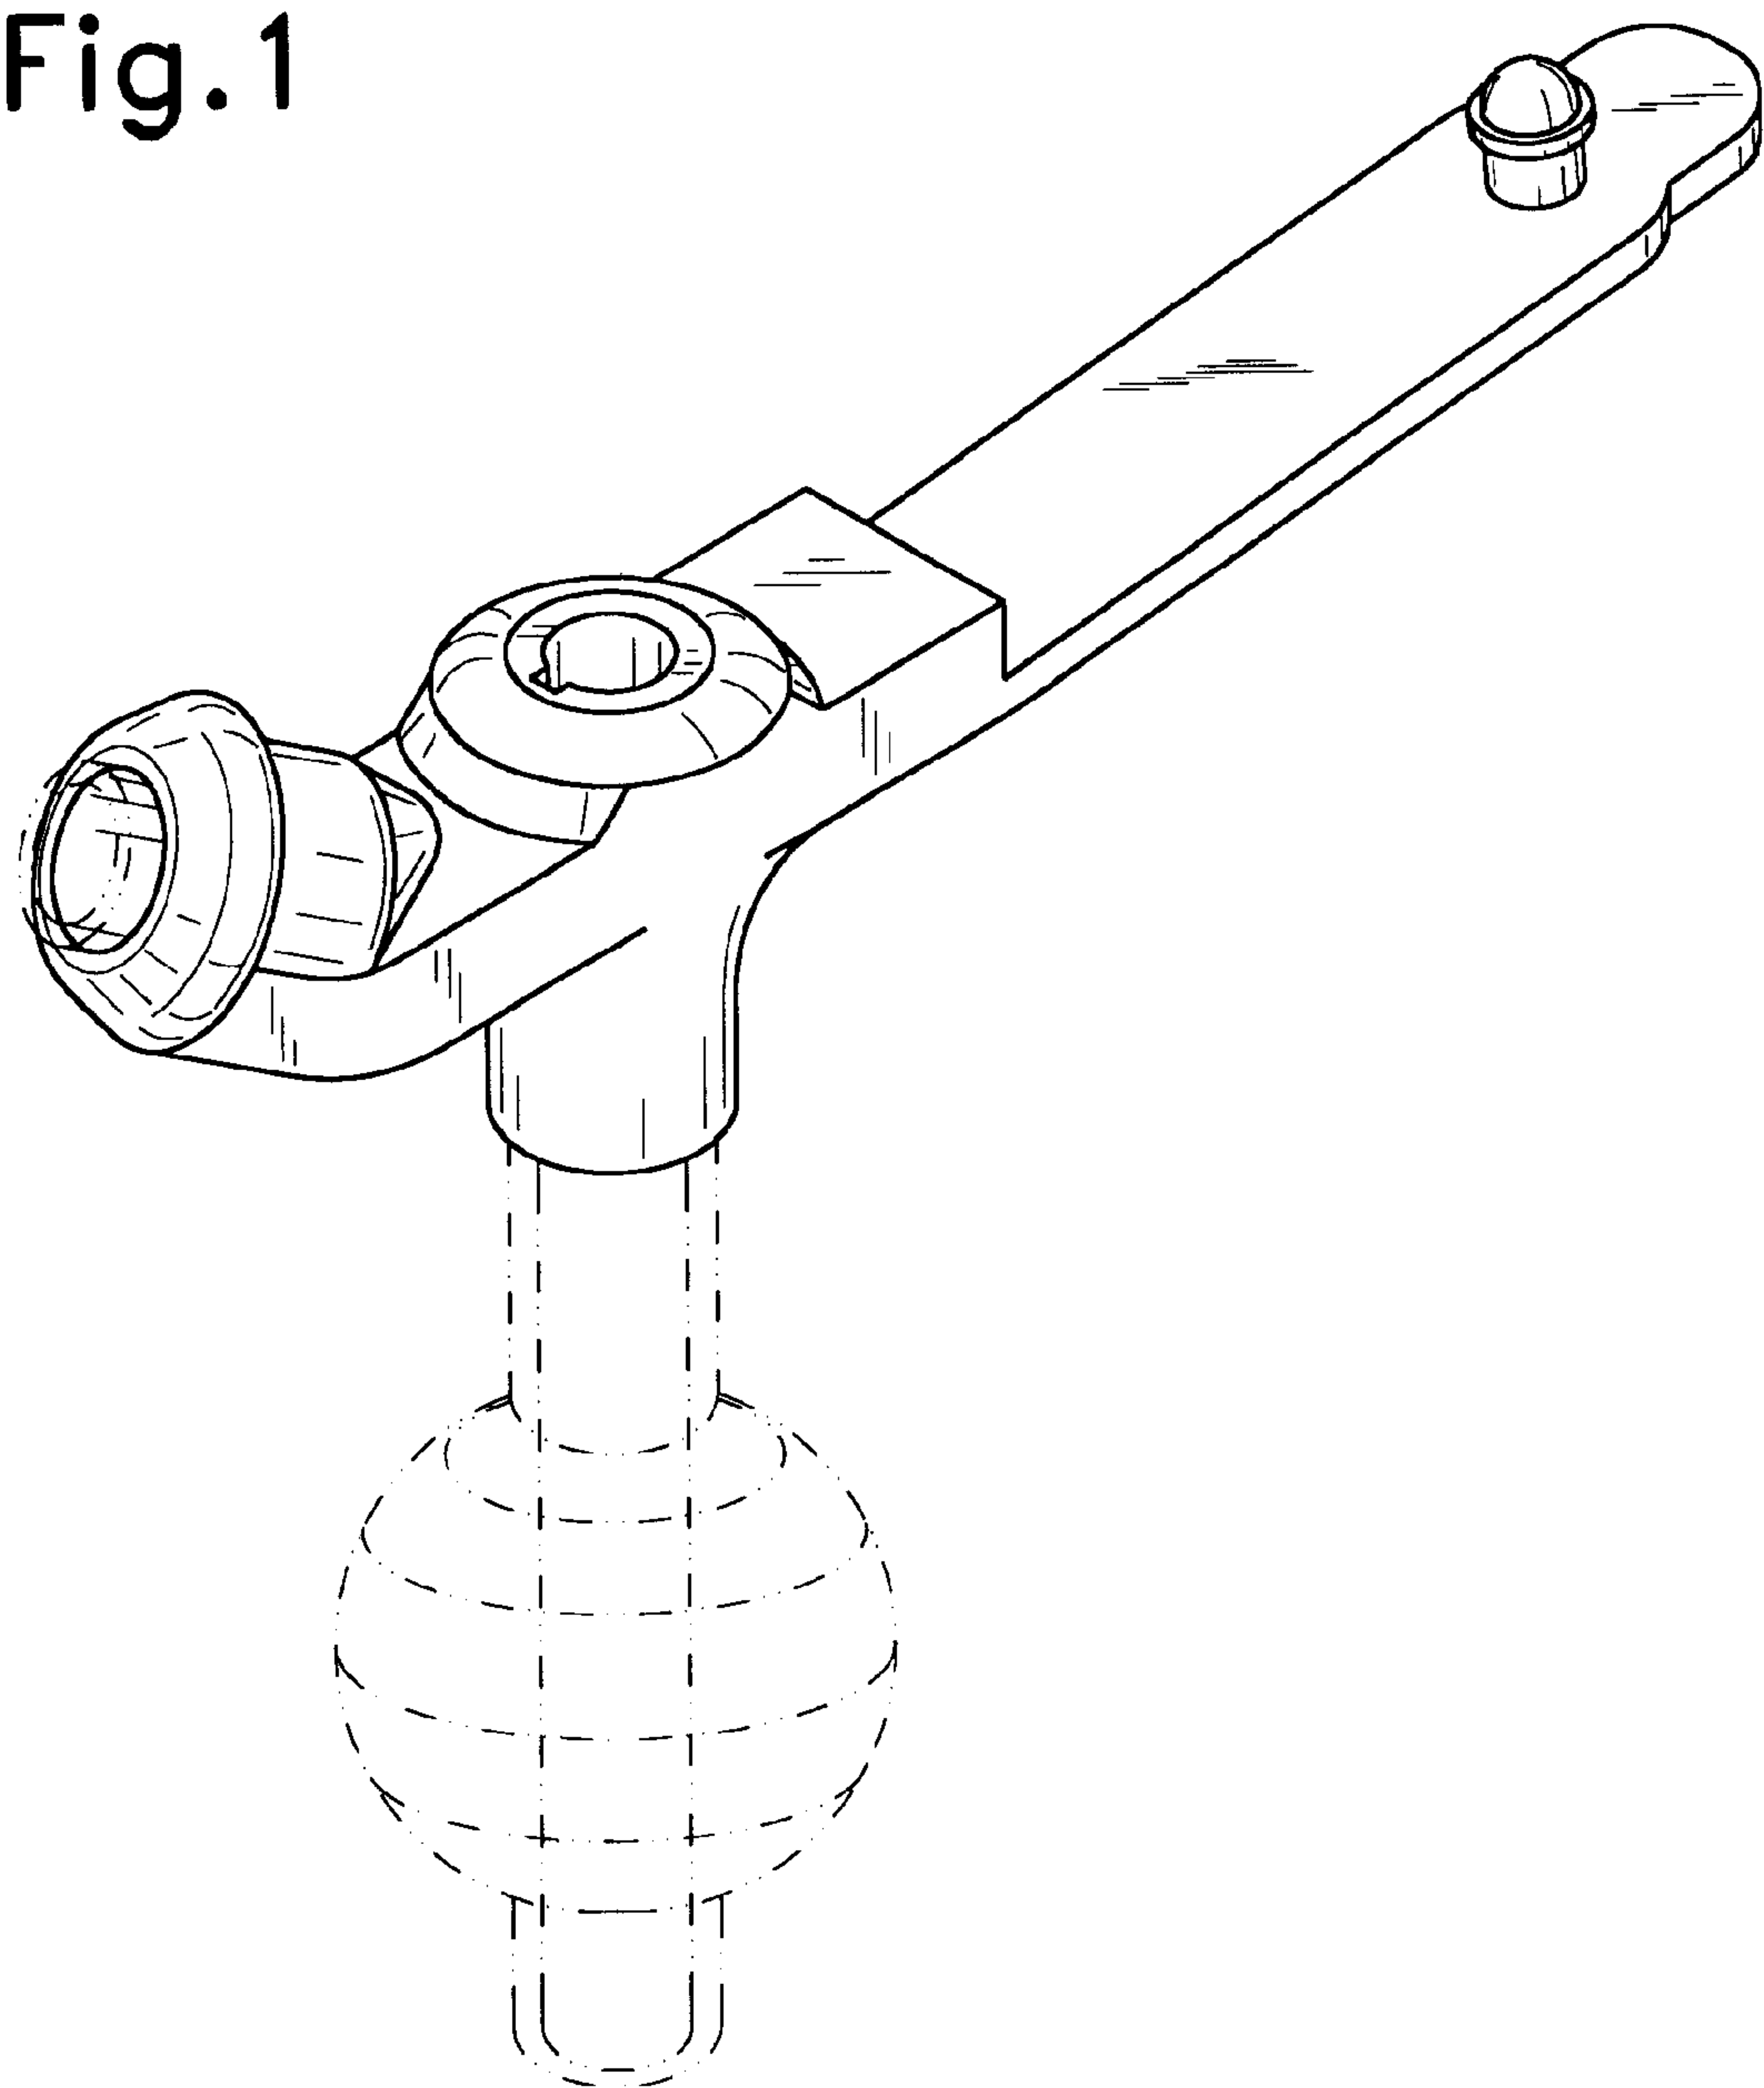

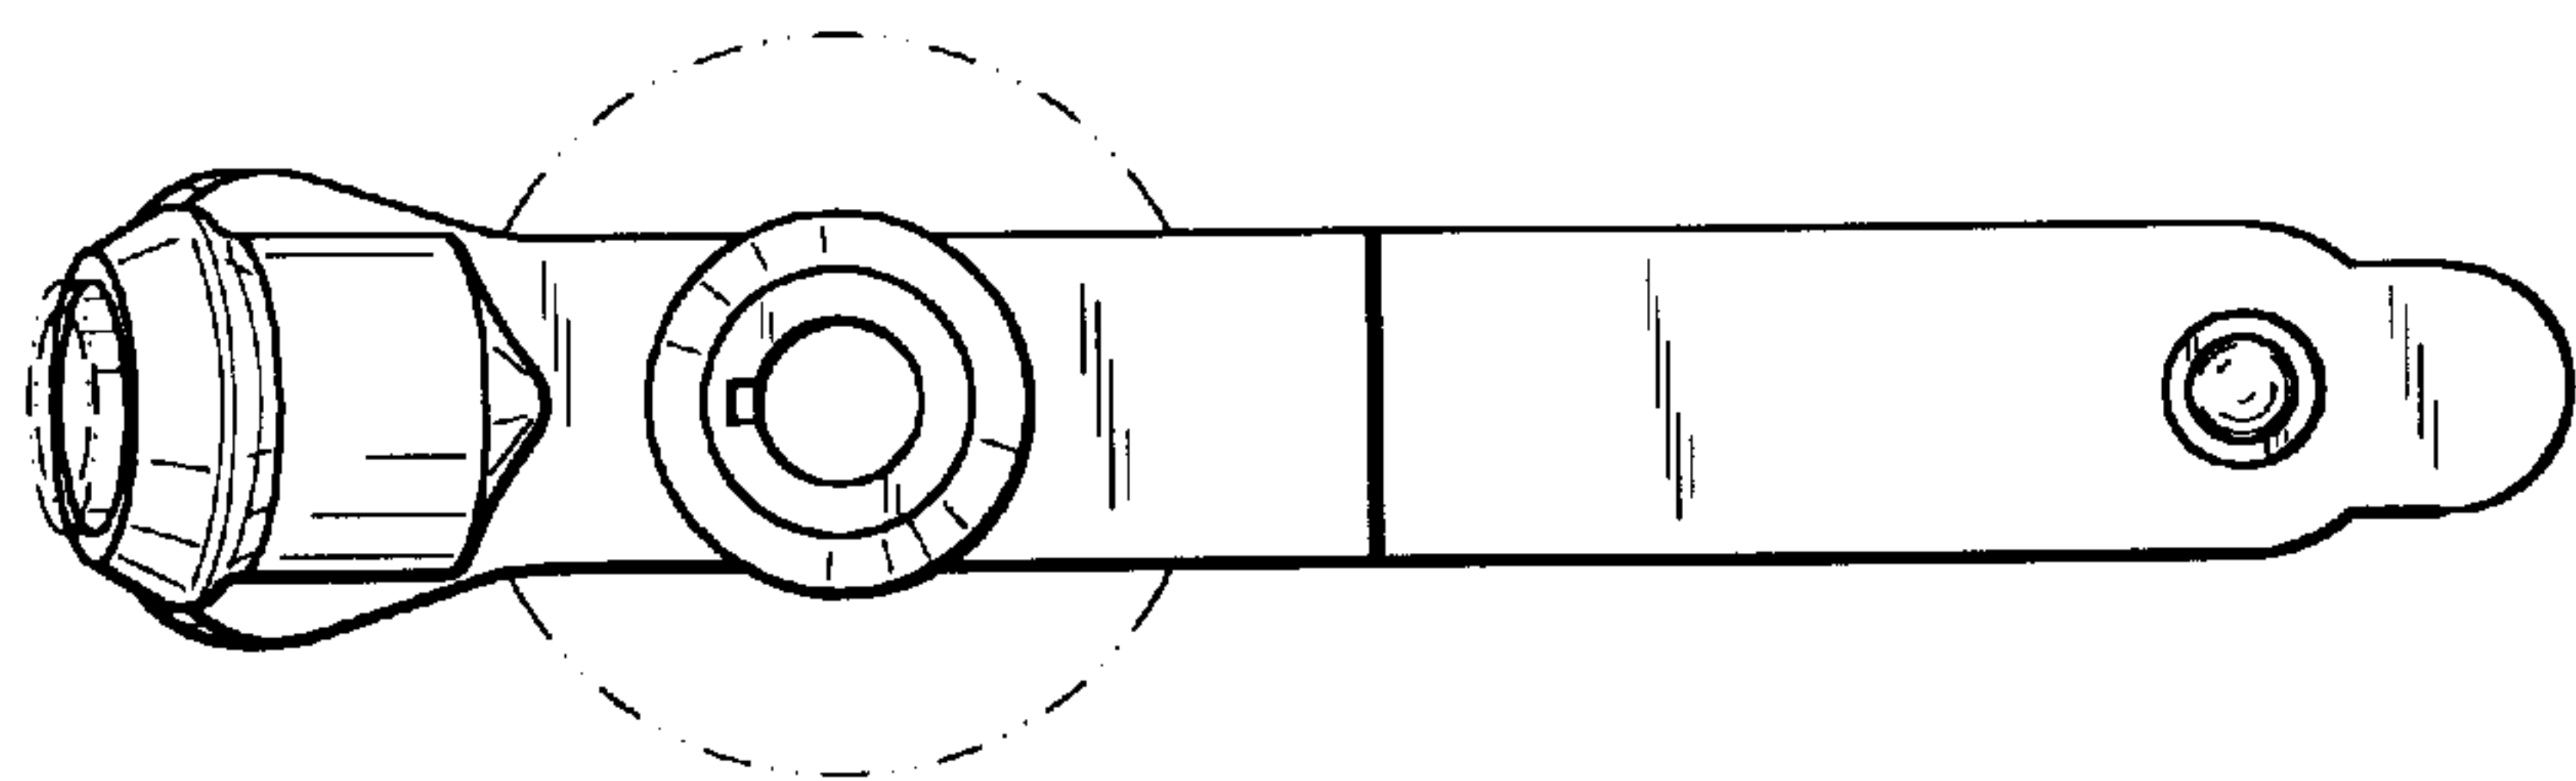


Fig.4

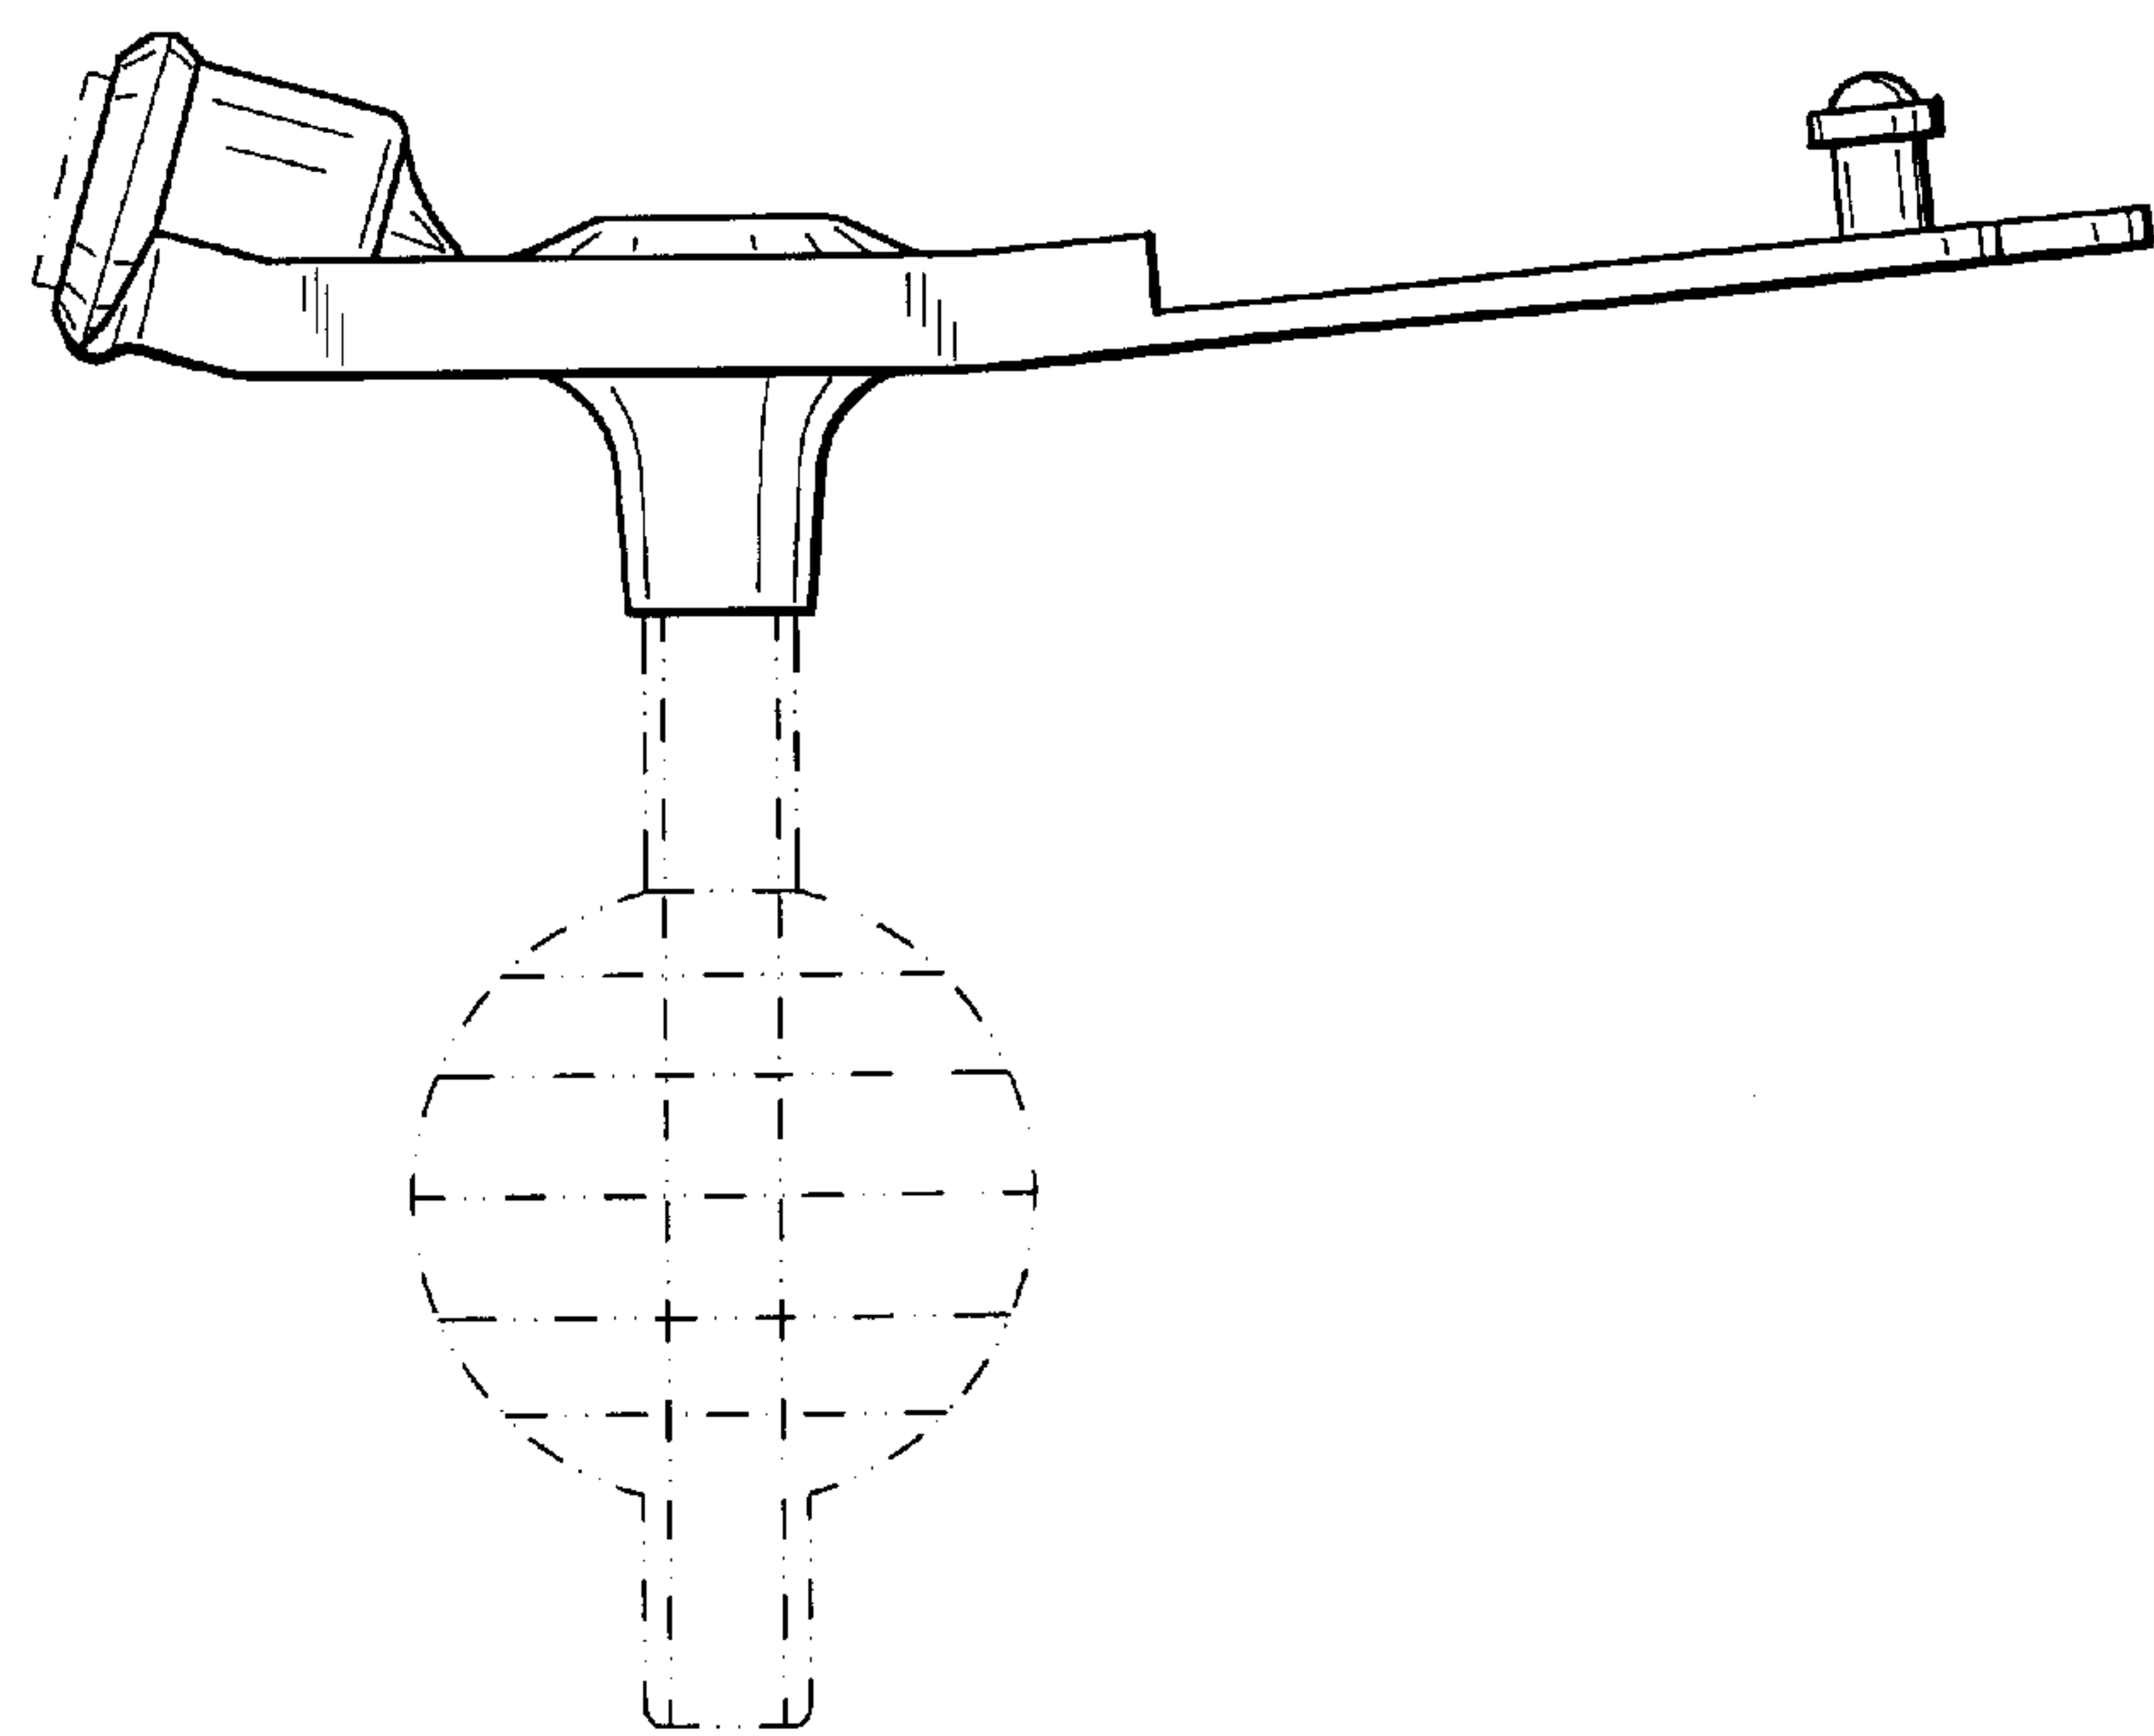


Fig.2

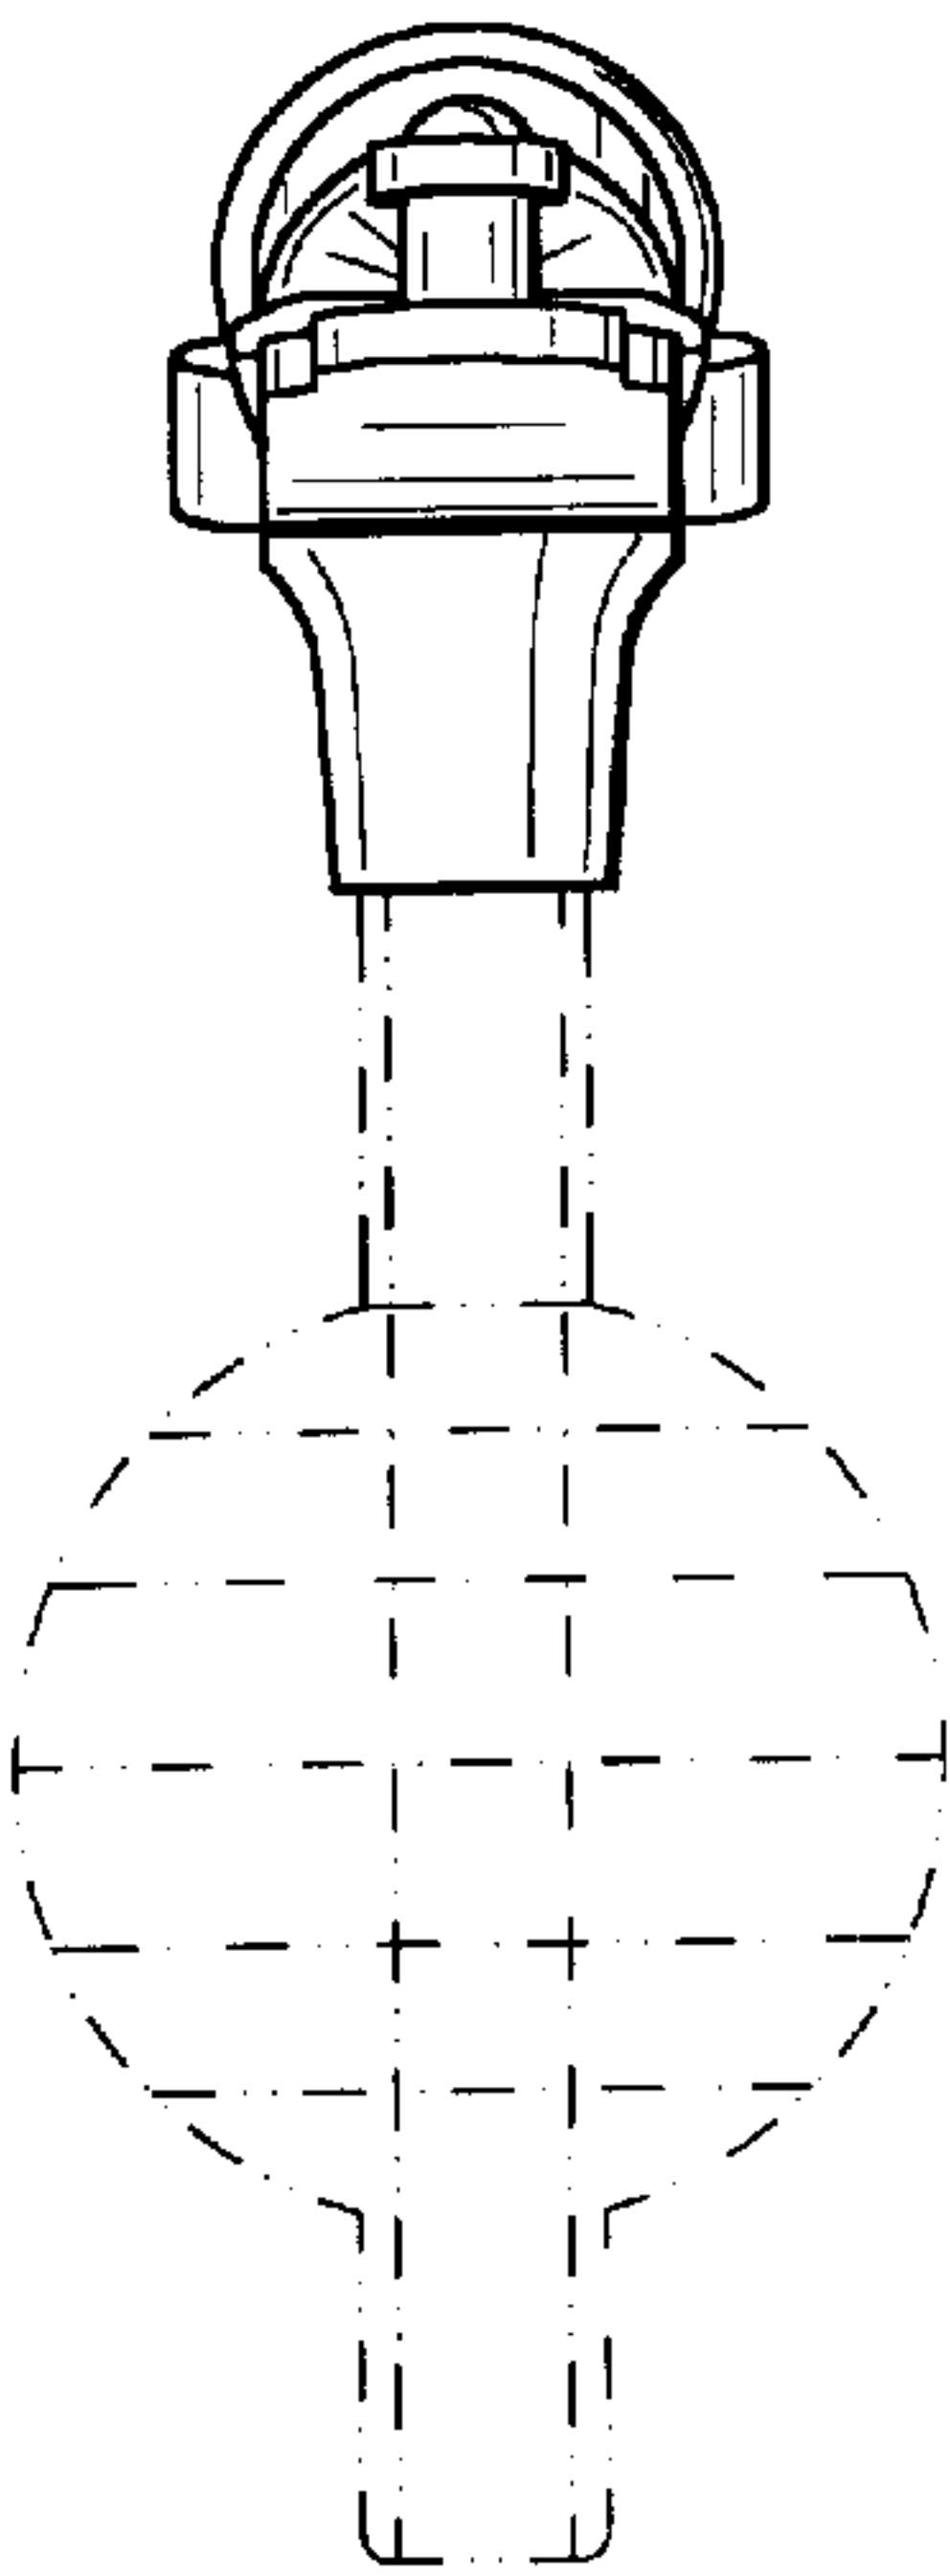


Fig.3

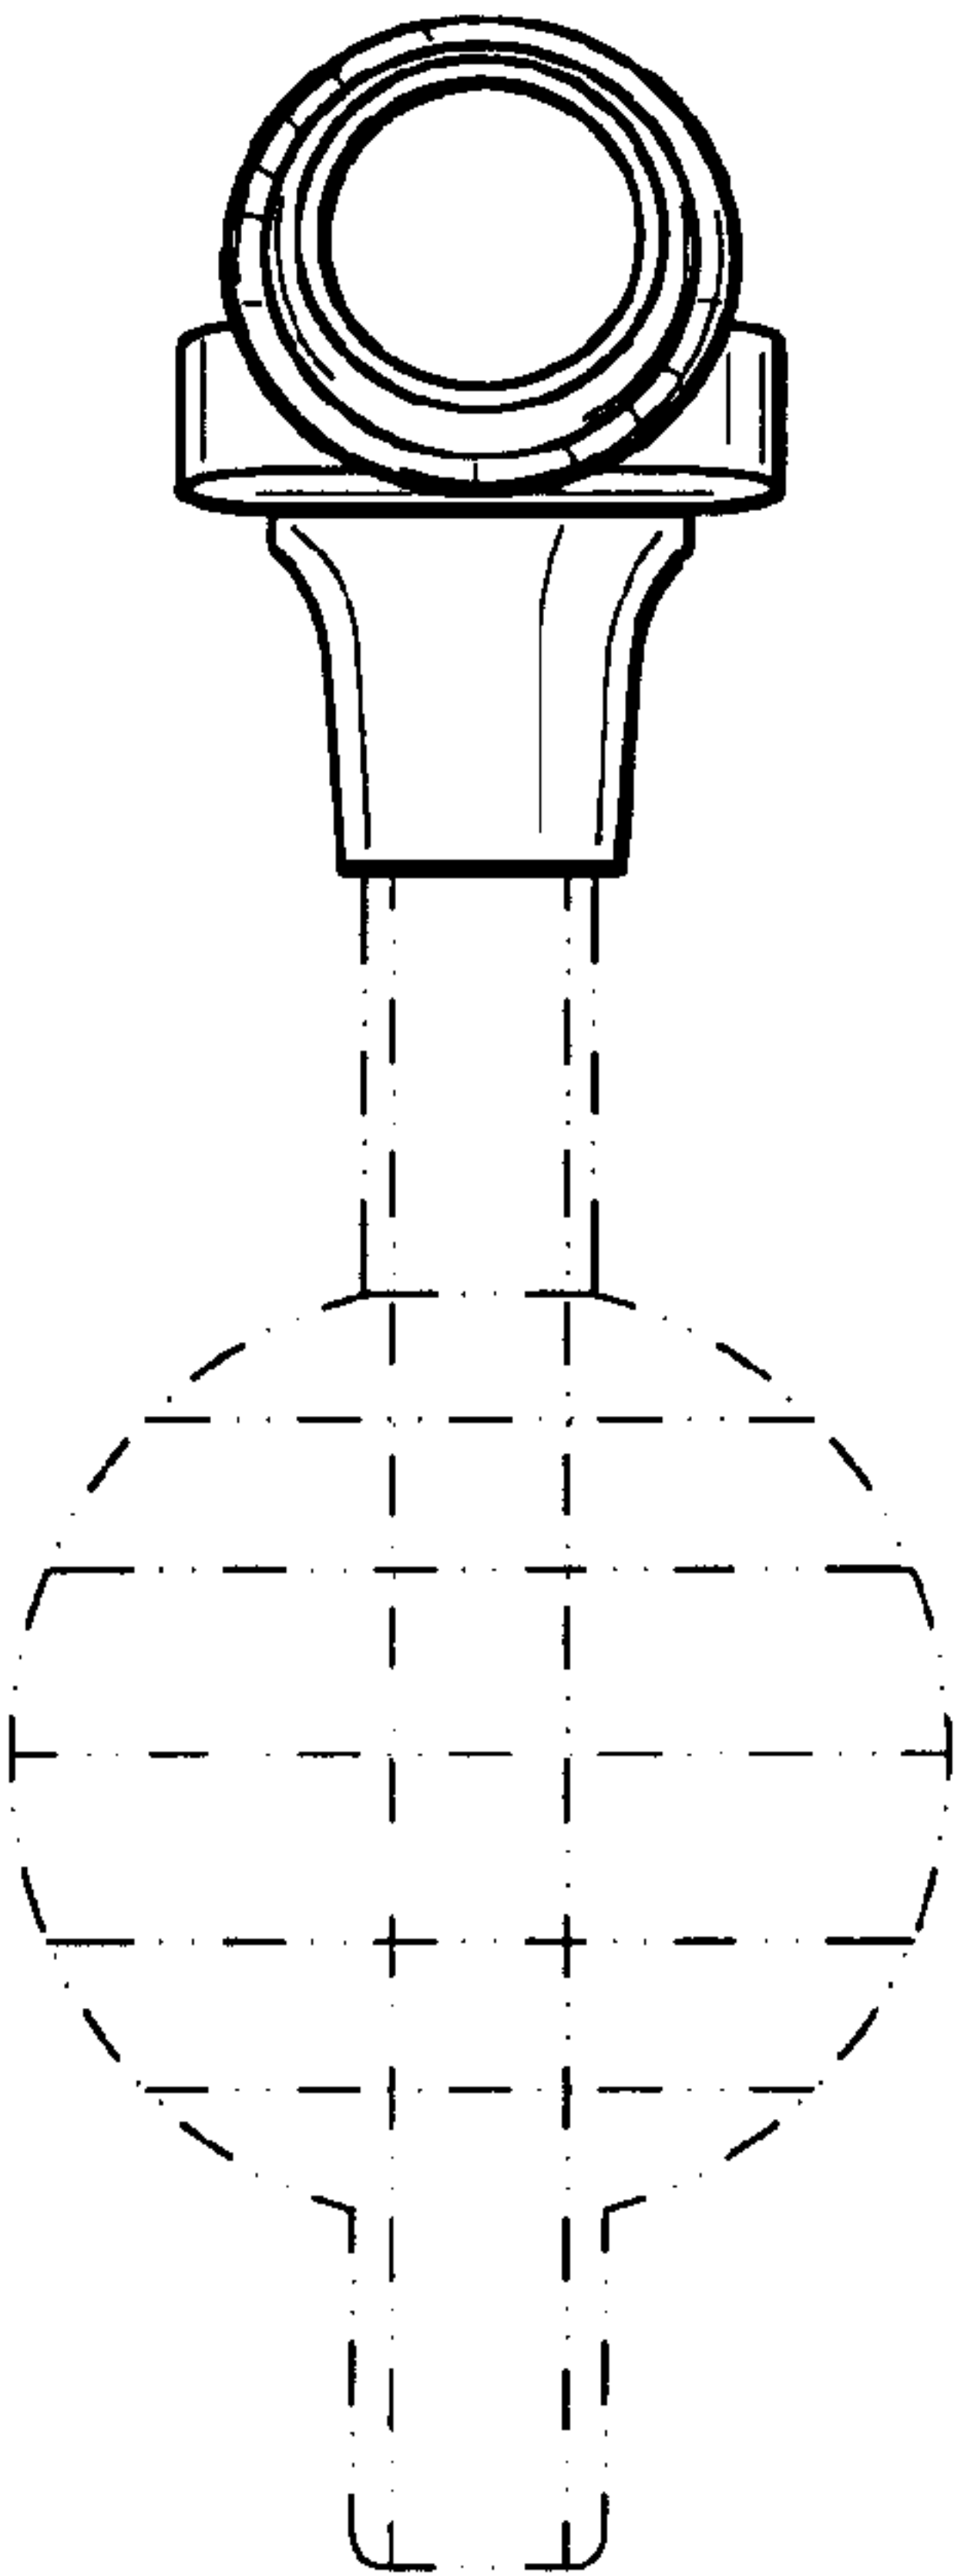


Fig.5

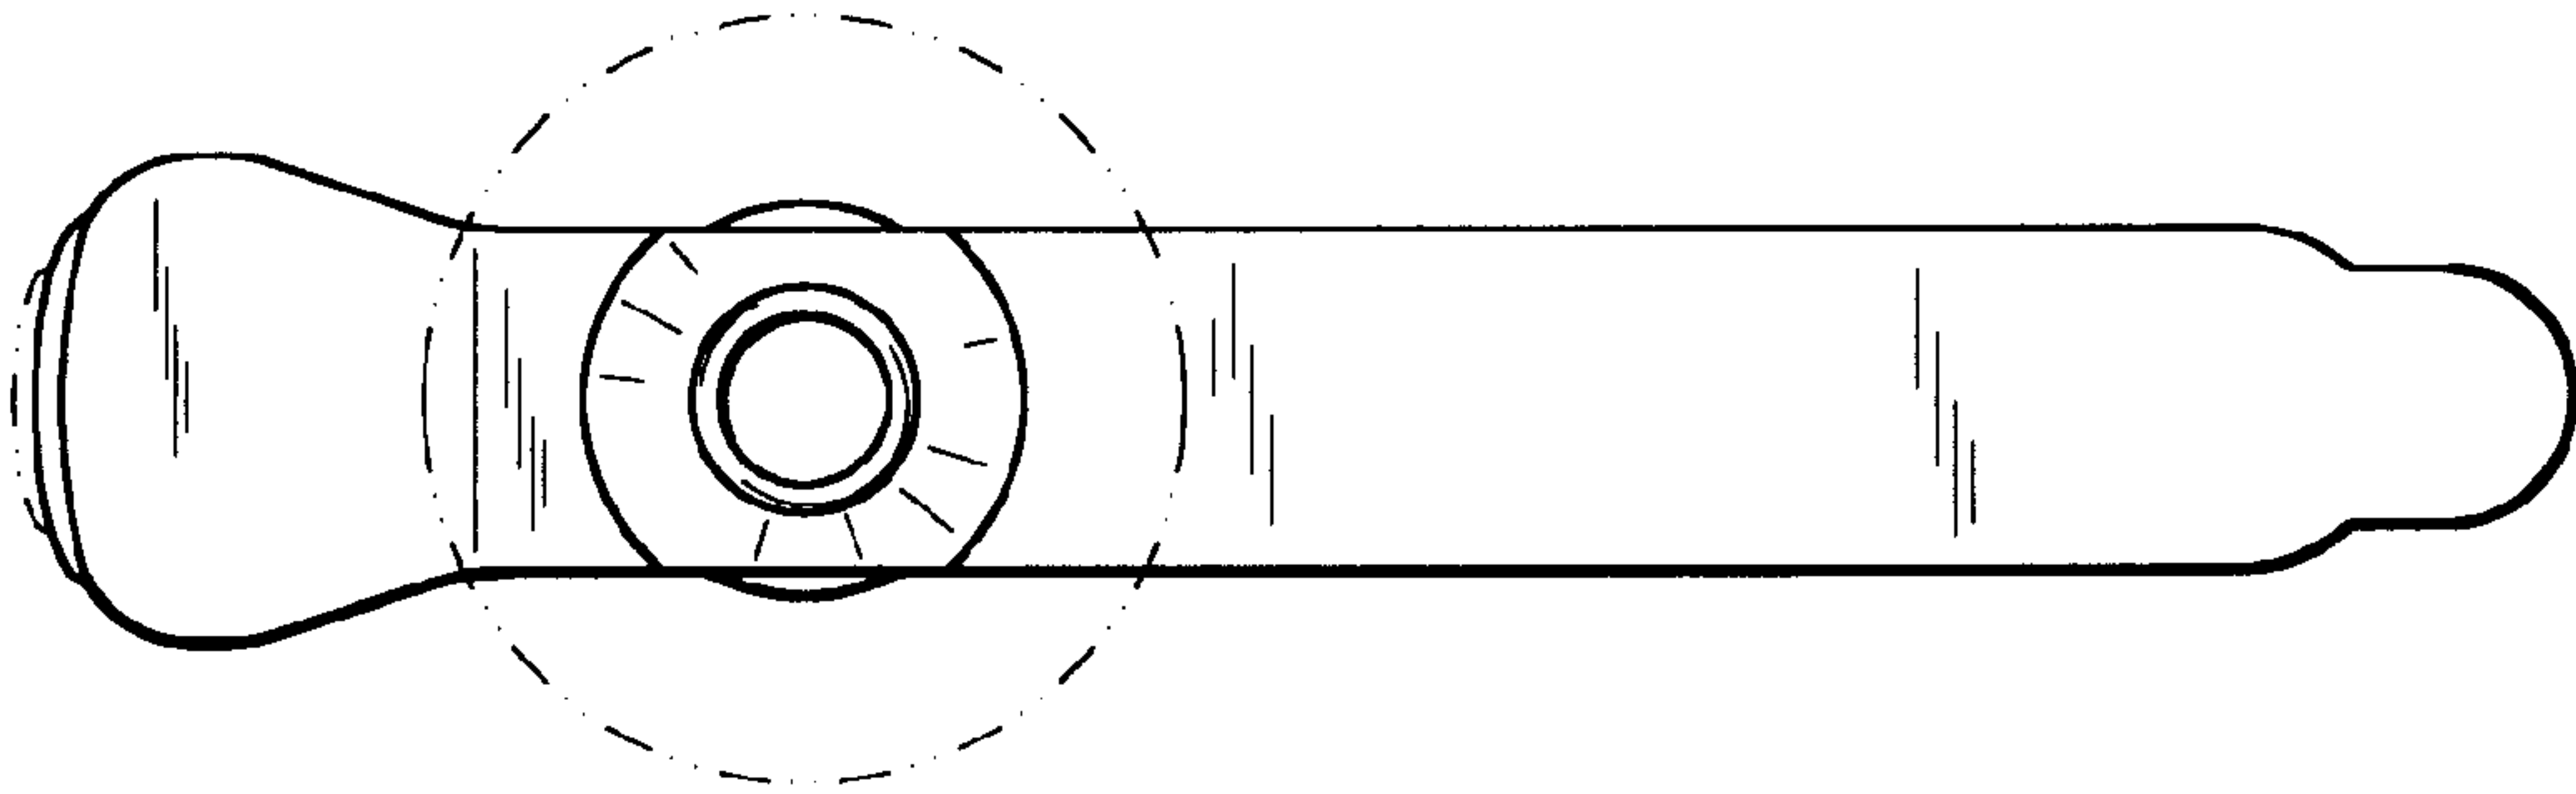


Fig.6