



US00D426298S

**United States Patent** [19]  
**Grannis et al.**

[11] **Patent Number: Des. 426,298**  
[45] **Date of Patent: \*\* Jun. 6, 2000**

[54] **FULL-FACE RESPIRATOR LENS**  
[75] Inventors: **Vaughn B. Grannis**, Inver Grove Heights; **David P. Knivslund**, North St. Paul; **Joseph G. Reischel**, Woodbury; **Gerald M. Brostrom**, Burnsville; **David C. Byram**, River Falls, all of Minn.

4,402,316	9/1983	Gadberry .....	128/201.15
4,414,973	11/1983	Matheson et al. ....	128/206.15
4,574,799	3/1986	Warncke .....	128/206.24
4,595,003	6/1986	Shoemaker et al. ....	128/201.19
4,739,755	4/1988	White et al. ....	128/206.12
4,756,308	7/1988	Ryback .....	128/201.19

(List continued on next page.)

[73] Assignee: **3M Innovative Properties Company**, St. Paul, Minn.

[\*\*] Term: **14 Years**

[21] Appl. No.: **29/090,916**

[22] Filed: **Jul. 20, 1998**

**Related U.S. Application Data**

[60] Continuation-in-part of application No. 29/067,529, Mar. 5, 1997, Pat. No. Des. 409,744, which is a division of application No. 29/060,111, Sep. 24, 1996, Pat. No. Des. 388,872.

[51] **LOC (7) Cl.** ..... **29-02**

[52] **U.S. Cl.** ..... **D24/110.2; D24/110.4**

[58] **Field of Search** ..... D24/110.1, 110.2, D24/110.3; 128/201.18, 206.21, 201.12, 201.15, 201.17, 201.28; 2/452

[56] **References Cited**

**U.S. PATENT DOCUMENTS**

D. 213,077	12/1968	Holloway .....	D83/1
D. 240,086	5/1976	Riblett et al. ....	D86/10 A
D. 249,368	9/1978	Watkins, Jr. ....	D29/9
D. 285,496	9/1986	Berman .....	D29/8
D. 331,988	12/1992	Markert .....	D29/9
D. 336,546	6/1993	Lybrand .....	D29/7
D. 351,226	10/1994	Parvatharaj .....	D24/110
D. 378,610	3/1997	Reischel et al. ....	D24/110.2
D. 388,882	1/1998	Grannis et al. ....	D24/110.4
3,545,436	12/1970	Holloway .....	128/141
3,602,219	8/1971	Warncke .....	128/146.5
3,680,555	8/1972	Warncke .....	128/141 R
4,057,057	11/1977	Backlund .....	128/142.4
4,069,516	1/1978	Watkins, Jr. ....	2/428
4,167,185	9/1979	Lewis .....	128/146.7
4,373,520	2/1983	Arbique .....	128/201.19

**FOREIGN PATENT DOCUMENTS**

0 511 593 A1	11/1992	European Pat. Off. ....	A62B 18/02
2 268 076	1/1994	United Kingdom .....	A62B 18/08
WO 91/01159	2/1991	WIPO .....	A62B 18/10
WO 92/19322	11/1992	WIPO .....	A62B 18/02
WO 93/14819	8/1993	WIPO .....	A62B 18/02

**OTHER PUBLICATIONS**

Cabot Safety Respirator Products—The Life Line product literature (1993).  
North RP-107 Air-Purifying Respiratory Protection Catalog (1991).

(List continued on next page.)

*Primary Examiner*—Stella Reid  
*Assistant Examiner*—I Simmons  
*Attorney, Agent, or Firm*—Karl G. Hanson


[57] **CLAIM**

The ornamental design for a full-face respirator lens, as shown and described.

**DESCRIPTION**

FIG. 1 is a perspective view of a full-face respirator lens showing the new design;  
FIG. 2 is a front elevational view thereof;  
FIG. 3 is a left side elevational view thereof;  
FIG. 4 is a right side elevational view thereof;  
FIG. 5 is a rear elevational view thereof; and,  
FIG. 6 is a bottom elevational view thereof;  
The broken lines shown in the drawing form no part of the claimed design.  
The shading shown in the drawings is provided merely to illustrate contour; it is not indicative of any particular texture.

**1 Claim, 6 Drawing Sheets**

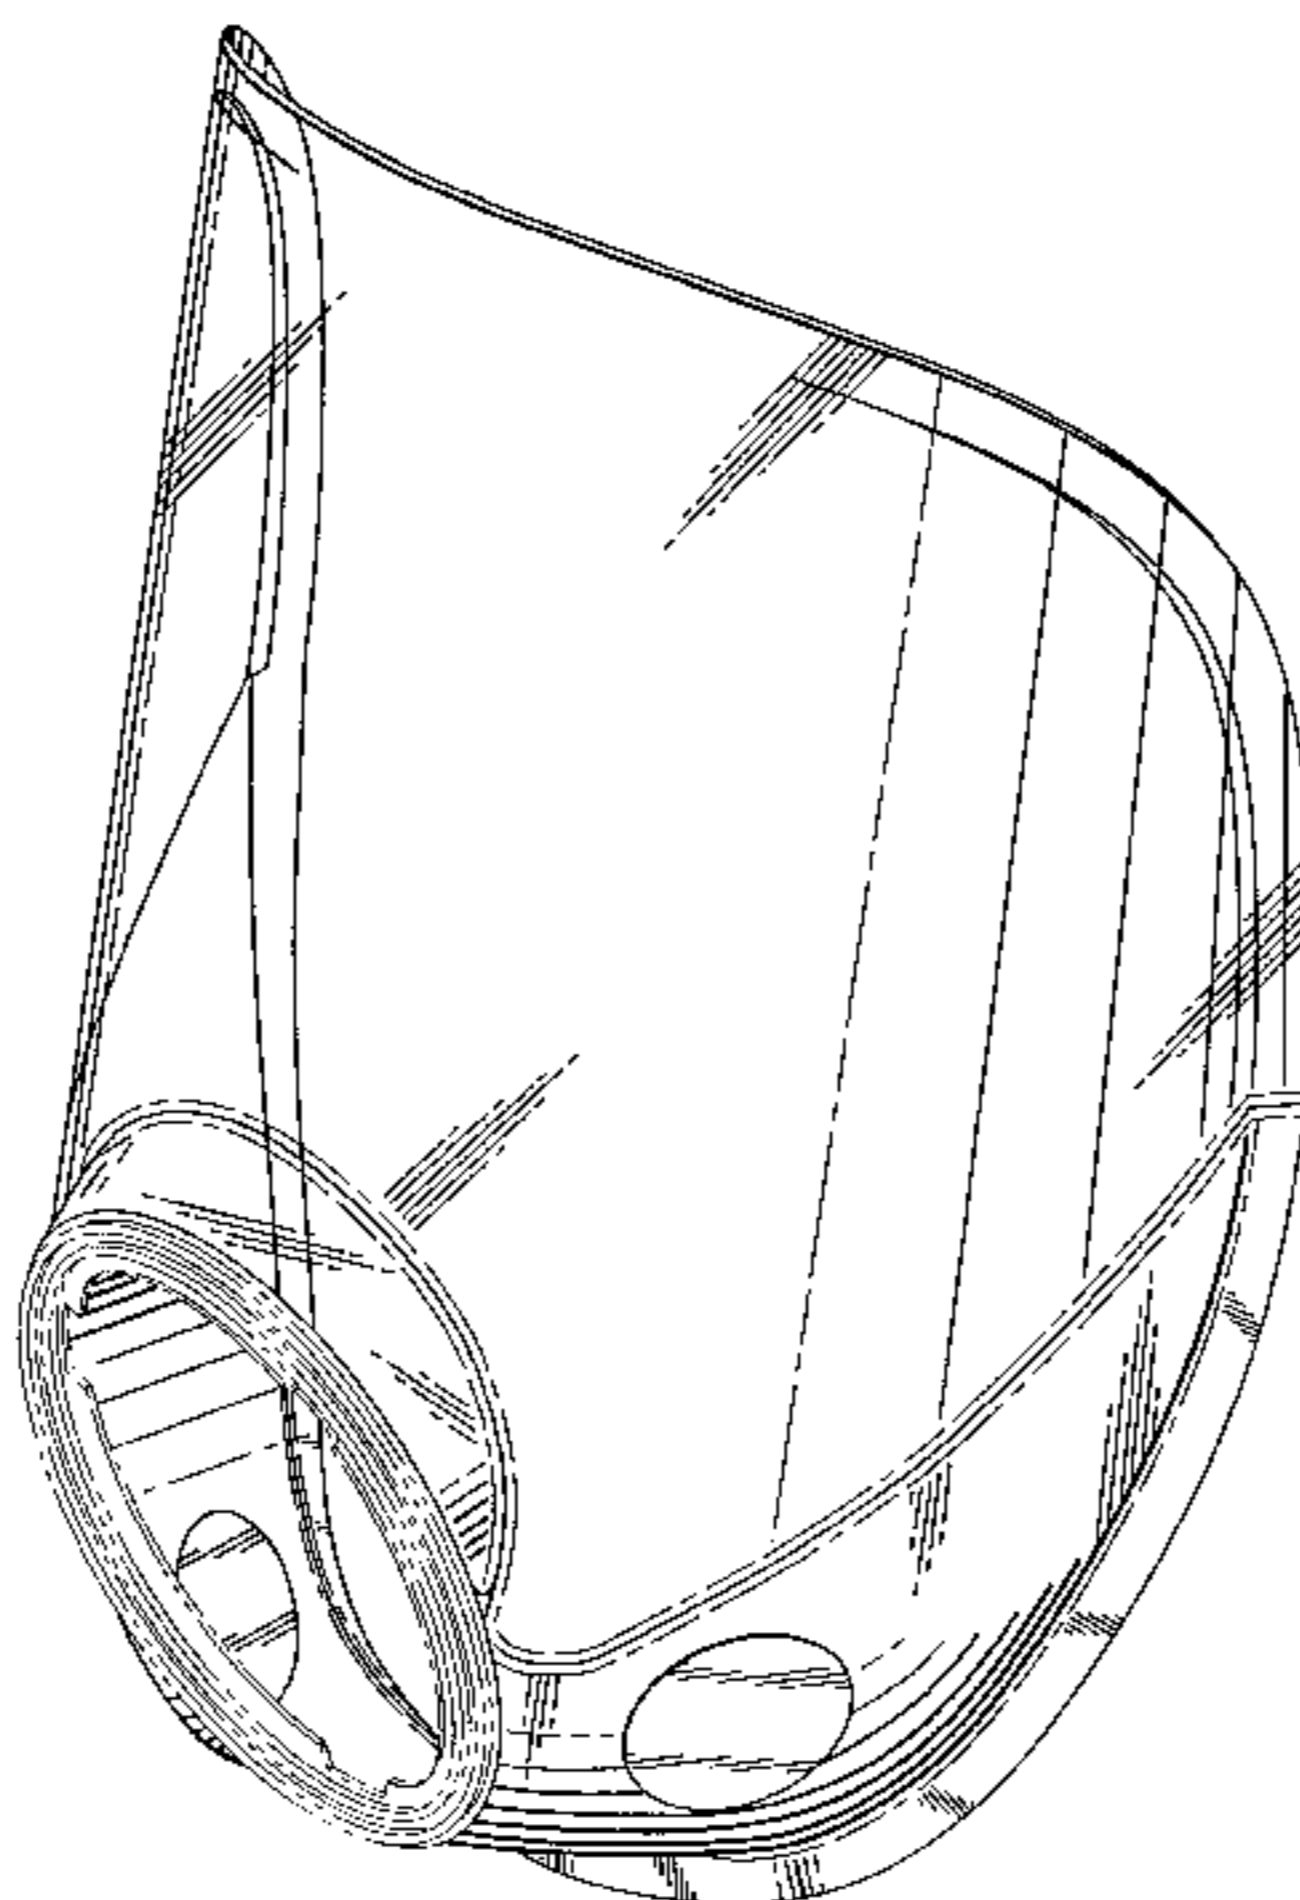

## U.S. PATENT DOCUMENTS

4,850,346	7/1989	Michel et al.	128/206.15
4,881,538	11/1989	Angell	128/201.15
4,960,121	10/1990	Nelson et al.	128/206.24
4,961,420	10/1990	Cappa et al.	128/207.12
5,069,205	12/1991	Urso	128/201.24
5,080,092	1/1992	Tenna	128/201.19
5,720,291	2/1998	Allen et al.	128/206.21 X

## OTHER PUBLICATIONS

MSA Comfo® II and Comfo Elite® Respirators products literature (1993).

MSA Comfo Classic Respirators product literature (1995).

MSA ComfoElite™ product literature (1990).

Gerson Signature Series 9000 product literature (1995).

Gerson Signature Series 8000 product literature (1995).

Willson product literature (1991).

The Lab Safety Supply Catalog "Respirators" pp. 130, 112, 110, 1994, Ex Room.

3M™ 6000 Series Full Facepiece Respirators product literature #70-0707-5770-6 (1264)ii (Dec. 1996).

3M 6000 Series Half and Full Facepiece Respirators product literature #70-07078-4558-4(1081)ii (Oct. 1998).

36 6000 Series Full Facepiece Respirator product literature #34-7045-4459-1 (1998).

ISI Facemask product literature.

Neoterik advertisement for the Technirama respirator.

Dräger Atemkomfort mit DrägerSchutz Panorama BelAir M product literature.

Fernez Cosmo The Innovative Mask product literature.

Cairns & Brother CairnsIRIS™ product literature.

Sekur Spa Sfera™ product literature.

SGE 600 product literature.

Dräger Atemkomfort mit DrägerSchutz: Panorama BelAir product literature (6 pages).

MSA Advantage 1000 Low-Maintenance Respirator product literature (1993).

Scott Weld-O-Vista™ product literature (1994).

MSA Constant Flow or Pressure Demand Duo-Flo™ and Duo-Twin™ Respirator product literature (1999).

MSA Optimair™ 6A Papr with Optifilter™ Catridges product literature (1988).


ProTech Respirators, Inc. product literature (1993).

Scott Health & Safety Full-Line Catalog product literature (May 1989).


MSA Ultra Elite™ Facepiece product literature dated (1994).

Dräger Luft holen . . . Der Atemschutz-Katalog (1993/94).


Scott respirator product literature (1992).

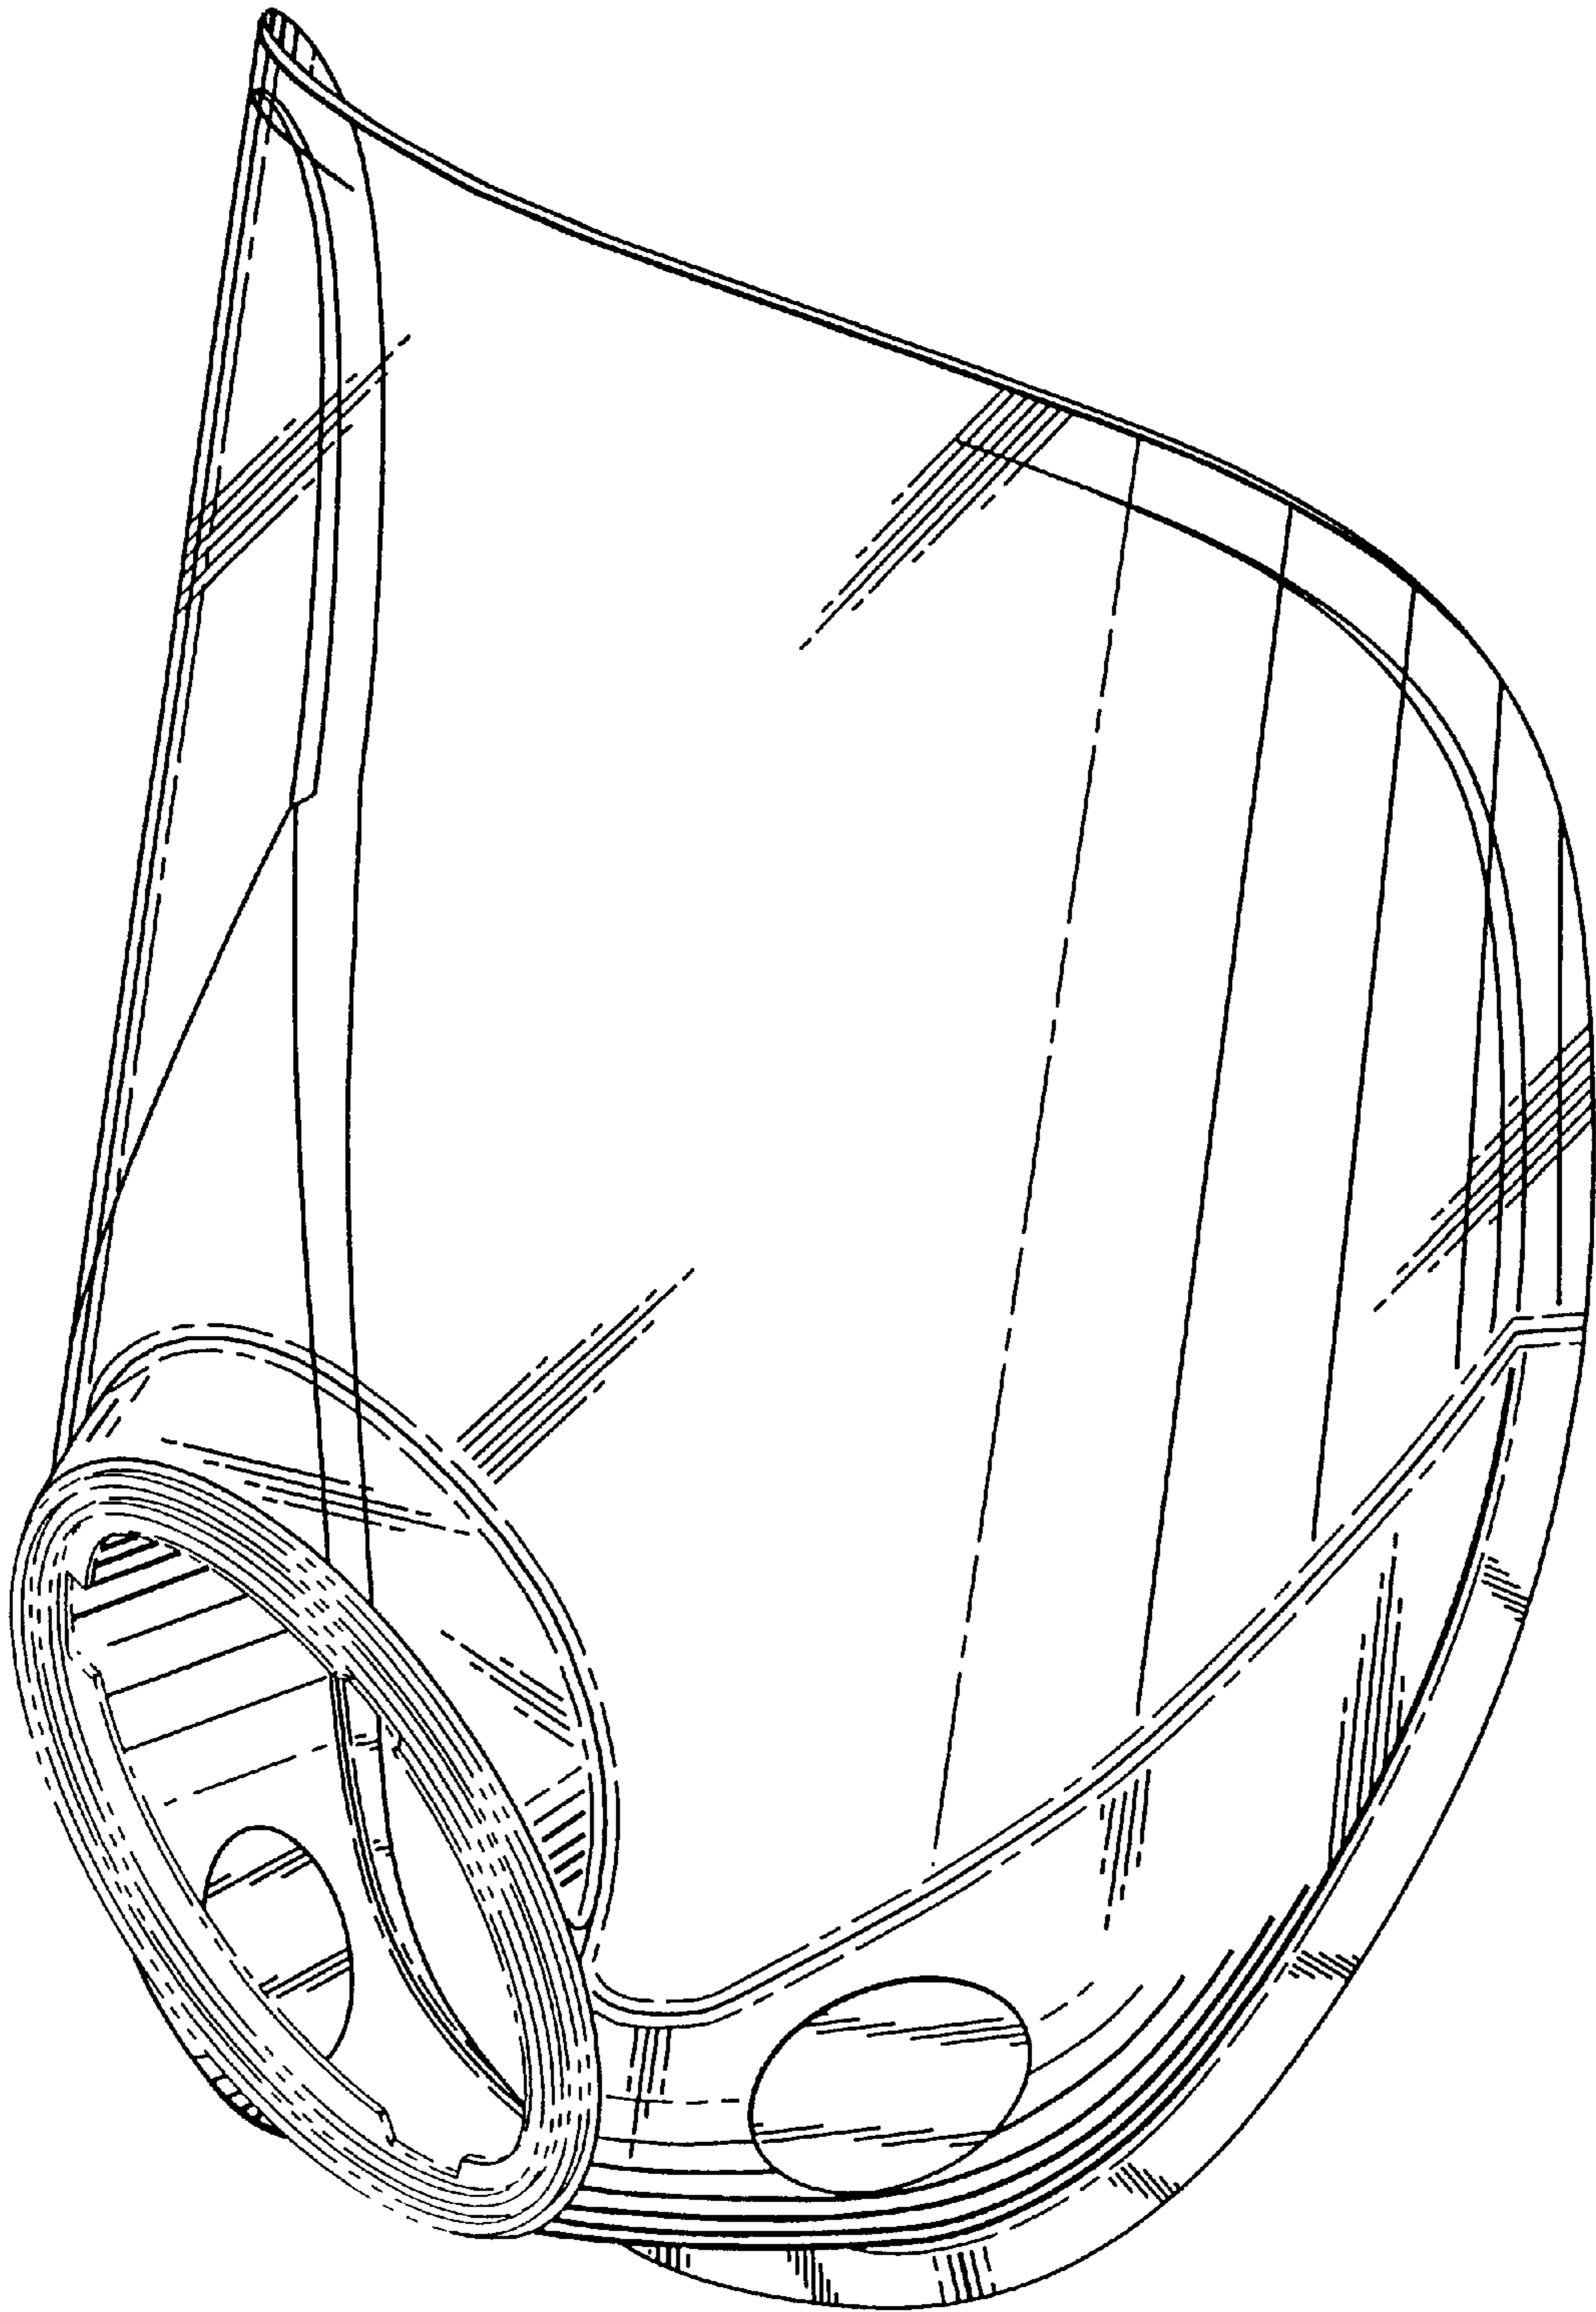


*Fig. 1*

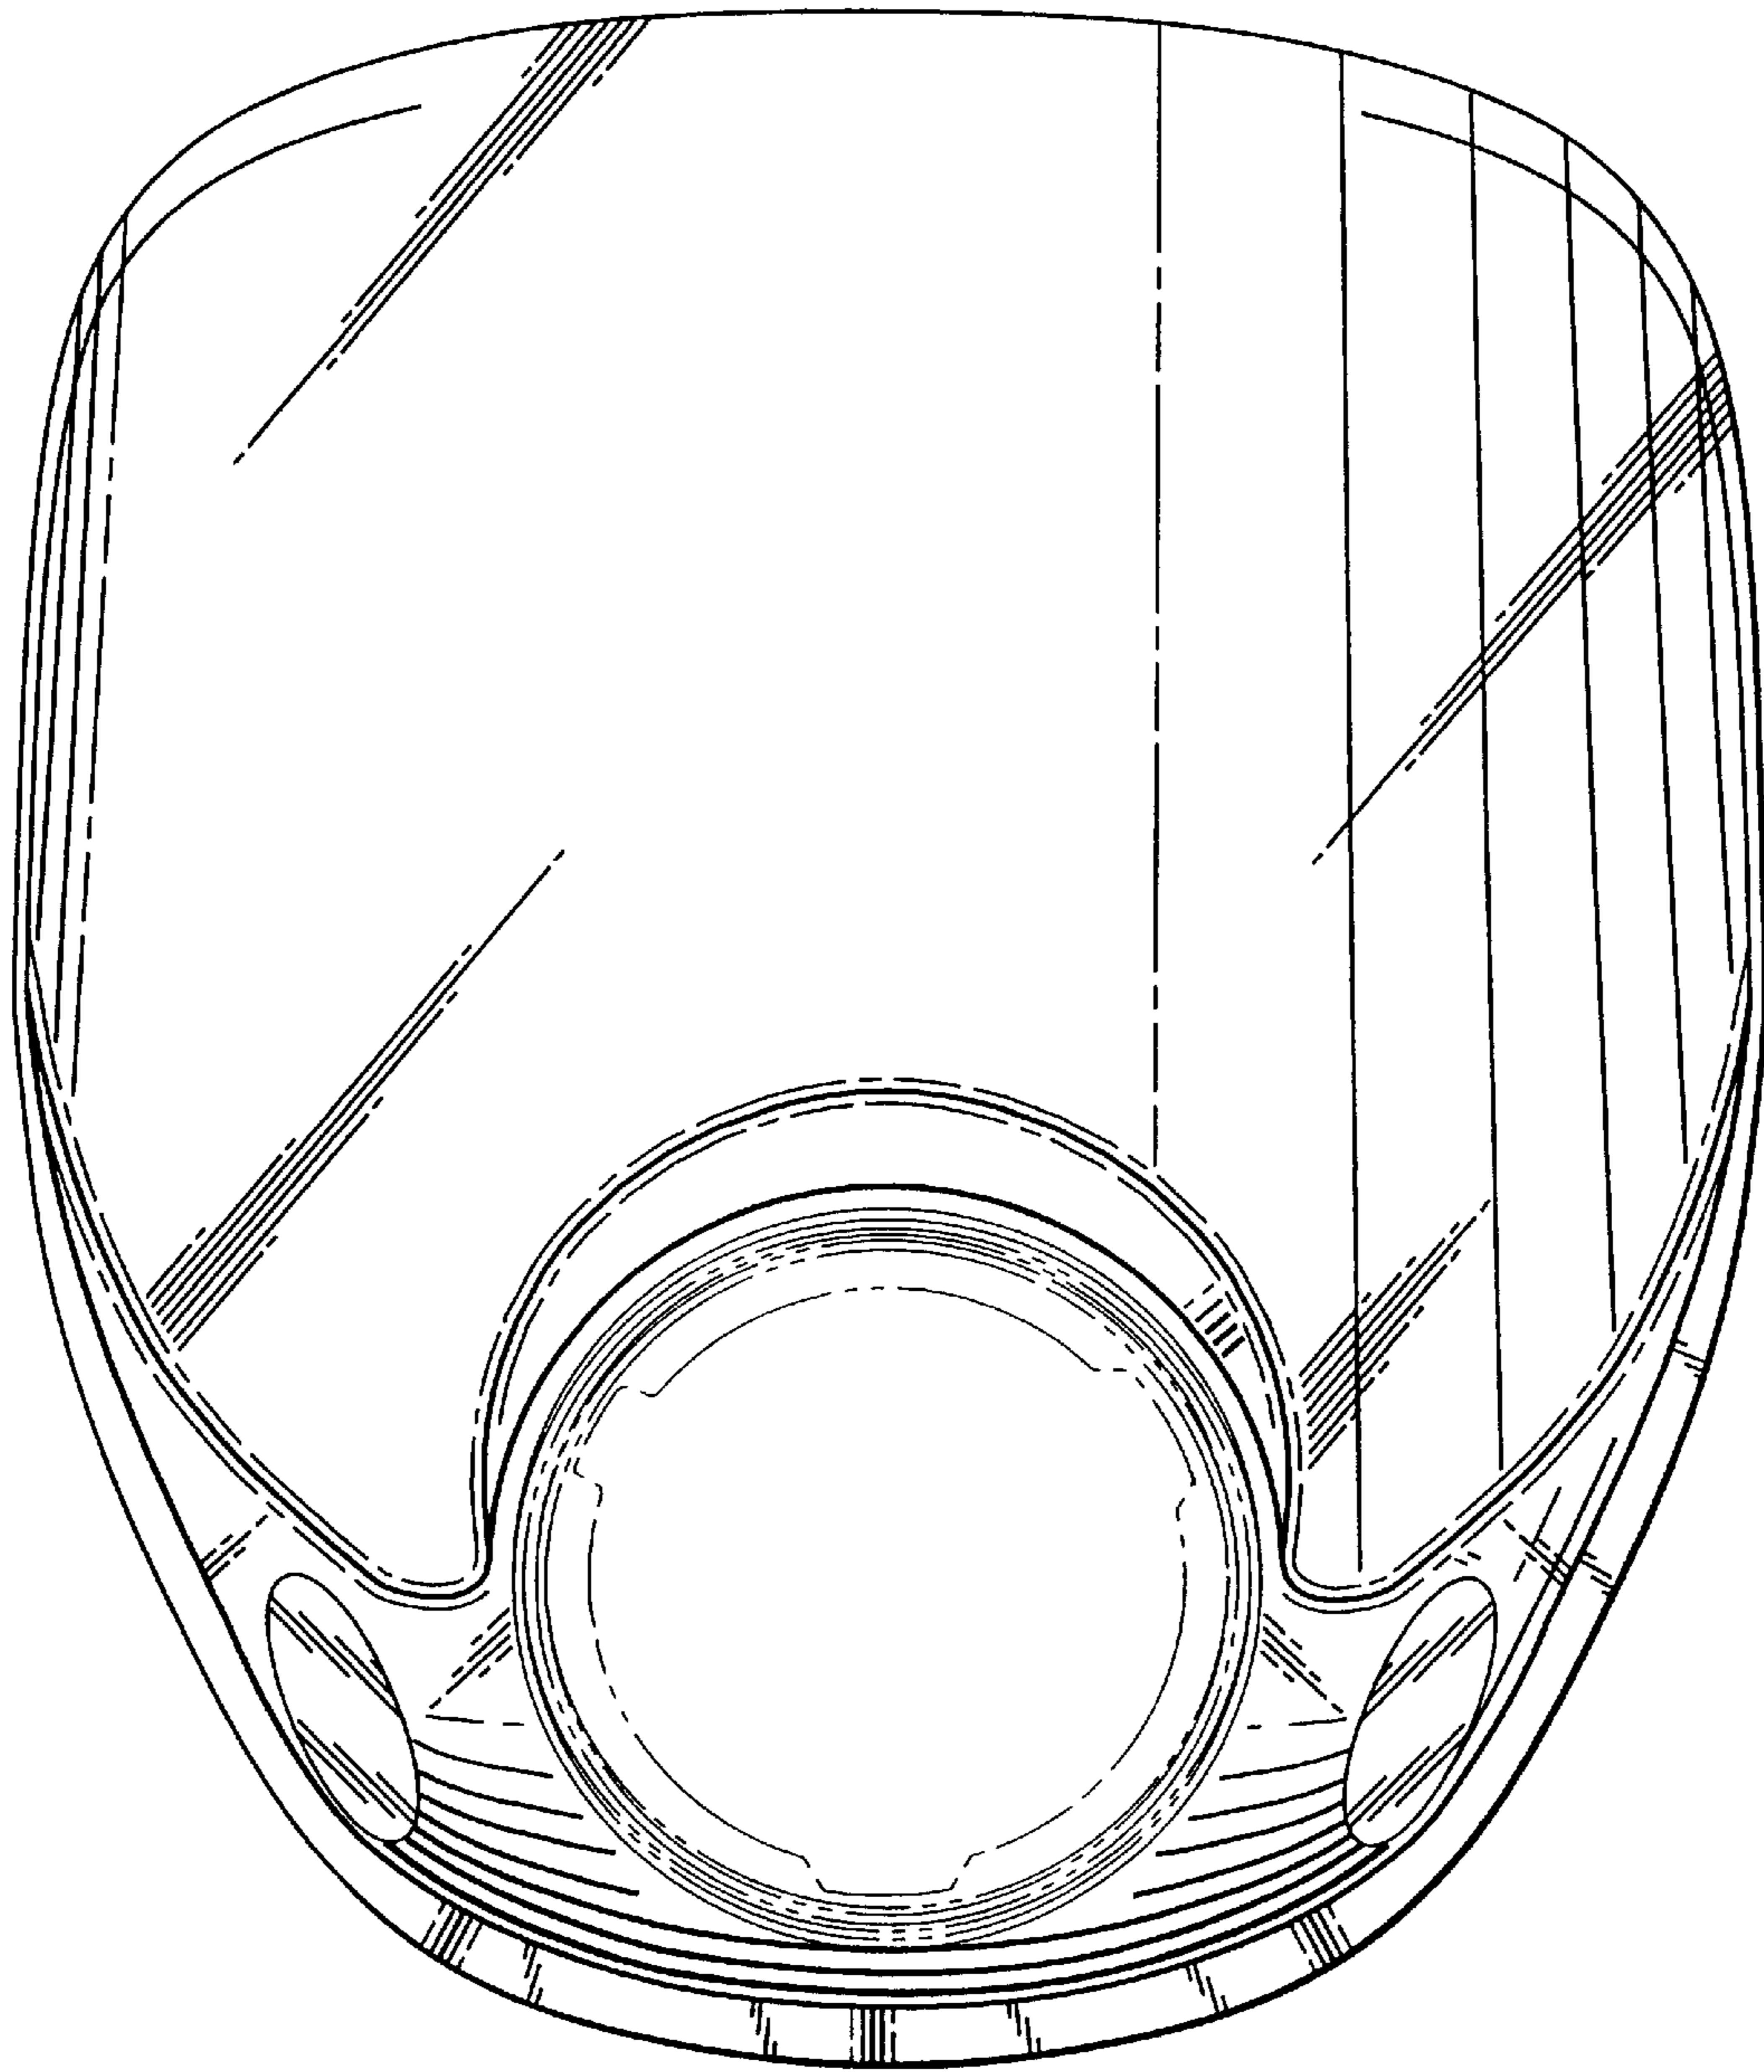


*Fig. 2*

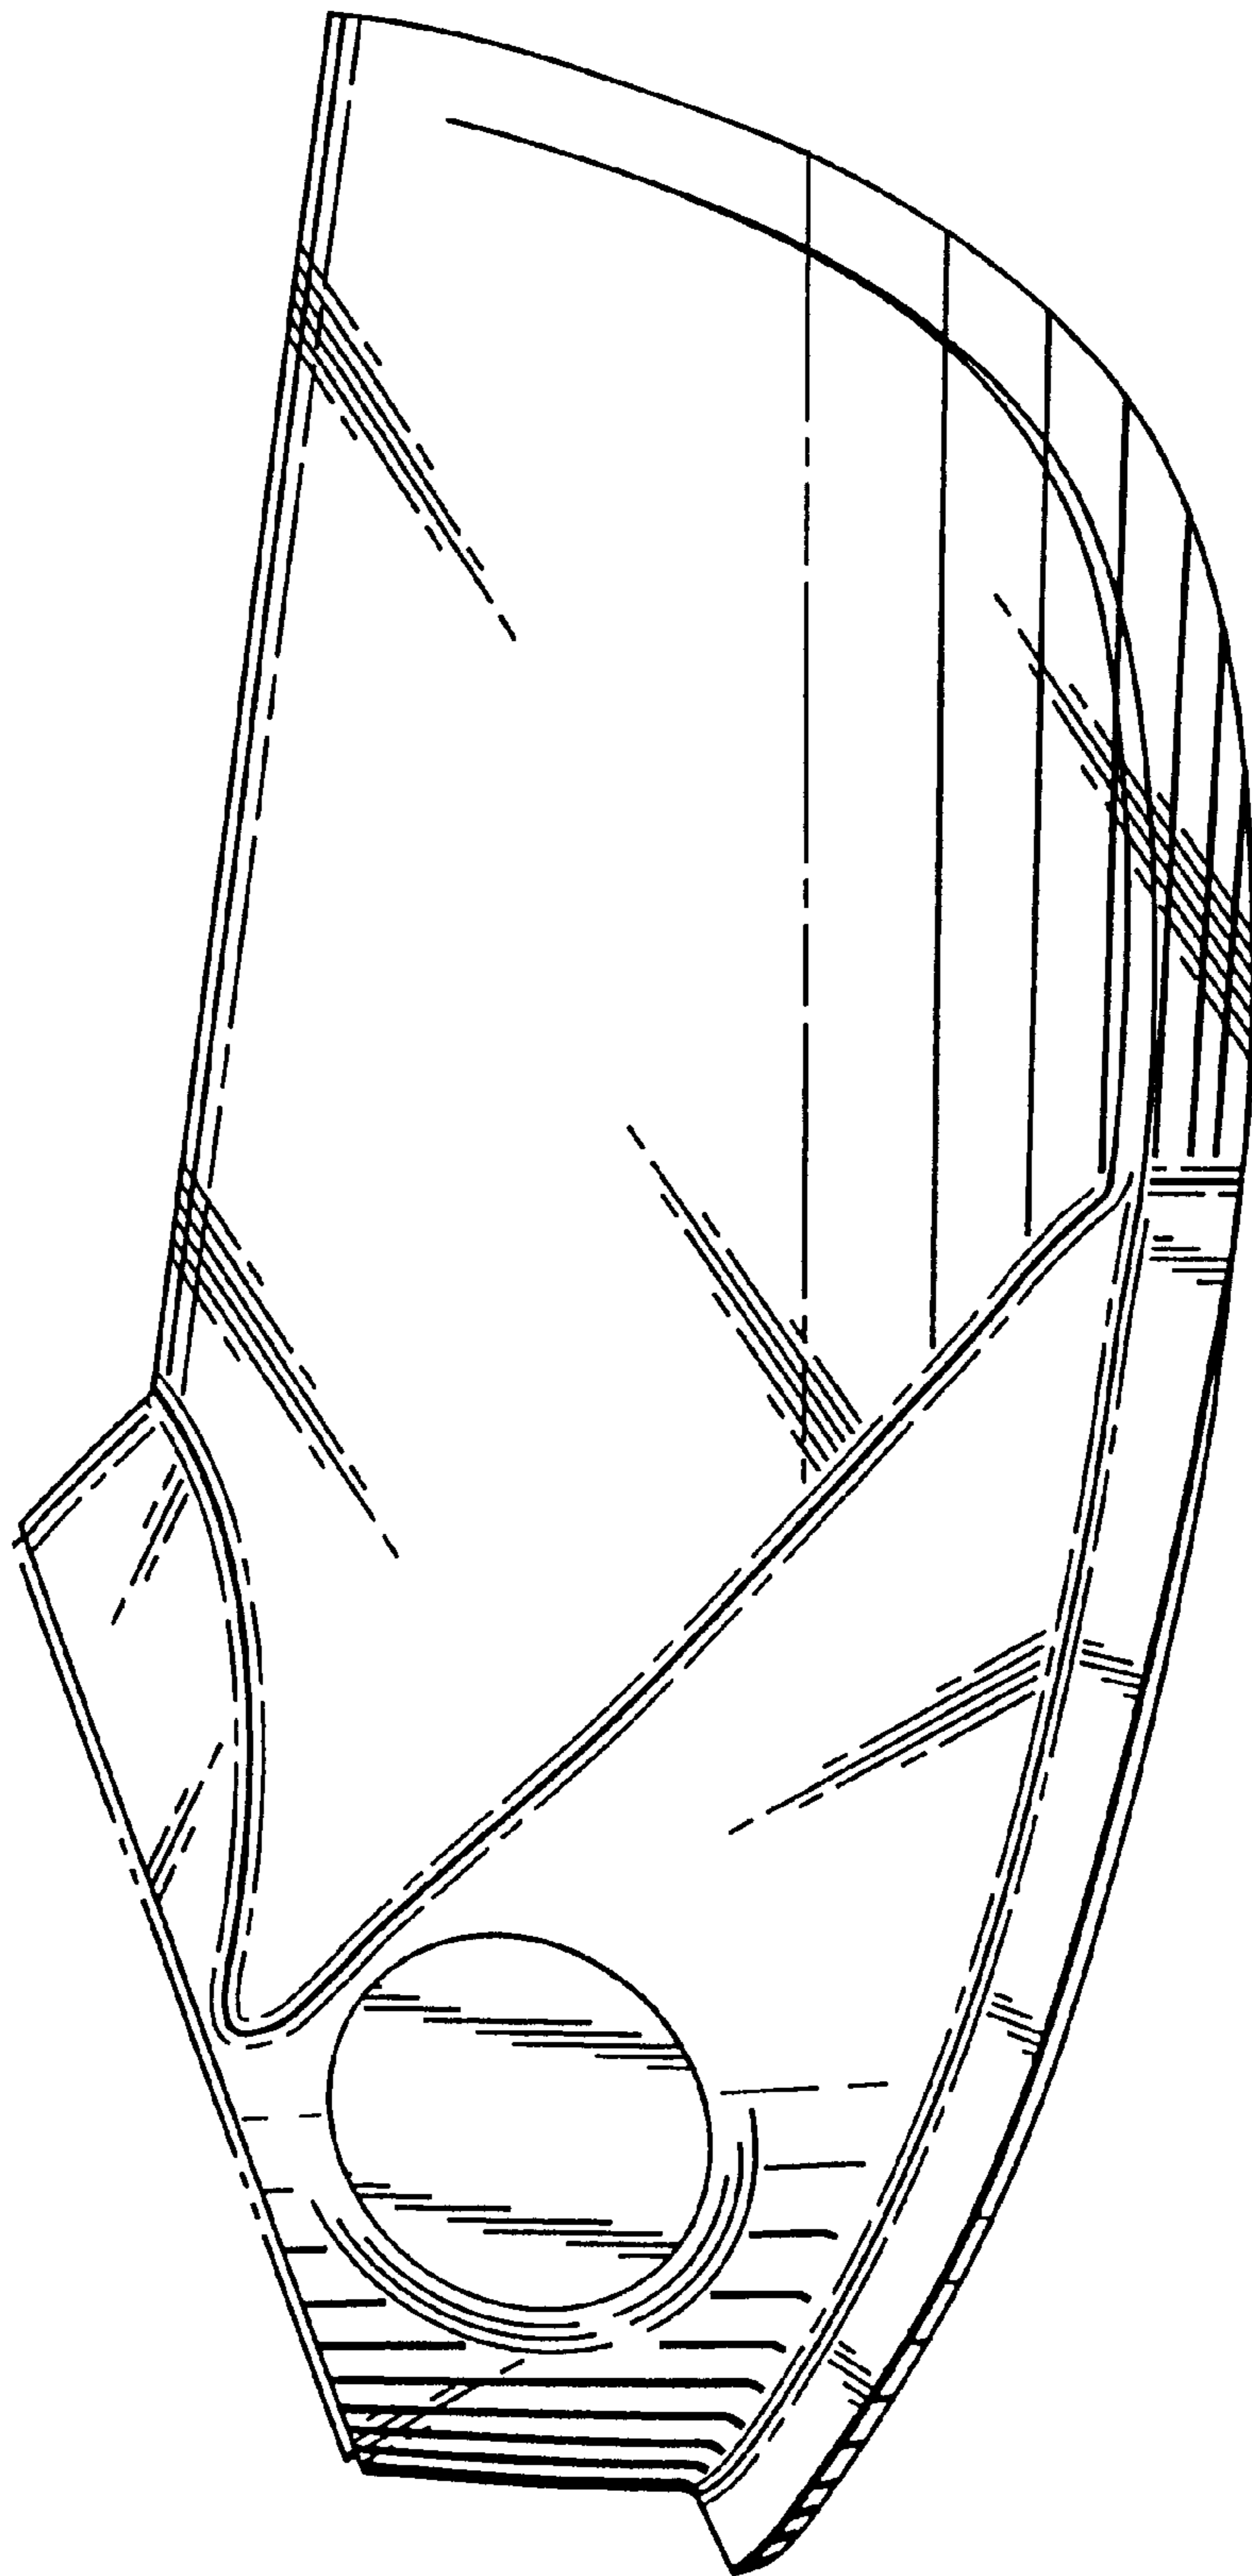


*Fig. 3*

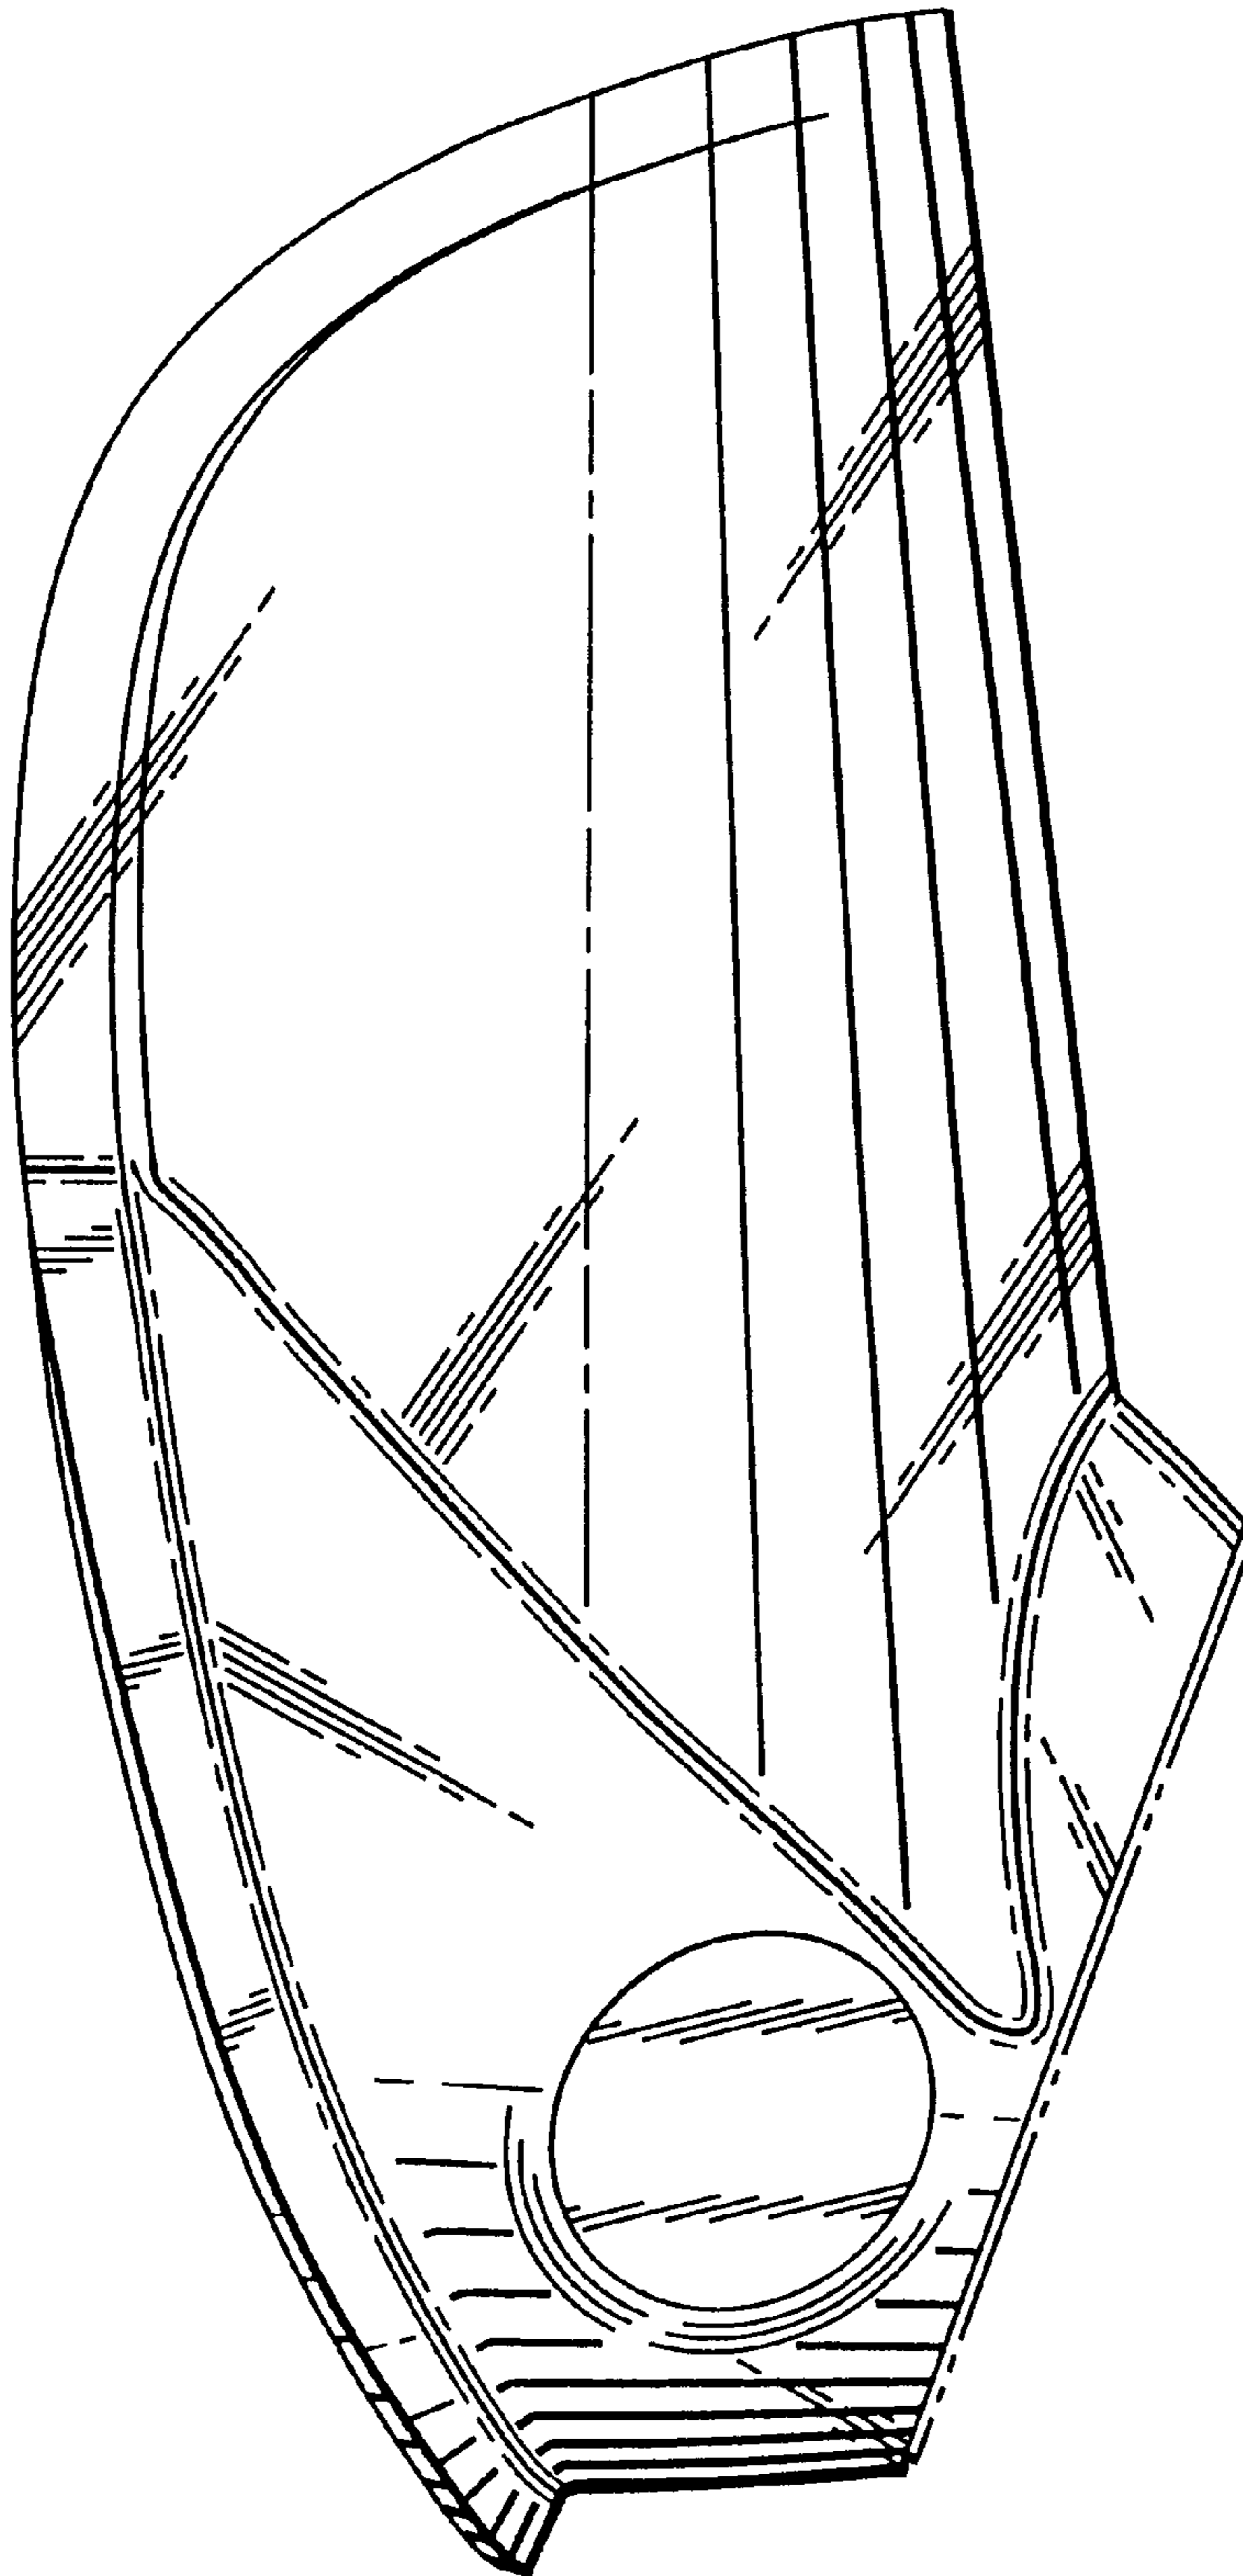


*Fig. 4*

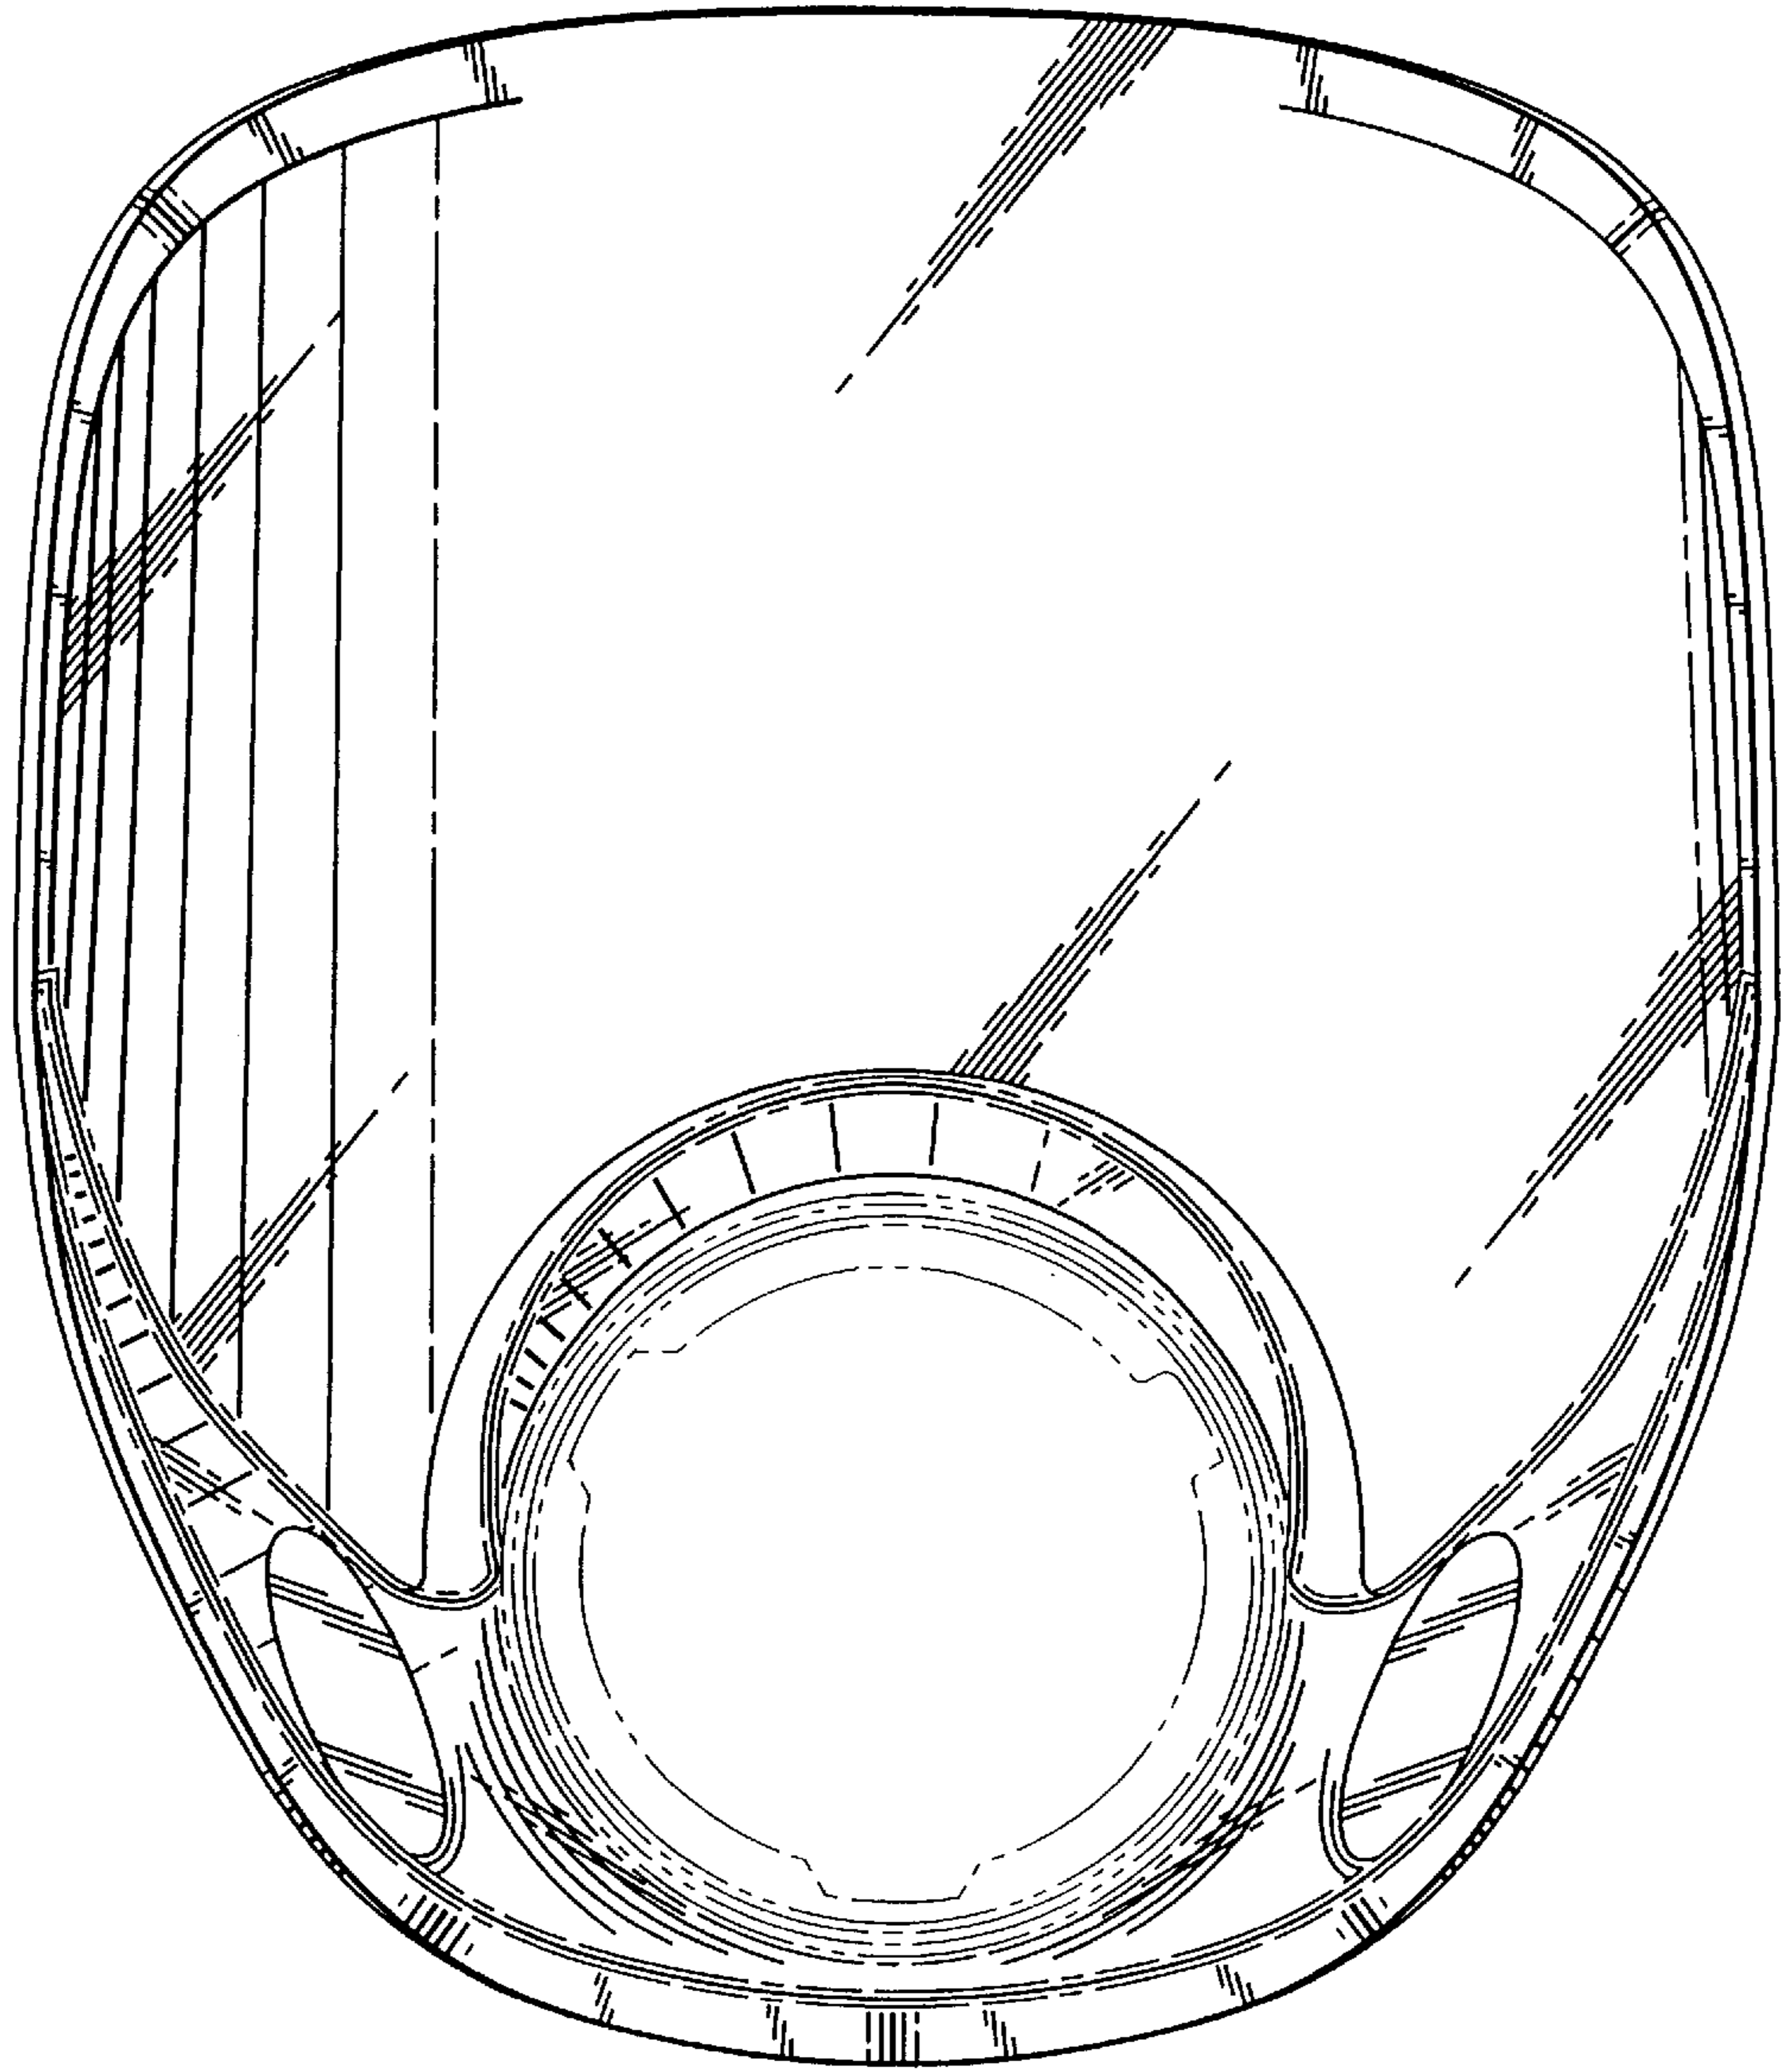

*Fig. 5*

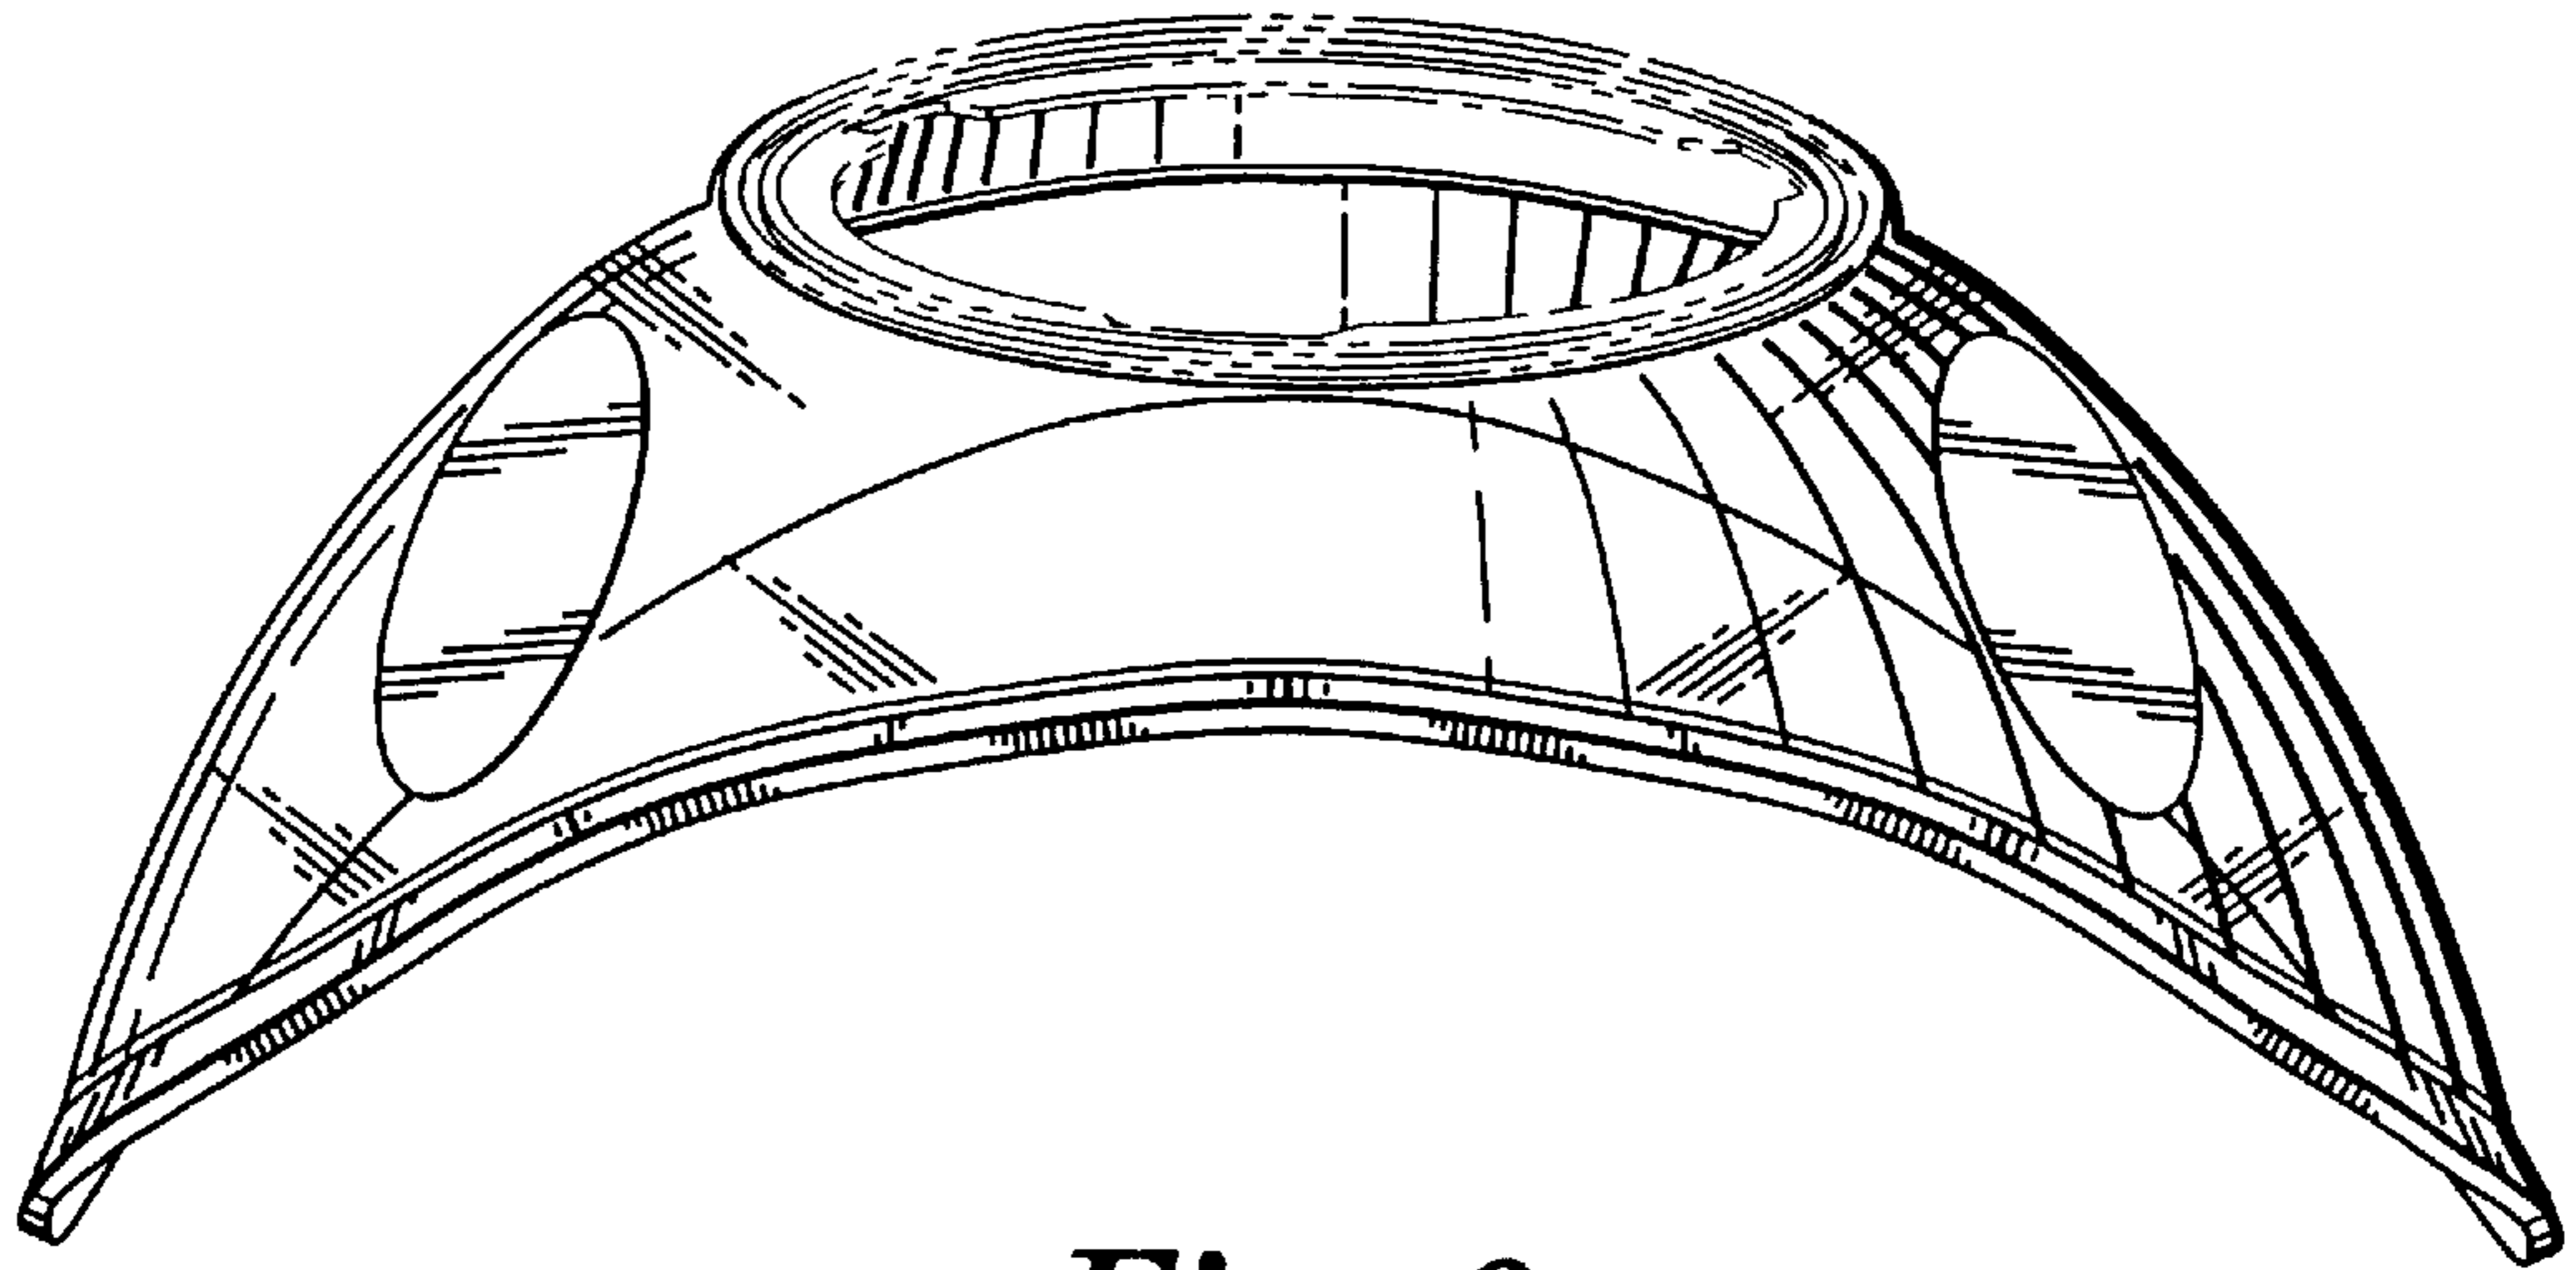

*Fig. 6*

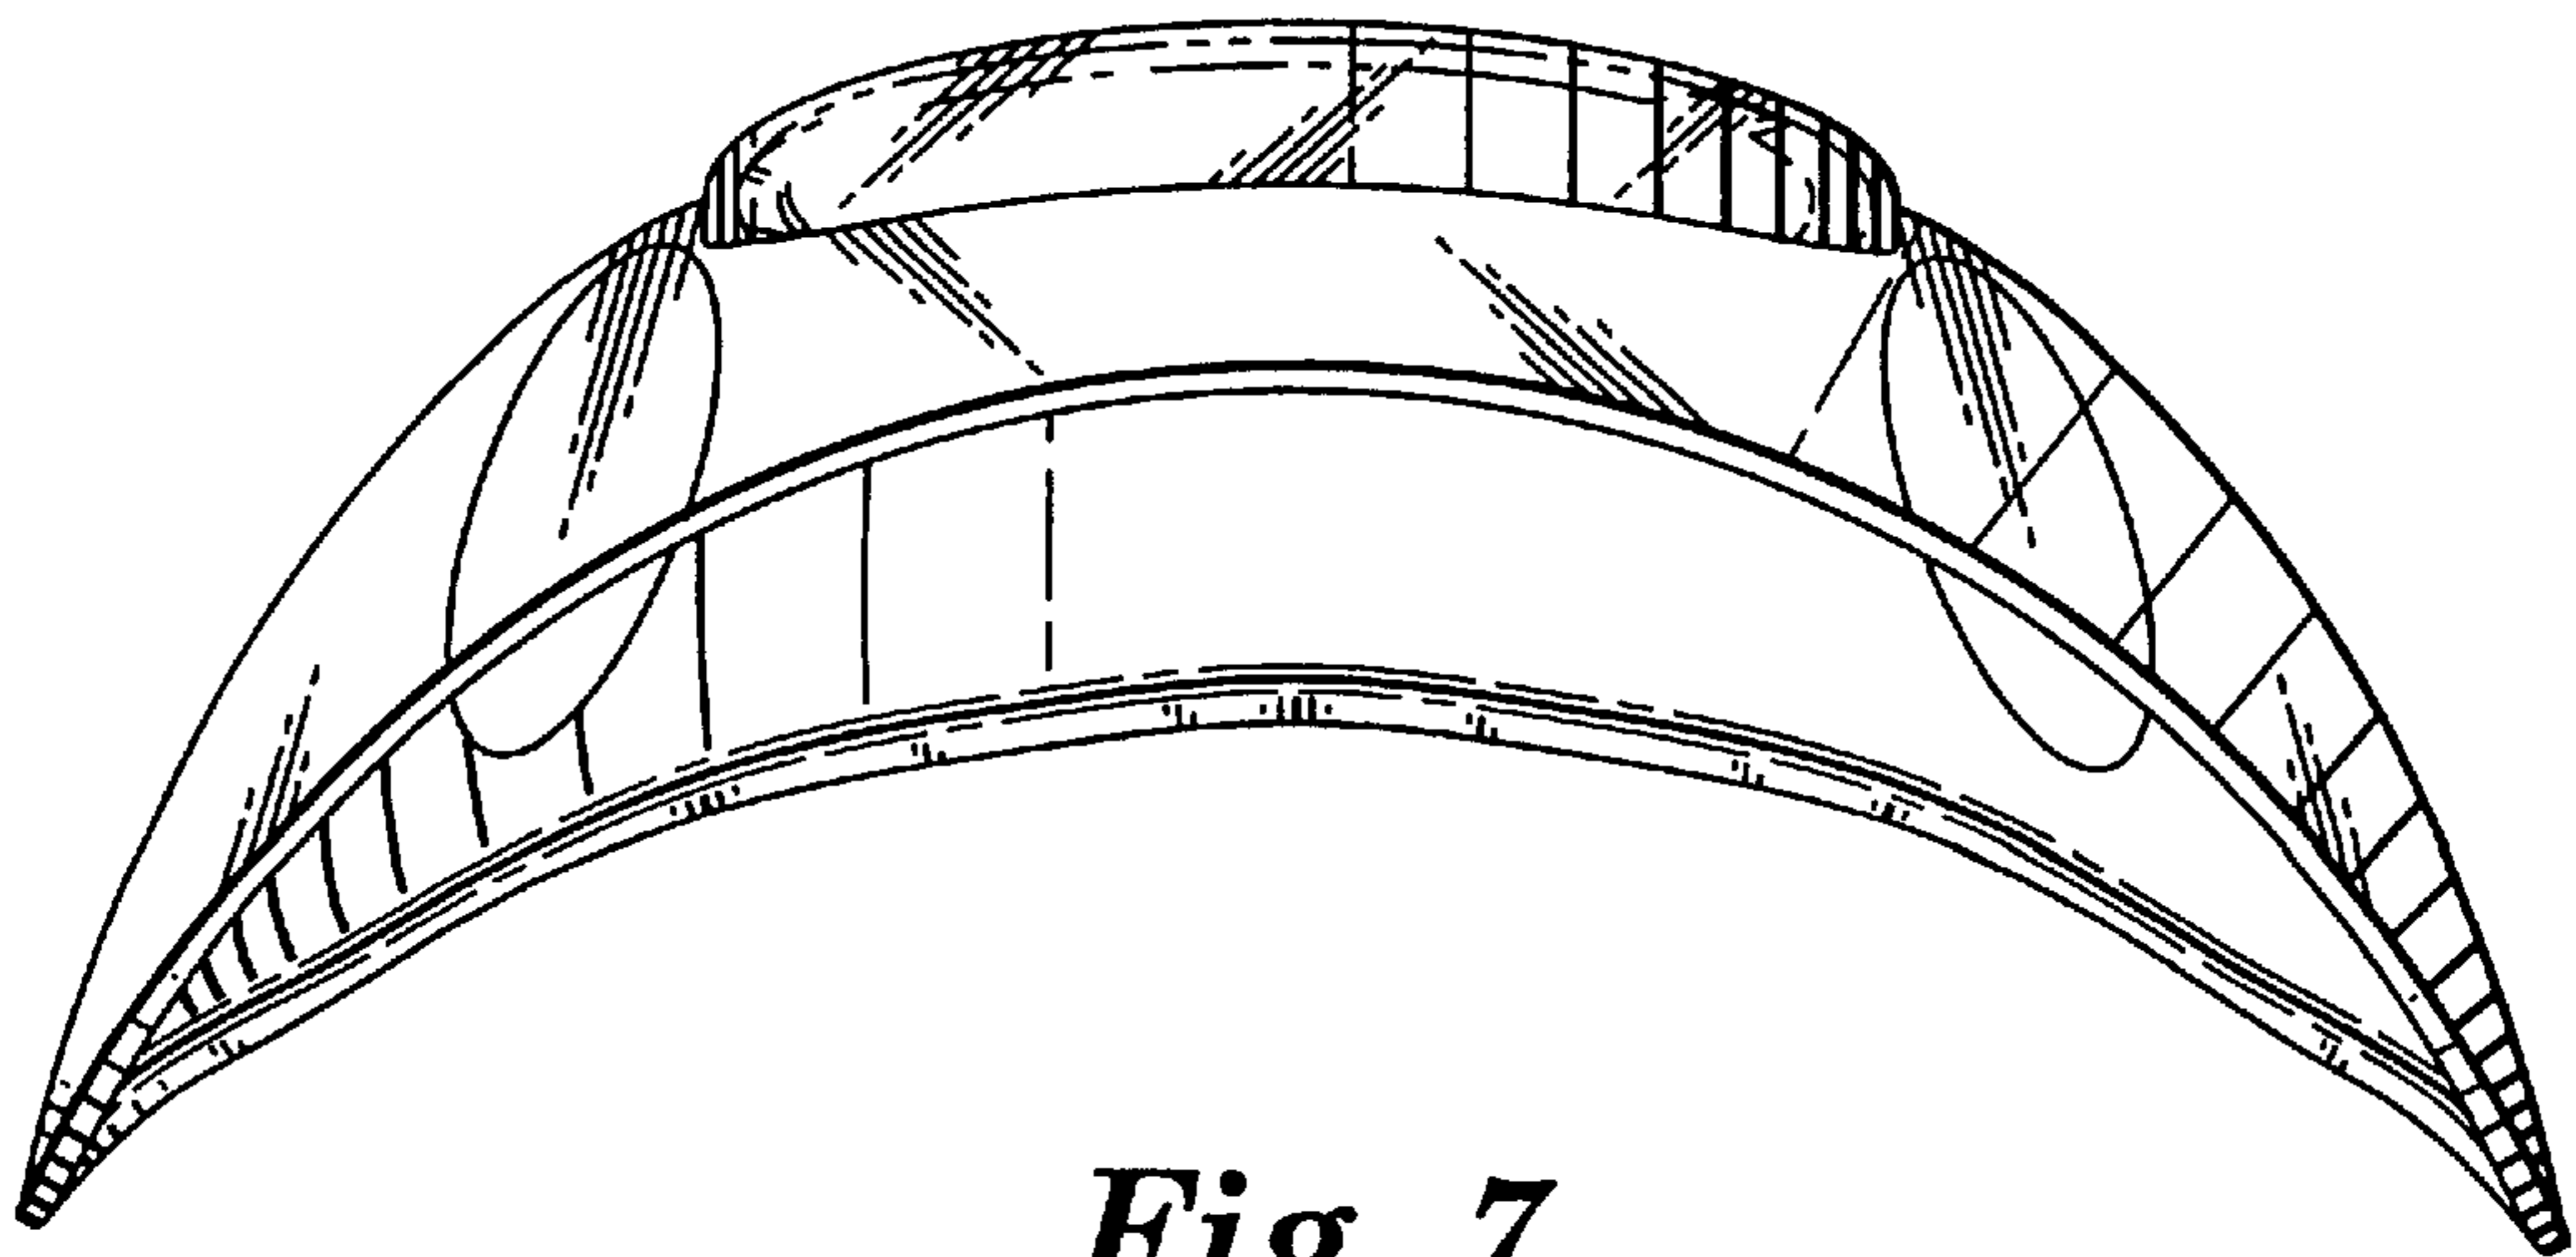

*Fig. 7*



UNITED STATES PATENT AND TRADEMARK OFFICE  
**CERTIFICATE OF CORRECTION**

PATENT NO.: Des. 426,298  
DATED: June 6, 2000  
INVENTOR(S): Grannis et al.

It is certified that error appears in the above-identified patent and that said Letters Patent is hereby corrected as shown below:

On the cover page, in the "Description", before the sentence beginning "The broken lines...", please insert --FIG. 7 is a top elevational view thereof.--

Signed and Sealed this  
Twenty-fourth Day of April, 2001

*Attest:*



NICHOLAS P. GODICI

*Attesting Officer*

*Acting Director of the United States Patent and Trademark Office*