



US00D427315S

United States Patent [19]

Saltzstein et al.

[11] Patent Number: Des. 427,315
[45] Date of Patent: ** Jun. 27, 2000

[54] VITAL SIGNS MONITORING UNIT

[75] Inventors: William E. Saltzstein, Woodinville, Wash.; Mohamed Sabri, Beaverton; Scott M. Burkhart, Hillsboro, both of Oreg.; Gregory T. Semler, Menlo Park, Calif.

[73] Assignee: Instromedix, Inc., Hillsboro, Oreg.

[**] Term: 14 Years

[21] Appl. No.: 29/081,456

[22] Filed: Jan. 2, 1998

[51] LOC (7) Cl. 24-01

[52] U.S. Cl. D24/186

[58] Field of Search D24/186; 600/345, 600/391, 393, 481, 484, 519, 513, 528, 532, 536, 538, 549, 586, 483, 485

[56] References Cited

U.S. PATENT DOCUMENTS

D. 238,905	2/1976	Sokol	D24/186
D. 264,128	4/1982	Barnes et al.	D24/186
D. 323,894	2/1992	Rosati et al.	D24/186
D. 392,043	3/1998	Cooper et al.	D24/186
3,886,314	5/1975	Pori .	
3,938,507	2/1976	Sarnoff et al. .	
3,971,980	7/1976	Jungfer et al. .	
3,972,320	8/1976	Kalman .	
4,108,166	8/1978	Schmid .	
4,120,294	10/1978	Wolfe .	
4,129,125	12/1978	Lester et al. .	
4,173,971	11/1979	Karz .	
4,216,462	8/1980	McGrath et al. .	
4,230,127	10/1980	Larson .	
4,256,117	3/1981	Perica et al. .	
4,347,851	9/1982	Jundanian	600/485
4,409,983	10/1983	Albert .	
4,425,921	1/1984	Fujisaki et al. .	
4,450,843	5/1984	Barney et al. .	

(List continued on next page.)

FOREIGN PATENT DOCUMENTS

0122888A2	10/1984	European Pat. Off. .
0645710A2	7/1994	European Pat. Off. .
0656718A2	6/1995	European Pat. Off. .

0645710A3	11/1995	European Pat. Off. .
81 19650	4/1983	France .
2845-679	4/1980	Germany .
27 53 165	6/1980	Germany .

OTHER PUBLICATIONS

James E. McKee, Noel E. Evans and Frank J. Owens, *A Simultaneous Full-Duplex Speech and Electrocardiogram Communications System*, Proceedings of the Annual International Conference of the IEEE Engineering in Medicine and Biology Society, Baltimore, Nov. 3-6, 1994, vol. 16, pp. 902-903.

William Stallings, *Data and Computer Communications*, 2d. Ed., pp. 103-113, MacMillan Publishing Co., 1988.

Bernard L. Segal et al., Telephone Phonocardiograph, *The American Journal of Medical Electronics*, pp. 189-191, Jul.-Sep., 1964.

Fisher, Anne B., *House Calls*, Inc., pp. 72-79, Jul. 1989.

Comparison of Duplex and Triplex Memory Reliability, pp. 503-507, IEEE Transactions on Computers, vol. 45. No. 4., Apr. 1996.

Symposium on the Engineering of Computer-Based Medical Systems, pp. 22-27, Jun. 8-10, 1998.

Kathy Brock, Inventors of Heart Monitor Tick Toward Prosperity, *The Business Journal*, p. 15, Sep. 17, 1990.

English language abstract of published European Patent Application No. 645,710A2, Derwent Info. Ltd., ©1998.

Primary Examiner—Stella Reid

Attorney, Agent, or Firm—Klarquist Sparkman Campbell Leigh & Whinston, LLP

[57] CLAIM

The ornamental design for a vital signs monitoring unit, as shown and described.

DESCRIPTION

FIG. 1 is an isometric view of a vital signs monitoring unit in accordance with the present invention;

FIG. 2 is a front view thereof;


FIG. 3 is a rear view thereof;

FIG. 4 is a right side thereof;

FIG. 5 is a left side view thereof; and,


FIG. 6 is a top view thereof.



1 Claim, 5 Drawing Sheets

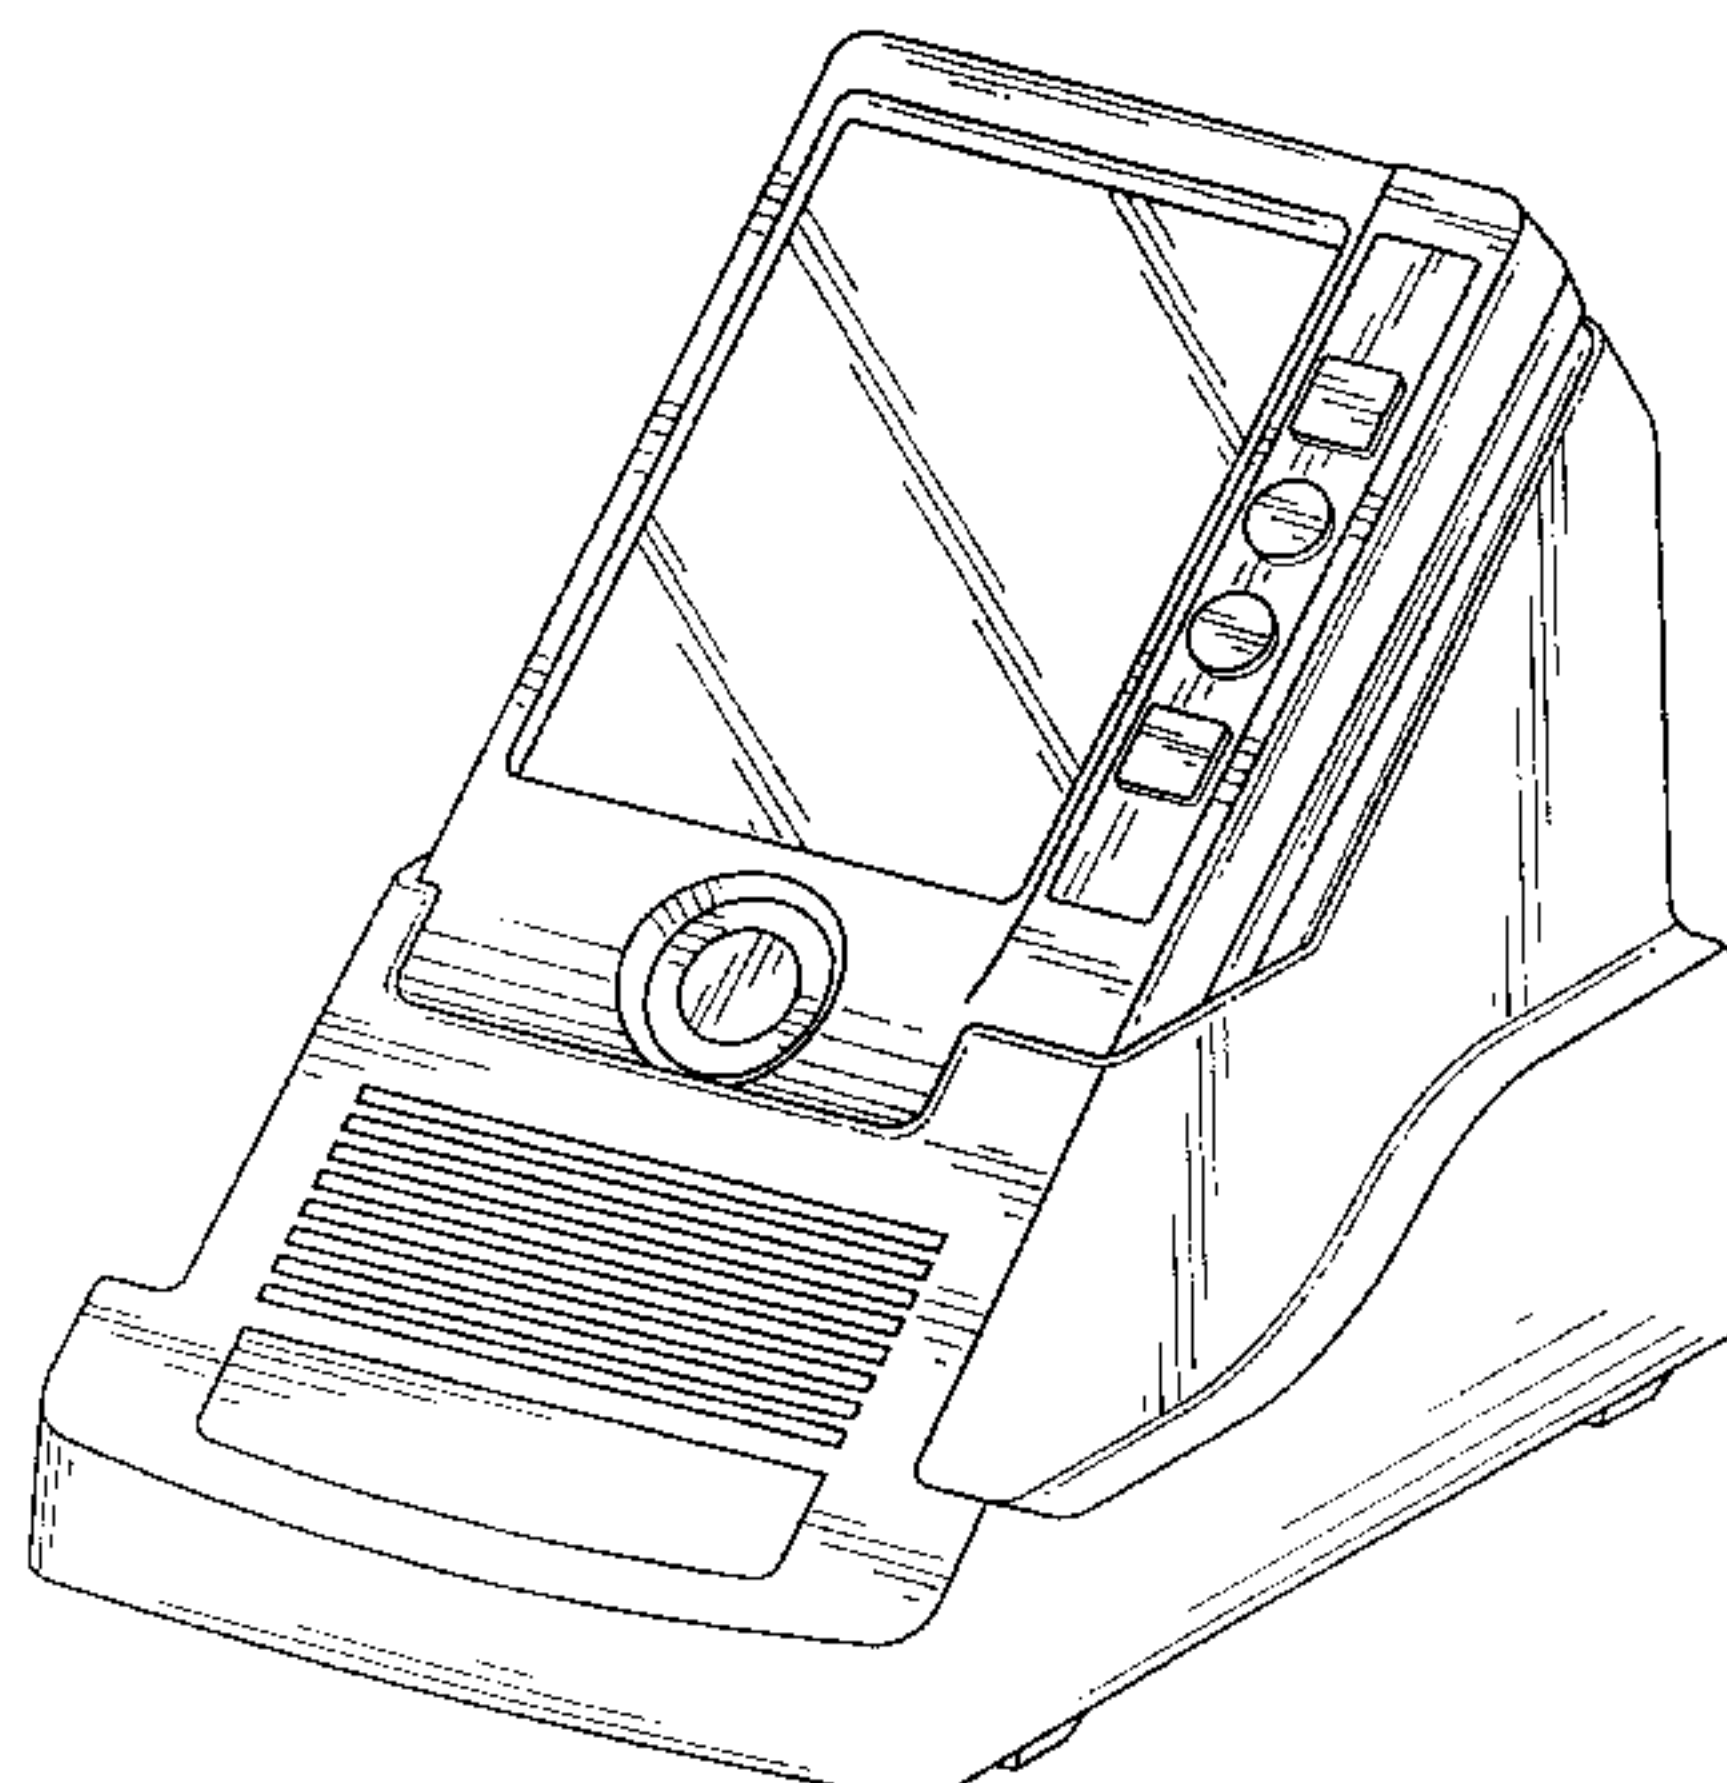

U.S. PATENT DOCUMENTS					
4,494,553	1/1985	Sciarra et al. .	5,024,225	6/1991	Fang .
4,531,527	7/1985	Reinhold, Jr. et al. .	5,025,794	6/1991	Albert et al. .
4,602,637	7/1986	Elmqvist et al. .	5,033,474	7/1991	Varelis et al. .
4,603,704	8/1986	Mund et al. .	5,036,513	7/1991	Greenblatt .
4,611,604	9/1986	Botvidsson et al. .	5,038,800	8/1991	Oba .
4,679,000	7/1987	Clark .	5,128,552	7/1992	Fang et al. .
4,715,381	12/1987	Moberg .	5,142,484	8/1992	Kaufman et al. .
4,724,844	2/1988	Rafelson 600/483	5,154,183	10/1992	Kreyenhagen et al. .
4,763,663	8/1988	Uphold et al. 600/484	5,185,861	2/1993	Valencia .
4,784,162	11/1988	Ricks et al. .	5,191,891	3/1993	Righter .
4,791,933	12/1988	Asai et al. .	5,216,596	6/1993	Weinstein .
4,799,491	1/1989	Eckerle .	5,226,431	7/1993	Bible et al. .
4,802,488	2/1989	Eckerle .	5,317,269	5/1994	Mills et al. .
4,803,625	2/1989	Fu et al. .	5,321,618	6/1994	Gessman .
4,838,275	6/1989	Lee .	5,333,616	8/1994	Mills et al. .
4,883,064	11/1989	Olson et al. .	5,339,823	8/1994	Reinhold, Jr. .
4,928,690	5/1990	Heilman et al. .	5,343,869	9/1994	Pross et al. .
4,933,873	6/1990	Kaufman et al. .	5,351,695	10/1994	Mills et al. .
4,938,228	7/1990	Righter et al. .	5,357,427	10/1994	Langen et al. .
4,945,477	7/1990	Edwards .	5,365,935	11/1994	Righter et al. .
4,949,046	8/1990	Seyfana .	5,381,798	1/1995	Burrows .
4,952,862	8/1990	Biagetti et al. .	5,390,238	2/1995	Kirk et al. .
4,958,641	9/1990	Digby et al. .	5,394,882	3/1995	Mawhinney .
4,967,756	11/1990	Hewitt .	5,462,051	10/1995	Oka et al. .
4,974,607	12/1990	Miwa .	5,467,773	11/1995	Bergelson et al. .
4,979,235	12/1990	Rumbaugh et al. .	5,474,090	12/1995	Begun et al. .
4,981,139	1/1991	Pfohl 600/528 X	5,544,661	8/1996	Davis et al. .
5,001,484	3/1991	Weiss .	5,553,609	9/1996	Chen et al. .
5,007,429	4/1991	Treatch et al. .	5,557,800	9/1996	Kasimov et al. .
5,010,890	4/1991	Pfohl 600/528	5,607,454	3/1997	Cameron et al. .
5,012,814	5/1991	Mills et al. .	5,613,495	3/1997	Mills et al. .
			5,704,364	1/1998	Saltzstein et al. .

FIG.1

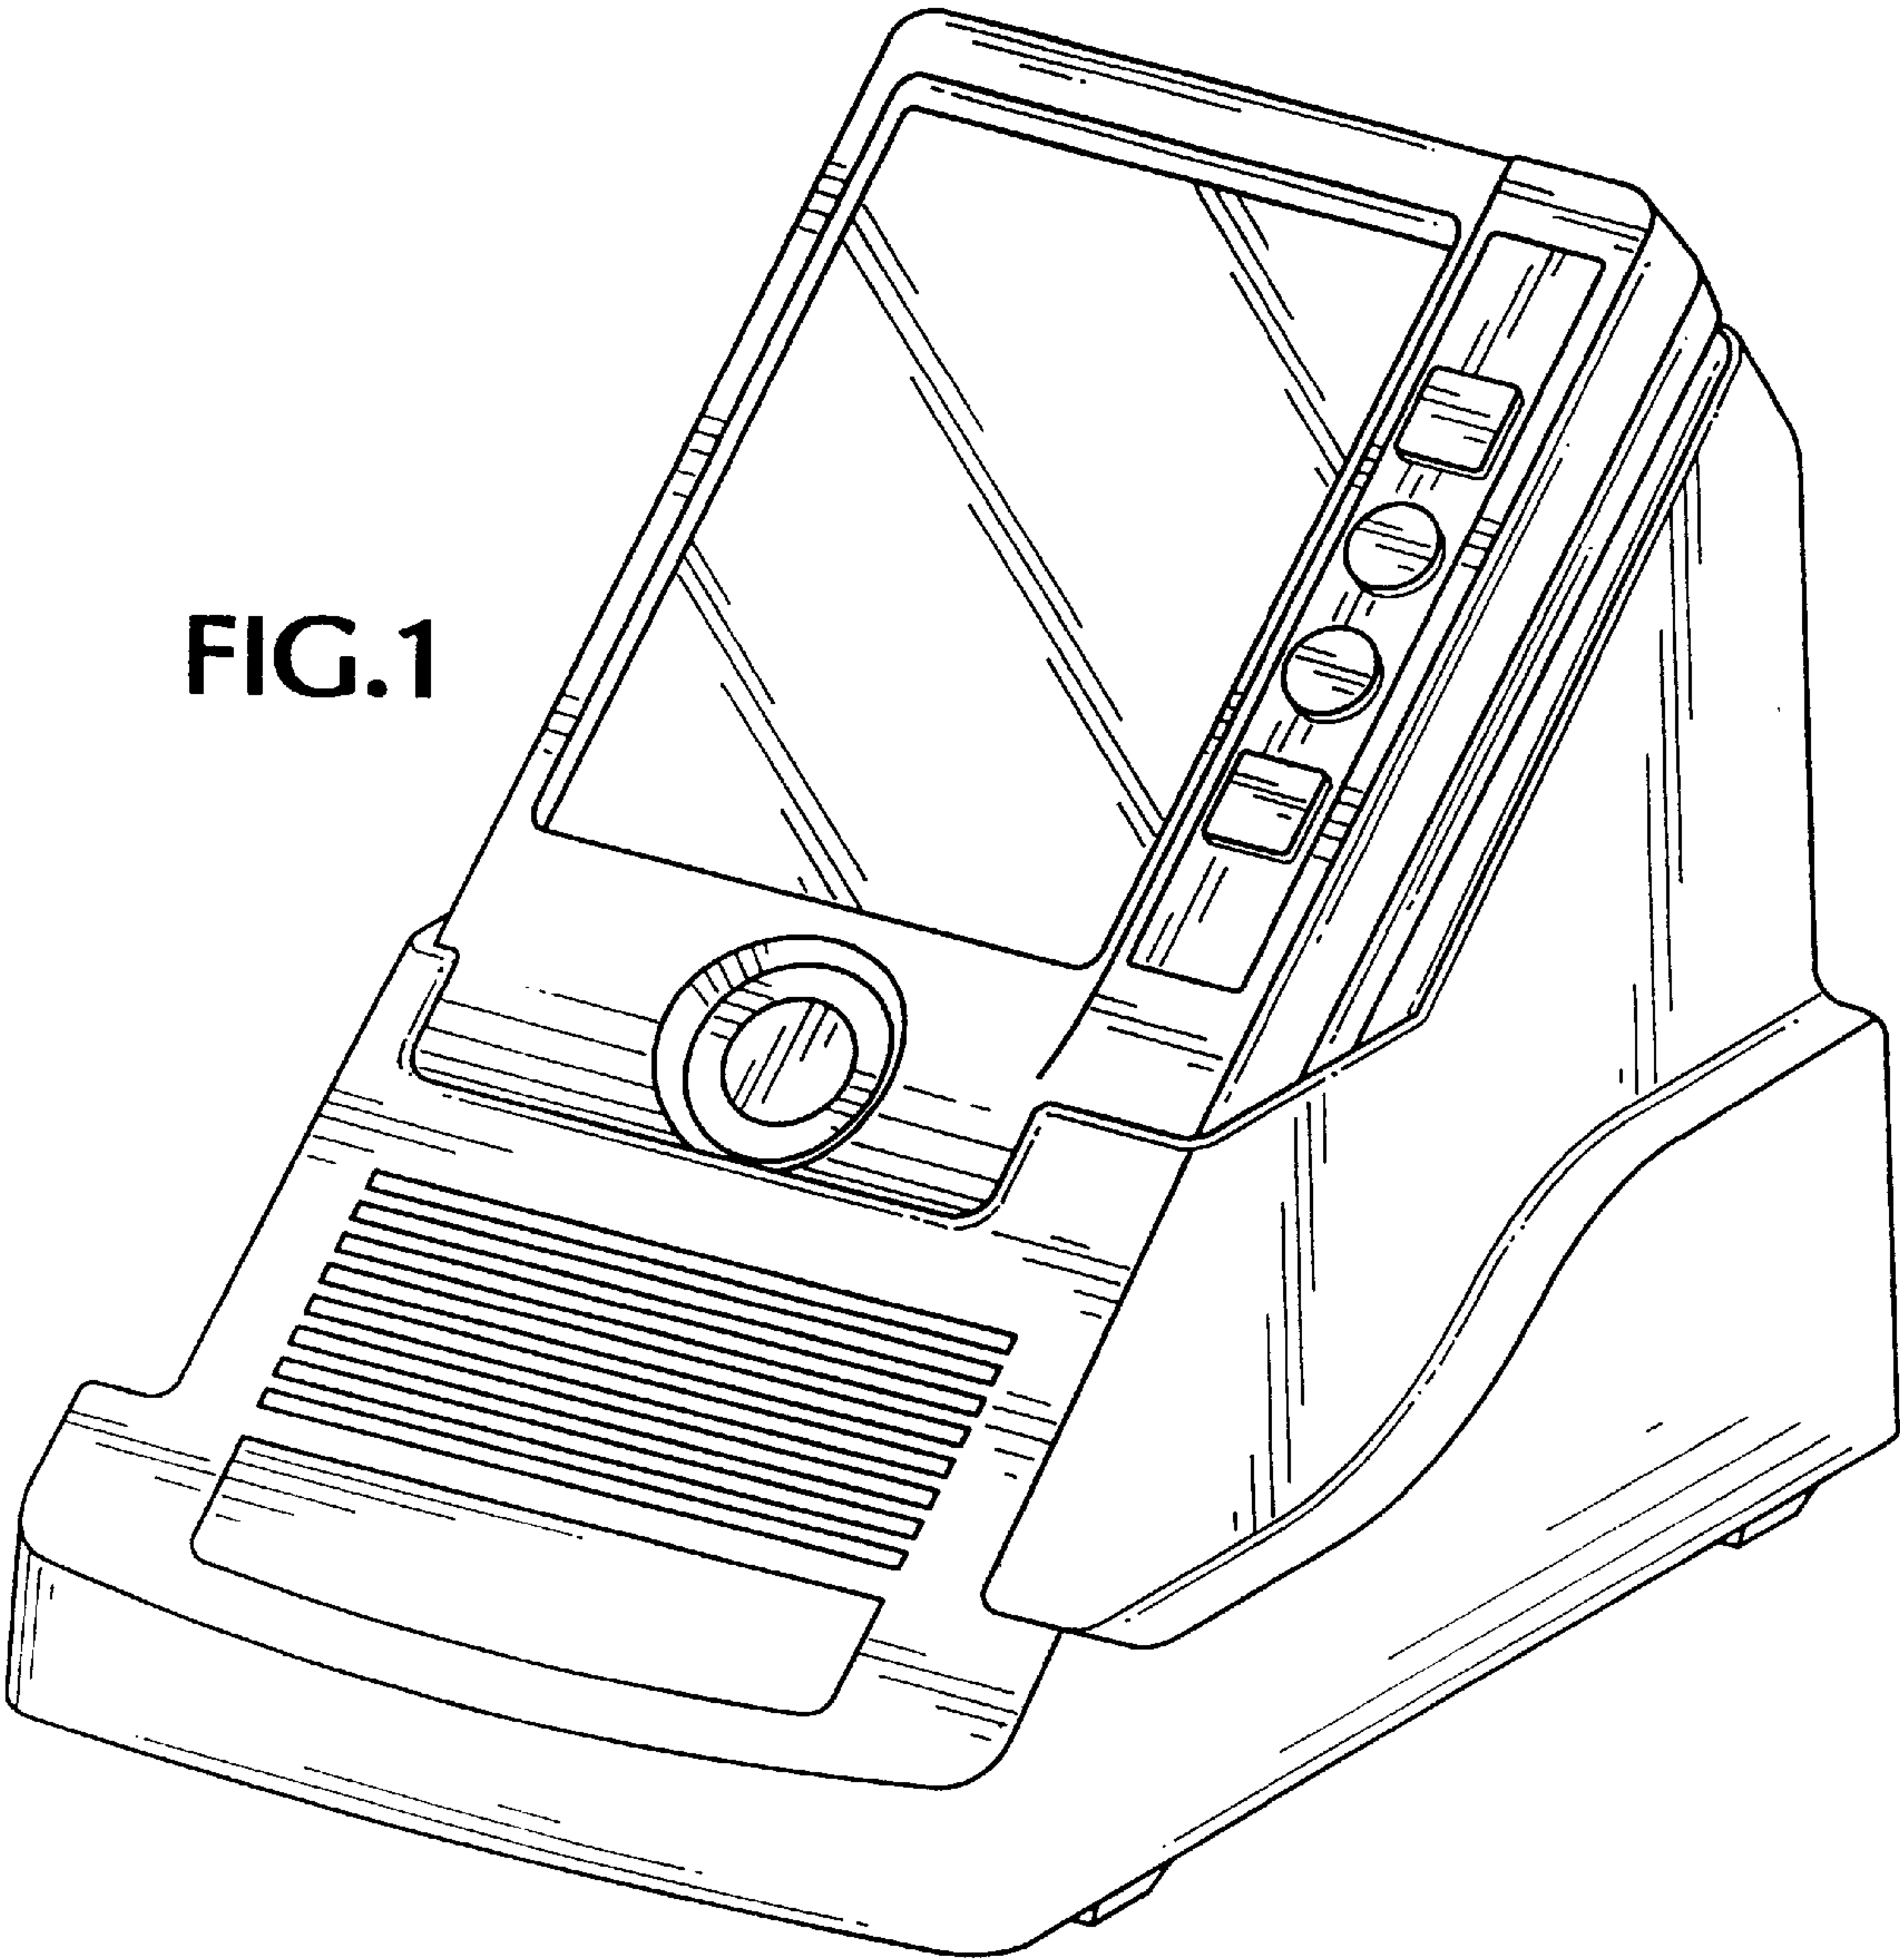

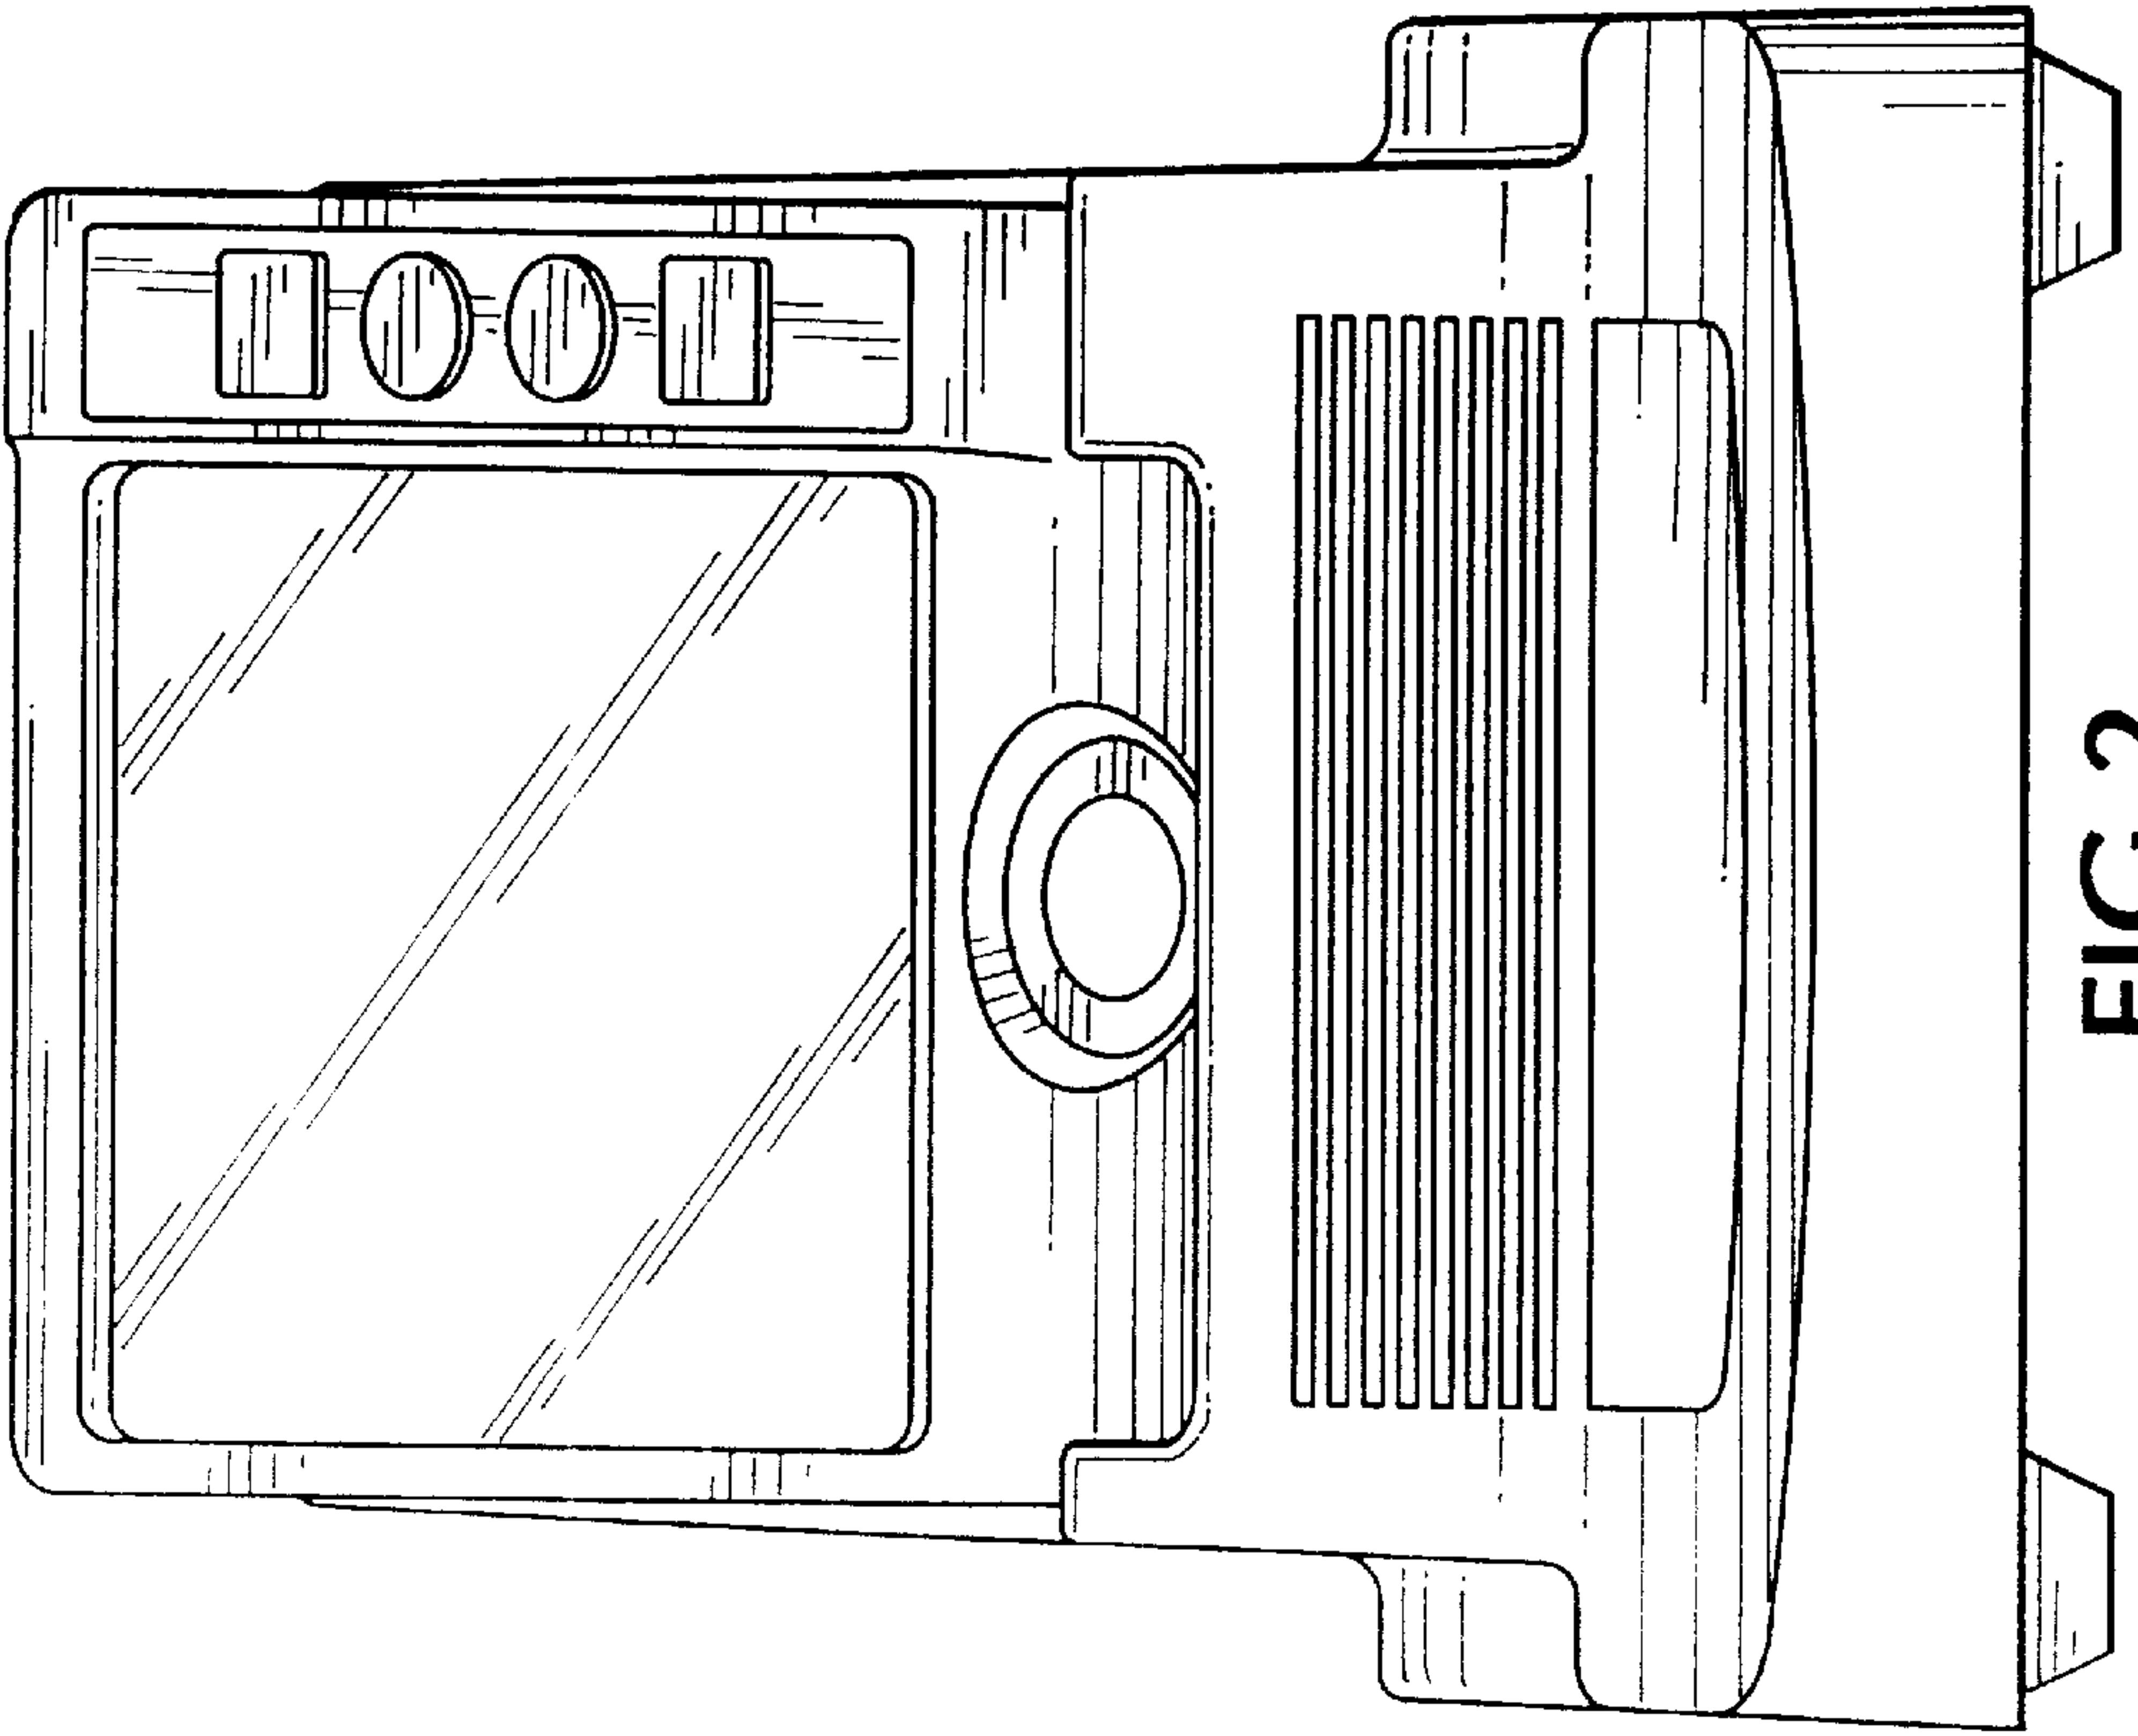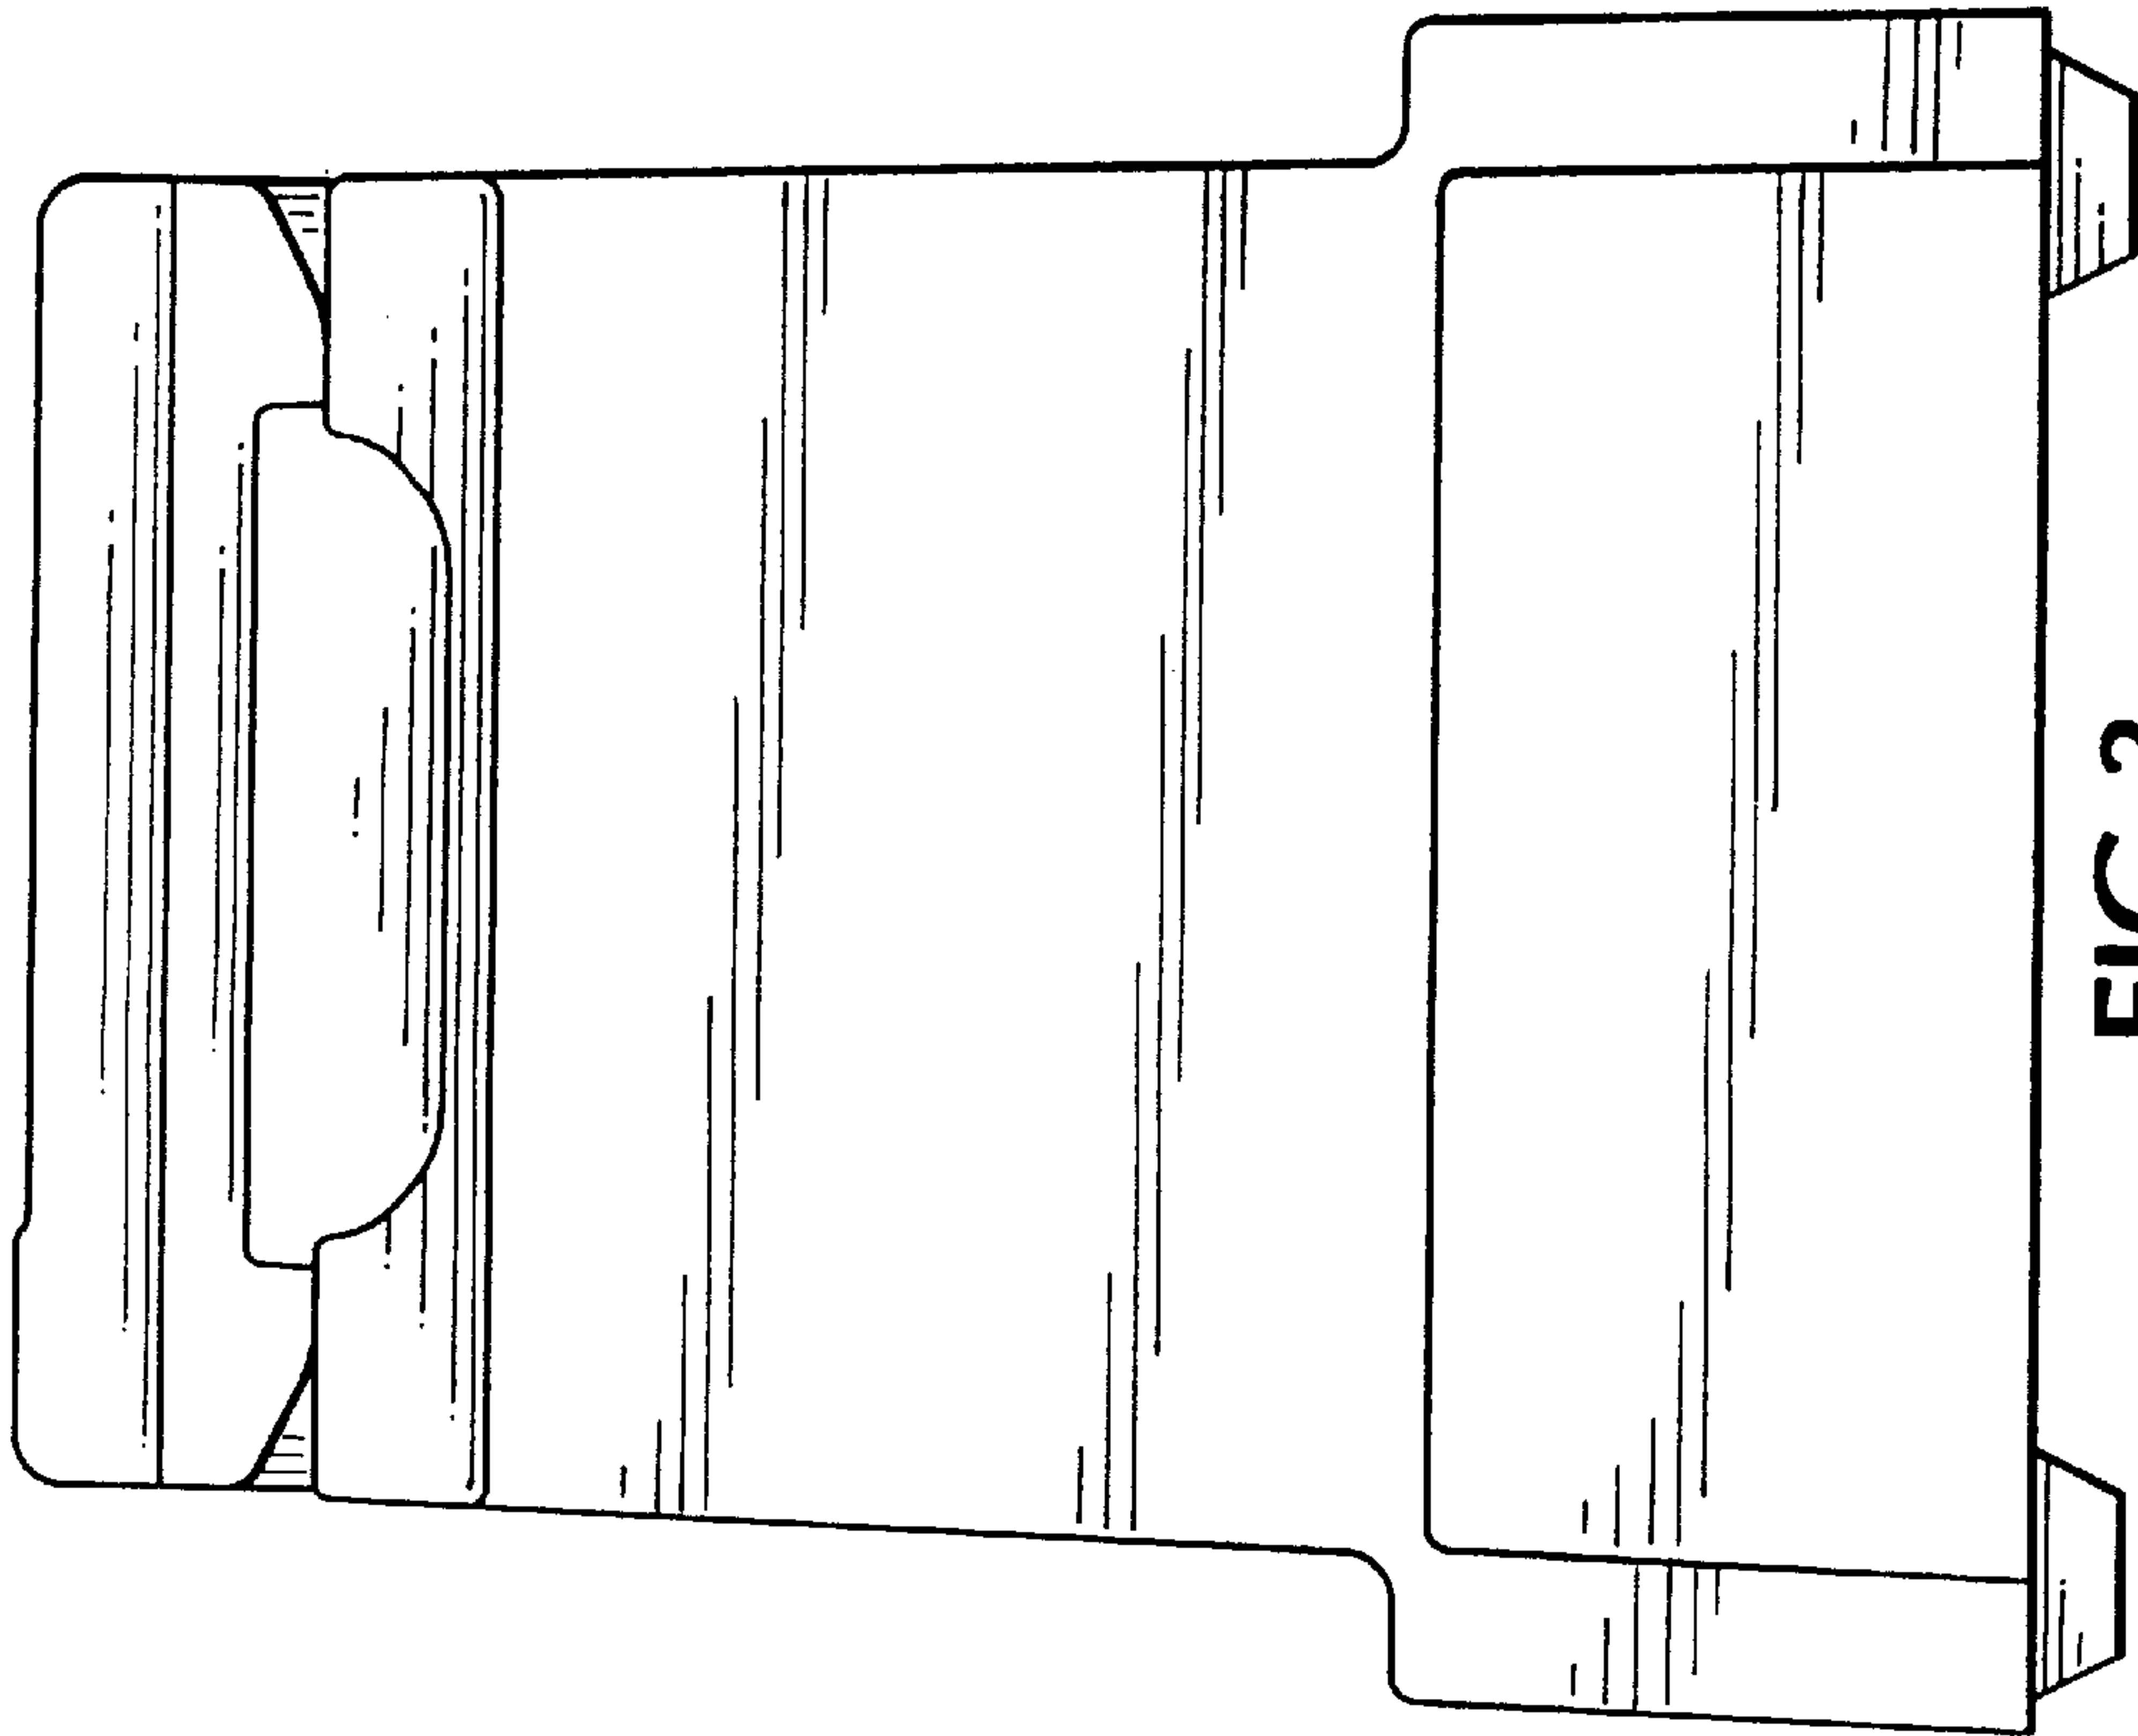

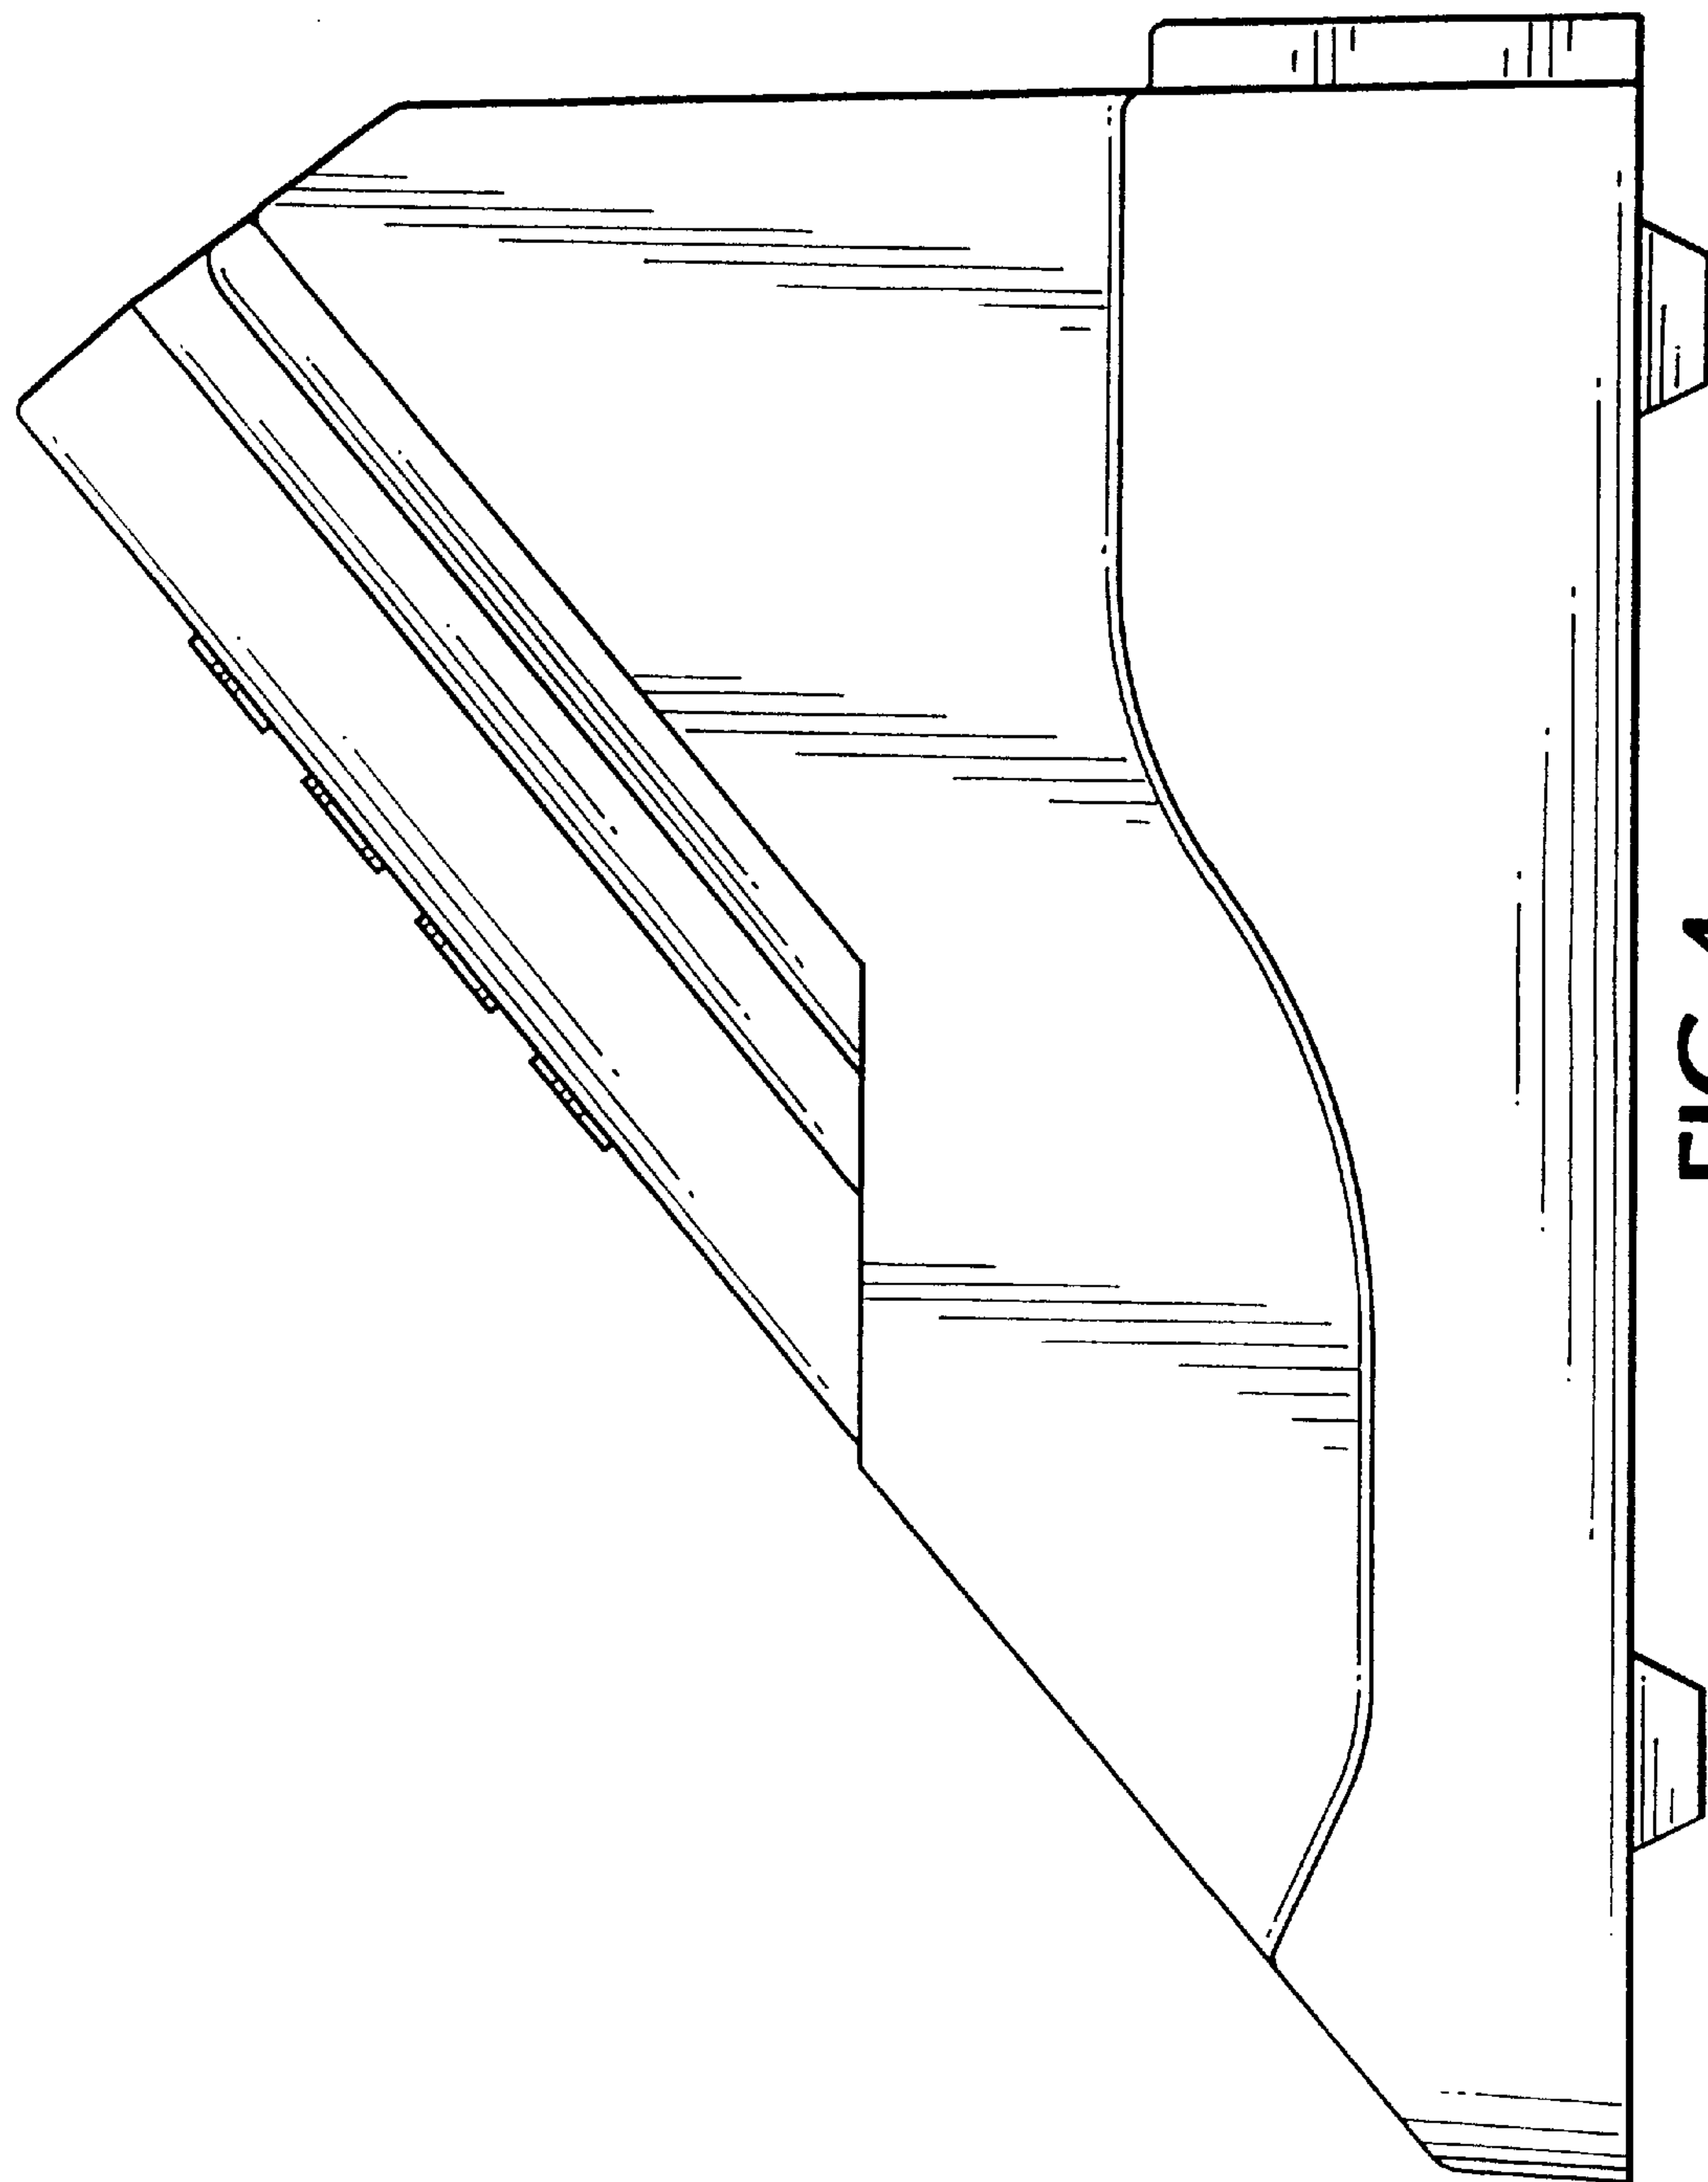


FIG.4

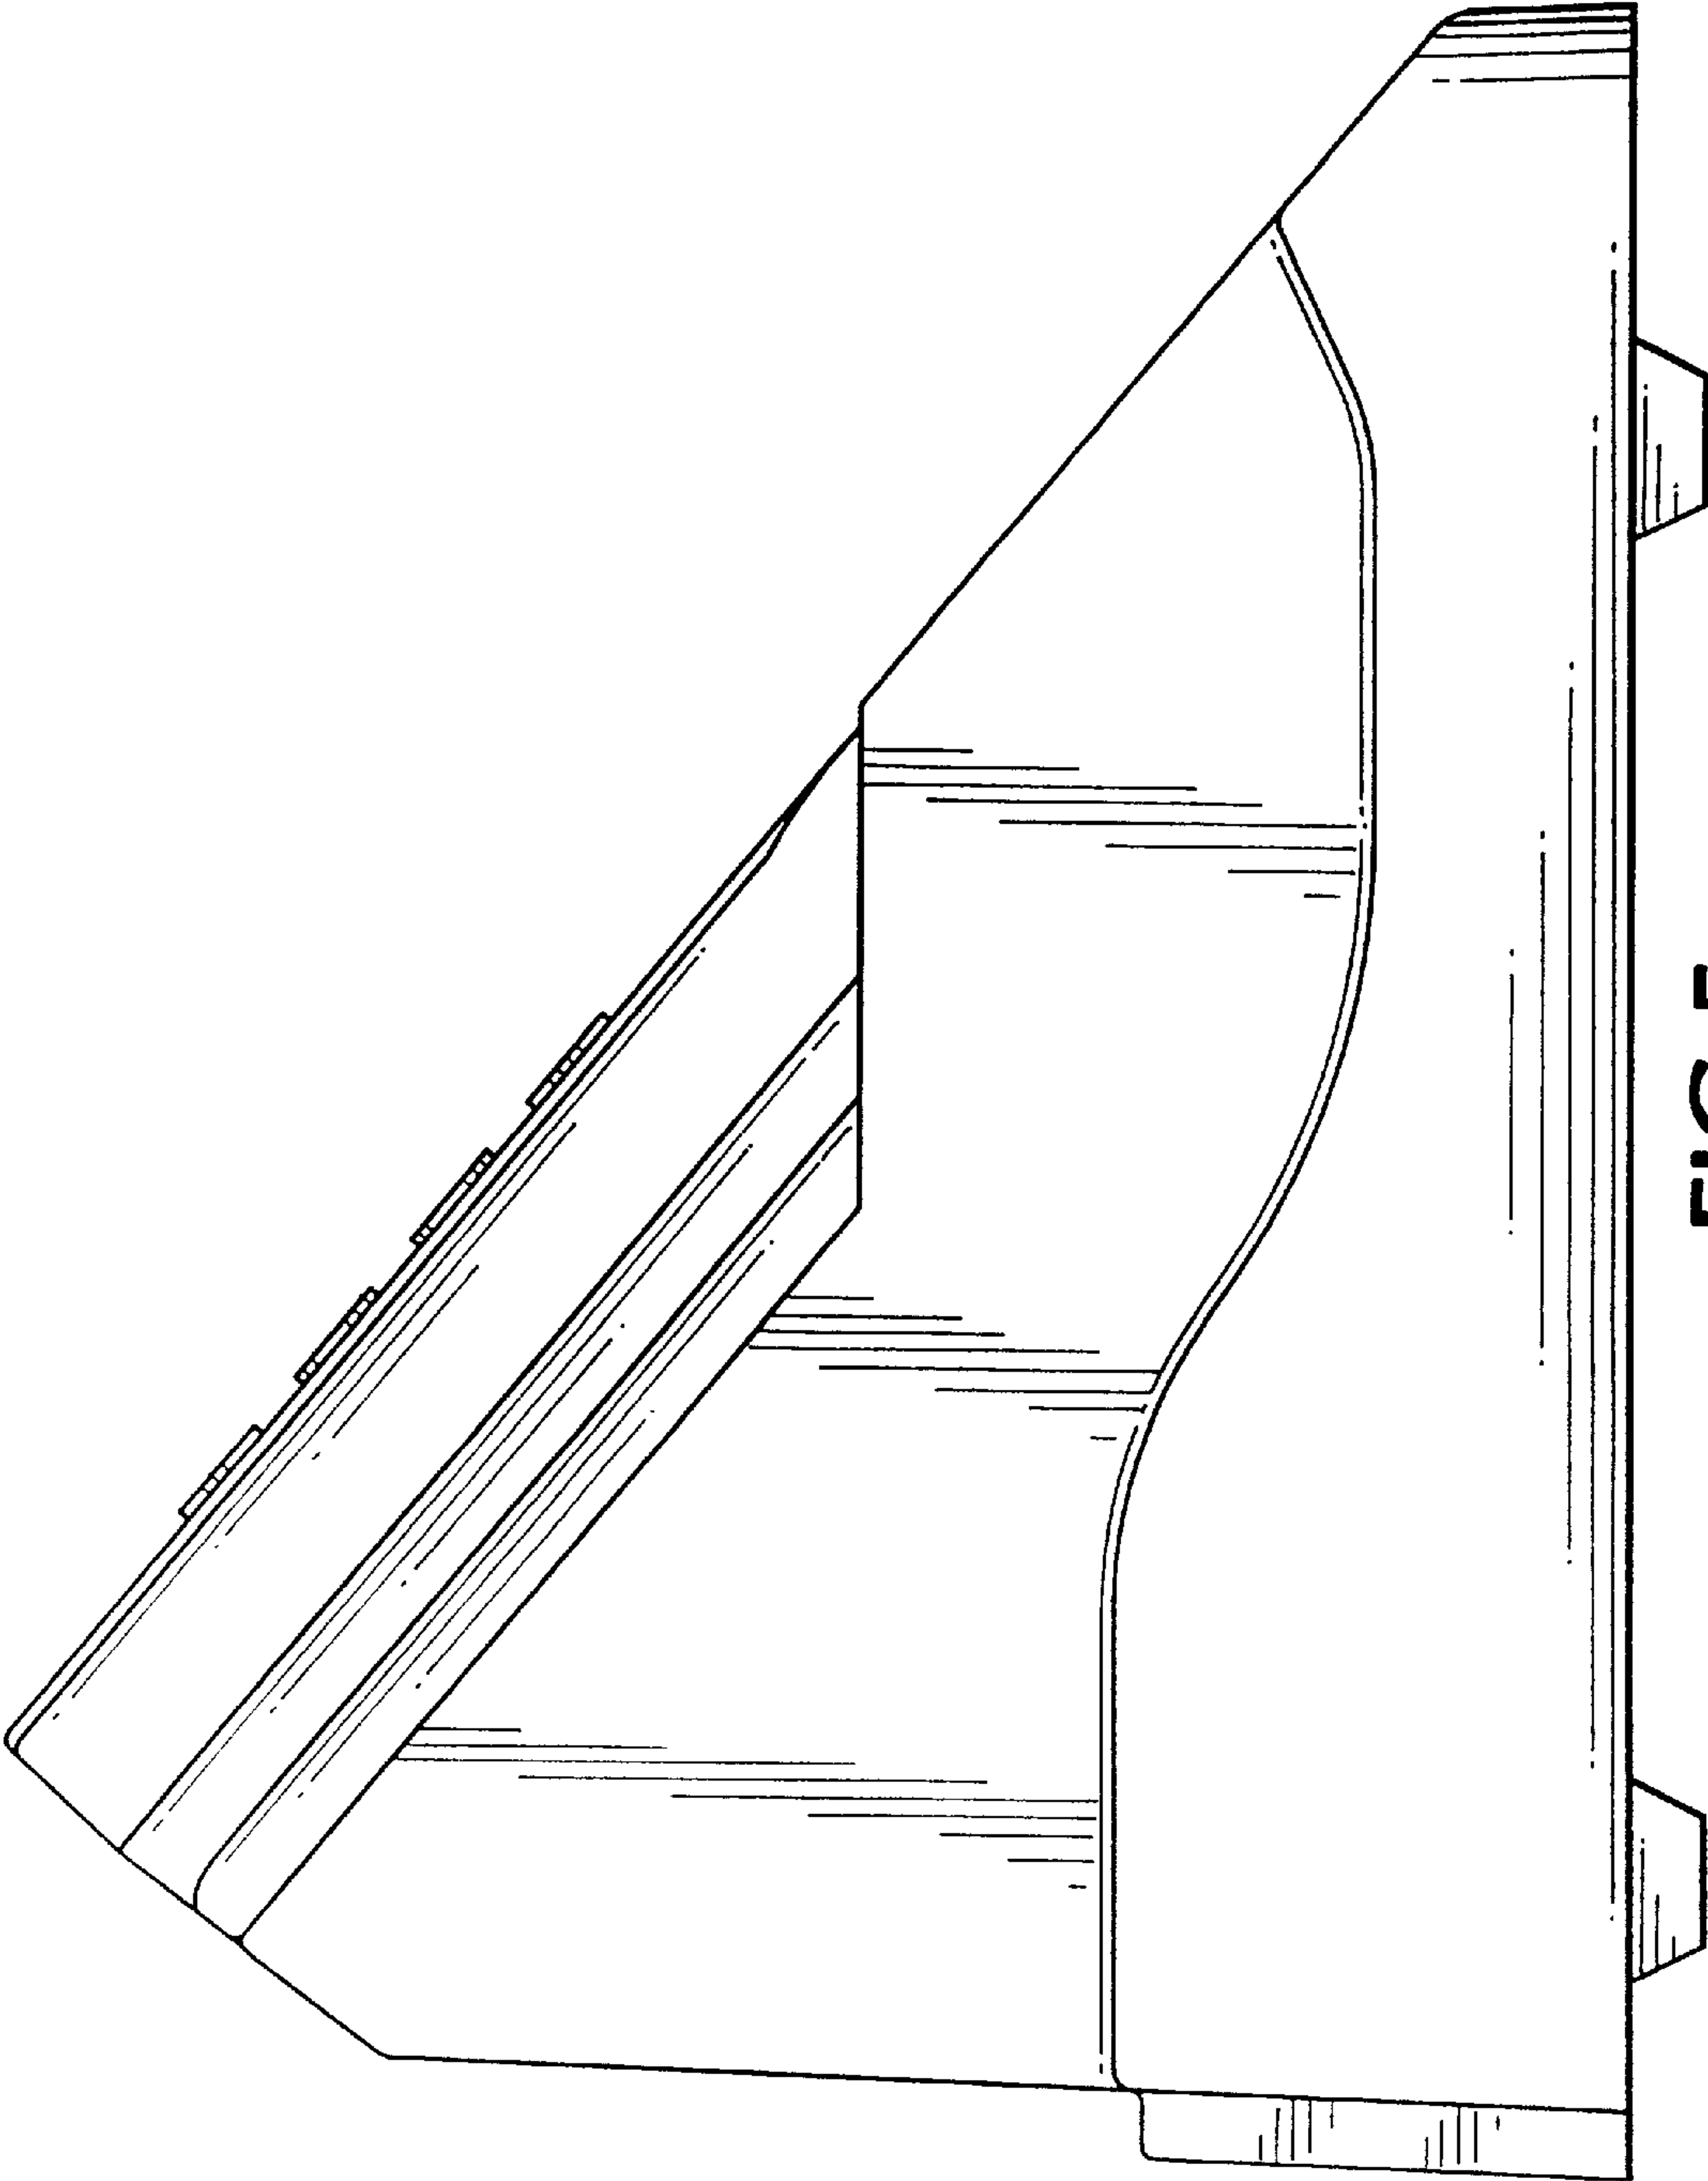


FIG.5

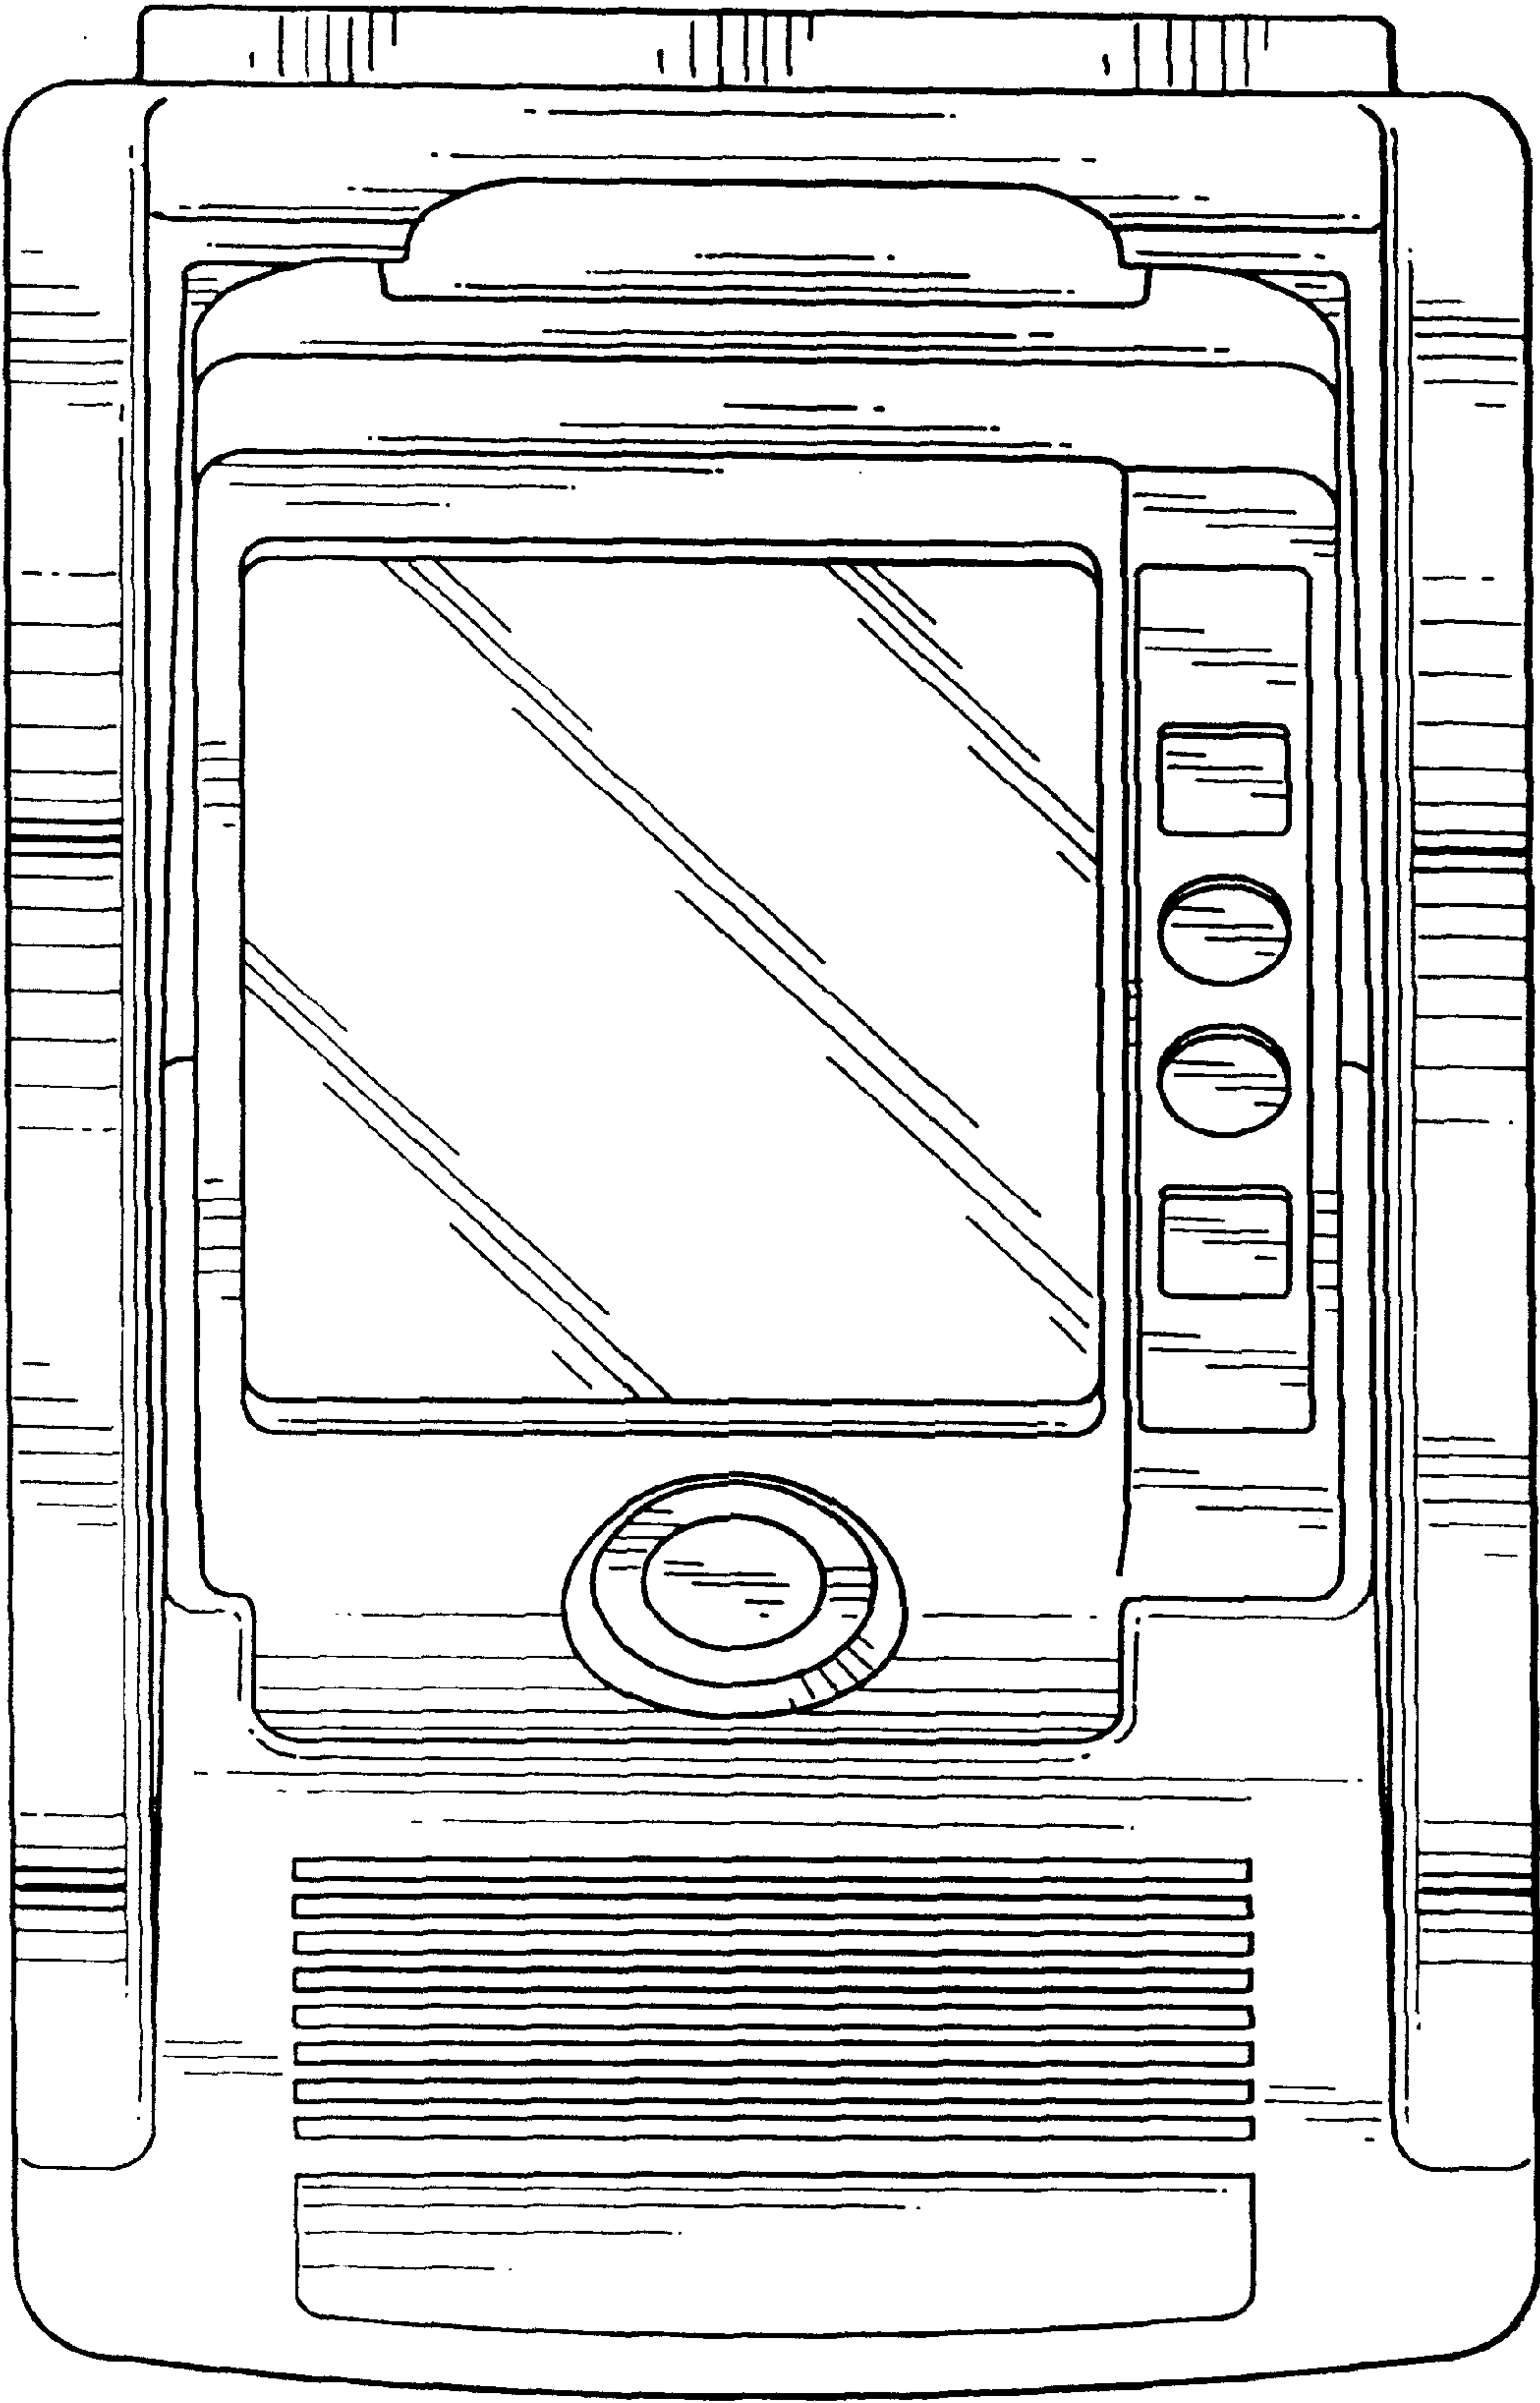


FIG.6

UNITED STATES PATENT AND TRADEMARK OFFICE
CERTIFICATE OF CORRECTION

PATENT NO. : D427,315

DATED : June 27, 2000

INVENTOR(S): William E. Saltzstein, Mohamed Sabri, Scott M. Burkhardt and Gregory T. Semler

It is certified that errors appear in the above-identified patent and that said Letters Patent is hereby corrected as shown below:

In the Description:

In Fig. 4, "right side thereof;" should read --right side view thereof;--.

Signed and Sealed this
Fifteenth Day of May, 2001



Attest:

NICHOLAS P. GODICI

Attesting Officer

Acting Director of the United States Patent and Trademark Office