



US00D441455S

(12) **United States Design Patent**
Feer et al.

(10) **Patent No.:** **US D441,455 S**

(45) **Date of Patent:** **** May 1, 2001**

(54) **PARAFFIN BATH**

(75) Inventors: **David Feer**, Wilton, NH (US); **Dov Glucksman**, Wemham, MA (US)

(73) Assignee: **Homedics, Inc.**, Commerce Township, MI (US)

(**) Term: **14 Years**

(21) Appl. No.: **29/123,574**

(22) Filed: **May 19, 2000**

(51) **LOC (7) Cl.** **24-04**

(52) **U.S. Cl.** **D24/200**

(58) **Field of Search** D24/200, 204;
607/96, 104, 108, 111; 604/291; D28/56,
61

(56) **References Cited**

U.S. PATENT DOCUMENTS

3,157,774 * 11/1964 Moore et al. 607/114

4,485,297 11/1984 Grise et al. .

4,656,339 4/1987 Grise .

4,782,835 * 11/1988 Bernardini 607/114

4,814,586 3/1989 Grise .

OTHER PUBLICATIONS

TheraBath® Paraffin Wax Therapy for arthritis, bursitis, tendonitis, www.1rehab.com/paraffin/index.htm, May 23, 2000, pp. 1–3.

Remington Products, Hand Care, www.remington-products.com/products/spatherapy/ahdn.html, May 23, 2000, pp. 1–3.

Photographs of Gena Paraffin Bath Product, pp. 1–2.

* cited by examiner

Primary Examiner—Stella Reid

(74) Attorney, Agent, or Firm—Brooks & Kushman PC

(57) **CLAIM**

The ornamental design for a paraffin bath, as shown and described.

DESCRIPTION

FIG. 1 is a perspective view of my new design;

FIG. 2 is a front elevation view of the new design;

FIG. 3 is a top plan view of the new design;

FIG. 4 is a right side elevation view of the new design, the left side view being a mirror image thereof;

FIG. 5 is a rear elevation view of the new design; and,

FIG. 6 is a bottom plan view of the new design.

The broken line in FIG. 5 is for illustrative purposes only and forms no part of the claimed design.

1 Claim, 3 Drawing Sheets

A perspective view of a paraffin bath device. The device has a rectangular body with rounded corners and a slightly raised rim. On the top surface, there is a central handle with a curved, ergonomic shape. The handle has a textured, possibly ribbed, surface. On the front face of the device, there are two circular control knobs or buttons, one on the left and one on the right. The device appears to be made of a solid material, possibly plastic or metal, and is designed for therapeutic use.

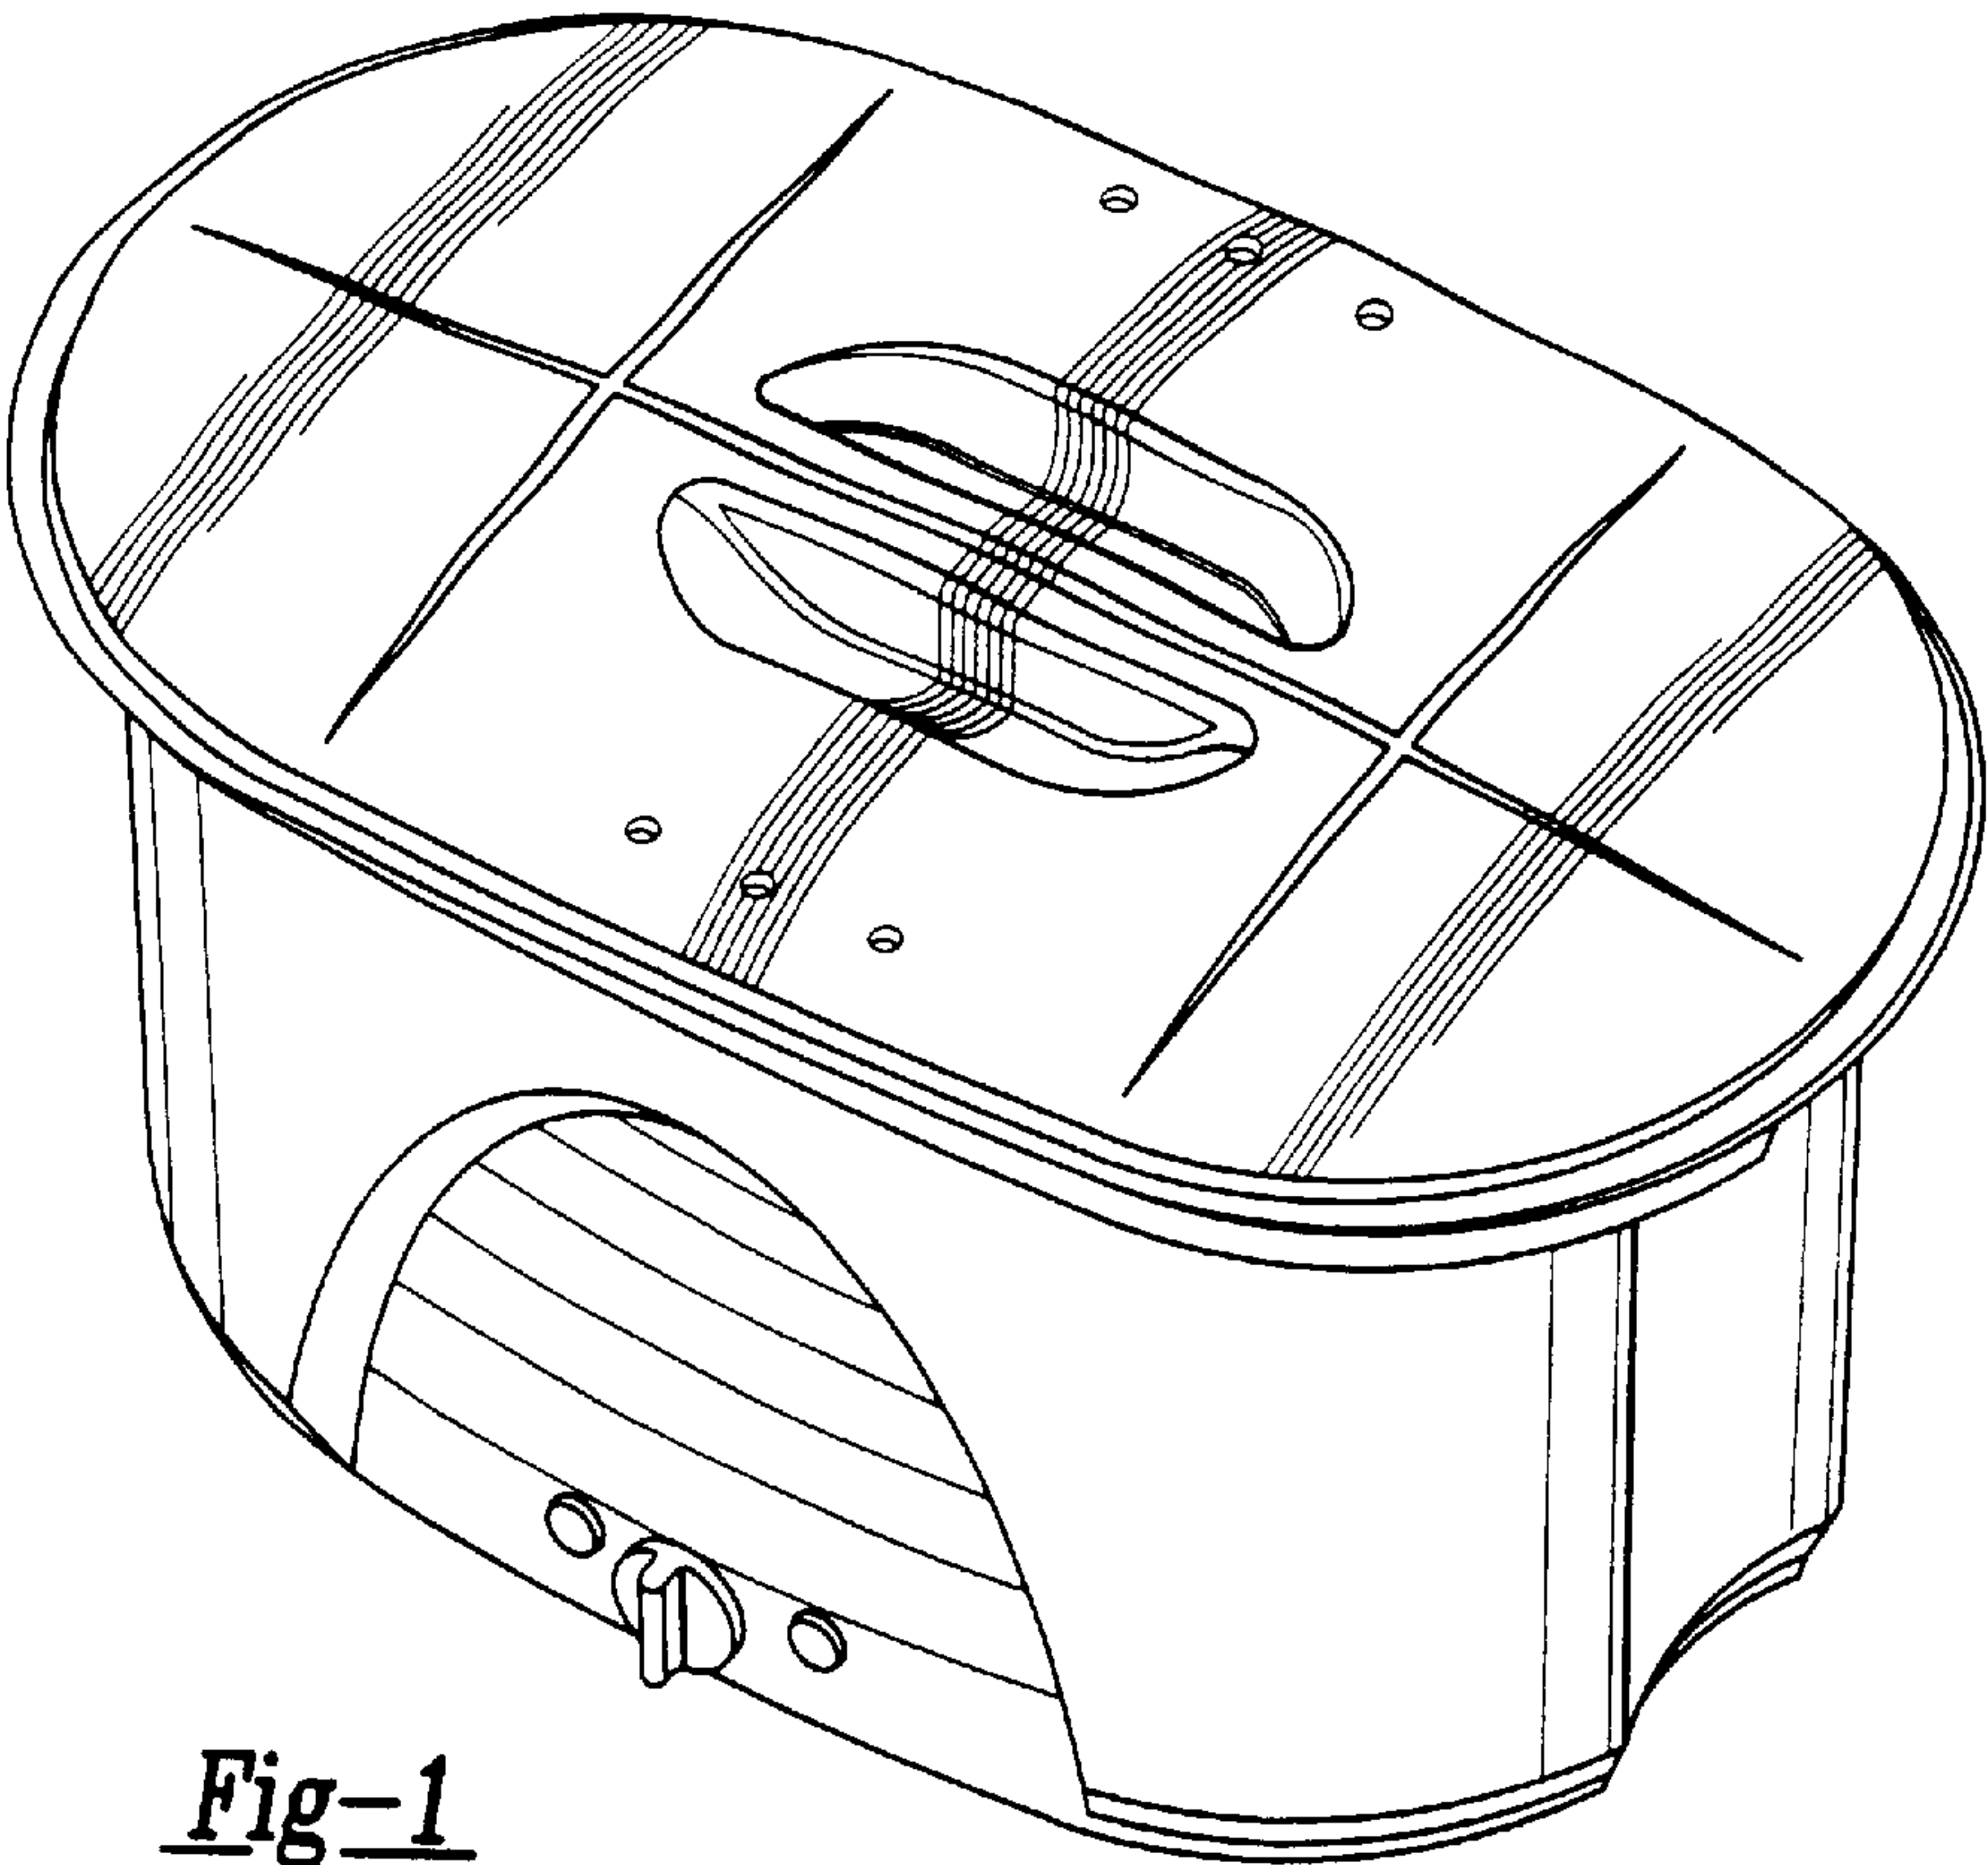


Fig-1

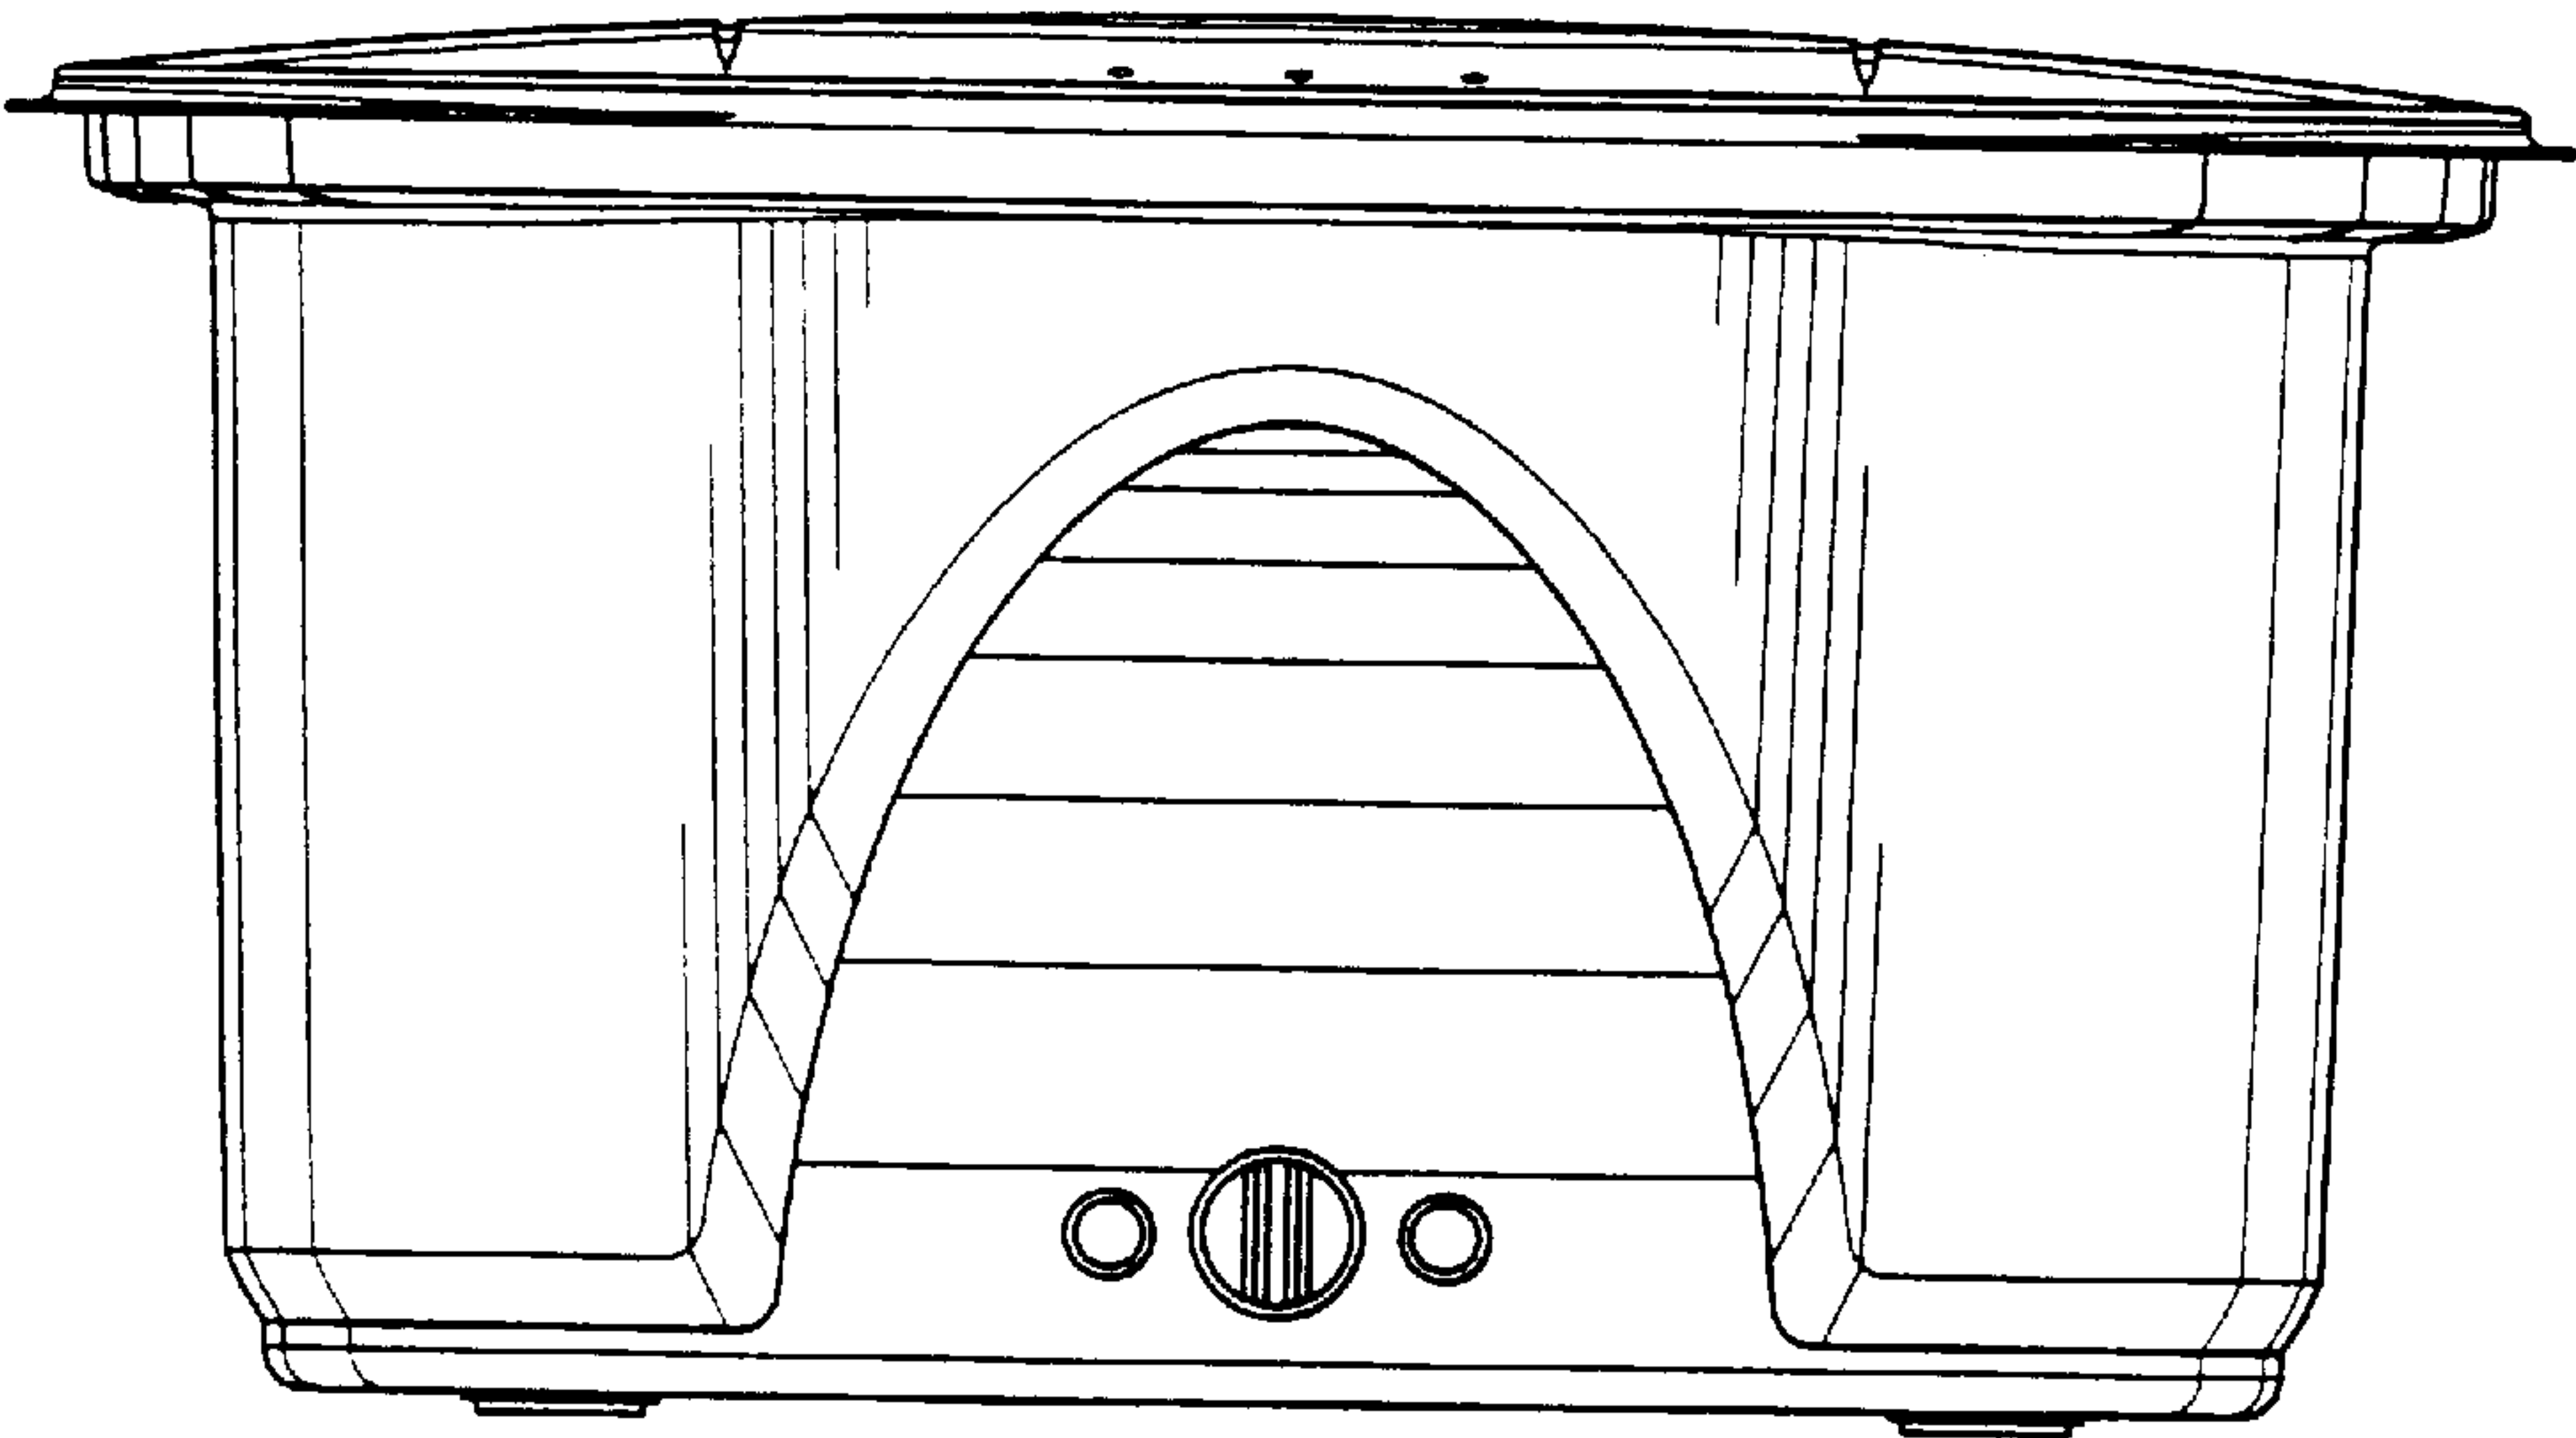


Fig-2

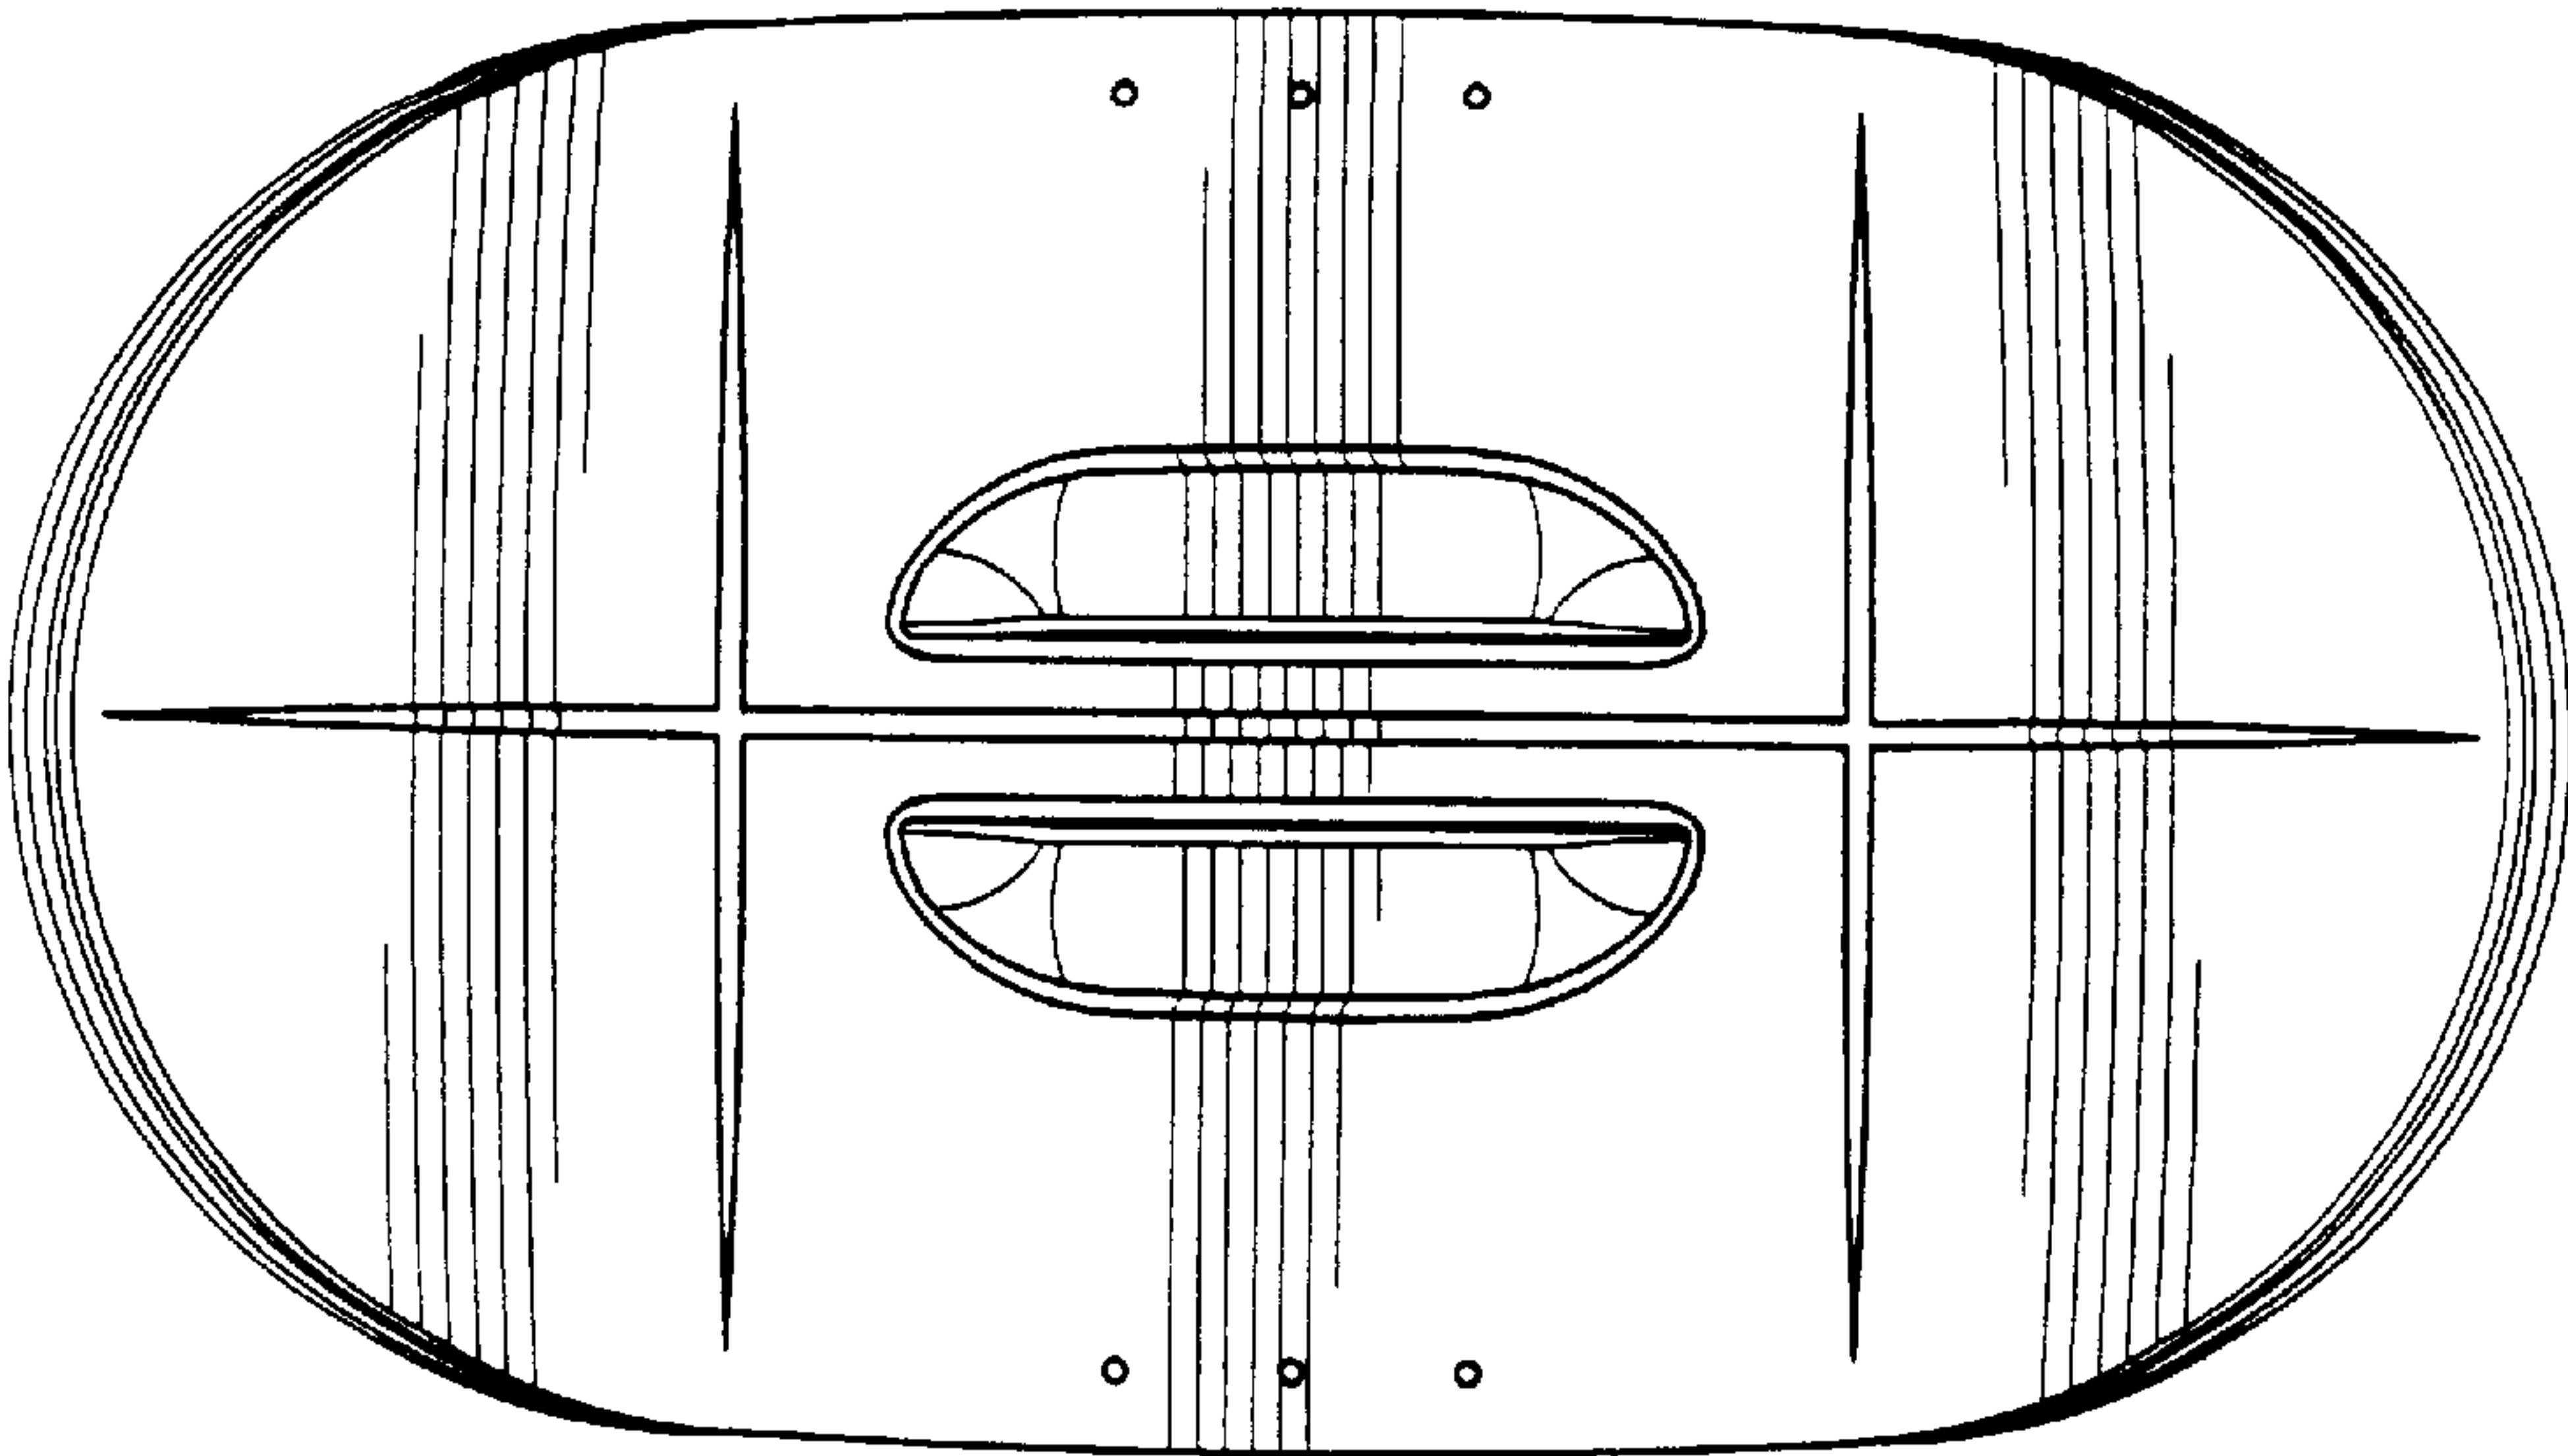
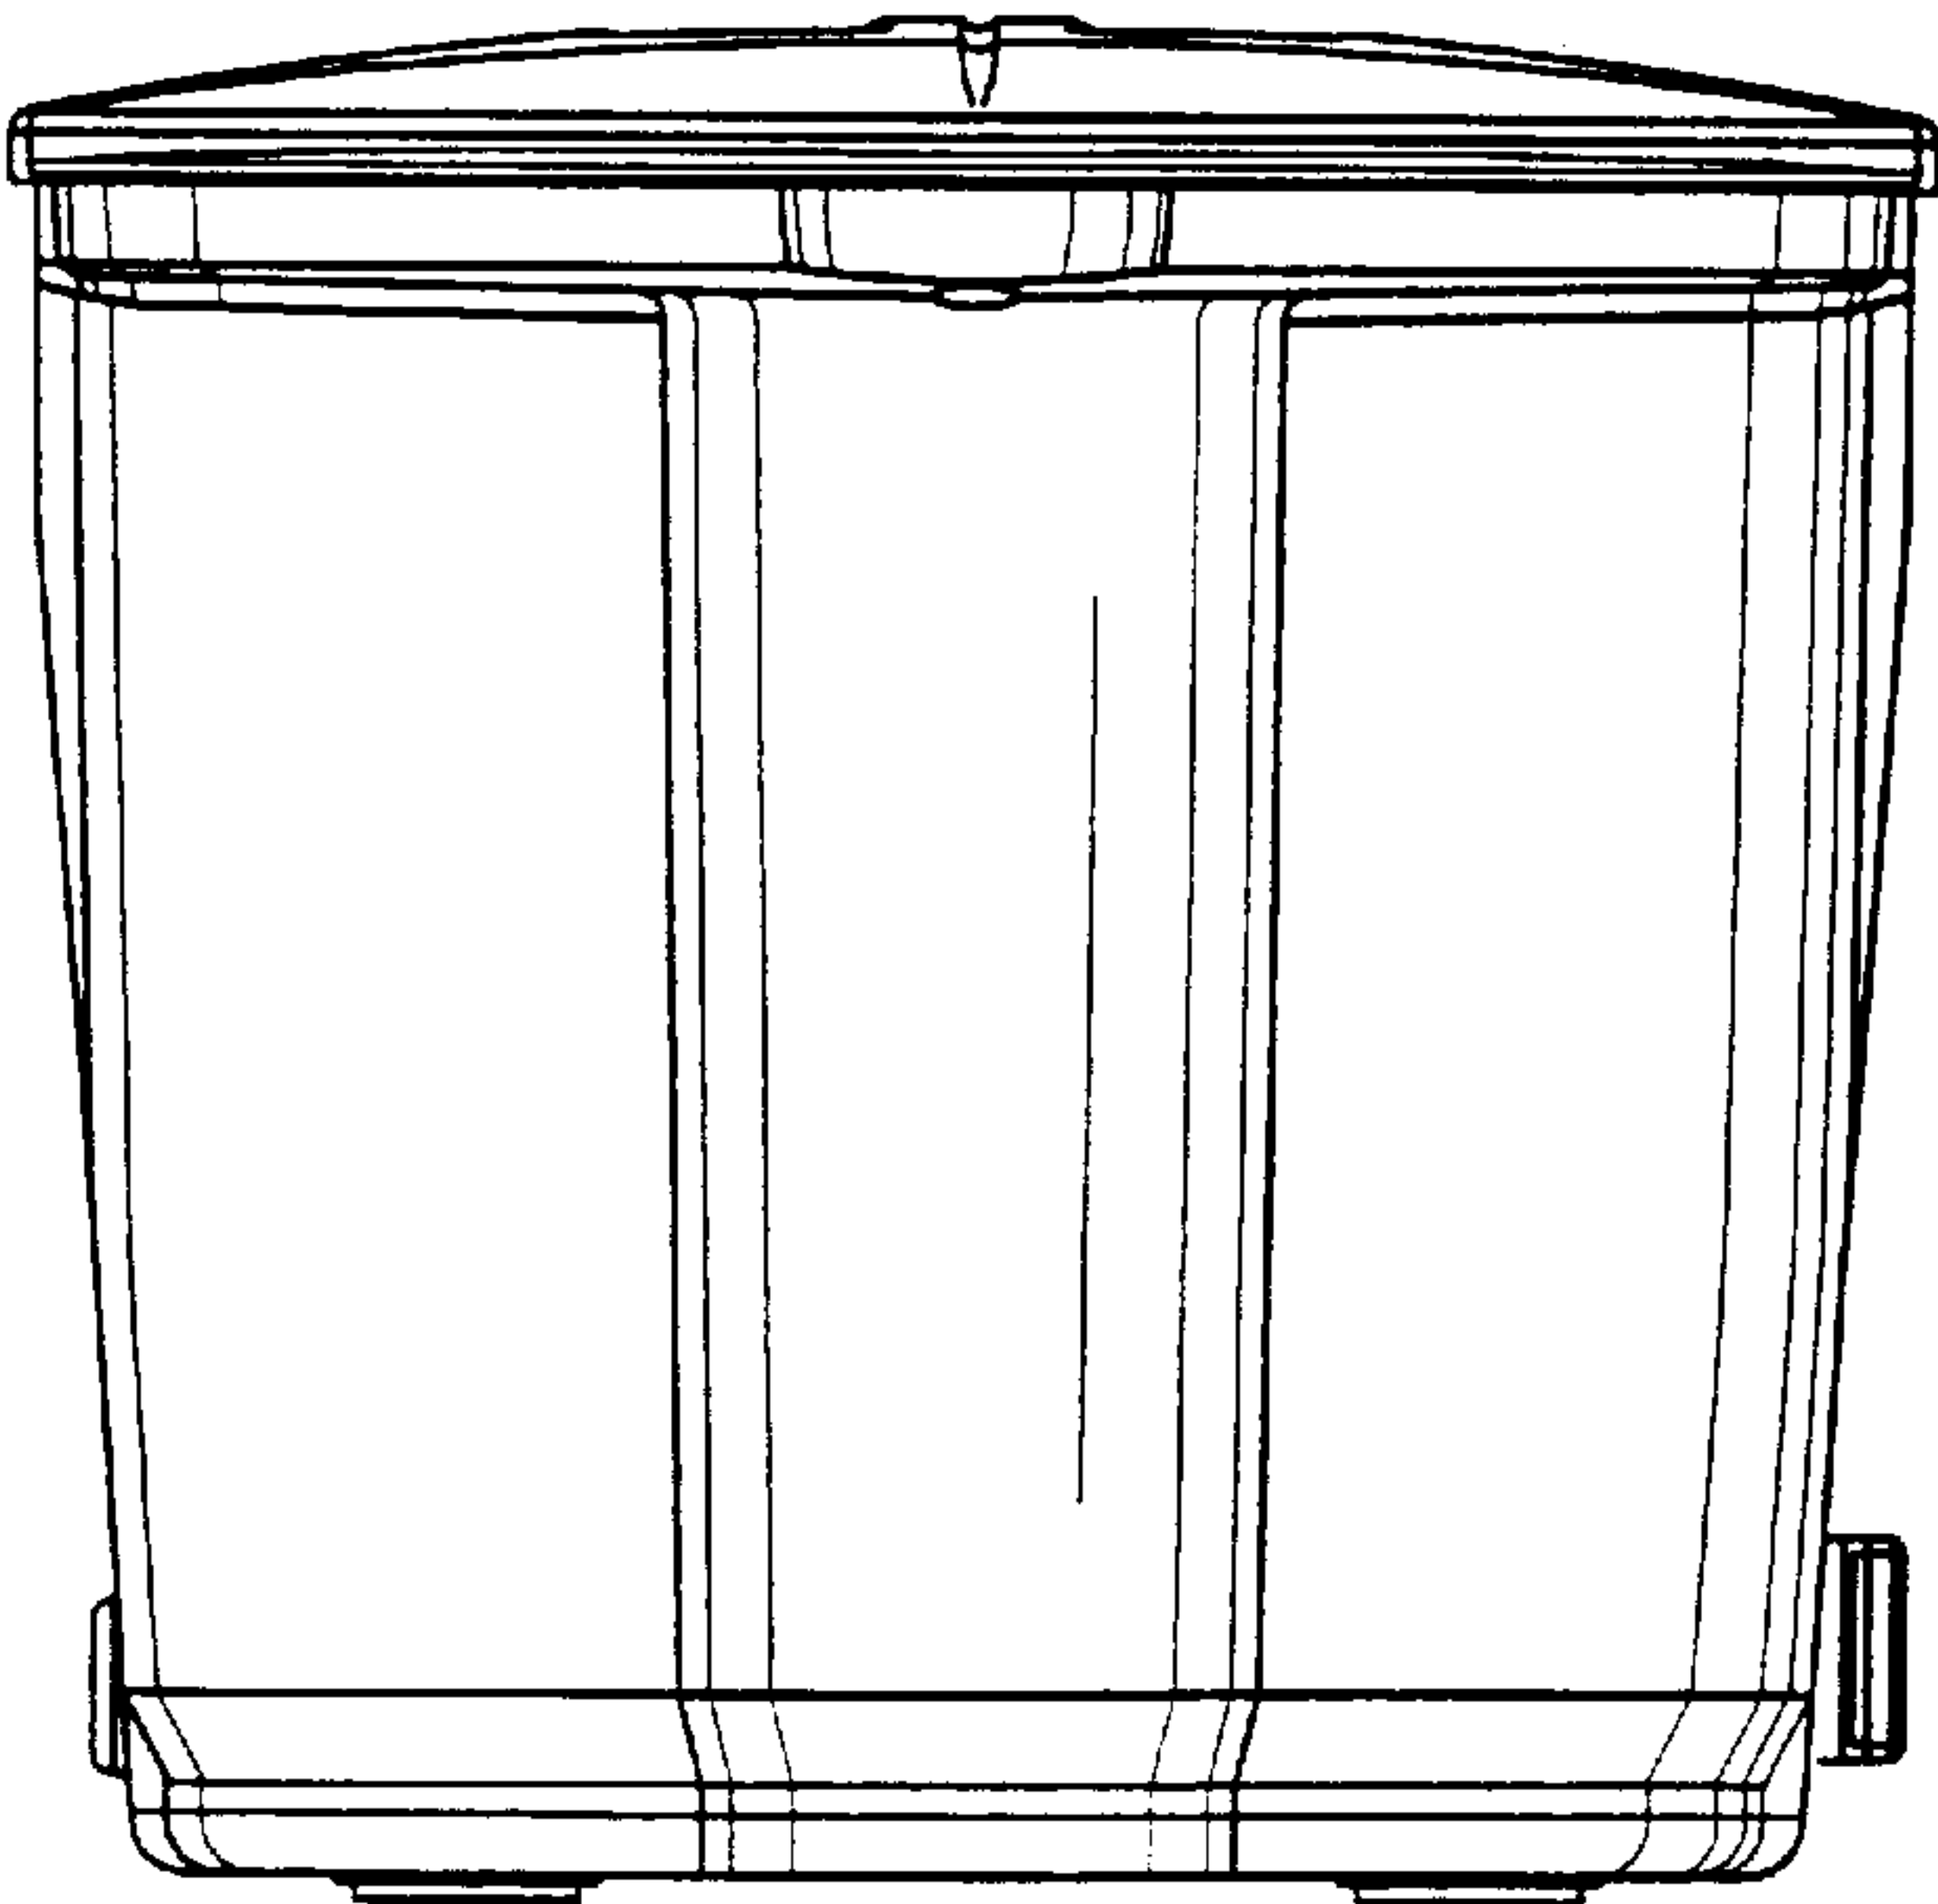


Fig-3

Fig-4



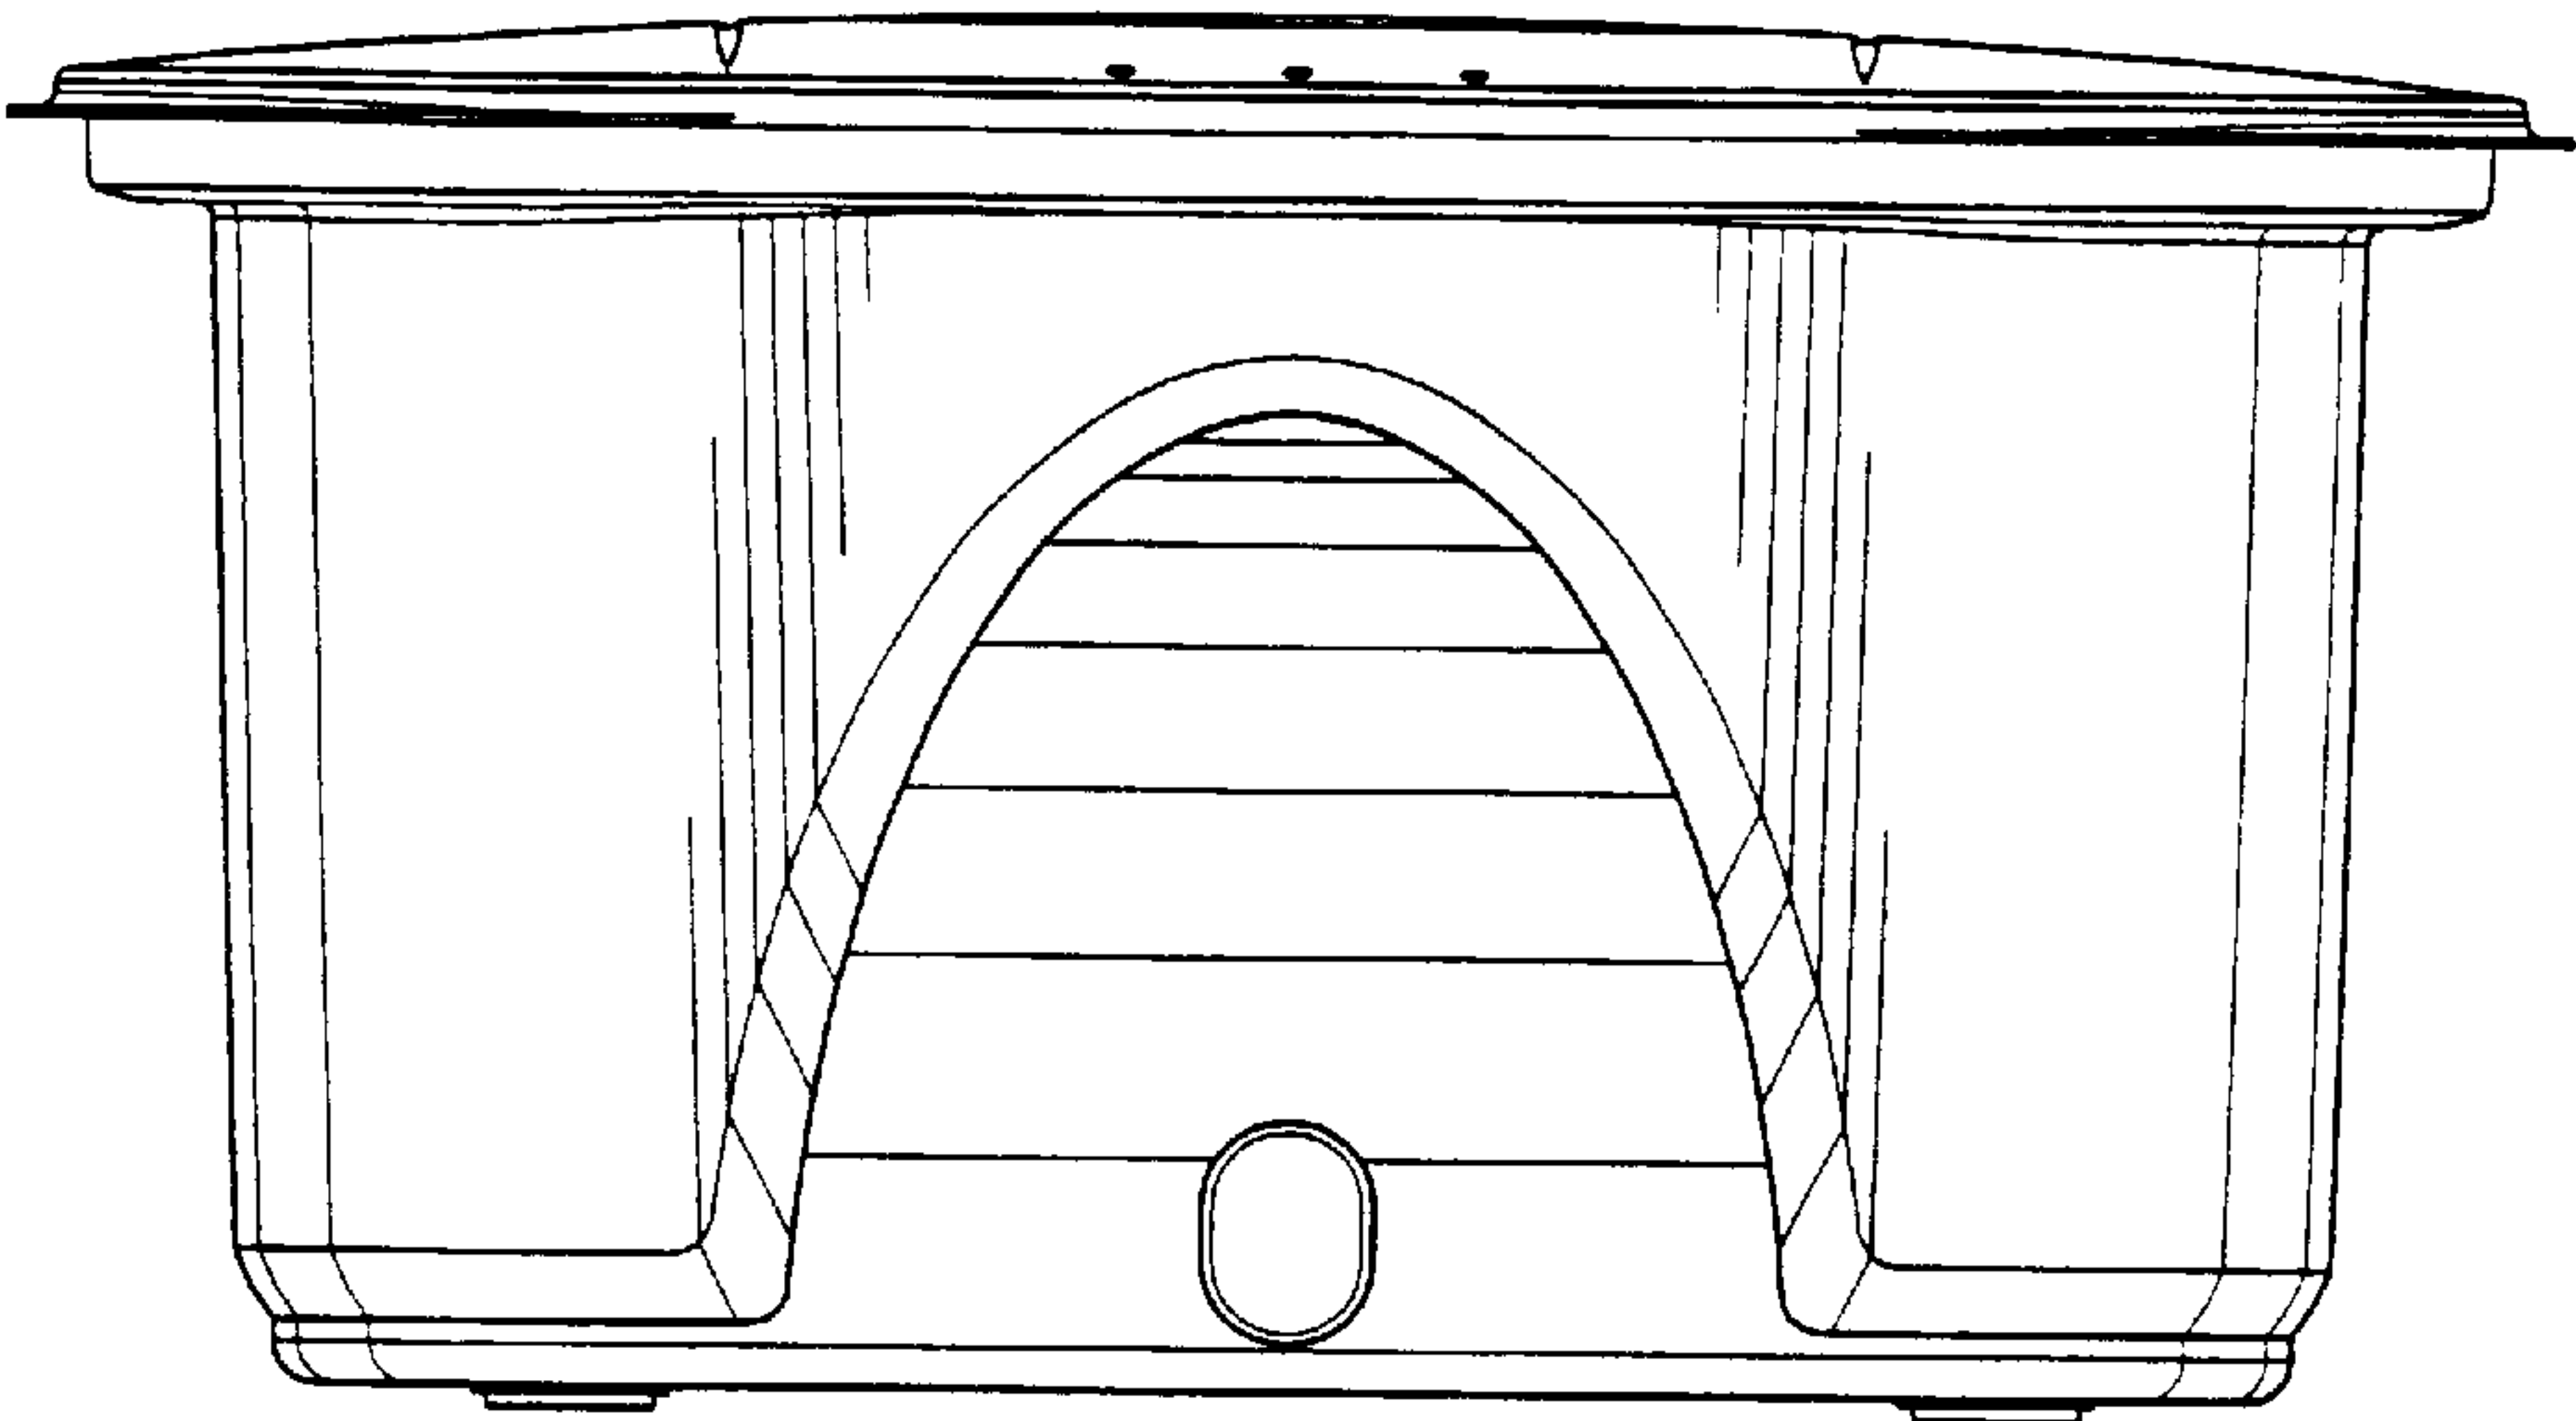


Fig-5

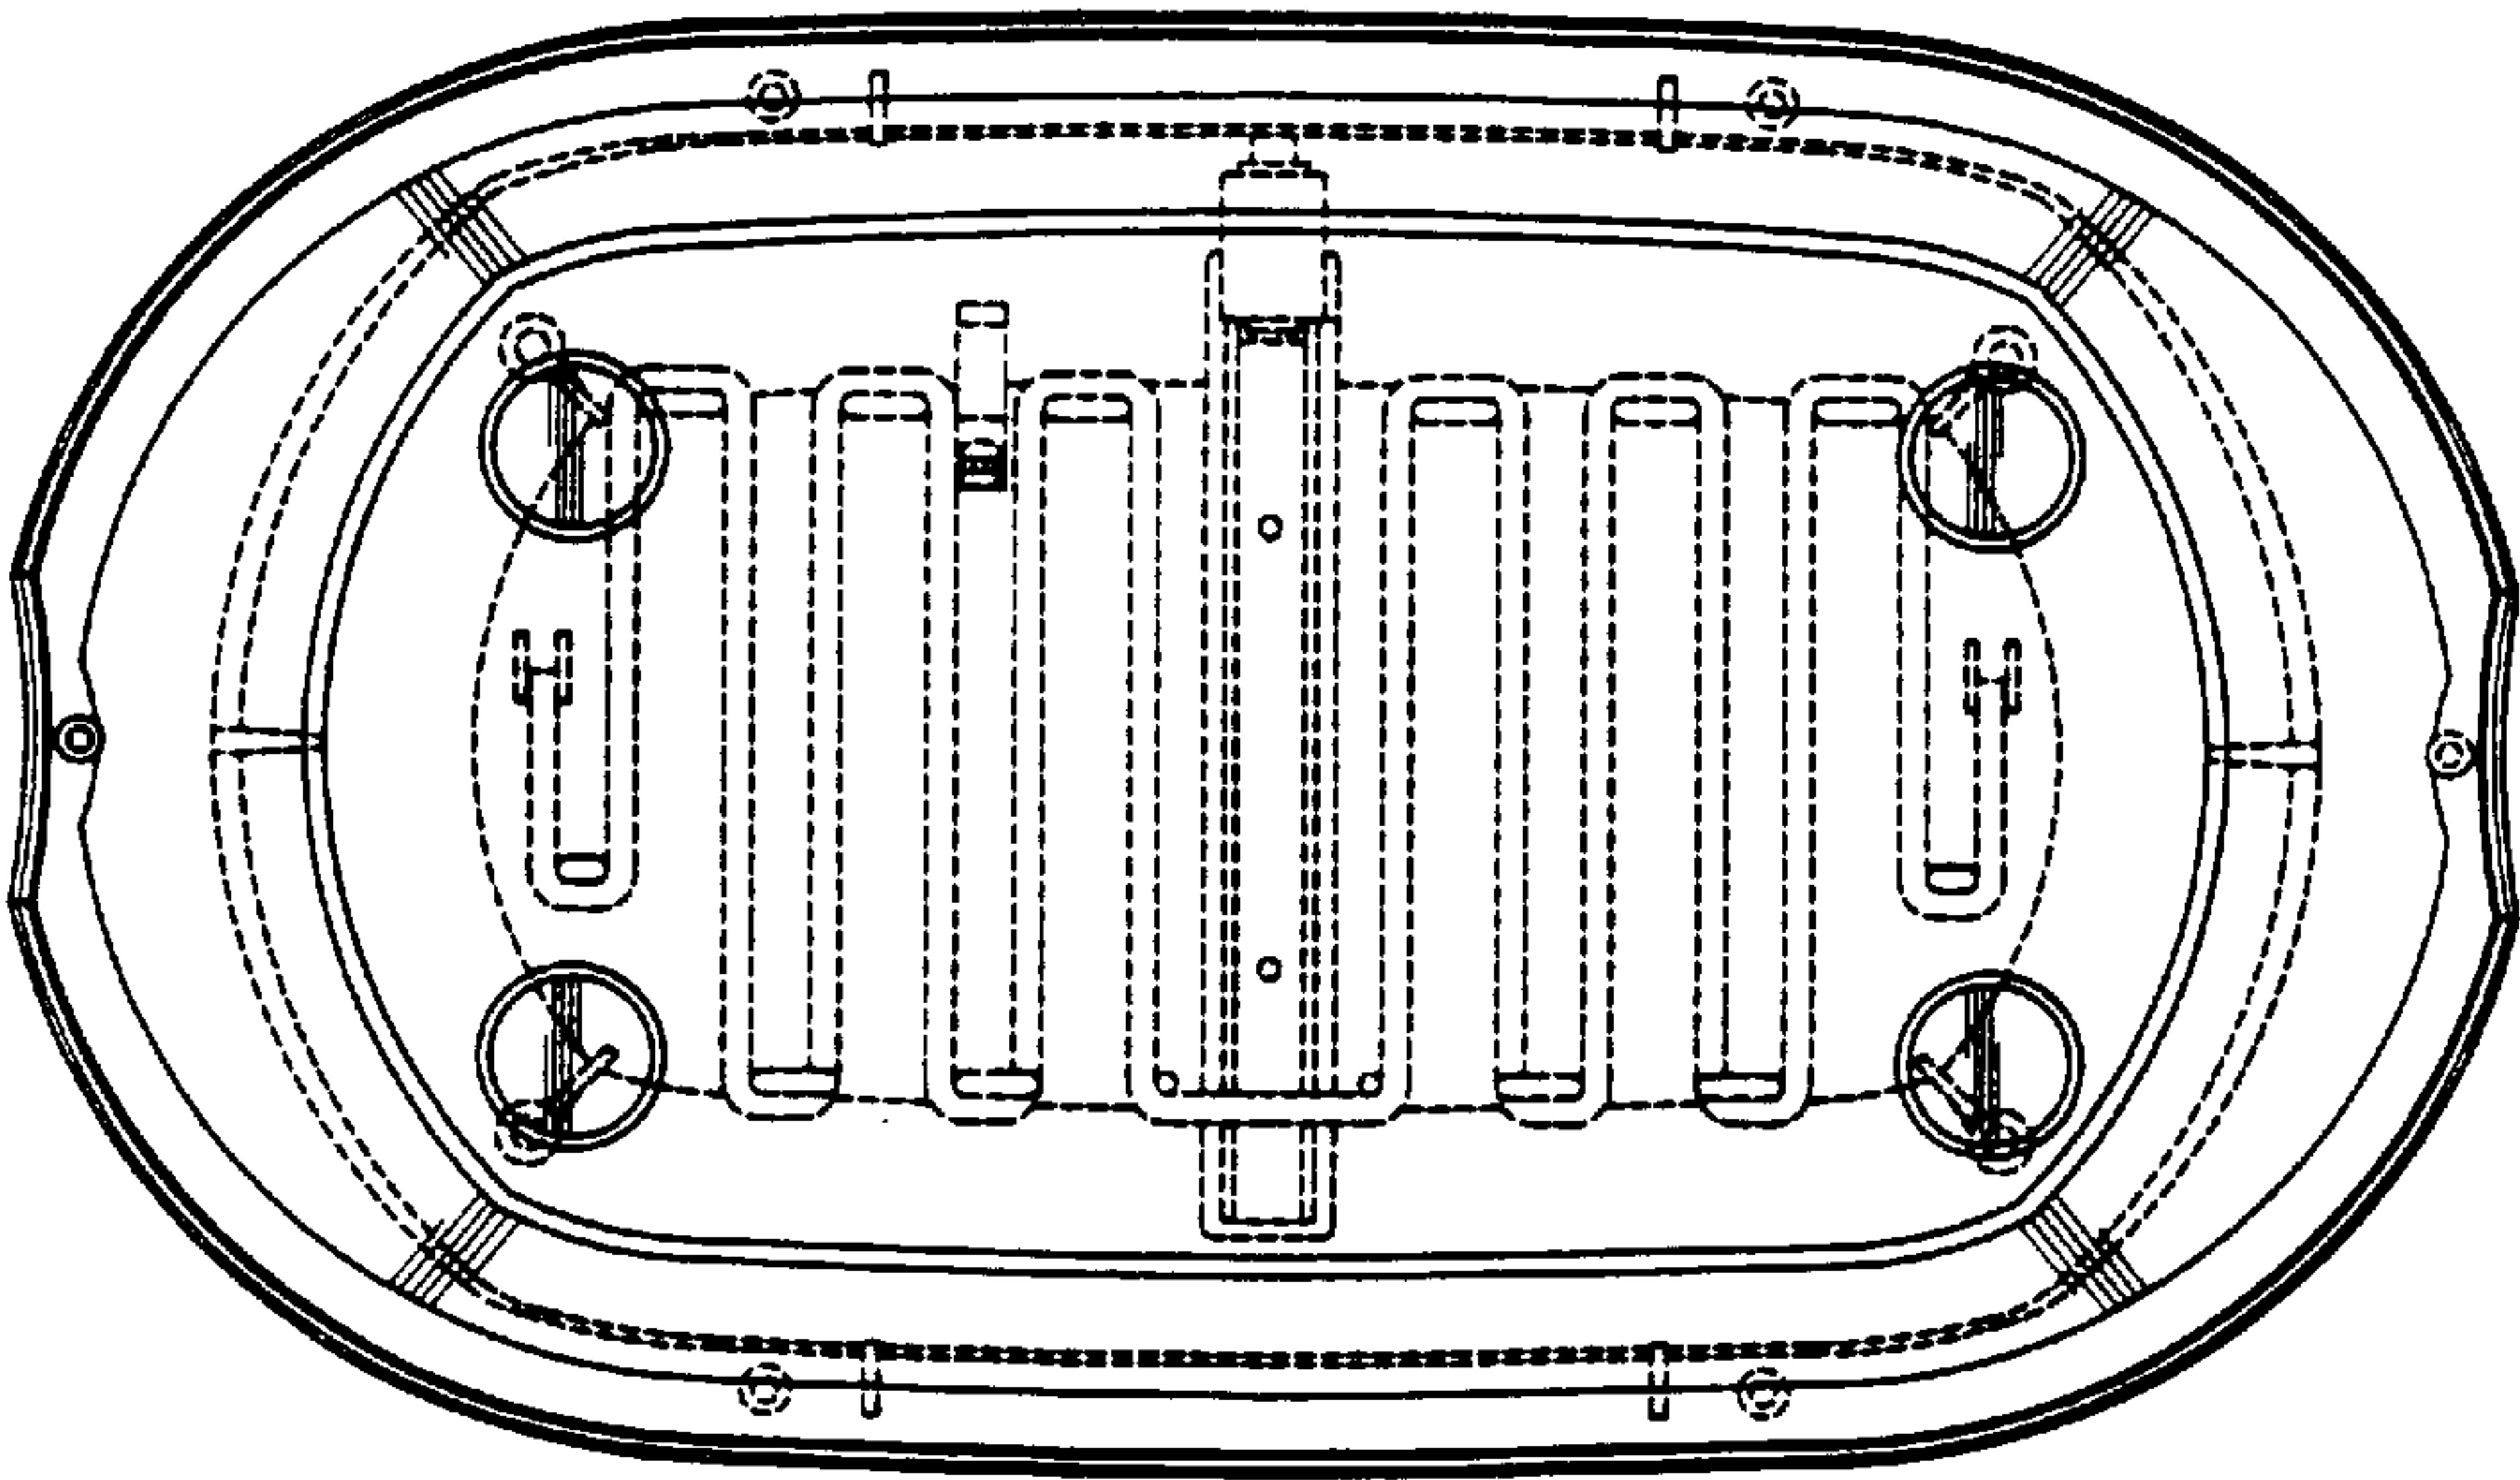


Fig-6