



US00D443695S

(12) **United States Design Patent**
Heitz et al.

(10) **Patent No.:** **US D443,695 S**

(45) **Date of Patent:** **** Jun. 12, 2001**

(54) **CONTAINER FOR DIAGNOSTIC ANALYZER**

(75) Inventors: **Bernhard H. Heitz; Rickey D. Burns,**
both of Roswell, GA (US)

(73) Assignee: **AVL Medical Instruments,**
Schaffhausen (CH)

(**) Term: **14 Years**

(21) Appl. No.: **29/123,892**

(22) Filed: **May 26, 2000**

(51) **LOC (7) Cl.** **24-02**

(52) **U.S. Cl.** **D24/224**

(58) **Field of Search** D24/224, 216,
D24/121; 422/102, 101, 103, 104, 61; 220/221,
403, 404; 204/401, 403; 73/862.51, 862.62,
862.22, 862.81

5,147,272	9/1992	Richison et al. .	
5,254,073	10/1993	Richison et al. .	
5,279,797	1/1994	Burns et al. .	
5,417,121	* 5/1995	Andersen et al.	73/864.22
5,501,982	3/1996	Saldivar, Jr. et al. .	
5,542,902	8/1996	Richison et al. .	
5,665,315	* 9/1997	Robert et al.	422/102
5,777,202	7/1998	Betts et al. .	
5,820,825	10/1998	Weinzierl et al. .	
5,882,602	3/1999	Savage et al. .	
5,885,533	3/1999	Savage et al. .	
5,913,232	6/1999	Betts et al. .	
5,980,830	11/1999	Savage et al. .	
5,985,218	11/1999	Goodale .	
5,986,453	10/1999	Shugart .	
6,016,683	1/2000	Betts et al. .	
6,178,832	* 1/2001	Mathur et al.	73/864.62

* cited by examiner

Primary Examiner—Ian Simmons

(74) *Attorney, Agent, or Firm*—Baker Botts L.L.P.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D. 305,360	1/1990	Fechtner .	
D. 337,164	7/1993	Lauks et al. .	
D. 347,067	5/1994	Shartle et al. .	
D. 403,259	12/1998	Tsubota et al. .	
D. 403,604	1/1999	Tsubota et al. .	
D. 407,485	3/1999	Lanza et al. .	
D. 433,149	* 10/2000	Fassbind et al.	D24/224
4,642,089	2/1987	Zupkas et al. .	
4,649,028	3/1987	Kaltenbach et al. .	
4,737,139	4/1988	Zupkas et al. .	
4,786,394	11/1988	Enzer et al. .	
4,871,439	10/1989	Enzer et al. .	
4,929,426	5/1990	Bodai et al. .	
4,970,053	11/1990	Fechtner .	
5,059,036	10/1991	Richison et al. .	
5,075,082	12/1991	Fechtner .	


(57) **CLAIM**

The ornamental design for a container for diagnostic analyzer, as shown and described.

DESCRIPTION

FIG. 1 is a perspective view of a container for diagnostic analyzer showing our new design, with the cover removed; FIG. 2 is a front view thereof; FIG. 3 is a rear view thereof; FIG. 4 is a right side view thereof; FIG. 5 is a left side view thereof; FIG. 6 is a top plan view thereof; FIG. 7 is a bottom plan view thereof; and, FIG. 8 is a perspective view thereof, with the cover in place.

1 Claim, 6 Drawing Sheets

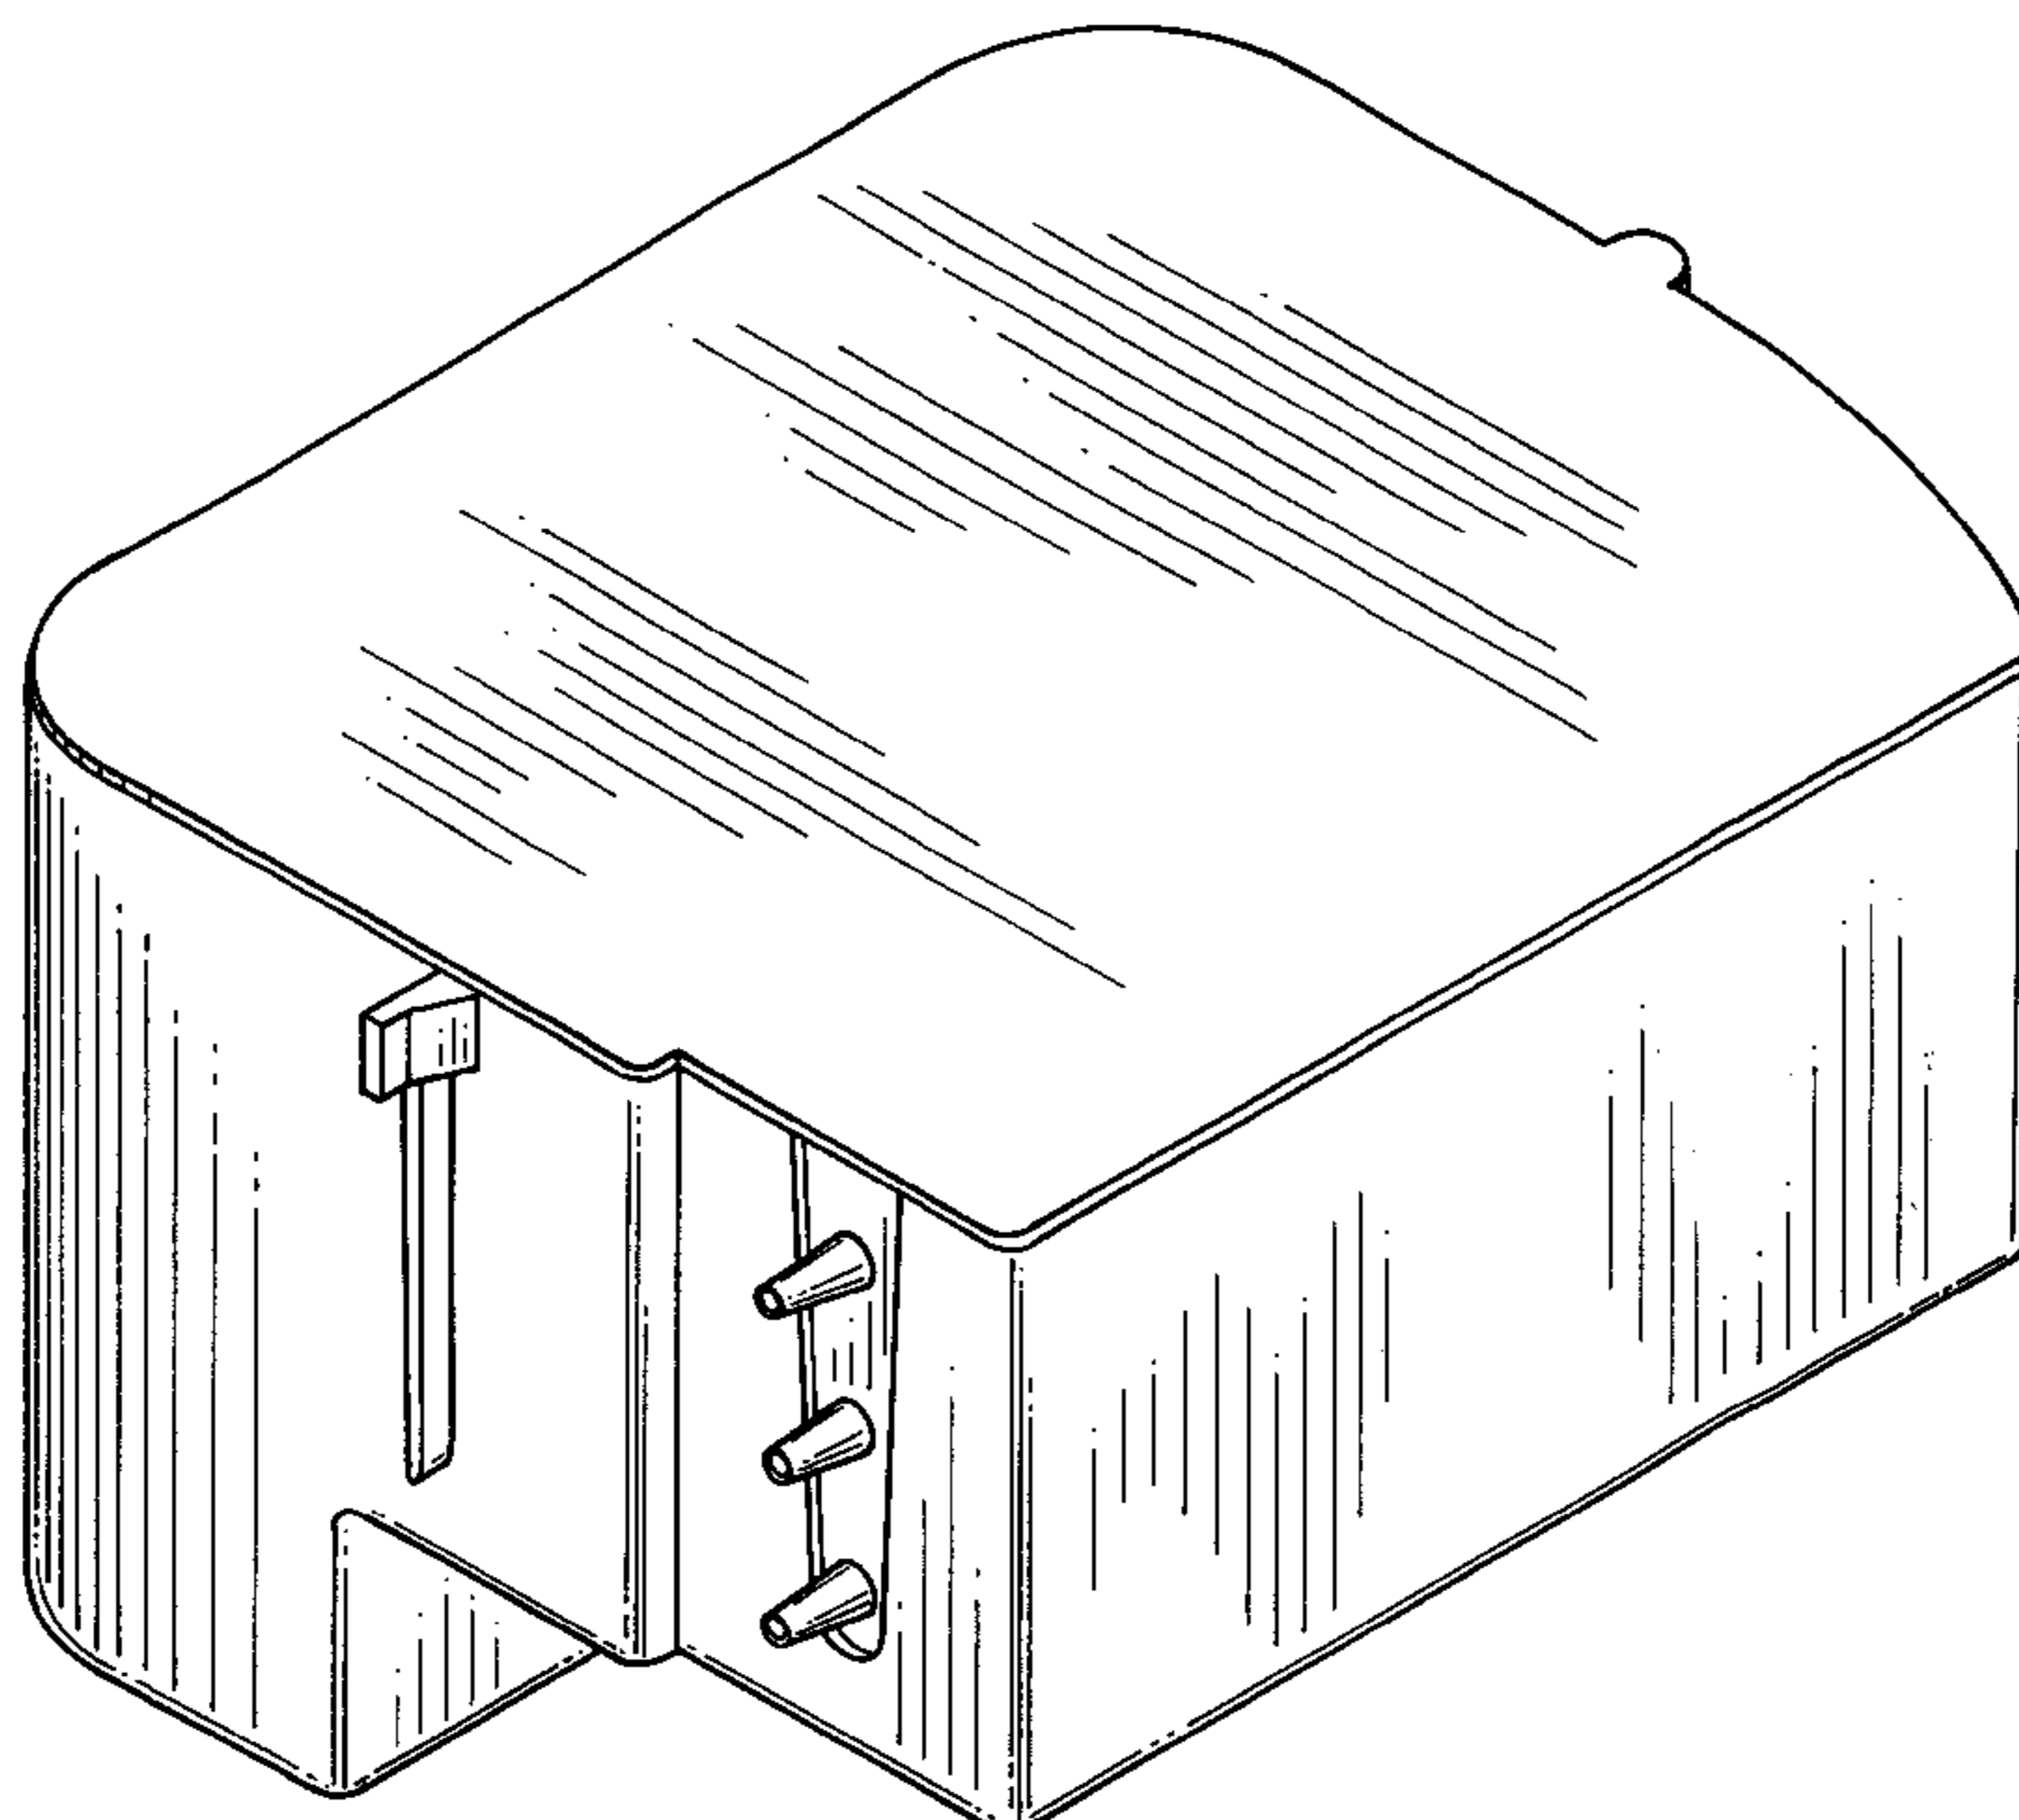

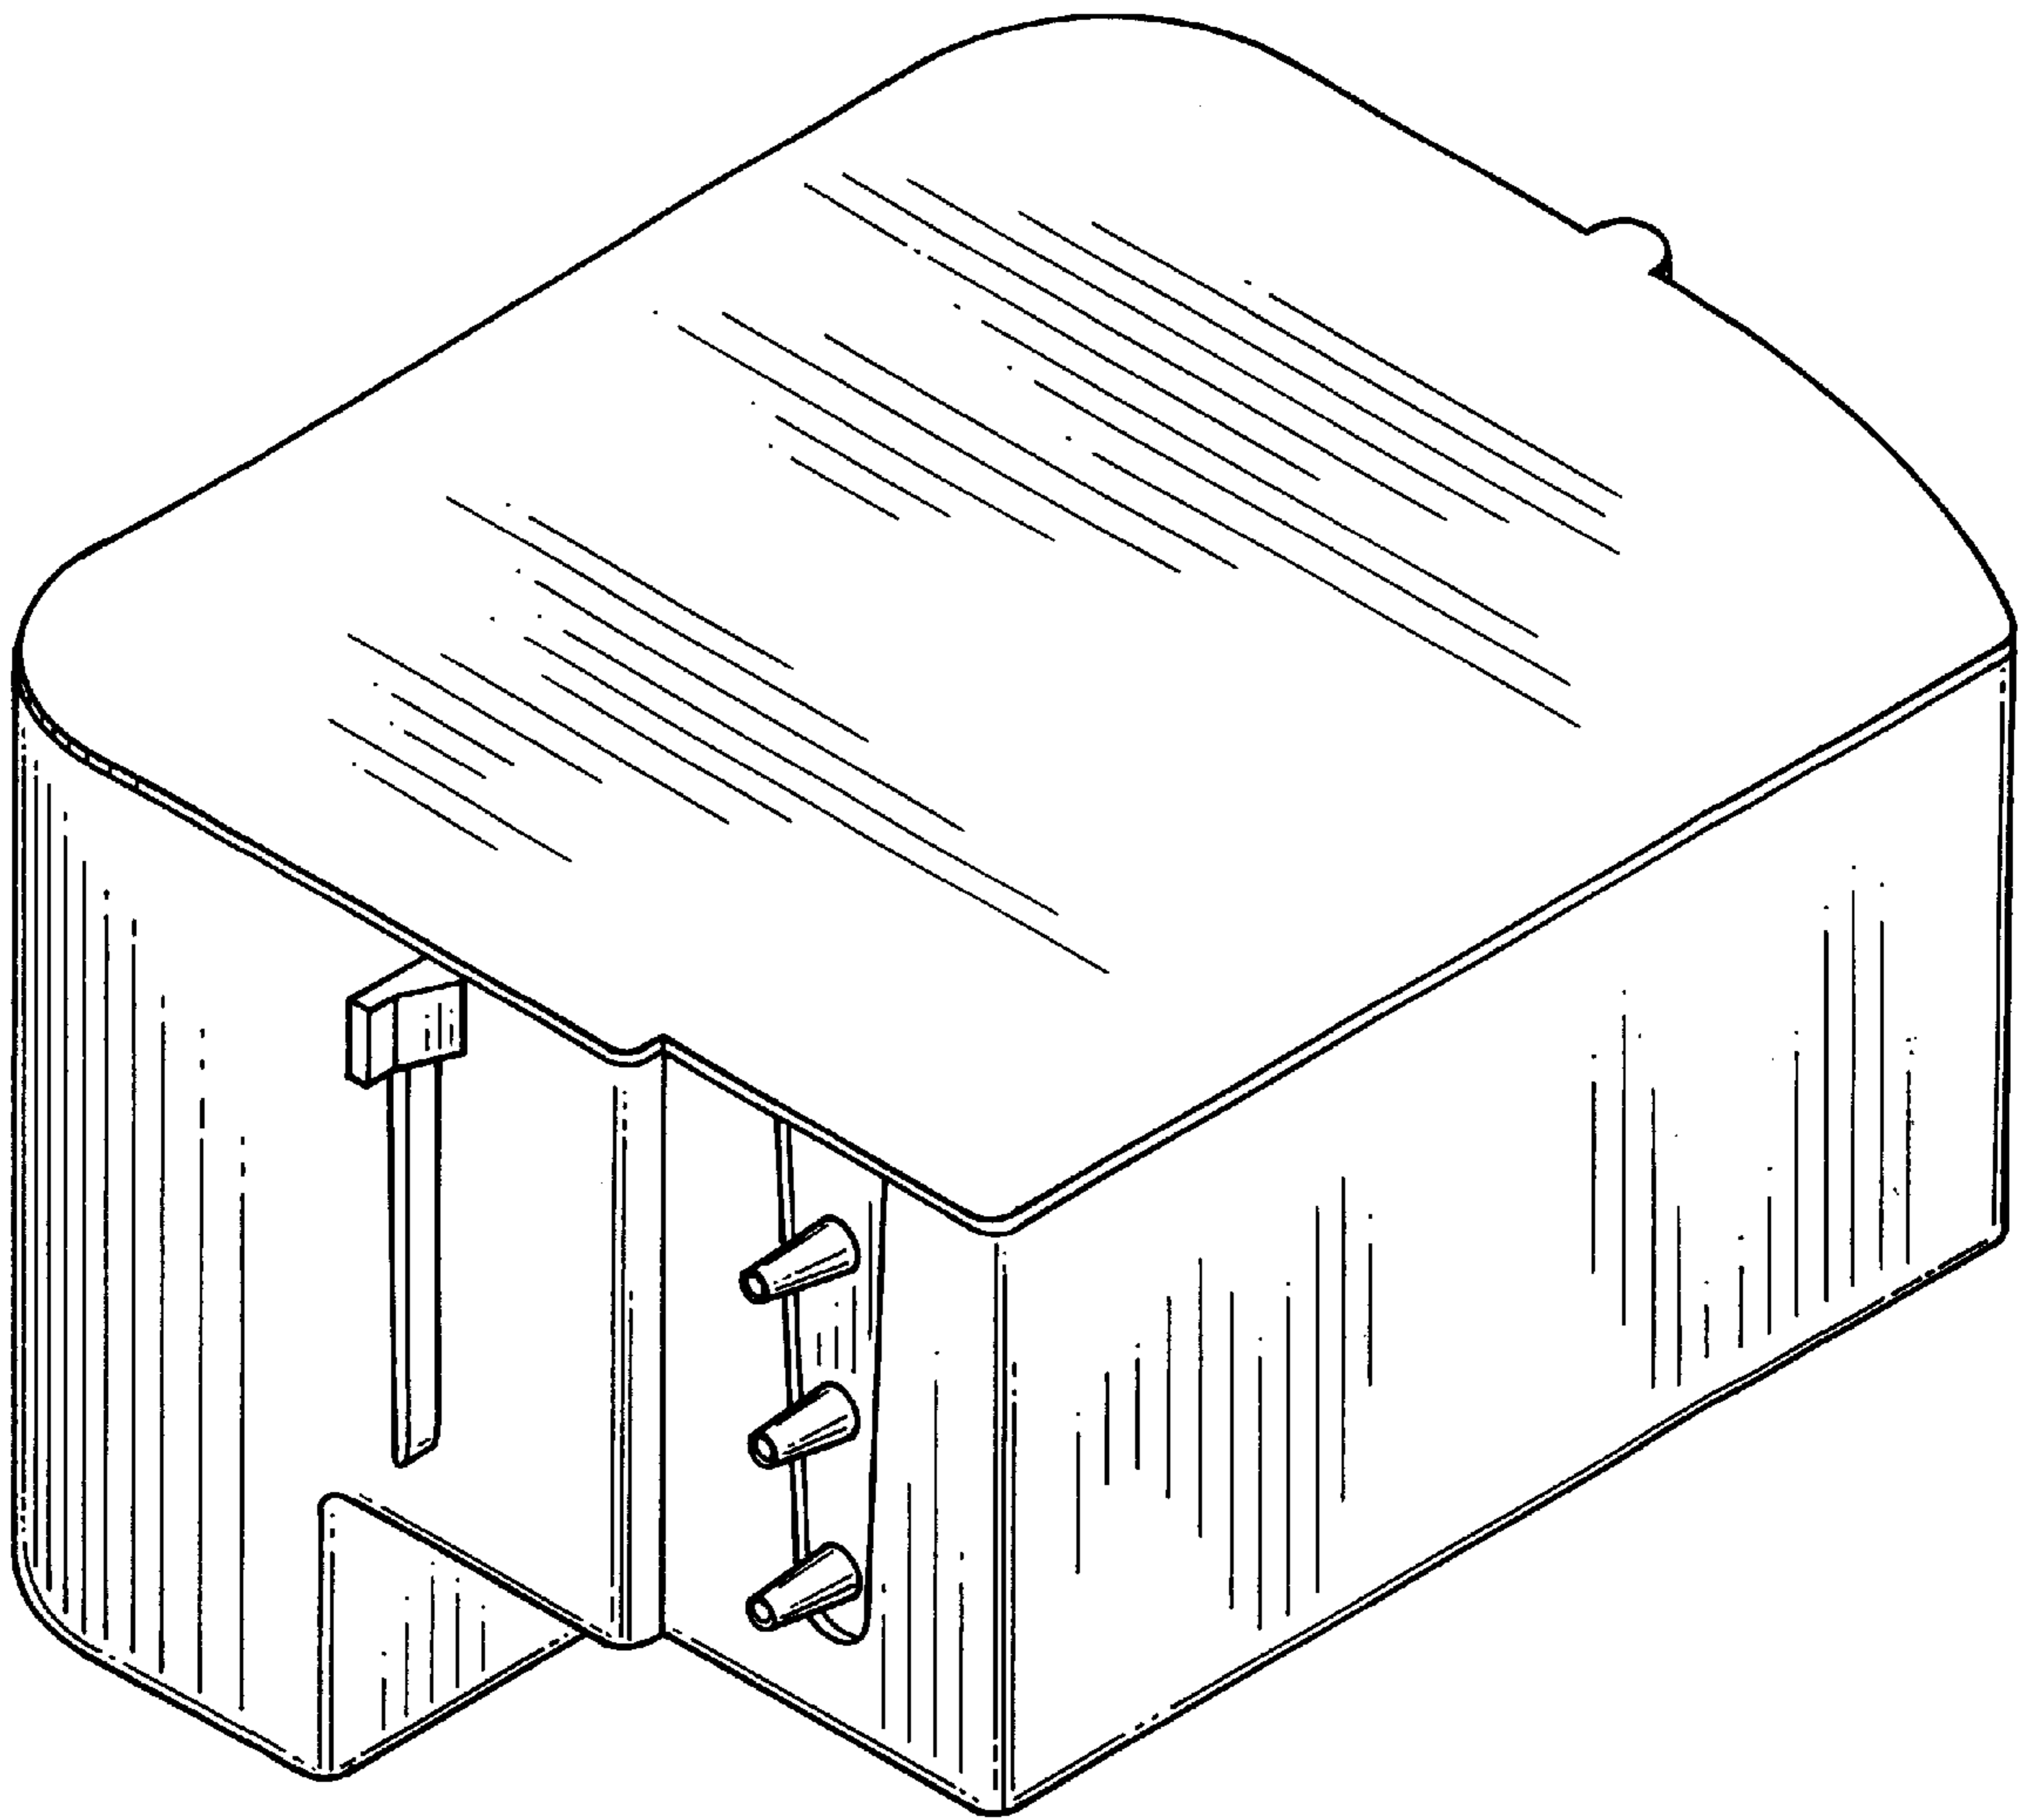


FIG. 1

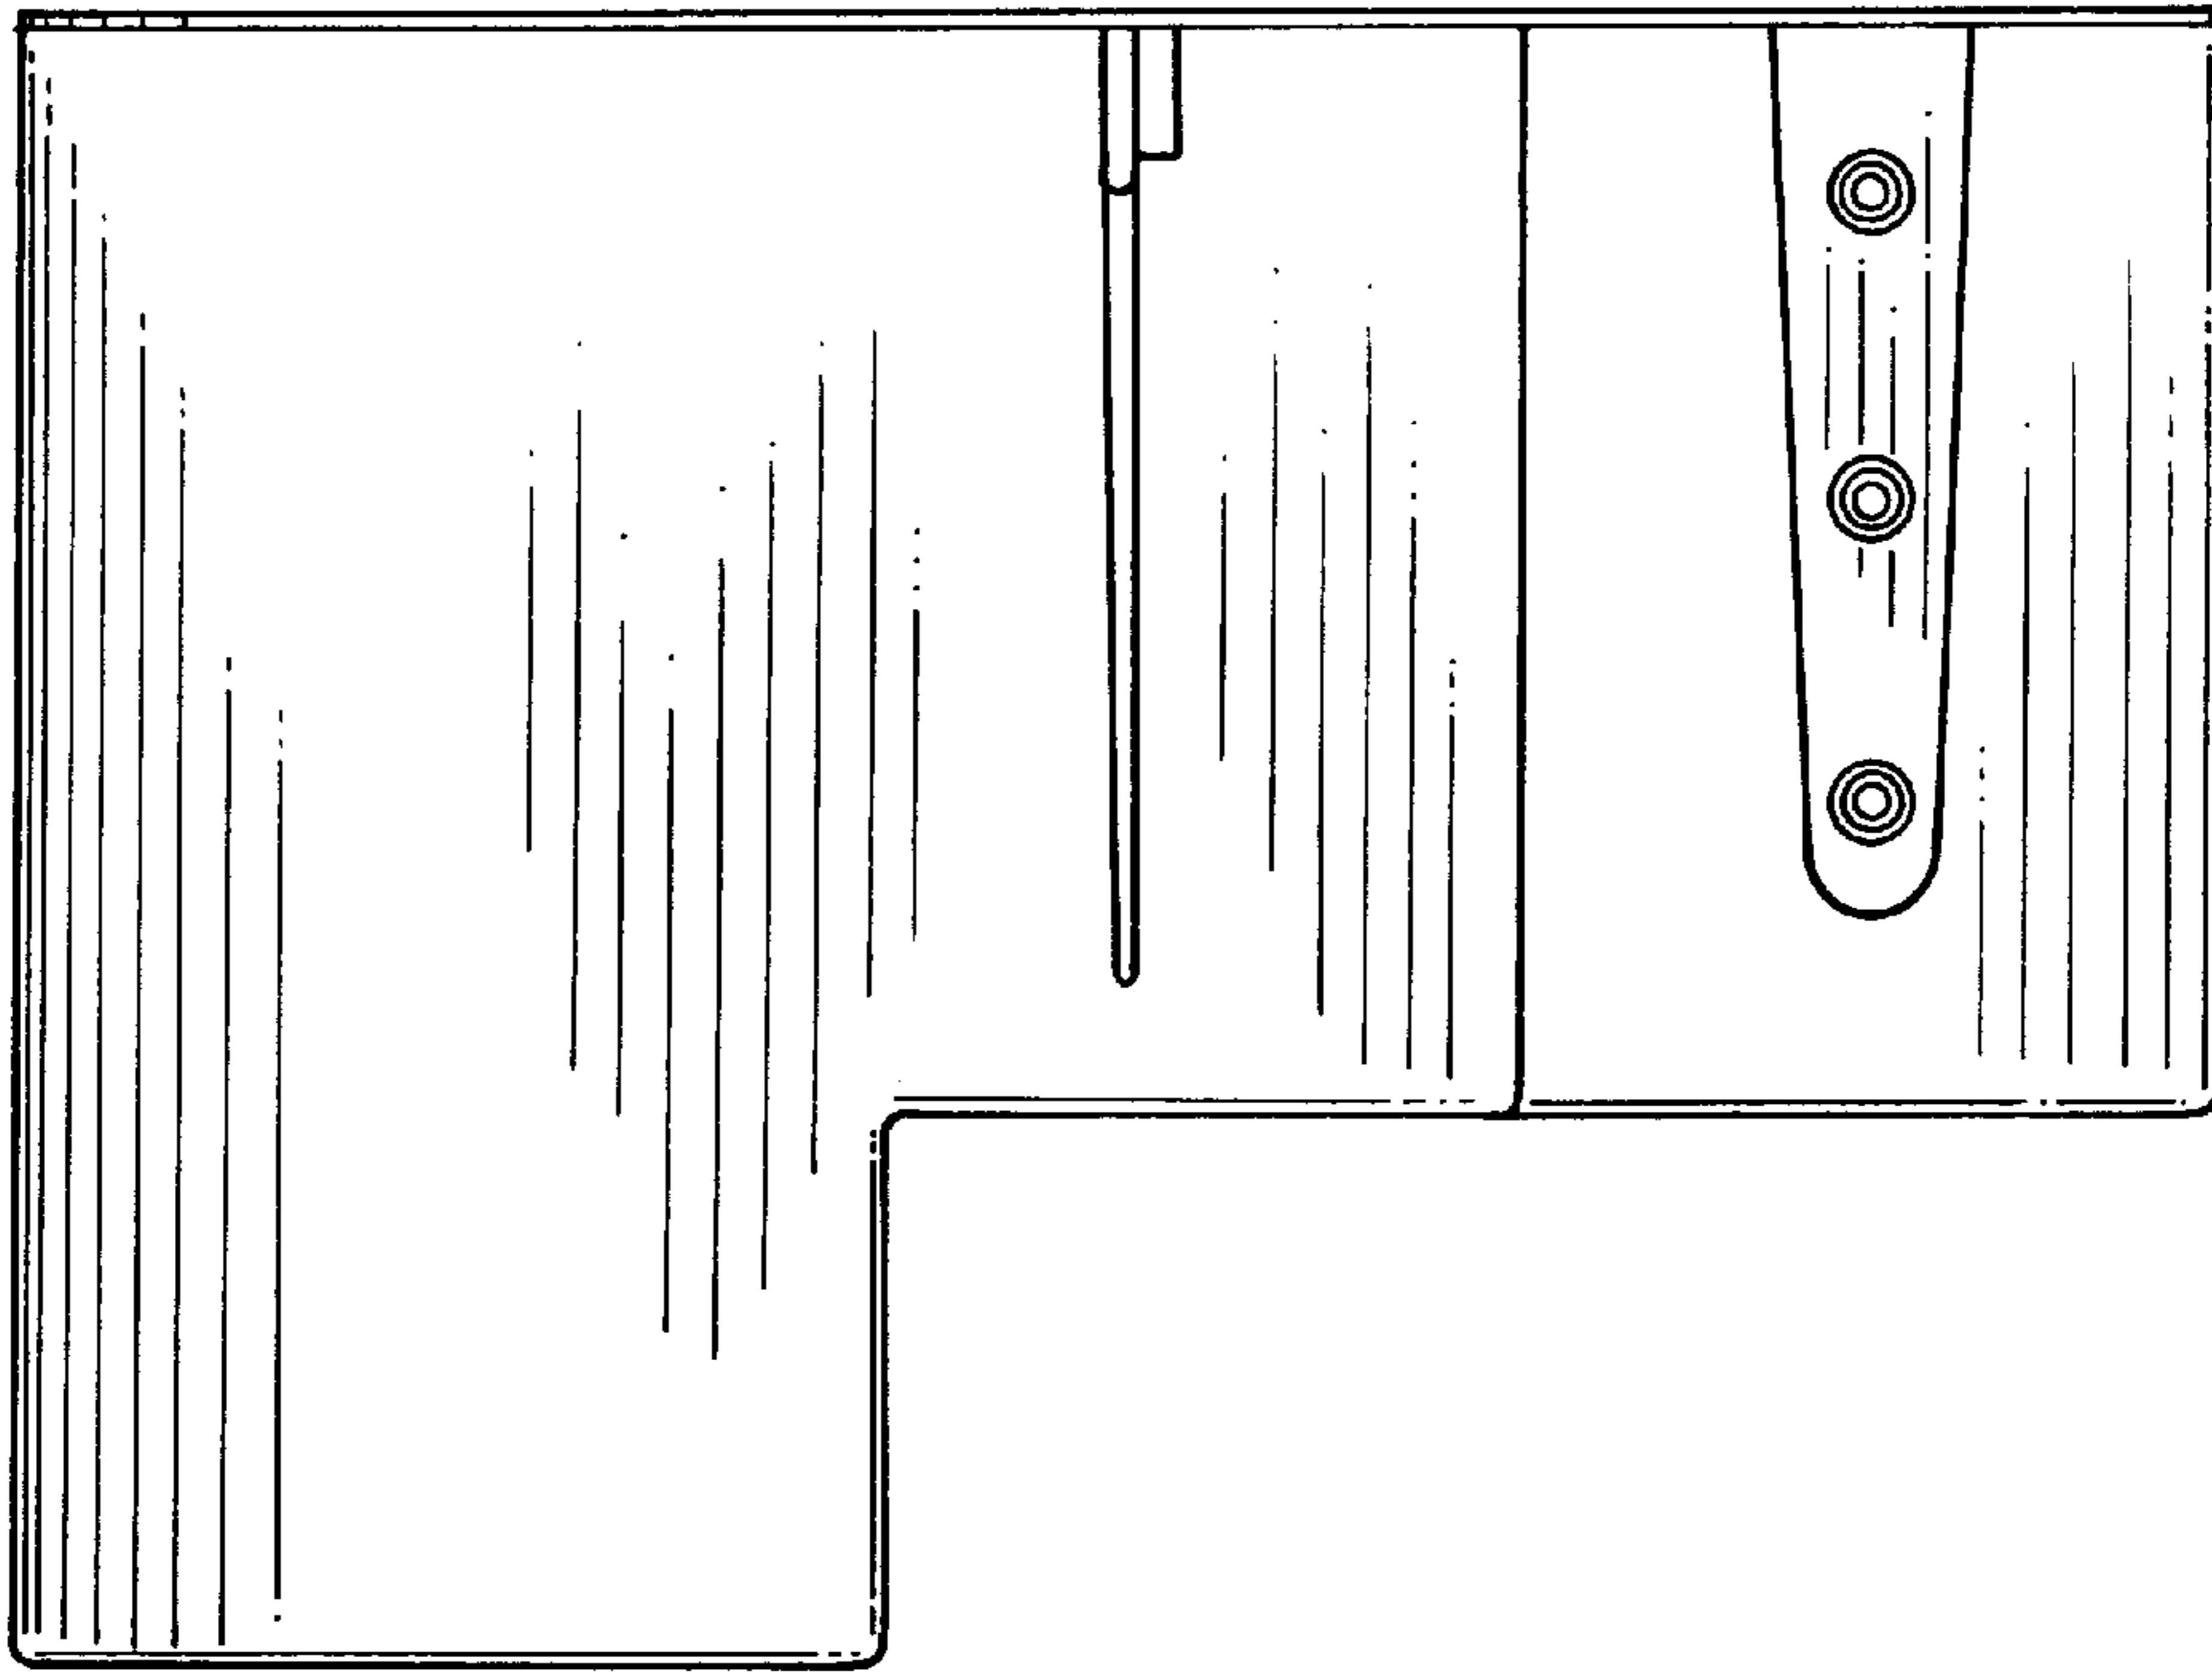


FIG. 2

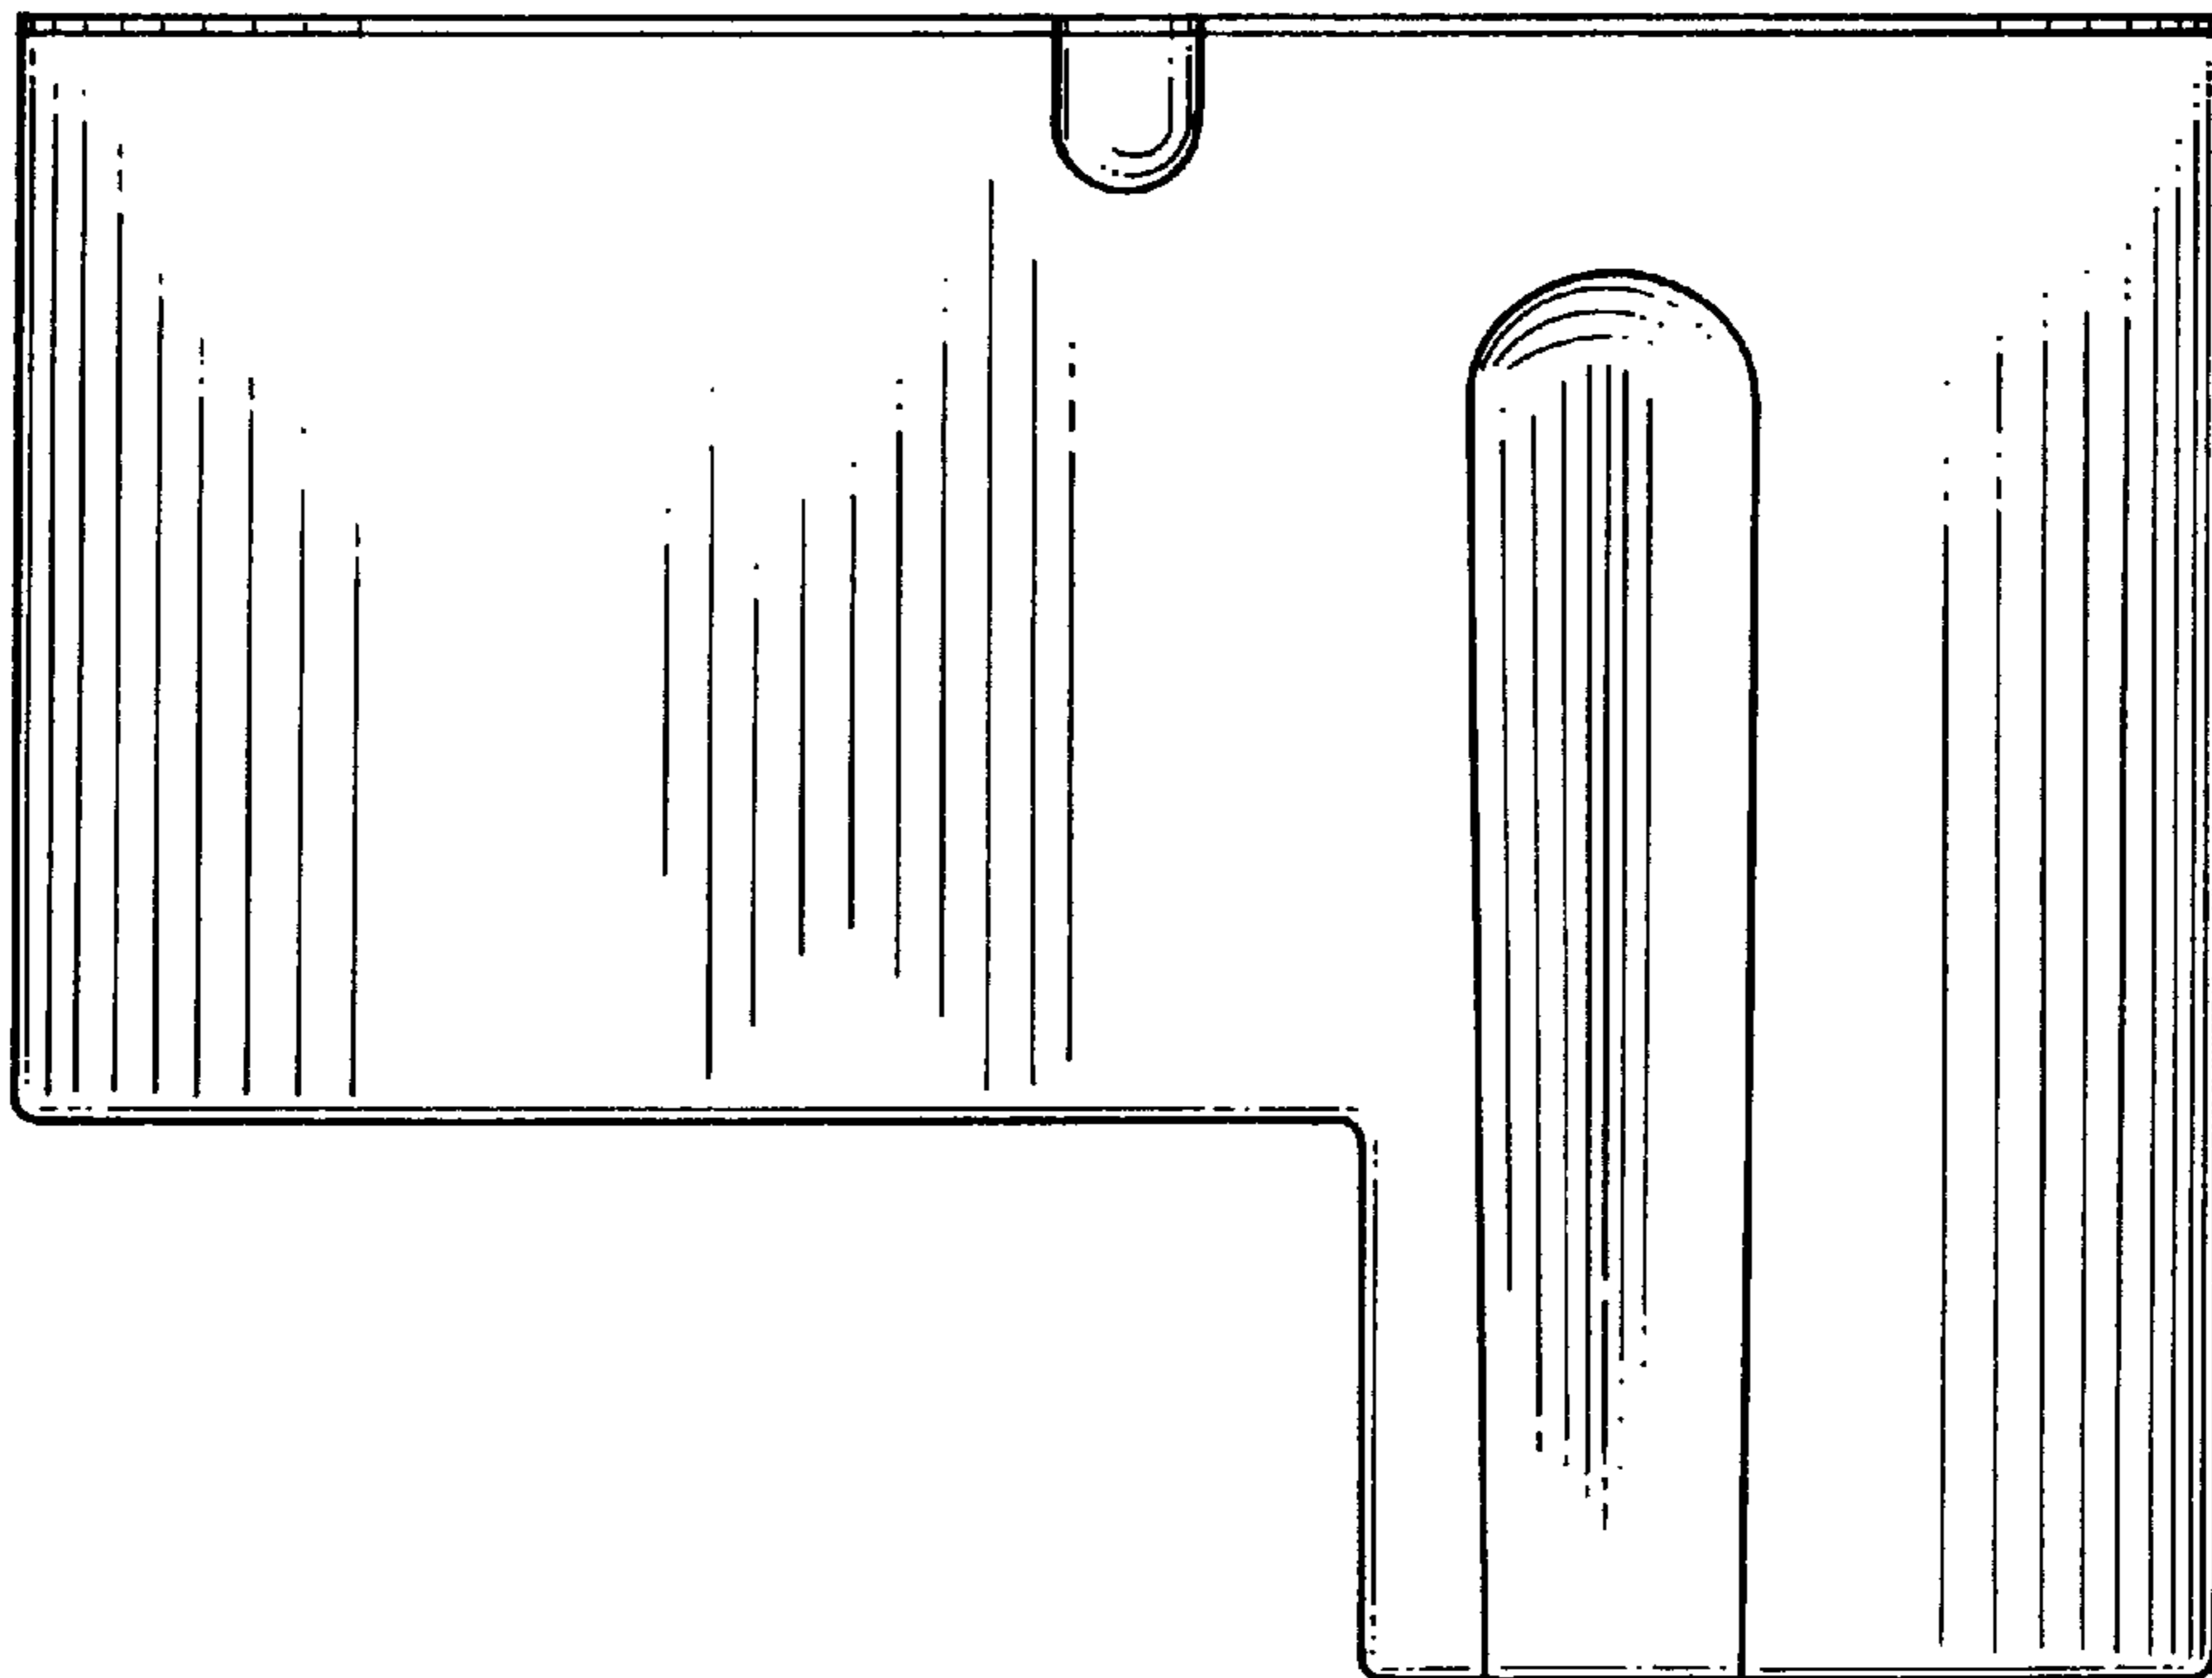


FIG. 3

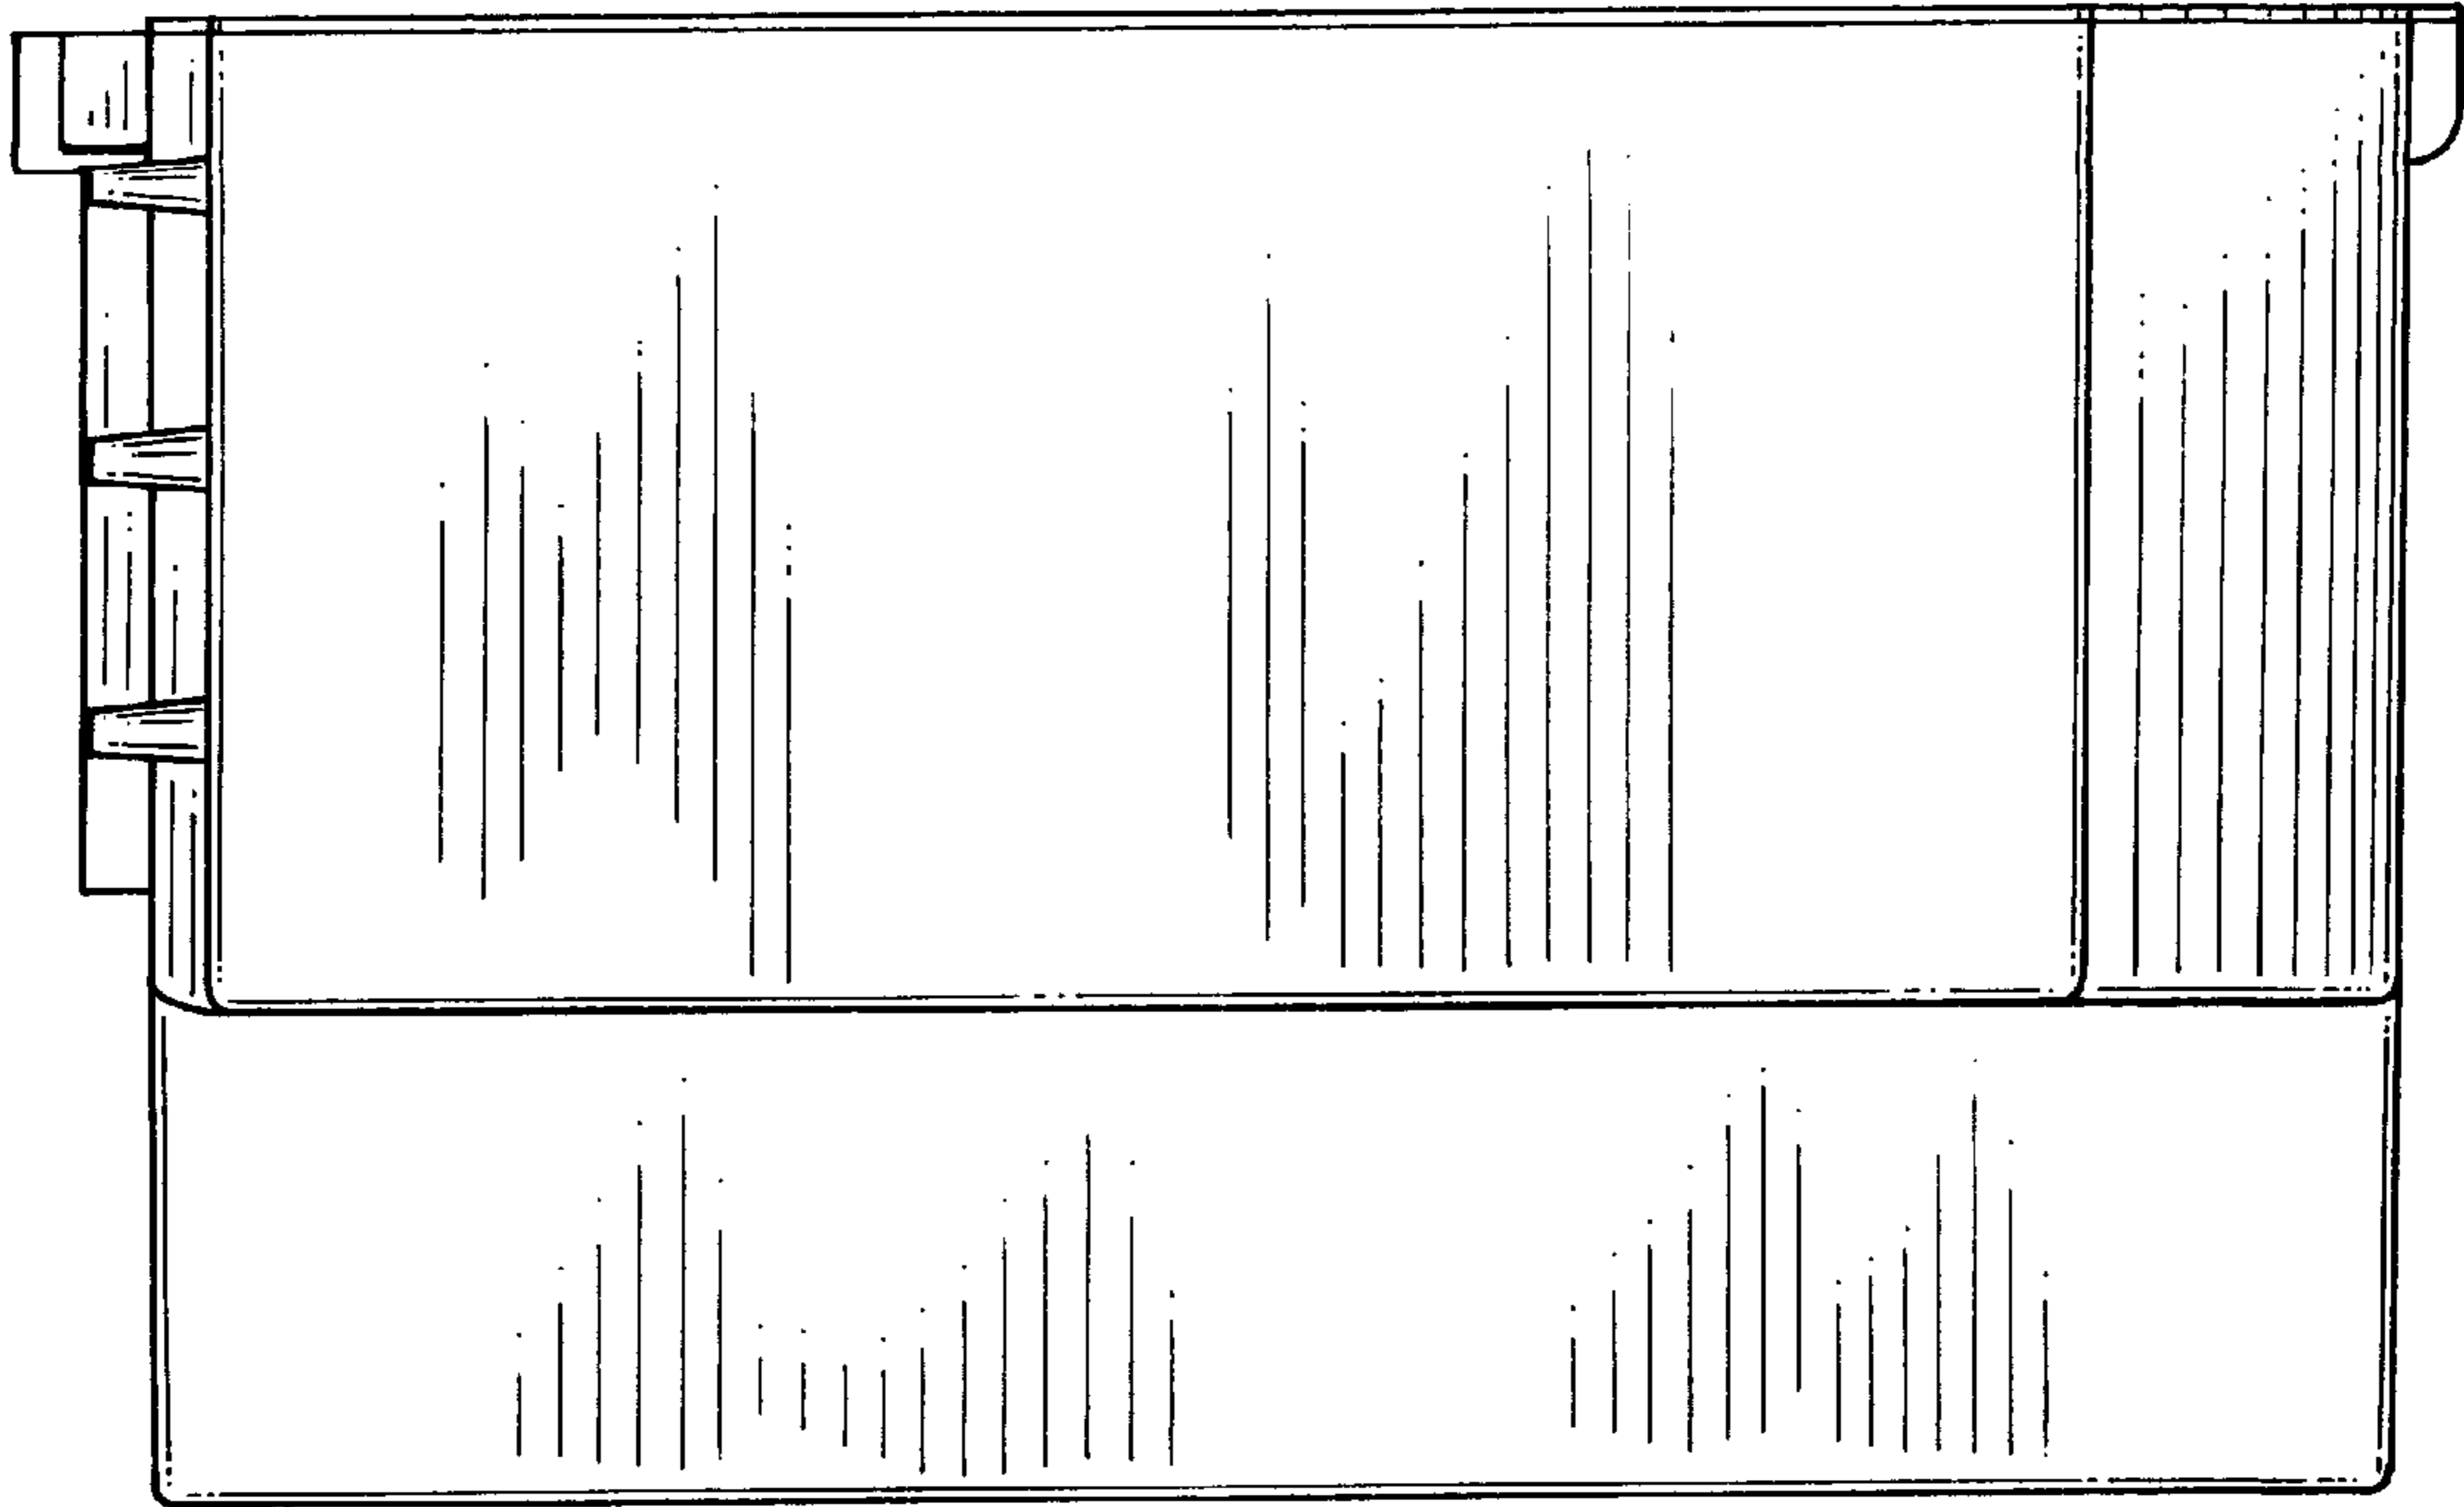


FIG. 4

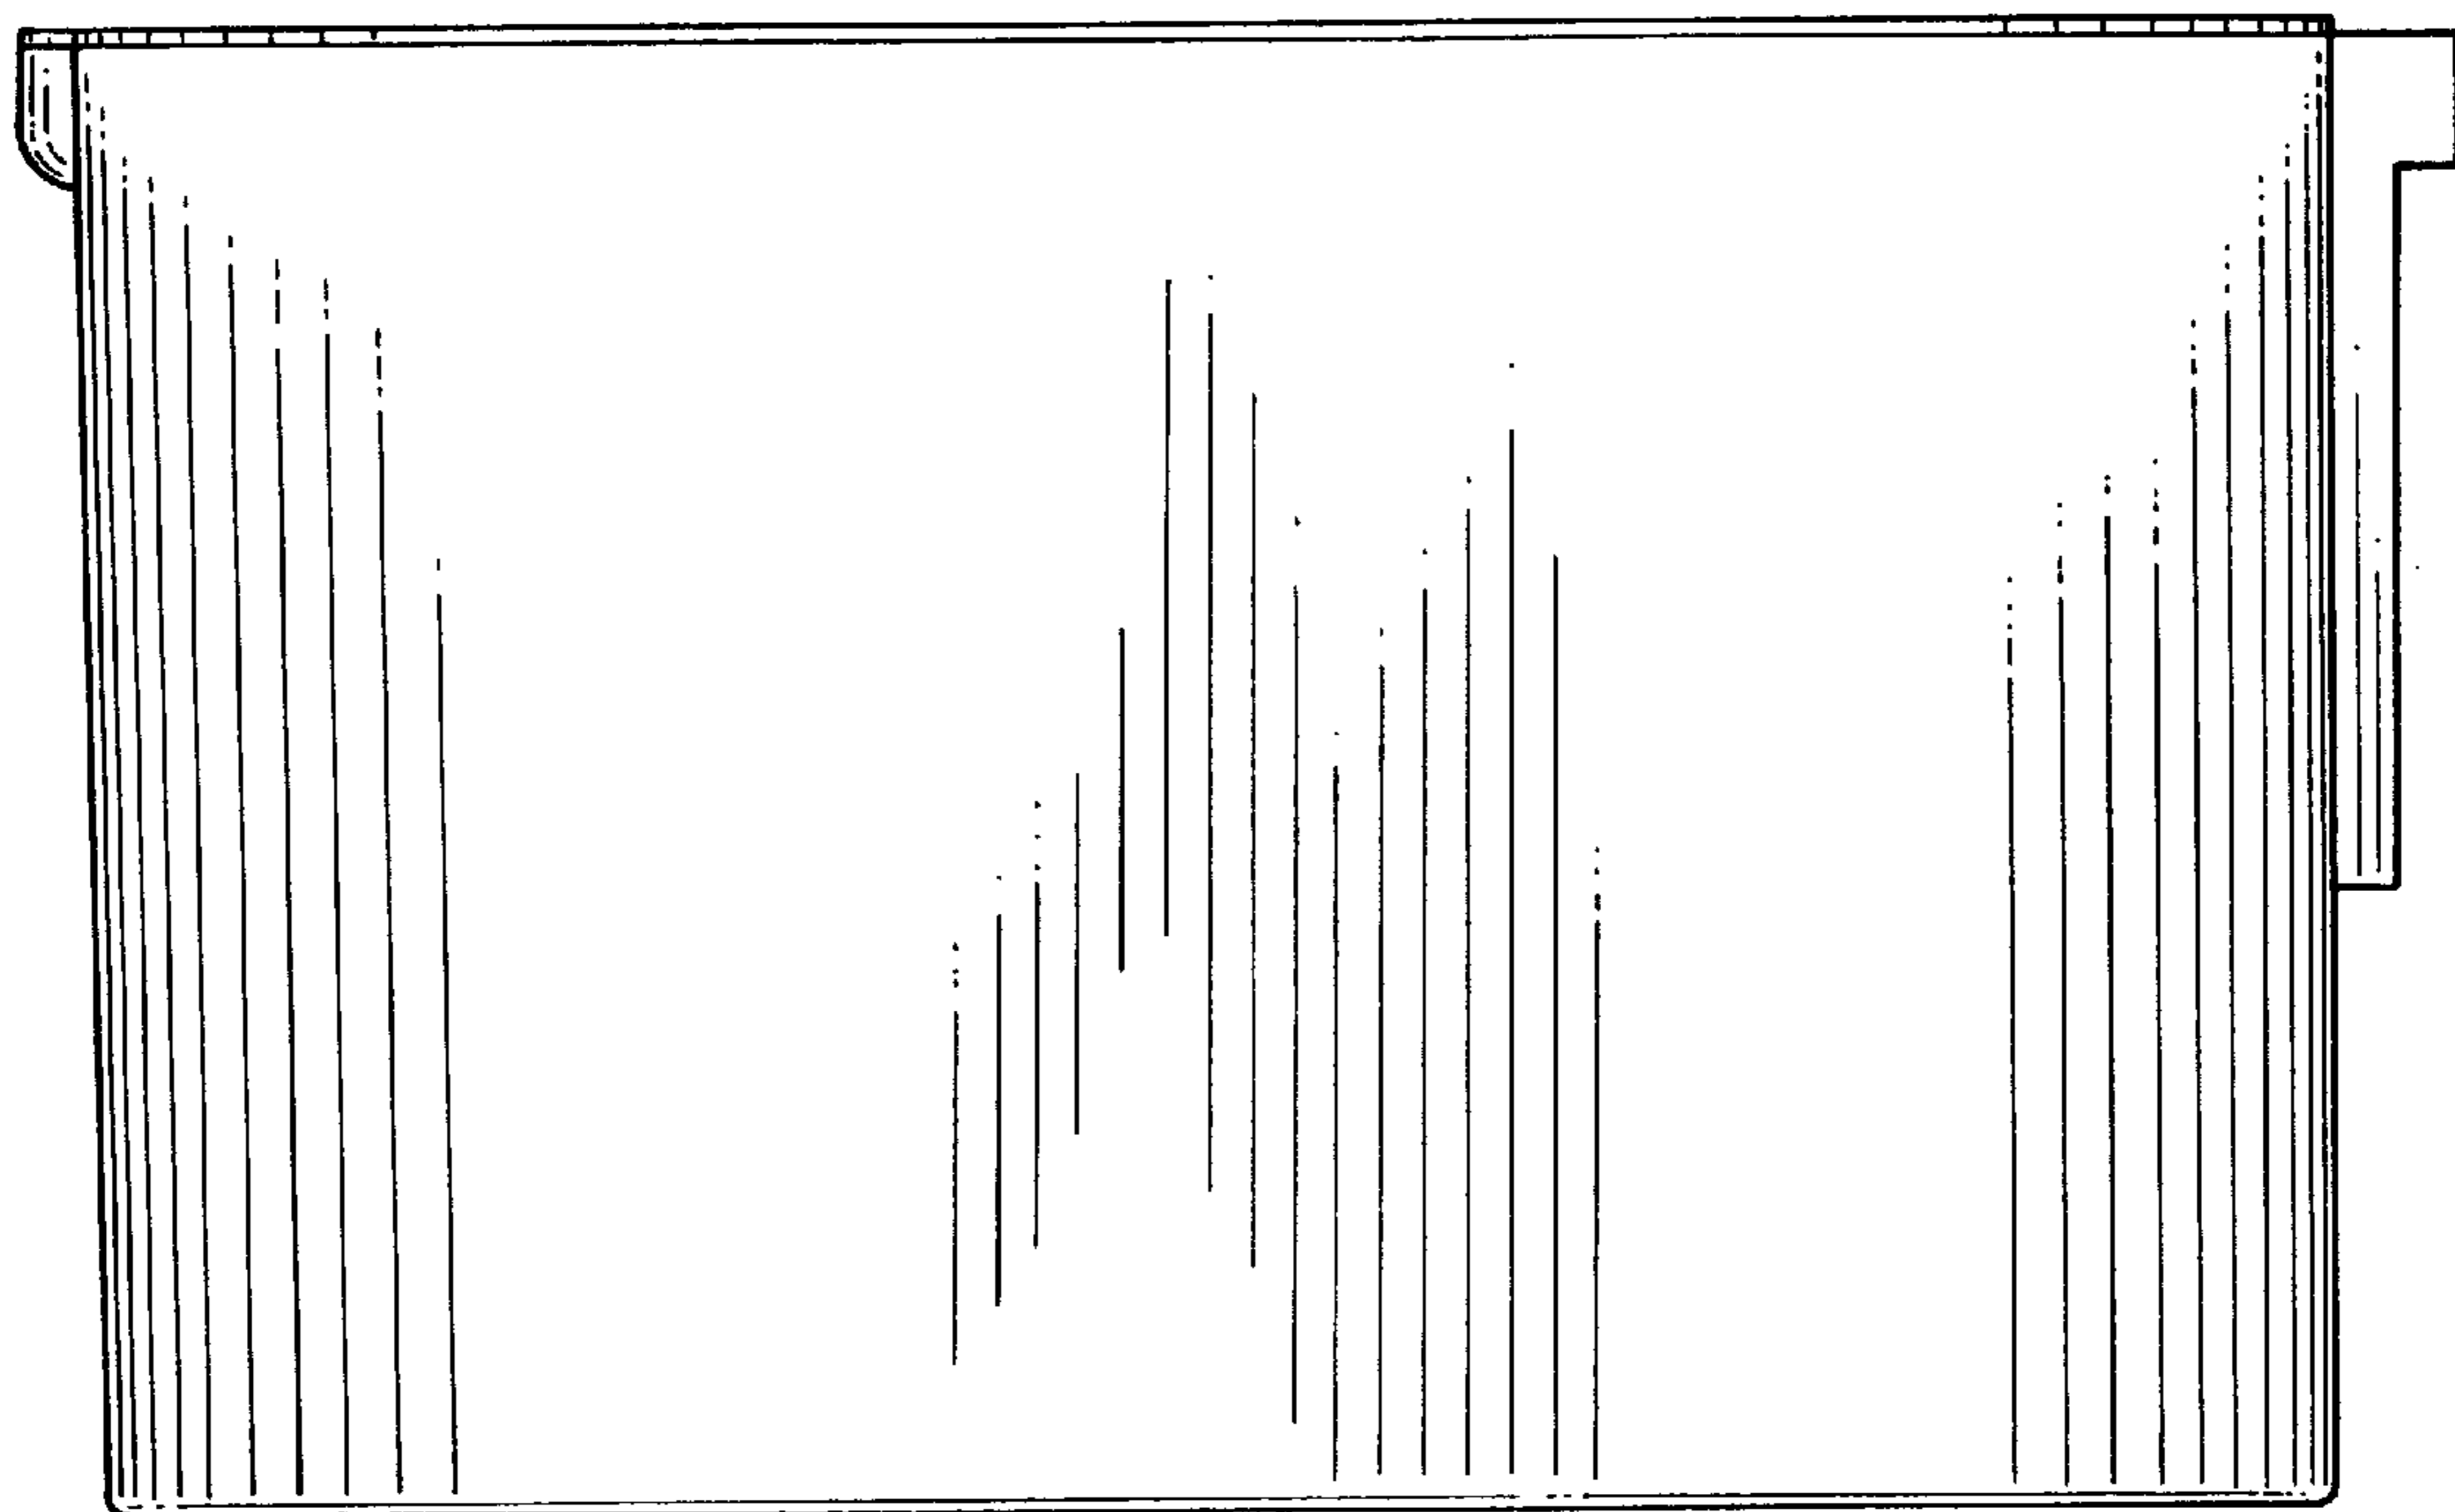


FIG. 5

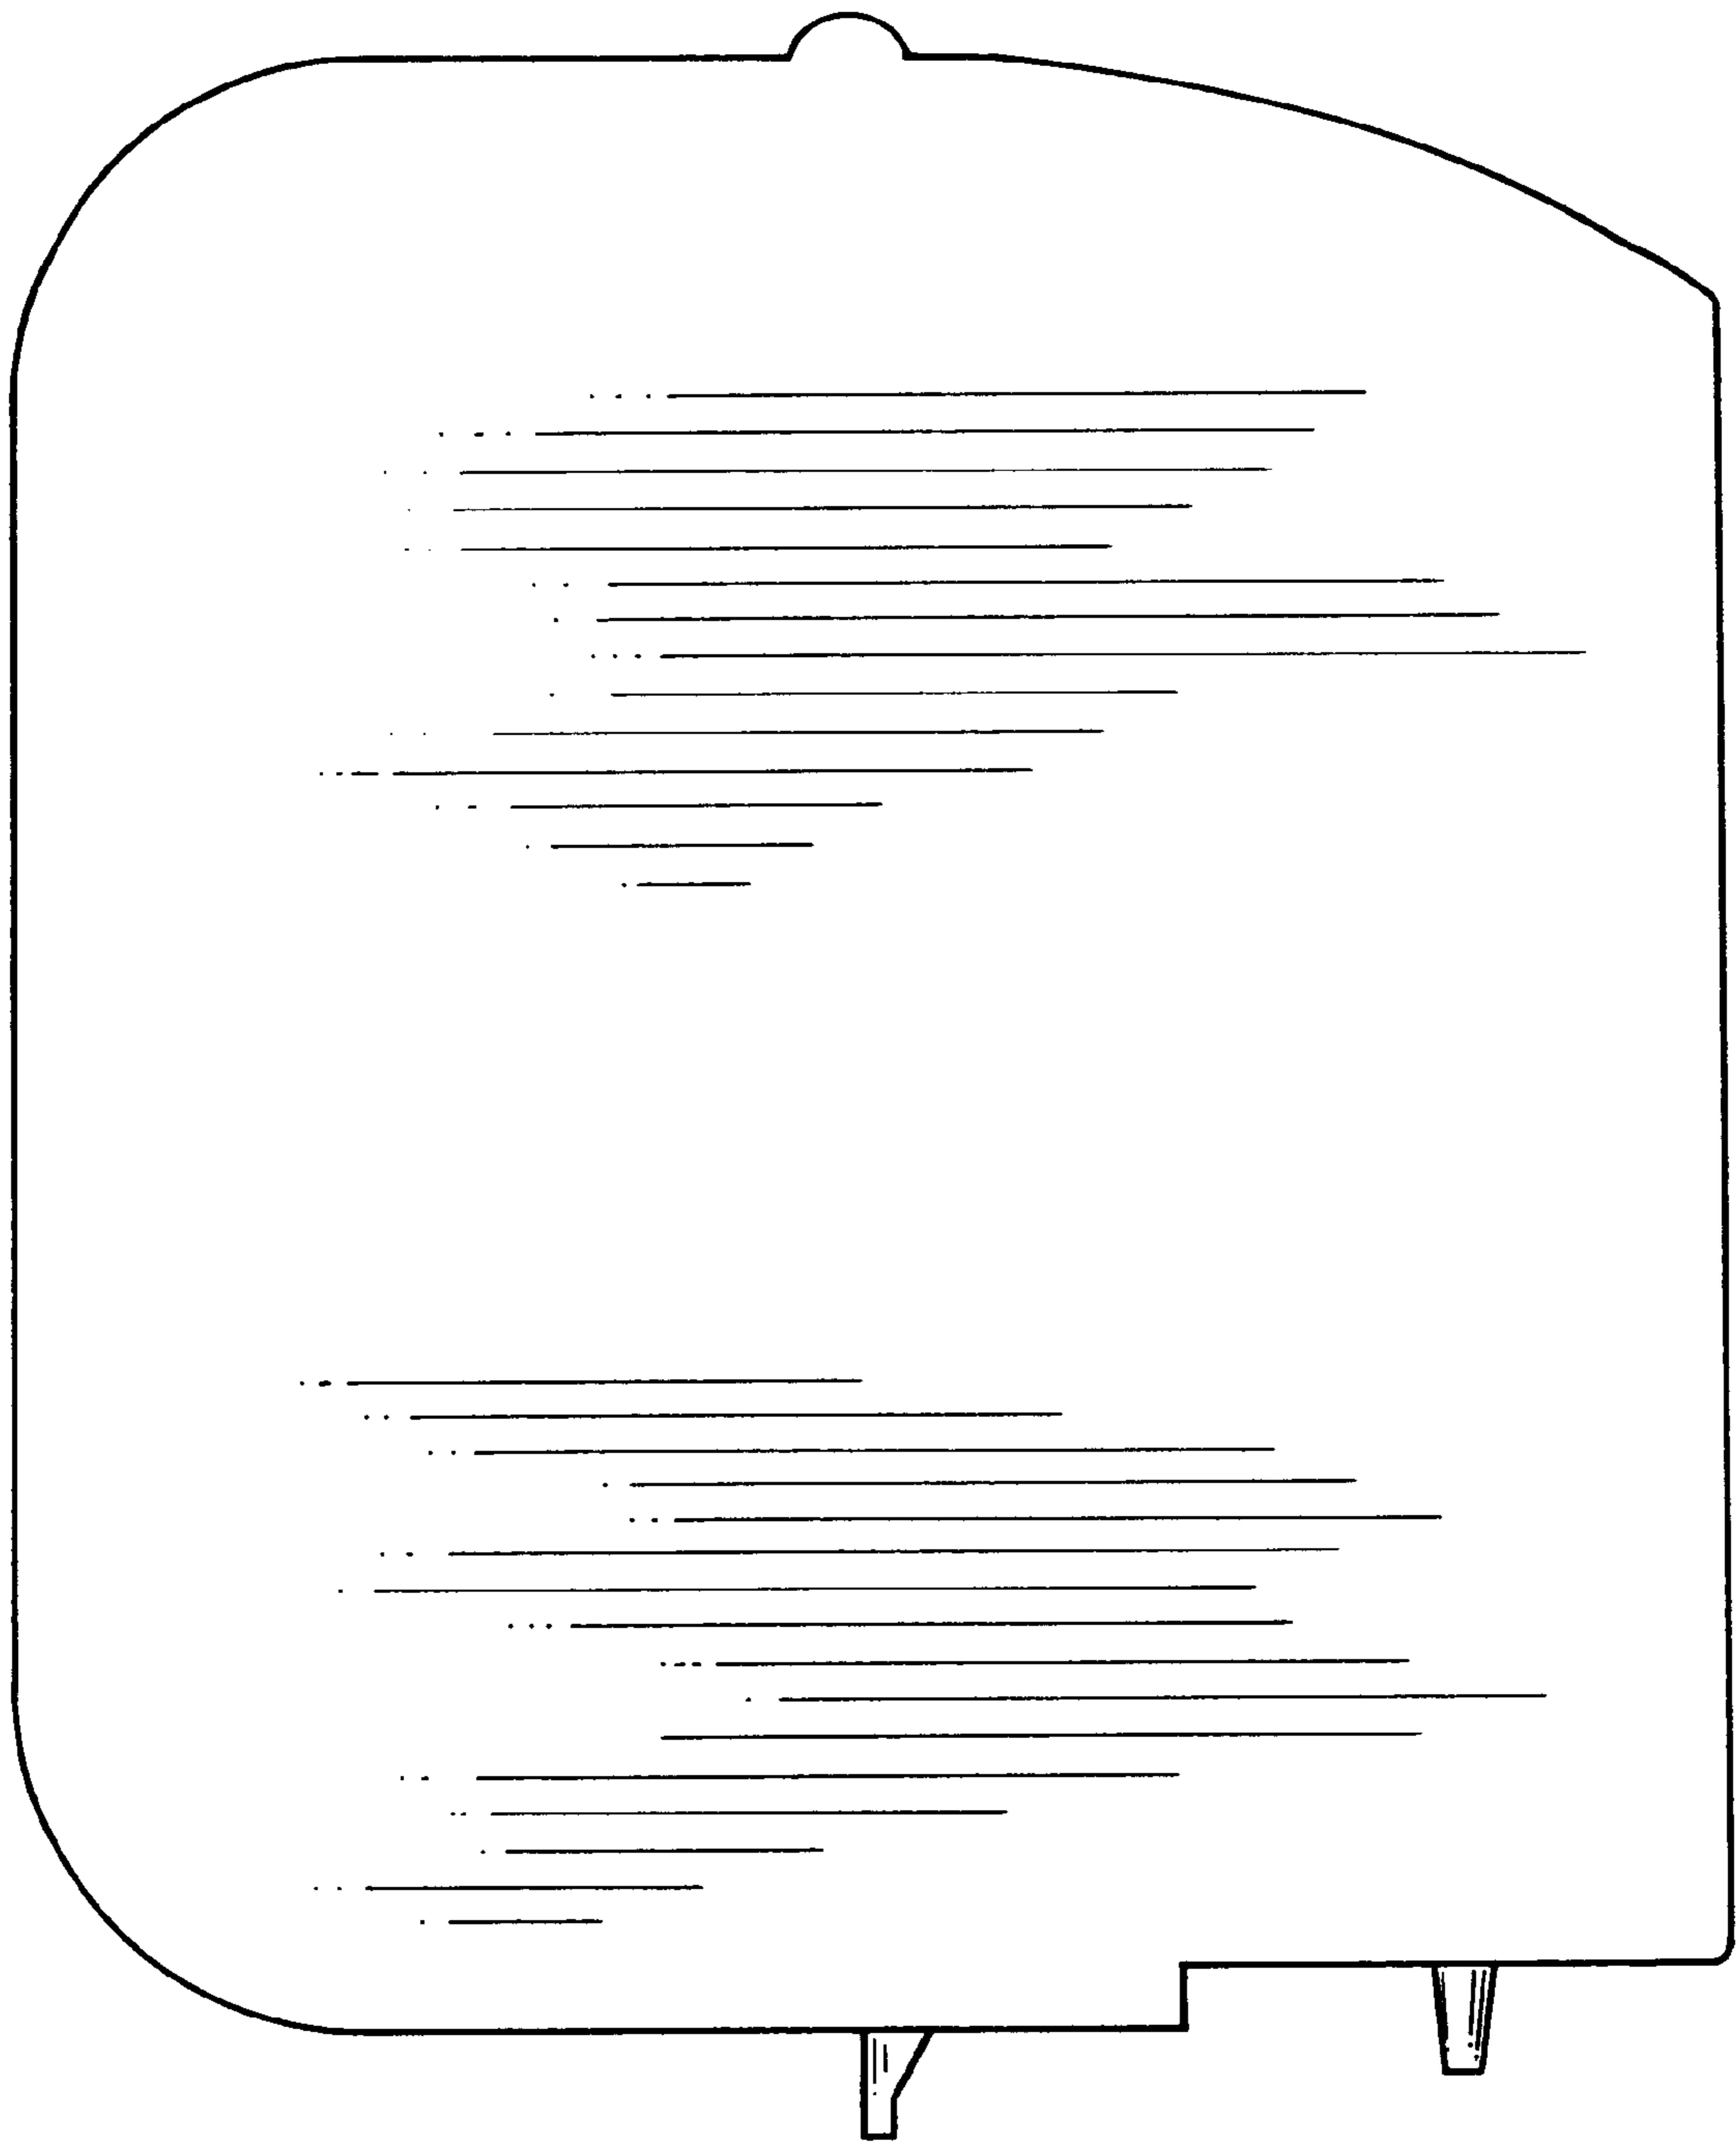


FIG. 6

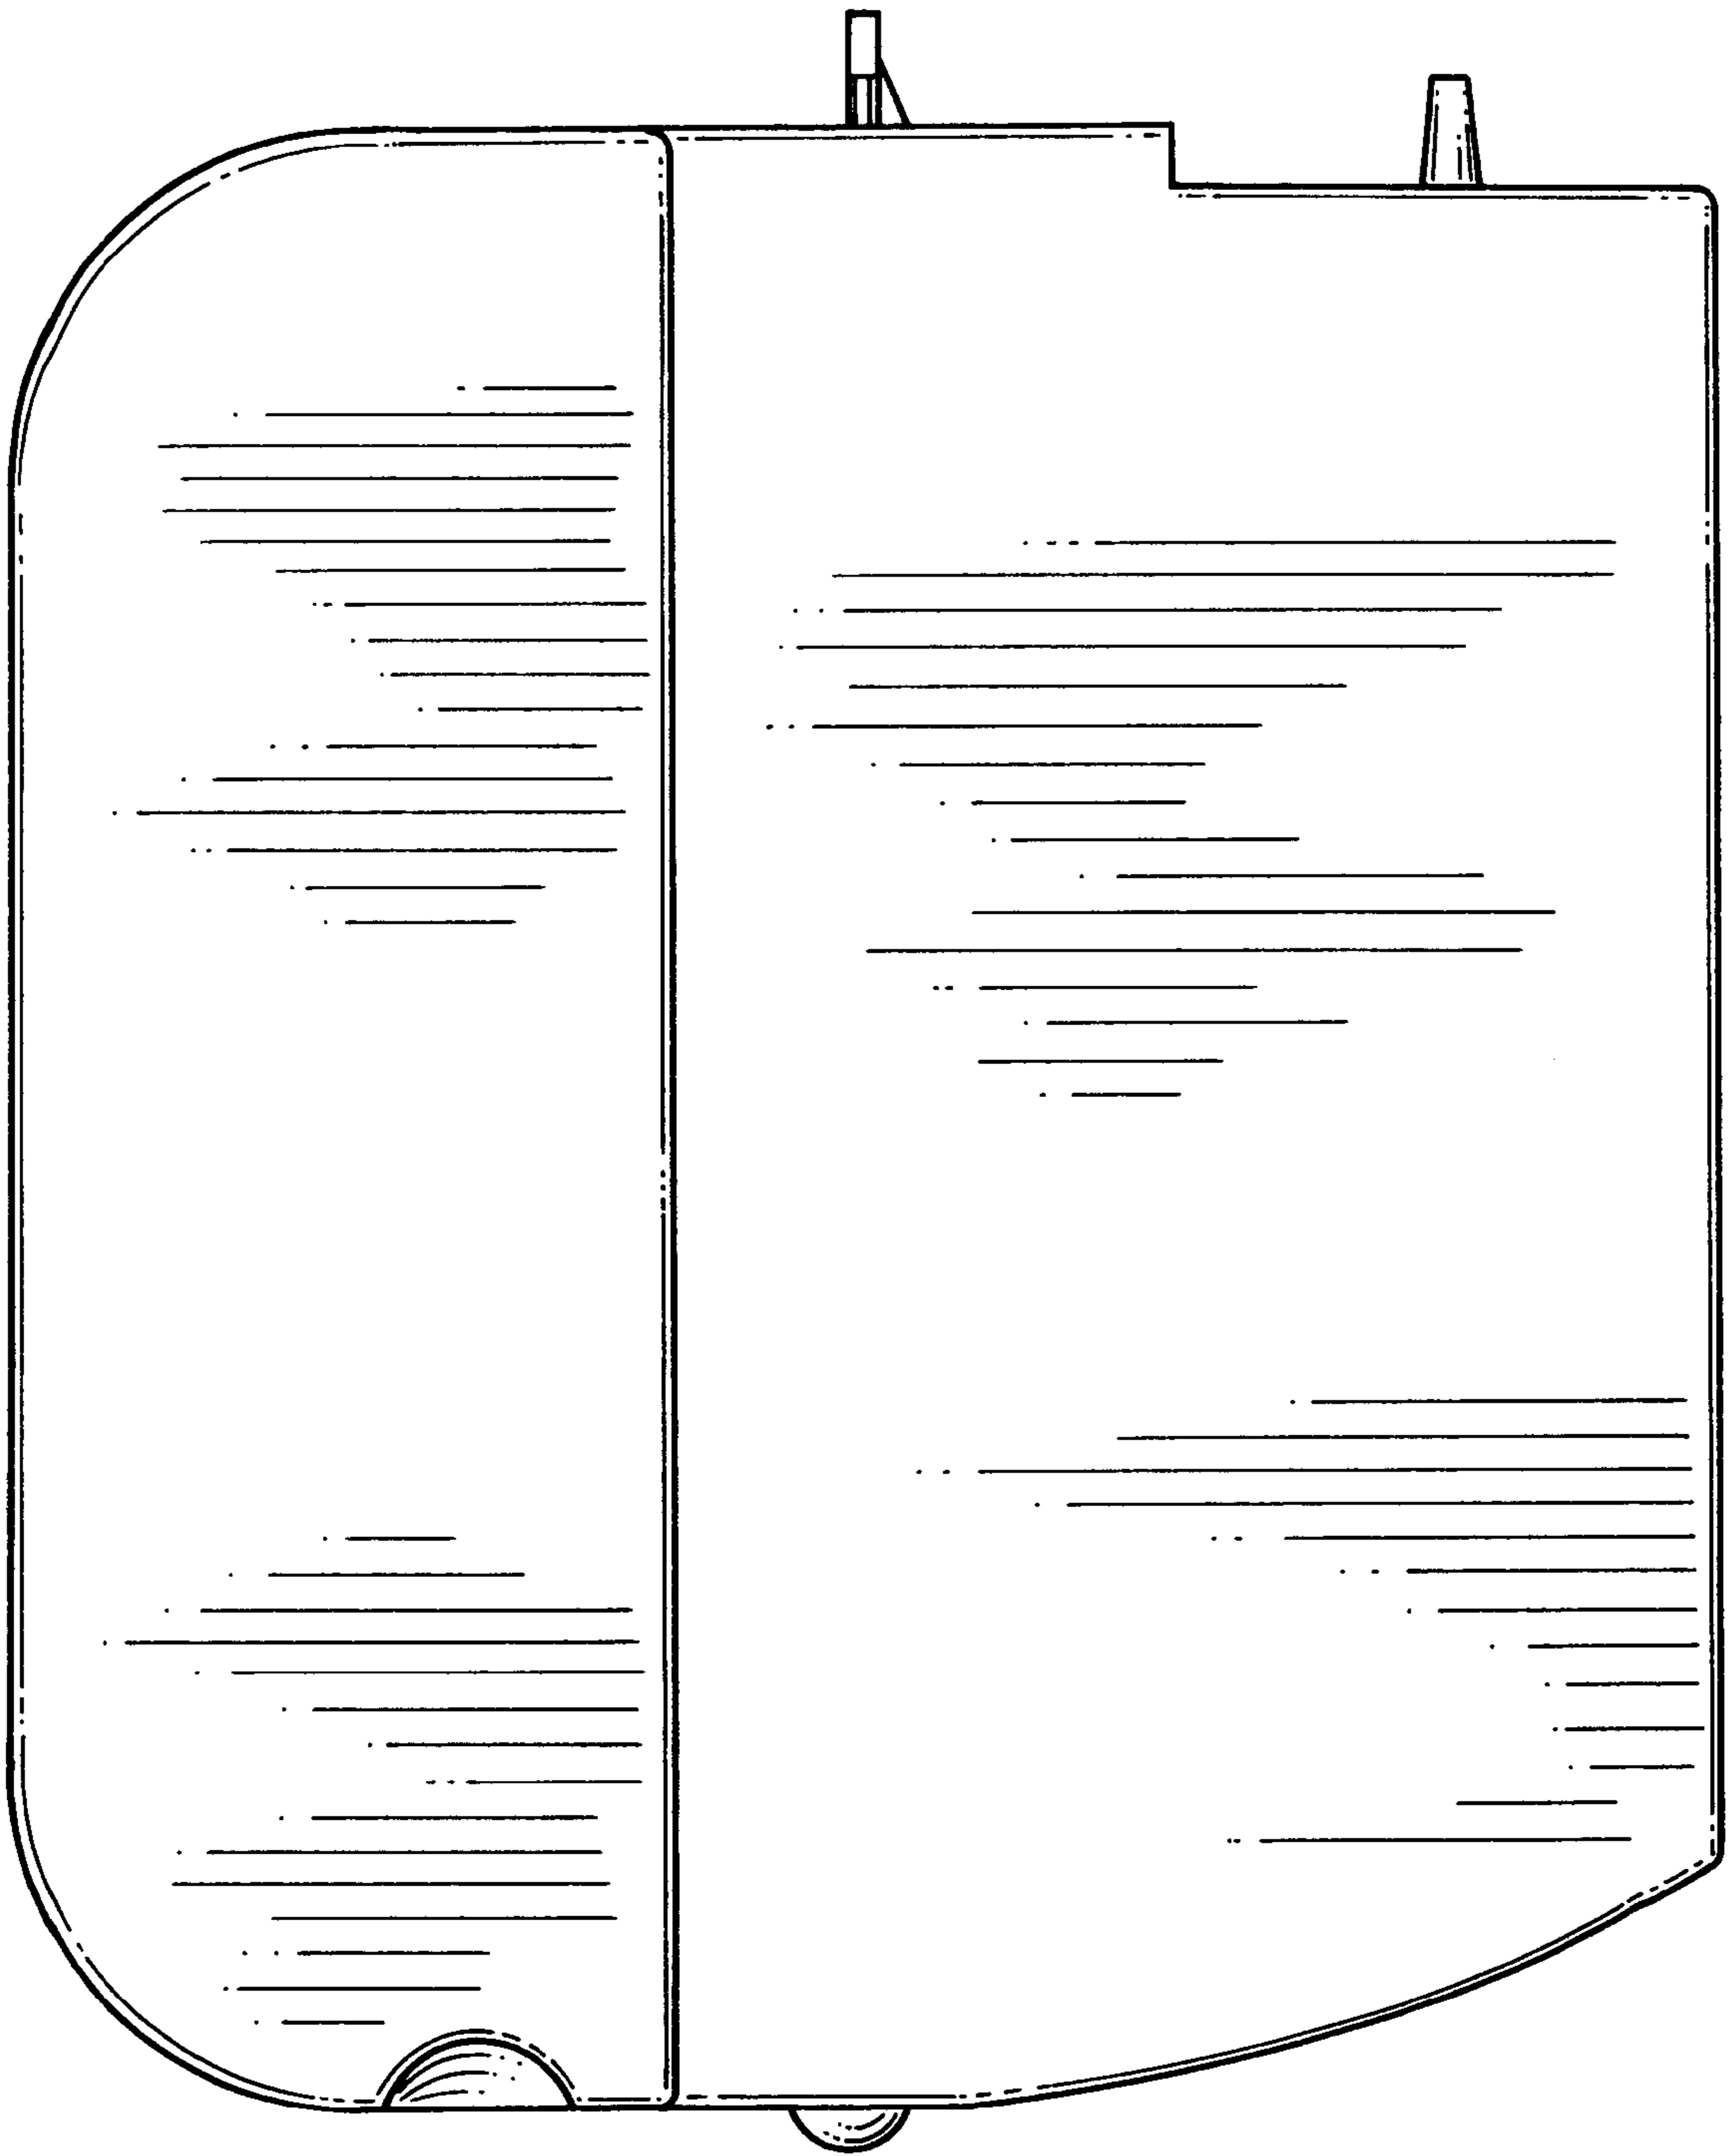


FIG. 7

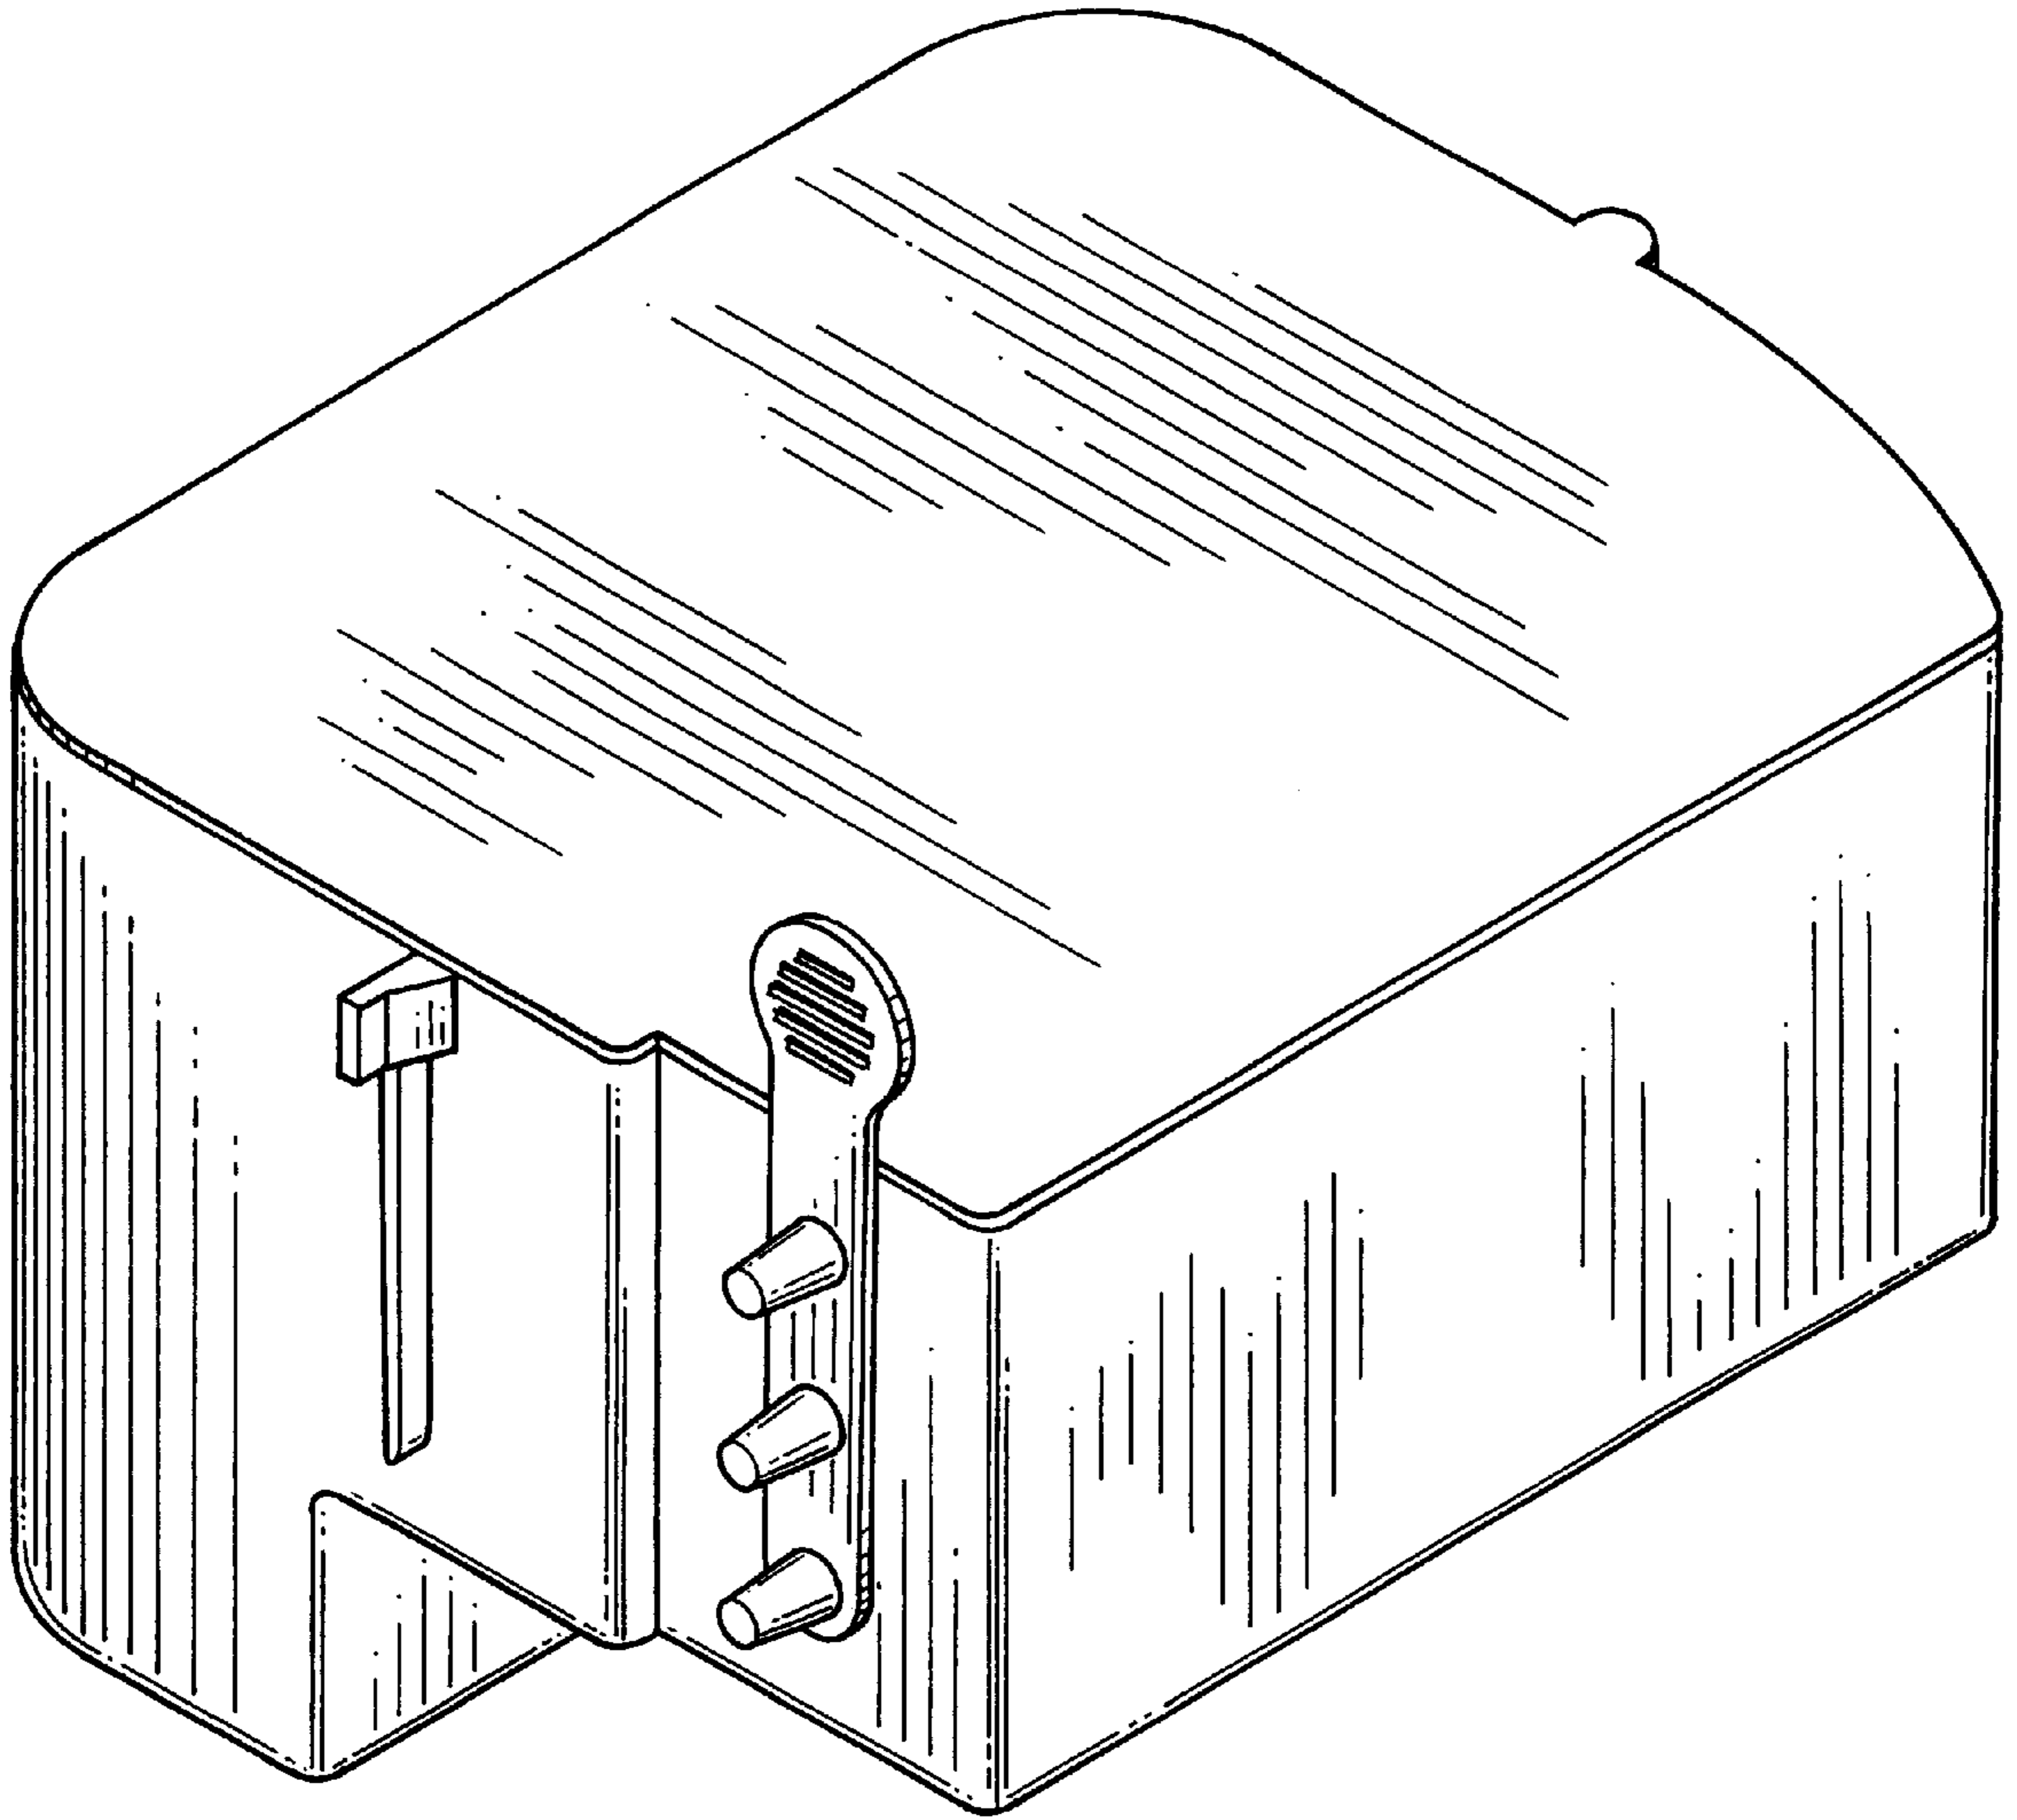


FIG. 8