



US00D446861B1

(12) **United States Design Patent**
Mezière et al.

(10) **Patent No.:** **US D446,861 S**

(45) **Date of Patent:** **** Aug. 21, 2001**

(54) **DIALYSIS MONITOR**

(75) Inventors: **Cyril Mezière**, Bron (FR); **Vicenzo Baraldi**, Quistello; **Marco Paraluppi**, Medolla, both of (IT)

(73) Assignee: **Hospal AG**, Basel (CH)

(**) Term: **14 Years**

(21) Appl. No.: **29/133,140**

(22) Filed: **Nov. 21, 2000**

(30) **Foreign Application Priority Data**

May 22, 2000 (XH) DM/051905

(51) **LOC (7) Cl.** **24-01**

(52) **U.S. Cl.** **D24/169**

(58) **Field of Search** D24/169; 600/473, 600/475, 476; 604/29, 34, 83, 66; 210/646, 645, 321.71, 321.65

(56) **References Cited**

U.S. PATENT DOCUMENTS

- D. 383,842 * 9/1997 Kenley et al. D24/169
- D. 389,916 * 1/1998 DiPerna et al. D24/169
- D. 406,894 3/1999 Menhennett et al. .

- 4,381,003 * 4/1983 Buoncristiani 604/29
- 4,585,436 * 4/1986 Davis et al. 604/29
- 4,756,706 * 7/1988 Kerns et al. 604/66
- 5,326,476 7/1994 Grogan et al. .

OTHER PUBLICATIONS

Cordis Dow Corp, Seratron Brochure "Seratron Dialysis Control System," Oct. 1979.

* cited by examiner

Primary Examiner—Stella Reid

(74) *Attorney, Agent, or Firm*—Edna M. O'Connor


(57) **CLAIM**

The ornamental design for a dialysis monitor, substantially as shown and described.

DESCRIPTION

FIG. 1 is a perspective view of a dialysis monitor showing our new design;
 FIG. 2 is a front view thereof;
 FIG. 3 is a rear view thereof;
 FIG. 4 is a side view thereof;
 FIG. 5 is a side view thereof, opposite that shown in FIG. 4;
 FIG. 6 is a top view thereof; and,
 FIG. 7 is a bottom view.

1 Claim, 3 Drawing Sheets

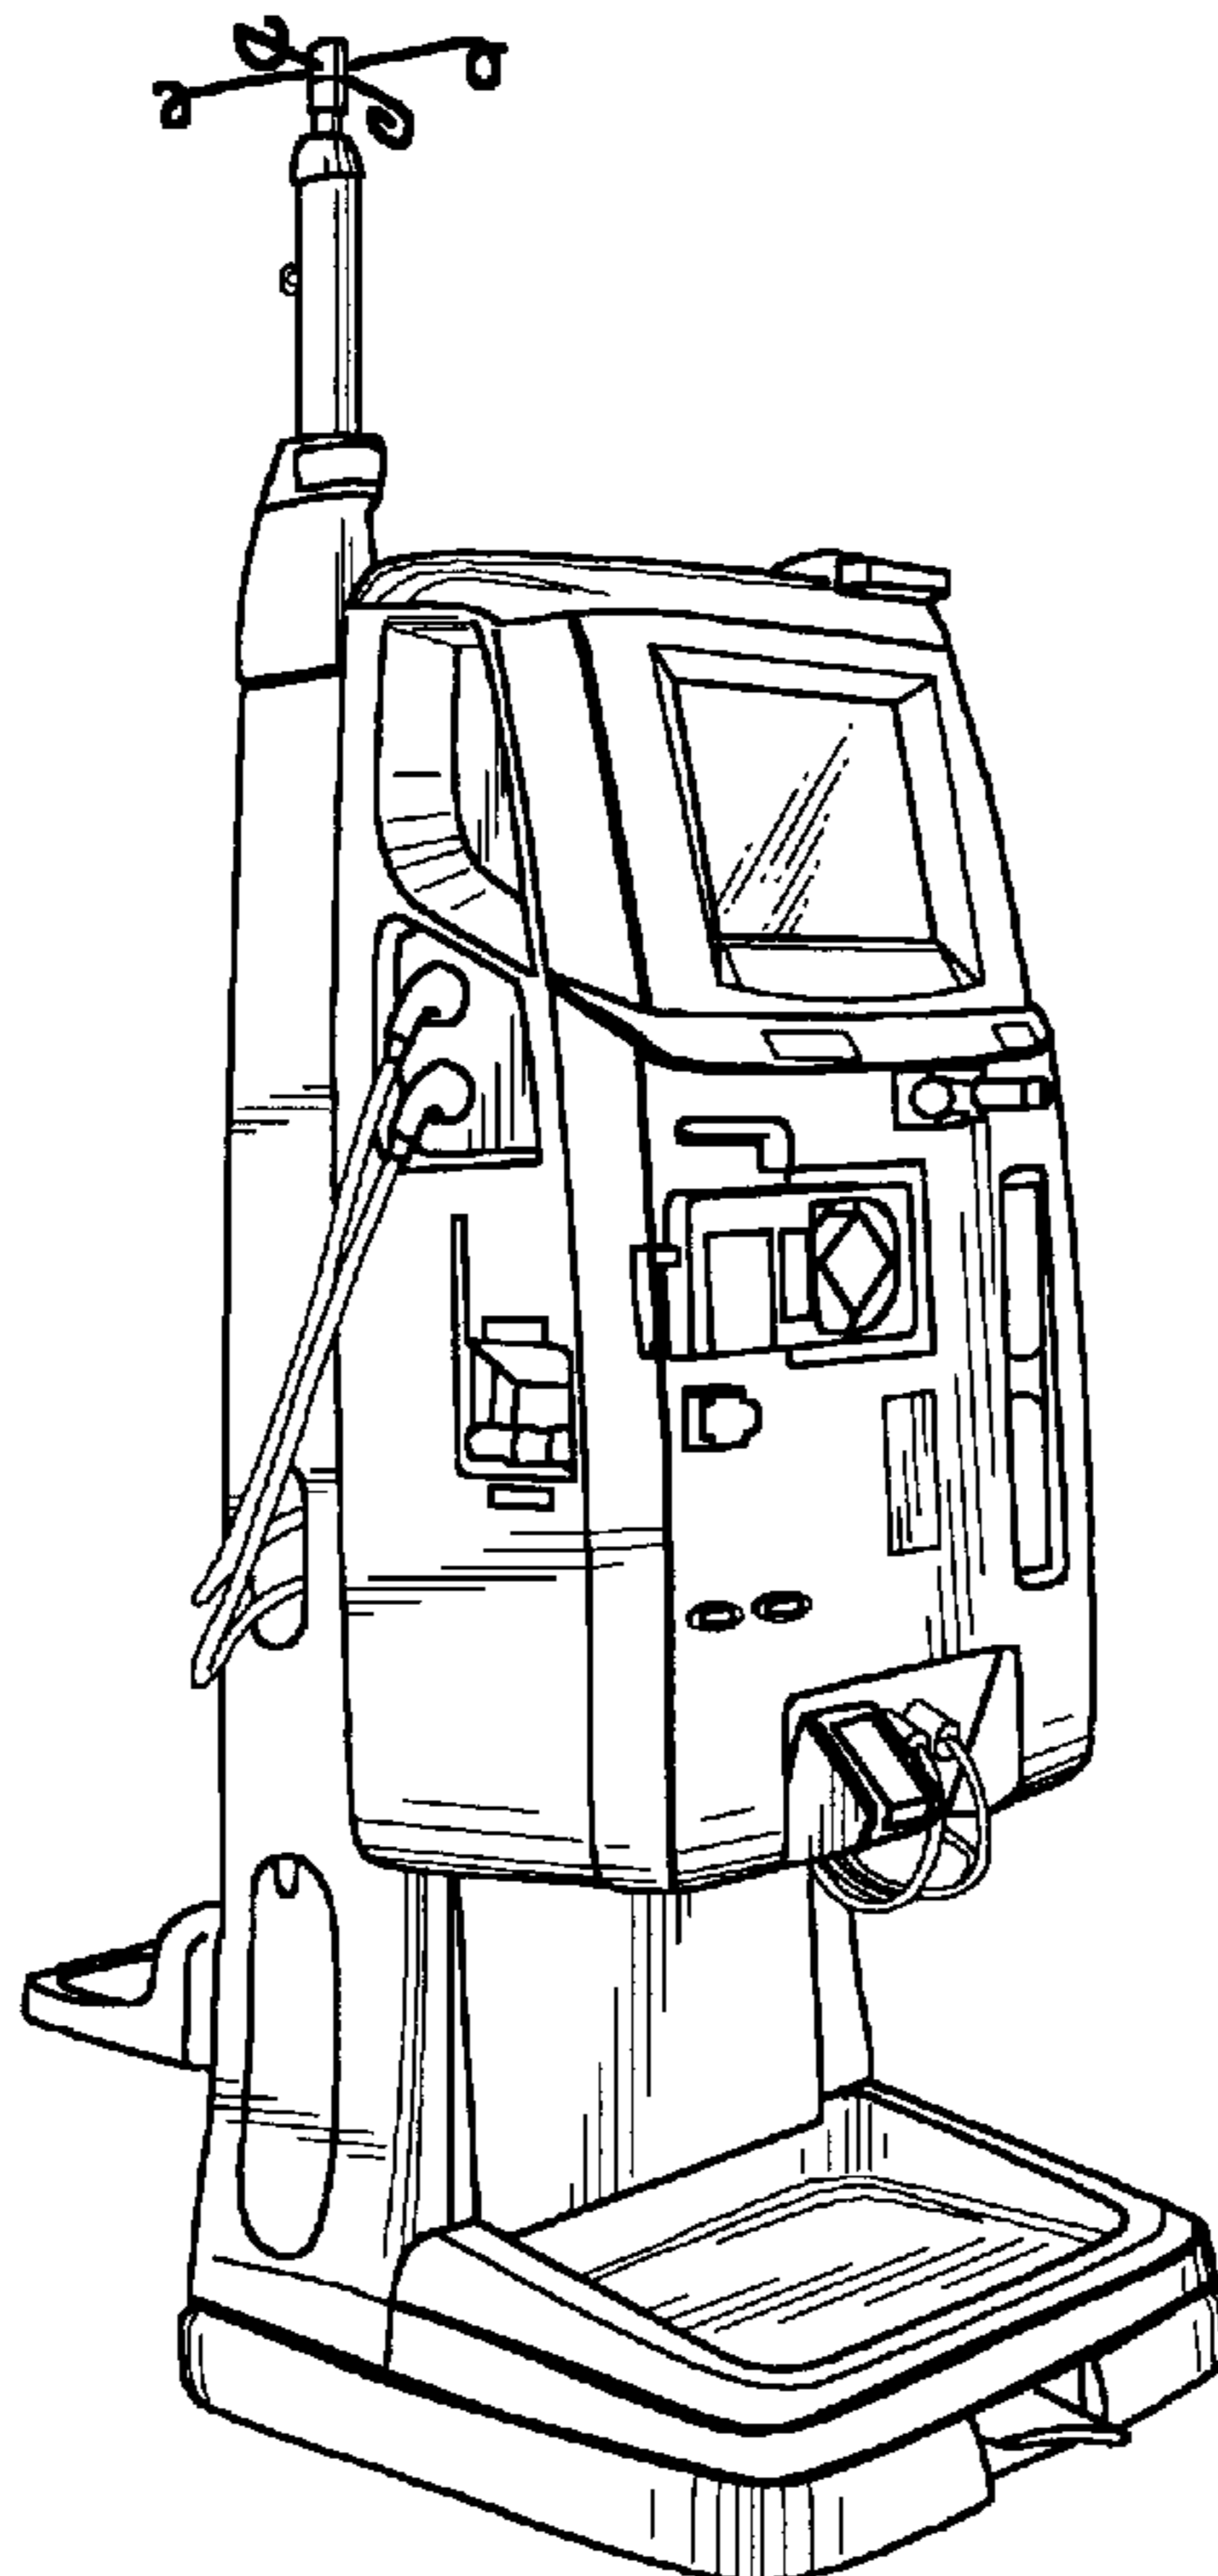

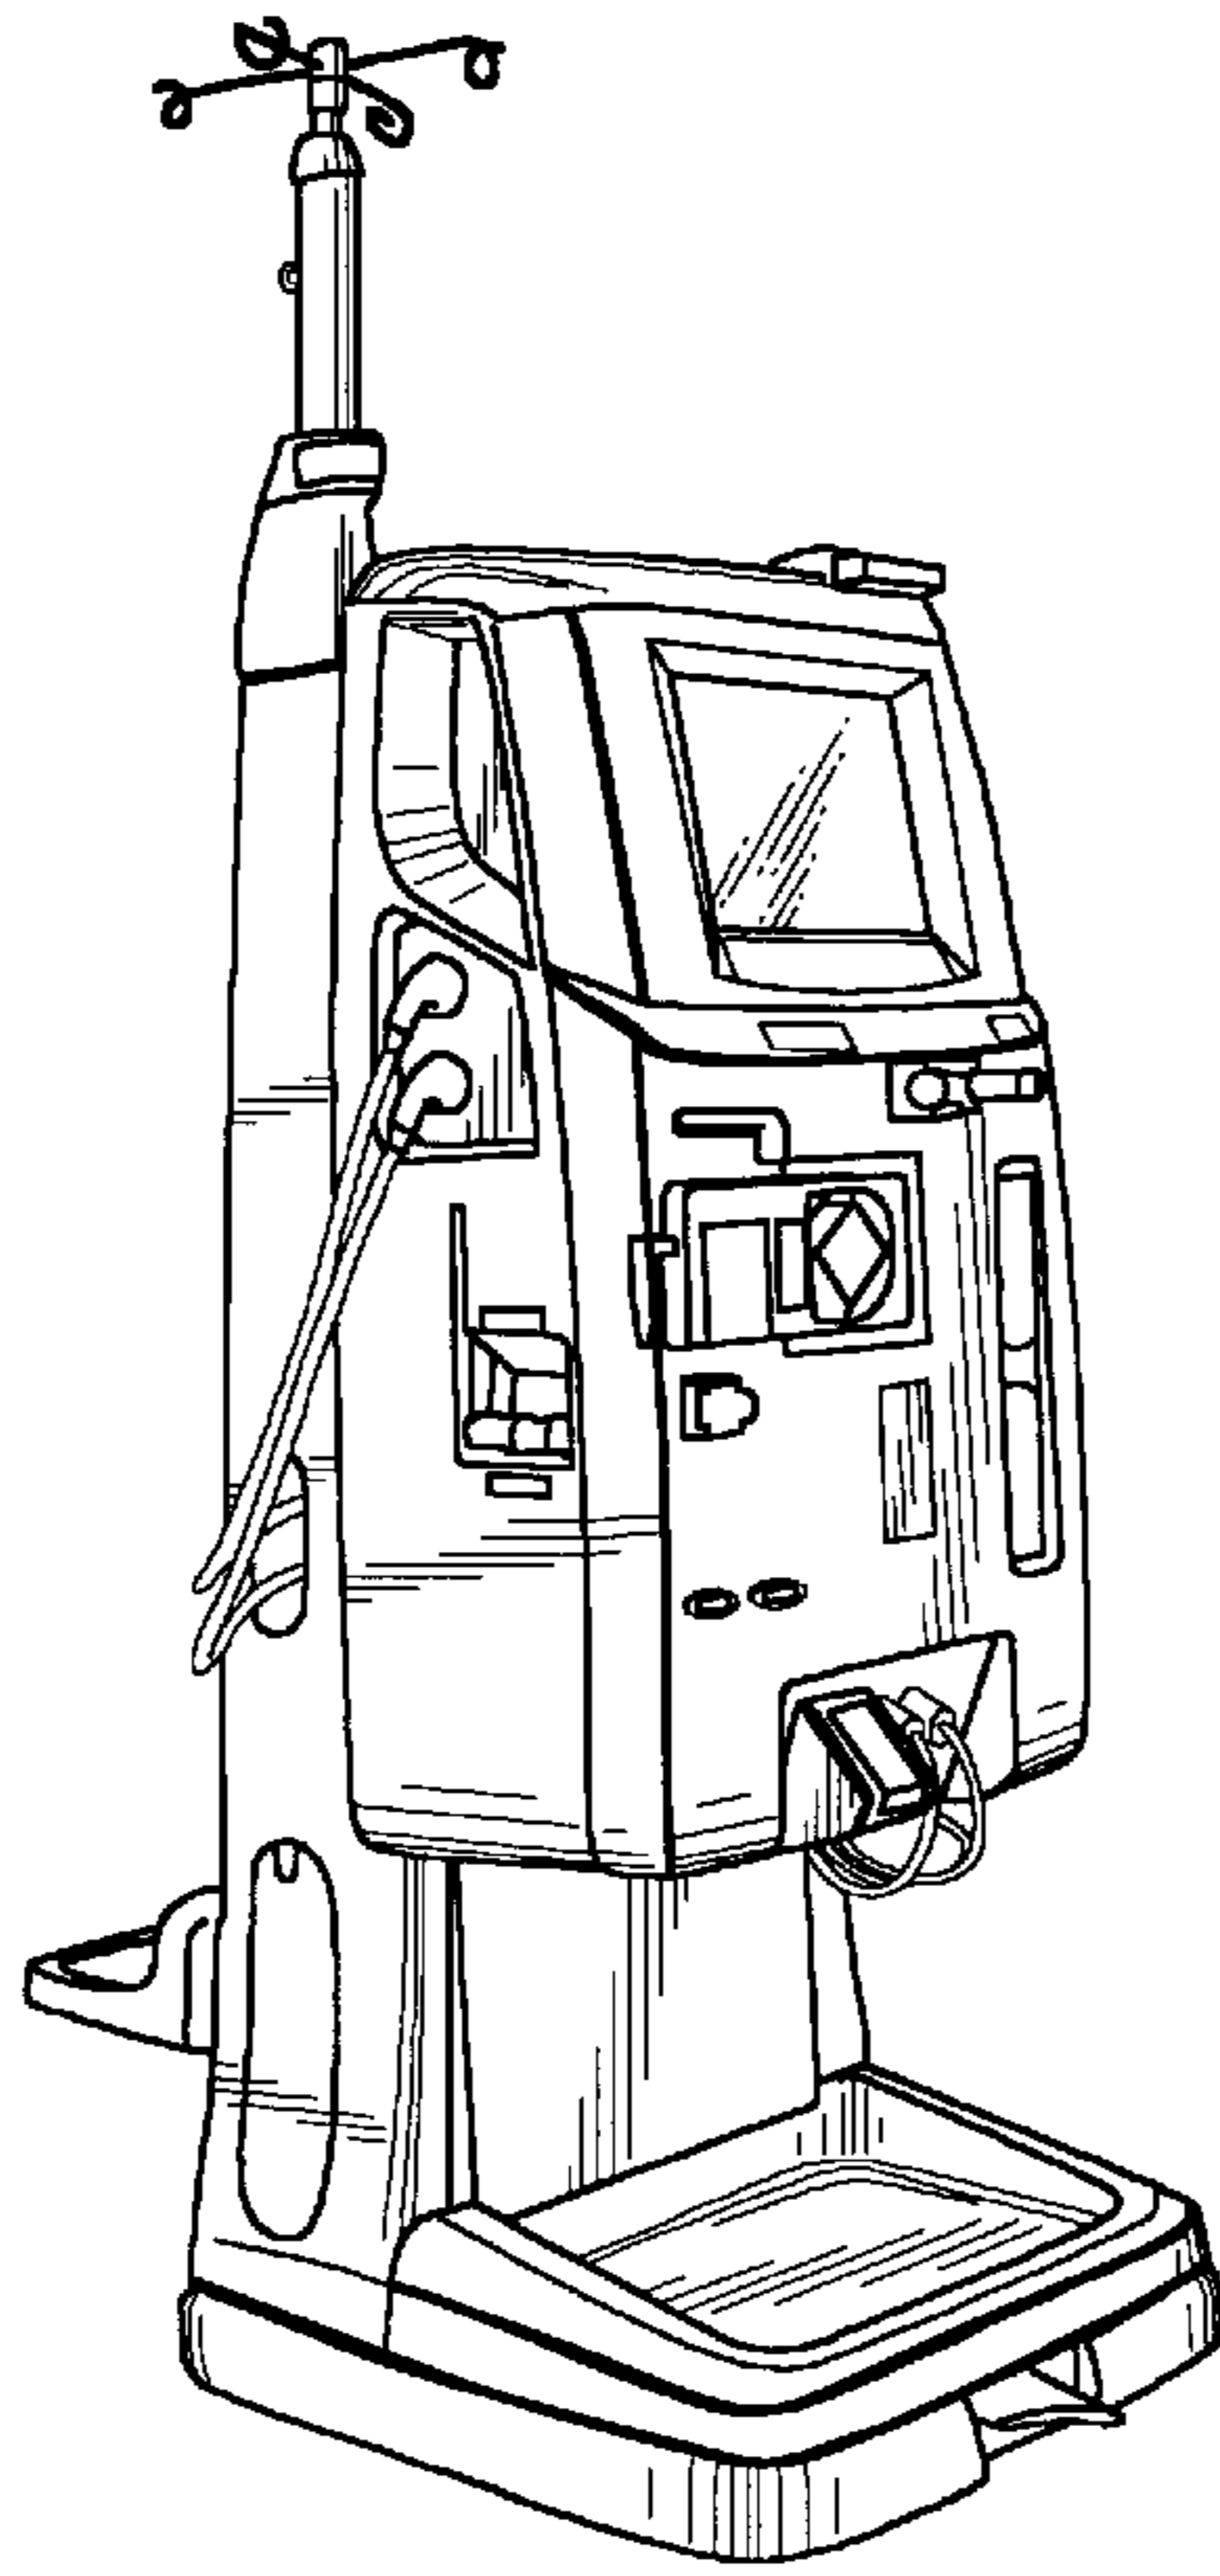


Figure 1

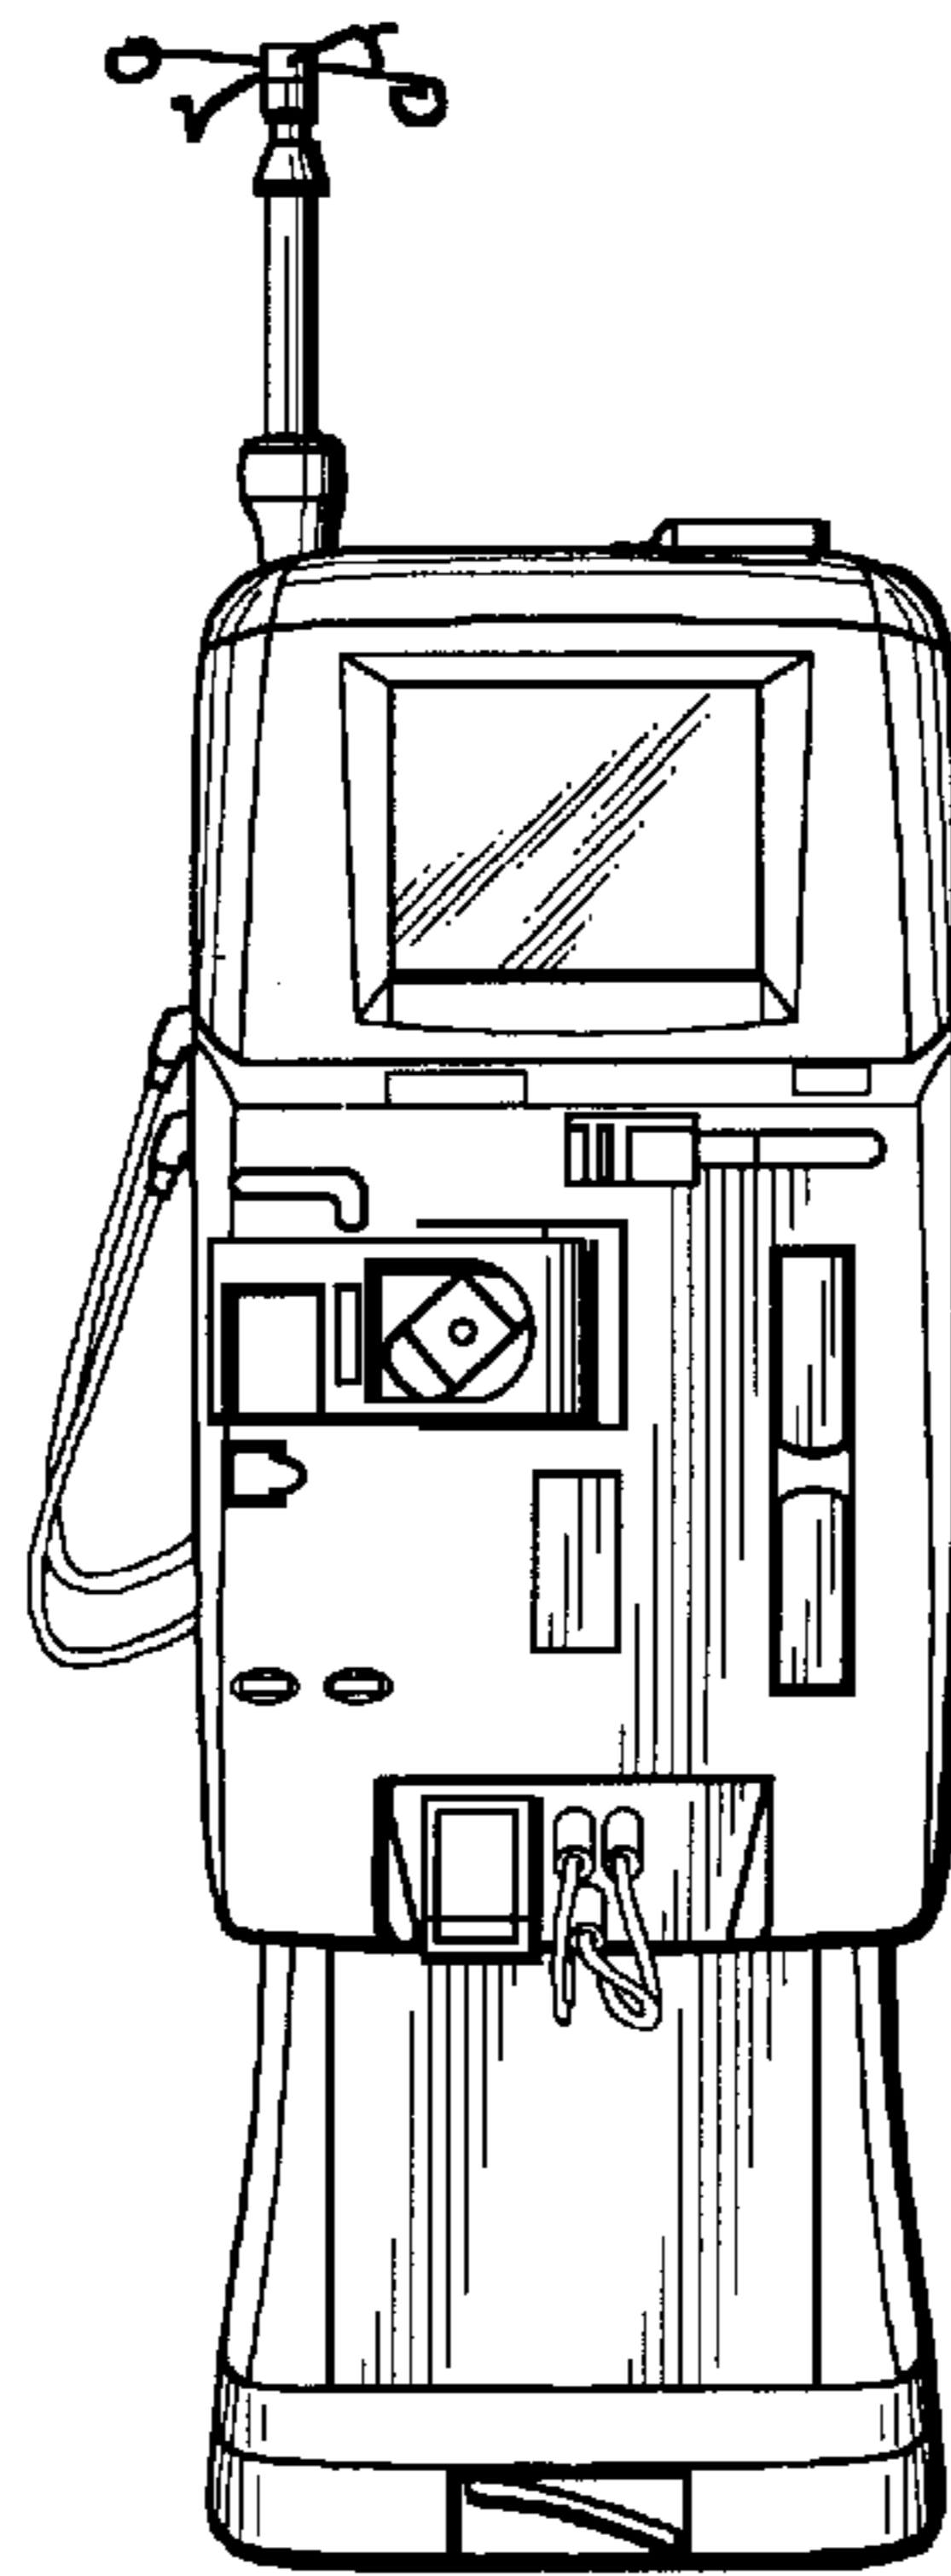


Figure 2

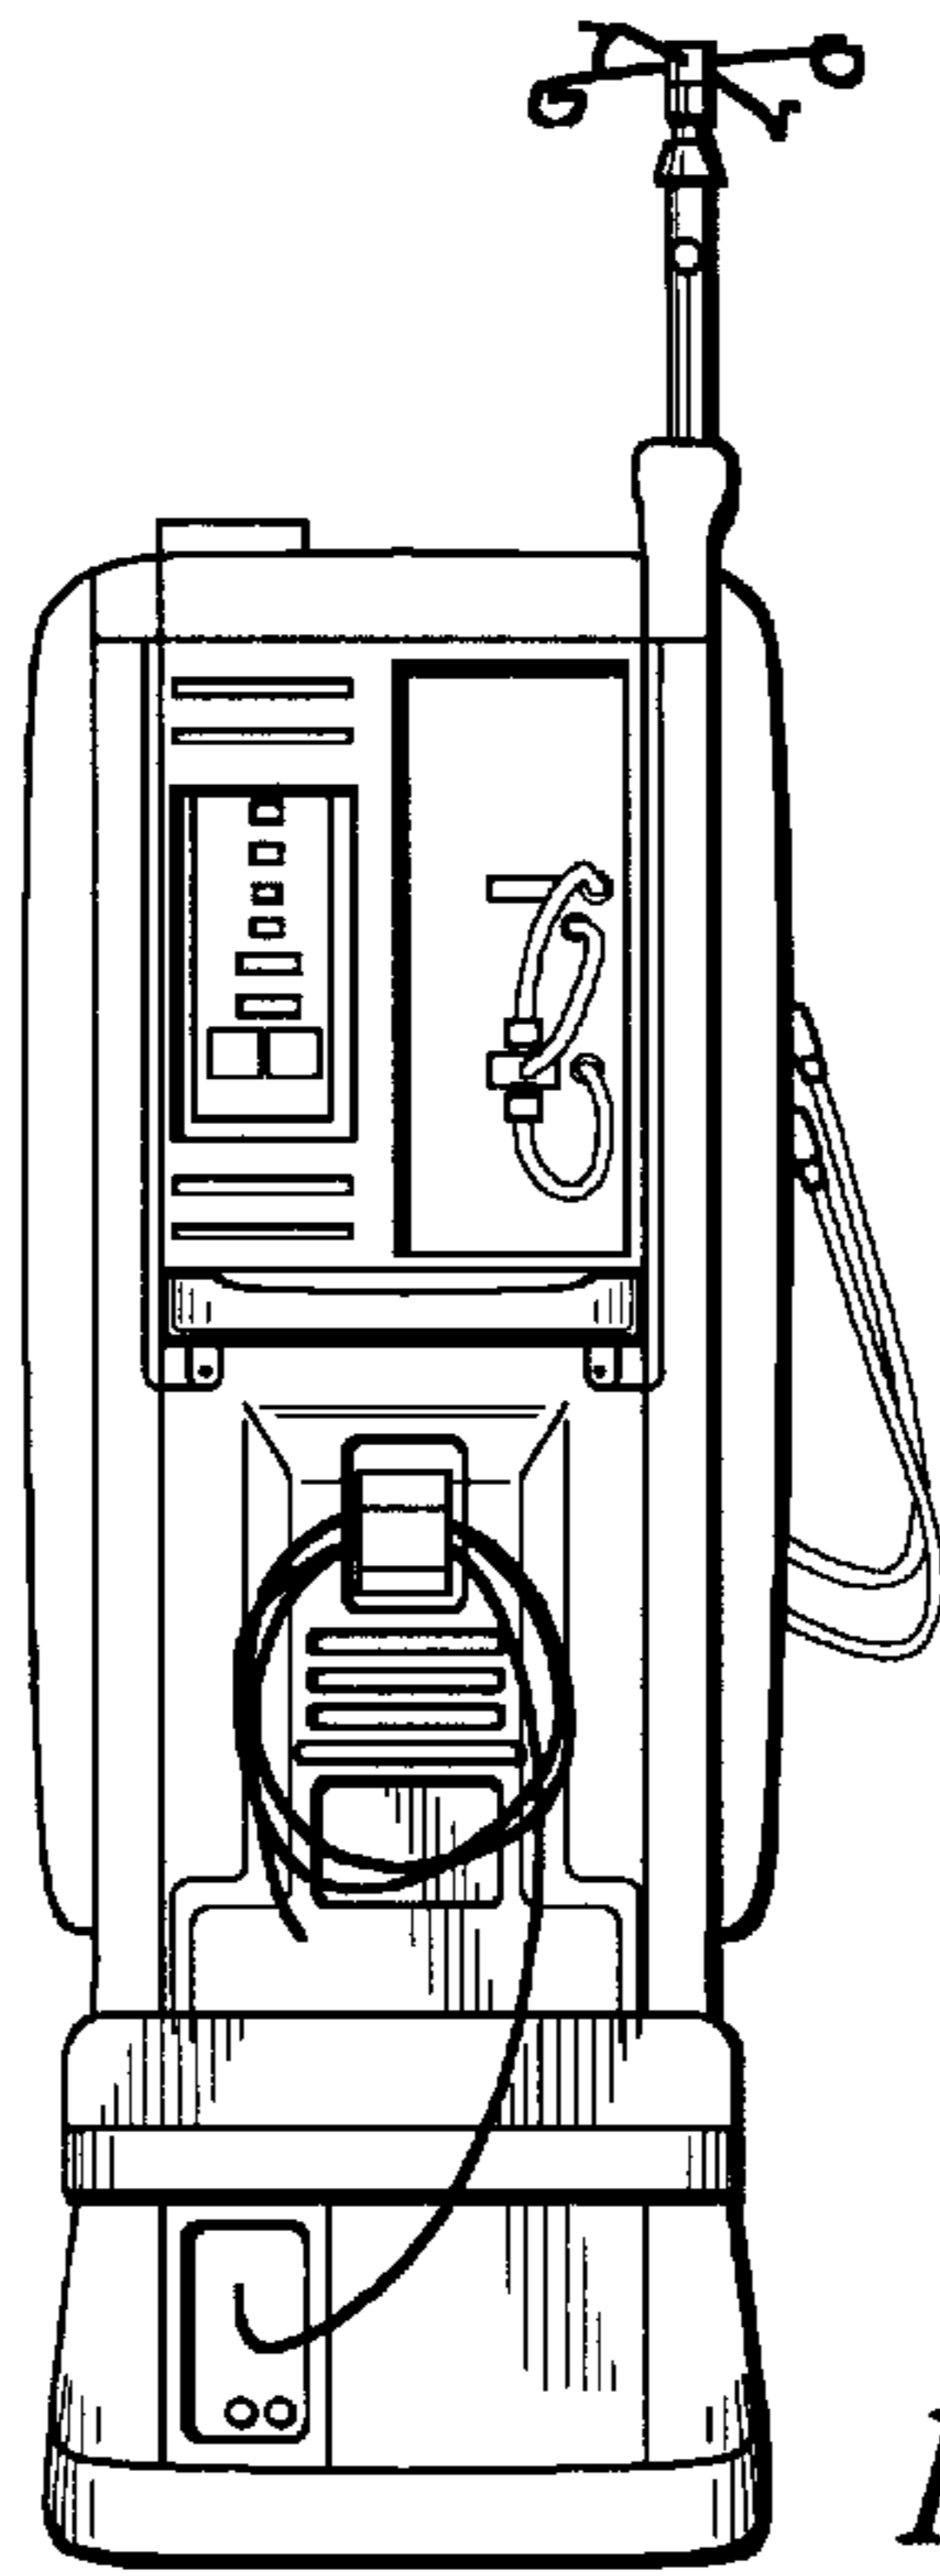


Figure 3

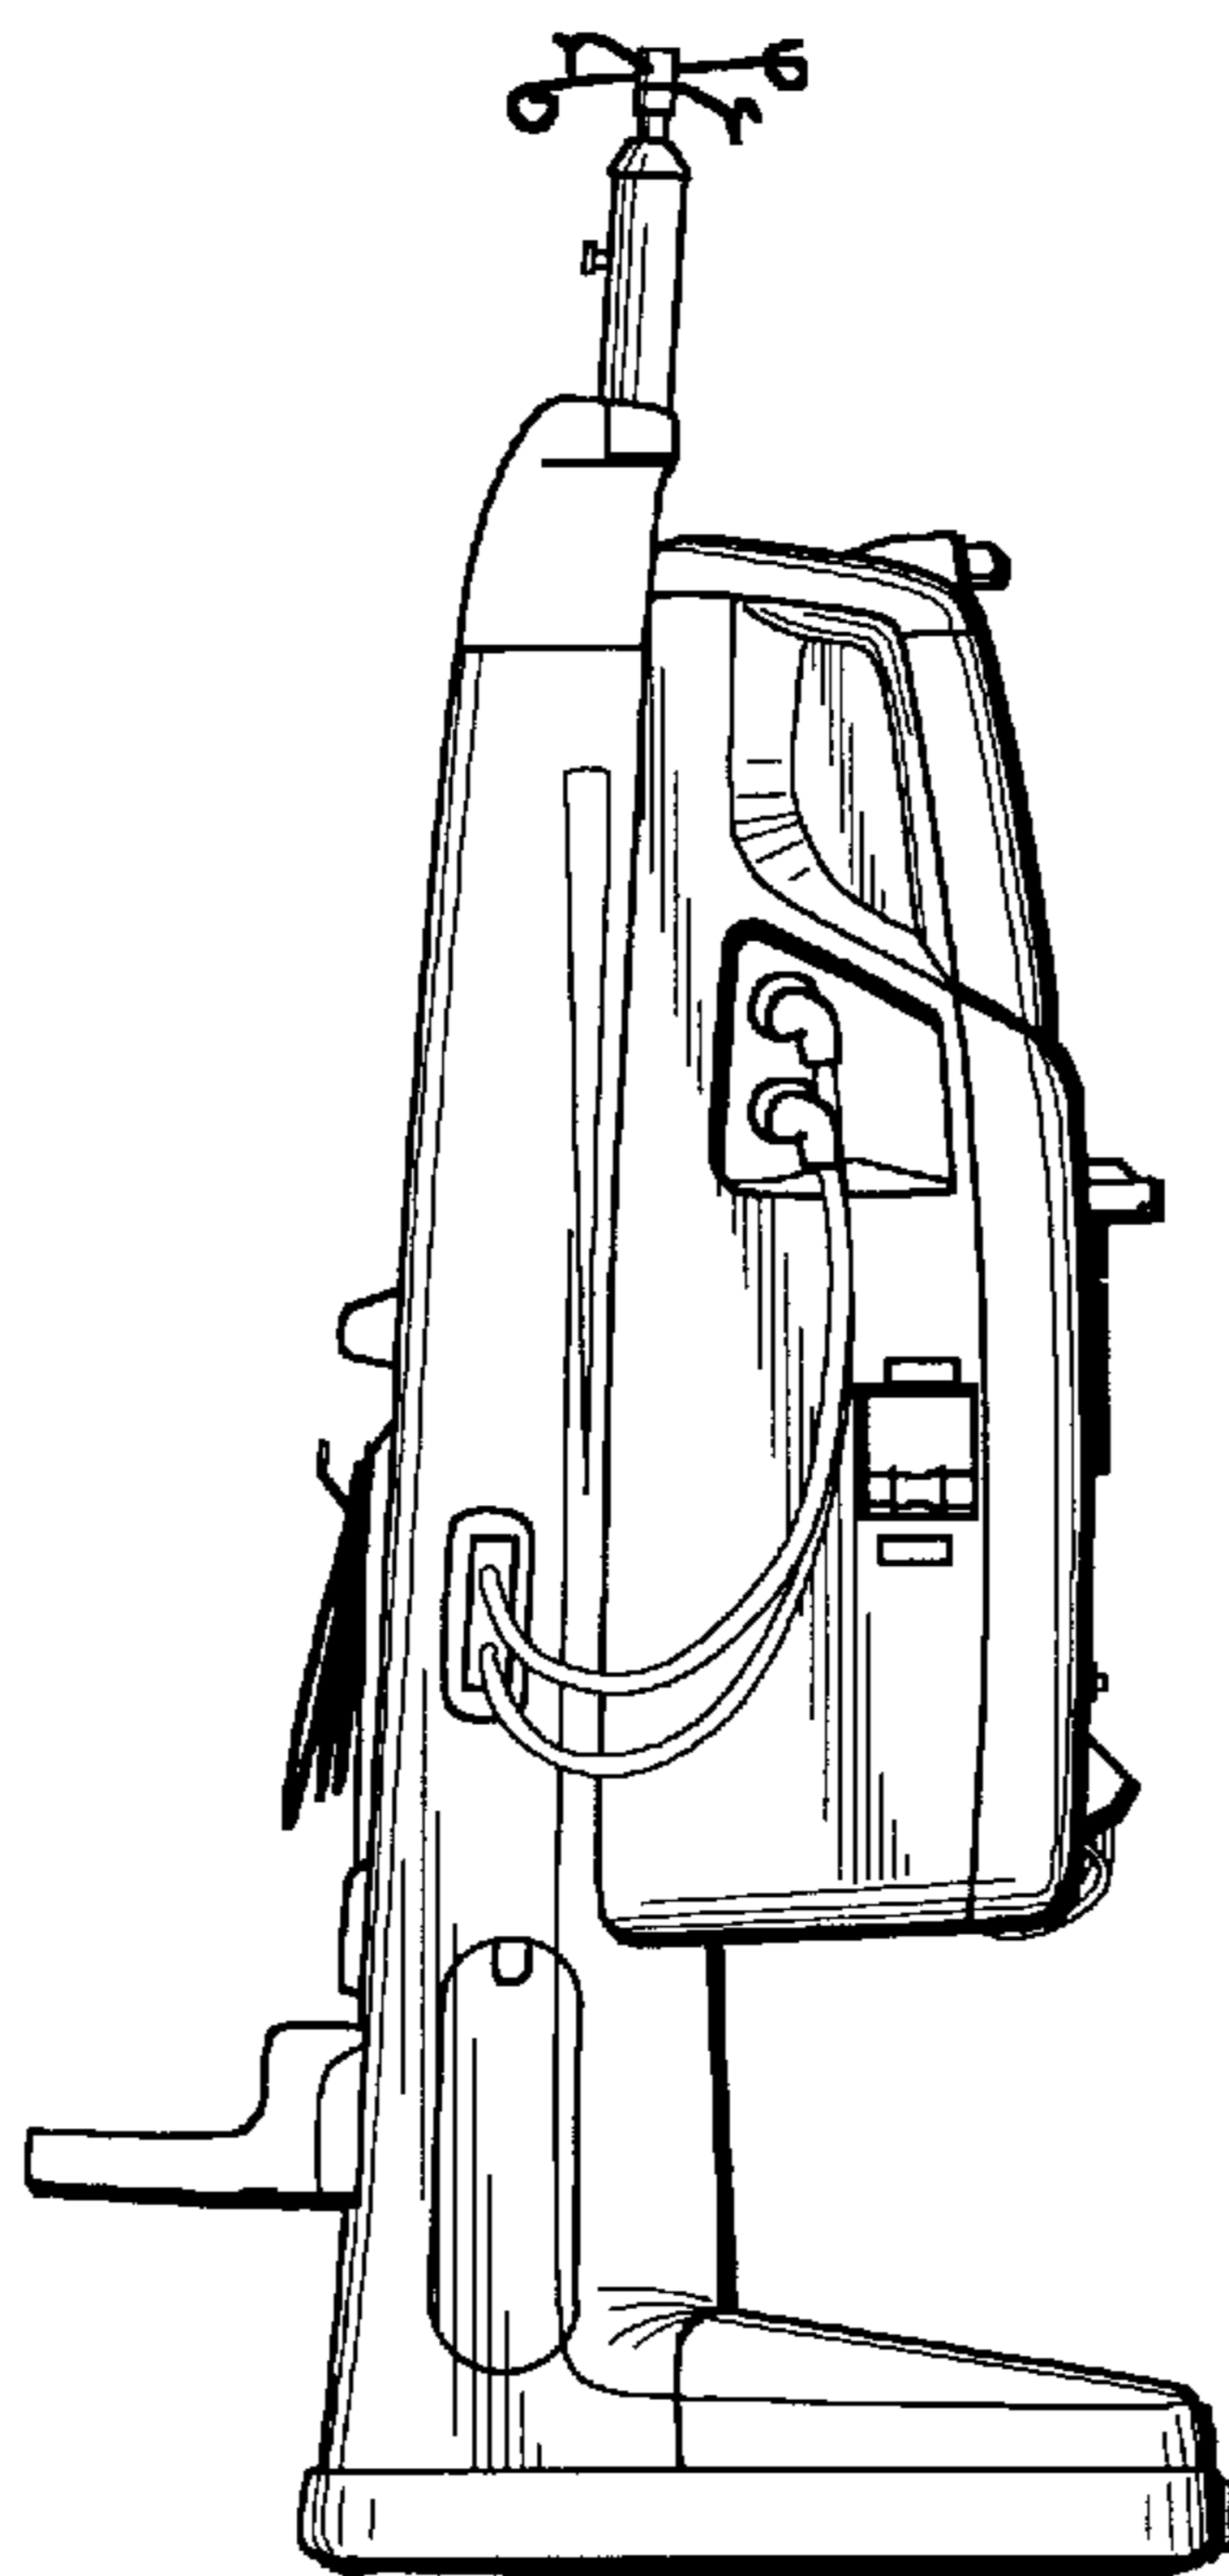


Figure 4

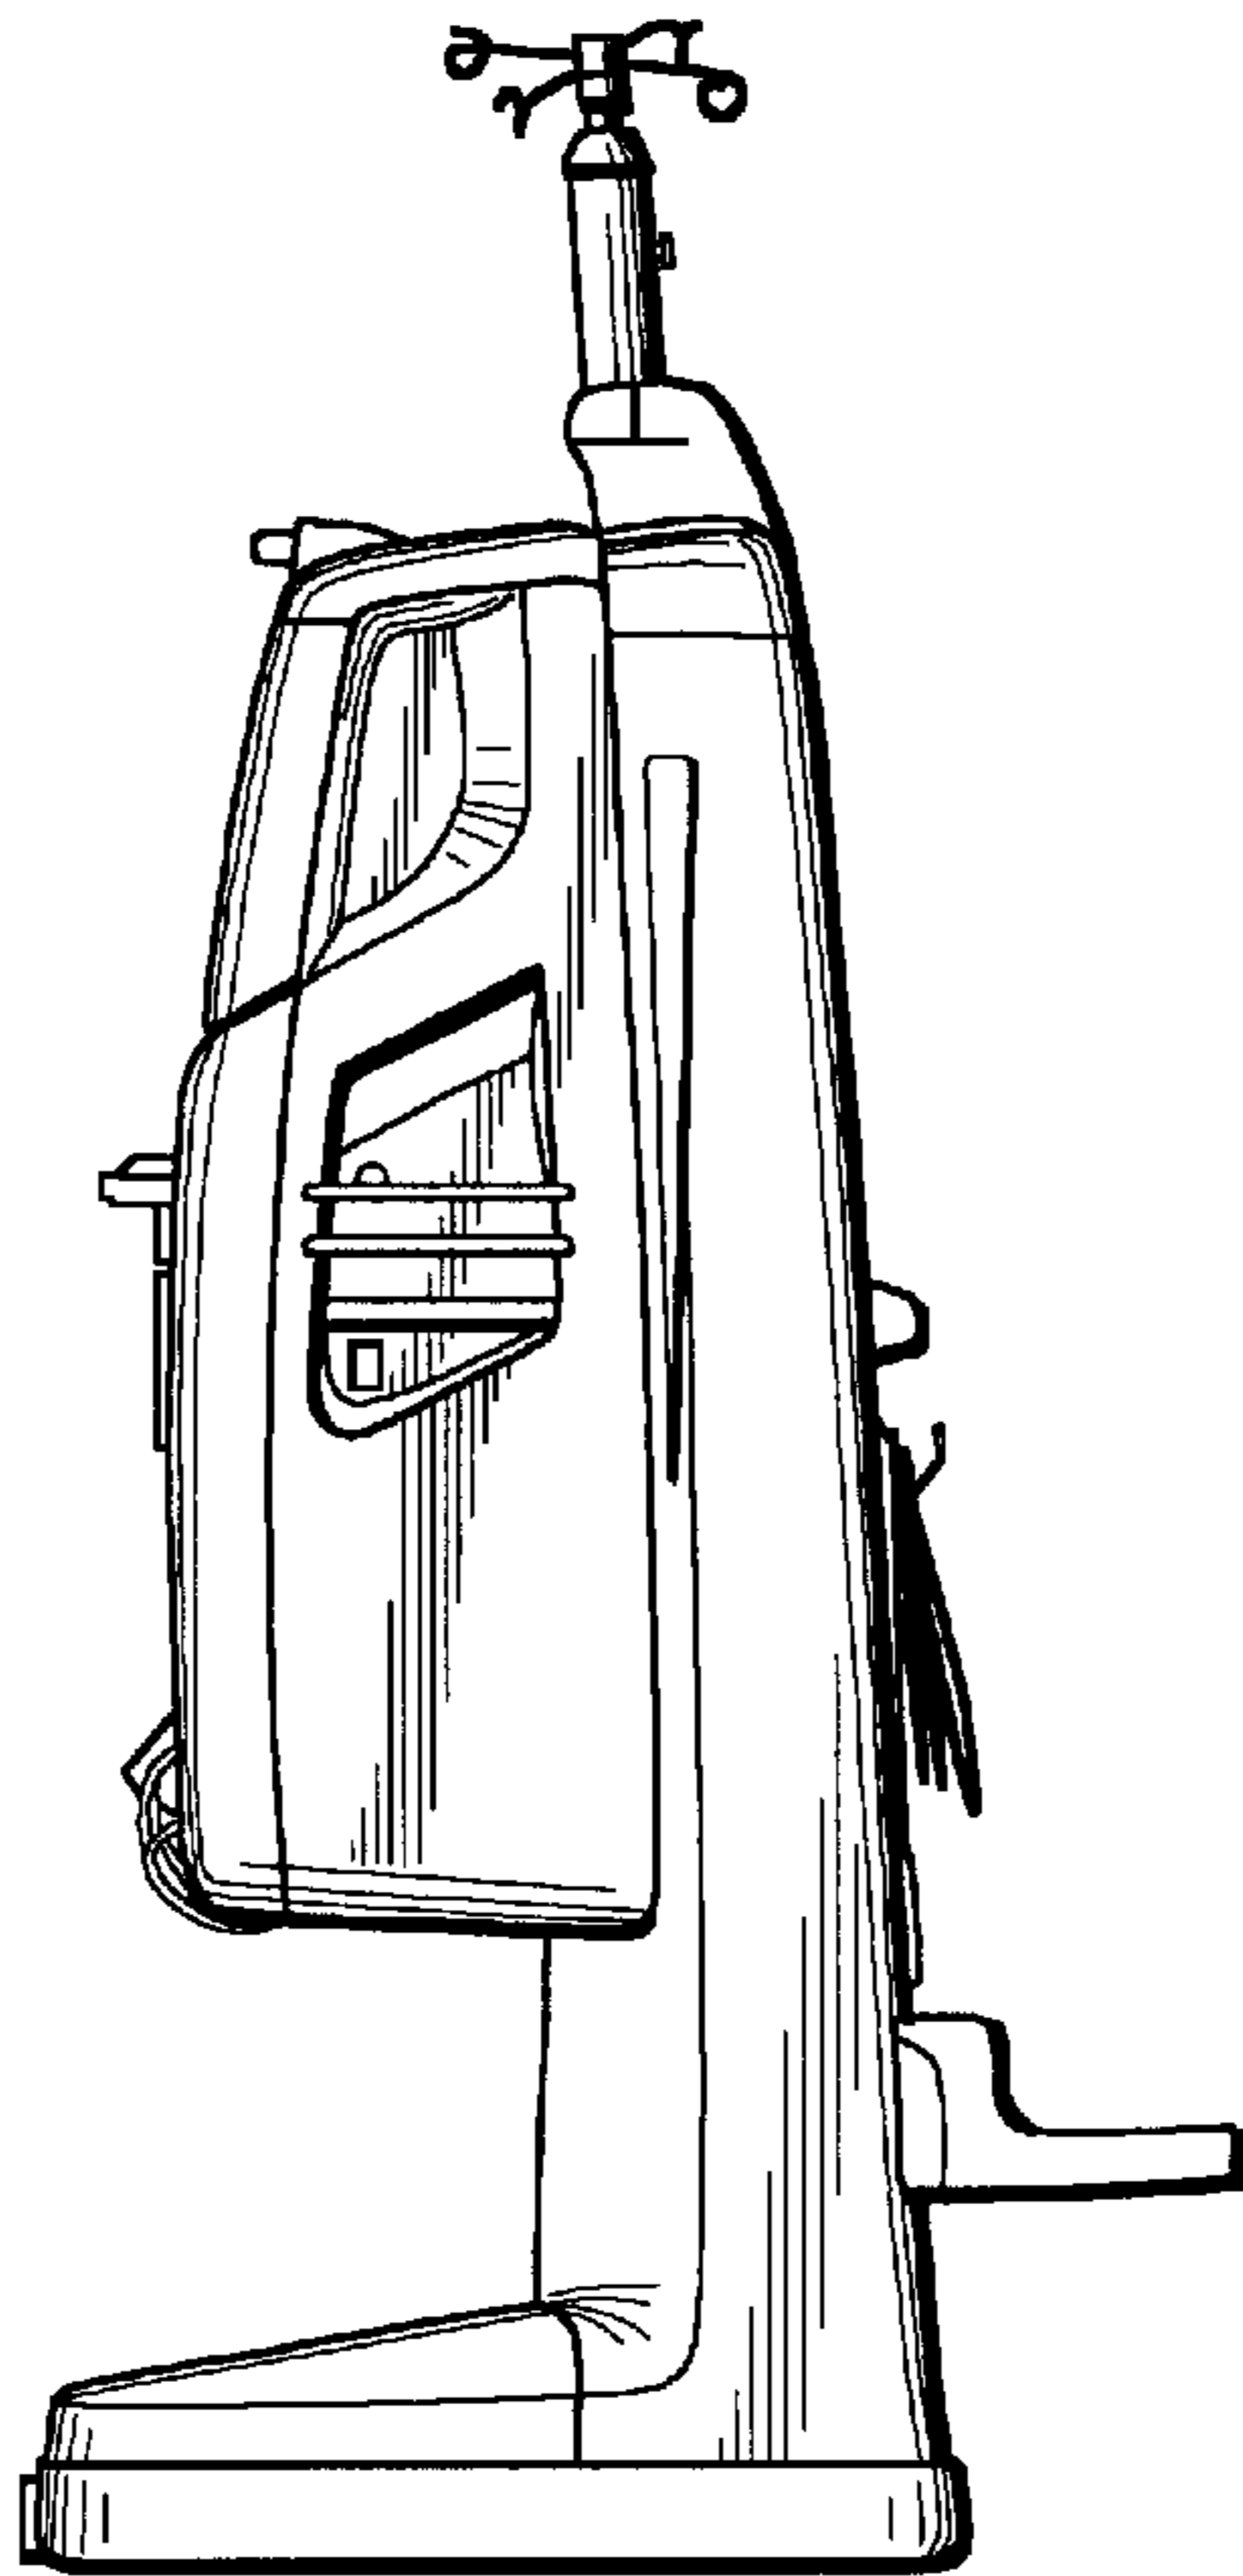


Figure 5

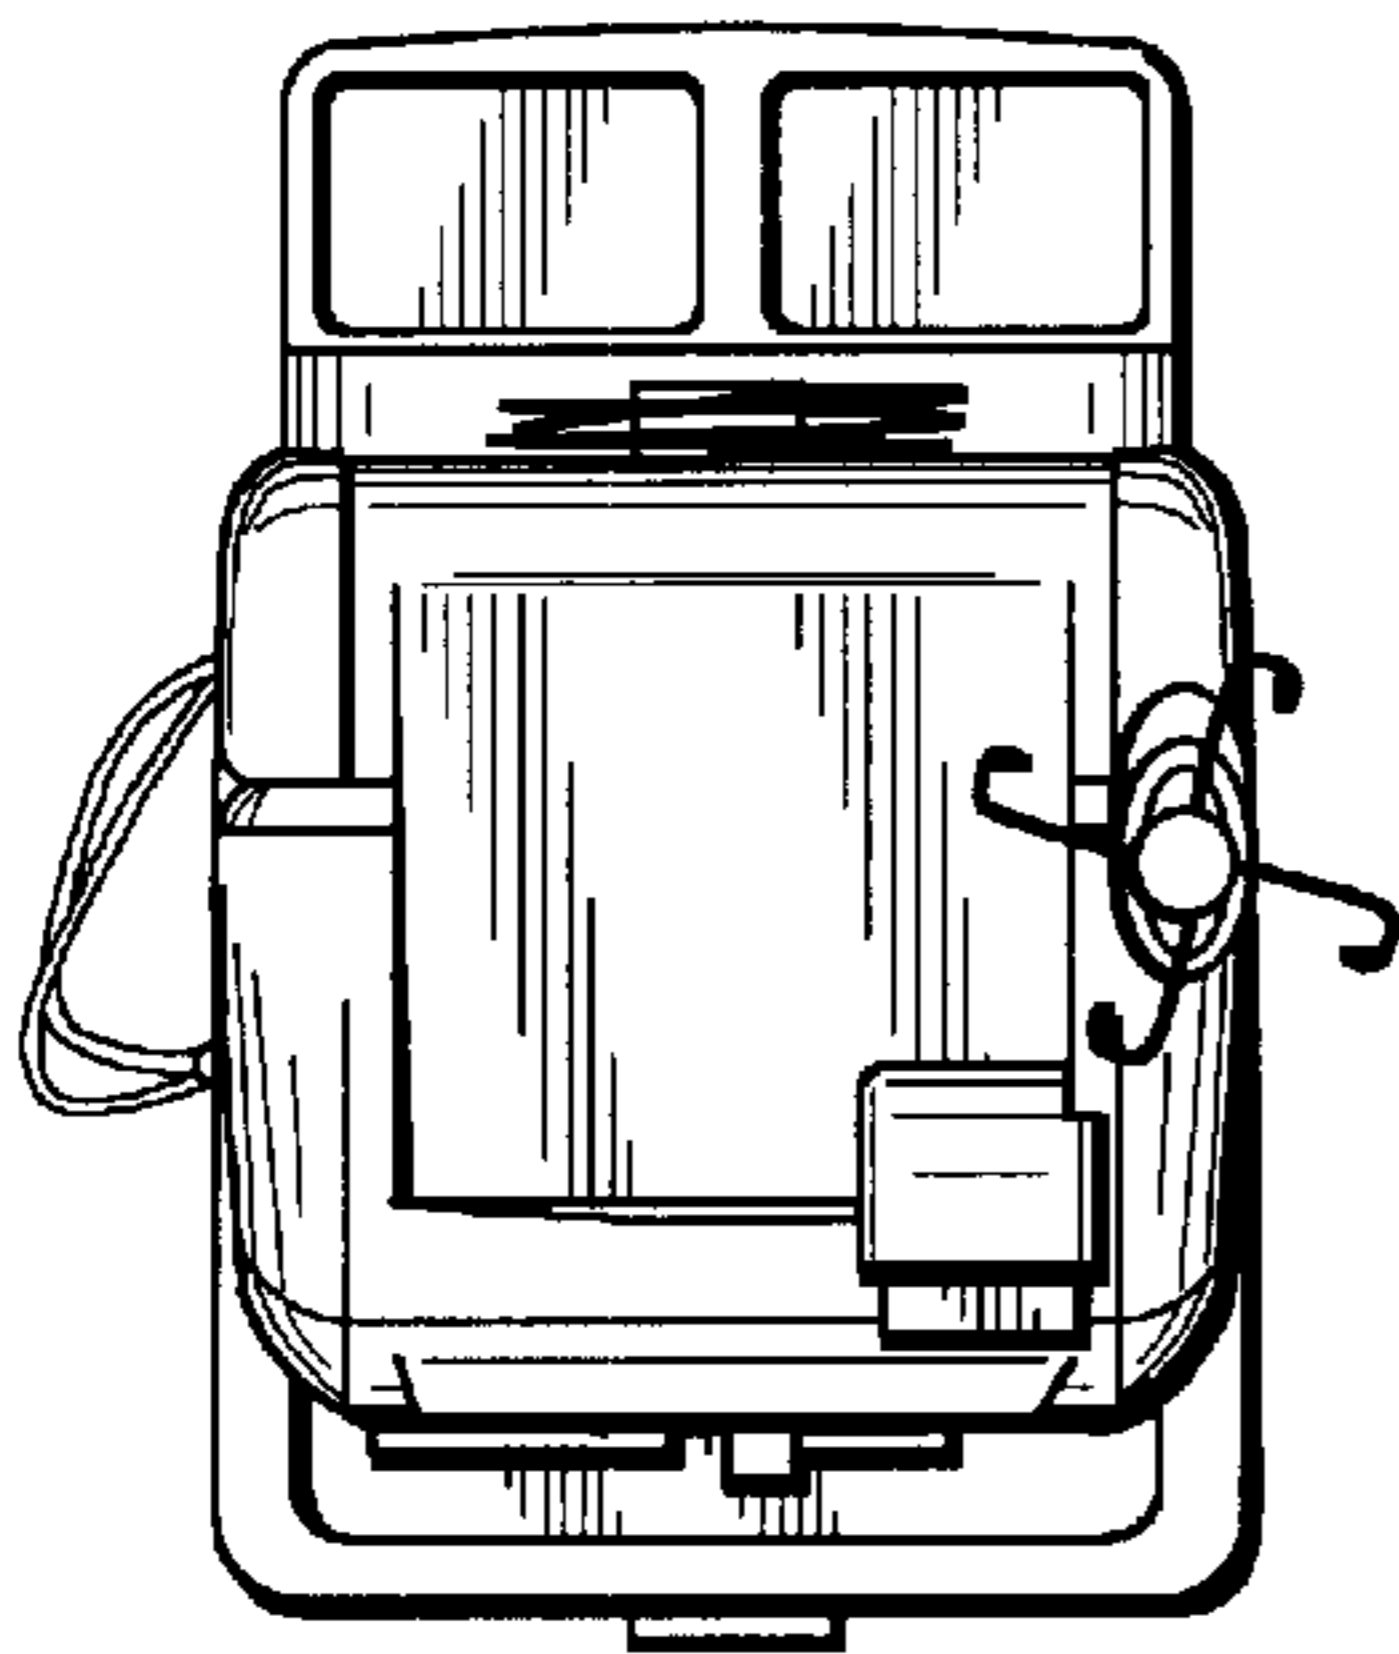


Figure 6

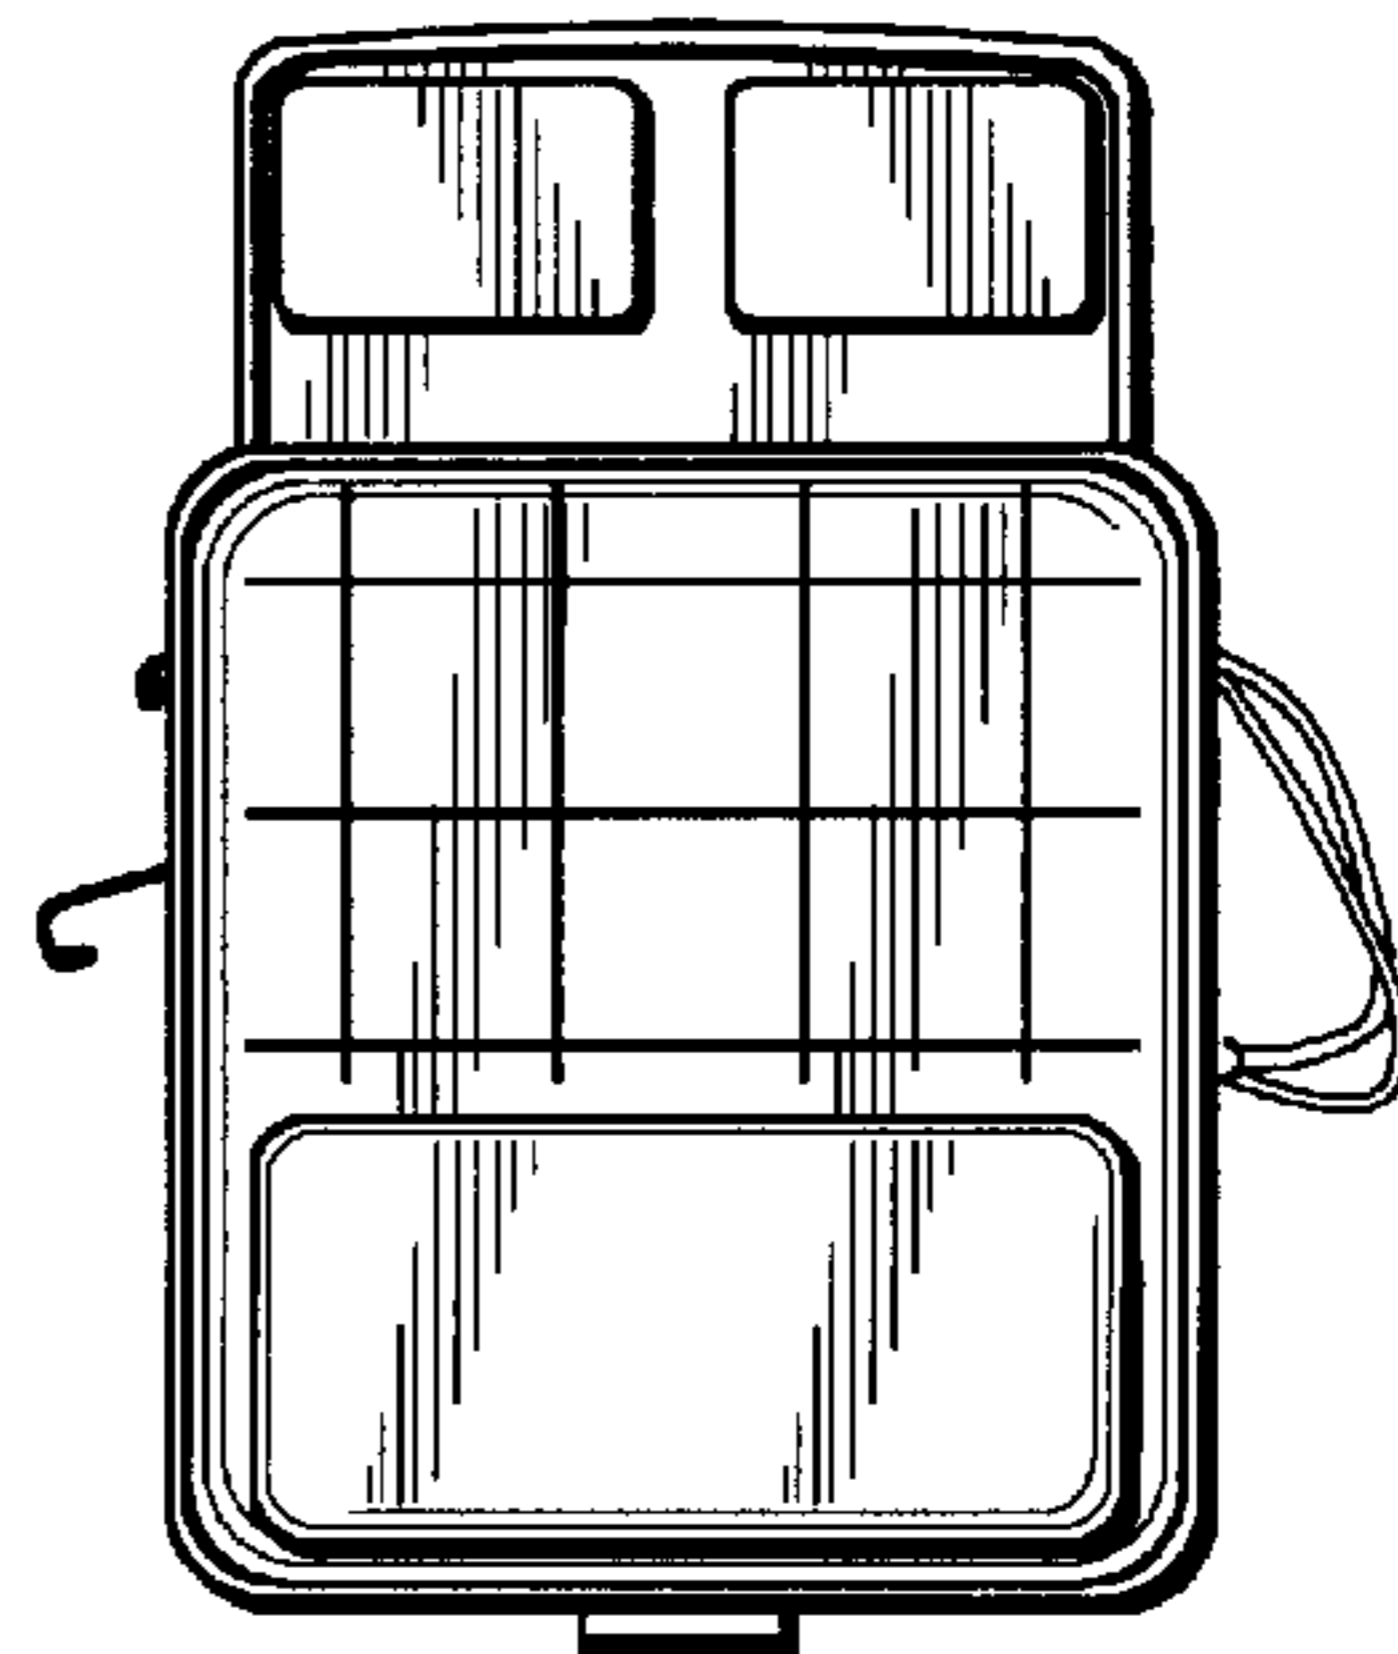


Figure 7