



US00D448119B1

(12) **United States Design Patent**  
**Neues**

(10) **Patent No.:** **US D448,119 S**

(45) **Date of Patent:** **\*\* Sep. 18, 2001**

(54) **CLEANING AND CALLUS REMOVING  
DEVICE FOR HAND AND FOOT CARE**

(75) **Inventor:** **Andreas Neues, Solingen (DE)**

(73) **Assignee:** **Excellent Gesellschaft für feine  
Schneidwaren mbH, Solingen (DE)**

(\*\*) **Term:** **14 Years**

(21) **Appl. No.:** **29/126,226**

(22) **Filed:** **Jul. 13, 2000**

(30) **Foreign Application Priority Data**

Jan. 31, 2000 (XH) ..... DM/050 628

(51) **LOC (7) Cl.** ..... **28-03**

(52) **U.S. Cl.** ..... **D28/57; D28/59; D28/63**

(58) **Field of Search** ..... D28/7, 56, 57,  
D28/59, 63; D4/119, 120, 129, 137, 138;  
D32/40, 52; D8/90-94; 132/73, 73.5, 75,  
75.6, 76.4, 76.5; 15/208, 209.1, 210.1,  
222, 229.11, 244.1, 244.3

(56) **References Cited**

**U.S. PATENT DOCUMENTS**

- D. 254,329 \* 2/1980 Tsukamoto et al. .... D28/59
- D. 281,729 \* 12/1985 Mast ..... D28/59
- D. 364,226 \* 11/1995 Hartmann ..... D28/59 X

- 3,923,070 \* 12/1975 Tsukamoto ..... 132/73
- 3,965,520 \* 6/1976 Maier ..... 15/104.94
- 4,049,010 \* 9/1977 Mitchell et al. .... 132/200
- 4,184,499 \* 1/1980 Seidler ..... 132/75.6
- 4,211,246 \* 7/1980 Hokama ..... 132/76.4
- 4,286,610 \* 9/1981 Jones et al. .... 132/76.4
- 4,366,828 \* 1/1983 Hokama ..... 132/75.6

\* cited by examiner

*Primary Examiner*—Philip S. Hyder

*Assistant Examiner*—C. Tuttle

(74) *Attorney, Agent, or Firm*—Schiff Hardin & Waite


(57) **CLAIM**

The ornamental design for a cleaning and callus removing device for hand and foot care, as shown and described.

**DESCRIPTION**

FIG. 1 is a top, left and rear perspective view of the cleaning and callus removing device for hand and foot care of the present invention;  
 FIG. 2 is a top plan view of the device of FIG. 1 with the bottom being a mirror image;  
 FIG. 3 is an elevational view of the left side of the device of FIG. 1 with the right side being a mirror image;  
 FIG. 4 is a rear elevational view of the device of FIG. 1; and,  
 FIG. 5 is a front end elevational view of the device of FIG. 1.

**1 Claim, 2 Drawing Sheets**

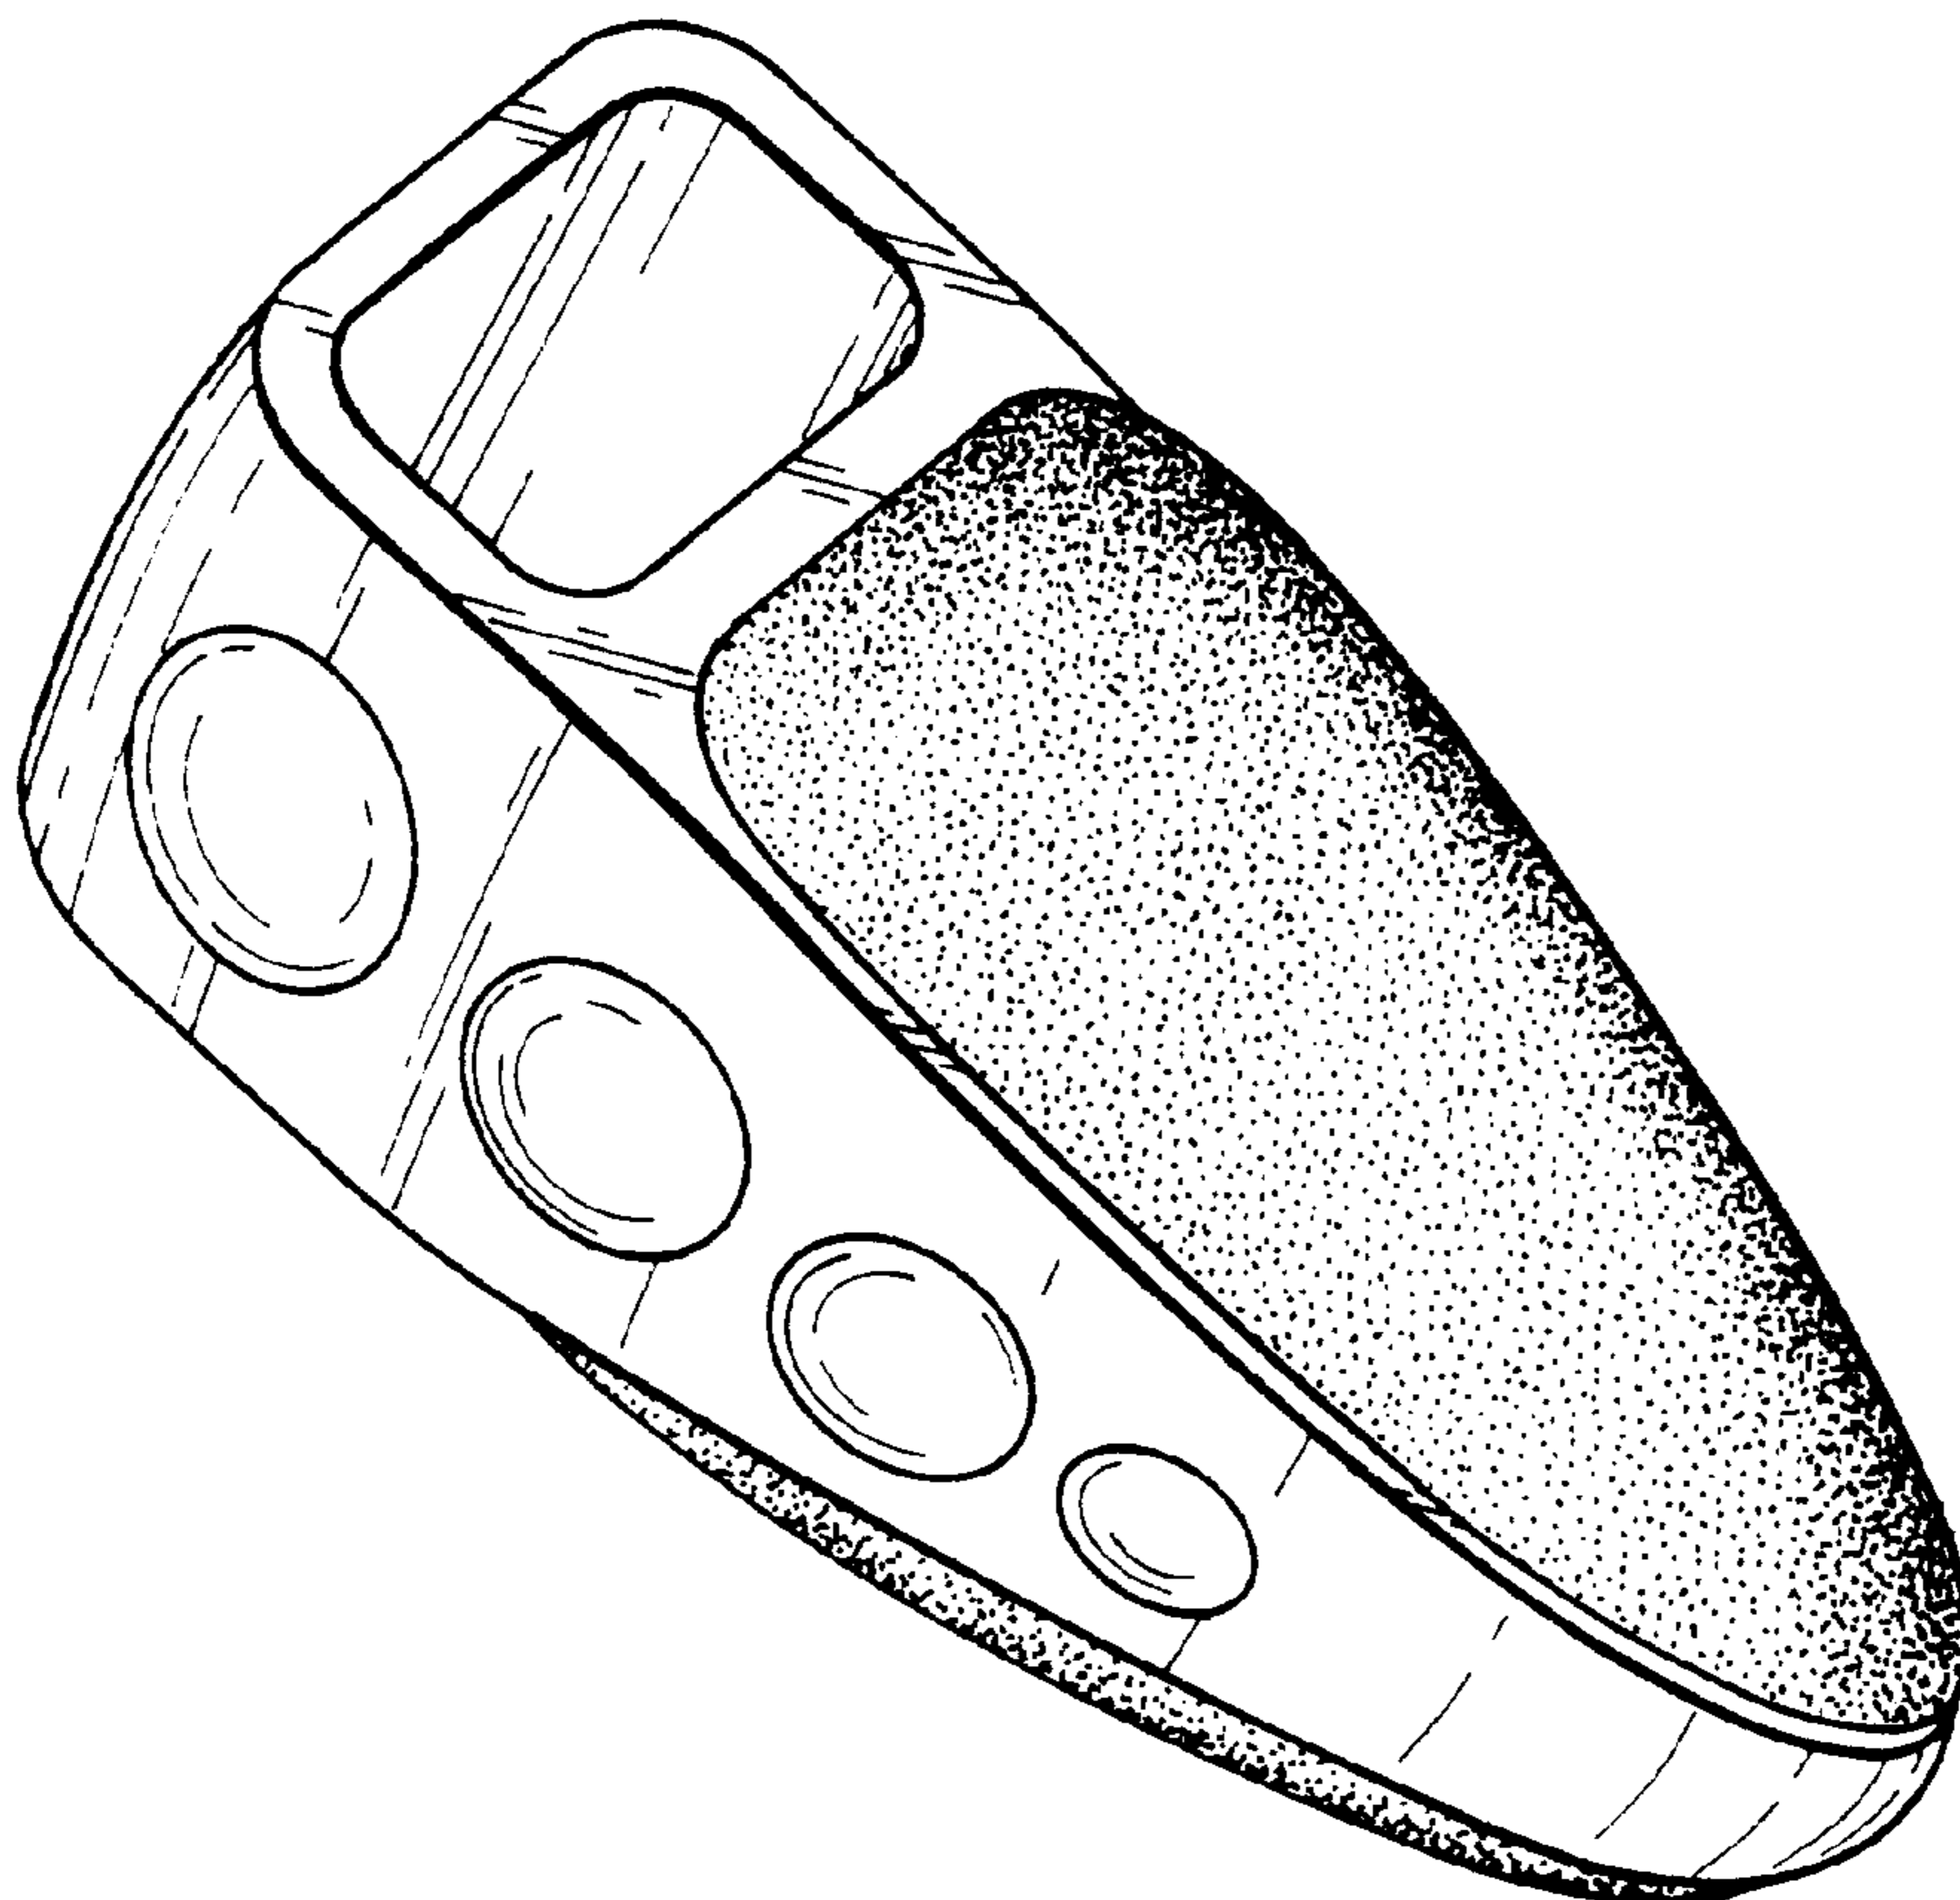

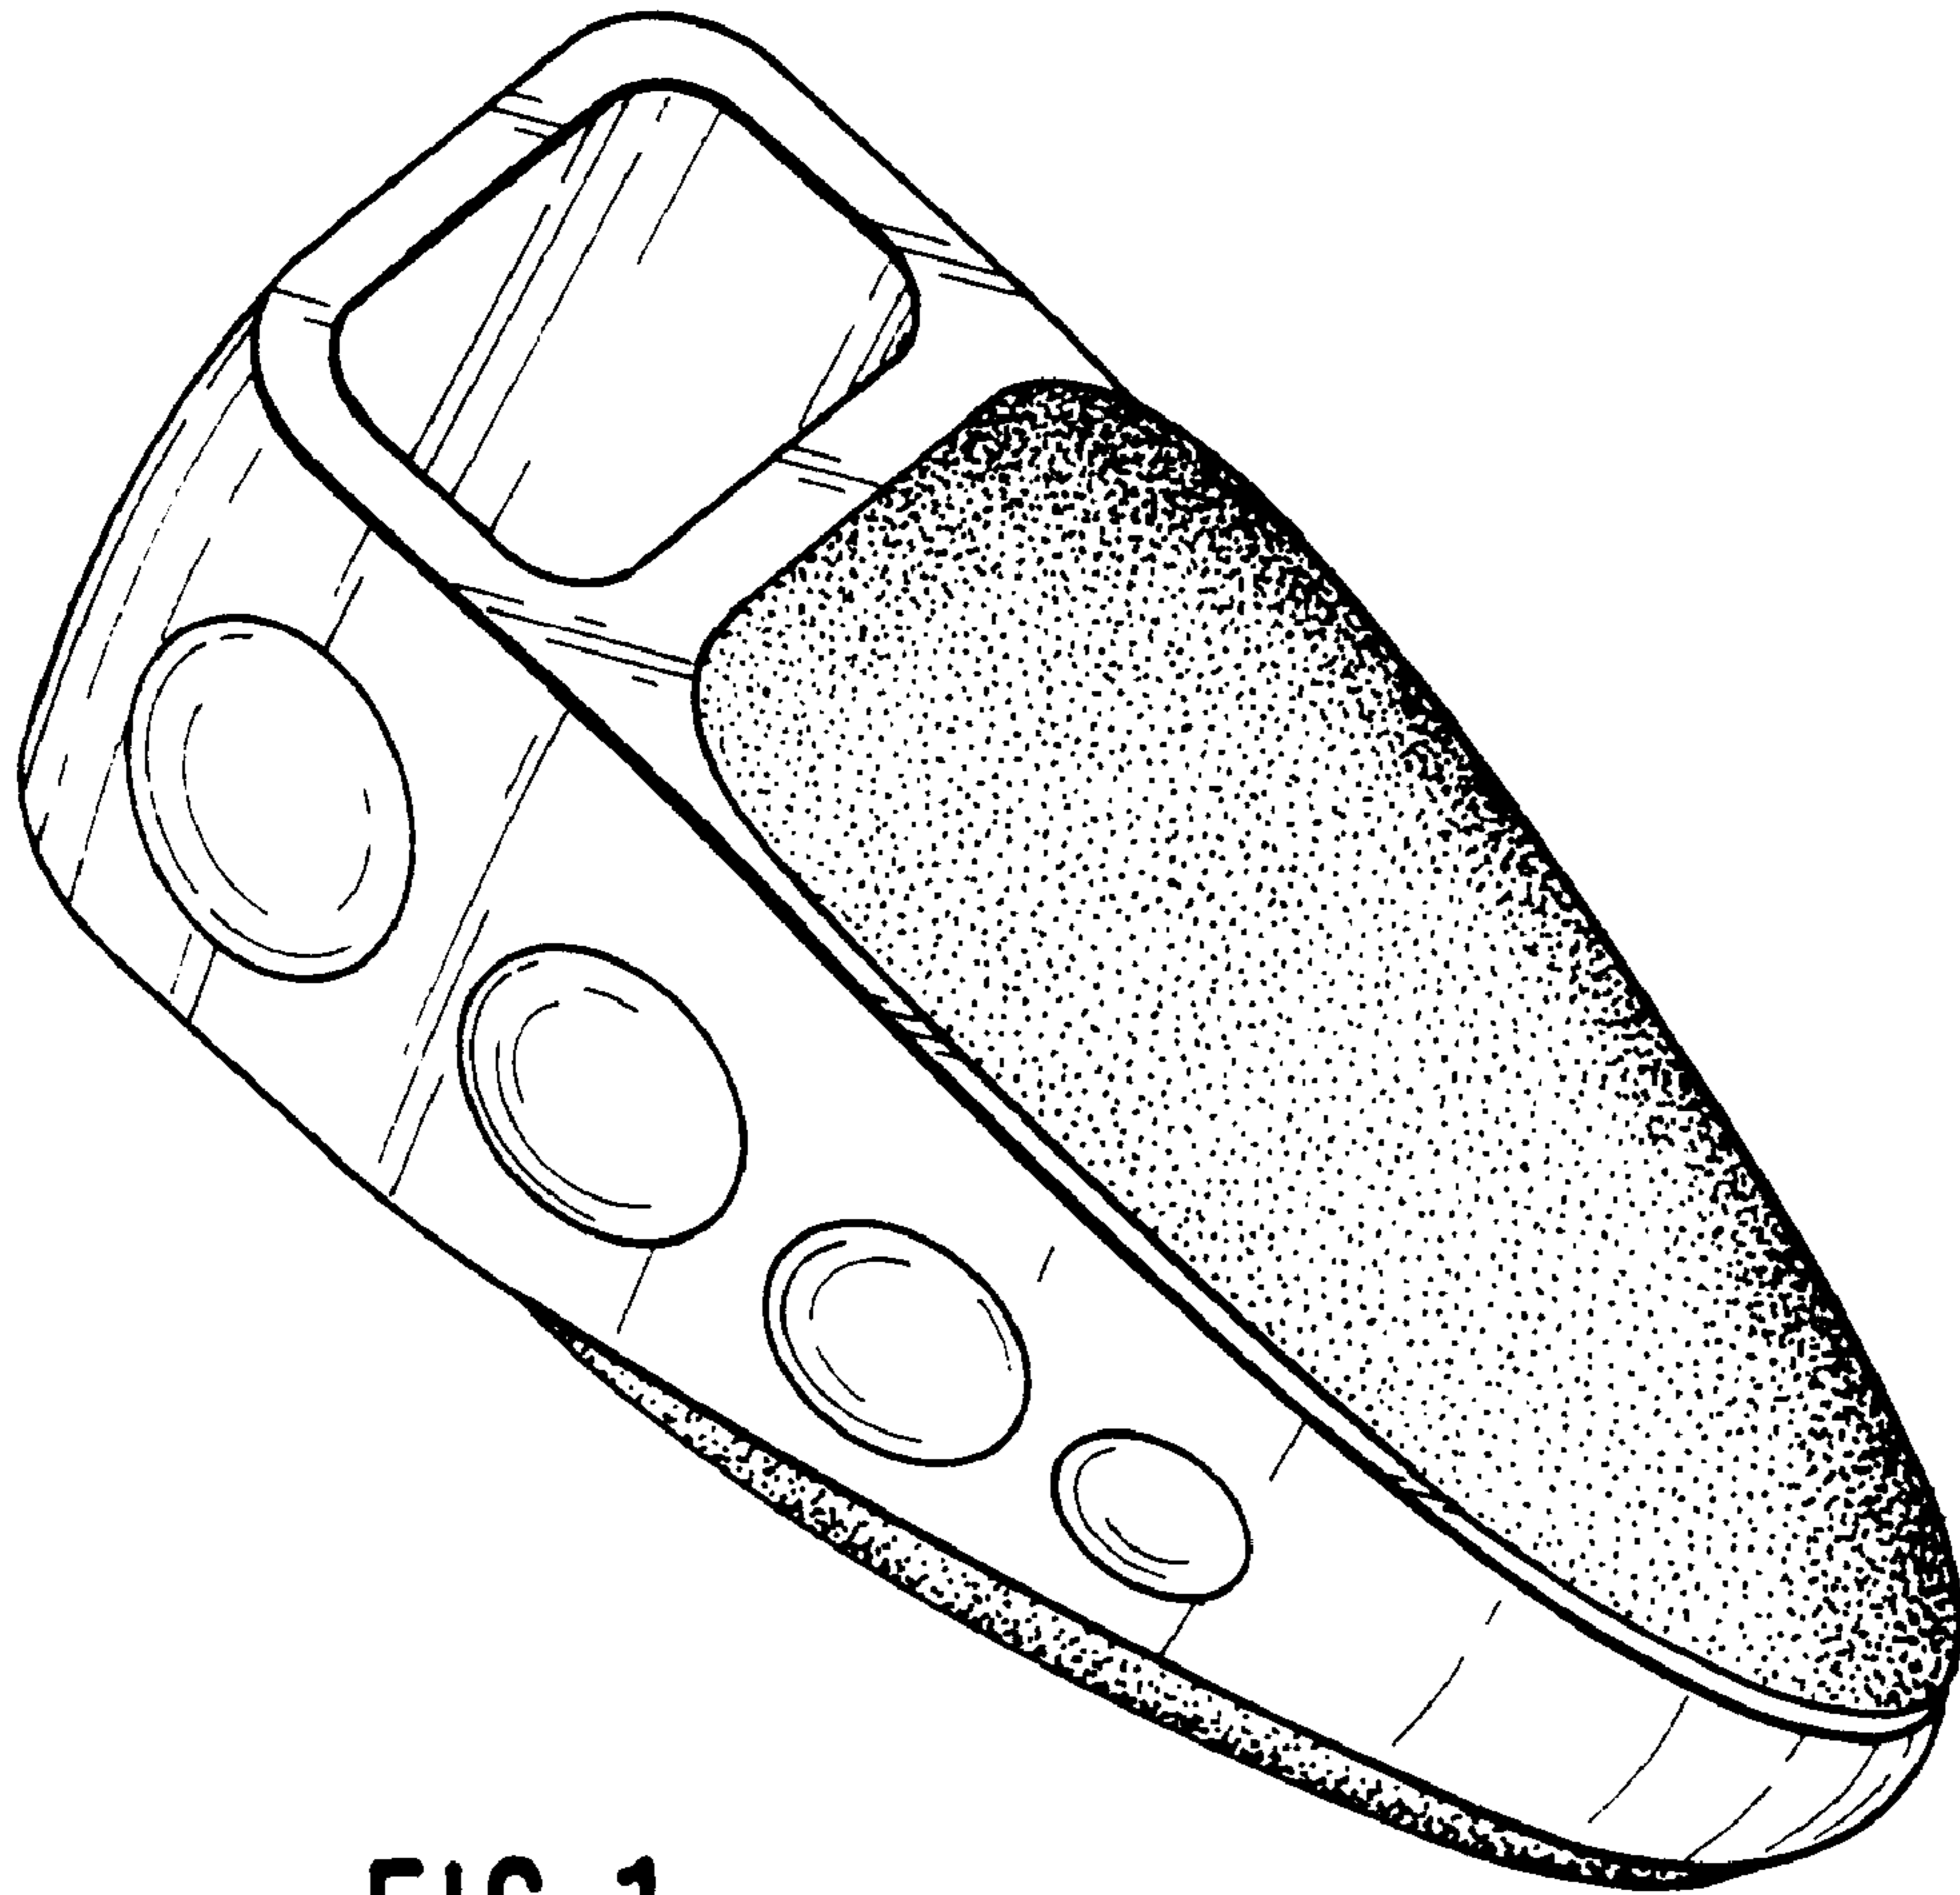


FIG. 1

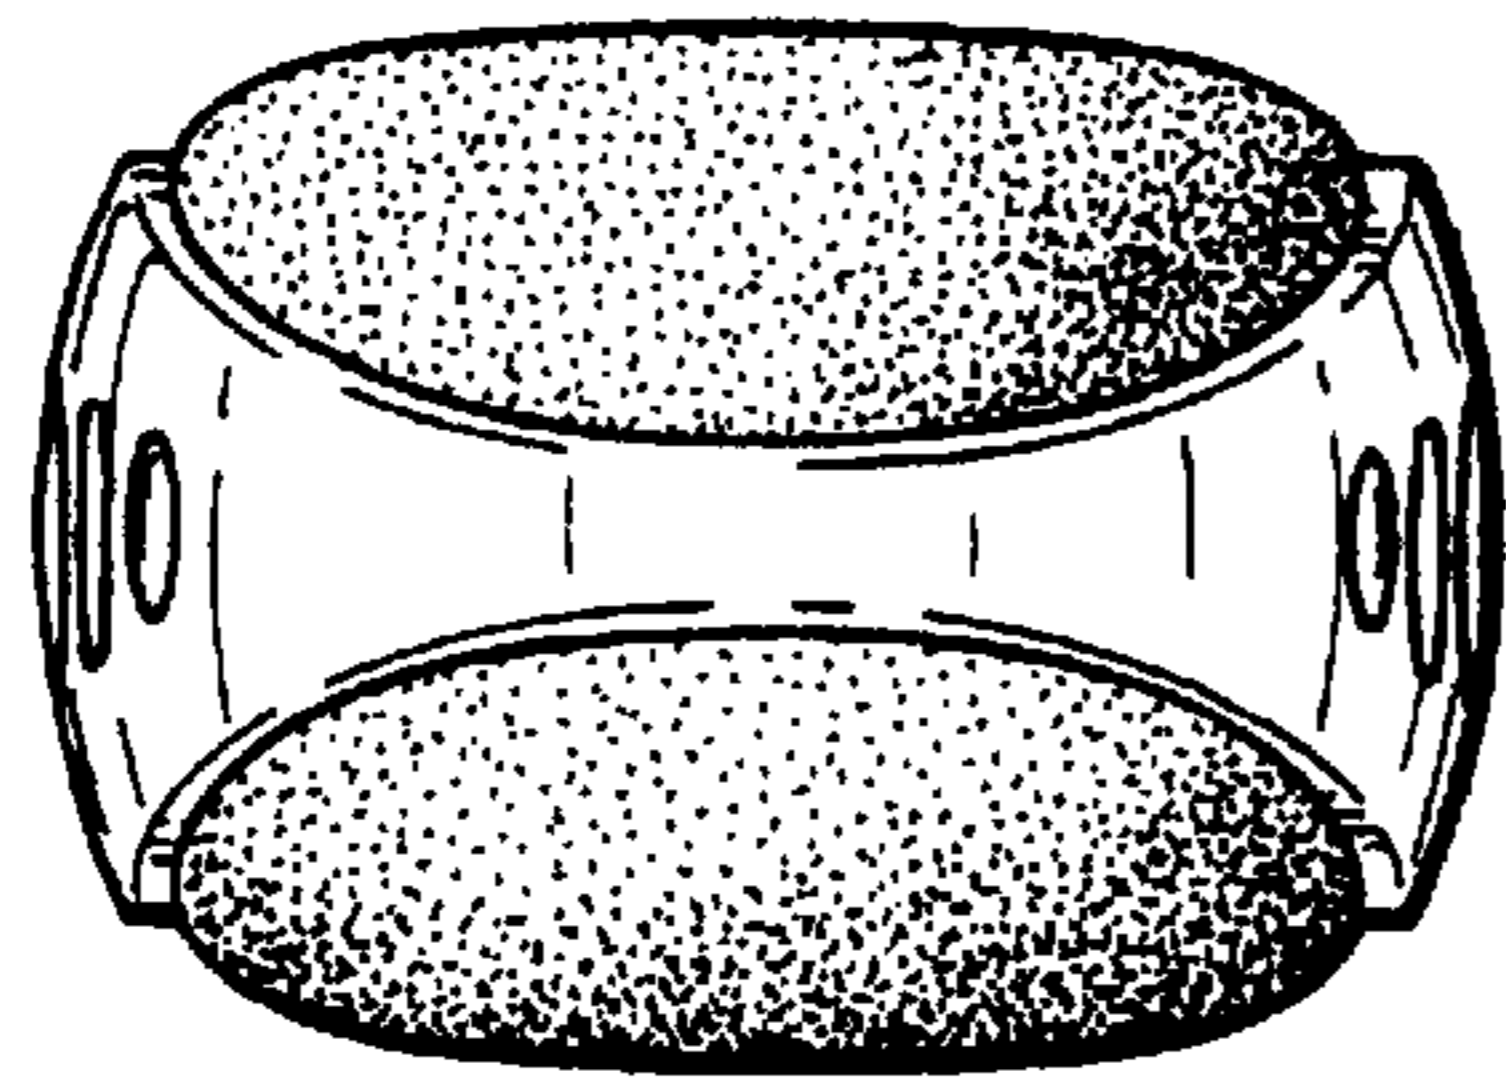


FIG. 4

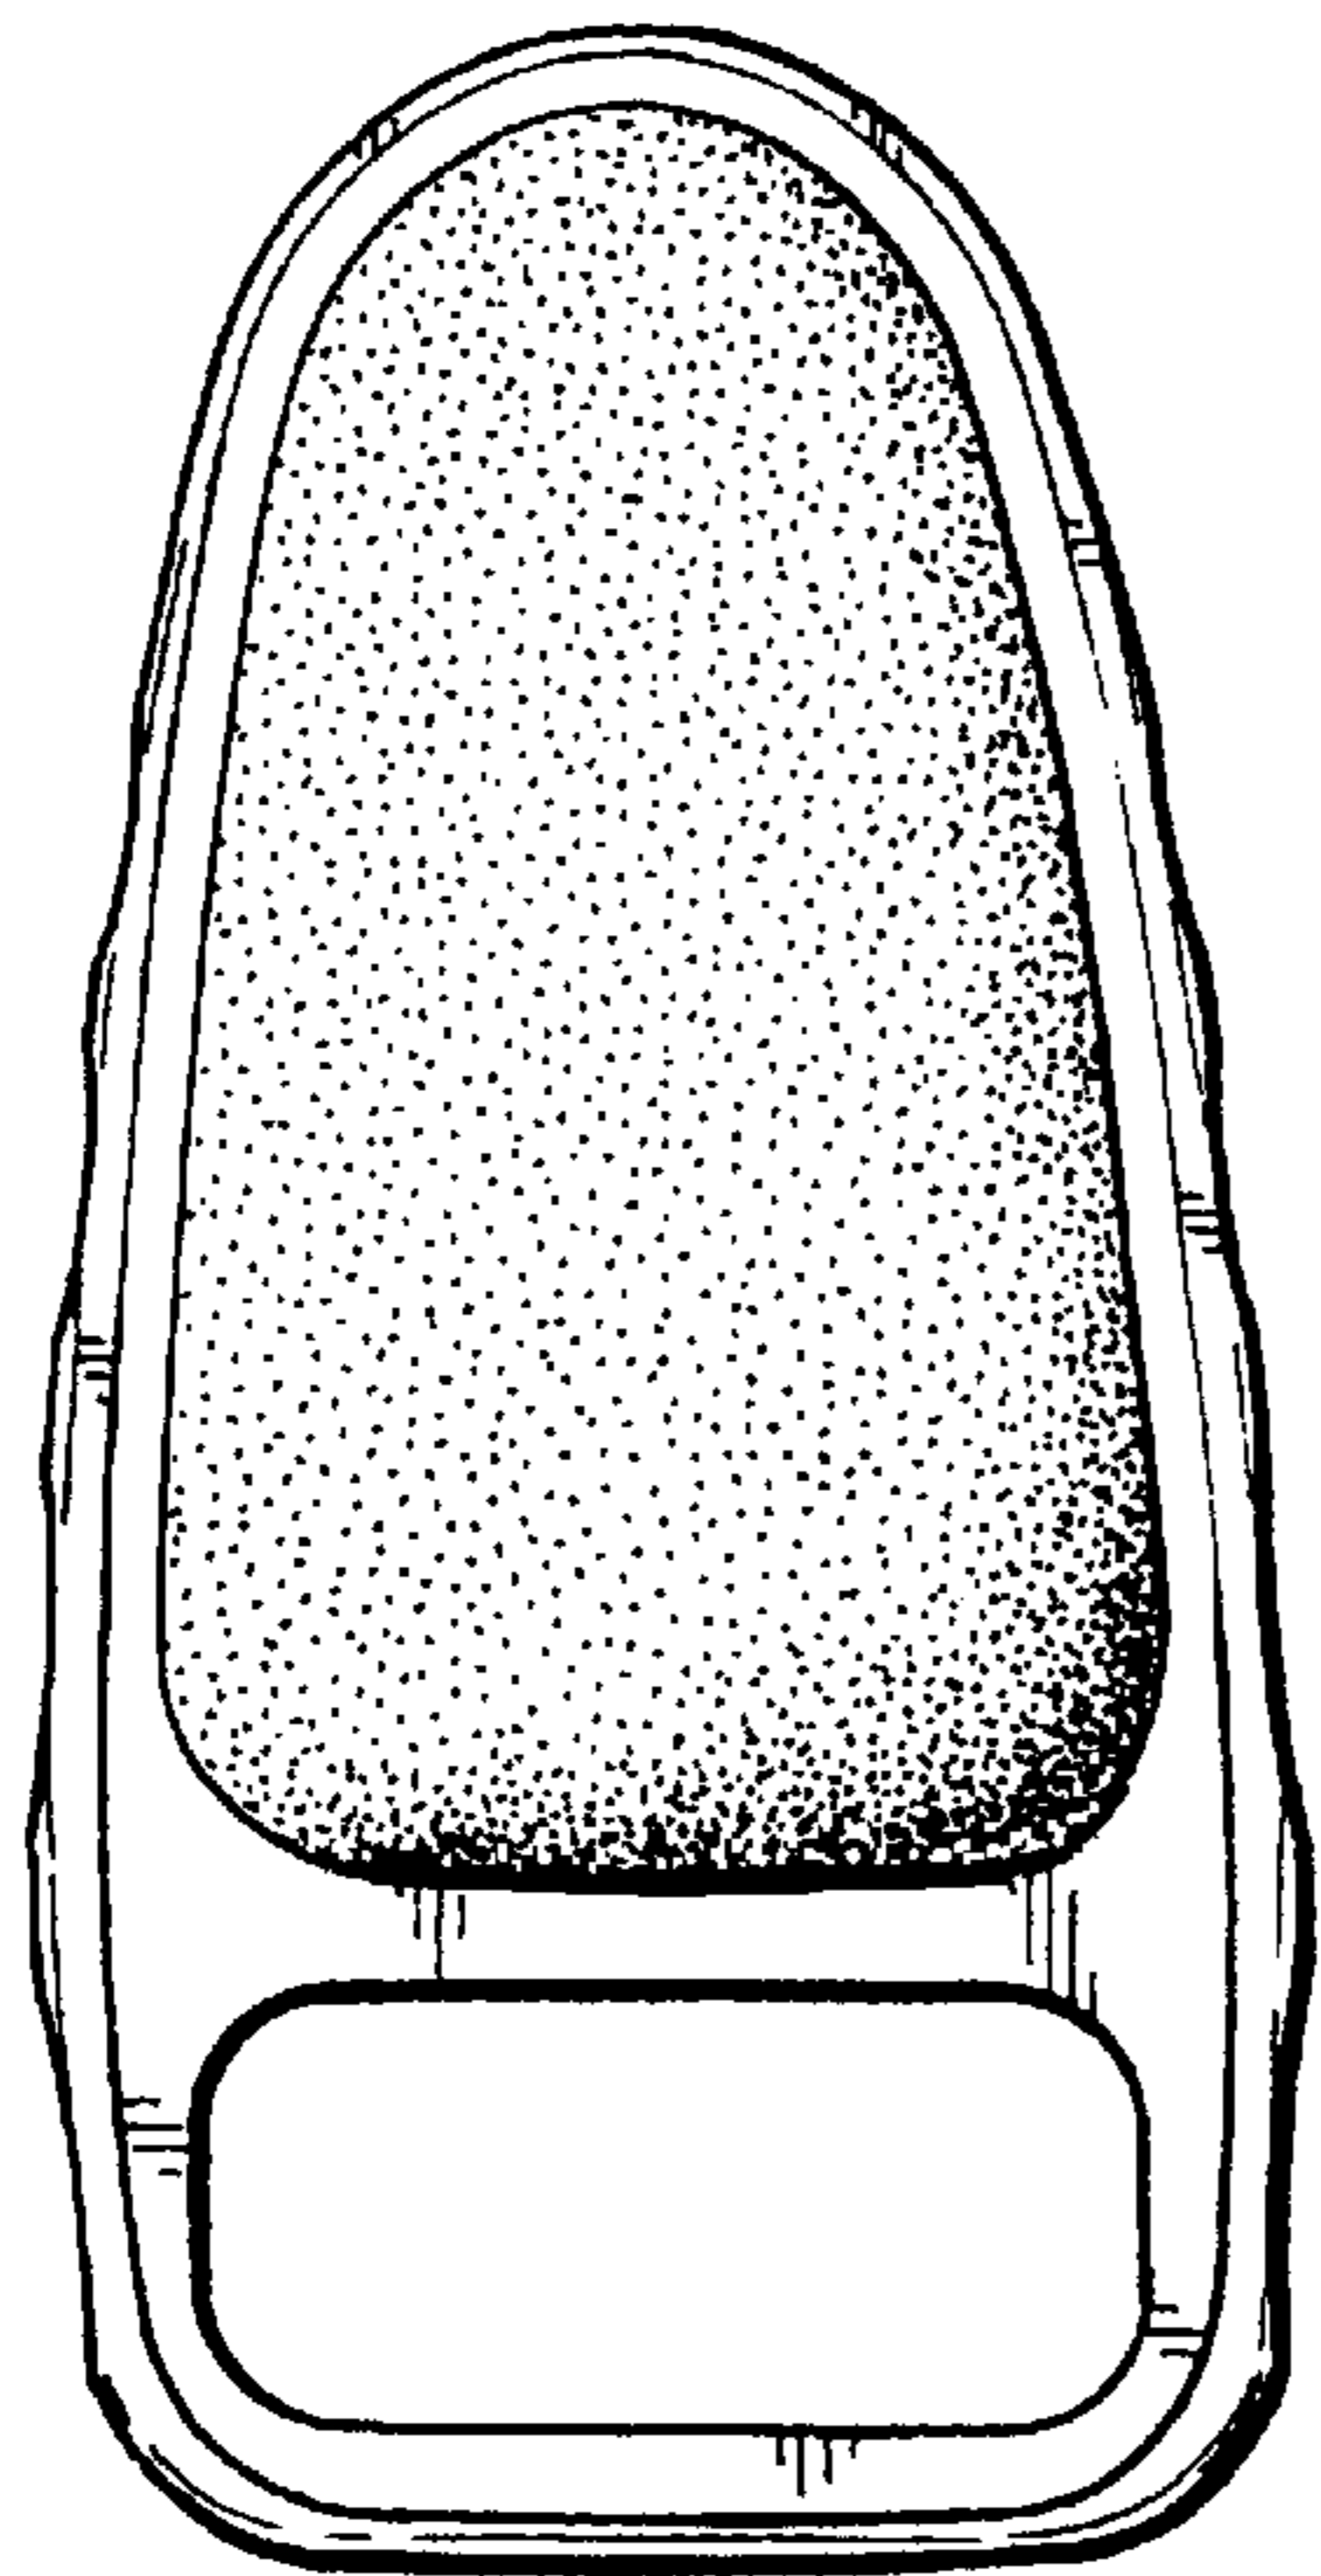


FIG. 2

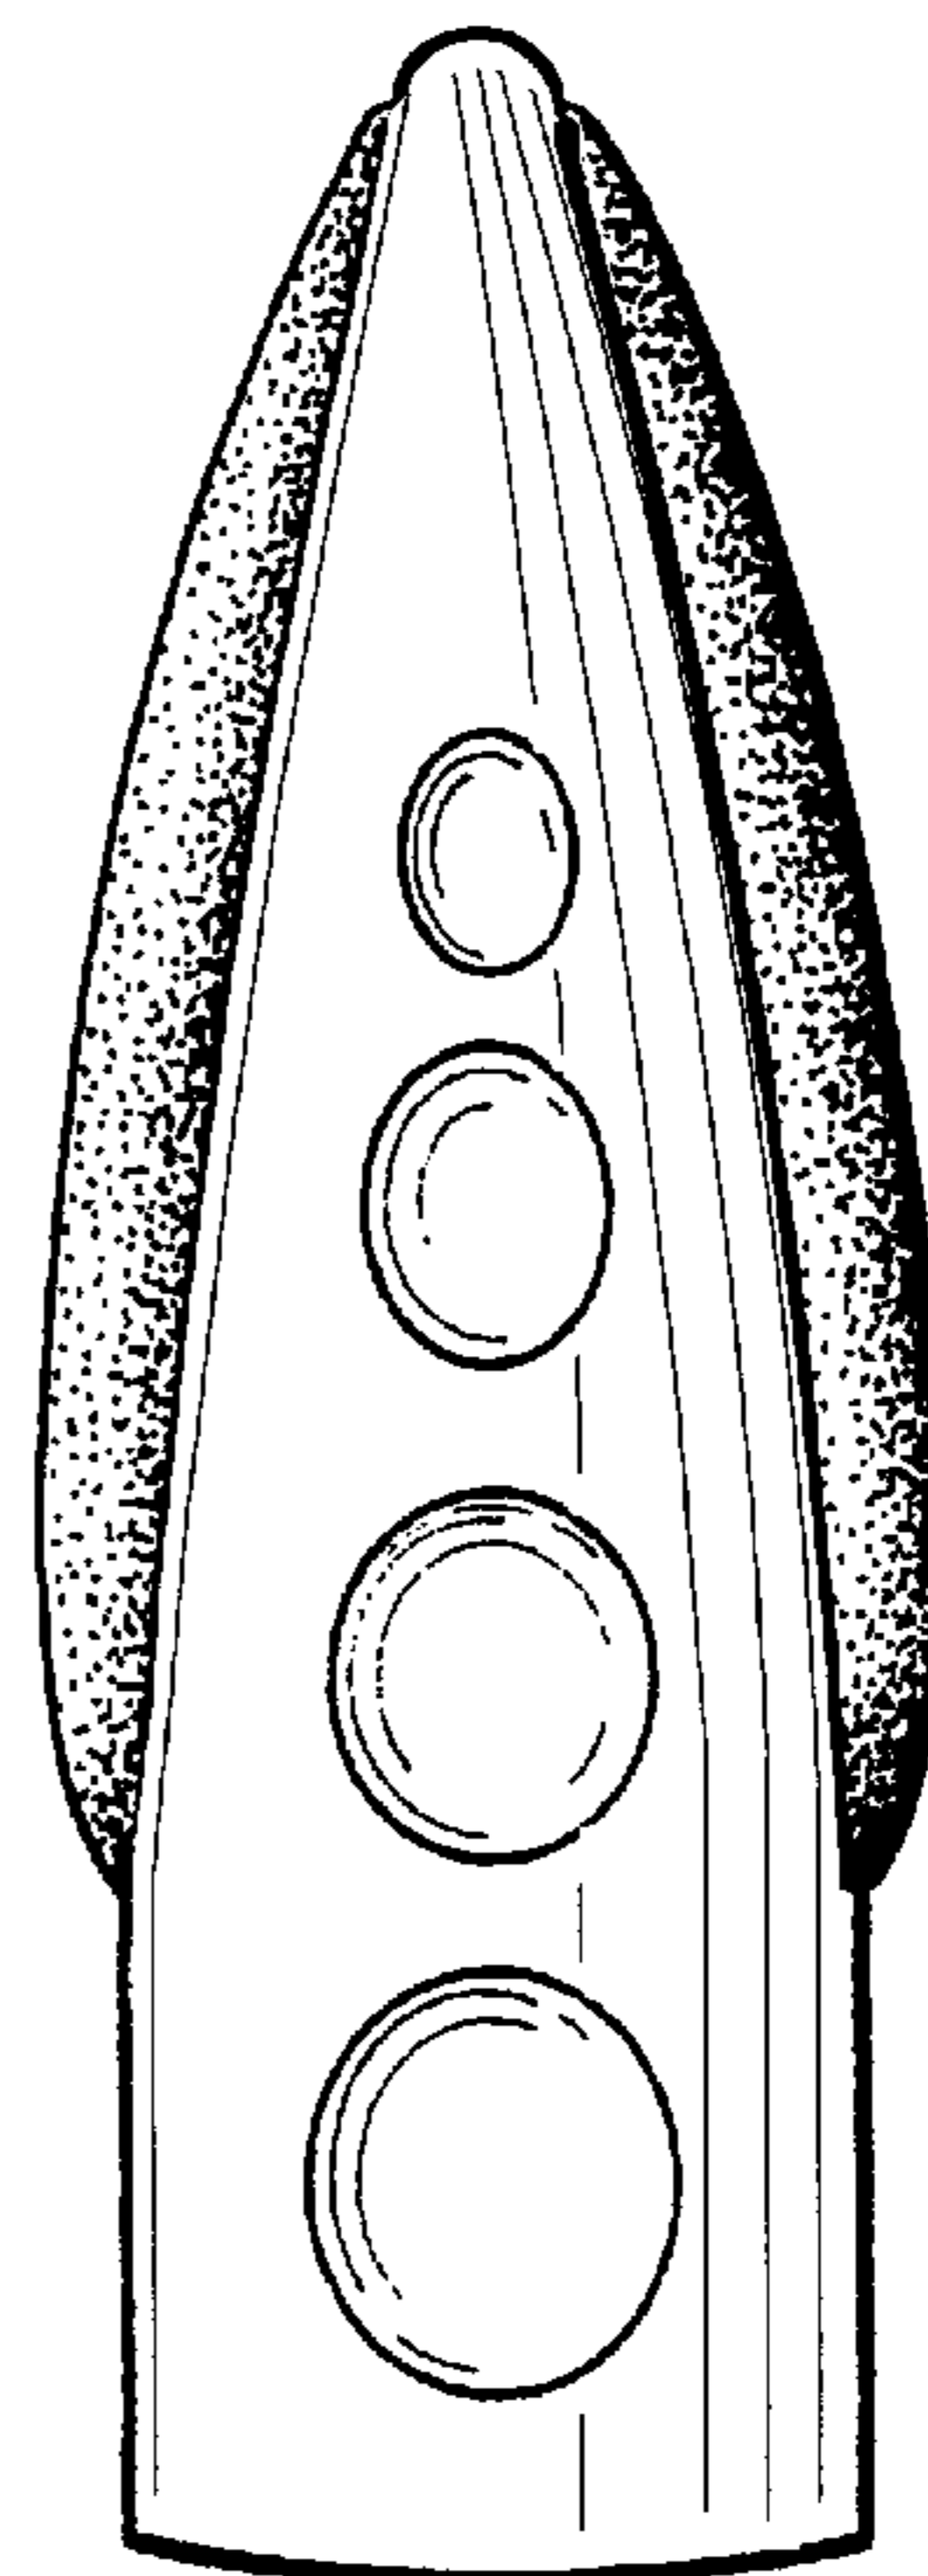


FIG. 3

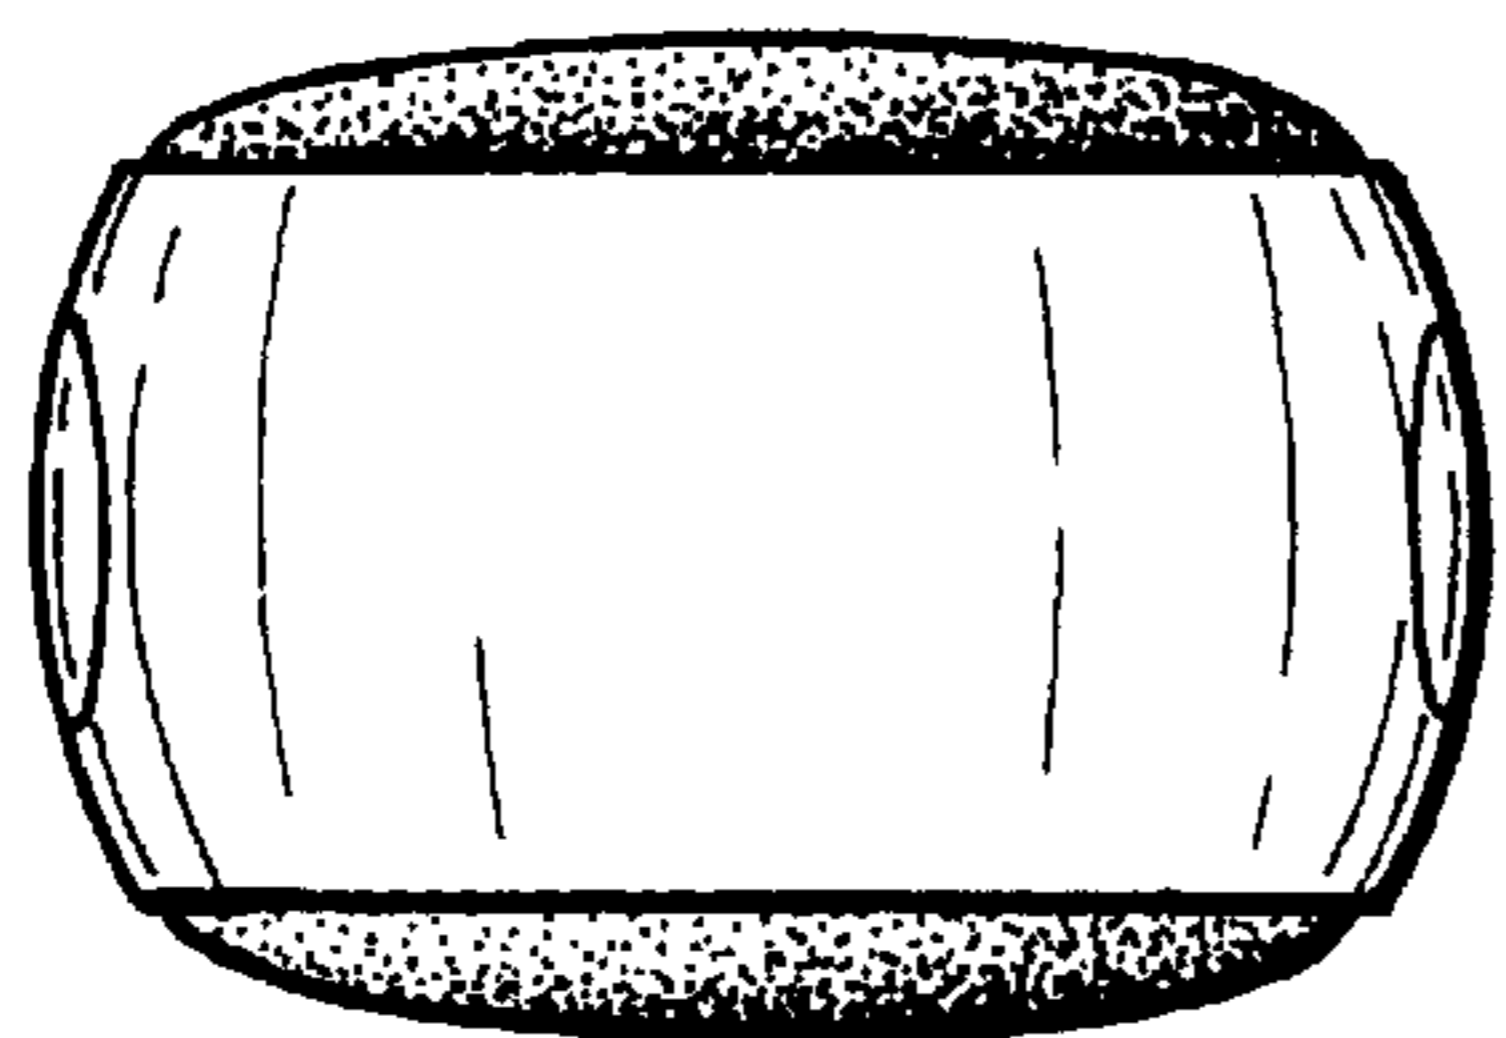


FIG. 5