



US00D449886B1

(12) **United States Design Patent**
Tetzlaff et al.

(10) **Patent No.:** **US D449,886 S**

(45) **Date of Patent:** **** Oct. 30, 2001**

(54) **FORCEPS WITH DISPOSABLE ELECTRODE**

5,250,047 10/1993 Rydell .
5,258,006 11/1993 Rydell et al. .

(75) Inventors: **Philip Mark Tetzlaff**, Golden; **Steven Paul Buysse**, Longmont; **Kate Ryland Lawes**, Boulder; **Dale Francis Schmaltz**, Fort Collins, all of CO (US)

(List continued on next page.)

FOREIGN PATENT DOCUMENTS

401367 11/1974 (SU) .

OTHER PUBLICATIONS

Sigel et al., "The Mechanism of Blood Vessel Closure by High Frequency Electrocoagulation", *Surgery Gynecology & Obstetrics*, Oct. 1965 pp. 823-831.

Bergdahl et al. "Studies on Coagulation and the Development of an Automatic Computerized Bipolar Coagulator", *J. Neurosurg*, vol. 75, Jul. 1991, pp. 148-151.

International Search Report—PCT/US98/18640.

International Search Report—PCT/US98/23950.

Primary Examiner—Louis S. Zarfes

Assistant Examiner—Eric Watterson

(73) Assignee: **Sherwood Services AG**, Schaffhausen (CH)

(**) Term: **14 Years**

(21) Appl. No.: **29/095,485**

(22) Filed: **Oct. 23, 1998**

(51) **LOC (7) Cl.** **24-02**

(52) **U.S. Cl.** **D24/144**

(58) **Field of Search** D24/143, 144,
D24/148; 606/40, 41, 45, 51, 52, 50, 205-208

(56) **References Cited**

U.S. PATENT DOCUMENTS

371,664	10/1887	Brannan et al. .
702,472	6/1902	Pignolet .
728,883	5/1903	Downes .
1,586,645	6/1926	Bierman .
2,002,594	5/1935	Wappler et al. .
2,176,479	10/1939	Willis .
3,651,811	3/1972	Hildebrandt et al. .
3,920,021	11/1975	Hiltebrandt .
3,938,527	2/1976	Rioux et al. .
3,952,749	4/1976	Fridolph et al. .
4,005,714	2/1977	Hiltebrandt .
4,370,980	2/1983	Lottick .
4,552,143	11/1985	Lottick .
4,597,379	7/1986	Kihn et al. .
4,671,274	6/1987	Sorochenko .
4,685,459	8/1987	Koch et al. .
4,887,612	12/1989	Esser et al. .
4,938,761	7/1990	Ensslin .
5,026,370	6/1991	Lottick .
5,116,332	5/1992	Lottick .
5,151,102	9/1992	Kamiyama et al. .
5,217,458	6/1993	Parins .

(57) **CLAIM**

We claim the ornamental design for a forceps with disposable electrode, as shown.

DESCRIPTION

FIG. 1 is a perspective view of a forceps with disposable electrode showing our new design;

FIG. 2 is a left side view of the forceps with disposable electrode;

FIG. 3 is a rear view of the forceps with disposable electrode;

FIG. 4 is a right side view of the forceps with disposable electrode;


FIG. 5 is a front view of the forceps with disposable electrode;

FIG. 6 is a top view of the forceps with disposable electrode assembly; and,

FIG. 7 is a bottom view of the forceps with disposable electrode.

The end portion shown broken away for ease of illustration.

1 Claim, 4 Drawing Sheets

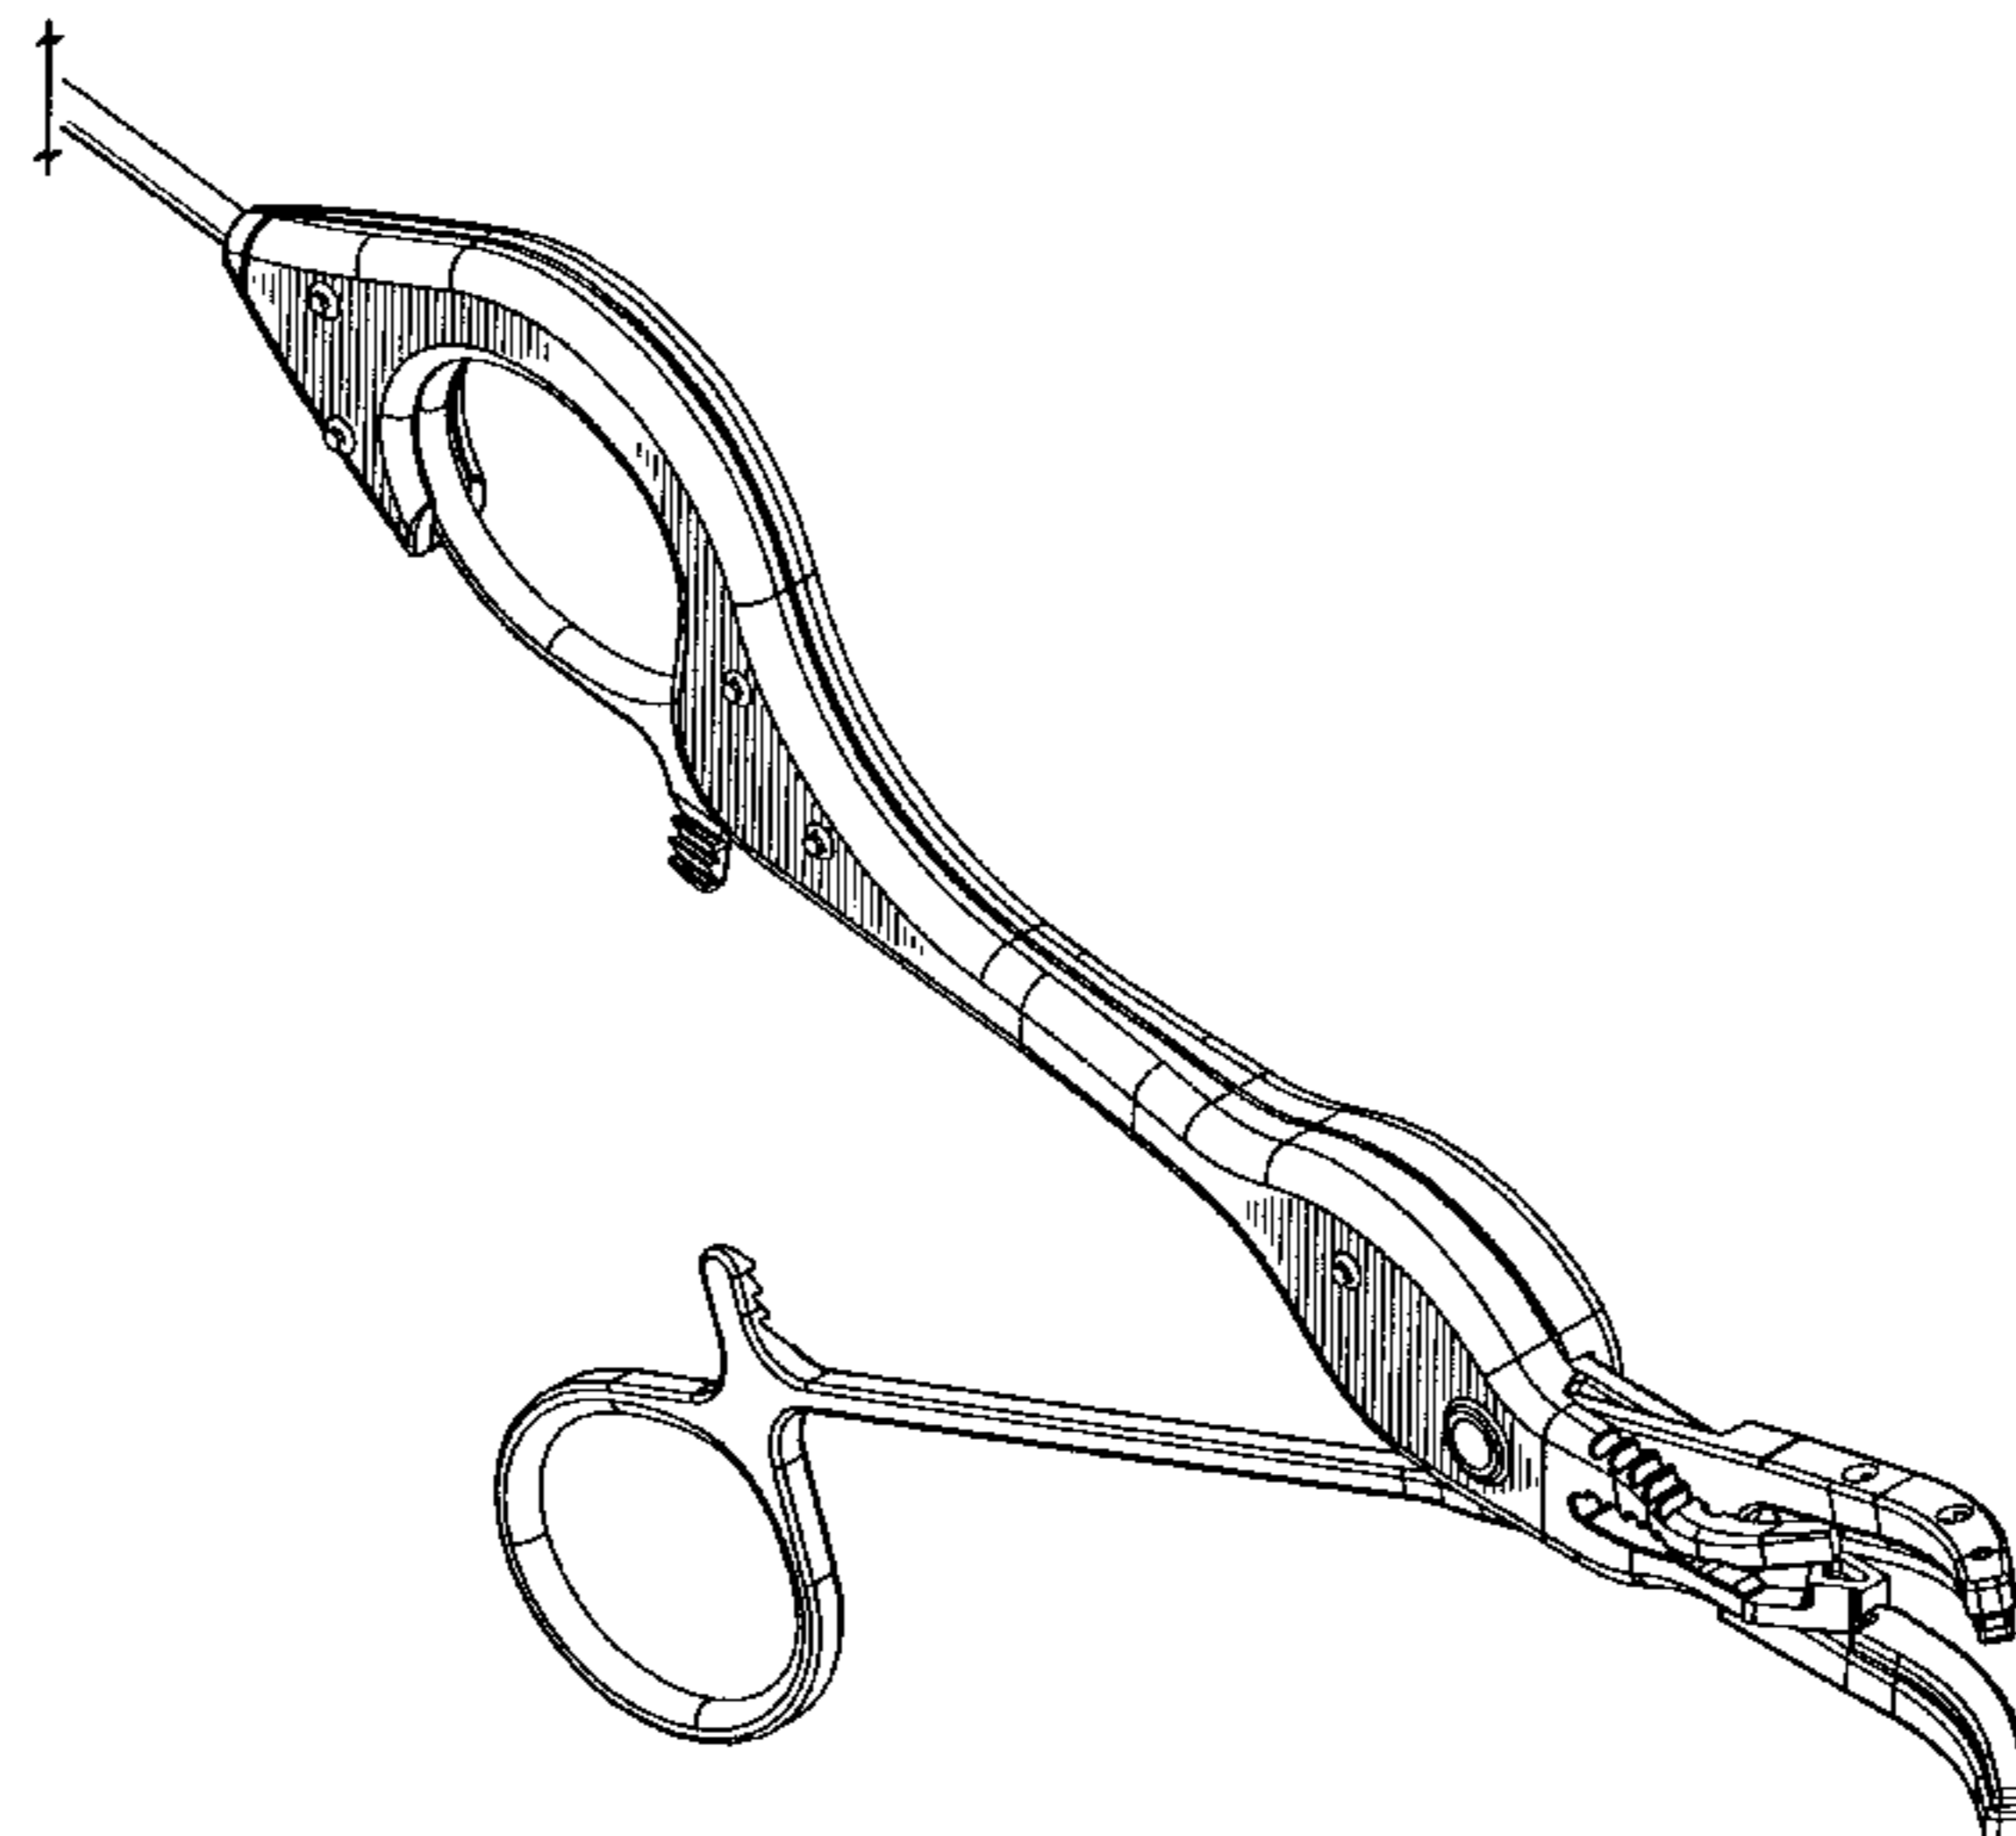

US D449,886 S

Page 2

U.S. PATENT DOCUMENTS

5,277,201	1/1994	Stern .	5,540,684	7/1996	Hassler, Jr. .	
5,324,289	6/1994	Eggers .	5,558,672	9/1996	Edwards et al. .	
5,330,471	7/1994	Eggers .	5,569,241	10/1996	Edwards .	
5,342,359	8/1994	Rydell .	5,573,535	11/1996	Viklund .	
5,352,222	10/1994	Rydell .	5,626,578	5/1997	Tihon .	
5,356,408	10/1994	Rydell .	5,626,609 *	5/1997	Zvenyatsky et al.	606/208
5,389,104	2/1995	Hahnen et al. .	5,637,110	6/1997	Pennybacker et al. .	
5,391,166	2/1995	Eggers .	5,658,281	8/1997	Heard .	
5,403,312	4/1995	Yates et al. .	5,667,526	9/1997	Levin .	
5,431,674	7/1995	Basile et al. .	5,674,220	10/1997	Fox et al. .	
5,443,463	8/1995	Stern et al. .	5,693,051	12/1997	Schulze et al. .	
5,443,464	8/1995	Russell et al. .	5,700,261	12/1997	Brinkerhoff .	
5,445,658	8/1995	Durrfeld et al. .	5,702,390	12/1997	Austin et al. .	
5,456,684	10/1995	Schmidt et al. .	5,735,849 *	4/1998	Baden et al.	606/51
5,462,546	10/1995	Rydell .	5,766,166	6/1998	Hooven .	
5,472,443	12/1995	Cordis et al. .	5,769,849	6/1998	Eggers .	
5,478,351	12/1995	Meade et al. .	5,776,128	7/1998	Eggers .	
5,484,436	1/1996	Eggers et al. .	5,776,130	7/1998	Buysse et al. .	
5,509,922	4/1996	Aranyi et al. .	5,817,128 *	10/1998	Storz	606/205
5,527,313	6/1996	Scott et al. .	5,827,281	10/1998	Levin .	
5,531,744	7/1996	Nardella et al. .				

* cited by examiner

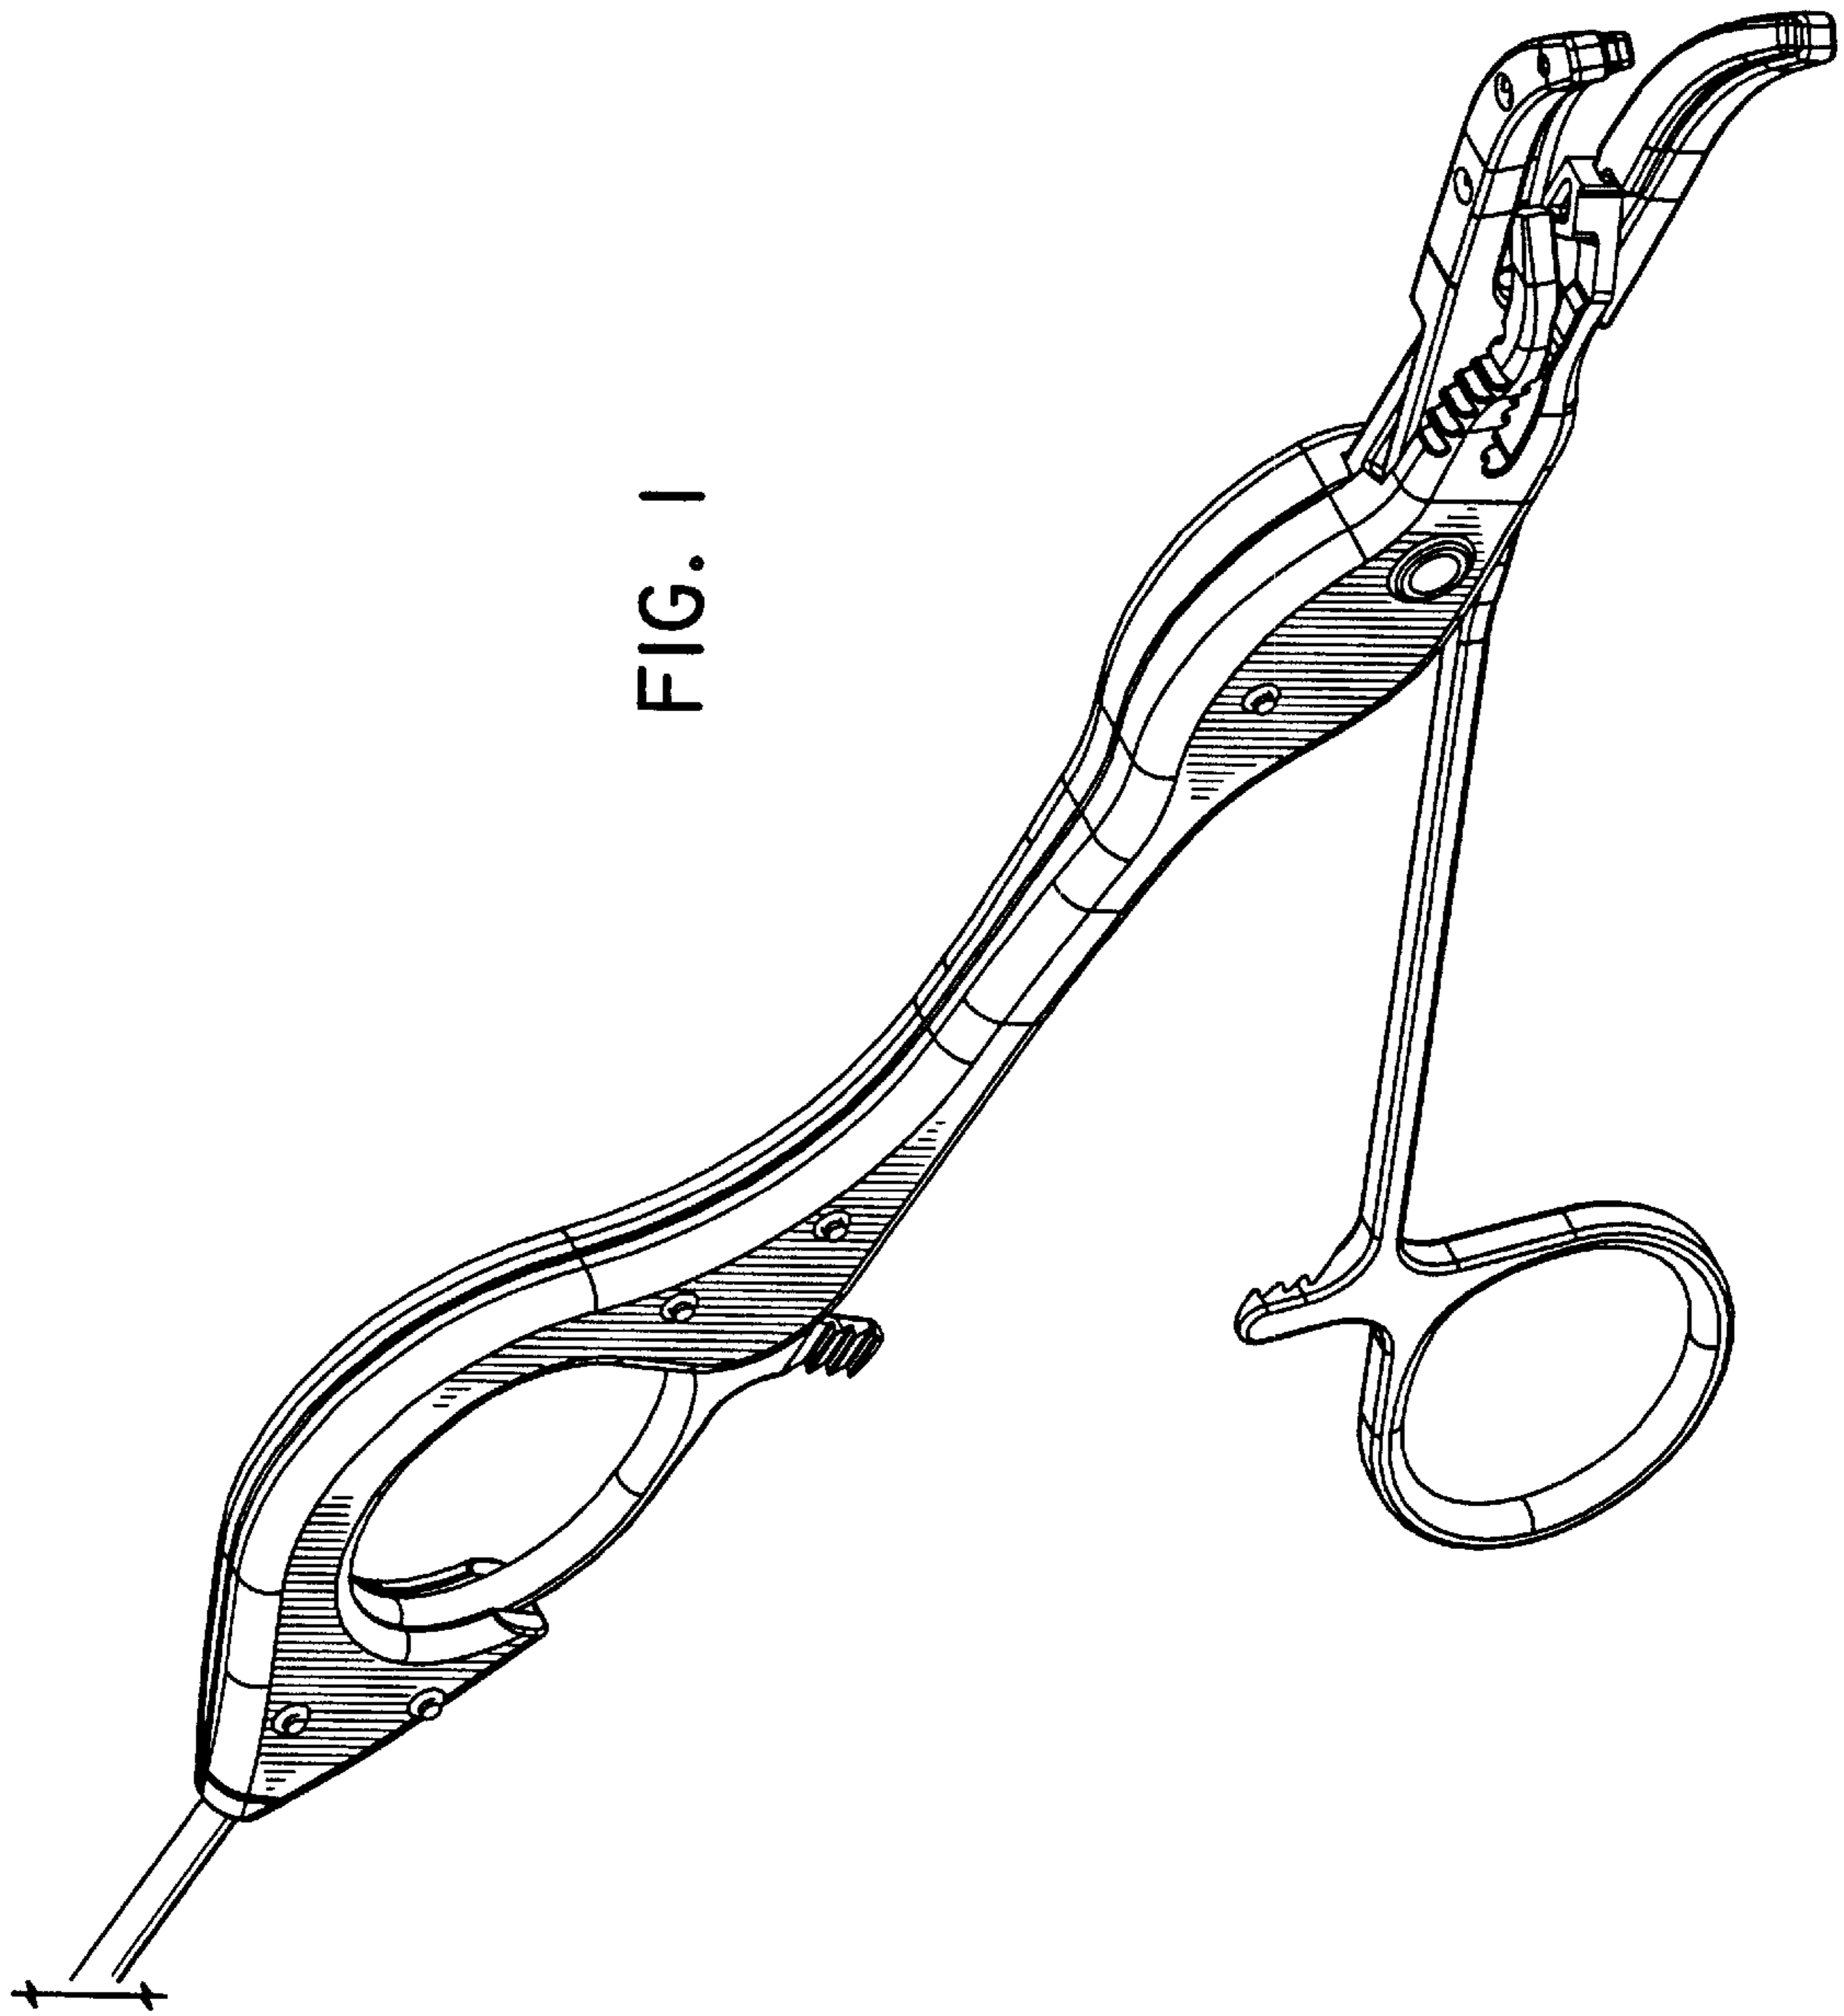


FIG. 1

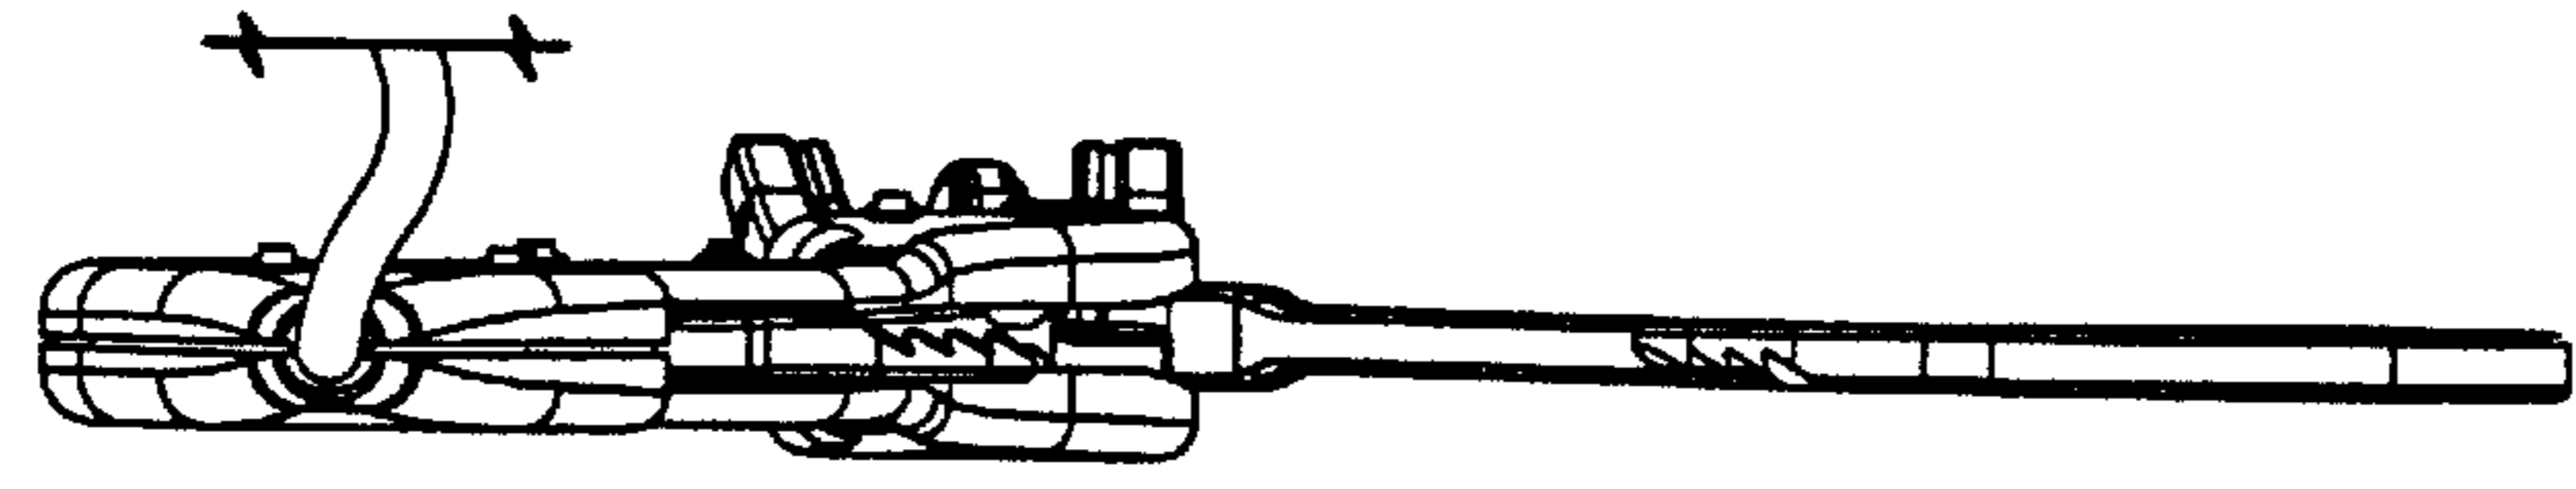


FIG. 3

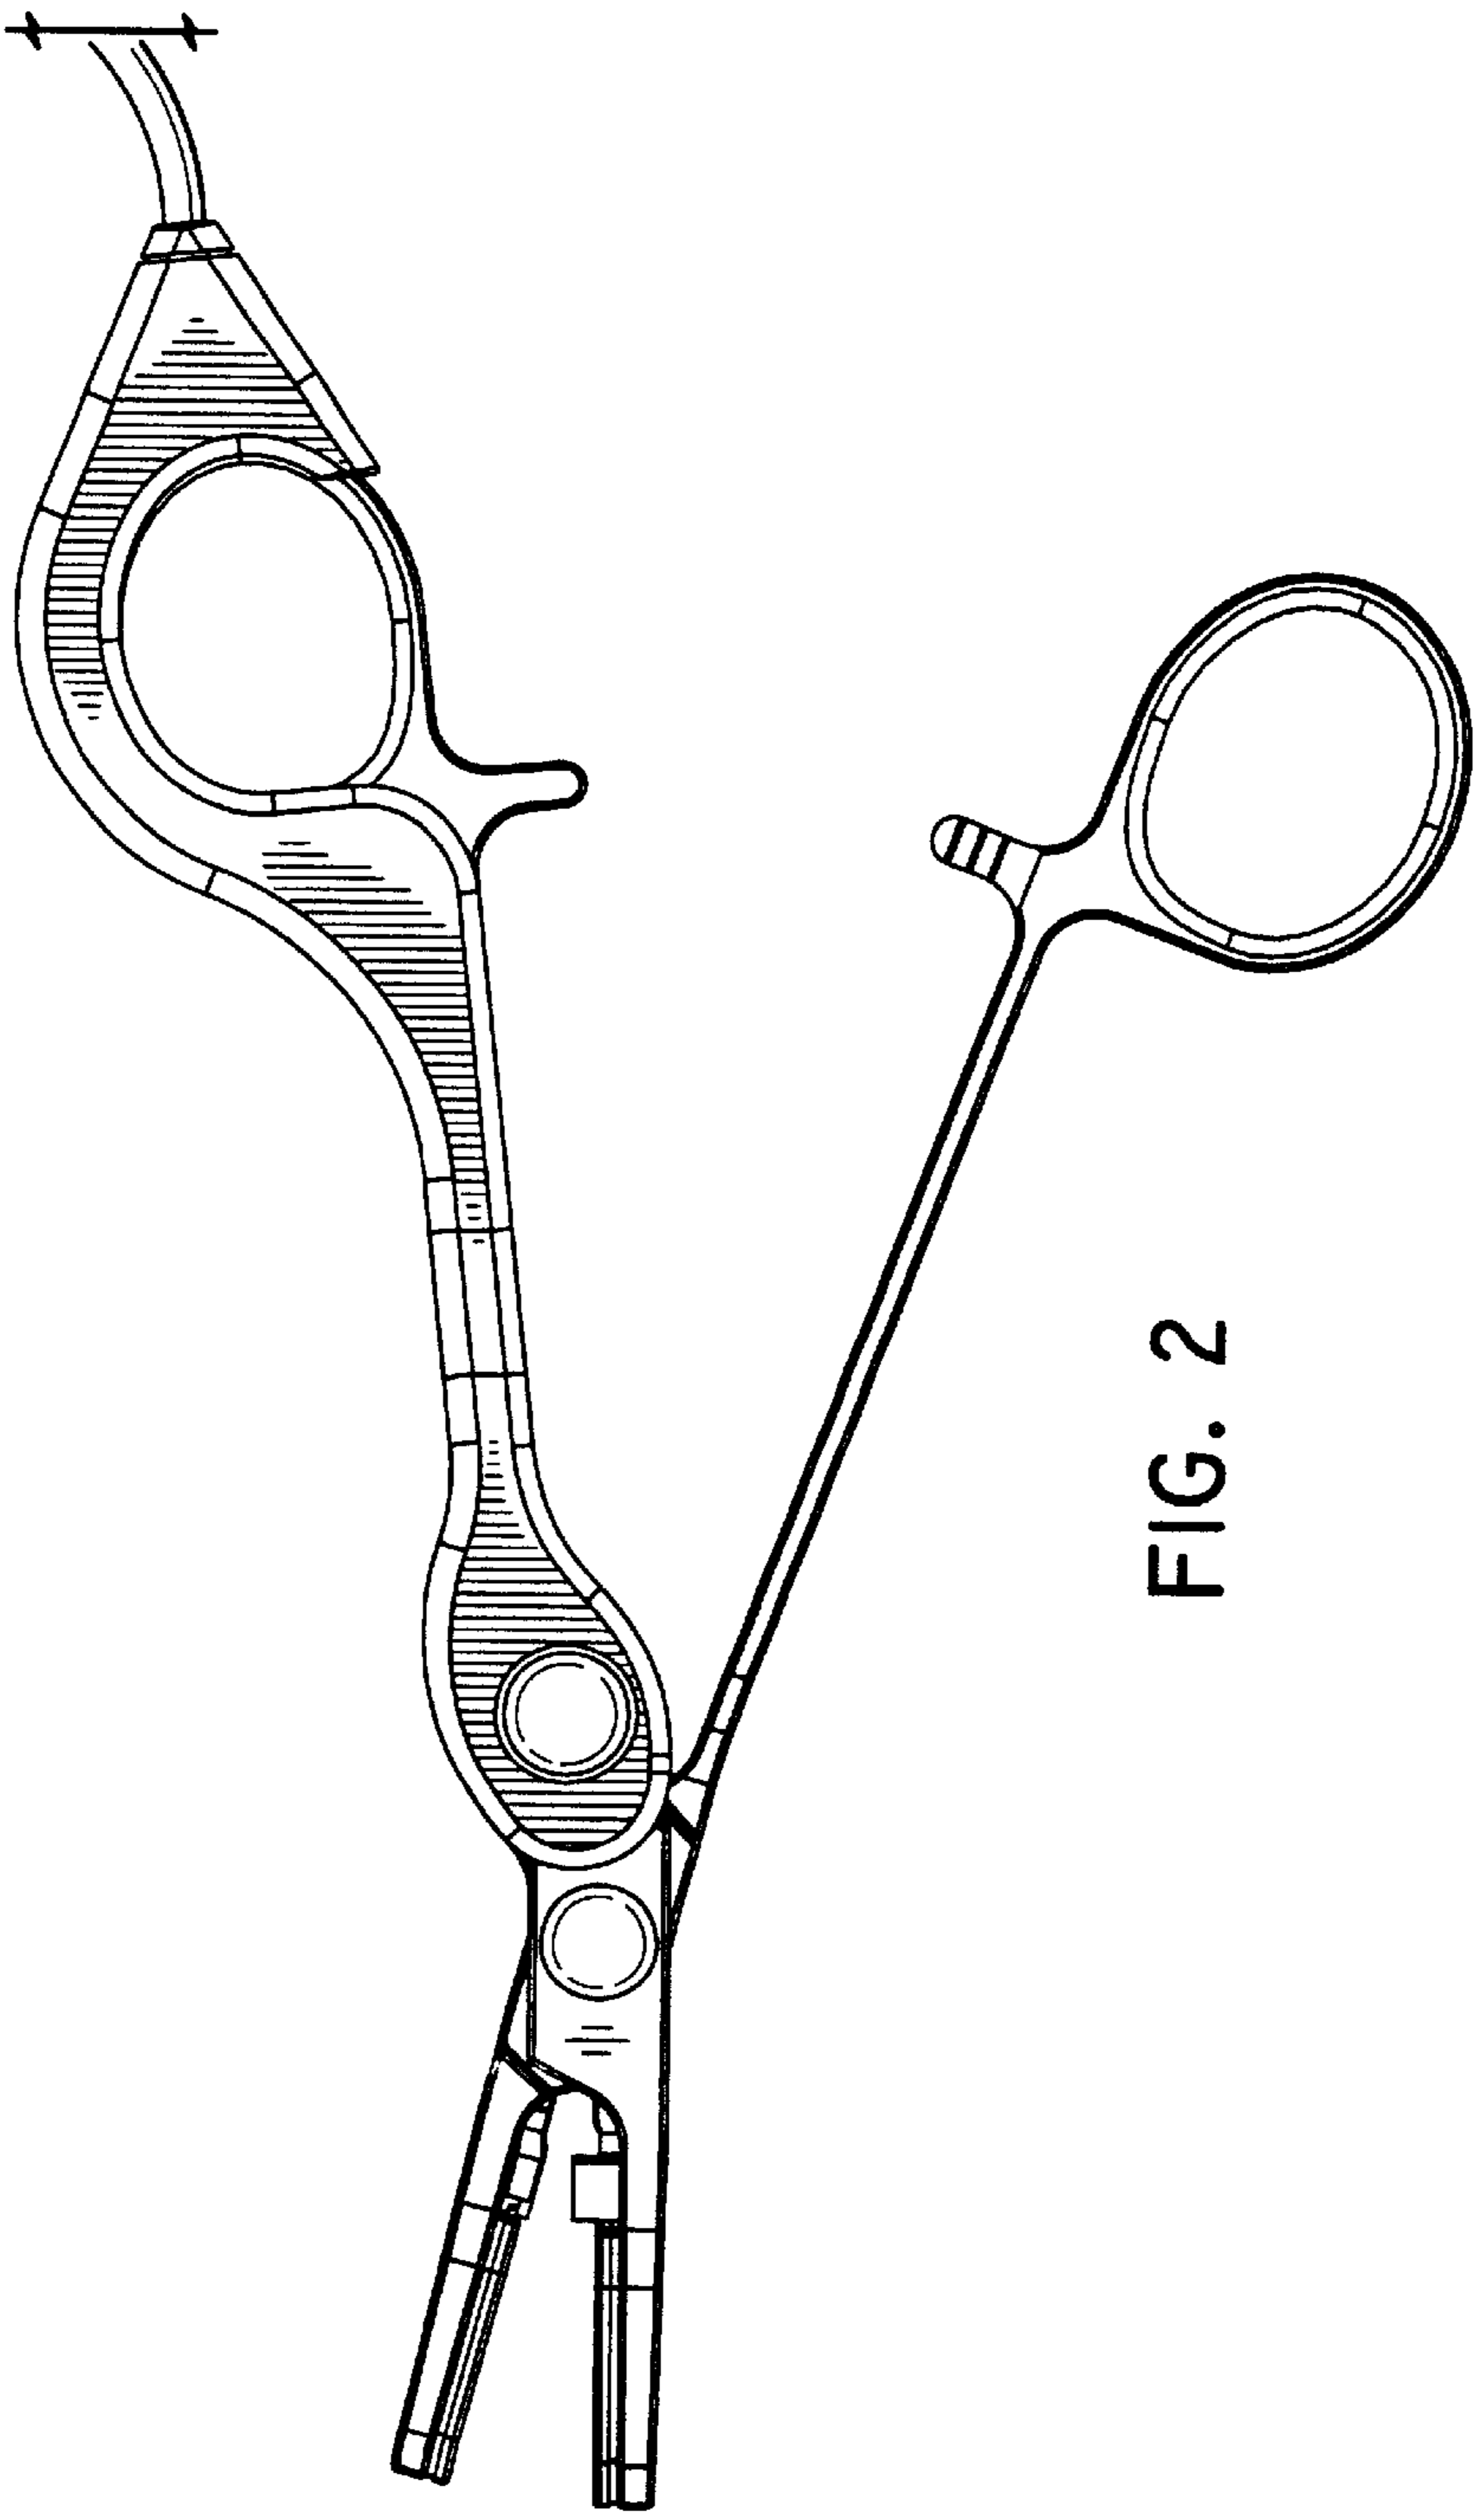


FIG. 2

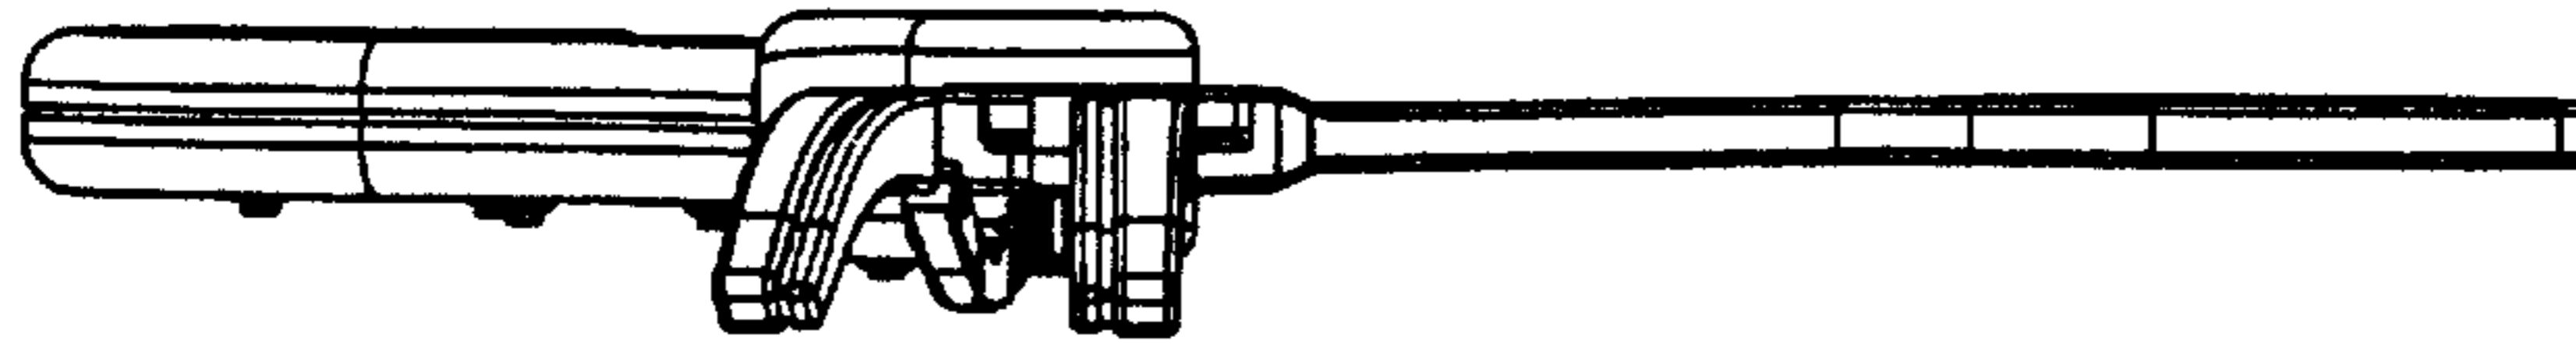


FIG. 5

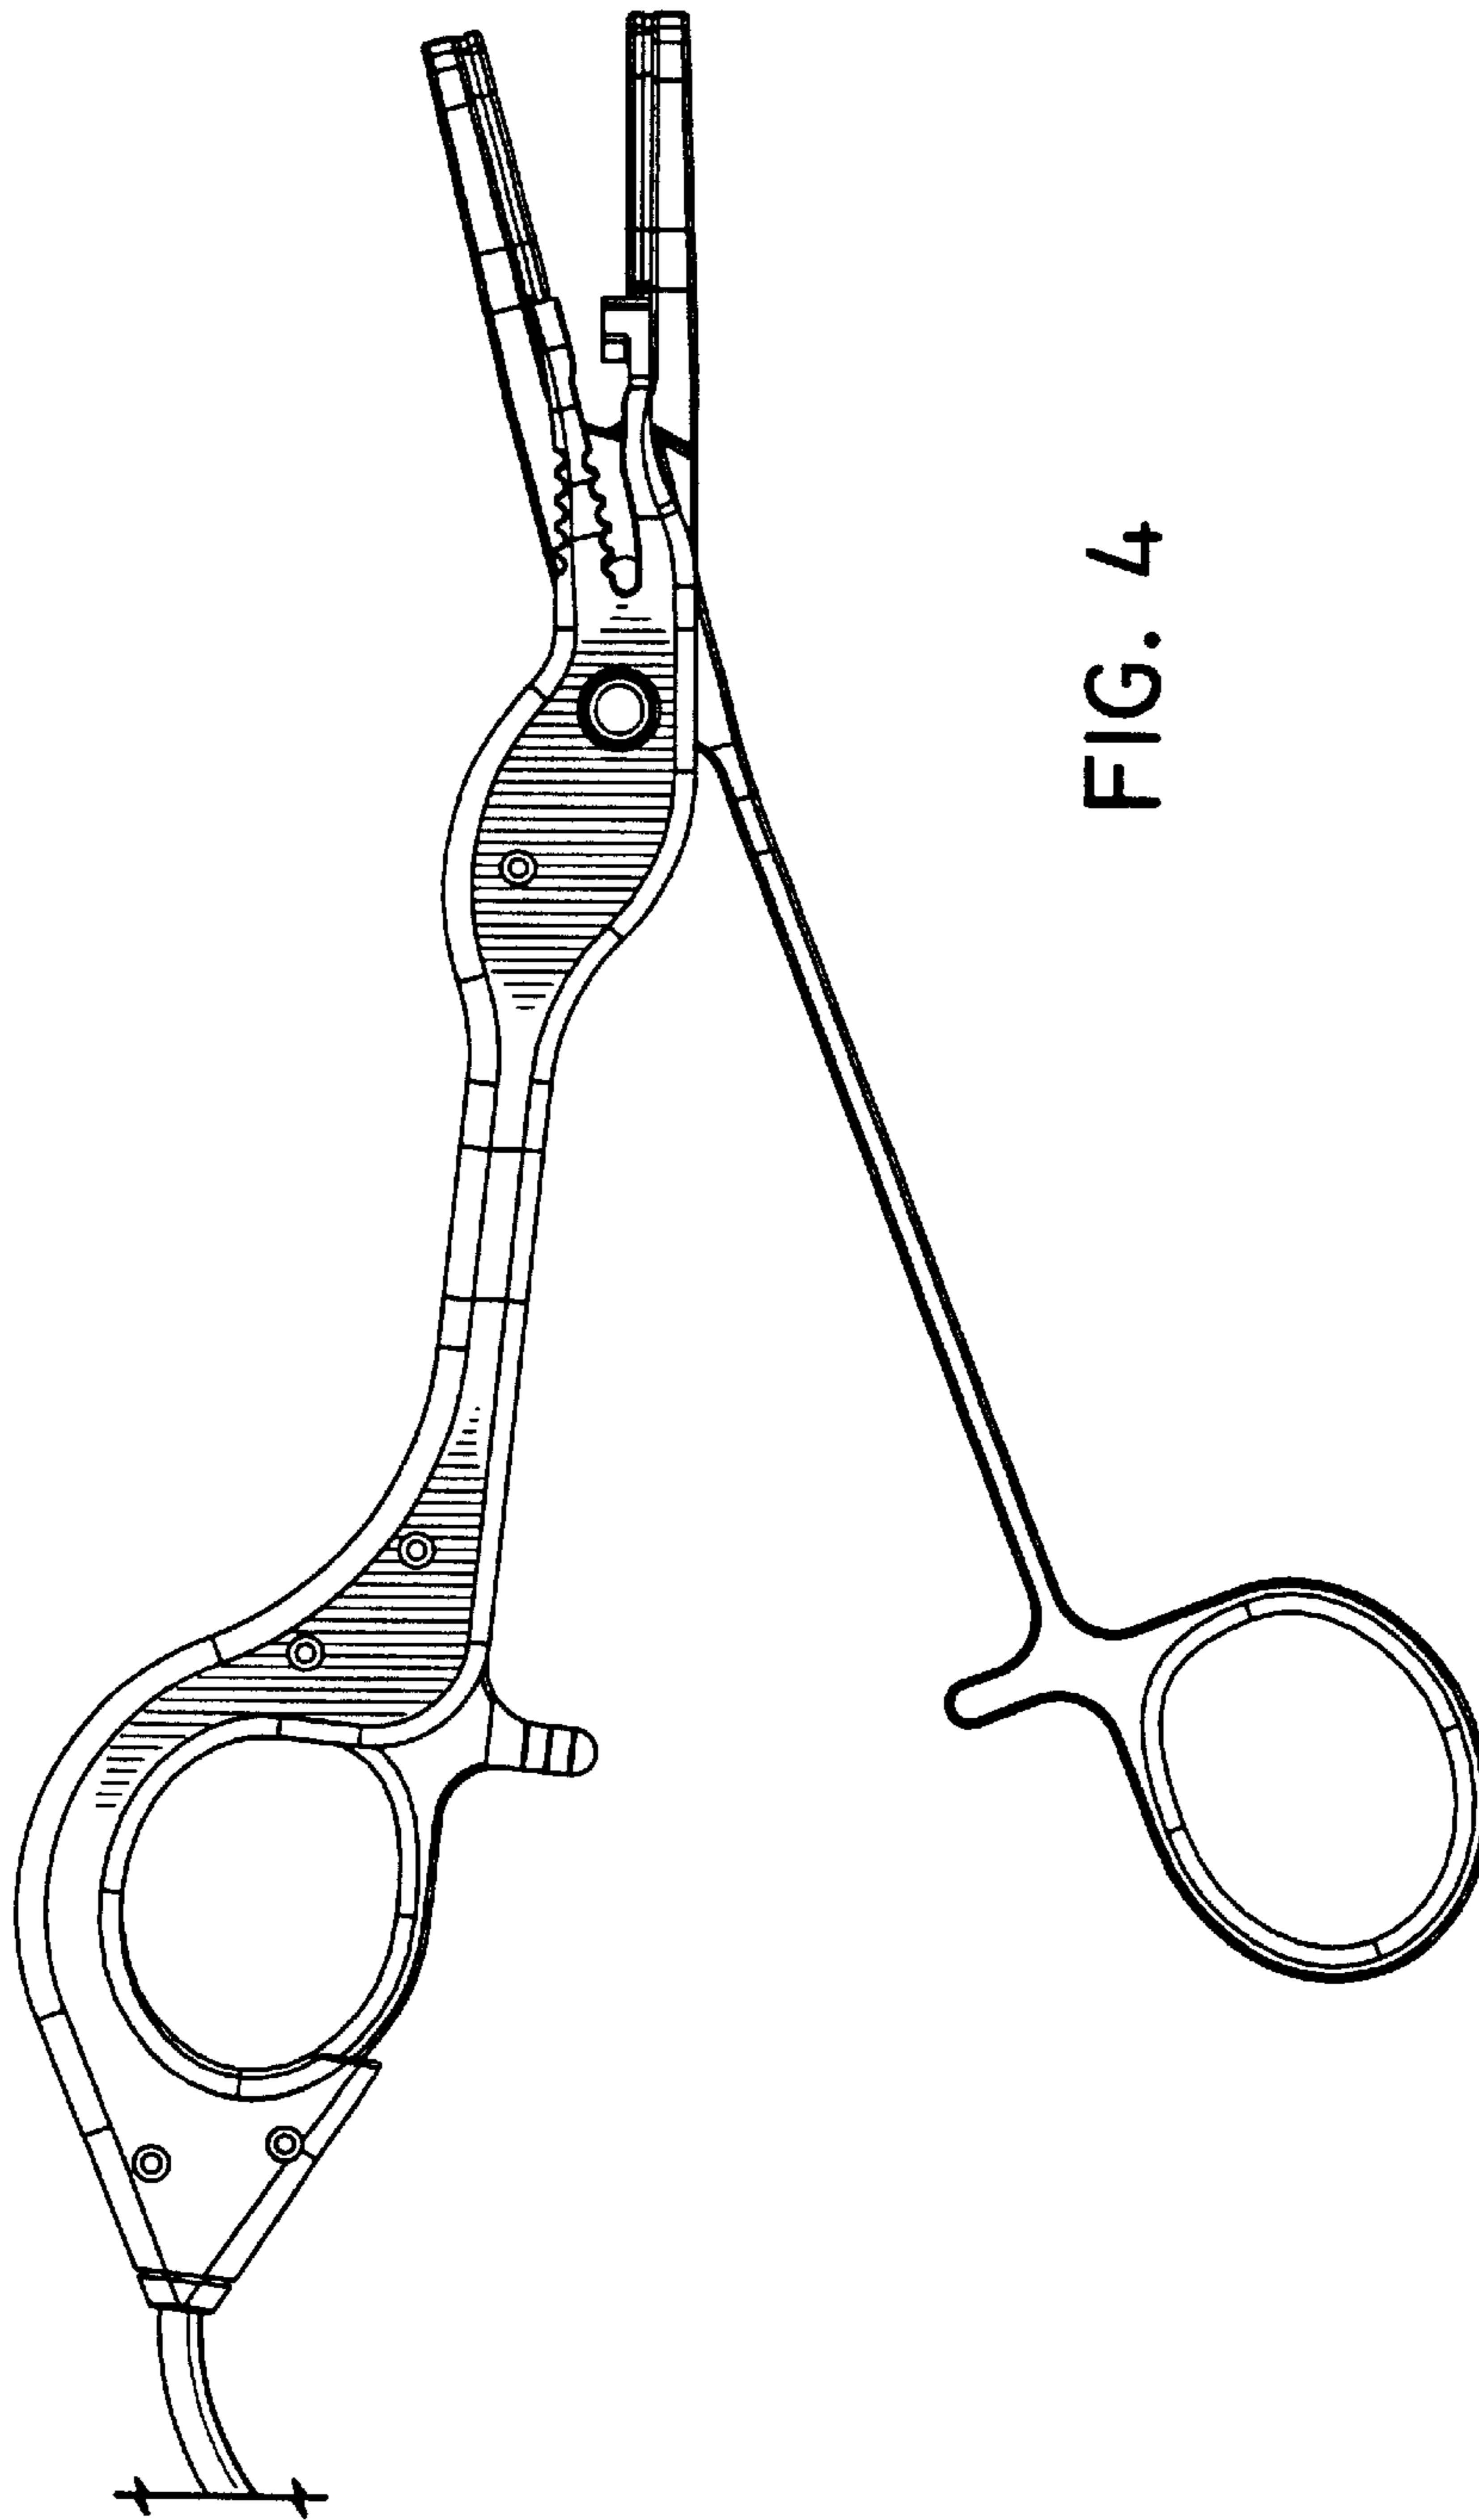


FIG. 4

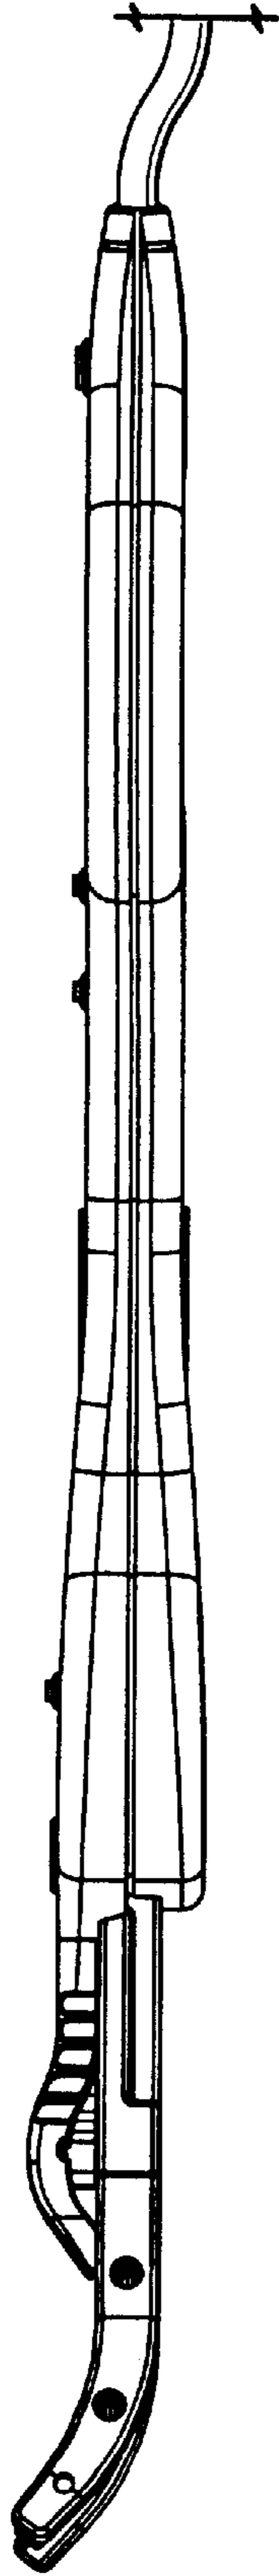


FIG. 6

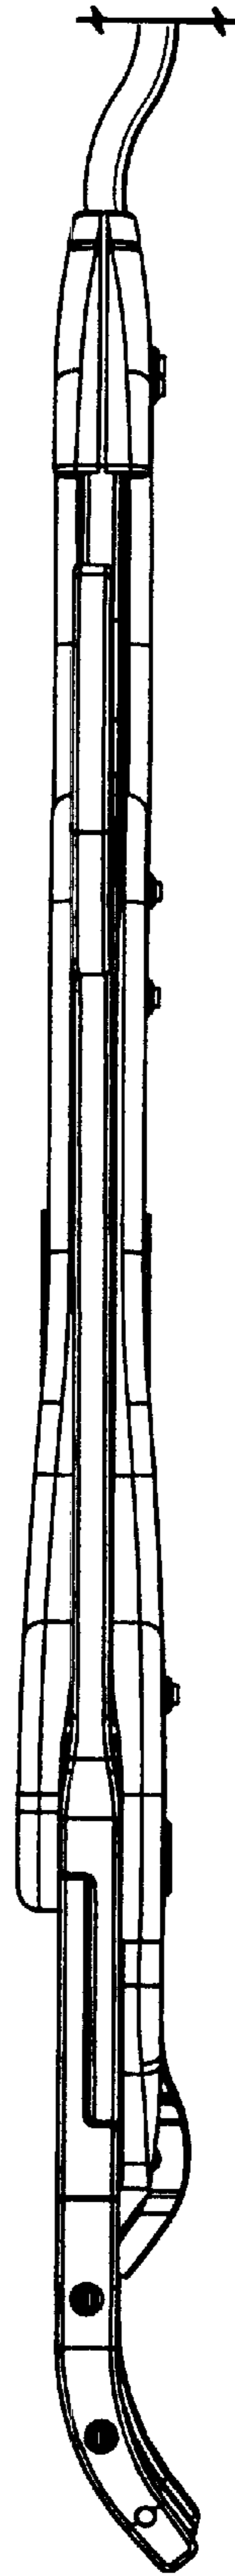


FIG. 7