



US00D456524S

(12) **United States Design Patent**
Hehenberger

(10) **Patent No.:** **US D456,524 S**

(45) **Date of Patent:** **** Apr. 30, 2002**

(54) **LIQUID PERACETIC ACID STERILIZATION INDICATOR**

(75) Inventor: **Rodney K. Hehenberger**, Apple Valley, MN (US)

(73) Assignee: **3M Innovative Properties Company**, St. Paul, MN (US)

(**) Term: **14 Years**

(21) Appl. No.: **29/085,454**

(22) Filed: **Mar. 24, 1998**

(51) **LOC (7) Cl.** **24-01**

(52) **U.S. Cl.** **D24/217**

(58) **Field of Search** D24/217, 224, D24/232; 206/528, 530, 461, 467, 468, 469, 470, 471; D9/306, 337; 422/50, 55, 58, 61; 435/31

(56) **References Cited**

U.S. PATENT DOCUMENTS

866,995 A *	9/1907	Wright	206/367
1,024,259 A *	4/1912	Henderson	206/524.1 X
D222,516 S	10/1971	Kelson	D24/99
4,113,097 A *	9/1978	Fin	206/528 X
D263,622 S *	3/1982	Harsson	D24/224 X
D265,981 S	8/1982	Chizacky	D10/87
D286,947 S	12/1986	Wootton	D2/226
4,839,291 A *	6/1989	Welsh et al.	D24/217 X
4,914,034 A *	4/1990	Welsh et al.	435/296
5,167,923 A *	12/1992	Van Iperen	422/58
5,489,739 A *	2/1996	Curry et al.	220/908
5,895,627 A *	4/1999	Khachatoorian	422/58

OTHER PUBLICATIONS

Brochure entitled "ATI Monitoring—Loadtest Integrator Test Park for EO Gas" from PyMaH Corporation, 1995.
Brochure entitled "3M Attest Rapid Readout Biological Indicators" from 3M Health Care, 1997, Form 70-2009-0438-4(57.5)ii.

Brochure entitled "3M Comply Chemical Integrators" from 3M Health Care, 1997, Form 70-2009-0620-7.

Brochure entitled "3M Comply Steam and EO Chemical Integrator Test Packs" from 3M Health Care, 1997, Form 70-2009-0367-5(471)ii.

Brochure entitled "3M Technical Information Sheet—3M Comply (SteriGage) EO Chemical Integrator" from 3M Health Care, 1997, Form 70-2009-0709-8(127.5)ii.

Brochure entitled "Equipment Control—keeping the mechanics of sterilization process monitoring running smoothly" from 3M Health Care, 1997, Form 70-2009-0363-4(1271.5)DPI.

Brochure entitled "Pack Control—the inside counts in sterilization monitoring" from 3M Health Care, 1997, Form 70-2009-0362-6(461)ii.

* cited by examiner

Primary Examiner—Ian Simmons

(74) *Attorney, Agent, or Firm*—Jeffrey J. Hohenshell

(57) **CLAIM**

The ornamental design for a liquid peracetic acid sterilization indicator, as shown.

DESCRIPTION


FIG. 1 is a perspective view showing my new design.

FIG. 2 is a front view showing my new design, the rear view being a mirror image thereof.

FIG. 3 is a top view showing my new design, the bottom view being a mirror image thereof; and,

FIG. 4 is a left side view showing my new design, the right side being a mirror image thereof.

1 Claim, 1 Drawing Sheet

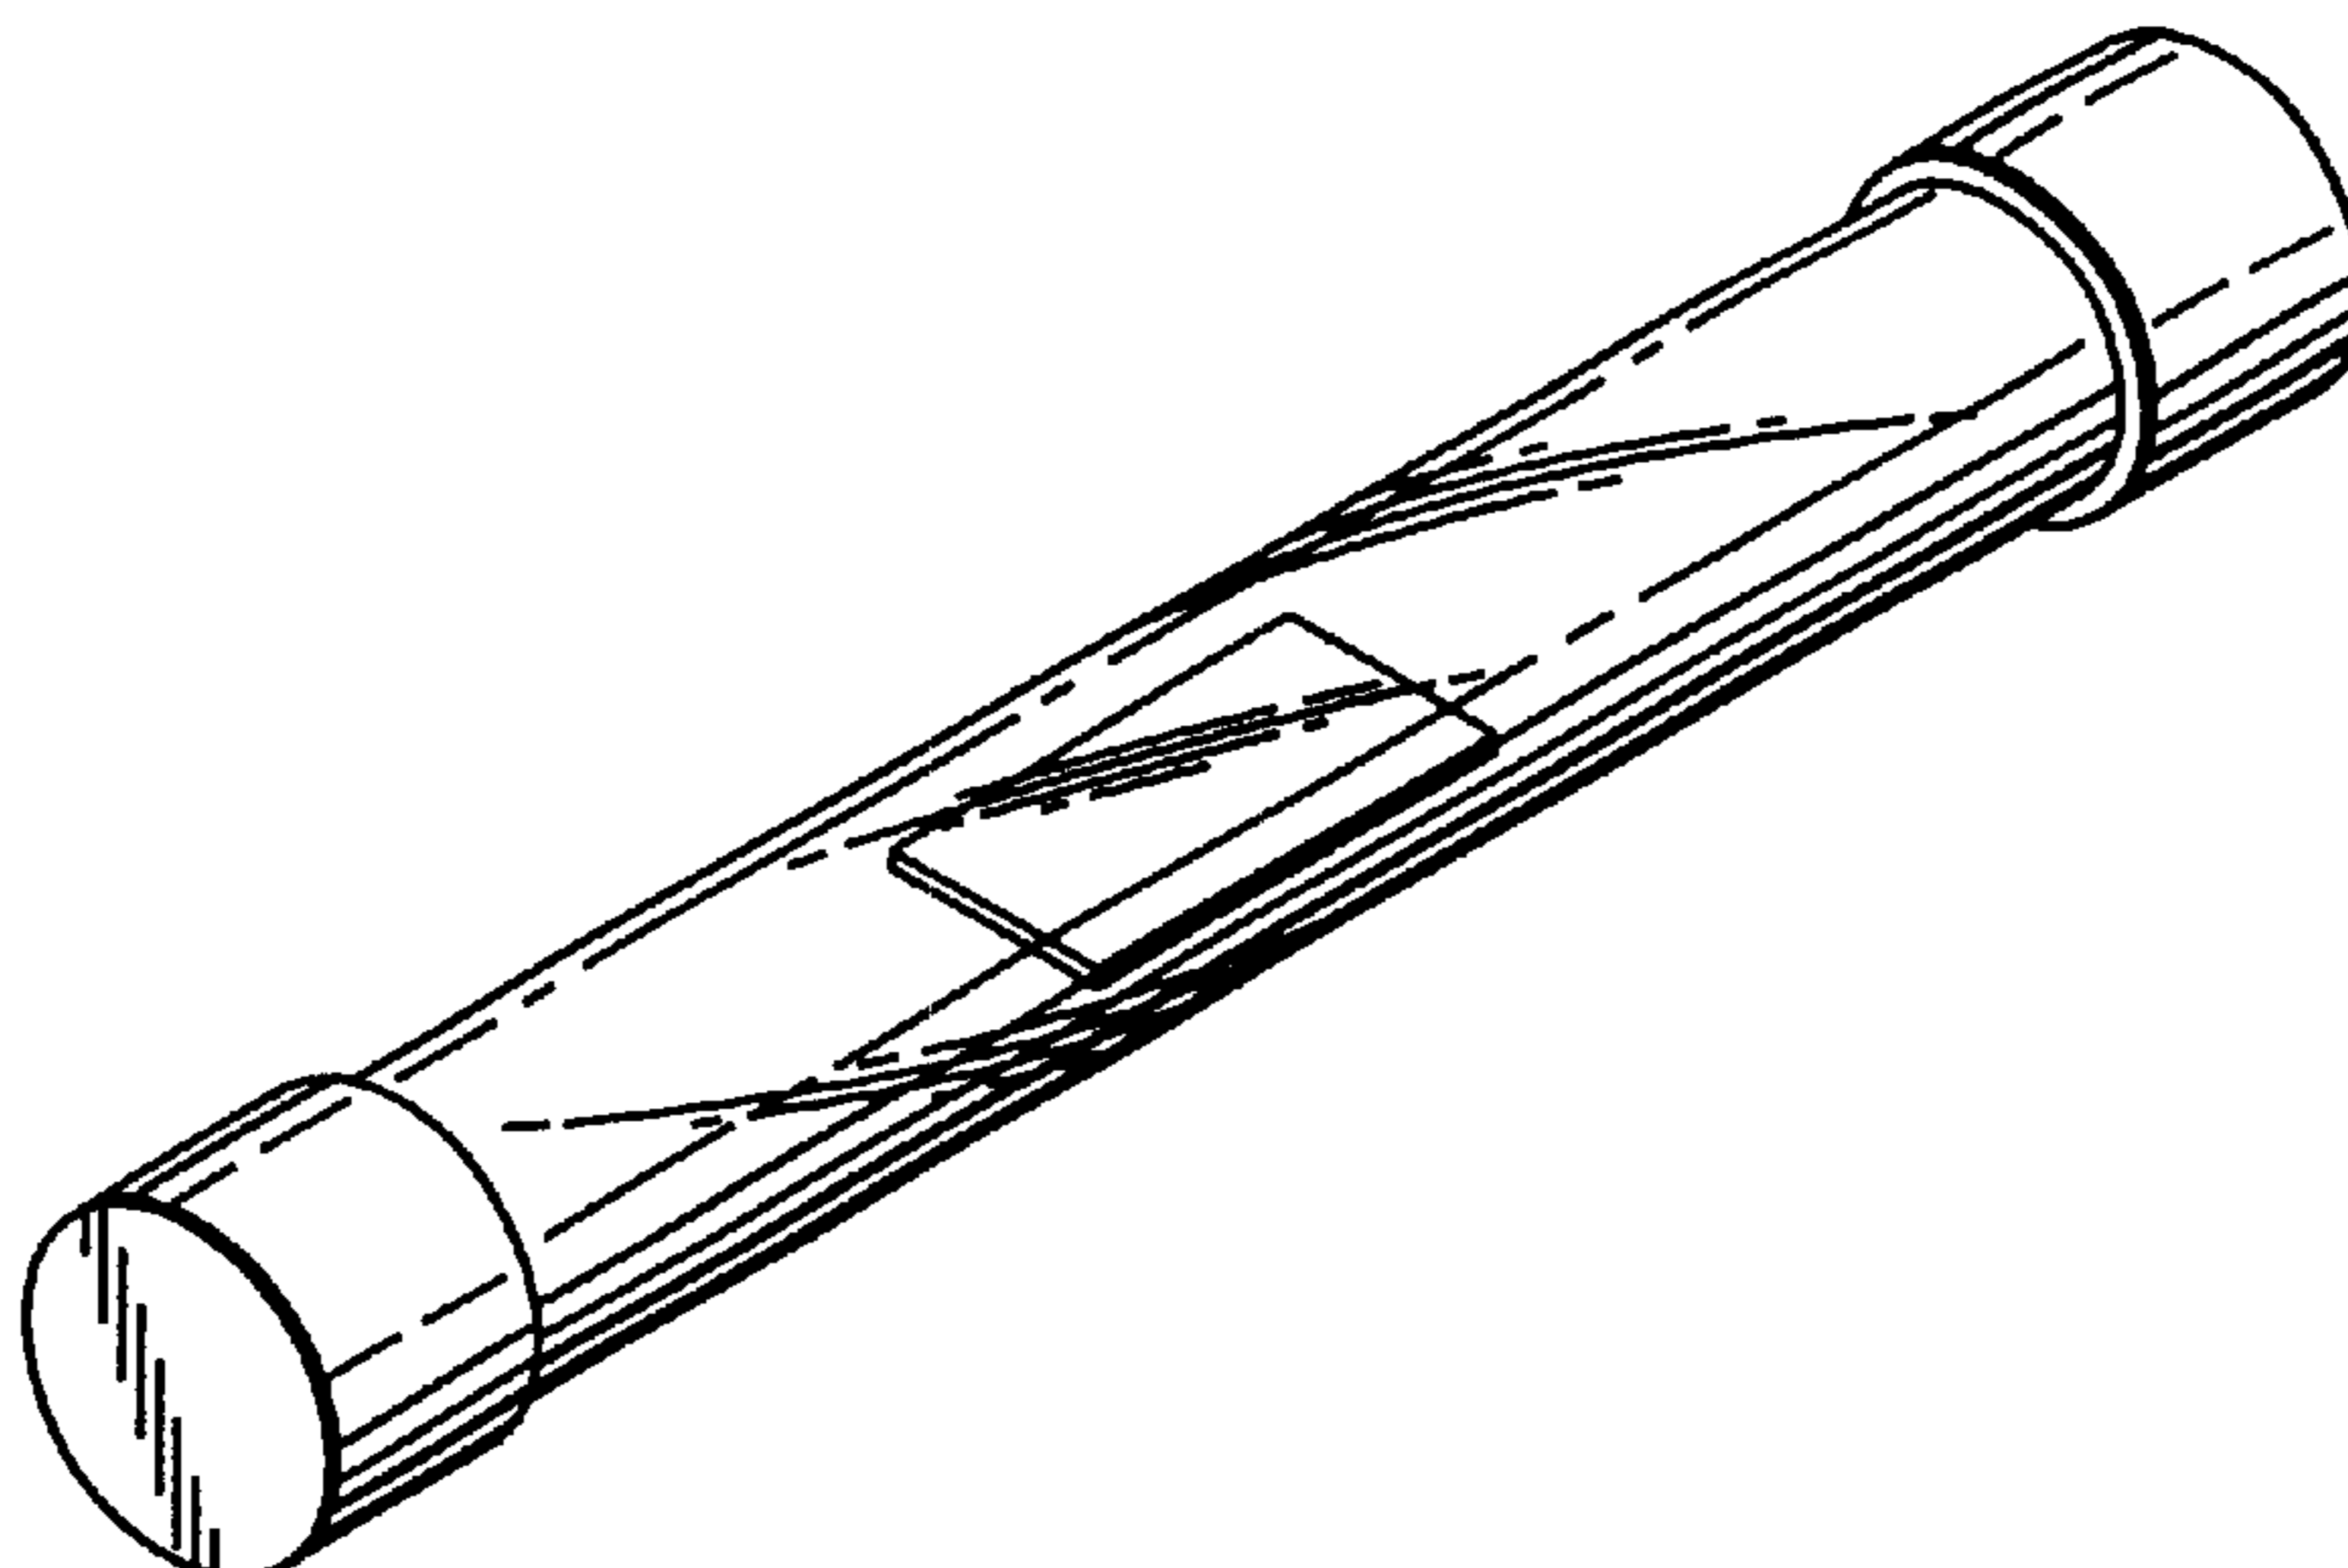

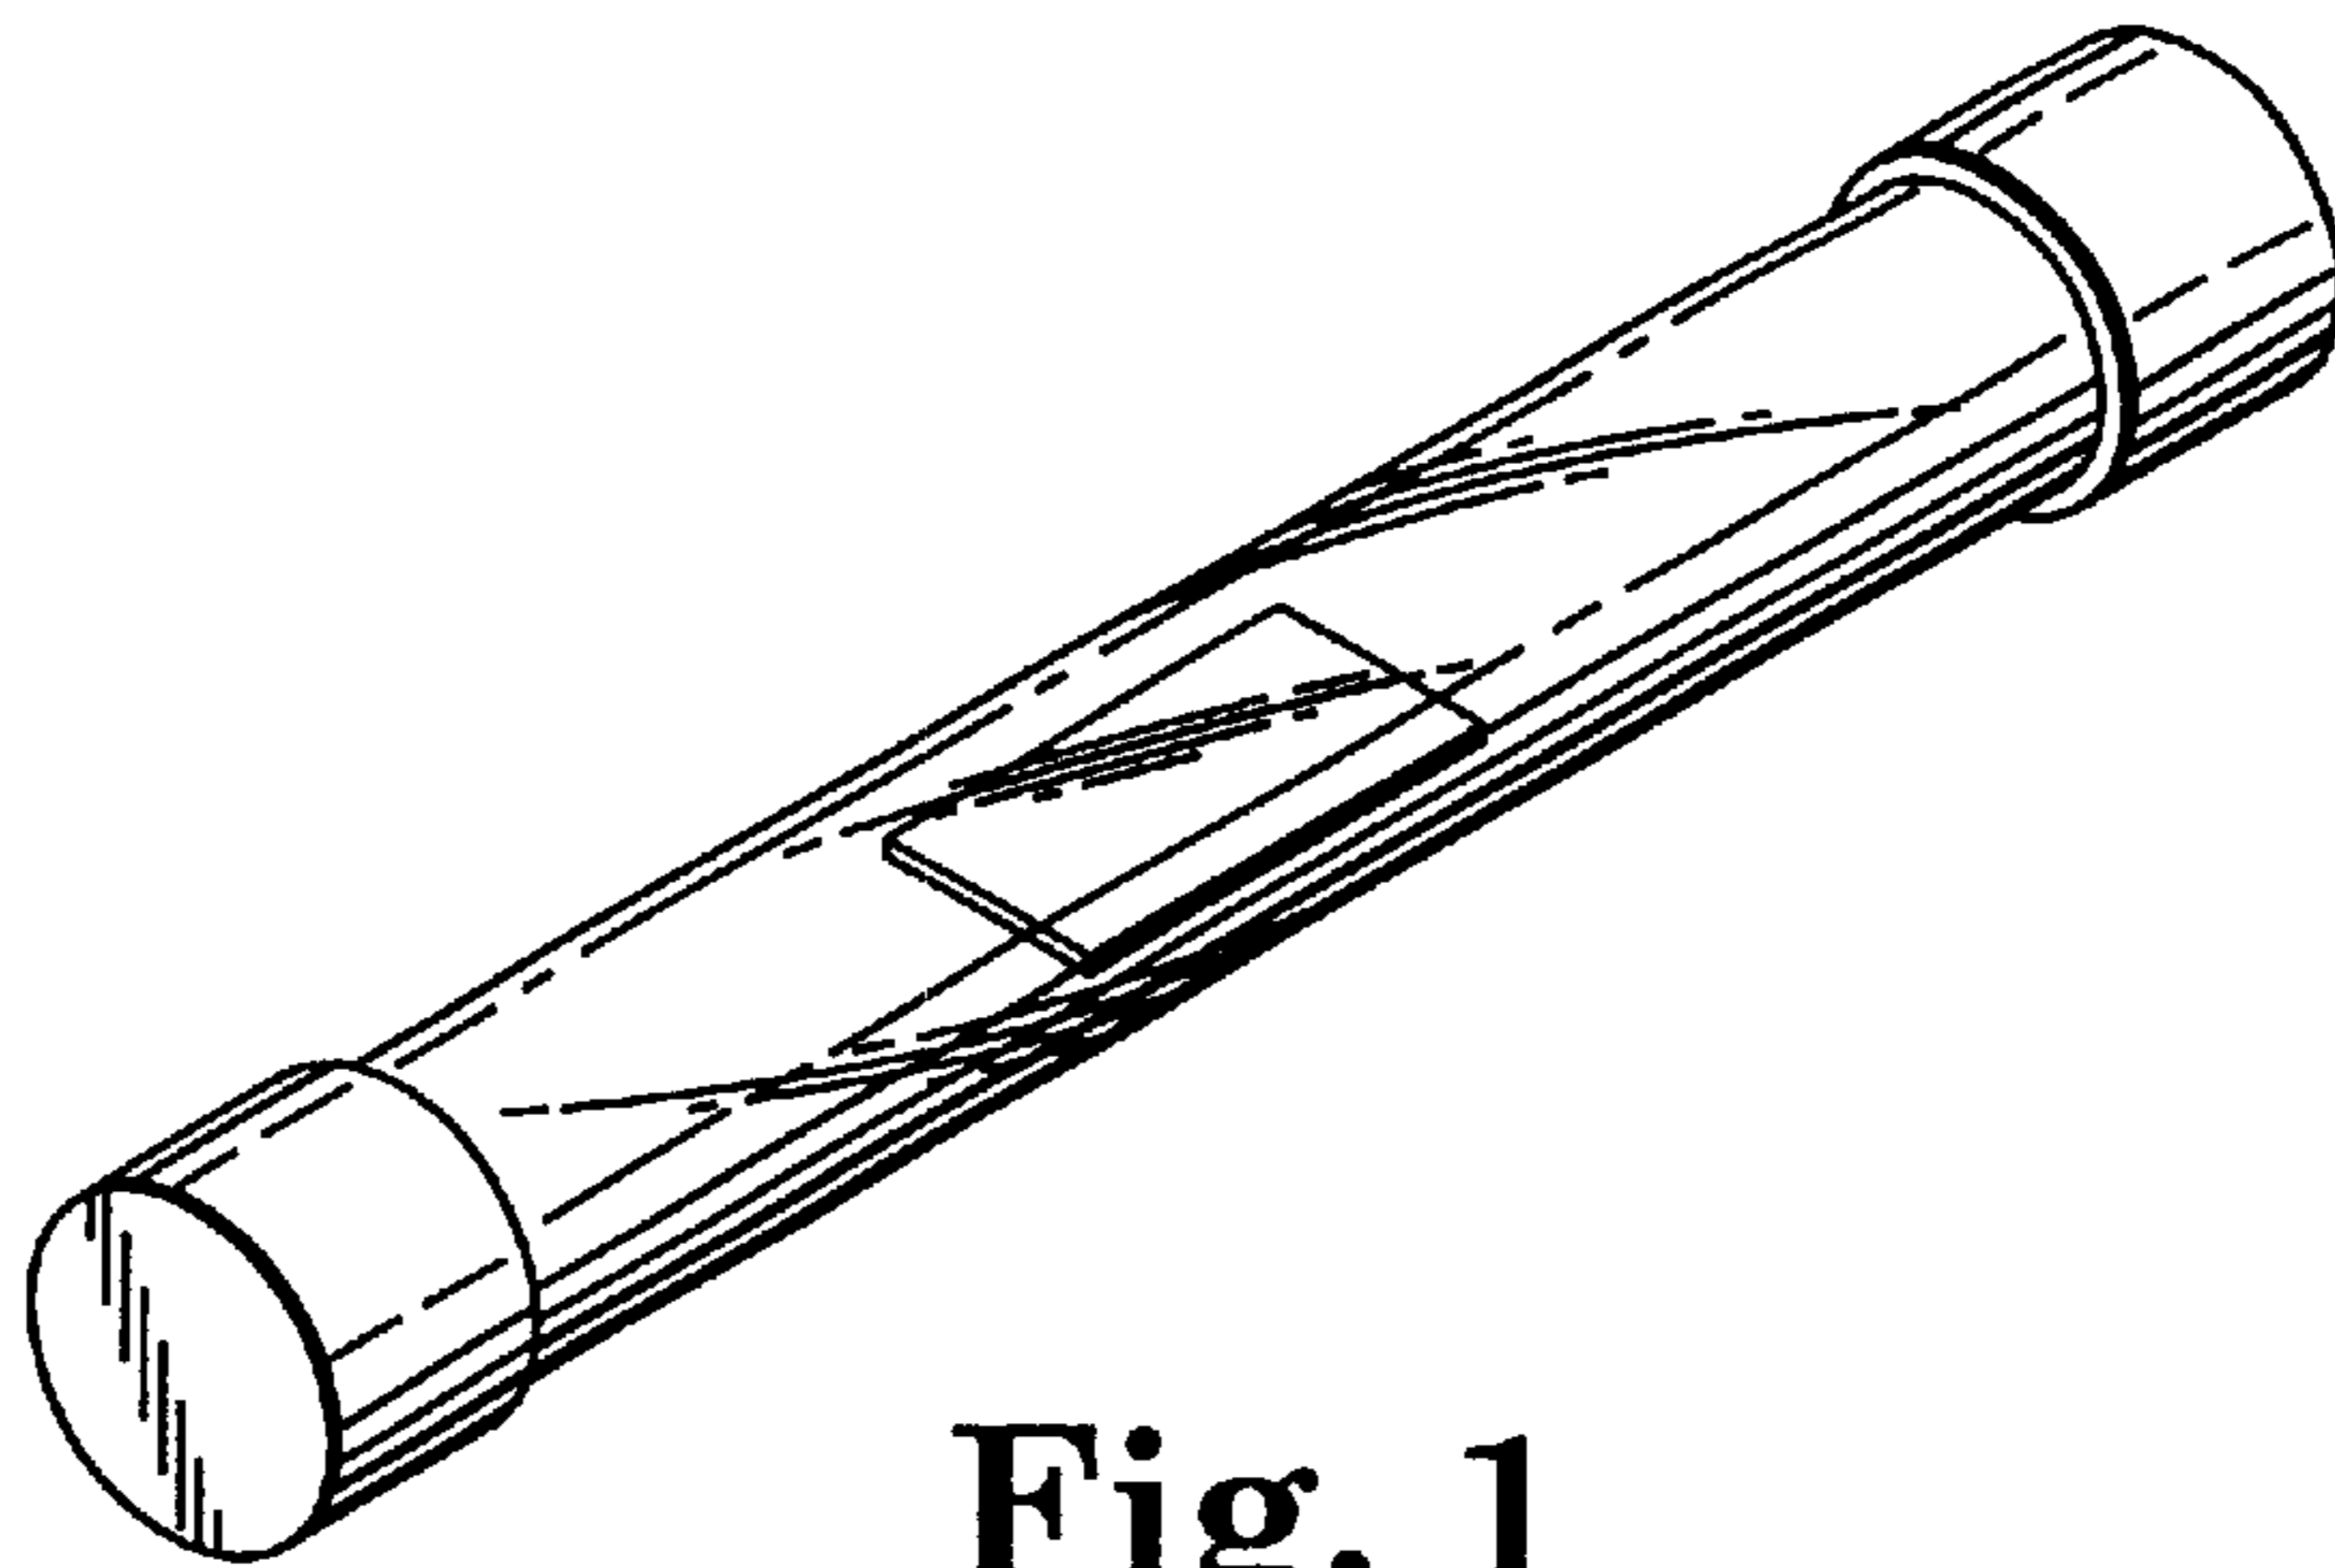


Fig. 1

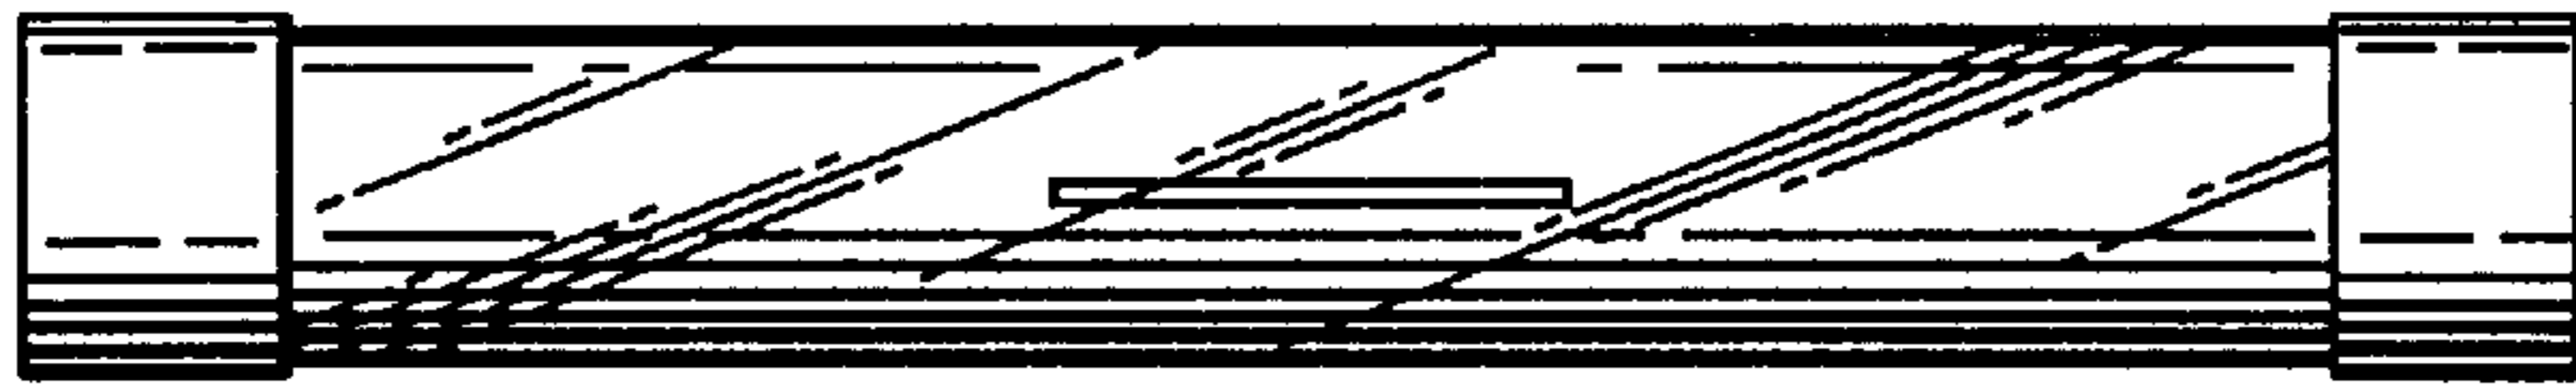


Fig. 2

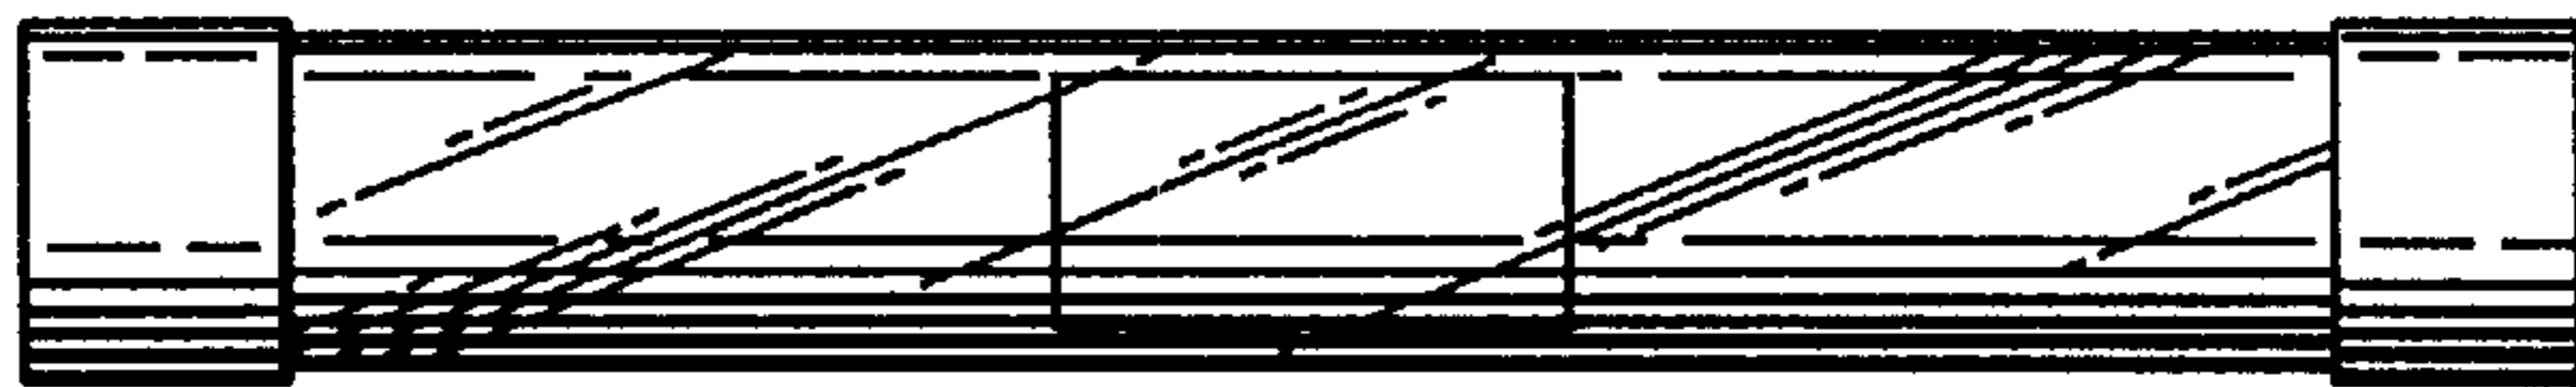


Fig. 3



Fig. 4