



US00D459811S

(12) **United States Design Patent**  
**Maus et al.**

(10) **Patent No.:** **US D459,811 S**

(45) **Date of Patent:** **\*\* Jul. 2, 2002**

(54) **SLIMLINE HEALTH MONITORING AND DIAGNOSTIC DEVICE**

(74) *Attorney, Agent, or Firm*—Michael J. Mehrman; Gardner Groff & Mehrman, PC

(75) Inventors: **Christopher Maus**, Sagle; **Jackson B. Connolly**, Post Falls, both of ID (US); **Jeffrey L. Bendio**, Spokane, WA (US)

(57) **CLAIM**

The ornamental design for a slimline health monitoring and diagnostic device, as shown and described.

(73) Assignee: **Lifestream Technologies, Inc.**, Post Falls, ID (US)

**DESCRIPTION**

(\*\*) Term: **14 Years**

(21) Appl. No.: **29/132,357**

FIG. 1 is a front perspective view of a slimline health monitoring and diagnostic device in a closed position.

FIG. 2 is a top view of a slimline health monitoring and diagnostic device in a closed position.

FIG. 3 is a left side view of a slimline health monitoring and diagnostic device in a closed position.

FIG. 4 is a front view of a slimline health monitoring and diagnostic device in a closed position.

FIG. 5 is a rear view of a slimline health monitoring and diagnostic device in a closed position.

FIG. 6 is a bottom view of a slimline health monitoring and diagnostic device in a closed position.

FIG. 7 is a front perspective view of an slimline health monitoring and diagnostic device in a open position.

FIG. 8 is a top view of an slimline health monitoring and diagnostic device in a open position.

FIG. 9 is a front view of a slimline health monitoring and diagnostic device in a open position.

FIG. 10 is a rear view of an slimline health monitoring and diagnostic device in a open position.

FIG. 11 is a left side view of an slimline health monitoring and diagnostic device in a open position; and,

FIG. 12 is a bottom view of an slimline health monitoring and diagnostic device in a open position.

The broken line showing is for illustrative purposes only and forms no part of the claimed design.

(22) Filed: **Nov. 7, 2000**

(51) **LOC (7) Cl.** ..... **24-01**

(52) **U.S. Cl.** ..... **D24/169**

(58) **Field of Search** ..... D24/169, 186; 600/583, 368, 322, 319, 309; 422/56

(56) **References Cited**

**U.S. PATENT DOCUMENTS**

D390,661 S	*	2/1998	Foggia	.....	D24/169
5,780,304 A	*	7/1998	Matzinger et al.	.....	436/169
D437,057 S	*	1/2001	Maus et al.	.....	D24/169
D444,235 S	*	6/2001	Roberts et al.	.....	D24/169
D452,564 S	*	12/2001	Micinski et al.	.....	D24/169



**OTHER PUBLICATIONS**


Double-gatefold color brochure for Accu-Chek® Instant-Plus™ Monitors and Test Strips; distributed by Boehringer Mannheim Corp., 9115 Hague road, Indianapolis, IN 46256. ©1997.

\* cited by examiner


*Primary Examiner*—Stella Reid

**1 Claim, 5 Drawing Sheets**

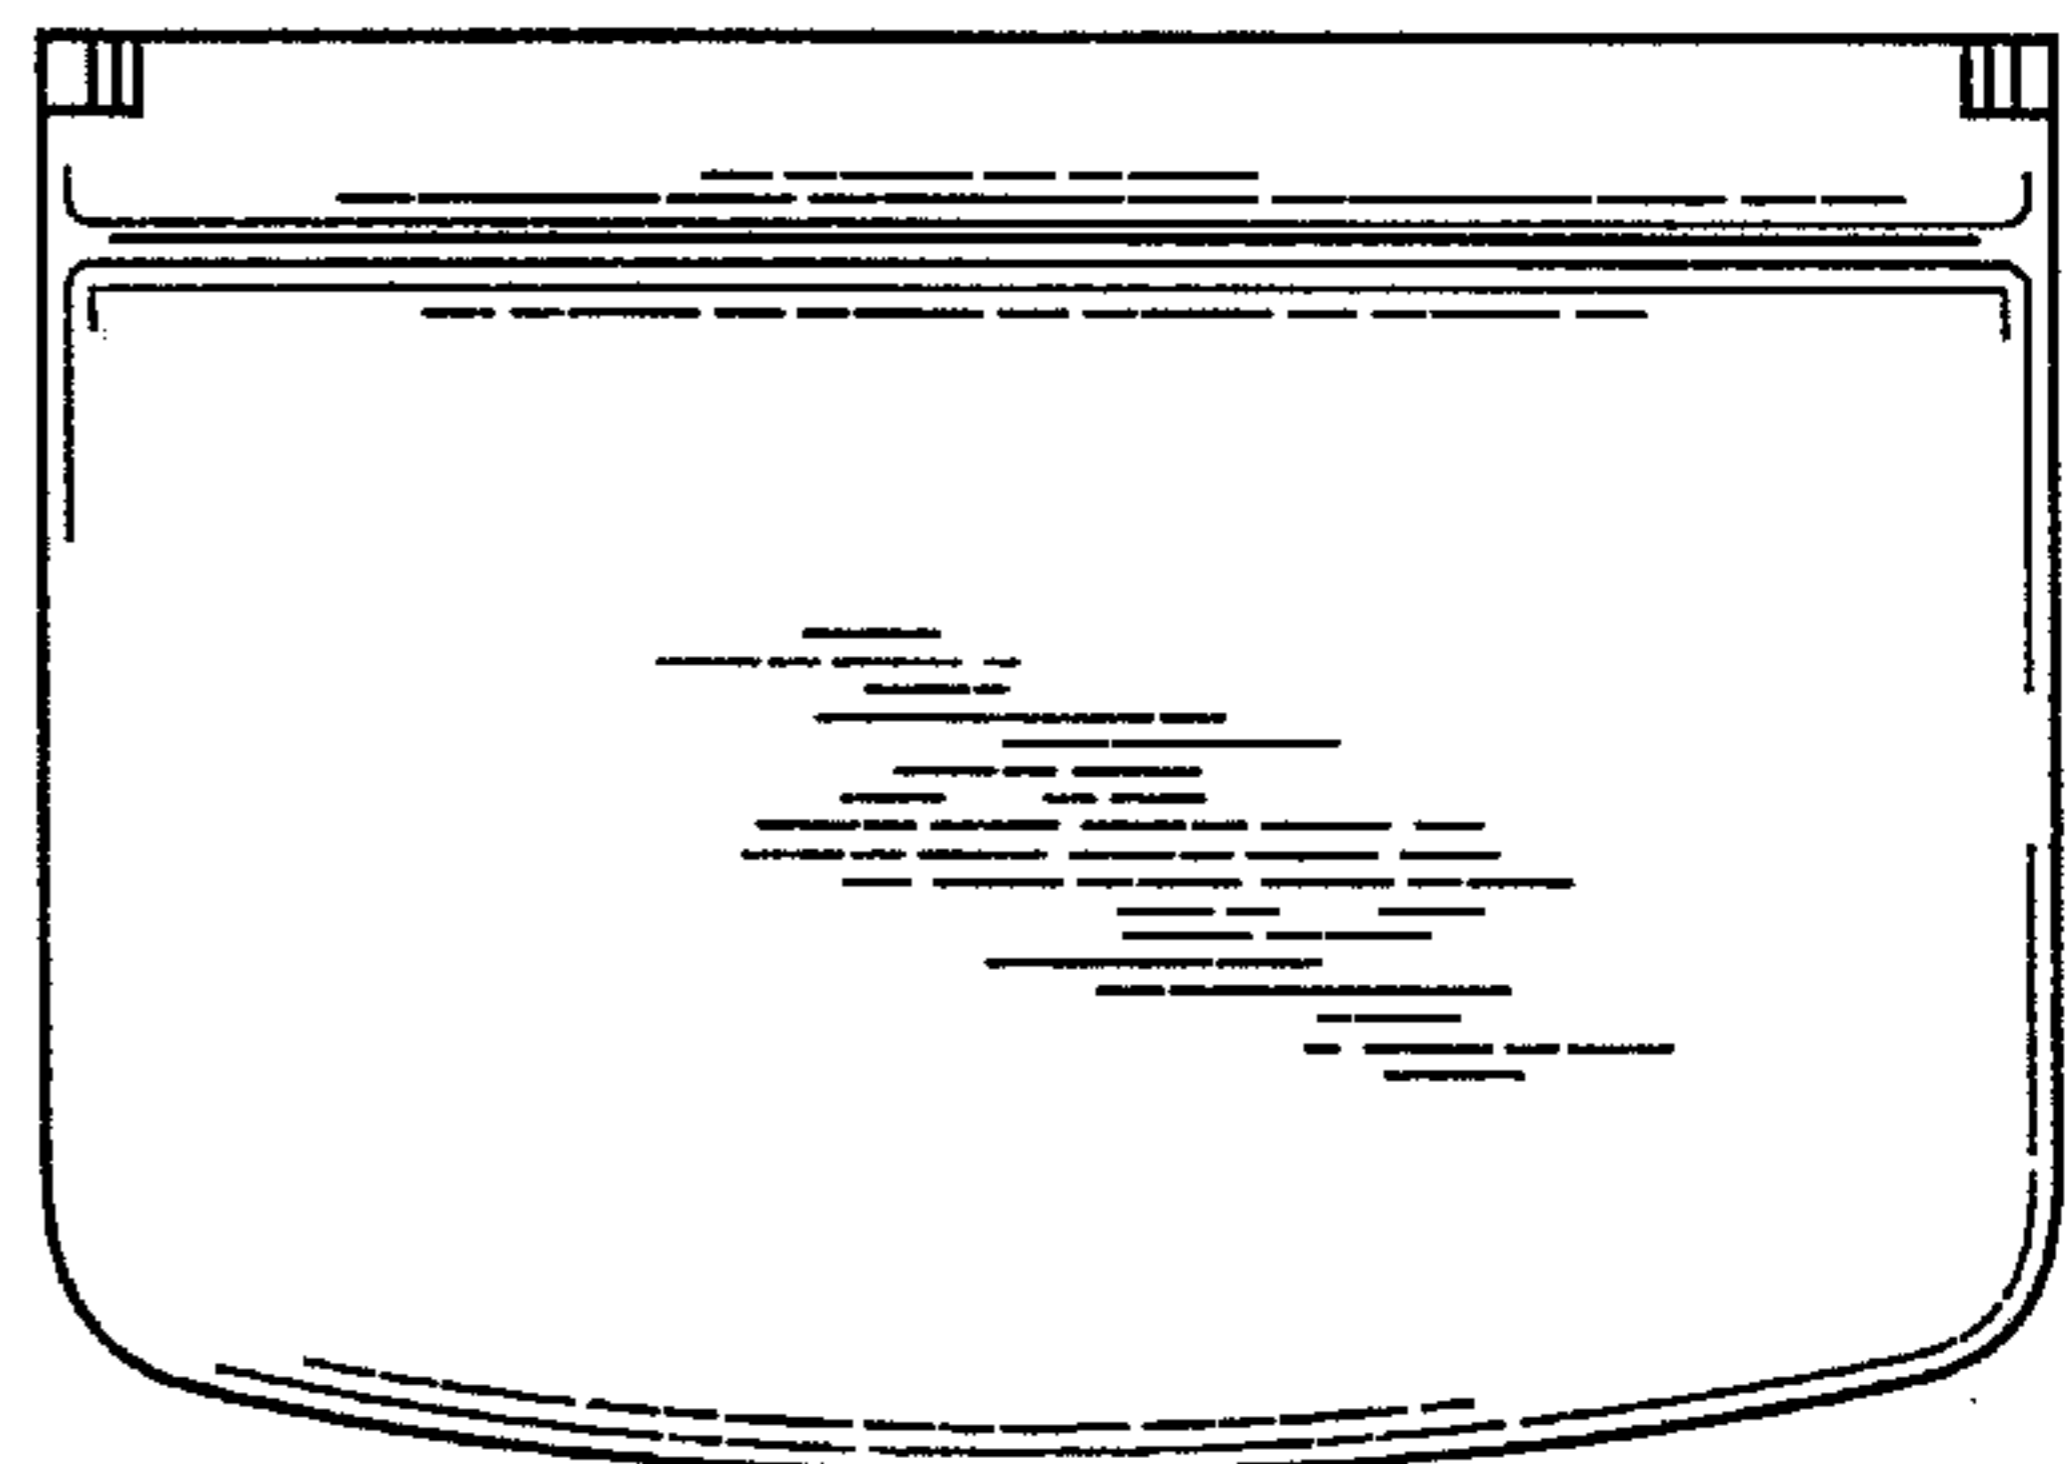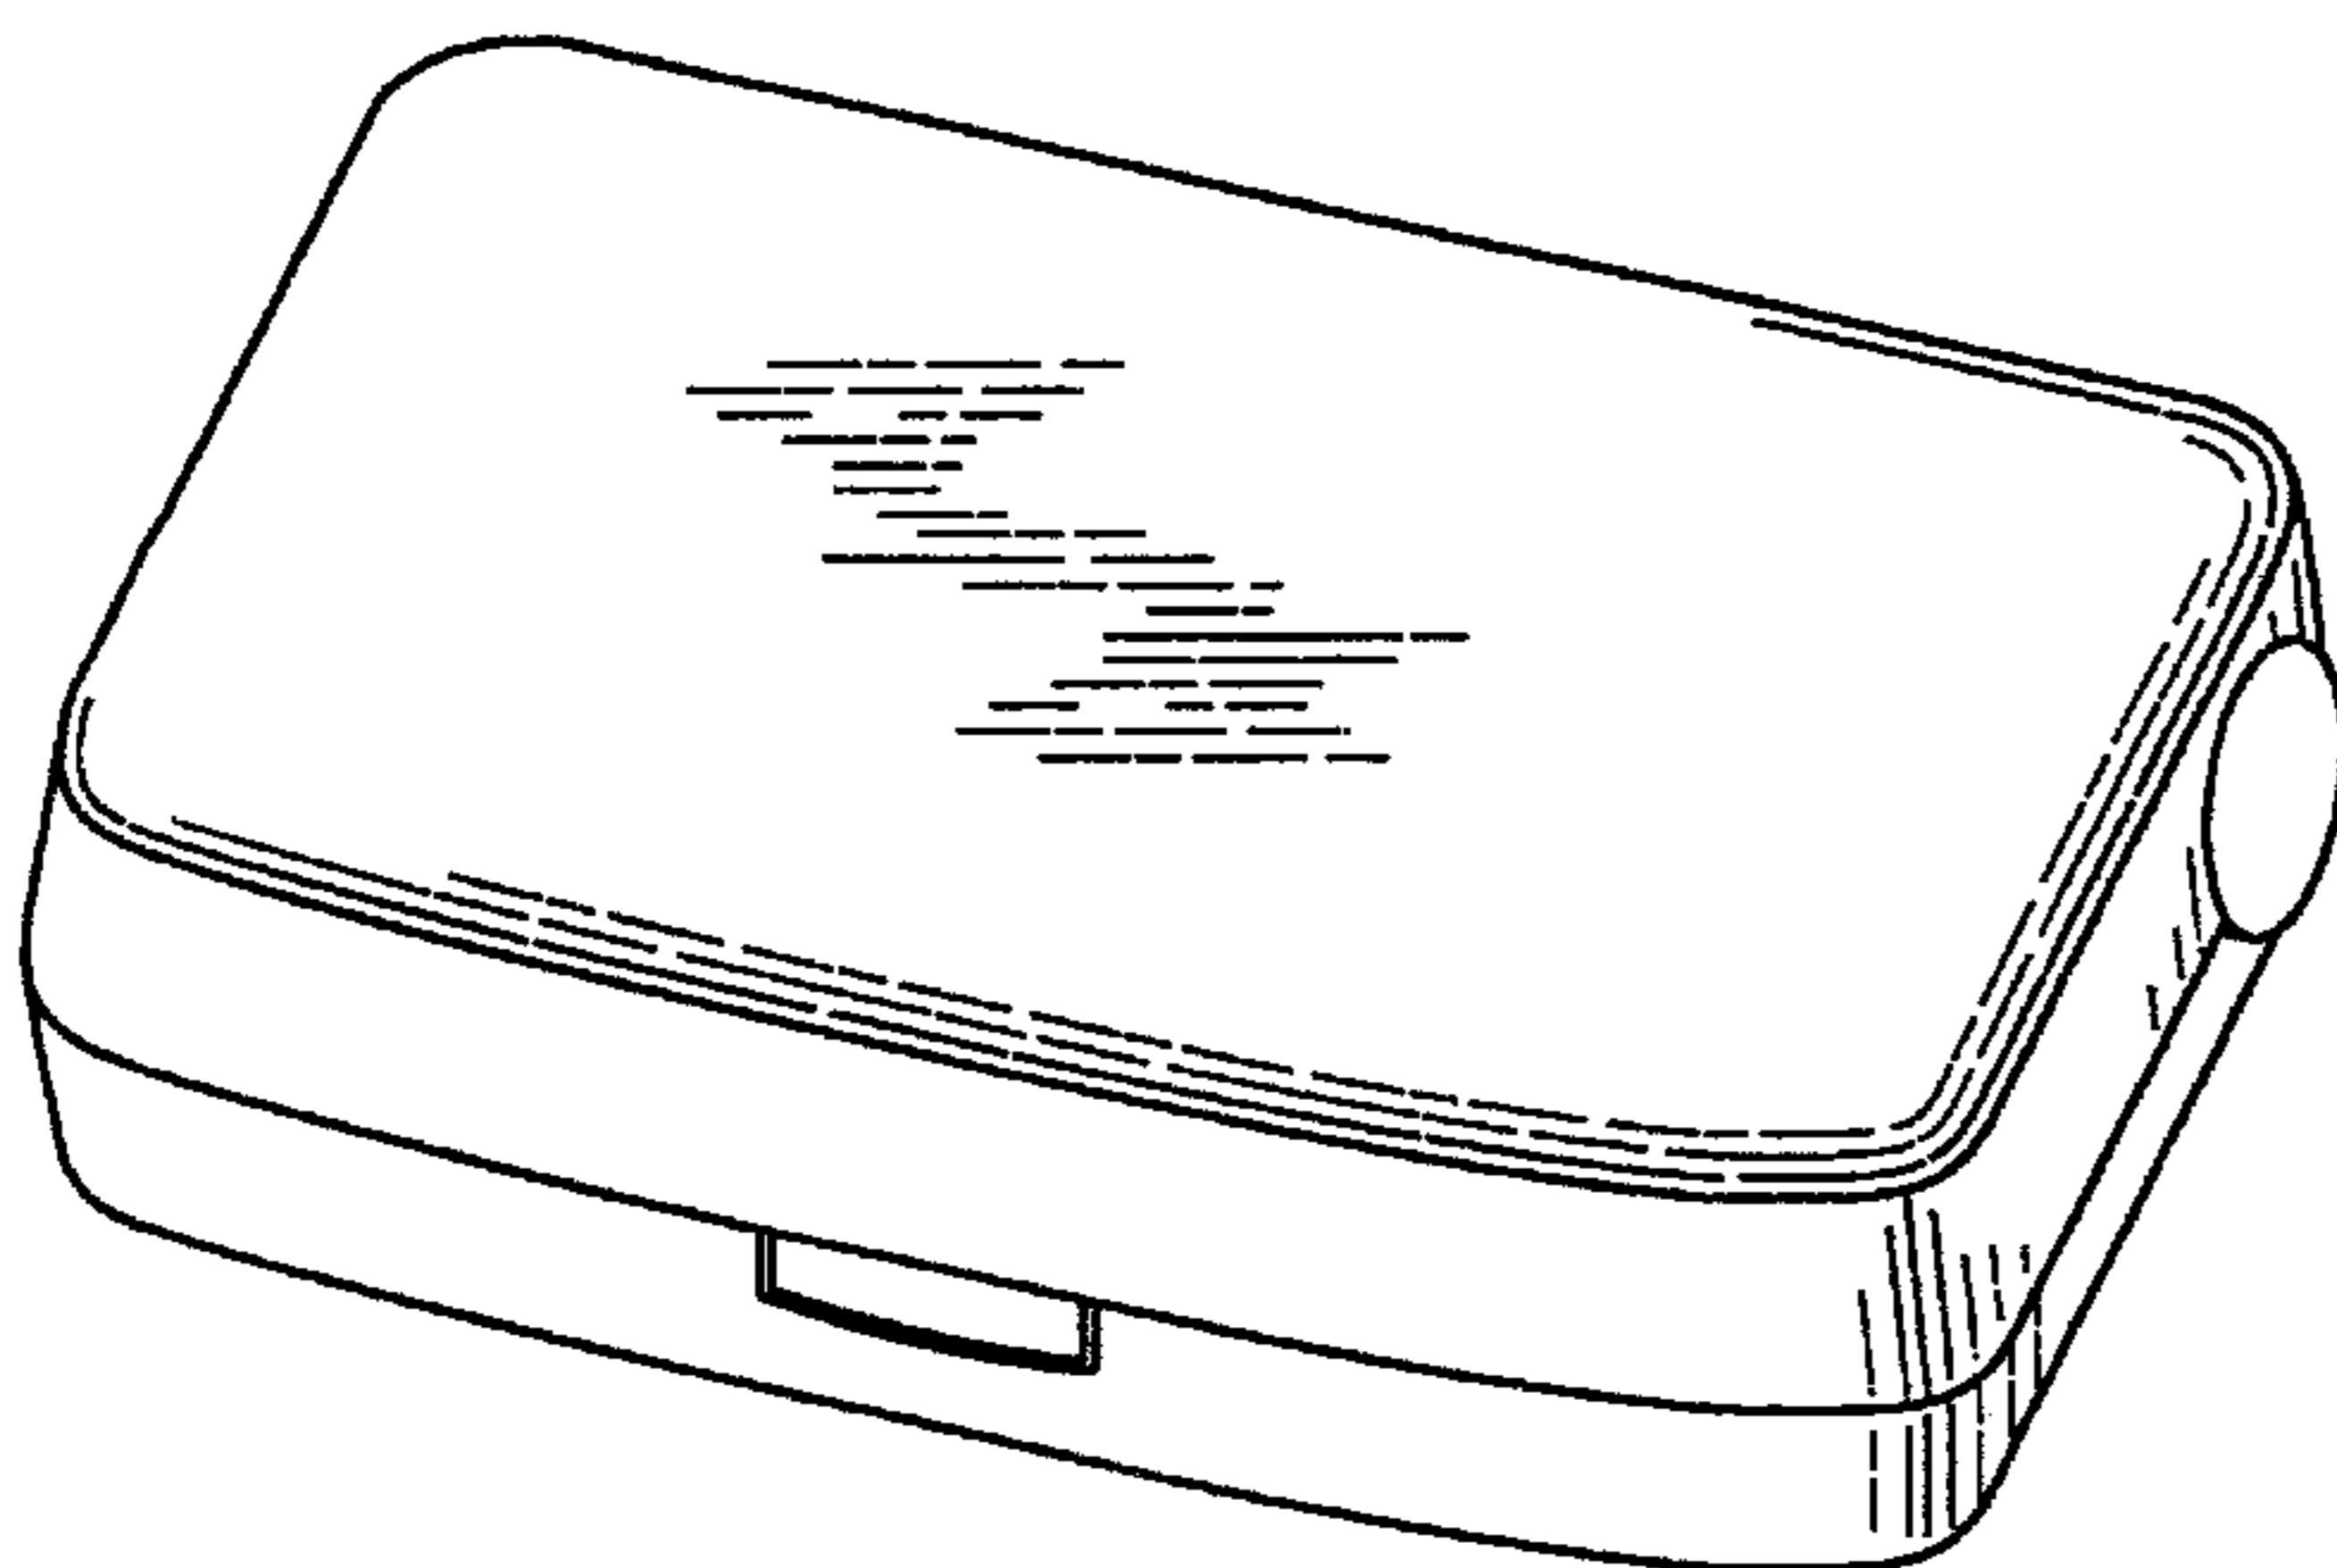


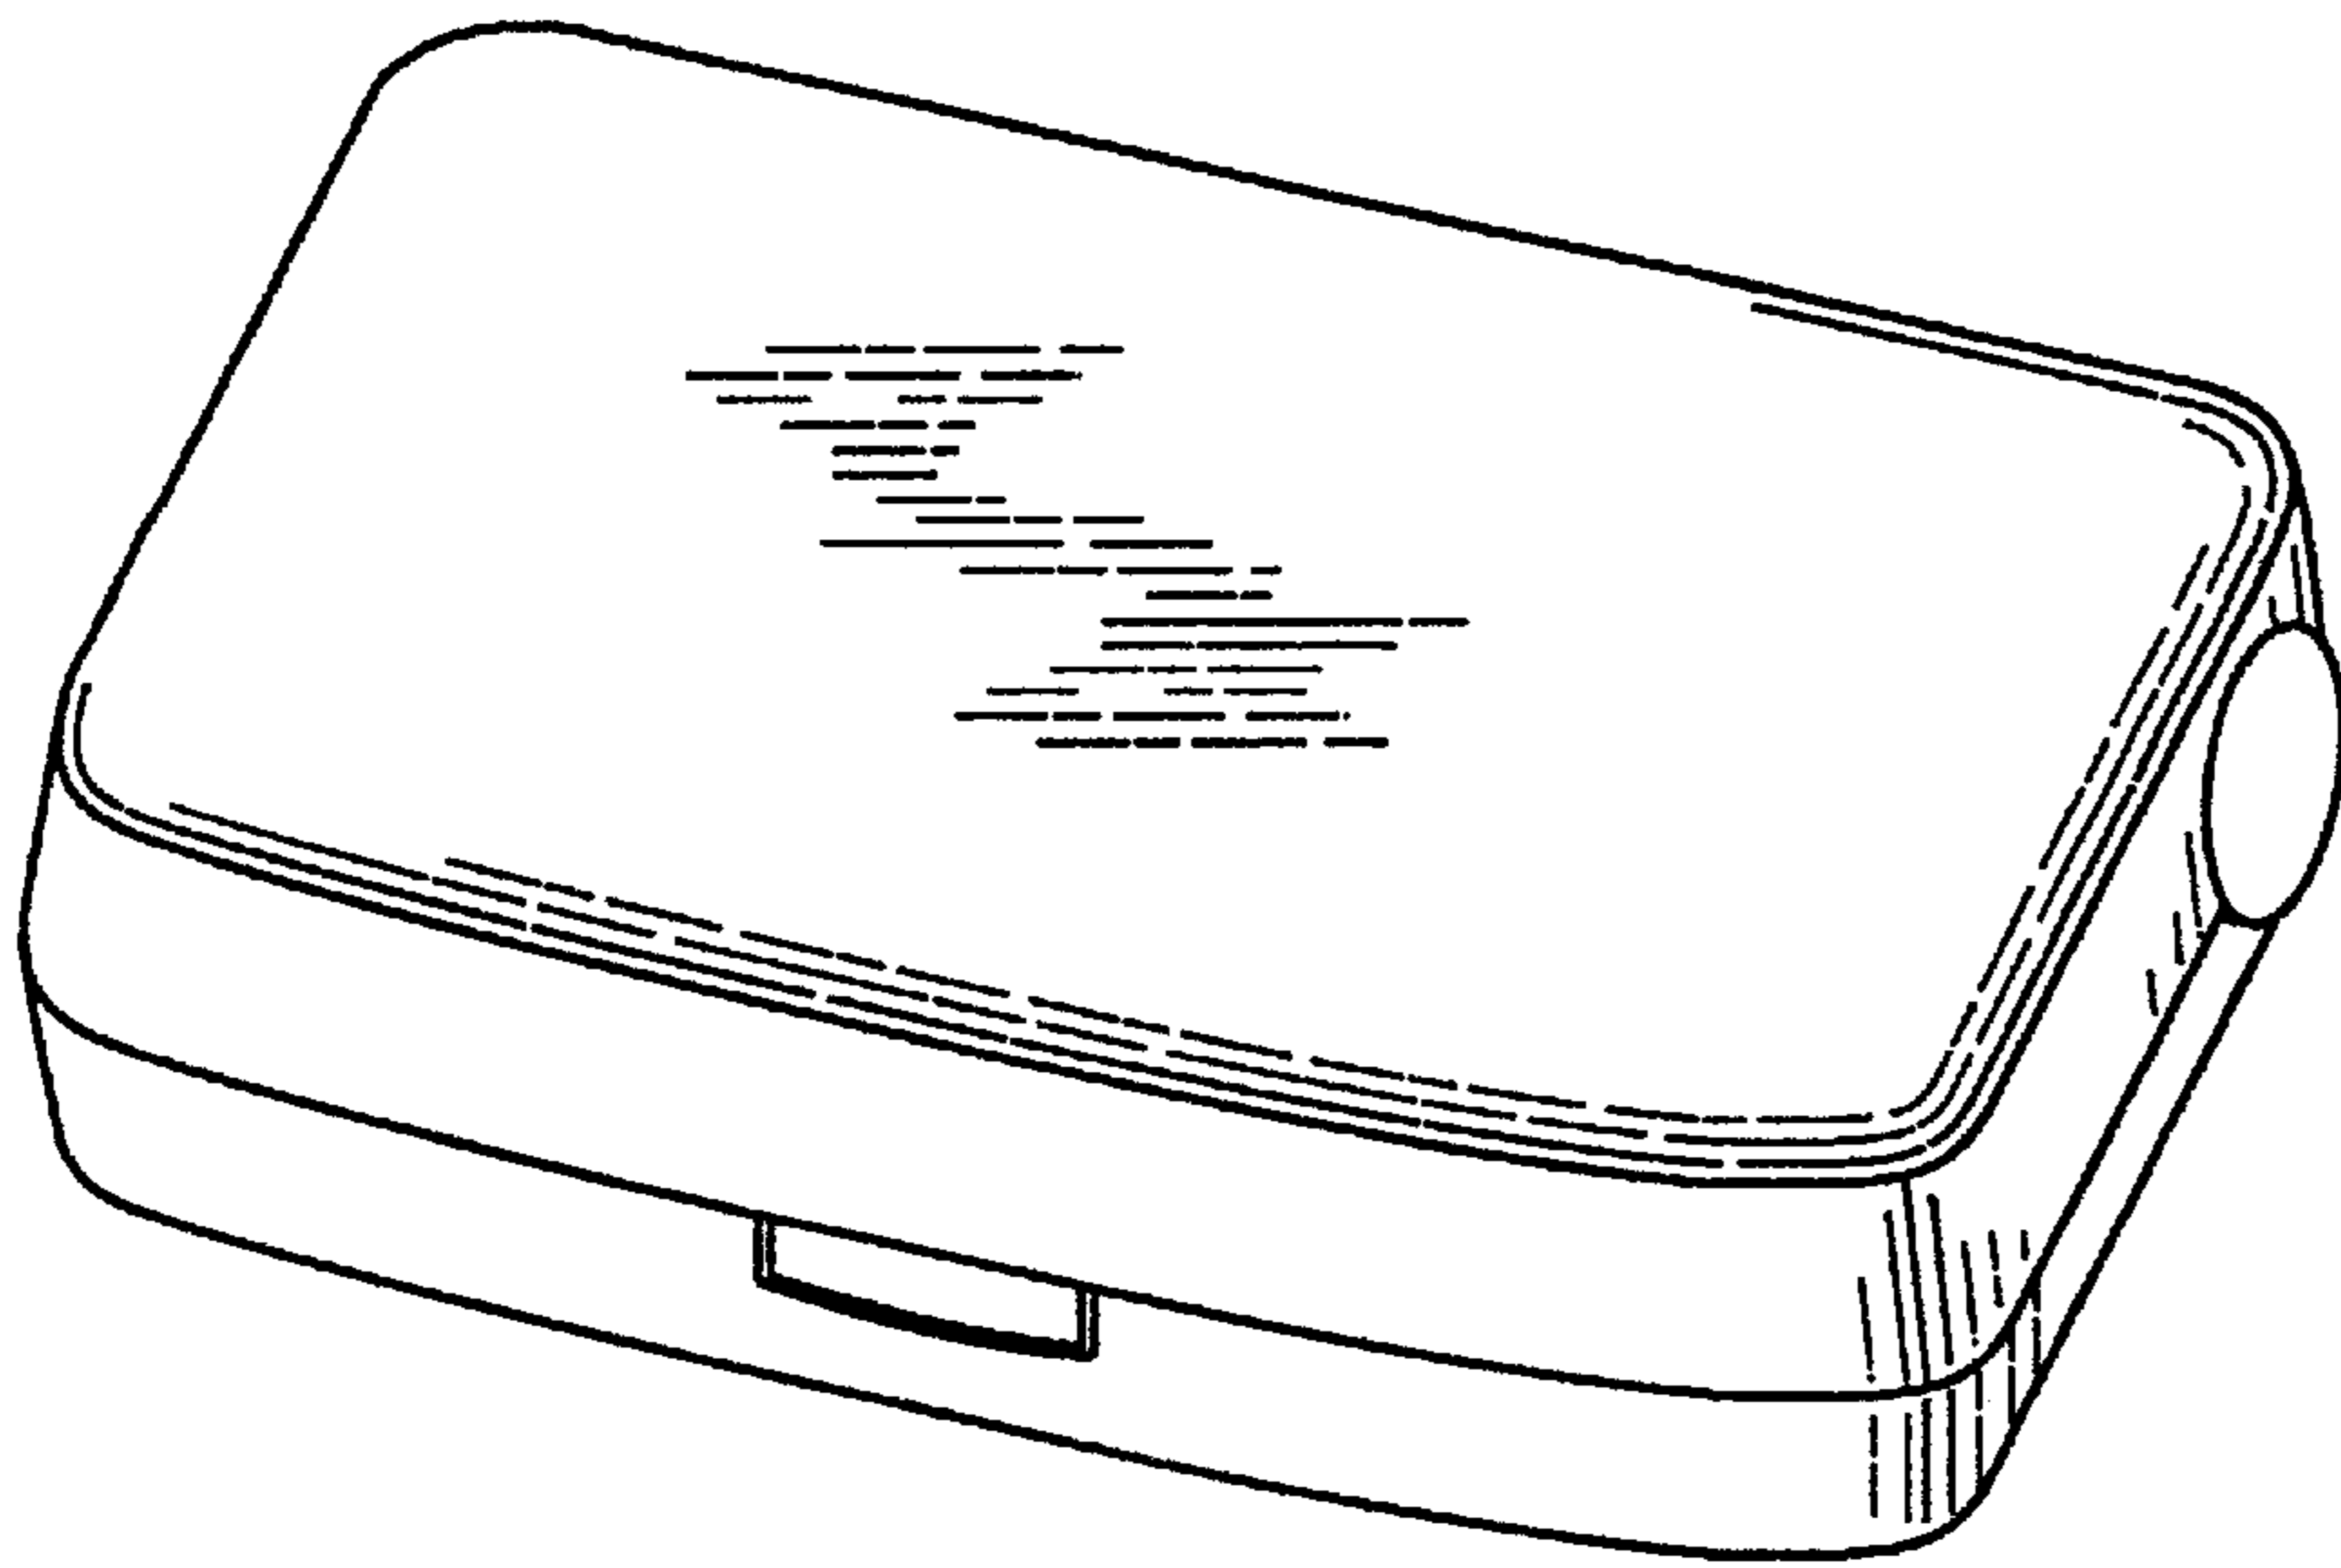


**FIG. 1**

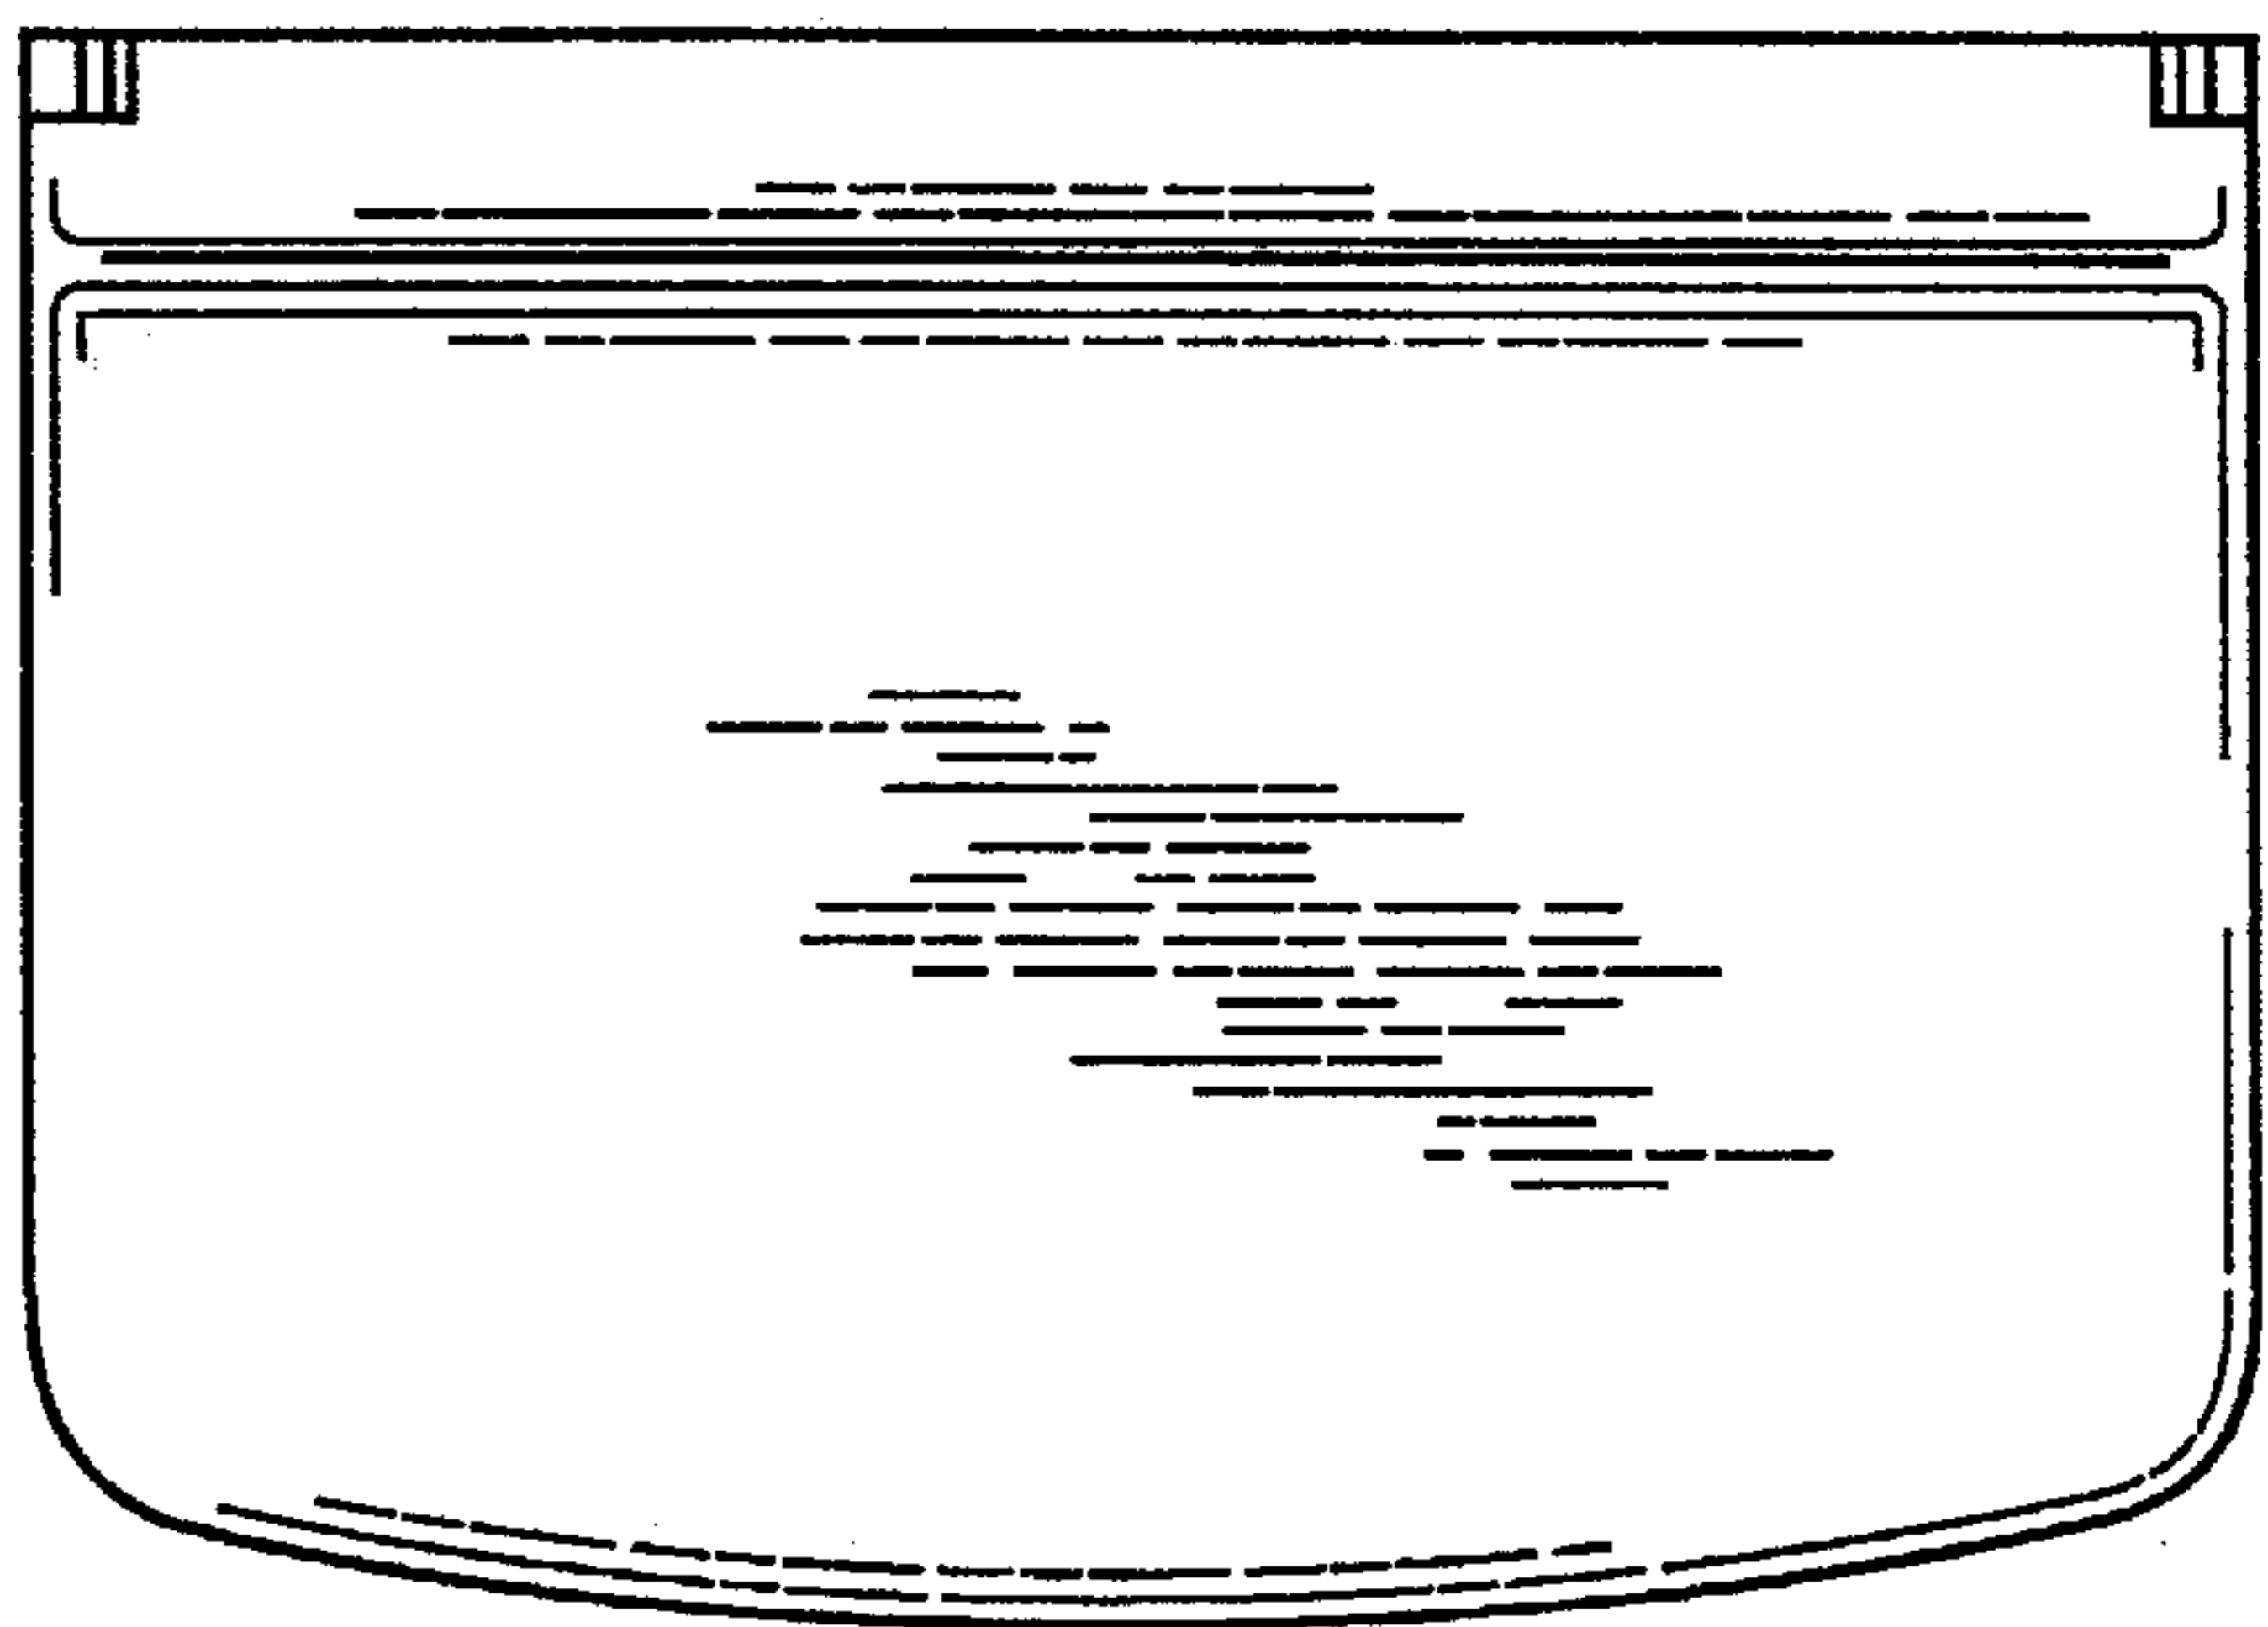


**FIG. 2**

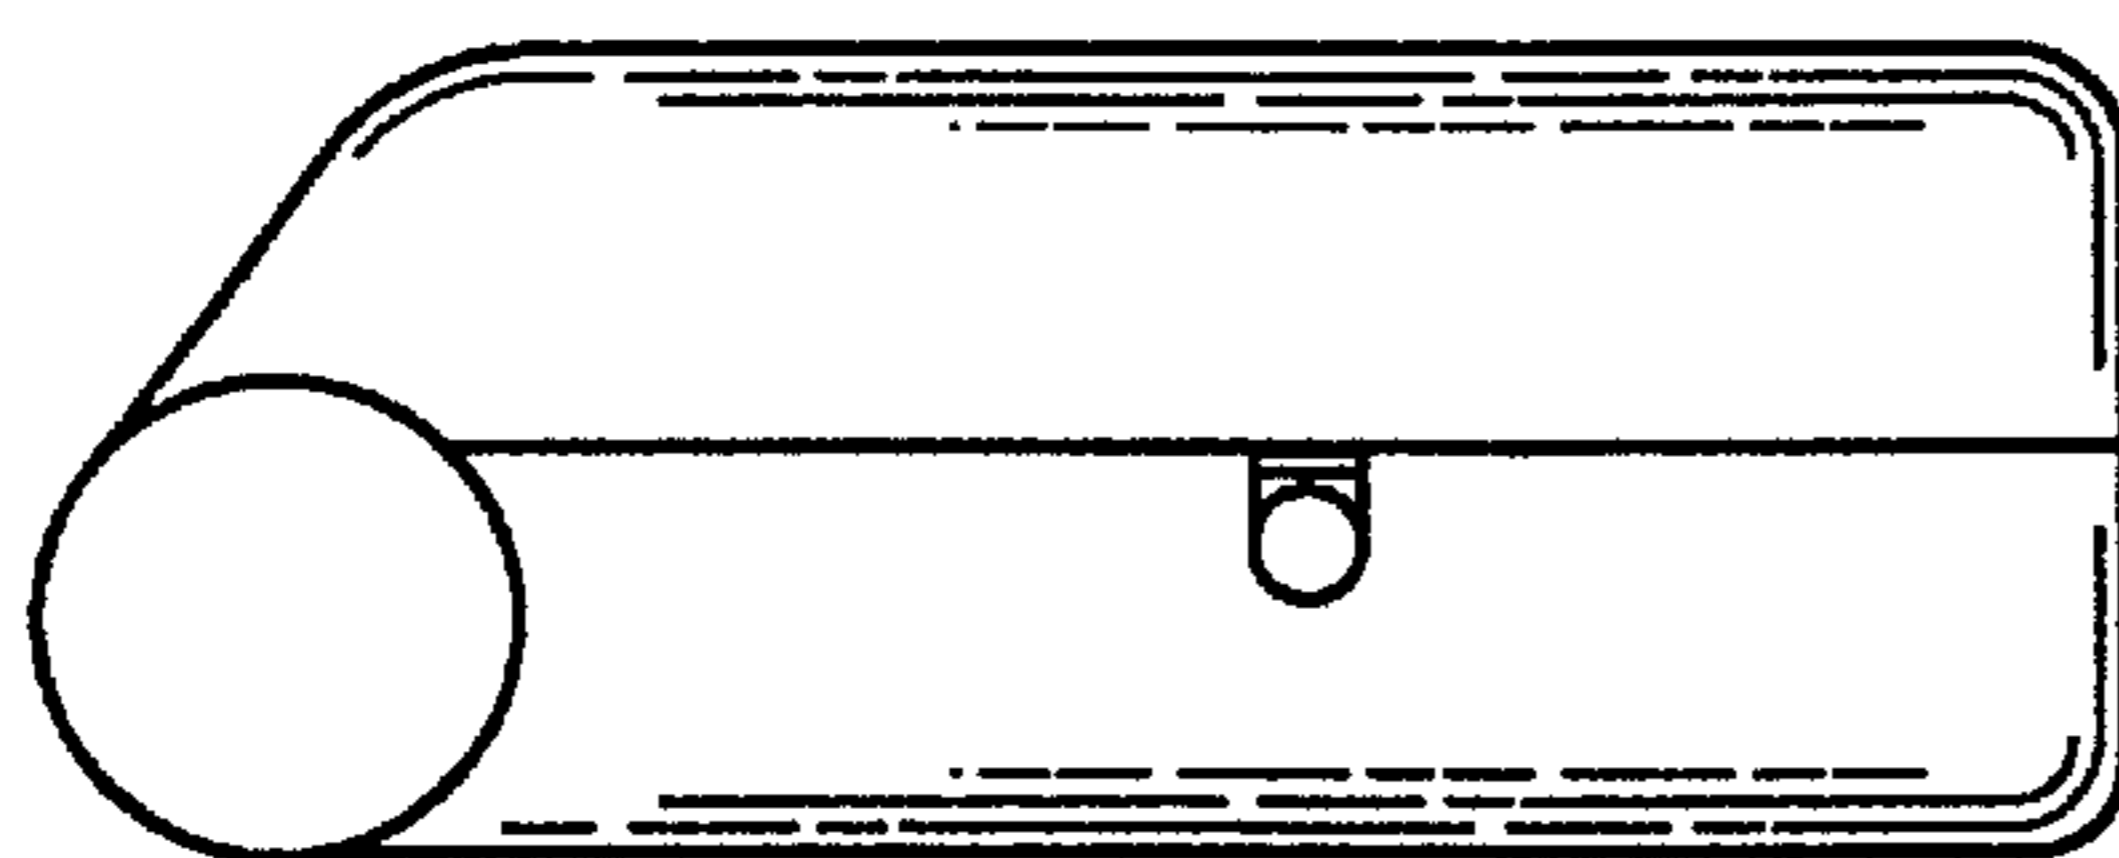


**FIG. 3**

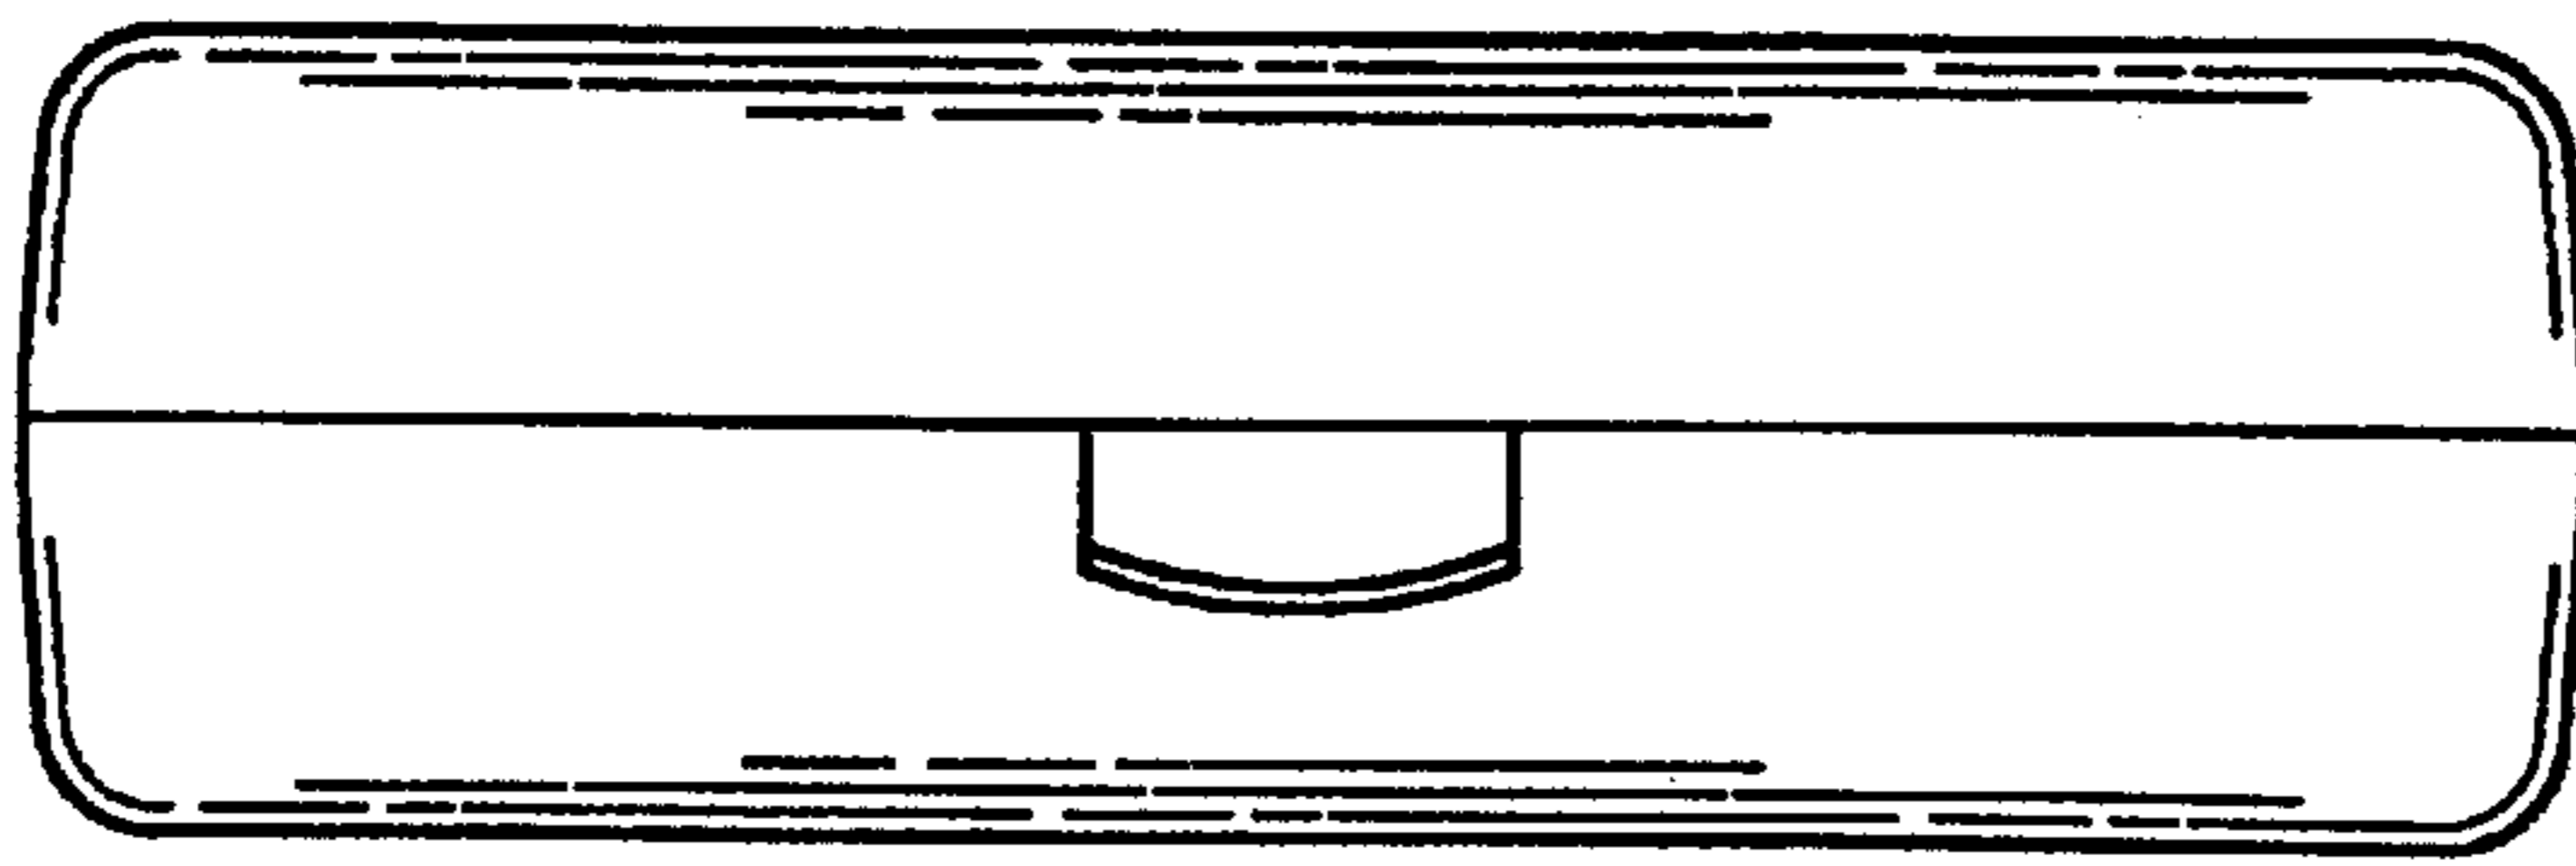


**FIG. 4**

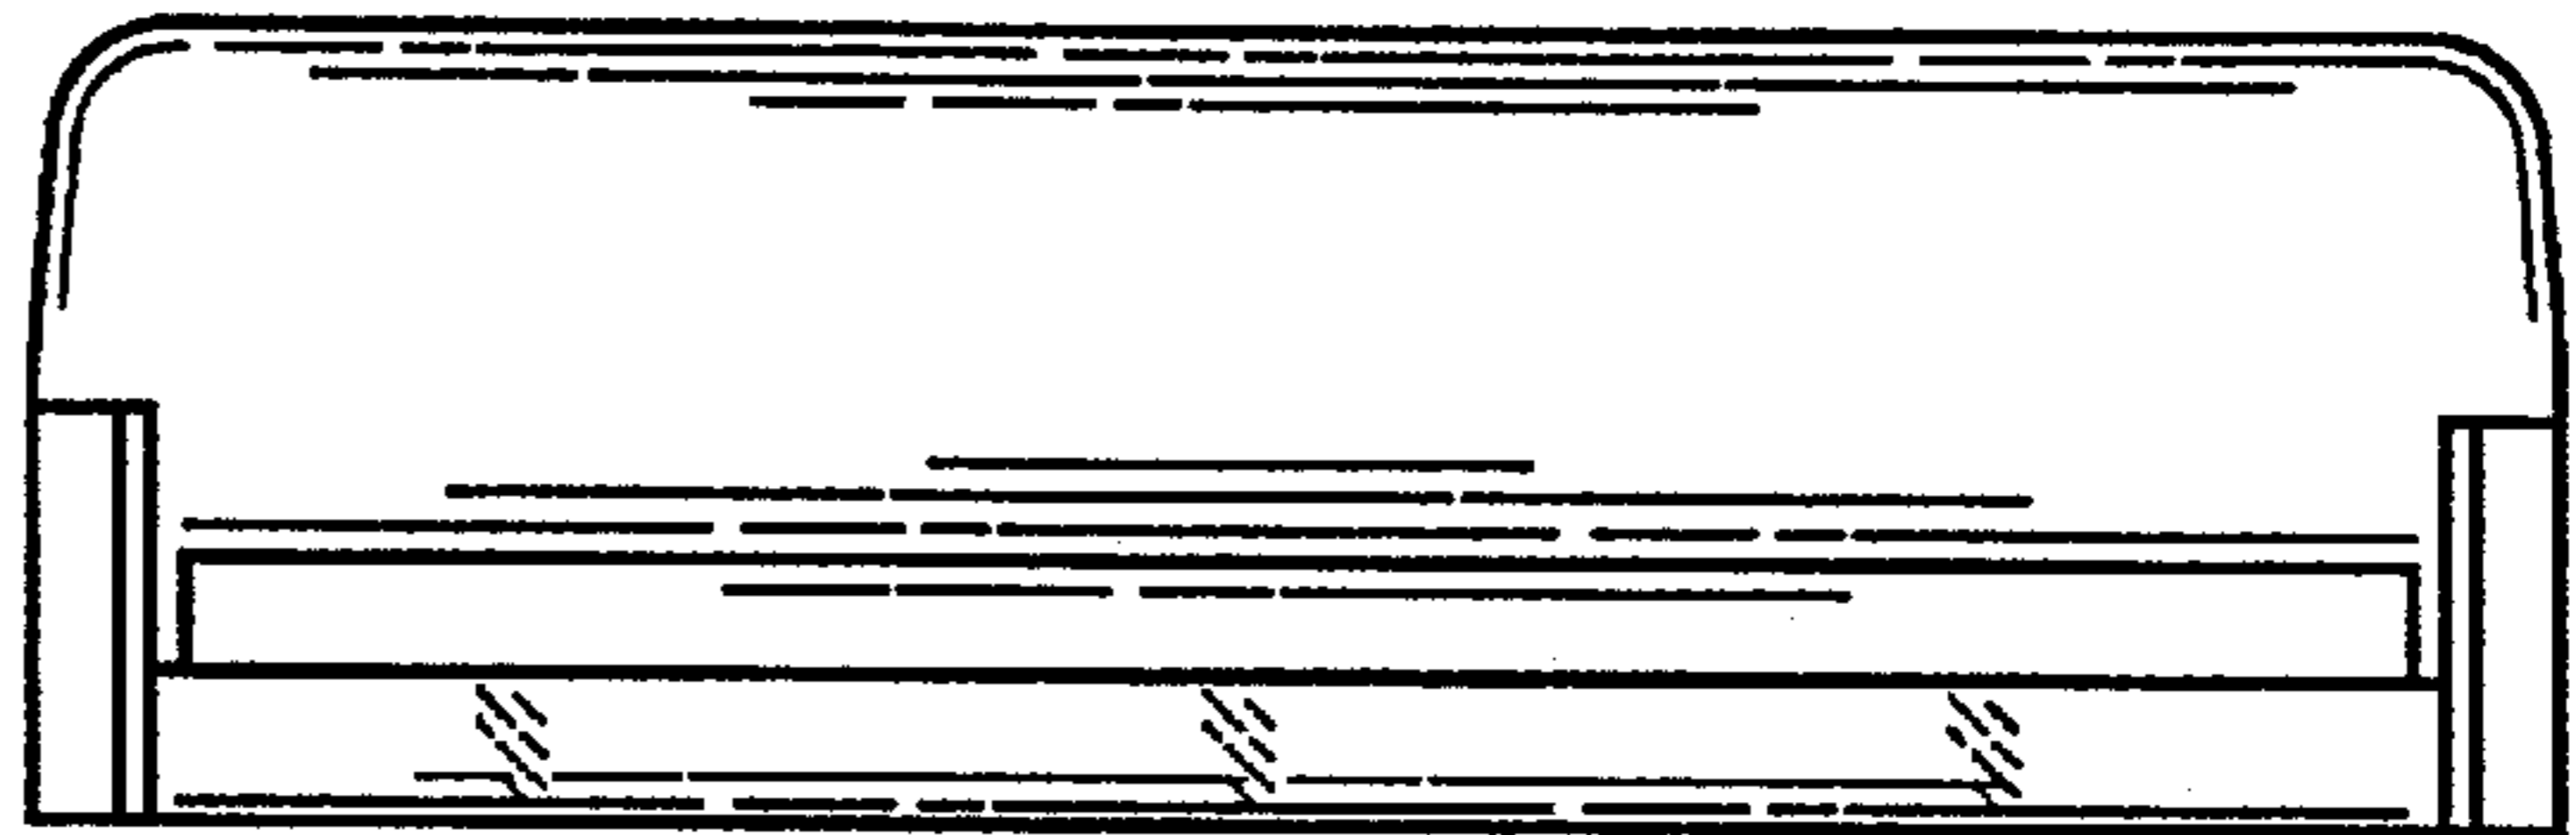


**FIG. 5**

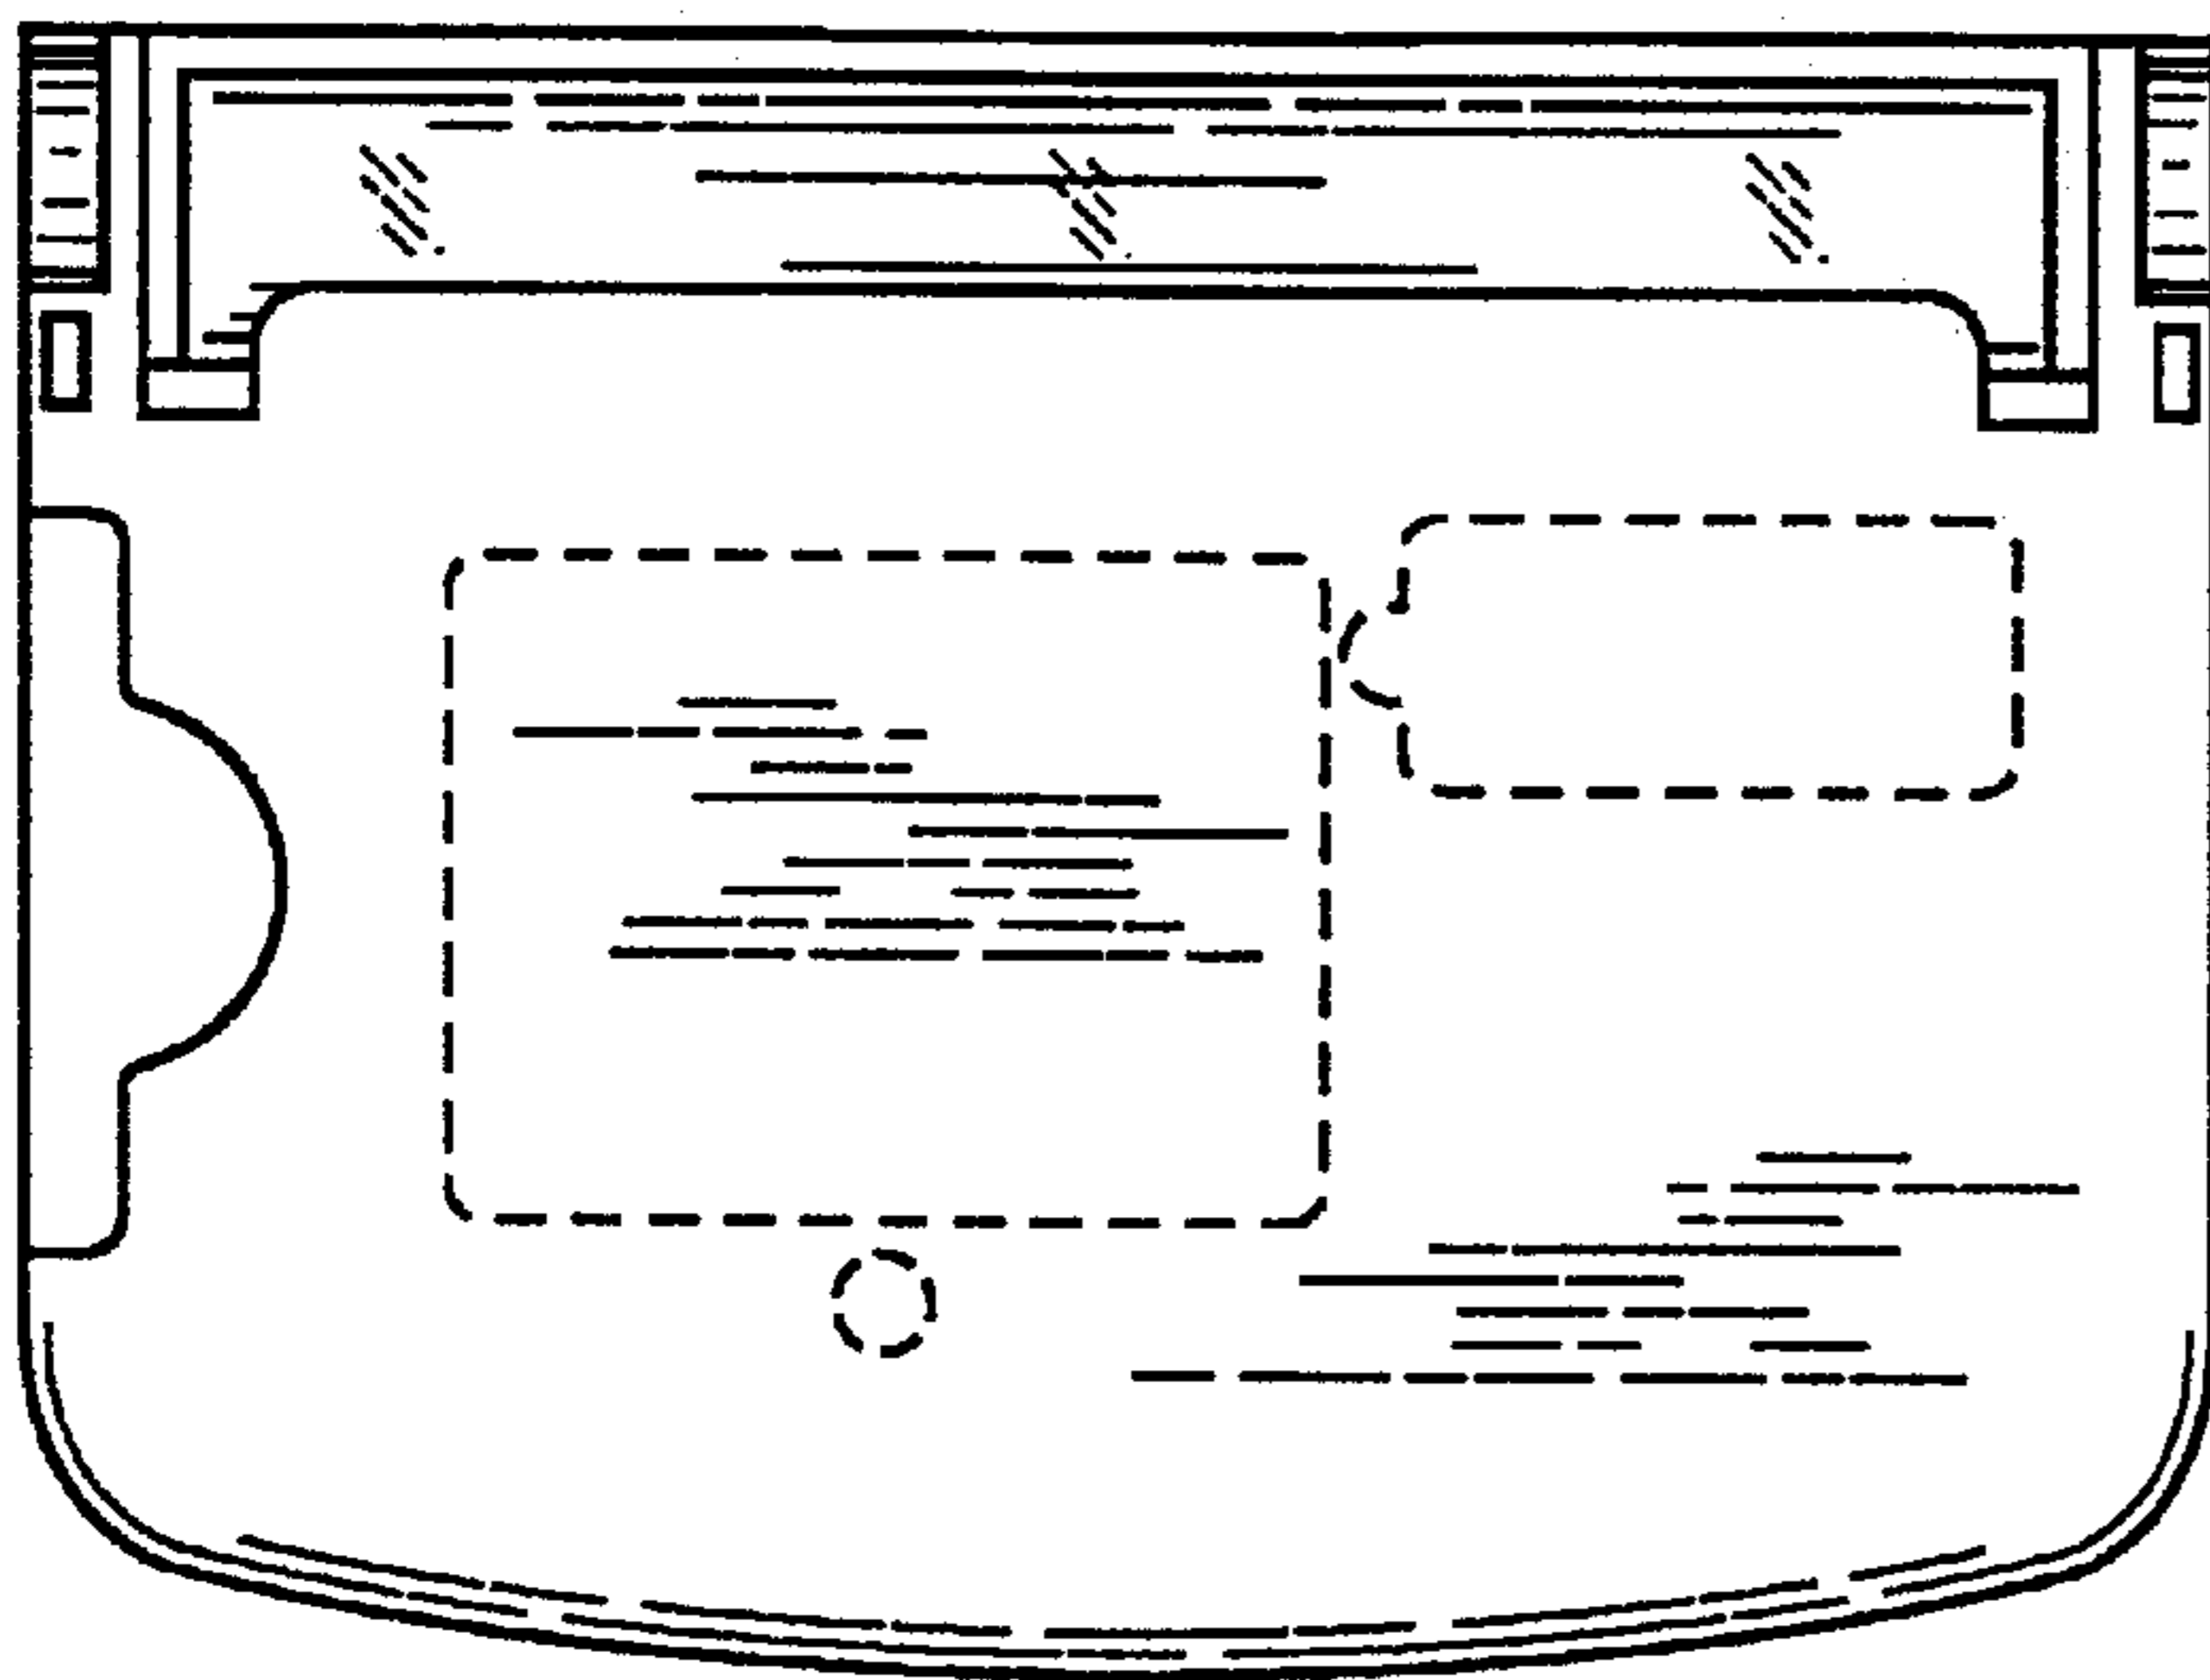


**FIG. 6**

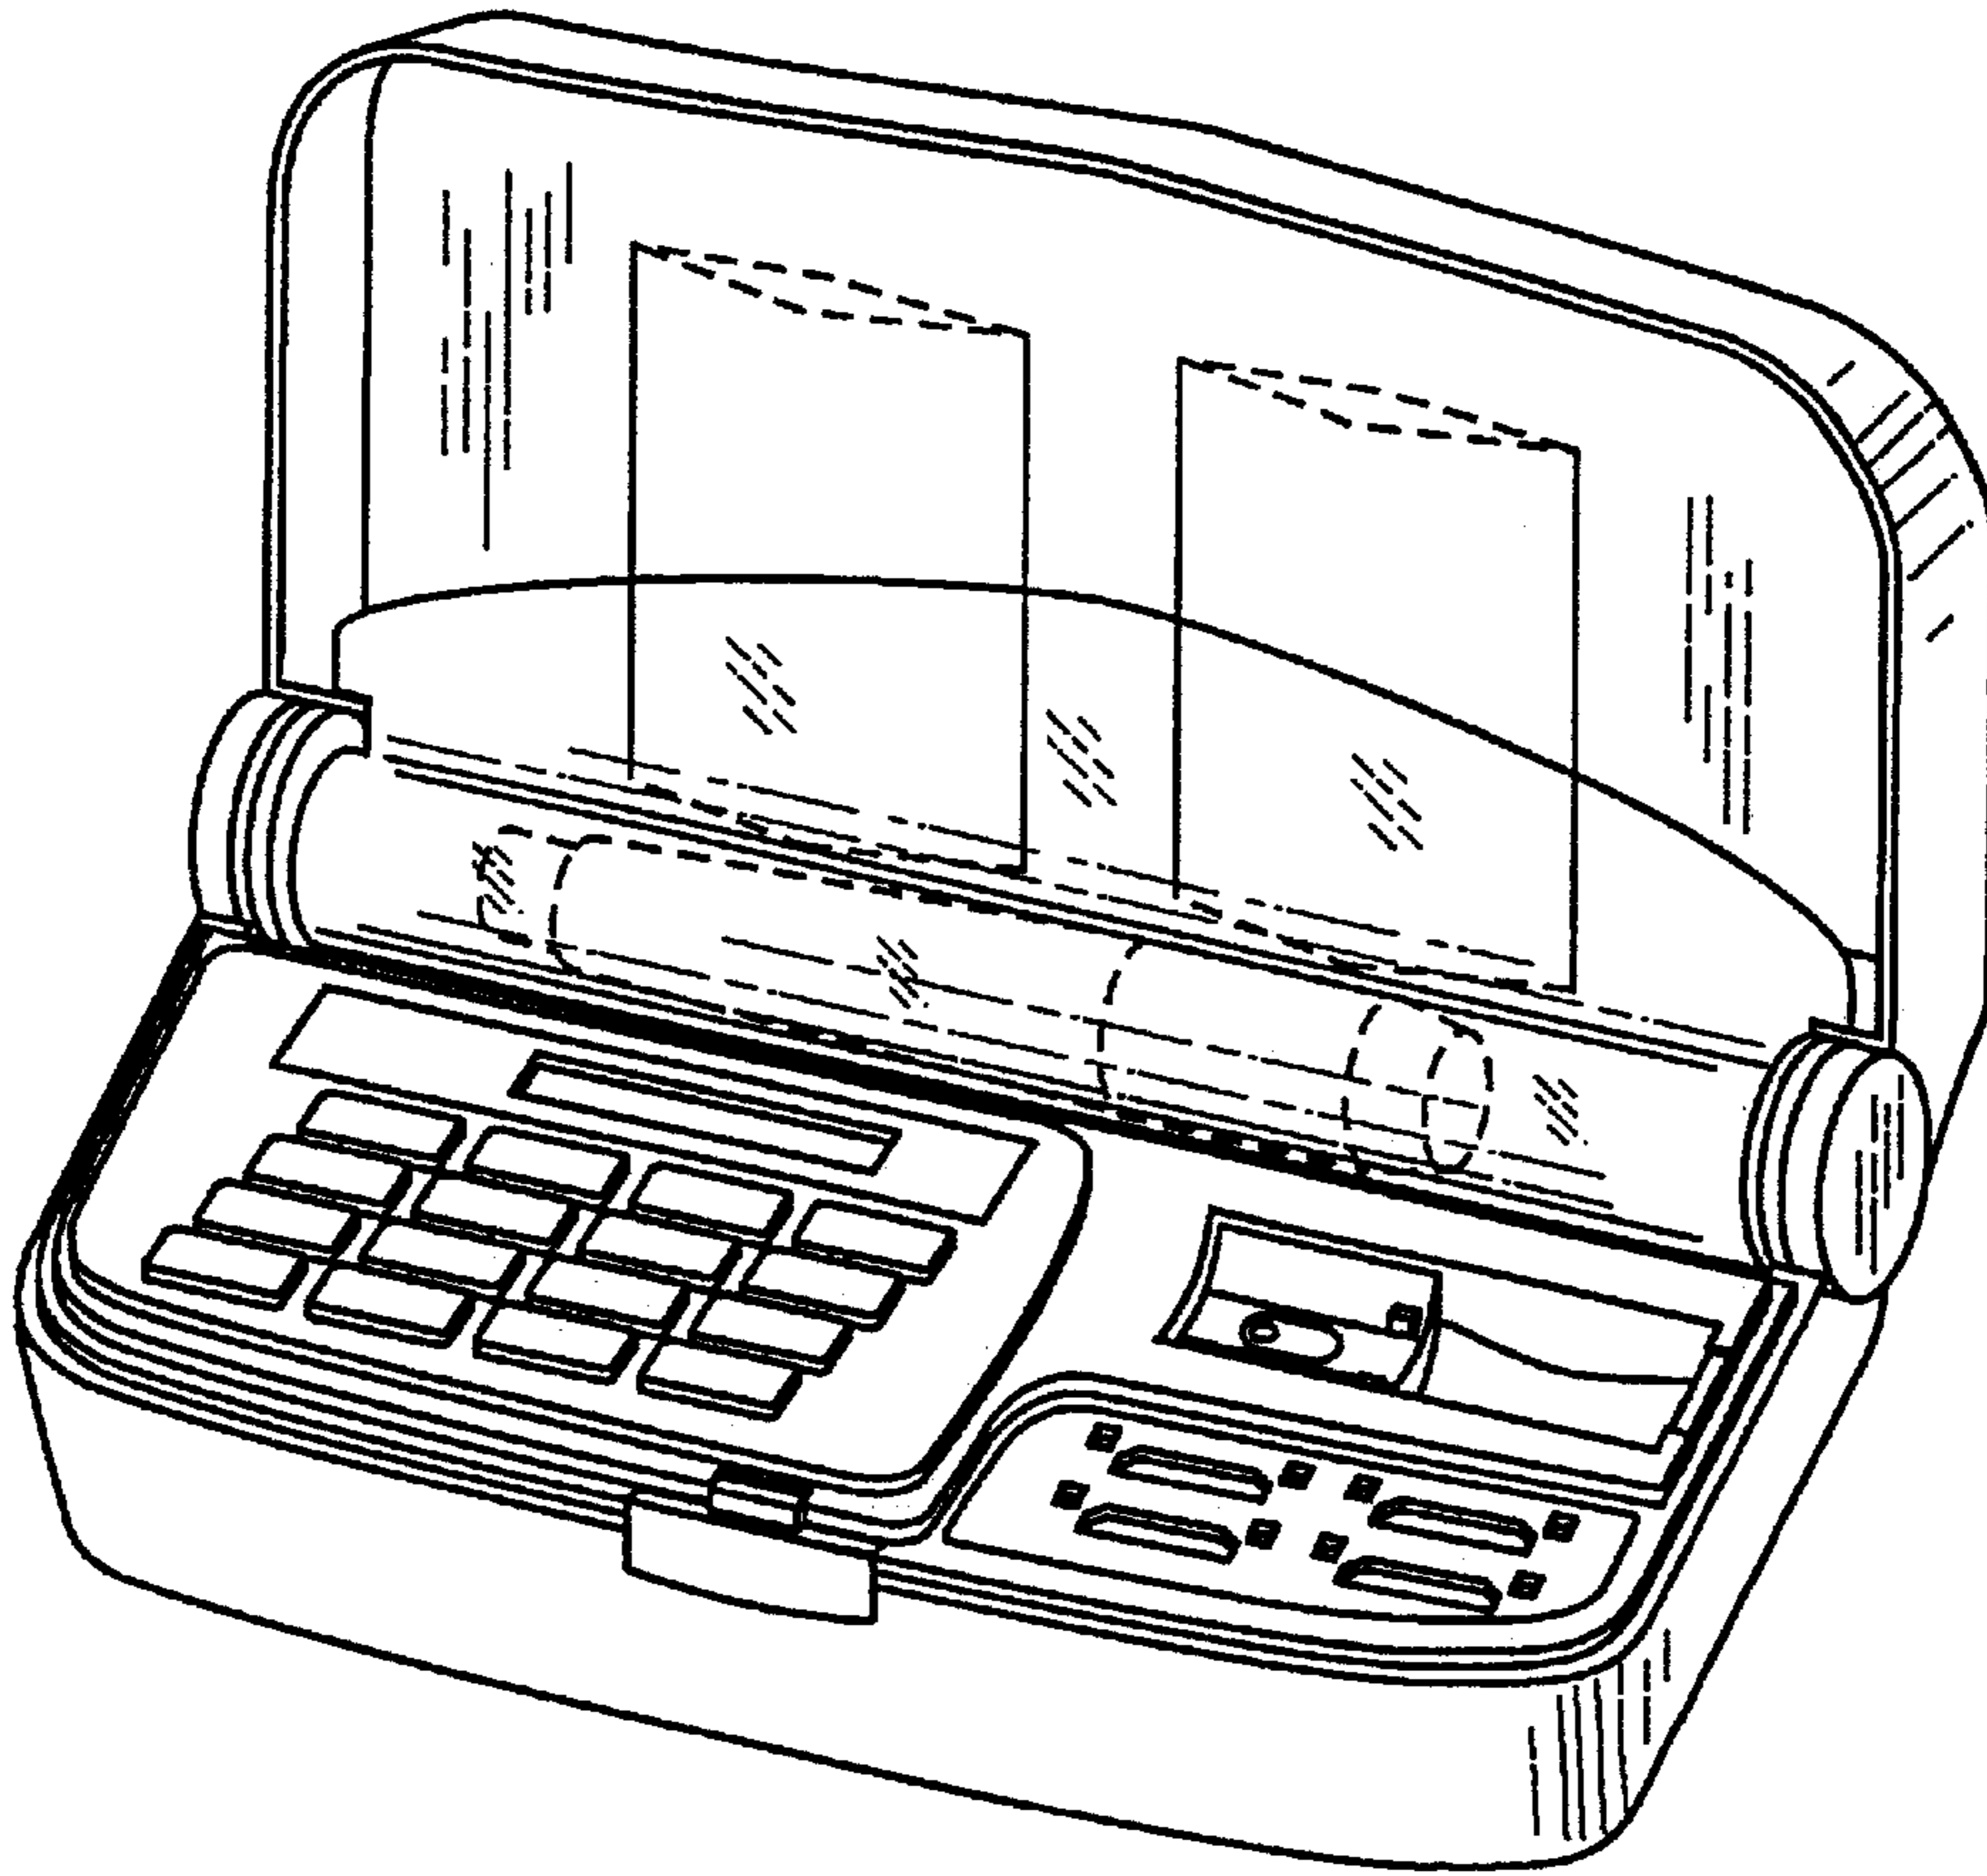


**FIG. 7**

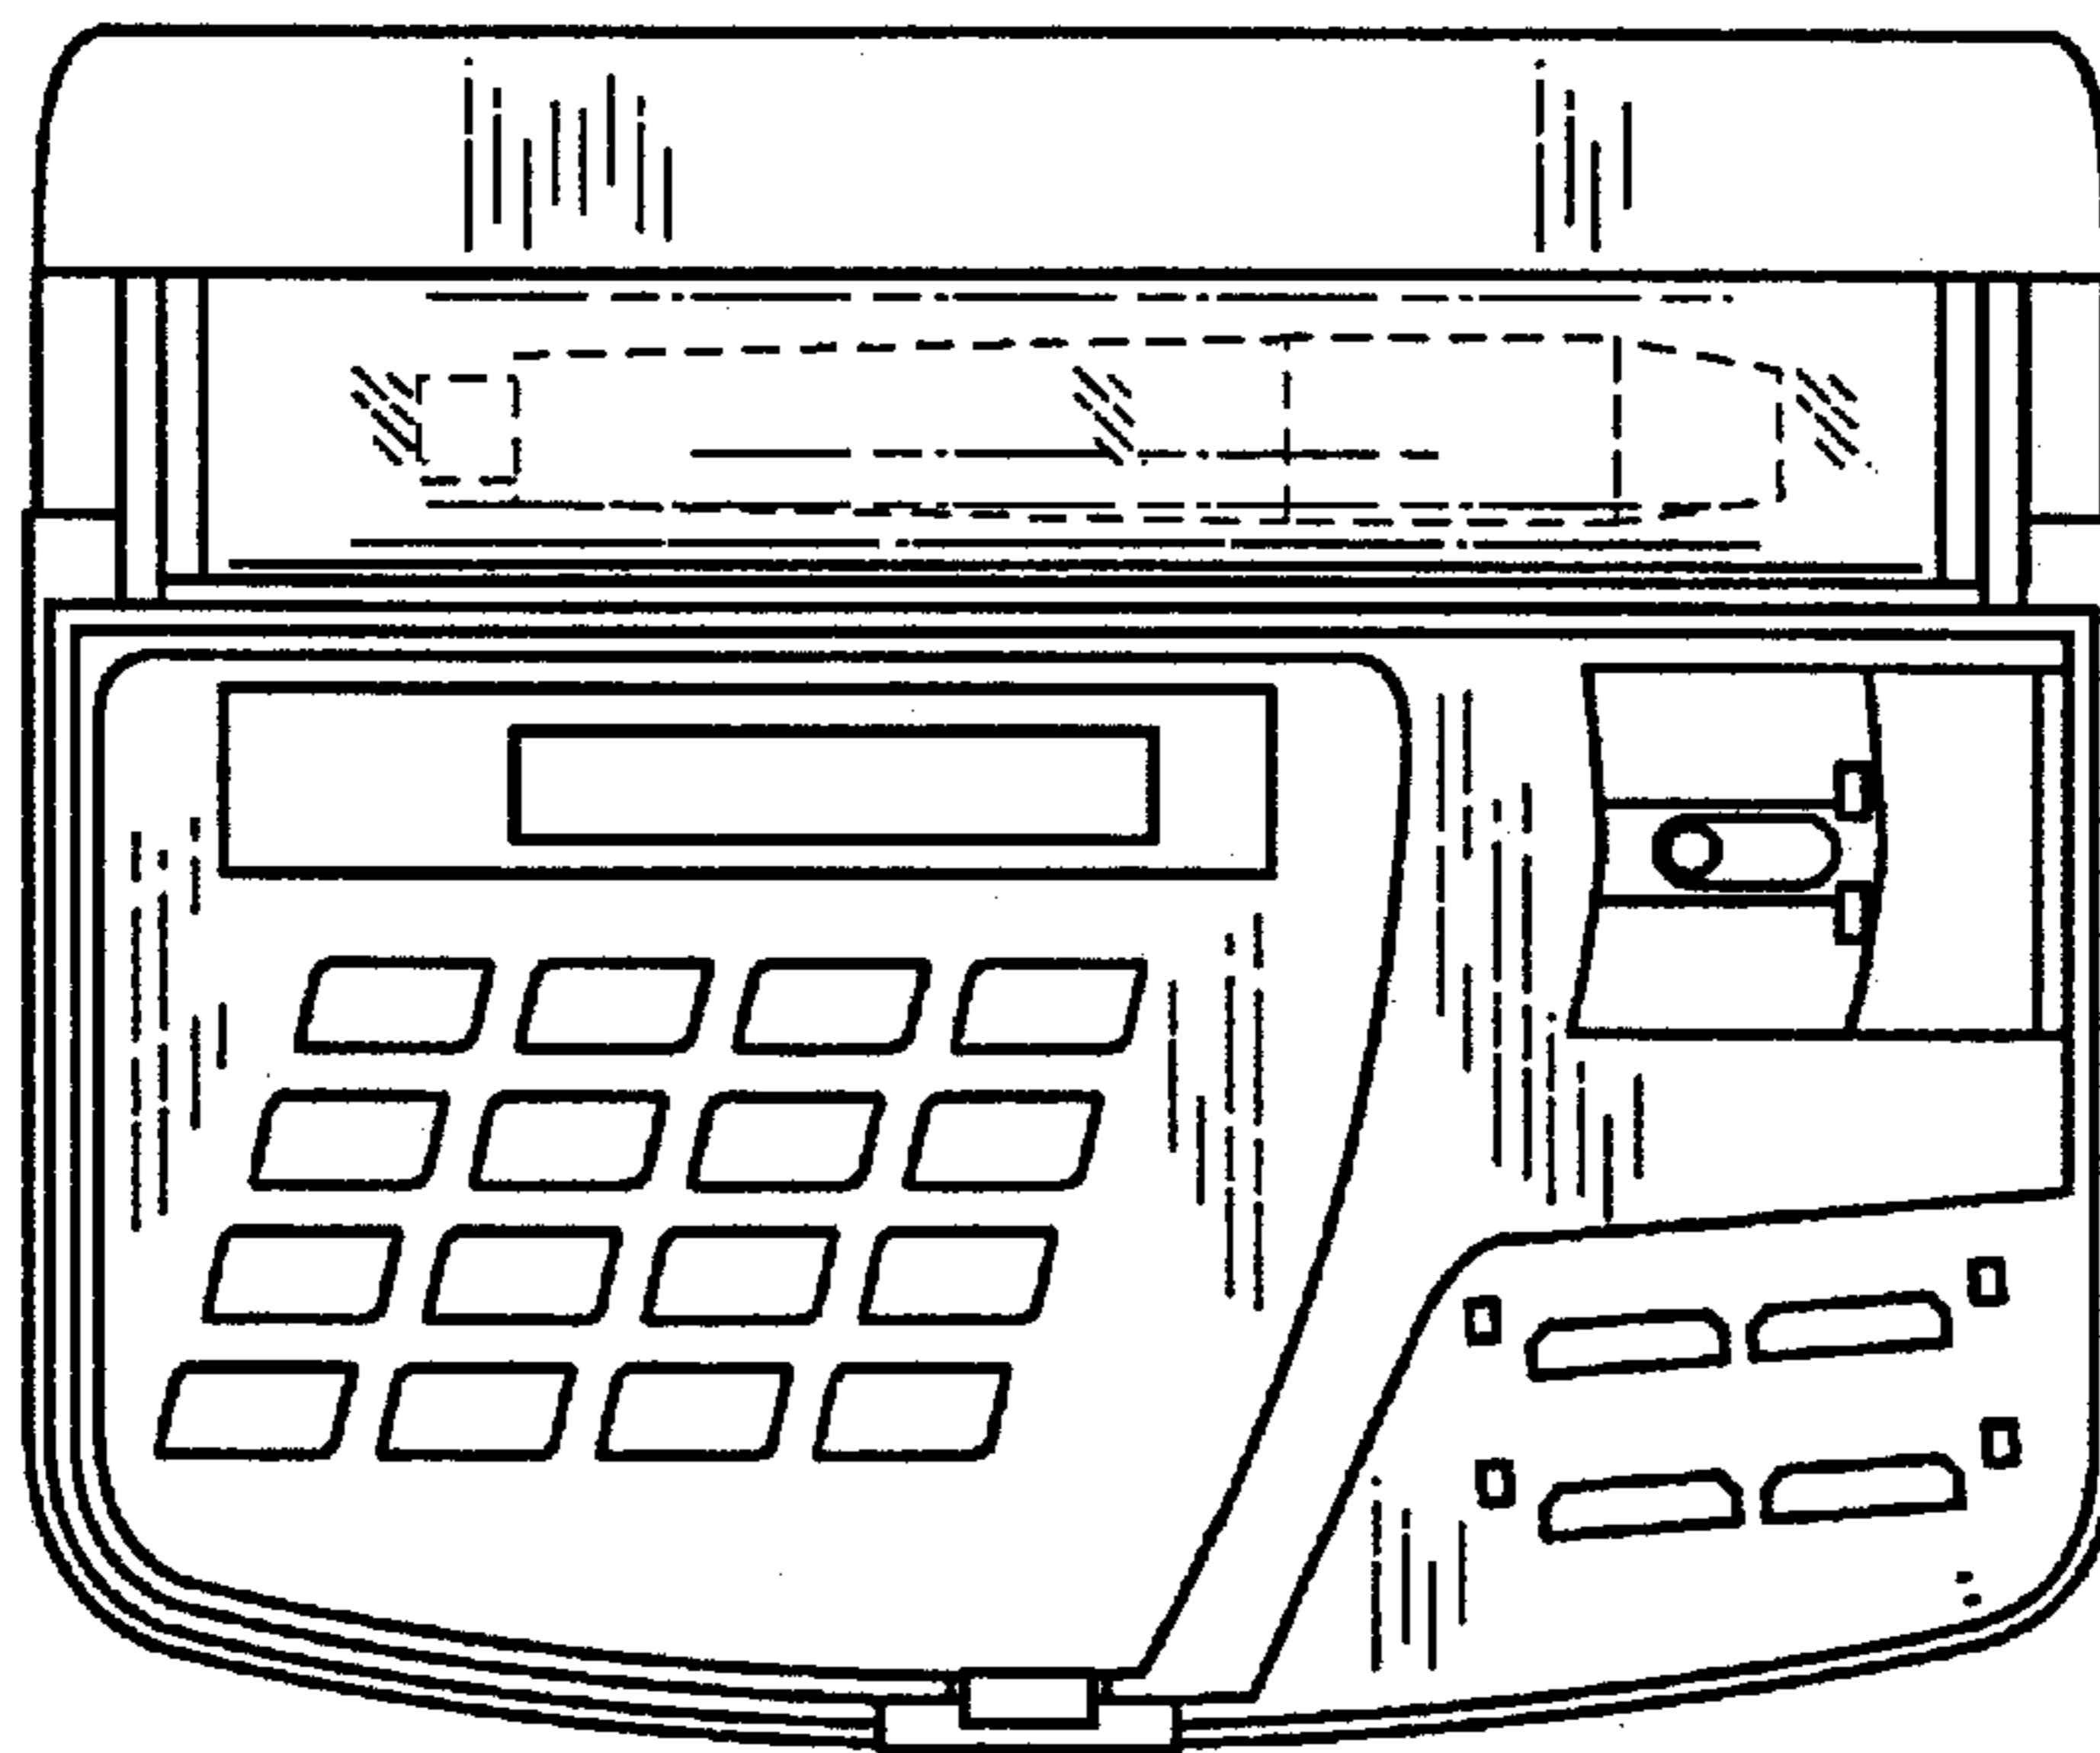


**FIG. 8**

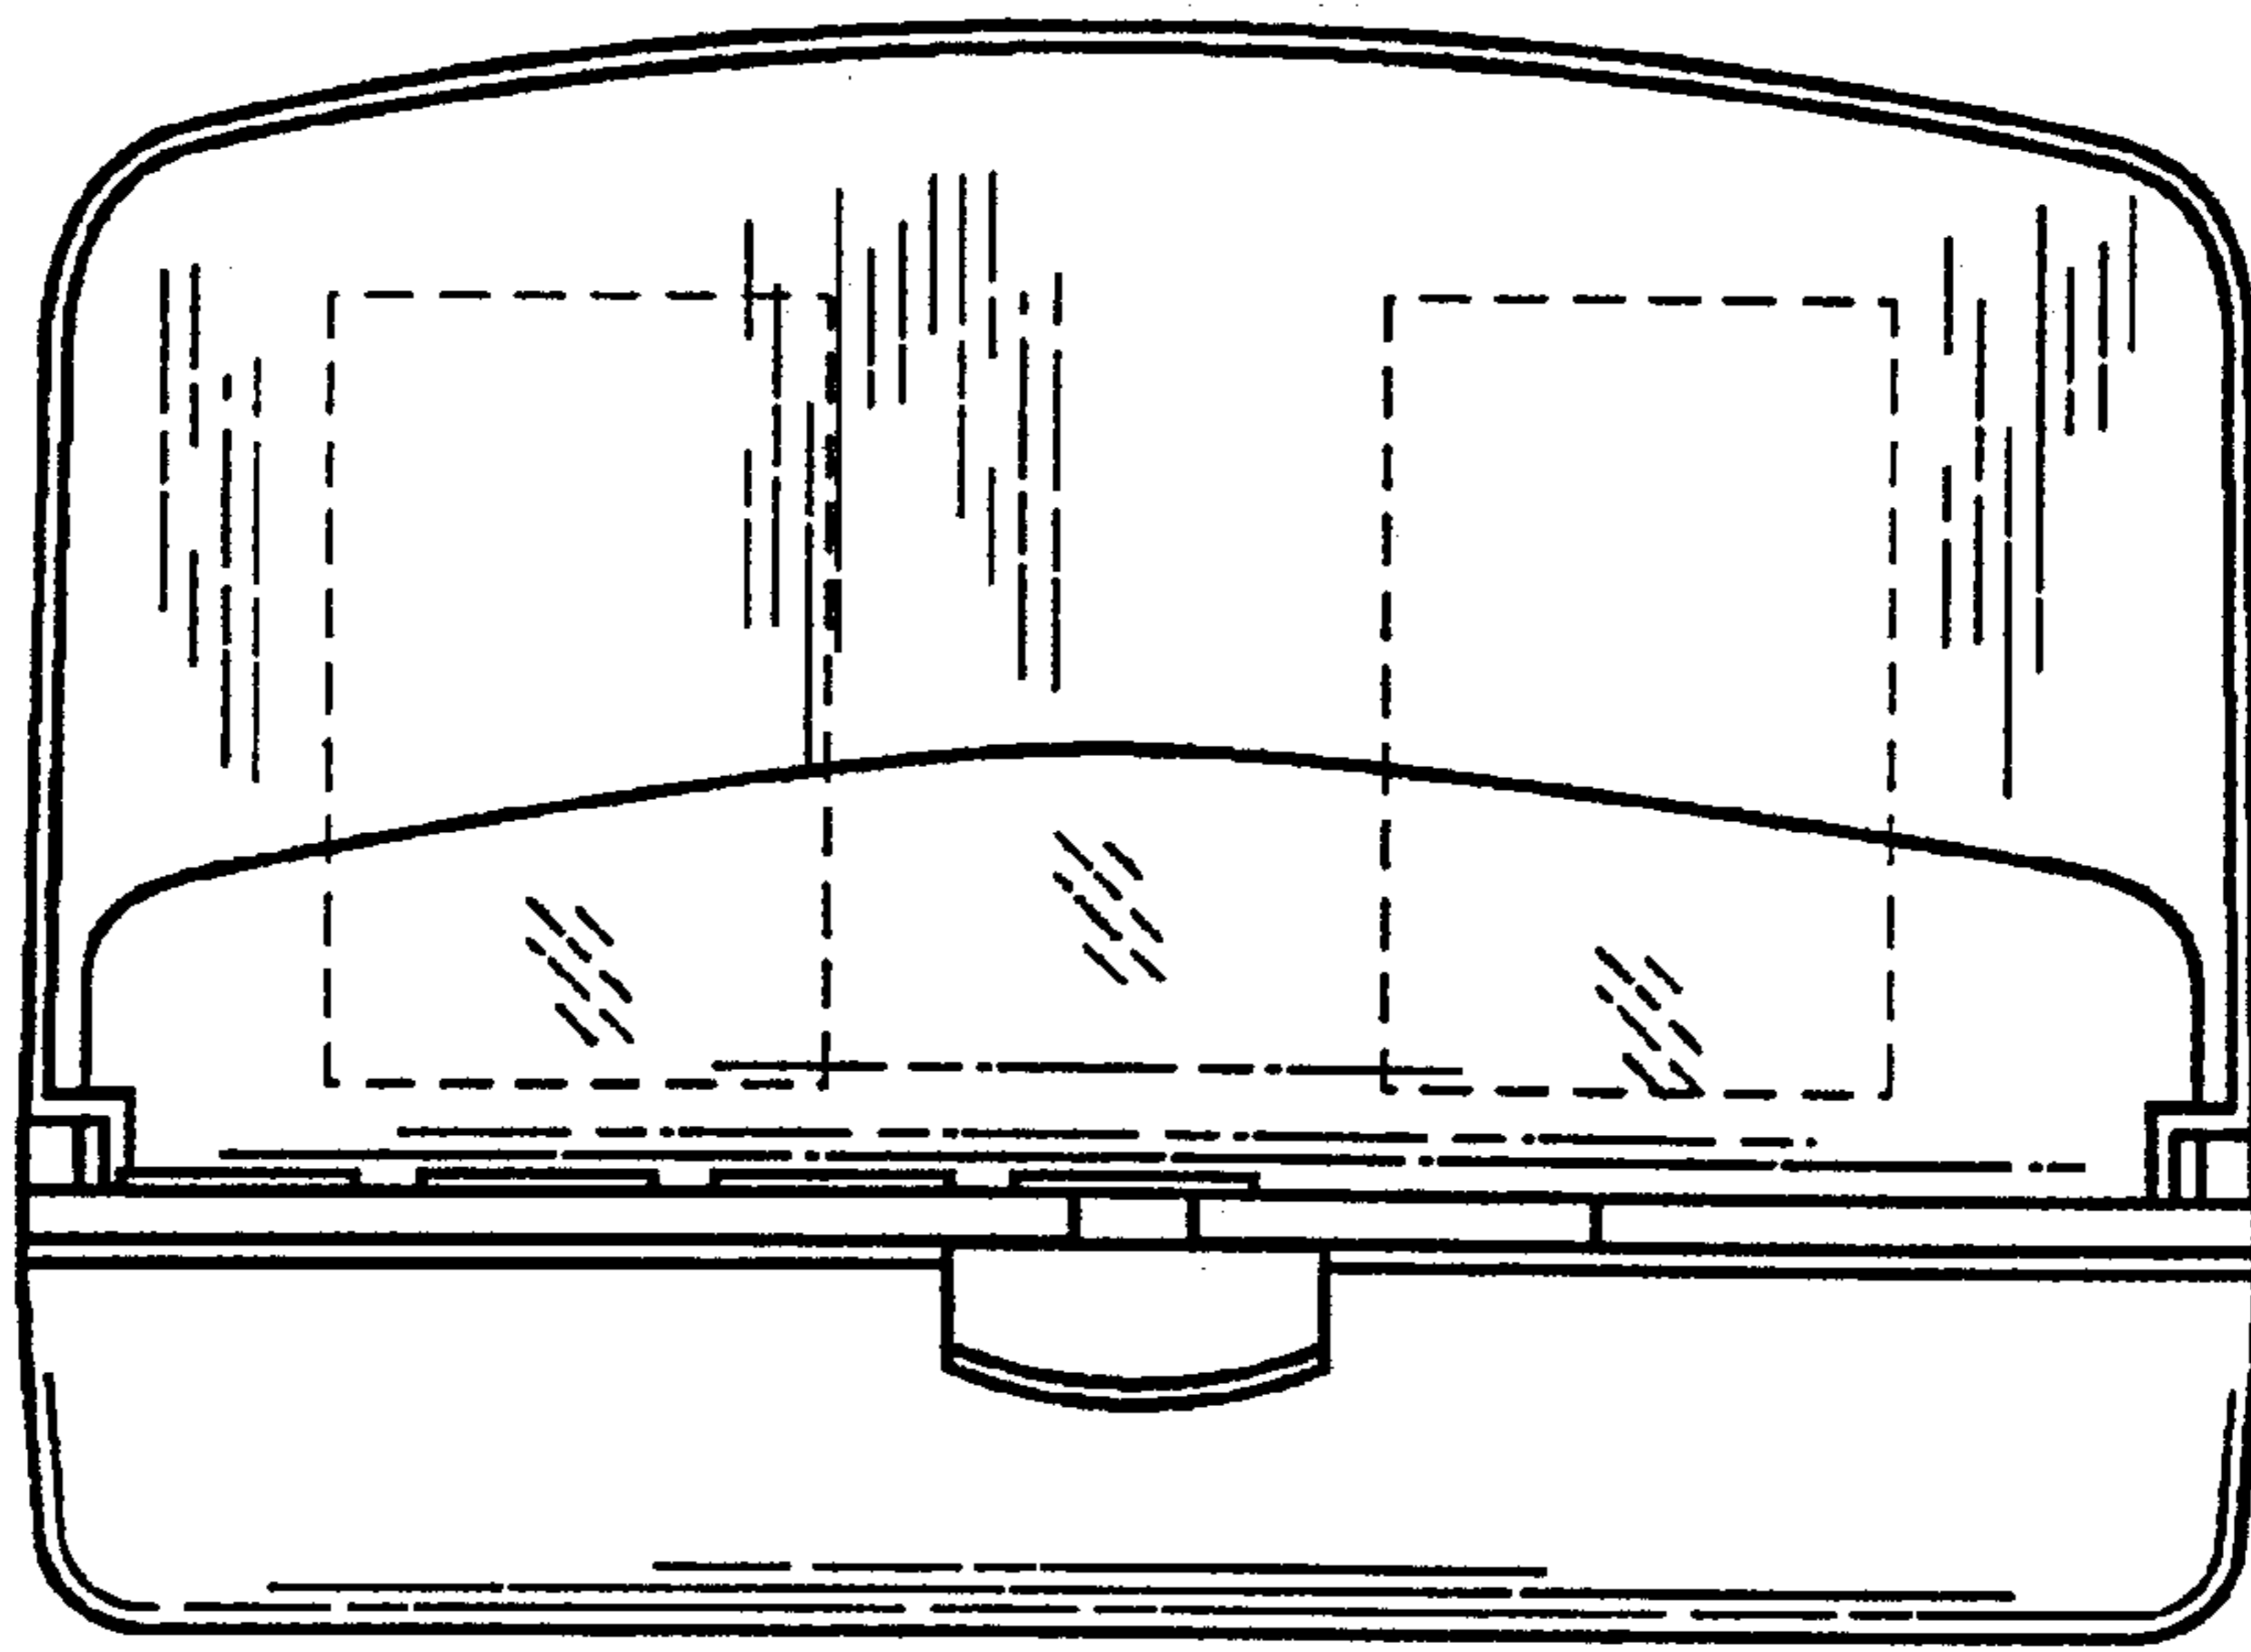


**FIG. 9**

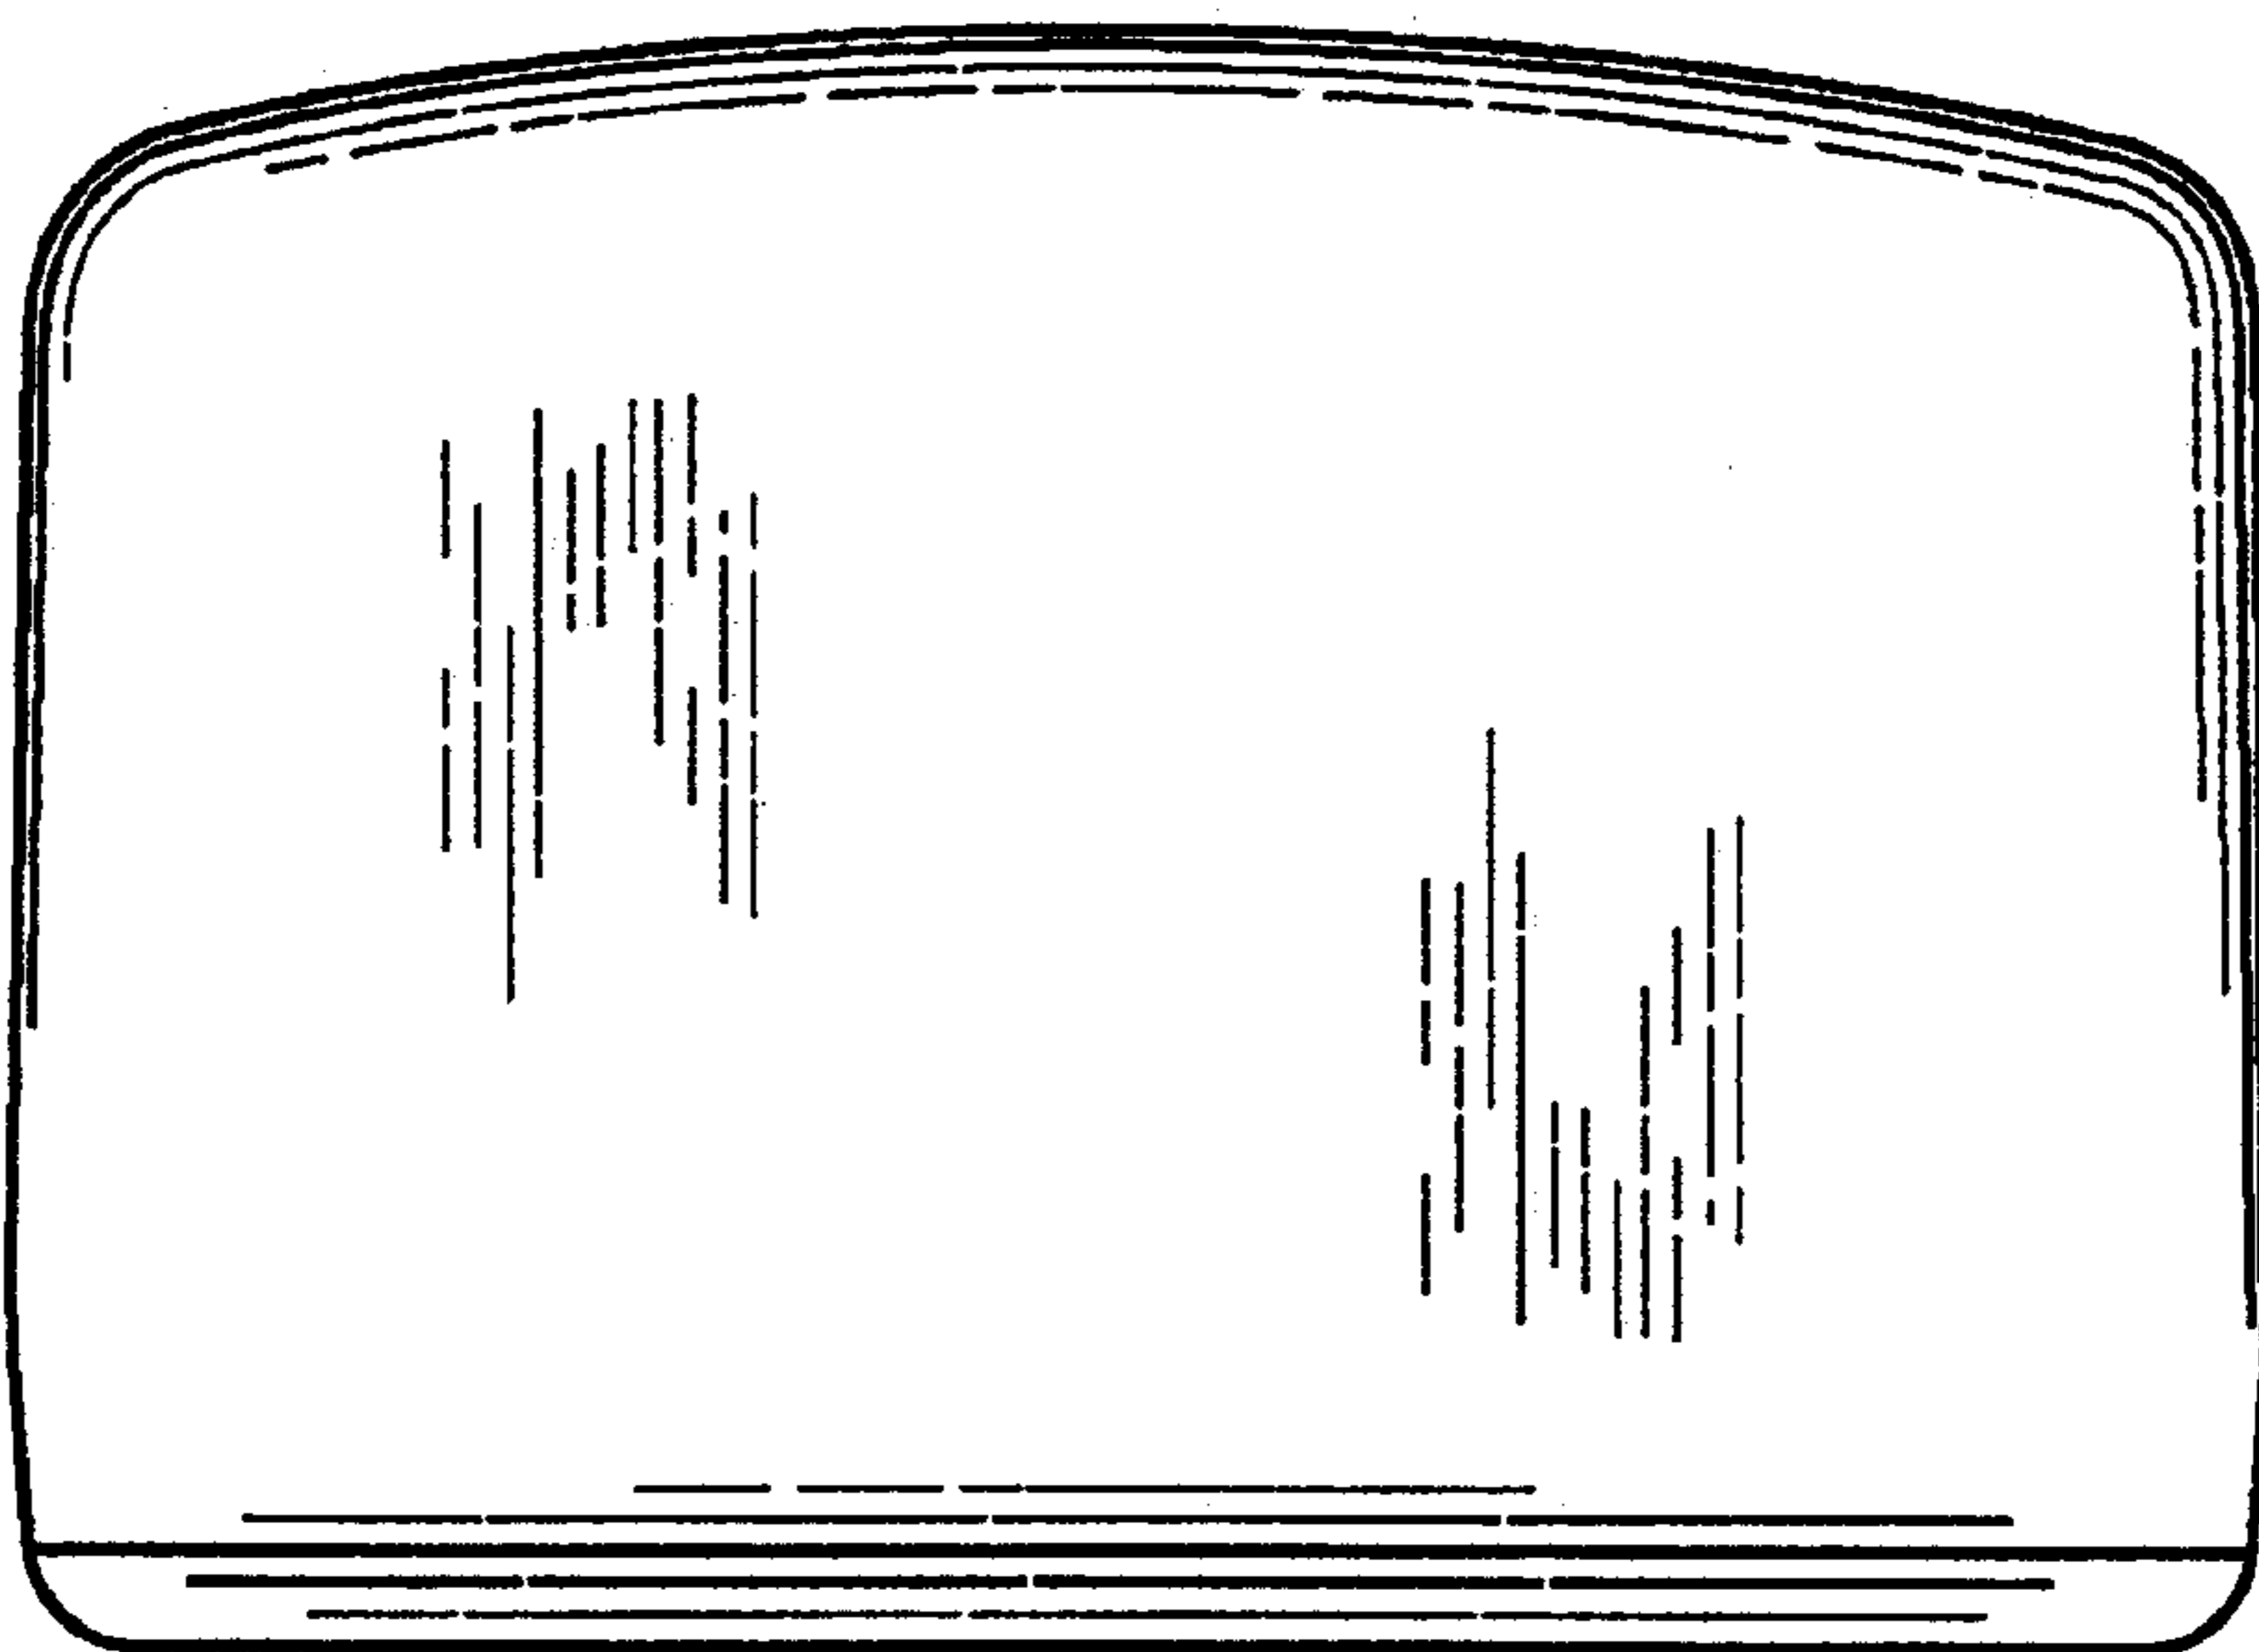

**FIG. 10**

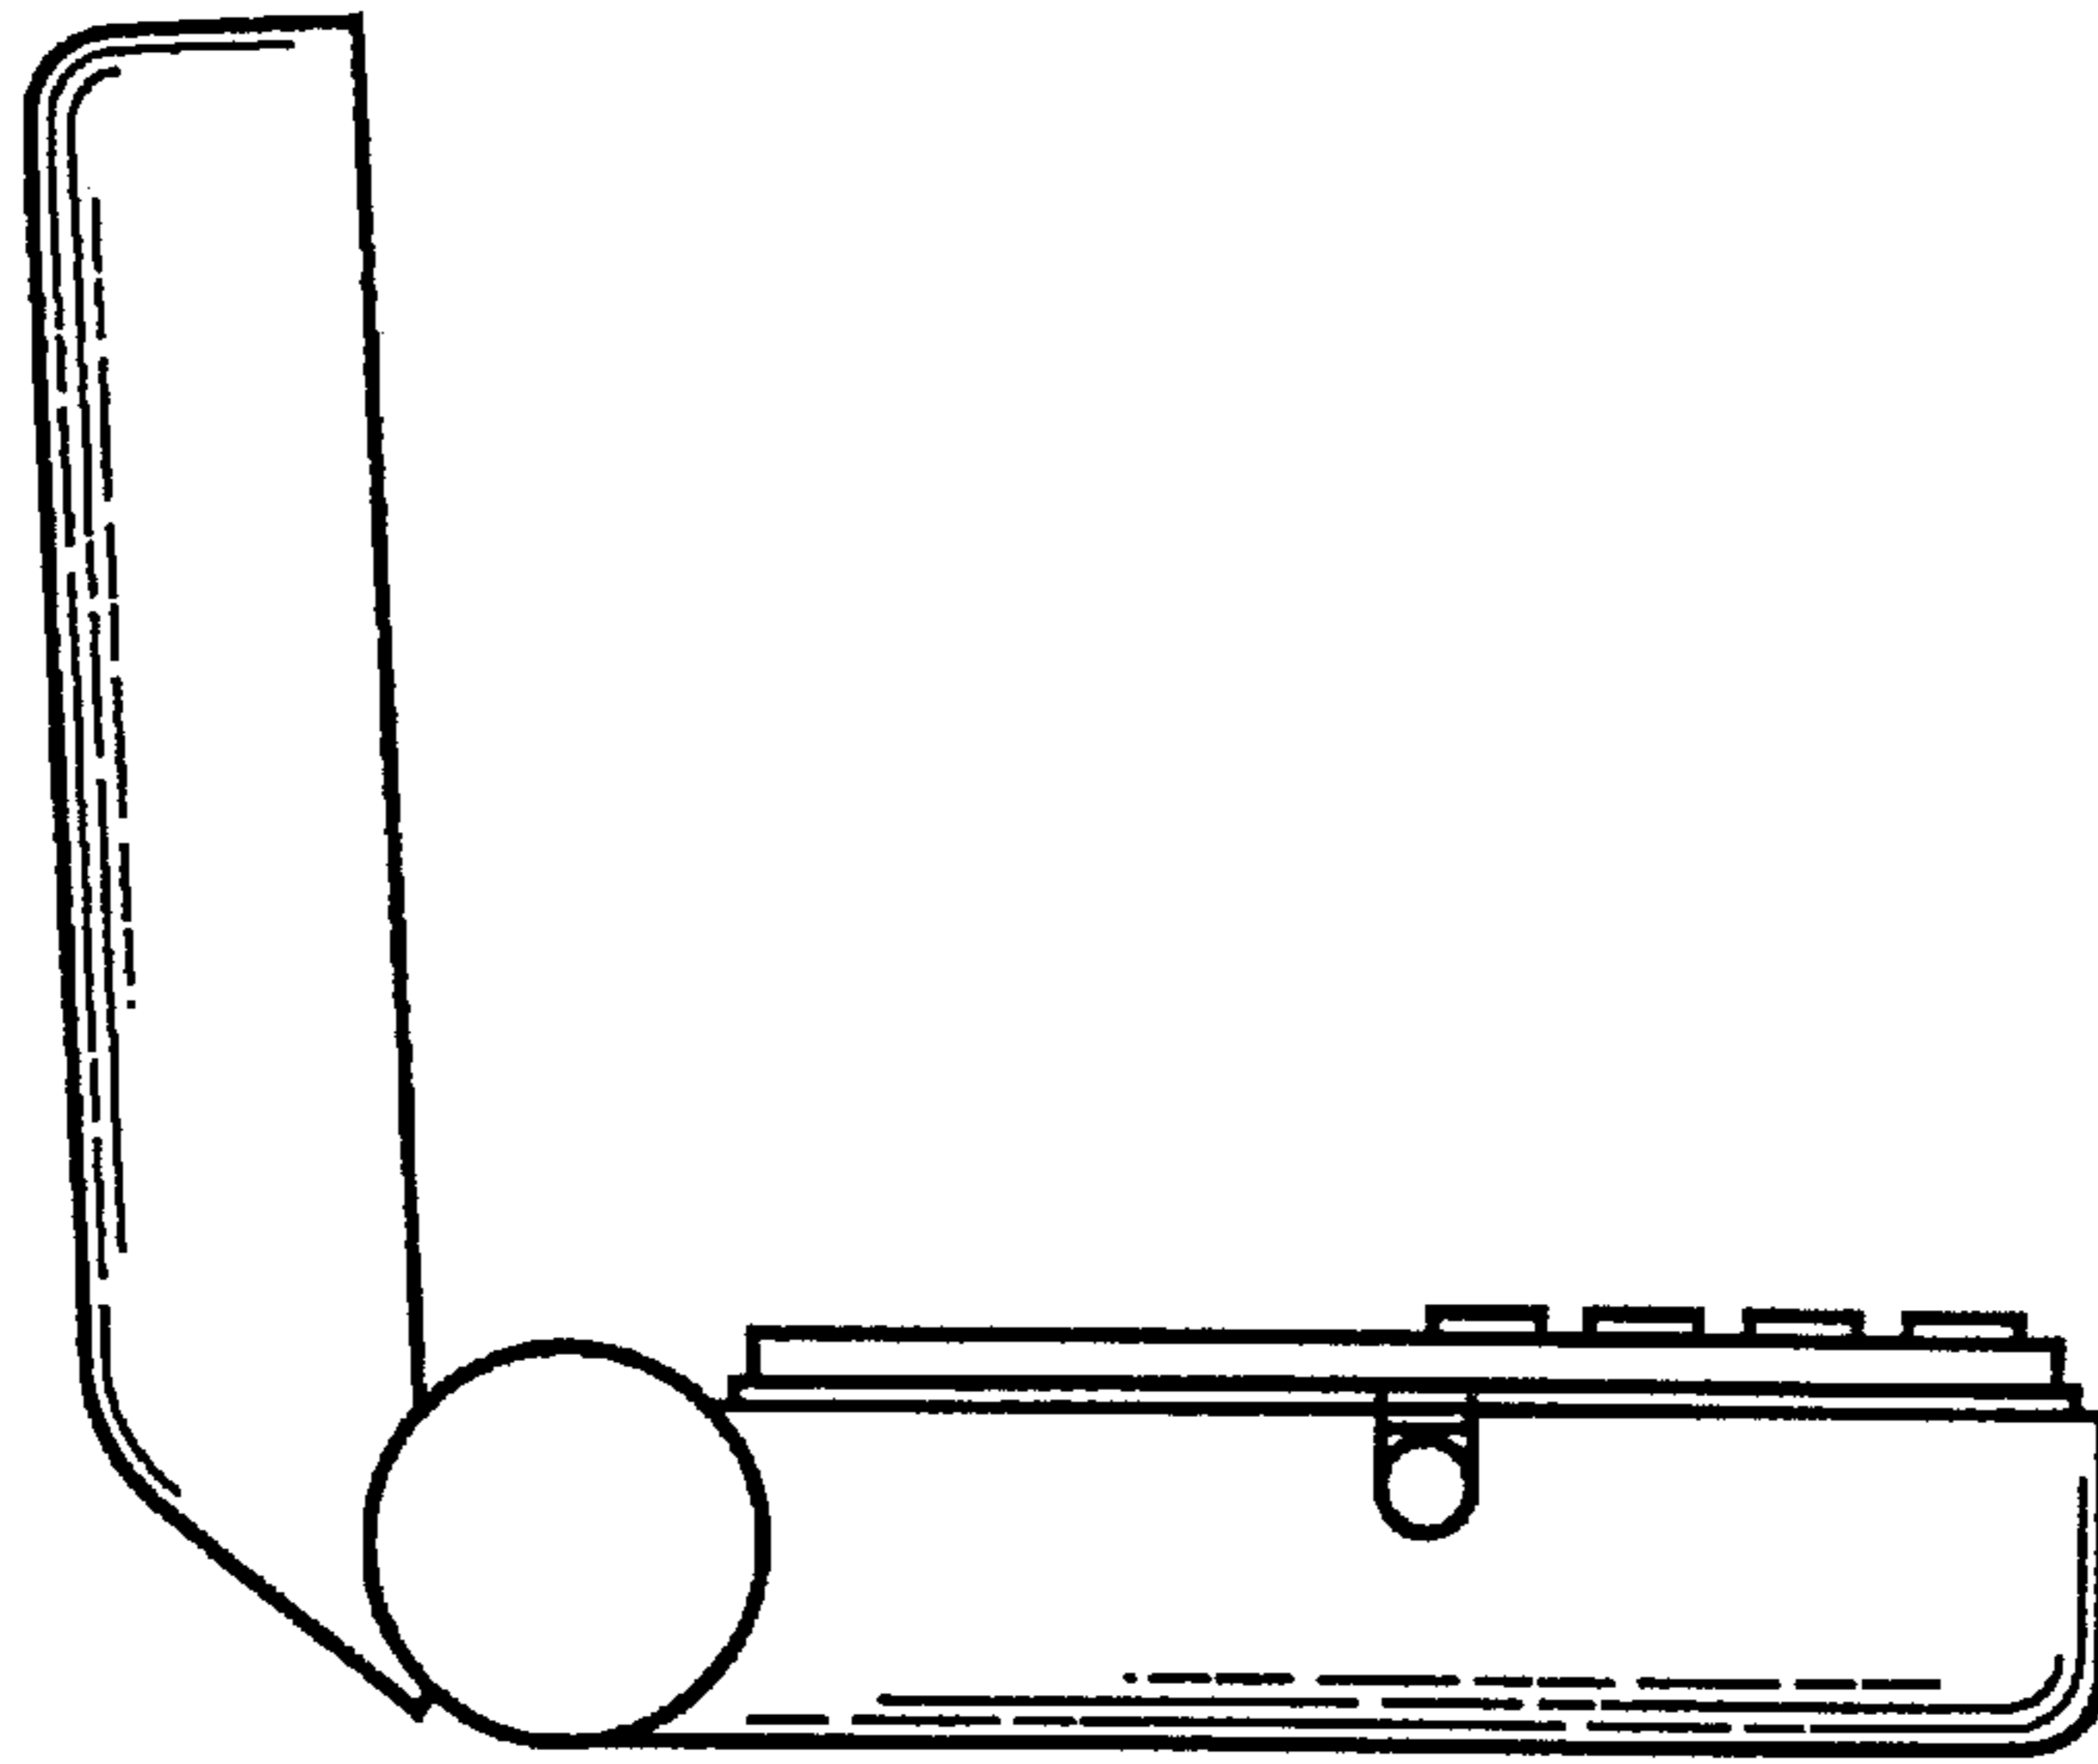

**FIG. 11**

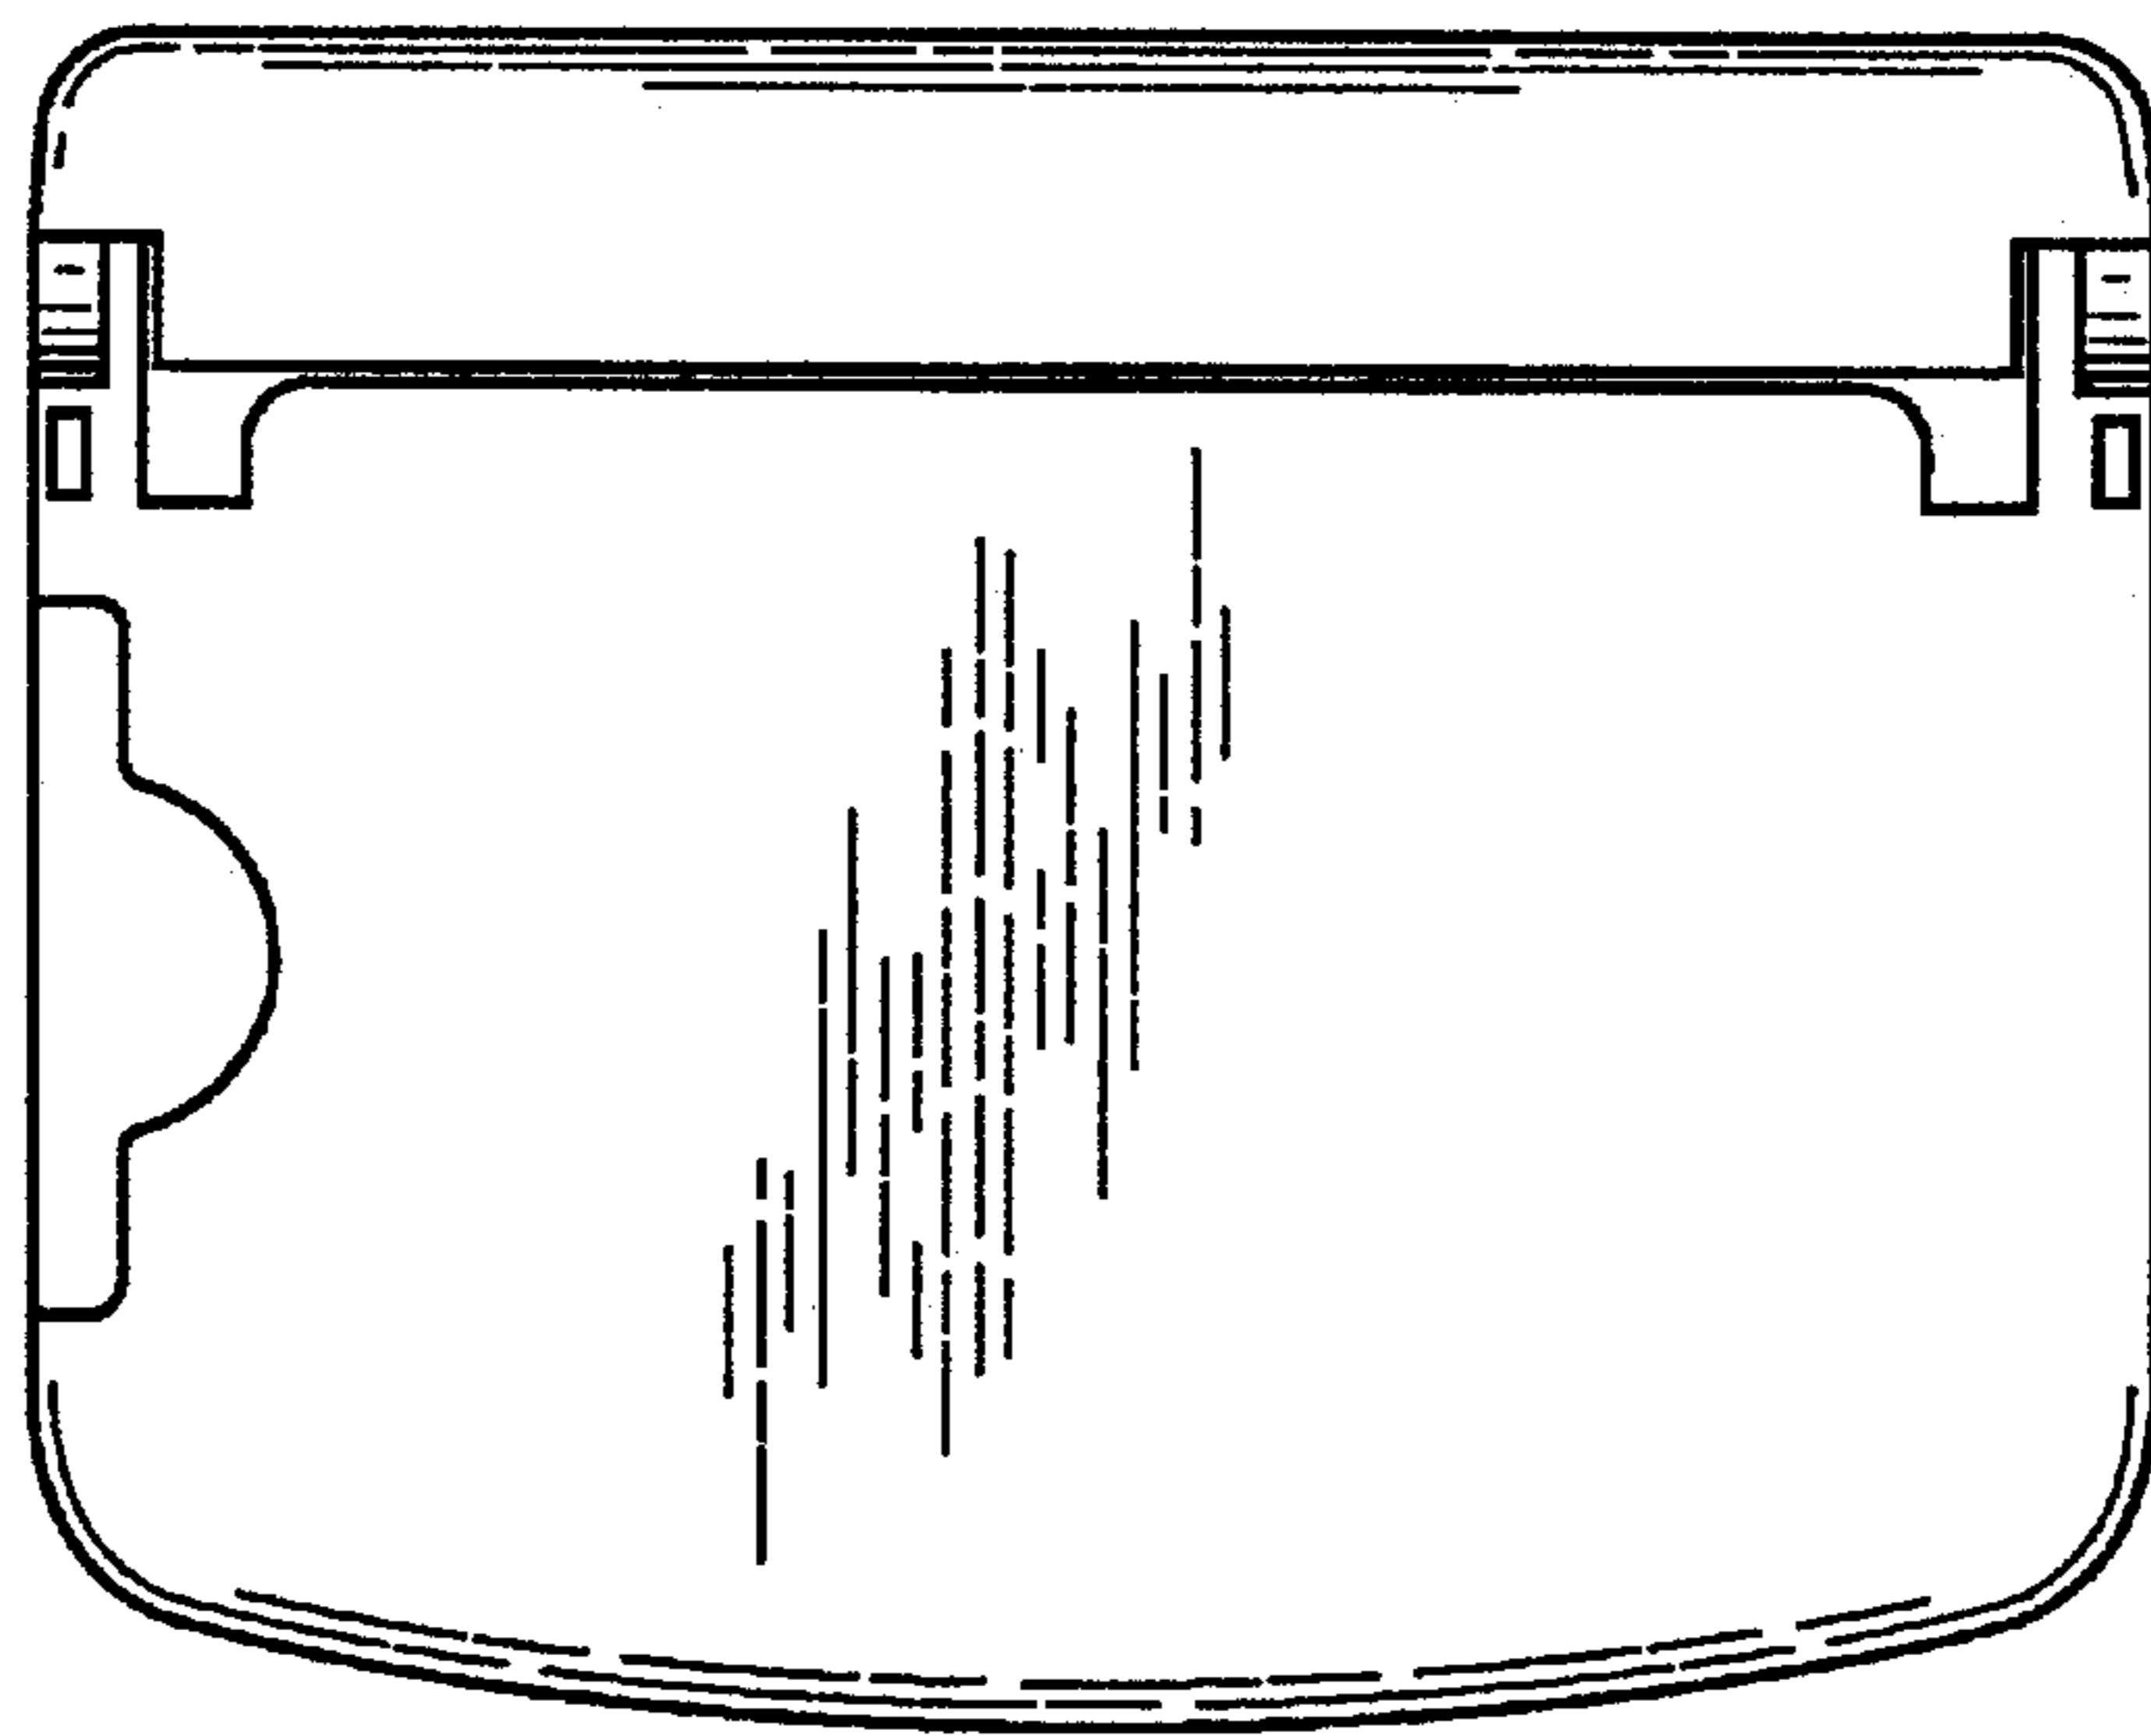

**FIG. 12**