



US00D479225S

(12) **United States Design Patent**
De Saulles

(10) **Patent No.:** **US D479,225 S**

(45) **Date of Patent:** **** Sep. 2, 2003**

(54) **HAND HELD CONTROL DEVICE**

(75) Inventor: **Stephen De Saulles**, London (GB)

(73) Assignee: **Patientline, plc**, Slough (GB)

(**) Term: **14 Years**

(21) Appl. No.: **29/148,273**

(22) Filed: **Sep. 15, 2001**

(30) **Foreign Application Priority Data**

Mar. 16, 2001 (GB) 2100364

(51) **LOC (7) Cl.** **14-03**

(52) **U.S. Cl.** **D14/218**

(58) **Field of Search** 200/43.17, 332.2;
D14/412, 416, 426, 428, 174, 217, 218,
137-139, 151, 191-193, 124, 299, 167-168;
D8/80, 107, 88, 102, 300, 308, 312; D4/642,
401.2; 30/340; D13/168, 162-164; D21/512-517,
566; D10/104, 106; 455/352-355, 151.1-151.4;
348/114, 734; D24/200

(56) **References Cited**

U.S. PATENT DOCUMENTS

3,511,951 A * 5/1970 Miller 200/332.2
D351,392 S * 10/1994 Bridges D14/226
D372,029 S * 7/1996 Young D14/218
D413,891 S * 9/1999 Walker D14/218
6,164,853 A * 12/2000 Foote 400/489
D458,264 S * 6/2002 MacGregor D14/426
D468,021 S * 12/2002 Gerth et al. D24/200
D469,542 S * 1/2003 Gerth D24/200

OTHER PUBLICATIONS

Brochure for BedWeb Integrated Patient System from Bedweb by Netherlands. Date believed to be not later than Sep., 2000. Four (4) sheets.

Product information sheet for Ascom Nira Telegration System from Ascom Holding Ltd. Switzerland. Date believed to be not later than Sep. 2000. One (1) sheet.

Product information sheet for Tyco system by Phillips. Date believed to be not later than Sep. 2000. One (1) sheet.

Partial product information sheet for Siemens AG television/radio/phone system. Date believed to be not later than Sep. 2000. One (1) sheet.

Photo of Zettler patient phone/television product from Zettler Electronics GmbH. Date believed to be not later than Sep. 2000. One (1) sheet.

Advertisement for Teleware bedside telephone and television from Teleware Systems Limited. Date believed to be not later than Sep. 2000. One (1) sheet.

Photo of HTS phone/television product from Health Television System, Inc. Date believed to be not later than Sep. 2000. One (1) sheet.

Website prints and product photos for the Patientline system from Patientline plc. Not later than Sep., 2000. Eleven (11) sheets).

Product literature for Ackerman. Date Unknown. Seven (7) sheets. www.ackerman.com/clino/index.html.

(List continued on next page.)

Primary Examiner—Louis S. Zarfaz

Assistant Examiner—Deanne Levy

(74) *Attorney, Agent, or Firm*—Clayton, Howarth & Cannon, P.C.


(57) **CLAIM**

I claim the ornamental design for a hand held control device, as shown and described.

DESCRIPTION

FIG. 1 is a perspective view thereof;
FIG. 2 is a top view thereof;
FIG. 3 is a bottom view thereof;
FIG. 4 is a right side view thereof;
FIG. 5 is a left side view thereof;
FIG. 6 is a front view thereof; and,
FIG. 7 is a rear view thereof.

1 Claim, 2 Drawing Sheets

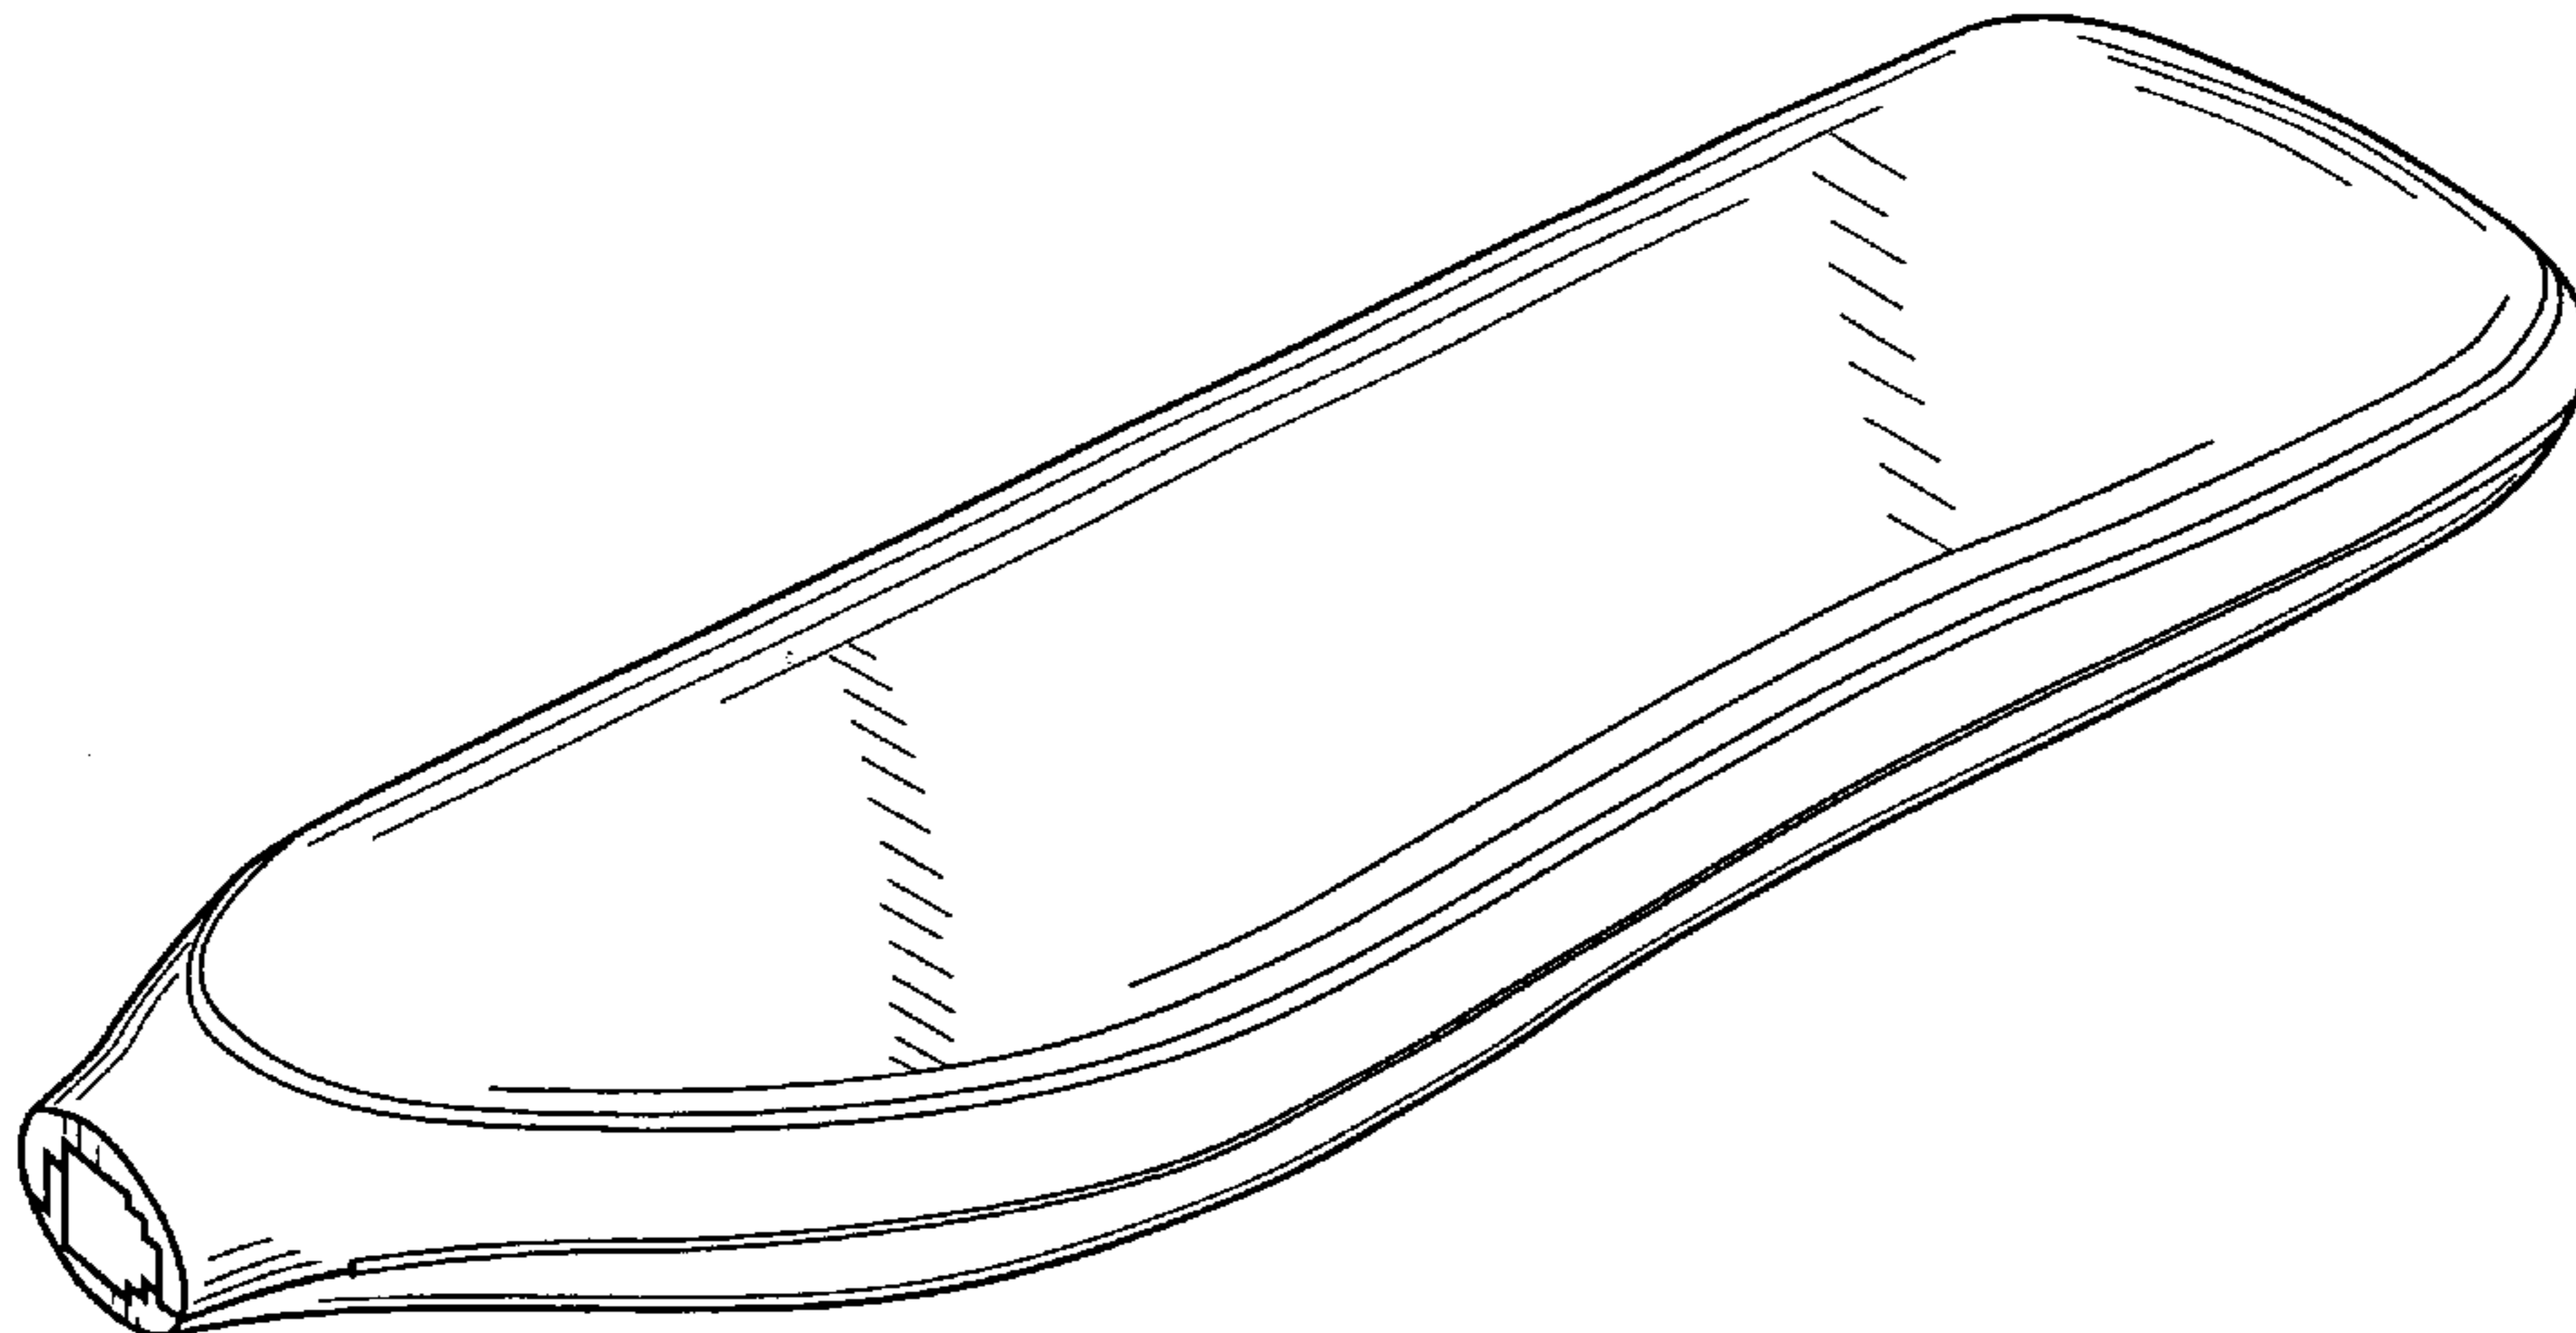

OTHER PUBLICATIONS

Product literature for HCIC+. Date Unknown. Three (3) sheets. www.hcic.com/products/television/index.htm.

Product literature for Kerfone. Date Unknow. Three (3) sheets. www.kerfone.co.uk/kerfone.htm.

Product literature for Schmelter. Date Unknown. Three (3) sheets. www.avm-schmelter.de/lcd.htm.

Product literature for Wandsworth. Date Unknown. One (1) sheet. www.wandsworth-electrical.com/page99.htm.

Product literature for Static Systems Group. Date Unknown. One (1) sheet. www.staticsystems.co.uk.

* cited by examiner

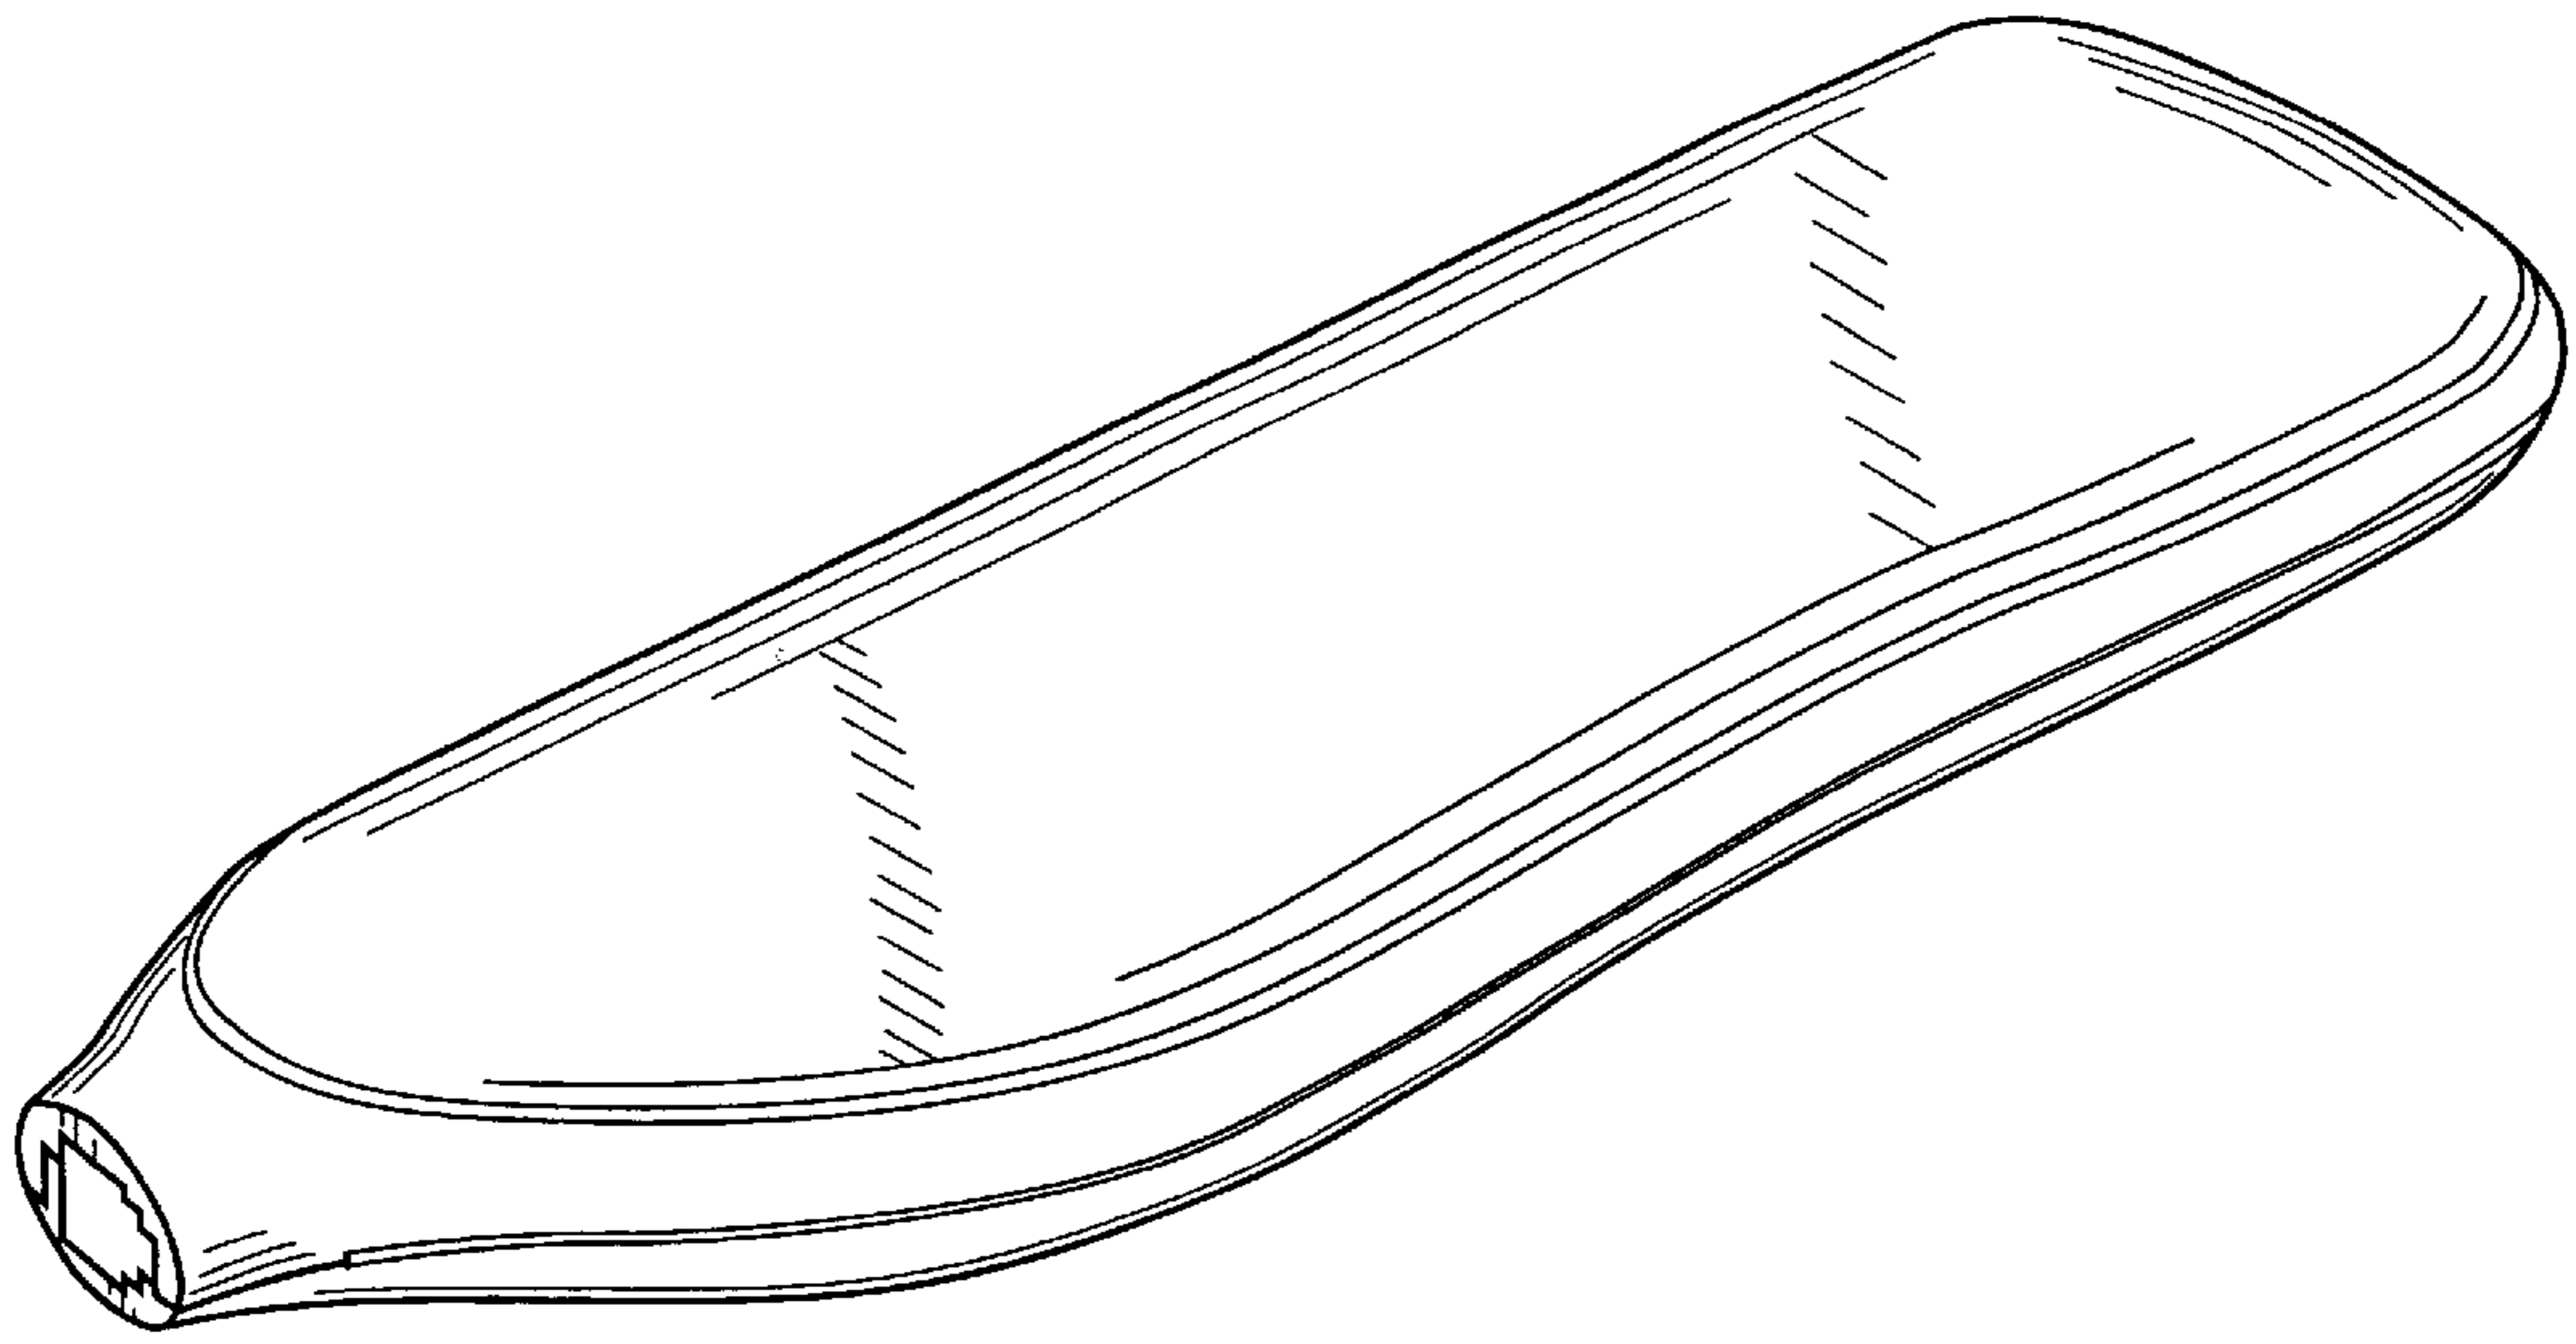


Fig. 1

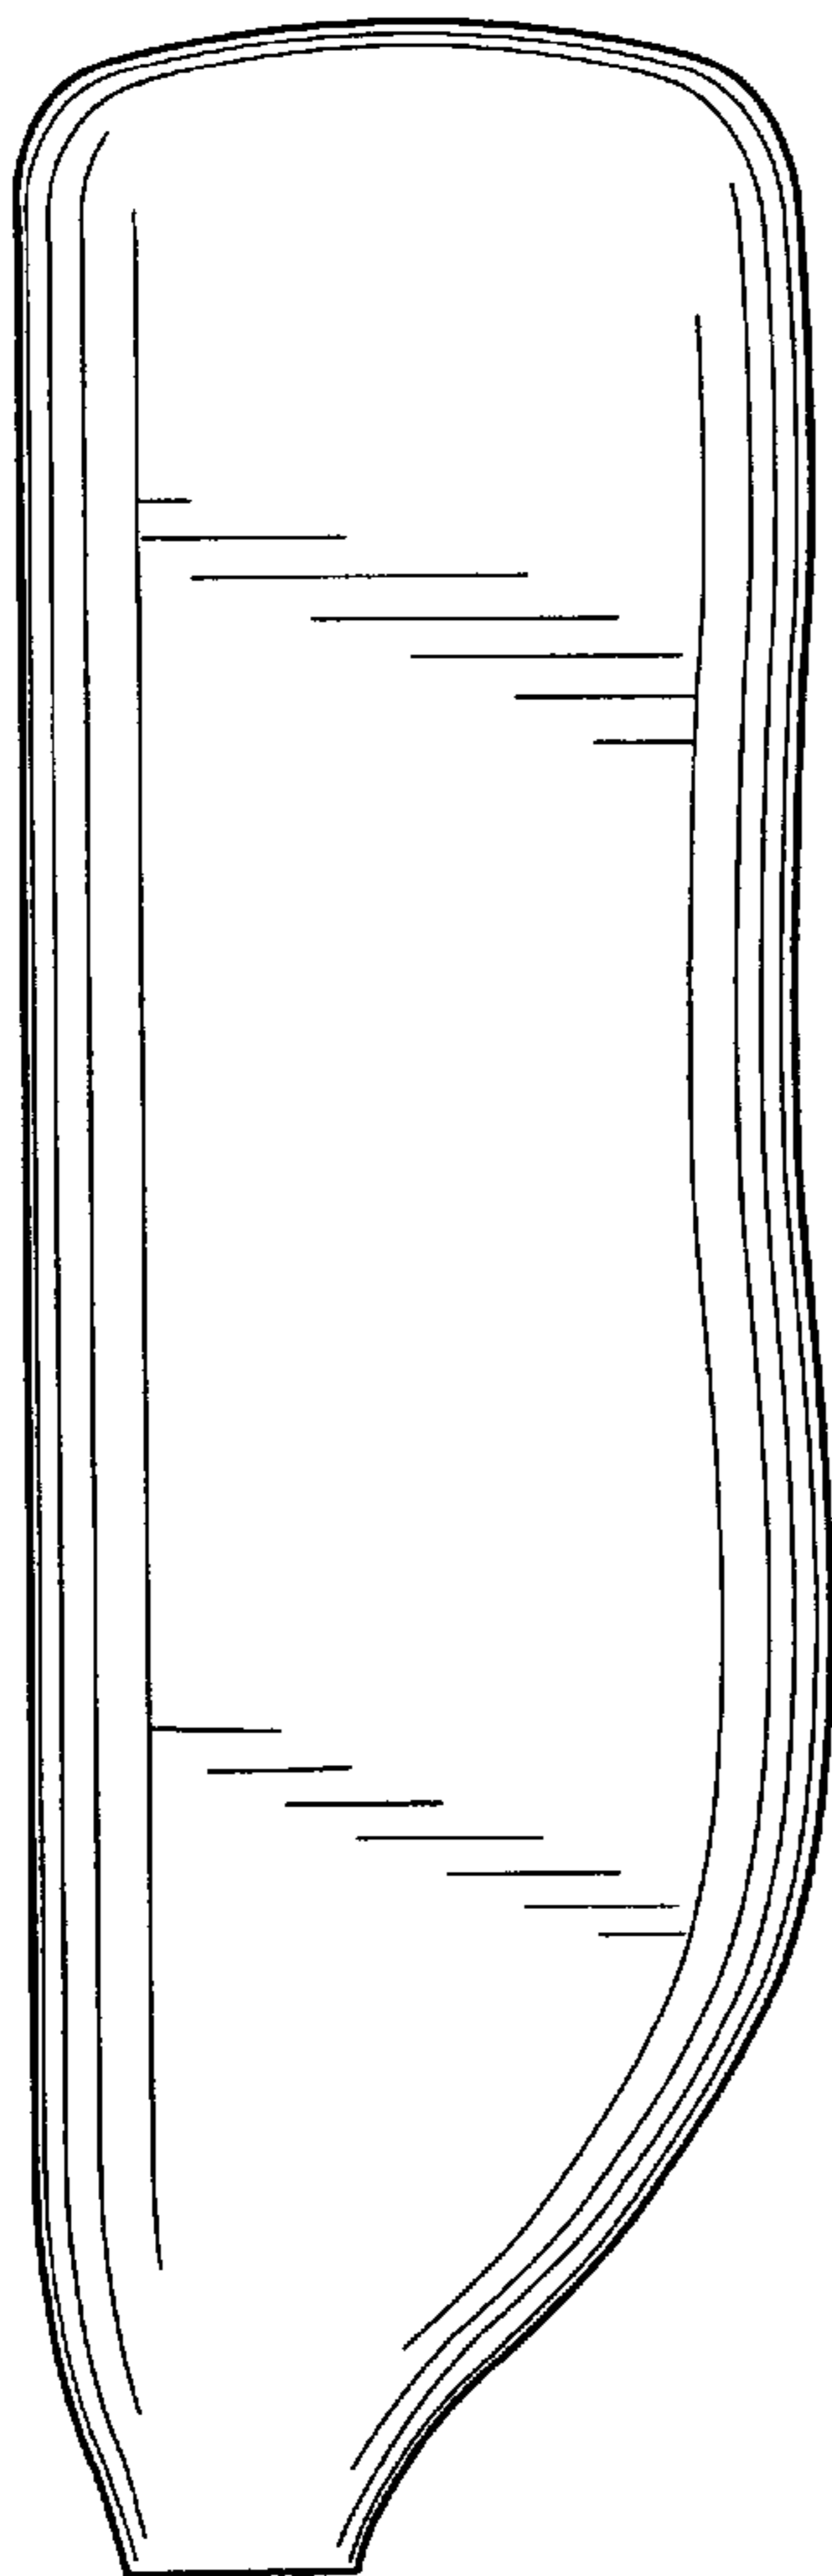


Fig. 2

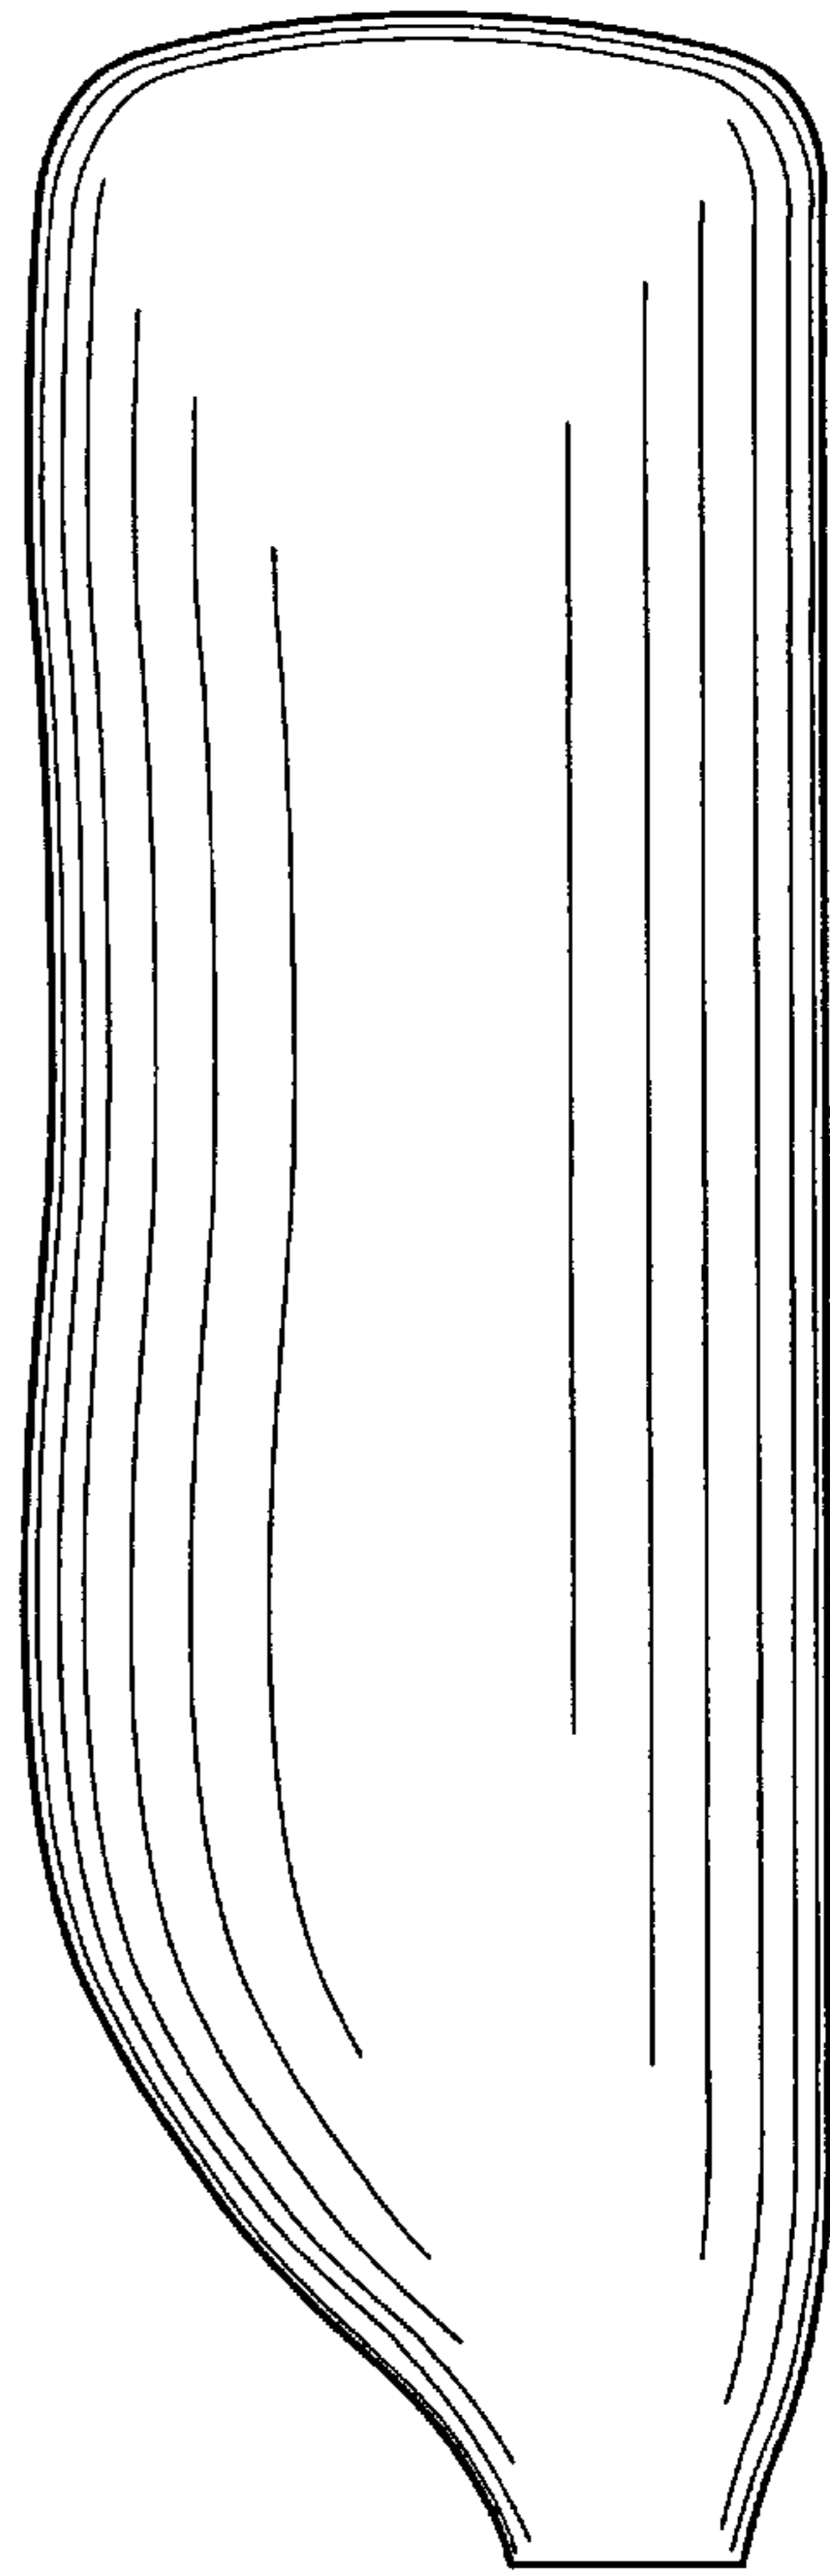


Fig. 3



Fig. 4



Fig. 5

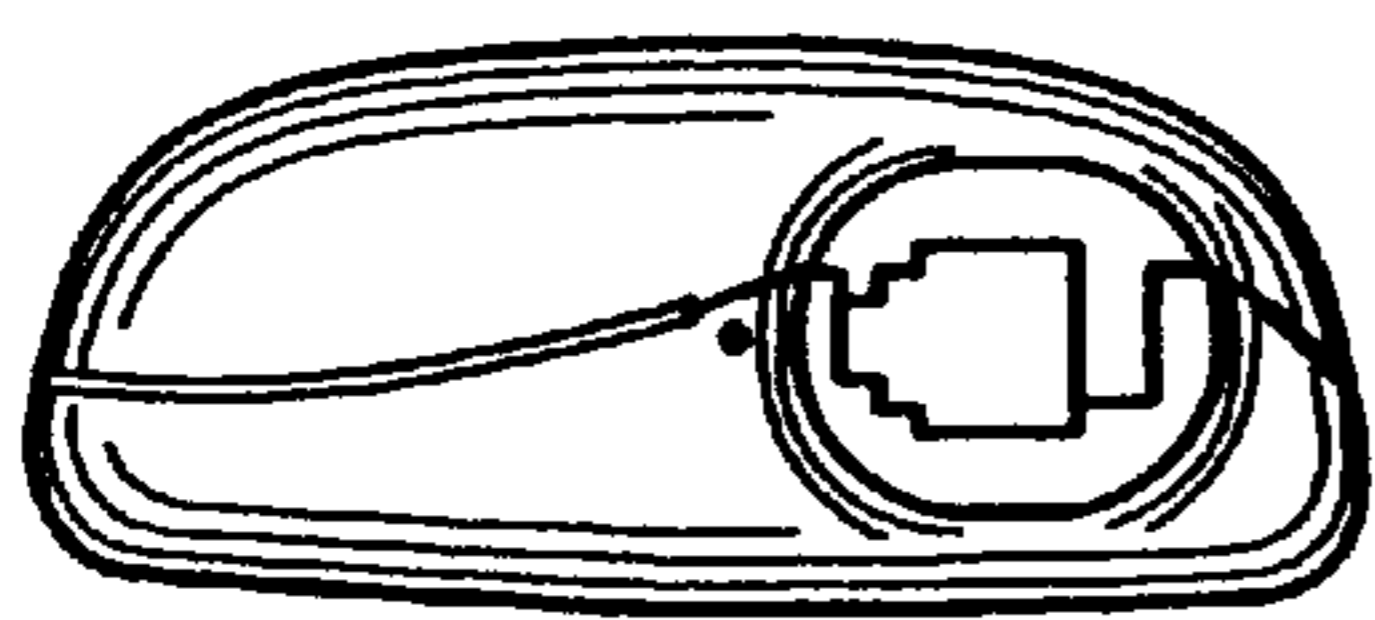


Fig. 6

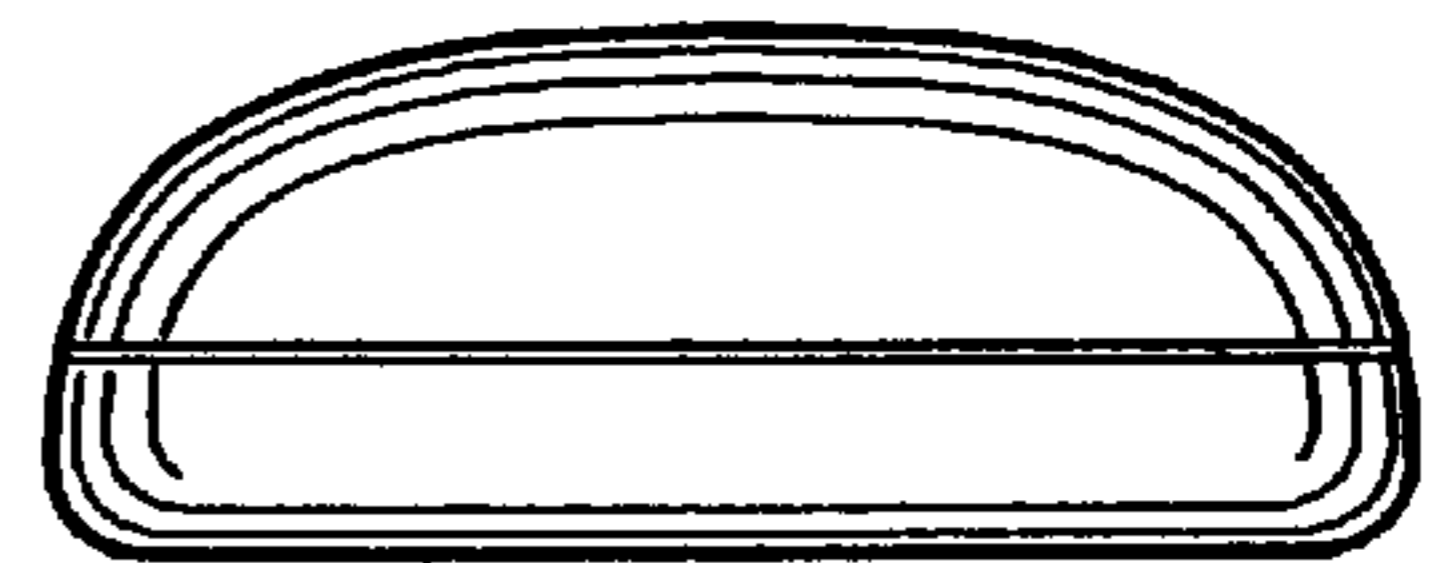


Fig. 7