



US00D479330S

(12) **United States Design Patent**  
**Nääs**

(10) **Patent No.:** **US D479,330 S**

(45) **Date of Patent:** **\*\* Sep. 2, 2003**

(54) **INTRA-OCULAR PRESSURE MEASUREMENT DEVICE**

(75) Inventor: **Marcus Nääs, Umeå (SE)**

(73) Assignee: **Bioresonator AB, Umeå (SE)**

(\*\*) Term: **14 Years**

(21) Appl. No.: **29/151,238**

(22) Filed: **Nov. 21, 2001**

(30) **Foreign Application Priority Data**

May 23, 2001 (SE) ..... 01-0929

(51) **LOC (7) Cl.** ..... **24-02**

(52) **U.S. Cl.** ..... **D24/150**

(58) **Field of Search** ..... D24/150, 172;  
D10/85; 600/398, 401, 405

(56) **References Cited**

**U.S. PATENT DOCUMENTS**

D298,856 S \* 12/1988 Feldon et al. .... D24/150  
5,174,292 A \* 12/1992 Kursar ..... 600/405

6,394,954 B1 \* 5/2002 Piletsky et al. .... 600/398

\* cited by examiner

*Primary Examiner*—Ian Simmons

(74) *Attorney, Agent, or Firm*—Renner, Otto, Boisselle & Sklar, LLP

(57) **CLAIM**

The ornamental design for a intra-ocular pressure measurement device, as shown and described.

**DESCRIPTION**

FIG. 1 is a upper left perspective view of the intra-ocular pressure measurement device showing my new design;


FIG. 2 is an upper right perspective view of the intra-ocular pressure measurement device;

FIG. 3 is a top view of the intra-ocular pressure measurement device; and

FIG. 4 is a front view of the intra-ocular pressure measurement device, the rear view being a mirror image thereof; and,

FIG. 5 is a bottom view of the intra-ocular pressure measurement device.

**1 Claim, 5 Drawing Sheets**

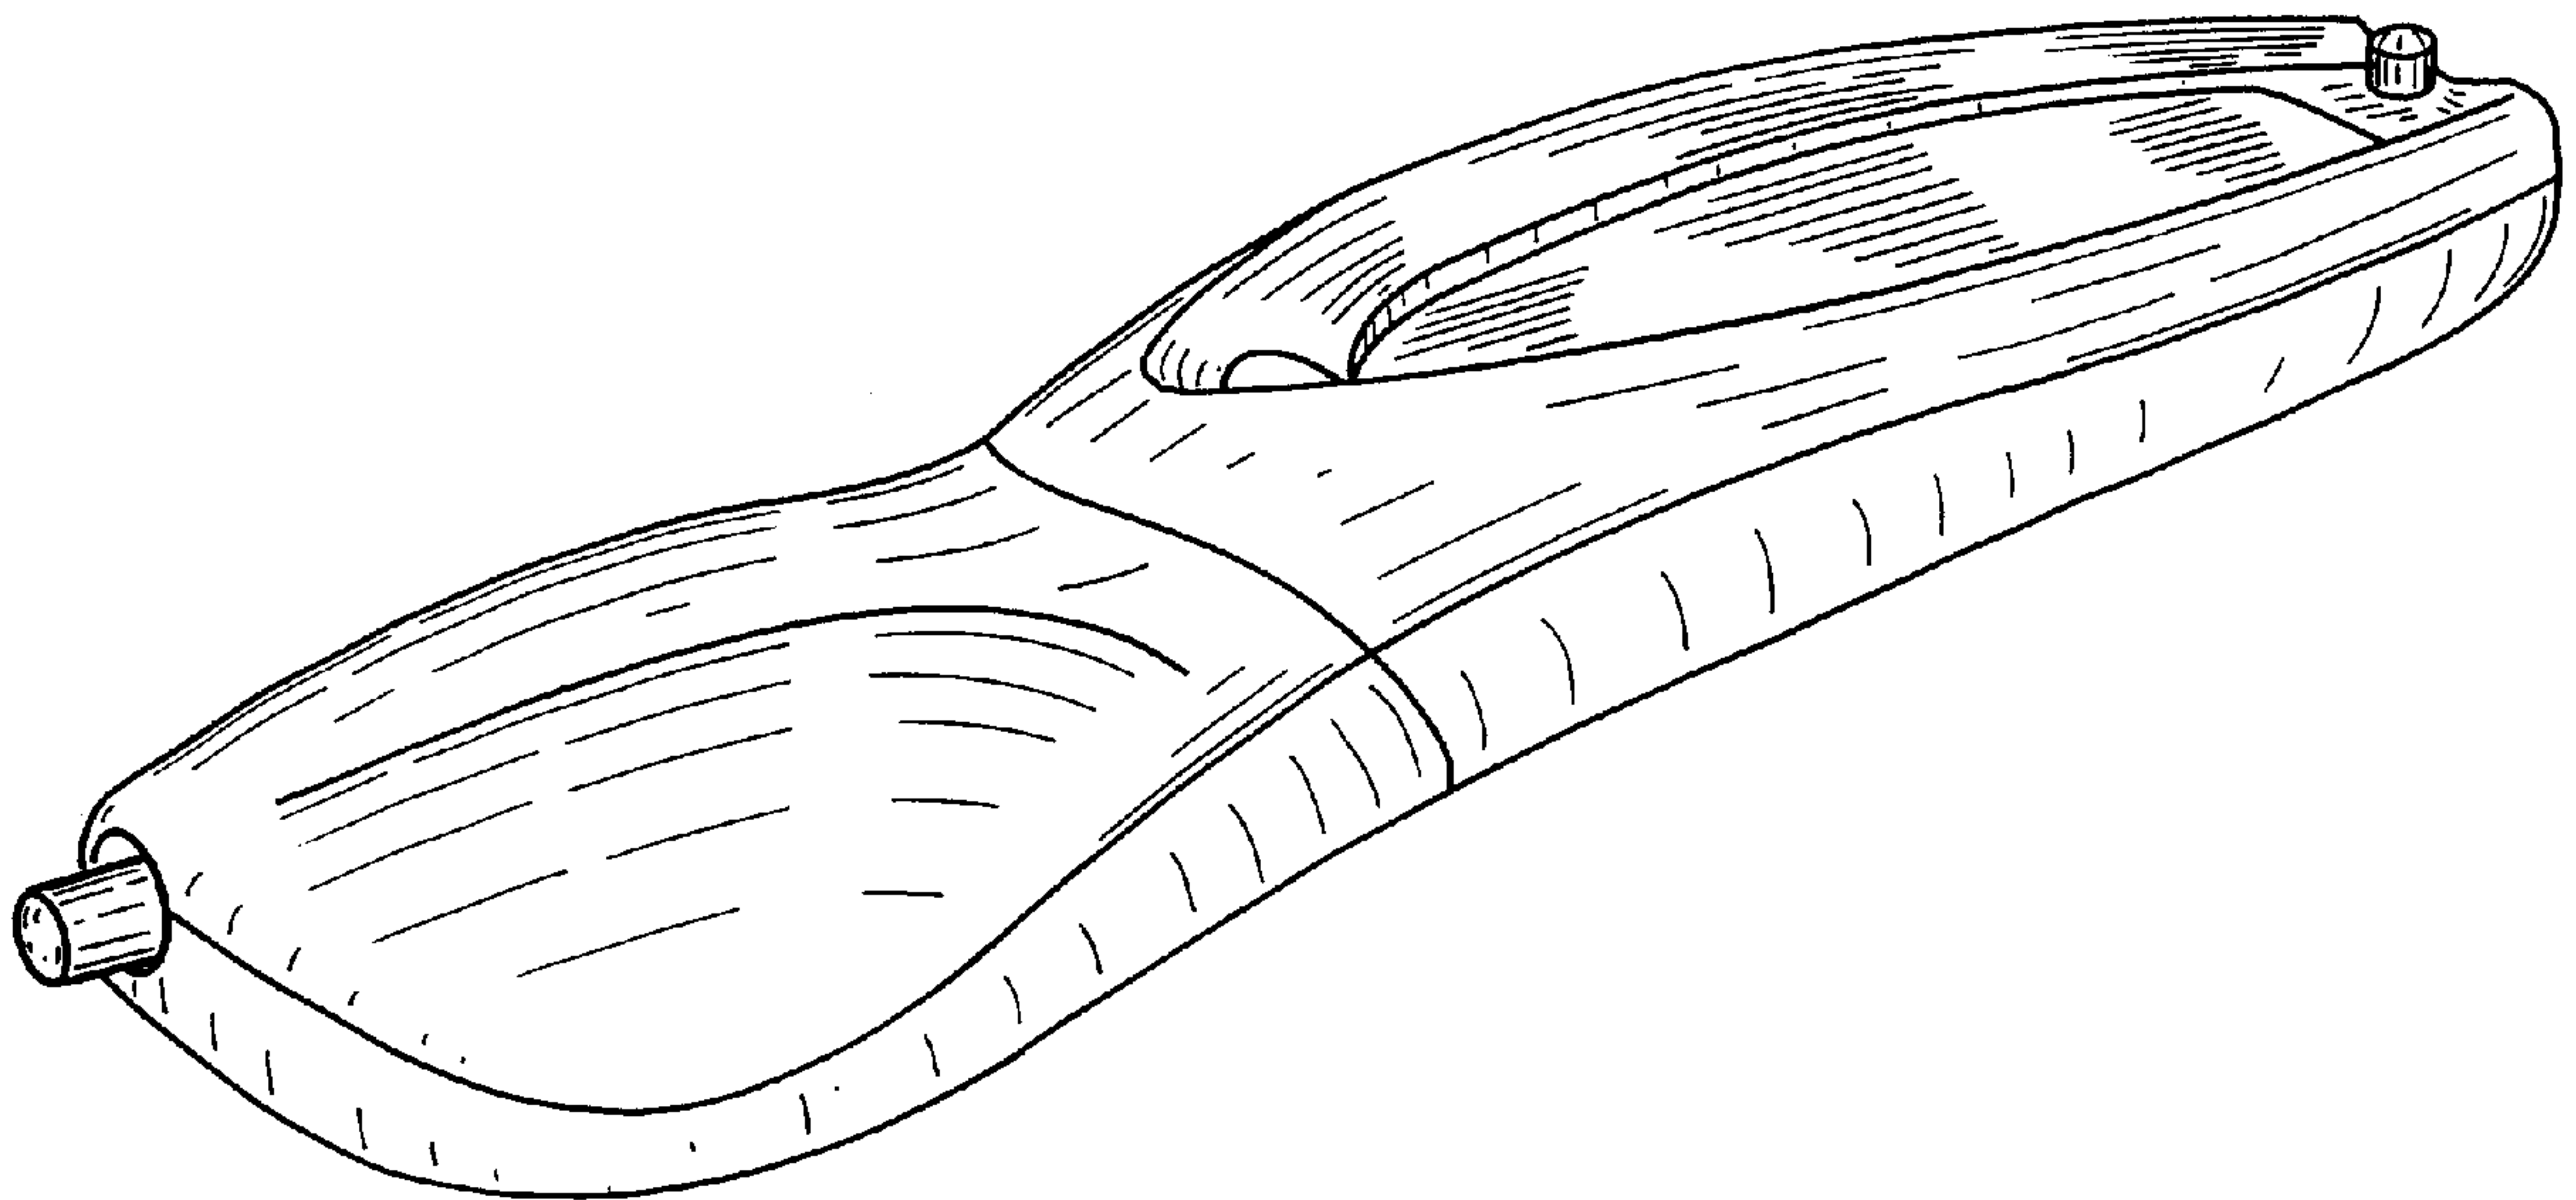

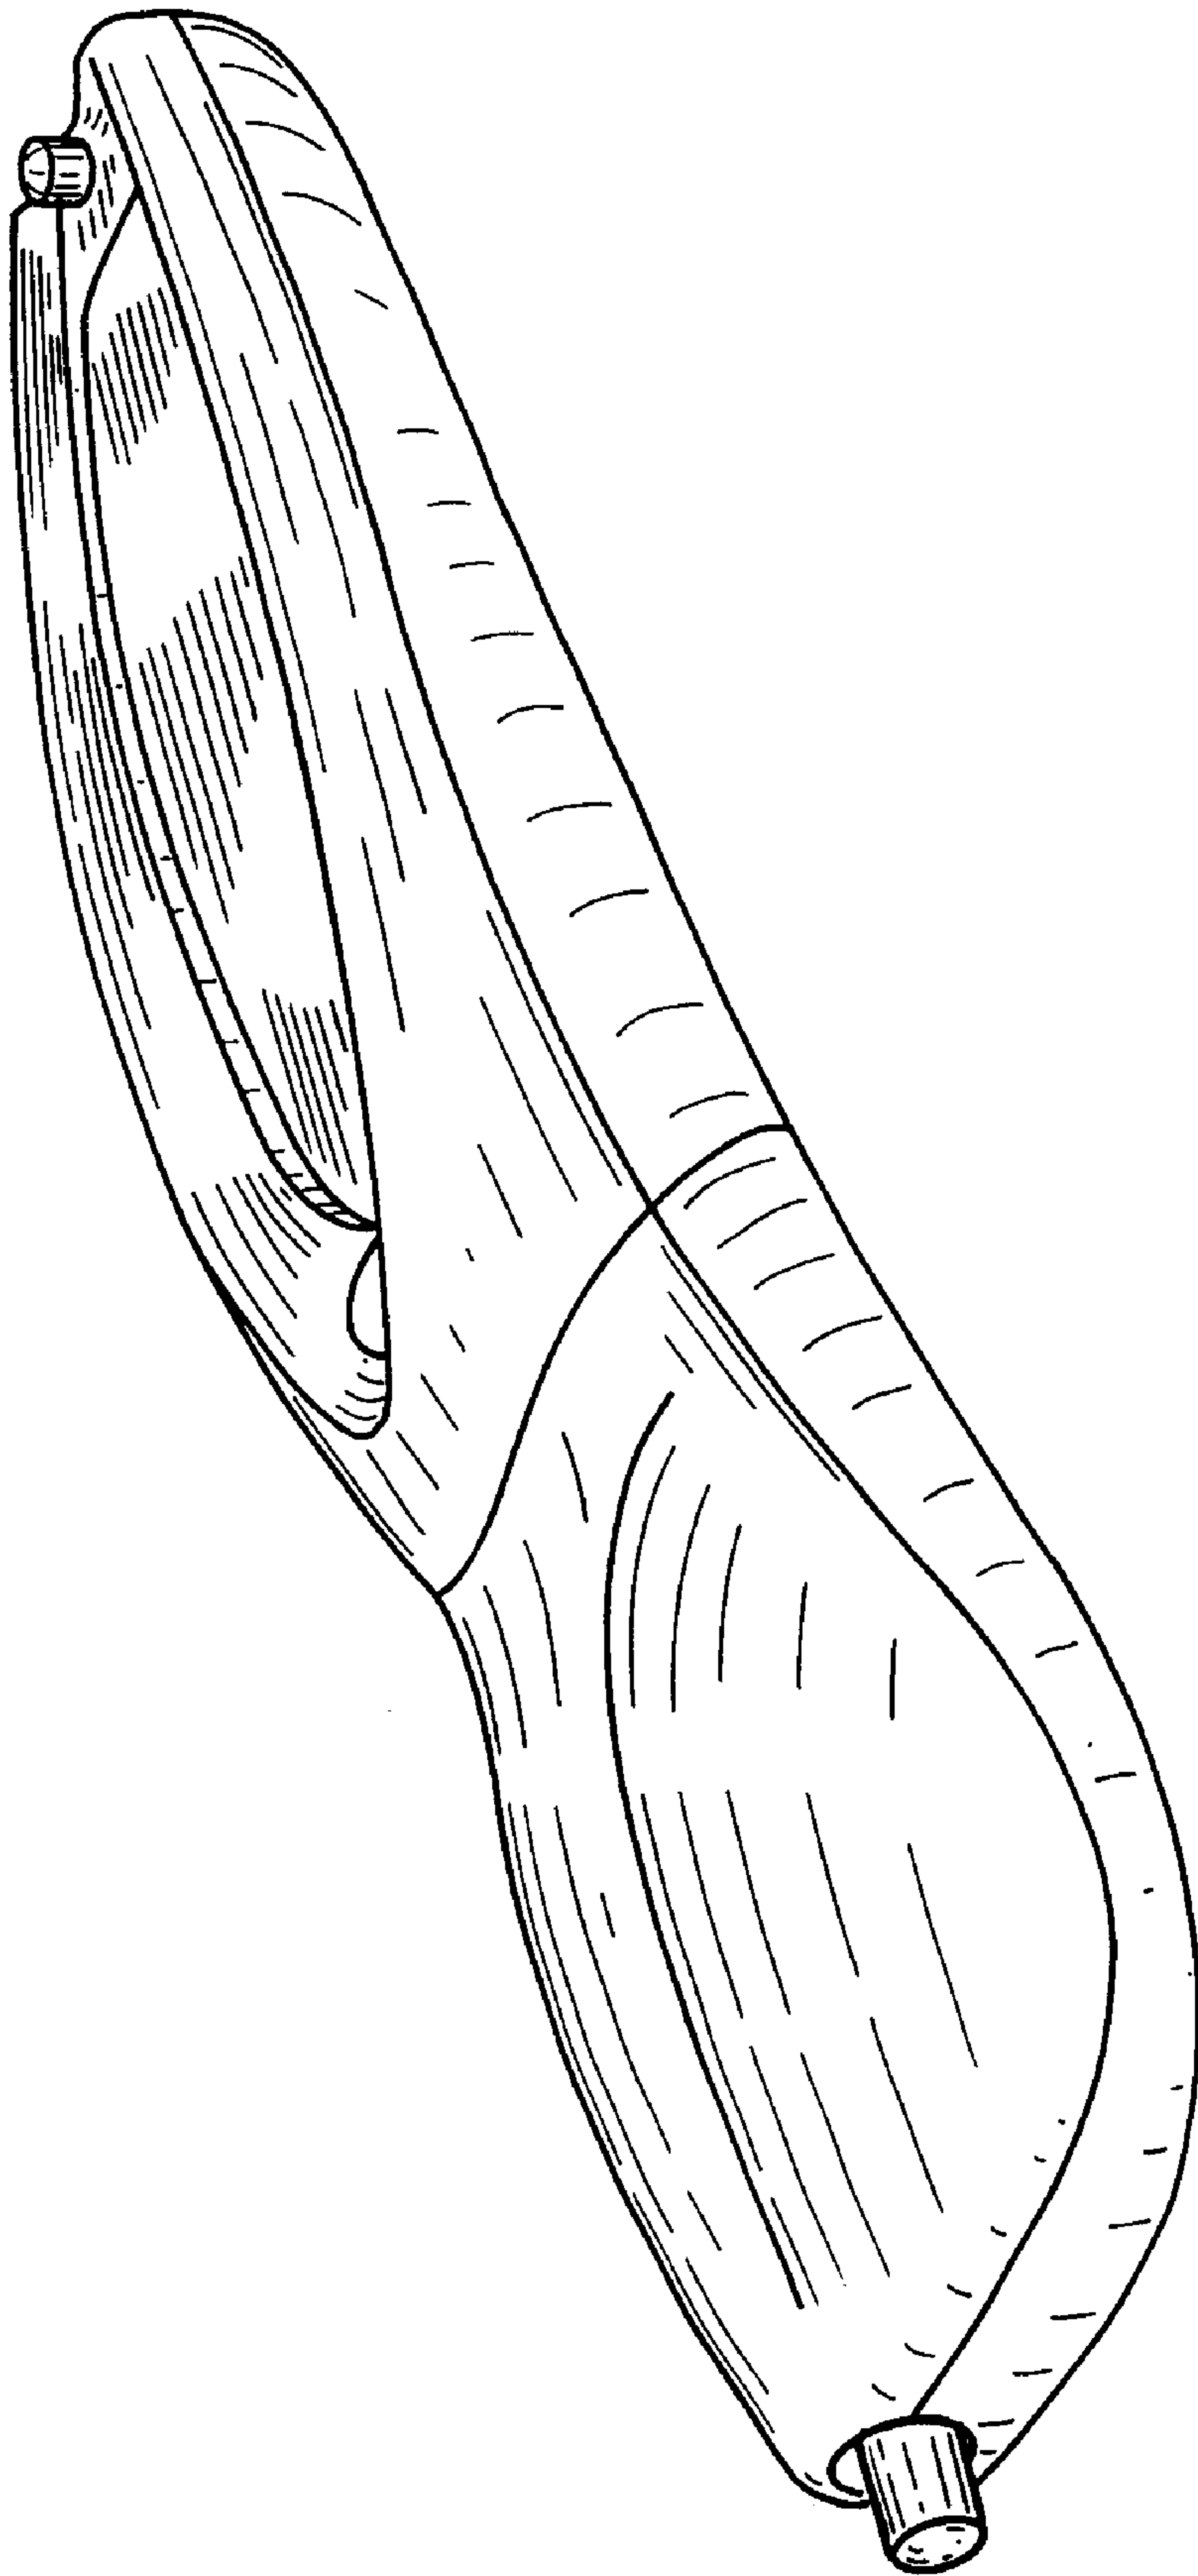


FIG. 1

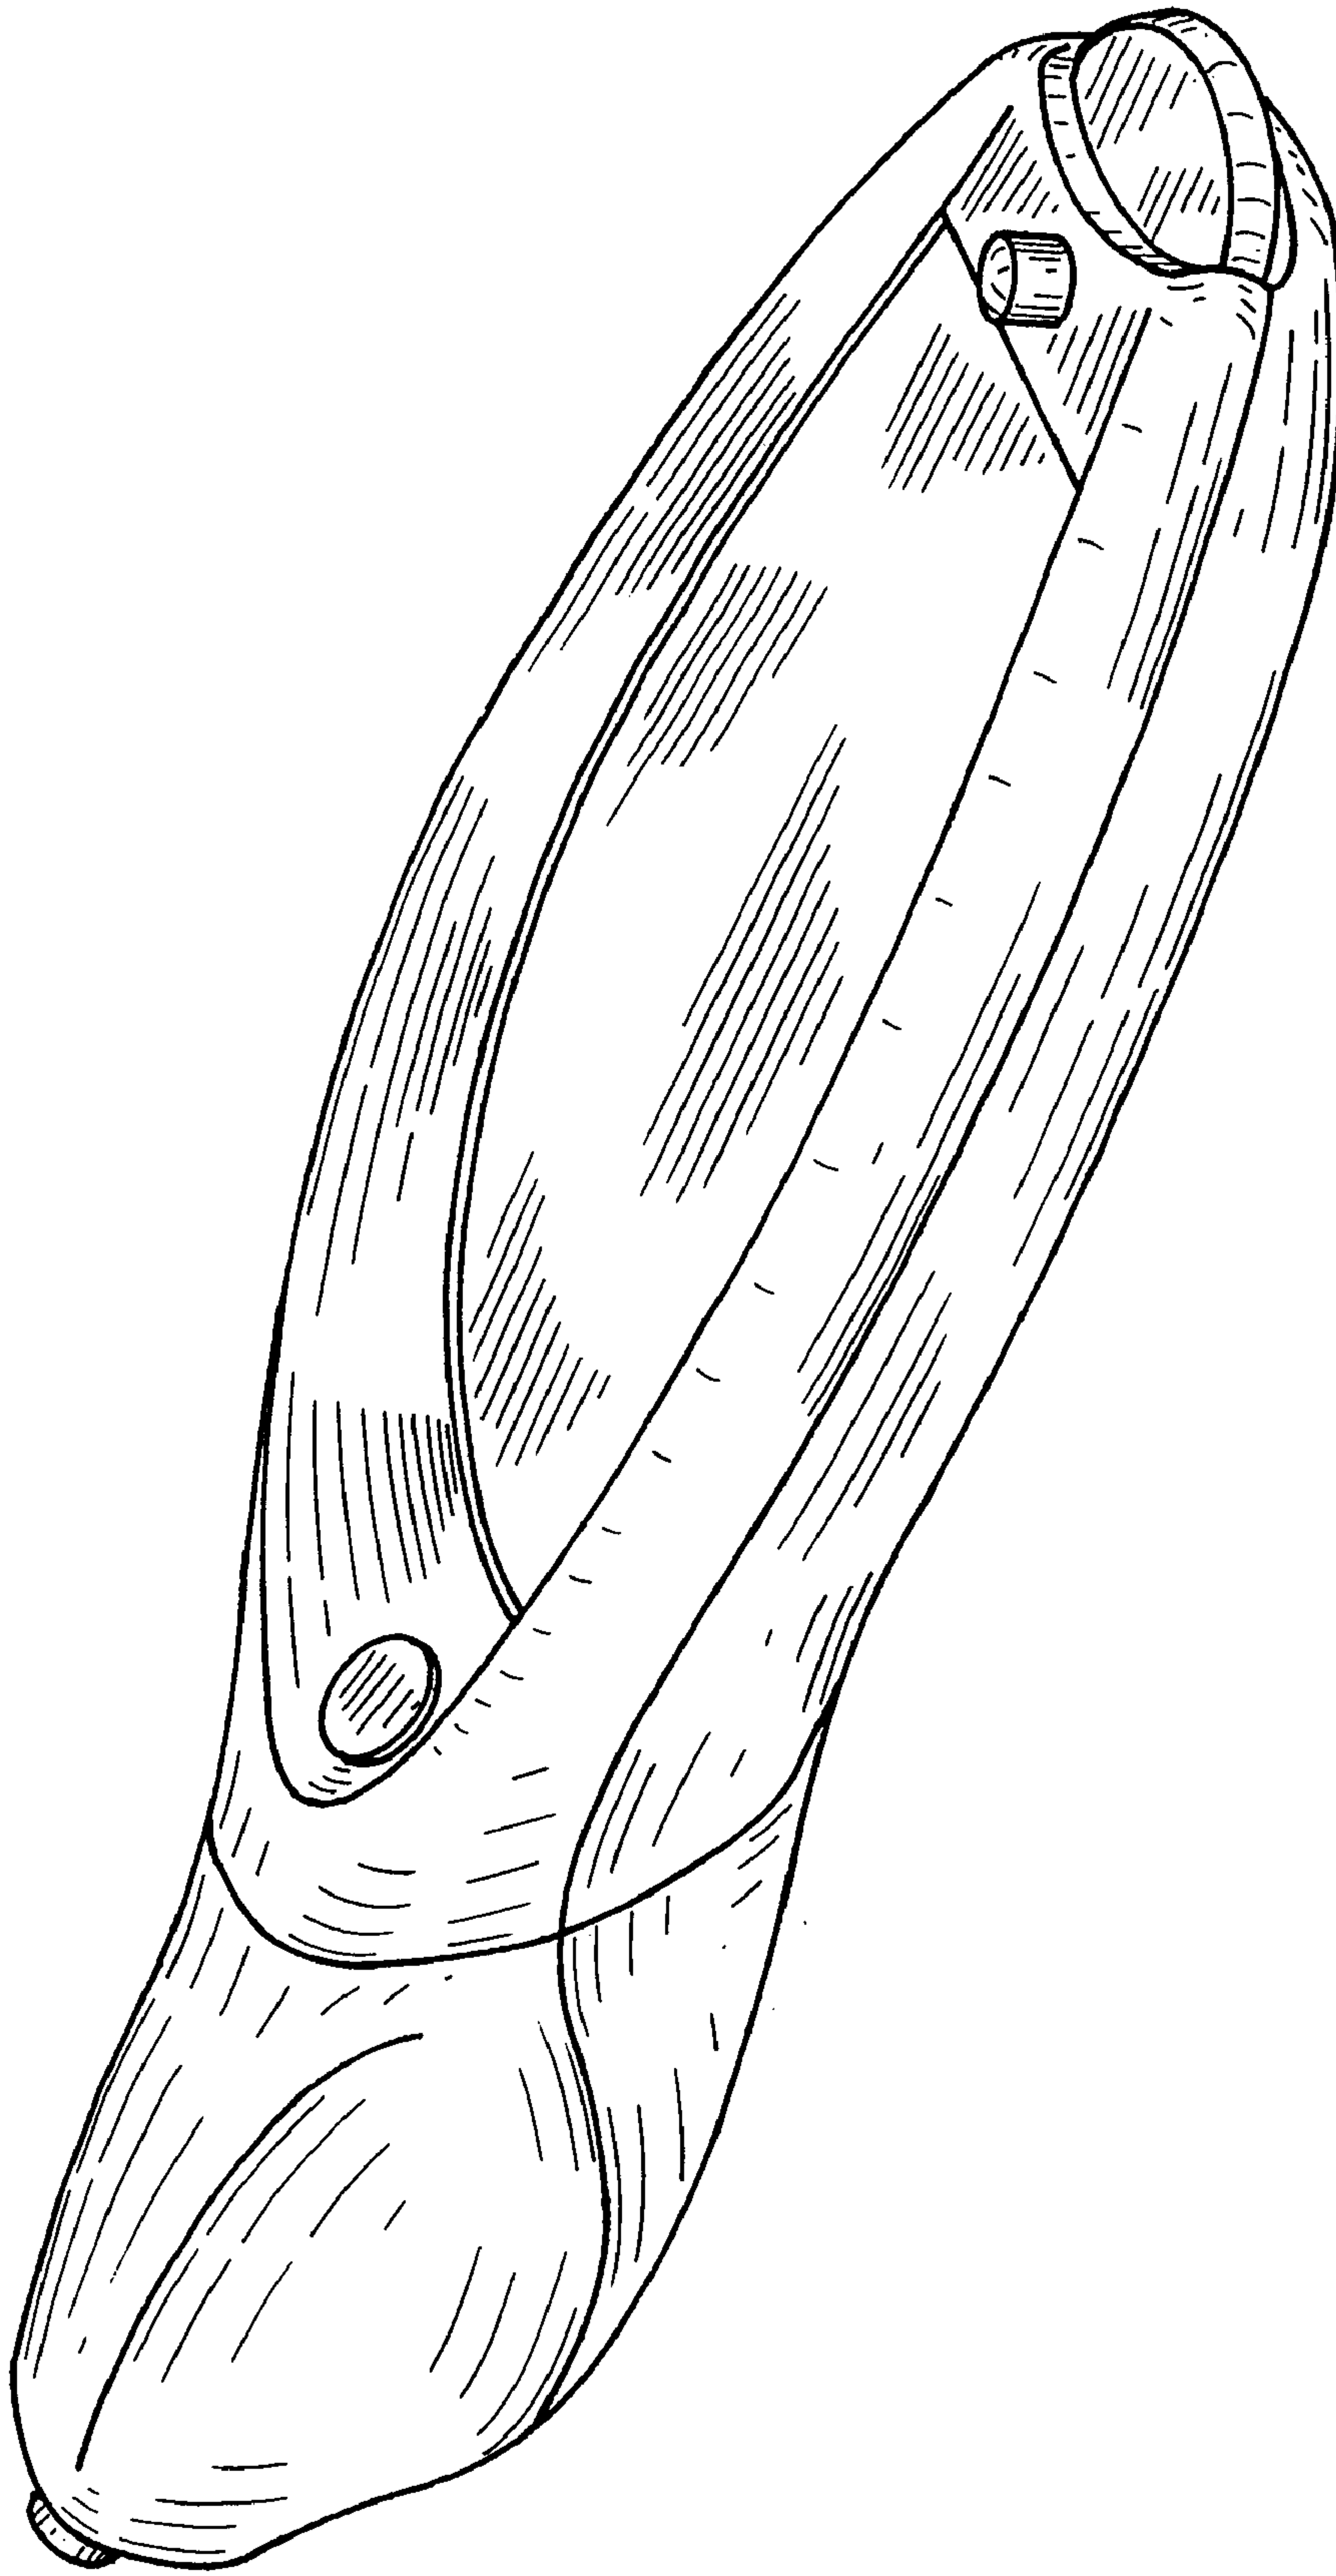


FIG. 2

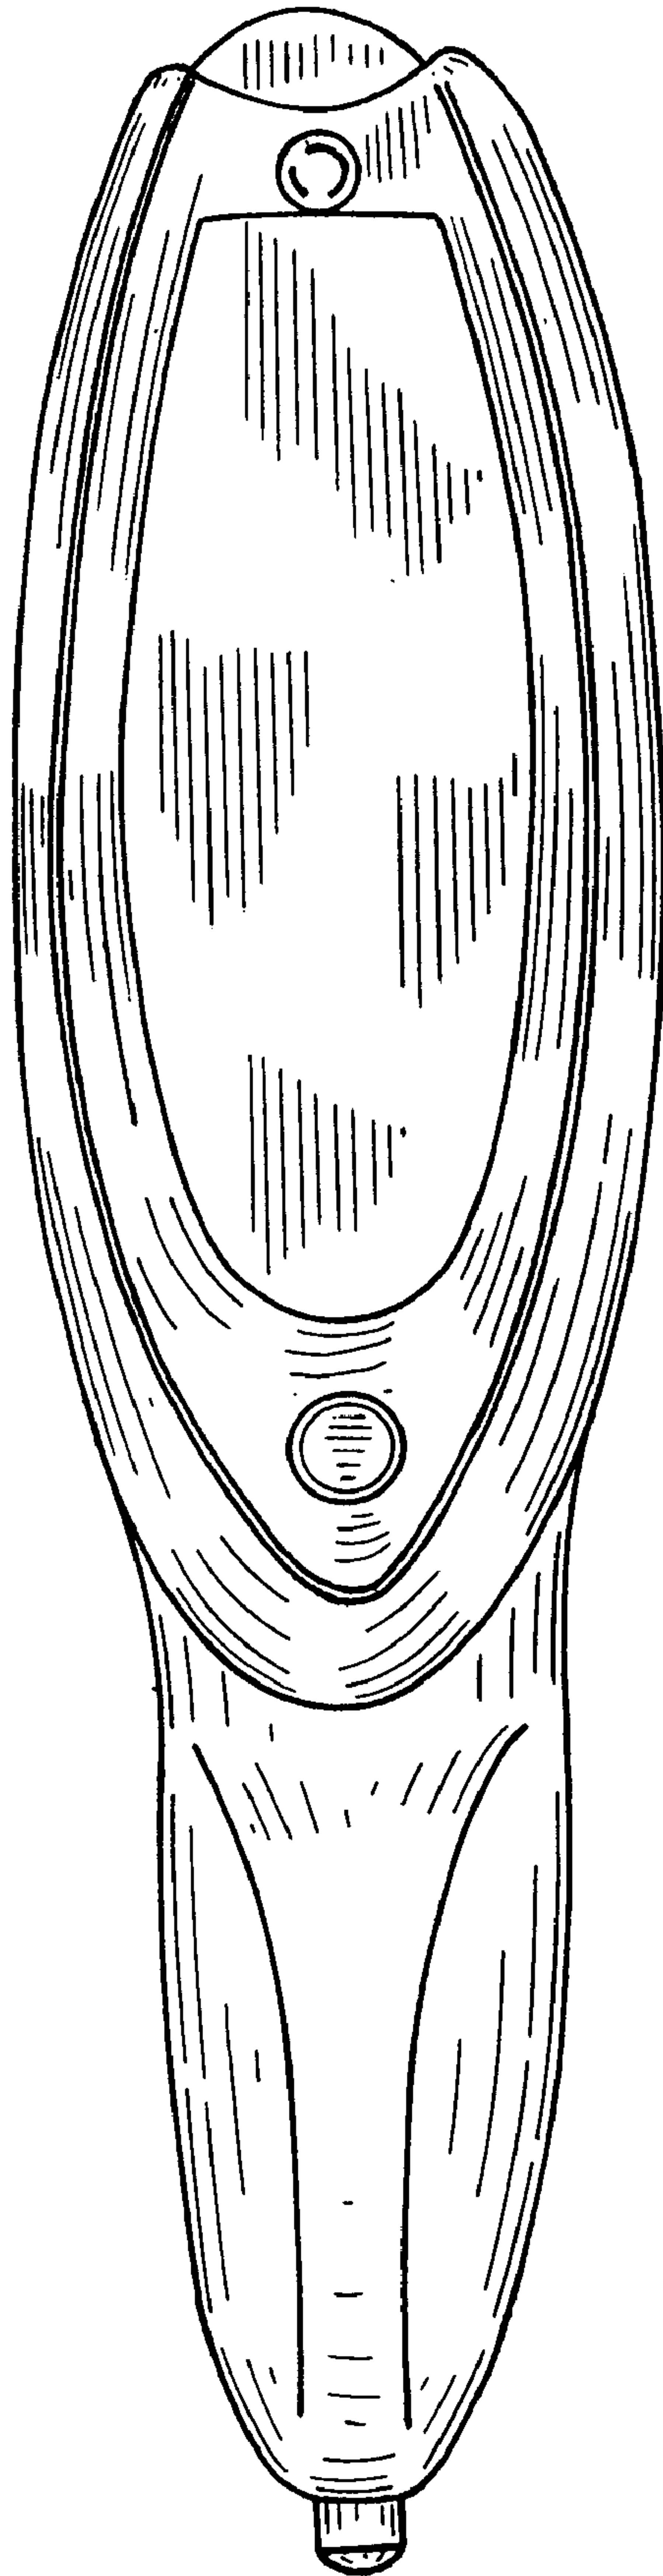


FIG. 3

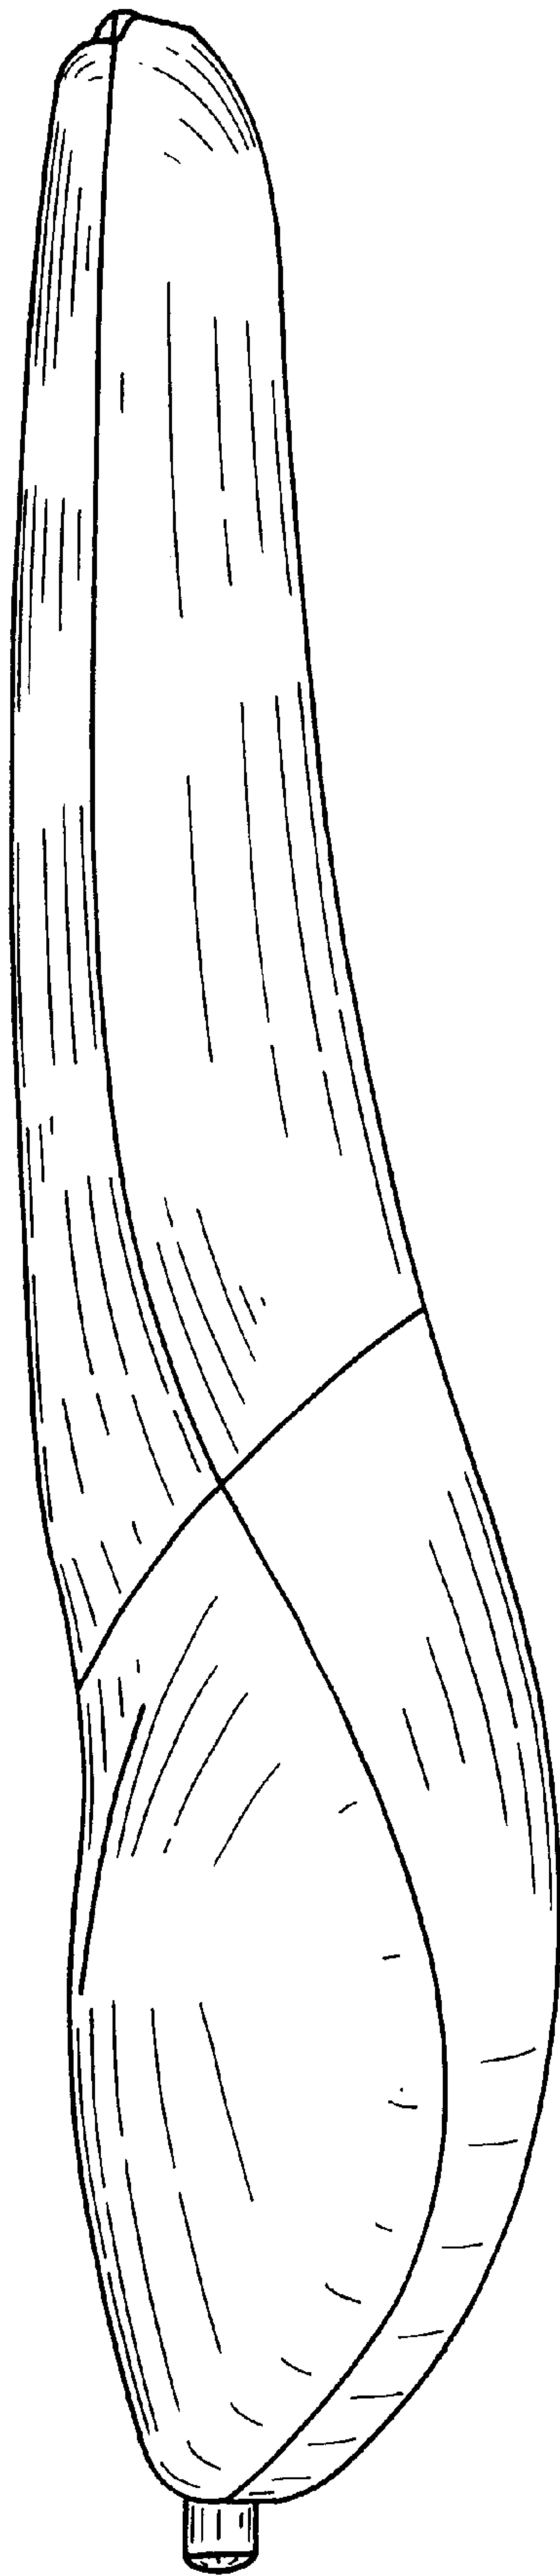


FIG. 4



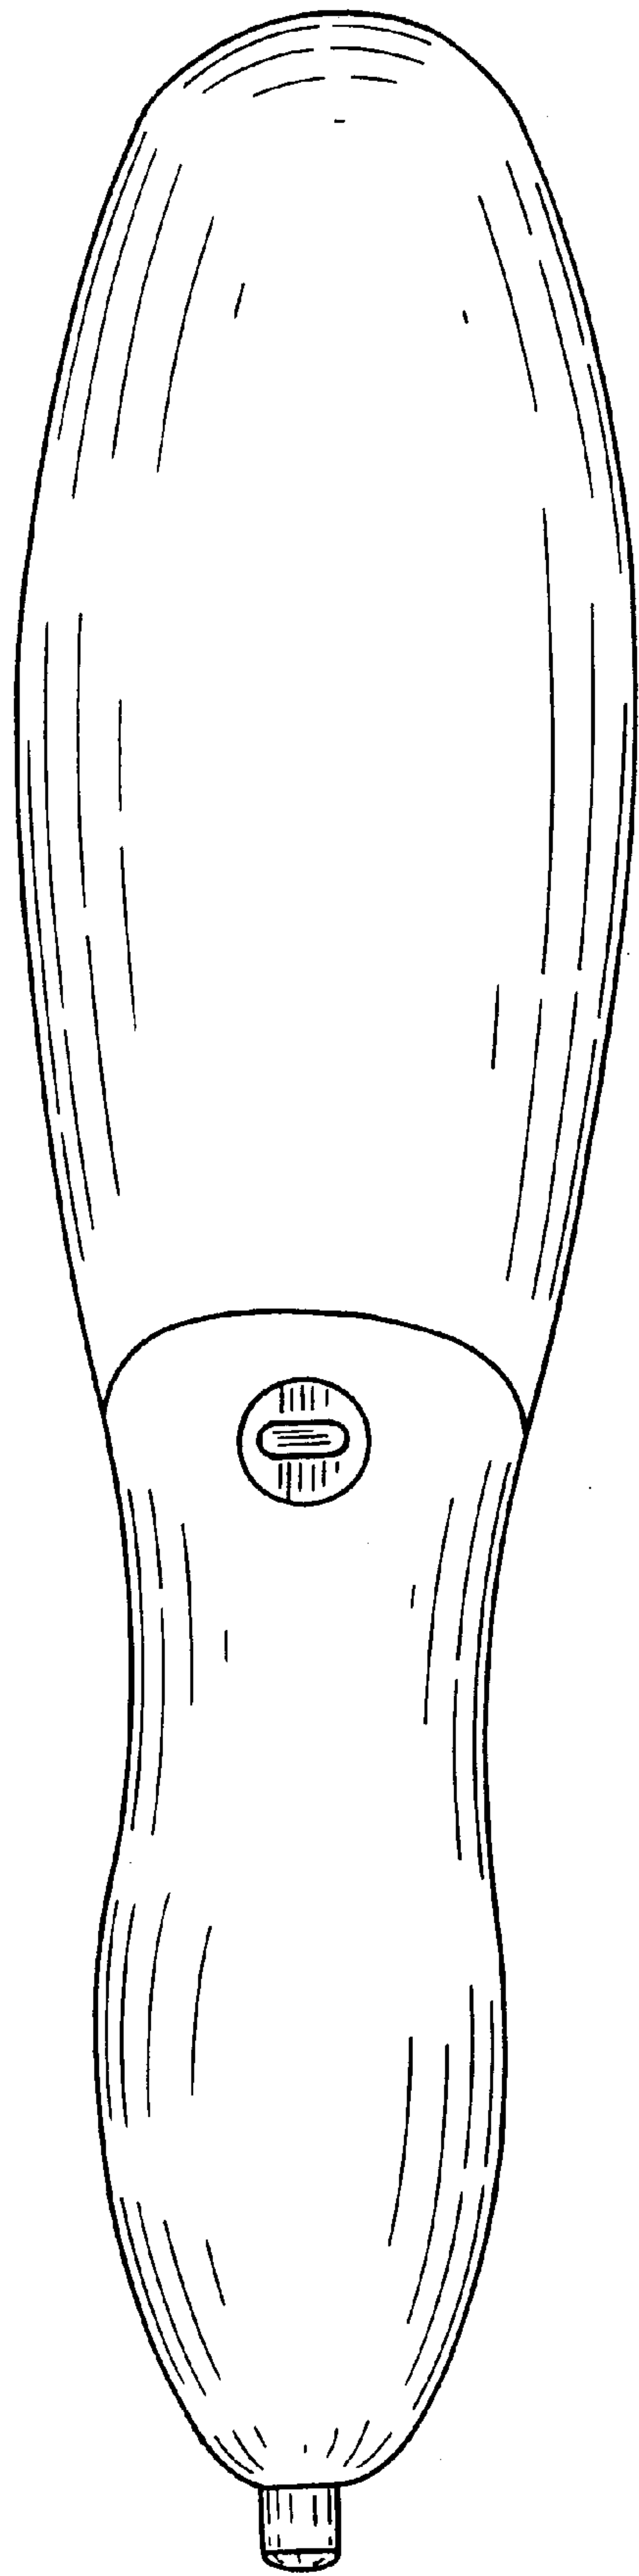


FIG. 5