



US00D479520S

(12) **United States Design Patent**  
**De Saulles**

(10) **Patent No.:** **US D479,520 S**

(45) **Date of Patent:** **\*\* Sep. 9, 2003**

(54) **AUDIOVISUAL CONTROL DEVICE**

(75) Inventor: **Stephen De Saulles**, London (GB)

(73) Assignee: **Patientline, plc**, Slough (GB)

(\*\*) Term: **14 Years**

(21) Appl. No.: **29/148,275**

(22) Filed: **Sep. 15, 2001**

(30) **Foreign Application Priority Data**

Mar. 16, 2001 (GB) ..... 2100364

(51) **LOC (7) Cl.** ..... **14-03**

(52) **U.S. Cl.** ..... **D14/218**

(58) **Field of Search** ..... D14/174, 217,  
D14/218, 137-139, 151, 191-193, 124,  
299, 167-168; D13/168, 162-164; D21/512-517,  
566; D10/104, 106; 455/352-355, 151.1-151.4;  
348/114, 734; D24/200

(56) **References Cited**

**U.S. PATENT DOCUMENTS**

D363,287 S	*	10/1995	Laituri	.....	D14/218
D371,794 S	*	7/1996	Kava et al.	.....	D14/218
D383,462 S	*	9/1997	Martz et al.	.....	D14/218
D417,875 S	*	12/1999	Choi	.....	D14/218
D437,310 S	*	2/2001	Gioscia	.....	D14/218
D467,005 S	*	12/2002	Gerth et al.	.....	D24/200
D469,184 S	*	1/2003	Gerth et al.	.....	D24/200

**OTHER PUBLICATIONS**

Product literature for Ackerman. Date Unknown. Seven (7) sheets. [www.ackerman.com/clino/index.html](http://www.ackerman.com/clino/index.html).

Product literature for BedWeb. Date Unknown. Four (4) sheet.

Product literature for Ascom Nira. Date Unknown. One (1) sheet.

Product literature for Tyco. Date Unknown. One (1) sheet.

Product literature for Siemens. Date Unknown. One (1) sheet.

Product literature for HCIC+. Date Unknown. Three (3) sheets. [www.hcic.com/products/television/index.htm](http://www.hcic.com/products/television/index.htm).

Product literature for Kerfone. Date Unknown. Three (3) sheets. [www.kerfone.co.uk/kerfone.htm](http://www.kerfone.co.uk/kerfone.htm).

Product literature for Schmelter. Date Unknown. Three (3) sheets. [www.aym-schmelter.de/lcd.htm](http://www.aym-schmelter.de/lcd.htm).

Photo of Zettler product. Date Unknown. One (1) sheet.

Product literature for Teleware. Date Unknown. One (1) sheet.

Photo of HTS product. Date Unknown. One (1) sheet.

Product literature for Wandsworth. Date Unknown. One (1) sheet. [www.wandsworth-electrical.com/page99.htm](http://www.wandsworth-electrical.com/page99.htm).

Product literature for Static Systems Group. Date Unknown. One (1) sheet. [www.staticsystems.co.uk](http://www.staticsystems.co.uk).

Brochure for BedWeb Integrated Patient System from Bedweb by Netherlands. Date believed to be not later than Sep. 2000. Four (4) sheets.

Product information sheet for Ascom Nira Telegration System from Ascom Holding Ltd. Switzerland. Date believed to be not later than Sep. 2000. One (1) sheet.

(List continued on next page.)

*Primary Examiner*—Louis S. Zarfaz

*Assistant Examiner*—Deanne Levy

(74) *Attorney, Agent, or Firm*—Clayton, Howarth & Cannon, P.C.

(57) **CLAIM**


I claim the ornamental design for an audiovisual control device, as shown and described.

**DESCRIPTION**

FIG. 1 is a perspective view thereof; and, FIG. 2 is a top view thereof.

The broken line showing of the hand held device is for illustrative purposes only and forms no part of the claimed design.

**1 Claim, 1 Drawing Sheet**

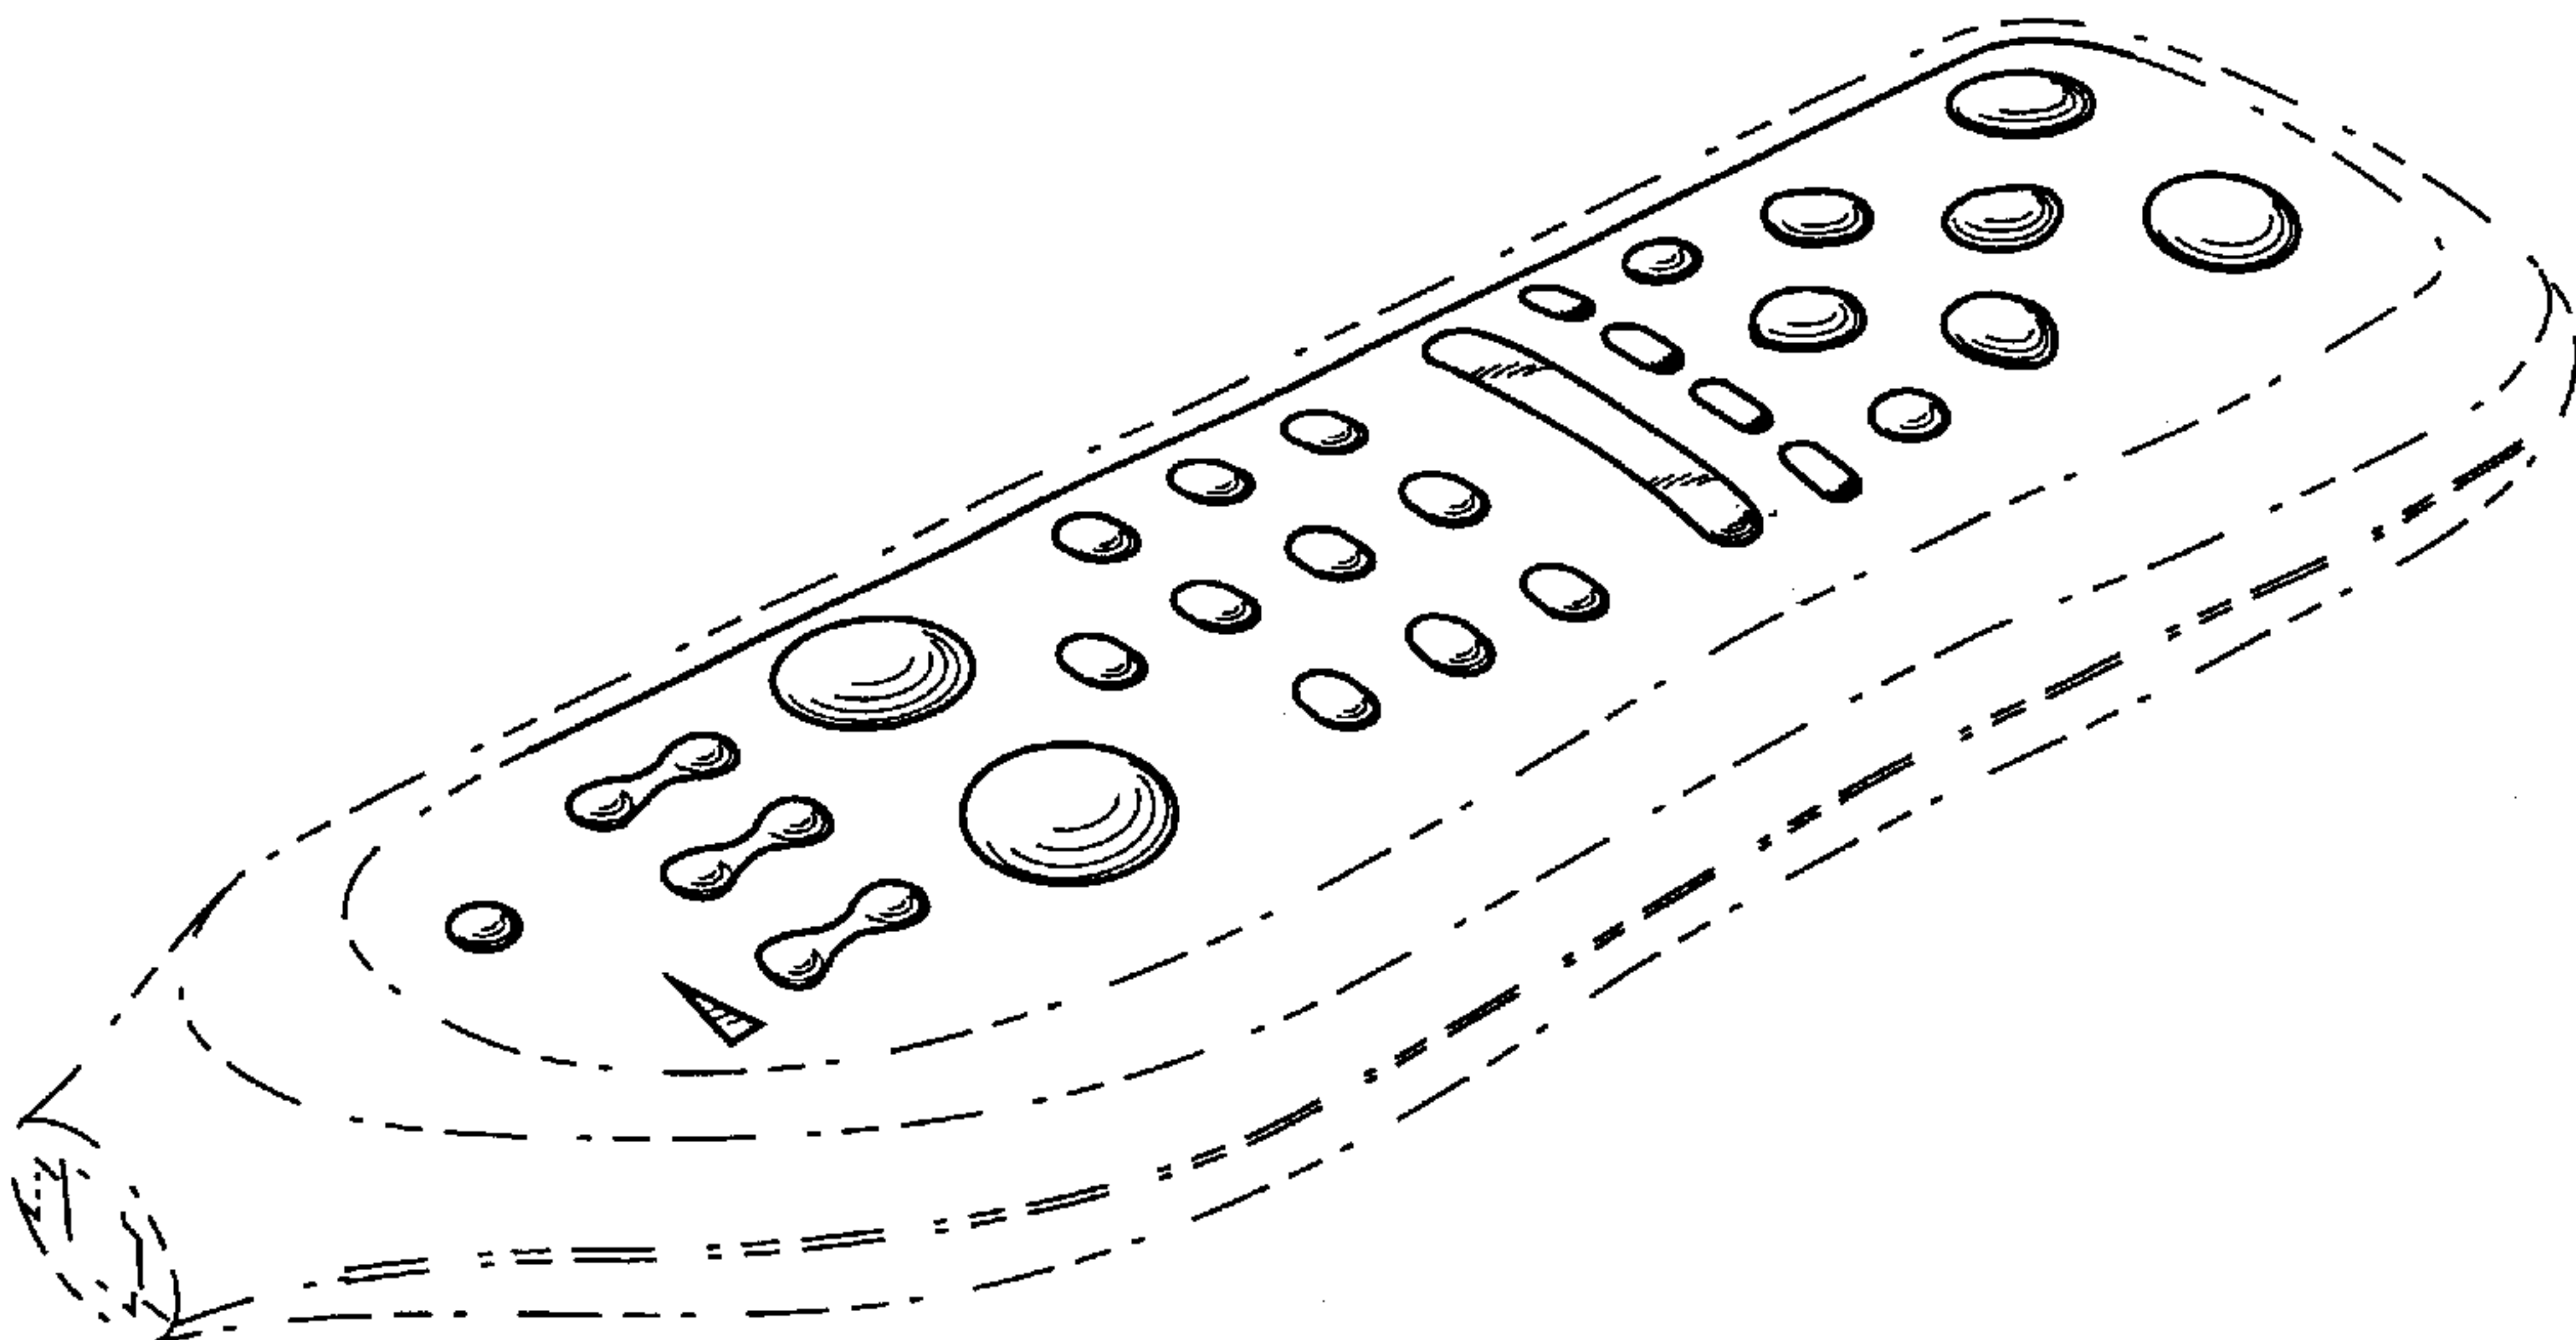

OTHER PUBLICATIONS

Product information sheet for Tyco system by Phillips. Date believed to be not later than Sep. 2000. One (1) sheet.

Partial product information sheet for Siemens AG television/radio/phone system. Date believed to be not later than Sep. 2000. One (1) sheet.

Photo of Zettler patient phone/television product from Zettler Electronics GMBH. Date believed to be not later than Sep. 2000. One (1) sheet.


Advertisement for Teleware bedside telephone and television from Teleware Systems Limited. Date believed to be not later than Sep. 2000. One (1) sheet.

Photo of HTS phone/television product from Health Television System, Inc. Date believed to be not later than Sep. 2000. One (1) sheet.


Website prints and product photos for the Patientline system from Patientline plc. Not later than Sep., 2000. Eleven (11) sheets).

Product literature for the Patientline system (website prints and product photos). Not later than Sep., 2000. Eleven (11) Sheets.

\* cited by examiner

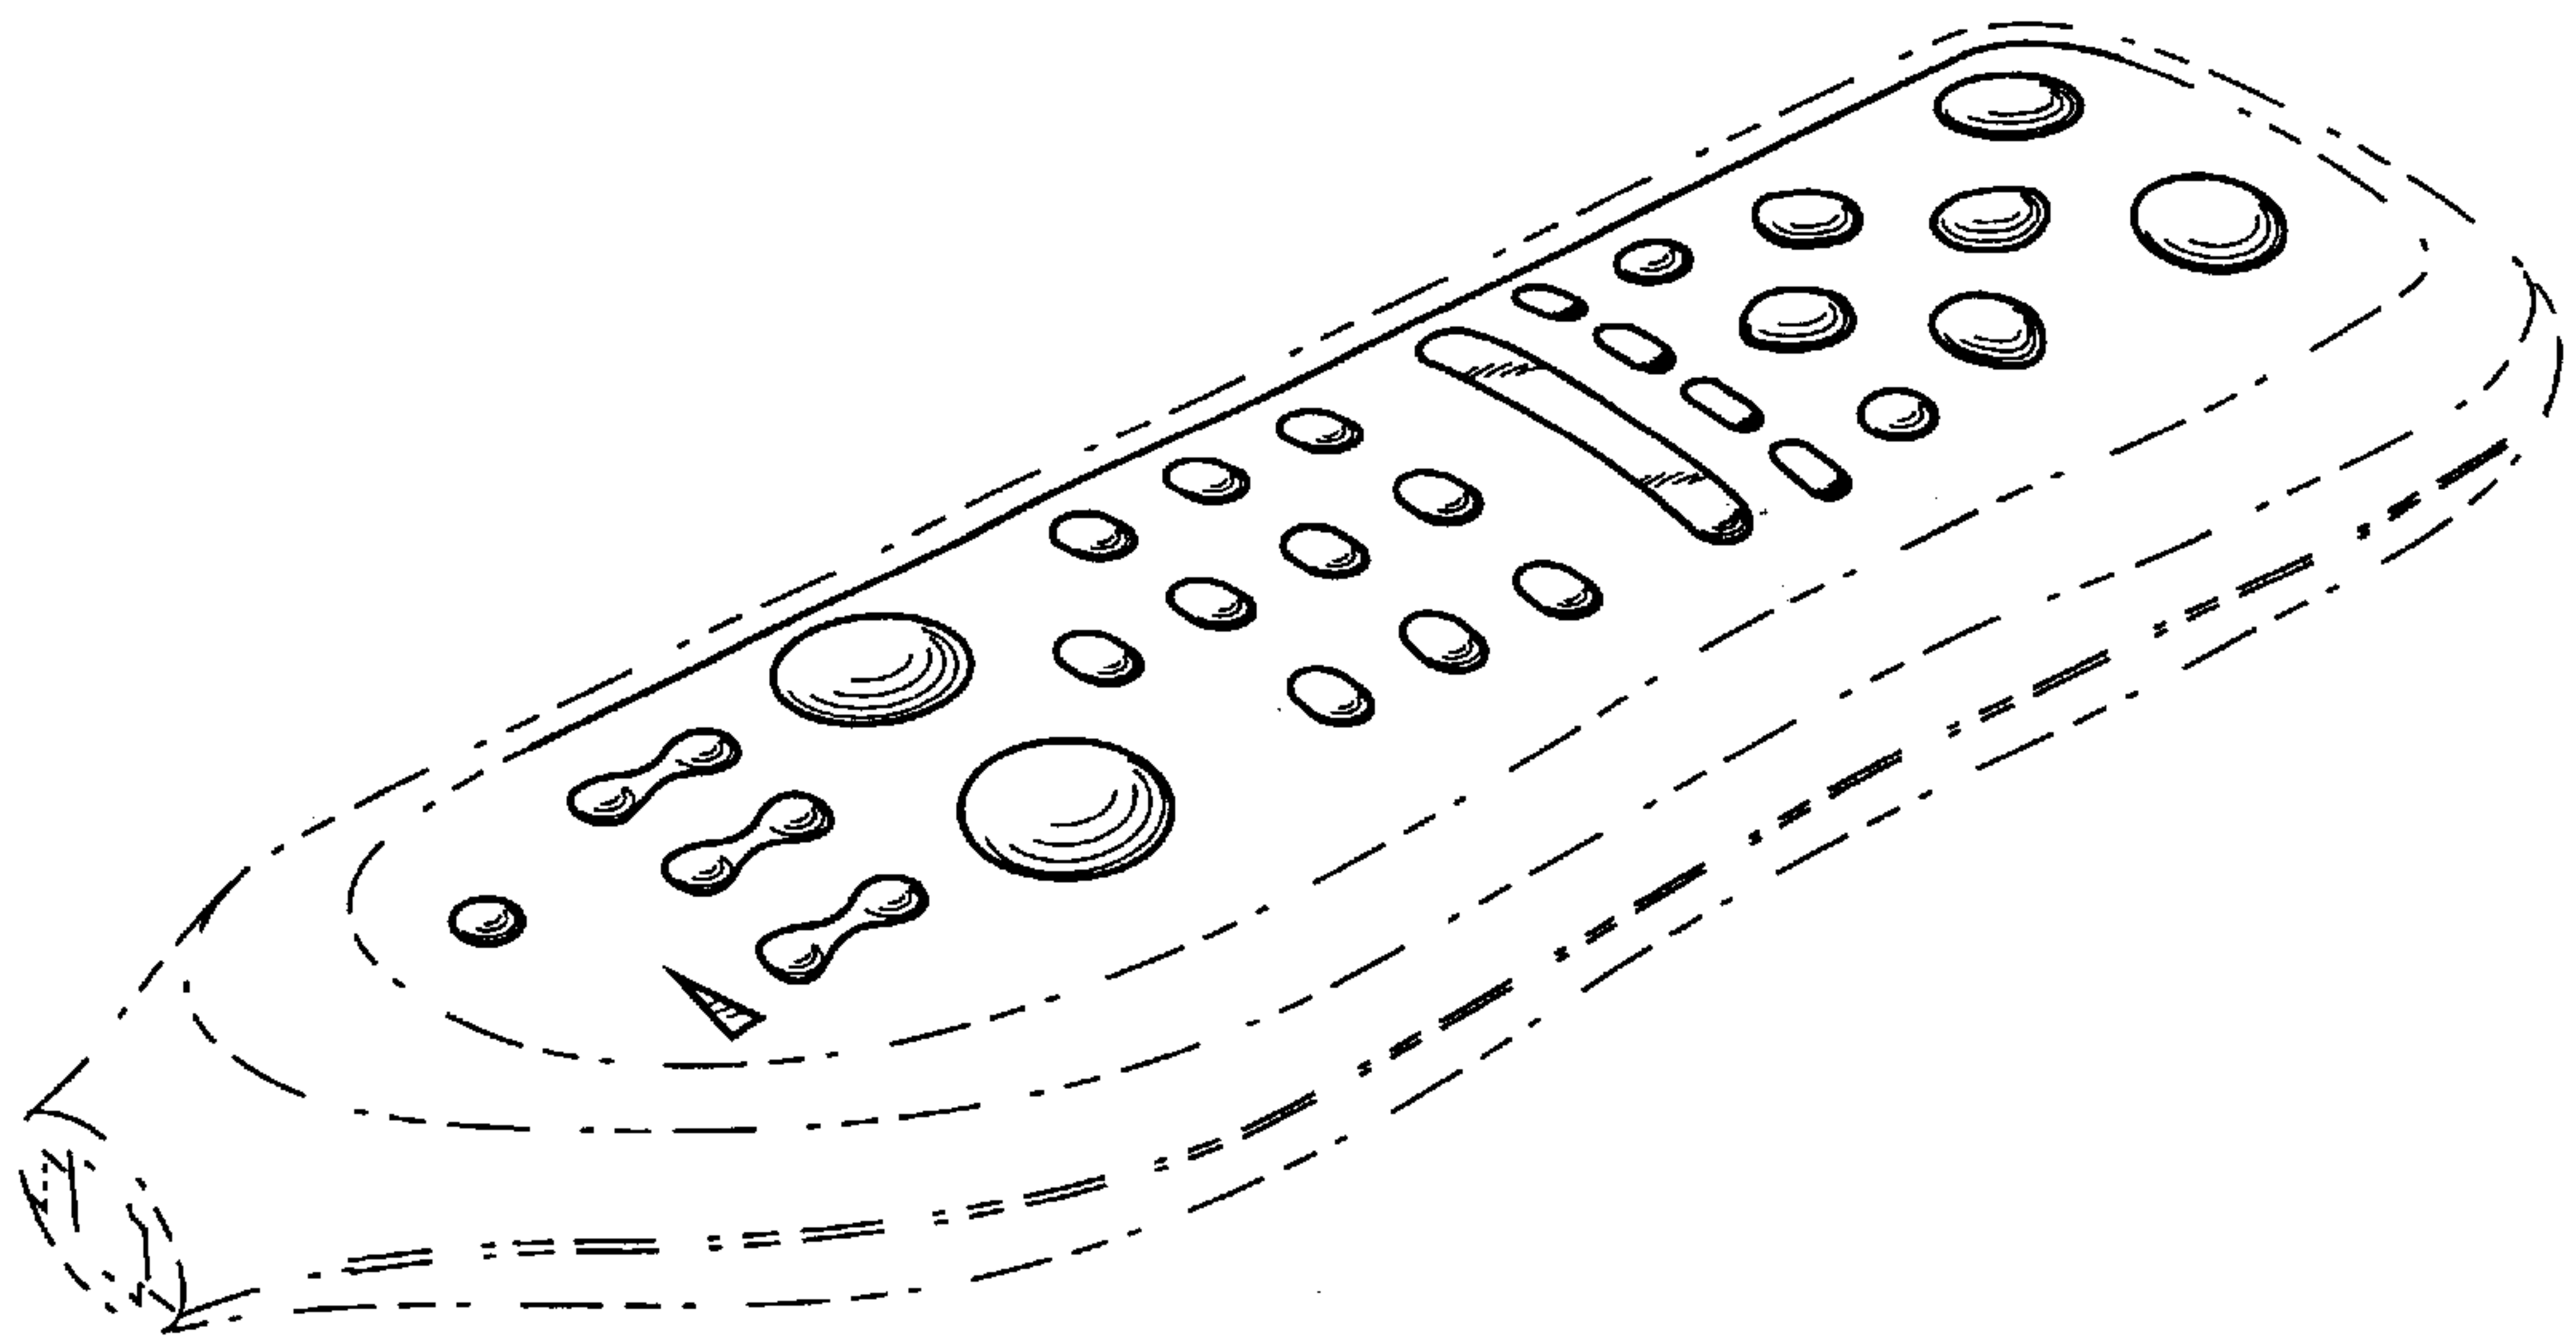

**Fig. 1**

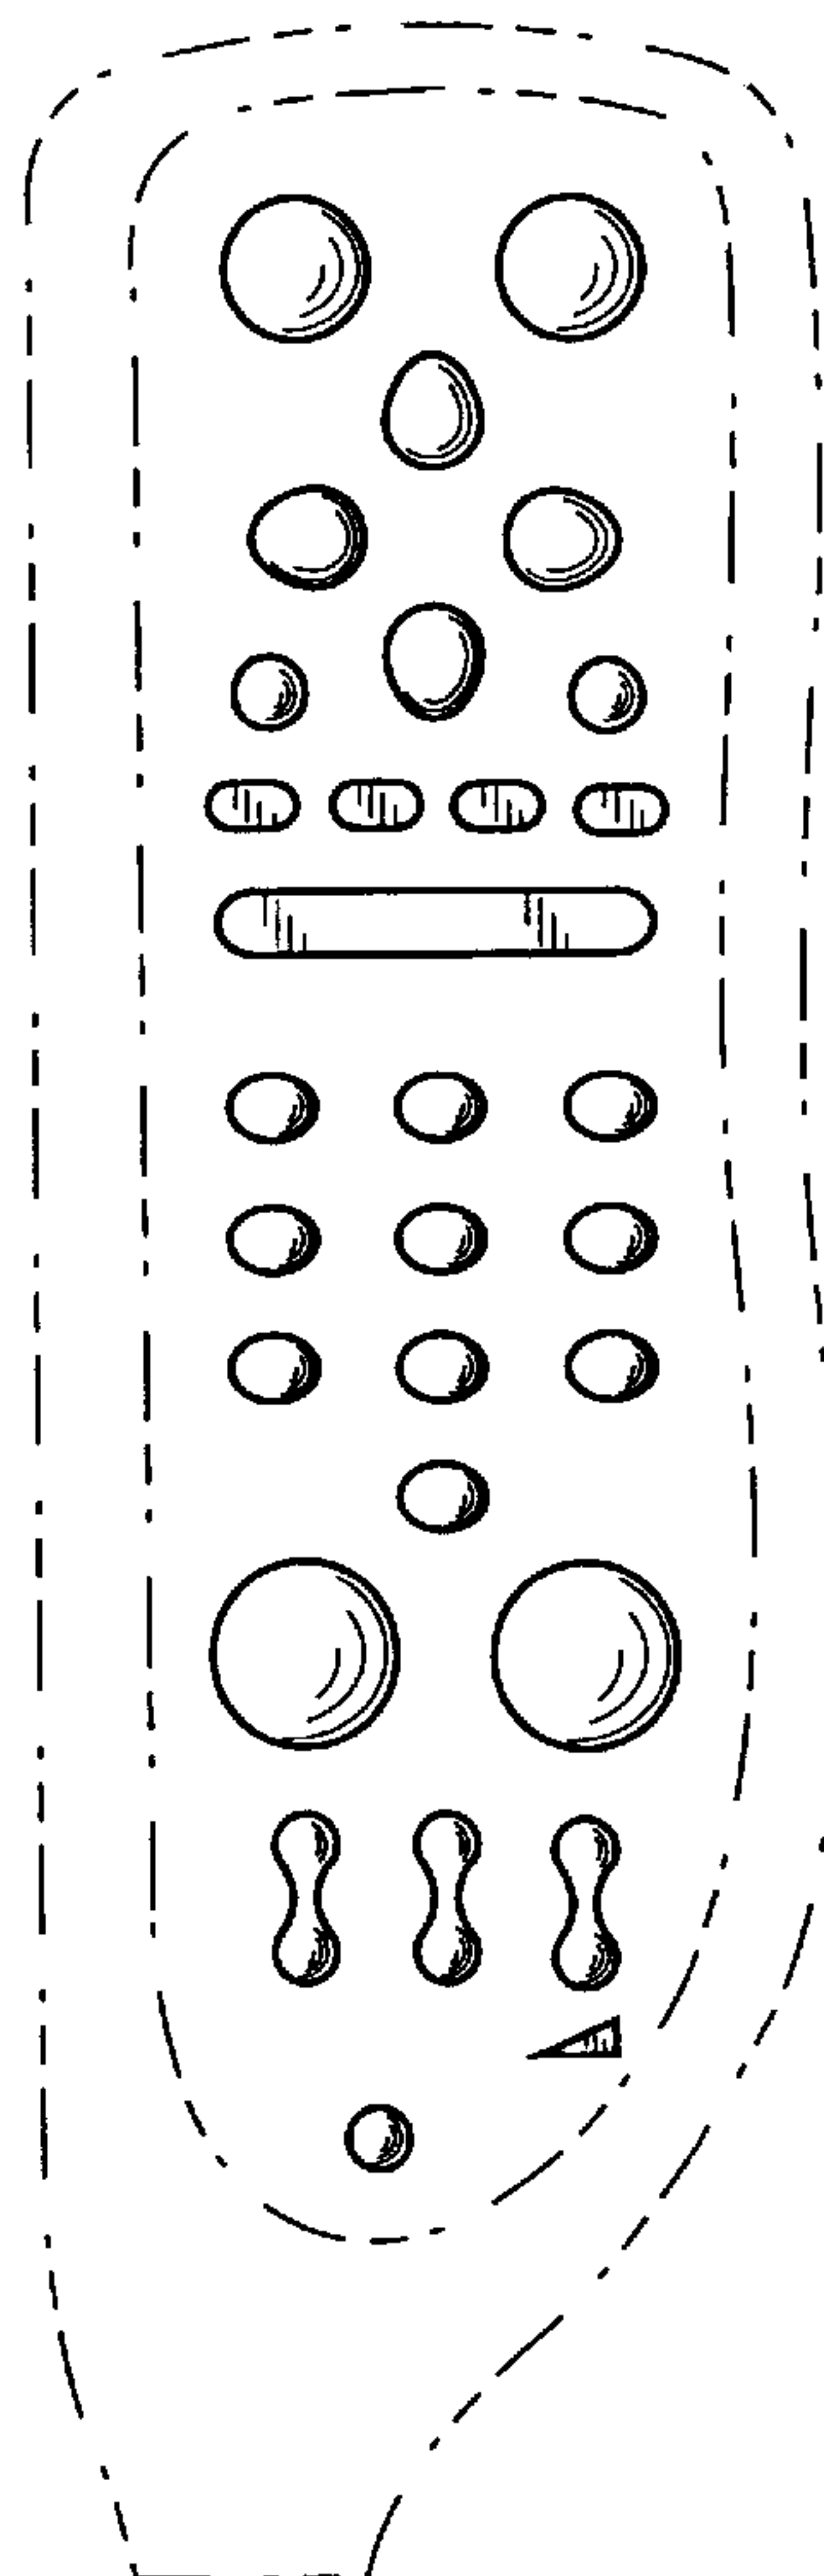

**Fig. 2**