



US00D482442S

(12) **United States Design Patent**
Pasternak

(10) **Patent No.:** **US D482,442 S**

(45) **Date of Patent:** **** Nov. 18, 2003**

(54) **INHALATION DEVICE**

(75) **Inventor:** **Gary Pasternak**, Bantford, CA (US)

(73) **Assignee:** **SmithKline Beecham Corporation**, Philadelphia, PA (US)

(**) **Term:** **14 Years**

(21) **Appl. No.:** **29/171,477**

(22) **Filed:** **Nov. 22, 2002**

(51) **LOC (7) Cl.** **29-02**

(52) **U.S. Cl.** **D24/110; D24/115**

(58) **Field of Search** **D24/110, 115; 128/200.22, 200.23, 203.23, 200.14, 200.12, 203.12, 203.15; 222/153.11, 153.13, 153.14**

(56) **References Cited**

U.S. PATENT DOCUMENTS

| | | | | | |
|------------|---|--------|---------|-------|---------|
| D320,083 S | * | 9/1991 | Casey | | D24/110 |
| D414,261 S | * | 9/1999 | Ritsche | | D24/110 |
| D468,423 S | * | 1/2003 | Renfrew | | D24/115 |

* cited by examiner

Primary Examiner—Ian Simmons

(74) *Attorney, Agent, or Firm*—James P. Riek

(57) **CLAIM**

The ornamental design for an inhalation device, as shown and described.

DESCRIPTION

FIG. 1 is a perspective view of the inhalation device of our new design (with an actuator cover cap);

FIG. 2 is a side view of of the inhalation device depicted in FIG. 1.

FIG. 3 is a rear view of the opposite side of the inhalation device.

FIG. 4 is a side view of the opposite side of the inhalation device depicted in FIG. 2;

FIG. 5 is a front view of the inhalation device depicted in FIG. 1;

FIG. 6 is a top view of the inhalation device depicted in FIG. 1;

FIG. 7 is a bottom view of the inhalation device depicted in FIG. 1;

FIG. 8 is a perspective view of the inhalation device of our new design (with a cover cap shown in relief);

FIG. 9 is a side view of the inhalation device depicted in FIG. 8 (without a cover cap).

FIG. 10 is a rear view of the opposite side of FIG. 9

FIG. 11 is a side view of the opposite side of the inhalation device depicted in FIG. 9.

FIG. 12 is a front view of the inhalation device as depicted in FIG. 8.

FIG. 13 is a top view of the inhalation device as depicted in FIG. 8; and,

FIG. 14 is a bottom view of the inhalation device as depicted in FIG. 8.

1 Claim, 4 Drawing Sheets

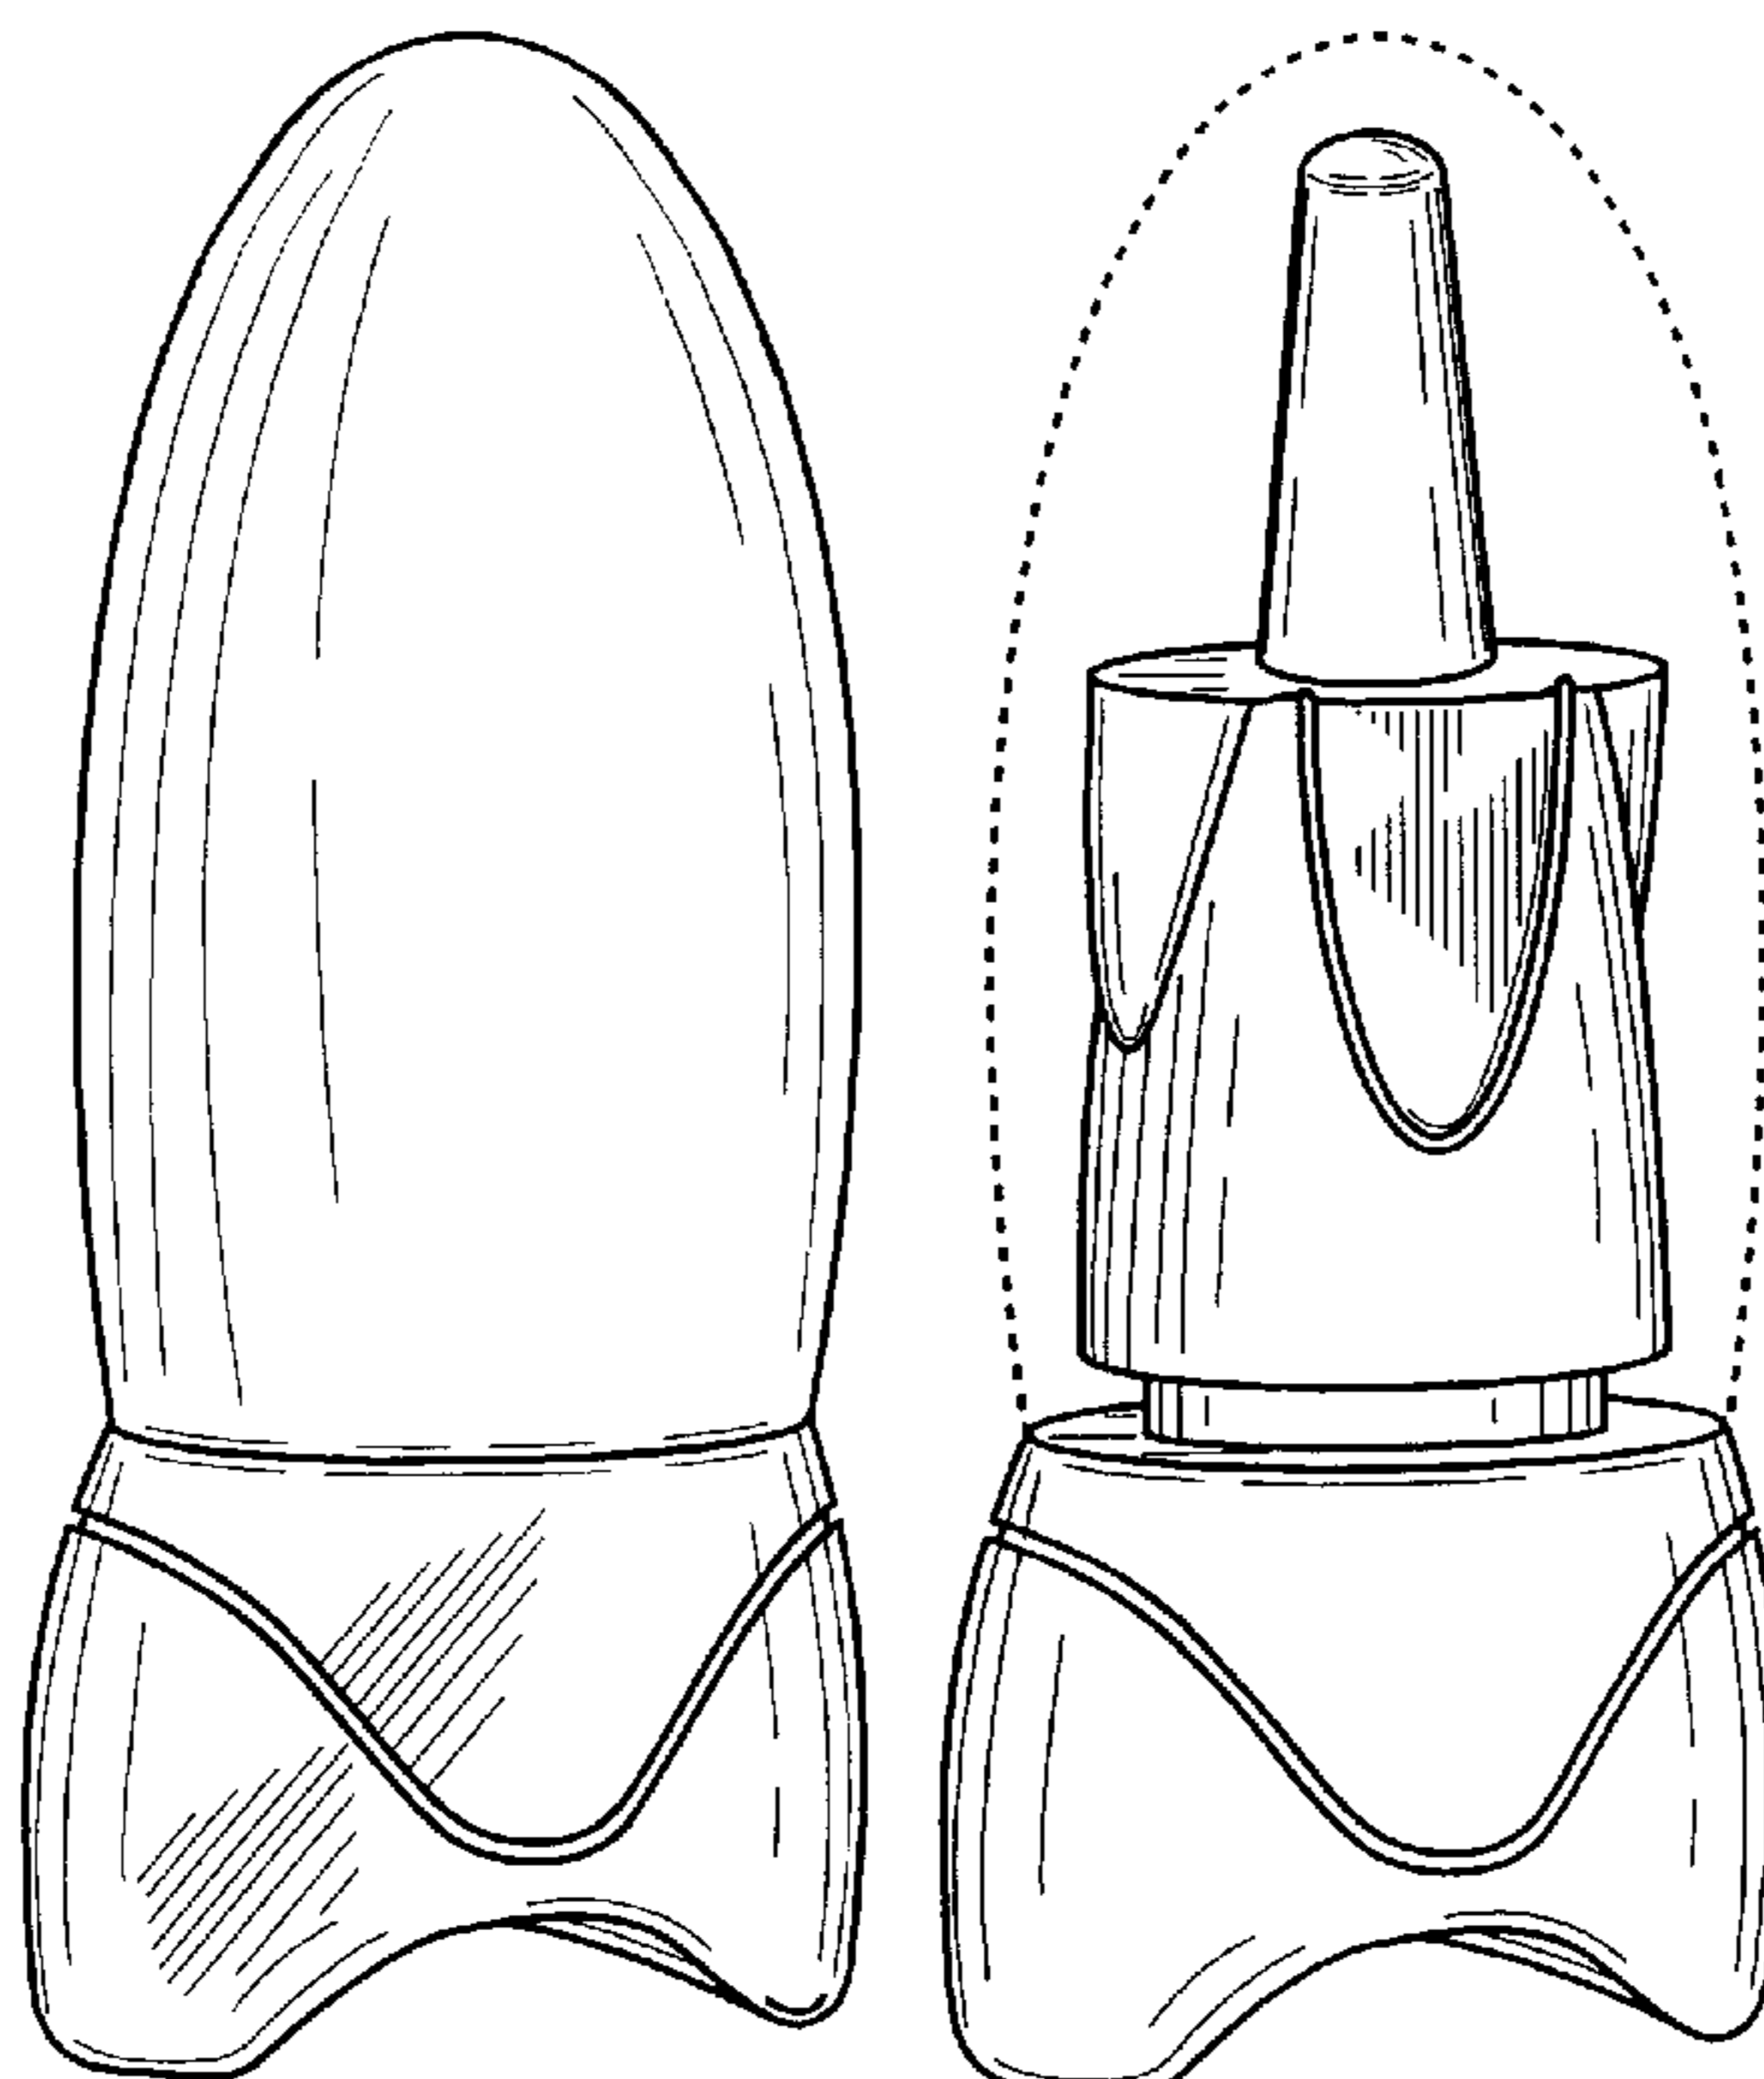


FIG. 1

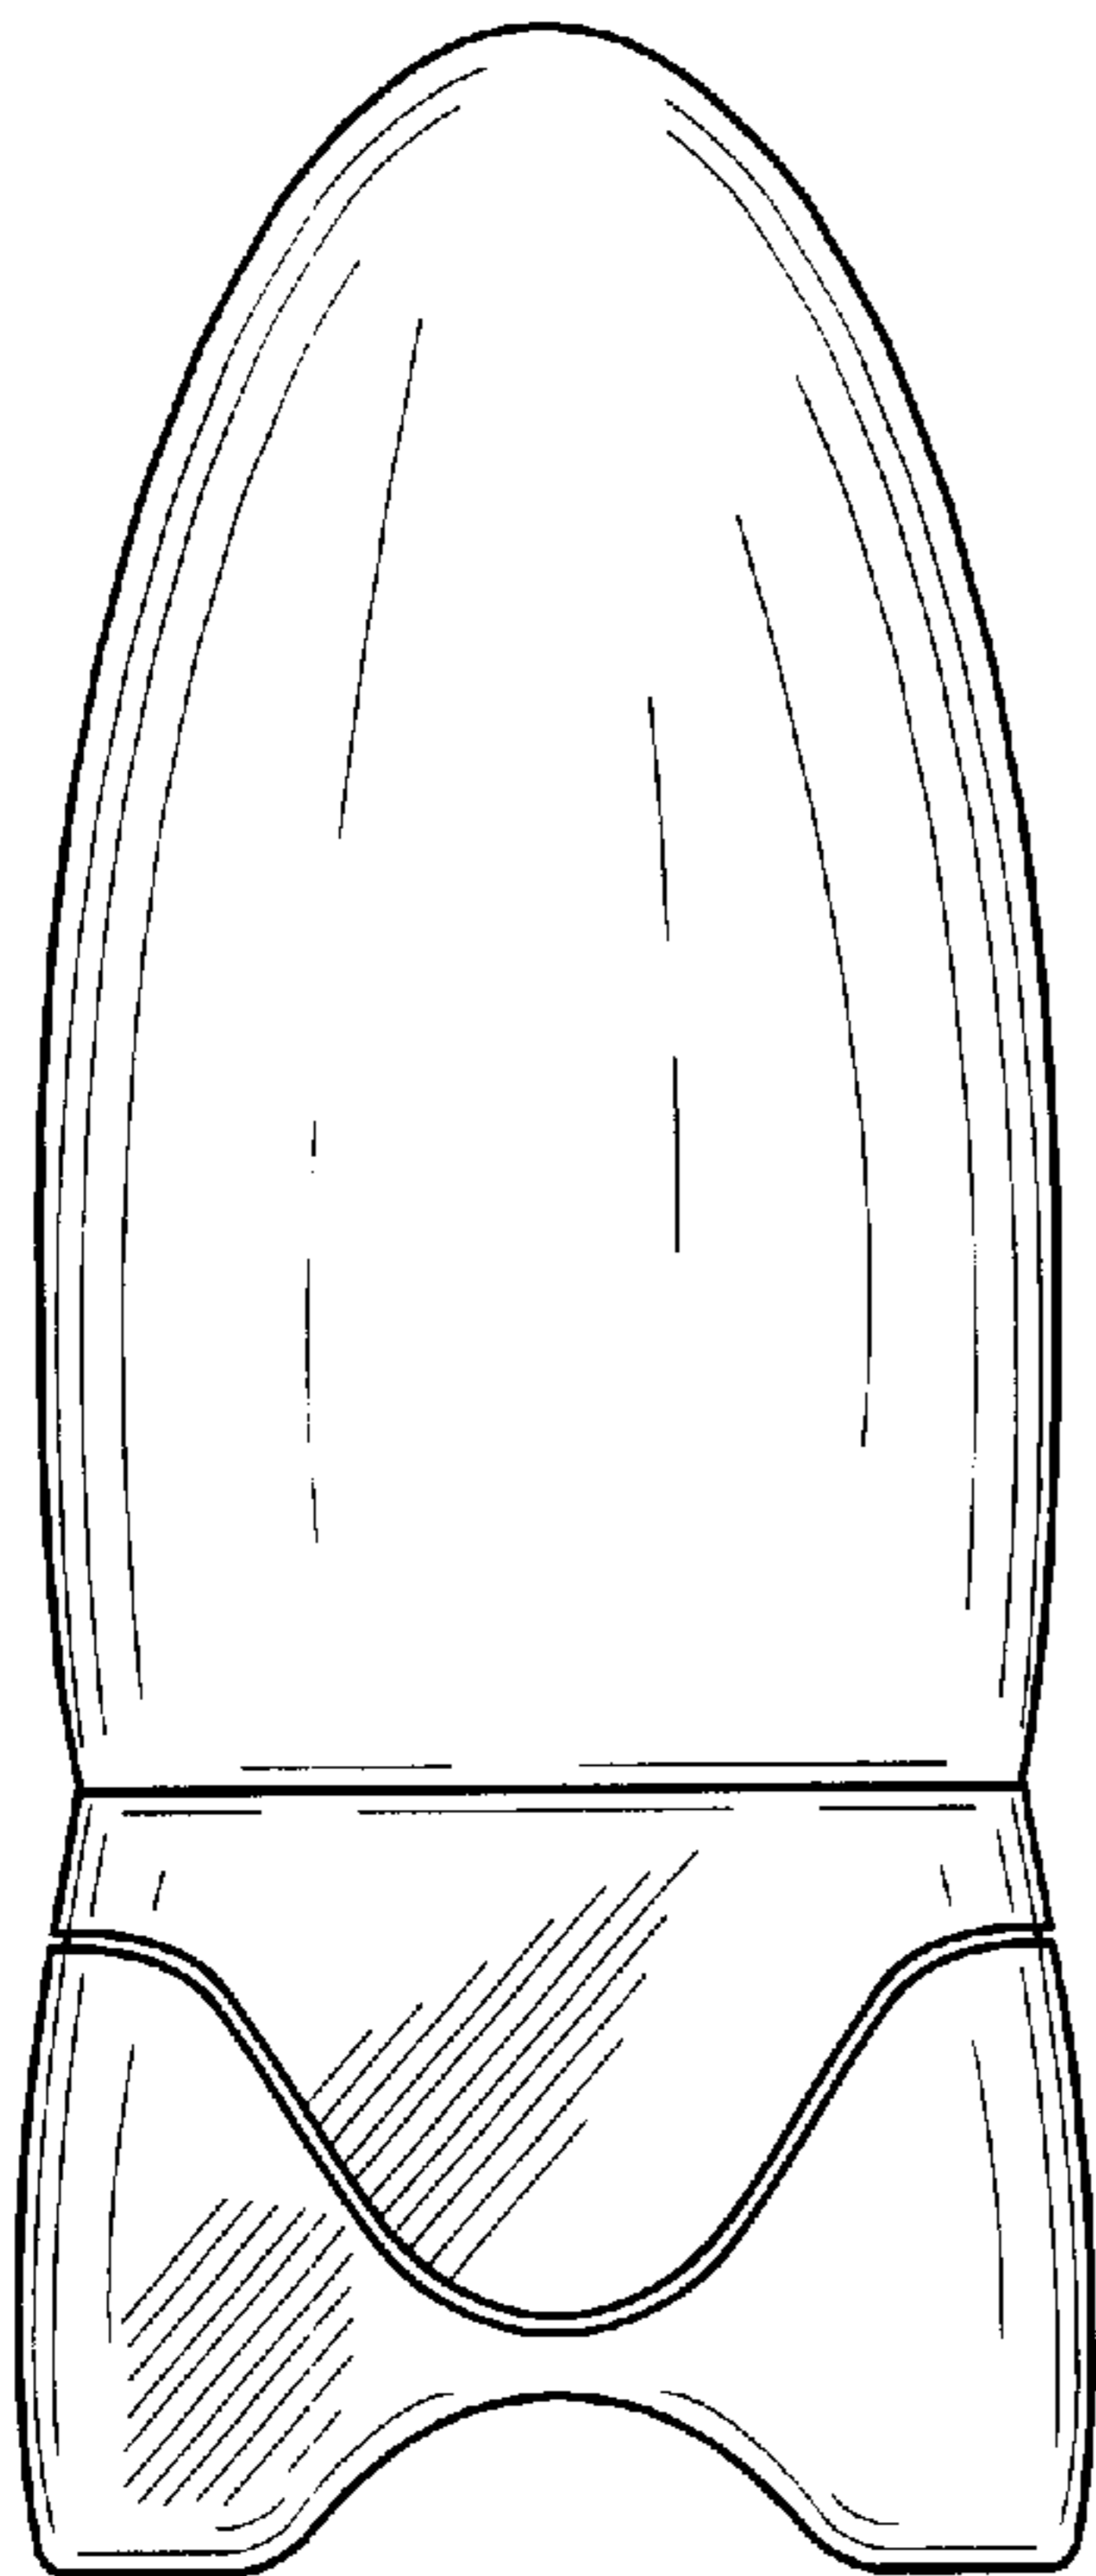
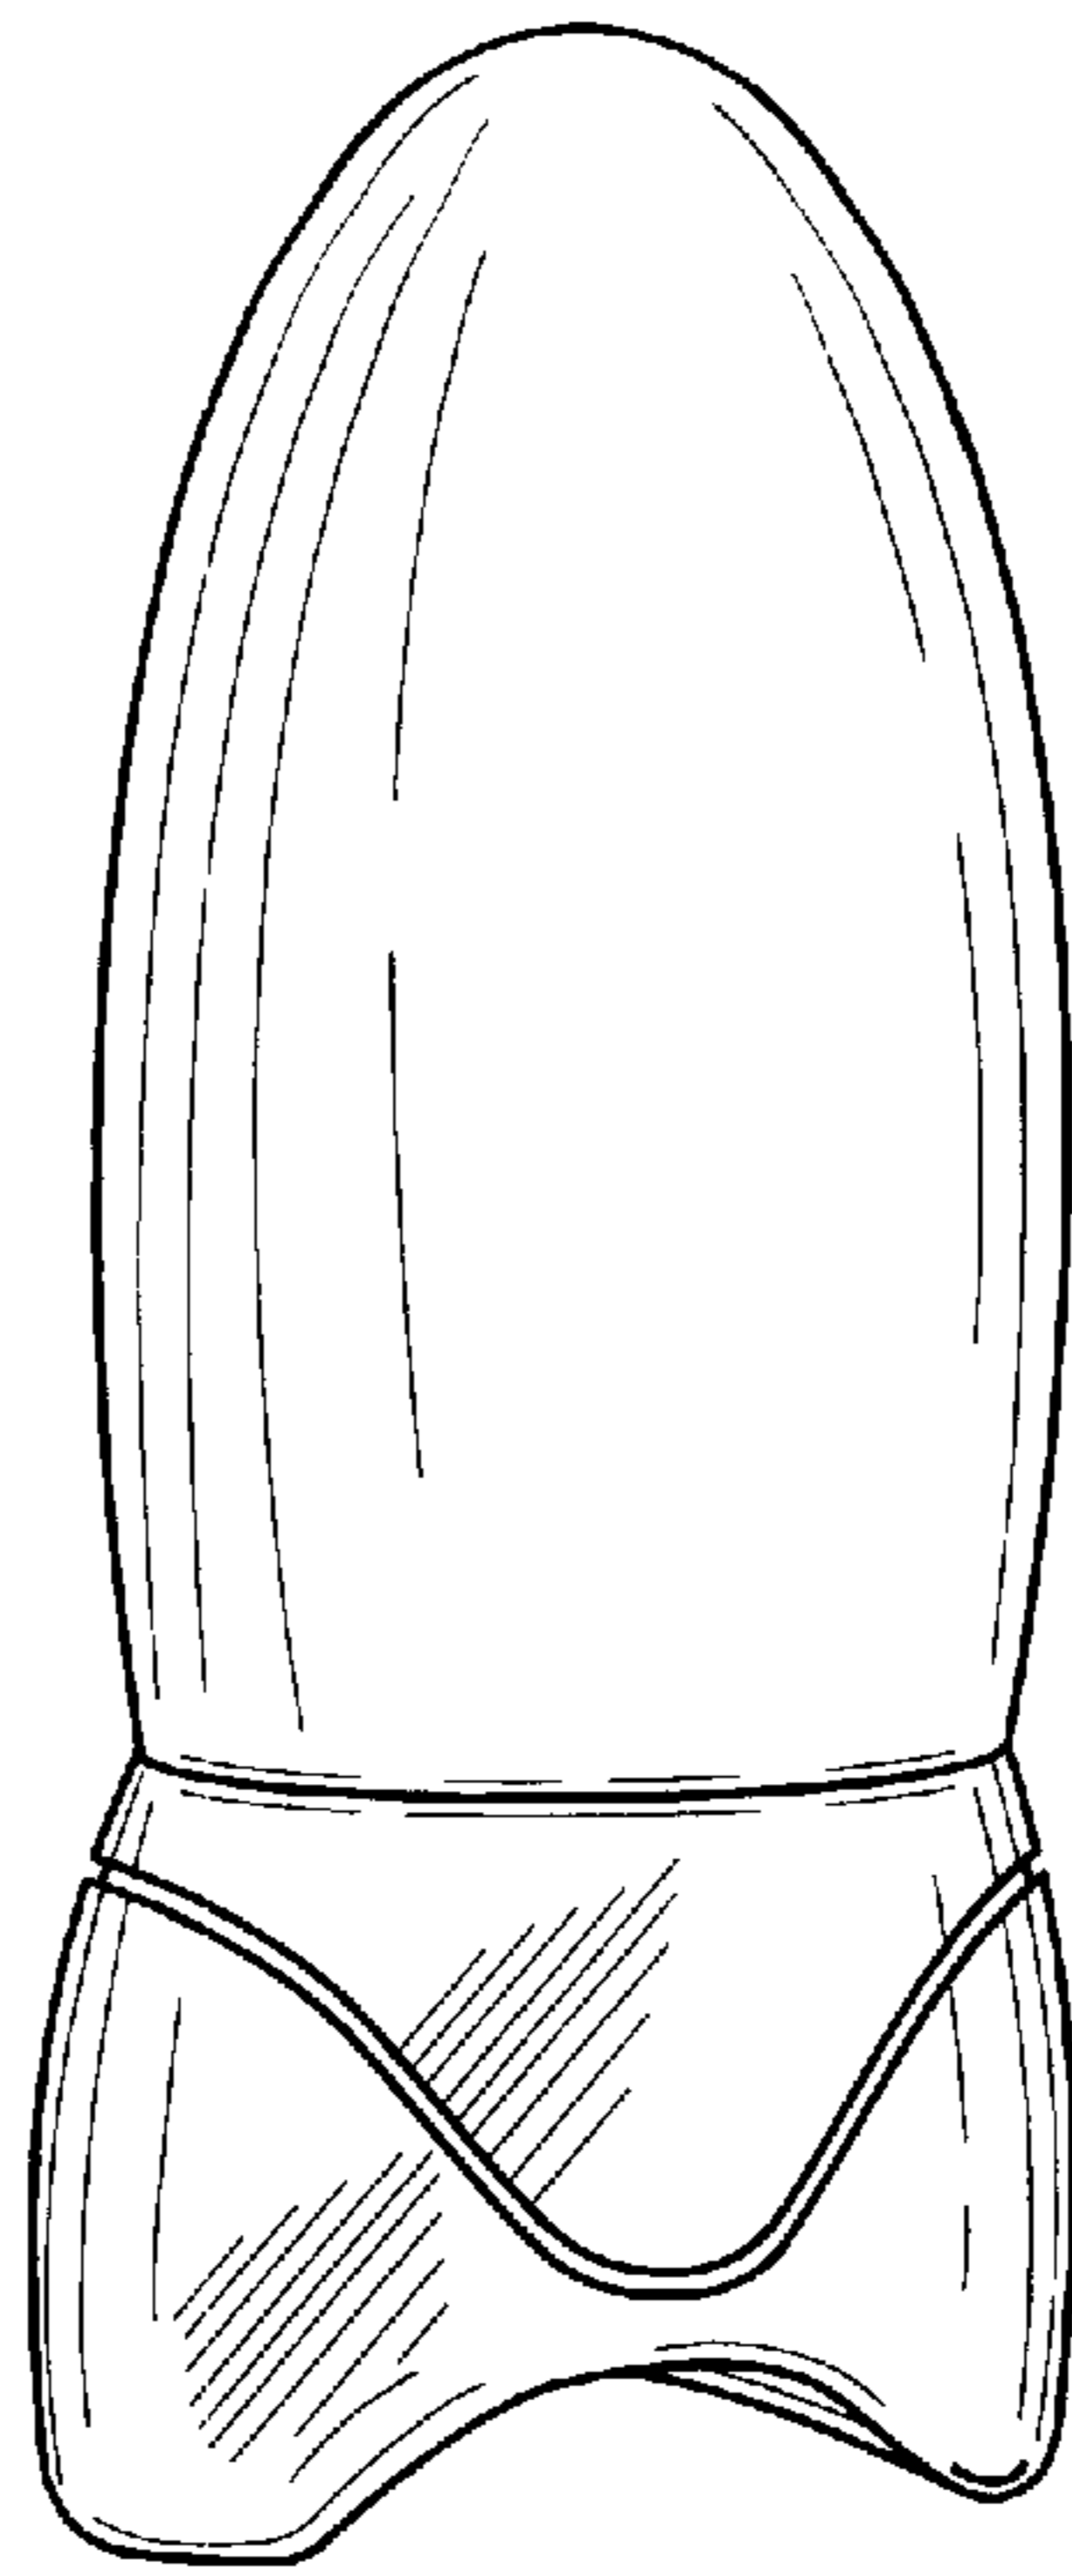


FIG. 2

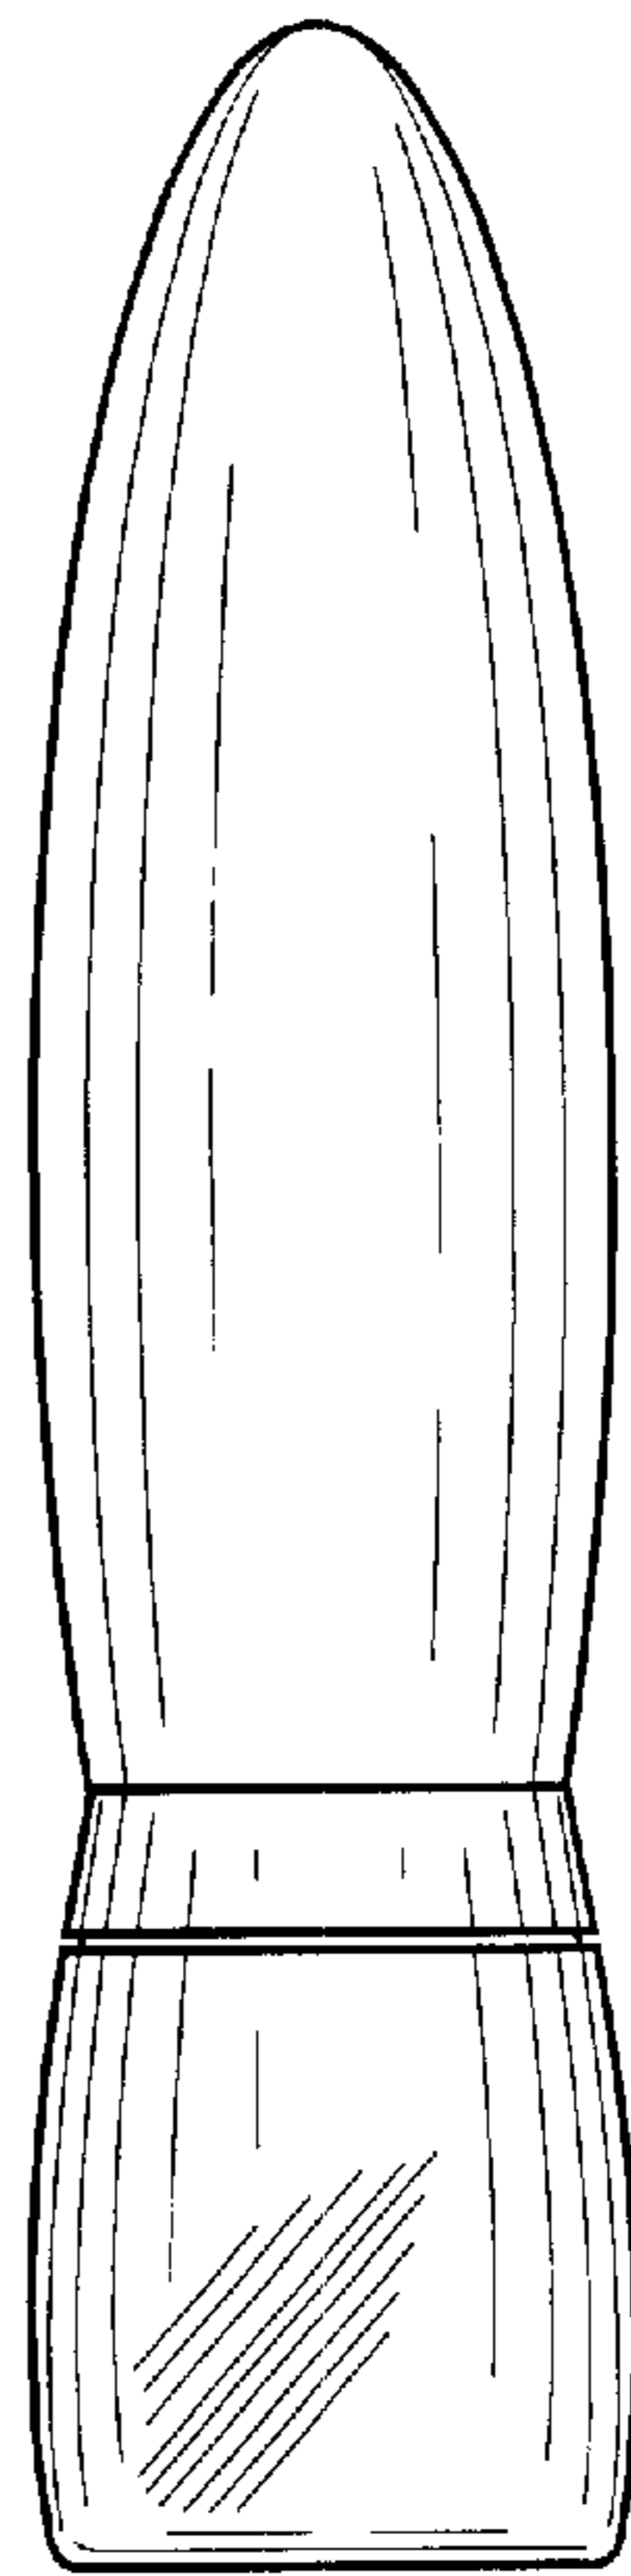


FIG. 3

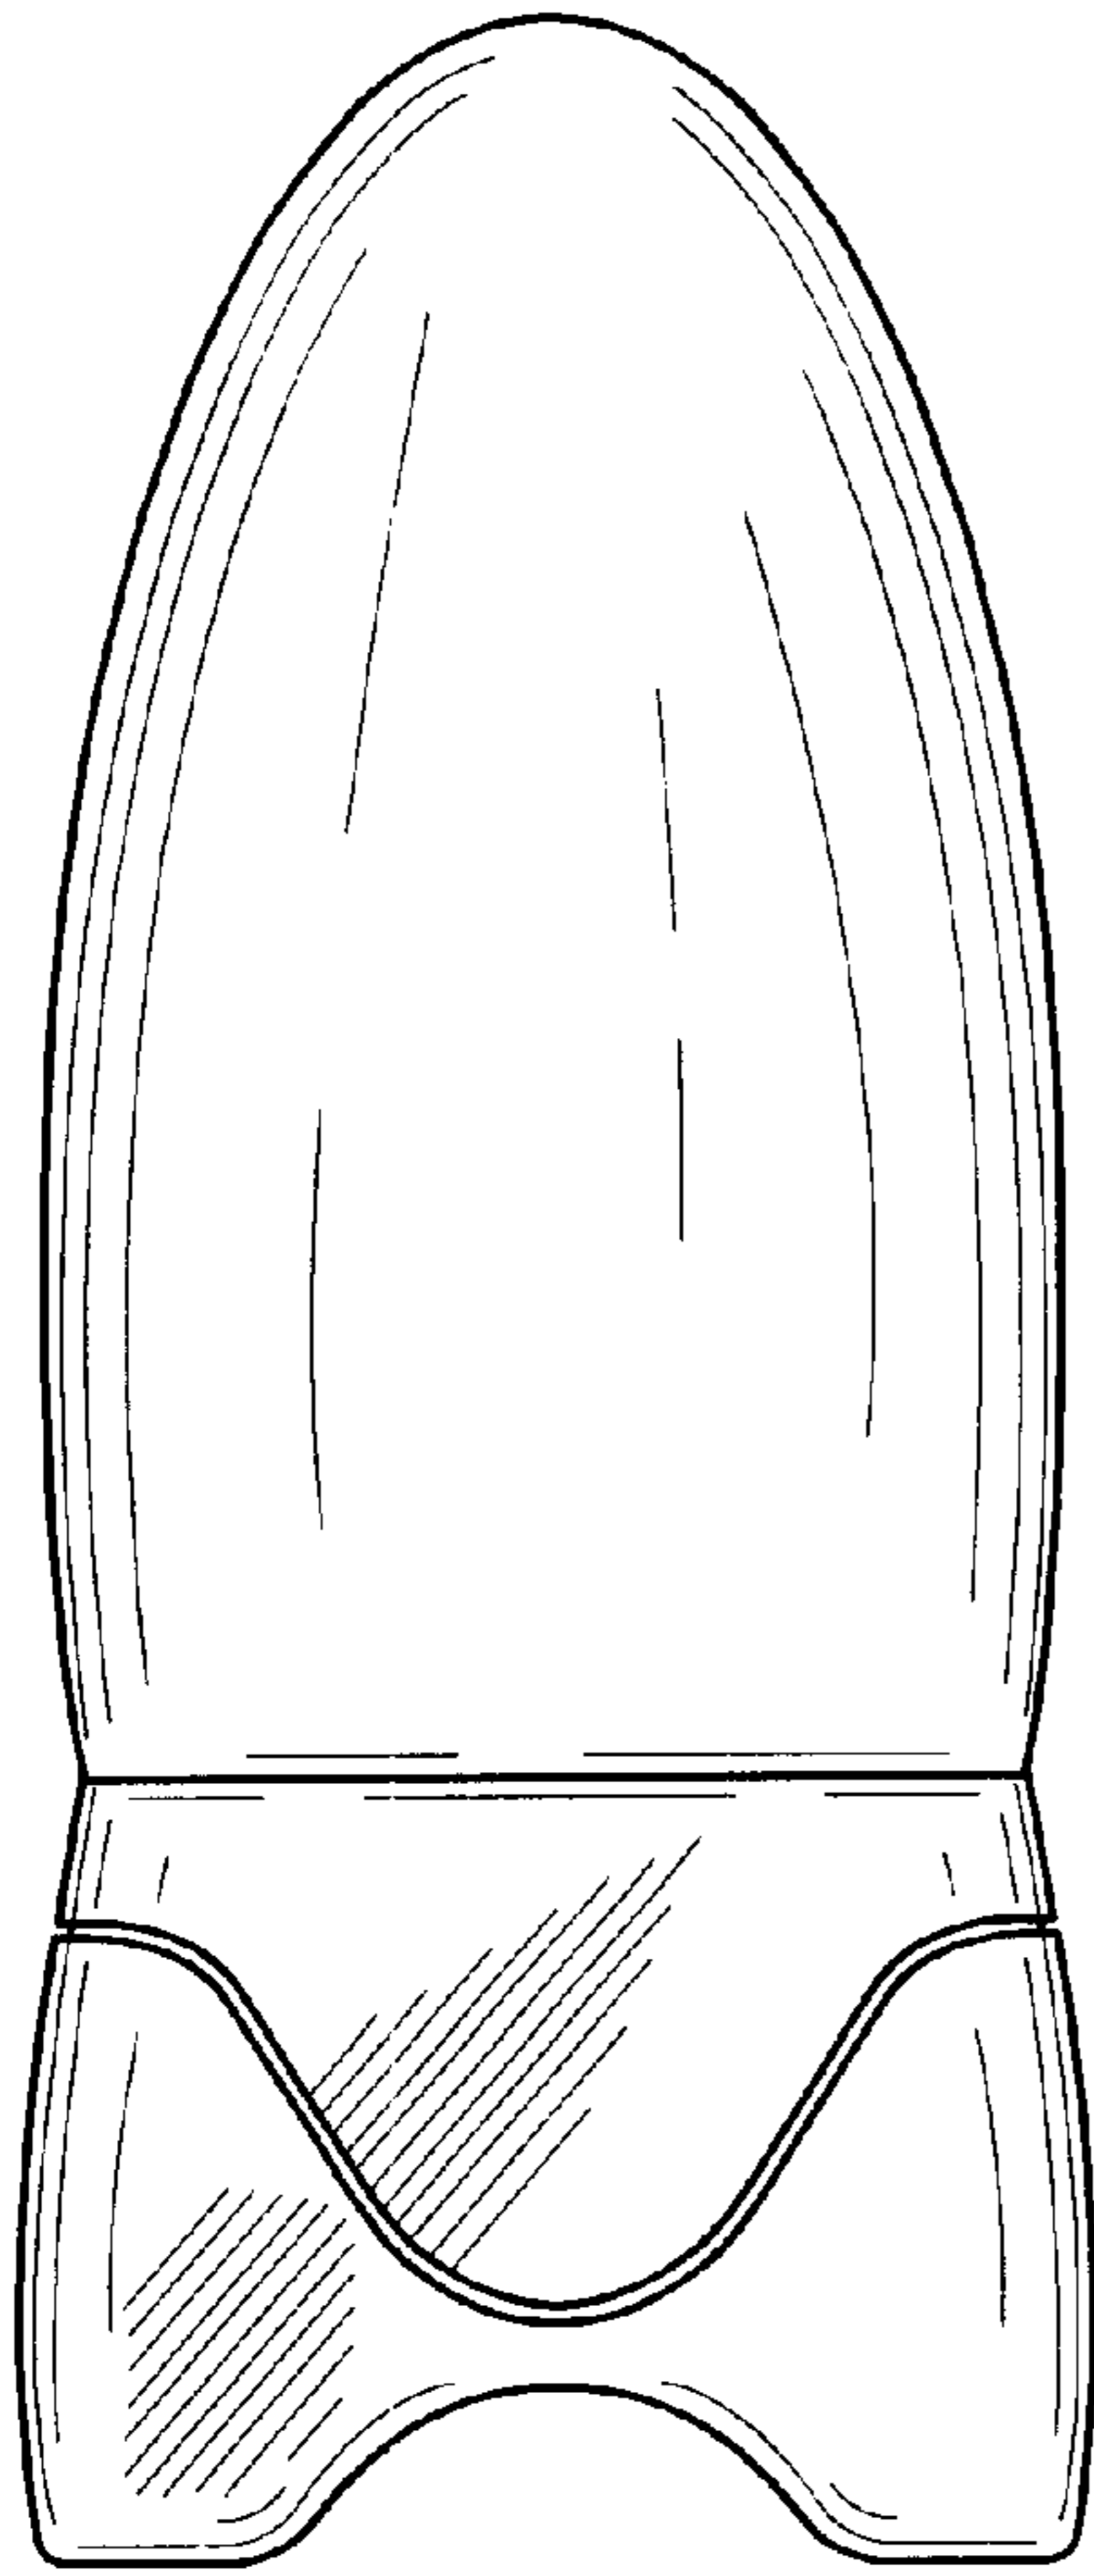


FIG. 4

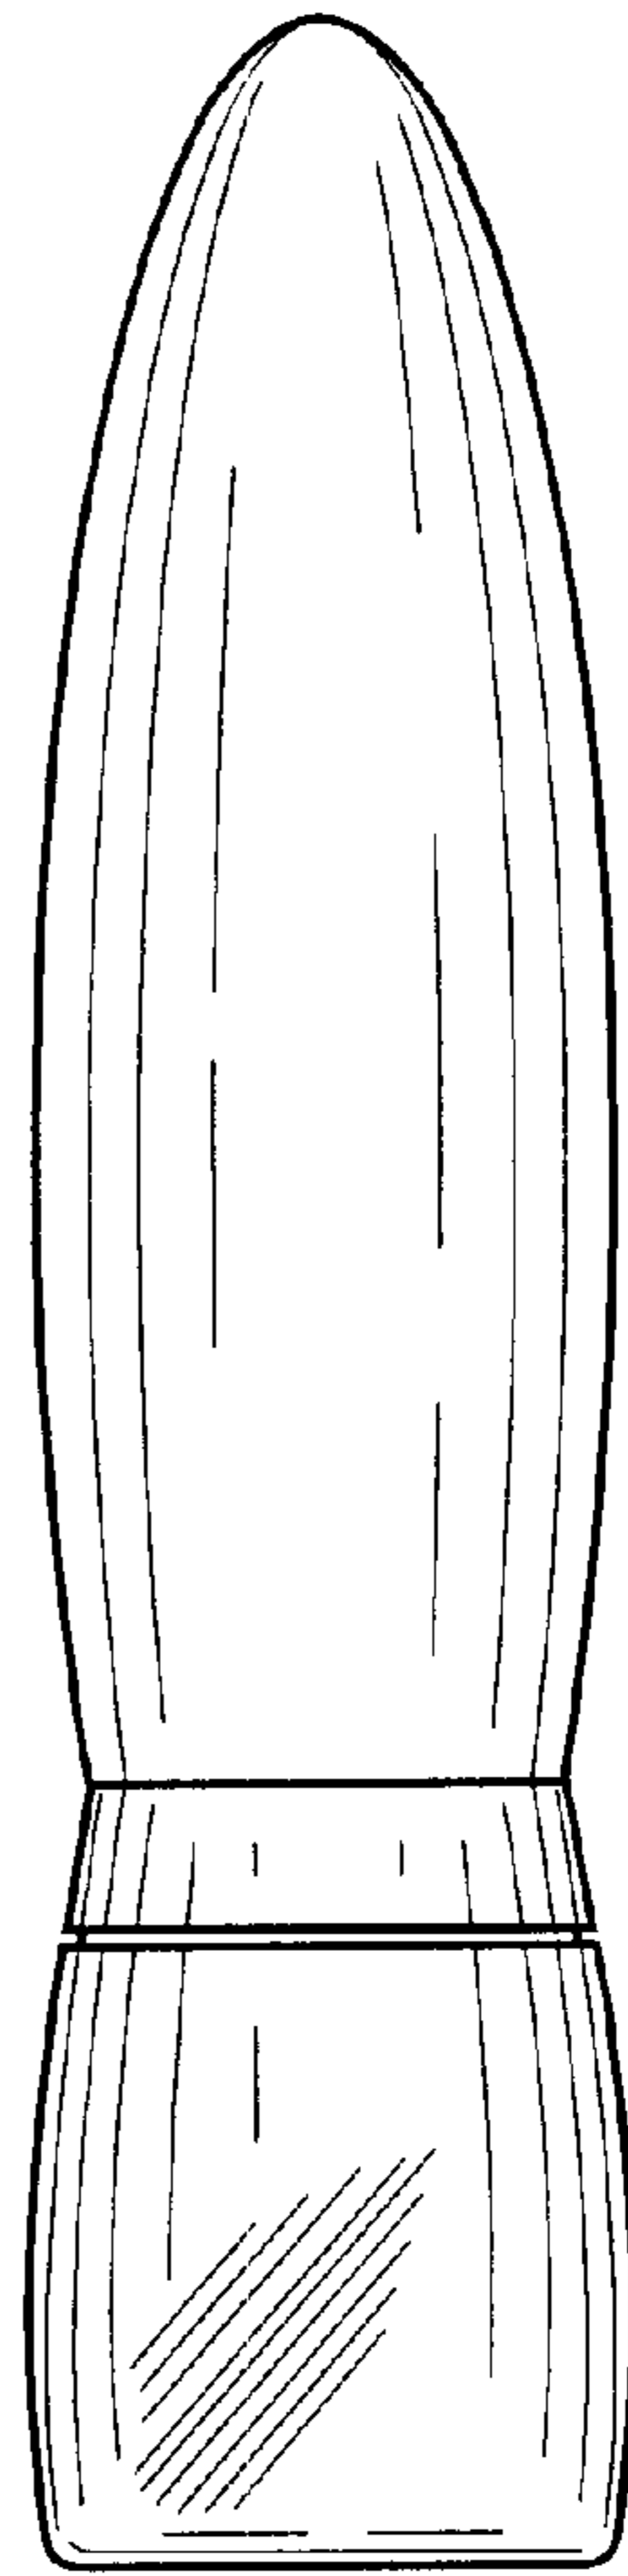


FIG. 5

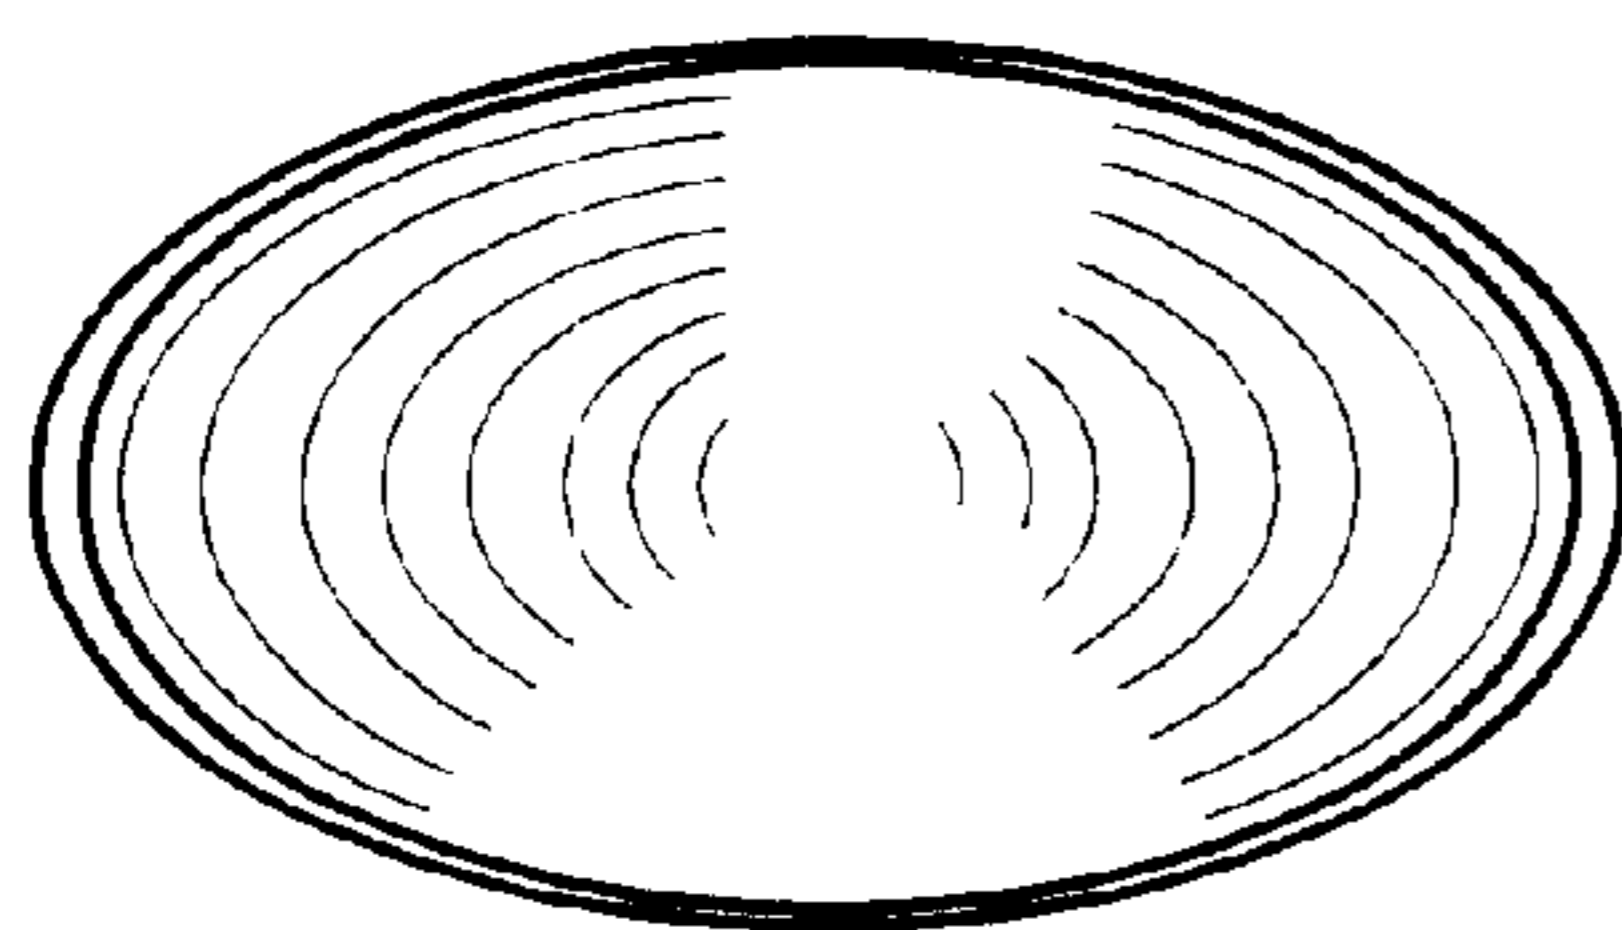


FIG. 6

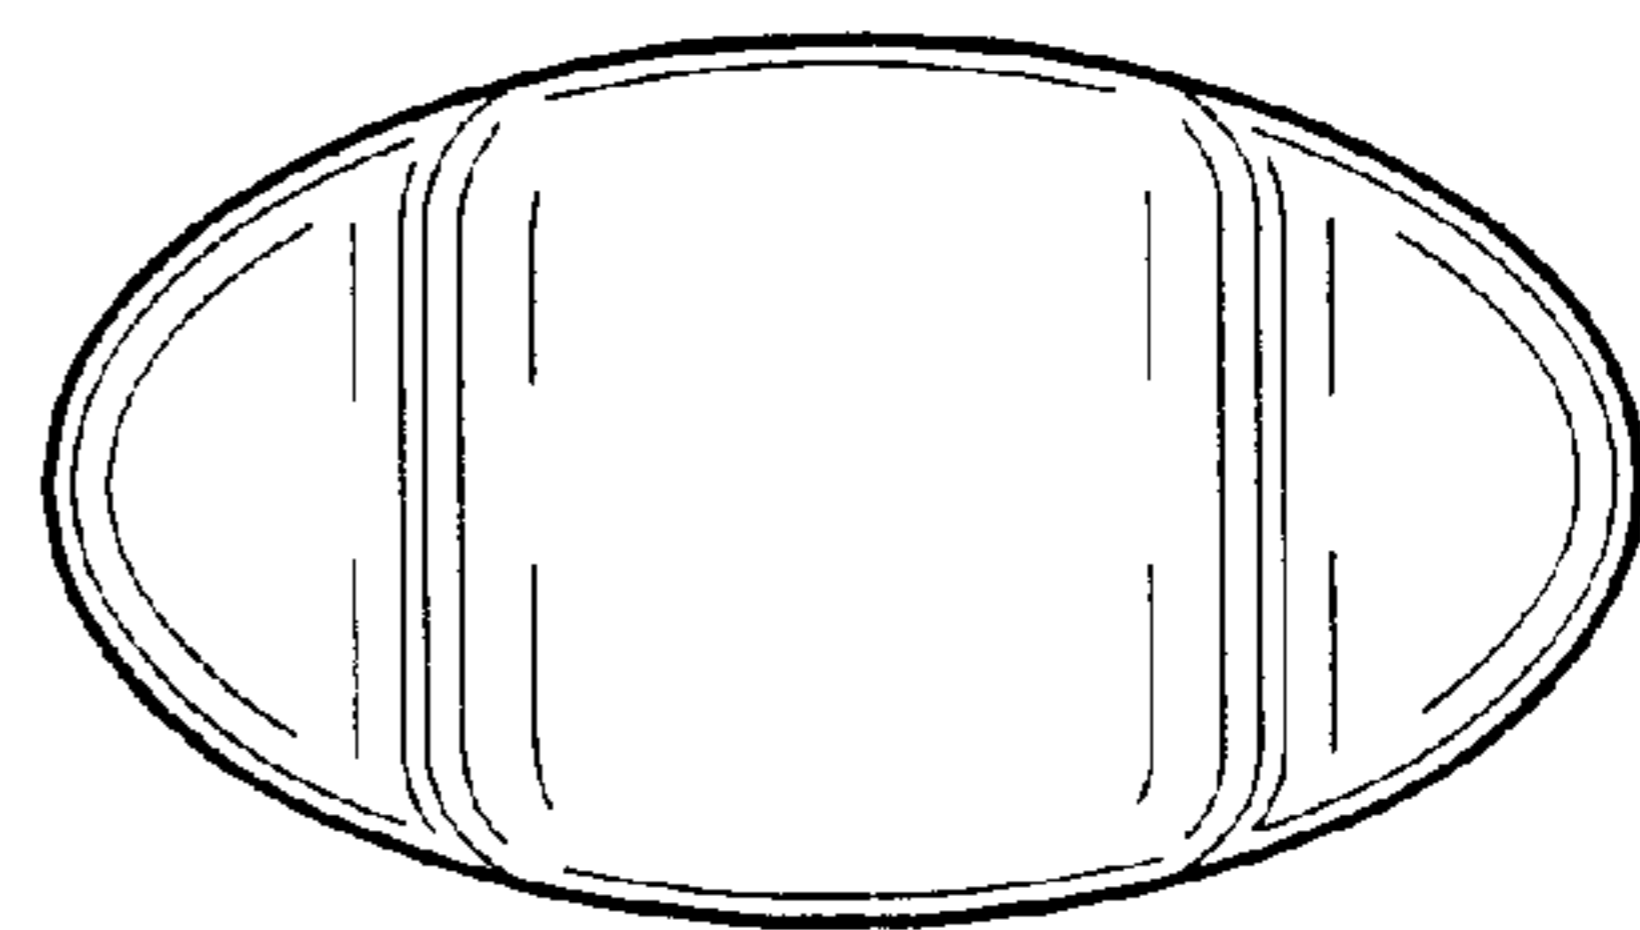


FIG. 7

FIG. 8

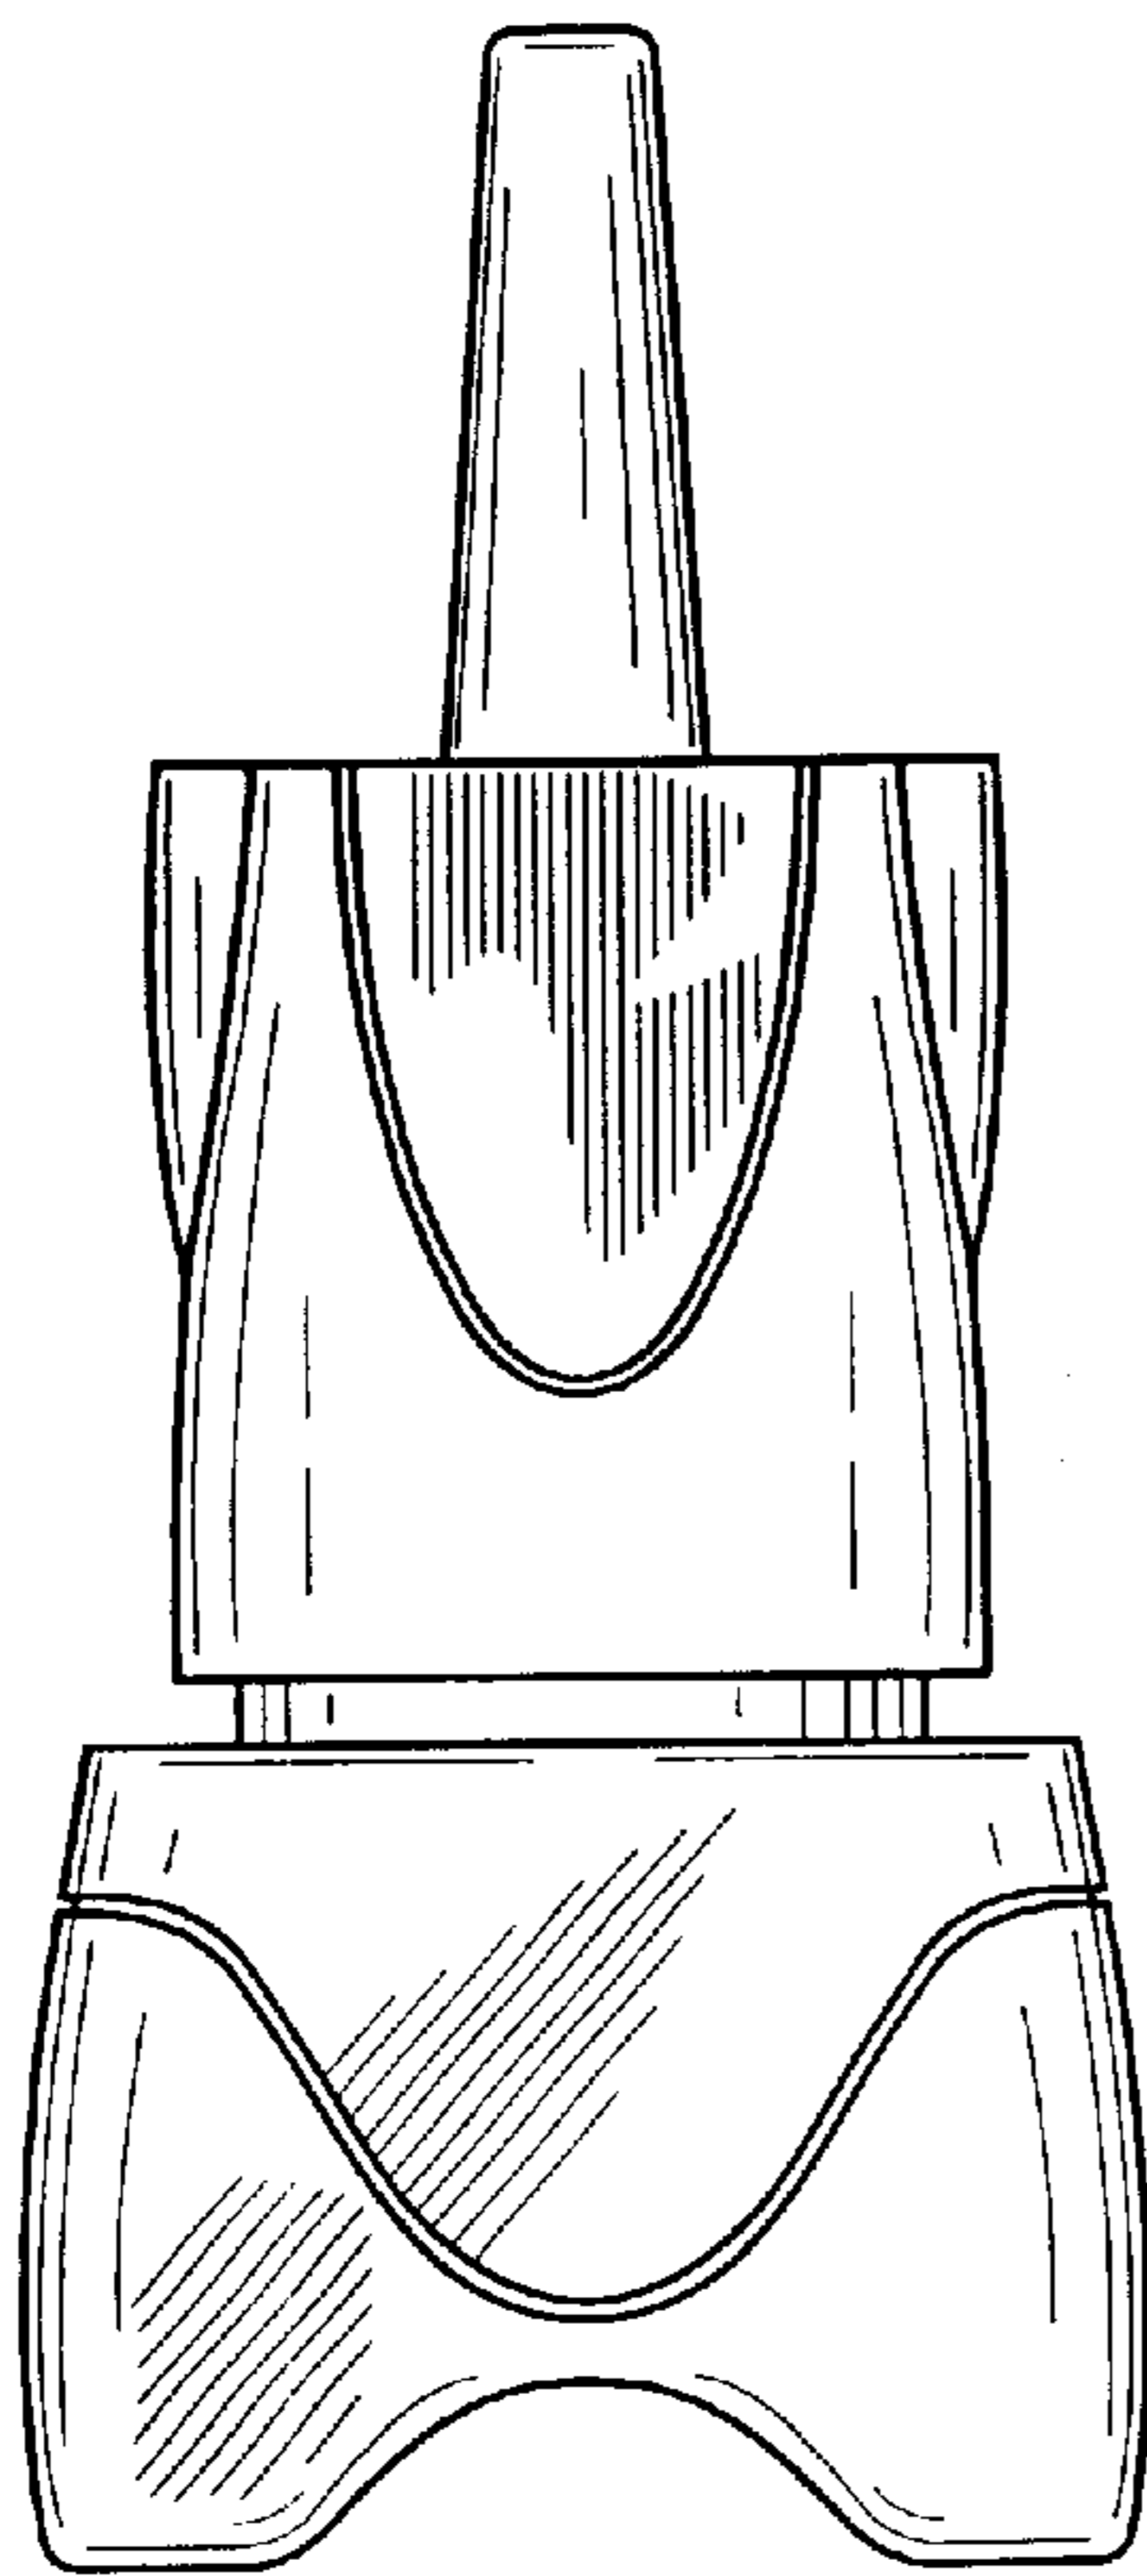
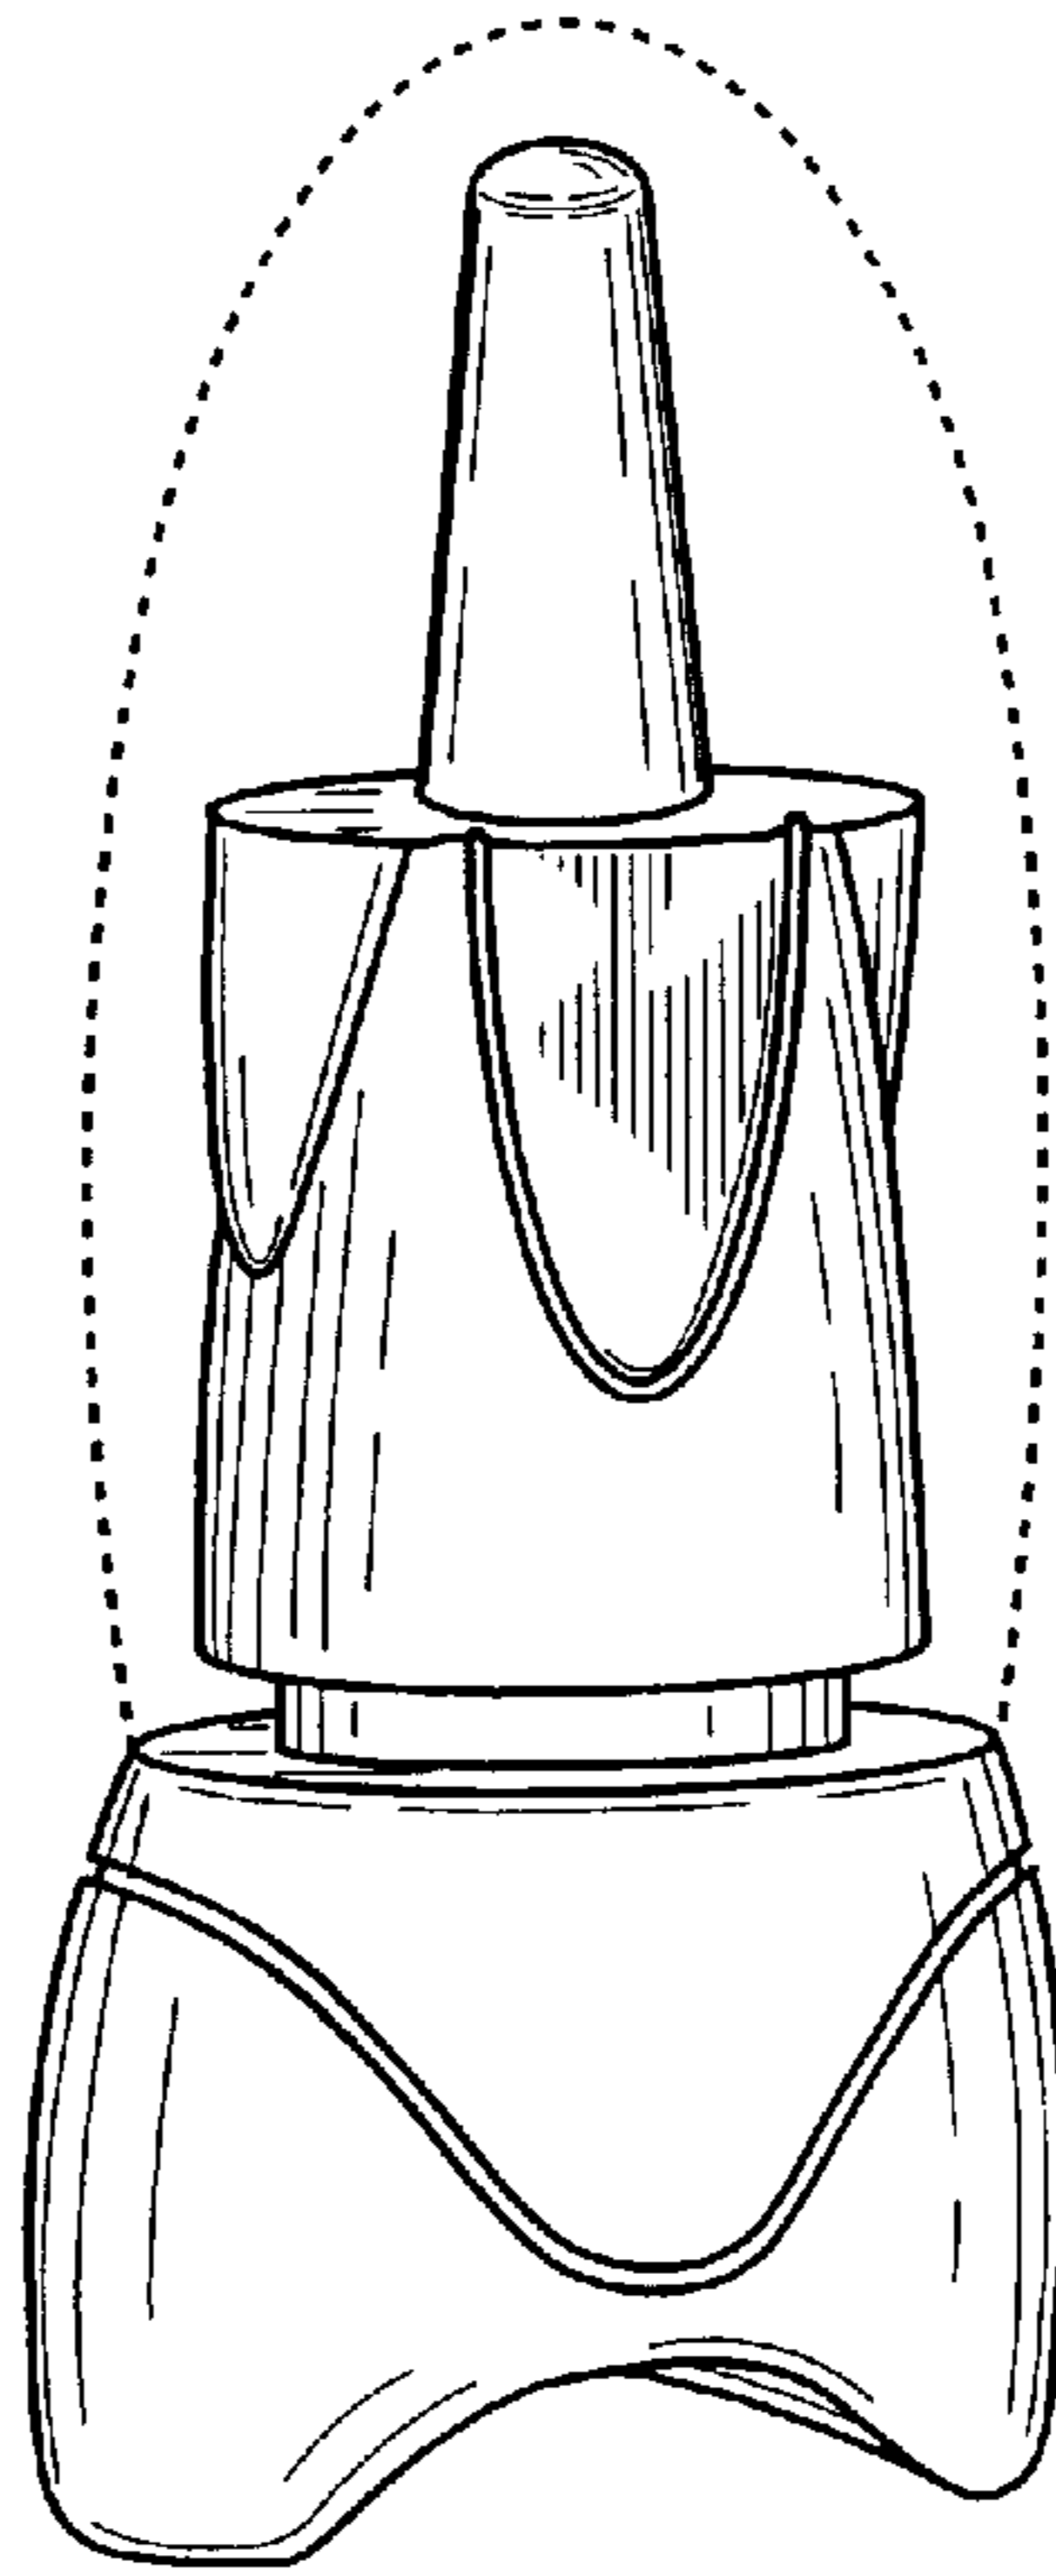


FIG. 9

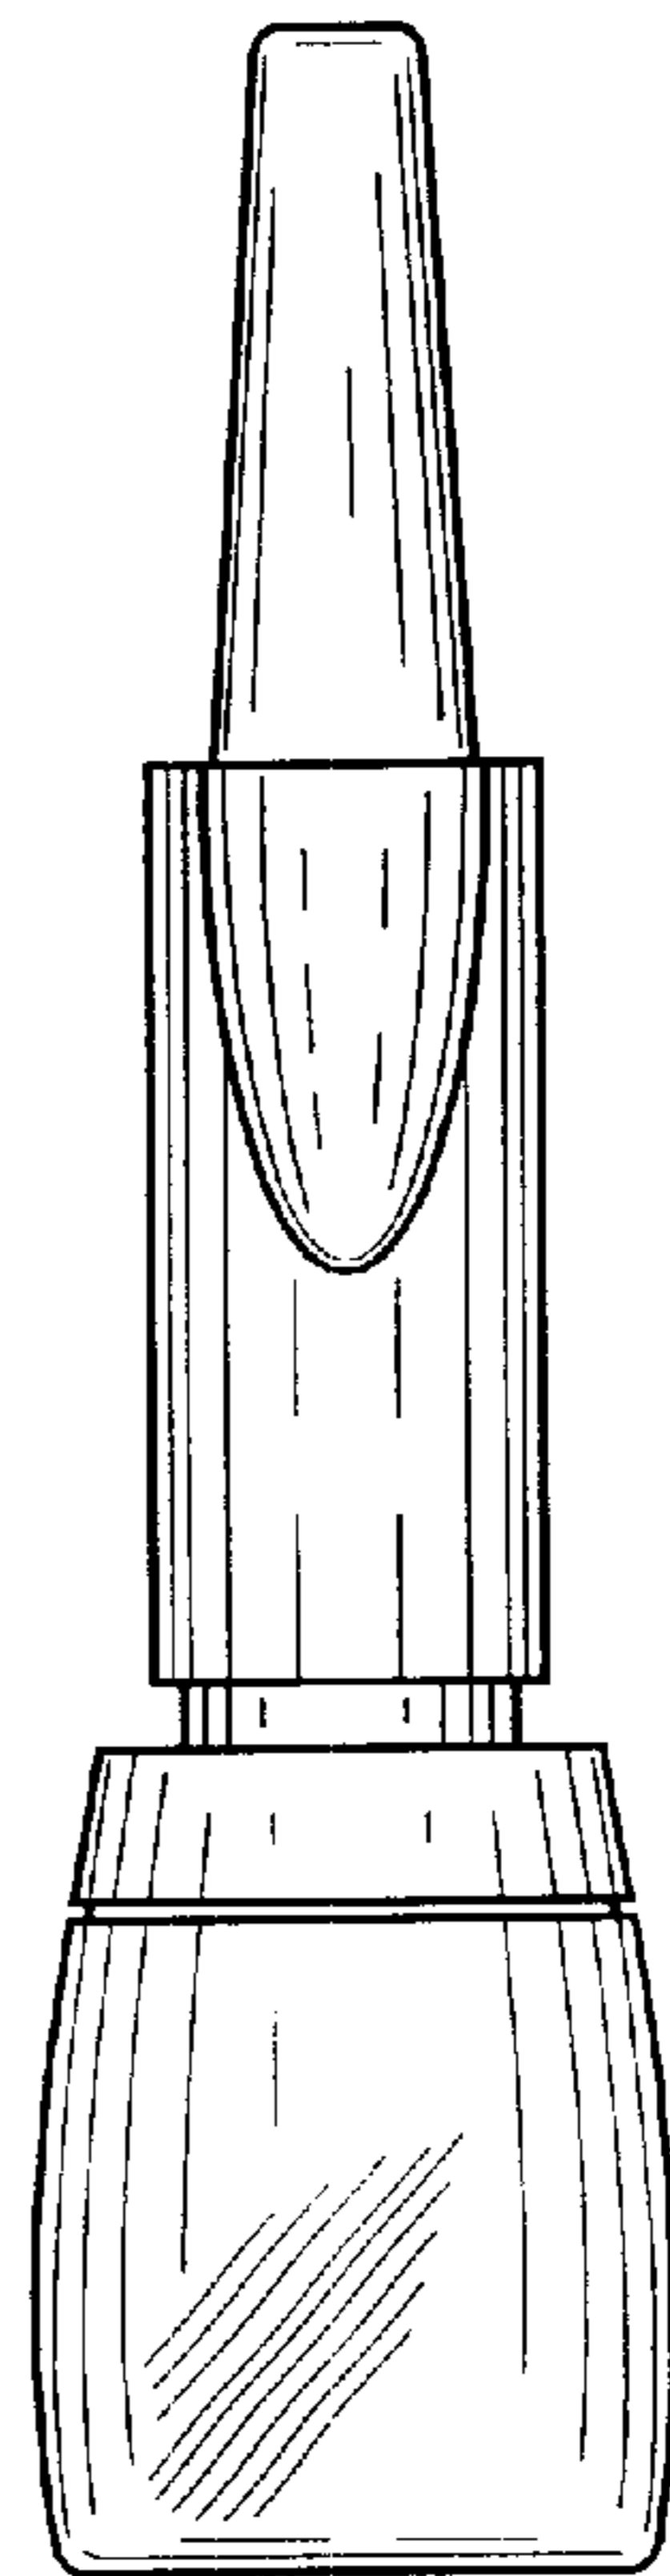


FIG. 10

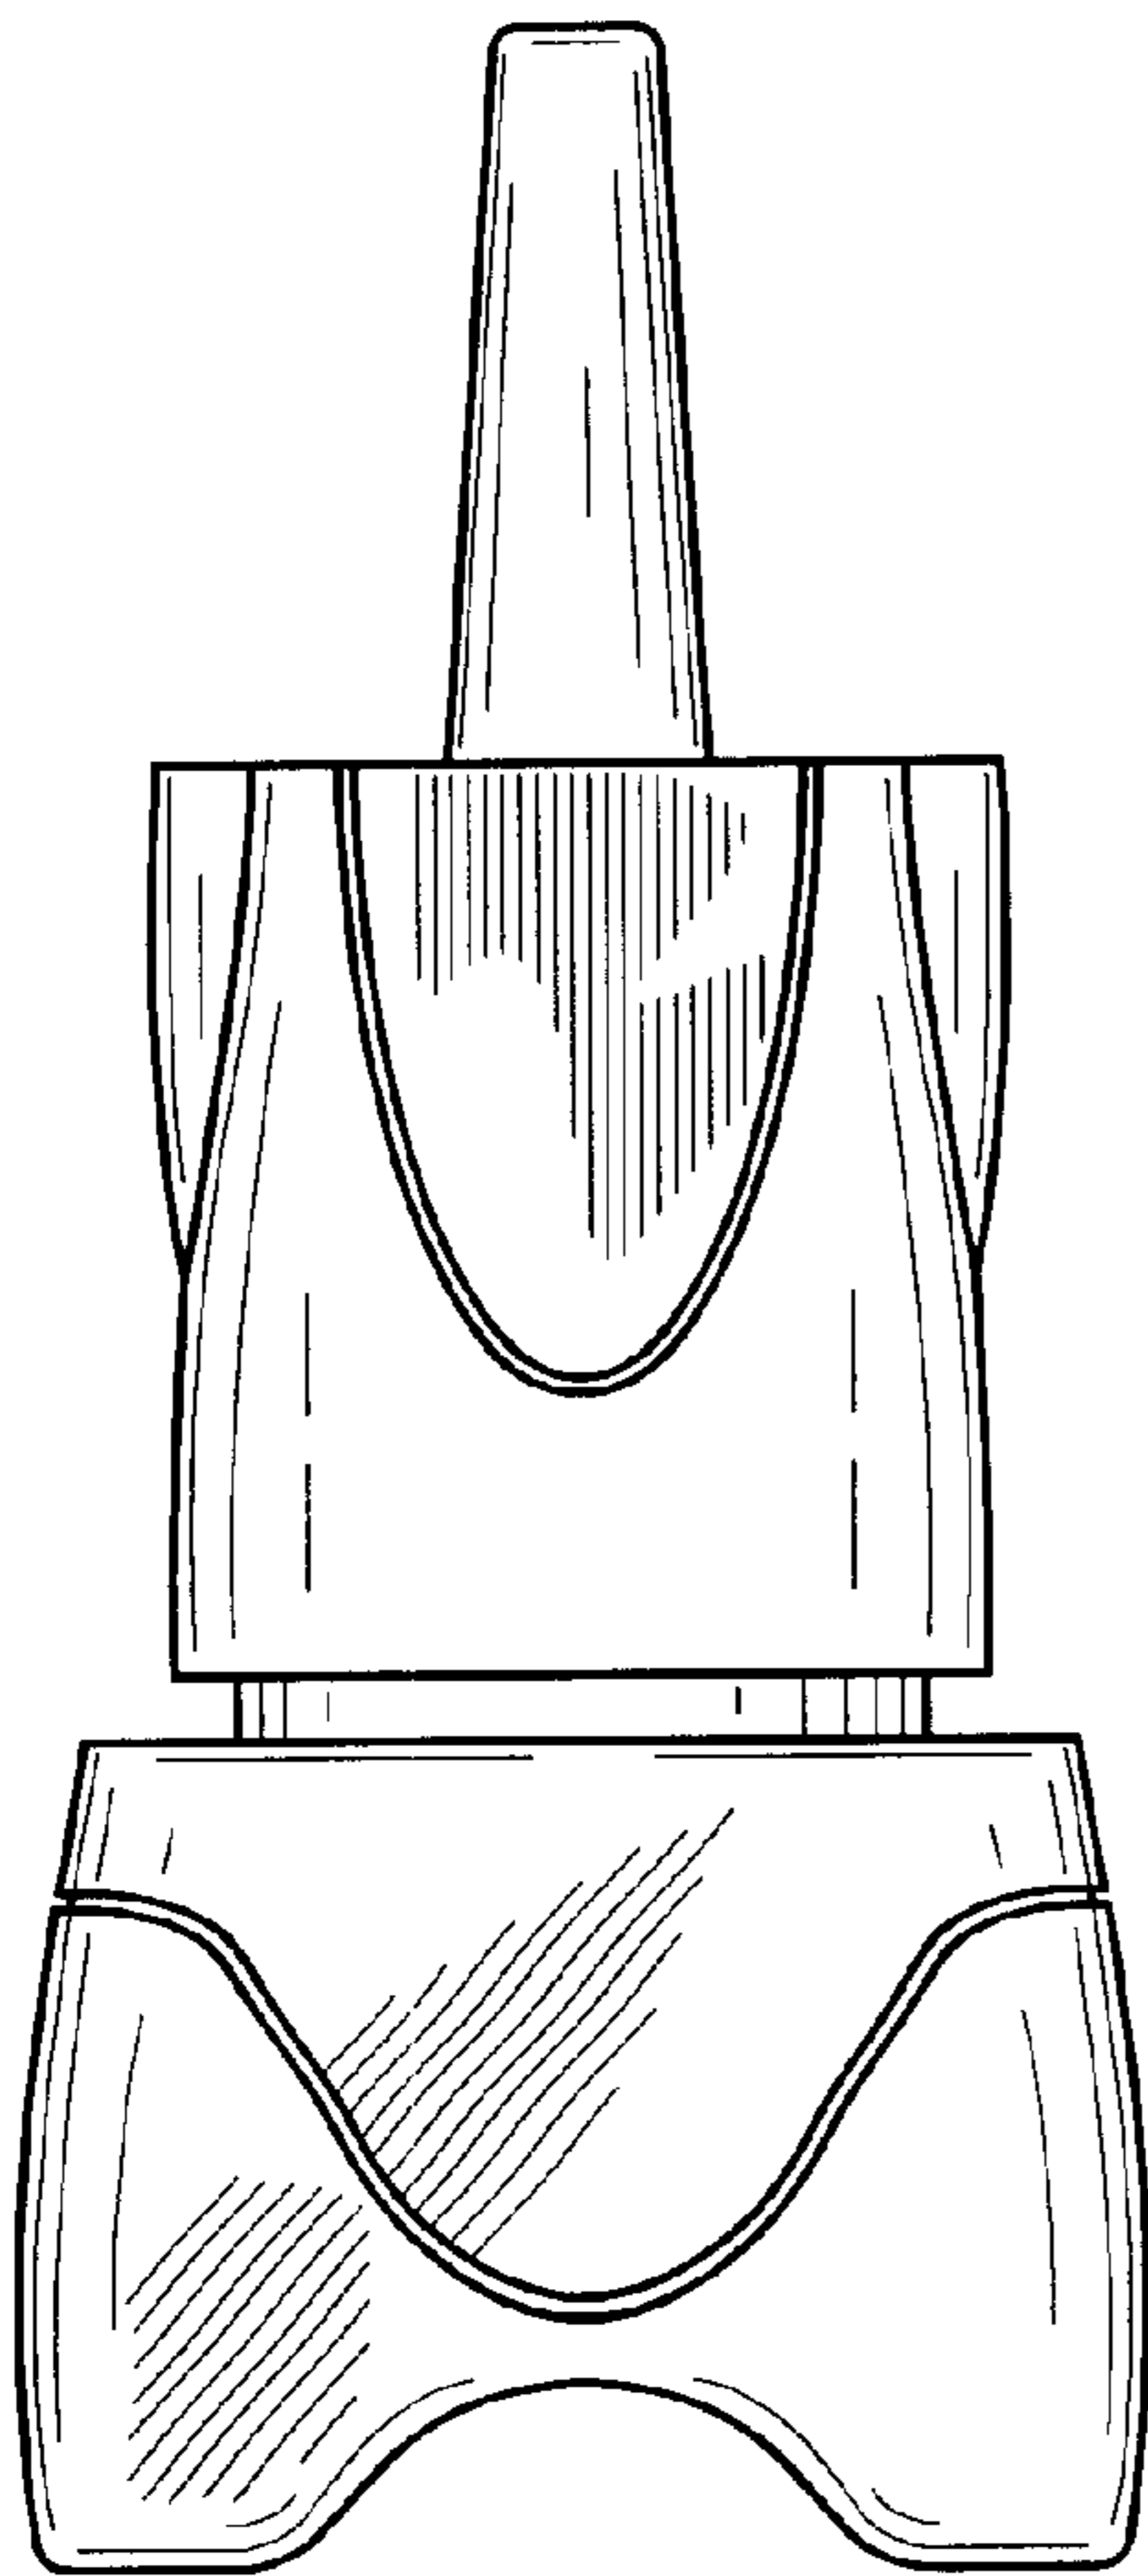


FIG. 11

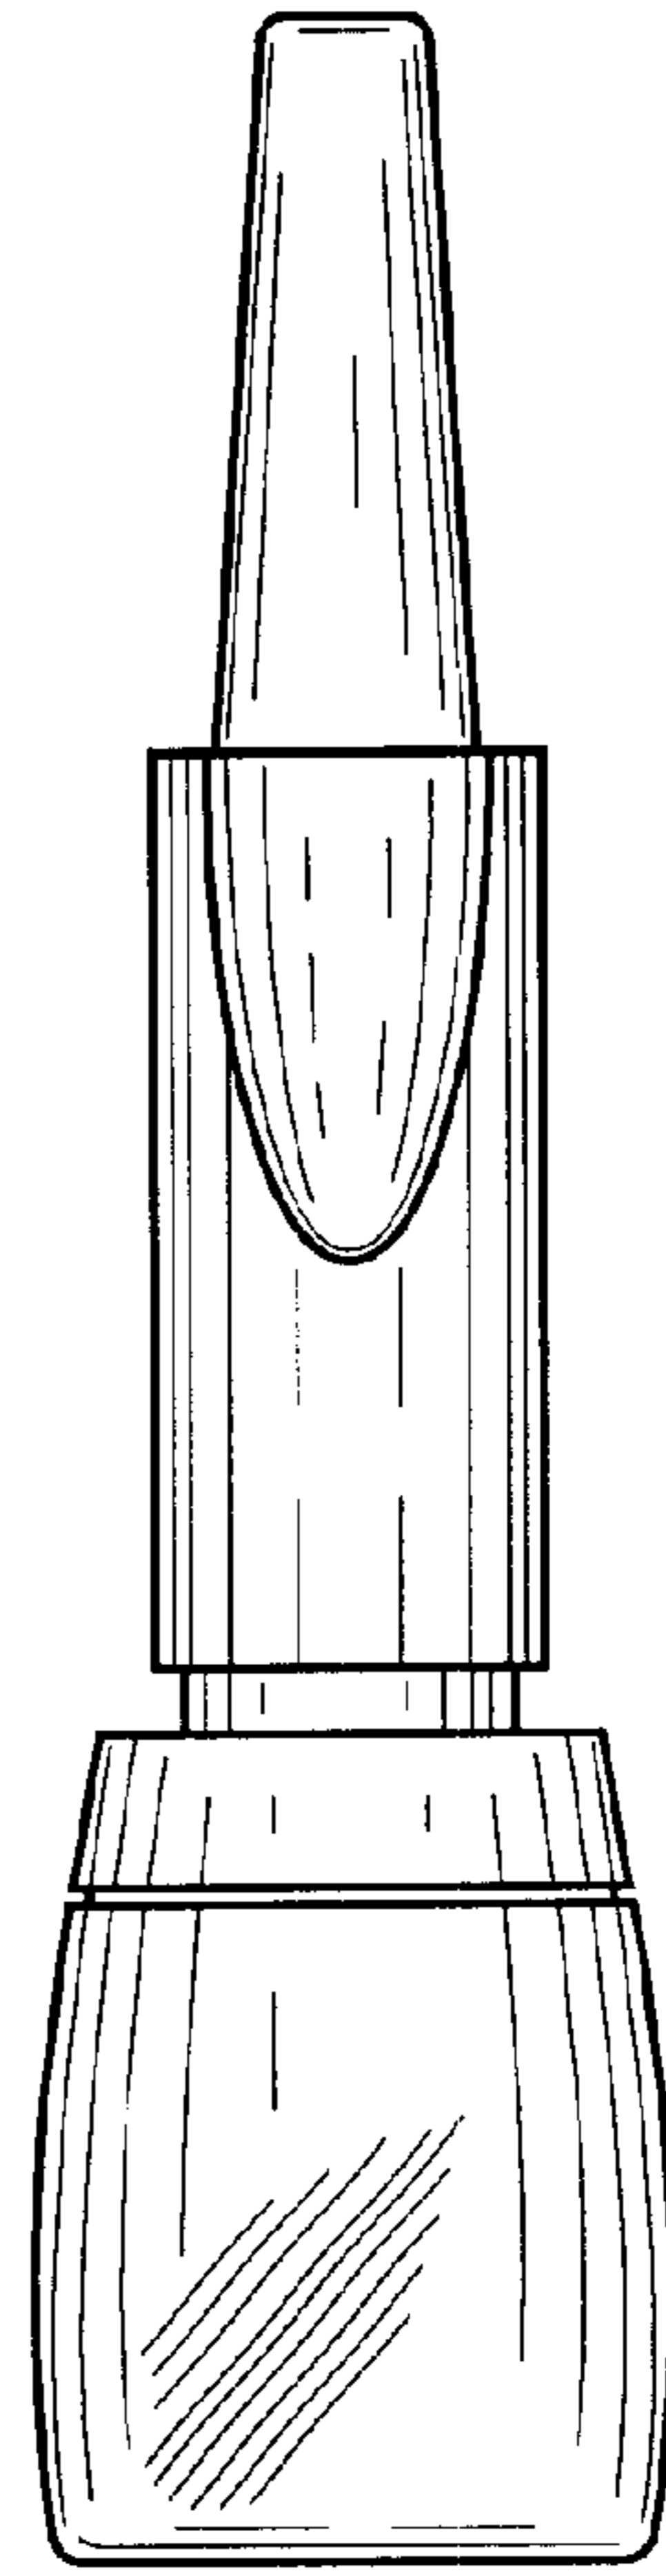


FIG. 12

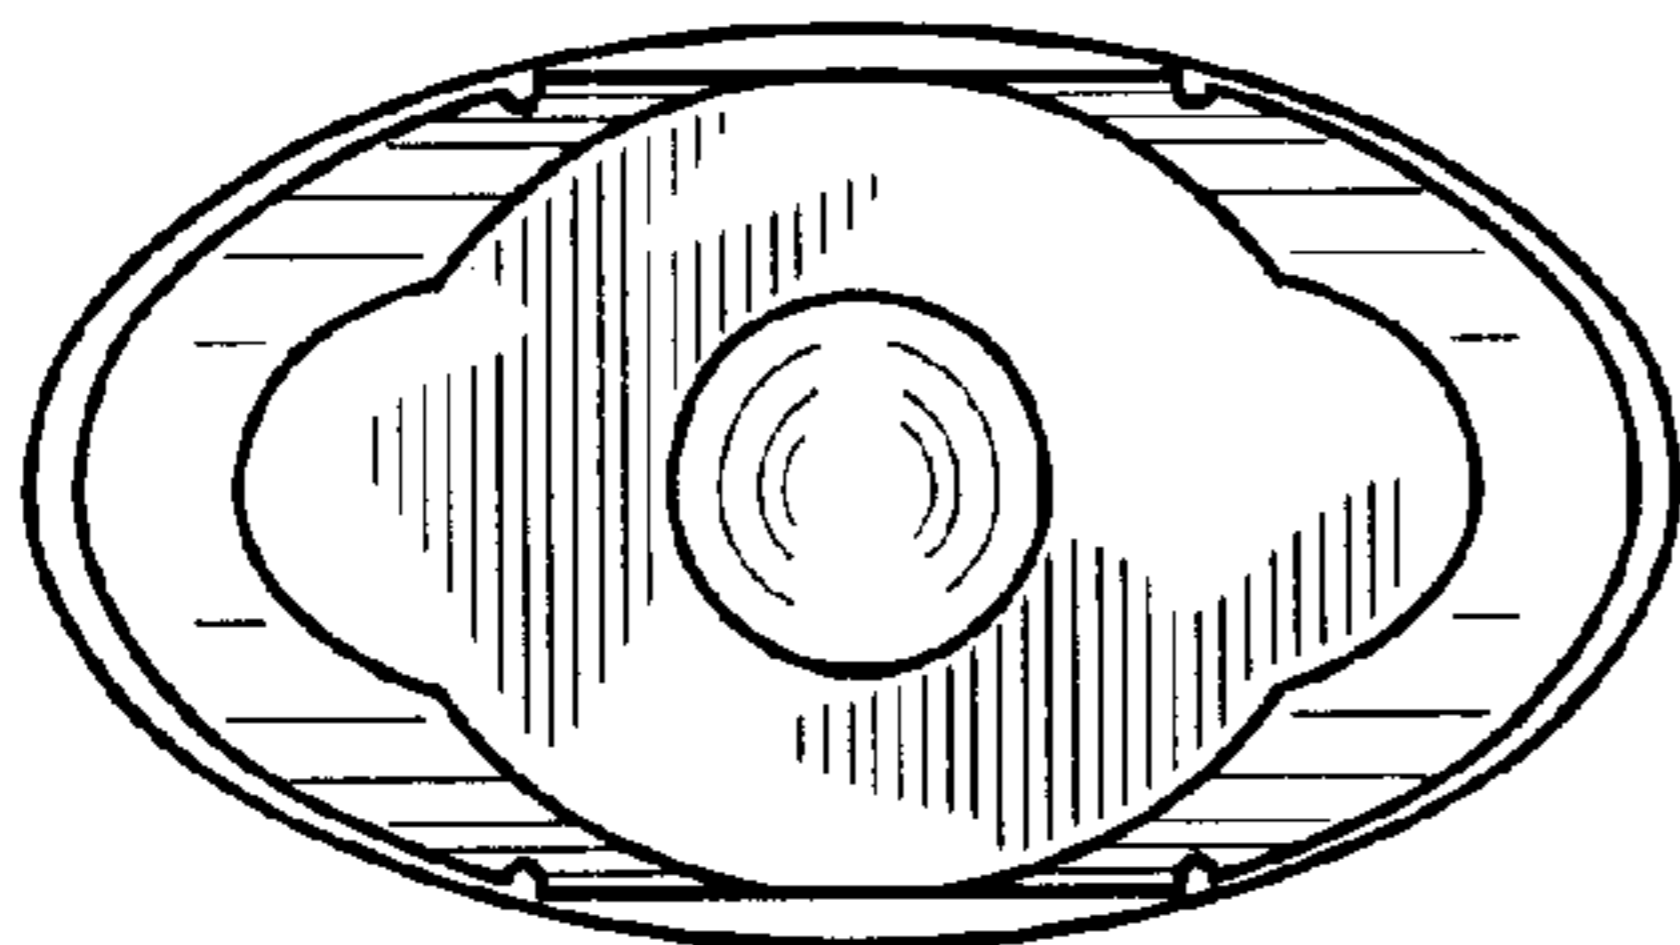


FIG. 13

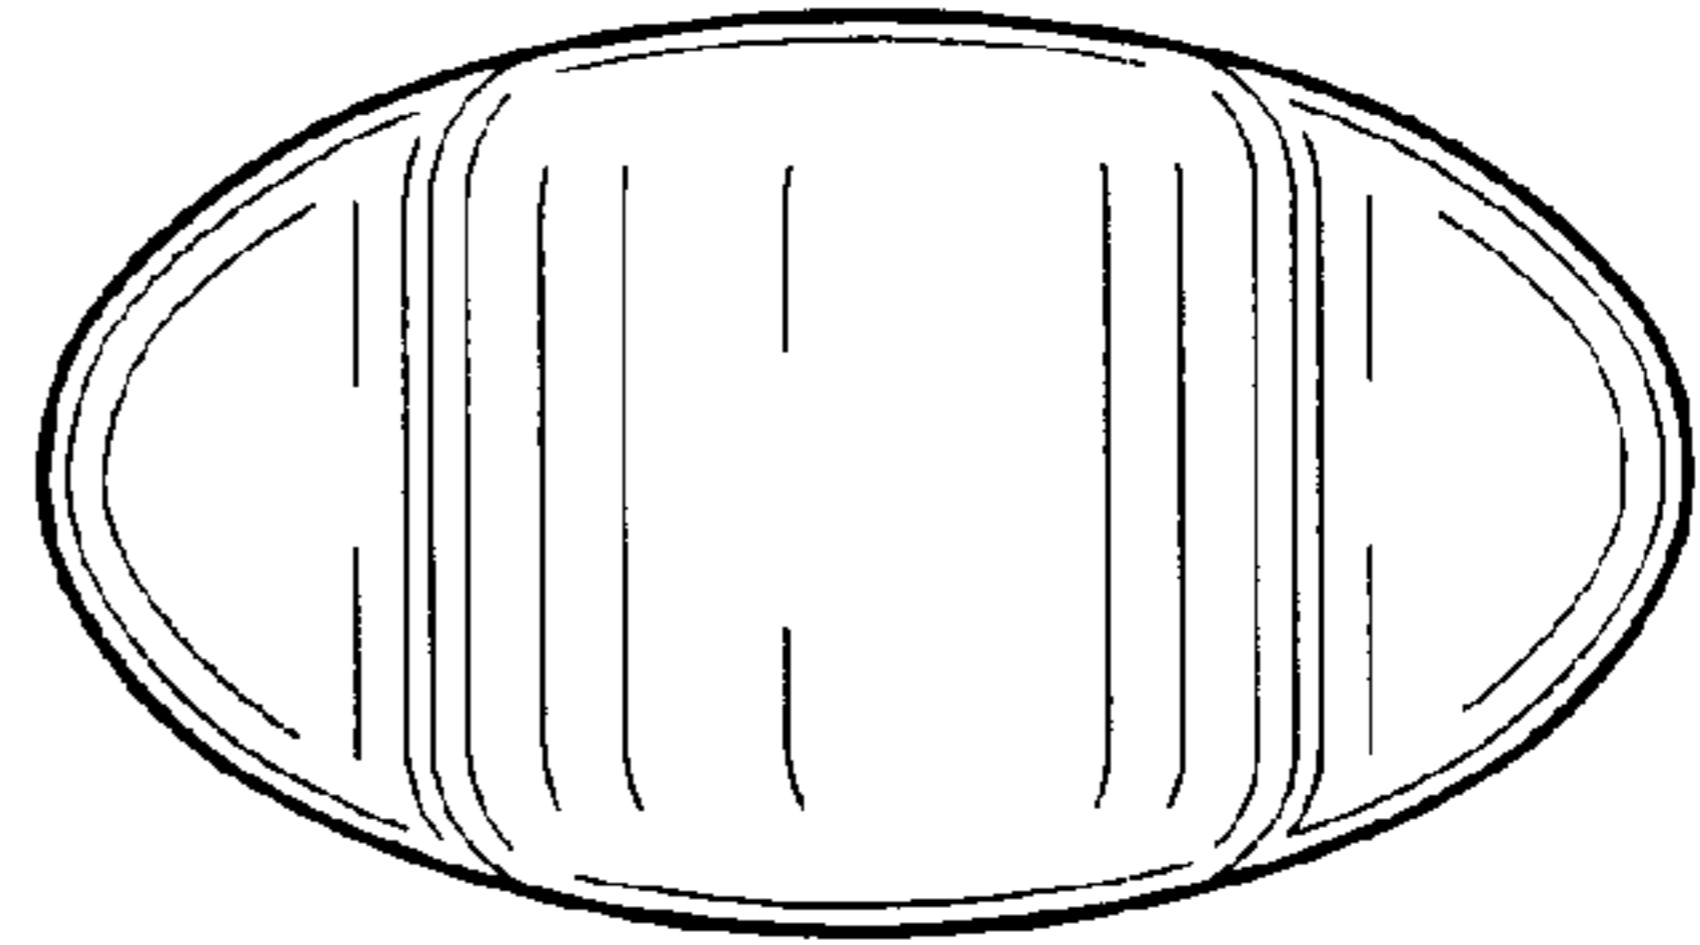


FIG. 14

UNITED STATES PATENT AND TRADEMARK OFFICE
CERTIFICATE OF CORRECTION

PATENT NO. : Des. 482,442 S
DATED : November 18, 2003
INVENTOR(S) : Gary Pasternak

Page 1 of 1

It is certified that error appears in the above-identified patent and that said Letters Patent is hereby corrected as shown below:

Title page,

Insert Item:

-- [73] Assignee: **Glaxo Group Limited**, Greenford, Middlesex (UK) --.

Signed and Sealed this

Seventh Day of February, 2006

A handwritten signature in black ink on a dotted background. The signature reads "Jon W. Dudas" in a cursive style.

JON W. DUDAS

Director of the United States Patent and Trademark Office