



US00D495049S1

(12) **United States Design Patent**
Austin

(10) **Patent No.:** **US D495,049 S**

(45) **Date of Patent:** **** Aug. 24, 2004**

(54) **OXYGEN CONSERVING REGULATOR**

6,612,307 B2 9/2003 Byrd
6,619,286 B2 * 9/2003 Patel 128/204.26

(75) **Inventor:** **Gary Austin**, Euclid, OH (US)

FOREIGN PATENT DOCUMENTS

(73) **Assignee:** **Taga Medical Technologies, Inc.**,
Eastlake, OH (US)

WO WO 97/11734 4/1997

(**) **Term:** **14 Years**

OTHER PUBLICATIONS

(21) **Appl. No.:** **29/185,301**

U.S. Byrd Patent Appln. Publication No. US 2002/0073998,
published Jun. 20, 2002 entitled "Oxygen Conserver".
U.S. Hamilton et al. Patent Appln. Publication No. US2002/
0162553, published Nov. 7, 2002 entitled "Postable Gas
Powered Positive Pressure Breathing Apparatus and
Method".

(22) **Filed:** **Jun. 24, 2003**

(51) **LOC (7) Cl.** **29-02**

(52) **U.S. Cl.** **D24/110.6**

(58) **Field of Search** D24/110.6, 129;
128/204.26, 205.24, 202.27, 205.11, 205.14,
207.16

U.S. Gale et al. Patent Appln. Publication No. US2003/
0075179, published Apr. 24, 2003, entitled "Pneumatic
Oxygen Conserving Device."

PB Puritan Bennett; "Companion® High Pressure Systems
. . . For Home Care".

PB Puritan Bennett; "Oxygen Therapy Regulators".

(56) **References Cited**

* cited by examiner

U.S. PATENT DOCUMENTS

| | | | | | |
|--------------|---|---------|-----------------|-------|-----------|
| D172,372 S | * | 6/1954 | Wagner | | D24/129 |
| D195,070 S | * | 4/1963 | Lecocq | | D24/110.6 |
| D202,319 S | * | 9/1965 | Shugarman | | D24/110.6 |
| 3,814,093 A | | 6/1974 | Gregory | | |
| 4,054,133 A | | 10/1977 | Myers | | |
| 4,328,798 A | | 5/1982 | Isaacson | | |
| 4,827,964 A | | 5/1989 | Guido et al. | | |
| 5,020,531 A | | 6/1991 | Garofalo | | |
| 5,275,153 A | | 1/1994 | Kay | | |
| 5,360,000 A | | 11/1994 | Garter | | |
| 5,645,055 A | | 7/1997 | Danon | | |
| 5,743,257 A | | 4/1998 | Koehler et al. | | |
| 5,755,224 A | | 5/1998 | Good et al. | | |
| 5,881,725 A | | 3/1999 | Hoffman et al. | | |
| D409,745 S | * | 5/1999 | Niemczyk | | D24/110.6 |
| D418,599 S | * | 1/2000 | McCombs et al. | | D24/110.6 |
| 6,116,242 A | | 9/2000 | Frye et al. | | |
| 6,364,161 B1 | | 4/2002 | Pryor | | |
| 6,378,520 B1 | | 4/2002 | Davenport | | |
| 6,394,088 B1 | | 5/2002 | Frye et al. | | |
| 6,425,396 B1 | | 7/2002 | Adriance et al. | | |
| 6,427,690 B1 | | 8/2002 | McCombs et al. | | |

Primary Examiner—Ian Simmons

(74) *Attorney, Agent, or Firm*—Pearne & Gordon LLP

(57) **CLAIM**

The ornamental design for a oxygen conserving regulator, as shown and described.

DESCRIPTION

FIG. 1 is a first perspective view of my new oxygen conserving regulator;
FIG. 2 is a second perspective view thereof;
FIG. 3 is a front view thereof;
FIG. 4 is a top view thereof;
FIG. 5 is a left side view thereof;
FIG. 6 is a right side view thereof;
FIG. 7 is a bottom view thereof; and,
FIG. 8 is a rear view thereof.

1 Claim, 4 Drawing Sheets

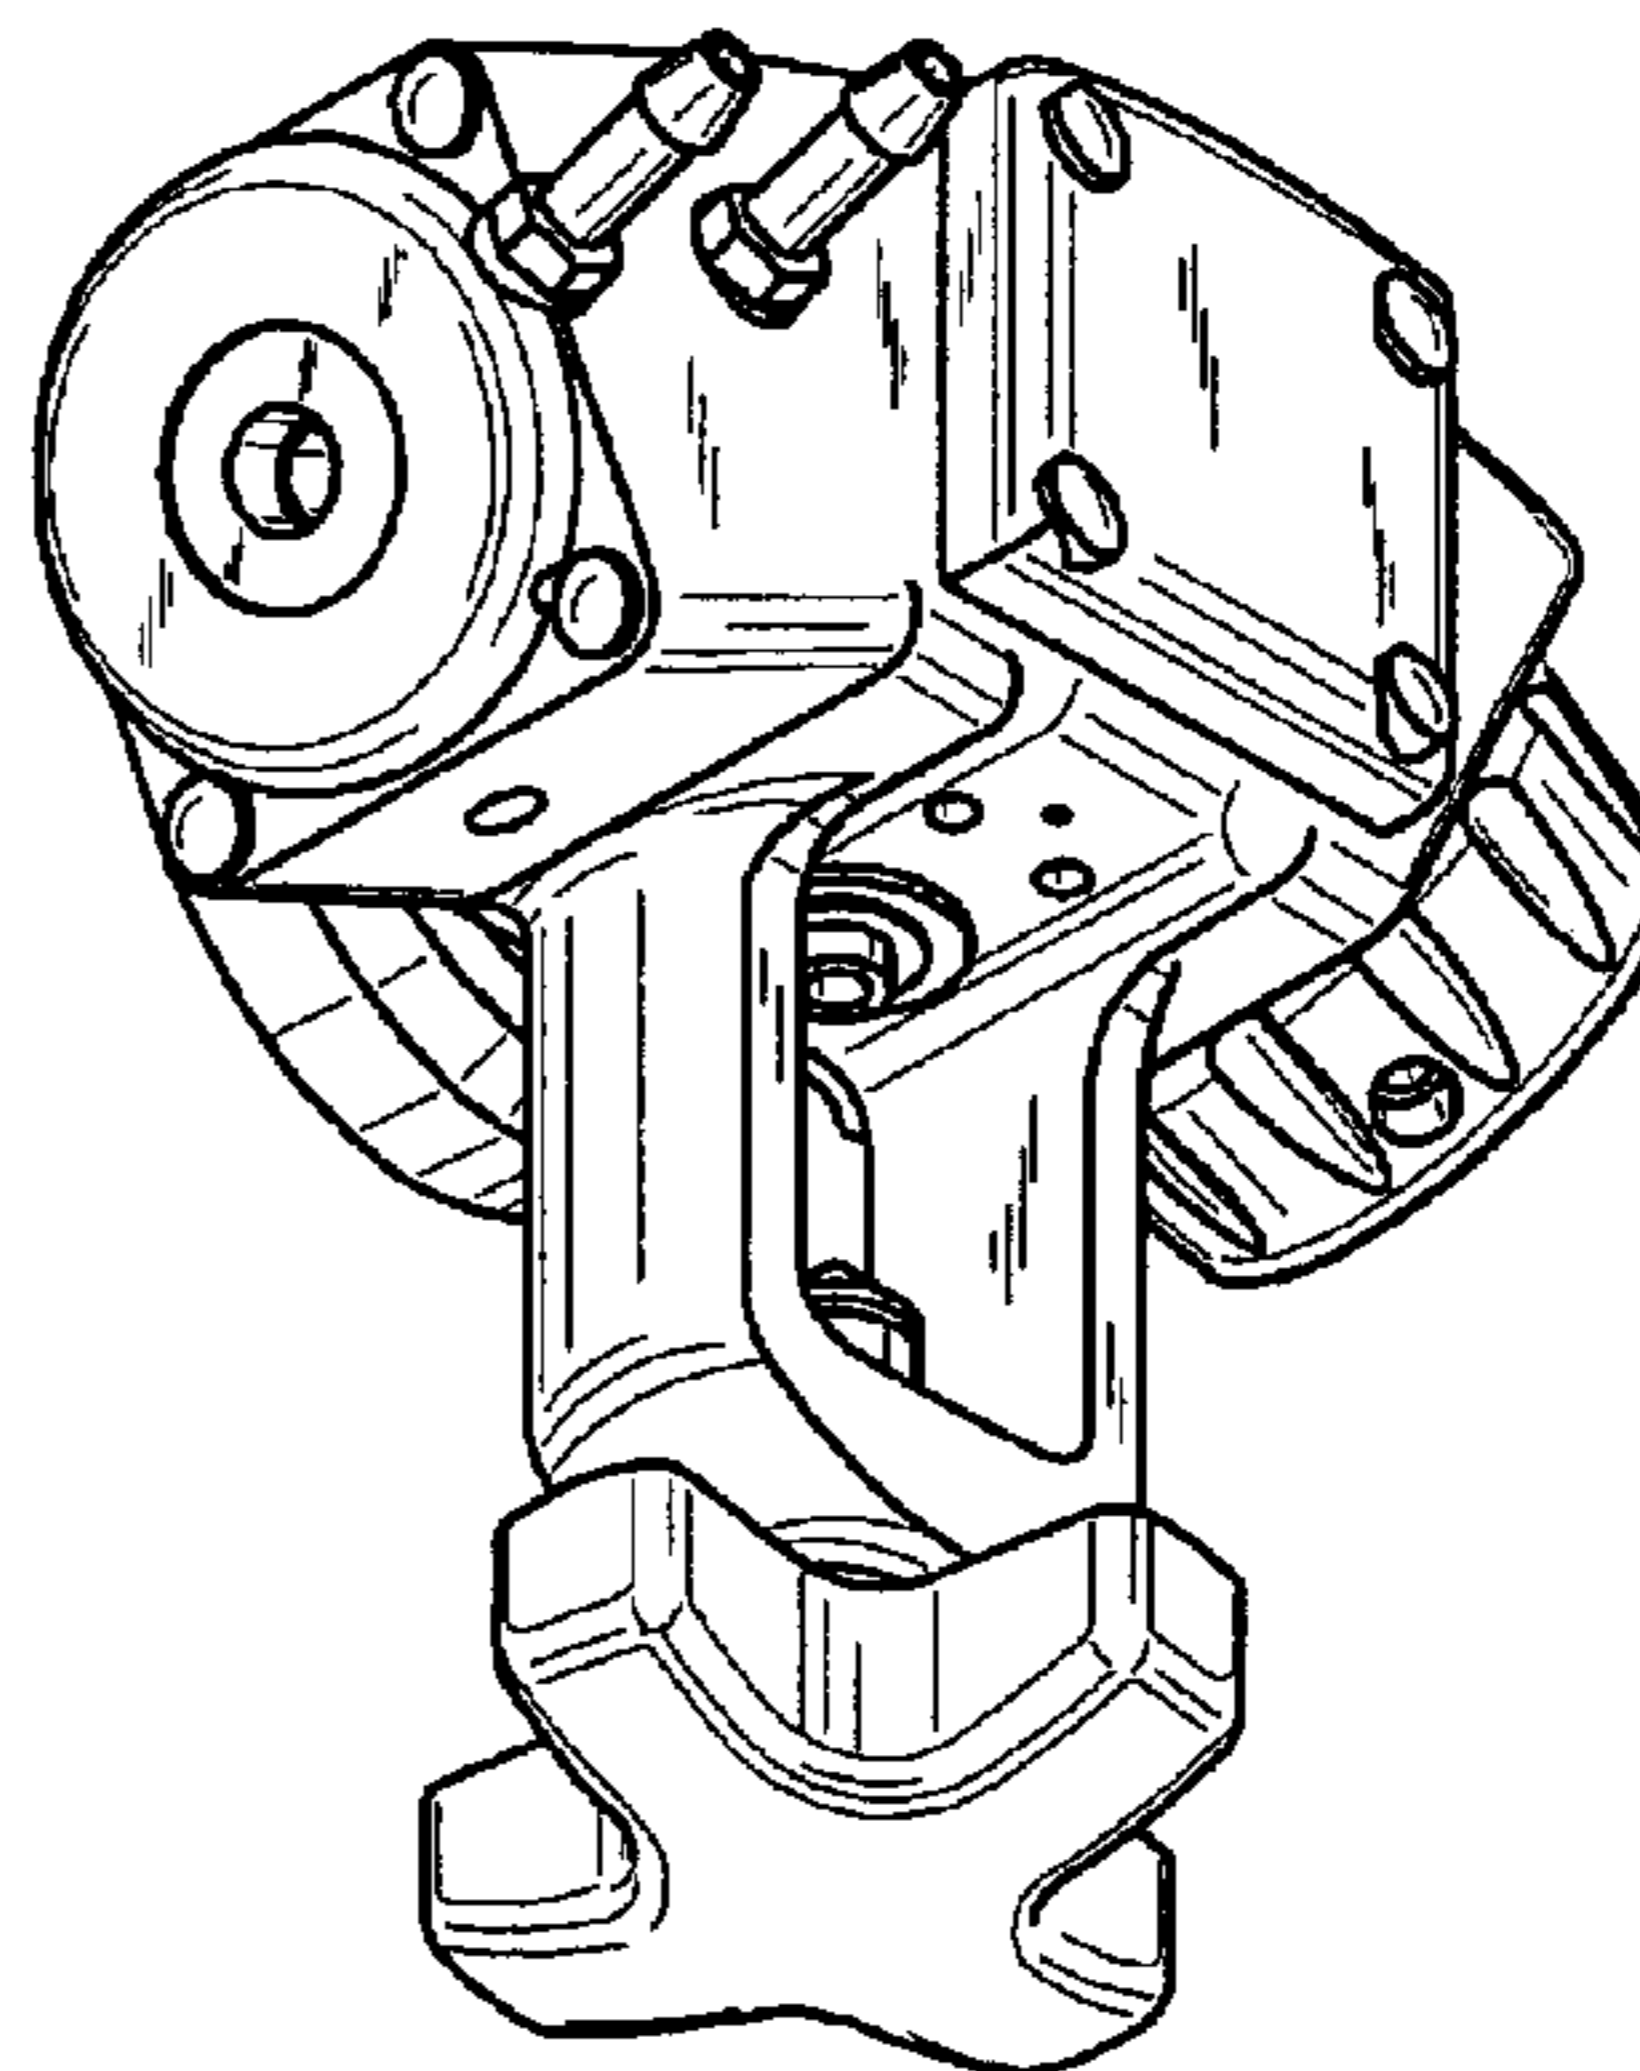
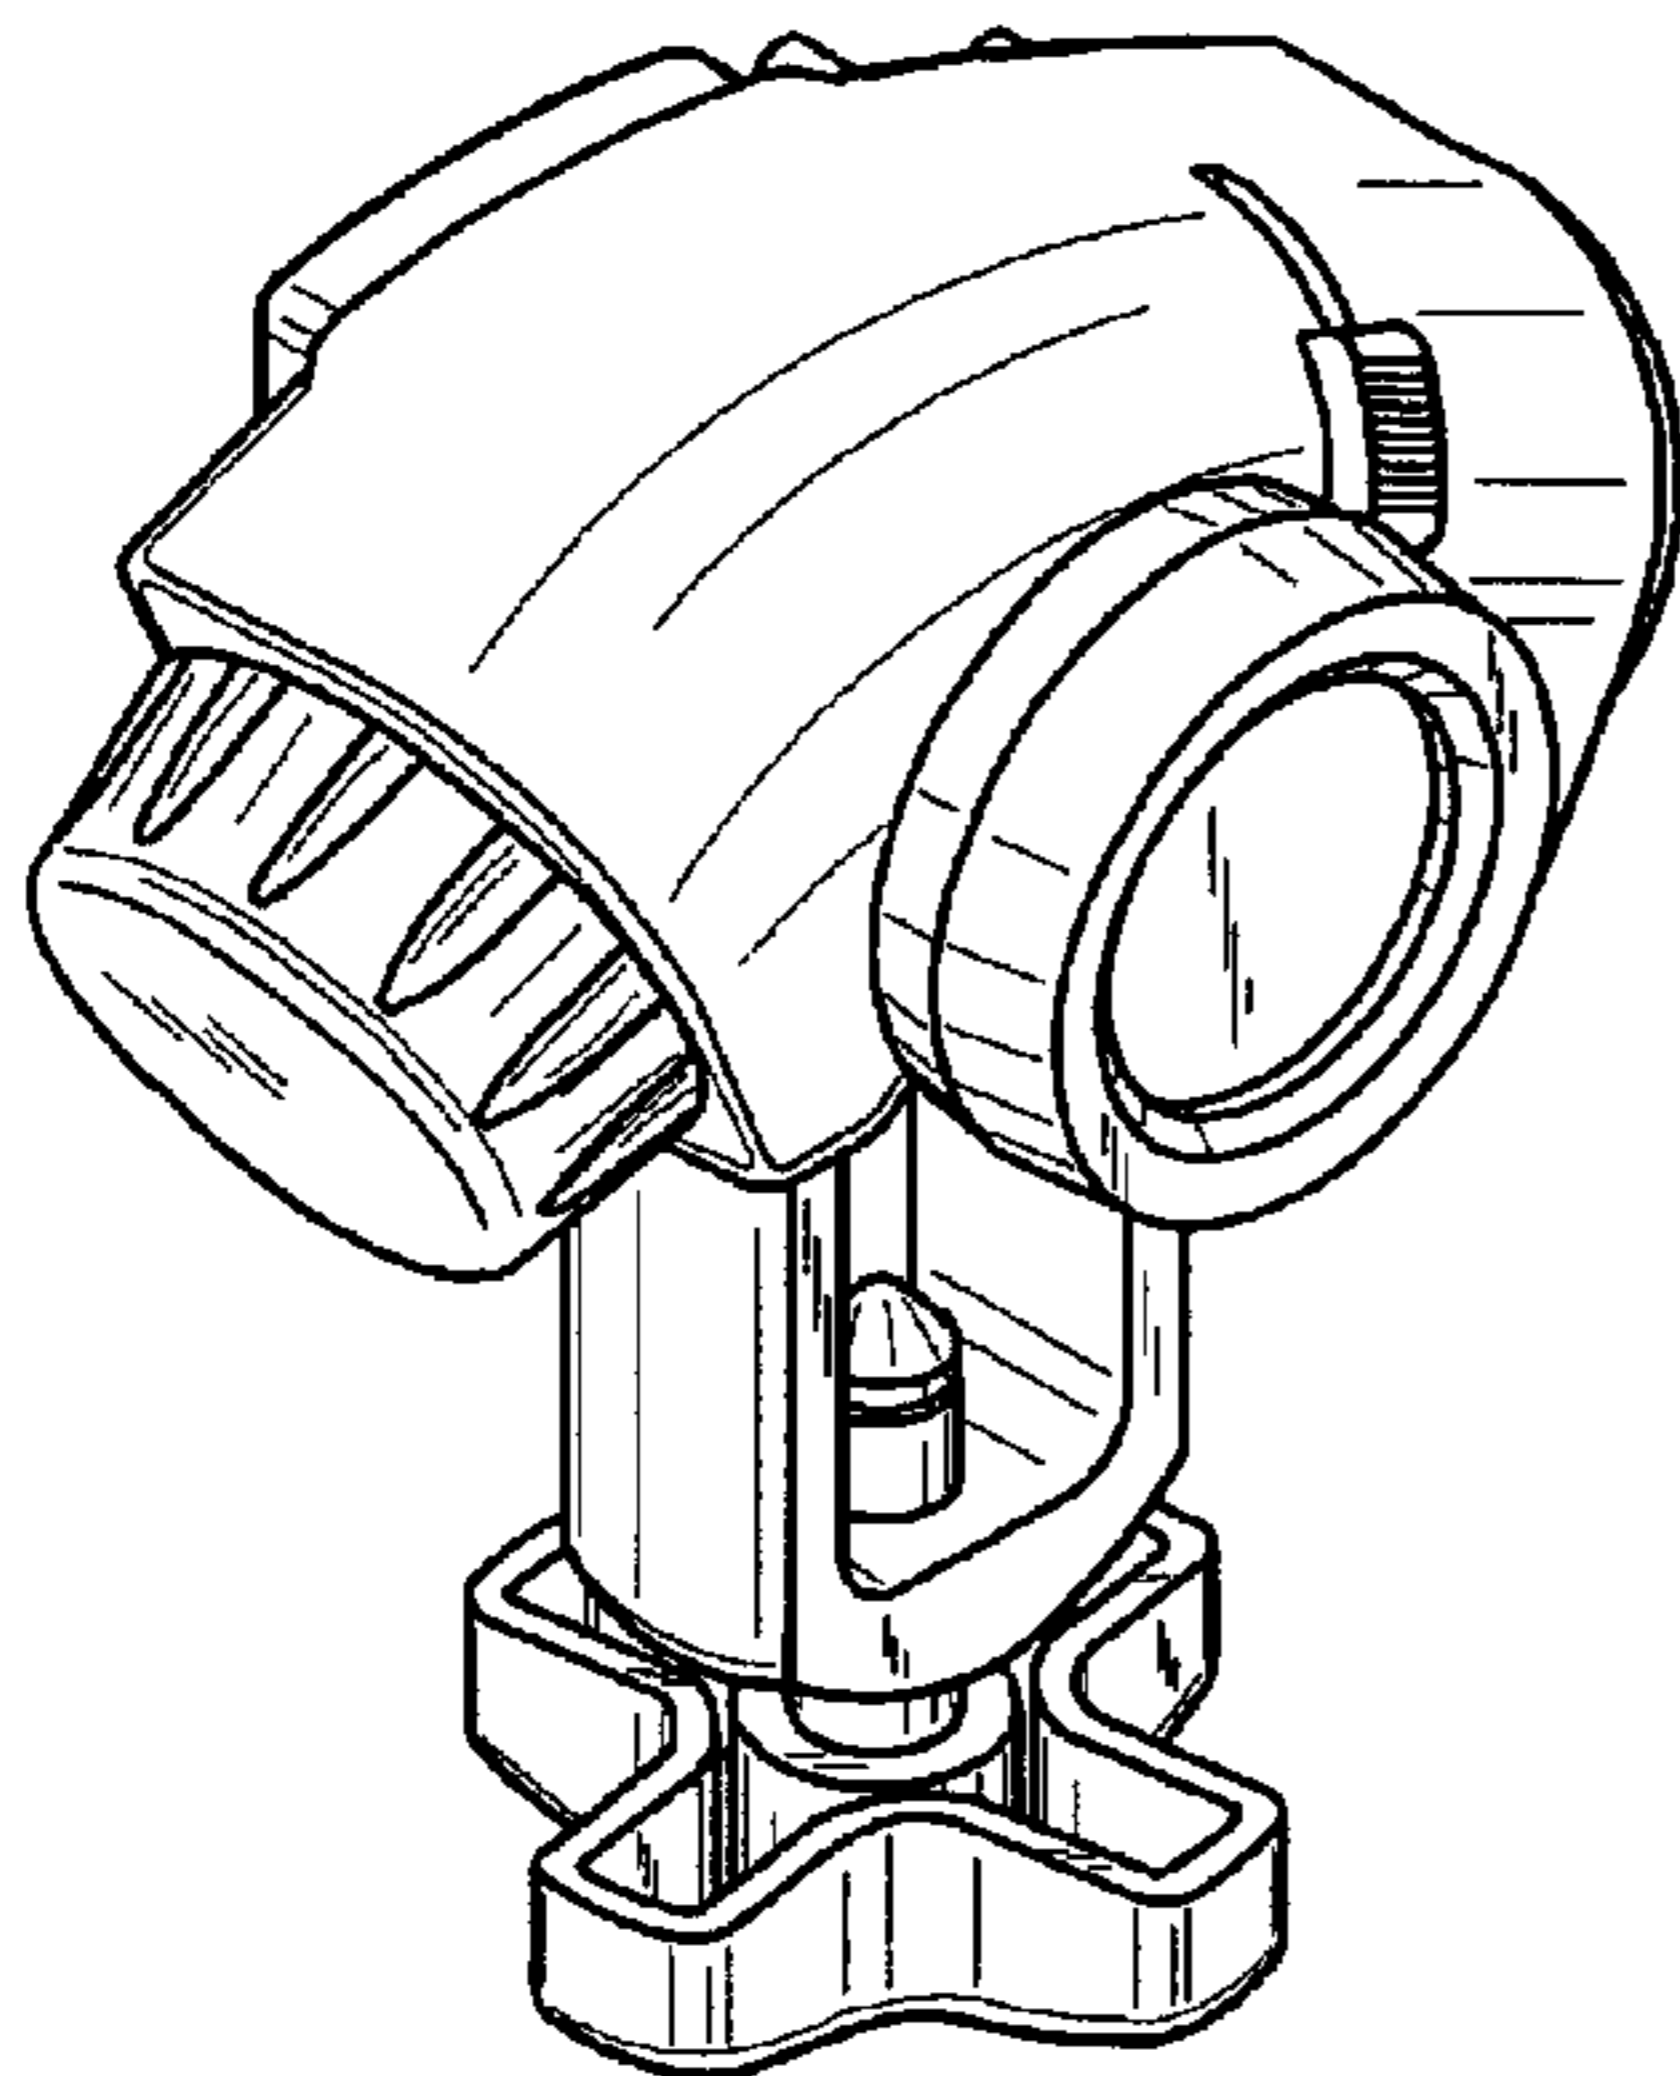


FIG. 1

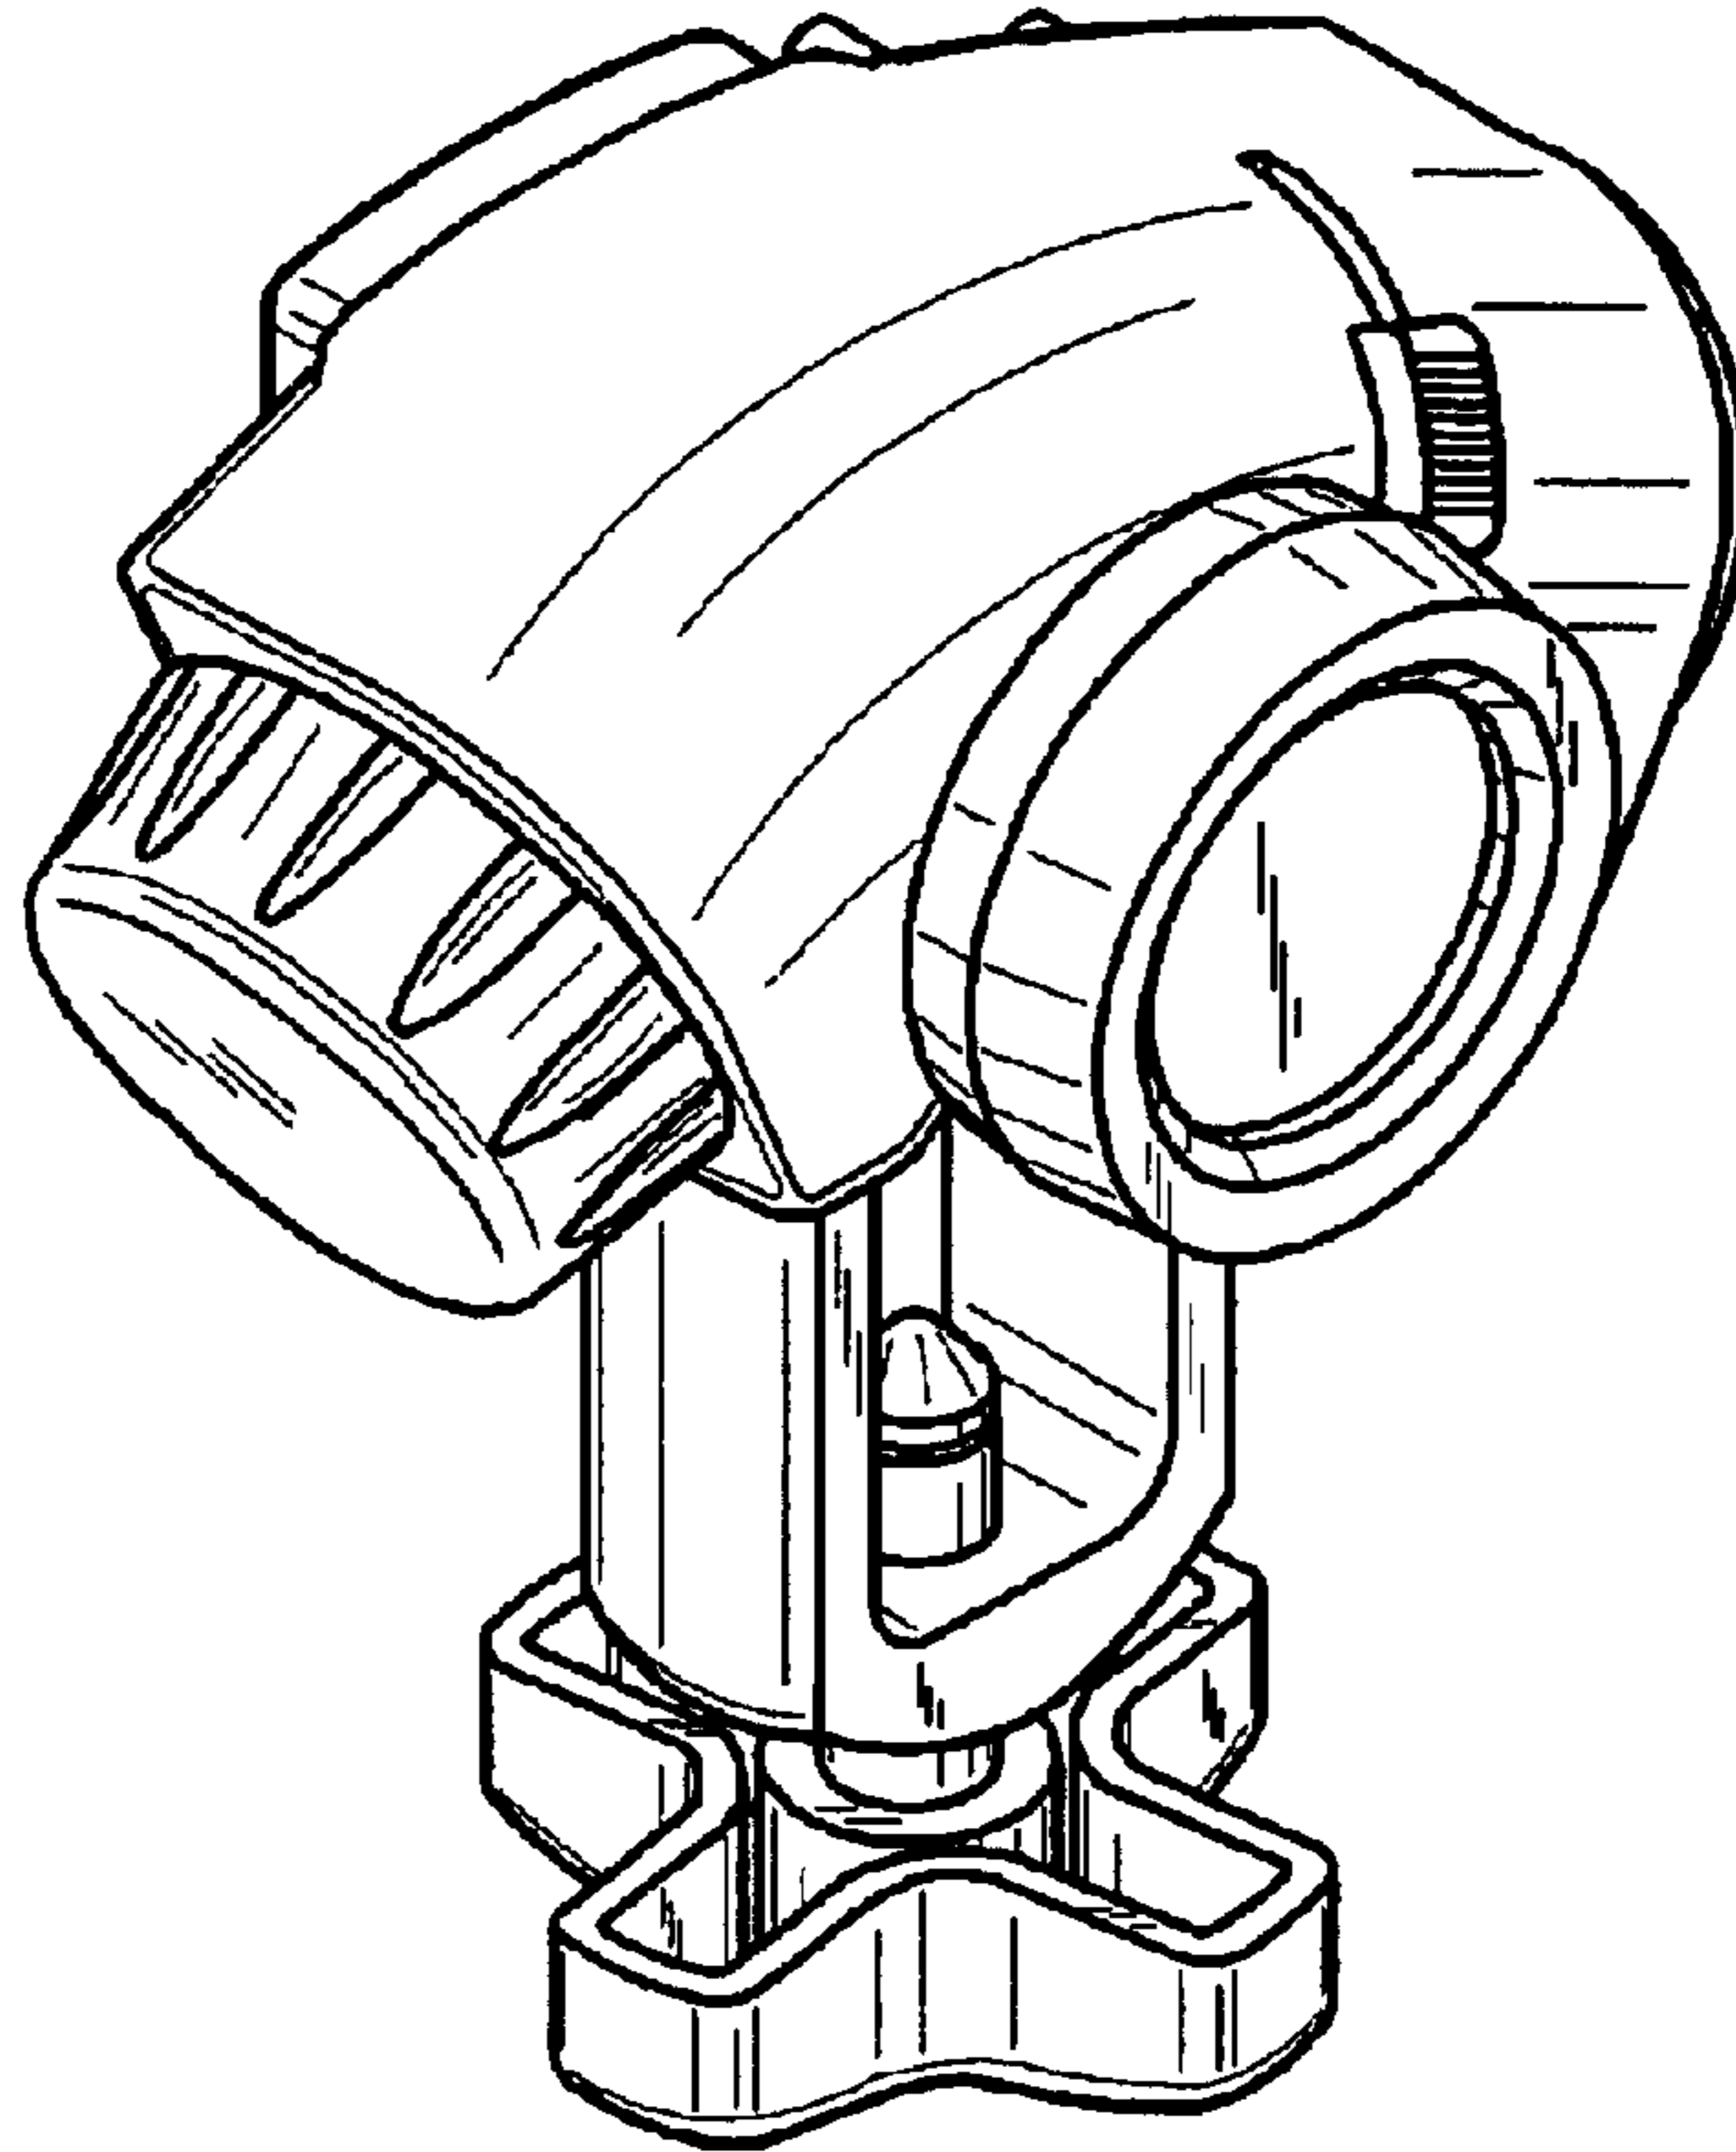
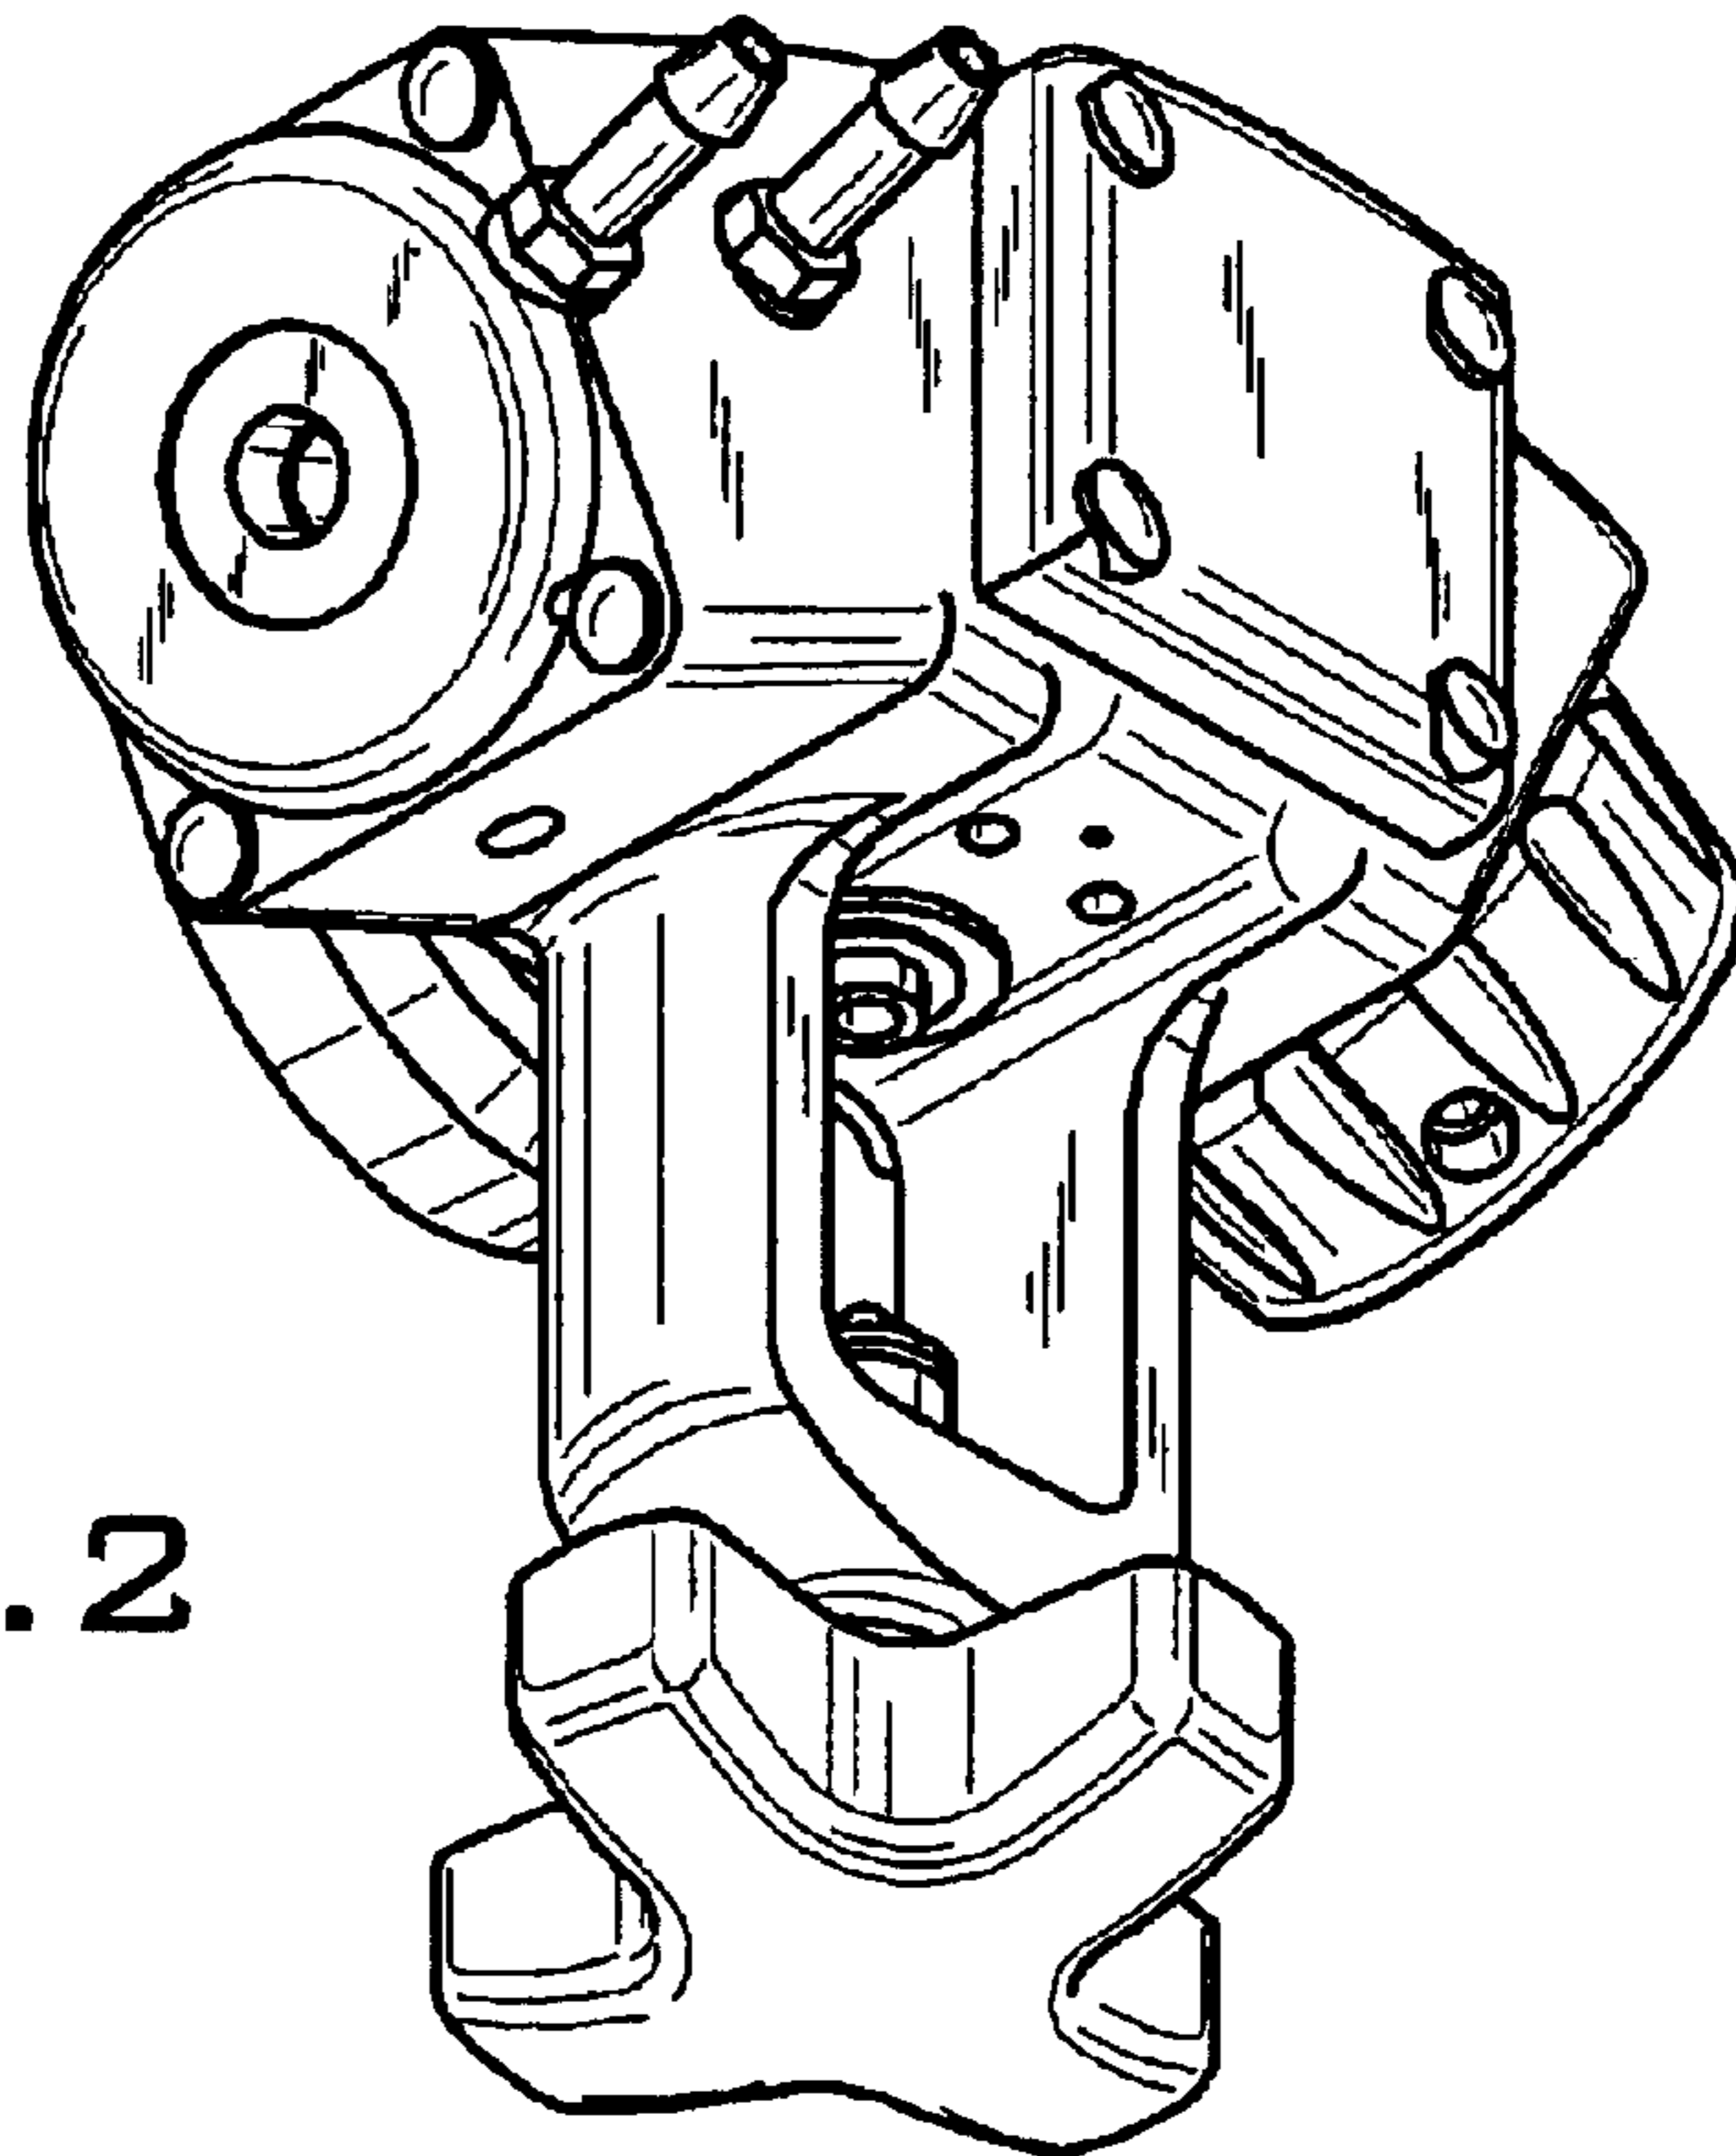


FIG. 2



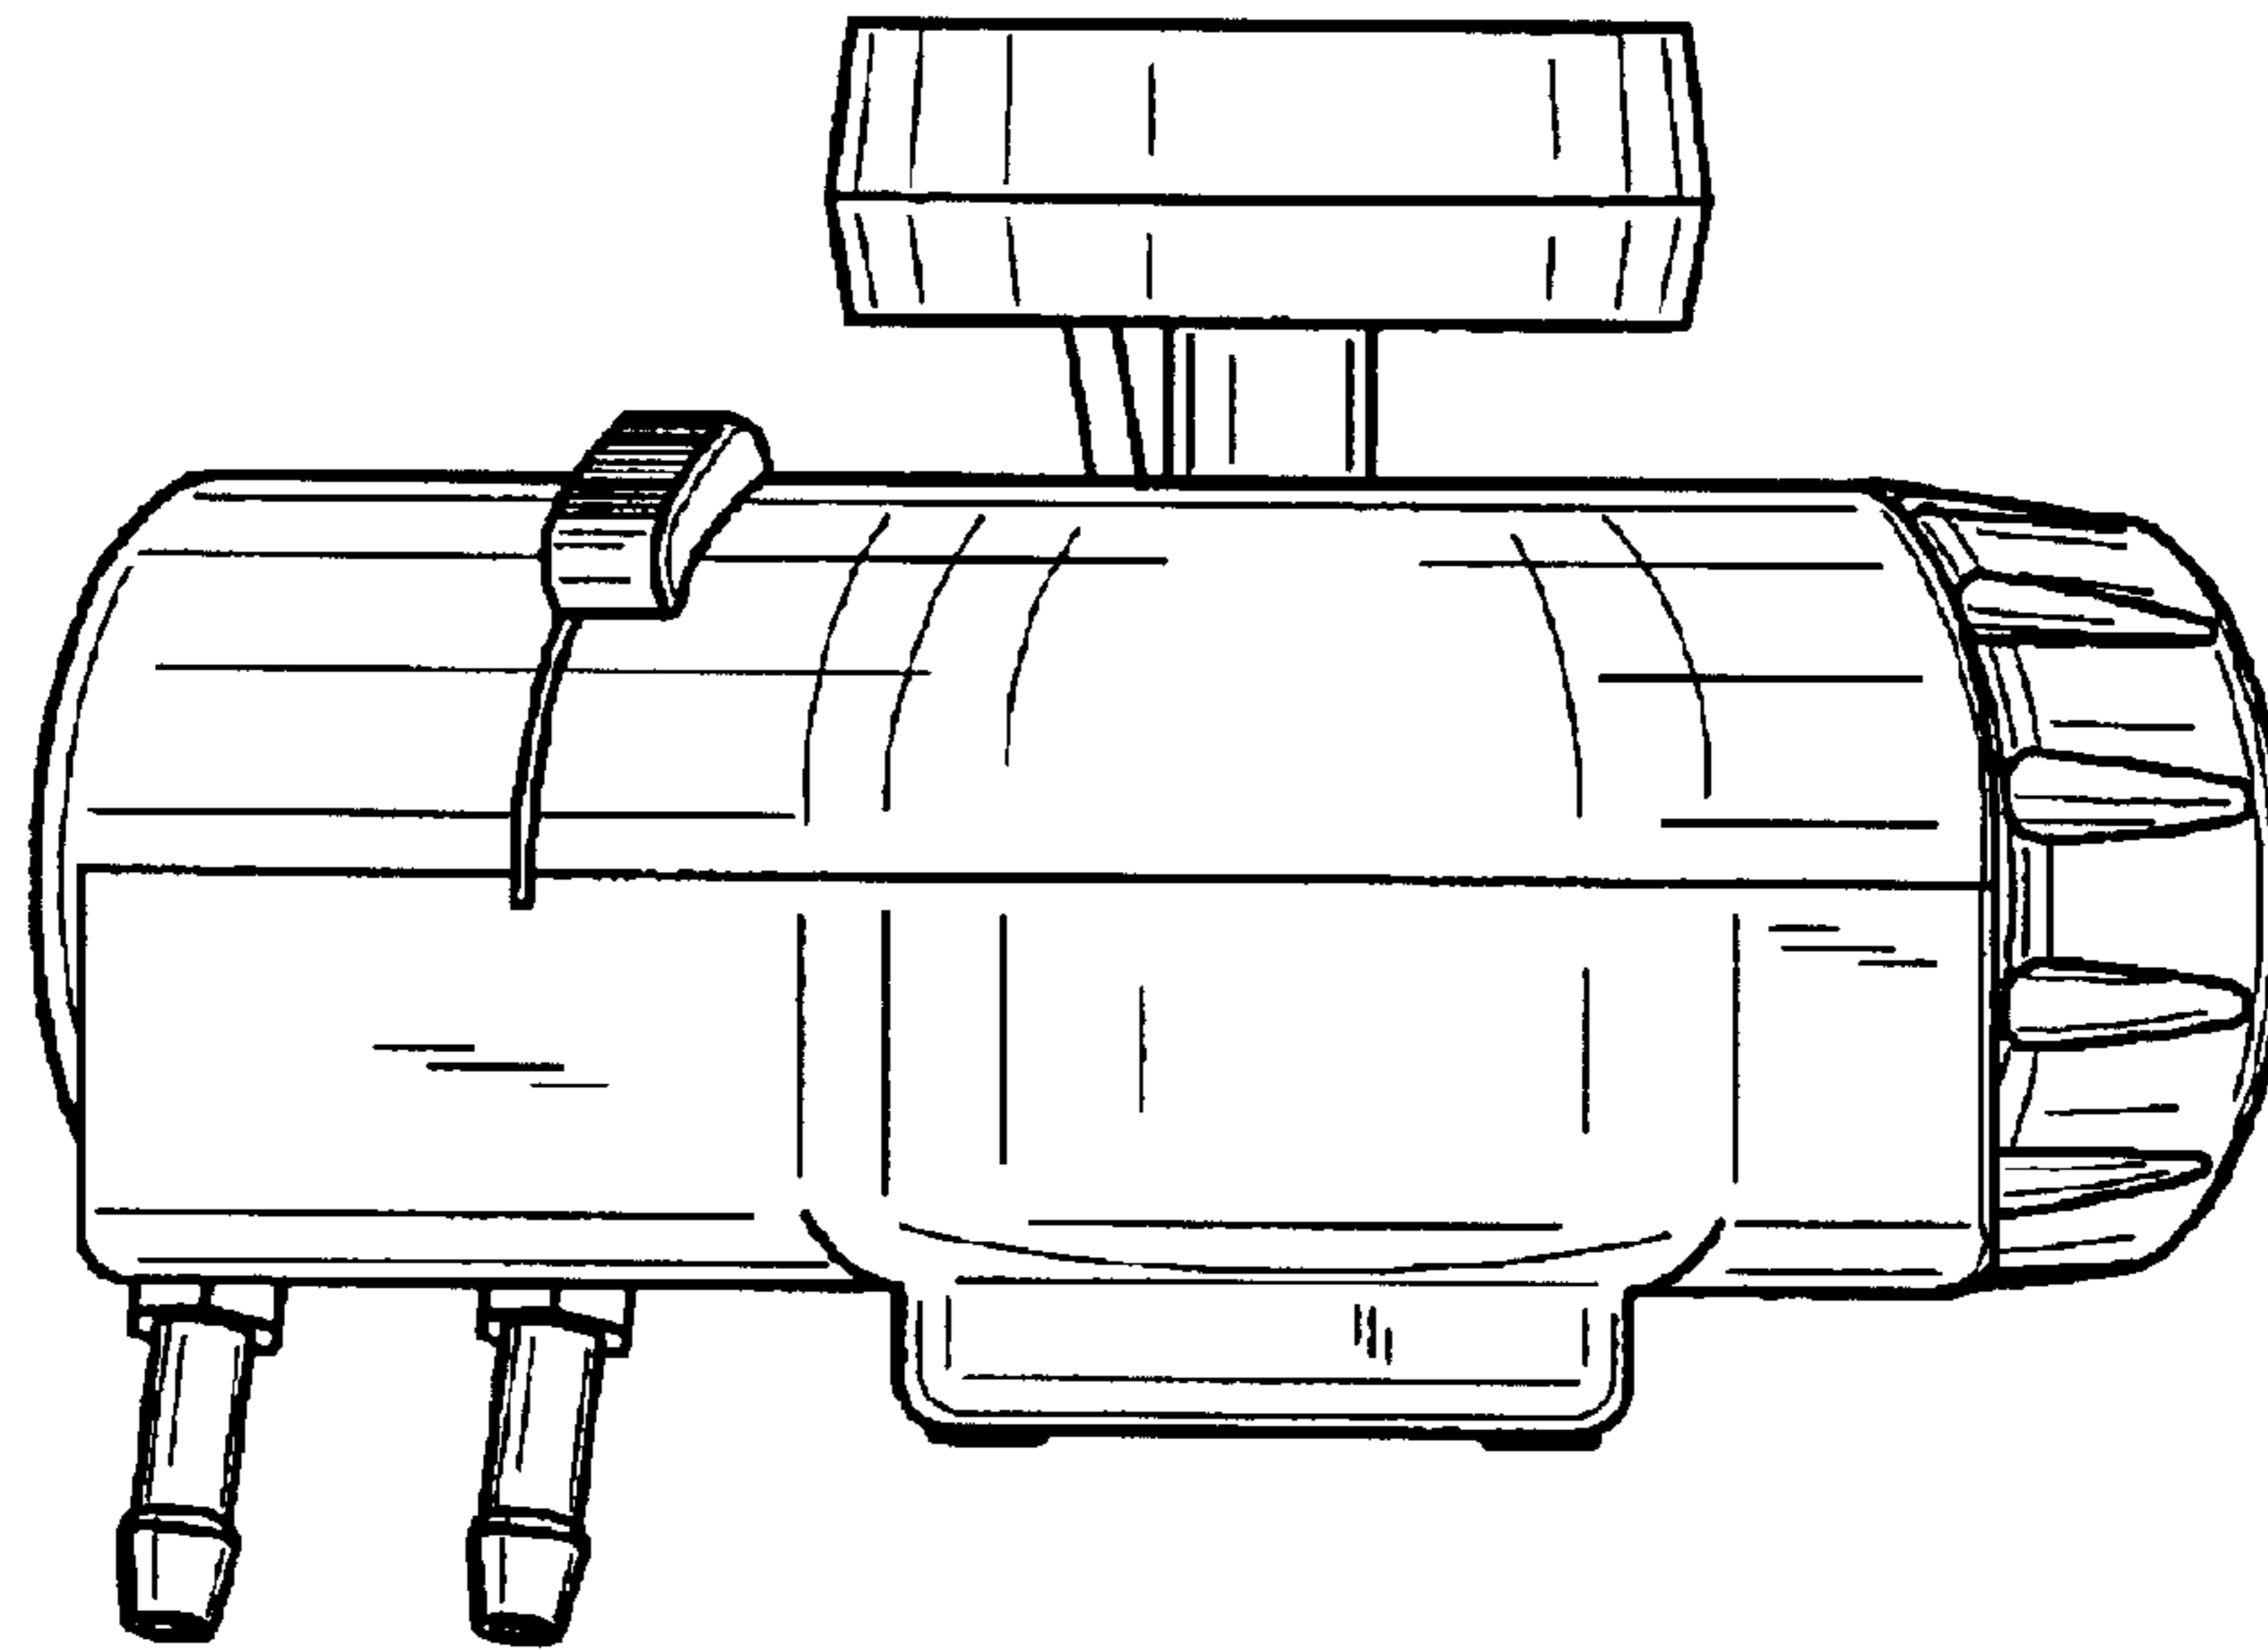


FIG. 3

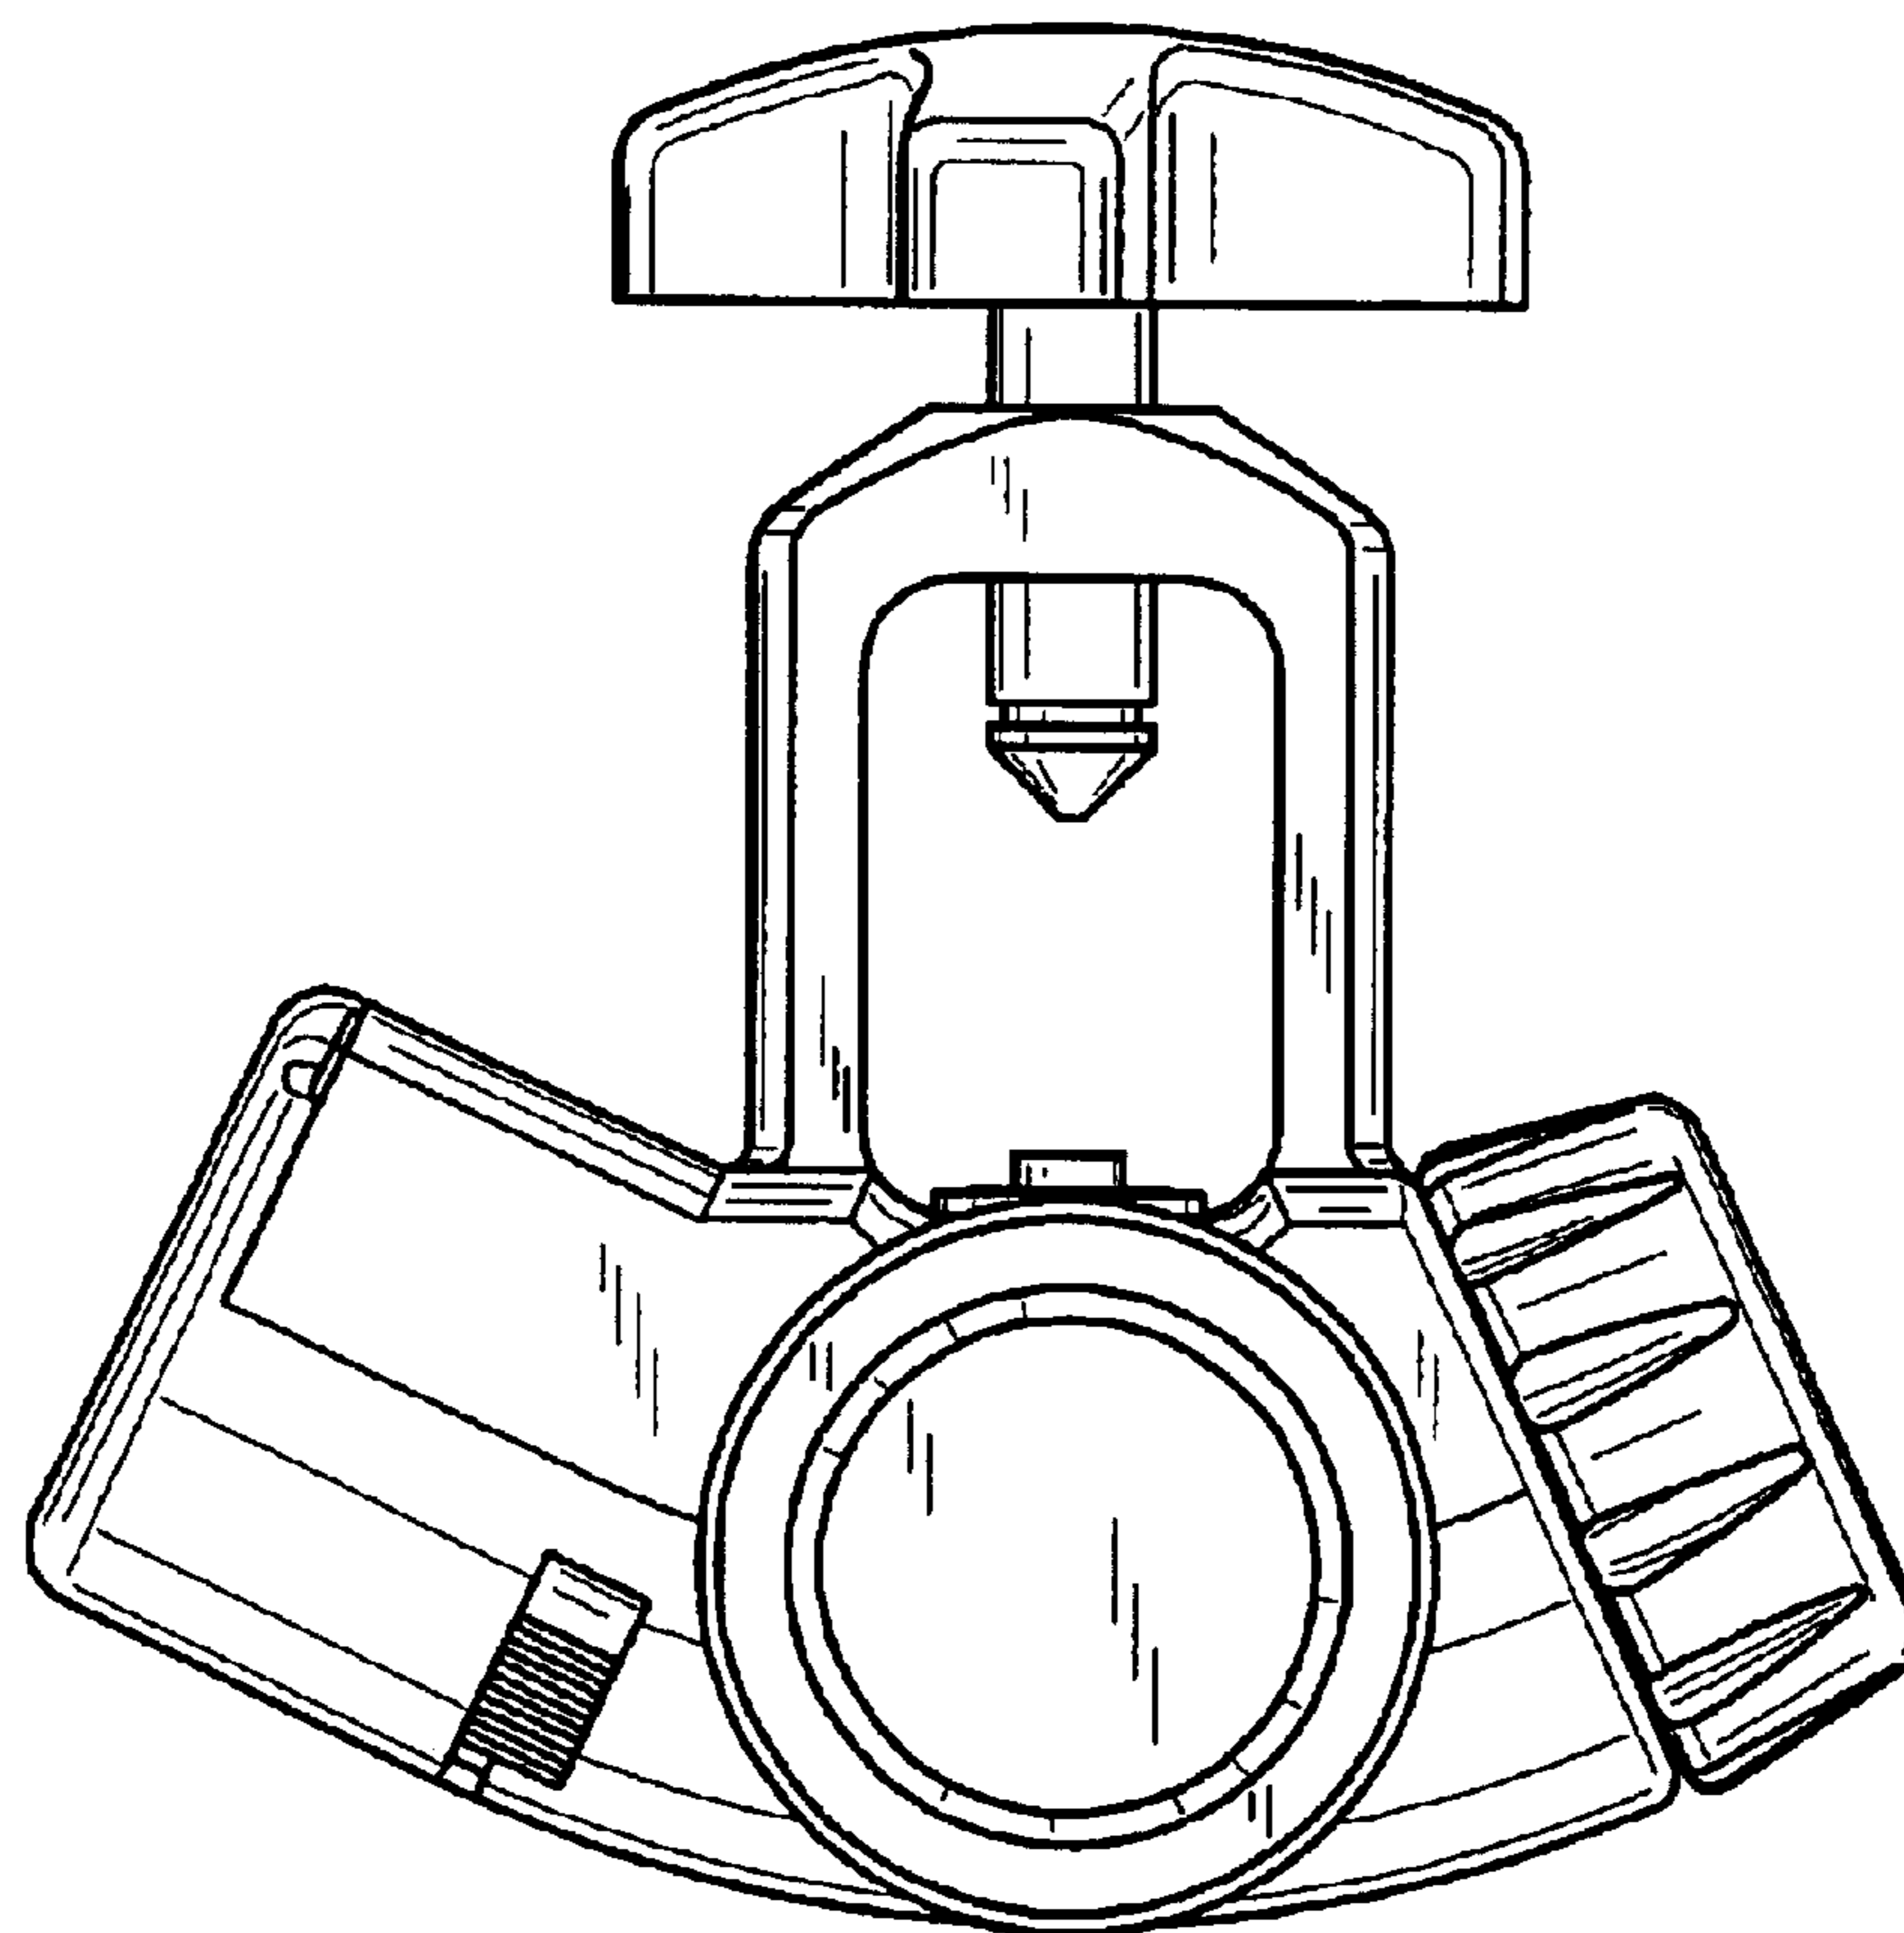


FIG. 4

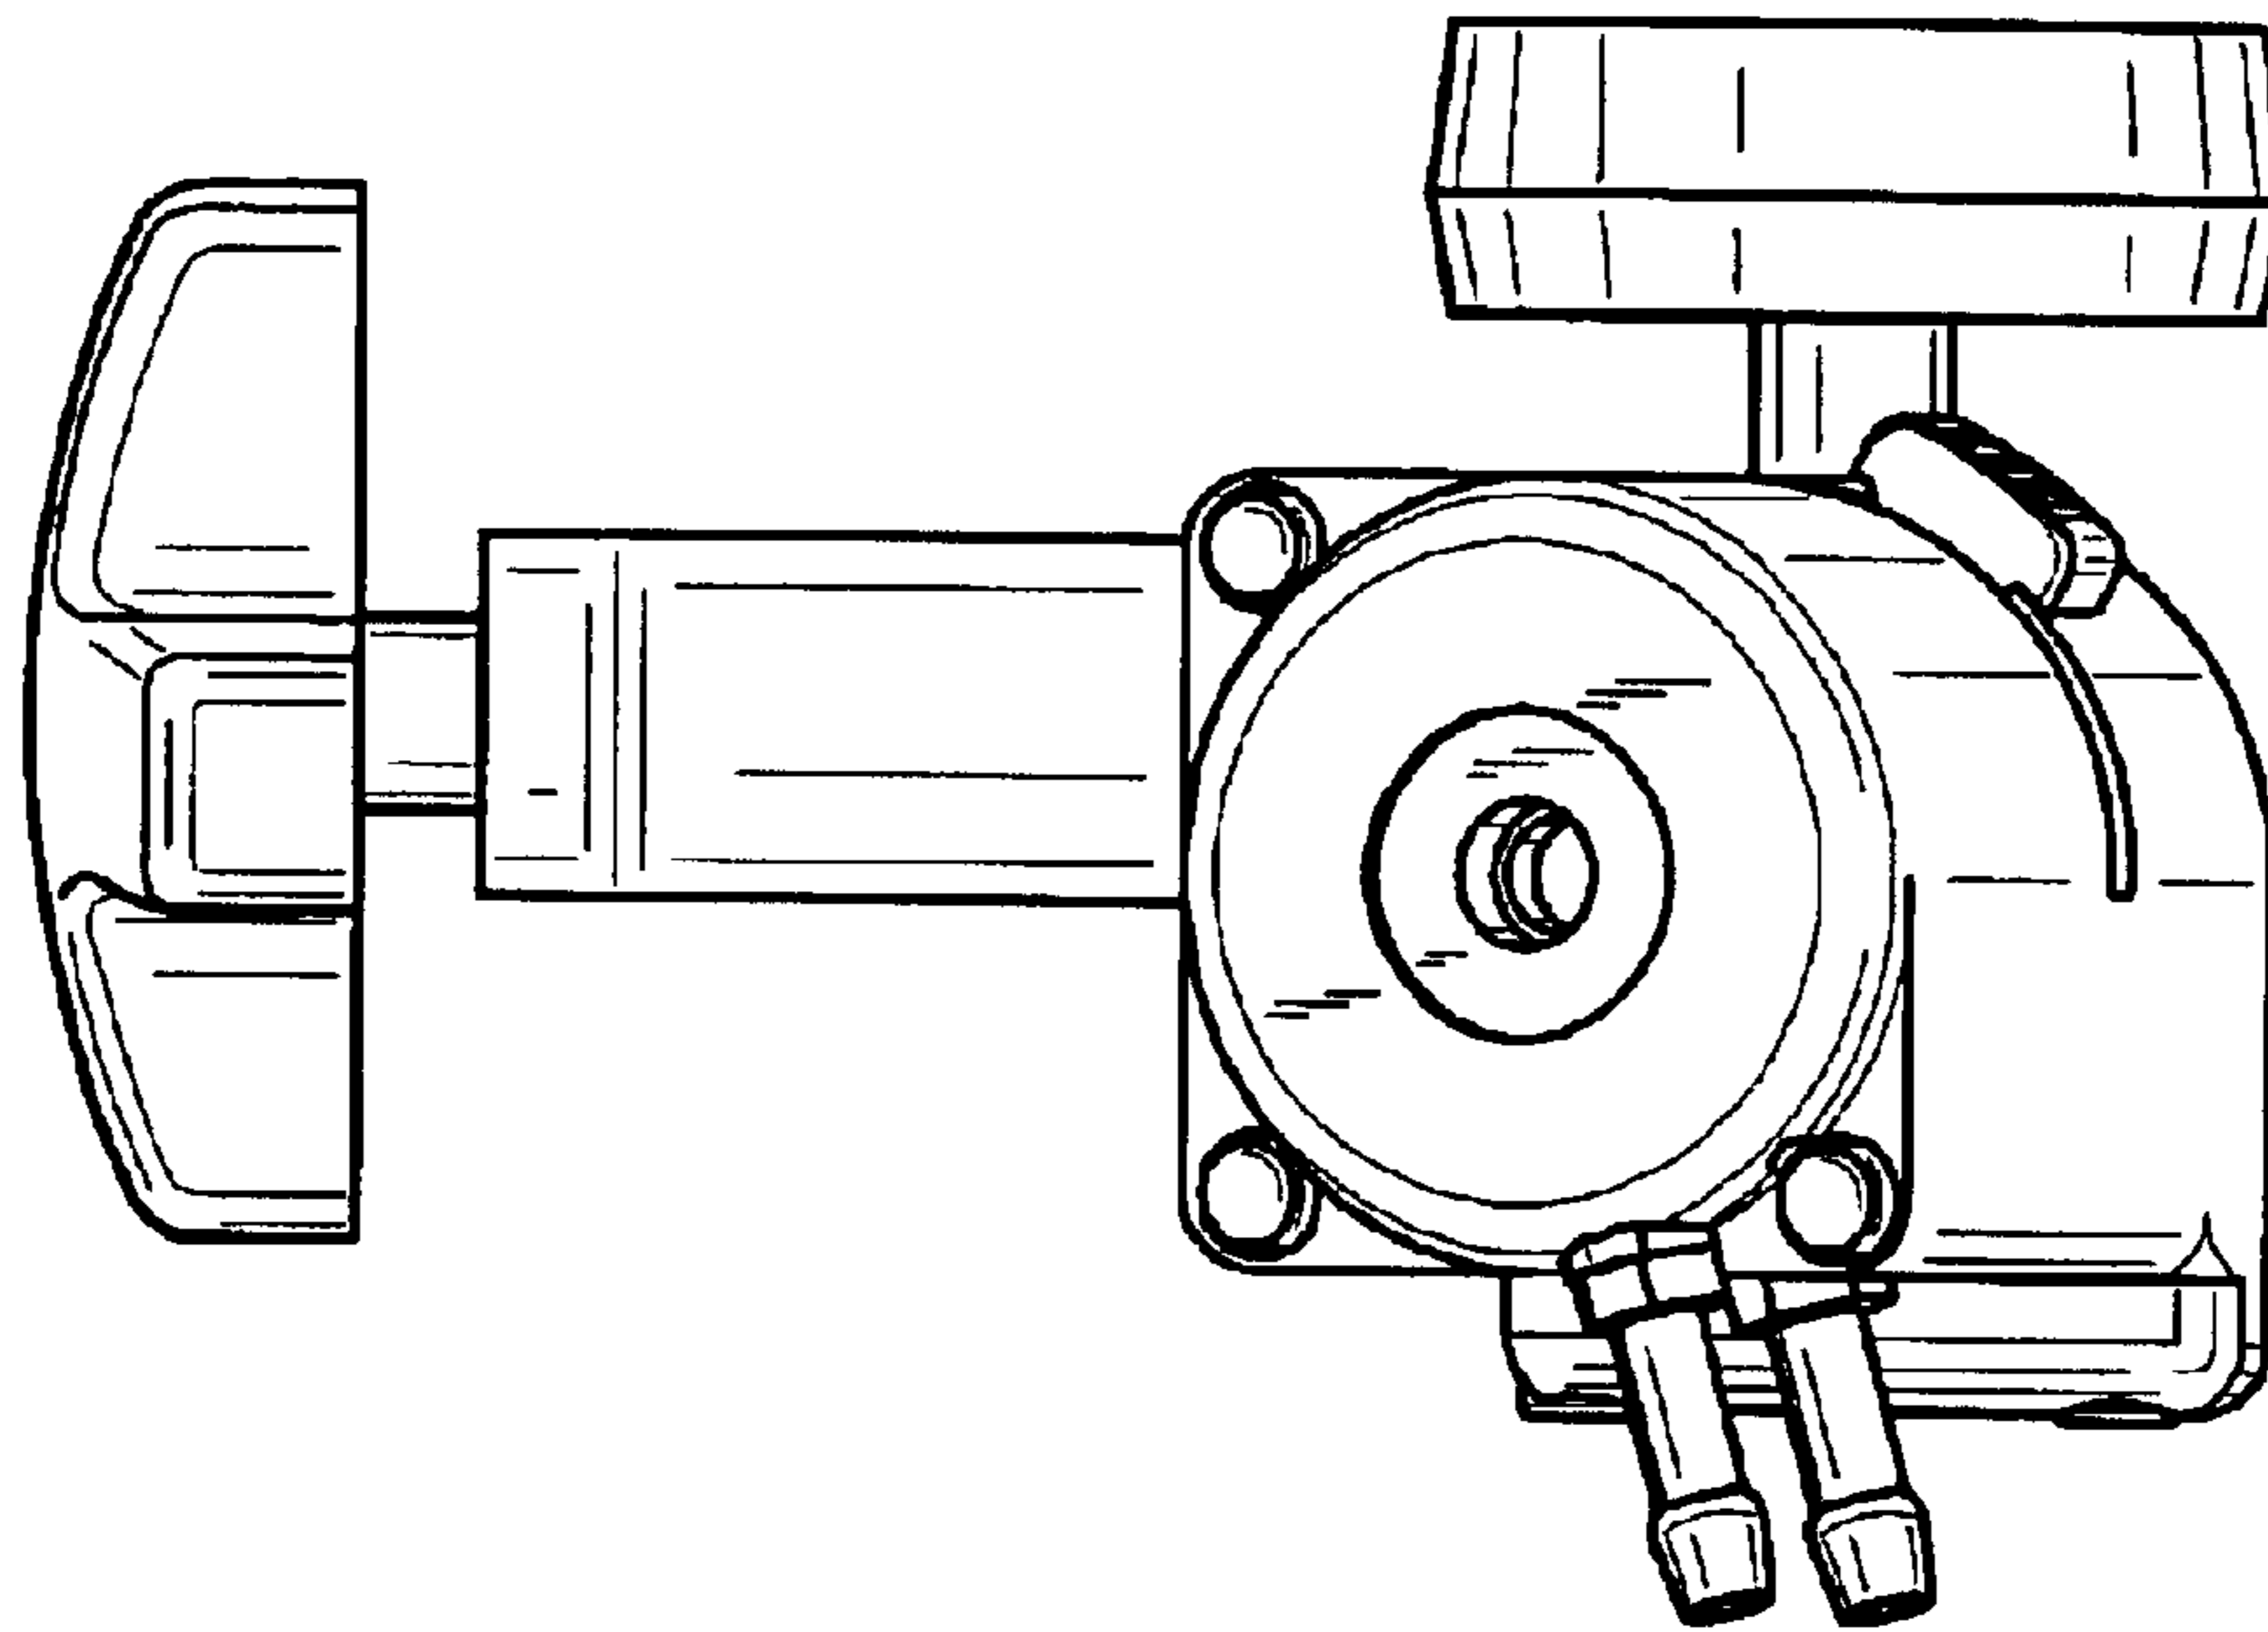


FIG. 5

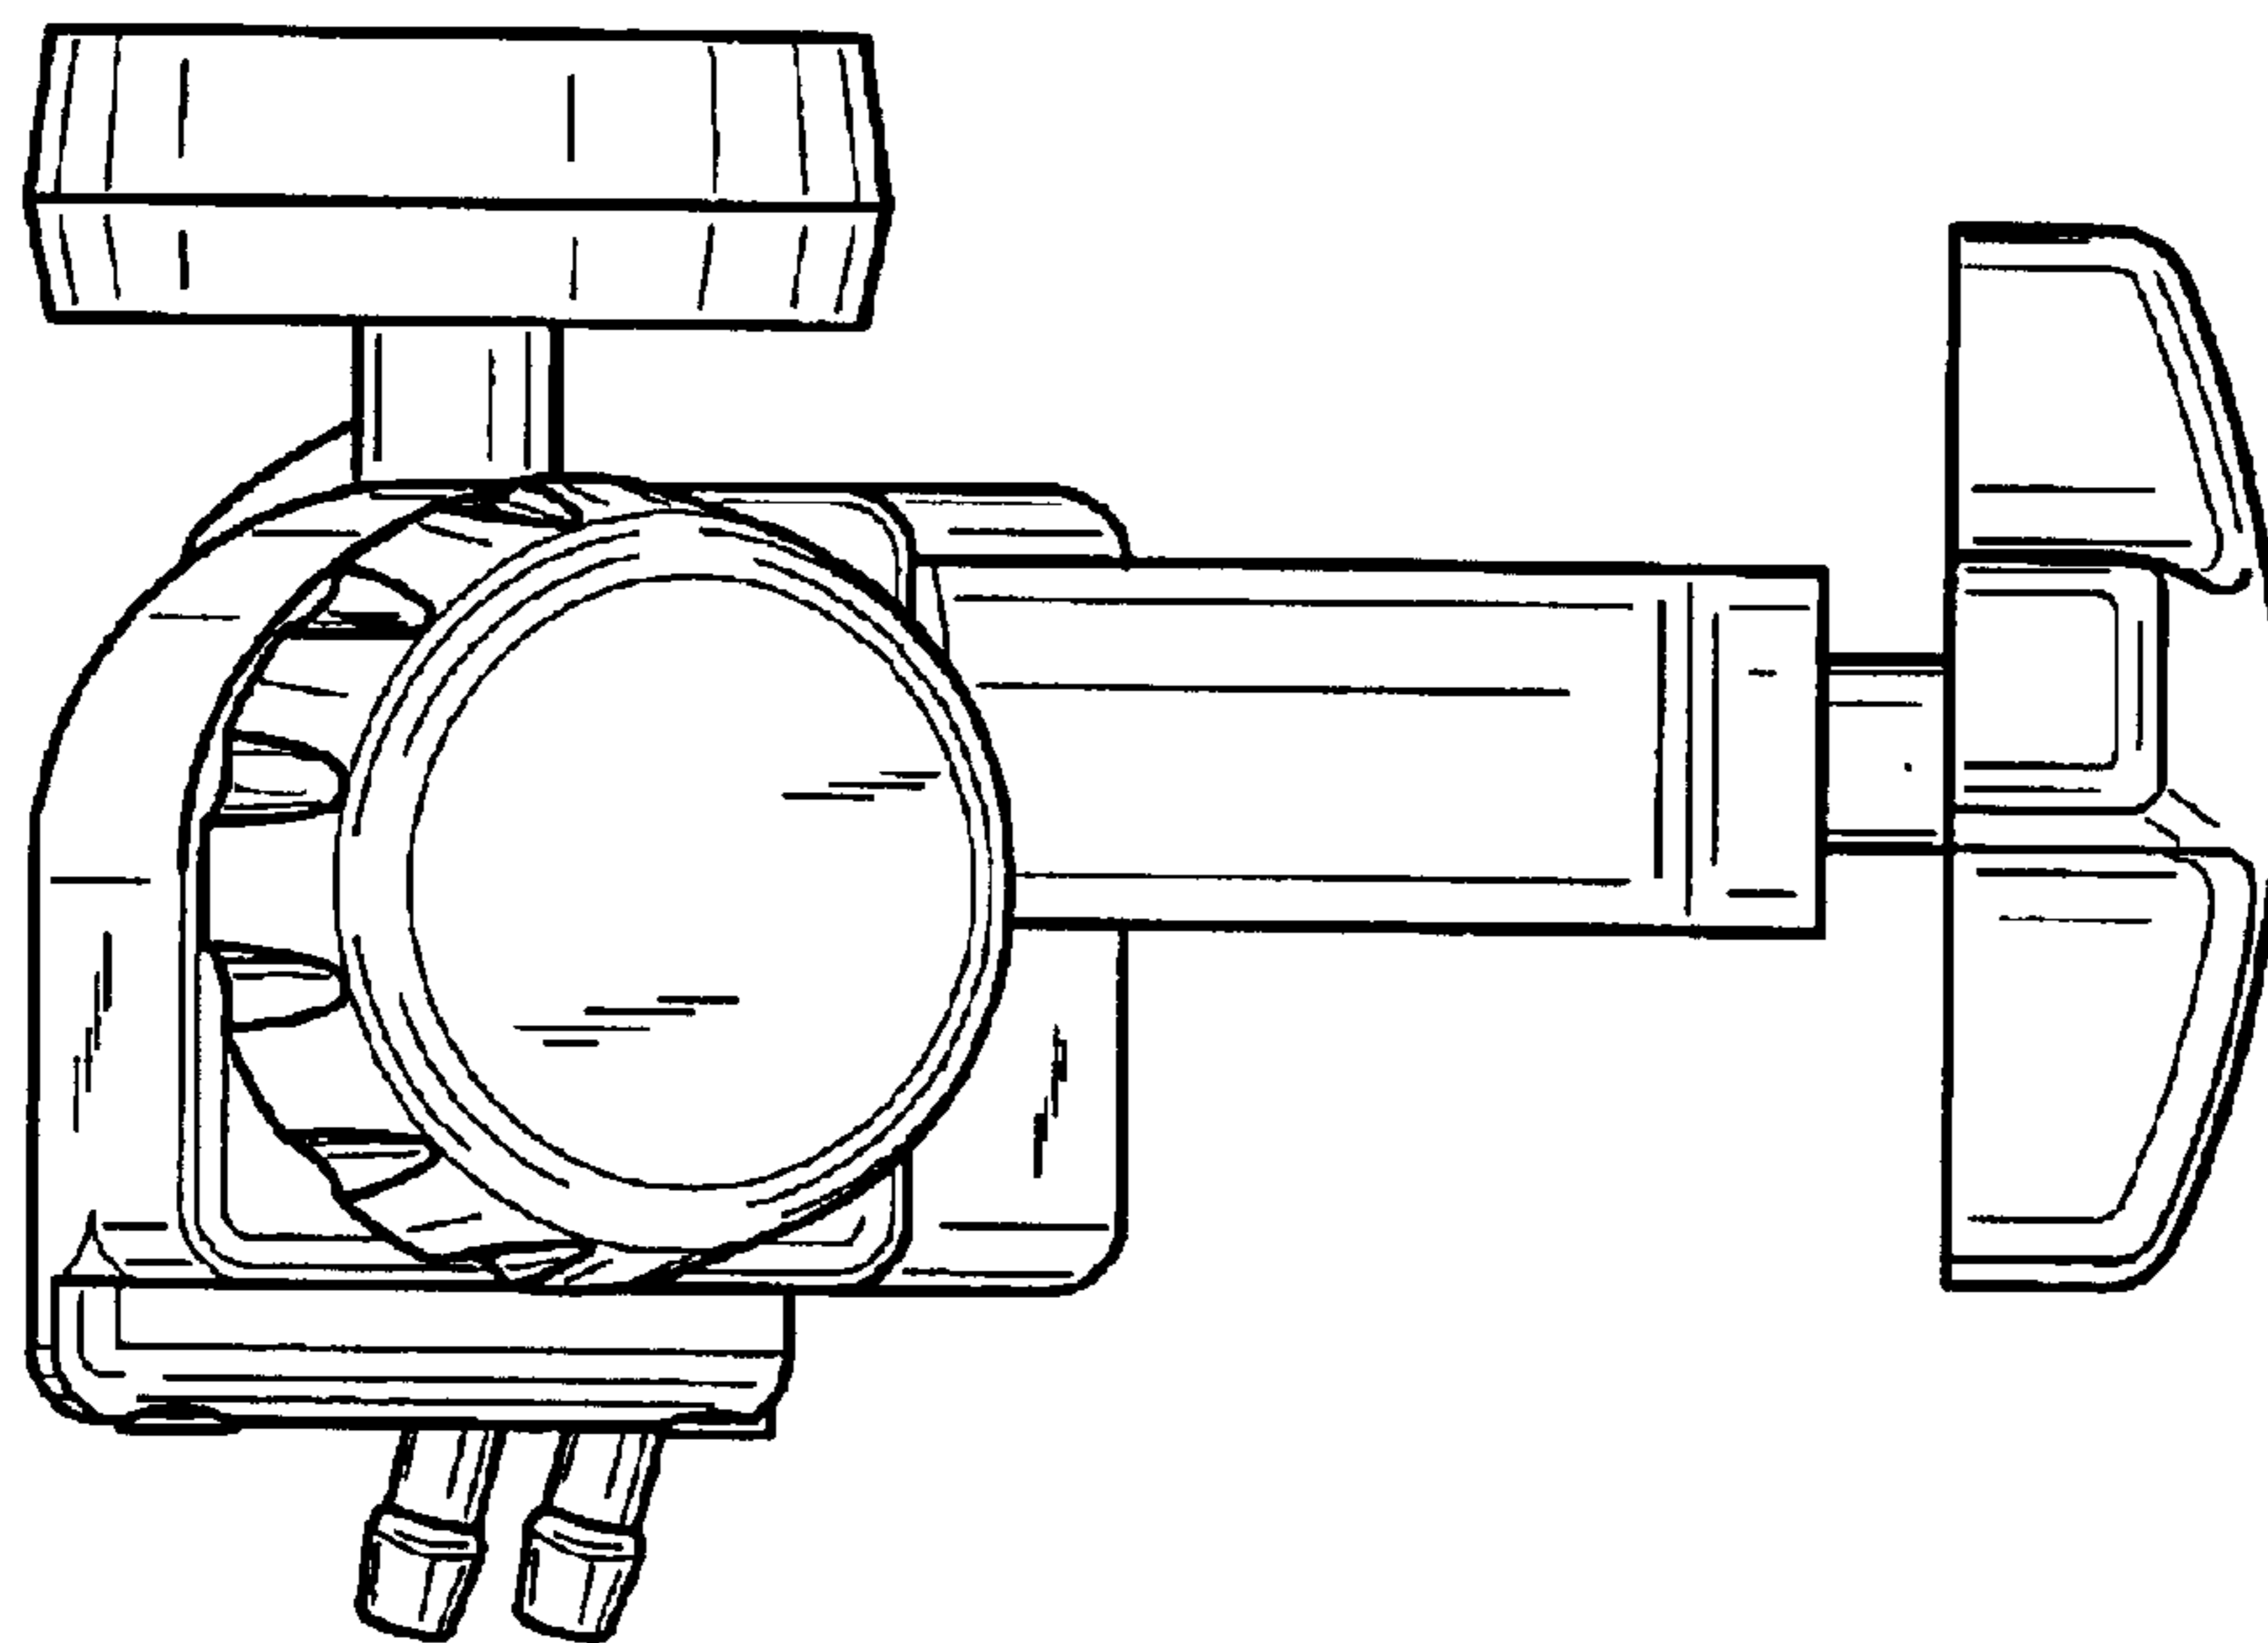


FIG. 6

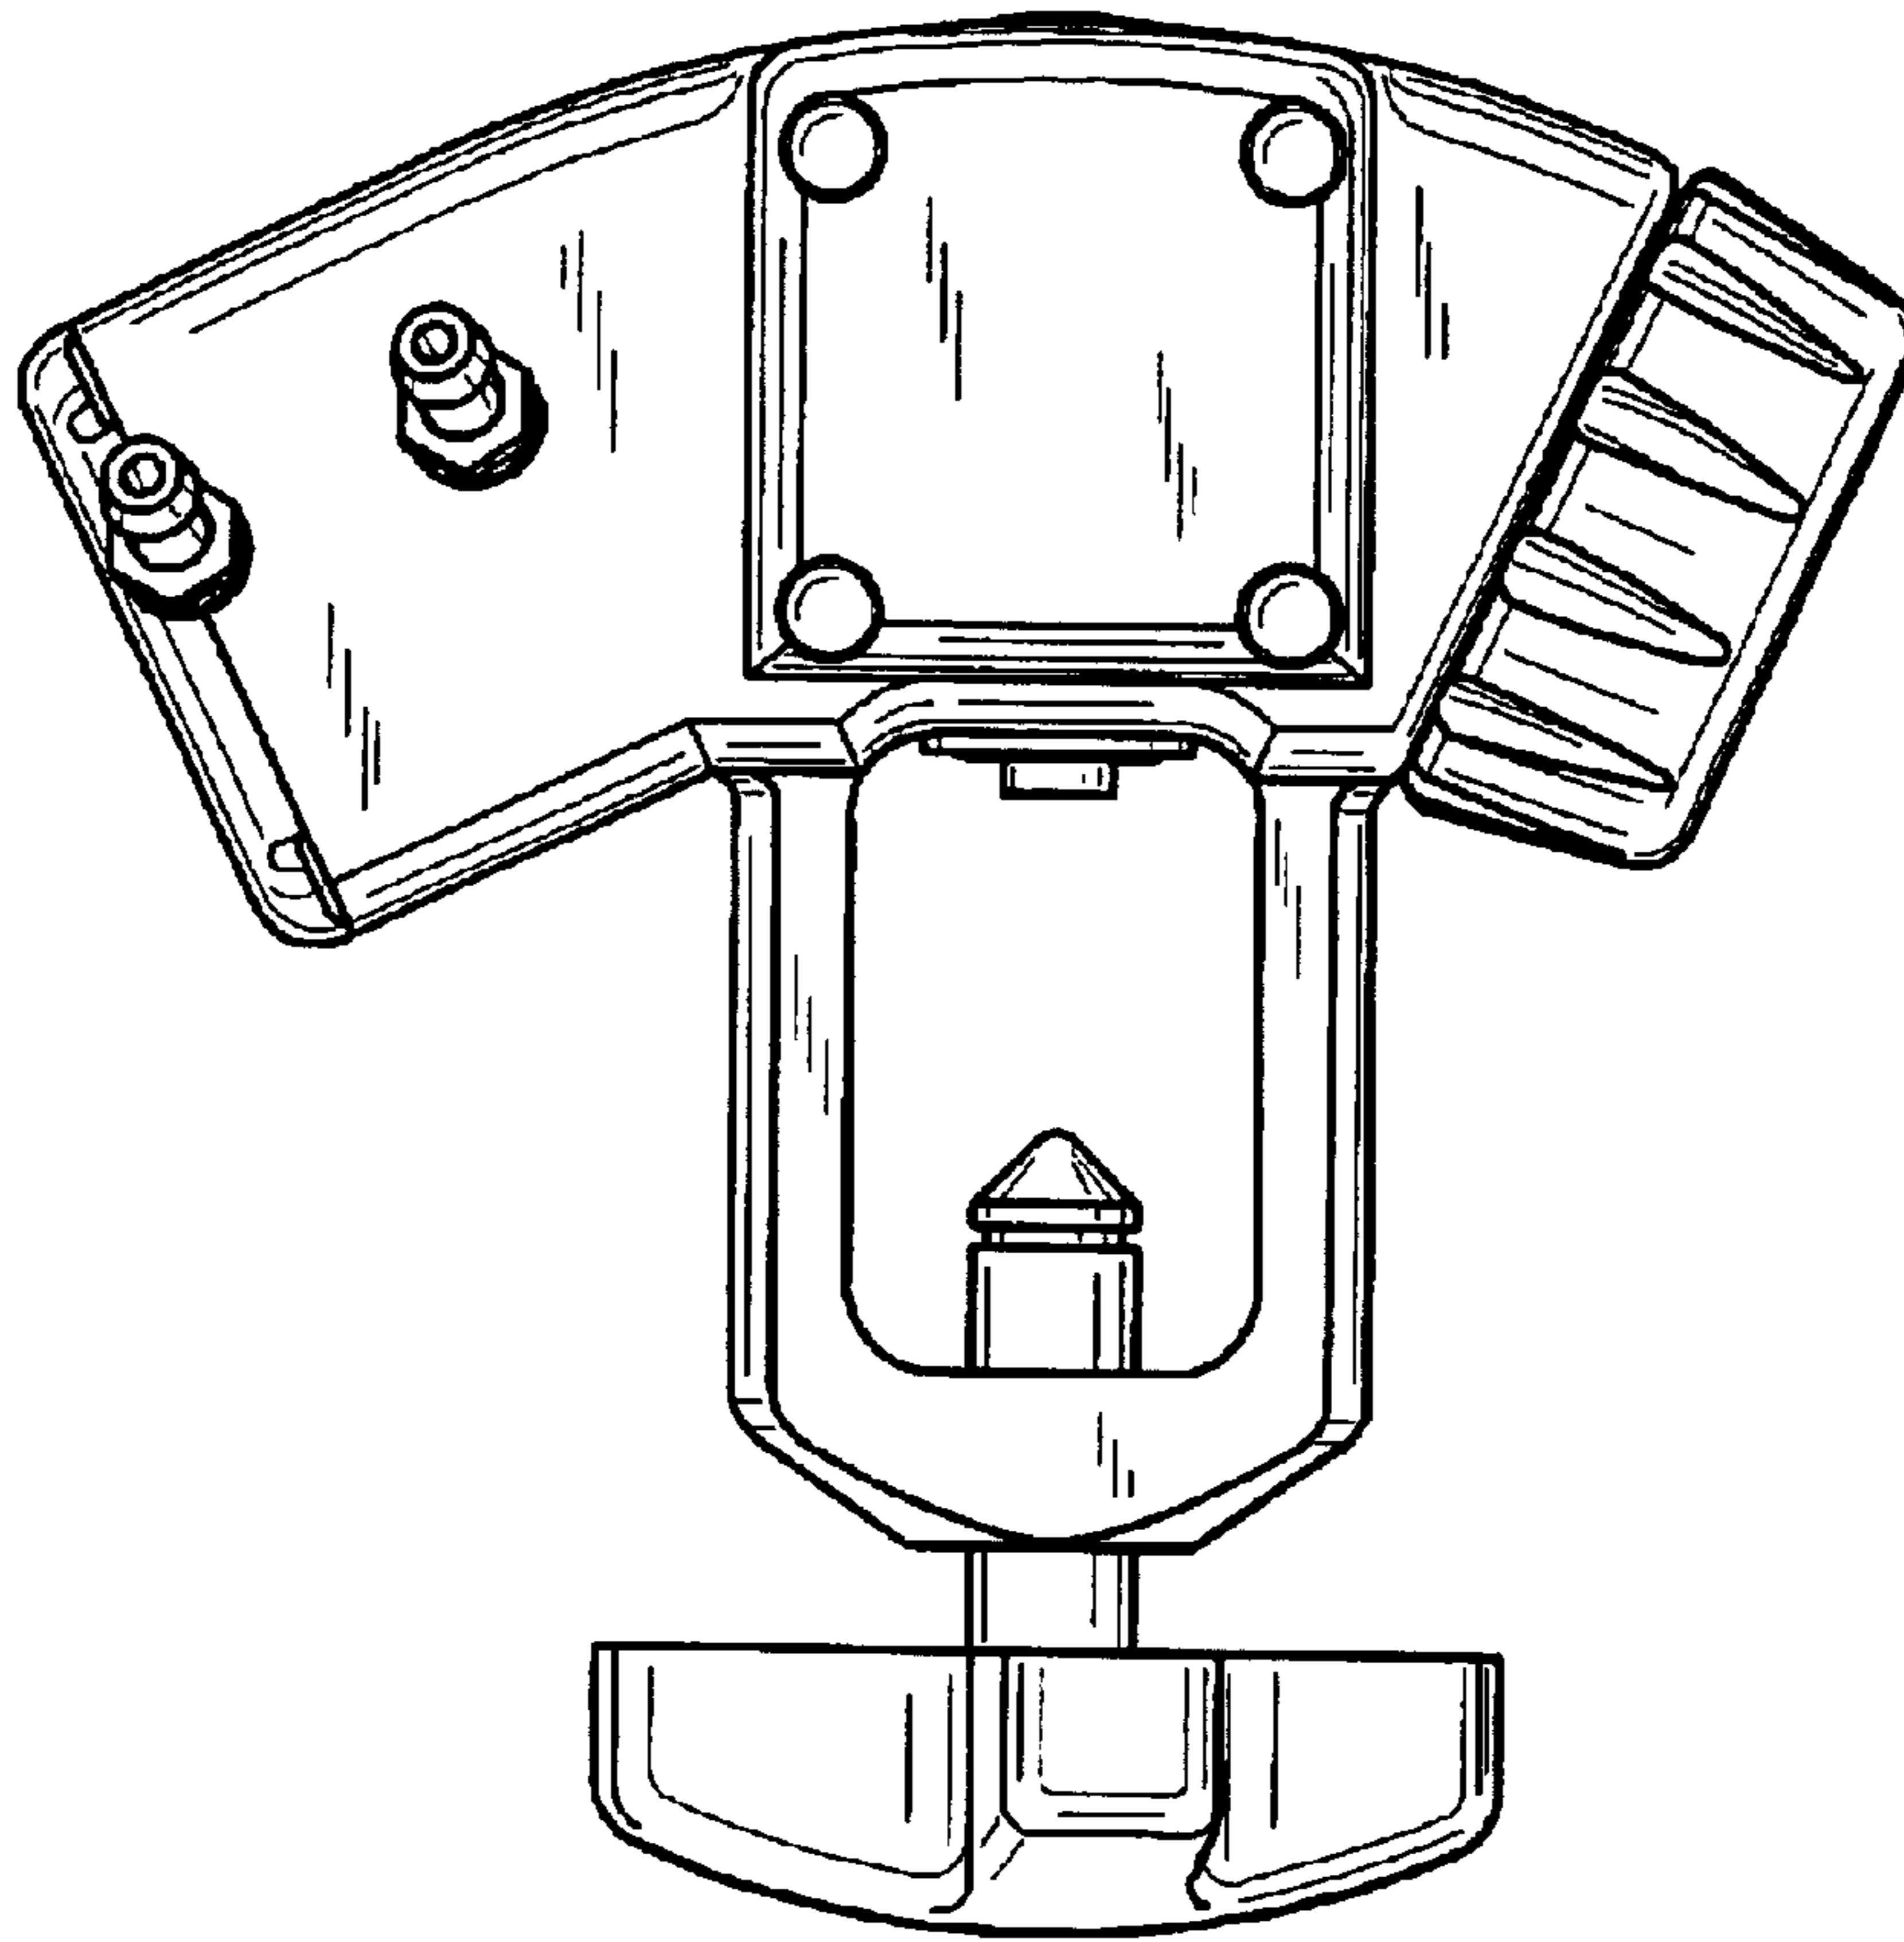


FIG. 7

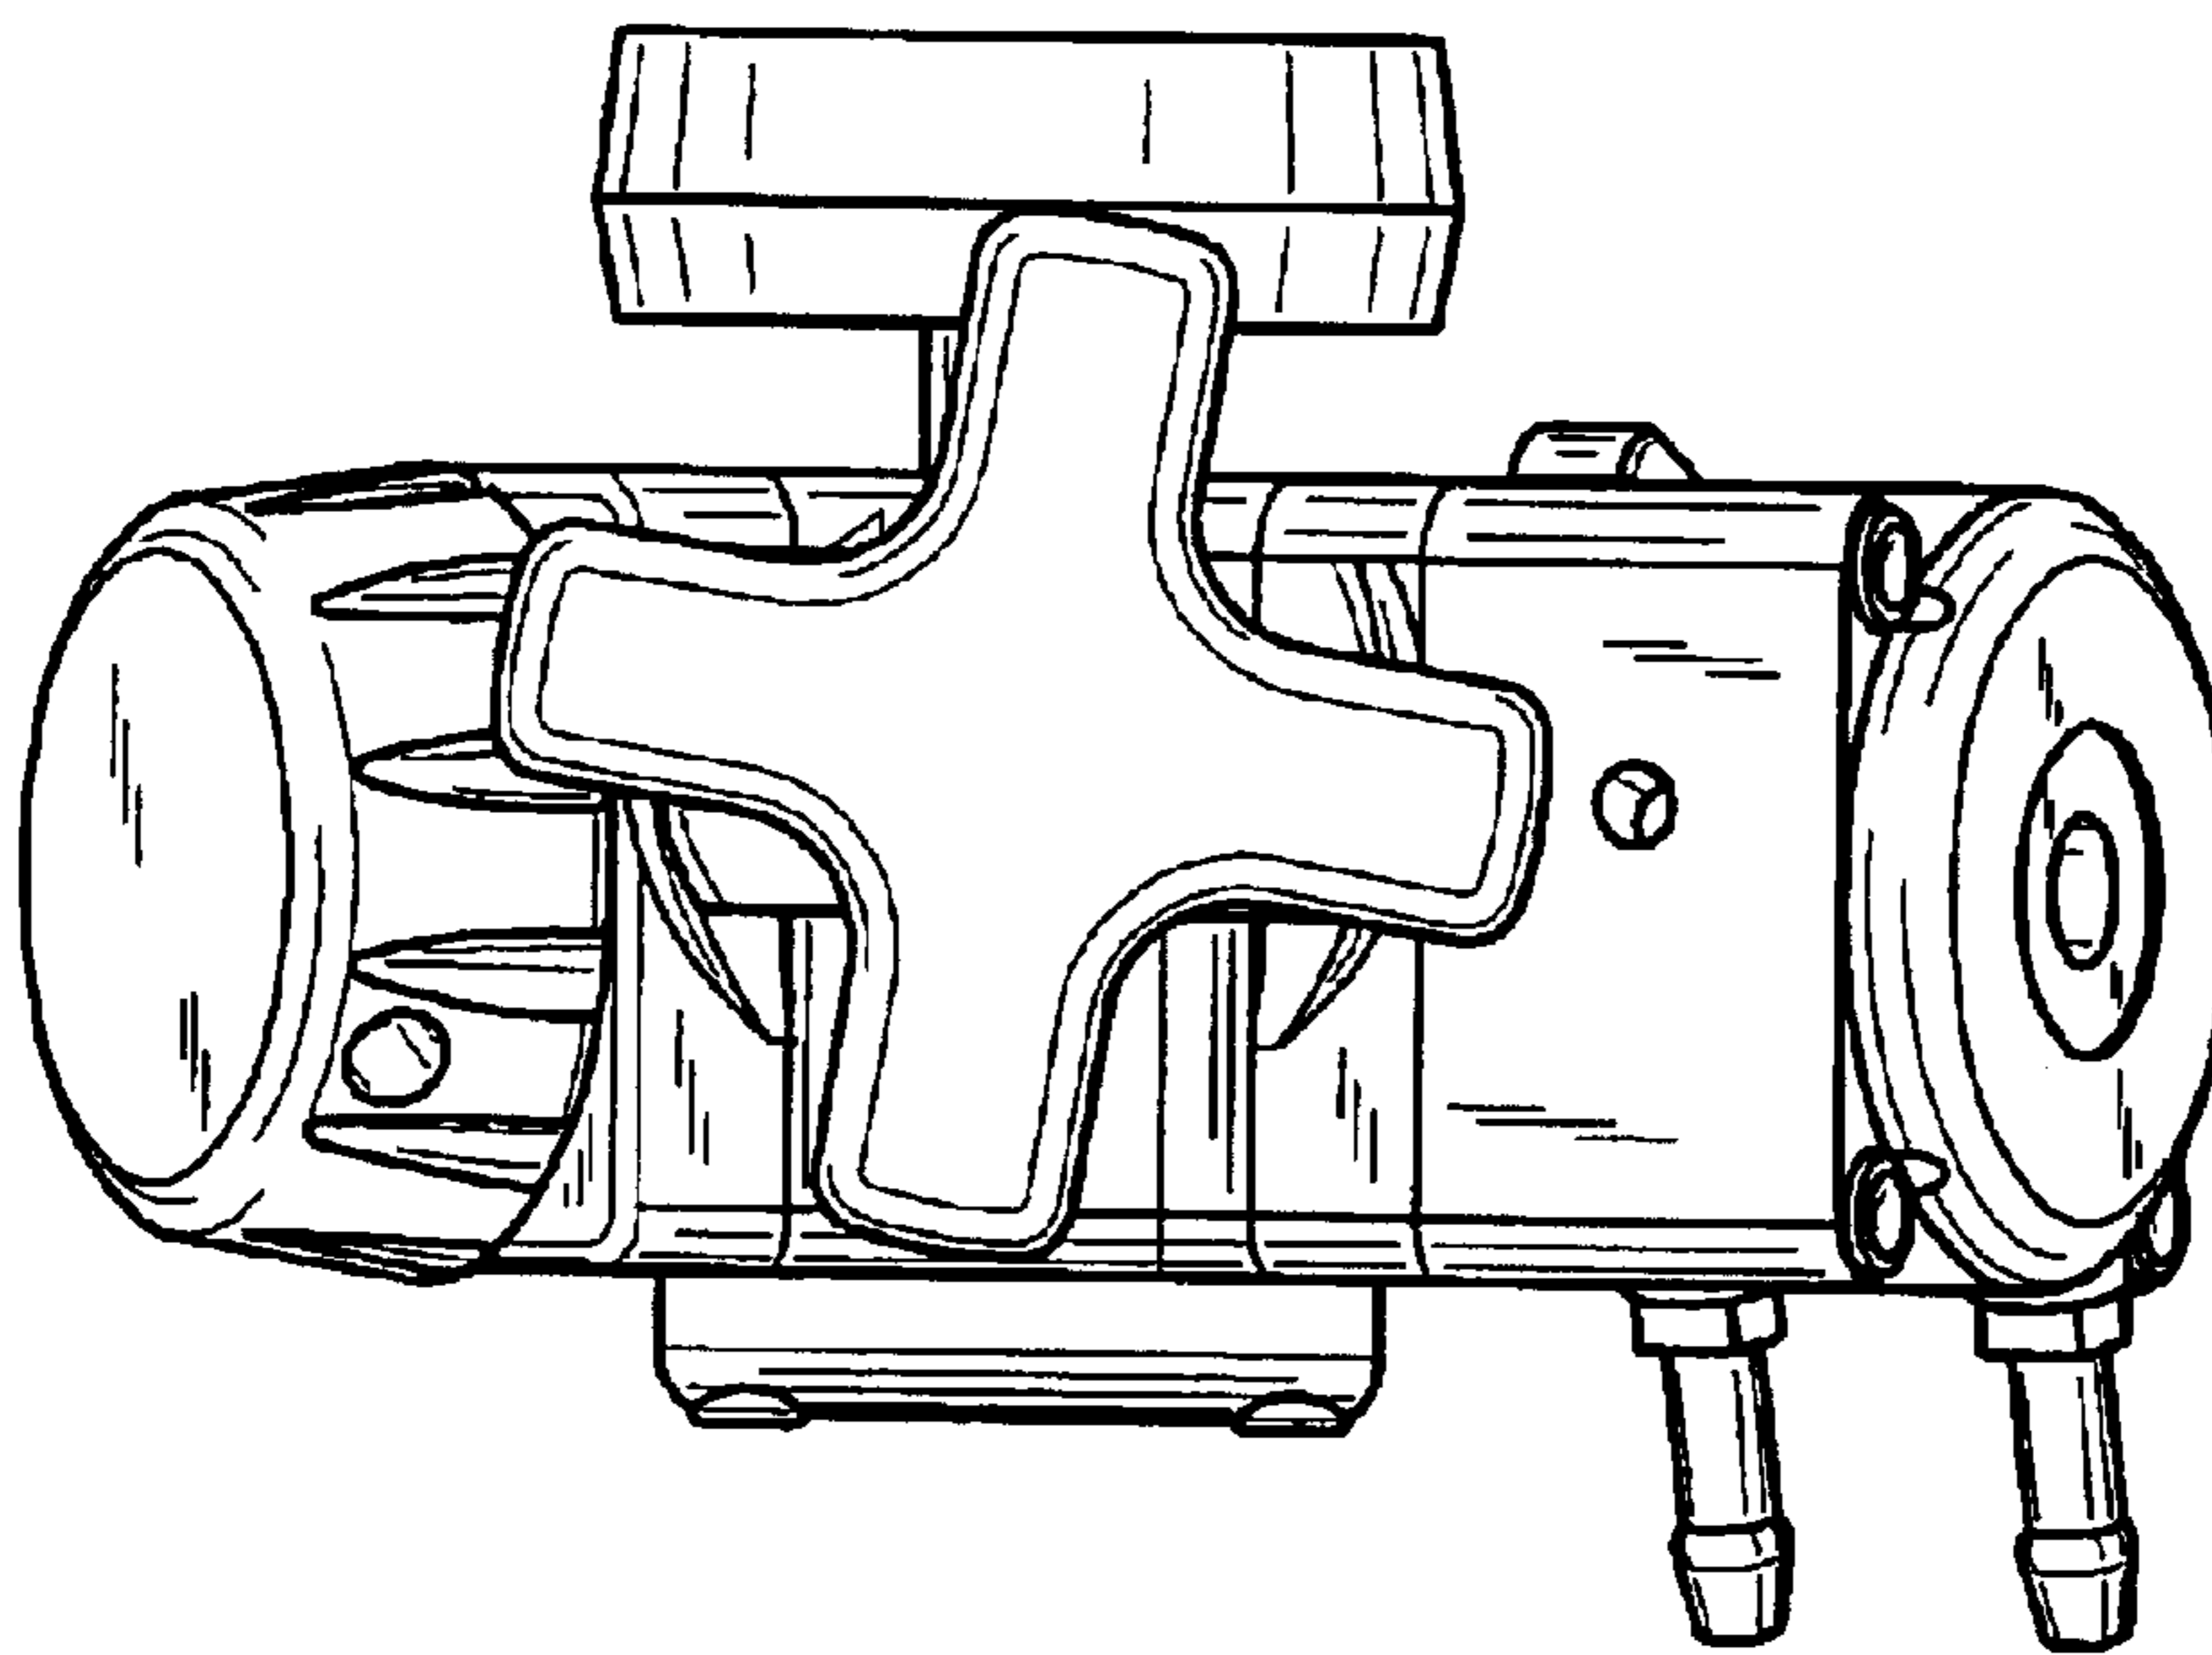


FIG. 8

UNITED STATES PATENT AND TRADEMARK OFFICE
CERTIFICATE OF CORRECTION

PATENT NO. : Des. 495,049 S
DATED : August 24, 2004
INVENTOR(S) : Gary Austin

Page 1 of 1


It is certified that error appears in the above-identified patent and that said Letters Patent is hereby corrected as shown below:

Title page.

Item [56], **References Cited**, OTHER PUBLICATIONS, "U.S. Byrd Patent Application" reference, please delete "Postable" and insert therefor -- Portable --.

Signed and Sealed this

Seventh Day of December, 2004

A handwritten signature in black ink on a light gray dotted background. The signature reads "Jon W. Dudas" in a cursive style.

JON W. DUDAS

Director of the United States Patent and Trademark Office