

US00D495054S1

(12) **United States Design Patent**
Laun et al.

(10) **Patent No.: US D495,054 S**
(45) **Date of Patent: ** Aug. 24, 2004**

(54) **CANNULA HEAD**
(75) Inventors: **Deborah A. Laun**, Syracuse, NY (US);
Daniel M. Wing, Utica, NY (US);
Frank J. Witkowski, Syracuse, NY
(US)

5,827,228 A 10/1998 Rowe 604/167
5,857,982 A 1/1999 Milliman et al. 600/567
5,865,807 A 2/1999 Blake, III 604/167

(List continued on next page.)

FOREIGN PATENT DOCUMENTS

(73) Assignee: **Conmed Corporation**, Utica, NY (US)
(**) Term: **14 Years**

EP 536549 A1 4/1993
WO WO 00/45720 8/2000

OTHER PUBLICATIONS

(21) Appl. No.: **29/180,774**
(22) Filed: **Apr. 28, 2003**

ConMed brochure entitled, "TroGard Finesse," dated Feb., 2000.

(List continued on next page.)

Related U.S. Application Data

(60) Division of application No. 29/168,574, filed on Oct. 4, 2002, and a division of application No. 10/264,530, filed on Oct. 4, 2002, which is a continuation-in-part of application No. 09/944,190, filed on Aug. 31, 2001.

Primary Examiner—Ian Simmons

(74) *Attorney, Agent, or Firm*—Heslin Rothenberg Farley & Mesiti P.C.

(51) **LOC (7) Cl.** **24-02**
(52) **U.S. Cl.** **D24/146**
(58) **Field of Search** D24/146, 147;
604/158, 161, 167.07, 164.04, 164.12, 164.1,
164.02, 164.11, 167; 606/185, 232

(57) **CLAIM**

The ornamental design for a cannula head, as shown and described.

DESCRIPTION

(56) **References Cited**

U.S. PATENT DOCUMENTS

4,909,798 A 3/1990 Fleischhacker et al. 604/256
5,129,885 A 7/1992 Green et al. 604/167
5,152,754 A 10/1992 Plyley et al. 604/164
5,203,769 A 4/1993 Clement et al. 604/32
5,209,736 A 5/1993 Stephens et al. 604/164
5,224,929 A 7/1993 Remiszewski 604/30
5,261,891 A 11/1993 Brinkerhoff et al. 604/165
5,263,937 A 11/1993 Shipp 604/164
5,346,459 A 9/1994 Allen 606/185
5,380,288 A 1/1995 Hart et al. 604/167
D358,209 S 5/1995 Petruschke et al. D24/146
5,556,411 A 9/1996 Taoda et al. 606/185
D379,229 S * 5/1997 Rodriguez et al. D24/146
5,669,875 A 9/1997 van Eerdenburg 604/22
5,807,338 A 9/1998 Smith et al. 604/164

A portion of the disclosure of this patent document contains material which is subject to copyright protection. The copyright owner has no objection to the facsimile reproduction by anyone of the patent document or the patent disclosure, as it appears in the Patent and Trademark Office patent file or records, but otherwise reserves all copyright rights whatsoever.

FIG. 1 is an isometric view of a cannula head in accordance with the new design;

FIG. 2 is a left side elevational view thereof;

FIG. 3 is a right side elevational view thereof;

FIG. 4 is a front elevational view thereof;


FIG. 5 is a rear elevational view thereof;

FIG. 6 is a top plan view thereof; and,

FIG. 7 is a bottom plan view thereof.

The broken lines in the figures are for illustrative purposes only and form no part of the claimed design.

1 Claim, 3 Drawing Sheets

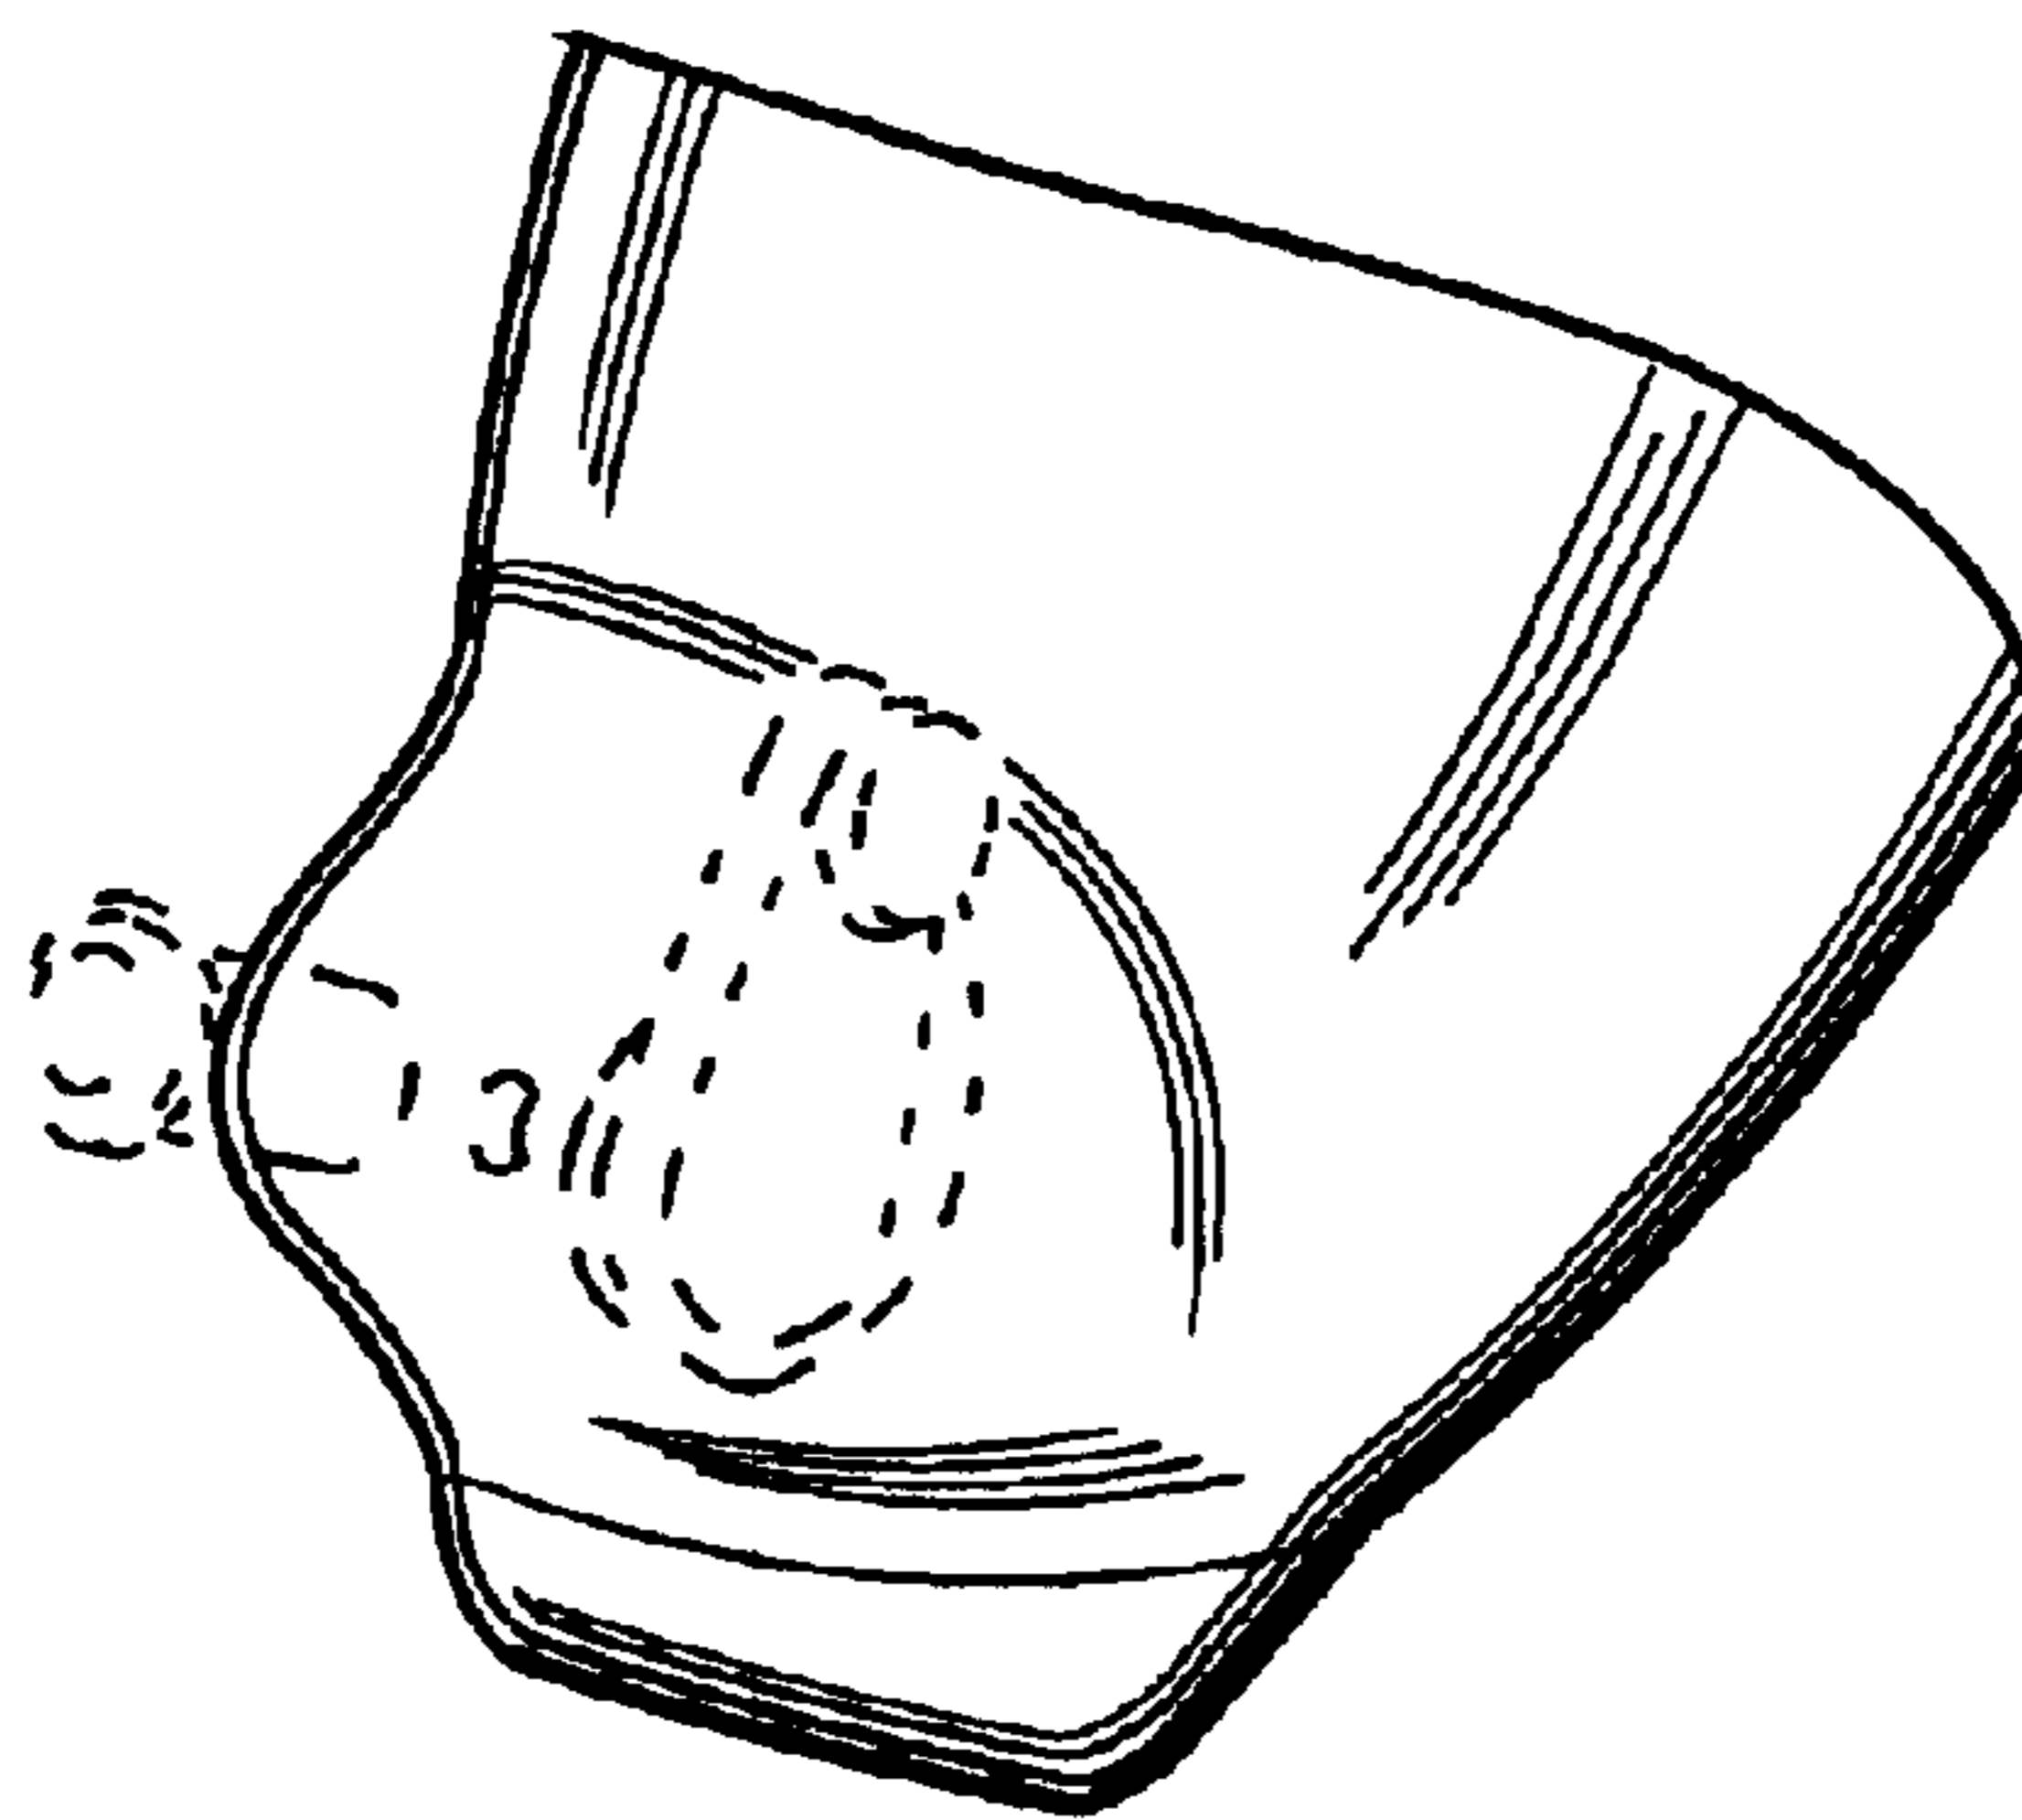

U.S. PATENT DOCUMENTS

| | | | | |
|--------------|------|---------|-------------------------|------------|
| 5,879,332 | A | 3/1999 | Schwemberger et al. ... | 604/164 |
| 5,904,699 | A | 5/1999 | Schwemberger et al. ... | 606/185 |
| 5,941,852 | A | 8/1999 | Dunlap et al. | 604/165 |
| 5,976,121 | A | 11/1999 | Matern et al. | 606/1 |
| 6,036,711 | A | 3/2000 | Mozdzierz et al. | 606/185 |
| 6,159,182 | A | 12/2000 | Davis et al. | 604/167.06 |
| 6,497,687 | B1 | 12/2002 | Blanco | 604/274 |
| 6,500,188 | B2 | 12/2002 | Harper et al. | 606/169 |
| 2003/0045834 | A1 * | 3/2003 | Wing et al. | 604/161 |
| 2003/0233114 | A1 * | 12/2003 | Merboth et al. | 606/185 |

OTHER PUBLICATIONS

ConMed brochure, entitled, "Advanced Patient Benefits, Single-Use Trocars," dated 2000.

ConMed brochure entitled, "Unsurpassed Control, Responsible Trocars," dated 1997.

Wing et al., pending U.S. Utility Patent Application, Ser. No. 09/944,190, filed Aug. 31, 2001, entitled "Obturator and Cannula for a Trocar Adapted for Ease of Insertion and removal".

Wing et al., pending U.S. Utility Patent Application, Ser. No. 10/264,530, filed Oct. 4, 2002, entitled "Trocar System".

Witkowski, pending U.S. Design Patent Application Serial No. 29/180,667, filed Apr. 28, 2003, entitled "Cannula Tube,".

Laun, pending U.S. Design Patent Application Serial No. 29/168,574, filed Oct. 4, 2002, entitled "Trocar".

Laun, pending U.S. Design Patent Application Serial No. 29/180,624, filed Apr. 28, 2003, entitled "Obturator,"

* cited by examiner

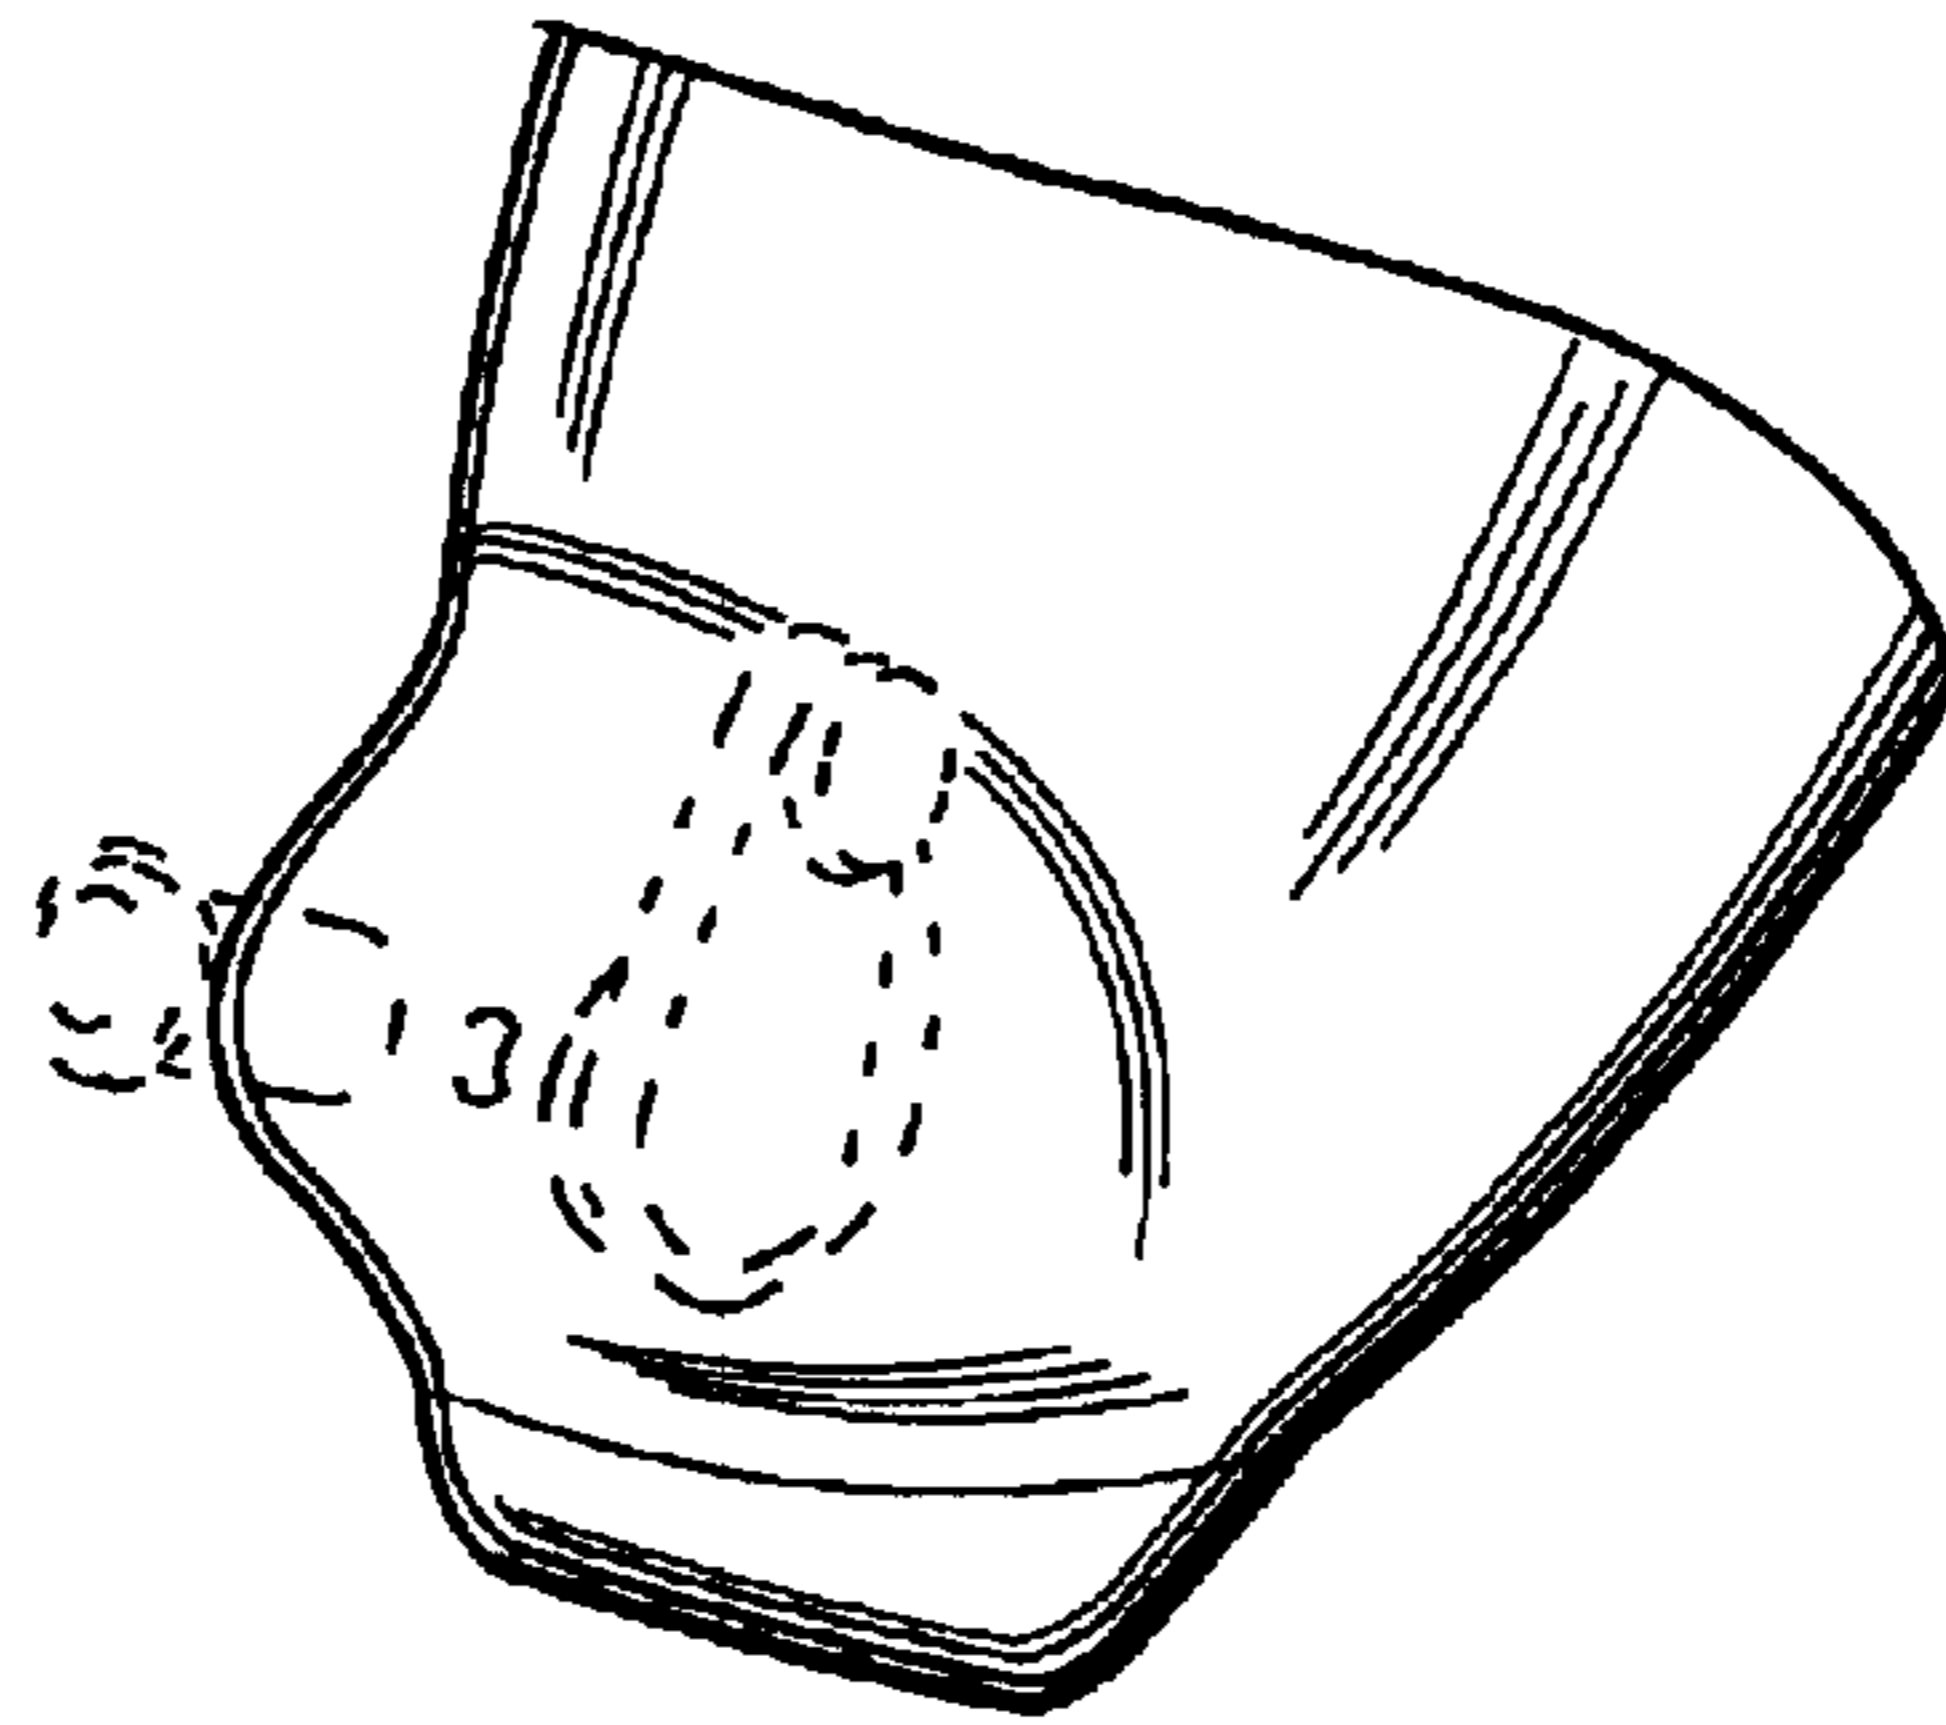


fig. 1

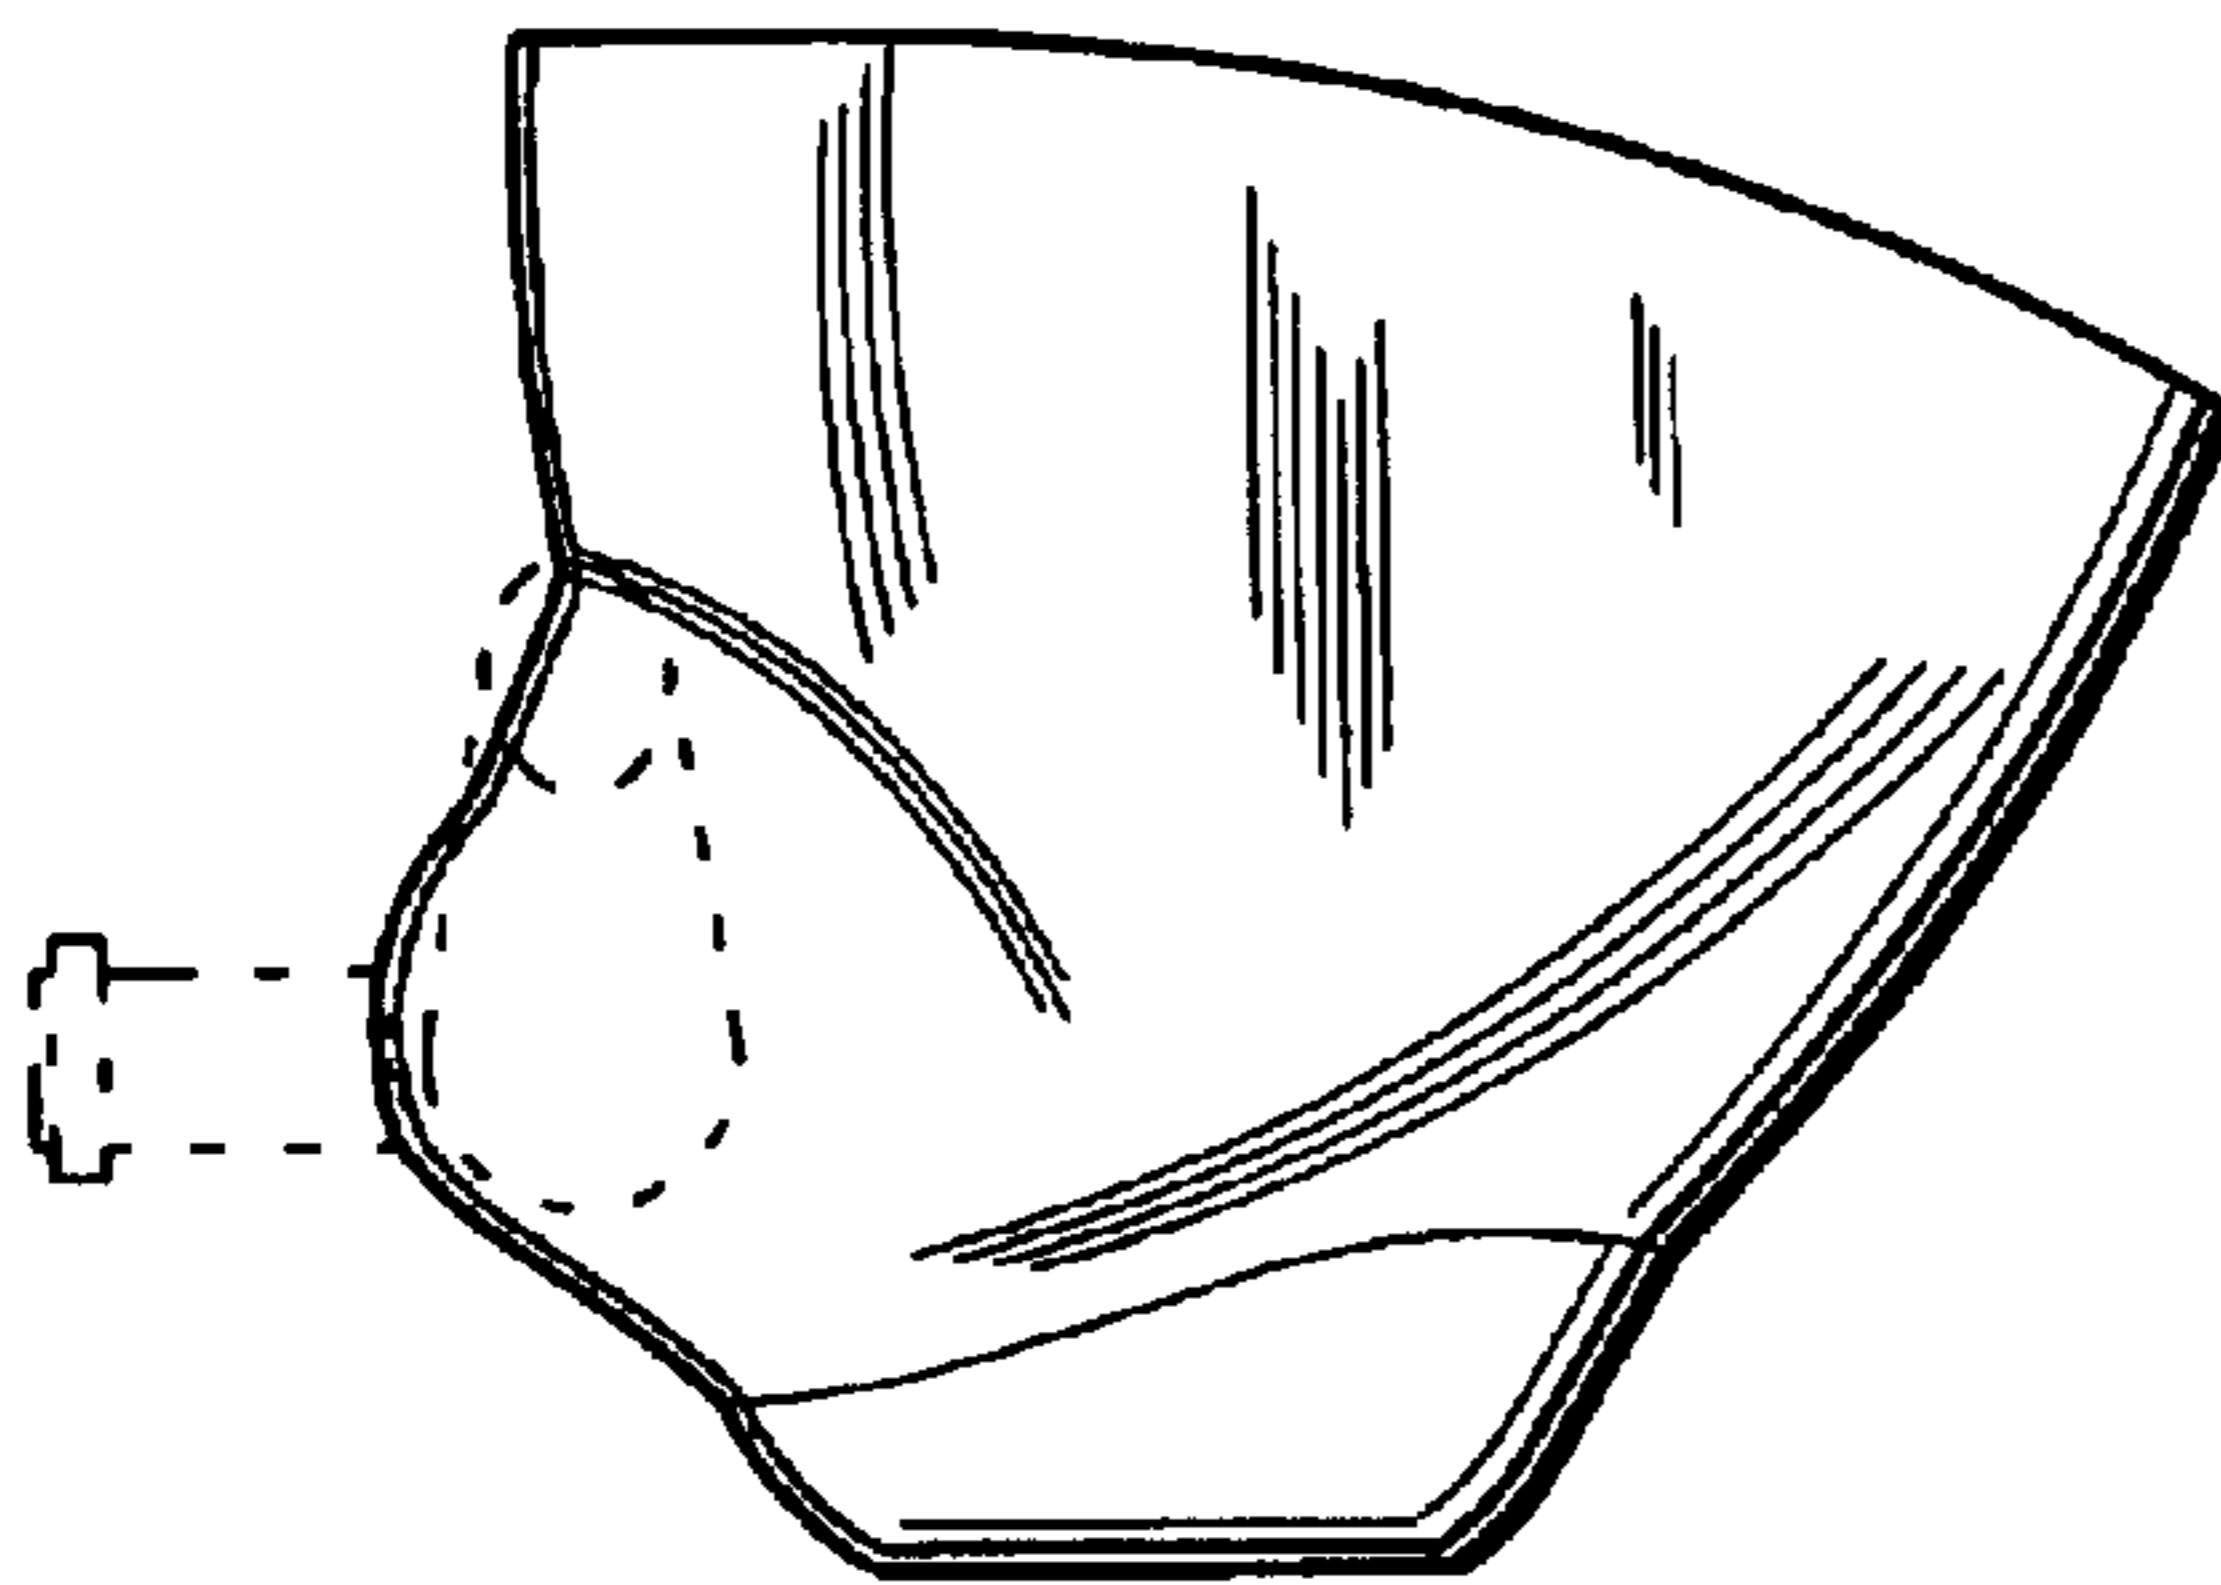


fig. 2

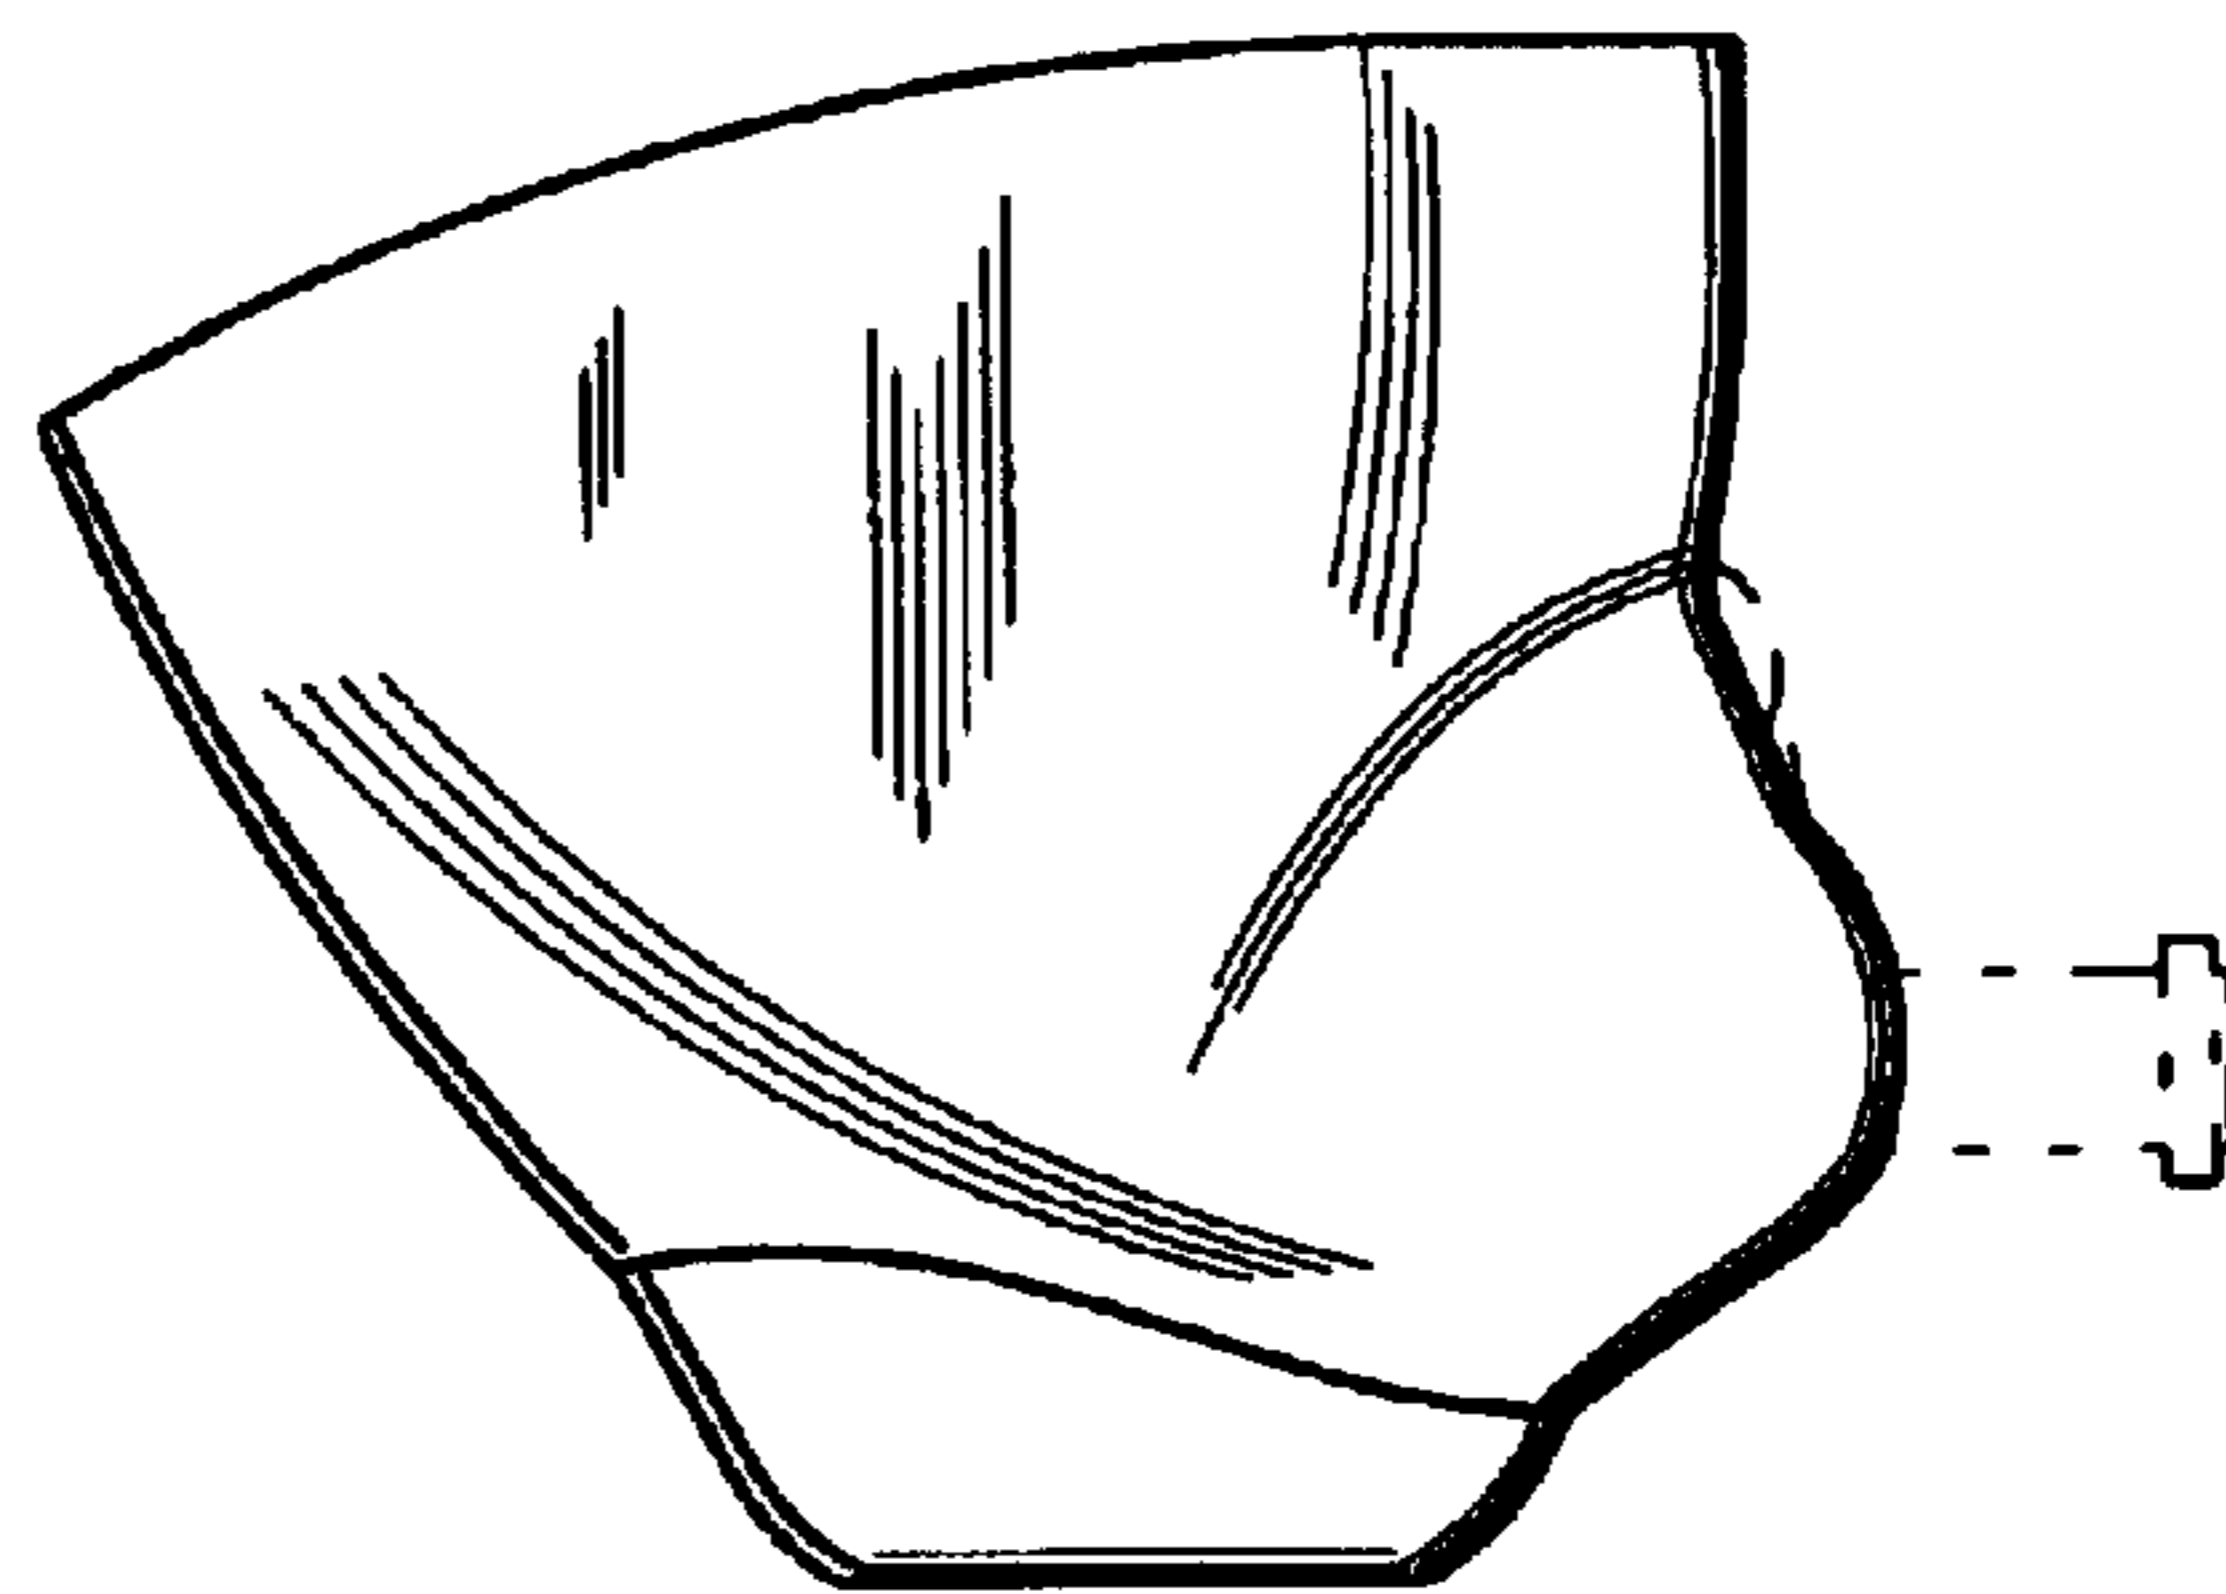


fig. 3

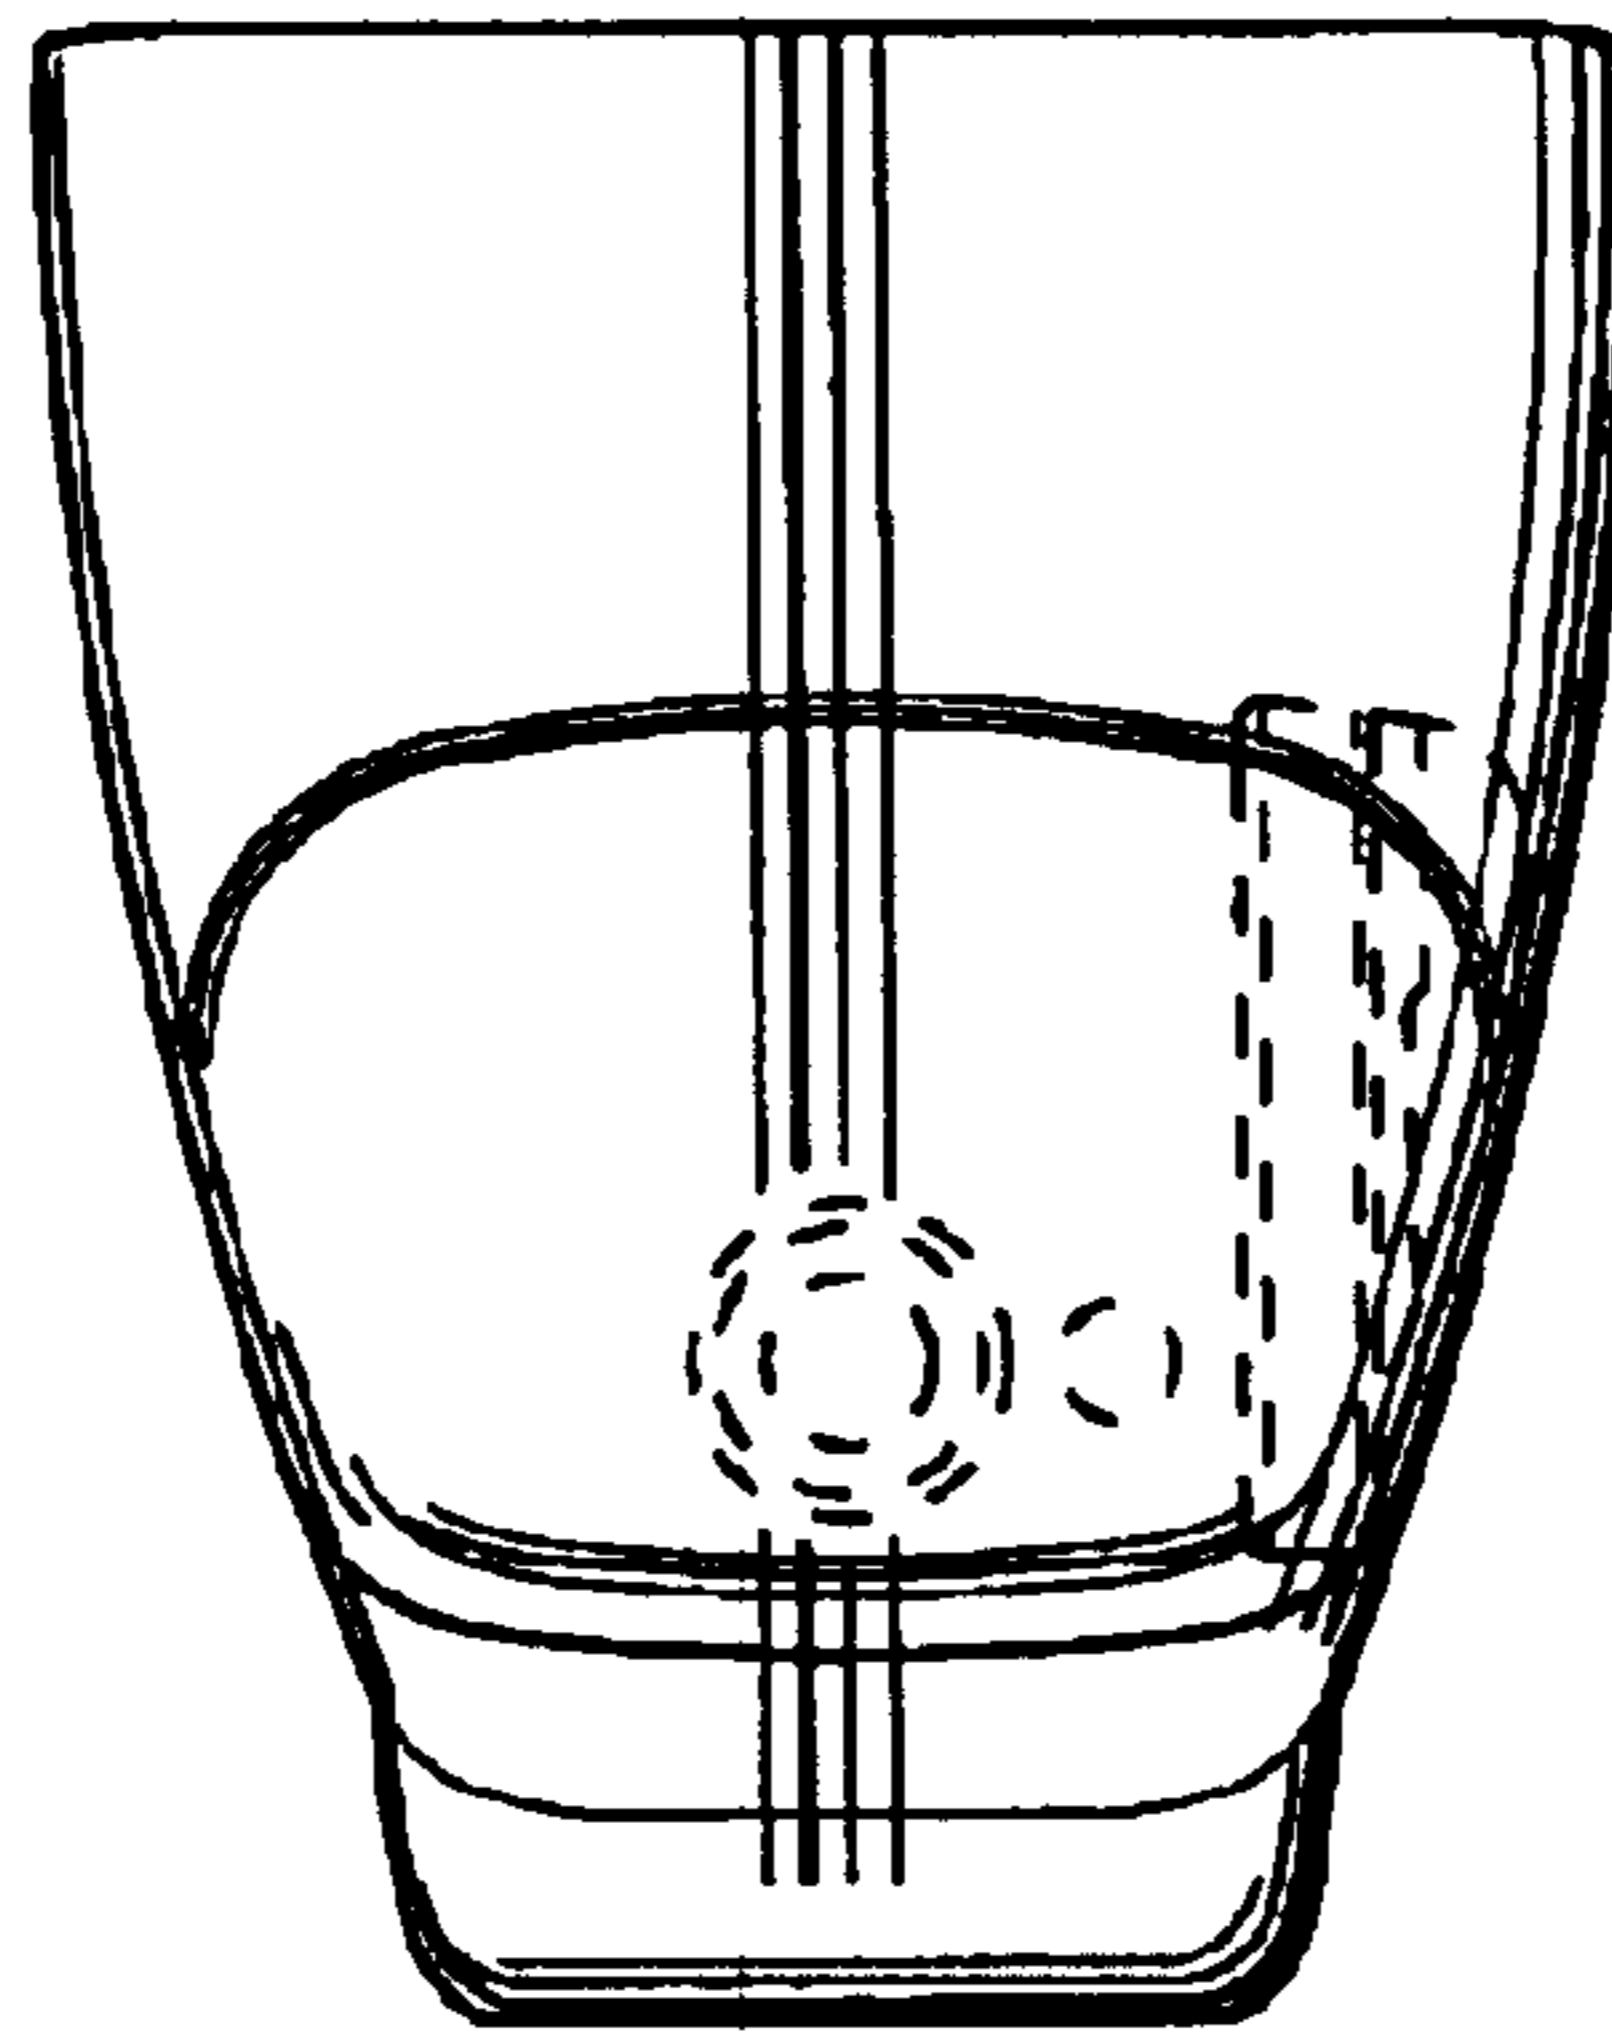


fig. 4

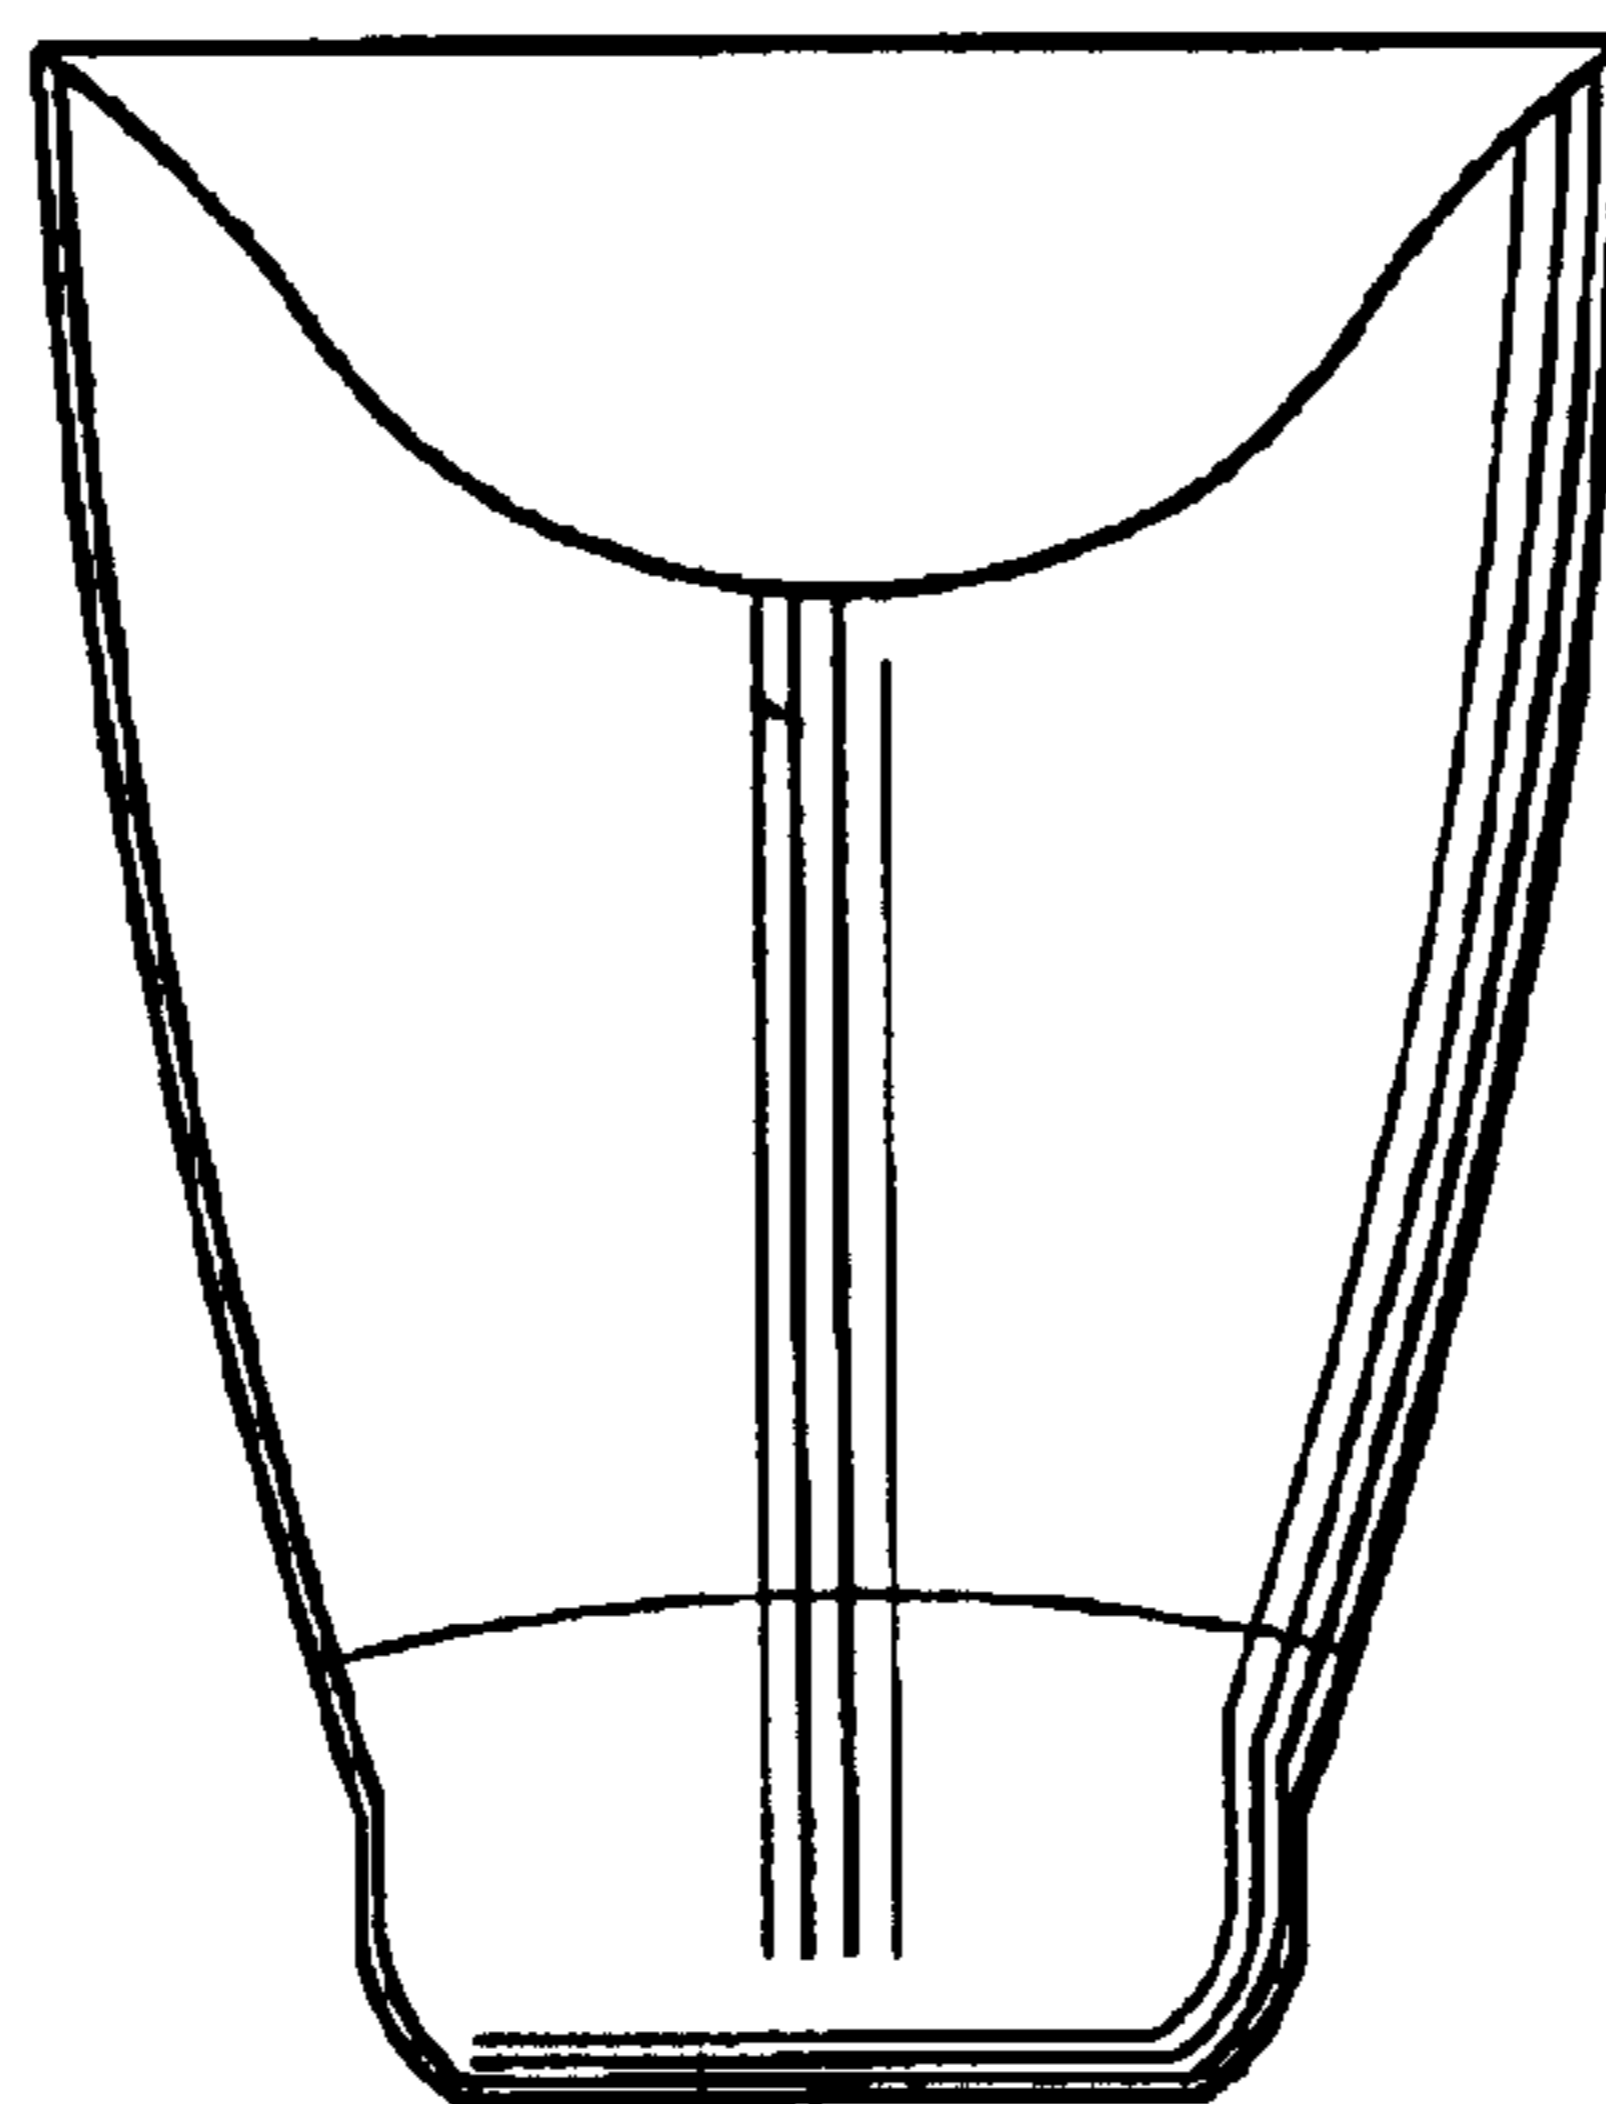


fig. 5

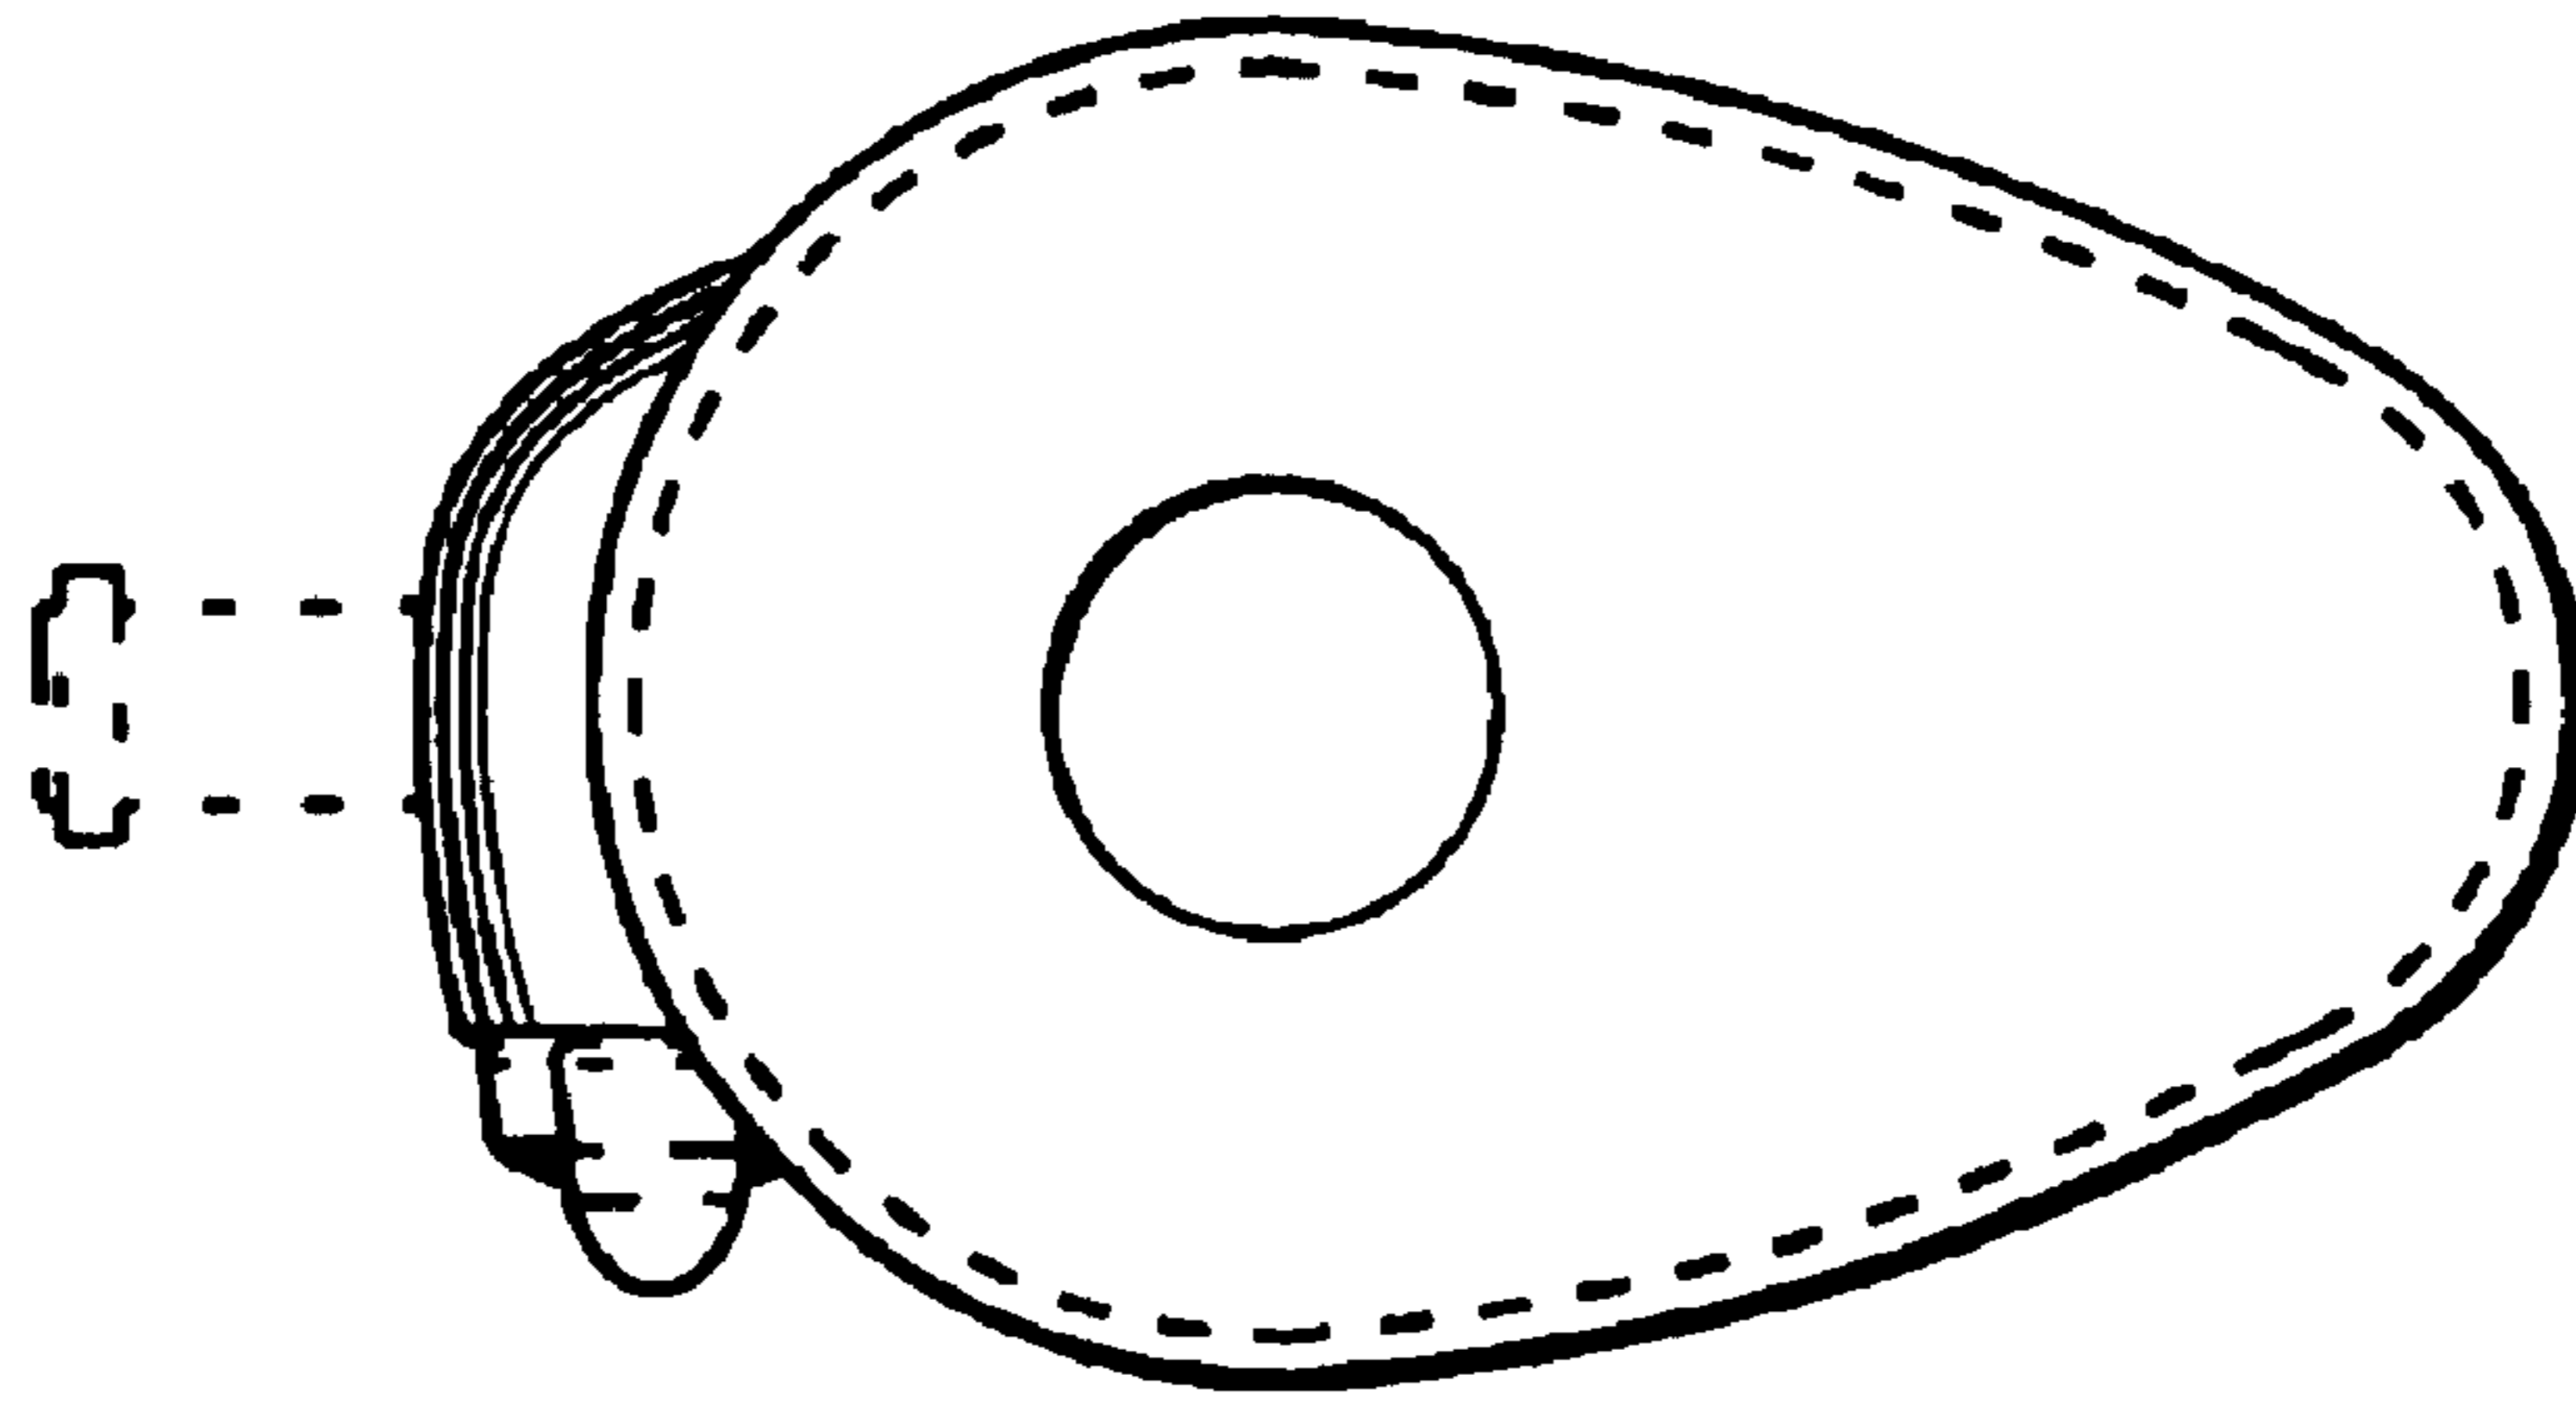


fig. 6

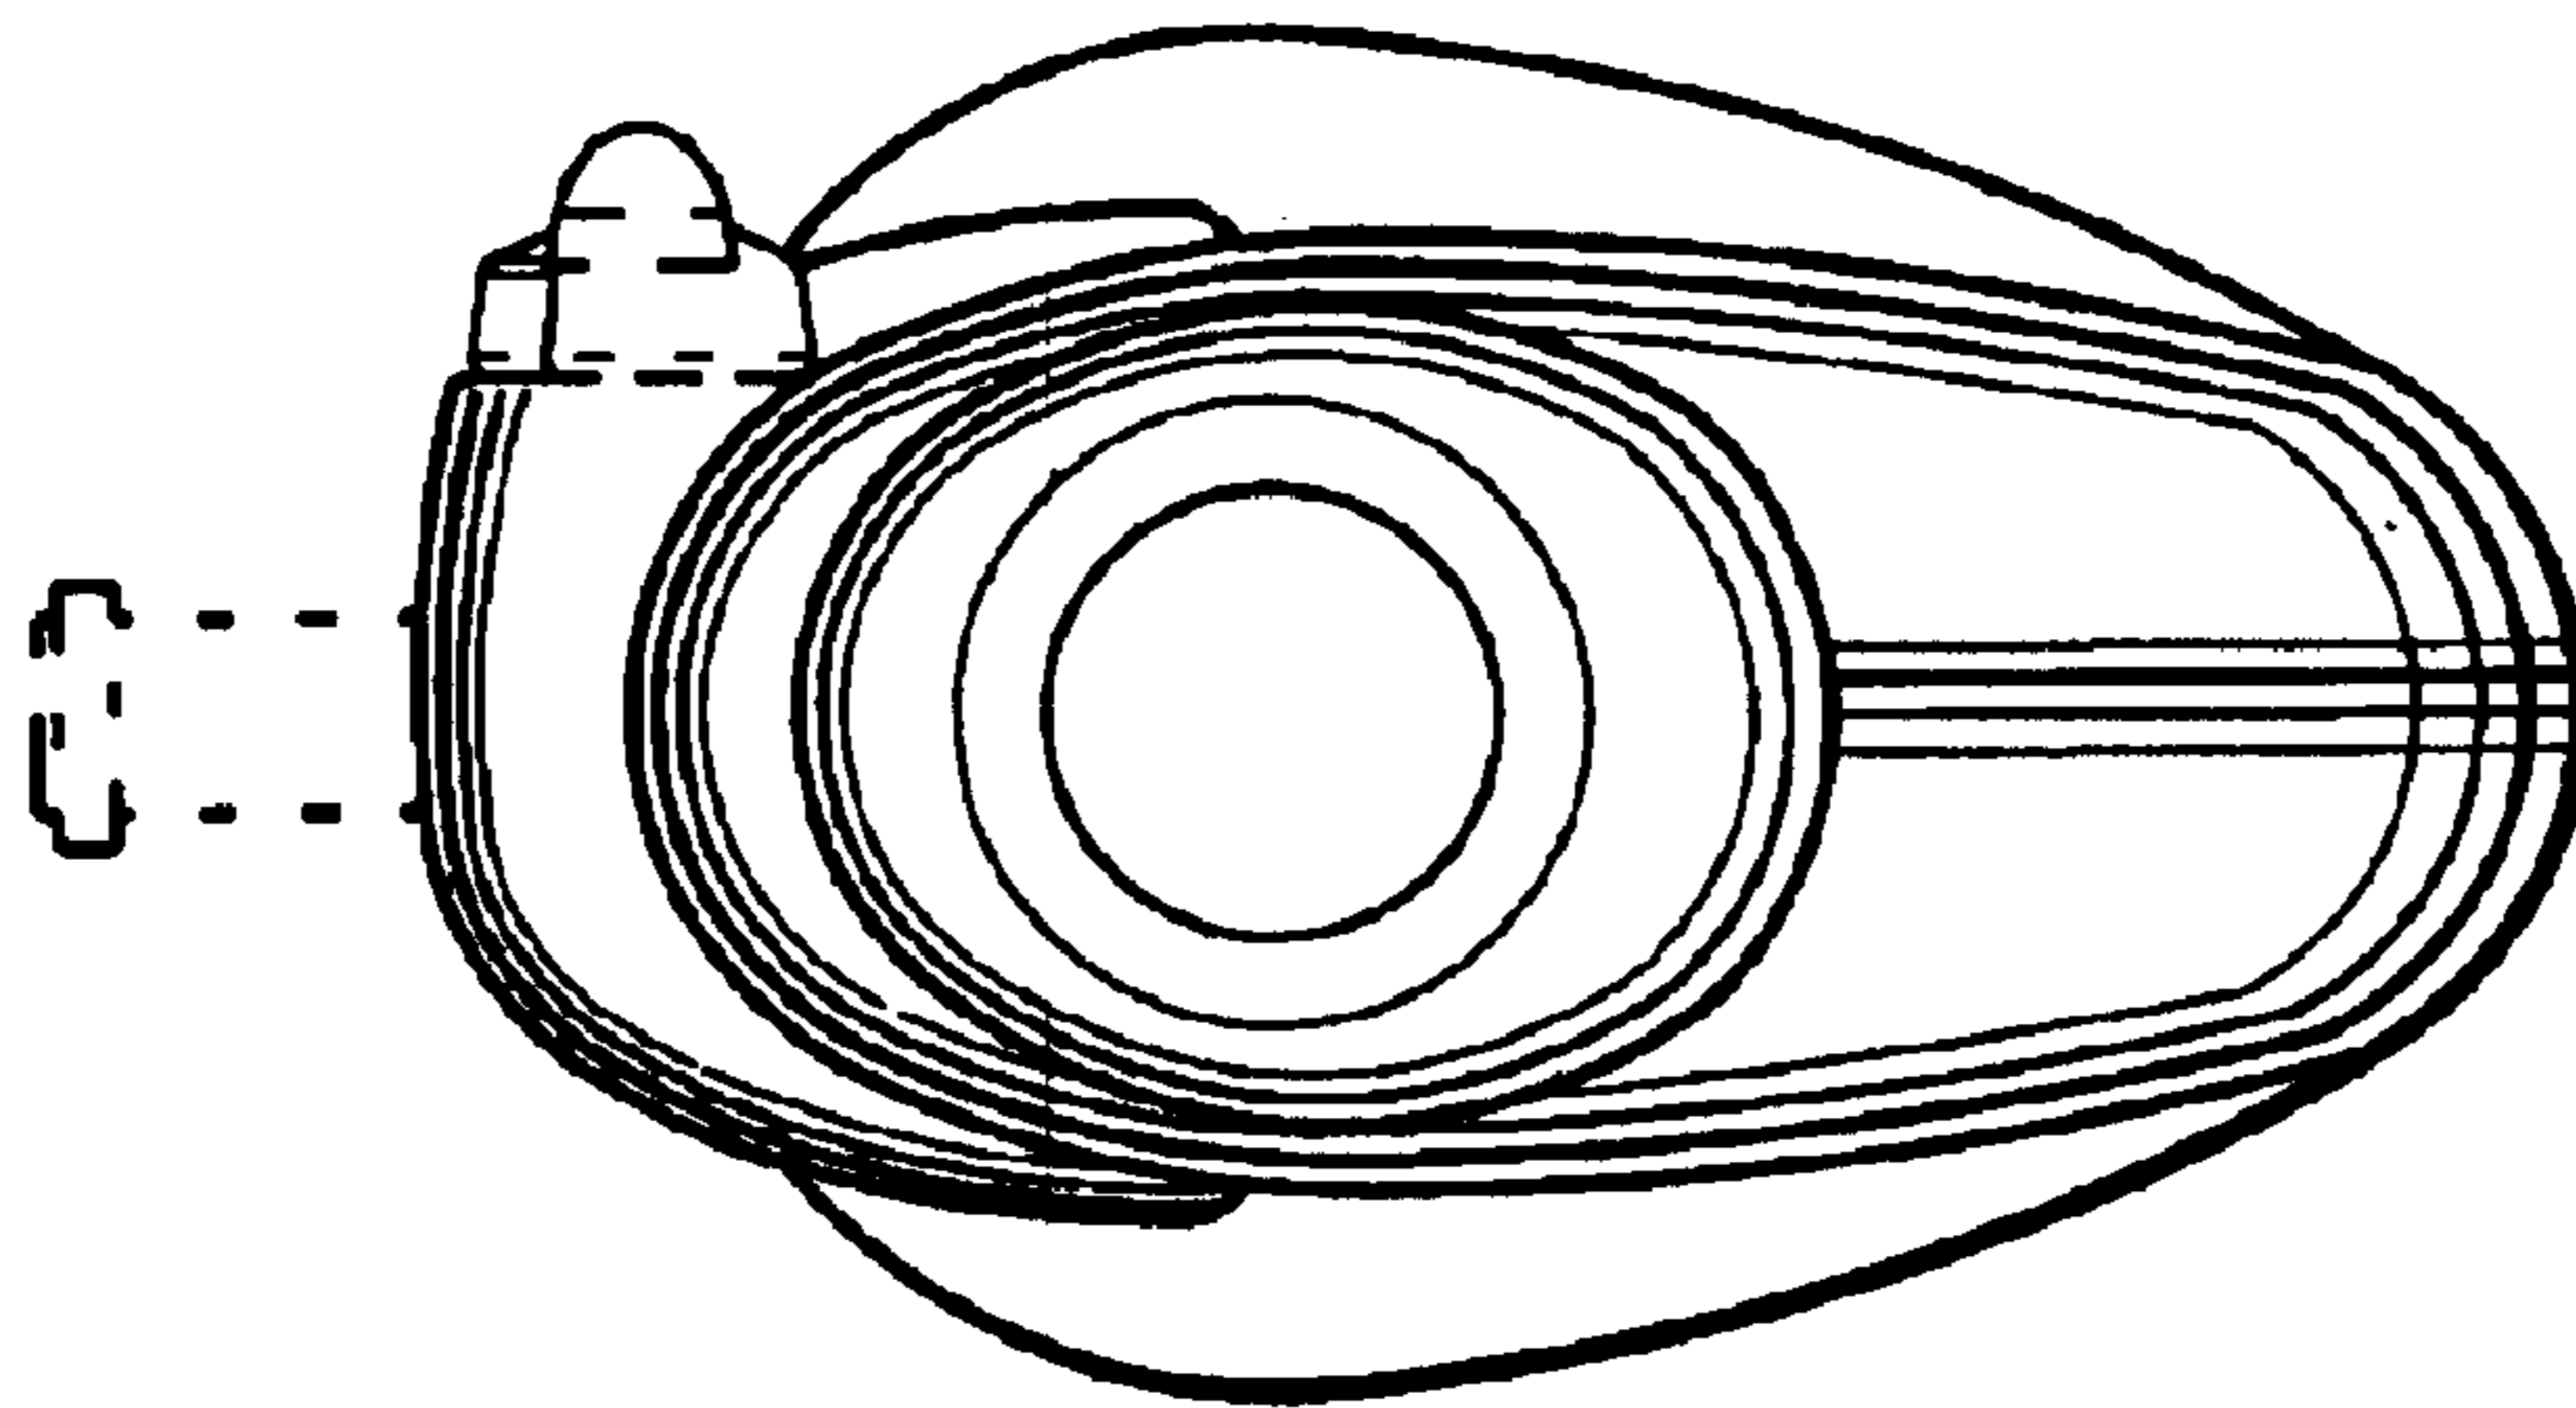


fig. 7

UNITED STATES PATENT AND TRADEMARK OFFICE
CERTIFICATE OF CORRECTION

PATENT NO. : Des. 495,054 S
DATED : August 24, 2004
INVENTOR(S) : Laun

Page 1 of 1

It is certified that error appears in the above-identified patent and that said Letters Patent is hereby corrected as shown below:

Title page.

Item [75], Inventors, delete “**Daniel M. Wing**, Utica, NY (US); and **Frank J. Witkowski**, Syracuse, NY (US)”

Signed and Sealed this

Fourteenth Day of December, 2004

A handwritten signature in black ink on a dotted background. The signature reads "Jon W. Dudas" in a cursive style.

JON W. DUDAS

Director of the United States Patent and Trademark Office