

US00D499805S

(12) **United States Design Patent** (10) **Patent No.:** **US D499,805 S**
D'Agostino (45) **Date of Patent:** **** Dec. 14, 2004**

(54) **METER FOR DETERMINING CONCENTRATION OF ANALYTES**

(75) Inventor: **Daniel M. D'Agostino**, Brighton, MA (US)

(73) Assignee: **Abbott Park**, Abbott Park, IL (US)

(**) Term: **14 Years**

(21) Appl. No.: **29/193,861**

(22) Filed: **Nov. 14, 2003**

(51) **LOC (7) Cl.** **24-01**

(52) **U.S. Cl.** **D24/169; D10/81**

(58) **Field of Search** D10/81; D24/169; 205/777.5; 422/56, 58, 68.1, 82.05, 99, 102, 104, 504; 436/44, 514; 600/300, 309, 316, 318, 322, 347, 365, 383, 578

(56) **References Cited**

U.S. PATENT DOCUMENTS

| | | | | |
|-----------|------|---------|---------------------|---------|
| 4,627,445 | A | 12/1986 | Garcia et al. | |
| 4,637,403 | A | 1/1987 | Garcia et al. | |
| 4,787,398 | A | 11/1988 | Garcia et al. | |
| D318,331 | S | 7/1991 | Phillips et al. | |
| 5,029,583 | A | 7/1991 | Meserol et al. | |
| 5,445,967 | A * | 8/1995 | Deuter | 436/164 |
| D369,864 | S | 5/1996 | Petersen | |
| 5,515,170 | A * | 5/1996 | Matzinger et al. | 356/423 |
| D371,198 | S | 6/1996 | Savage et al. | |
| D371,440 | S | 7/1996 | Petersen | |
| D378,612 | S | 3/1997 | Clark et al. | |
| 5,714,123 | A * | 2/1998 | Sohrab | 422/99 |
| D393,313 | S | 4/1998 | Meisner et al. | |
| D393,314 | S | 4/1998 | Meisner et al. | |
| D399,565 | S | 10/1998 | Prokop et al. | |
| D399,959 | S | 10/1998 | Prokop et al. | |
| D399,960 | S | 10/1998 | Prokop et al. | |
| D402,369 | S | 12/1998 | Prokop et al. | |
| D411,621 | S * | 6/1999 | Eisenbarth et al. | D24/169 |
| D417,504 | S * | 12/1999 | Love et al. | D24/169 |
| D418,602 | S | 1/2000 | Prokop et al. | |
| 6,424,847 | B1 * | 7/2002 | Mastrototaro et al. | 600/316 |
| 6,506,168 | B1 * | 1/2003 | Fathallah et al. | 600/578 |

| | | | | |
|--------------|------|---------|--------------------|-----------|
| D471,983 | S * | 3/2003 | Hippolyte et al. | D24/169 |
| 6,562,625 | B2 * | 5/2003 | Modzelewski et al. | 436/44 |
| 2002/0115912 | A1 * | 8/2002 | Muraki et al. | 600/300 |
| 2002/0161288 | A1 * | 10/2002 | Shin et al. | 600/316 |
| 2003/0021729 | A1 * | 1/2003 | Moller et al. | 422/68.1 |
| 2003/0119202 | A1 * | 6/2003 | Kaylor et al. | 436/514 |
| 2003/0159944 | A1 * | 8/2003 | Pottgen et al. | 205/777.5 |
| 2004/0073095 | A1 * | 4/2004 | Causey et al. | 600/300 |

OTHER PUBLICATIONS

MediSense, Inc., ExactTech® R.S.G.™, Blood Glucose Testing System for In vitro Diagnostic Use, User's Manual, ©1996. Rev. 9/96.

Lifescan, Inc., SureStep™, Complete Blood Glucose Monitoring System, Owner's Booklet, © 1995.

(List continued on next page.)

Primary Examiner—Antoine D. Davis

(74) *Attorney, Agent, or Firm*—David L. Weinstein

(57) **CLAIM**

I claim the ornamental design for a meter for determining concentration of analytes, as shown and described.

DESCRIPTION

FIG. 1 is a perspective view of the front of a meter for determining concentration of analytes, hereinafter referred to as the meter.

FIG. 2 is a perspective view of the rear of the meter of FIG. 1.

FIG. 3 is a top plan view of the front of the meter of FIG. 1.

FIG. 4 is a view in elevation of the top of the meter of FIG. 1.


FIG. 5 is a view in elevation of the bottom of the meter of FIG. 1.

FIG. 6 is a side view in elevation of the right side of the meter of FIG. 1.

FIG. 7 is a side view in elevation of the left side of the meter of FIG. 1; and,

FIG. 8 is a top plan view of the rear of the meter of FIG. 1.

1 Claim, 4 Drawing Sheets

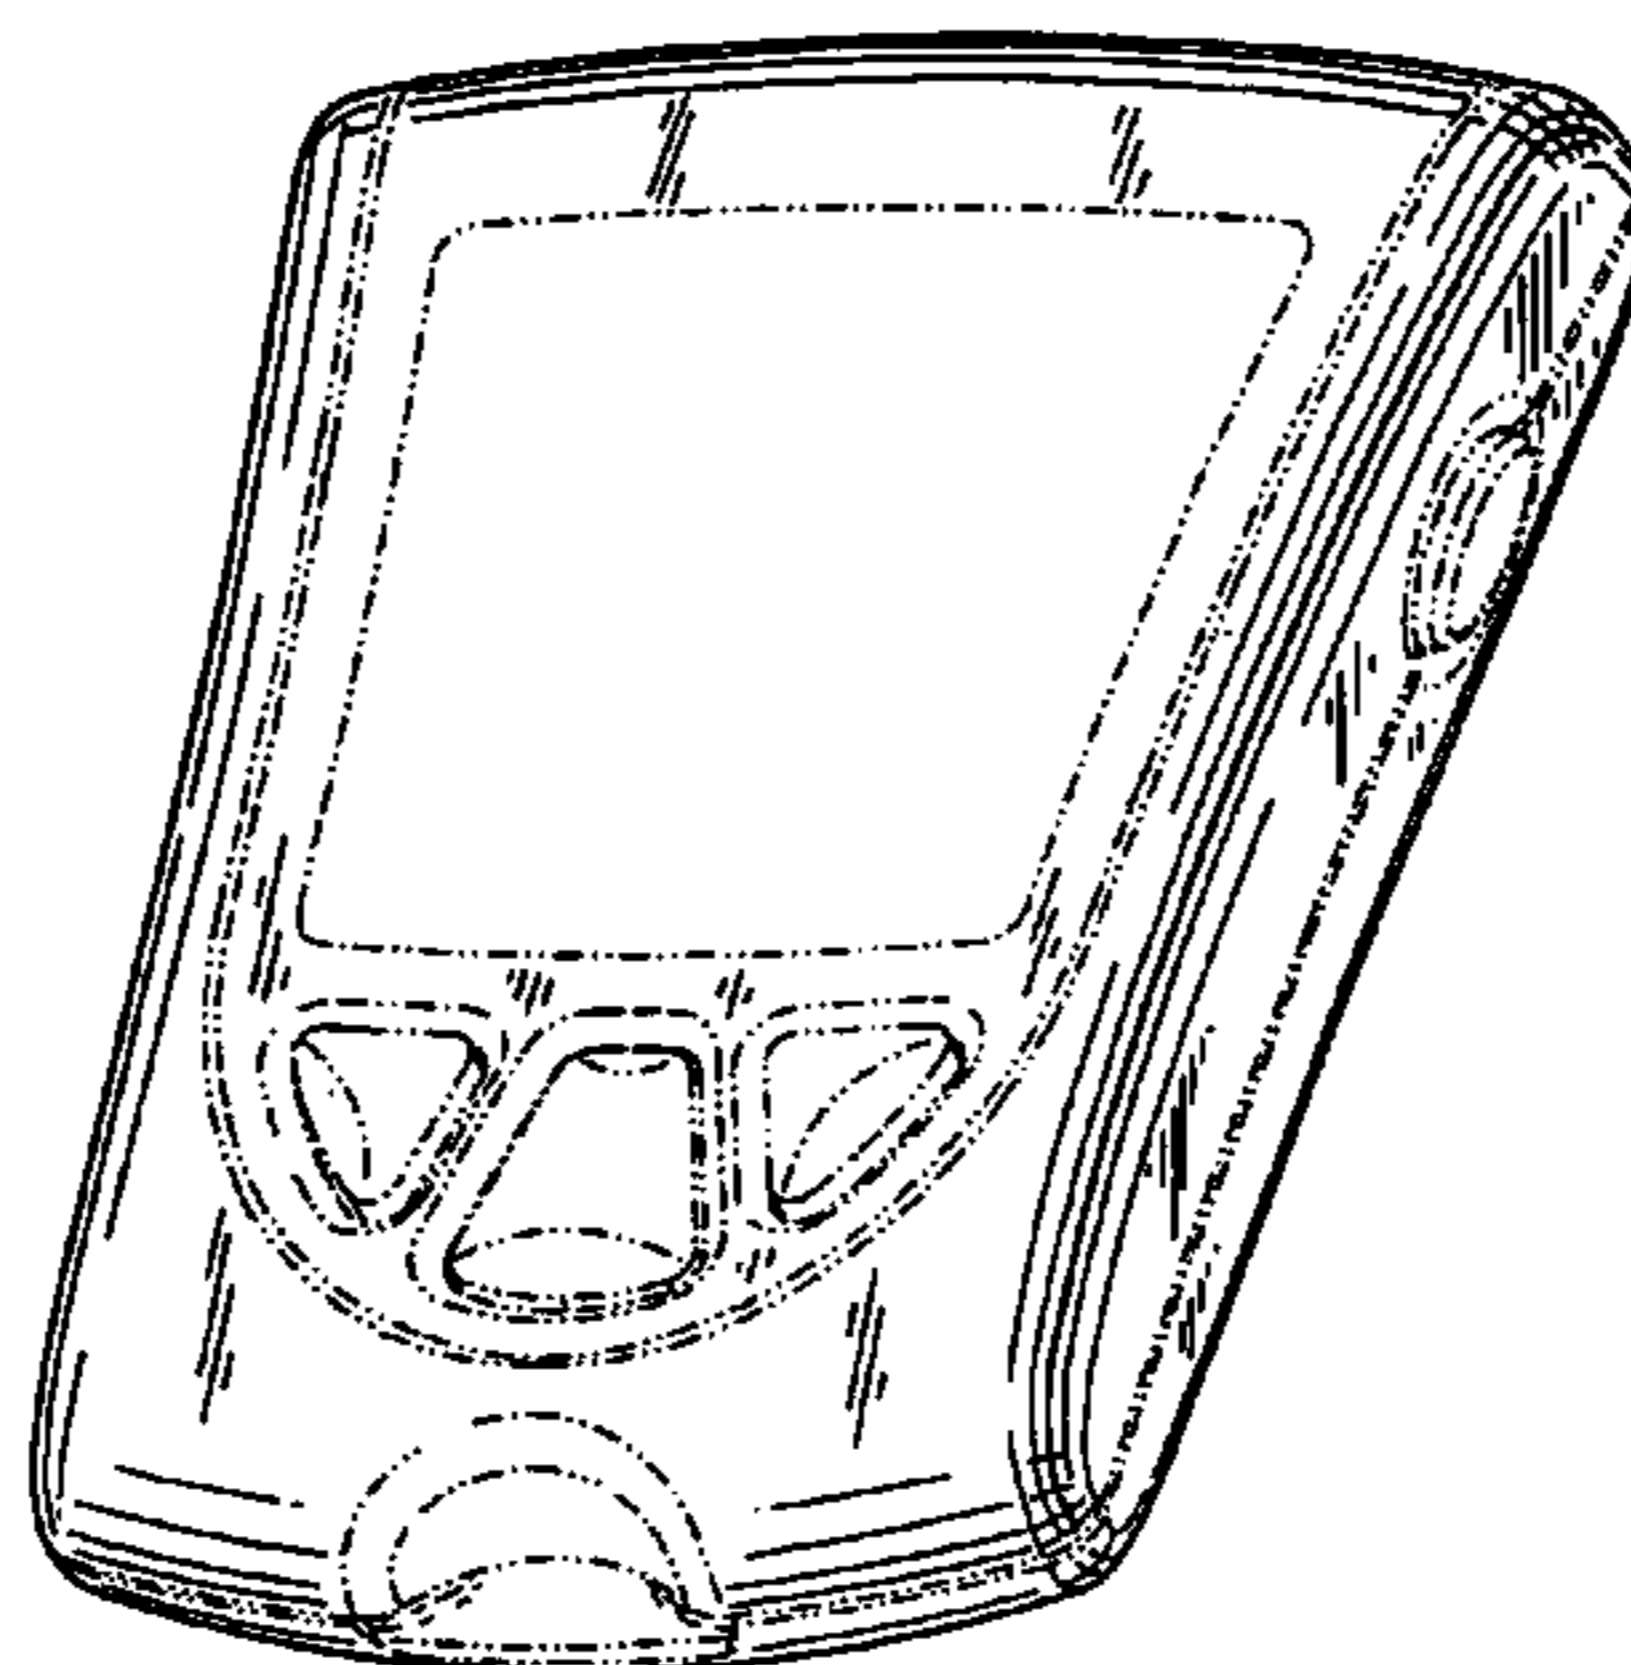

OTHER PUBLICATIONS

Lifescan, Inc., One Touch® Profile™, Diabetes Tracking System, Owner's Booklet, ©1995.

Miles, Inc., Glucometer ENCORE™, Diabetes Care System, User Guide, ©1994. Rev. 3/94.

MediSense, Inc., Pen™2 Companion™2 Sensor, Blood Glucose Testing System, User's Manual, ©1992. Rev. 12/92.

Lifescan, Inc., One Touch® Basic™, Blood Glucose Monitoring System, Owner's Booklet, ©1993. Rev. 2/93.

Miles, Inc., Glucometer ELITE™, Diabetes Care System, User guide, ©1993. Rev. 2/93.

MediSense, Inc., Precision Q.I.D™, Blood Glucose Testing System for In Vitro Diagnostic Use, User's Manual. ©1994. Rev. 12/94.

MediSense, Inc., MediSense® 2, Blood Glucose Testing System for In Vitro Diagnostic Use, User's Manual, ©1994, Rev. 12/94.

Boehringer Mannheim Corp., Accu-Chek® Easy™, Blood Glucose Monitoring System, User's Manual, ©1995.

Boehringer Mannheim Corp., Accu-Chek® Instant™, Blood Glucose Monitoring System, User's Manual.

Boehringer Mannheim Corp., Accu-Chek® ADVANTAGE™, Blood Glucose Monitor, User's Manual.

Lifescan, Inc., One Touch®, Ultra Smart™, Blood Glucose Monitoring System, Owner's Booklet, © 2002, cover pages and pages x, 2.

* cited by examiner

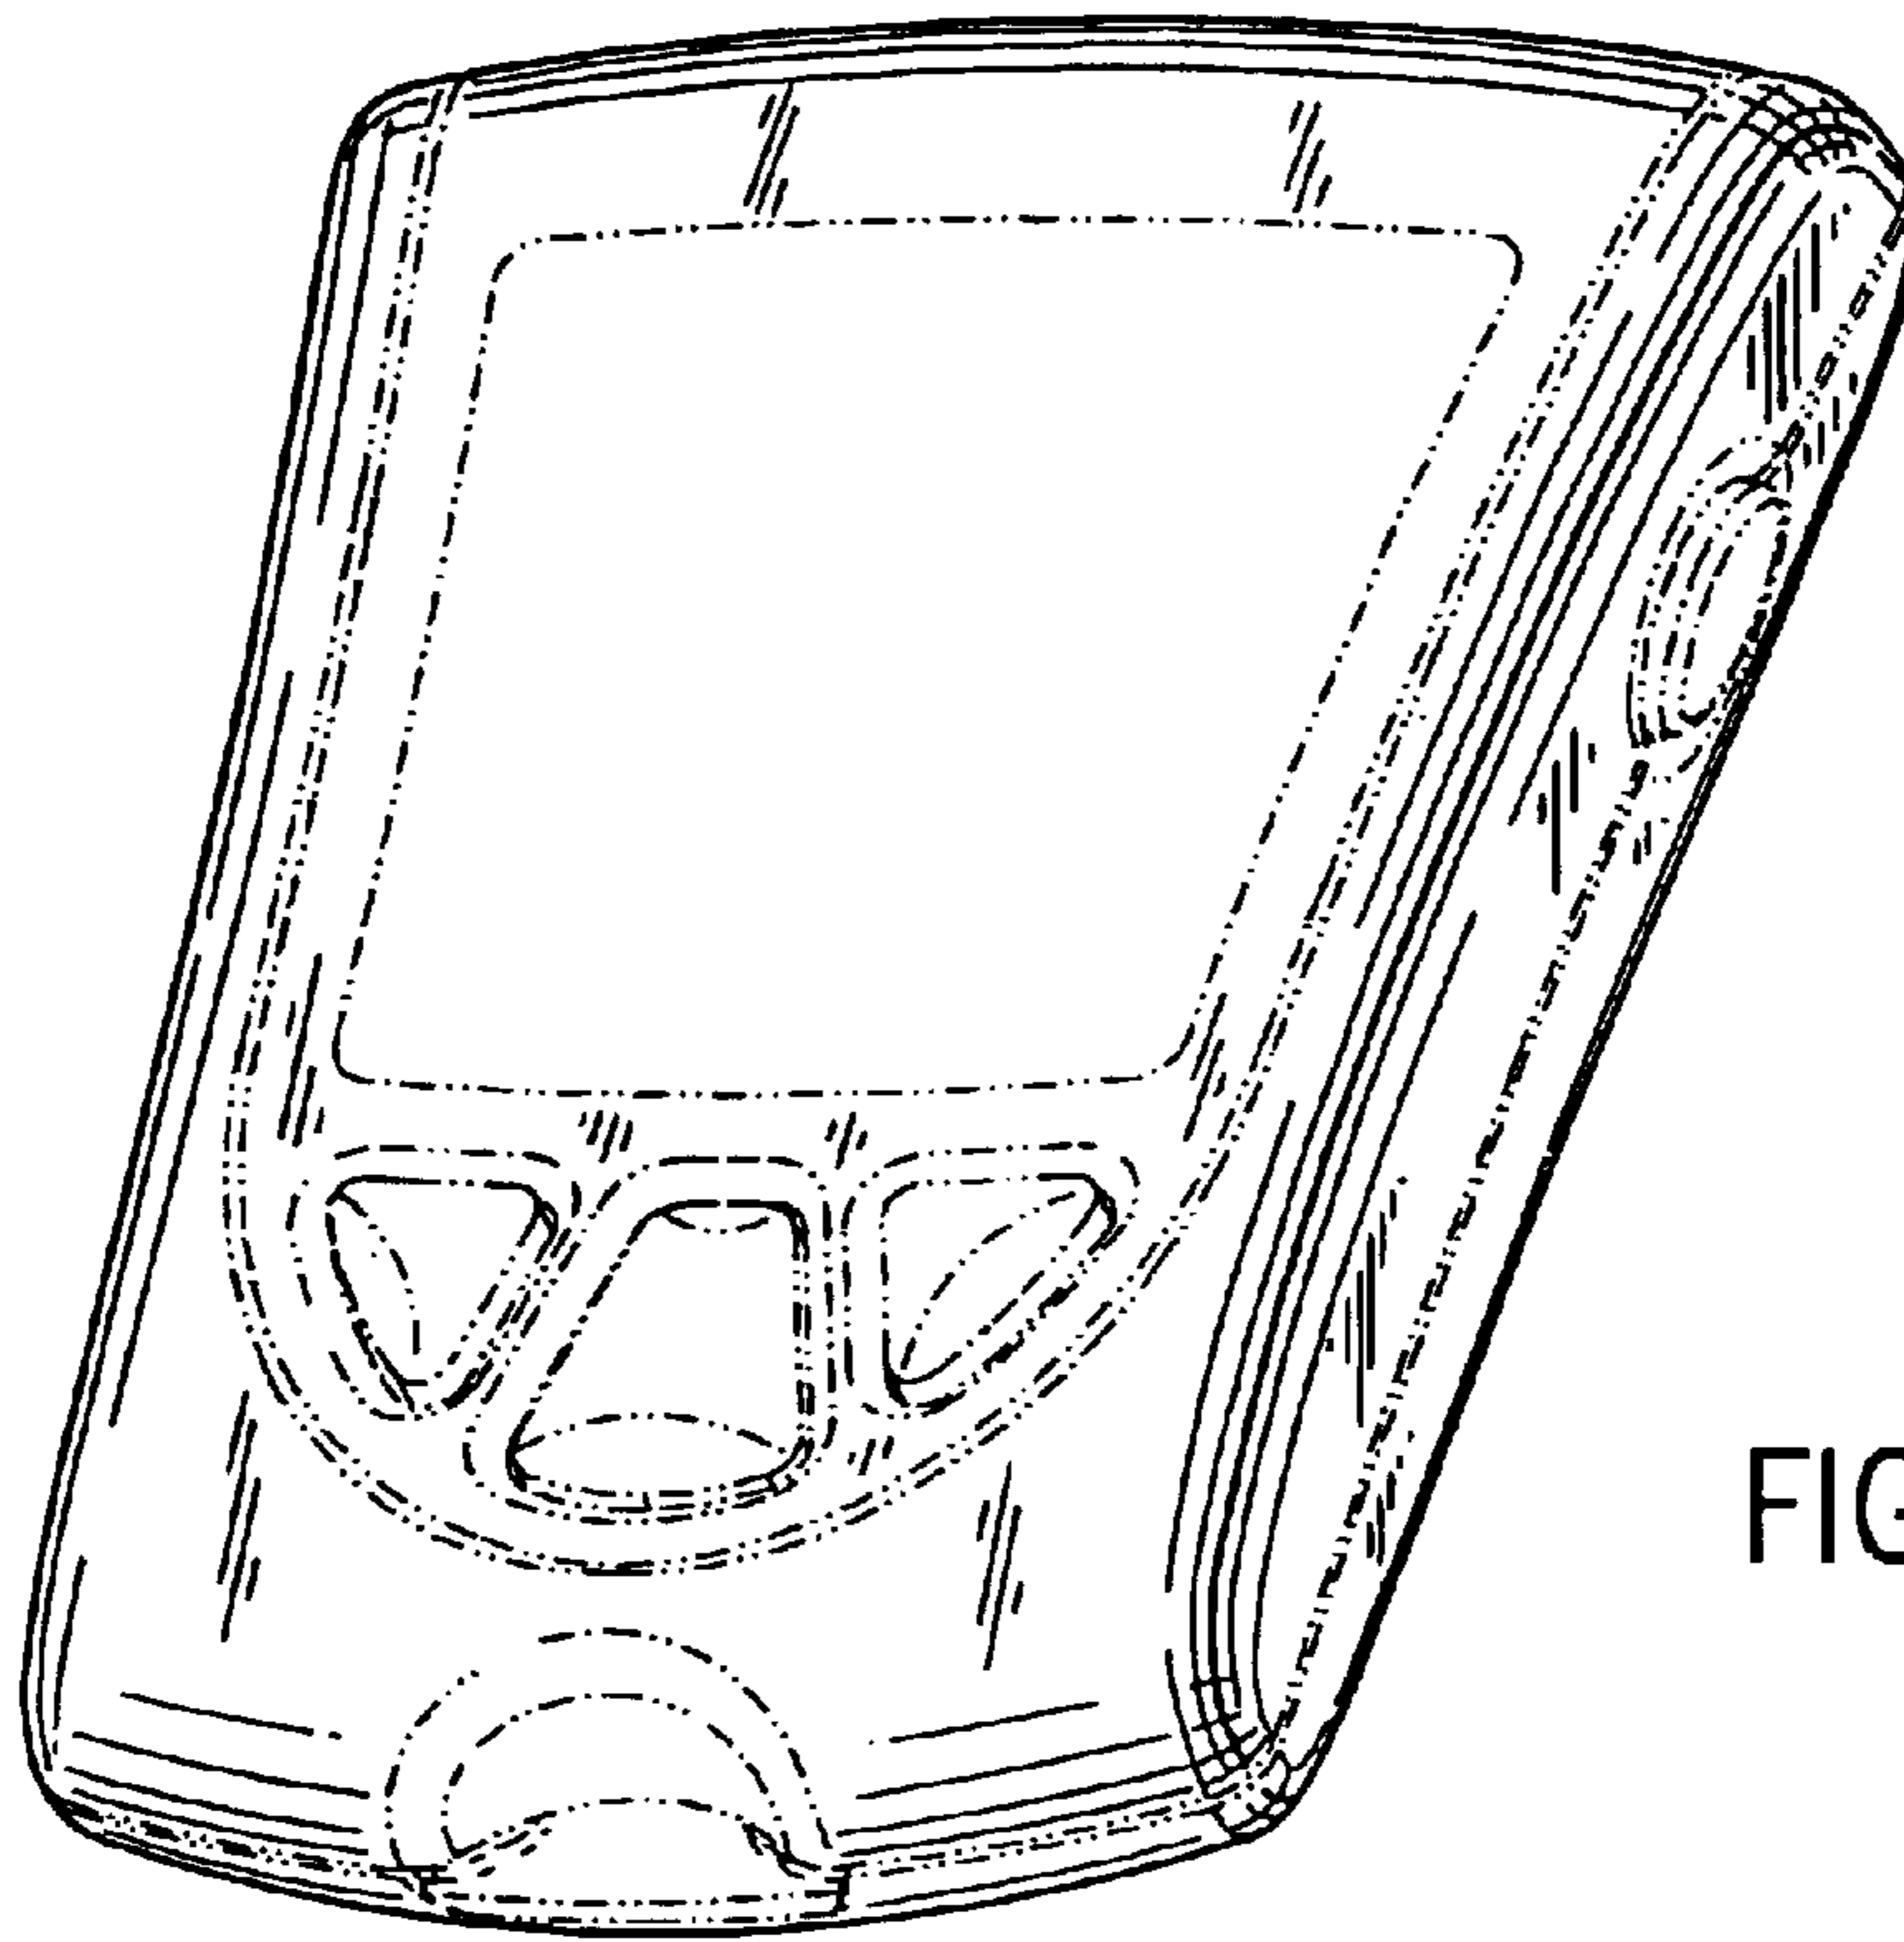


FIG. 1

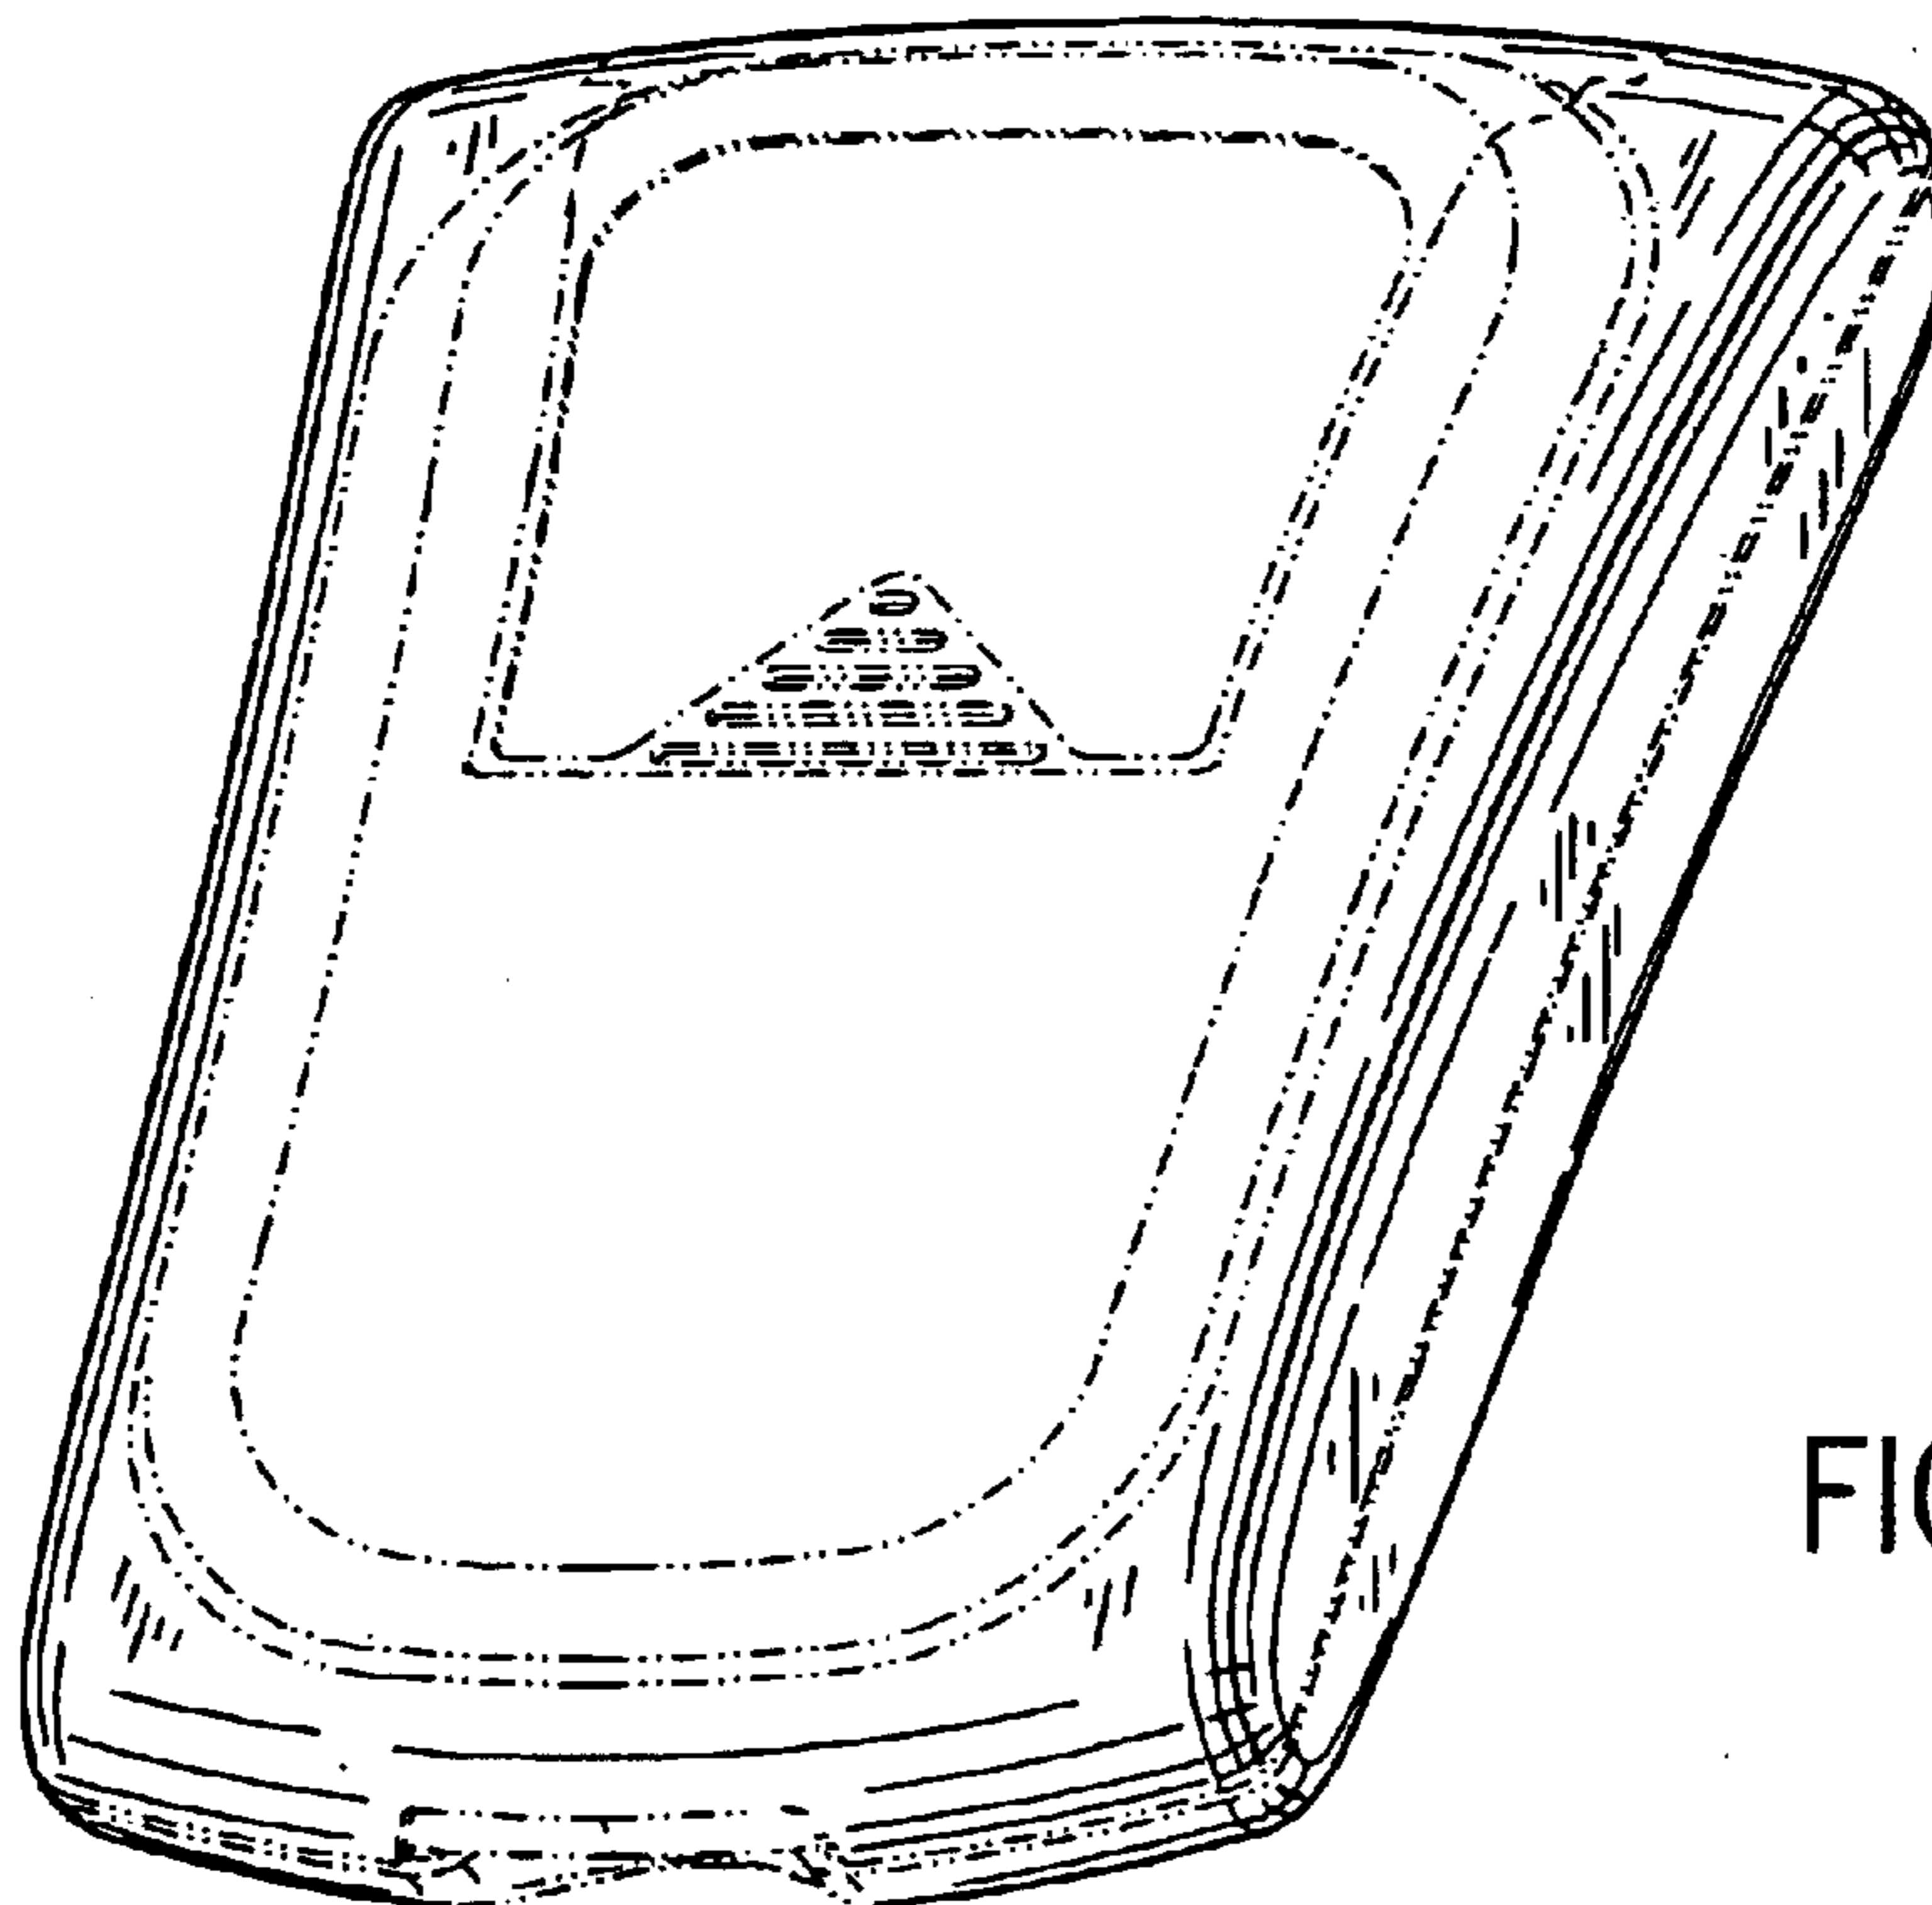


FIG. 2

FIG. 3

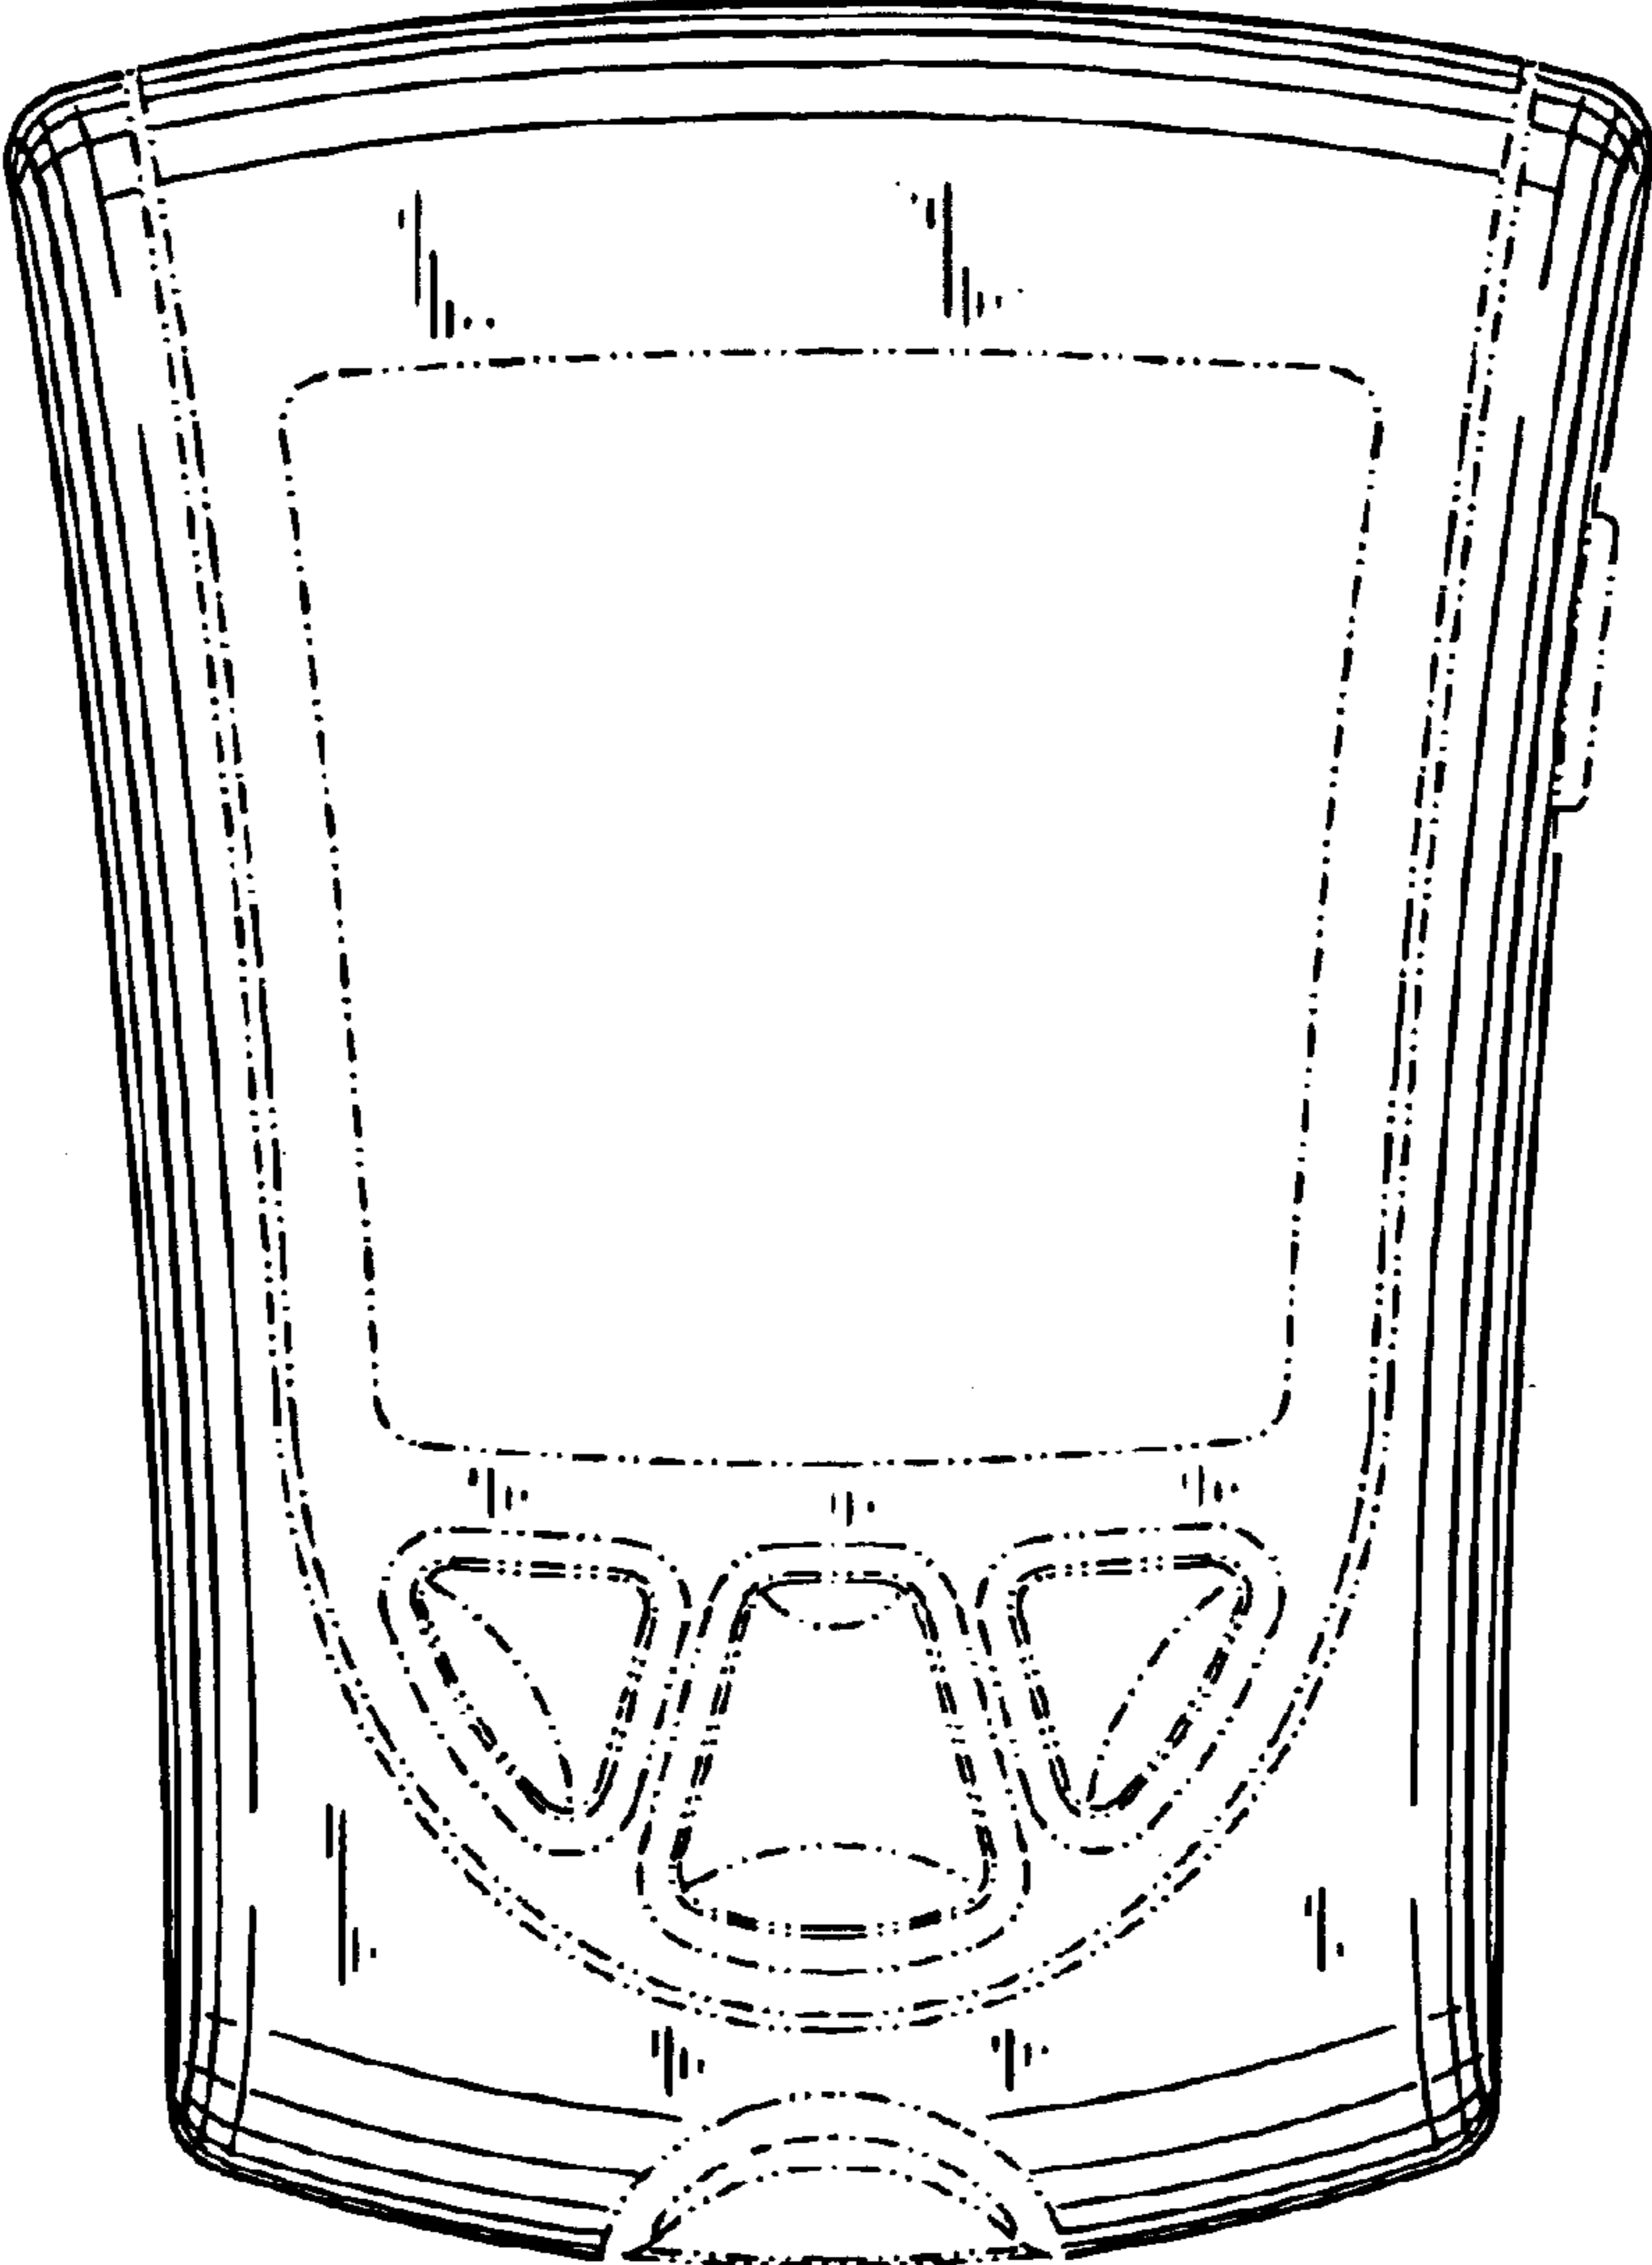


FIG. 4

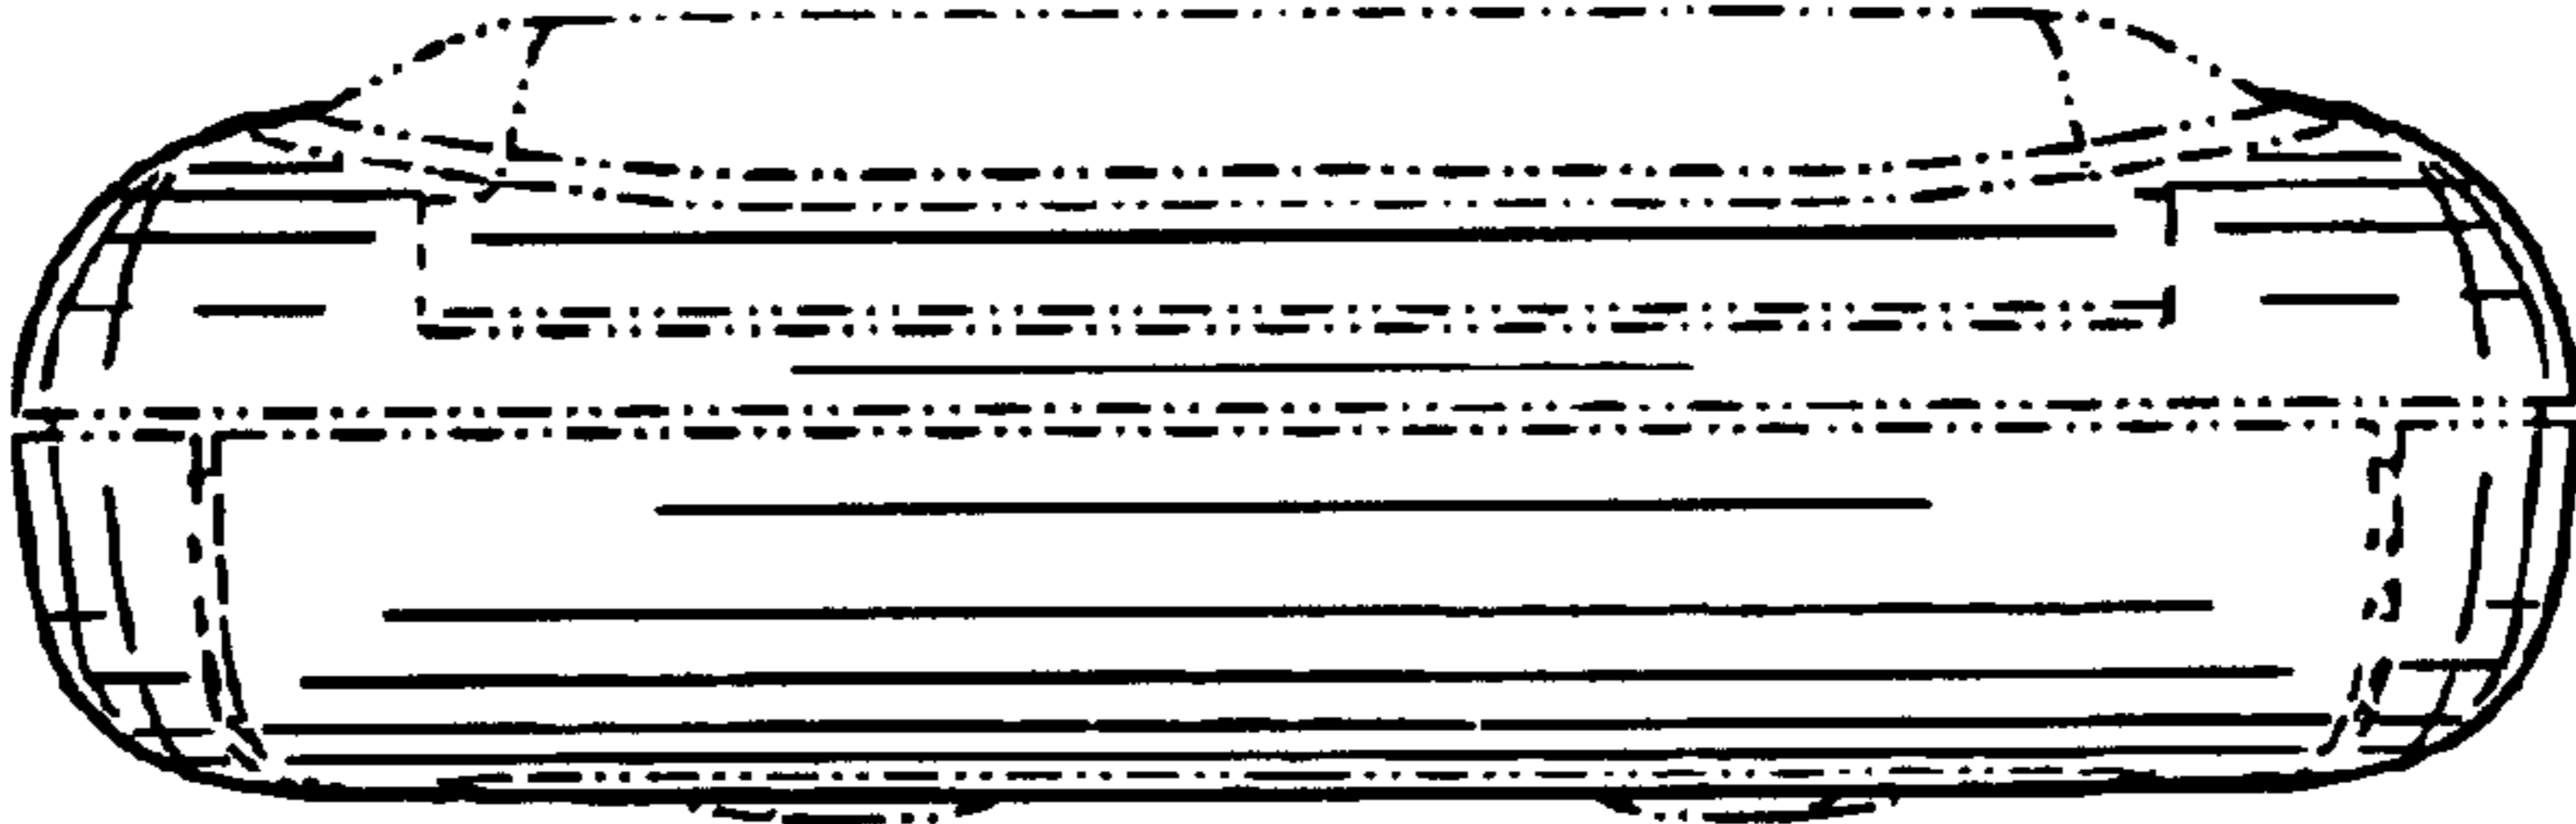


FIG. 5

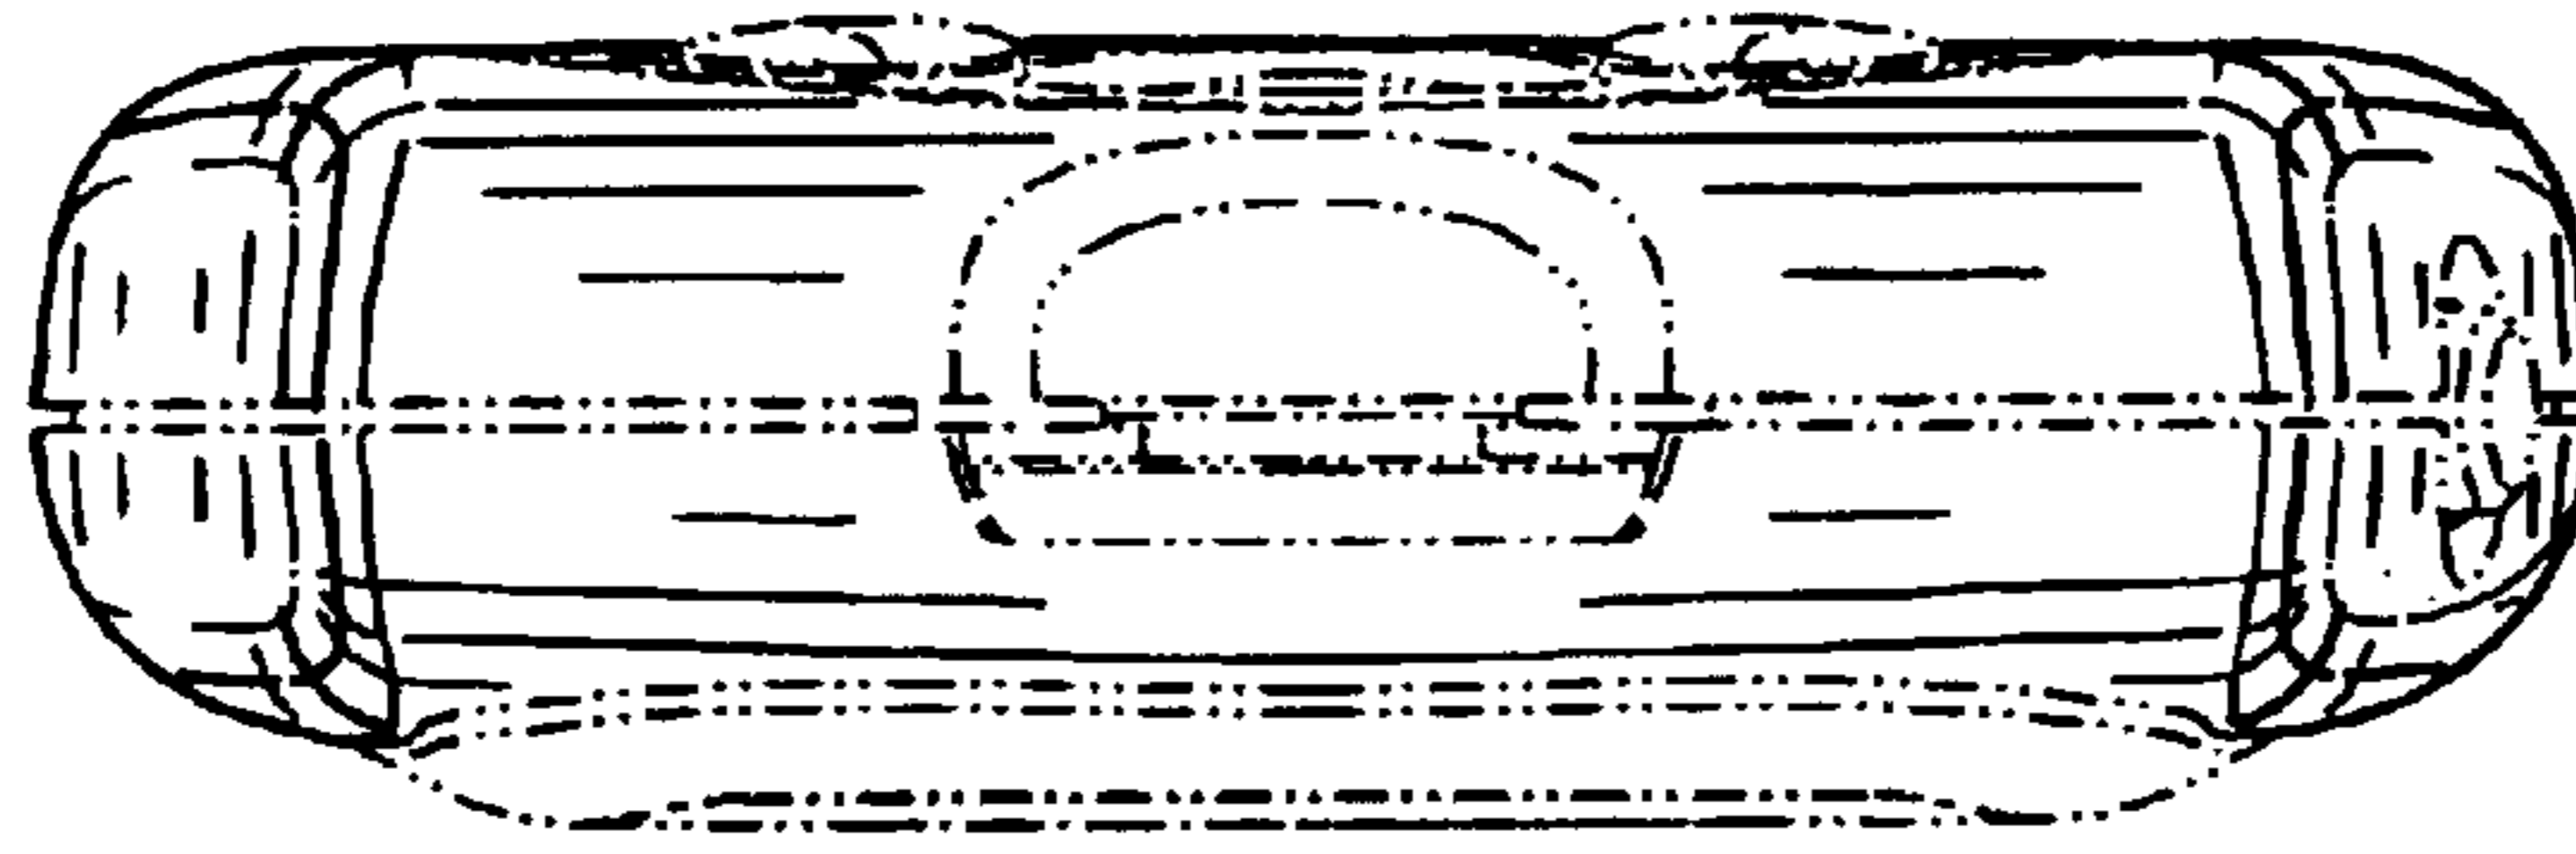


FIG. 6

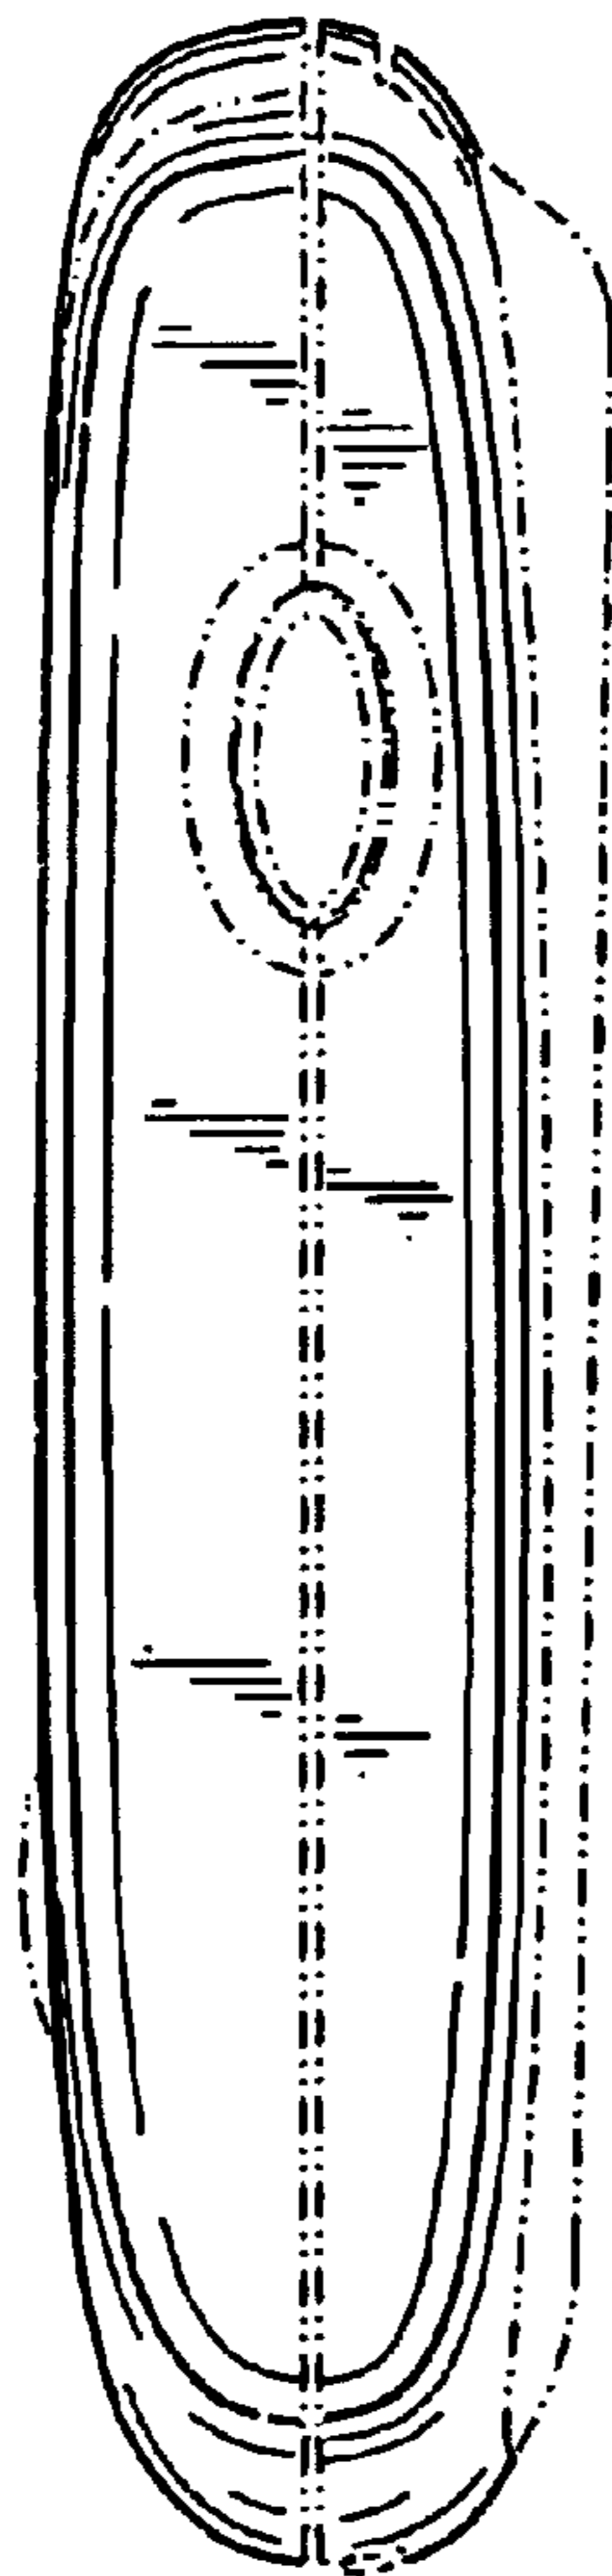
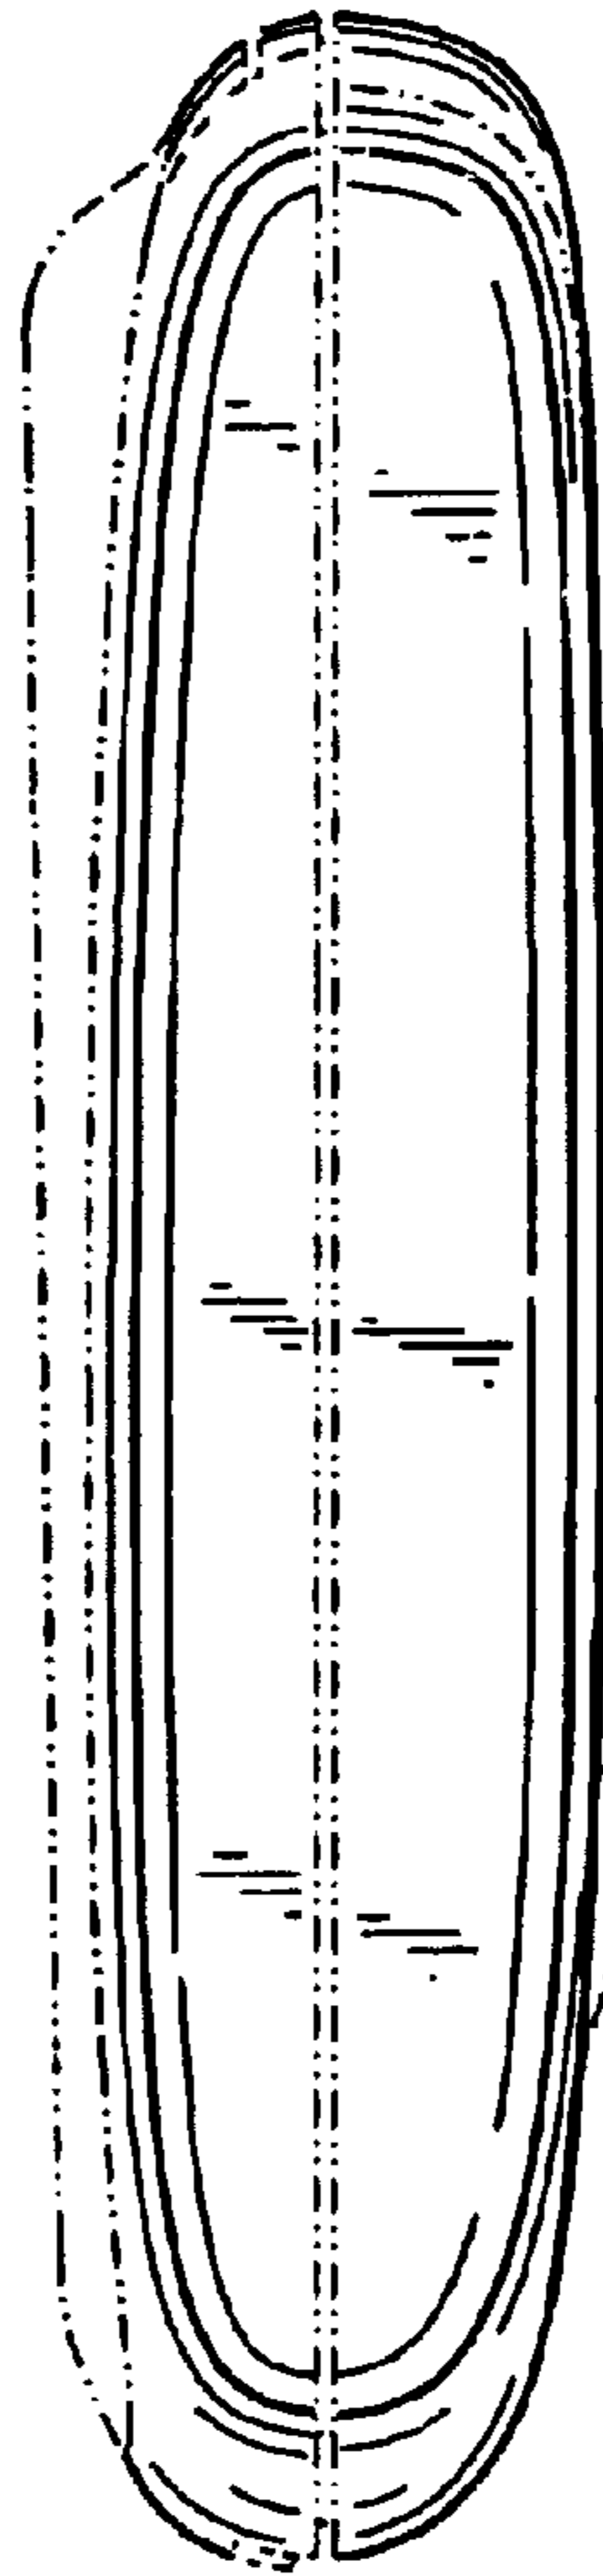


FIG. 7



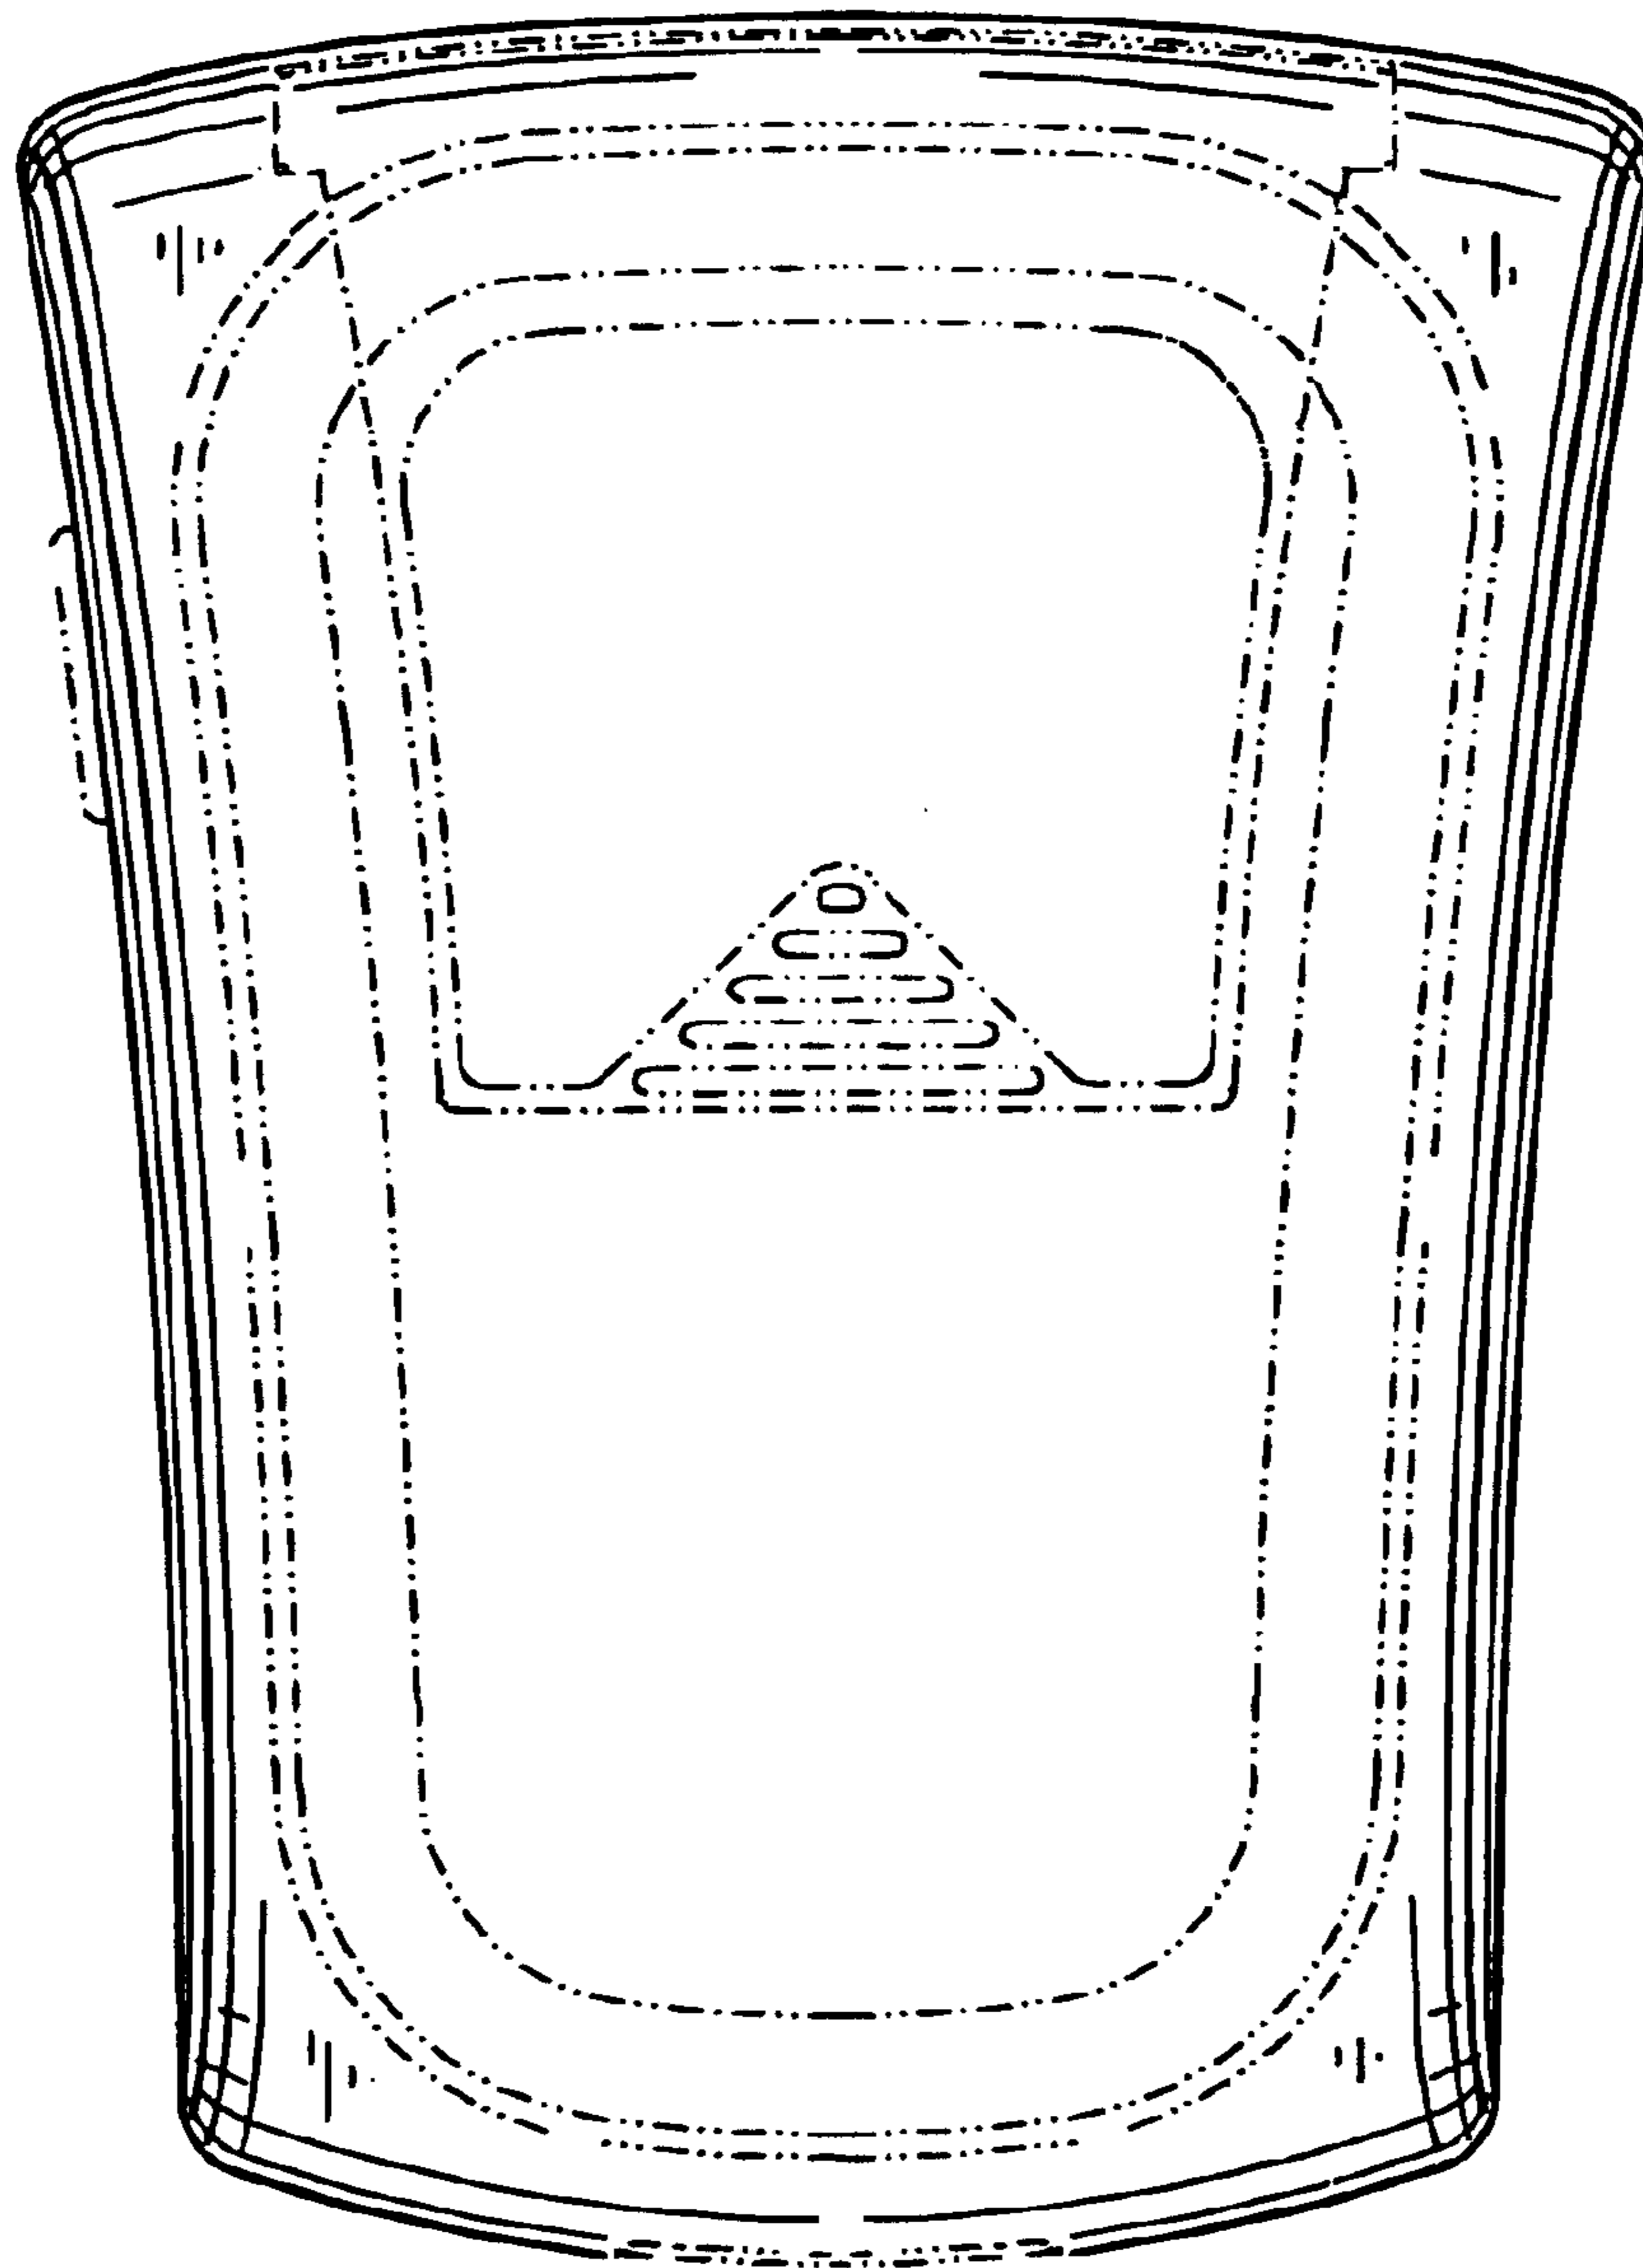


FIG. 8