



US00D512512S

(12) **United States Design Patent** (10) **Patent No.:** **US D512,512 S**  
**Bell et al.** (45) **Date of Patent:** **\*\* Dec. 6, 2005**

(54) **BLOOD GLUCOSE TEST STRIP**

(75) Inventors: **Douglas E. Bell**, Coral Springs, FL (US); **Gary T. Neel**, Weston, FL (US); **Houston F. Voss**, Fort Lauderdale, FL (US)

(73) Assignee: **Wachovia Bank, National Association**, Jacksonville, FL (US)

(\*\*) Term: **14 Years**

(21) Appl. No.: **29/182,200**

(22) Filed: **May 21, 2003**

(51) **LOC (8) Cl.** ..... **24-02**

(52) **U.S. Cl.** ..... **D24/225**

(58) **Field of Search** ..... D24/225, 226, D24/216, 223, 164, 187, 169; D10/81; 600/583, 373, 372, 381; 422/82.01, 99, 58, 56, 102; 204/403.1, 403.11, 403.13, 403.14, 403.2

(56) **References Cited**

**U.S. PATENT DOCUMENTS**

D383,550 S	9/1997	Larson et al.	
6,071,391 A	6/2000	Gotoh et al.	
6,120,676 A	9/2000	Heller et al.	
6,143,164 A	11/2000	Heller et al.	
6,156,173 A	12/2000	Gotoh et al.	
6,258,229 B1	7/2001	Winarta et al.	
6,287,451 B1	9/2001	Winarta et al.	
6,299,757 B1	10/2001	Feldman et al.	
D450,854 S	11/2001	Lipman et al.	
6,338,790 B1	1/2002	Feldman et al.	
D456,083 S	4/2002	Clark et al.	
D456,910 S	5/2002	Clark et al.	
6,447,657 B1 *	9/2002	Bhullar et al. ....	204/403.01
6,461,496 B1	10/2002	Feldman et al.	
6,503,381 B1	1/2003	Gotoh et al.	
6,531,040 B2 *	3/2003	Musho et al. ....	204/403.1
6,572,745 B2 *	6/2003	Rappin et al. ....	204/403.14

6,743,635 B2 *	6/2004	Neel et al. ....	422/82.01
6,749,740 B2 *	6/2004	Liamos et al. ....	204/403.02
2002/0053523 A1	5/2002	Liamos et al.	
2002/0061260 A1 *	5/2002	Husar .....	422/102
2002/0084196 A1	7/2002	Liamos et al.	
2002/0148739 A2	10/2002	Liamos et al.	
2002/0157948 A2	10/2002	Liamos et al.	
2004/0028558 A1 *	2/2004	Pollock et al. ....	422/58

**FOREIGN PATENT DOCUMENTS**

EP	1256798 A1	11/2002
EP	1281955 A1	2/2003

\* cited by examiner

*Primary Examiner*—Ian Simmons


(57) **CLAIM**

The ornamental design for a blood glucose test strip, as shown and described.

**DESCRIPTION**

FIG. 1 is a perspective view of a blood glucose test strip; FIG. 2 is a top view of the blood glucose test strip of FIG. 1; FIG. 3 is a bottom view of the blood glucose test strip of FIG. 1; FIG. 4 is a left view of the blood glucose test strip of FIG. 1; FIG. 5 is right view of the blood glucose test strip of FIG. 1; FIG. 6 is front view of the blood glucose test strip of FIG. 1; FIG. 7 is rear view of the blood glucose test strip of FIG. 1; FIG. 8 is a perspective view of a second embodiment of a blood glucose test strip, with the bottom, left, right, front and rear views being the same as that shown in FIGS. 3, 4, 5, 6 and 7; and, FIG. 9 is a top view of the blood glucose test strip of FIG. 8.

**1 Claim, 5 Drawing Sheets**

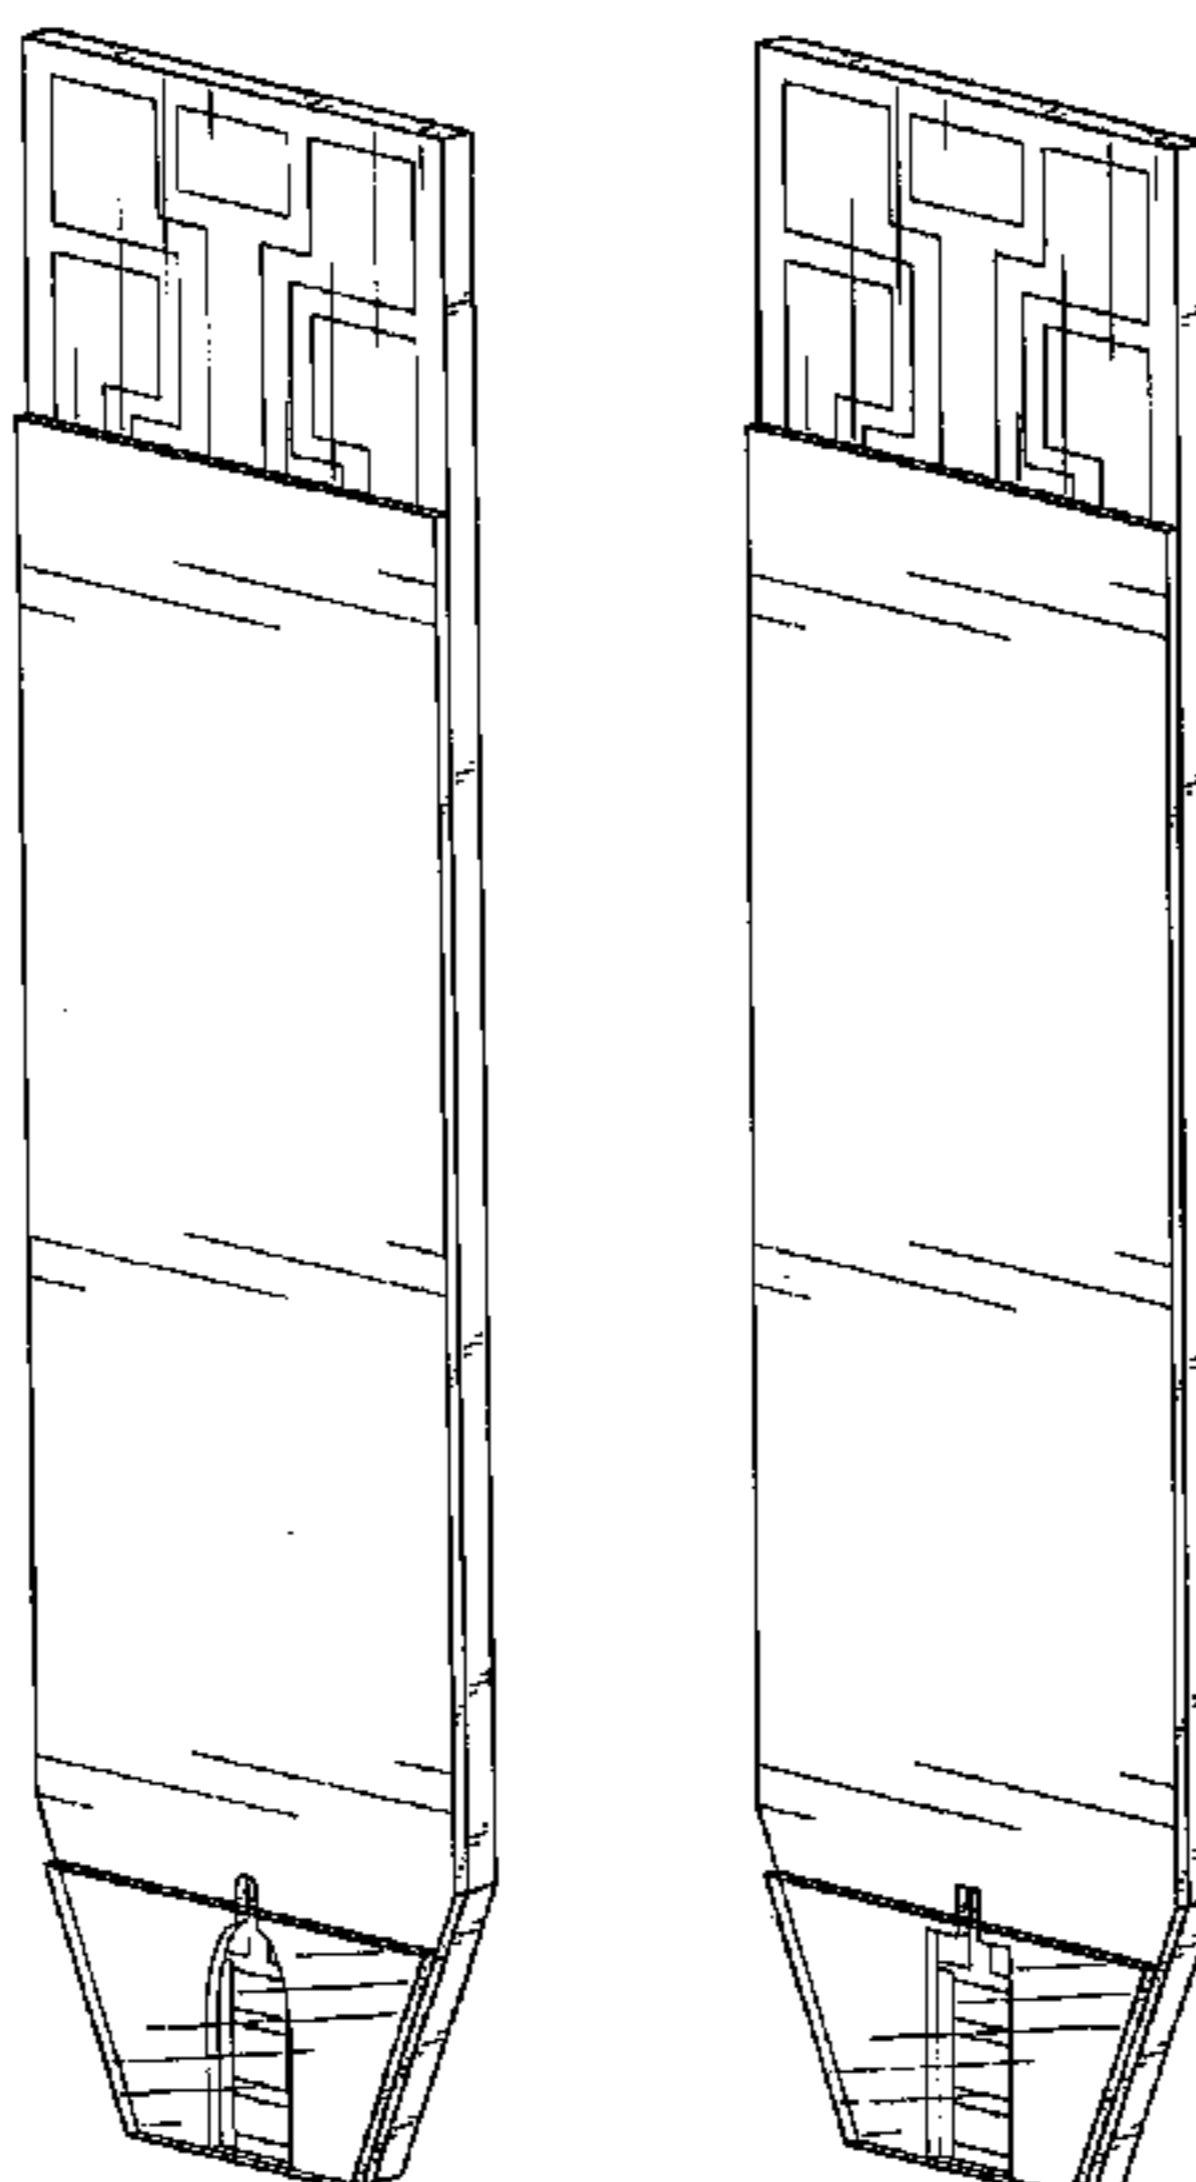

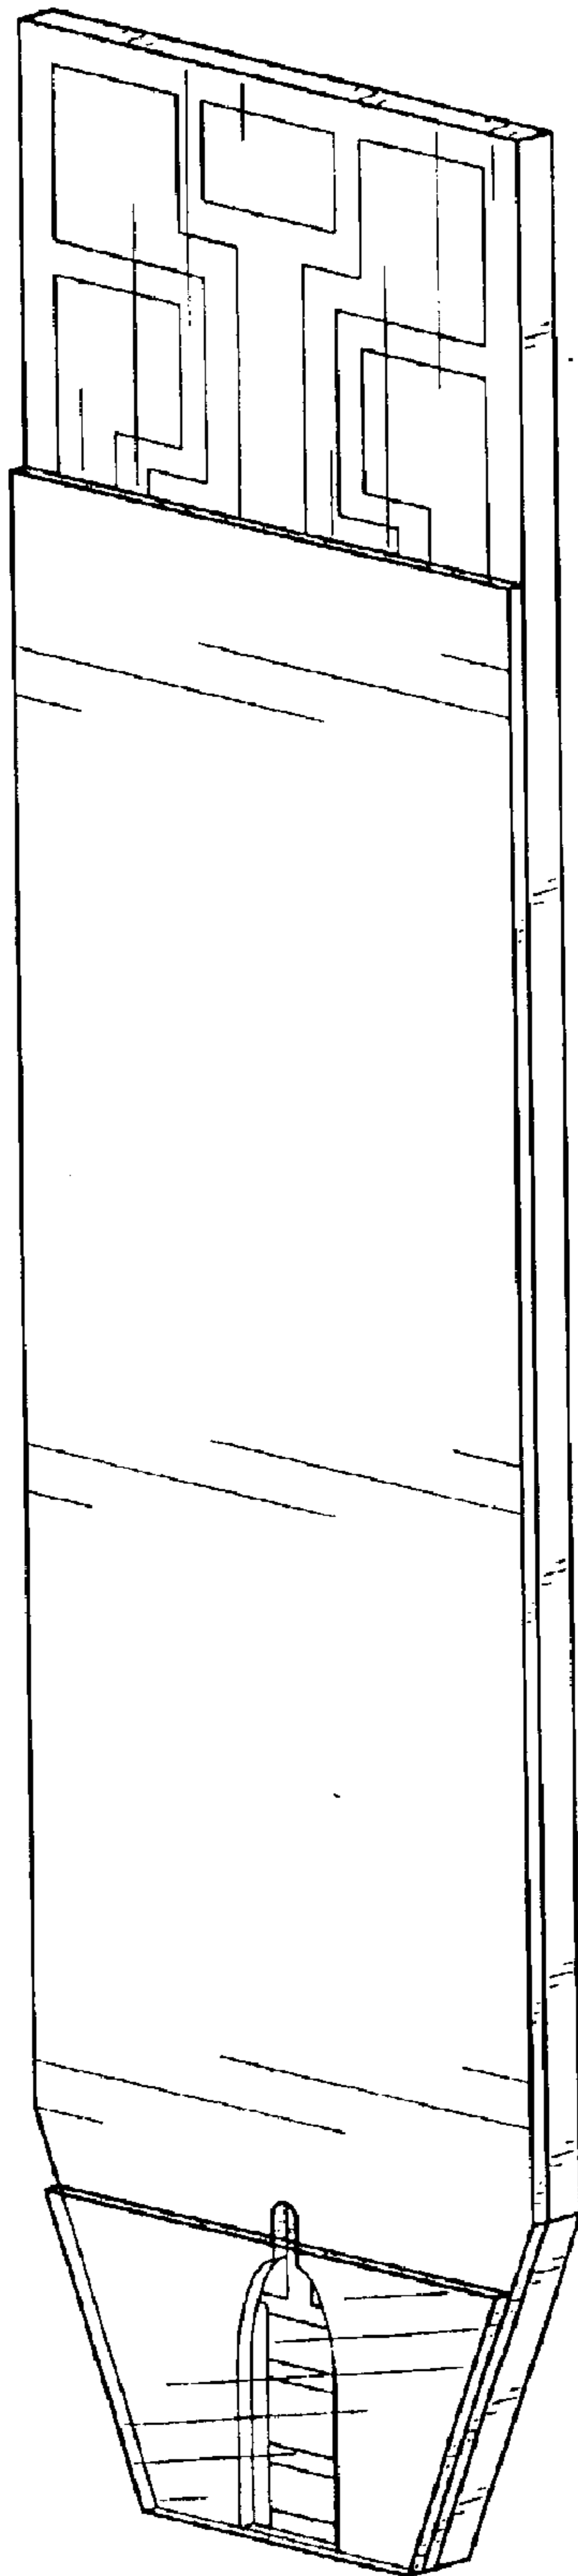


FIG. 1

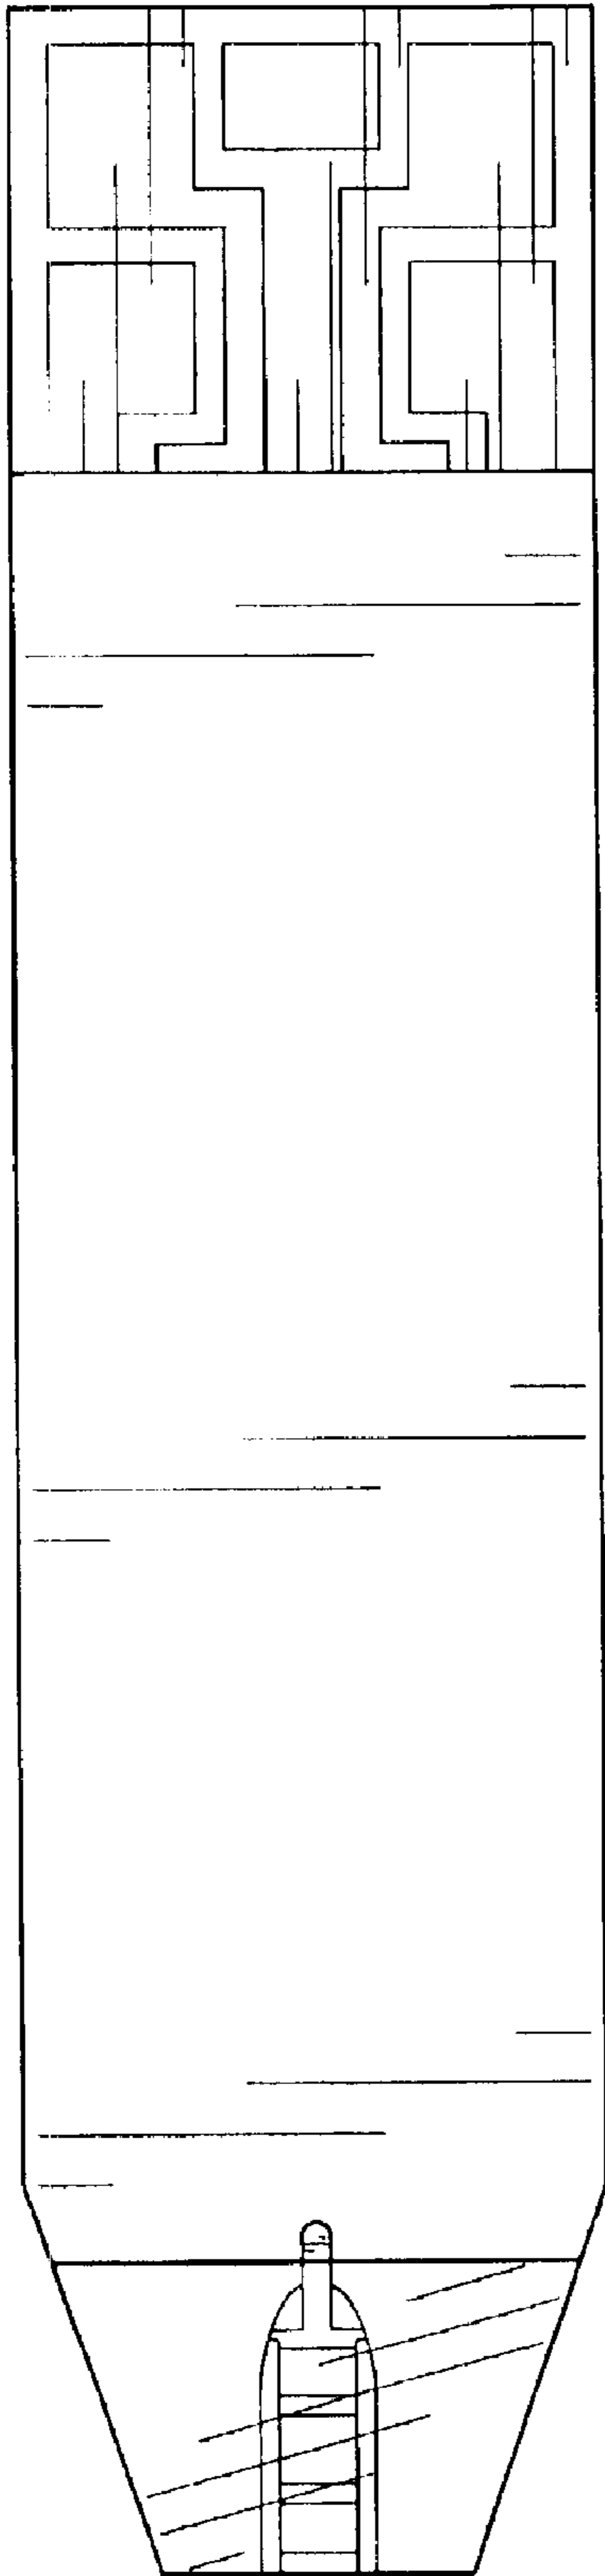


FIG. 2

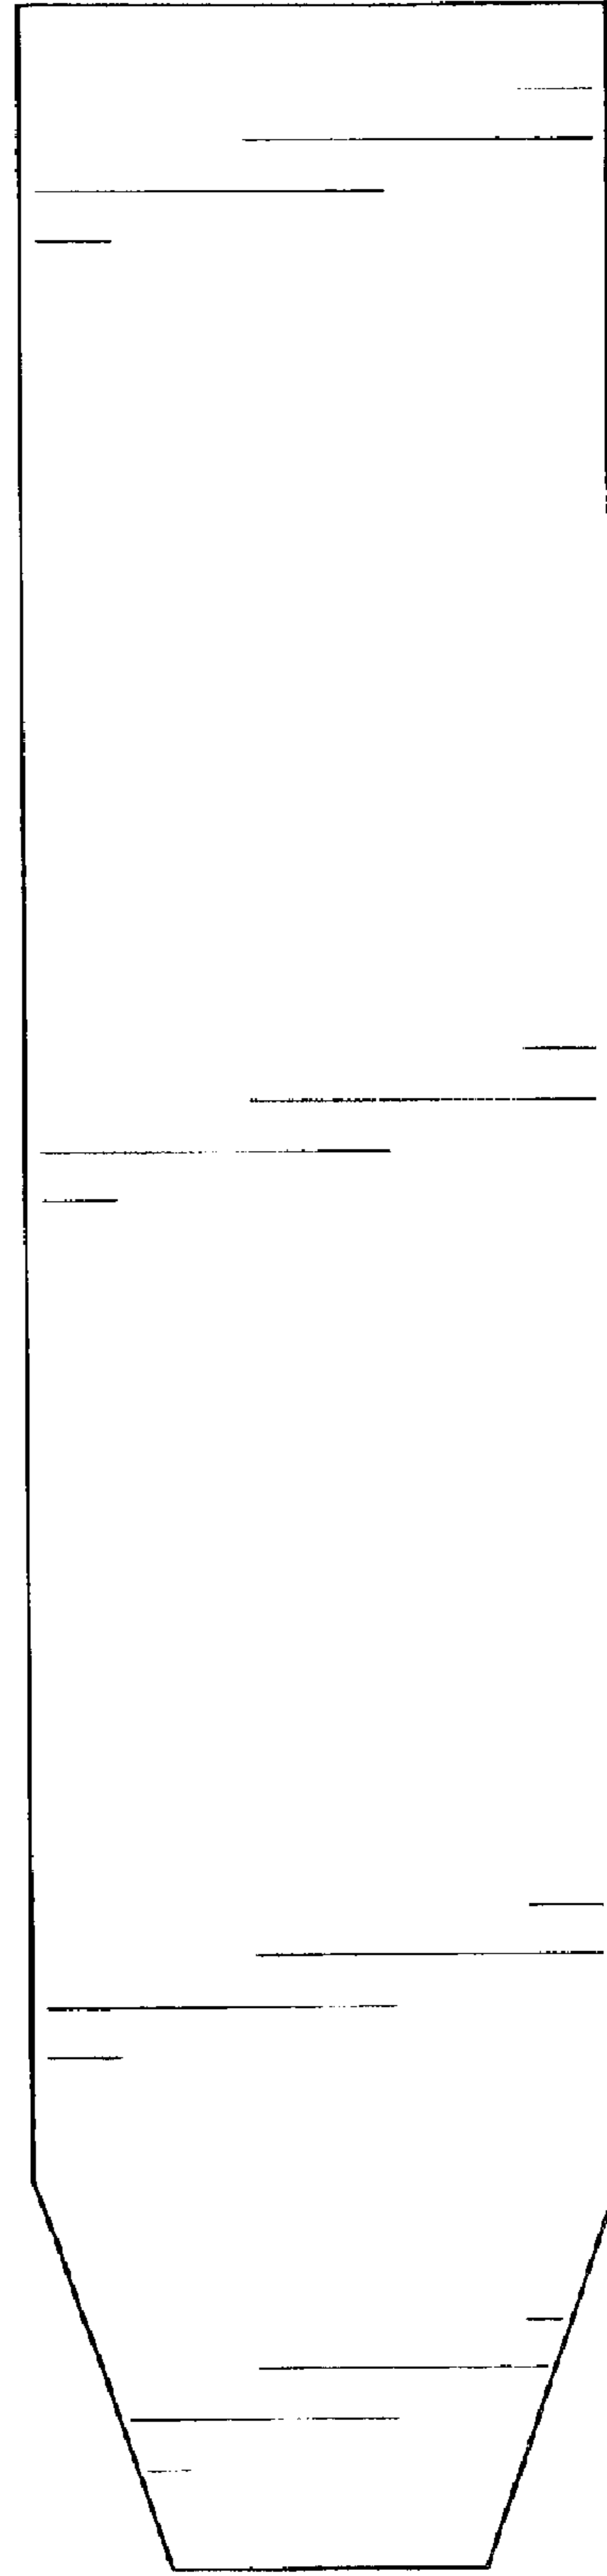


FIG. 3



FIG. 4



FIG. 5

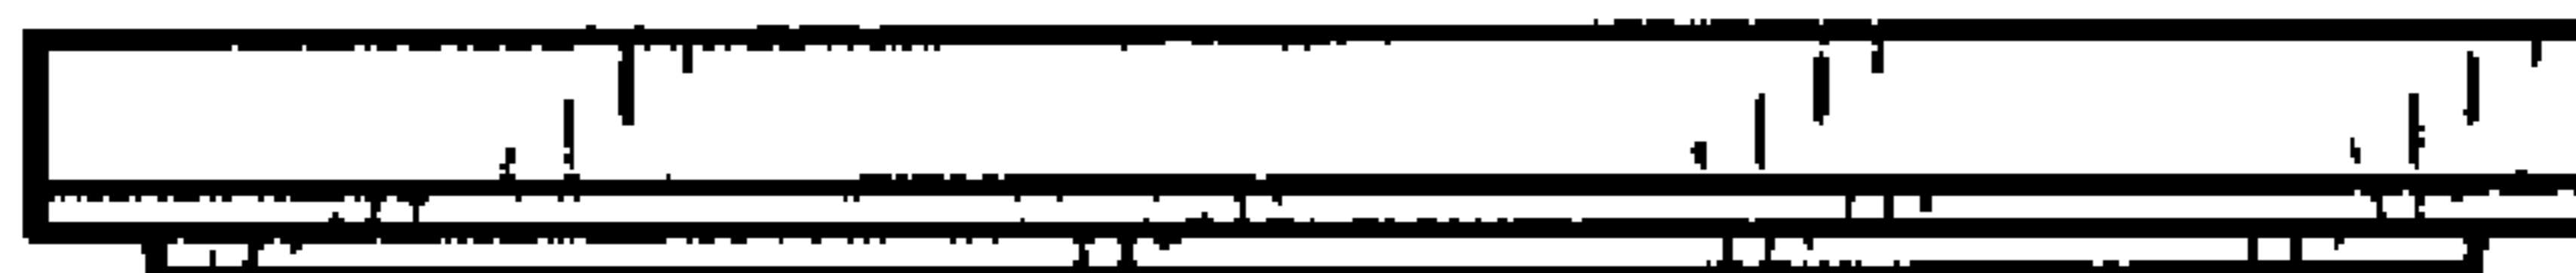


FIG. 6



FIG. 7

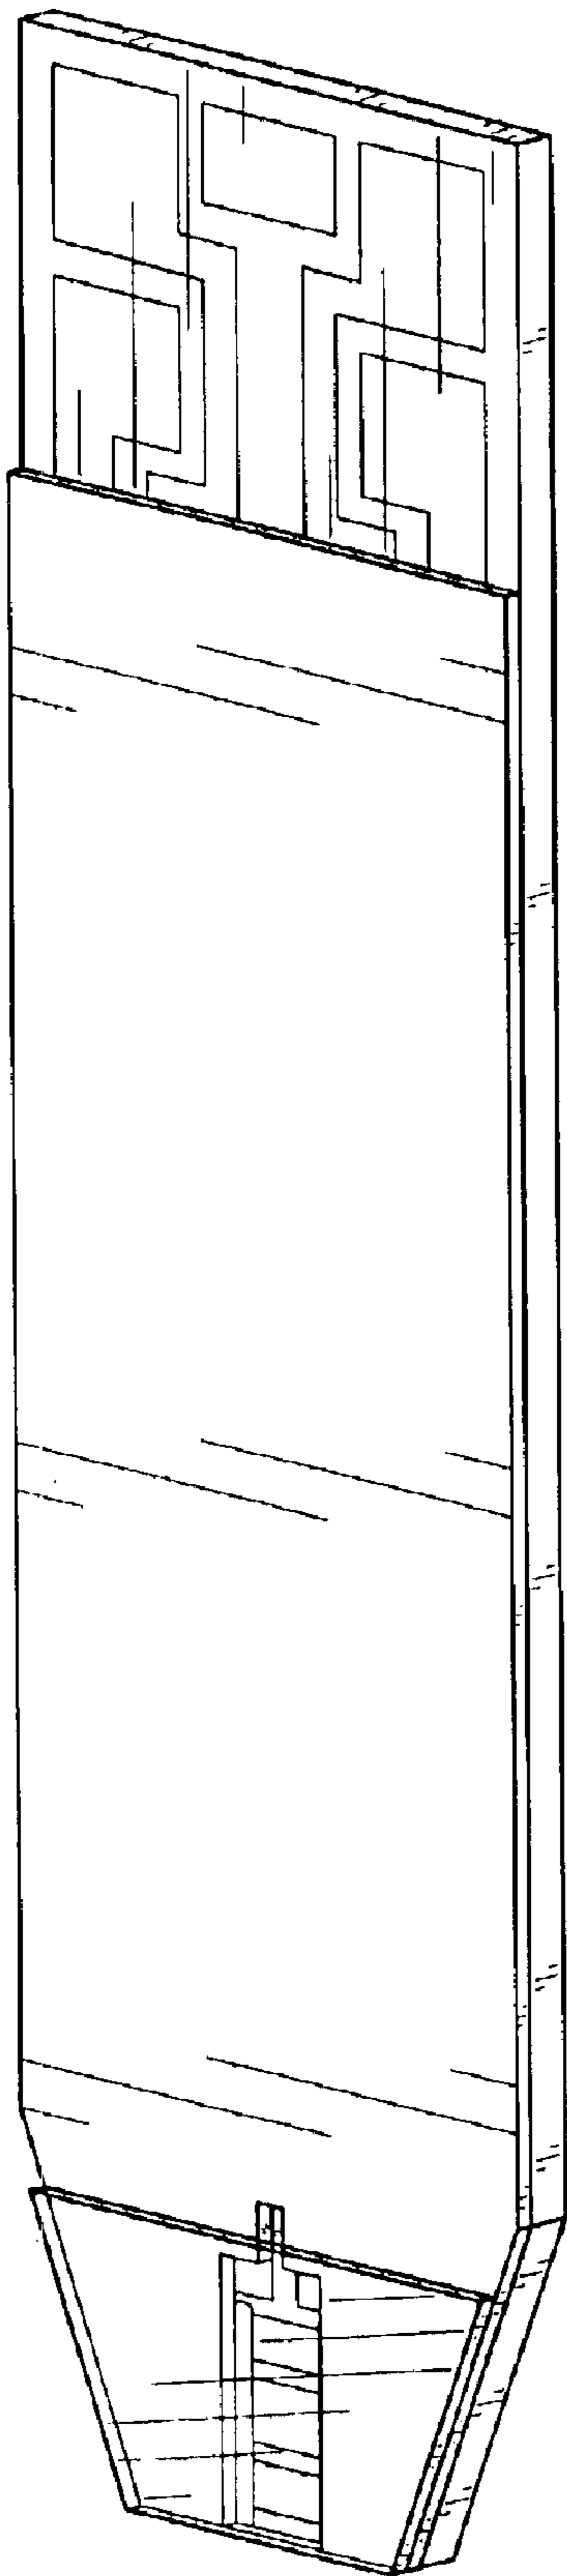


FIG. 8

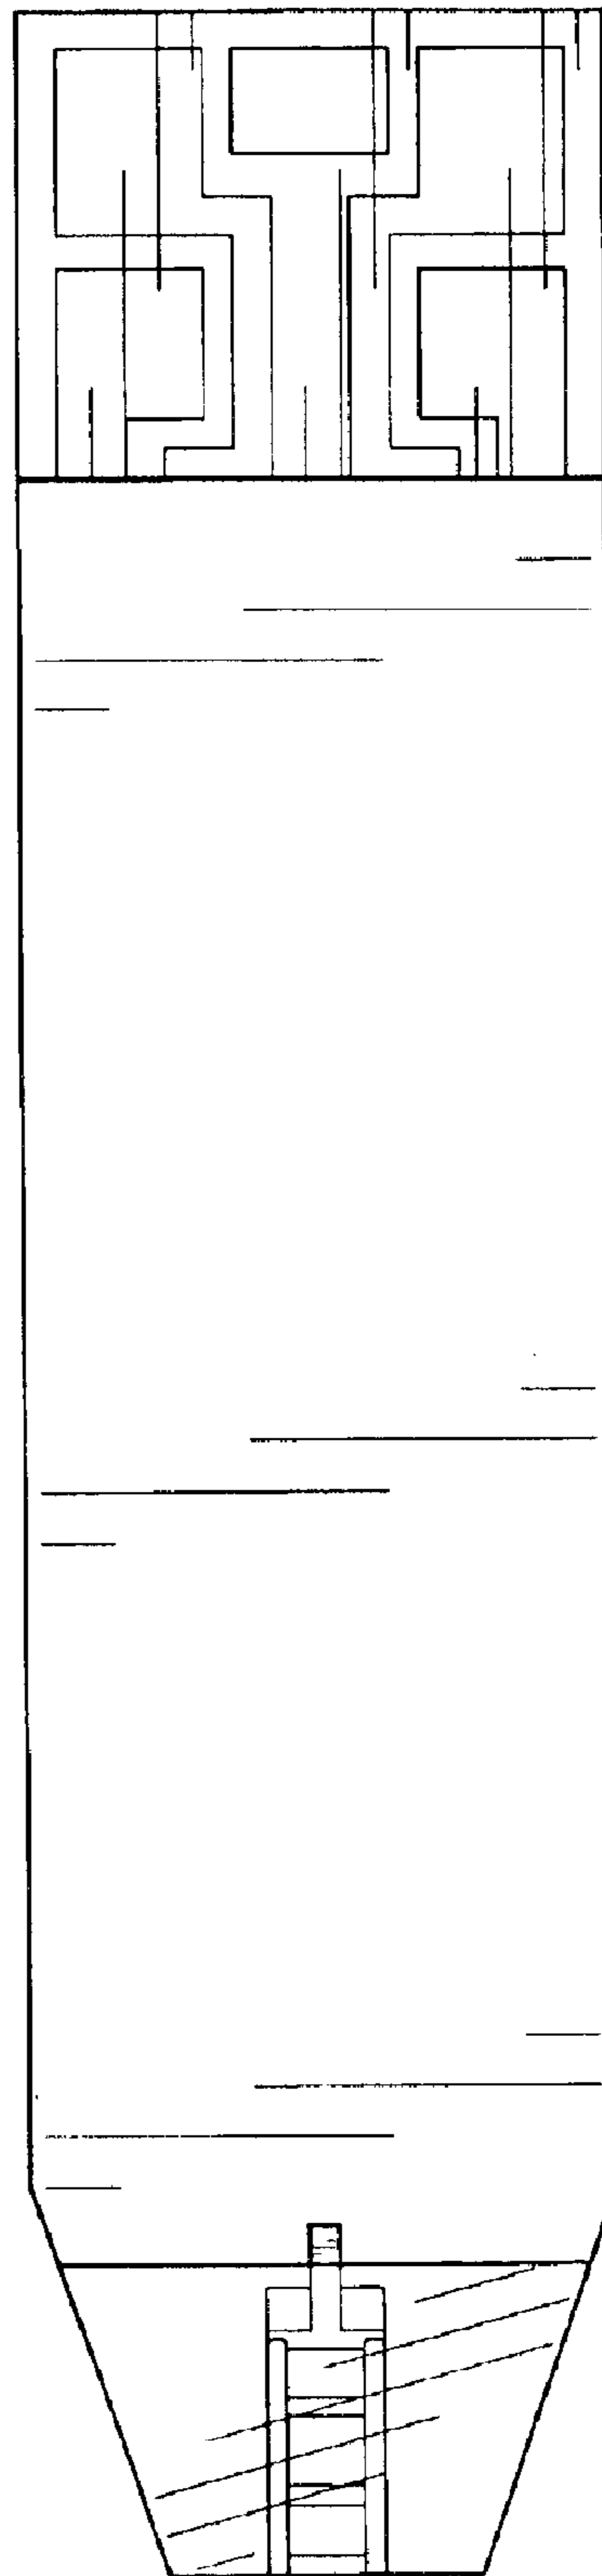


FIG. 9

UNITED STATES PATENT AND TRADEMARK OFFICE  
**CERTIFICATE OF CORRECTION**

PATENT NO. : Des. 512,512 S  
DATED : December 6, 2005  
INVENTOR(S) : Bell et al.

Page 1 of 1

It is certified that error appears in the above-identified patent and that said Letters Patent is hereby corrected as shown below:

Title page.

Item [73], Assignee, "**Wachovia Bank, National Association**, Jacksonville FL (US)" should read -- **Home Diagnostics, Inc.**, Fort Lauderdale, FL (US) --.

Signed and Sealed this

Twenty-first Day of March, 2006

A handwritten signature in black ink on a dotted background. The signature reads "Jon W. Dudas" in a cursive style.

JON W. DUDAS

*Director of the United States Patent and Trademark Office*