

US00D518576S

(12) **United States Design Patent**
Sevier et al.

(10) **Patent No.:** **US D518,576 S**
(45) **Date of Patent:** **** Apr. 4, 2006**

(54) **INSTRUMENT FOR DIAGNOSING AND TREATING SOFT TISSUE ABNORMALITIES**

(75) Inventors: **Thomas L. Sevier**, Muncie, IN (US);
Robert H. Helfst, Jr., Muncie, IN (US);
Sue A. Stover, Upland, IN (US);
Eric W. Tisdale, Indianapolis, IN (US)

(73) Assignee: **Performance Dynamics, Inc.**, Muncie, IN (US)

(**) Term: **14 Years**

(21) Appl. No.: **29/226,104**

(22) Filed: **Mar. 24, 2005**

Related U.S. Application Data

(60) Continuation of application No. 10/677,281, filed on Sep. 26, 2003, now Pat. No. 6,887,211, which is a division of application No. 09/898,623, filed on Jul. 3, 2001, now Pat. No. 6,641,547, which is a division of application No. 08/695,873, filed on Aug. 12, 1996, now Pat. No. 6,254,555.

(51) **LOC (8) Cl.** **28-03**

(52) **U.S. Cl.** **D24/214; D24/200**

(58) **Field of Classification Search** D24/200,
D24/214, 215, 211; D21/386; 601/135, 137,
601/134, 138, 1

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D30,230 S	2/1899	Barnet	
1,373,970 A	4/1921	Peasley	
1,612,343 A	12/1926	Amussen	
1,769,872 A	7/1930	Weeks	
1,987,390 A	1/1935	Davis	
2,044,112 A	6/1936	Wildmann	
2,219,436 A	10/1940	Anderson	
D155,773 S	11/1949	Becker	
2,752,623 A	7/1956	Tupper	
2,806,470 A	9/1957	Ferrier	
3,107,665 A	10/1963	Nordgren	
D208,608 S	* 9/1967	Madl et al. D24/214

D211,549 S	6/1968	Christopher	
3,389,418 A	6/1968	Sencabaugh	
3,557,776 A	1/1971	Boots	
D223,418 S	* 4/1972	Hess D24/214
3,888,241 A	6/1975	Fischer	
D237,313 S	10/1975	Harris	
D237,323 S	10/1975	Inohara	
D262,908 S	2/1982	Pesco	
D263,077 S	2/1982	Stanton	
D264,754 S	6/1982	Vitra	
4,378,007 A	3/1983	Kachadourian	
D272,090 S	1/1984	Hosid	
4,461,285 A	7/1984	Courtin	
4,483,328 A	11/1984	Wolocko	
4,590,926 A	5/1986	Courtin	
D285,116 S	8/1986	Hoff	
D288,847 S	3/1987	Kaesar	
4,648,387 A	3/1987	Simmons	

(Continued)

Primary Examiner—Ian Simmons
(74) *Attorney, Agent, or Firm*—Woodard, Emhardt, Moriarty, McNett & Henry LLP

(57) **CLAIM**

The ornamental design for an instrument for diagnosing and treating soft tissue abnormalities, as shown and described.

DESCRIPTION

FIG. 1 is a view in perspective of an instrument for diagnosing and treating soft tissue abnormalities showing our new design.

FIG. 2 is a view in front elevation of the instrument shown in FIG. 1.


FIG. 3 is a view in rear elevation of the instrument shown in FIG. 1.

FIG. 4 is a top plan view of the instrument shown in FIG. 1. FIG. 5 is a bottom plan view of the instrument shown in FIG. 1.

FIG. 6 is a view in right side elevation of the instrument shown in FIG. 1; and,

FIG. 7 is a view in left side elevation of the instrument shown in FIG. 1.

1 Claim, 2 Drawing Sheets

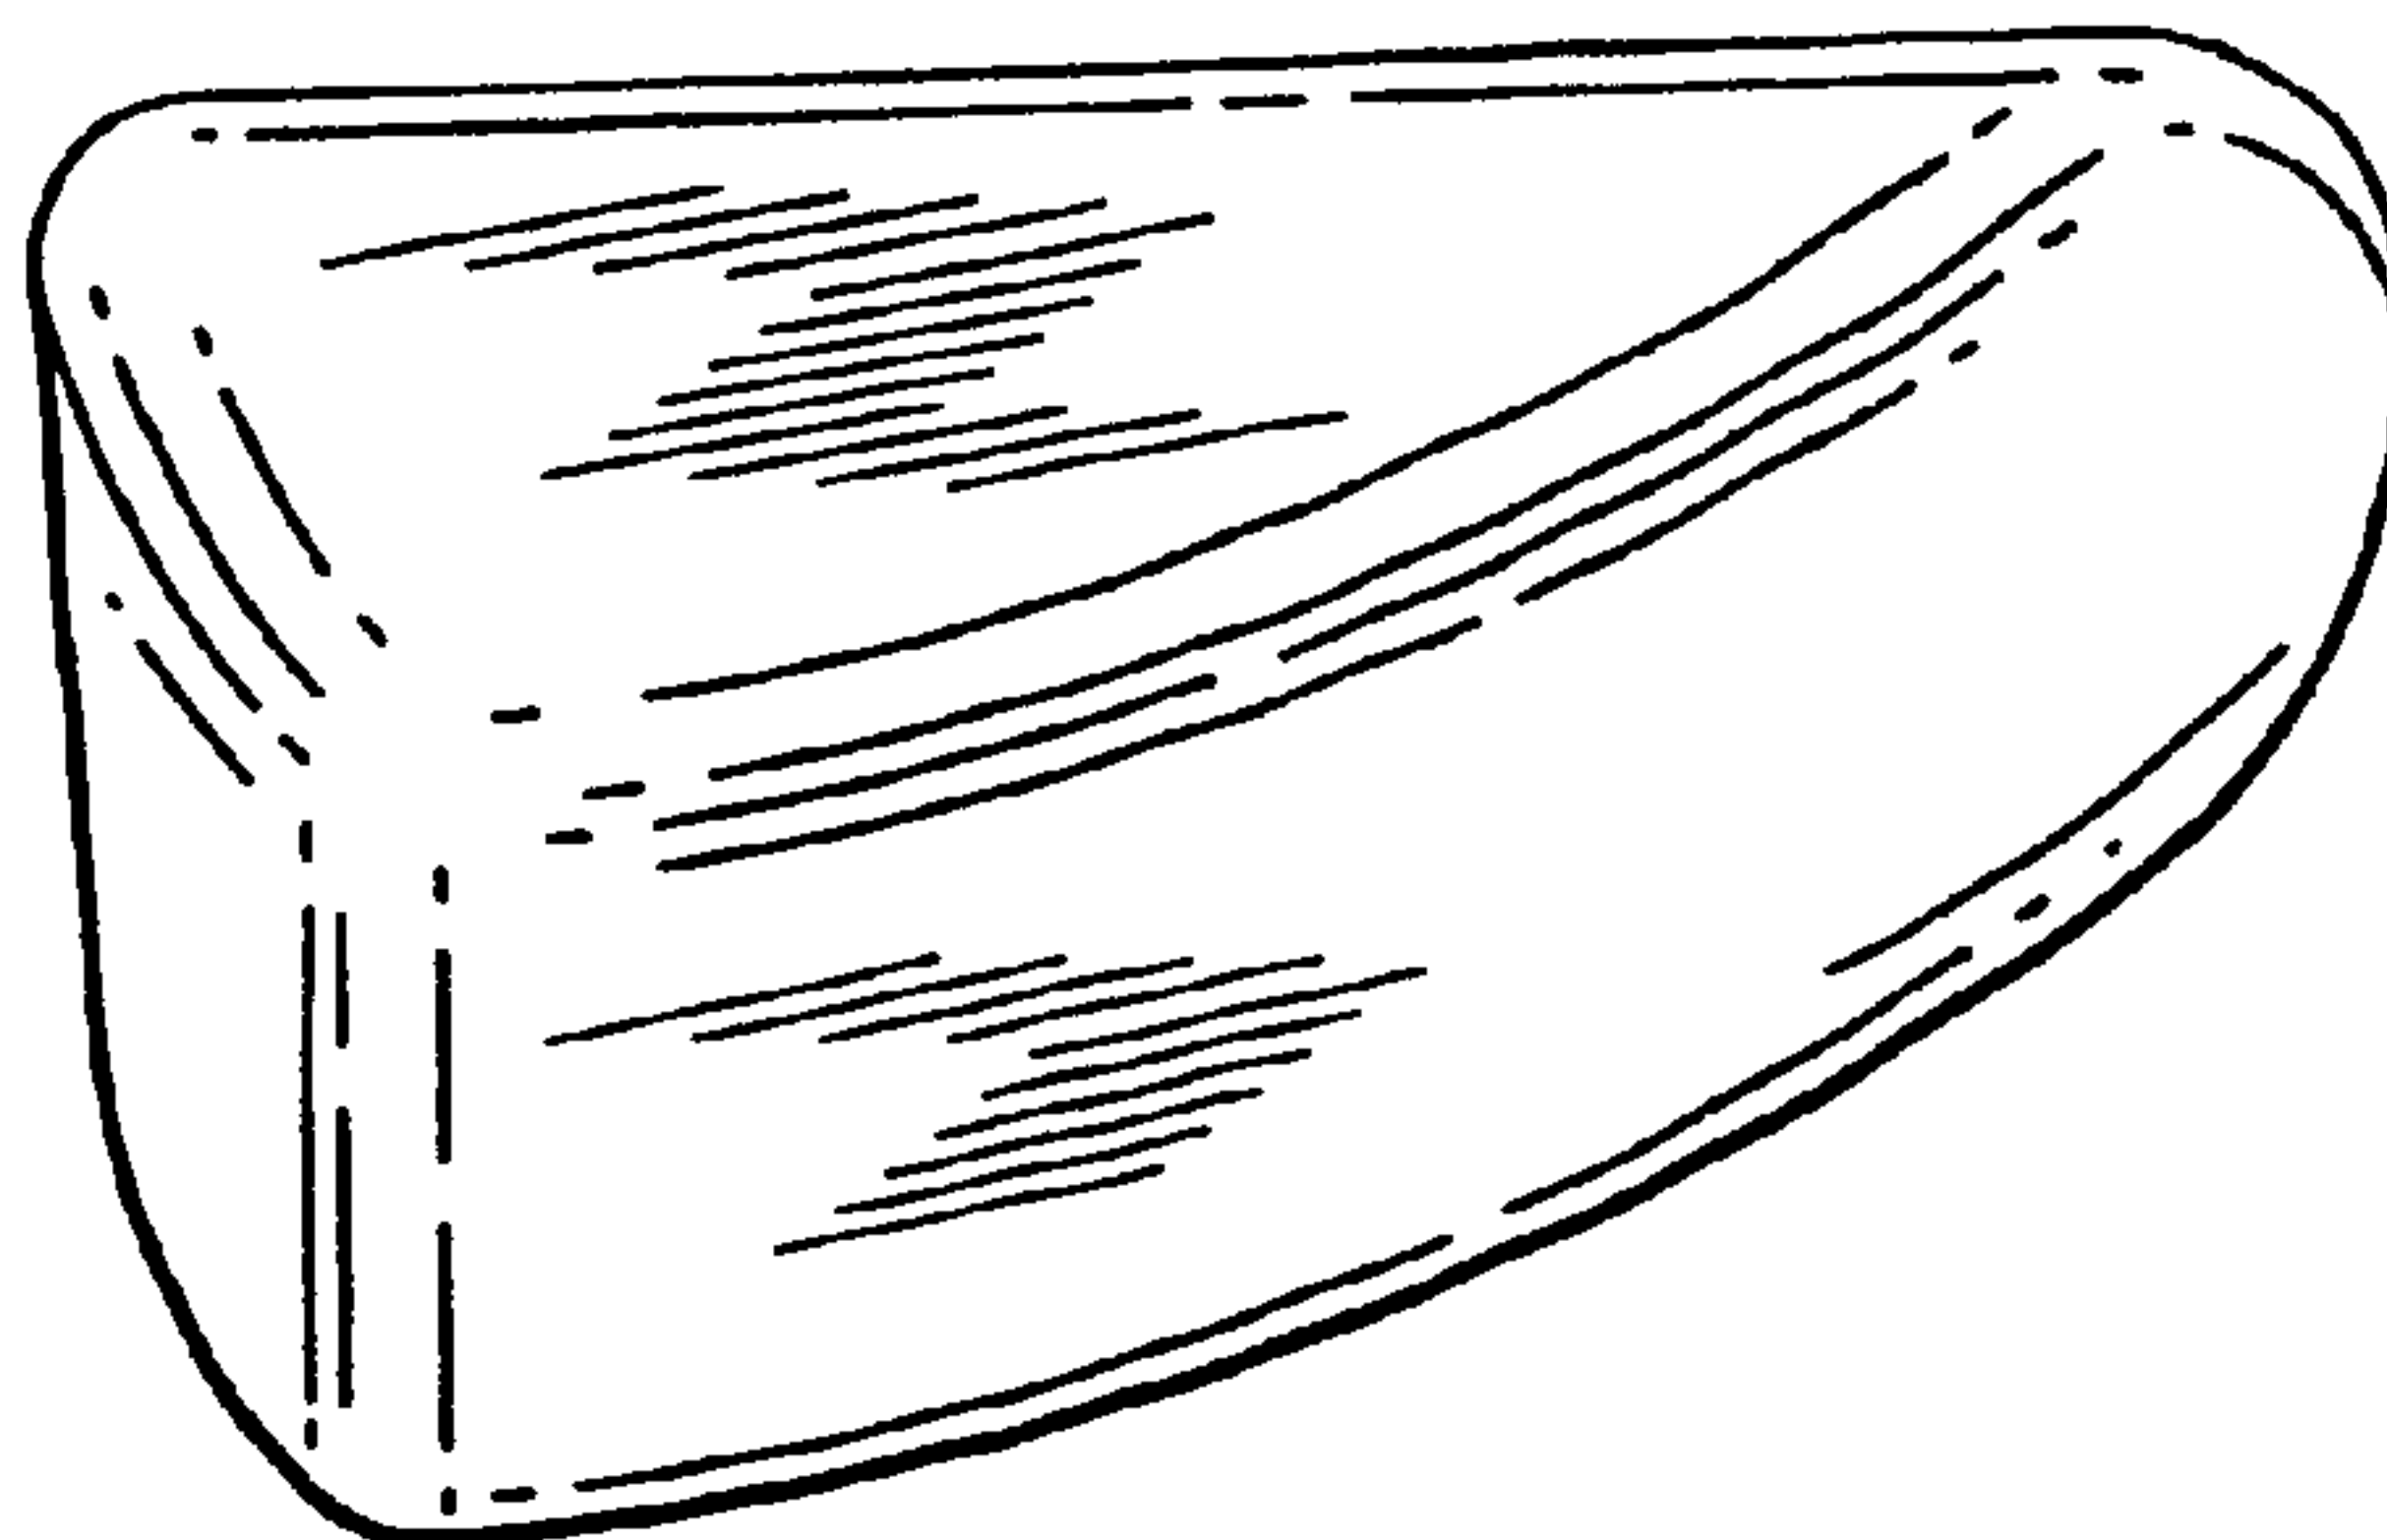

US D518,576 S

Page 2

U.S. PATENT DOCUMENTS

4,705,030	A	11/1987	Tepperberg	D342,999	S	1/1994	Gonsalves, Jr.
4,732,142	A	3/1988	Hurlburt et al.	D345,801	S	4/1994	Bosch
D304,495	S	11/1989	Tyo et al.	5,307,816	A	5/1994	Hashimoto et al.
D312,694	S	* 12/1990	Yanazaki D24/215	5,366,437	A	11/1994	Graston
4,993,408	A	2/1991	Schweisfurth	D357,322	S	4/1995	Matthews
D317,204	S	5/1991	Henneseey	5,441,478	A	8/1995	Graston
D323,035	S	1/1992	Yang	D362,307	S	9/1995	Cirone
5,080,111	A	1/1992	Pallin	D373,197	S	8/1996	Schepper
5,085,207	A	2/1992	Fiore	5,624,385	A	4/1997	Hwang
5,103,809	A	4/1992	DeLuca et al.	D386,879	S	* 11/1997	Daniels D24/214
D328,328	S	7/1992	Juarez	6,077,239	A	6/2000	Lin
D338,964	S	8/1993	Tarjoto	6,254,555	B1	7/2001	Sevier et al.
5,231,977	A	8/1993	Graston	6,641,547	B1	11/2003	Sevier et al.

* cited by examiner

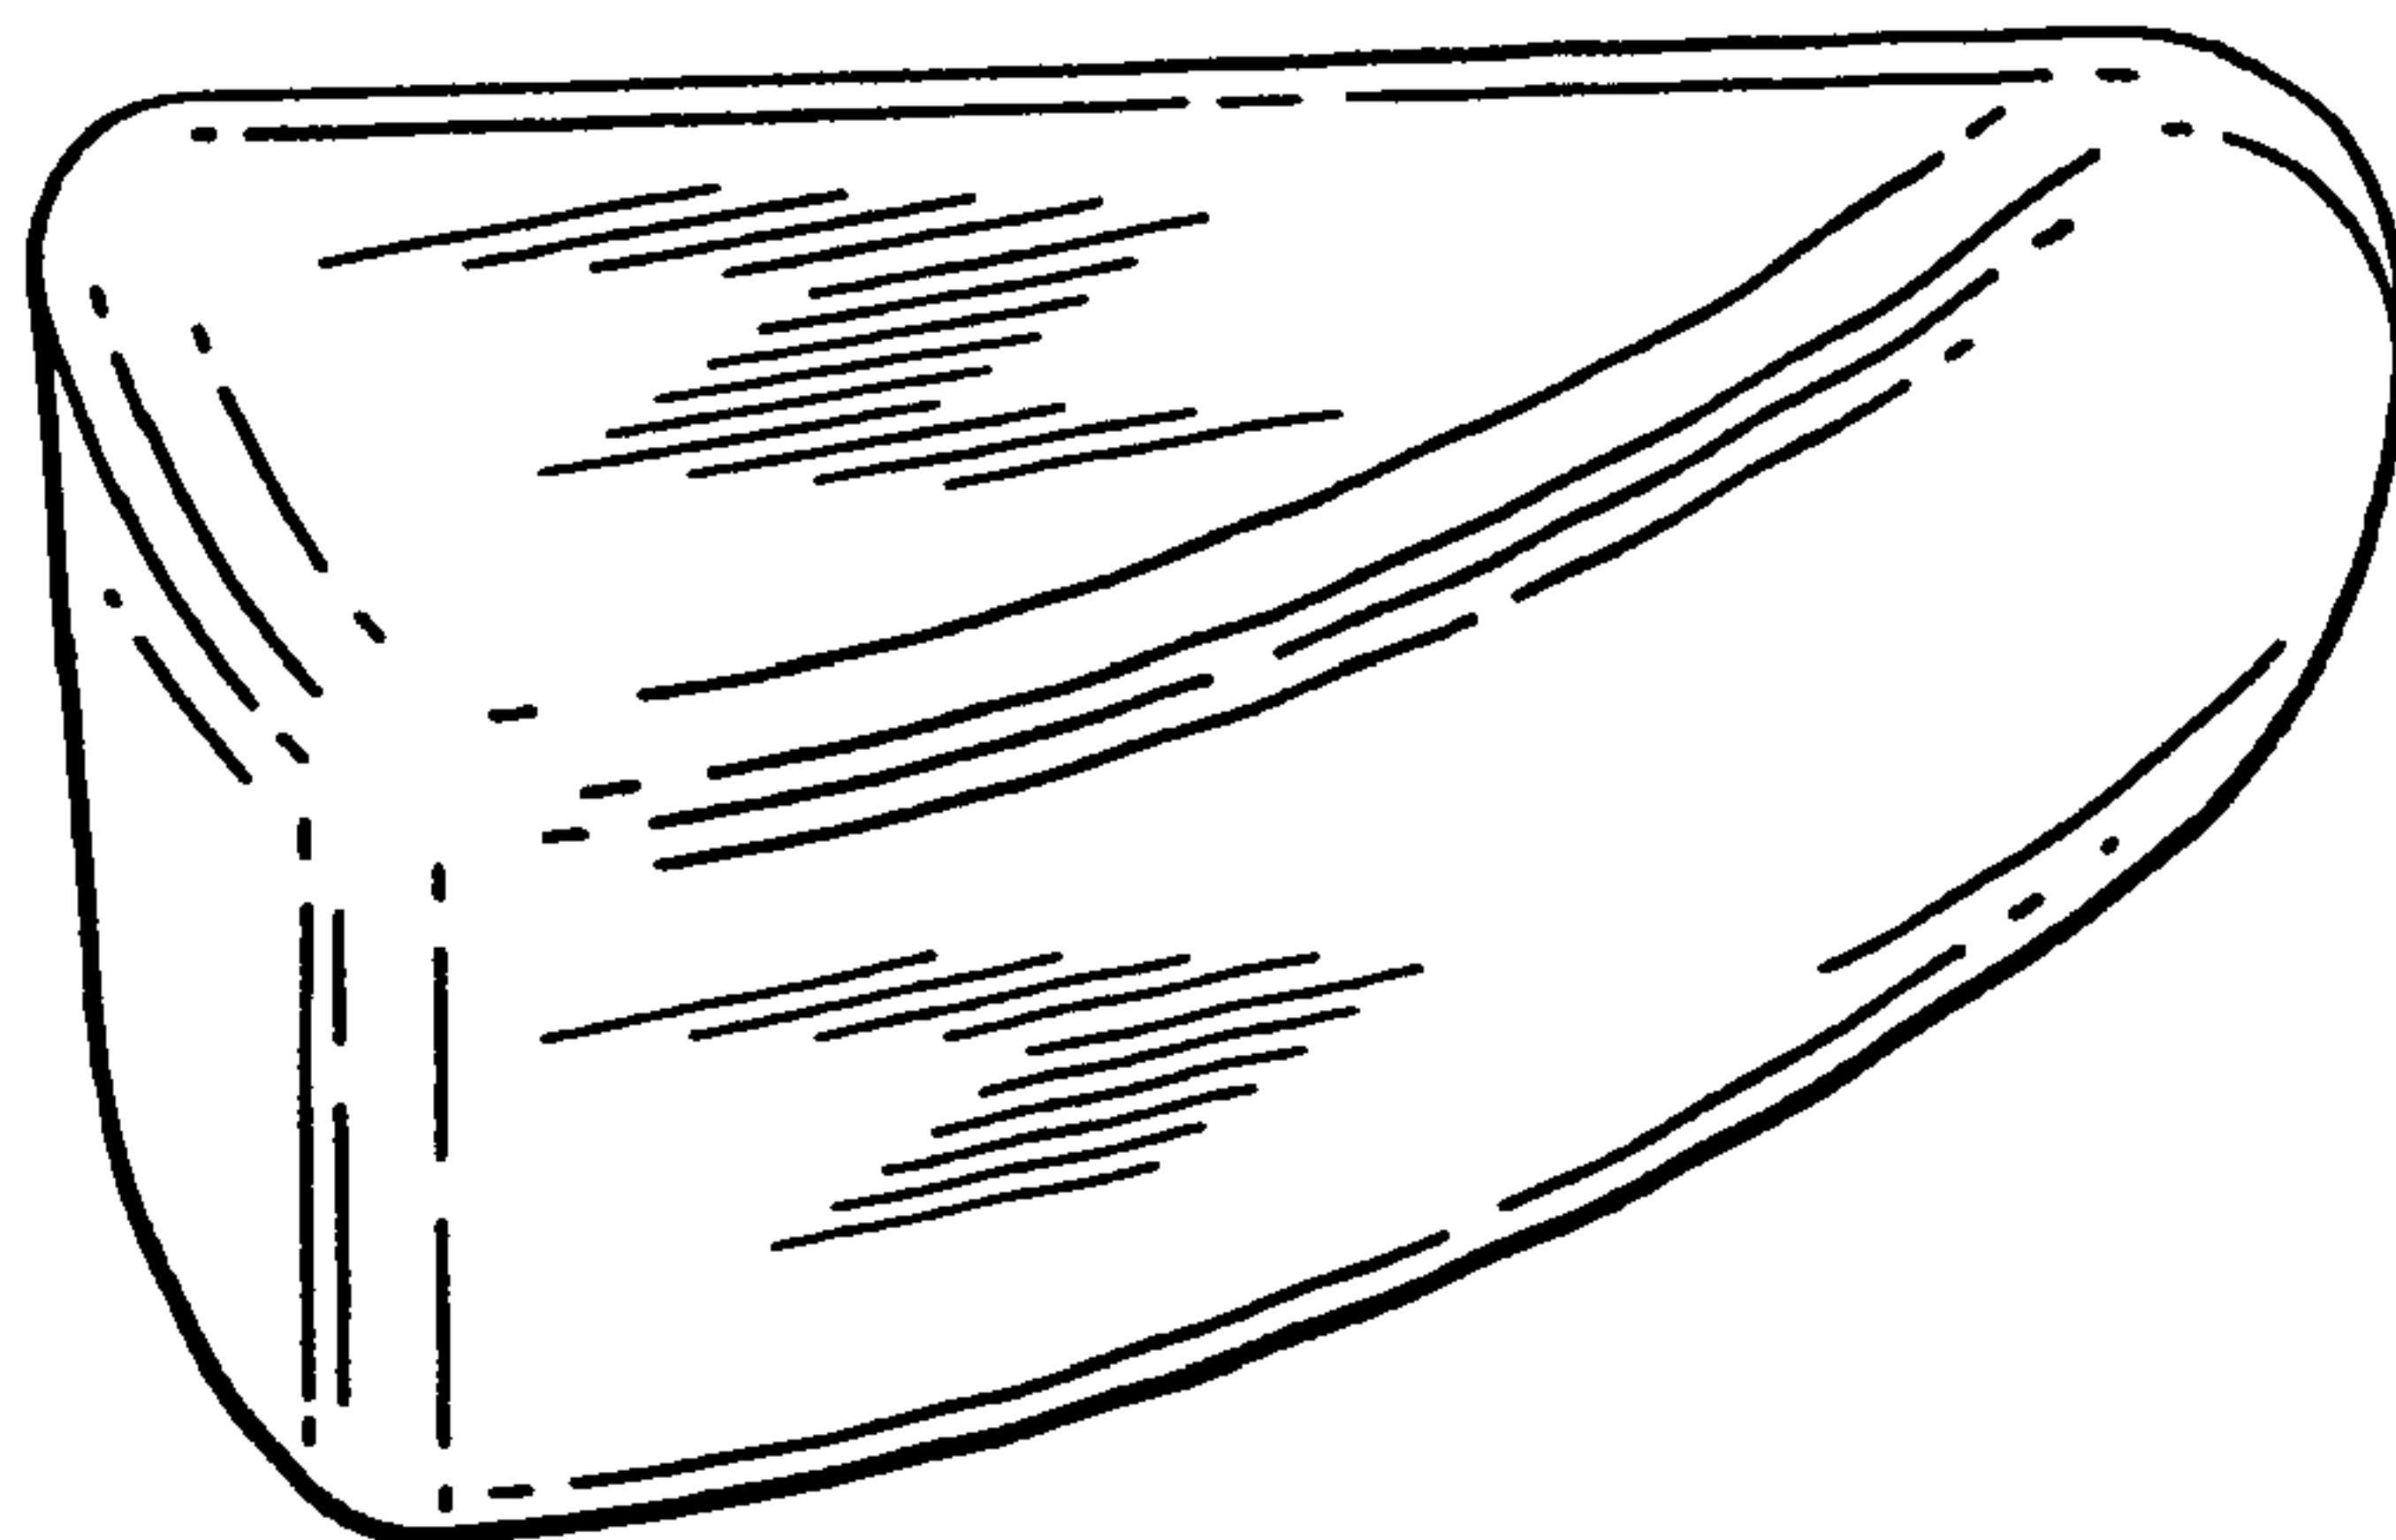


Fig. 1

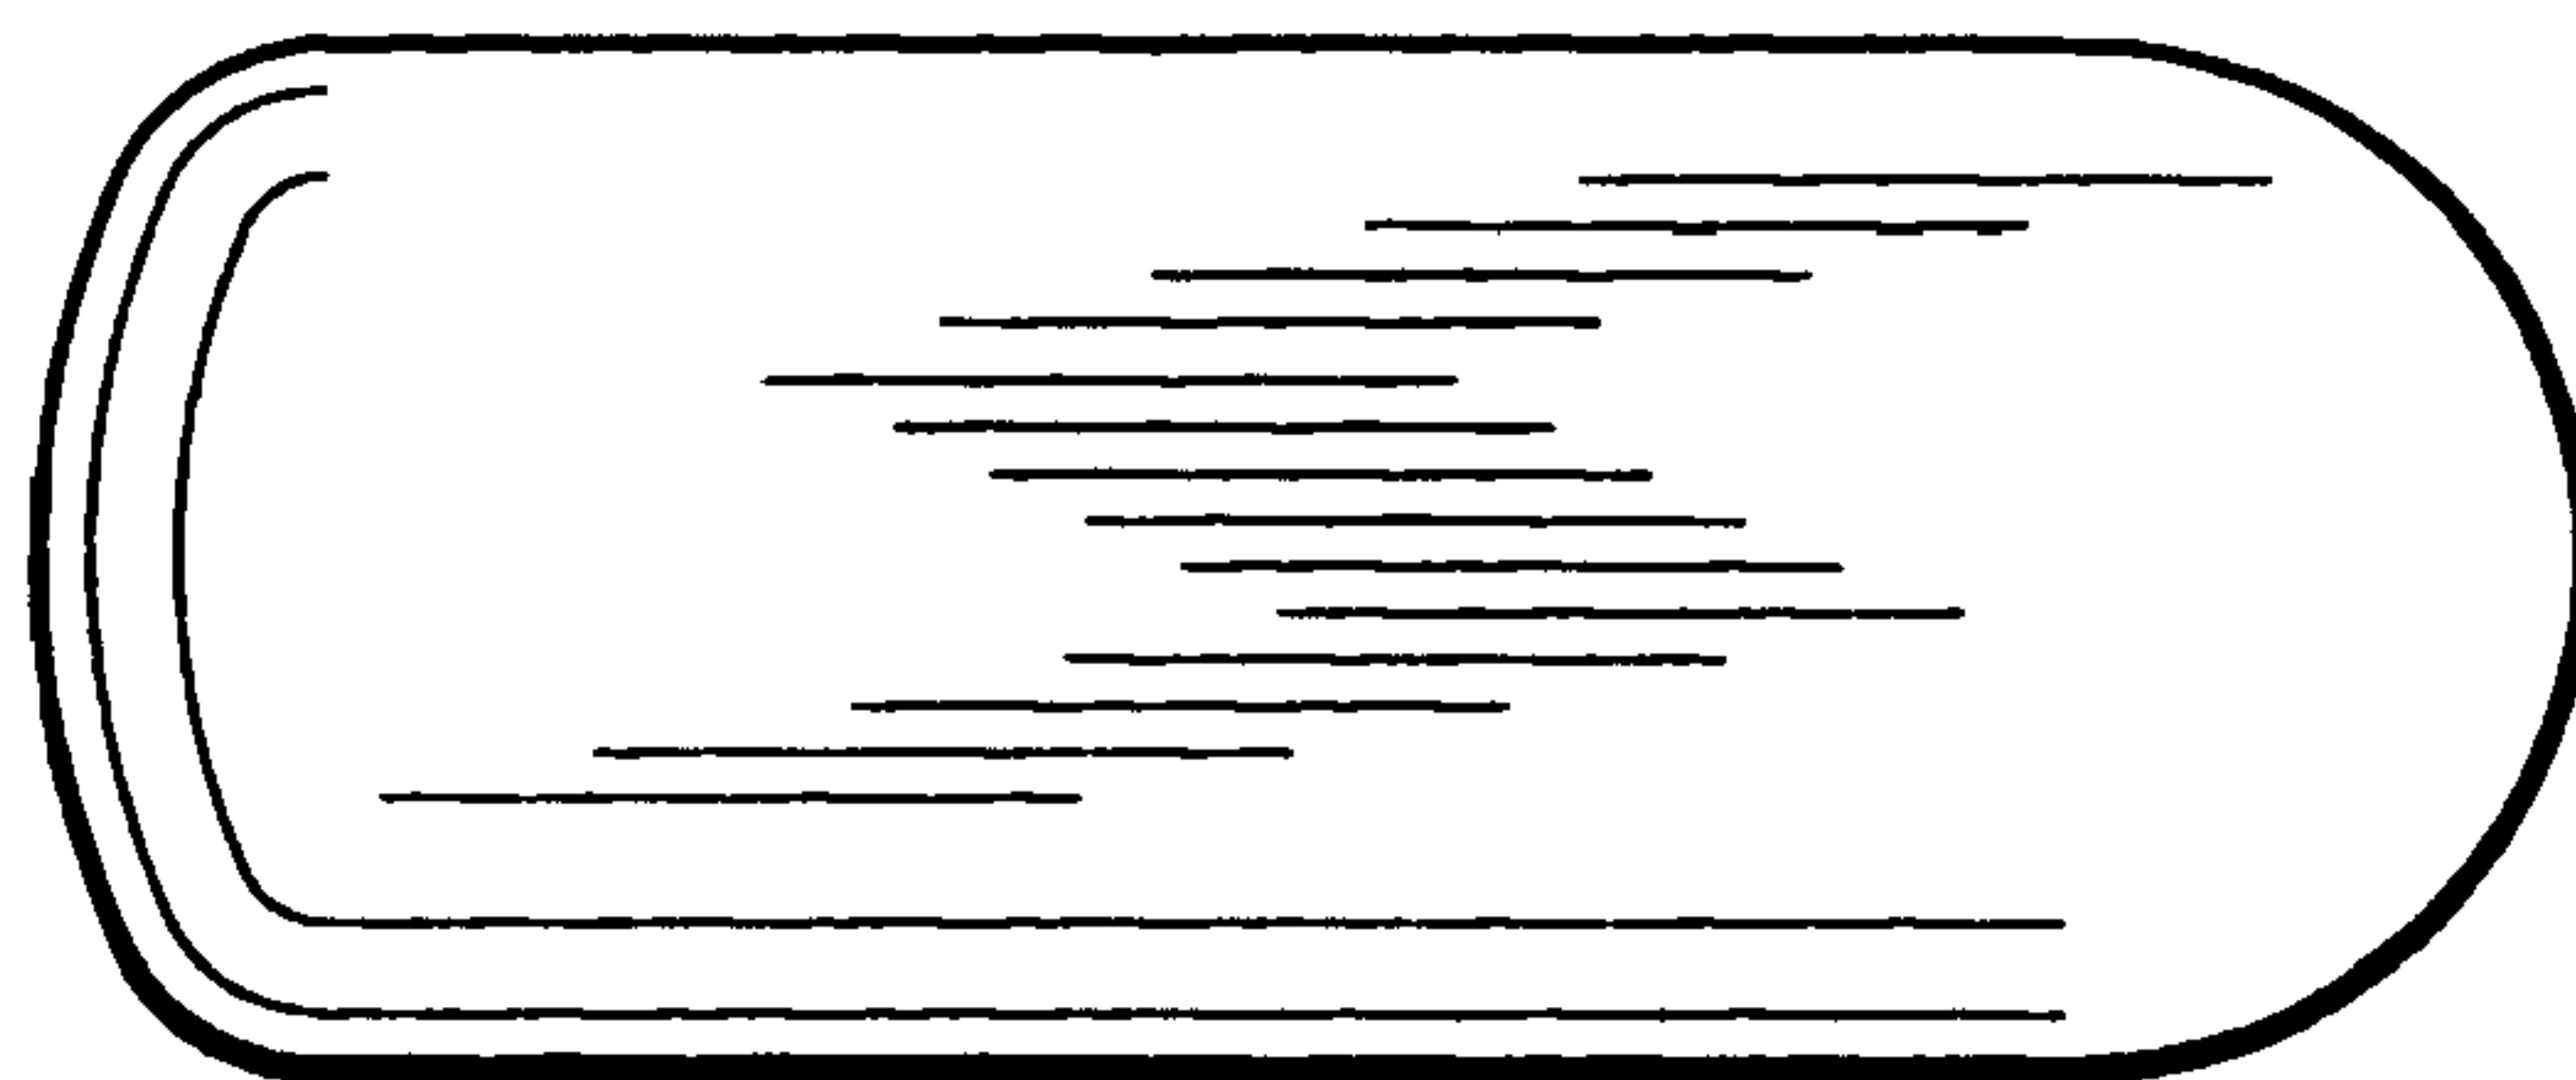


Fig. 2

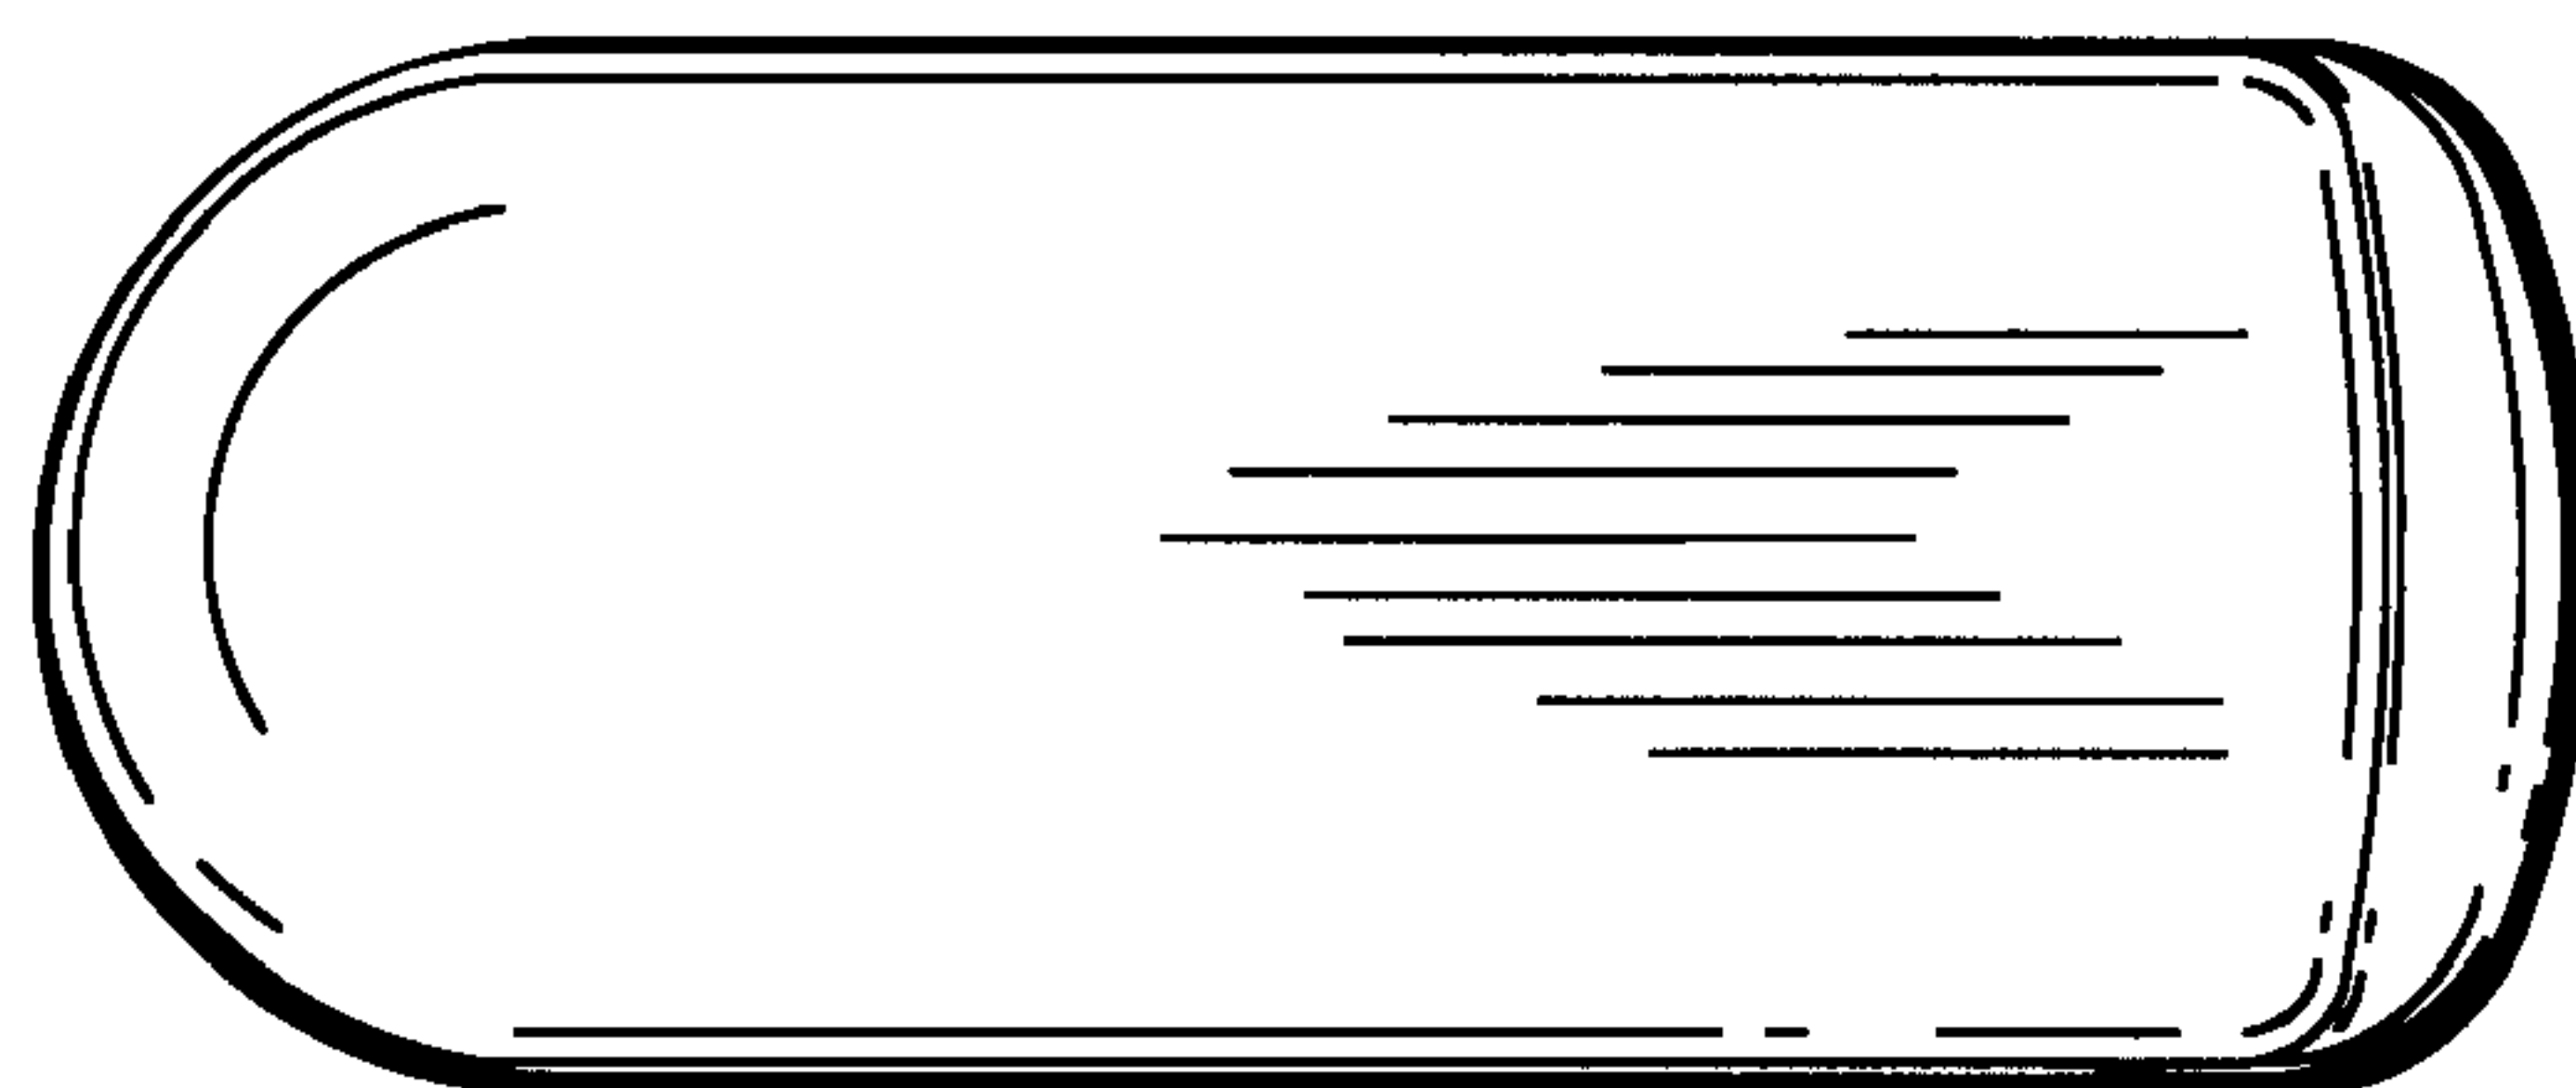


Fig. 3

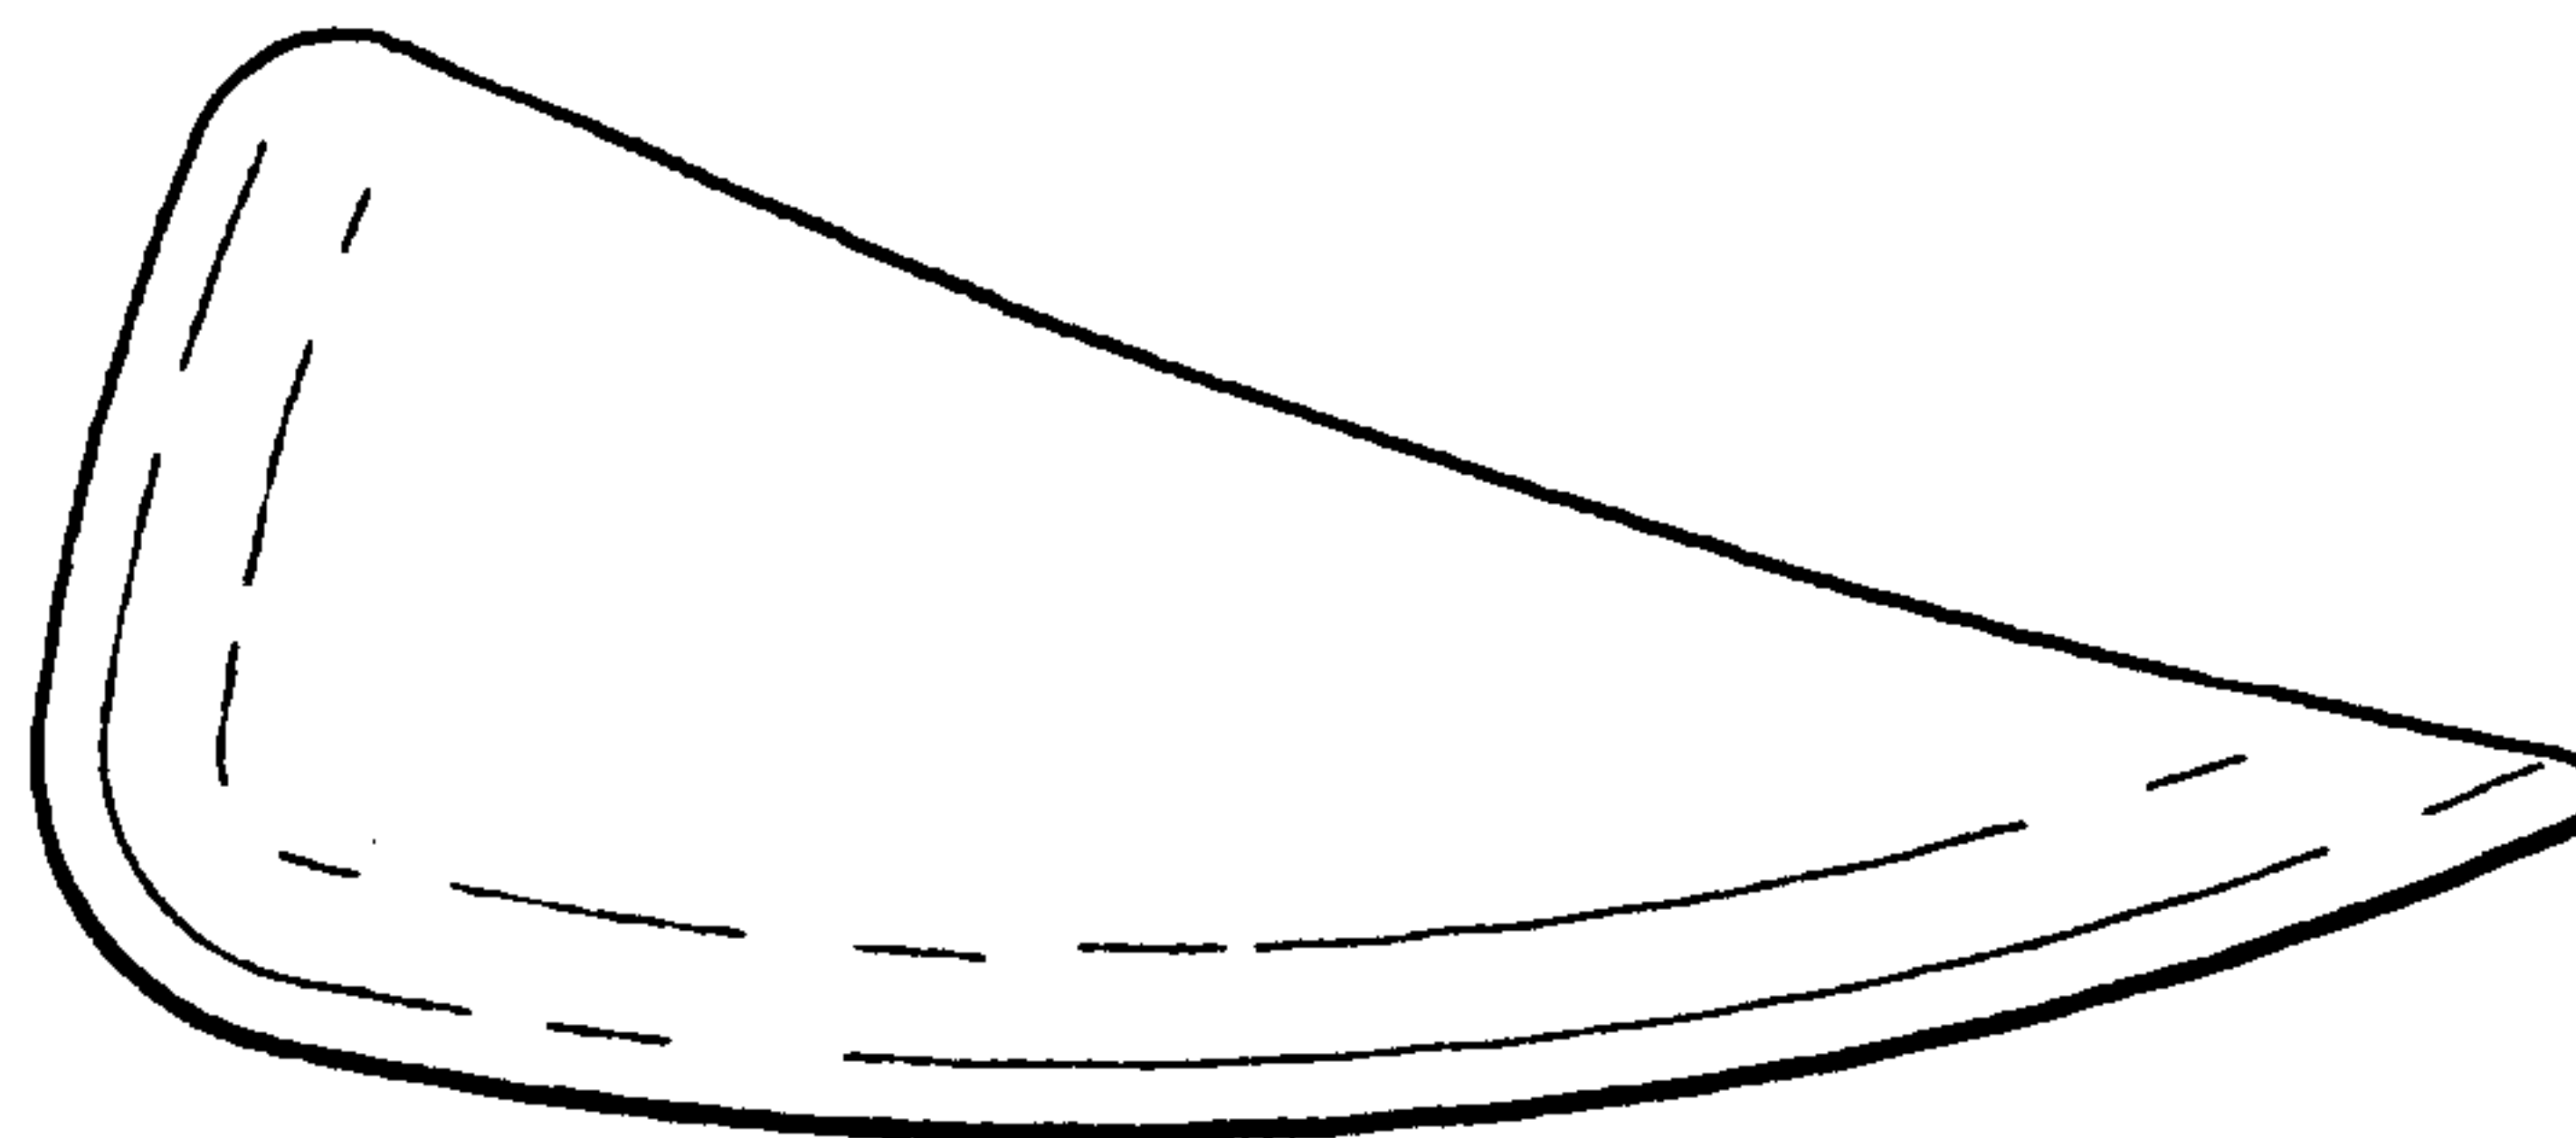


Fig. 4



Fig. 5

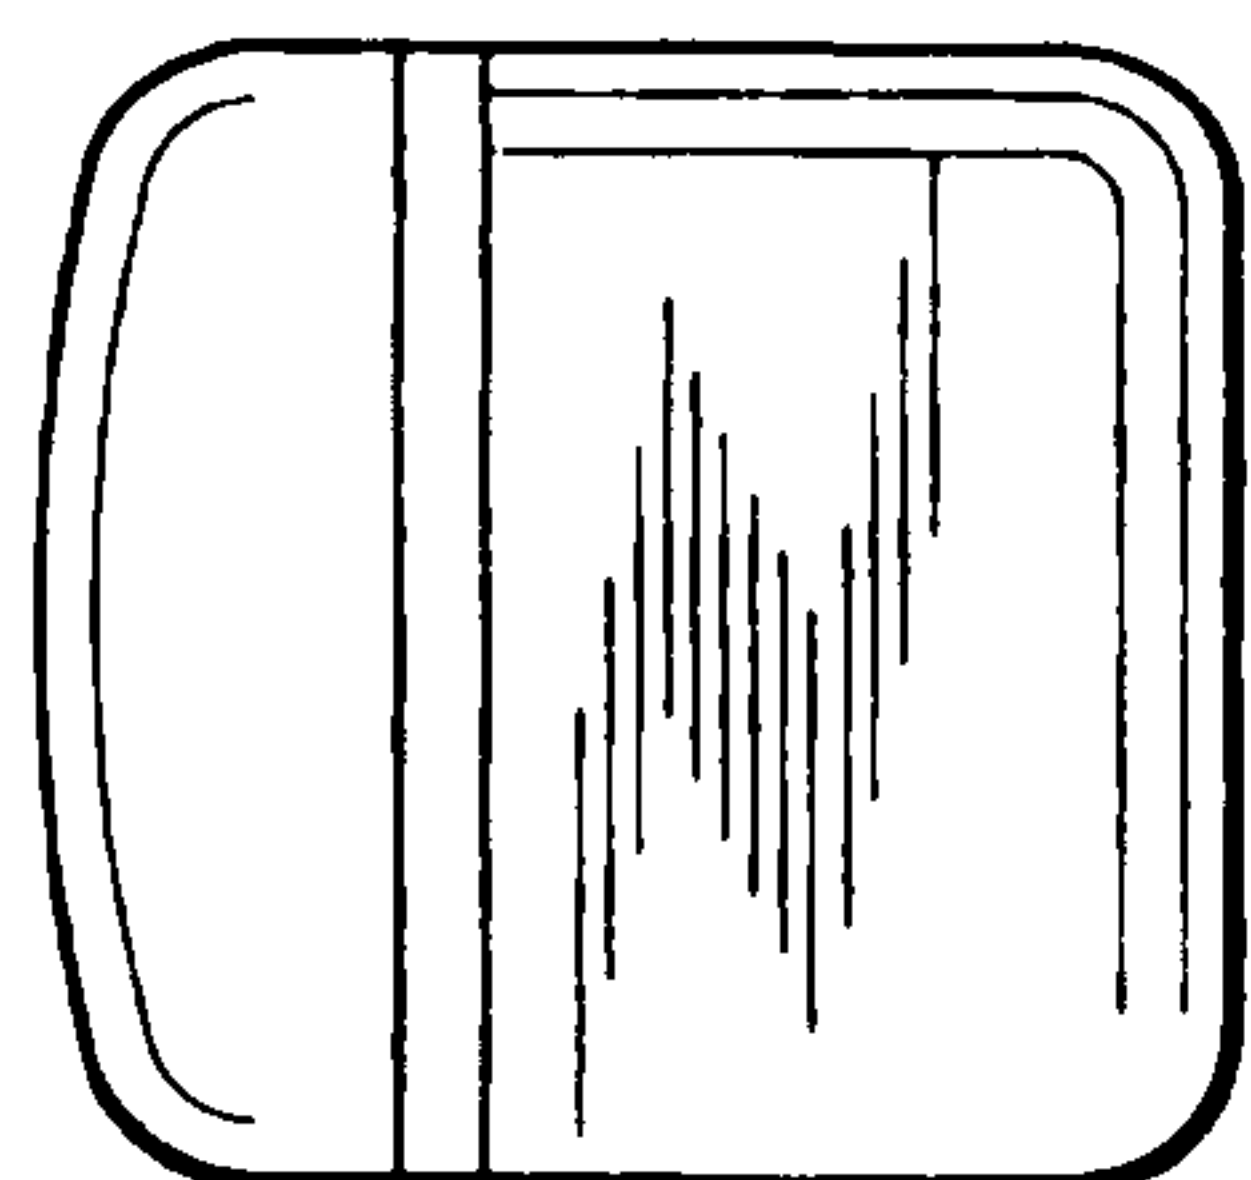


Fig. 6

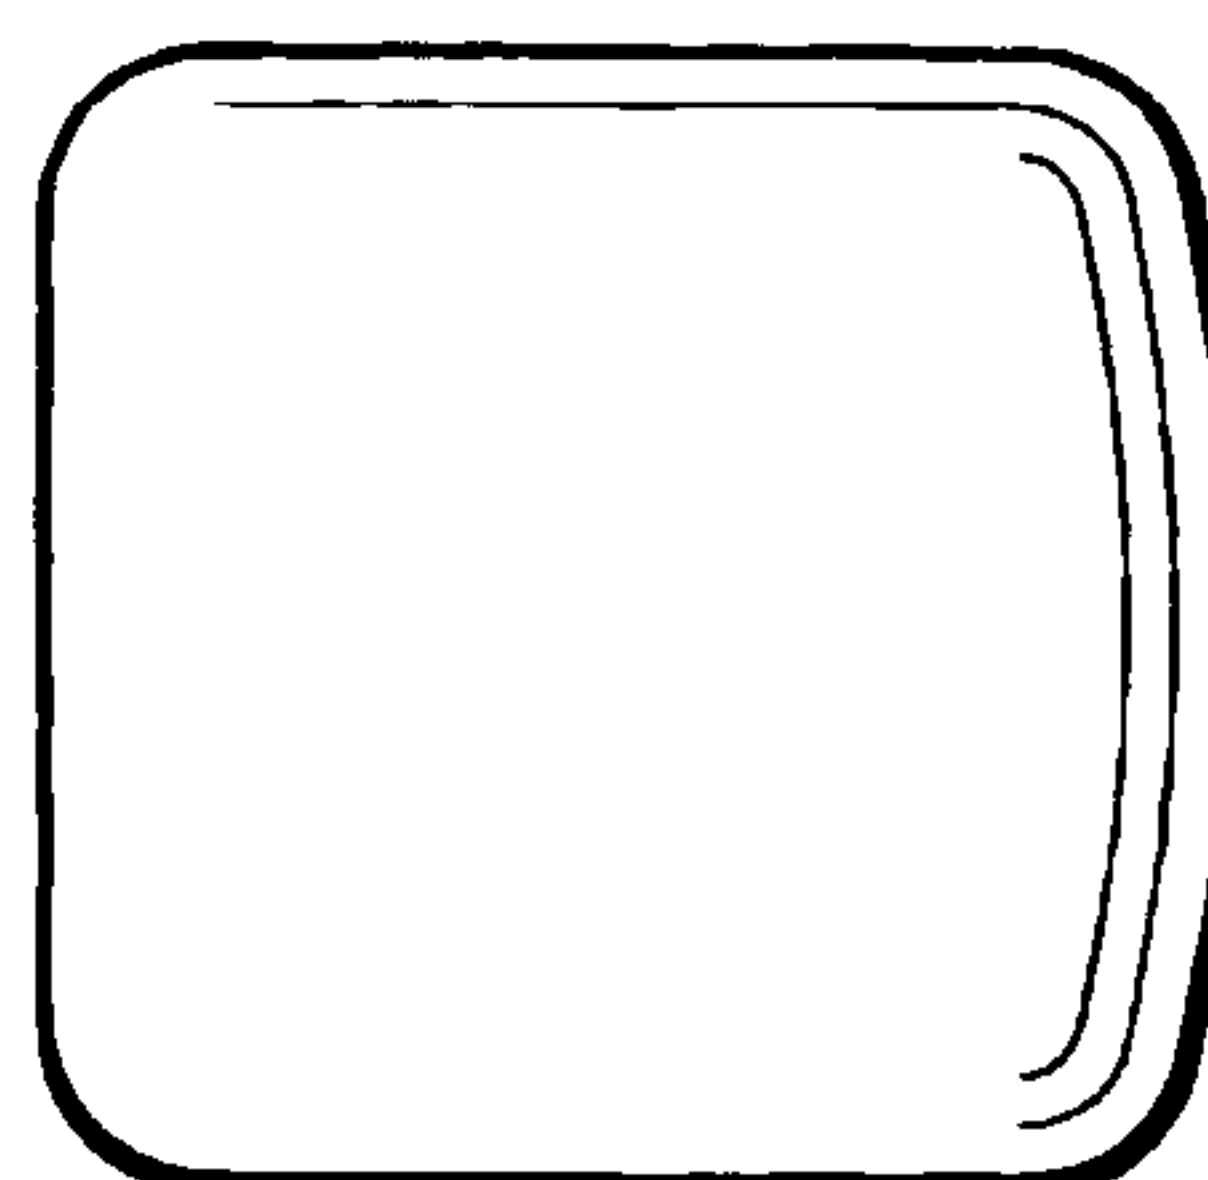


Fig. 7