

US00D526415S

(12) **United States Design Patent**  
**Yang**

(10) **Patent No.:** **US D526,415 S**

(45) **Date of Patent:** **\*\* Aug. 8, 2006**

(54) **ELECTRONIC HEMADYNAMOMETER**

D254,806 S \* 4/1980 Kitai et al. .... D24/169  
D445,190 S \* 7/2001 Byler et al. .... D24/165  
D496,104 S \* 9/2004 Eda et al. .... D24/165

(75) Inventor: **Lin-Wen Yang**, Taipei (TW)

\* cited by examiner

(73) Assignee: **Rossmax International Ltd.**, Taipei (TW)

*Primary Examiner*—Louis S. Zarfaz

*Assistant Examiner*—Daniel Yu

(\*\*) Term: **14 Years**

(74) *Attorney, Agent, or Firm*—Thomas, Kayden, Horstemeyer & Risley

(21) Appl. No.: **29/211,390**

(57) **CLAIM**

(22) Filed: **Aug. 16, 2004**

A new design for an electronic hemadynamometer, as shown and described.

(30) **Foreign Application Priority Data**

Jun. 7, 2004 (TW) ..... 93303405

**DESCRIPTION**

(51) **LOC (8) Cl.** ..... **24-02**

(52) **U.S. Cl.** ..... **D24/169**

(58) **Field of Classification Search** ..... D24/165,  
D24/169; 600/485, 494, 500, 480, 490, 491,  
600/493, 495

See application file for complete search history.


FIG. 1 is a front perspective view of an electronic hemadynamometer showing my new design;  
FIG. 2 is a front elevational view thereof;  
FIG. 3 is a left side elevational view thereof;  
FIG. 4 is a right side elevational view thereof;  
FIG. 5 is a top plan view thereof;  
FIG. 6 is a bottom plan view thereof;  
FIG. 7 is a rear elevational view thereof; and,  
FIG. 8 is a rear perspective view of an electronic hemadynamometer showing my new design.

(56) **References Cited**

**U.S. PATENT DOCUMENTS**

D247,575 S \* 3/1978 Bartkus ..... D24/169  
D253,427 S \* 11/1979 Ohie et al. .... D24/169

**1 Claim, 8 Drawing Sheets**

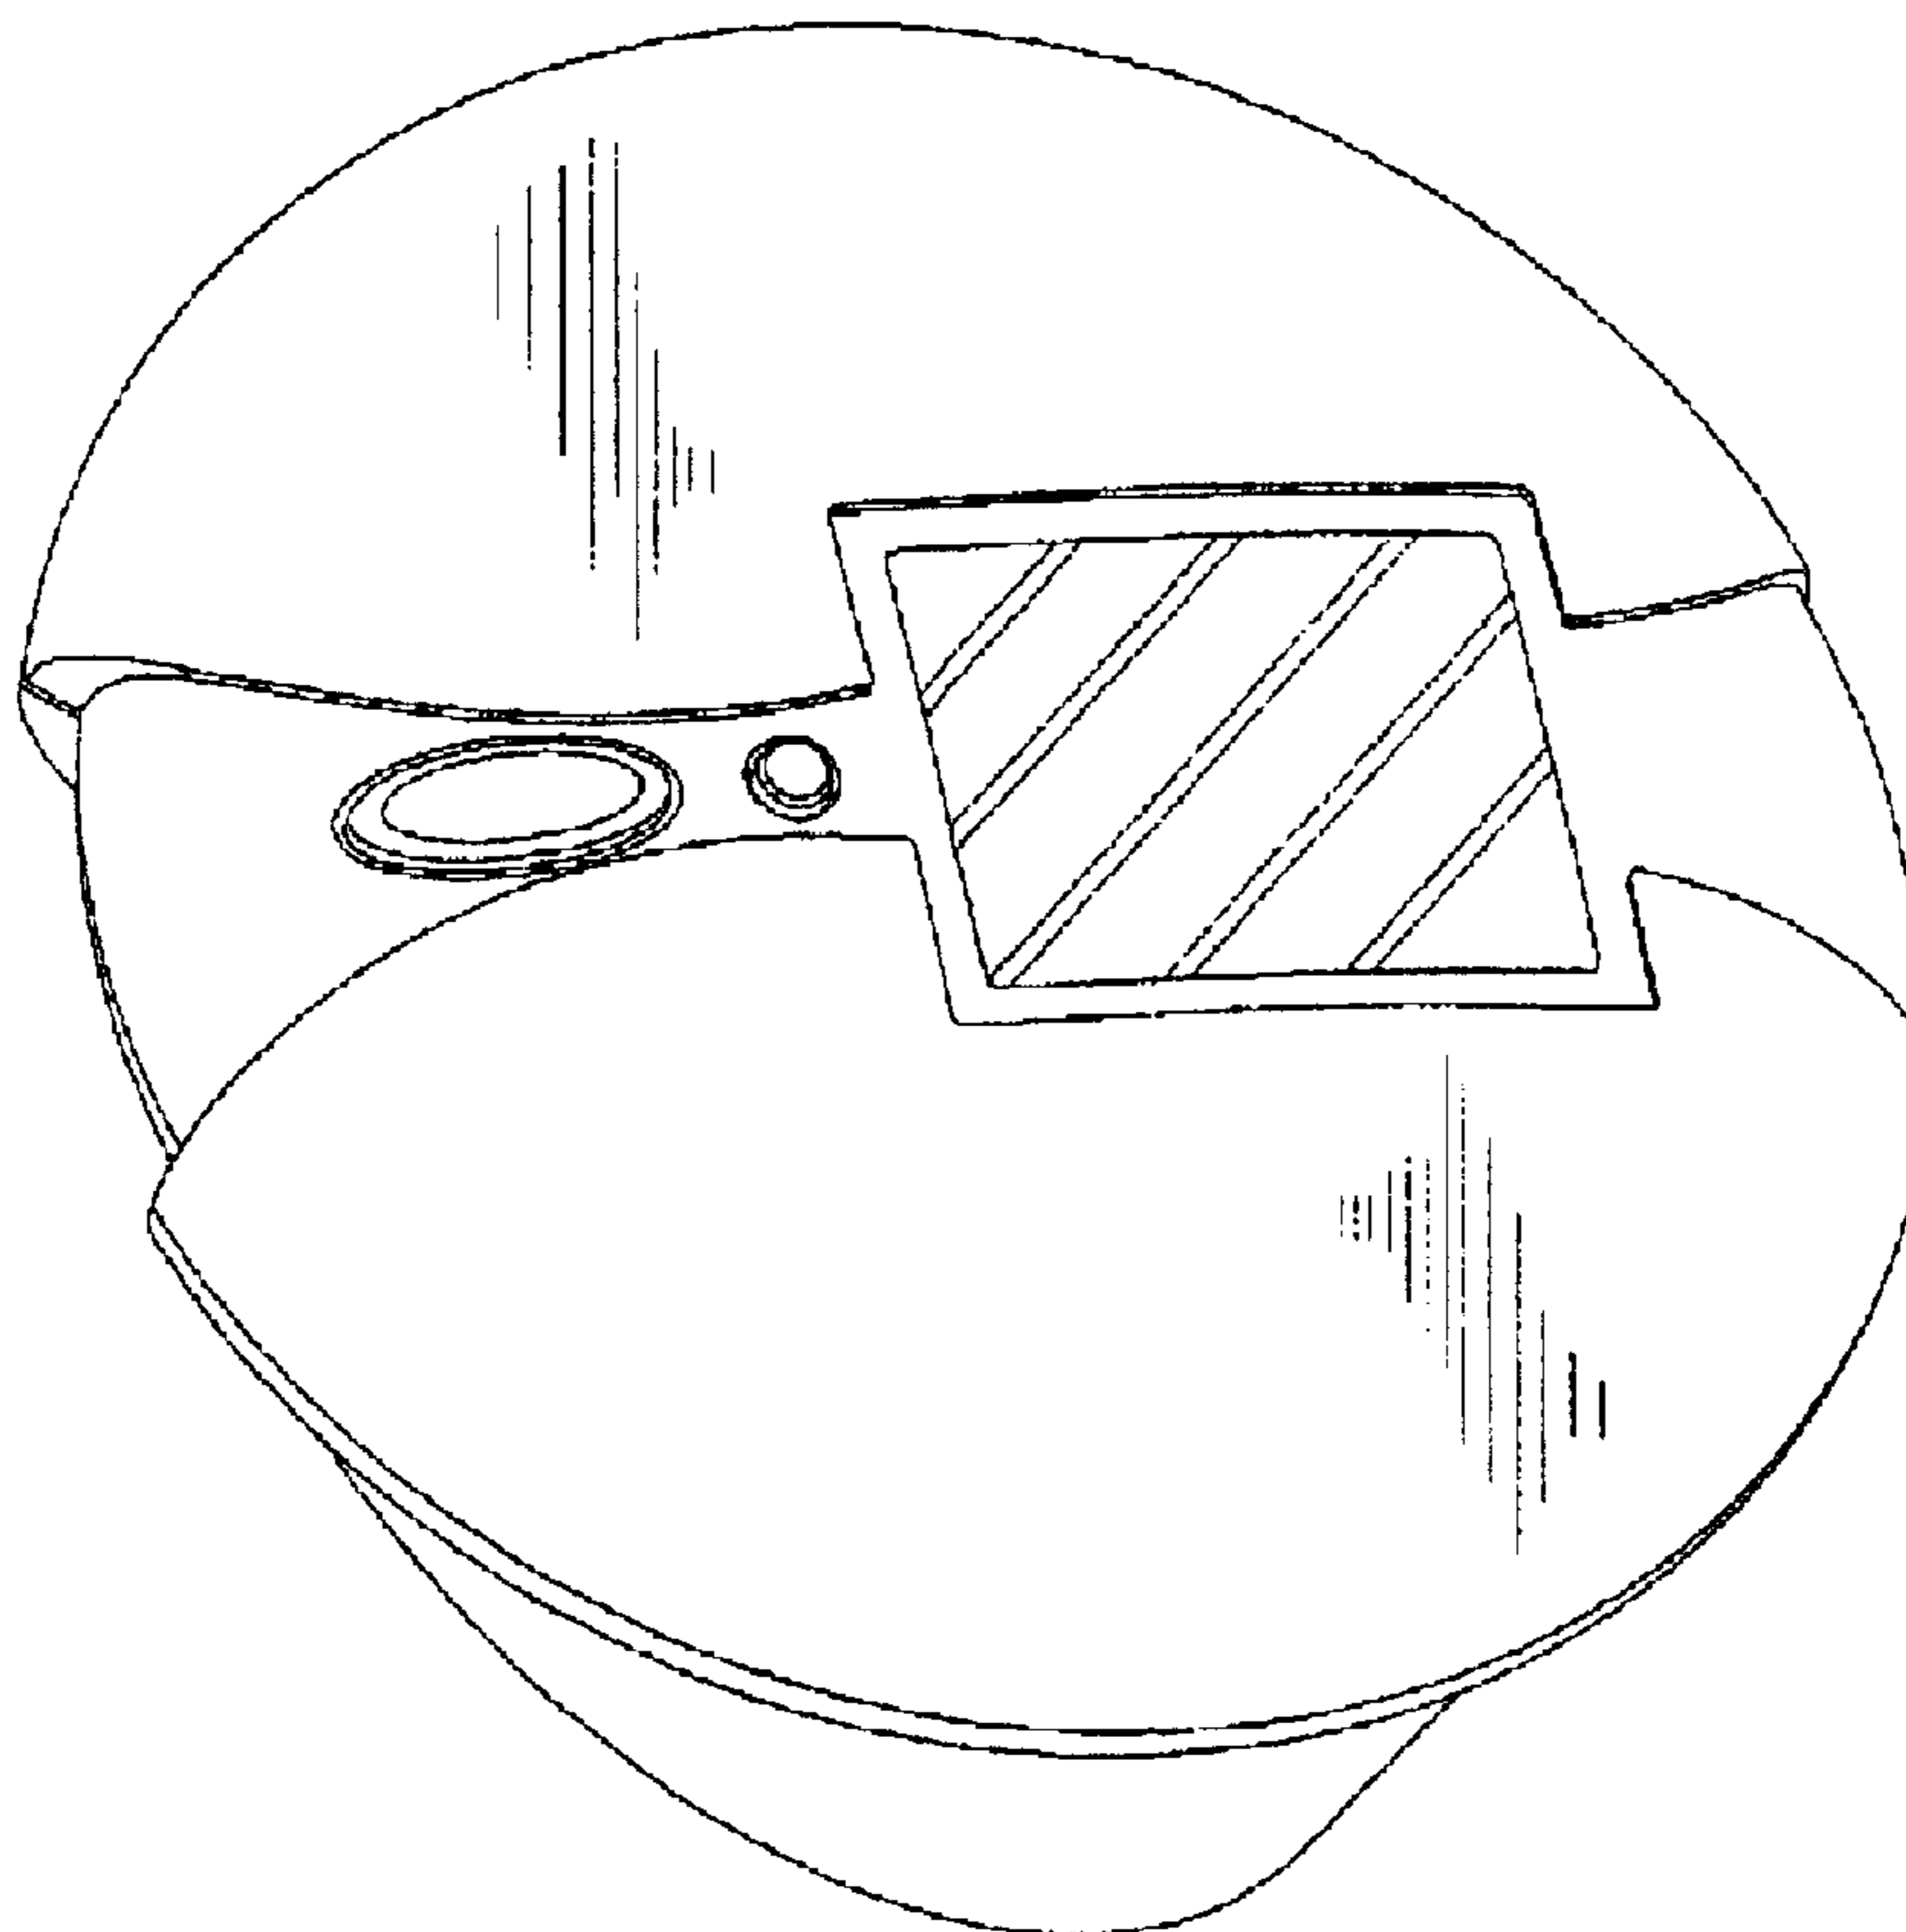

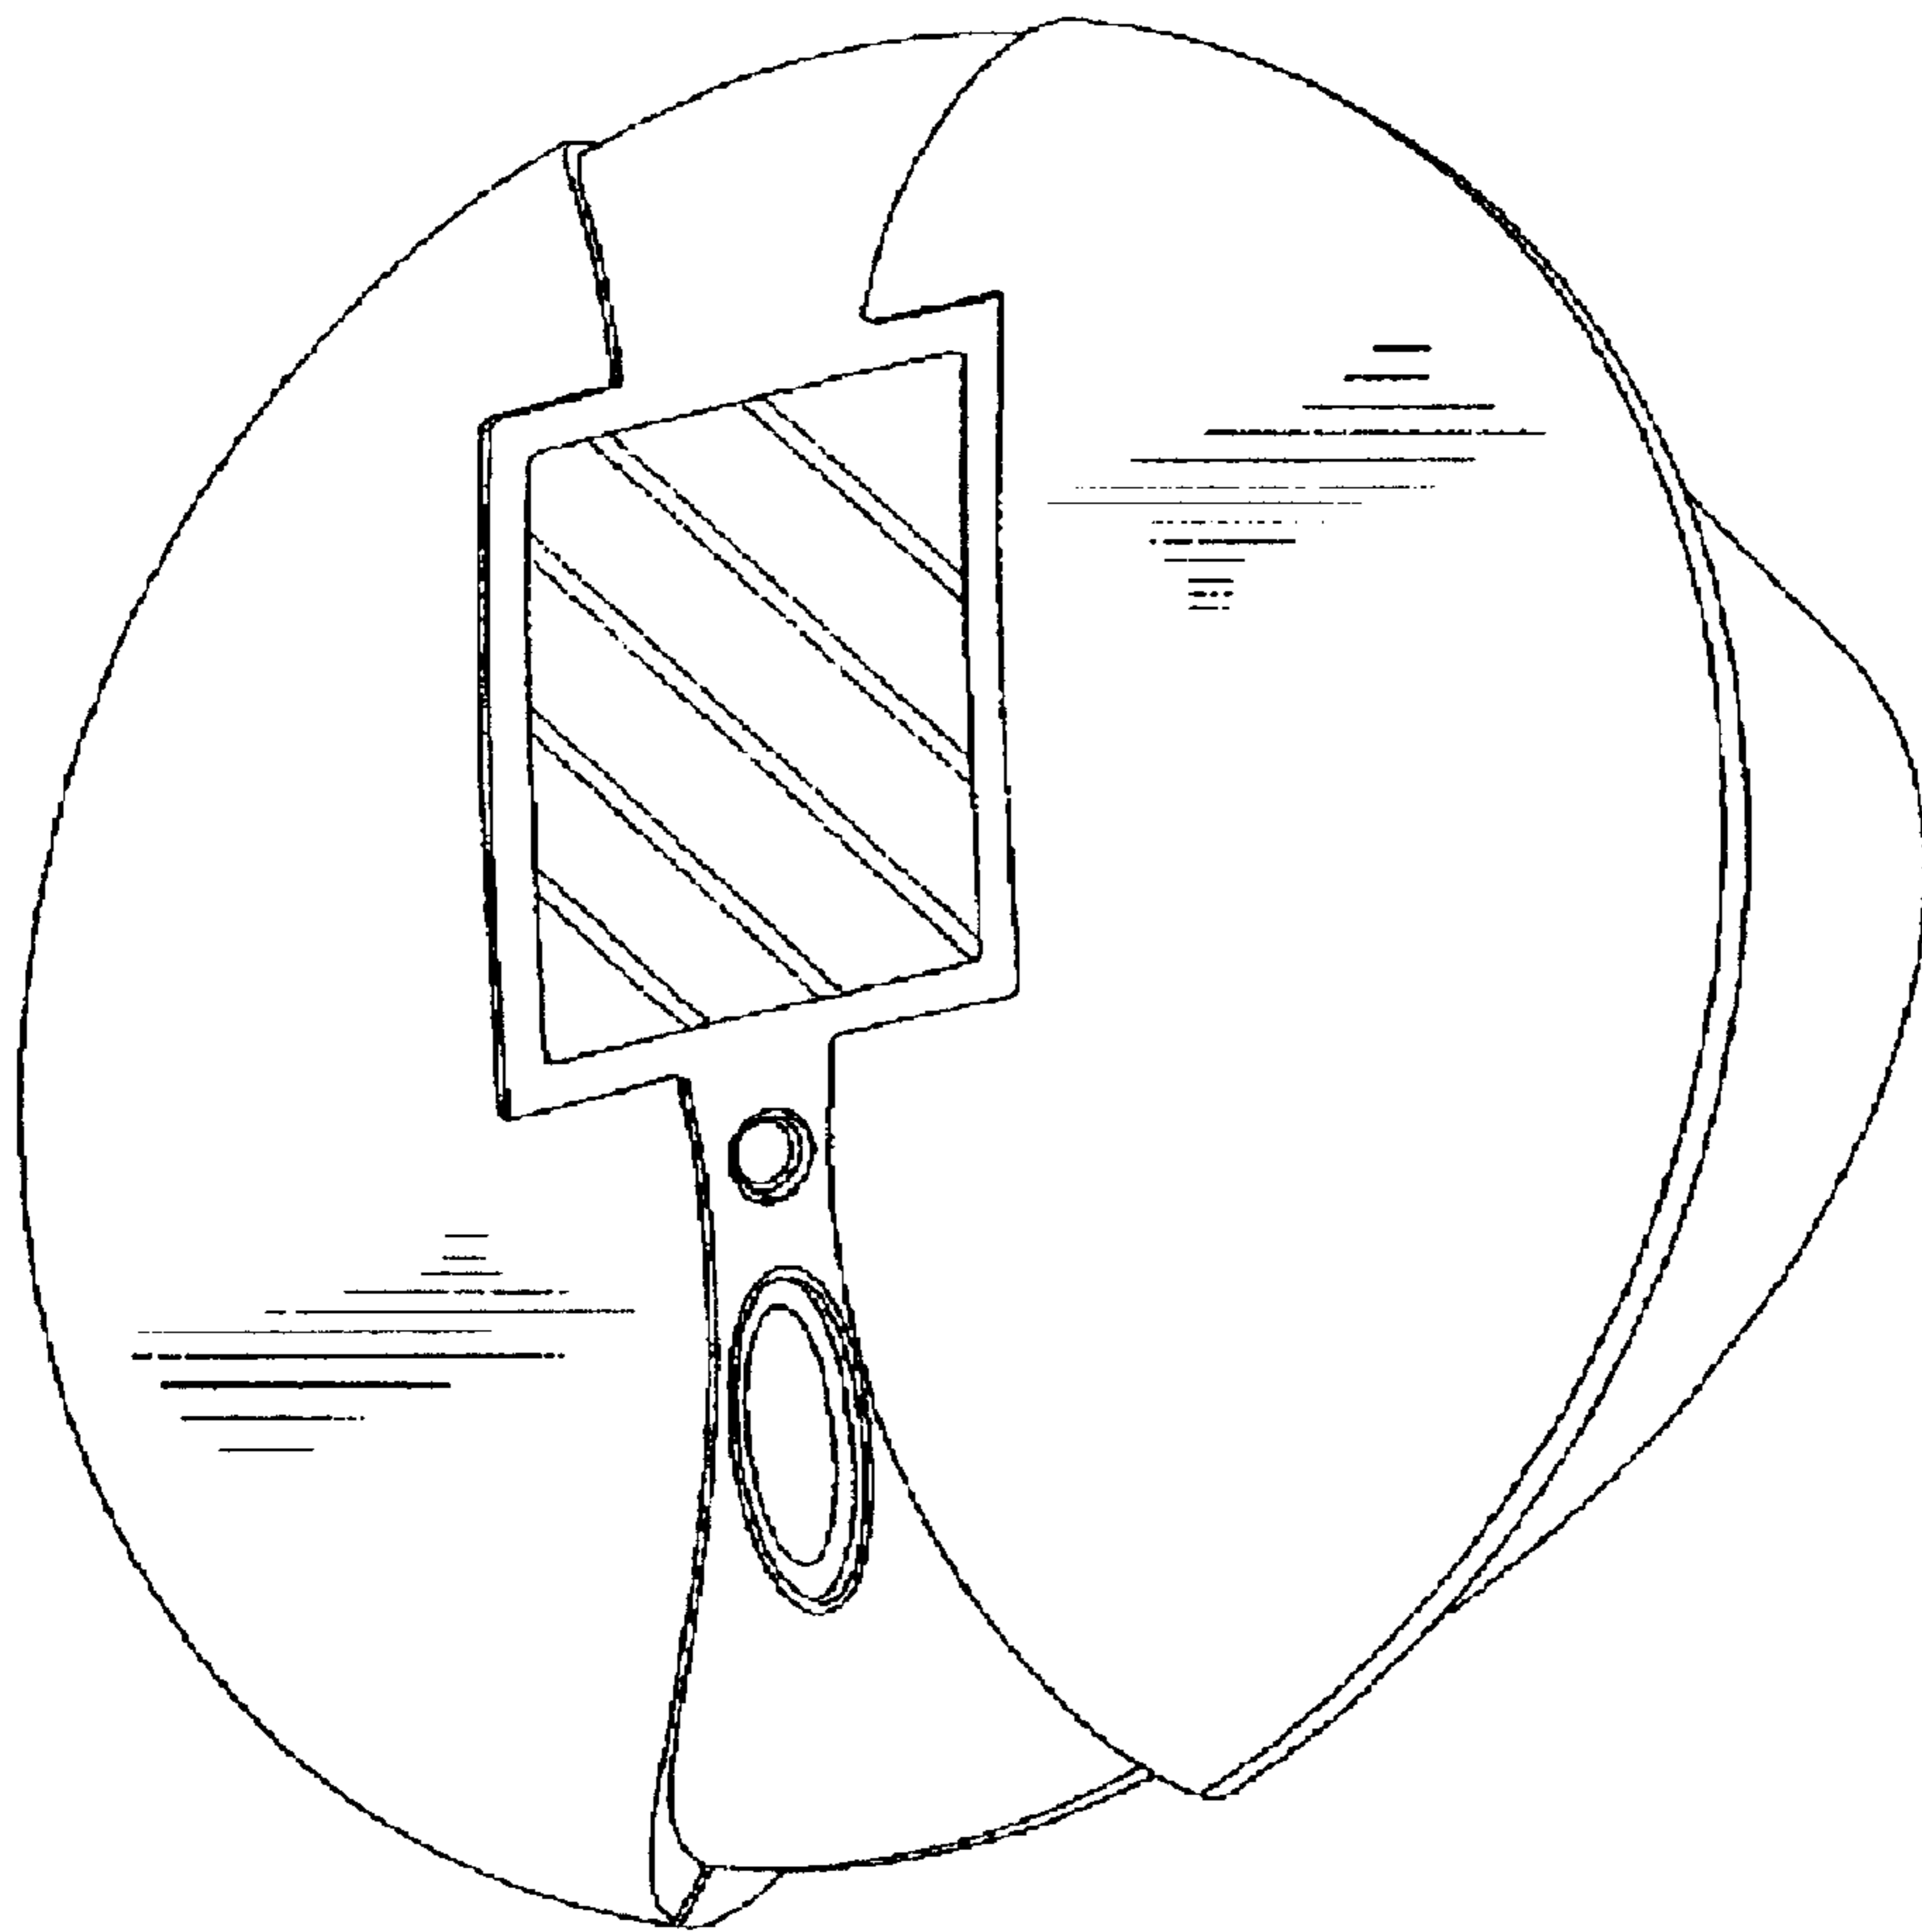


FIG. 1

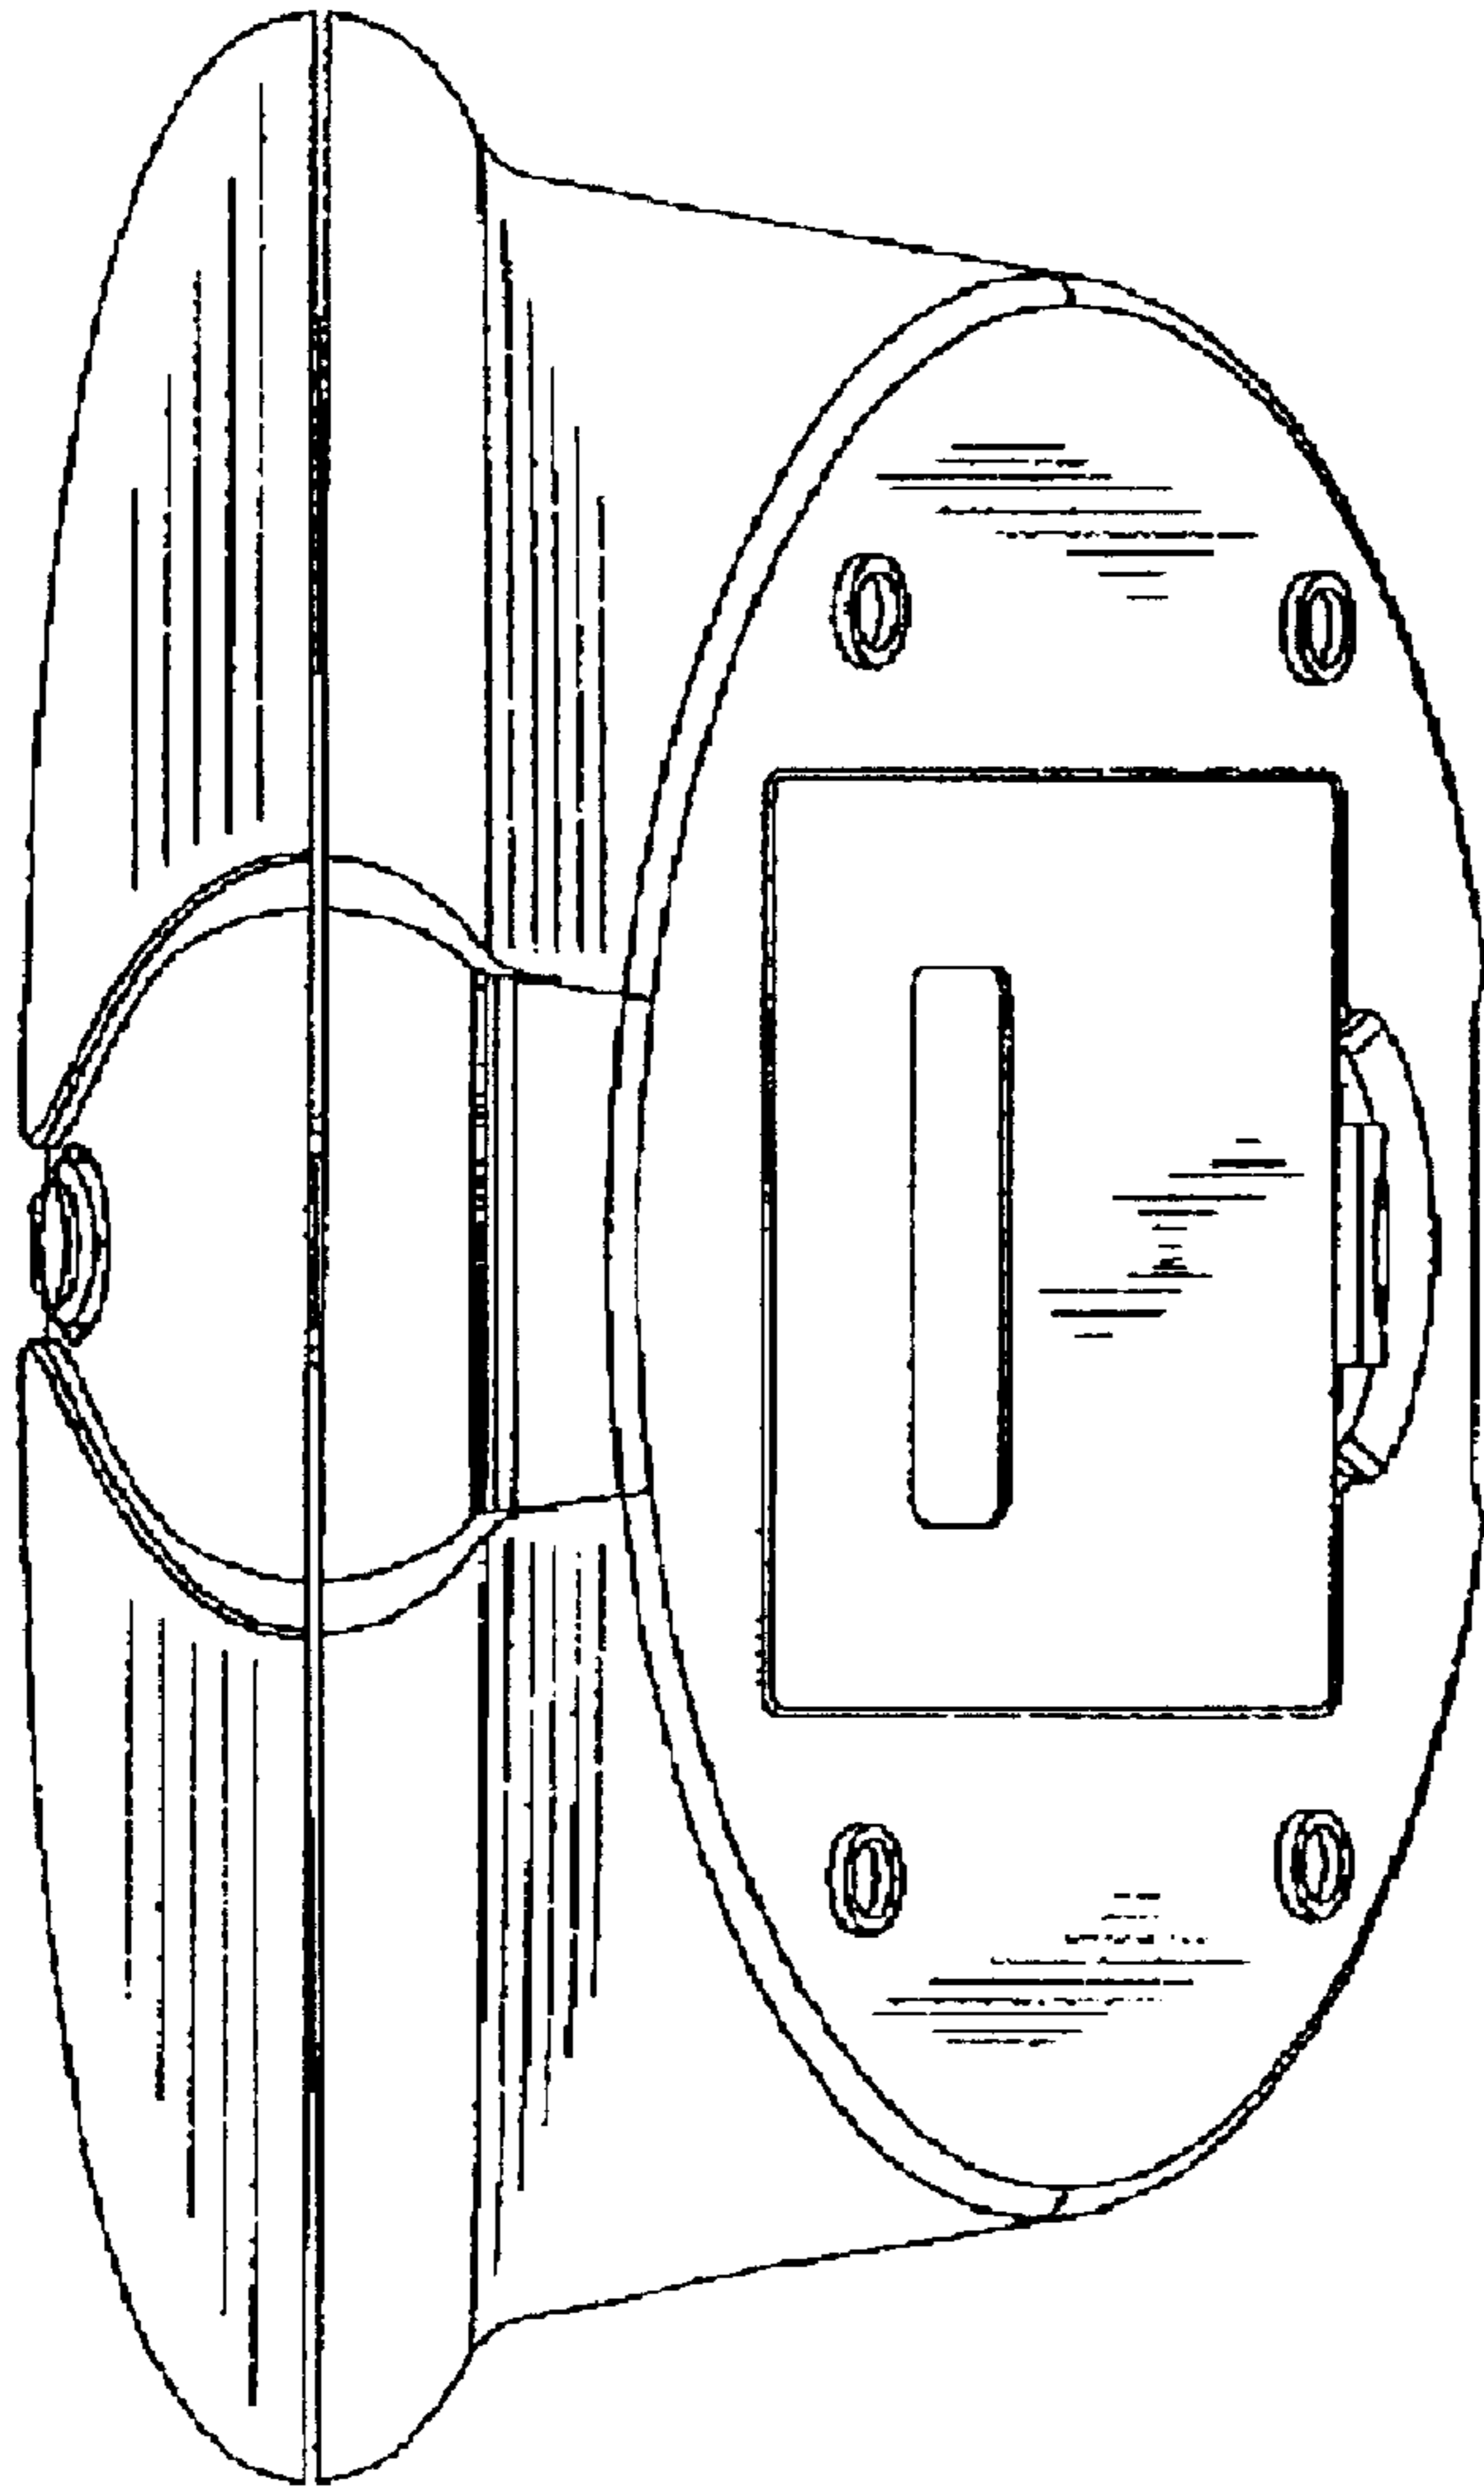


FIG. 2

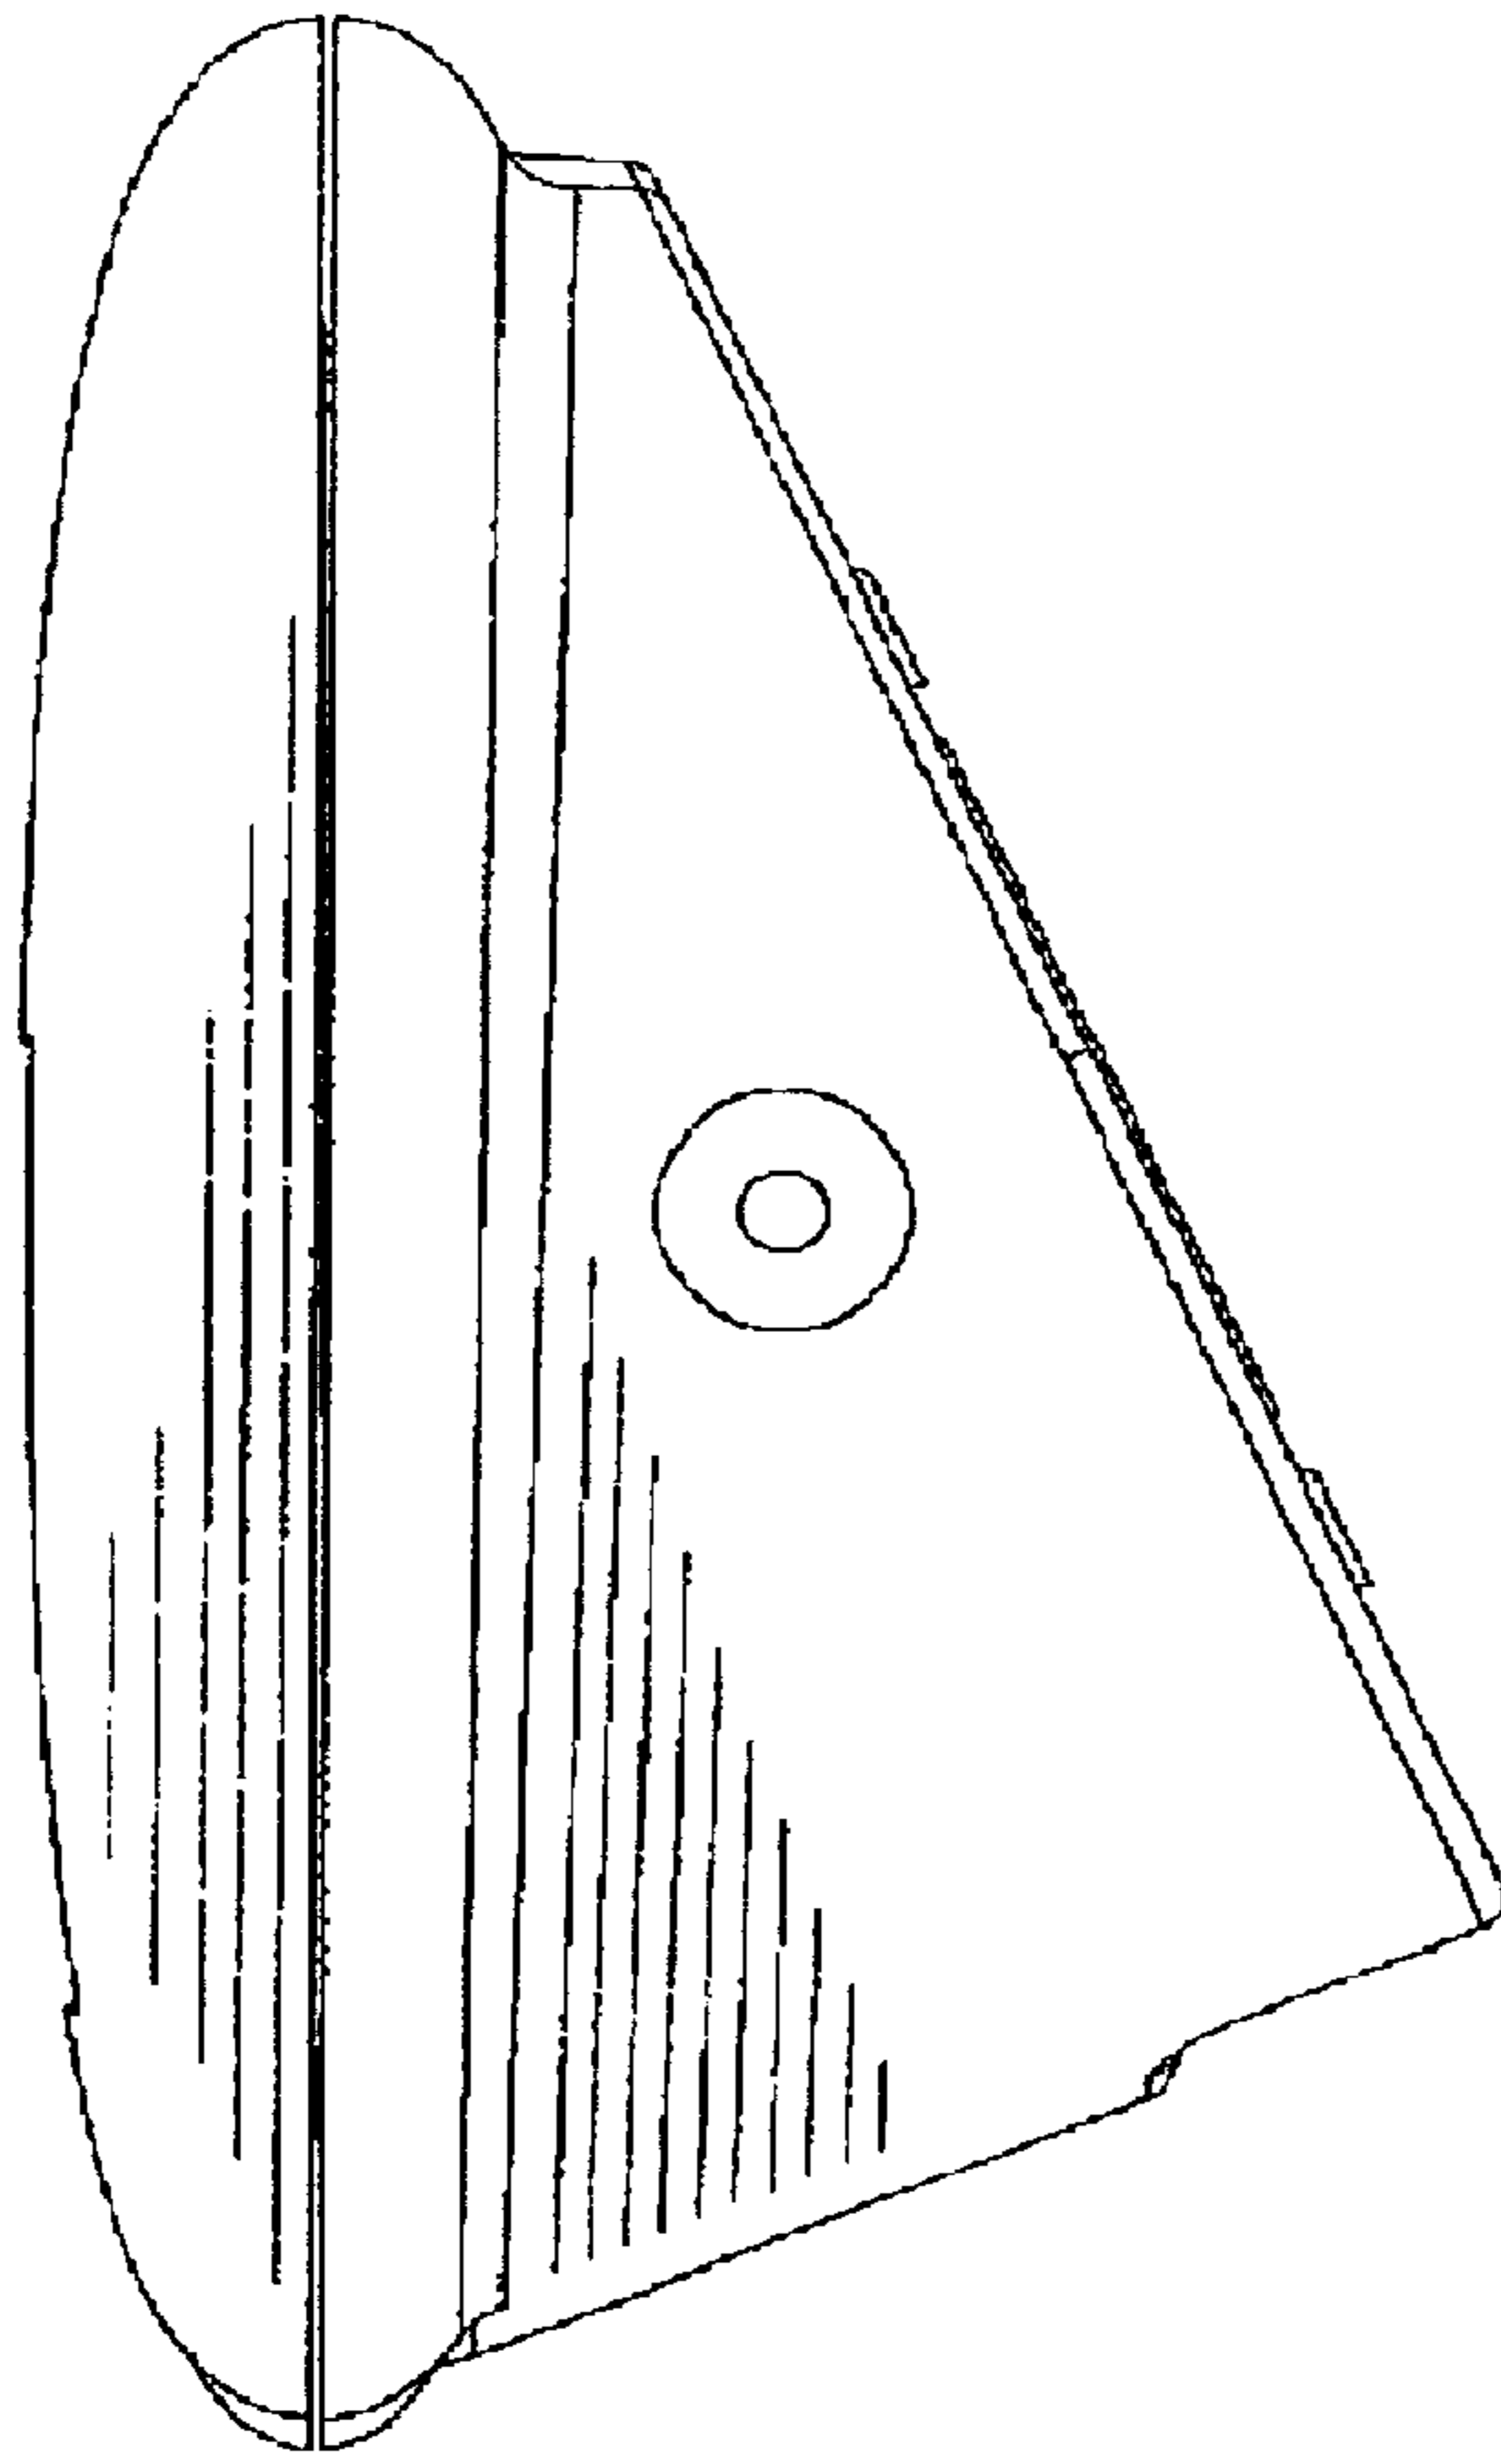


FIG. 3

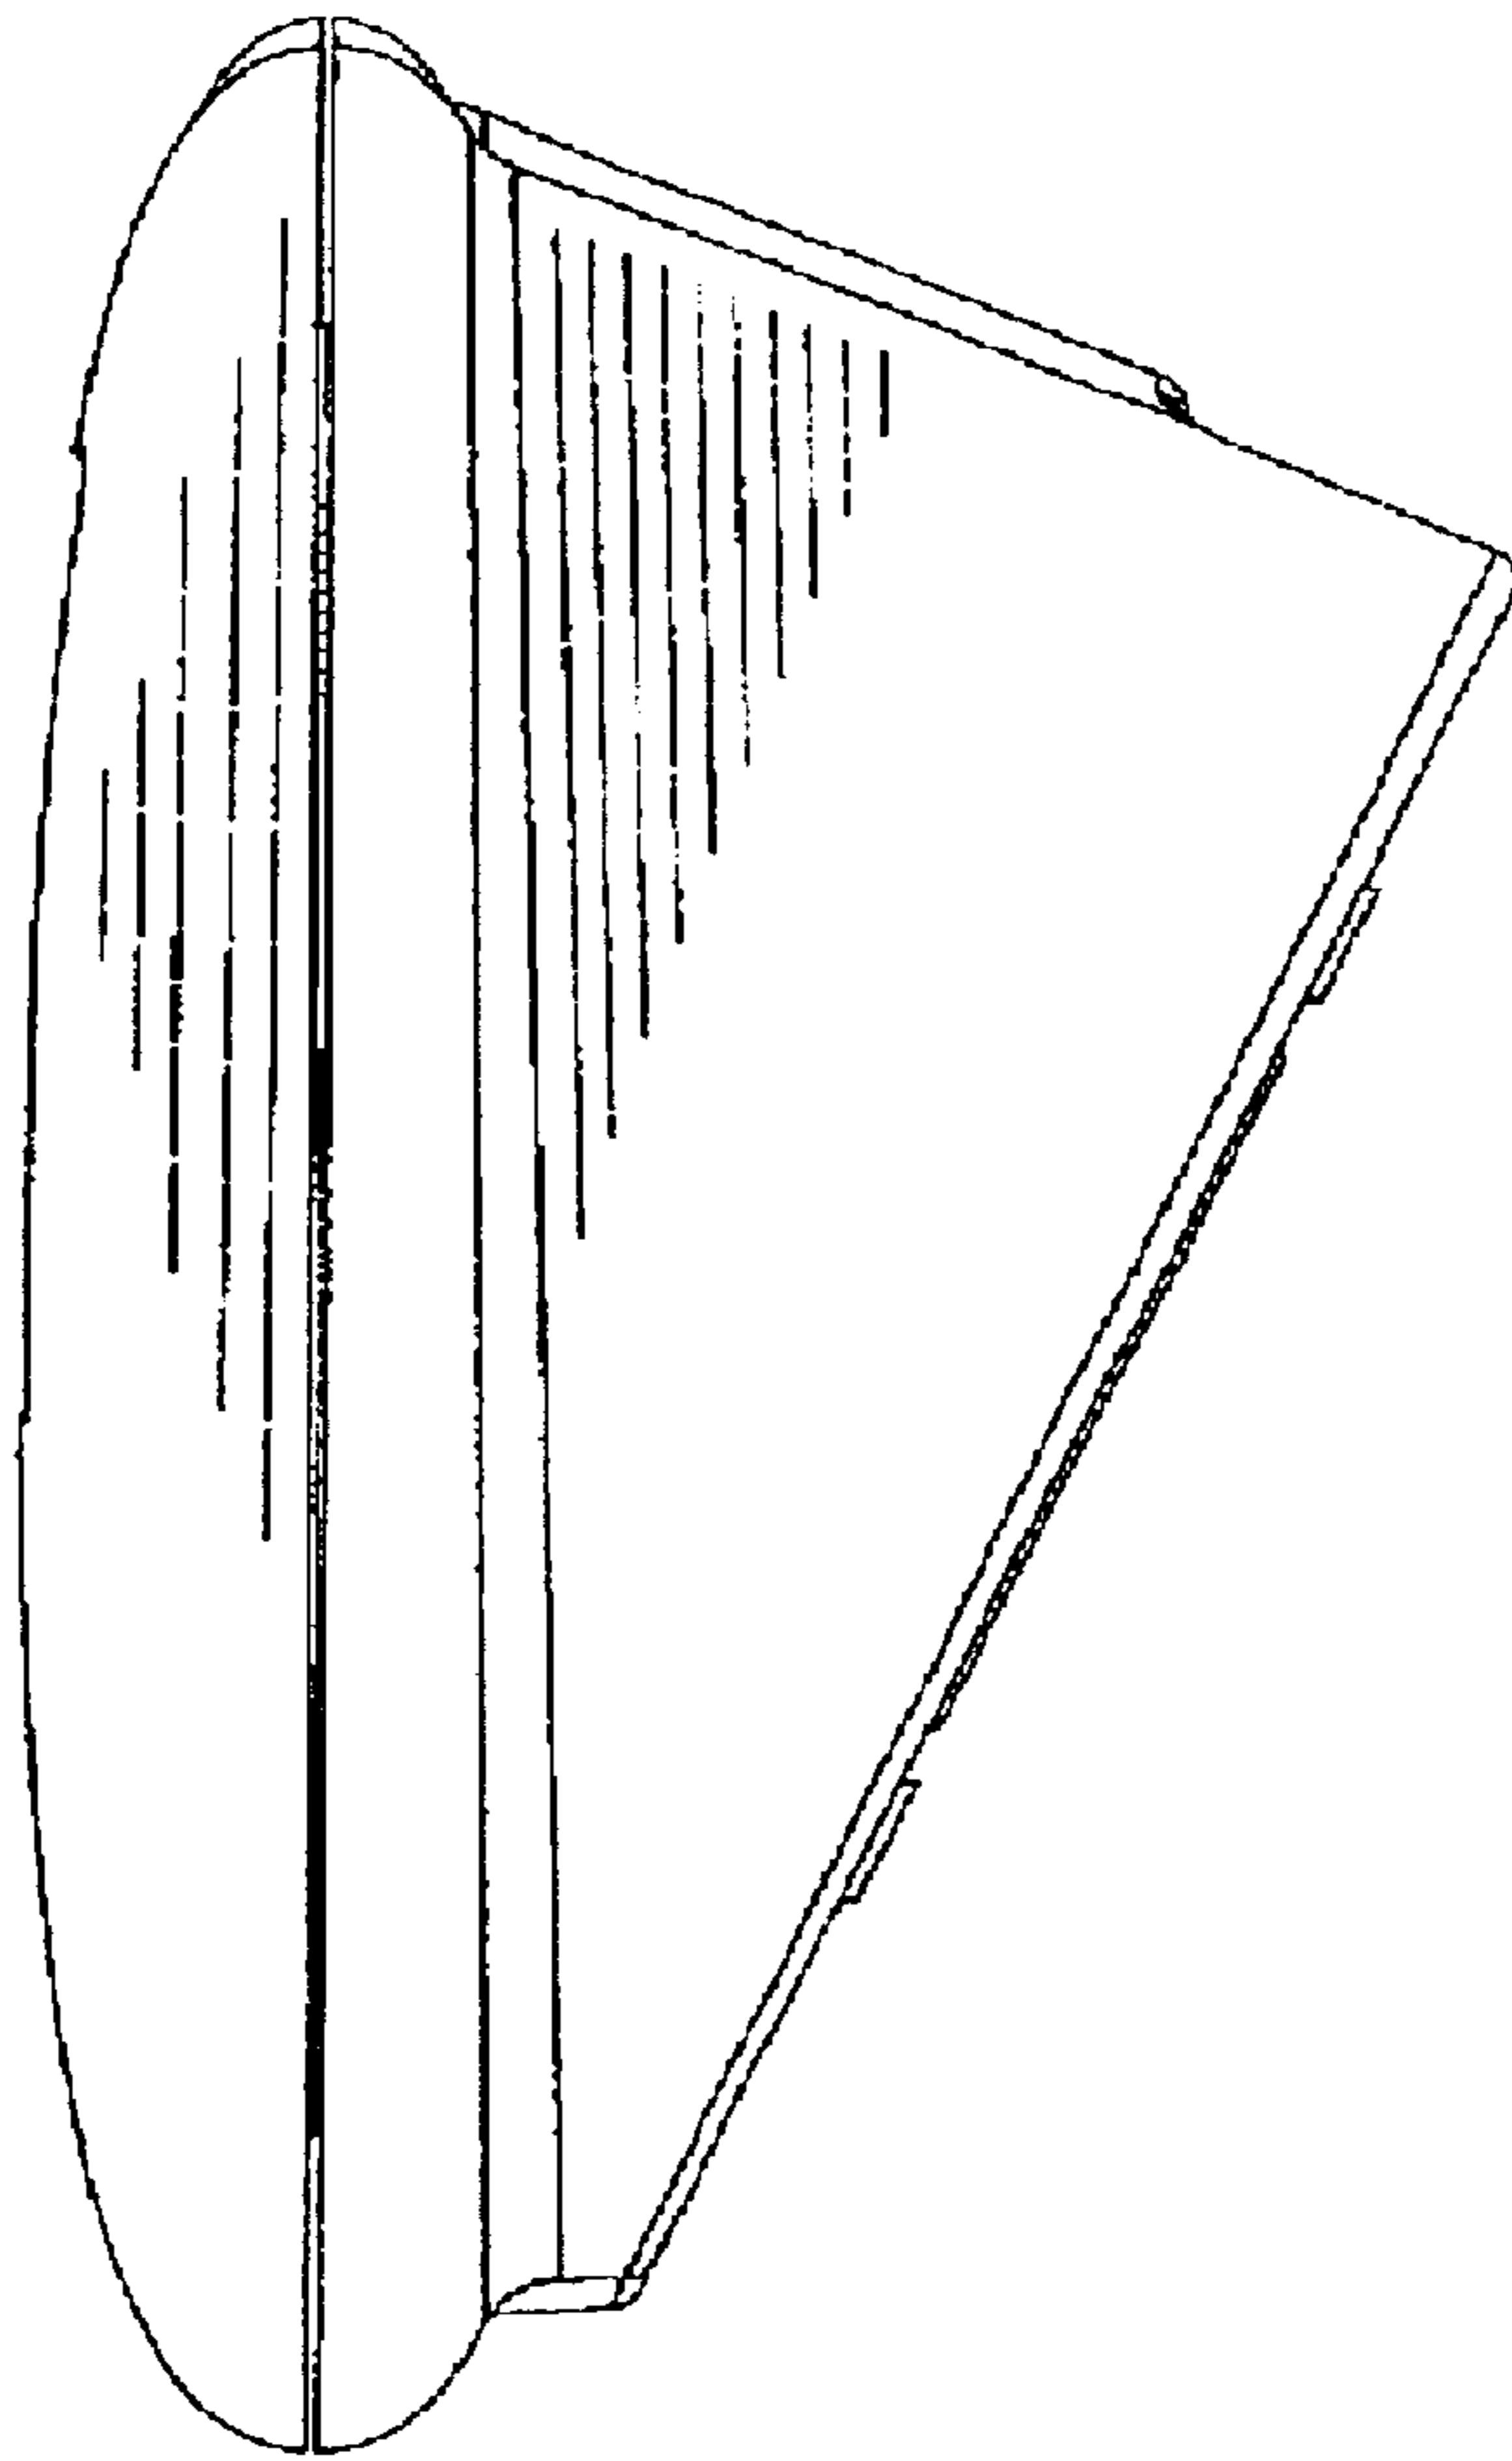


FIG. 4

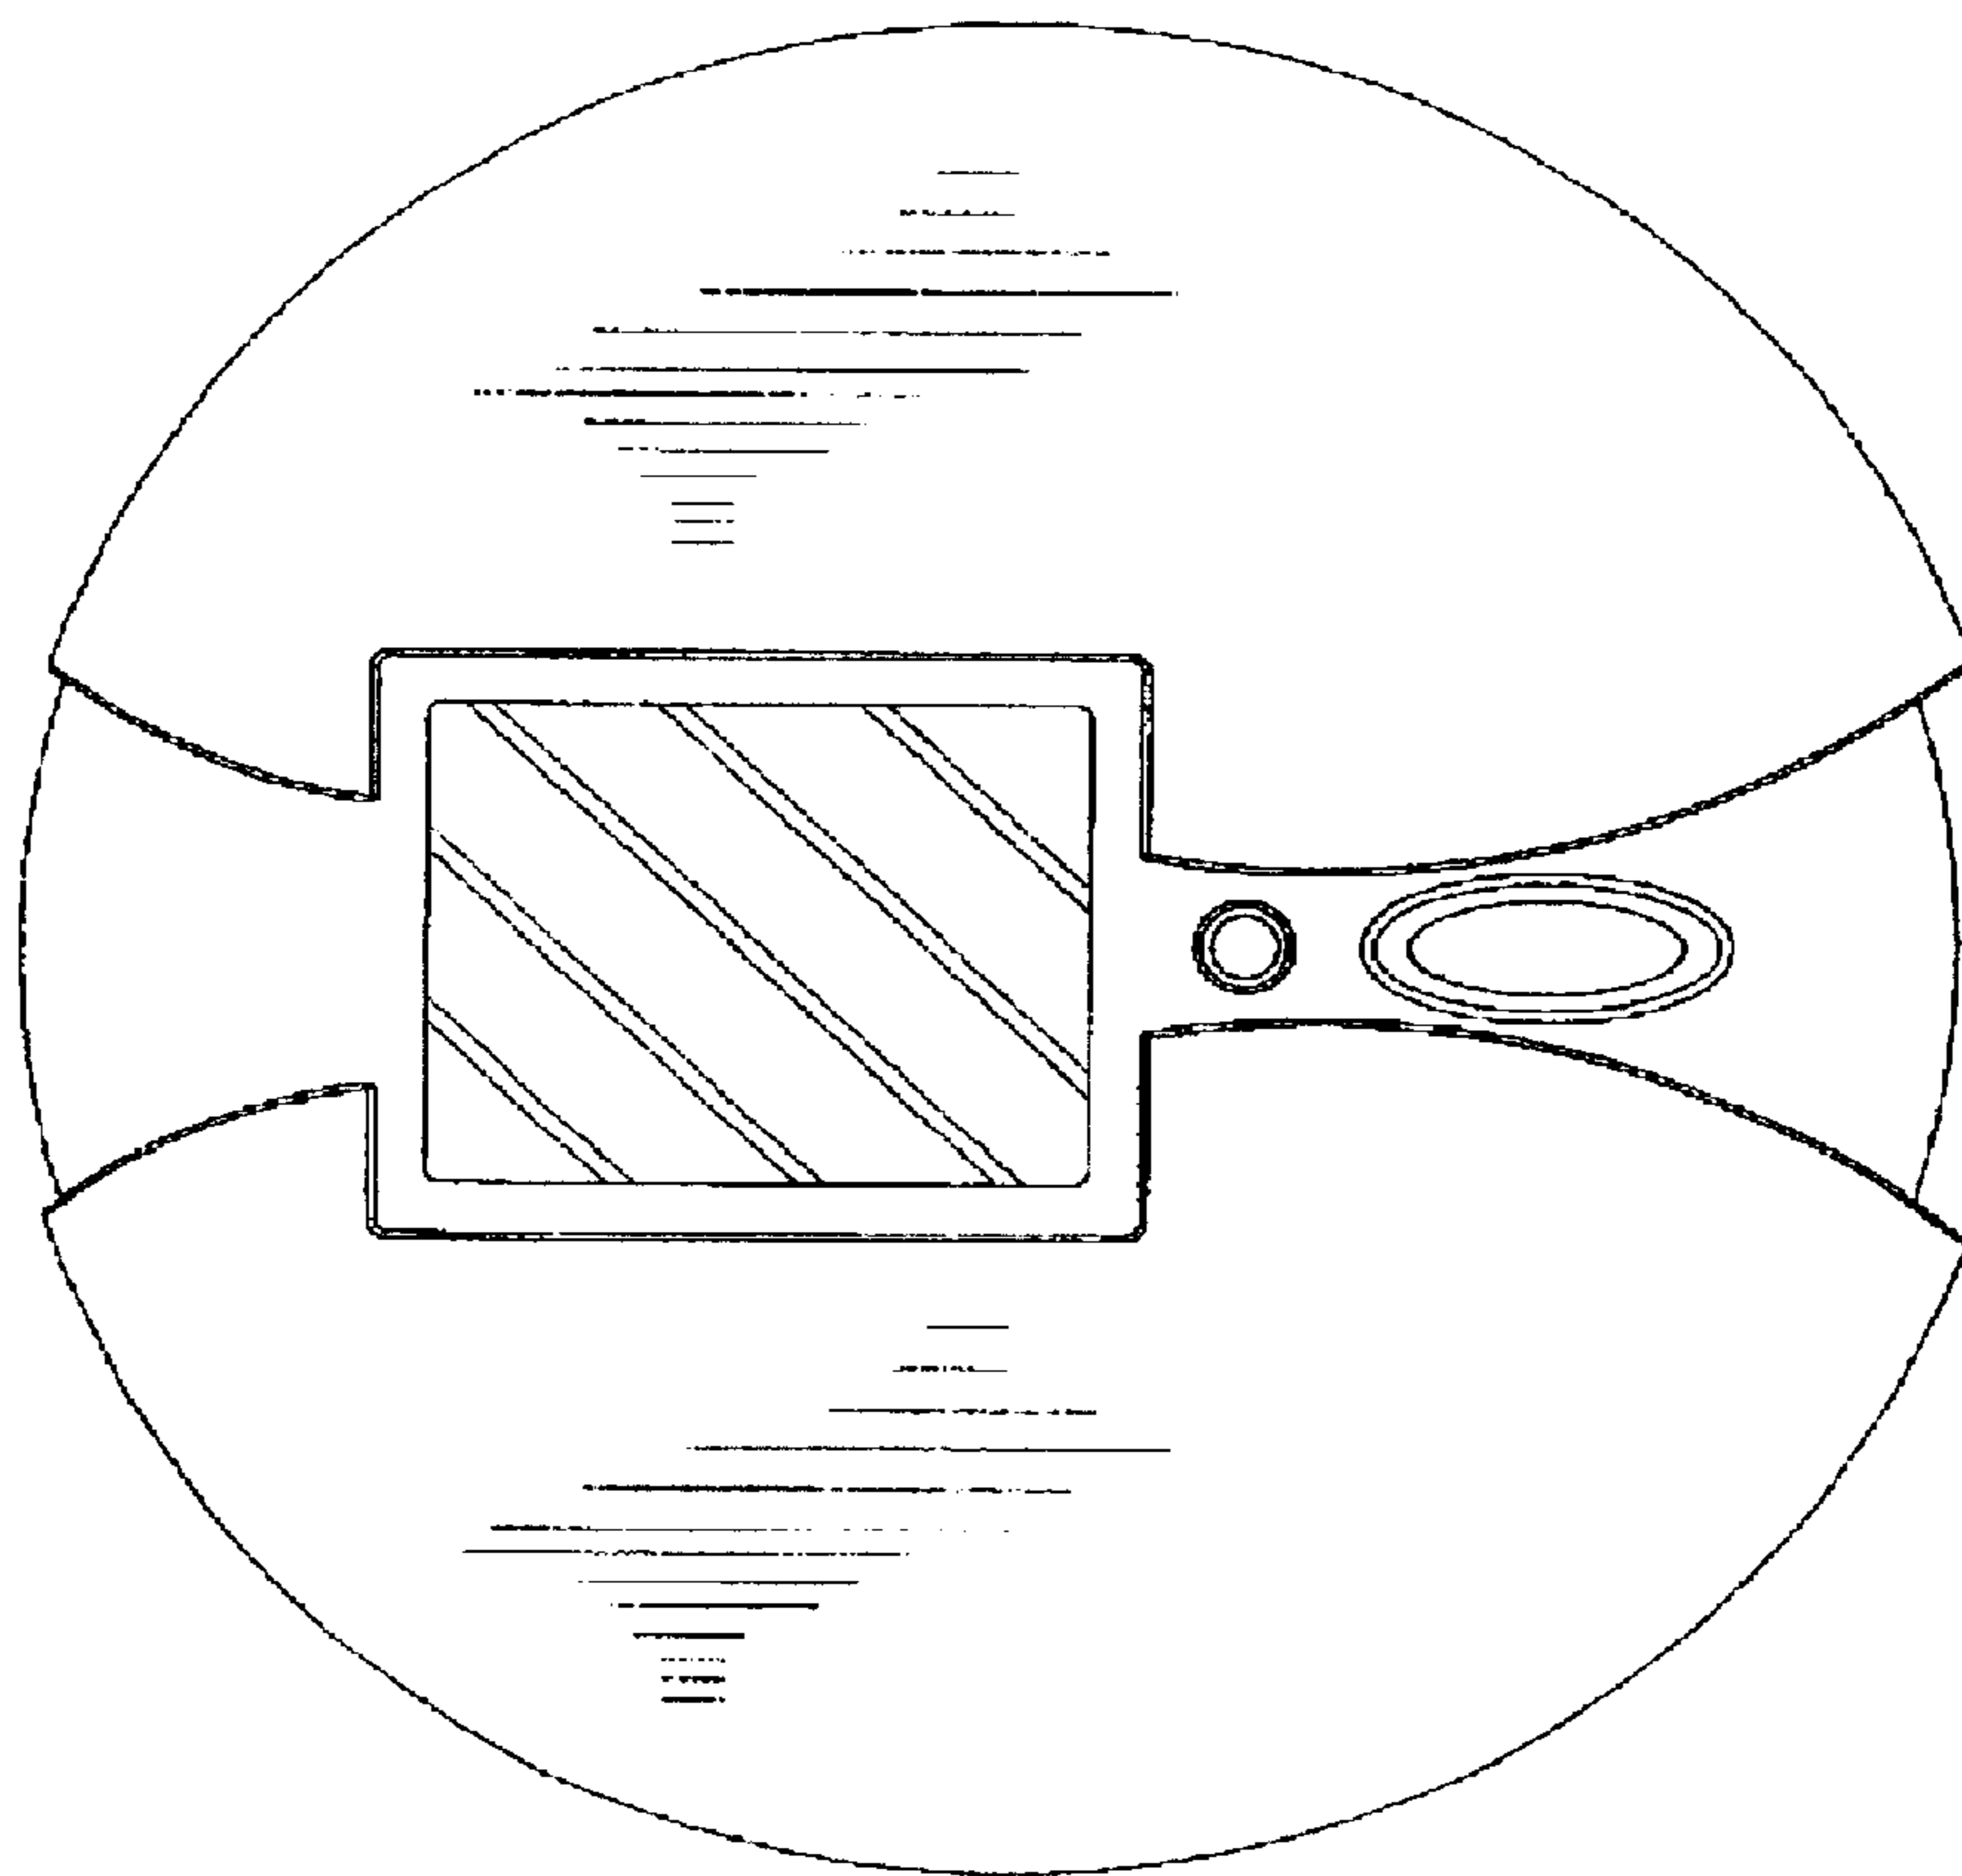


FIG. 5

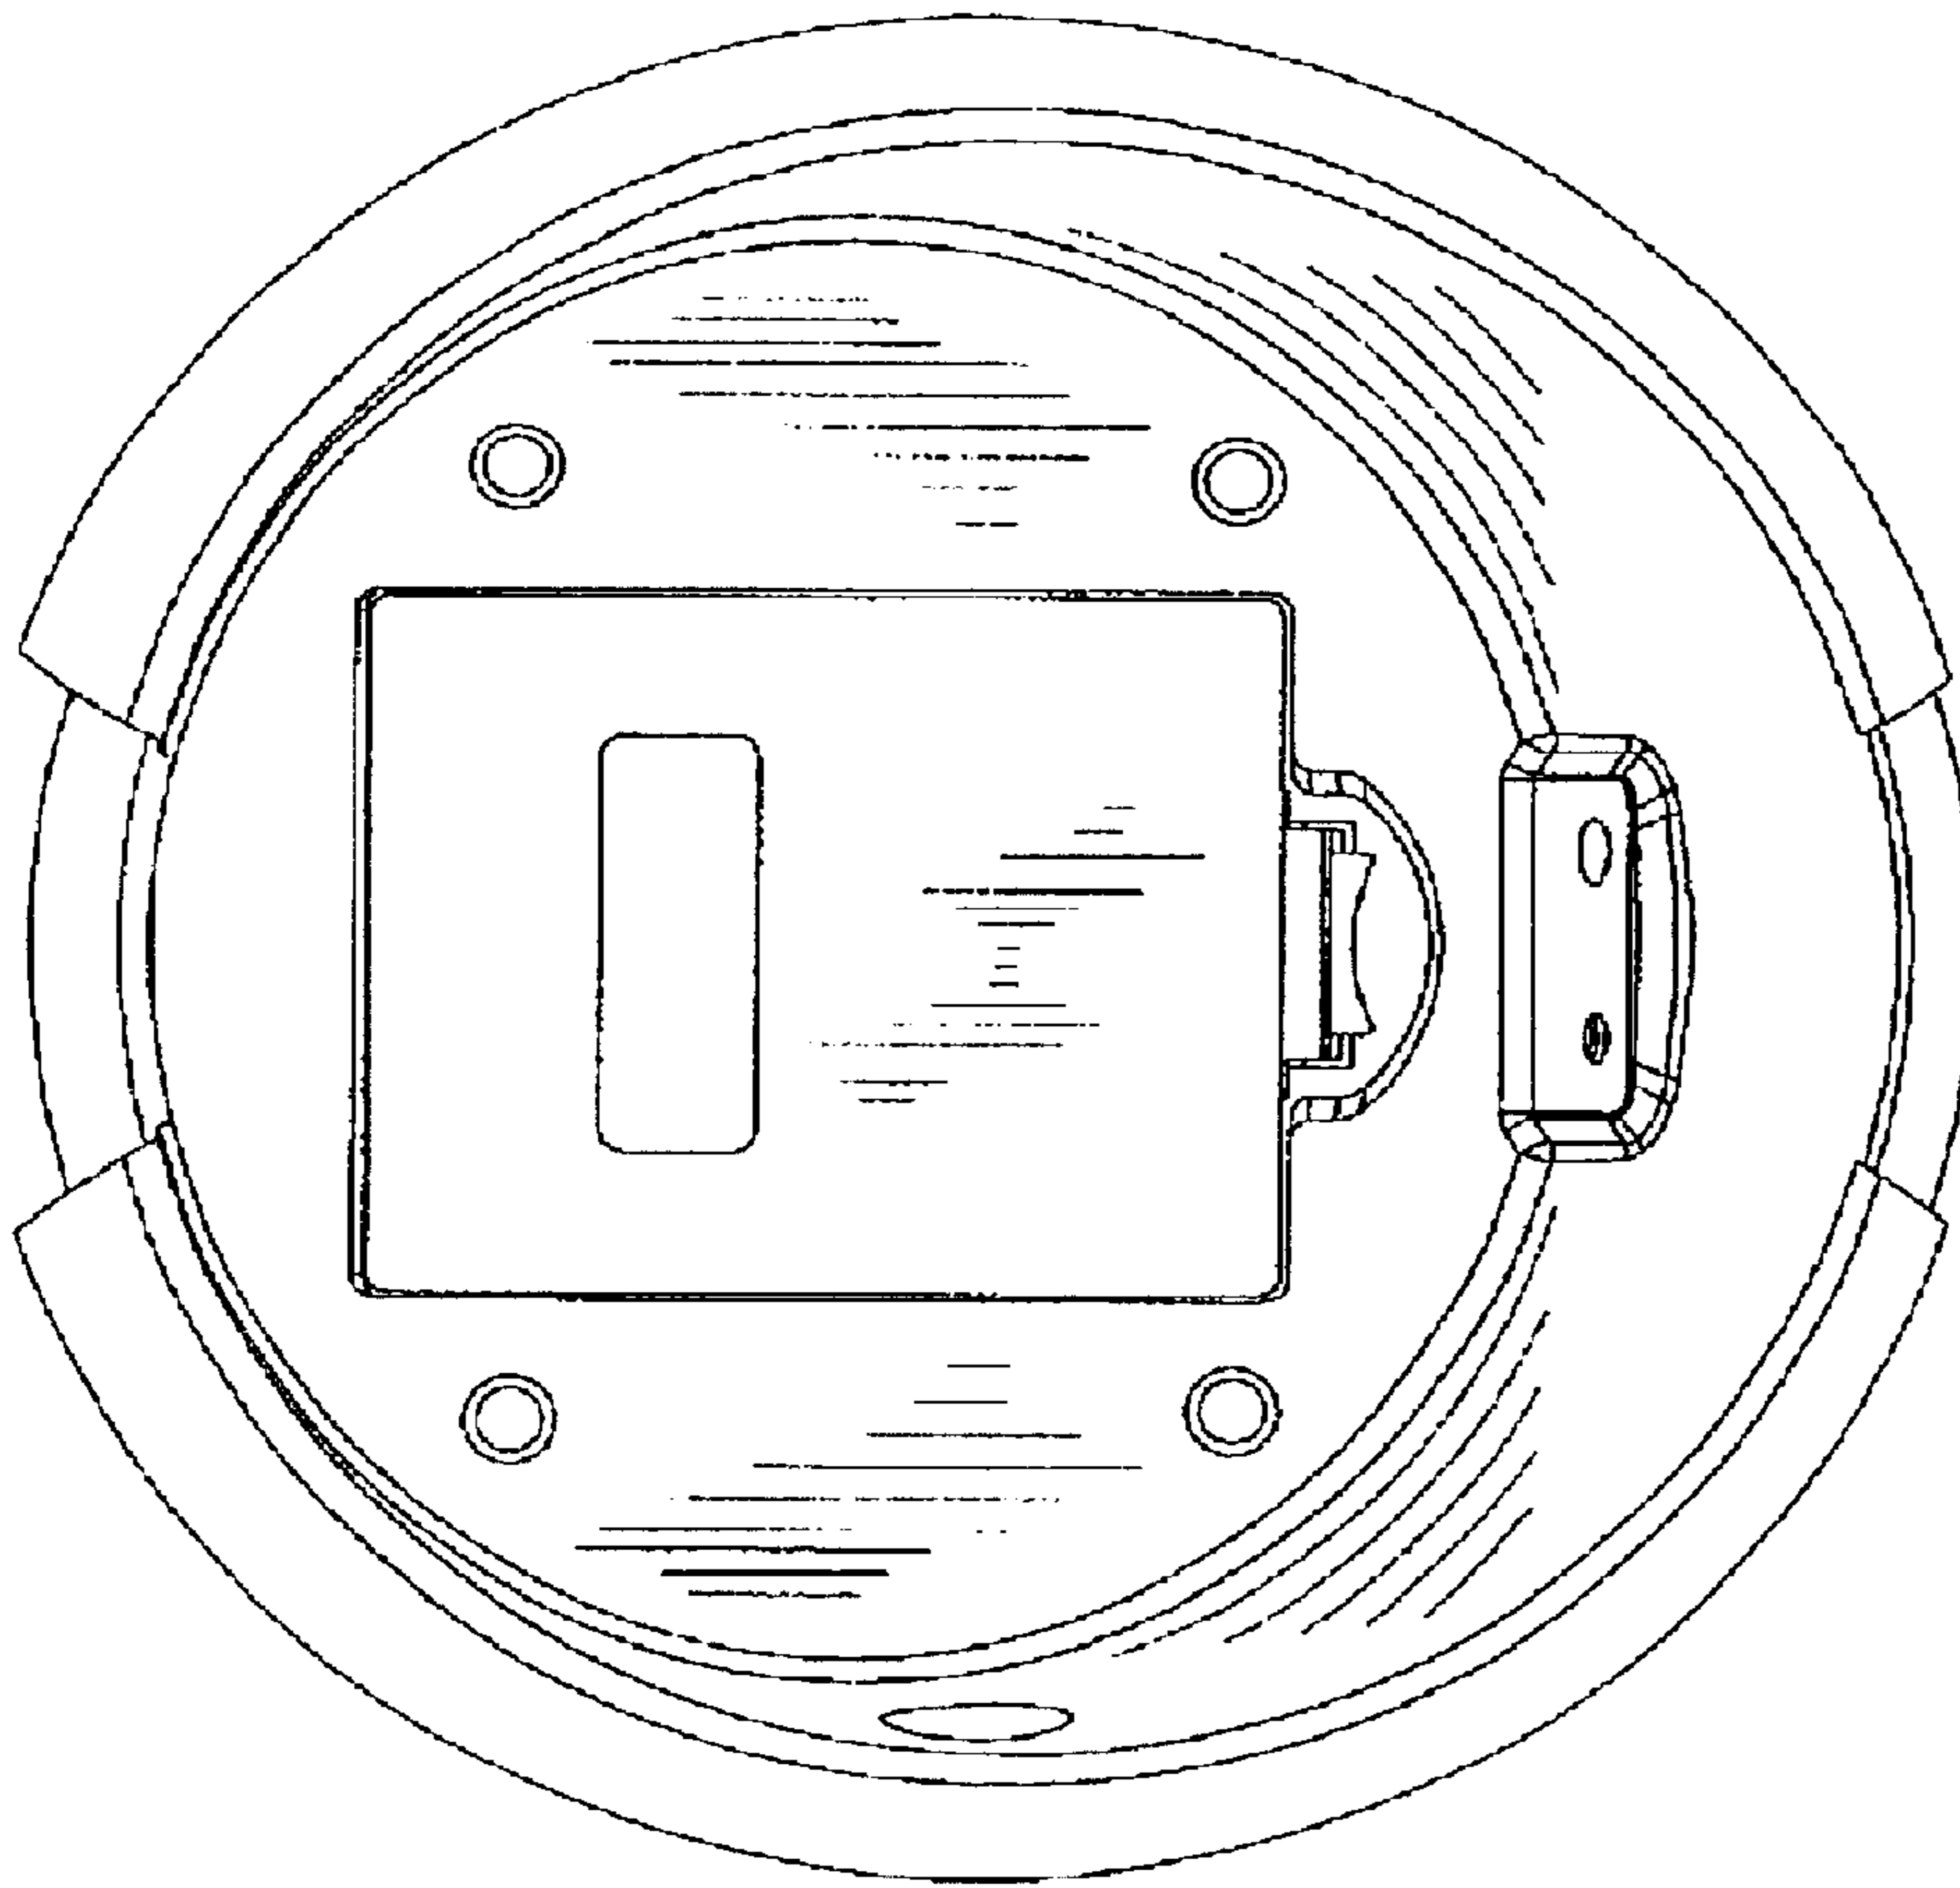


FIG. 6

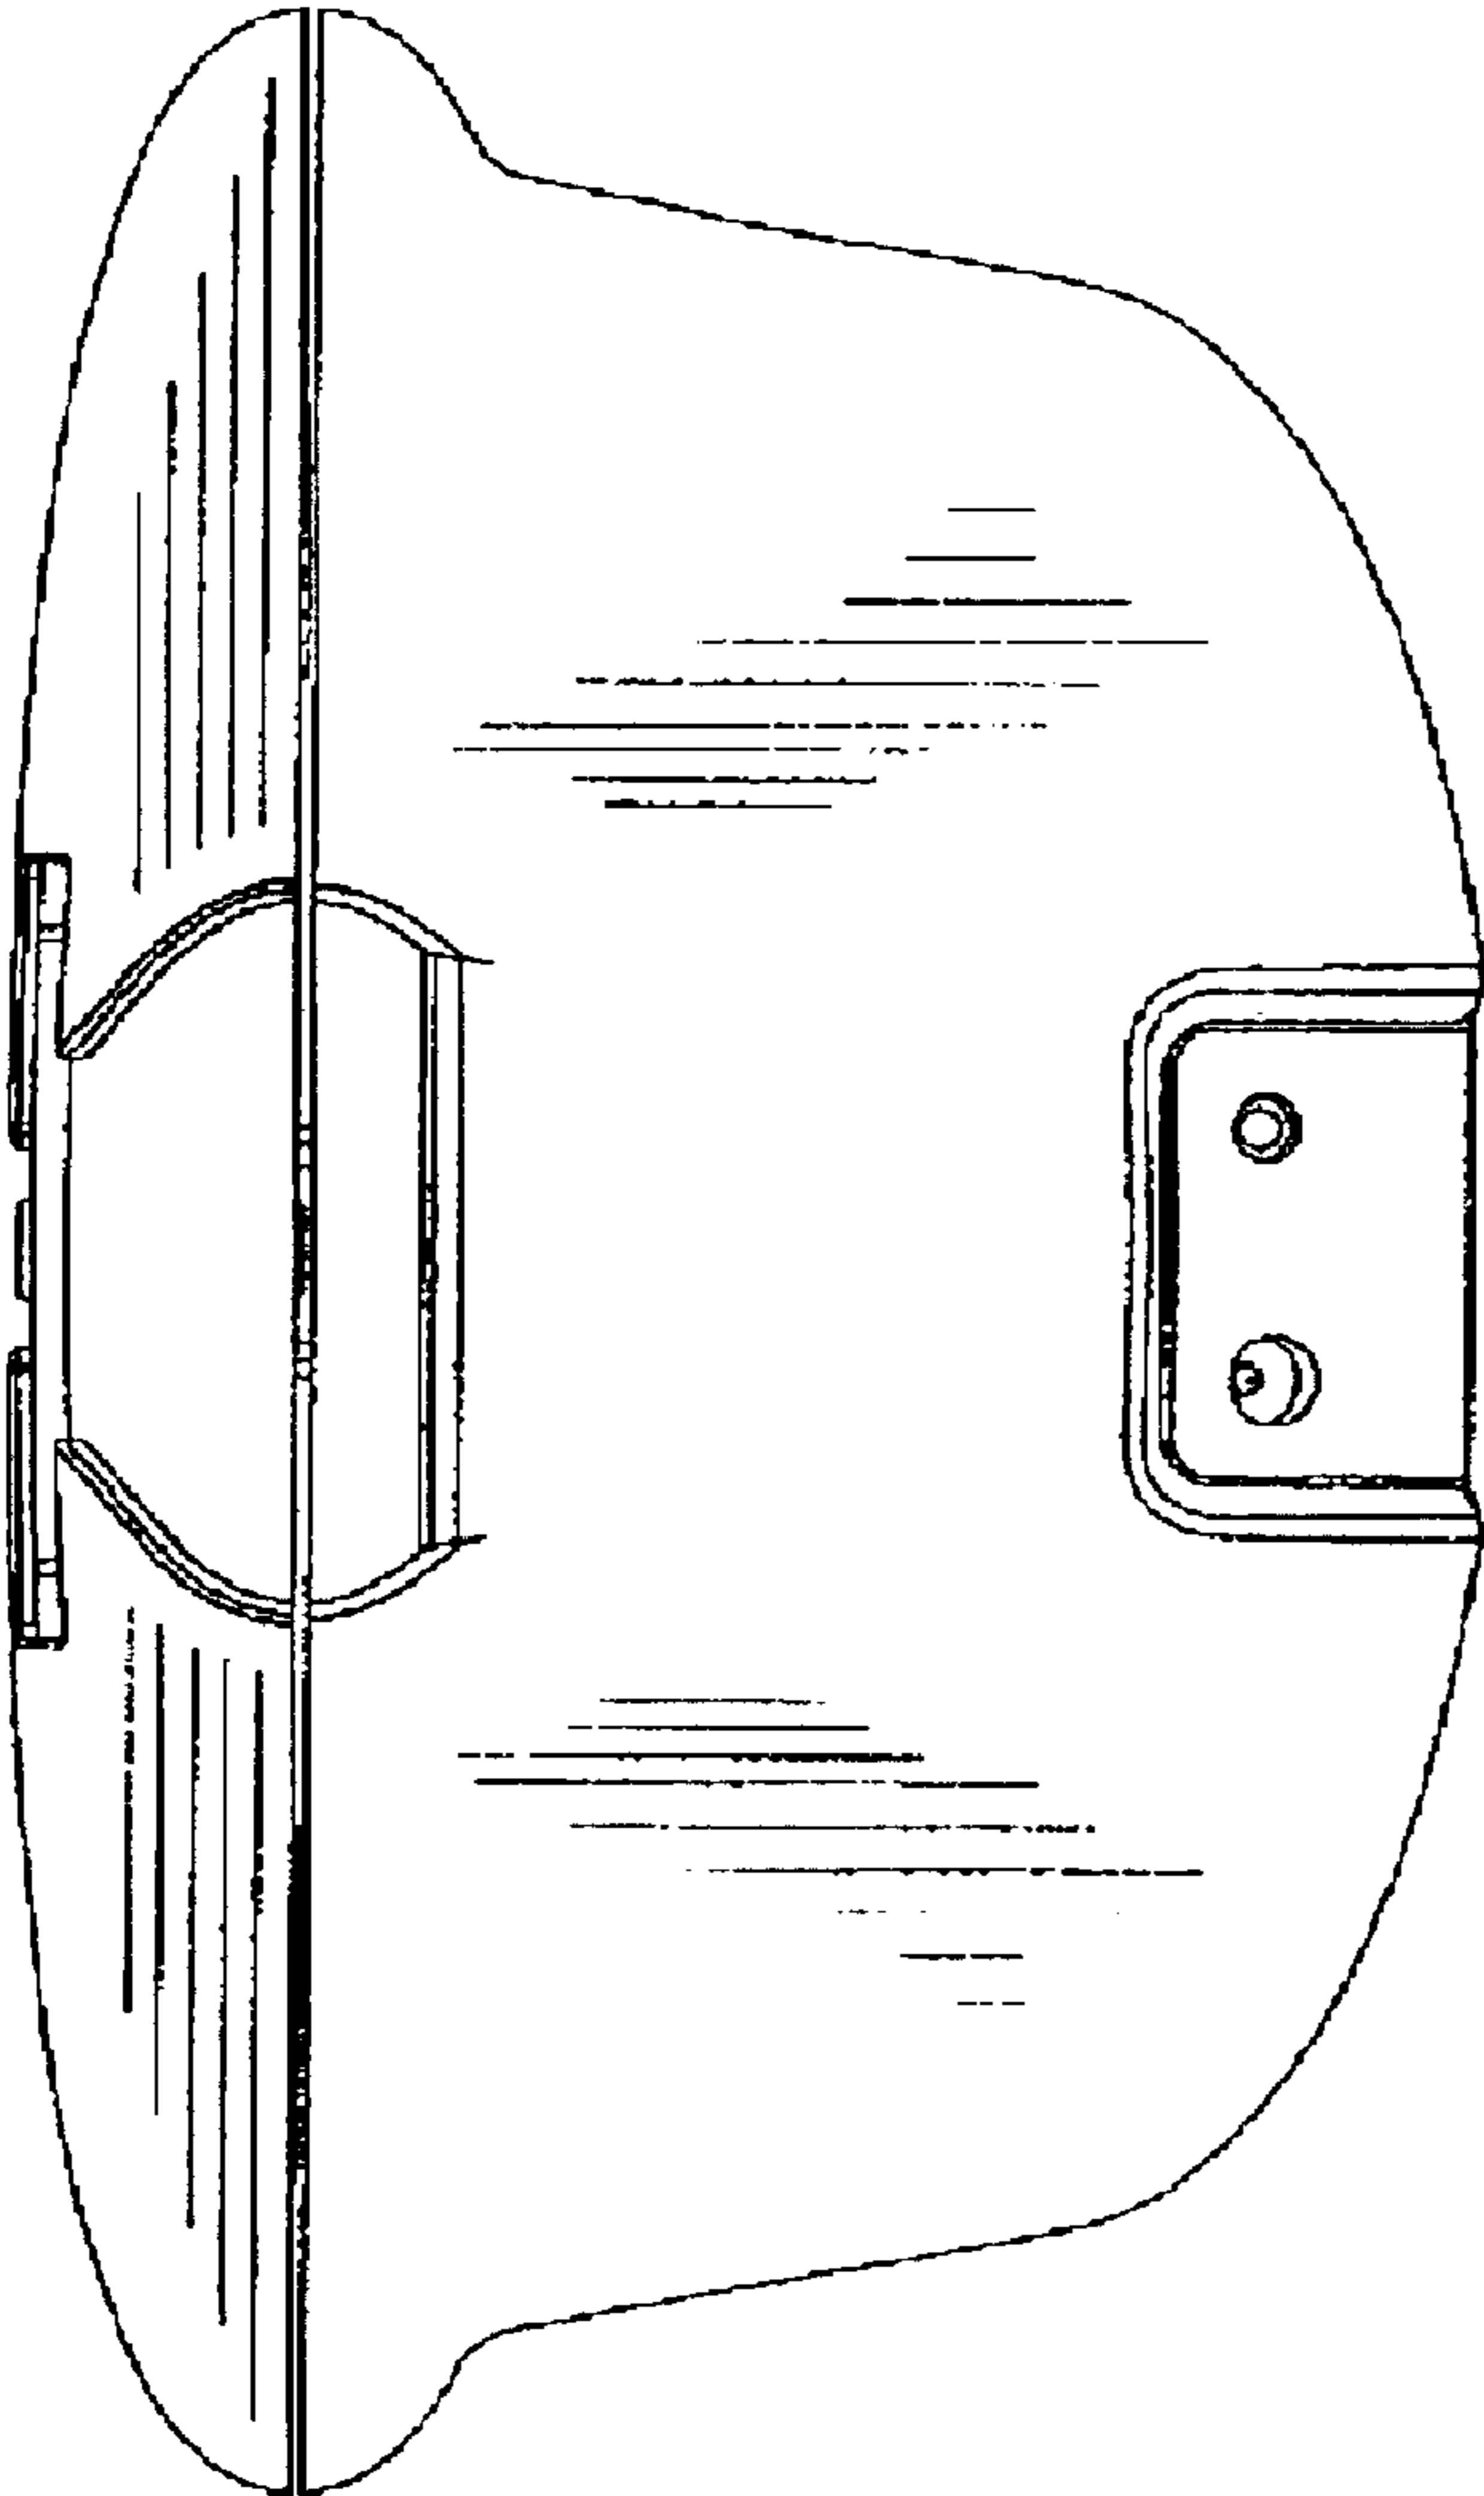


FIG. 7



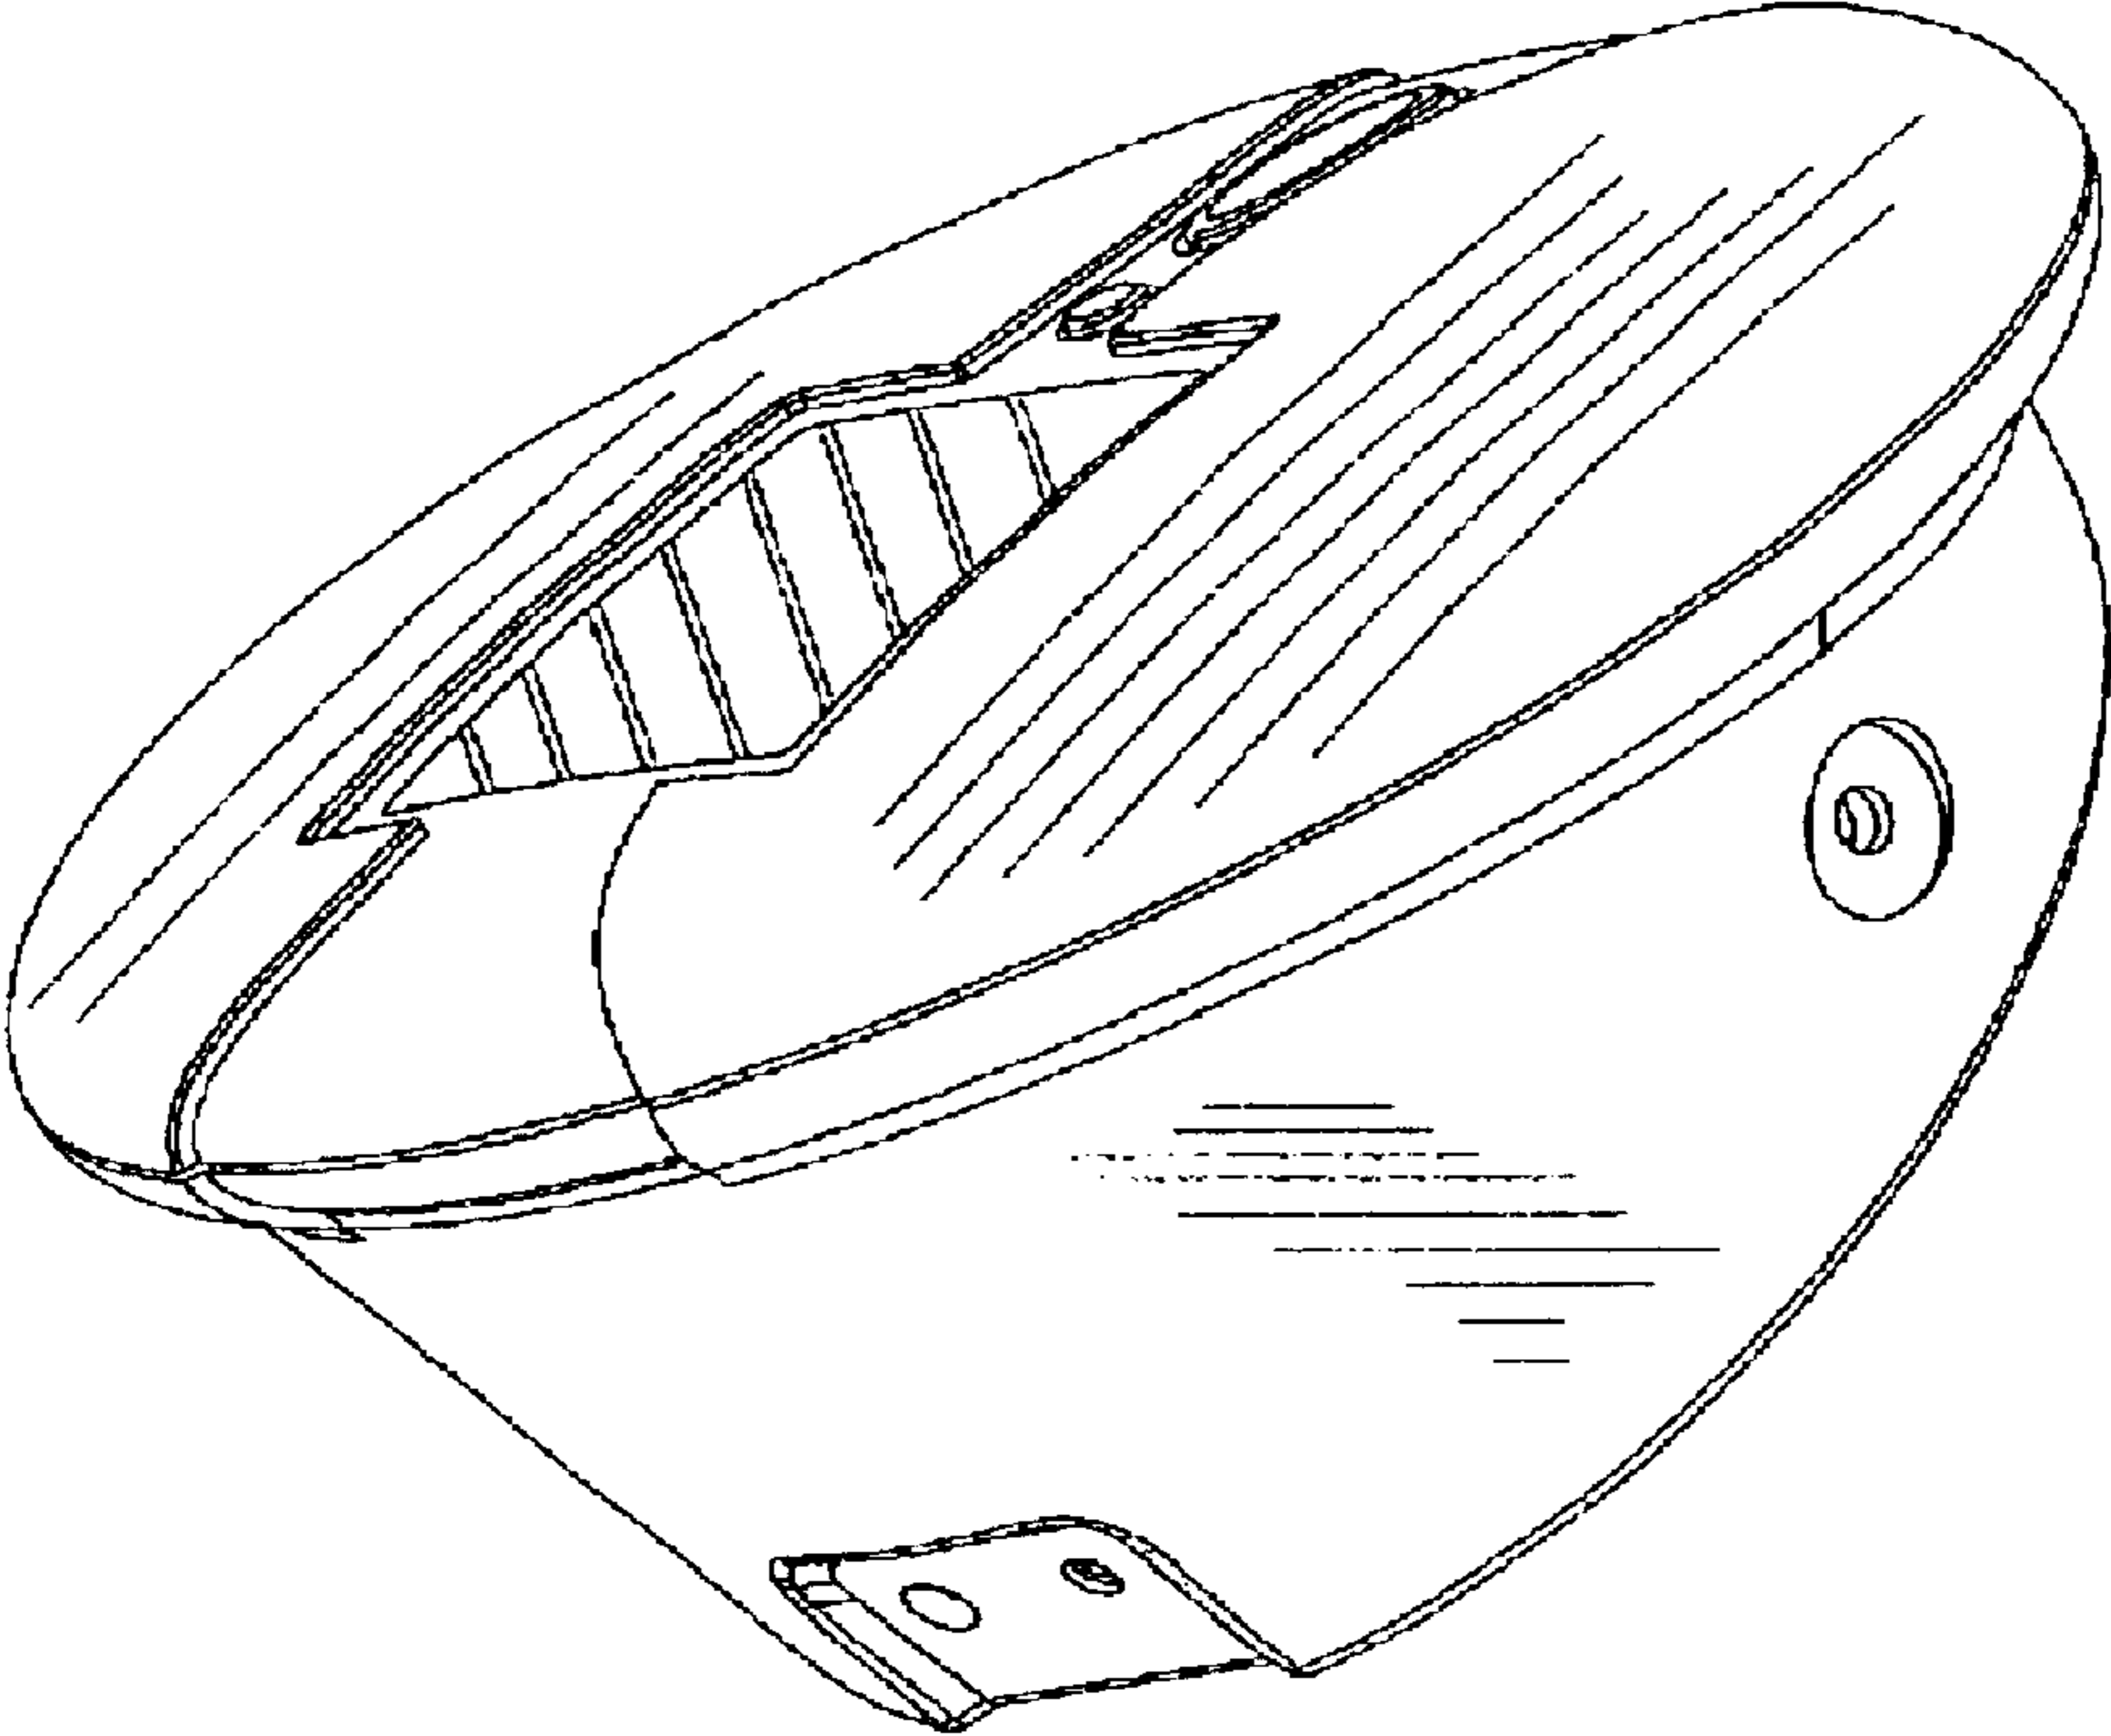


FIG. 8