



US00D531319S

(12) **United States Design Patent** (10) **Patent No.:** **US D531,319 S**
Schein et al. (45) **Date of Patent:** **** Oct. 31, 2006**

(54) **TUBE FRAME FOR ORGAN TRANSPORTER**

WO WO 96/29865 10/1996

WO WO 96/30111 10/1996

(75) Inventors: **Douglas A. Schein**, Des Plaines, IL
(US); **Lee W. Travis**, Littleton, CO
(US)

WO WO 97/43899 11/1997

WO WO 97/45527 12/1997

WO WO 99/15011 4/1999

WO WO 00/18226 4/2000

(73) Assignee: **Organ Recovery Systems**, Des Plaines,
IL (US)

OTHER PUBLICATIONS

(**) Term: **14 Years**“Organ Preservation”, J.H. Southard, Ph.D. and F.O. Belzer,
M.D., *Principles of Organ Transplantation*, Chapter 10, pp.
194–215, 1989.(21) Appl. No.: **29/179,034**“Organko Servierungsmachine OKM 82”, Von Dietmer
Scholz et al., East German Article, 1983.(22) Filed: **Apr. 4, 2003**

(Continued)

(51) **LOC (8) Cl.** **24-02**(52) **U.S. Cl.** **D24/216; D24/107**(58) **Field of Classification Search** D24/111,
D24/216, 108, 133, 107, 121, 128; 435/1.2,
435/284.1, 307.1, 303.1; 62/306, 78, 371;
128/DIG. 26; 604/19

See application file for complete search history.

Primary Examiner—Ian Simmons*Assistant Examiner*—Christopher Lee(74) *Attorney, Agent, or Firm*—Oliff & Berridge, PLC

(57)

CLAIMThe ornamental design for a tube frame for organ trans-
porter, as shown and described.

(56)

References Cited

U.S. PATENT DOCUMENTS

3,406,531	A	10/1968	Swenson et al.
3,545,221	A	12/1970	Swenson et al.
3,607,646	A	9/1971	de Roissart
3,654,085	A	4/1972	Norr et al.
3,660,241	A	5/1972	Michielsen
3,777,507	A	12/1973	Burton et al.

(Continued)

FOREIGN PATENT DOCUMENTS

DE	38 08 942	1/1989
EP	0 096 997	12/1983
EP	0 376 763 A2	7/1990
GB	1442356 A	7/1976
JP	2-258701	10/1990
SU	760972	9/1980
WO	WO 91/03934	4/1991
WO	WO 91/14364	10/1991
WO	93/00808	1/1993
WO	96/05727	2/1996
WO	WO 96/13288	5/1996

DESCRIPTIONFIG. 1 is a perspective view of a tube frame for organ
transporter made of an opaque material;

FIG. 2 is a top view thereof;

FIG. 3 is a bottom view thereof;

FIG. 4 is a front view thereof;

FIG. 5 is a rear view thereof;

FIG. 6 is a left-side view thereof; and

FIG. 7 is a right-side view thereof.

FIG. 8 is a perspective view of the tube frame for organ
transporter made of a transparent material;

FIG. 9 is a top view thereof;

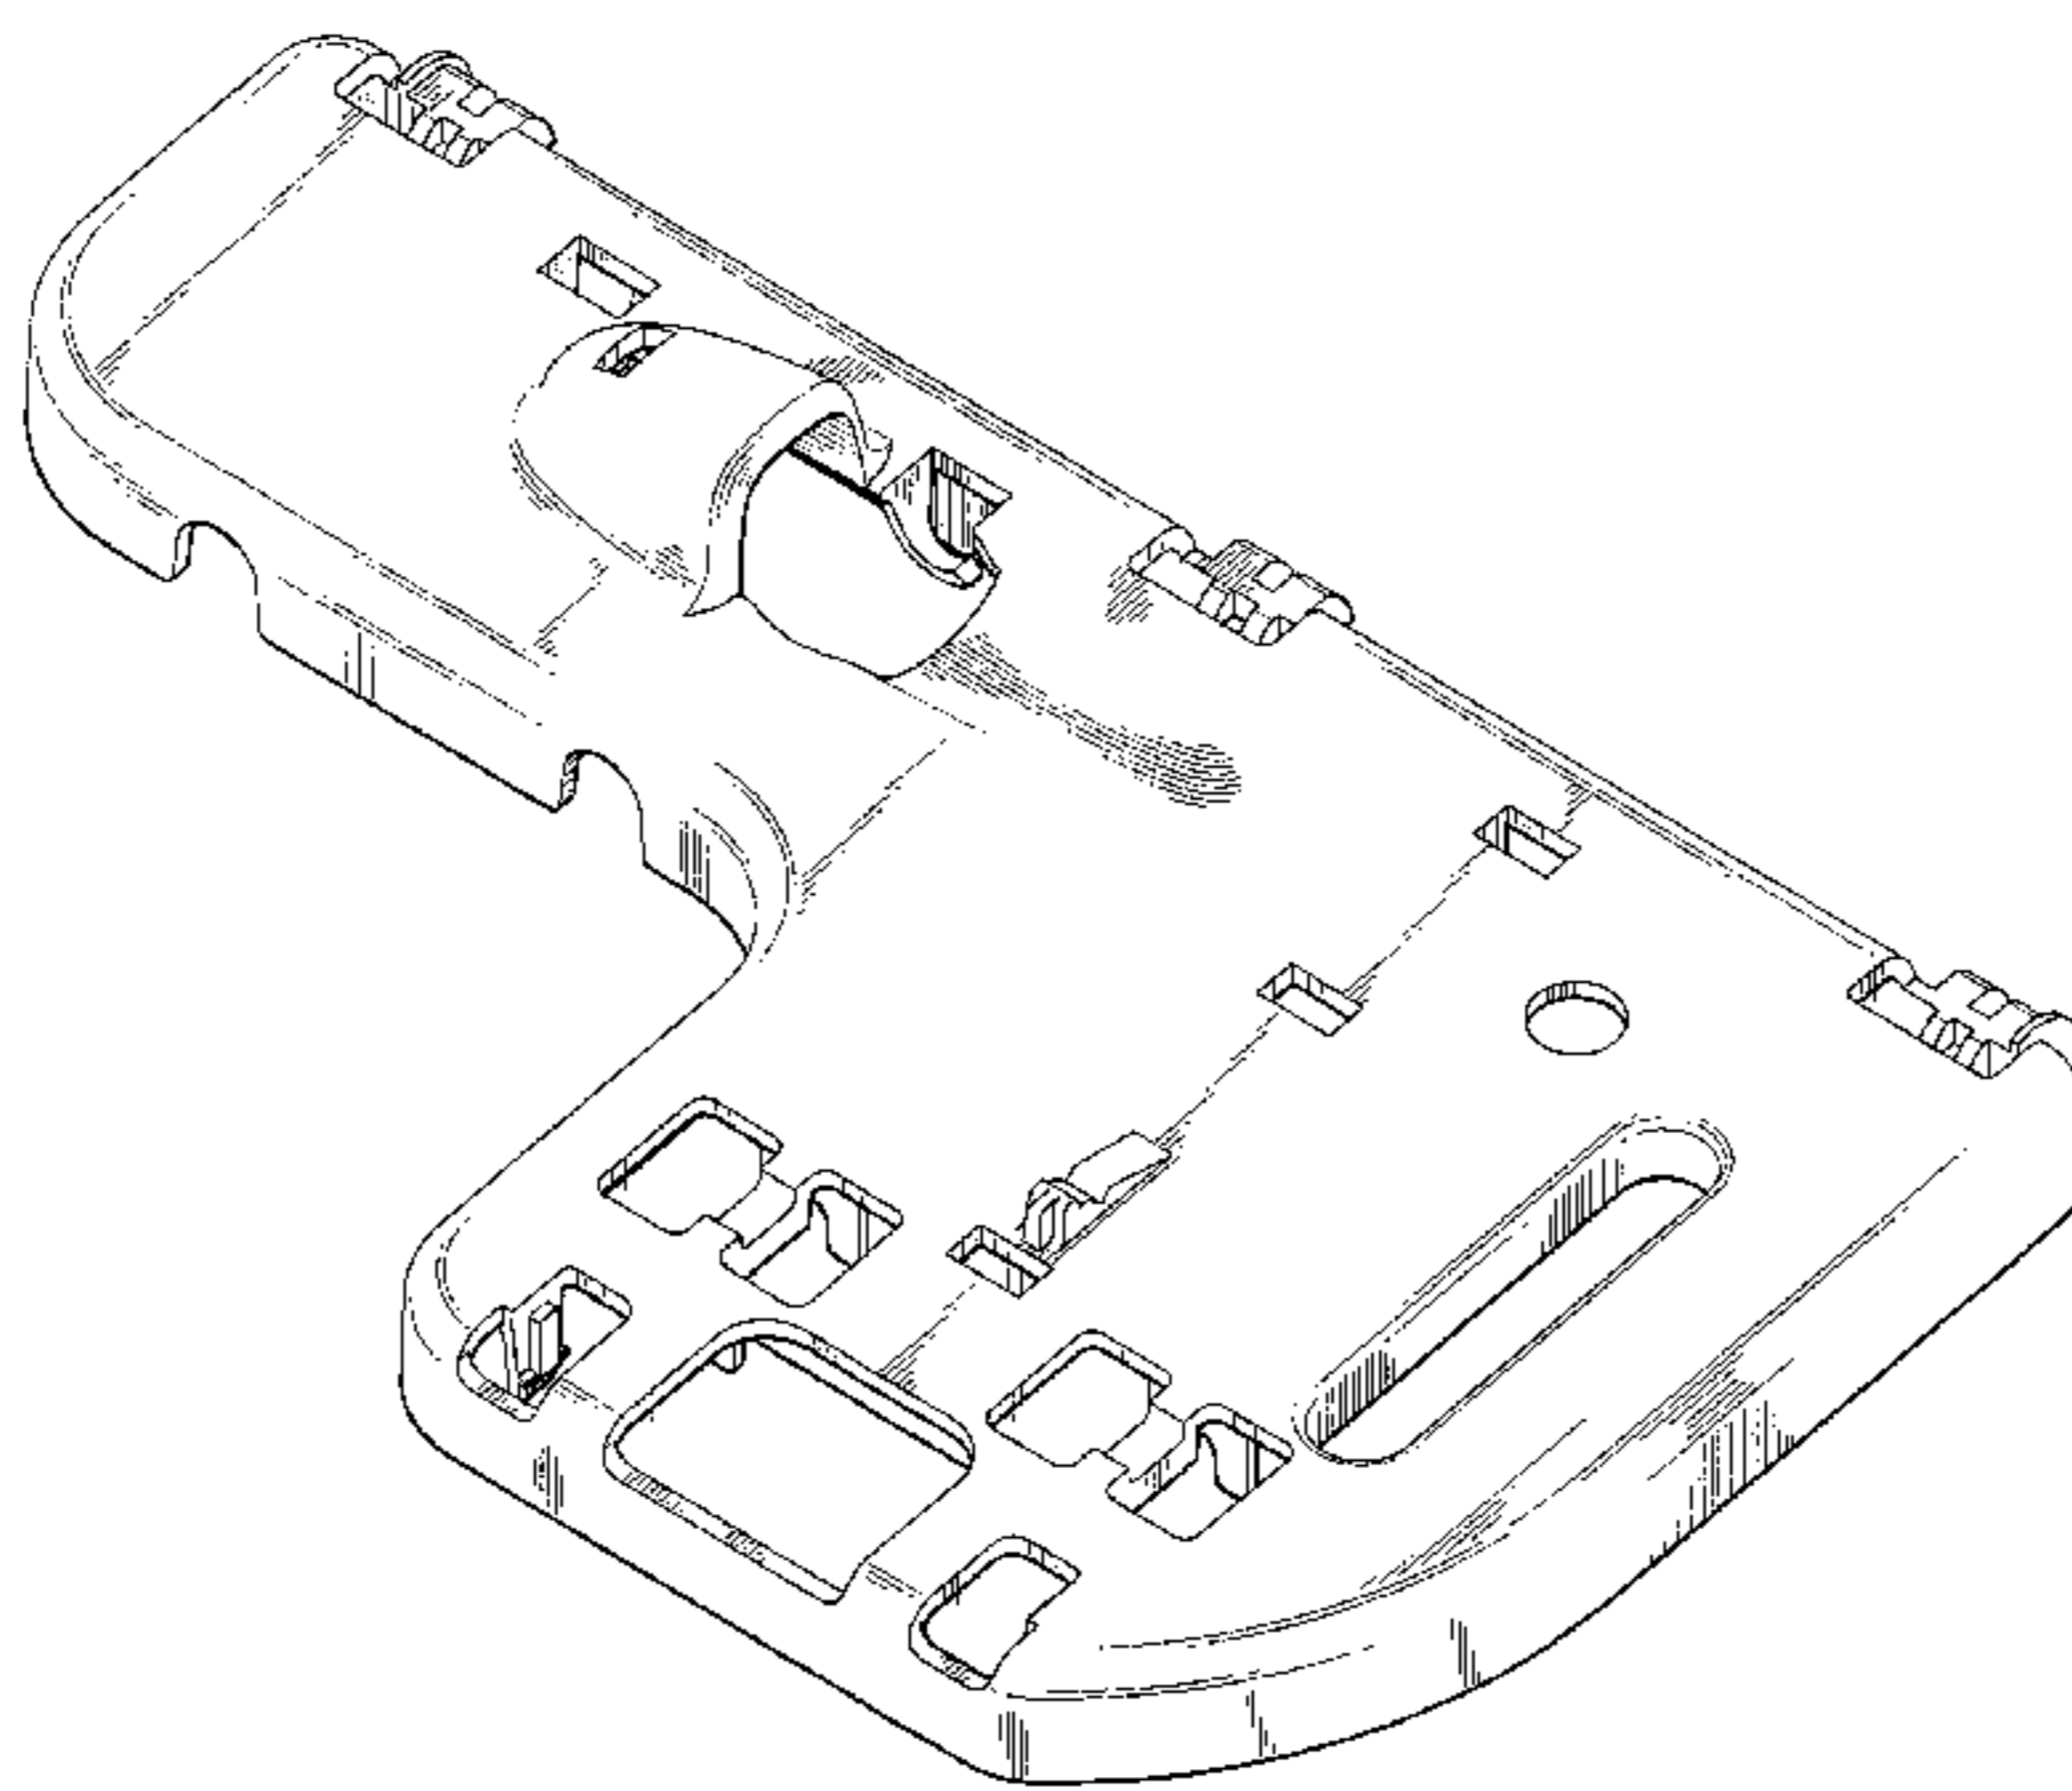
FIG. 10 is a bottom view thereof;

FIG. 11 is a front view thereof;

FIG. 12 is a rear view thereof;

FIG. 13 is a left-side view thereof; and,

FIG. 14 is a right-side view thereof.

The broken line showing is for illustrative purposes only and
does not form part of the claimed design.**1 Claim, 10 Drawing Sheets**

U.S. PATENT DOCUMENTS

3,810,367 A 5/1974 Peterson
 3,843,455 A 10/1974 Bier
 3,877,843 A 4/1975 Fischel
 3,881,990 A 5/1975 Burton et al.
 3,914,954 A 10/1975 Doerig
 3,935,065 A 1/1976 Doerig
 3,995,444 A 12/1976 Clark et al.
 4,186,565 A 2/1980 Toledo-Pereyra
 4,242,883 A 1/1981 Toledo-Pereyra
 4,462,215 A 7/1984 Kuraoka et al.
 4,471,629 A 9/1984 Toledo-Pereyra
 4,473,637 A 9/1984 Guibert
 4,474,016 A 10/1984 Winchell
 4,494,385 A 1/1985 Kuraoka et al.
 4,502,295 A 3/1985 Toledo-Pereyra
 4,723,974 A 2/1988 Ammerman
 4,745,759 A 5/1988 Bauer et al.
 4,766,740 A 8/1988 Bradley et al.
 4,837,390 A 6/1989 Reneau
 4,951,482 A 8/1990 Gilbert
 4,958,506 A 9/1990 Guilhem et al.
 5,141,847 A 8/1992 Sugimachi et al.
 5,157,930 A 10/1992 McGhee et al.
 5,217,860 A 6/1993 Fahy et al.
 5,285,657 A 2/1994 Bacchi et al.
 5,326,706 A 7/1994 Yland et al.
 D350,823 S * 9/1994 Lanigan D24/111
 5,356,771 A 10/1994 O'Dell
 5,362,622 A 11/1994 O'Dell et al.
 5,383,854 A 1/1995 Safar et al.
 5,385,821 A 1/1995 O'Dell et al.
 D357,312 S * 4/1995 Riquier et al. D24/111
 5,434,045 A 7/1995 Jost

5,472,876 A 12/1995 Fahy
 D367,323 S * 2/1996 Carr et al. D24/111
 5,586,438 A 12/1996 Fahy
 5,681,740 A 10/1997 Messier et al.
 5,723,282 A 3/1998 Fahy et al.
 5,821,045 A 10/1998 Fahy et al.
 5,856,081 A 1/1999 Fahy
 5,965,433 A 10/1999 Gardetto et al.
 6,046,046 A 4/2000 Hassanein
 D477,867 S * 7/2003 O'Mahony et al. D24/108
 6,673,594 B1 * 1/2004 Owen et al. 435/284.1
 2004/0235142 A1 * 11/2004 Schein et al. 435/284.1

OTHER PUBLICATIONS

“Preservation of Cerebral Function During Circulatory Arrest and Resuscitation: Hypothermic Protective Considerations”, Robert J. White, *Resuscitation*, vol. I, pp. 107–115, 1972.
 “Storage and Transport of Heart and Heart–Lung Donor Organs With Inflatable Cushions and Eutectoid Cooling”, D.R. Wheeldon et al., *The Journal of Heart Transplantation*, vol. 7, pp. 265–268, 1988.
 “MOX®–100 Renal Preservation System”, Waters Instruments Medical Group, pp. 2–7, 1992.
 “Organ Perfusion Systems: An Evaluation Criteria”, Fereydoon Sadri, Ph.D., *T.O.P.S. Medical Corporation*, pp. 1–8, 1987.
 Gauke Kootstra et al, “A New Device Towards Intermediate Term Kidney Preservation—An Experimental Study,” 1980, pp. 86–89.

* cited by examiner

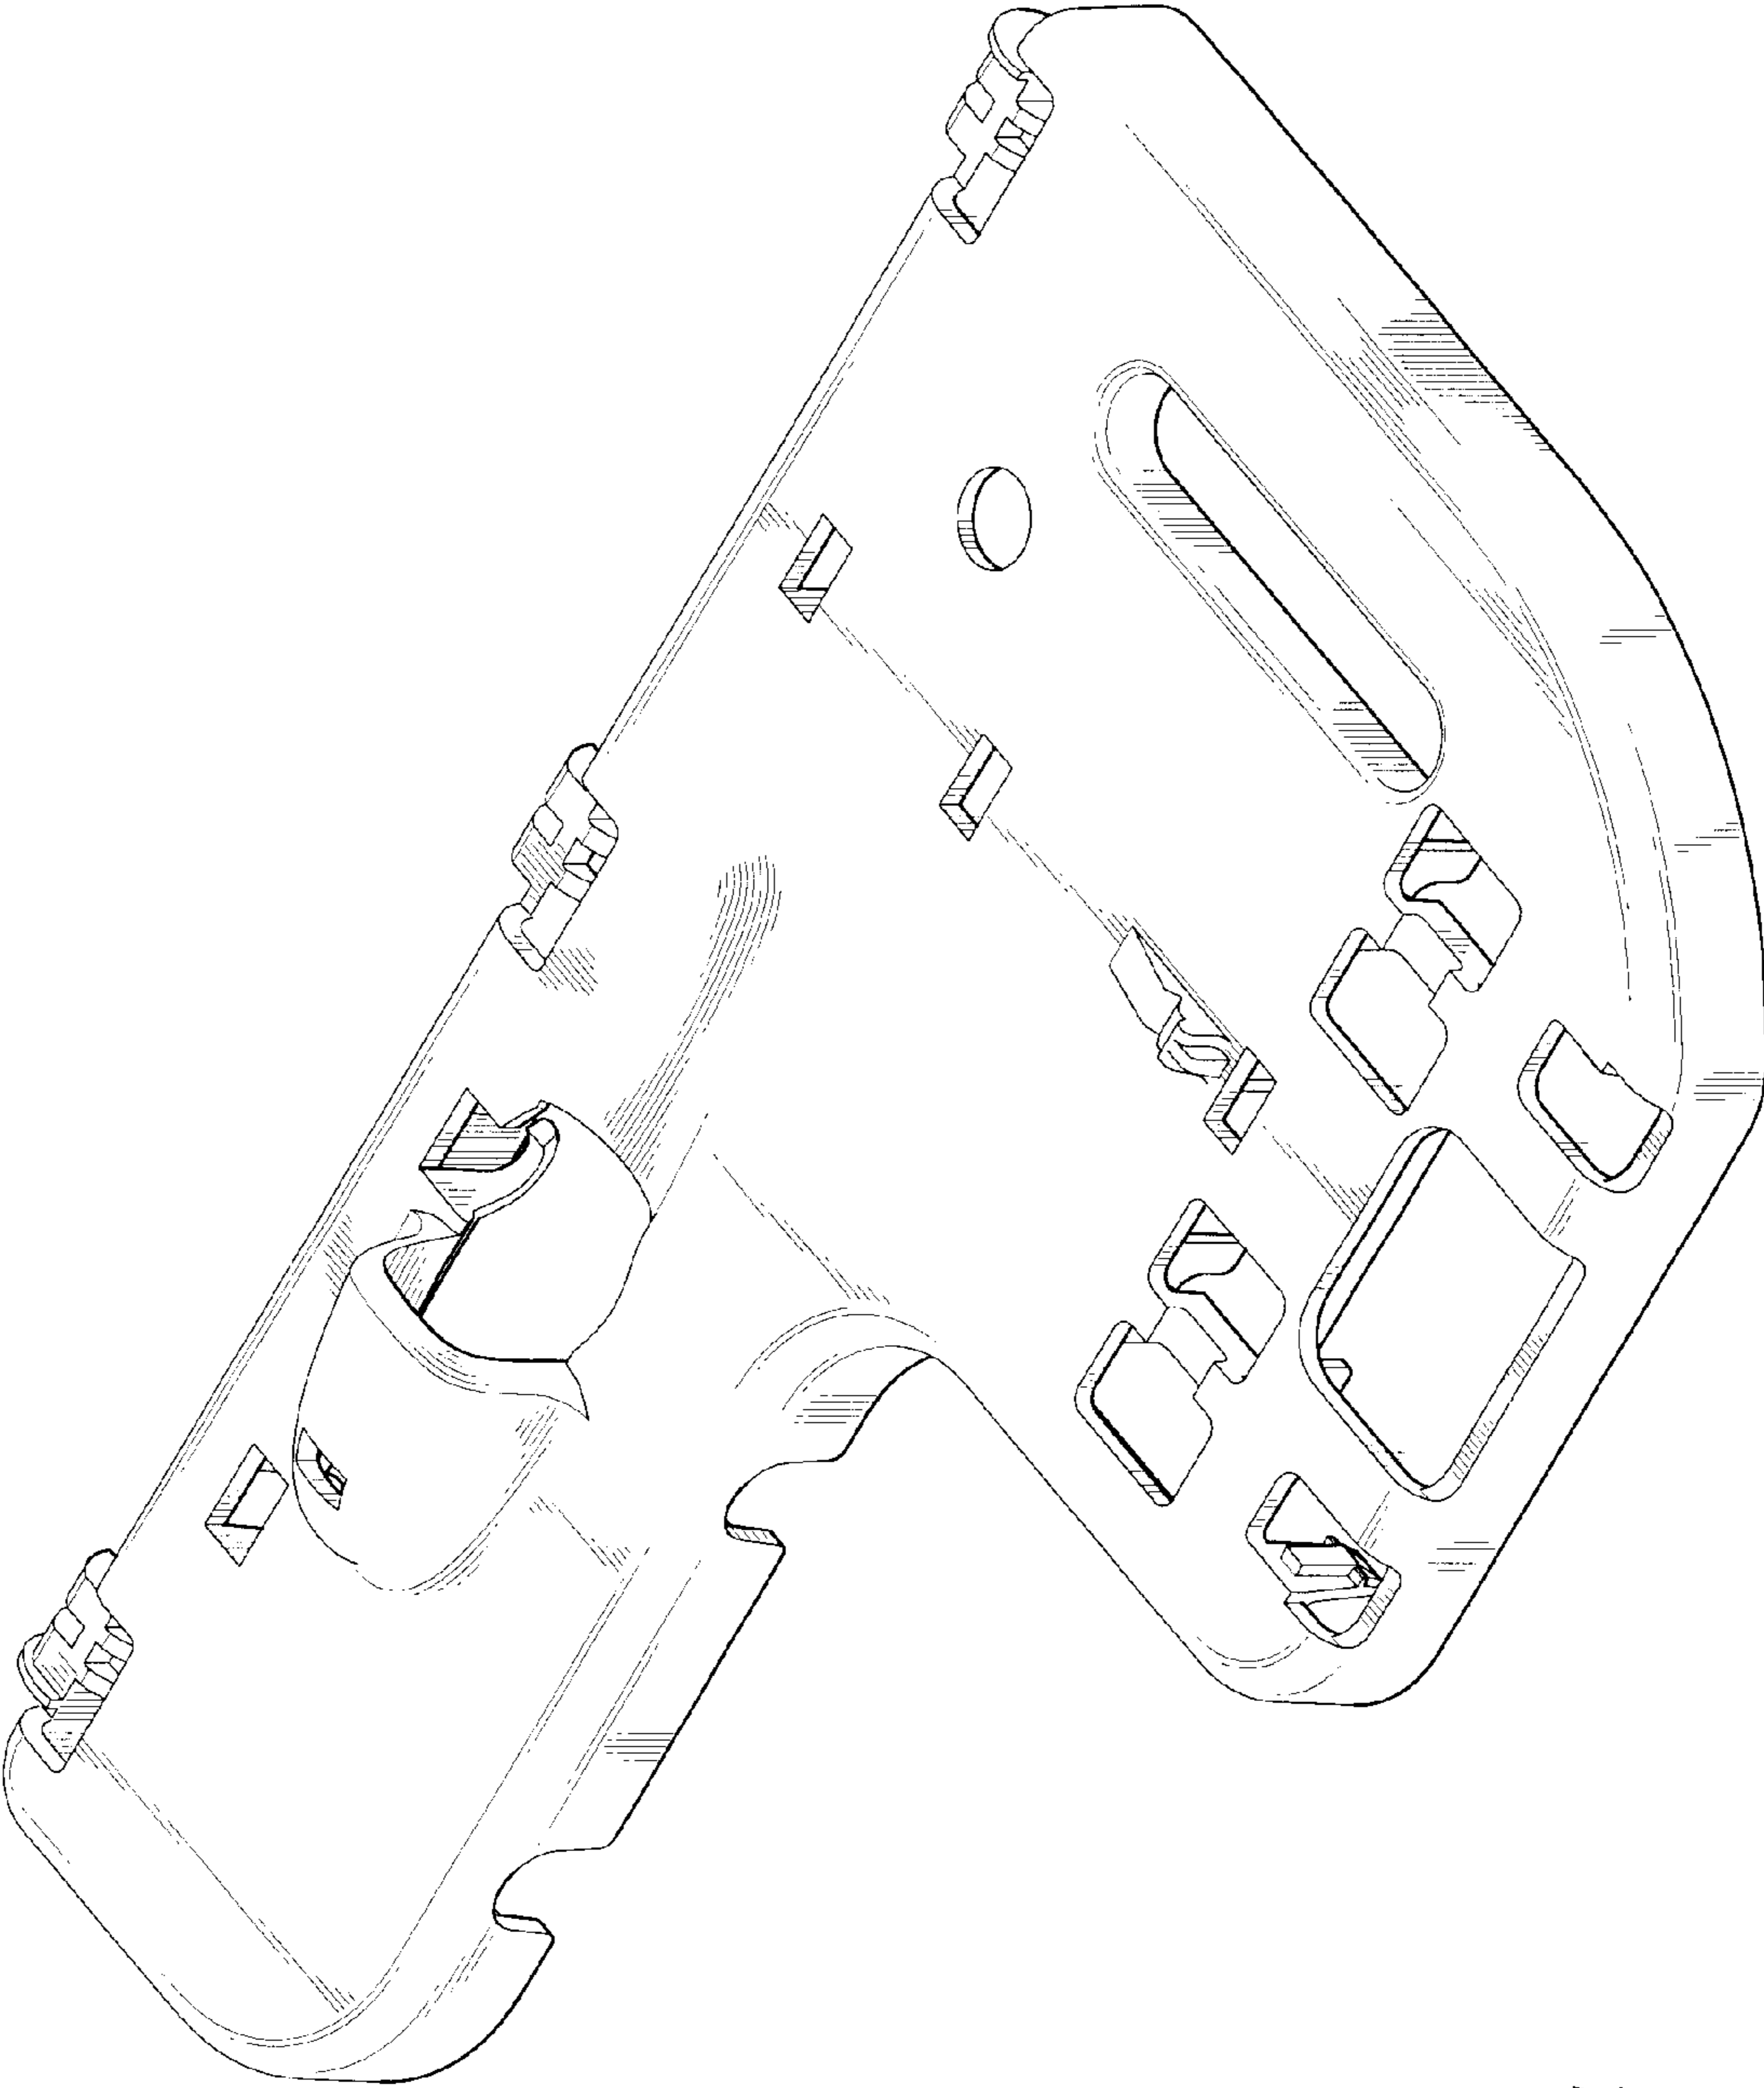


Fig. 1

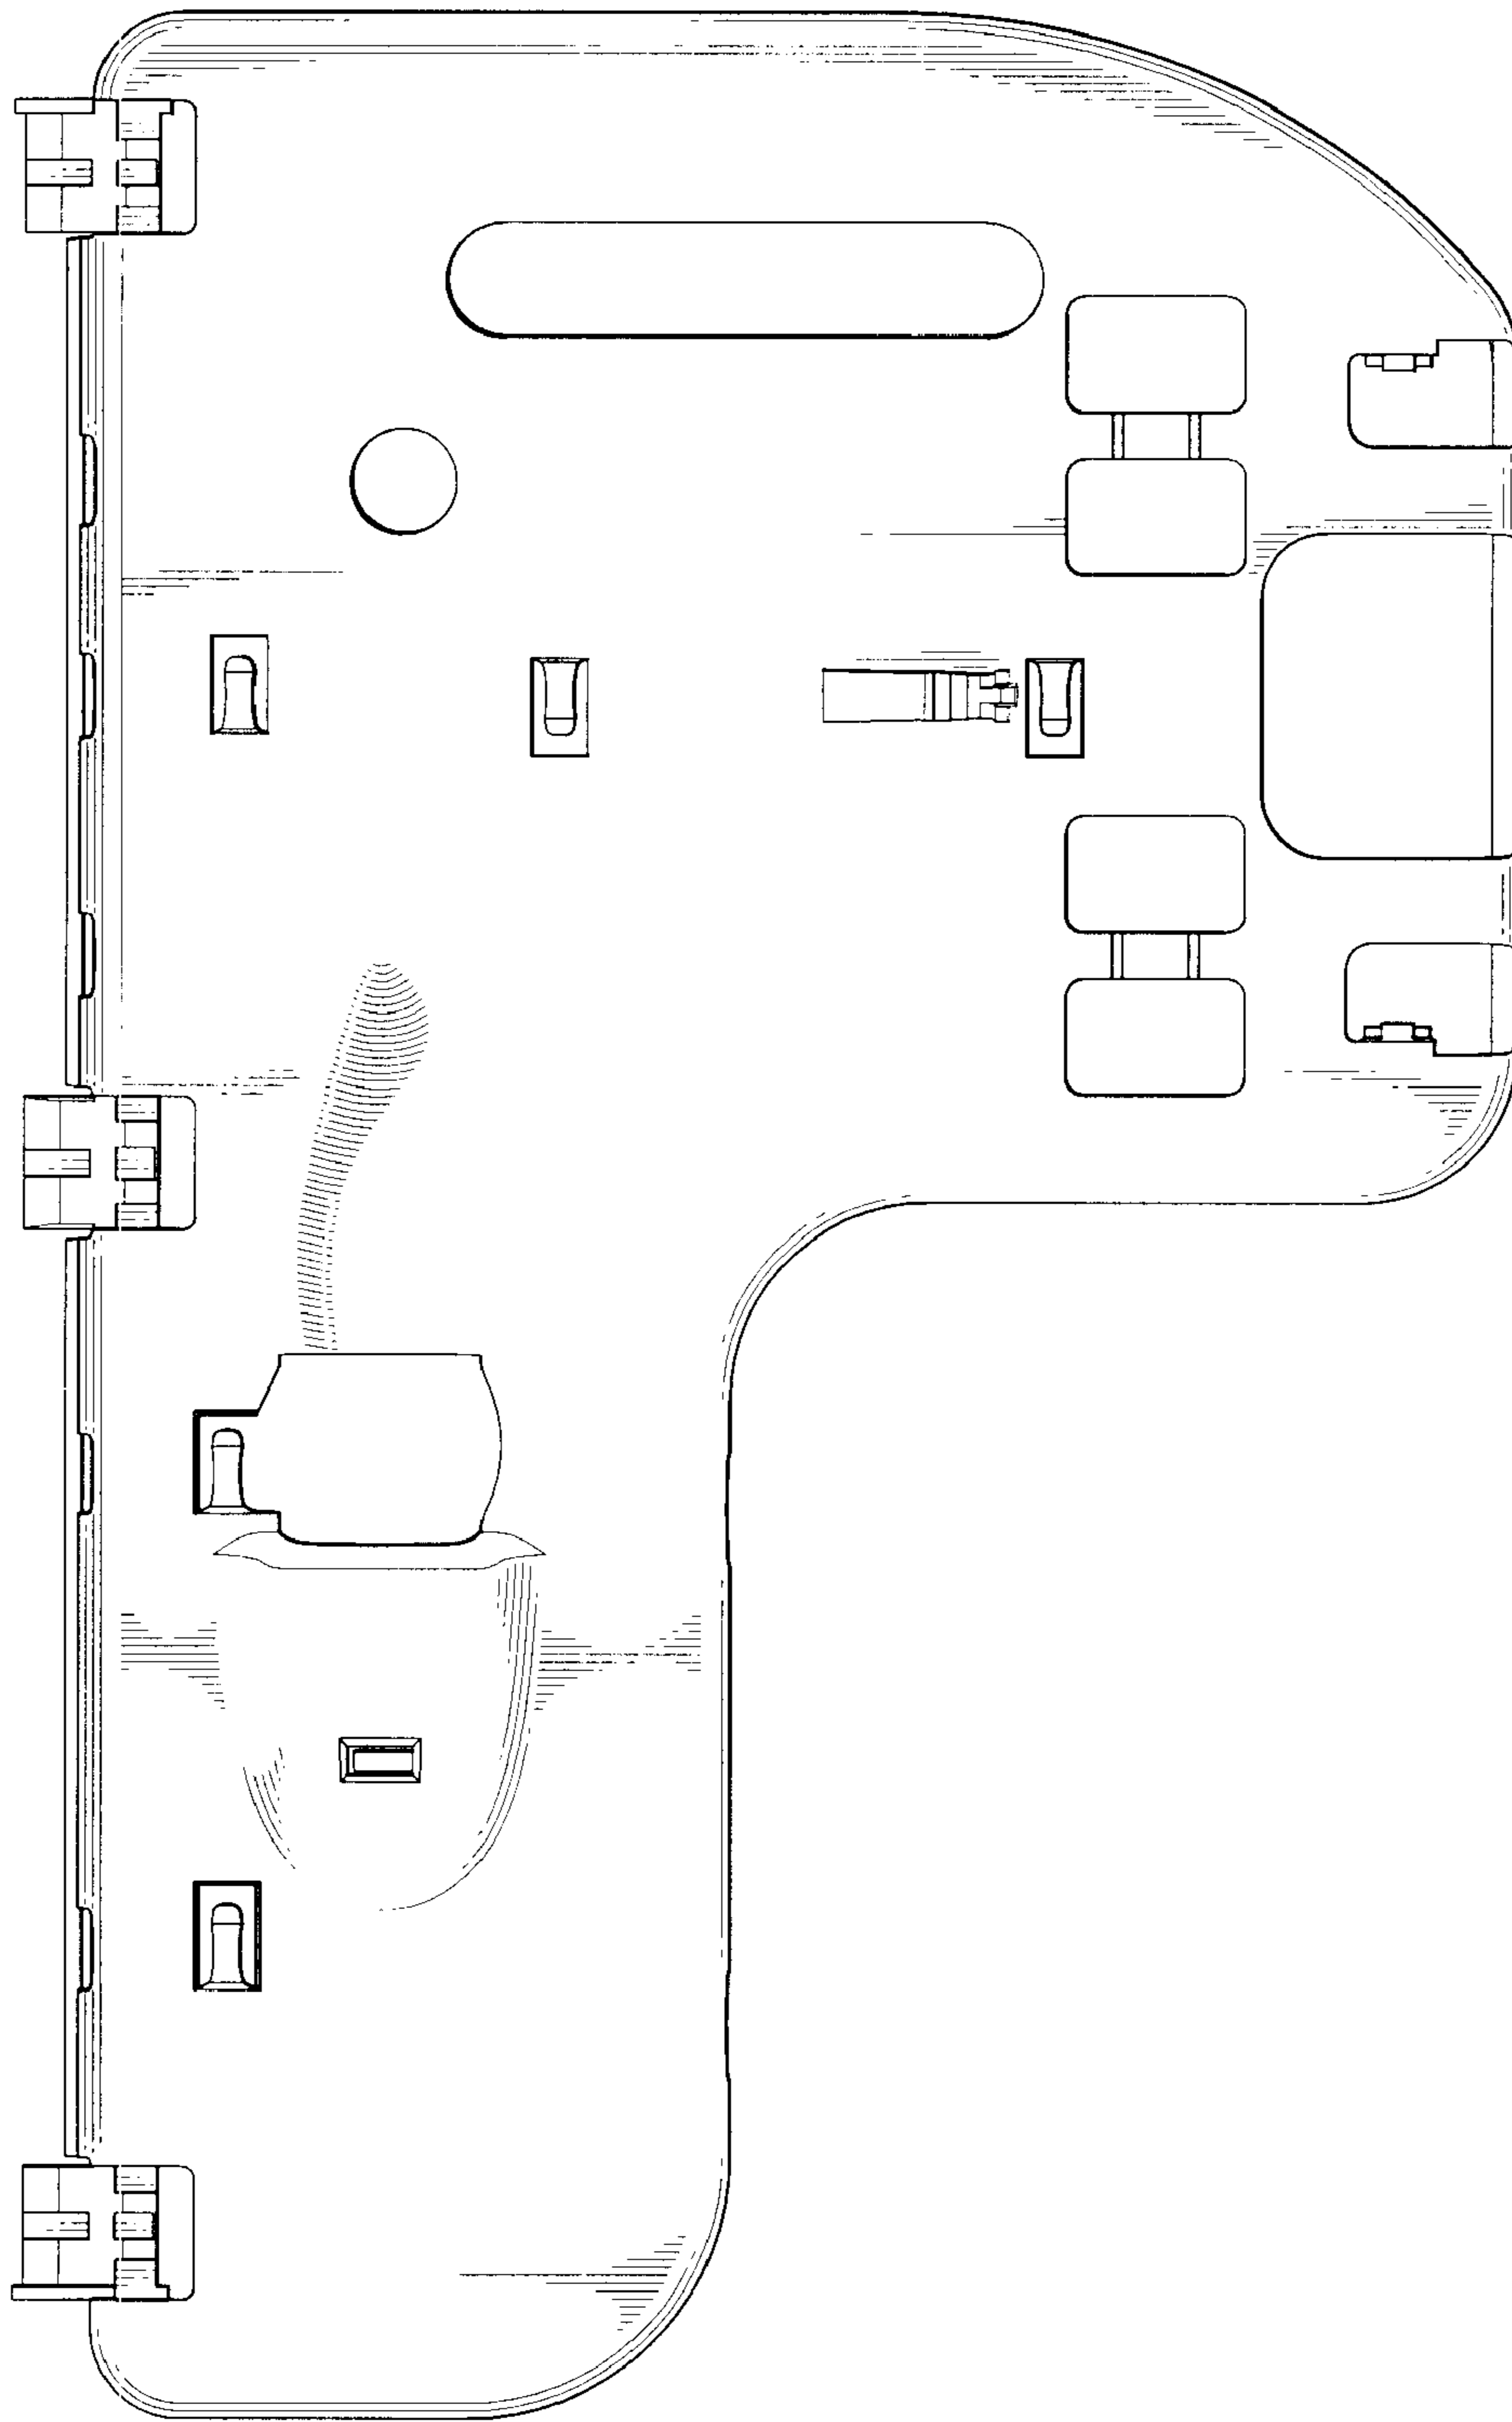


Fig. 2

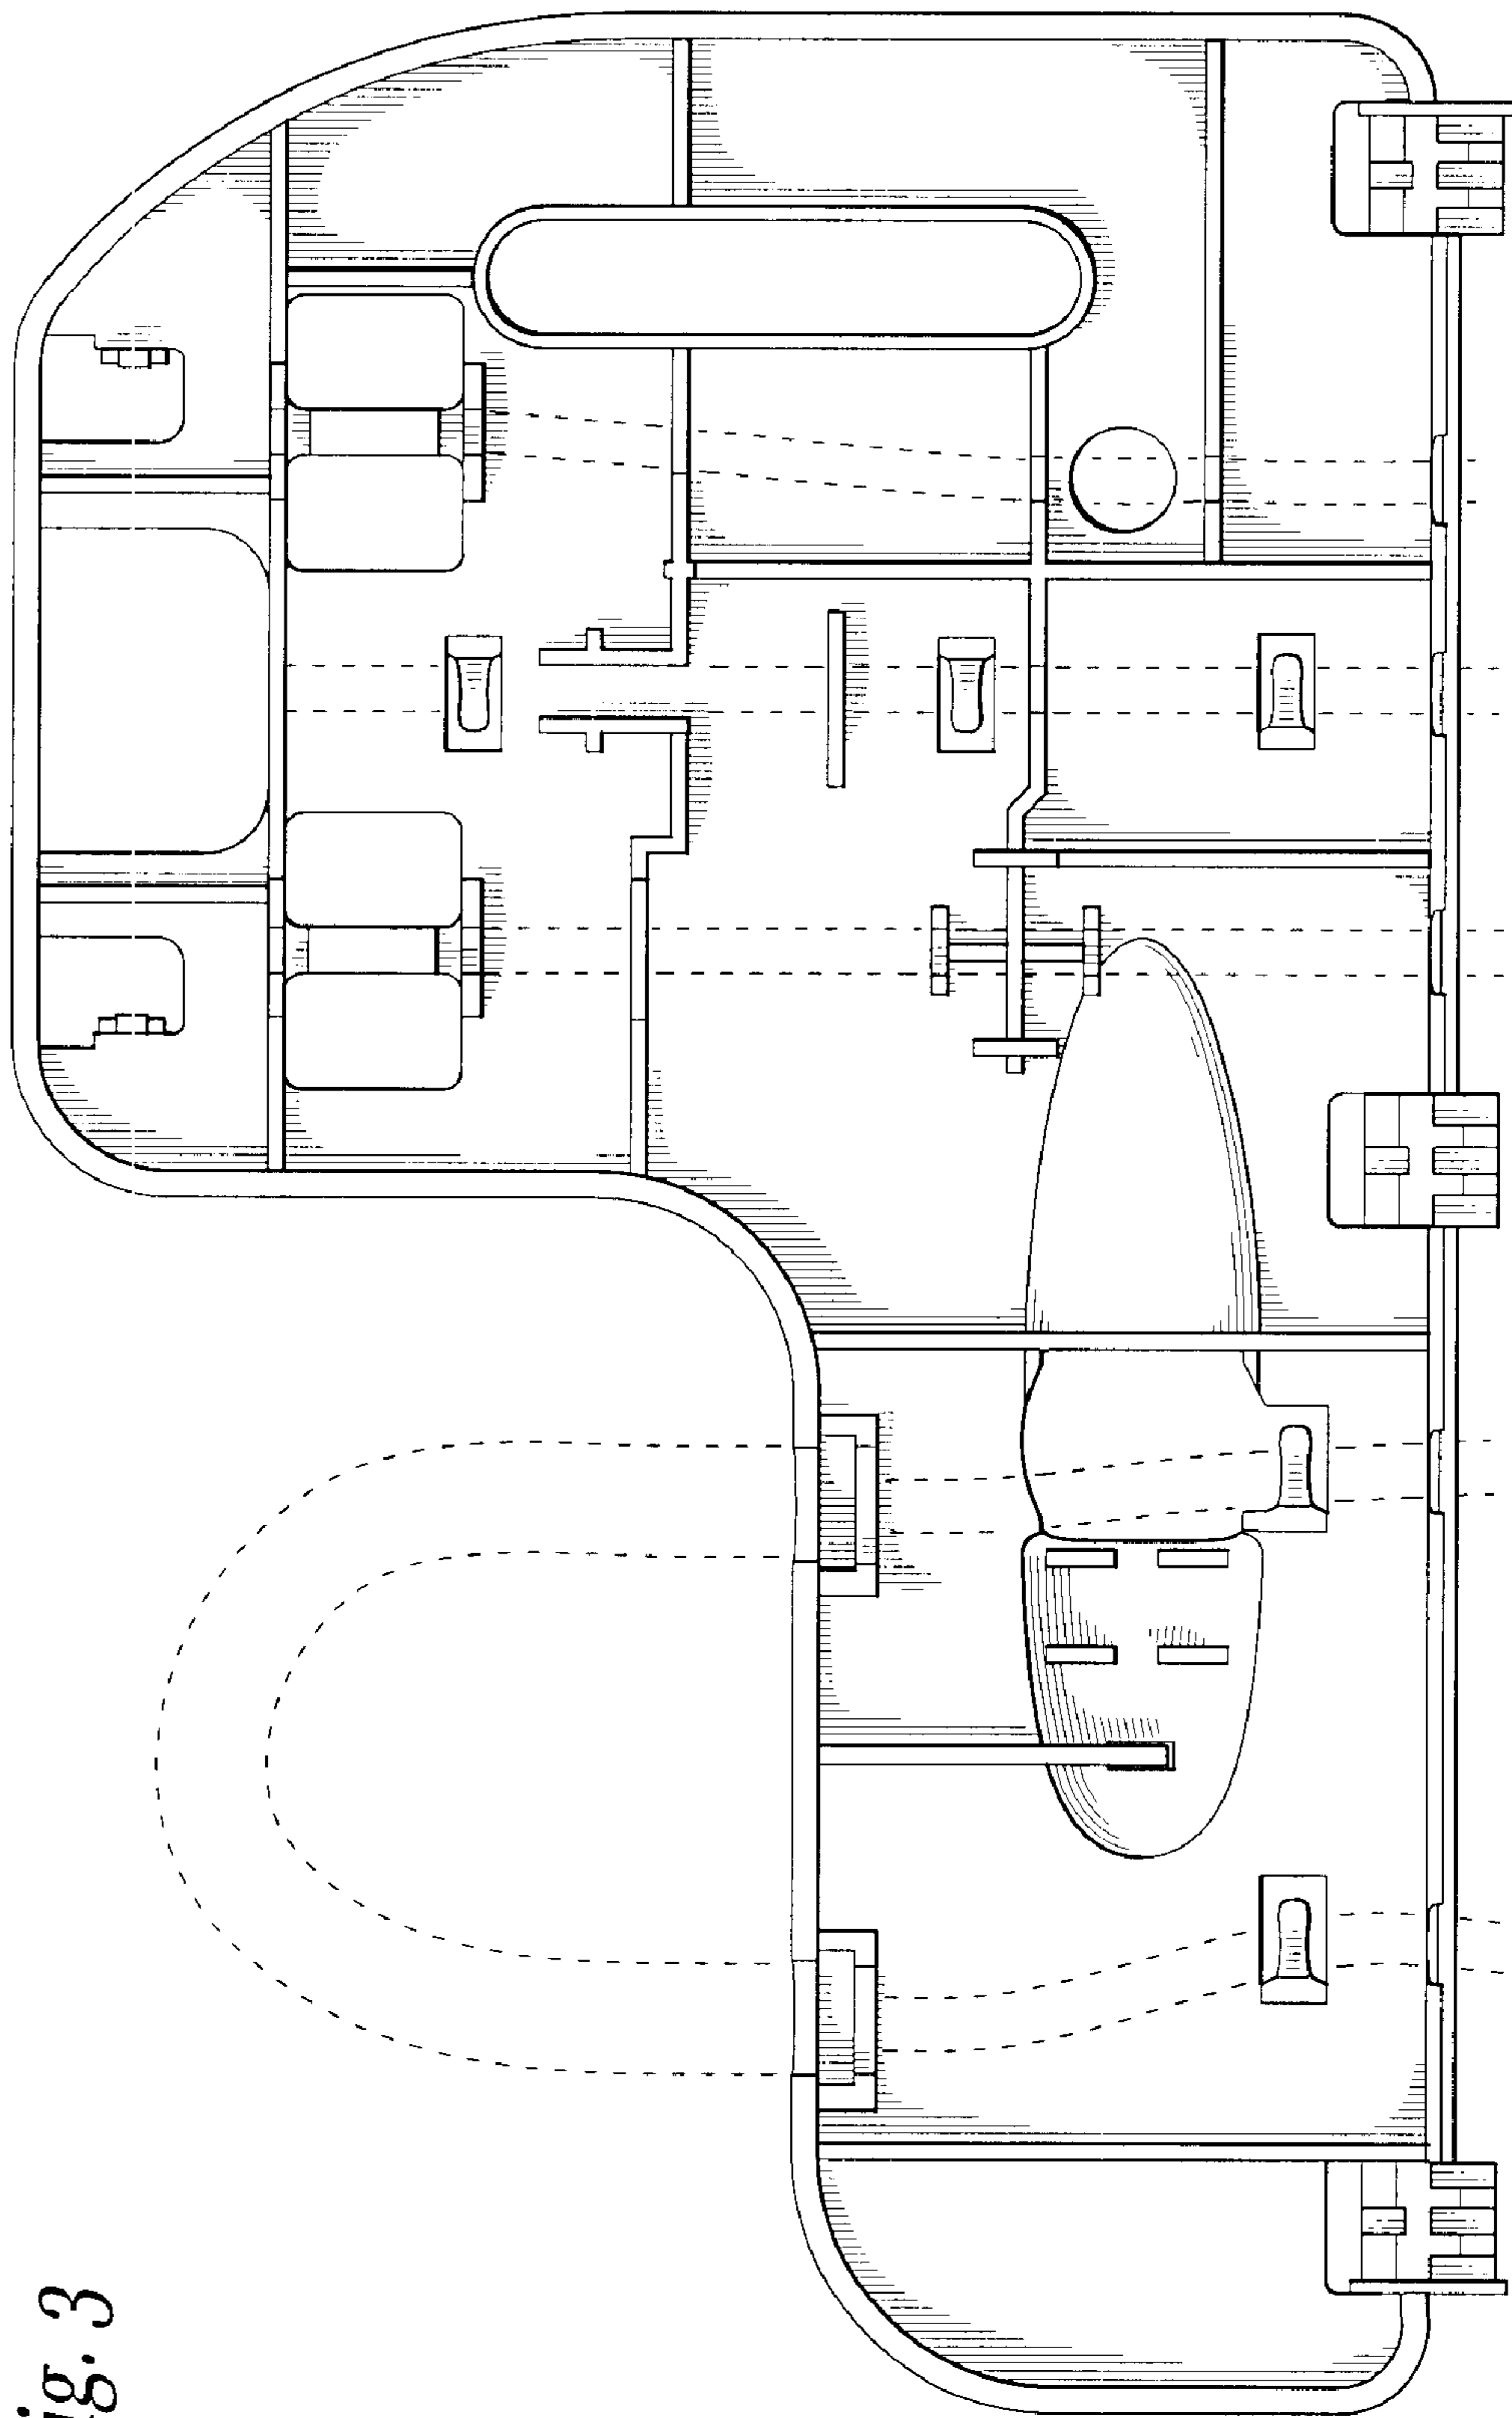


Fig. 3

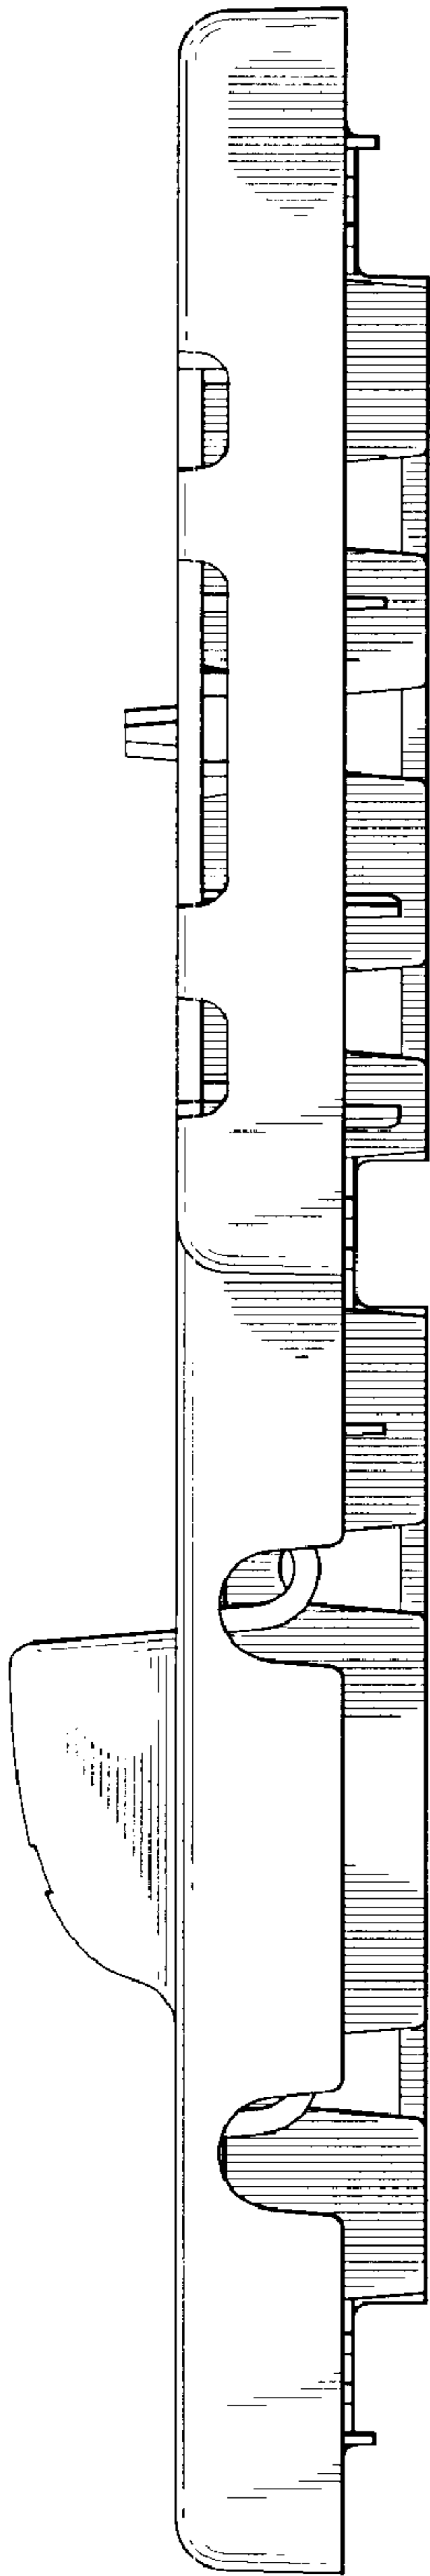


Fig. 4

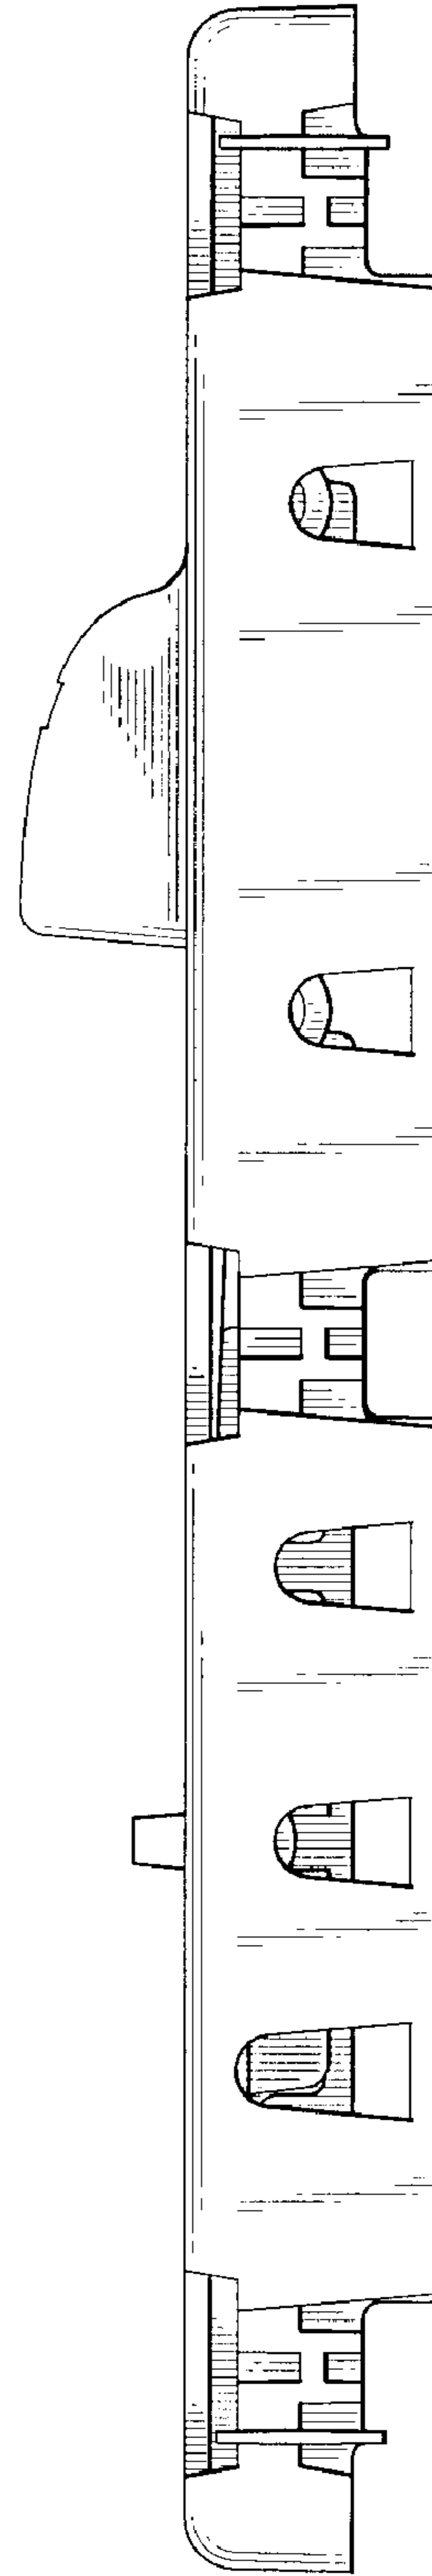


Fig. 5

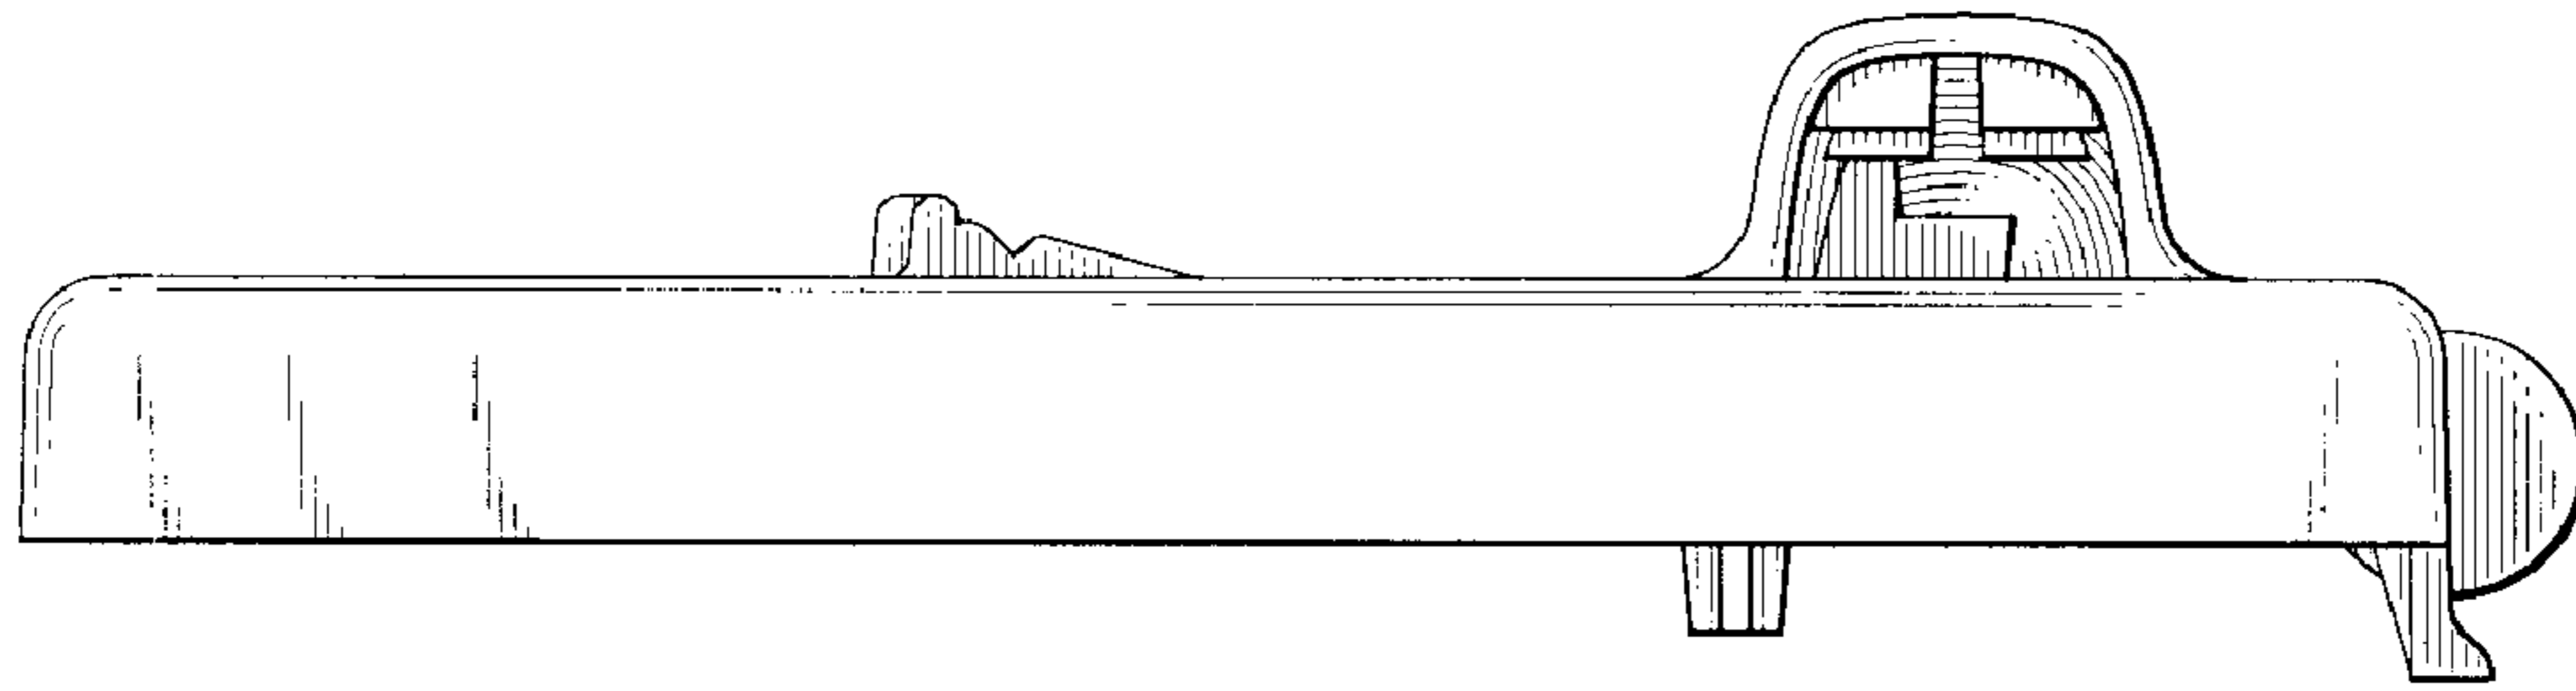


Fig. 6

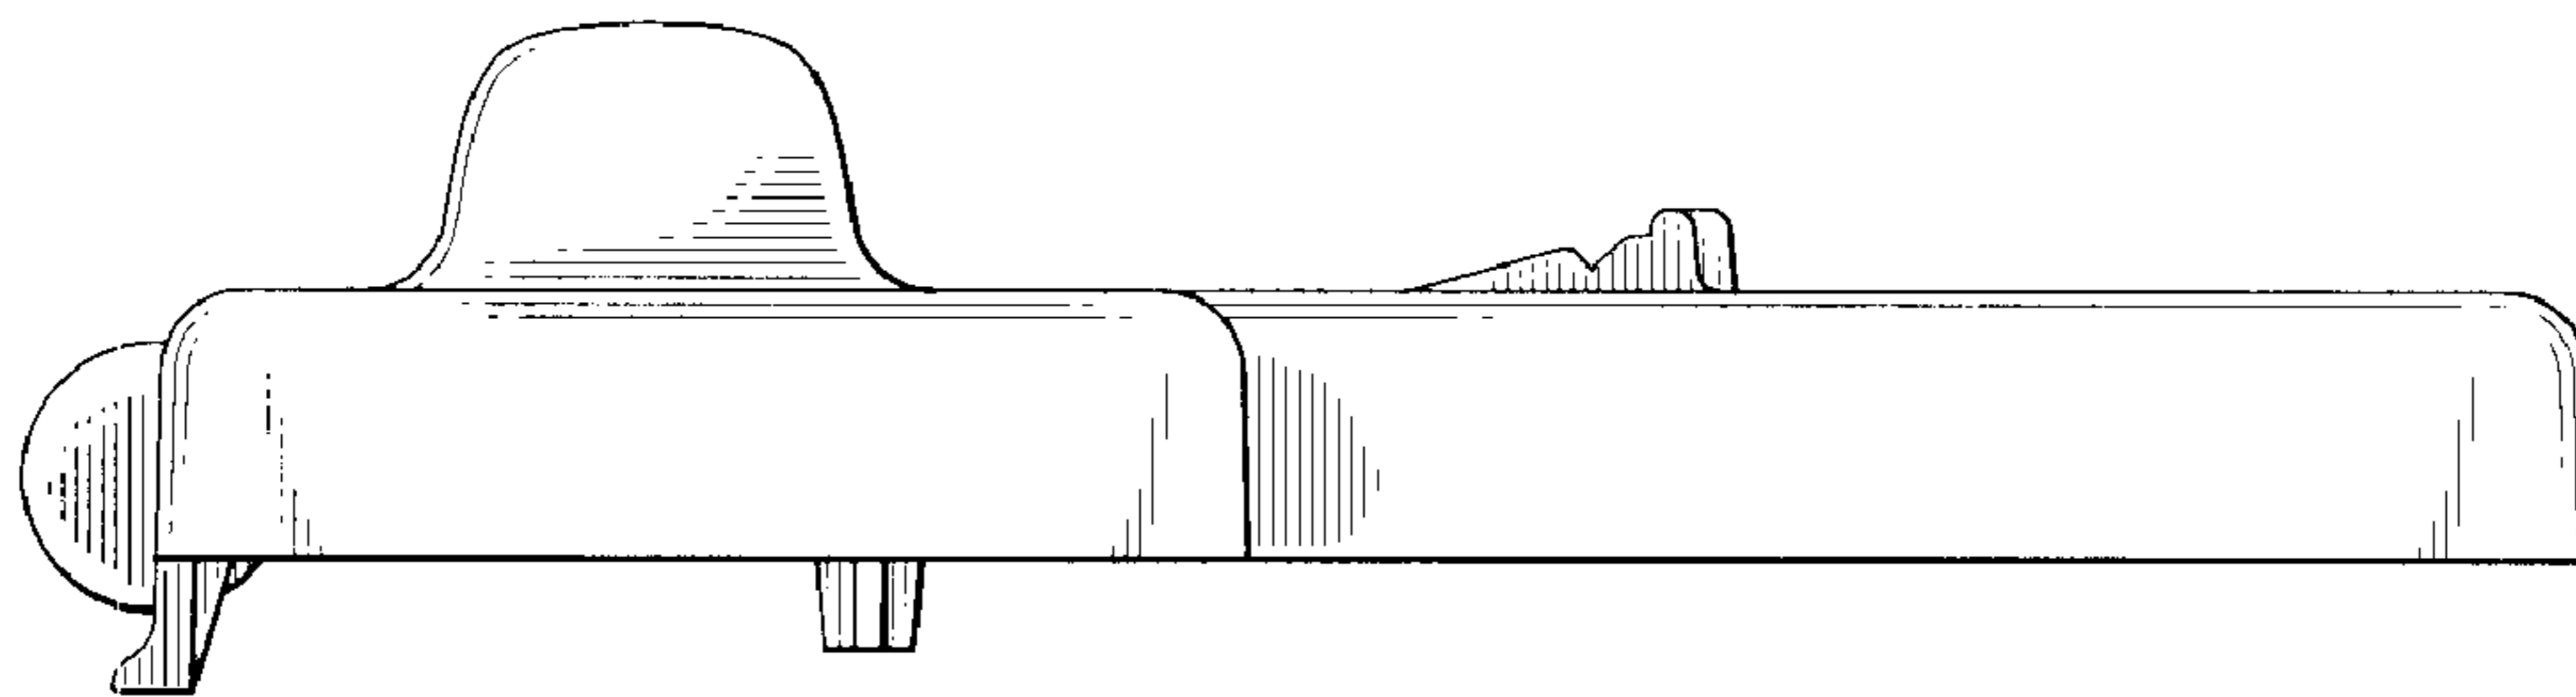


Fig. 7

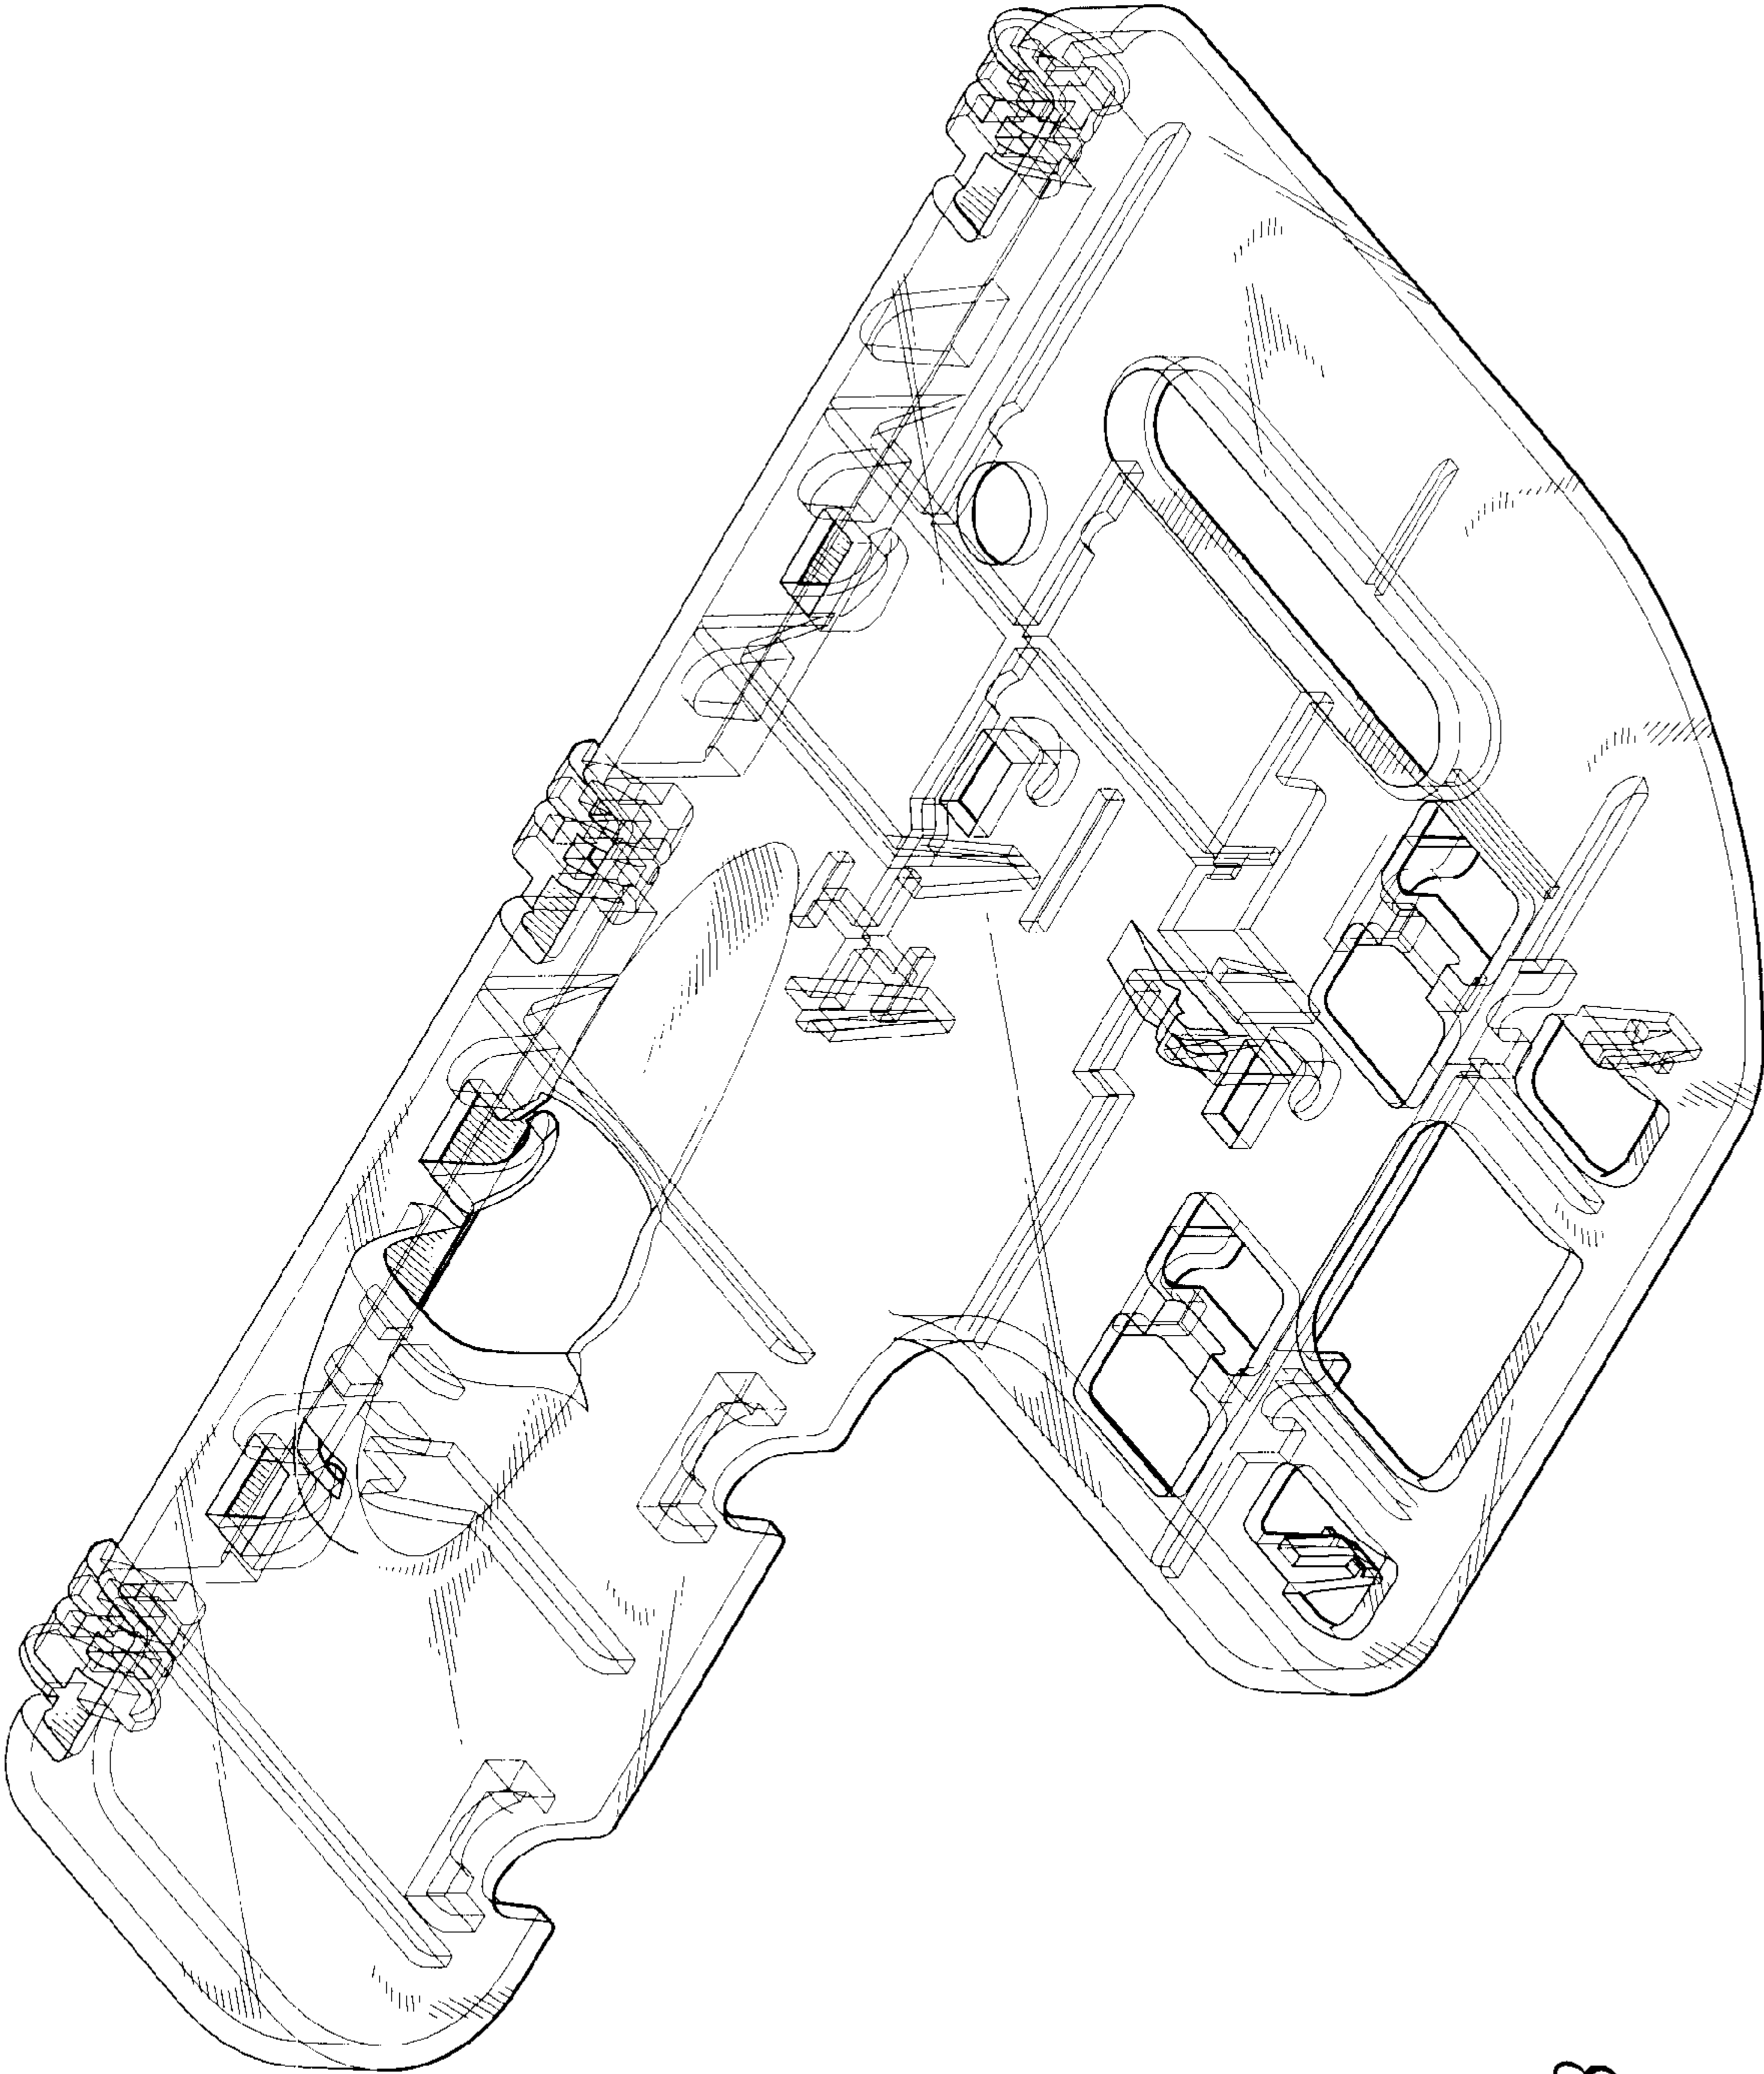


Fig. 8

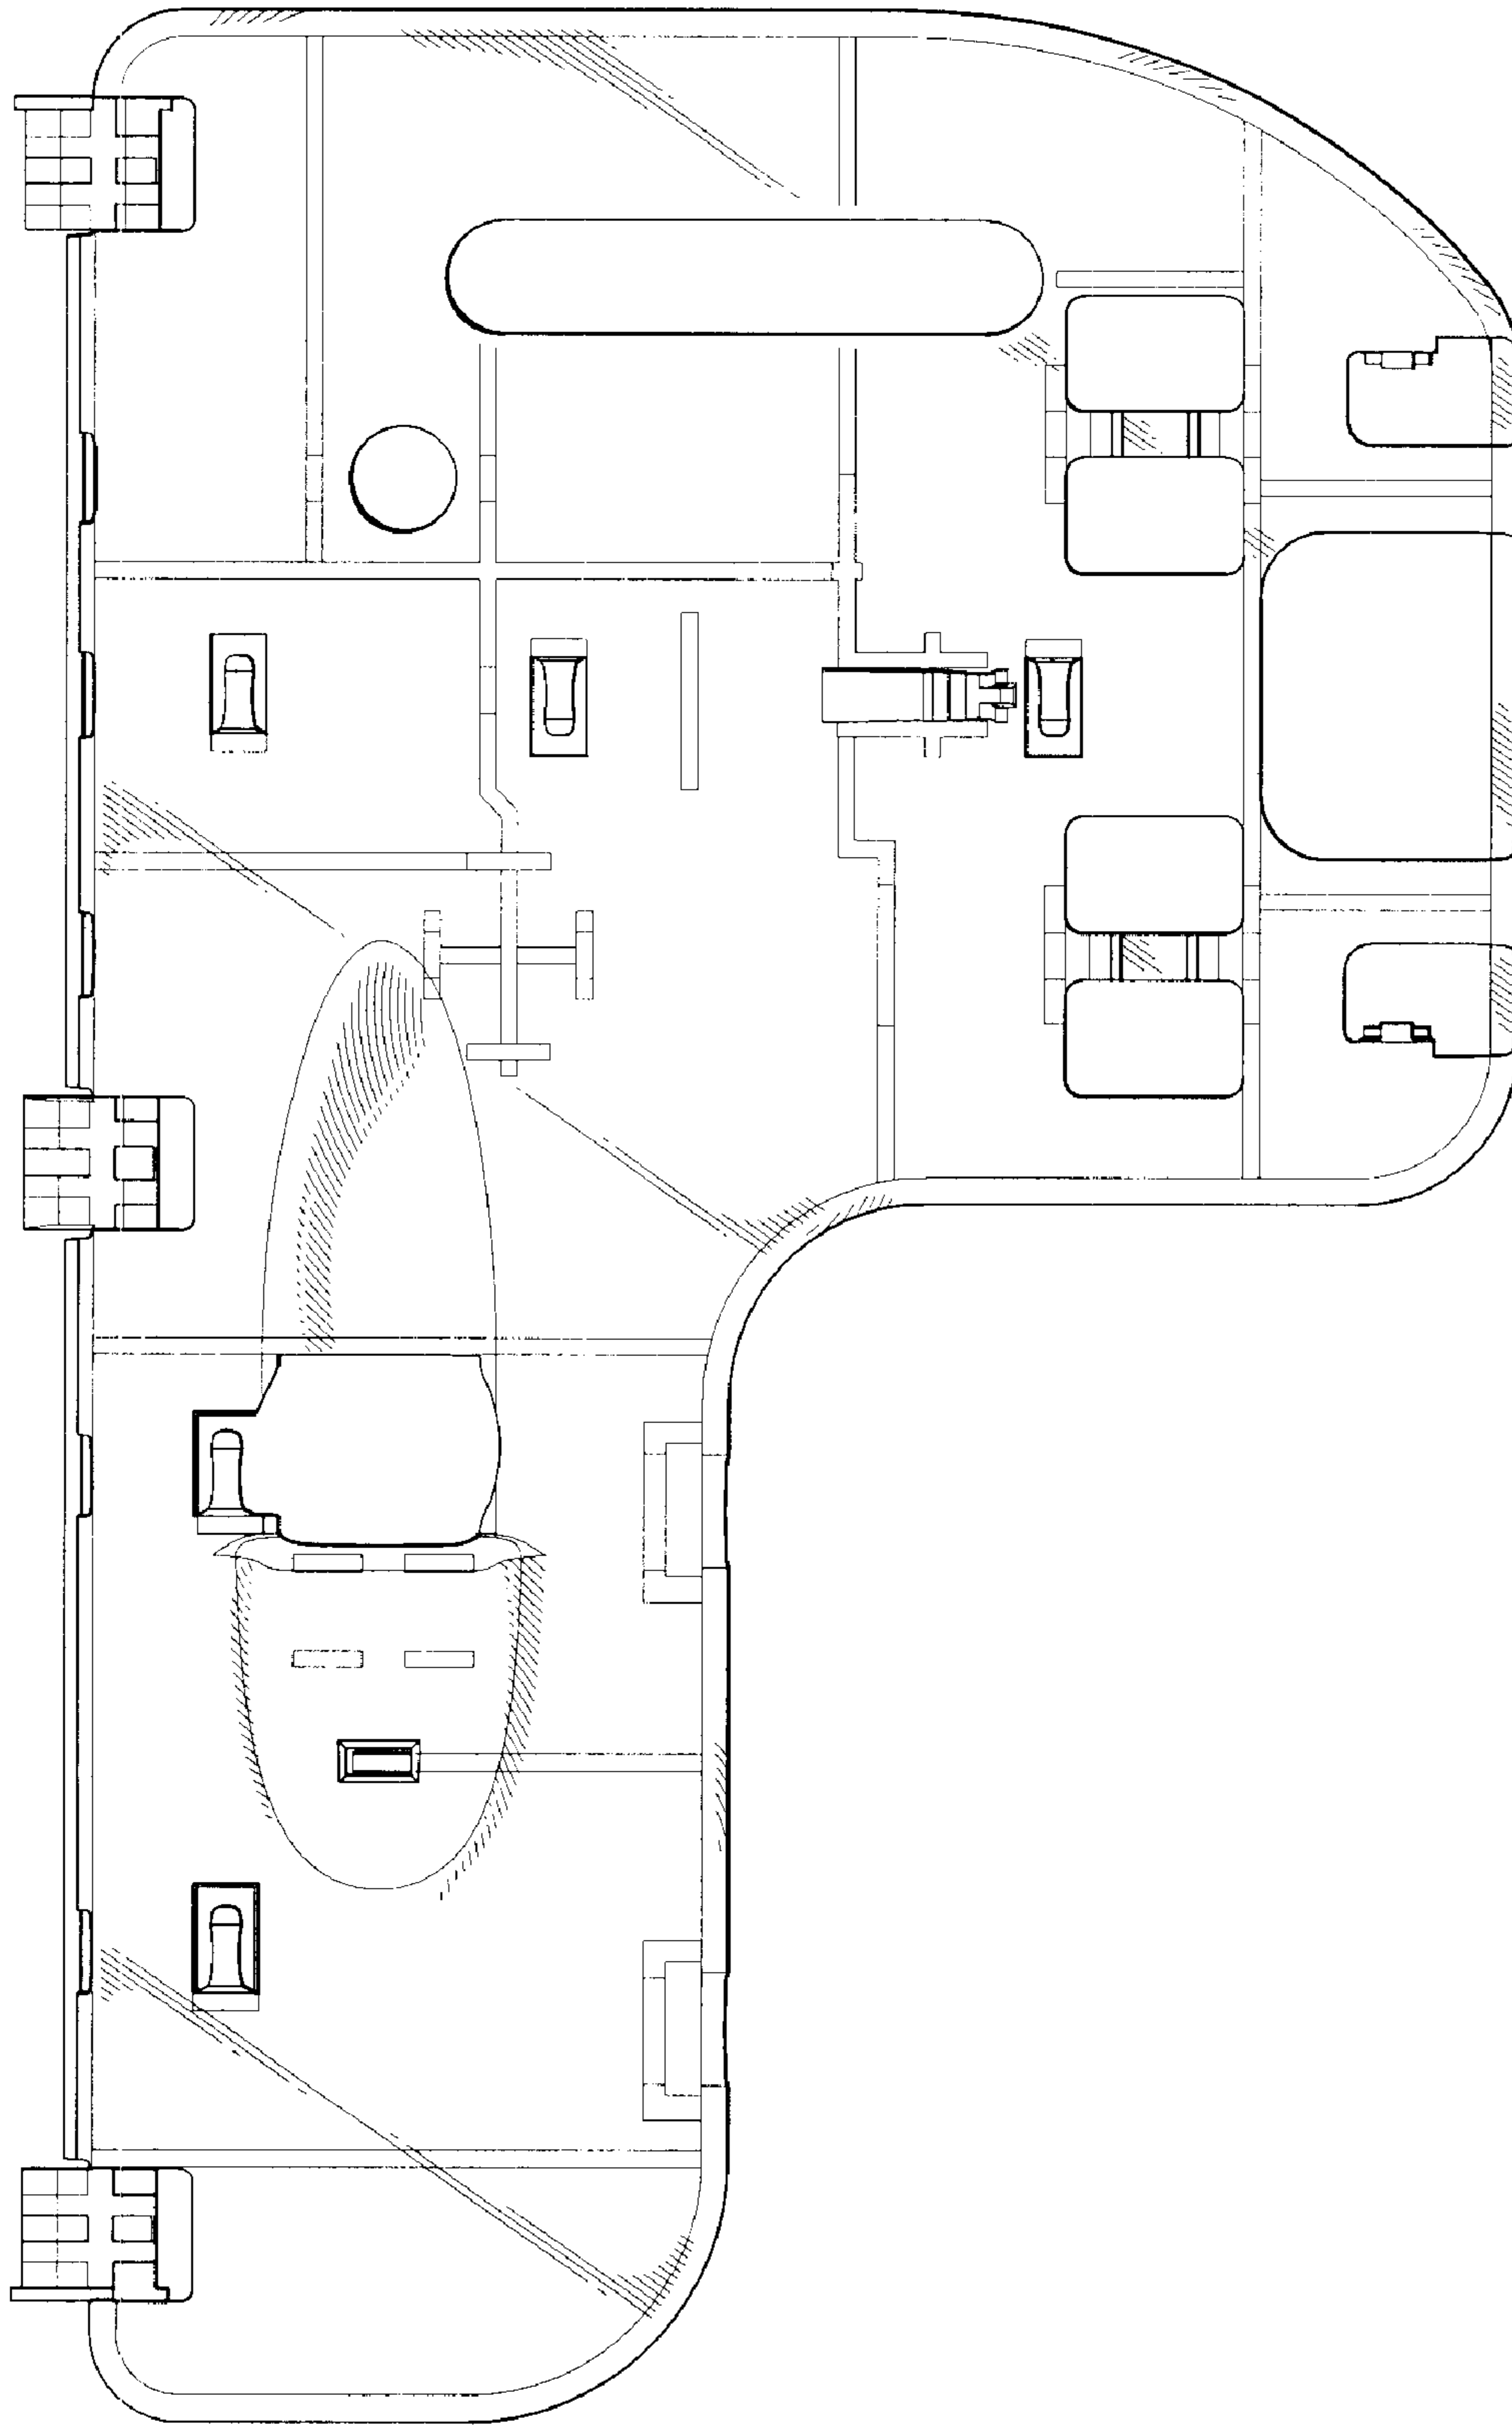


Fig. 9

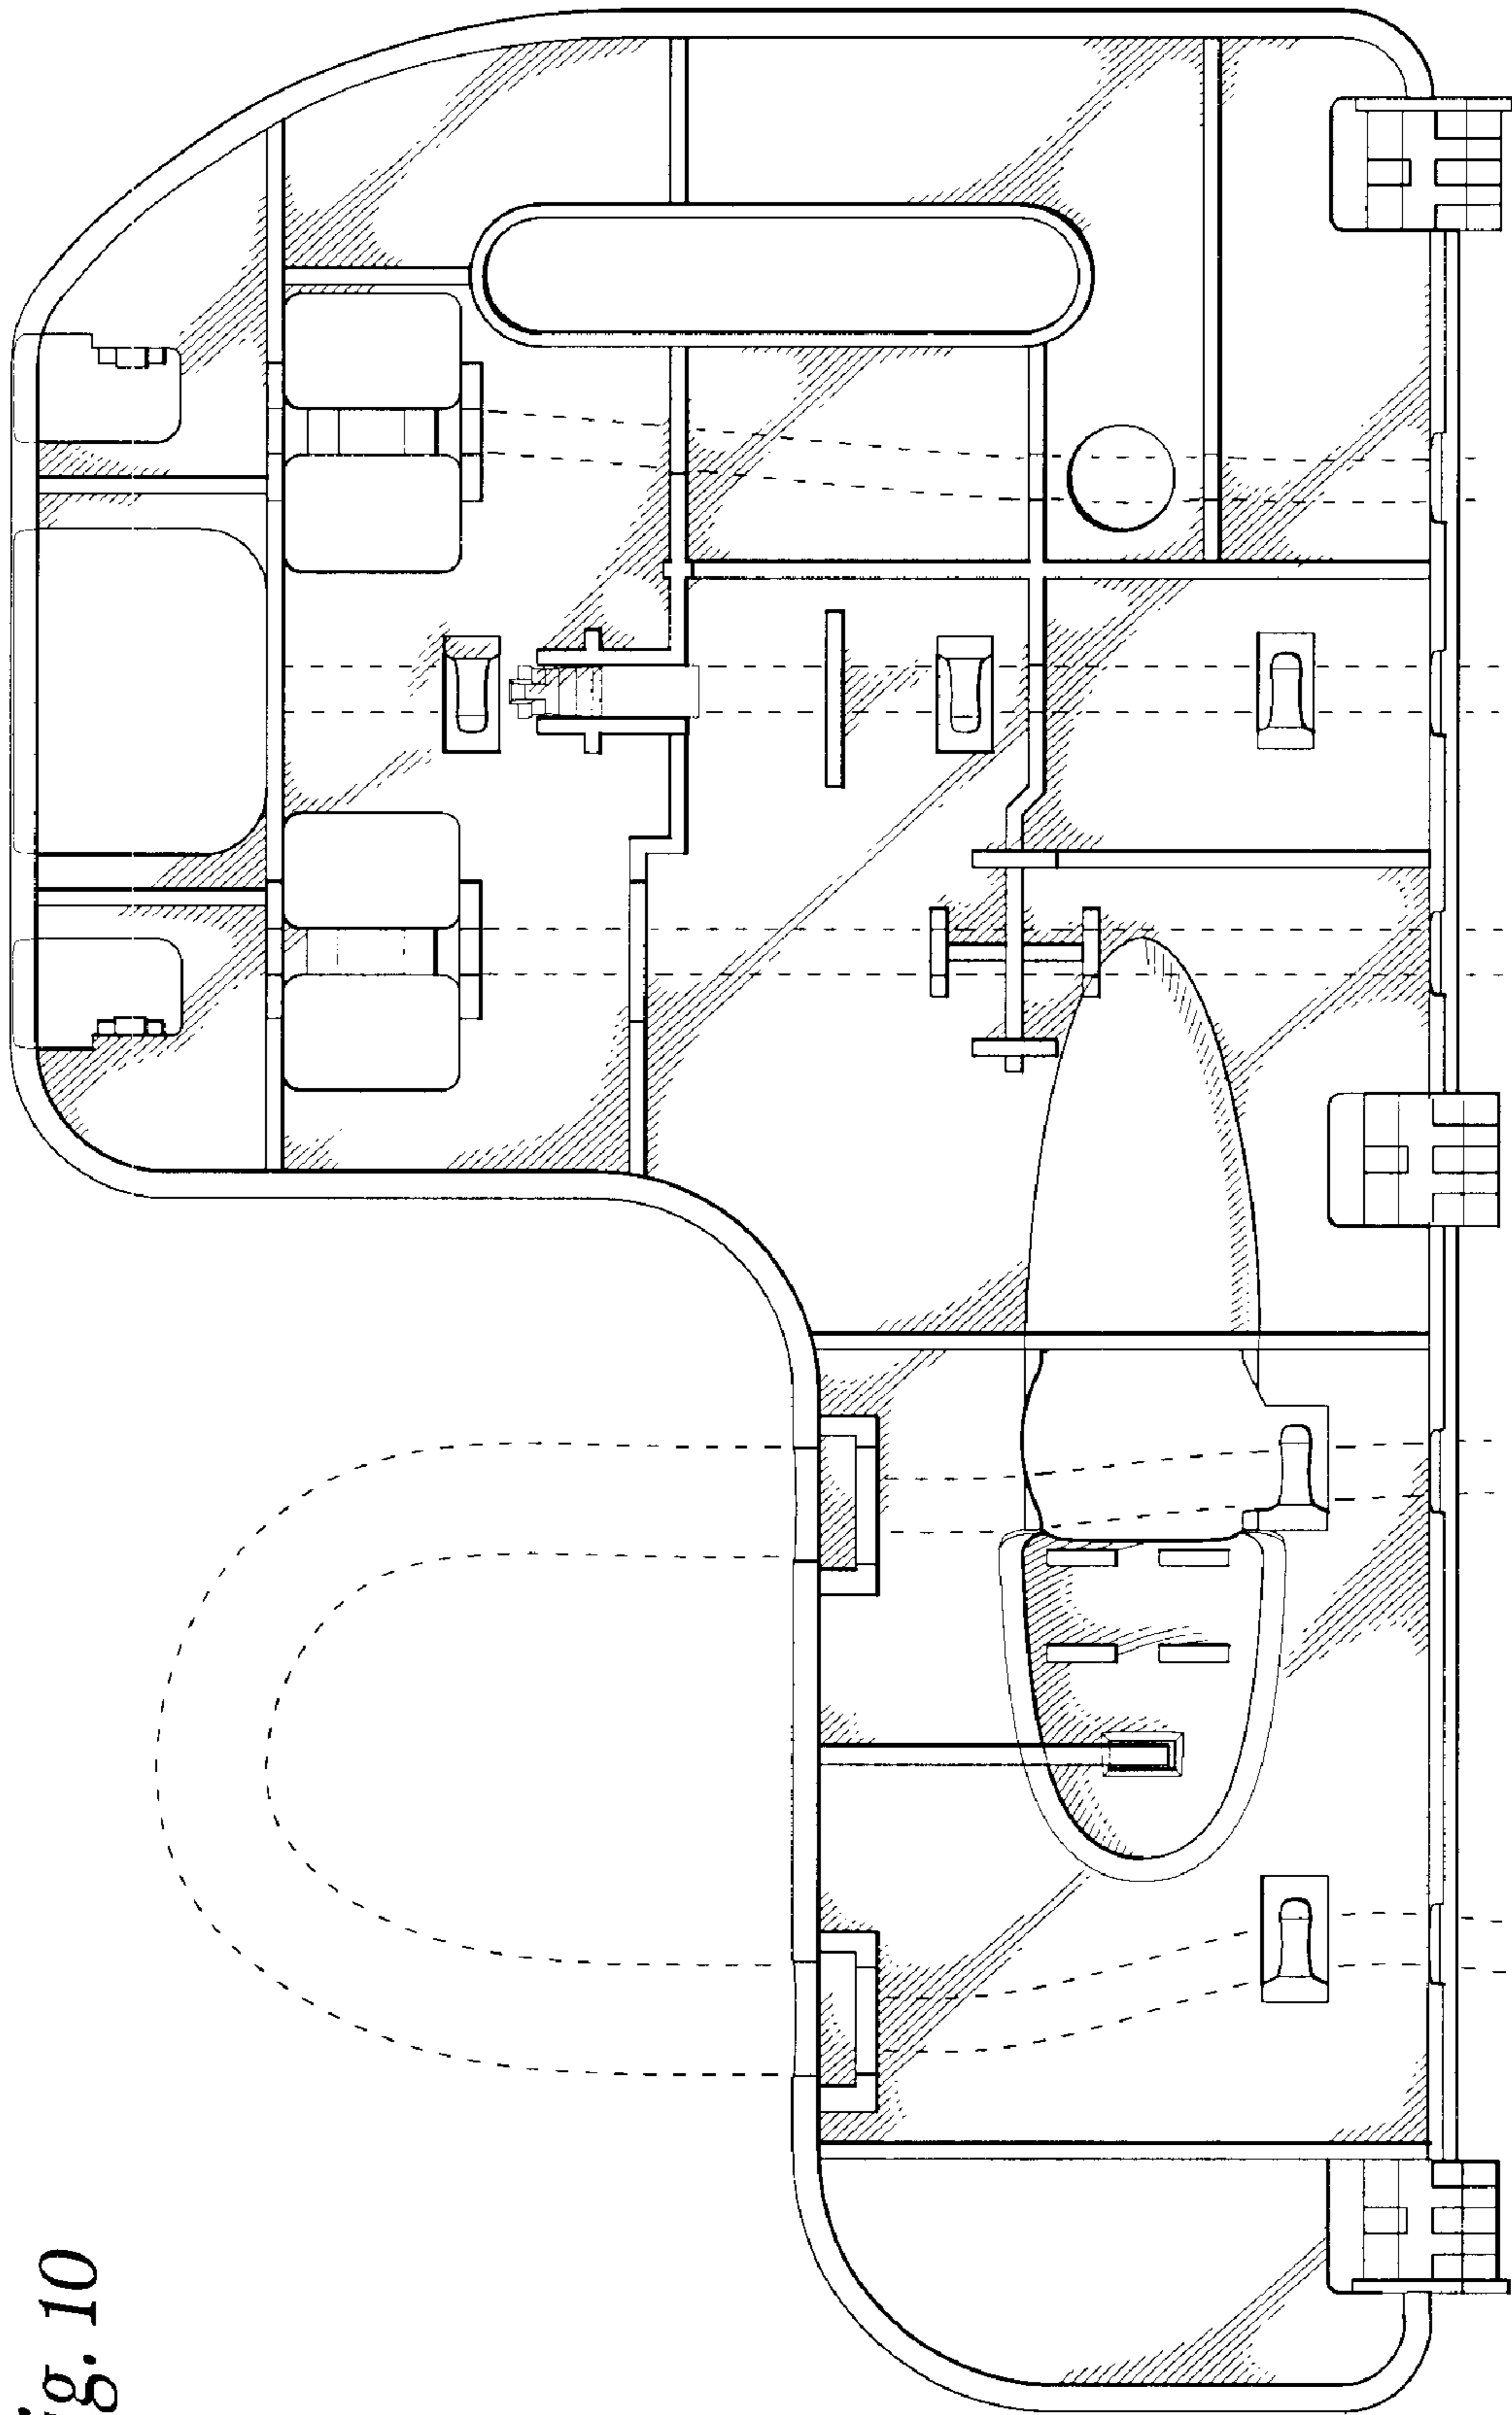


Fig. 10

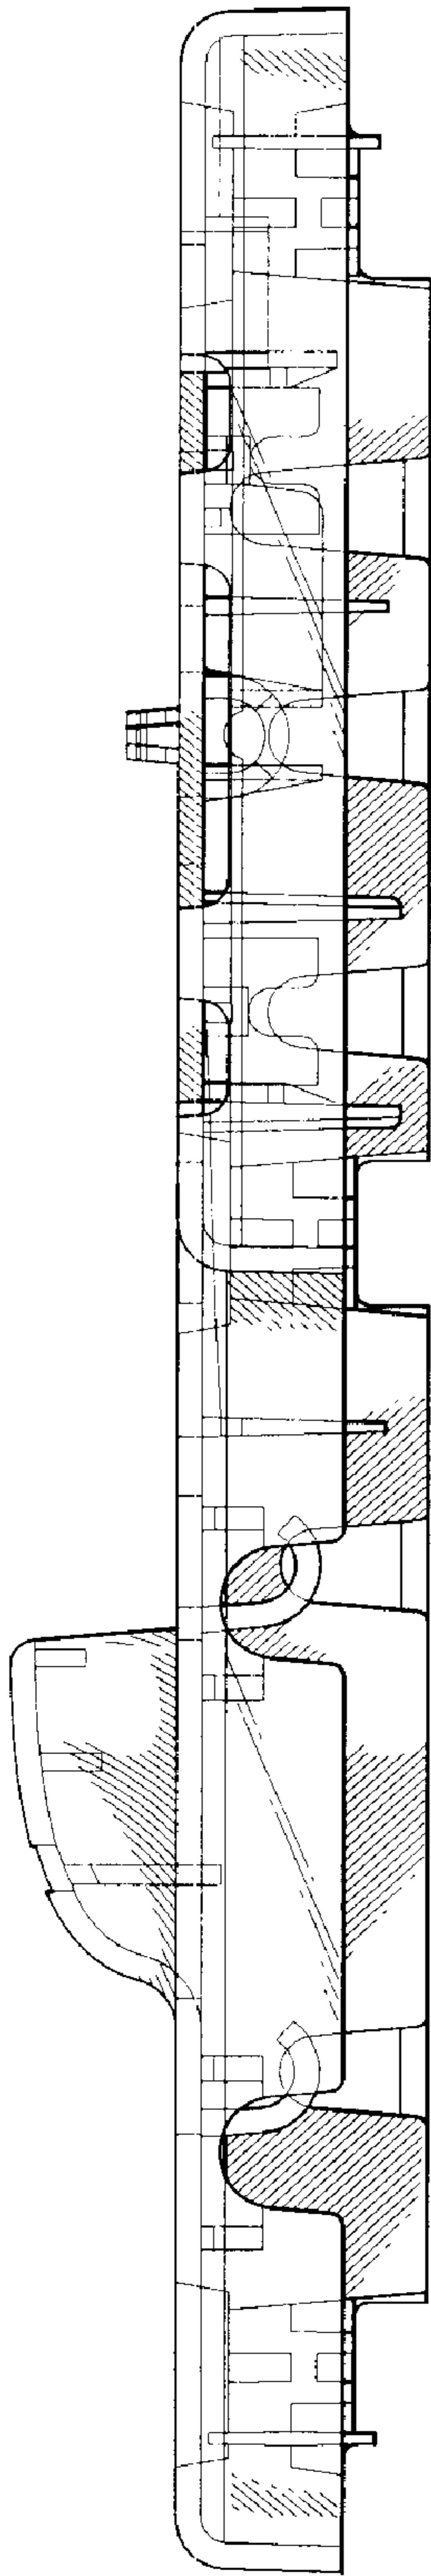


Fig. 11

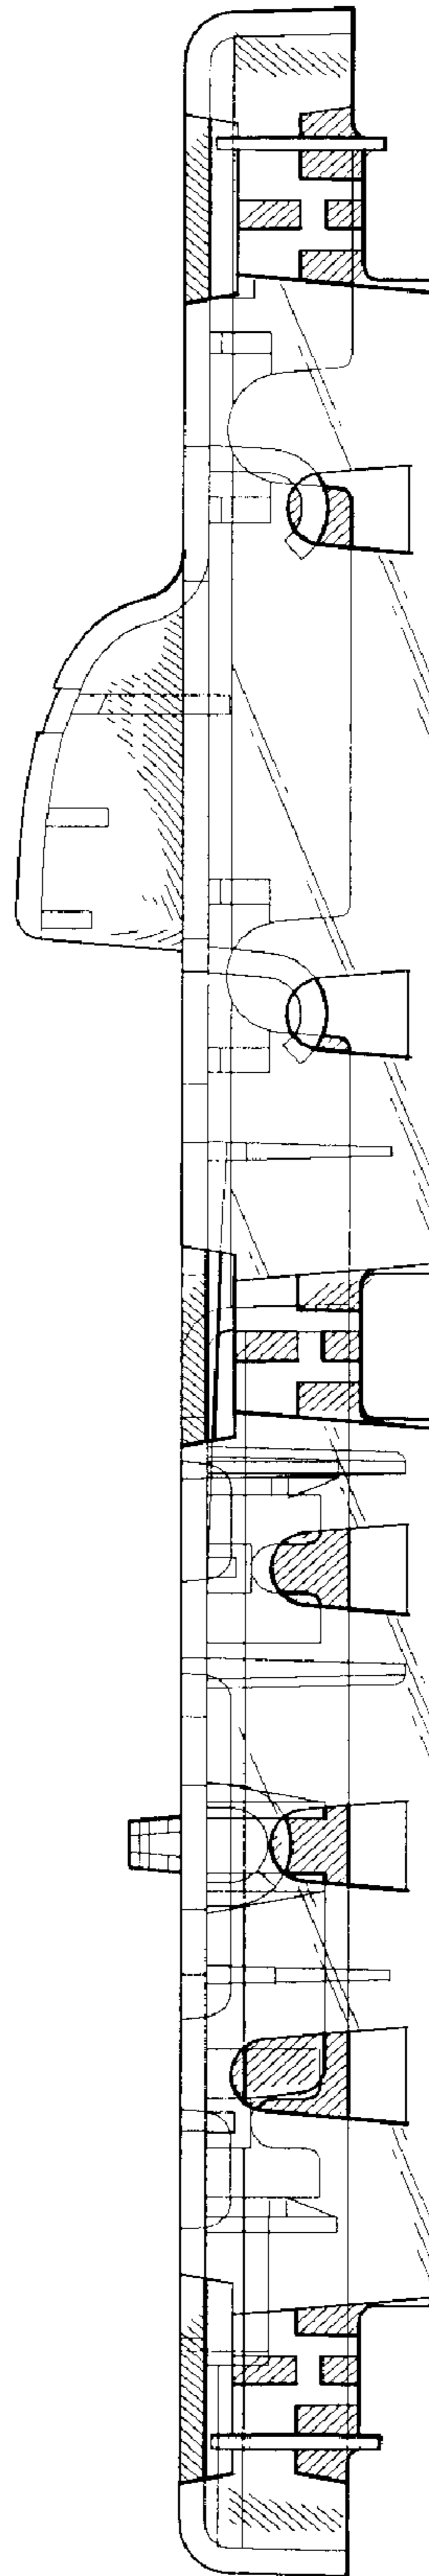


Fig. 12

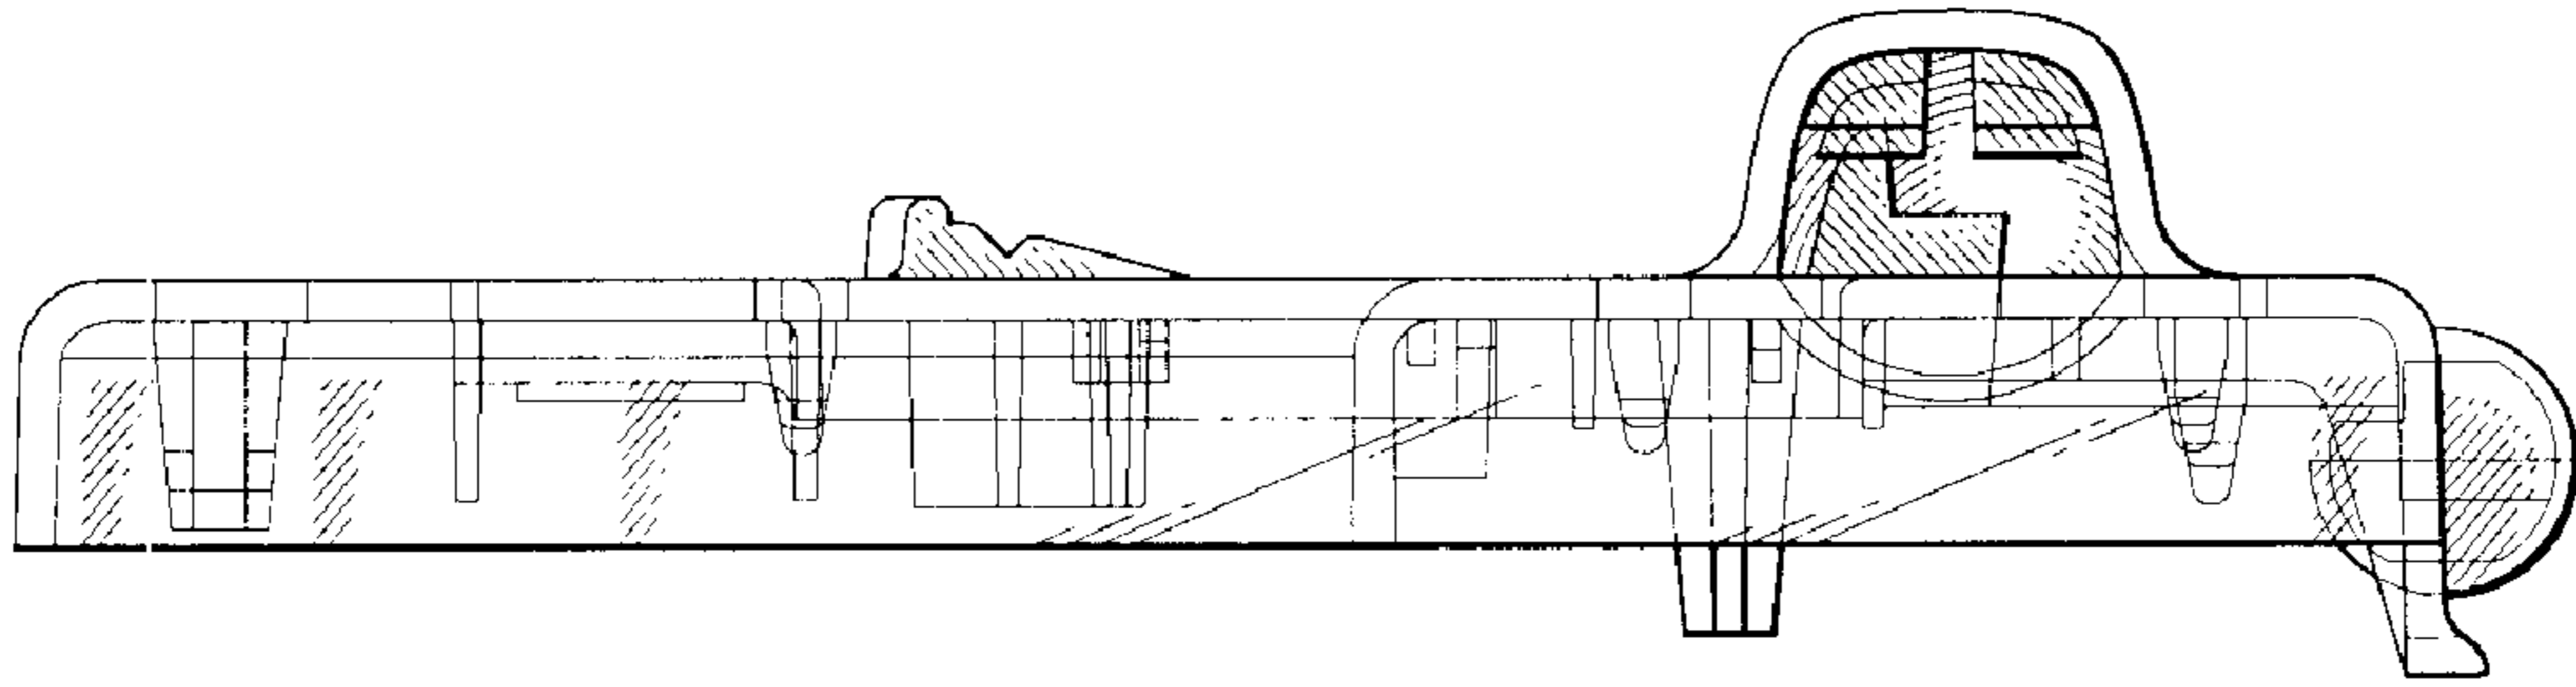


Fig. 13

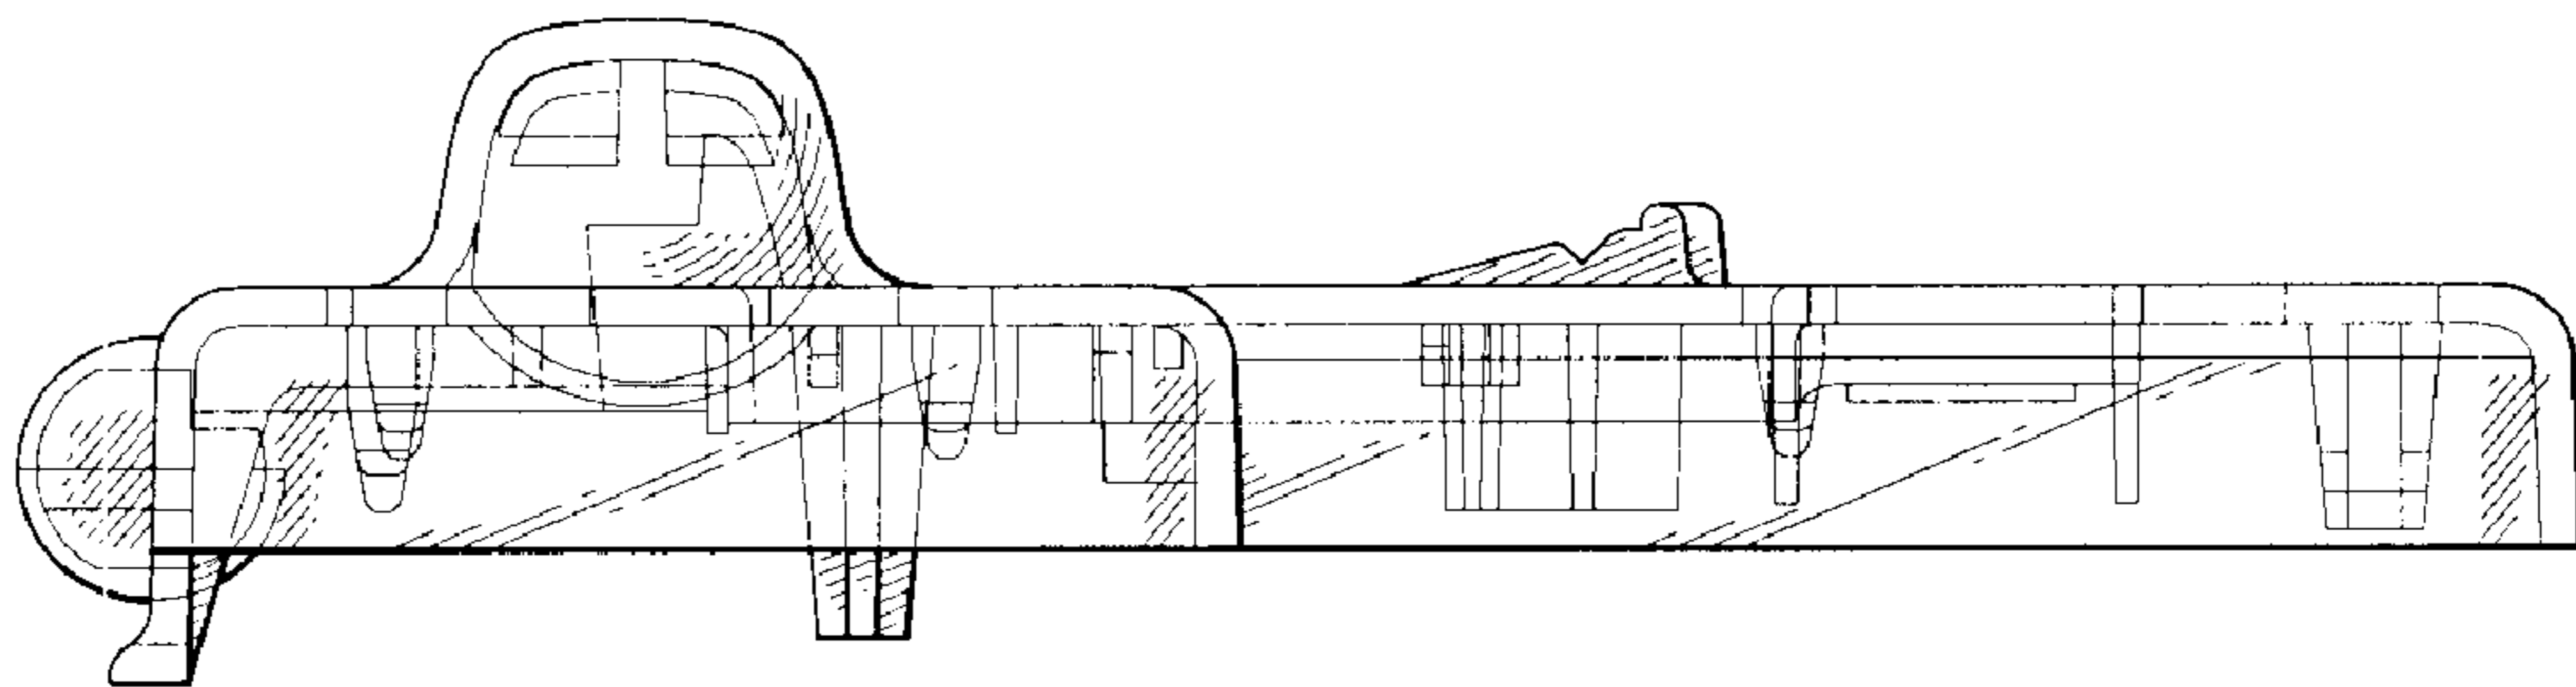


Fig. 14