

US00D532515S

(12) **United States Design Patent**
Büttler et al.

(10) **Patent No.:** **US D532,515 S**

(45) **Date of Patent:** **** Nov. 21, 2006**

(54) **BASIS FOR SURGICAL AIMING DEVICE**

(75) Inventors: **Markus Büttler**, Oensingen (CH);
André Schlienger, Arlesheim (CH);
Patrick Streff, Weil am Rhein (DE)

(73) Assignee: **Synthes USA**, West Chester, PA (US)

(**) Term: **14 Years**

(21) Appl. No.: **29/209,626**

(22) Filed: **Jul. 19, 2004**

(30) **Foreign Application Priority Data**

Jan. 19, 2004 (CH) 130413

(51) **LOC (8) Cl.** **24-02**

(52) **U.S. Cl.** **D24/140; D24/133**

(58) **Field of Classification Search** D24/133,
D24/140, 146, 147; 606/62, 86-89, 96, 98
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

- 4,708,139 A * 11/1987 Dunbar, IV 606/96
- 4,923,458 A * 5/1990 Fischer 606/59
- D357,534 S * 4/1995 Hayes D24/140
- D359,557 S * 6/1995 Hayes D24/140
- D466,609 S * 12/2002 Glossop D24/140
- 6,527,775 B1 * 3/2003 Warburton 606/62
- D496,996 S * 10/2004 Jensen et al. D24/140
- 2004/0210232 A1 * 10/2004 Patel et al. 606/96

2005/0177171 A1 * 8/2005 Wetzler et al. 606/96

* cited by examiner

Primary Examiner—Antoine D. Davis

Assistant Examiner—Christopher Lee

(74) *Attorney, Agent, or Firm*—Jones Day

(57) **CLAIM**

The ornamental design for a basis for surgical aiming device, as shown and described.

DESCRIPTION

In use, the basis for surgical aiming device interacts with a surgical aiming device, the details of which are shown and described in co-pending U.S. Design patent application Ser. No.; 29/209,625, entitled surgical aiming device, filed on even date herewith the entire disclosure of which is incorporate herein by reference.

FIG. 1 is a perspective view of a first embodiment of the basis for surgical aiming device;

FIG. 2 is a right side view of the basis for surgical aiming device of FIG. 1;


FIG. 3 is a bottom view of the basis for surgical aiming device of FIG. 1;

FIG. 4 is a top view of the basis for surgical aiming device of FIG. 1;

FIG. 5 is a rear view of the basis for surgical aiming device of FIG. 1; and,

FIG. 6 is a front view of the basis for surgical aiming device of FIG. 1.

1 Claim, 6 Drawing Sheets

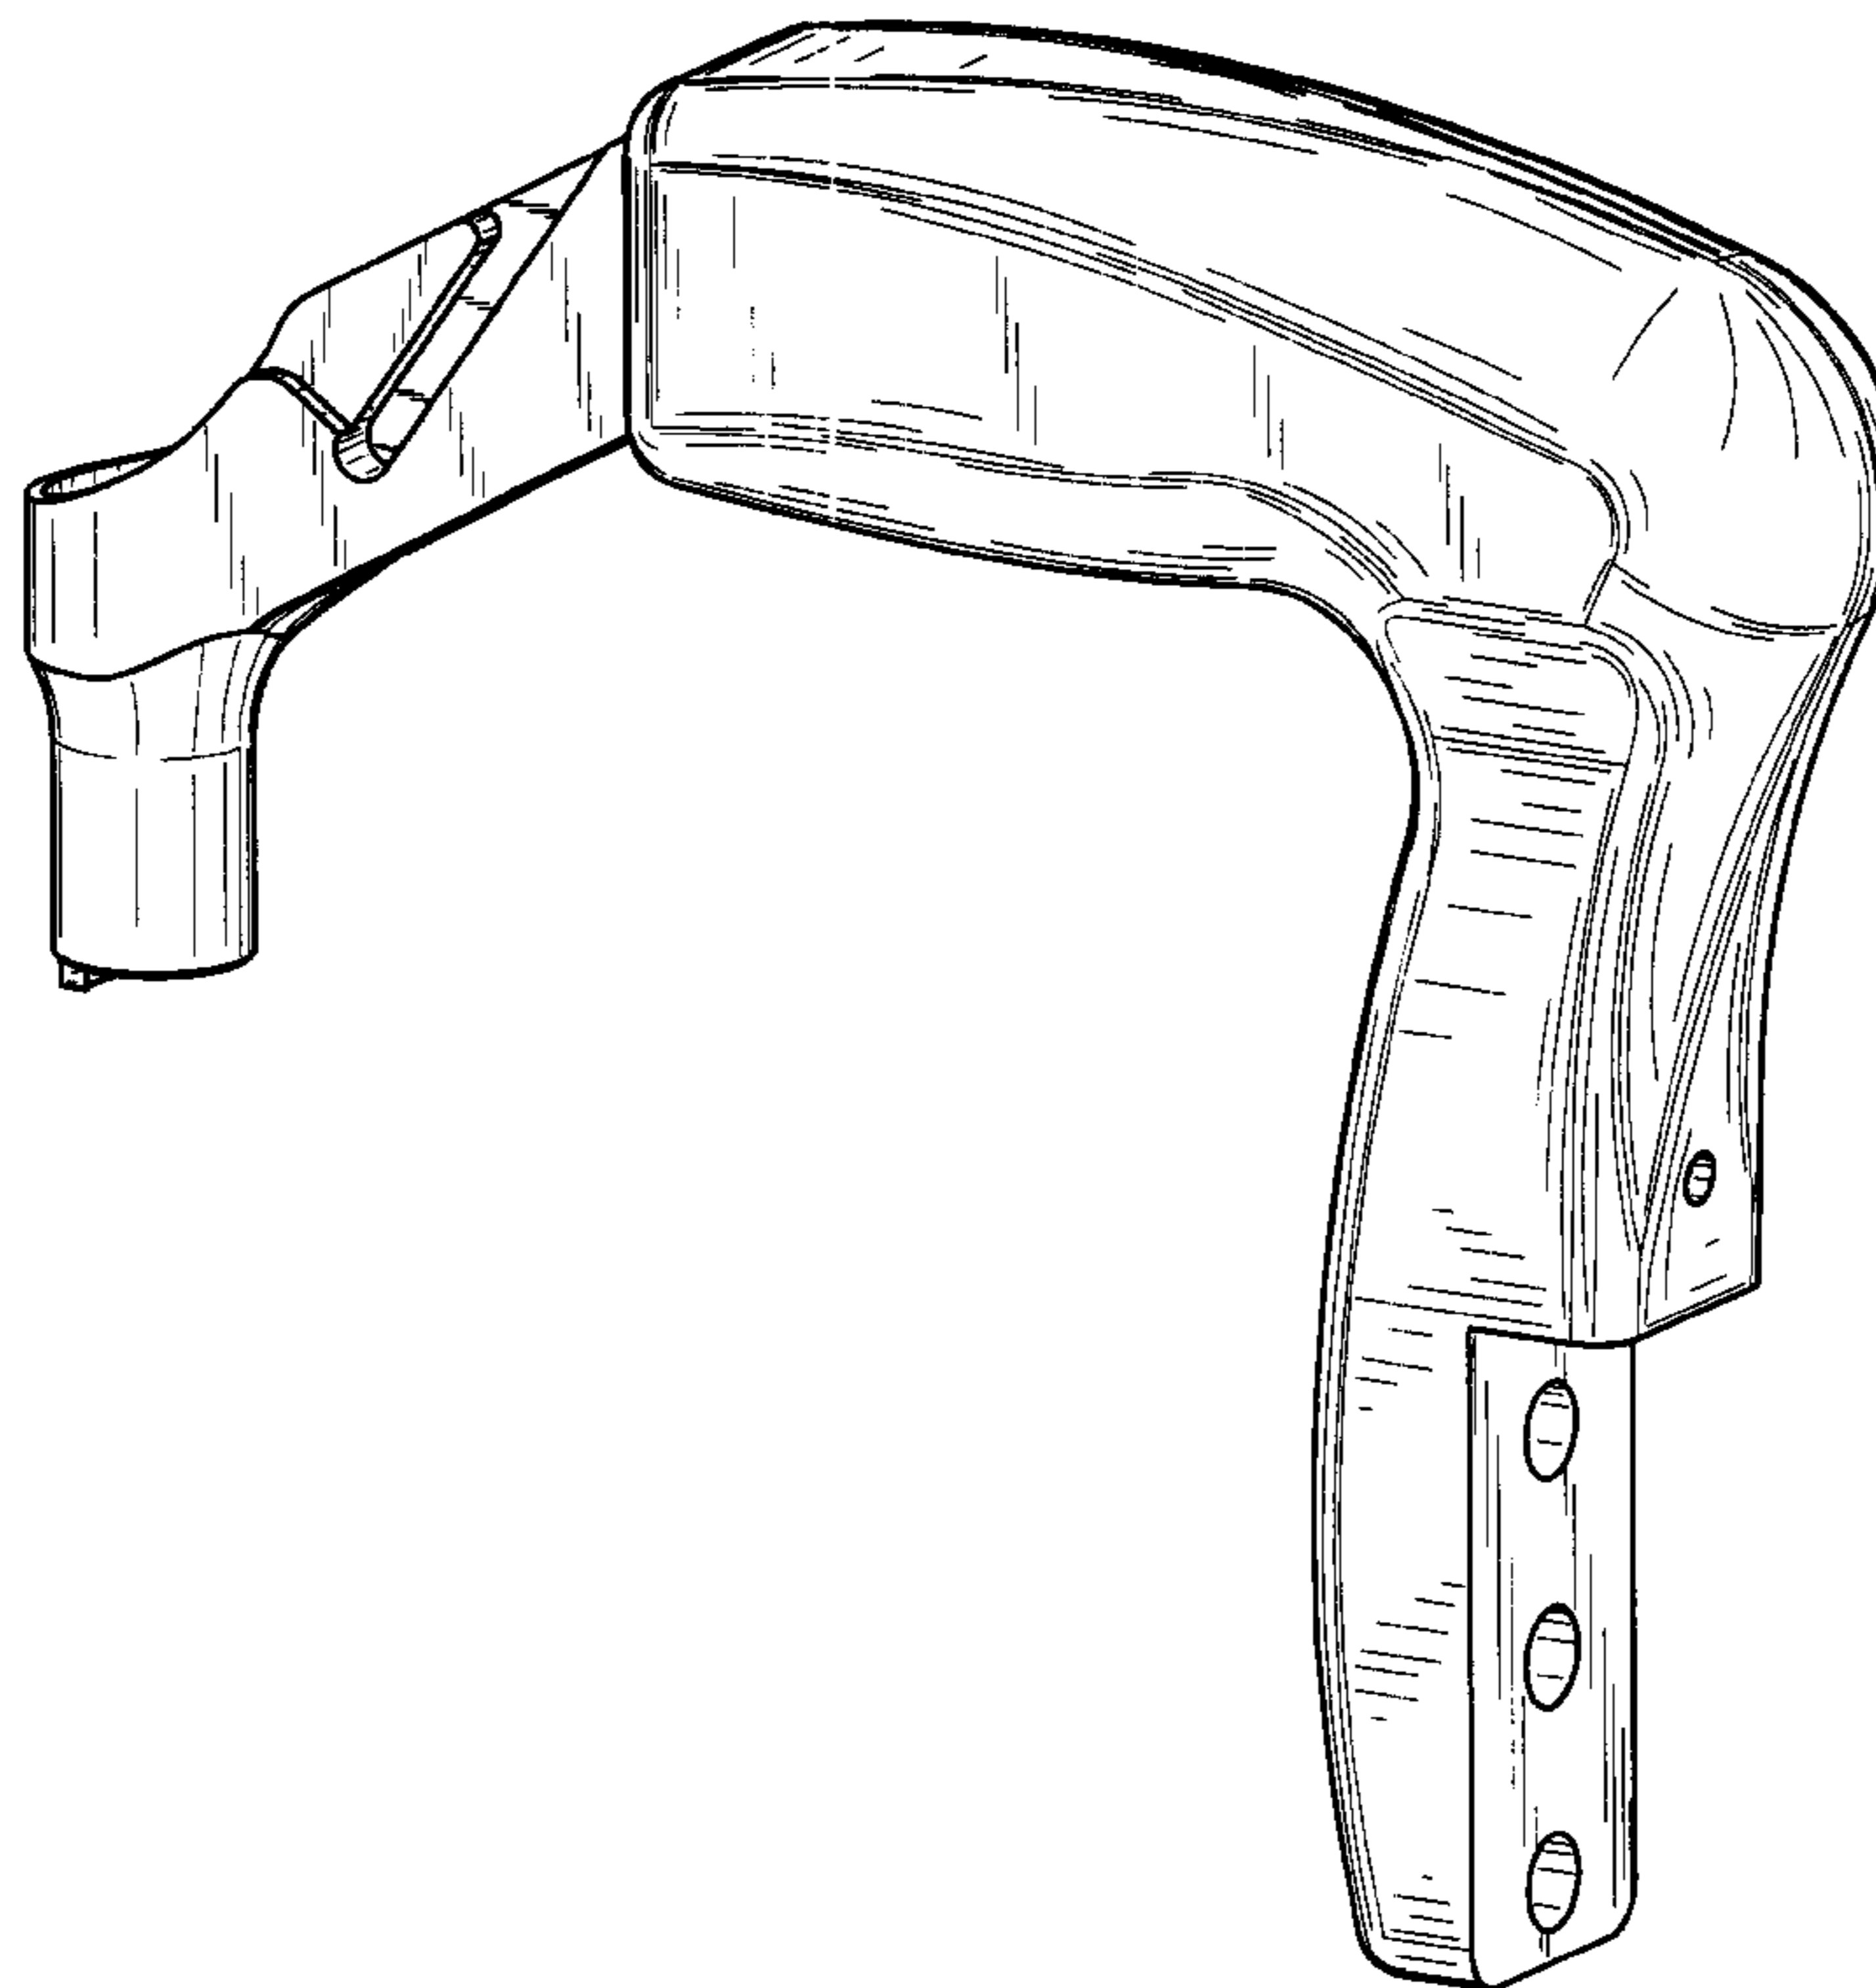

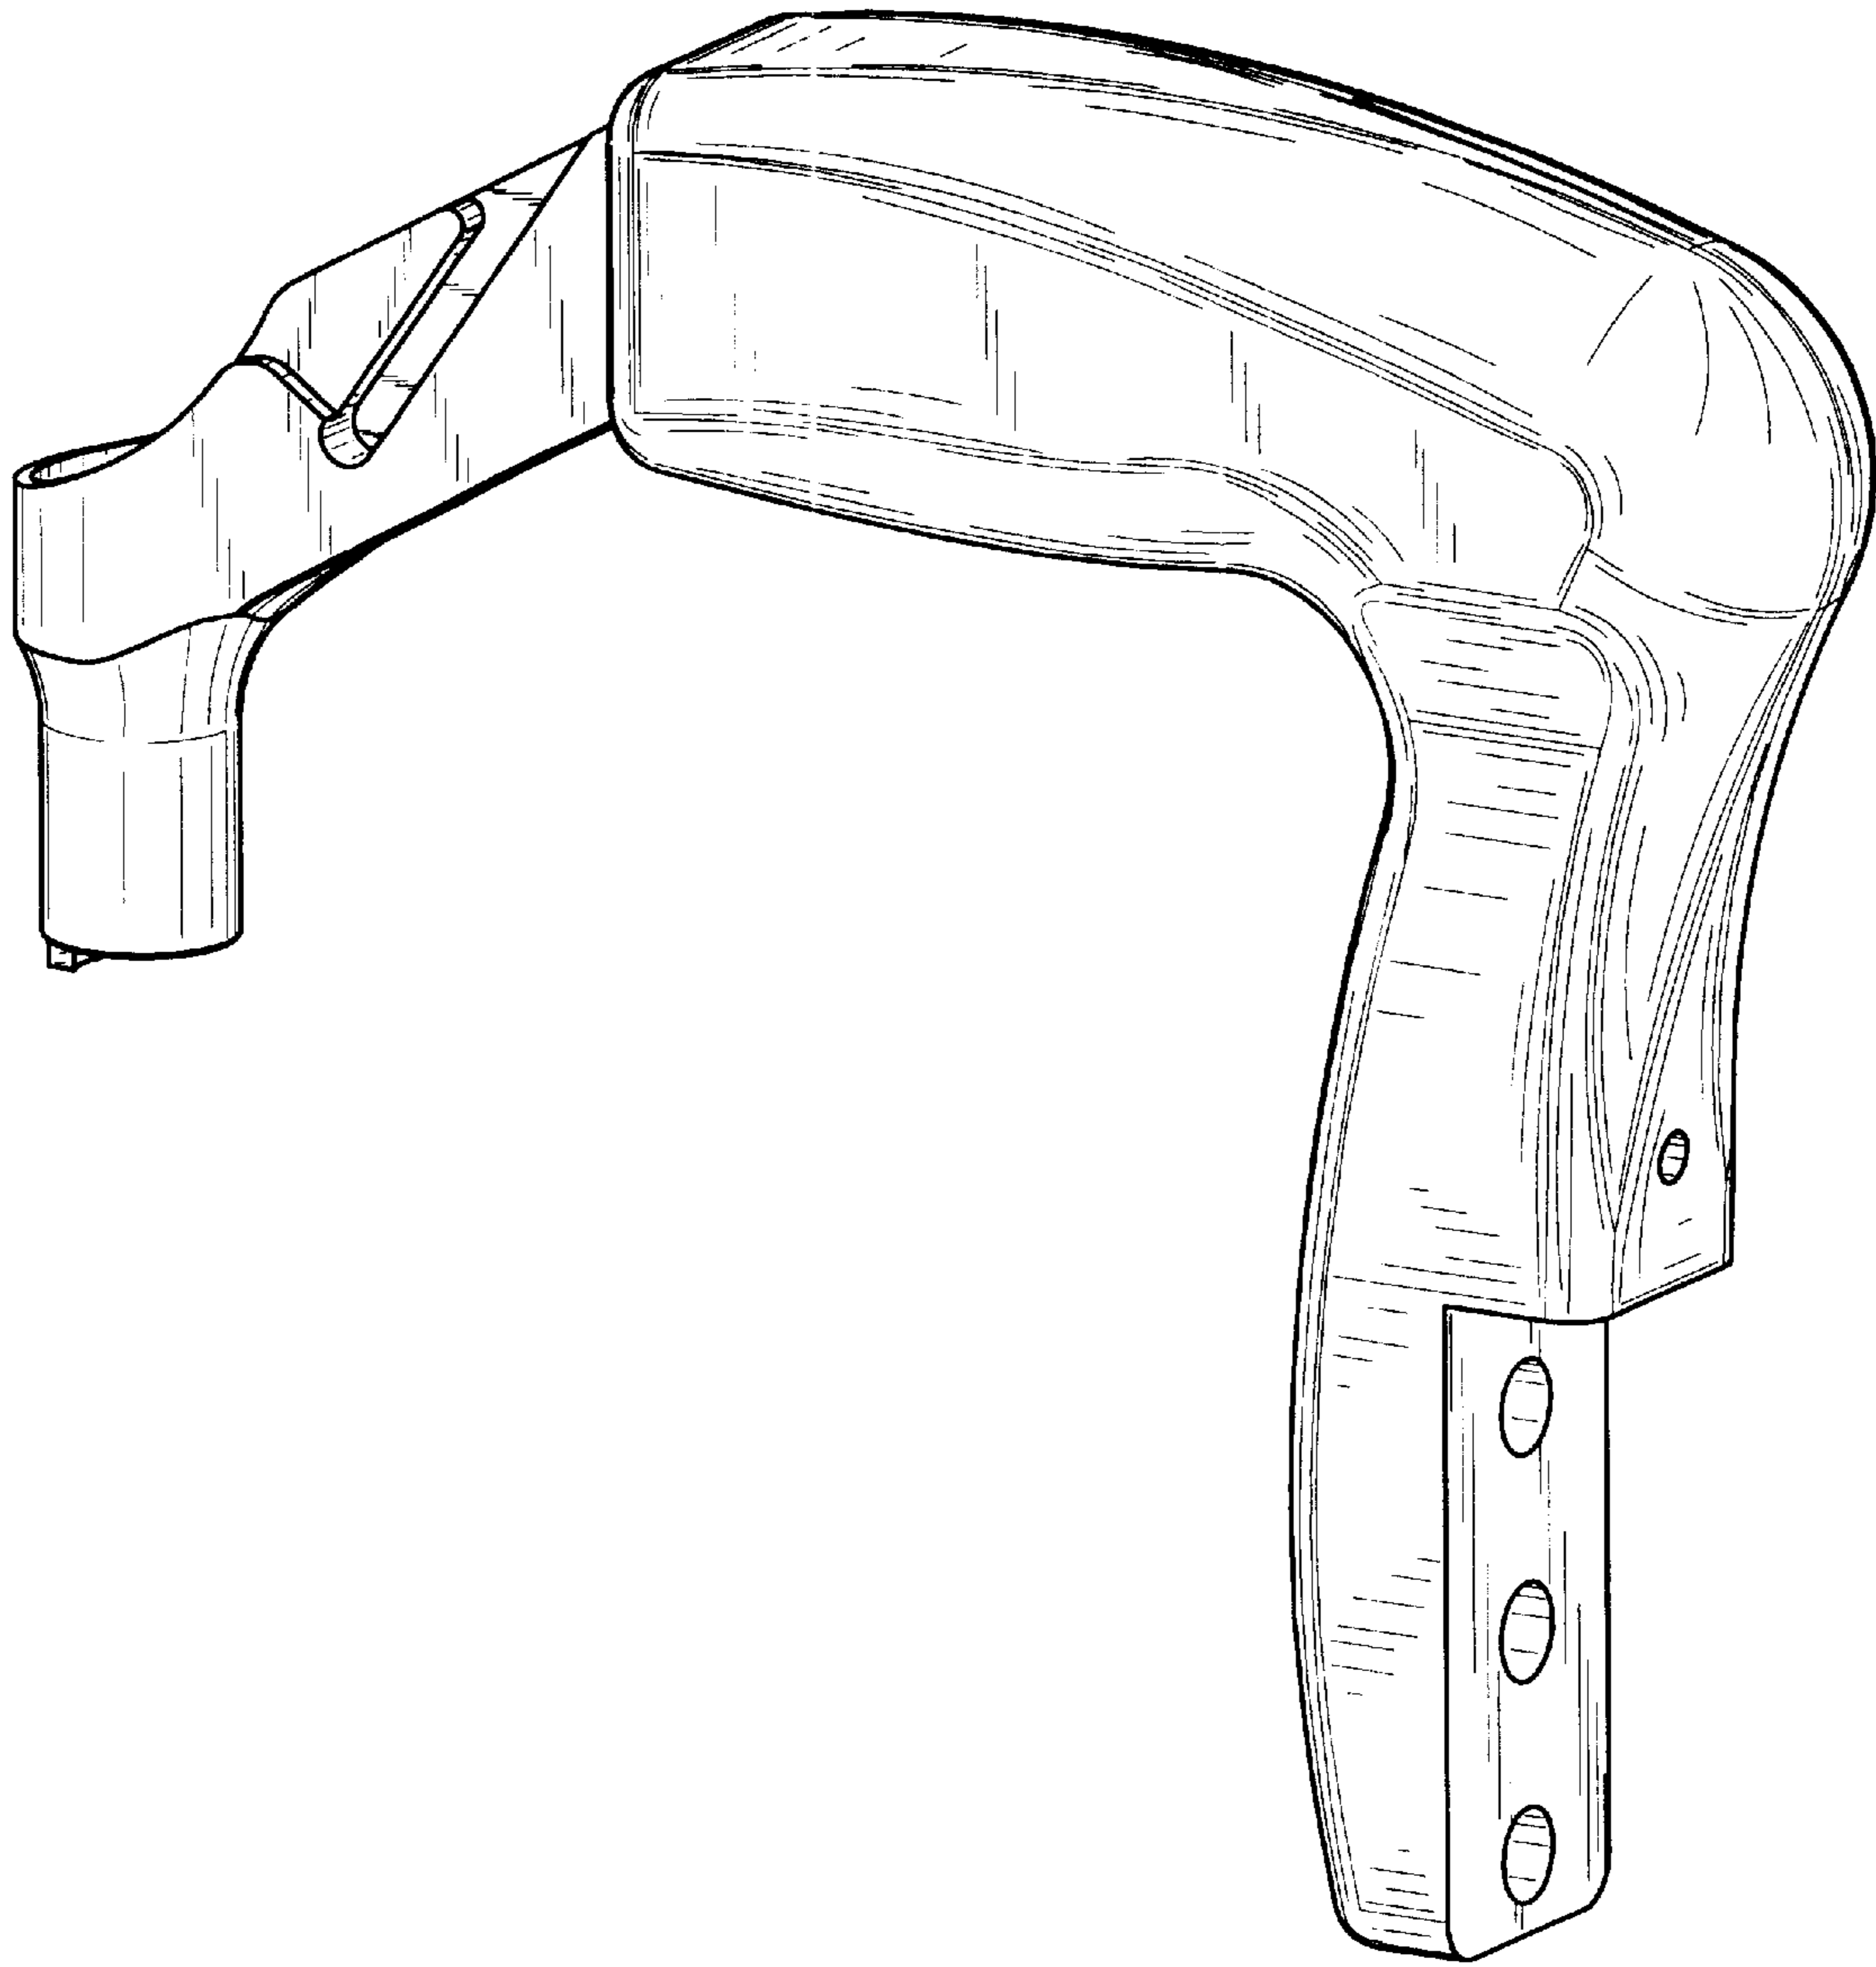


Fig.1

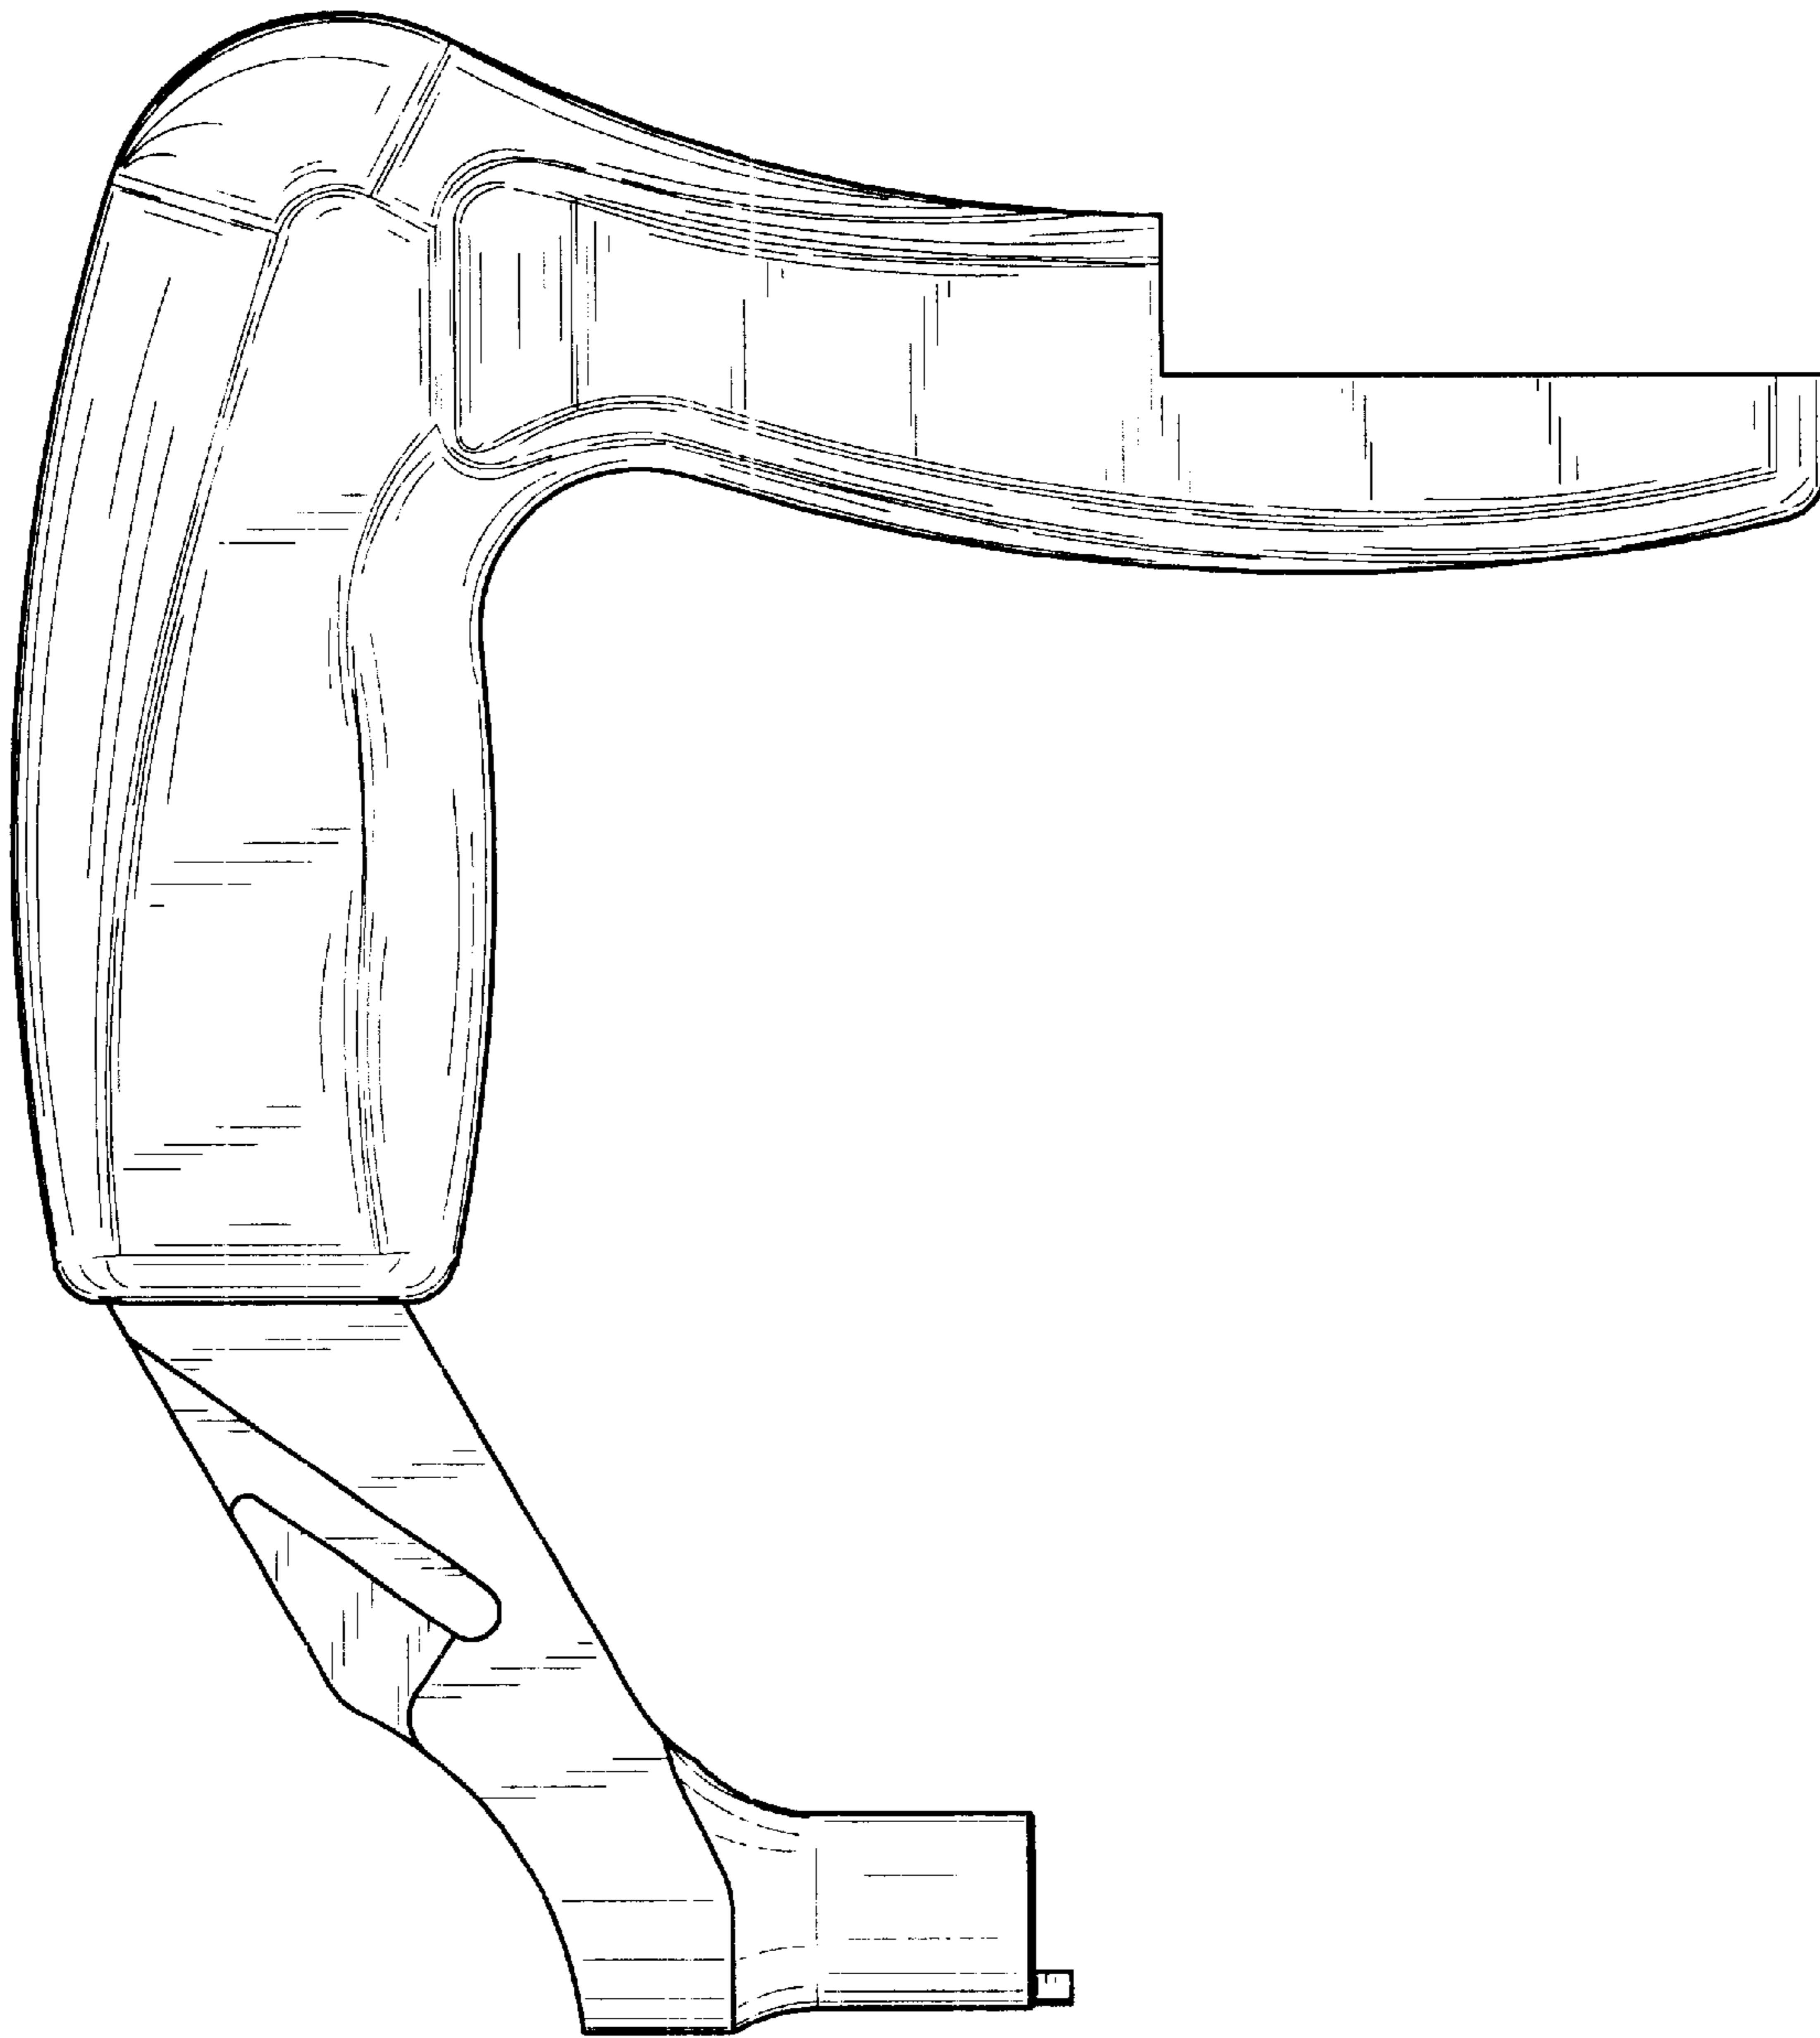


Fig.2

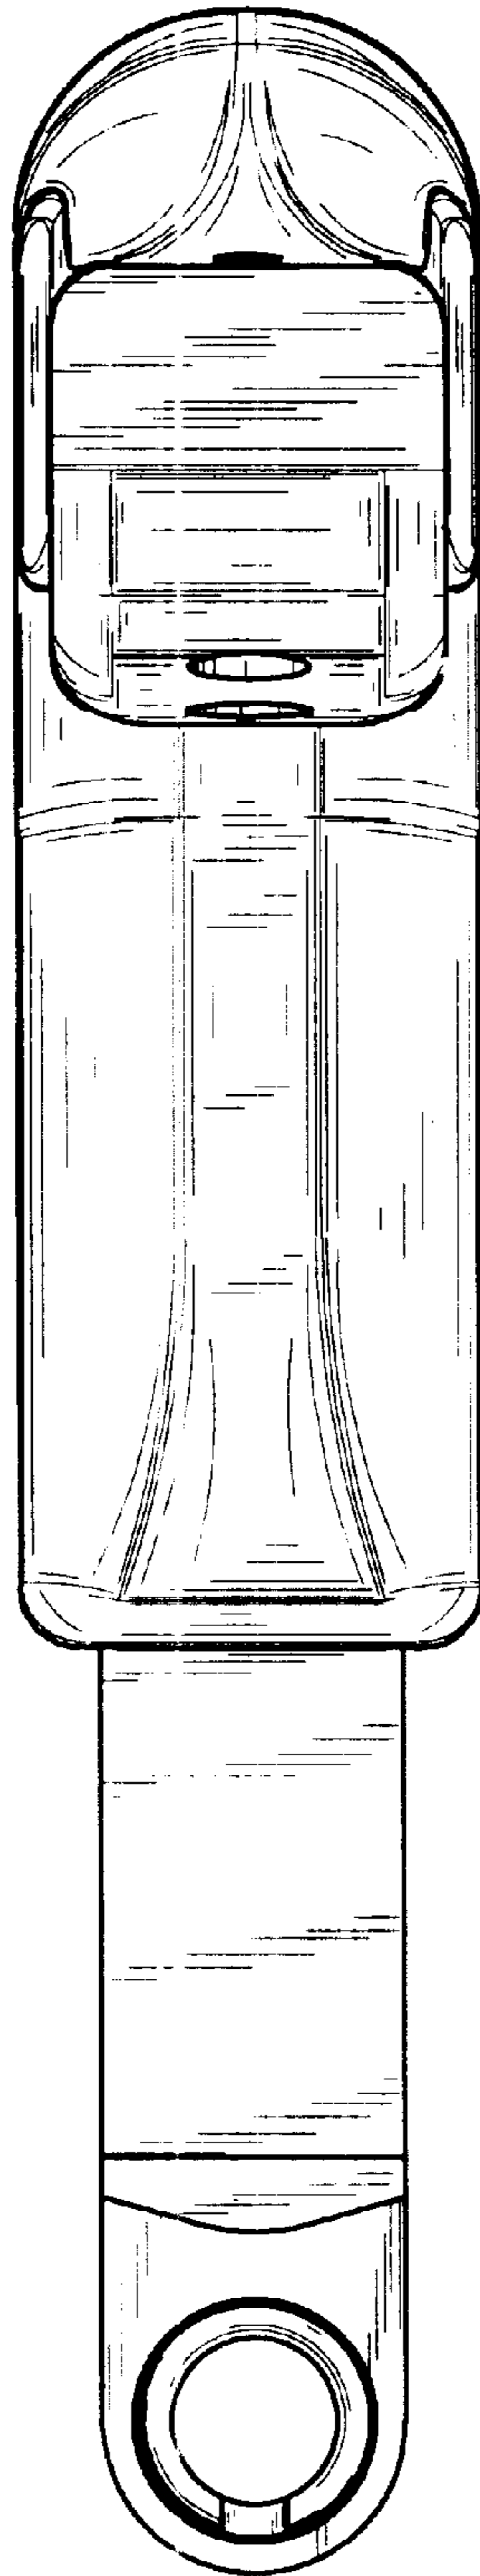


Fig.3

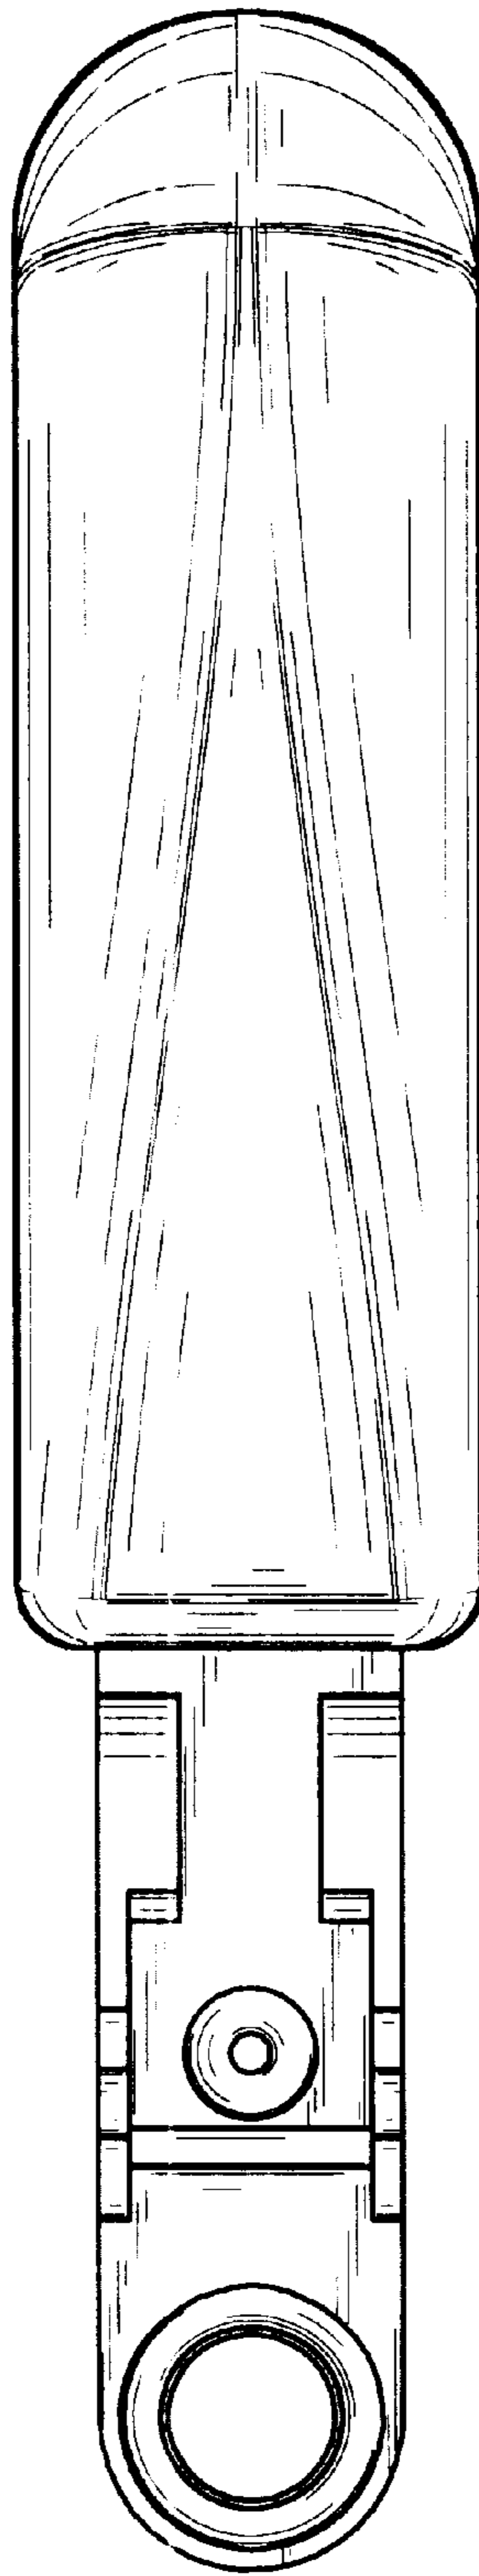


Fig.4

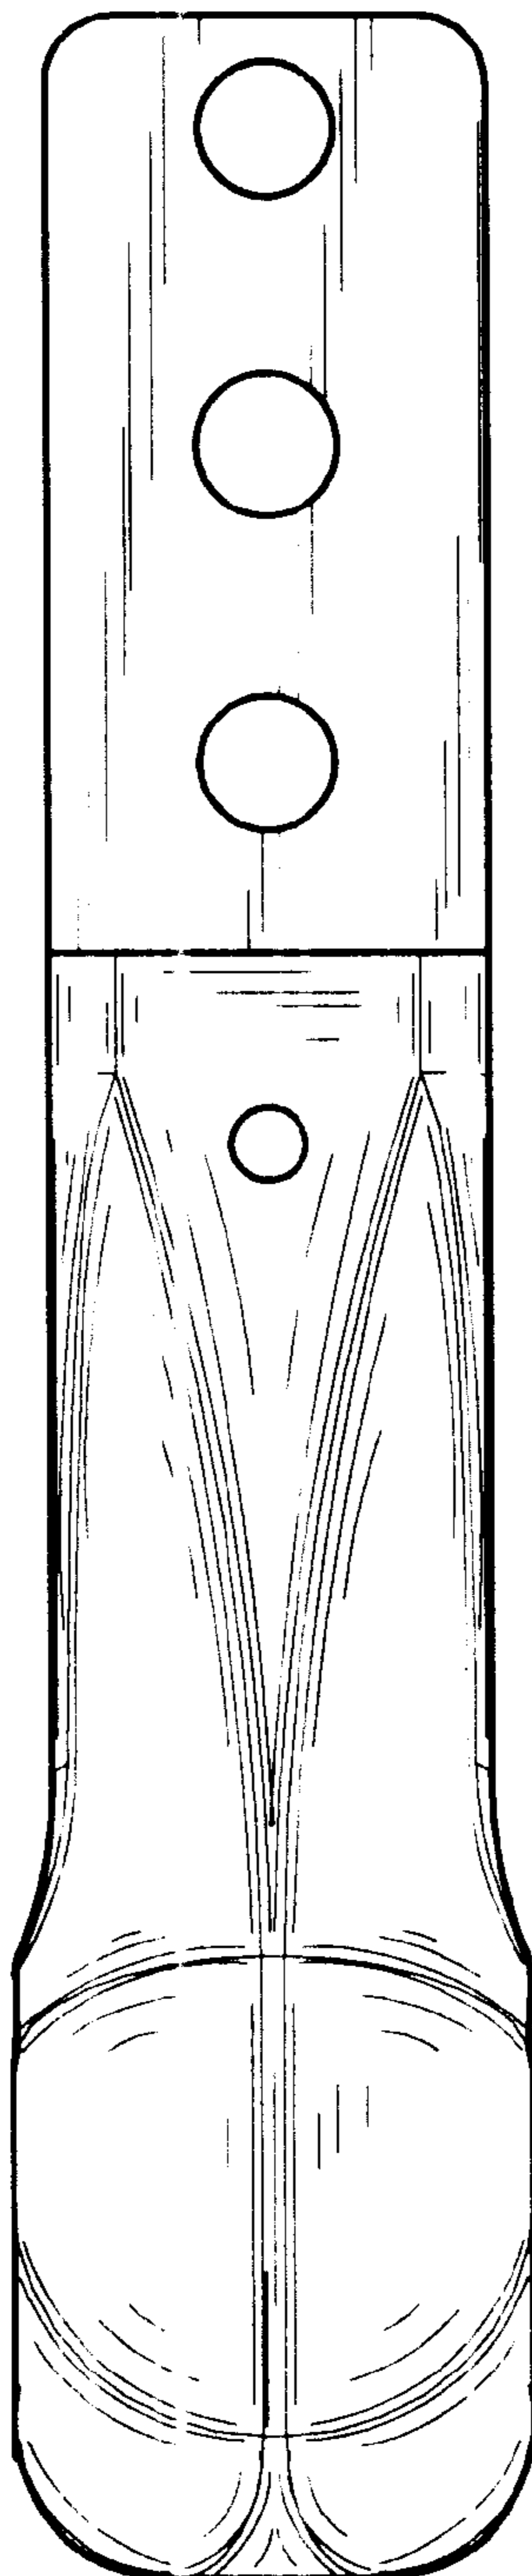


Fig.5

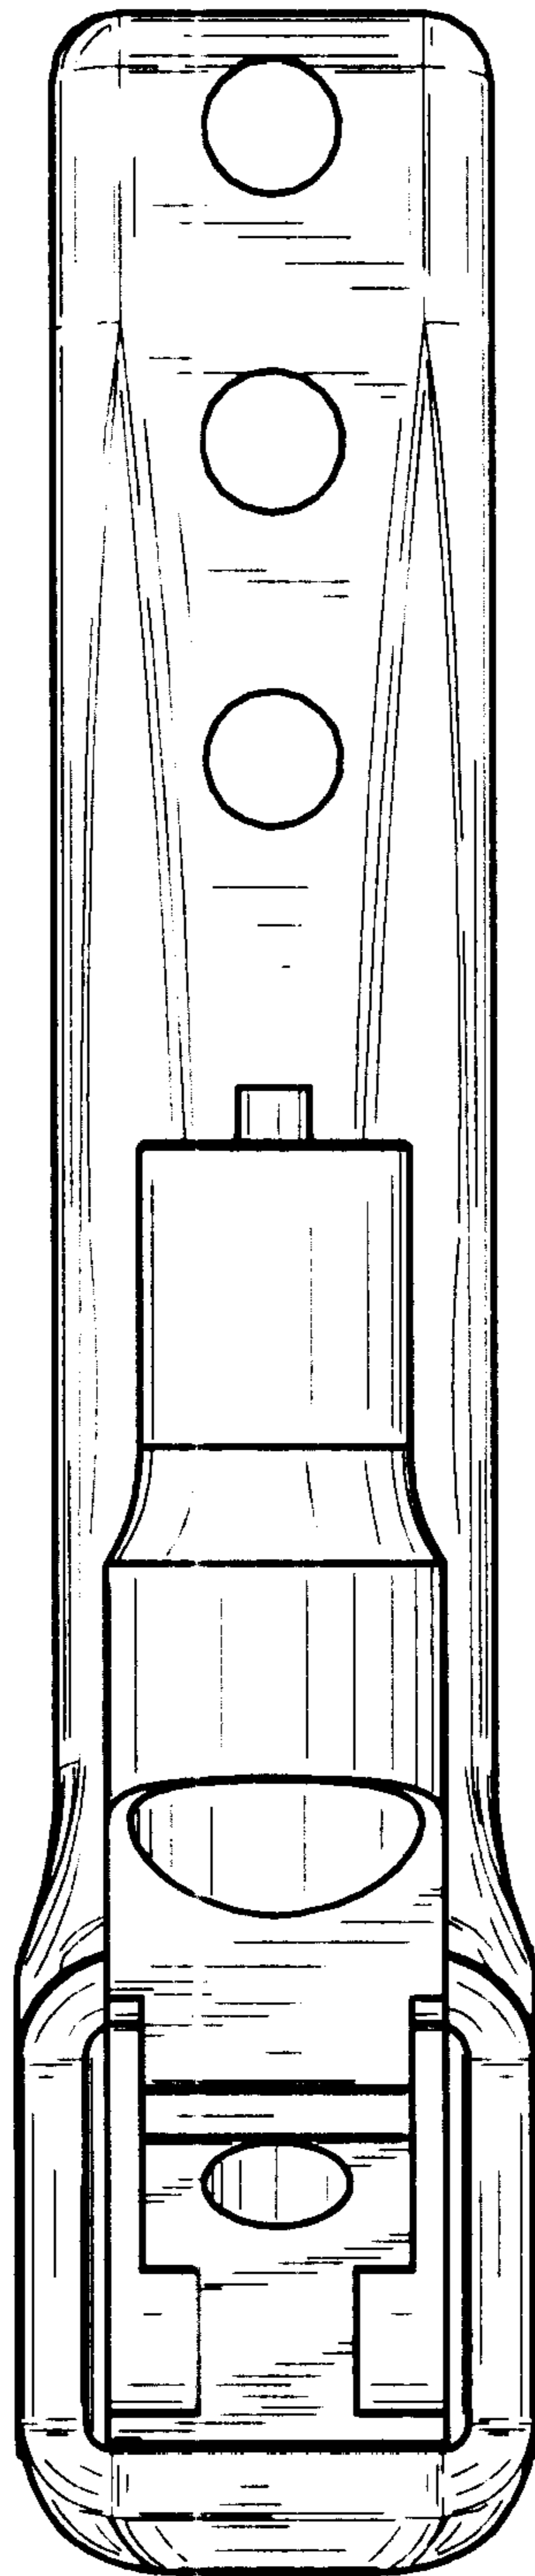


Fig.6