



US00D533664S

(12) **United States Design Patent** (10) **Patent No.:** **US D533,664 S**
Büttler et al. (45) **Date of Patent:** **** Dec. 12, 2006**

(54) **SURGICAL AIMING DEVICE**

(75) Inventors: **Markus Büttler**, Oensingen (CH);
André Schlienger, Arlesheim (CH);
Patrick Streff, Weil am Rhein (DE)

(73) Assignee: **HFSC Company**, West Chester, PA
(US)

(**) Term: **14 Years**

(21) Appl. No.: **29/209,625**

(22) Filed: **Jul. 19, 2004**

(30) **Foreign Application Priority Data**

Jan. 19, 2004 (CH) 130414

(51) **LOC (8) Cl.** **24-02**

(52) **U.S. Cl.** **D24/140; D24/133**

(58) **Field of Classification Search** D24/133,
D24/140, 146, 147; 606/62, 86-89, 96, 98
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

4,708,139 A * 11/1987 Dunbar, IV 606/96
4,923,458 A * 5/1990 Fischer 606/59
D357,534 S * 4/1995 Hayes D24/140
D359,557 S * 6/1995 Hayes D24/140

D466,609 S * 12/2002 Glossop D24/140
6,527,775 B1 * 3/2003 Warburton 606/62
D496,996 S * 10/2004 Jensen et al. D24/140
2004/0210232 A1 * 10/2004 Patel et al. 606/96
2005/0177171 A1 * 8/2005 Wtzler et al. 606/96

* cited by examiner

Primary Examiner—Antoine D. Davis

Assistant Examiner—Christopher Lee

(74) *Attorney, Agent, or Firm*—Jones Day

(57) **CLAIM**

The ornamental design for a surgical aiming device, as shown and described.

DESCRIPTION

In use, the surgical aiming device interacts with a basis for surgical aiming device, the details of which are shown and described in co-pending U.S. Design patent application No. 29/209,626, entitled Basis for Surgical Aiming Device, filed on even date herewith, the entire disclosure of which is incorporated herein by reference.

FIG. 1 is a perspective view of the surgical aiming device;

FIG. 2 is top view of the surgical aiming device;


FIG. 3 is a right side view of the surgical aiming device;

FIG. 4 is a left side view of the surgical aiming device;

FIG. 5 is a rear view of the surgical aiming device; and,

FIG. 6 is a front view of the surgical aiming device.

1 Claim, 6 Drawing Sheets

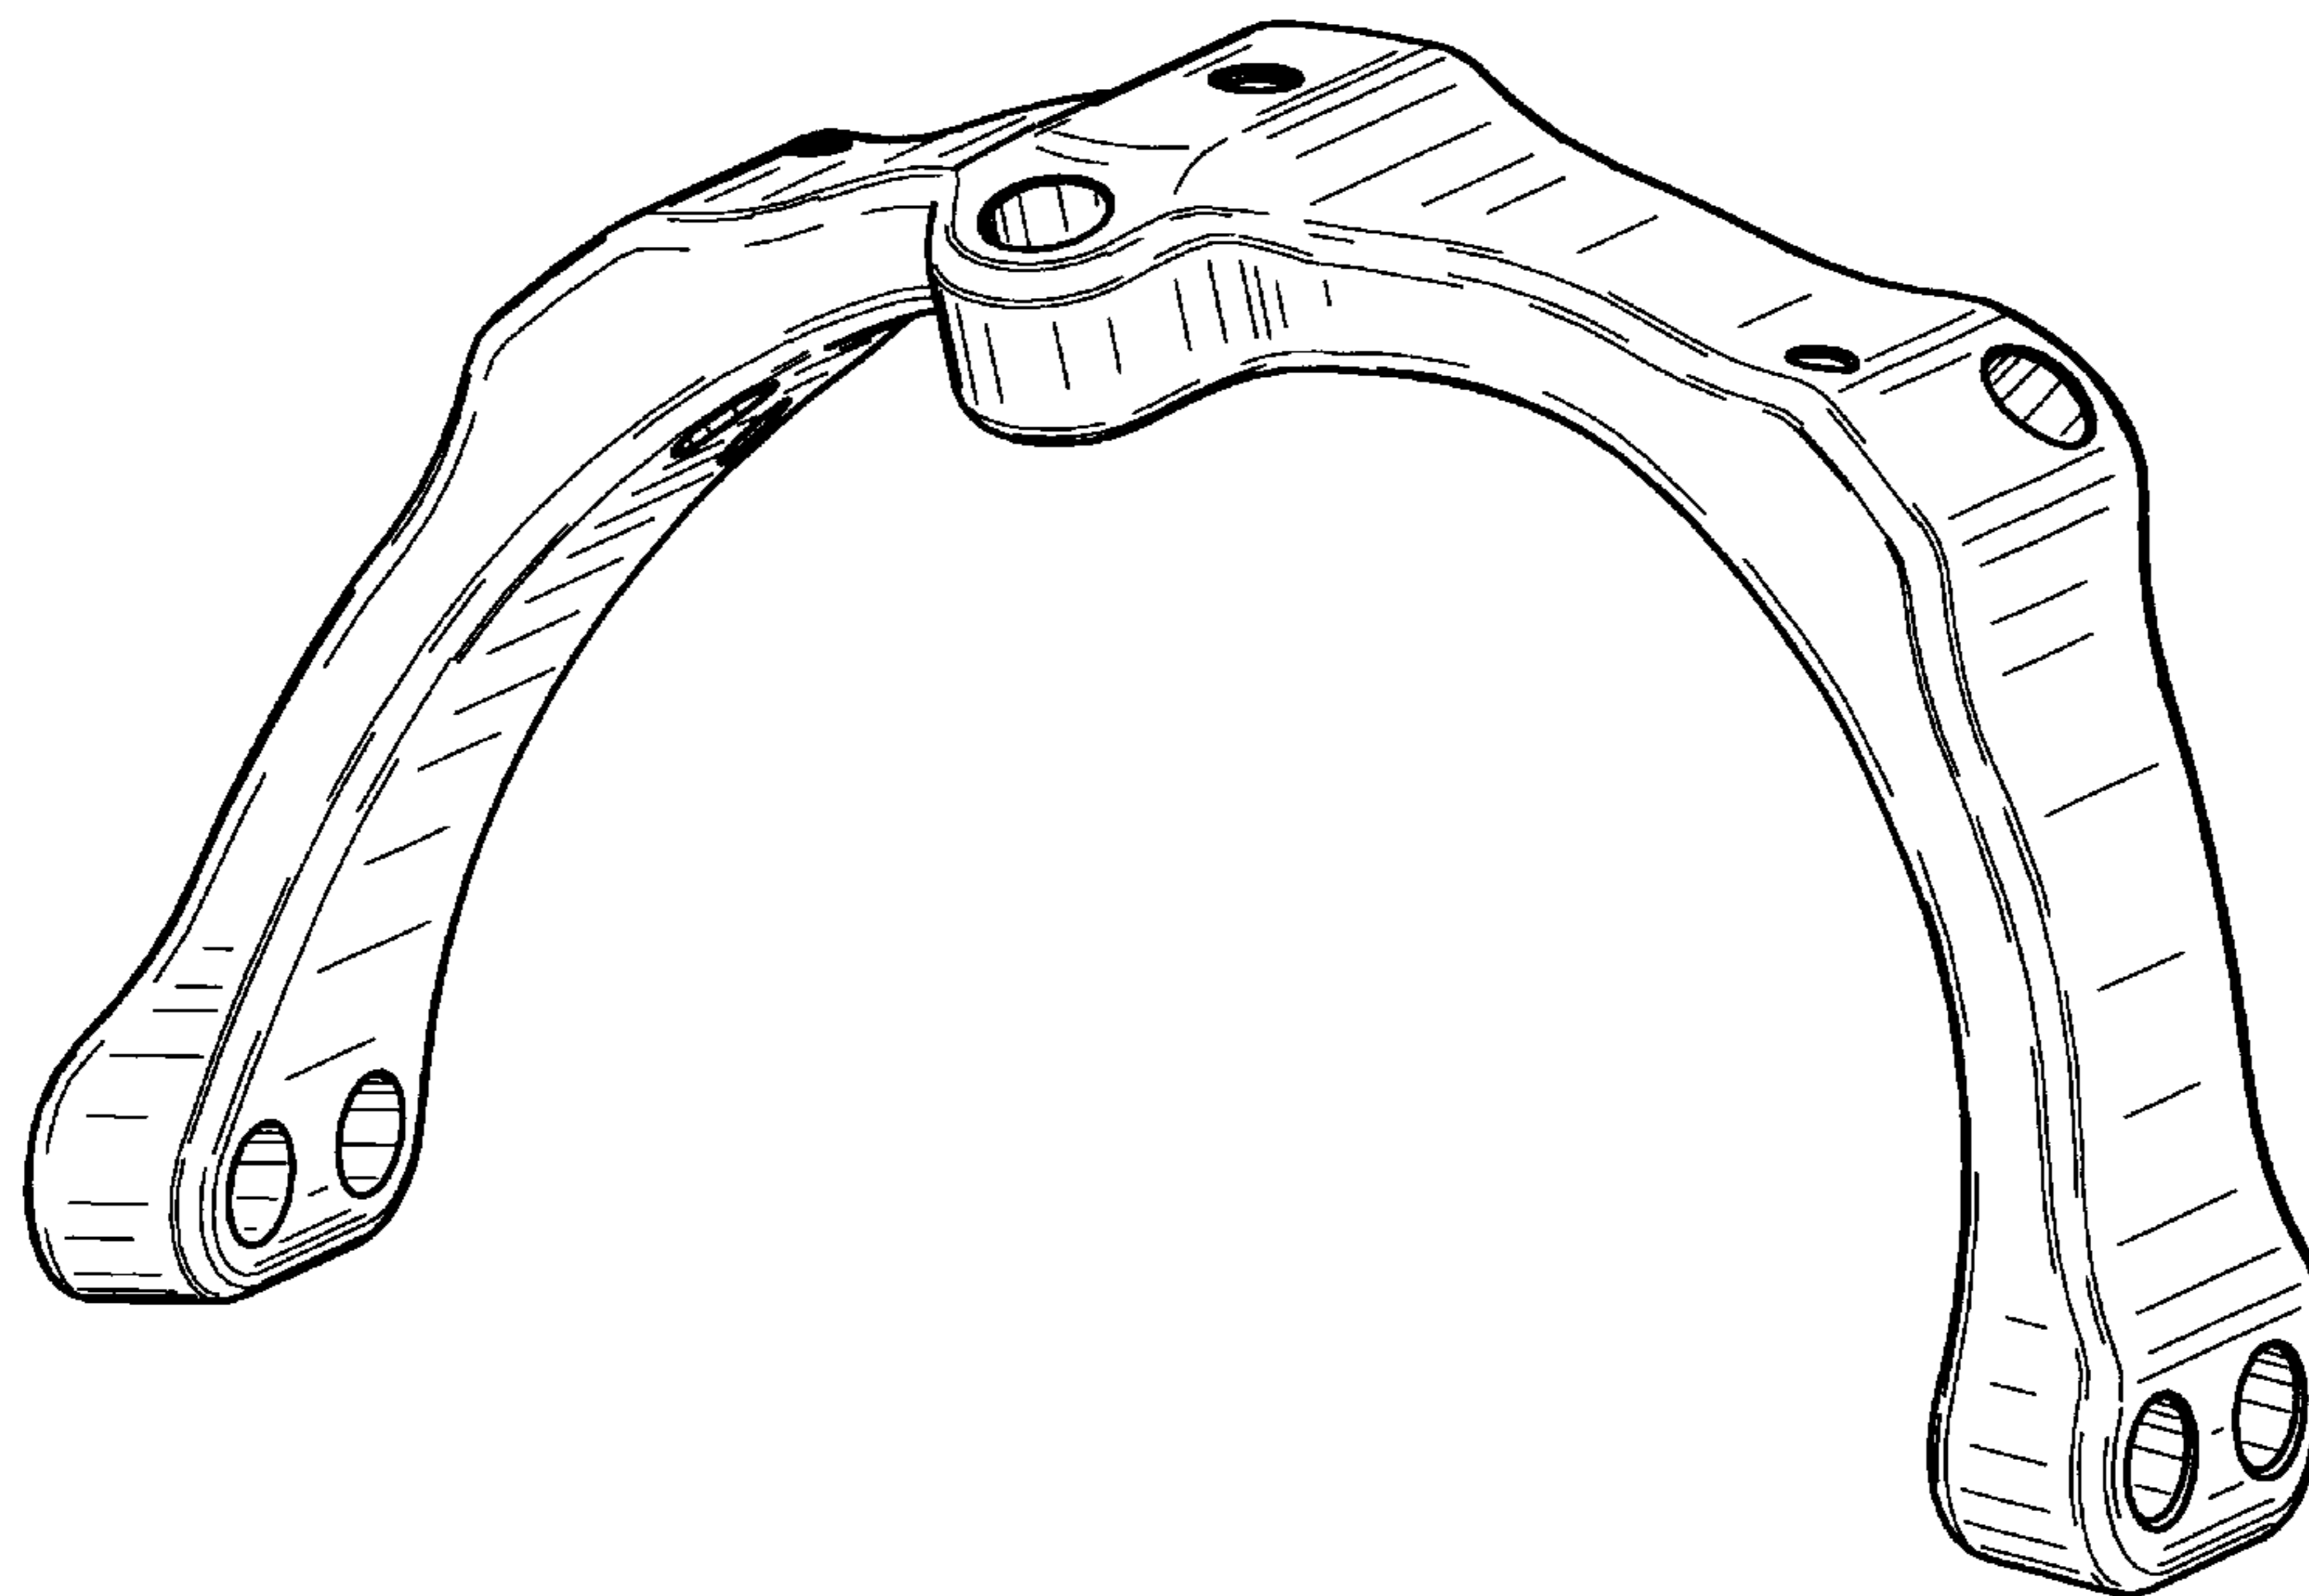

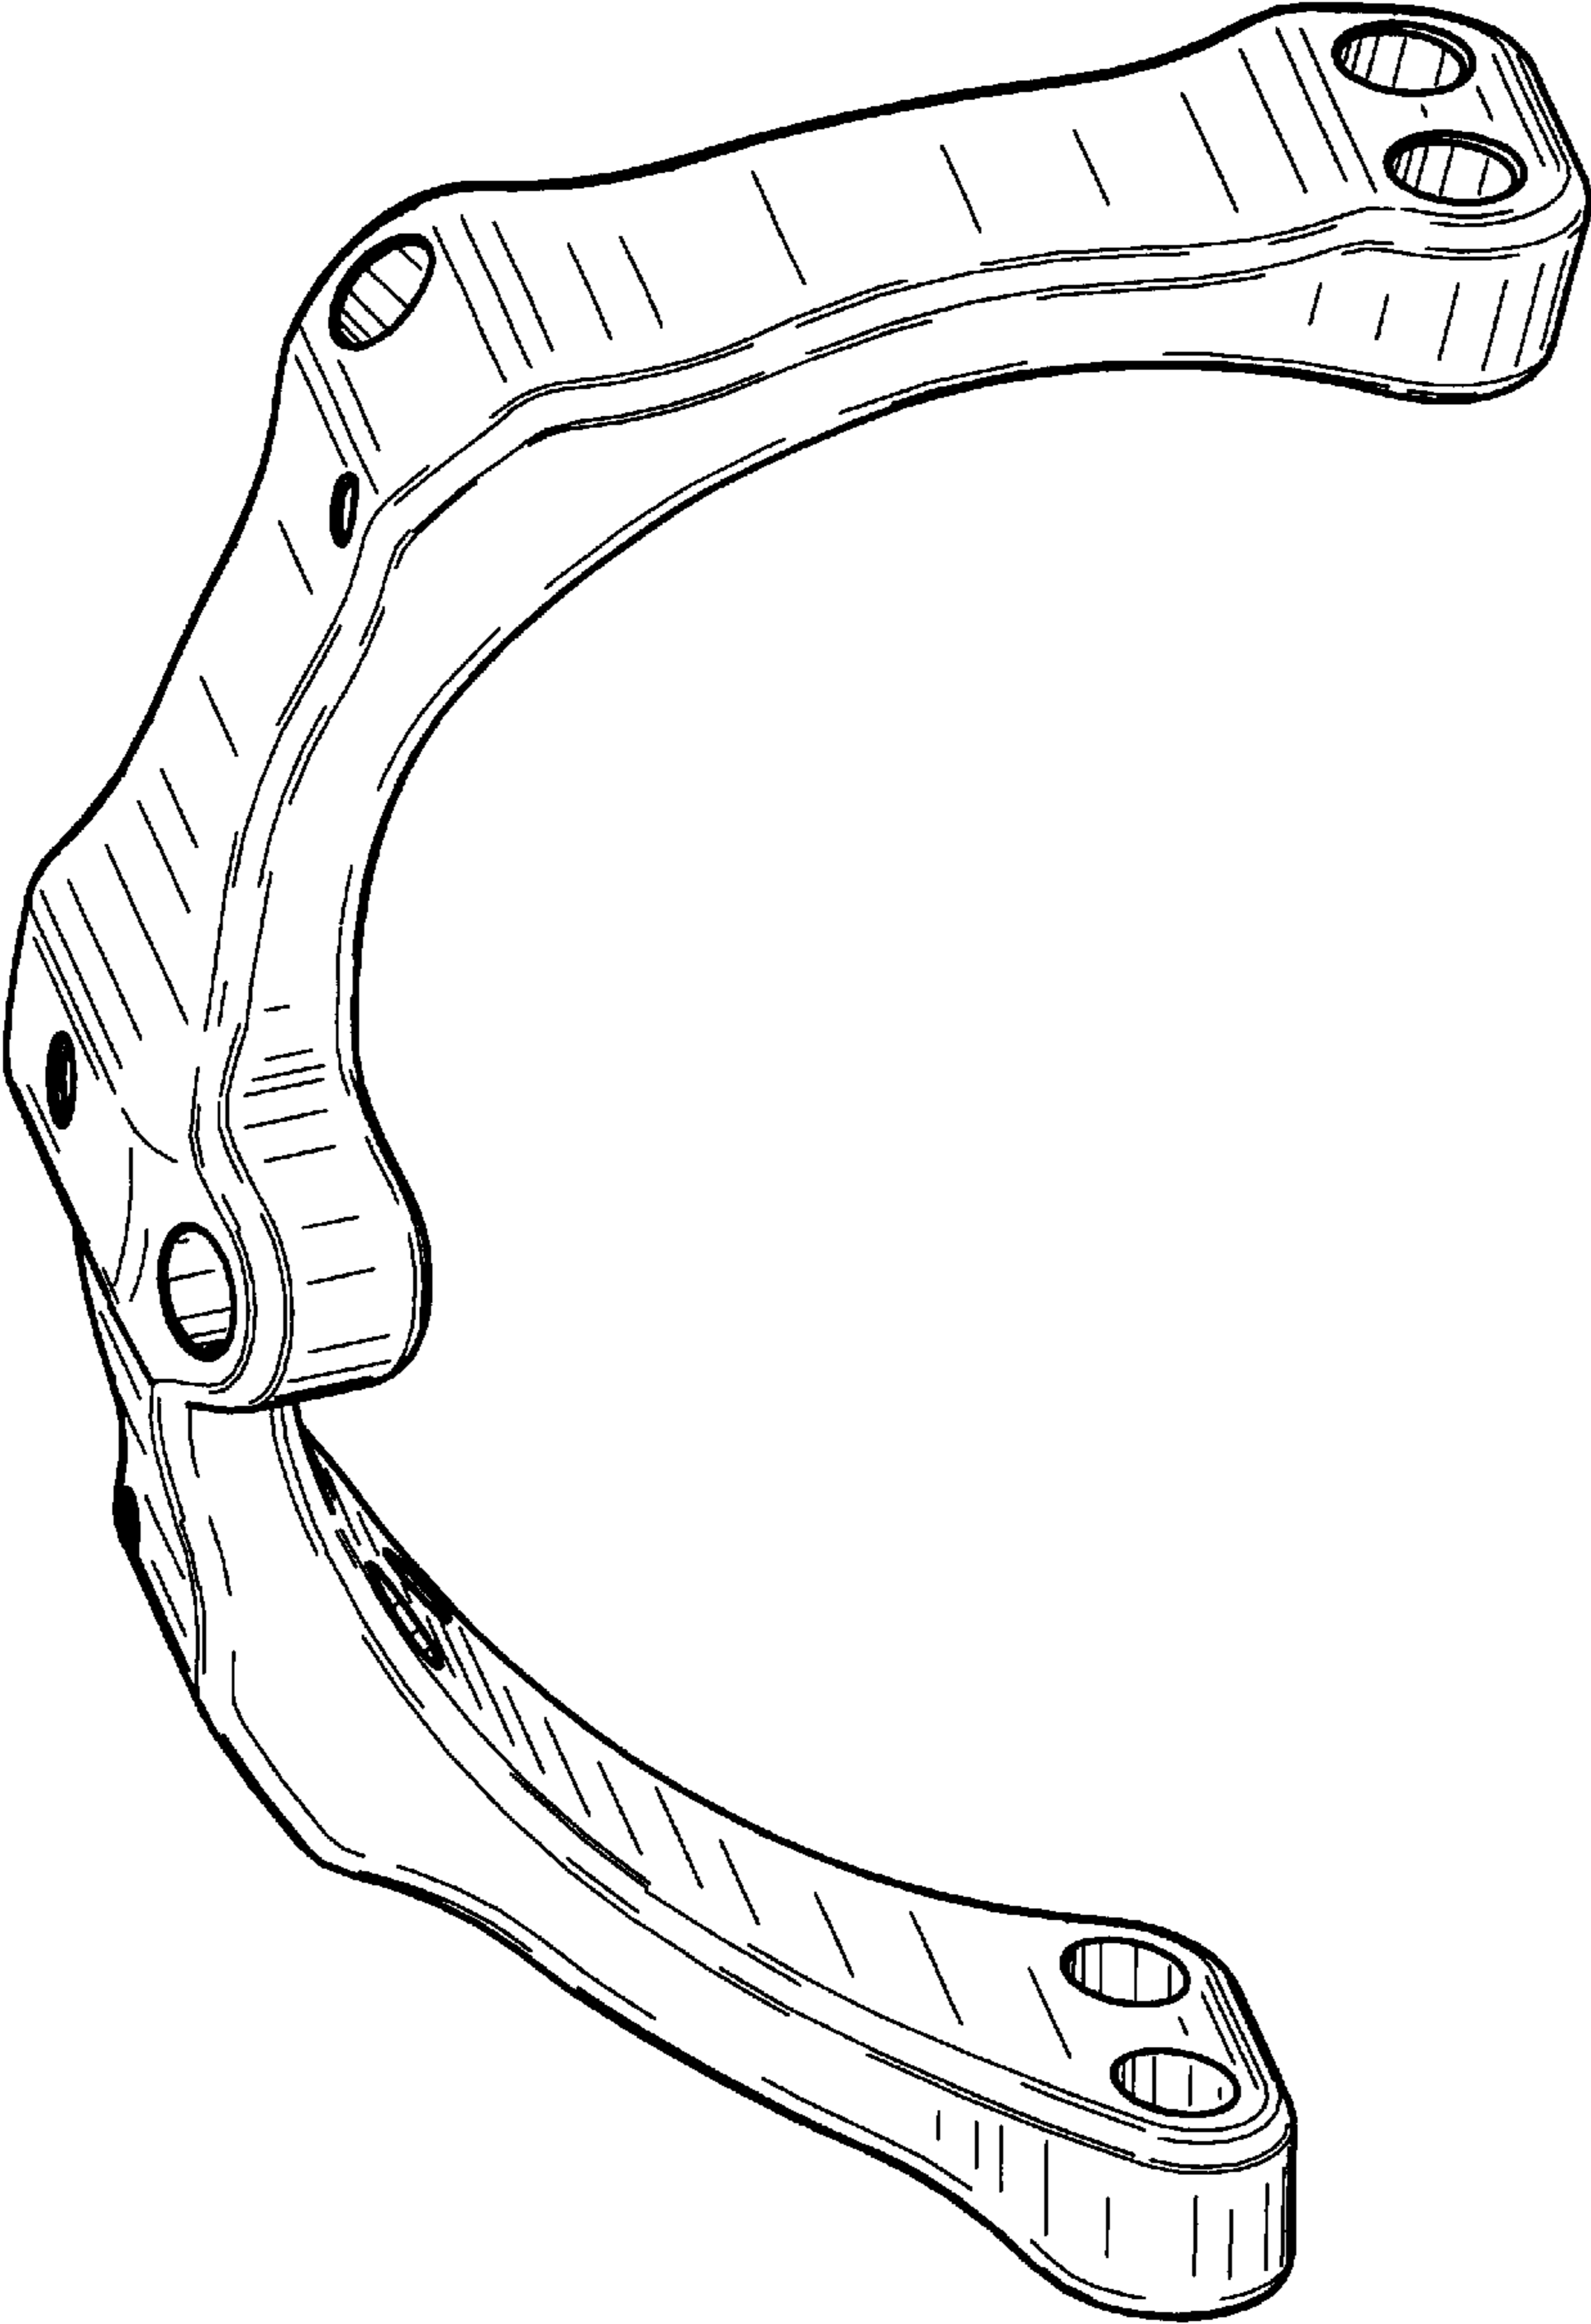


FIG. 1

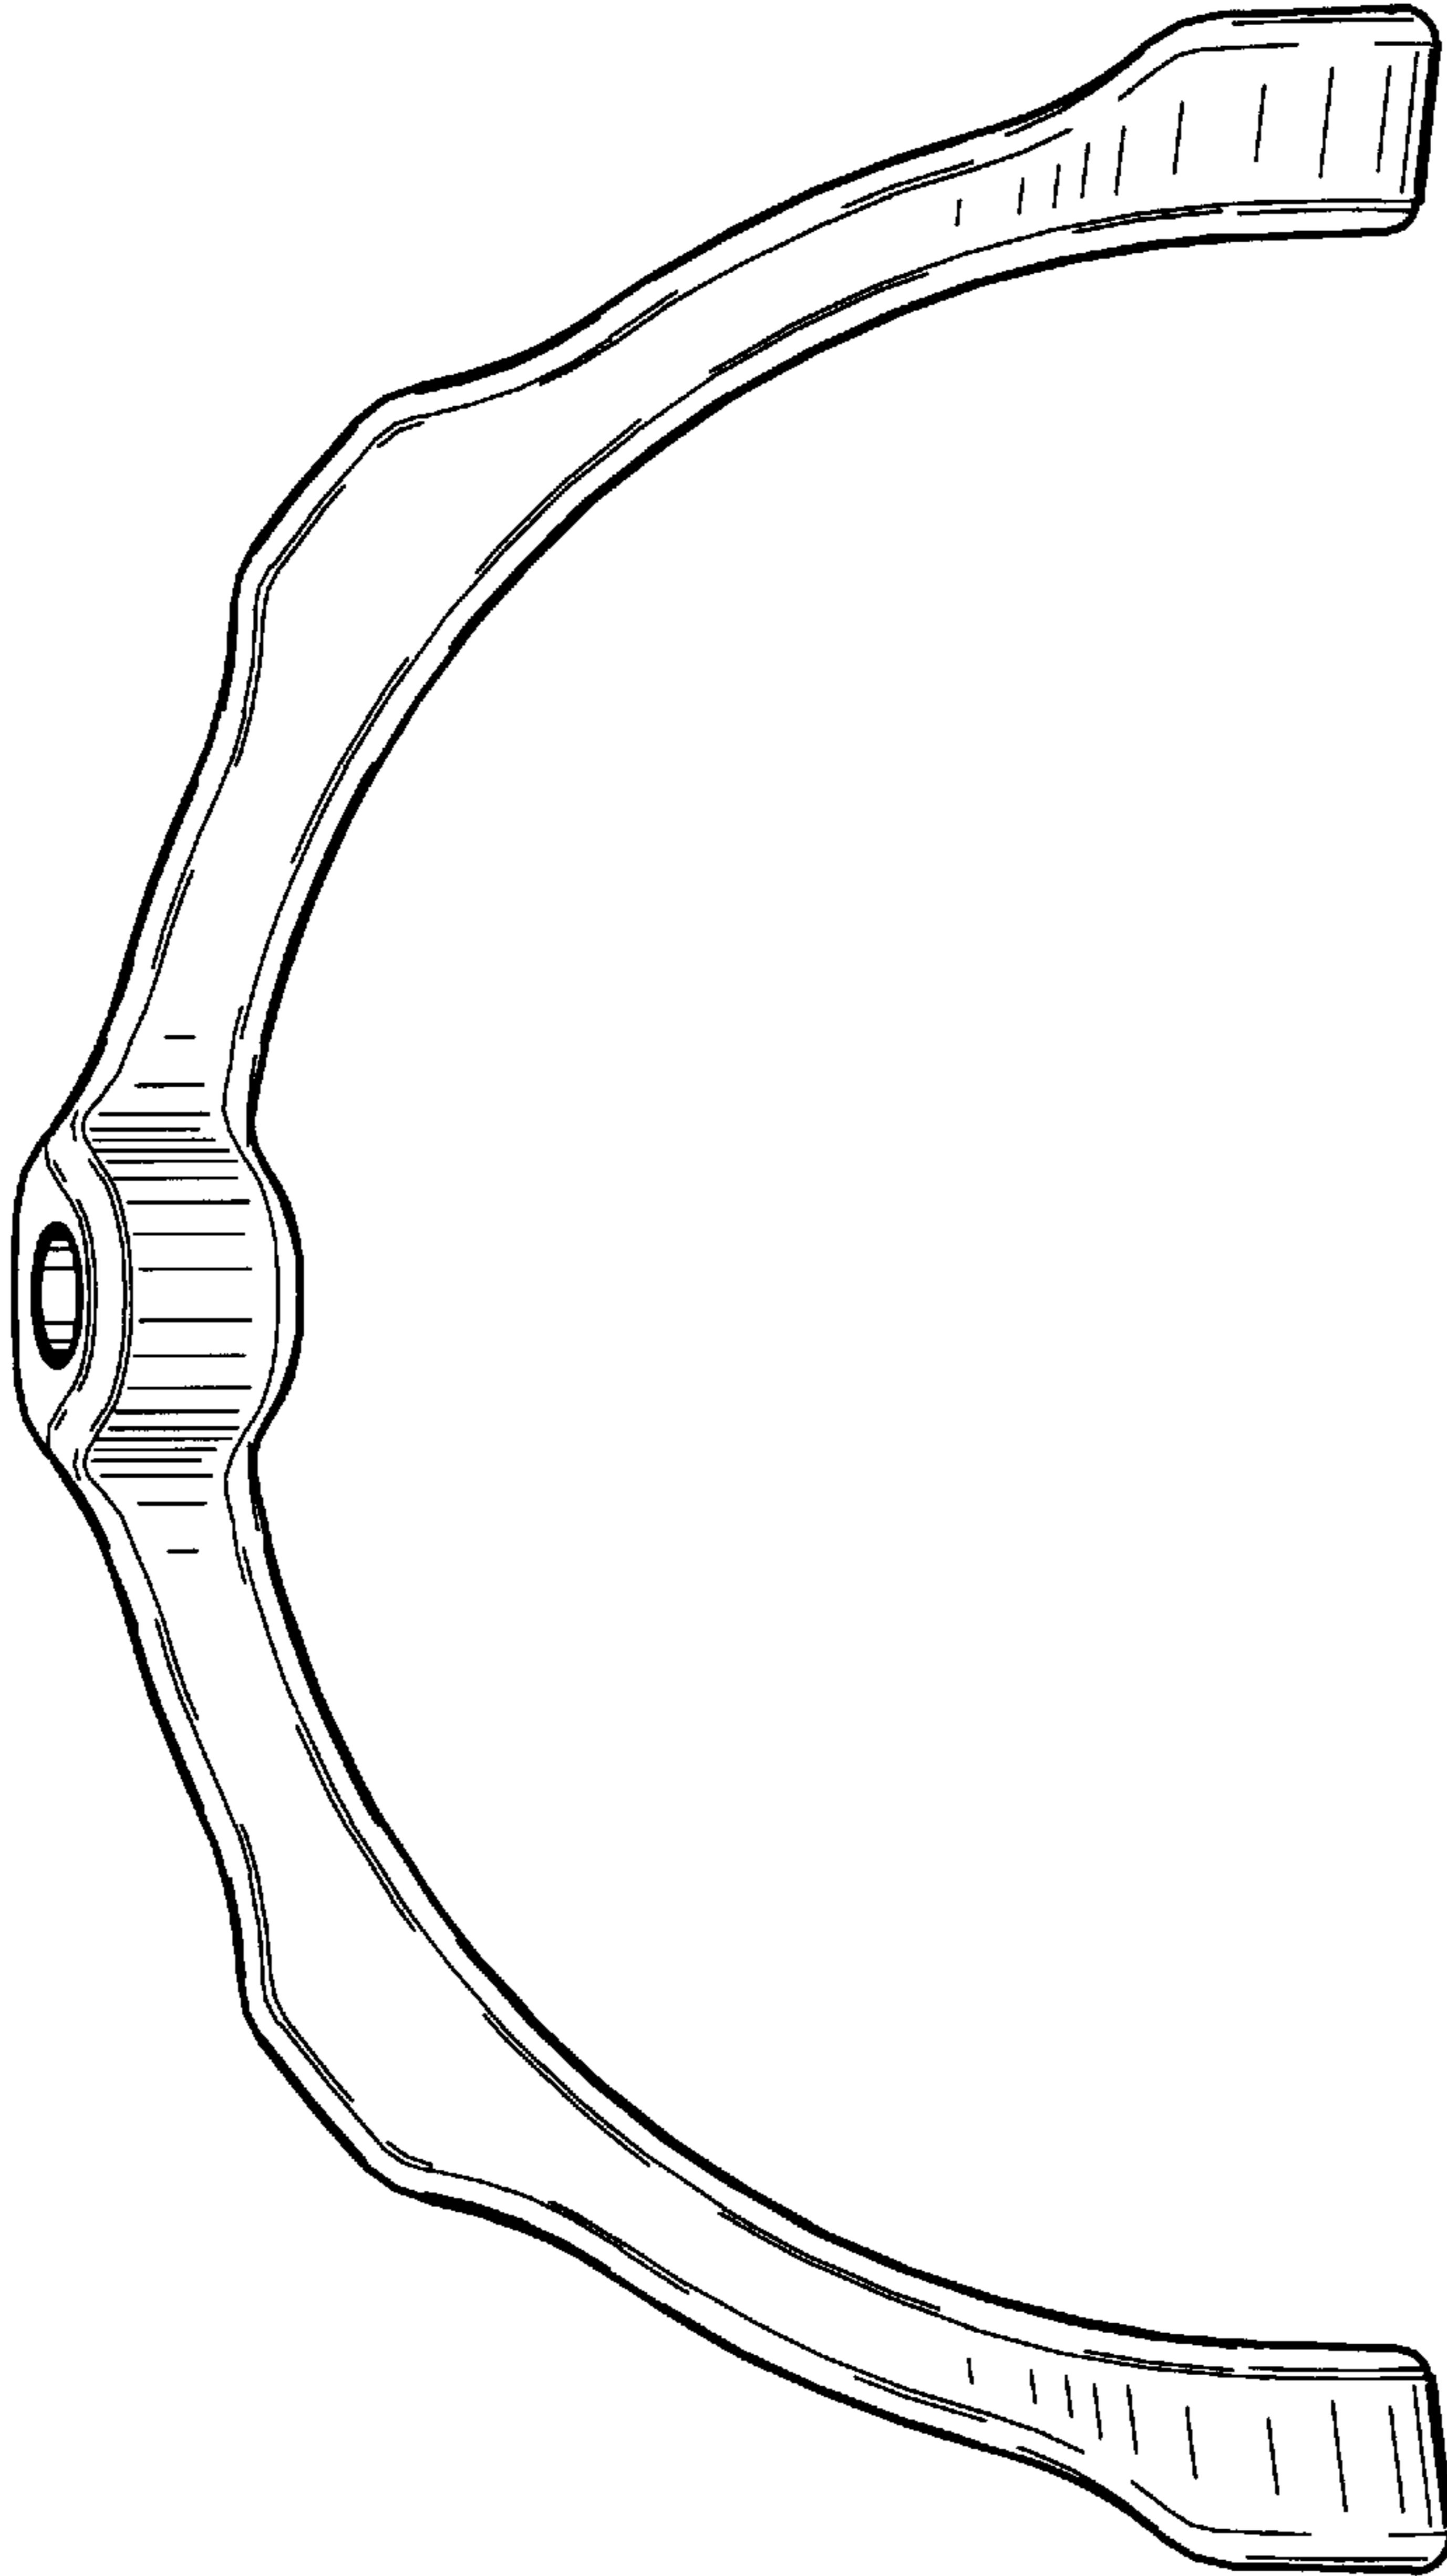


FIG. 2

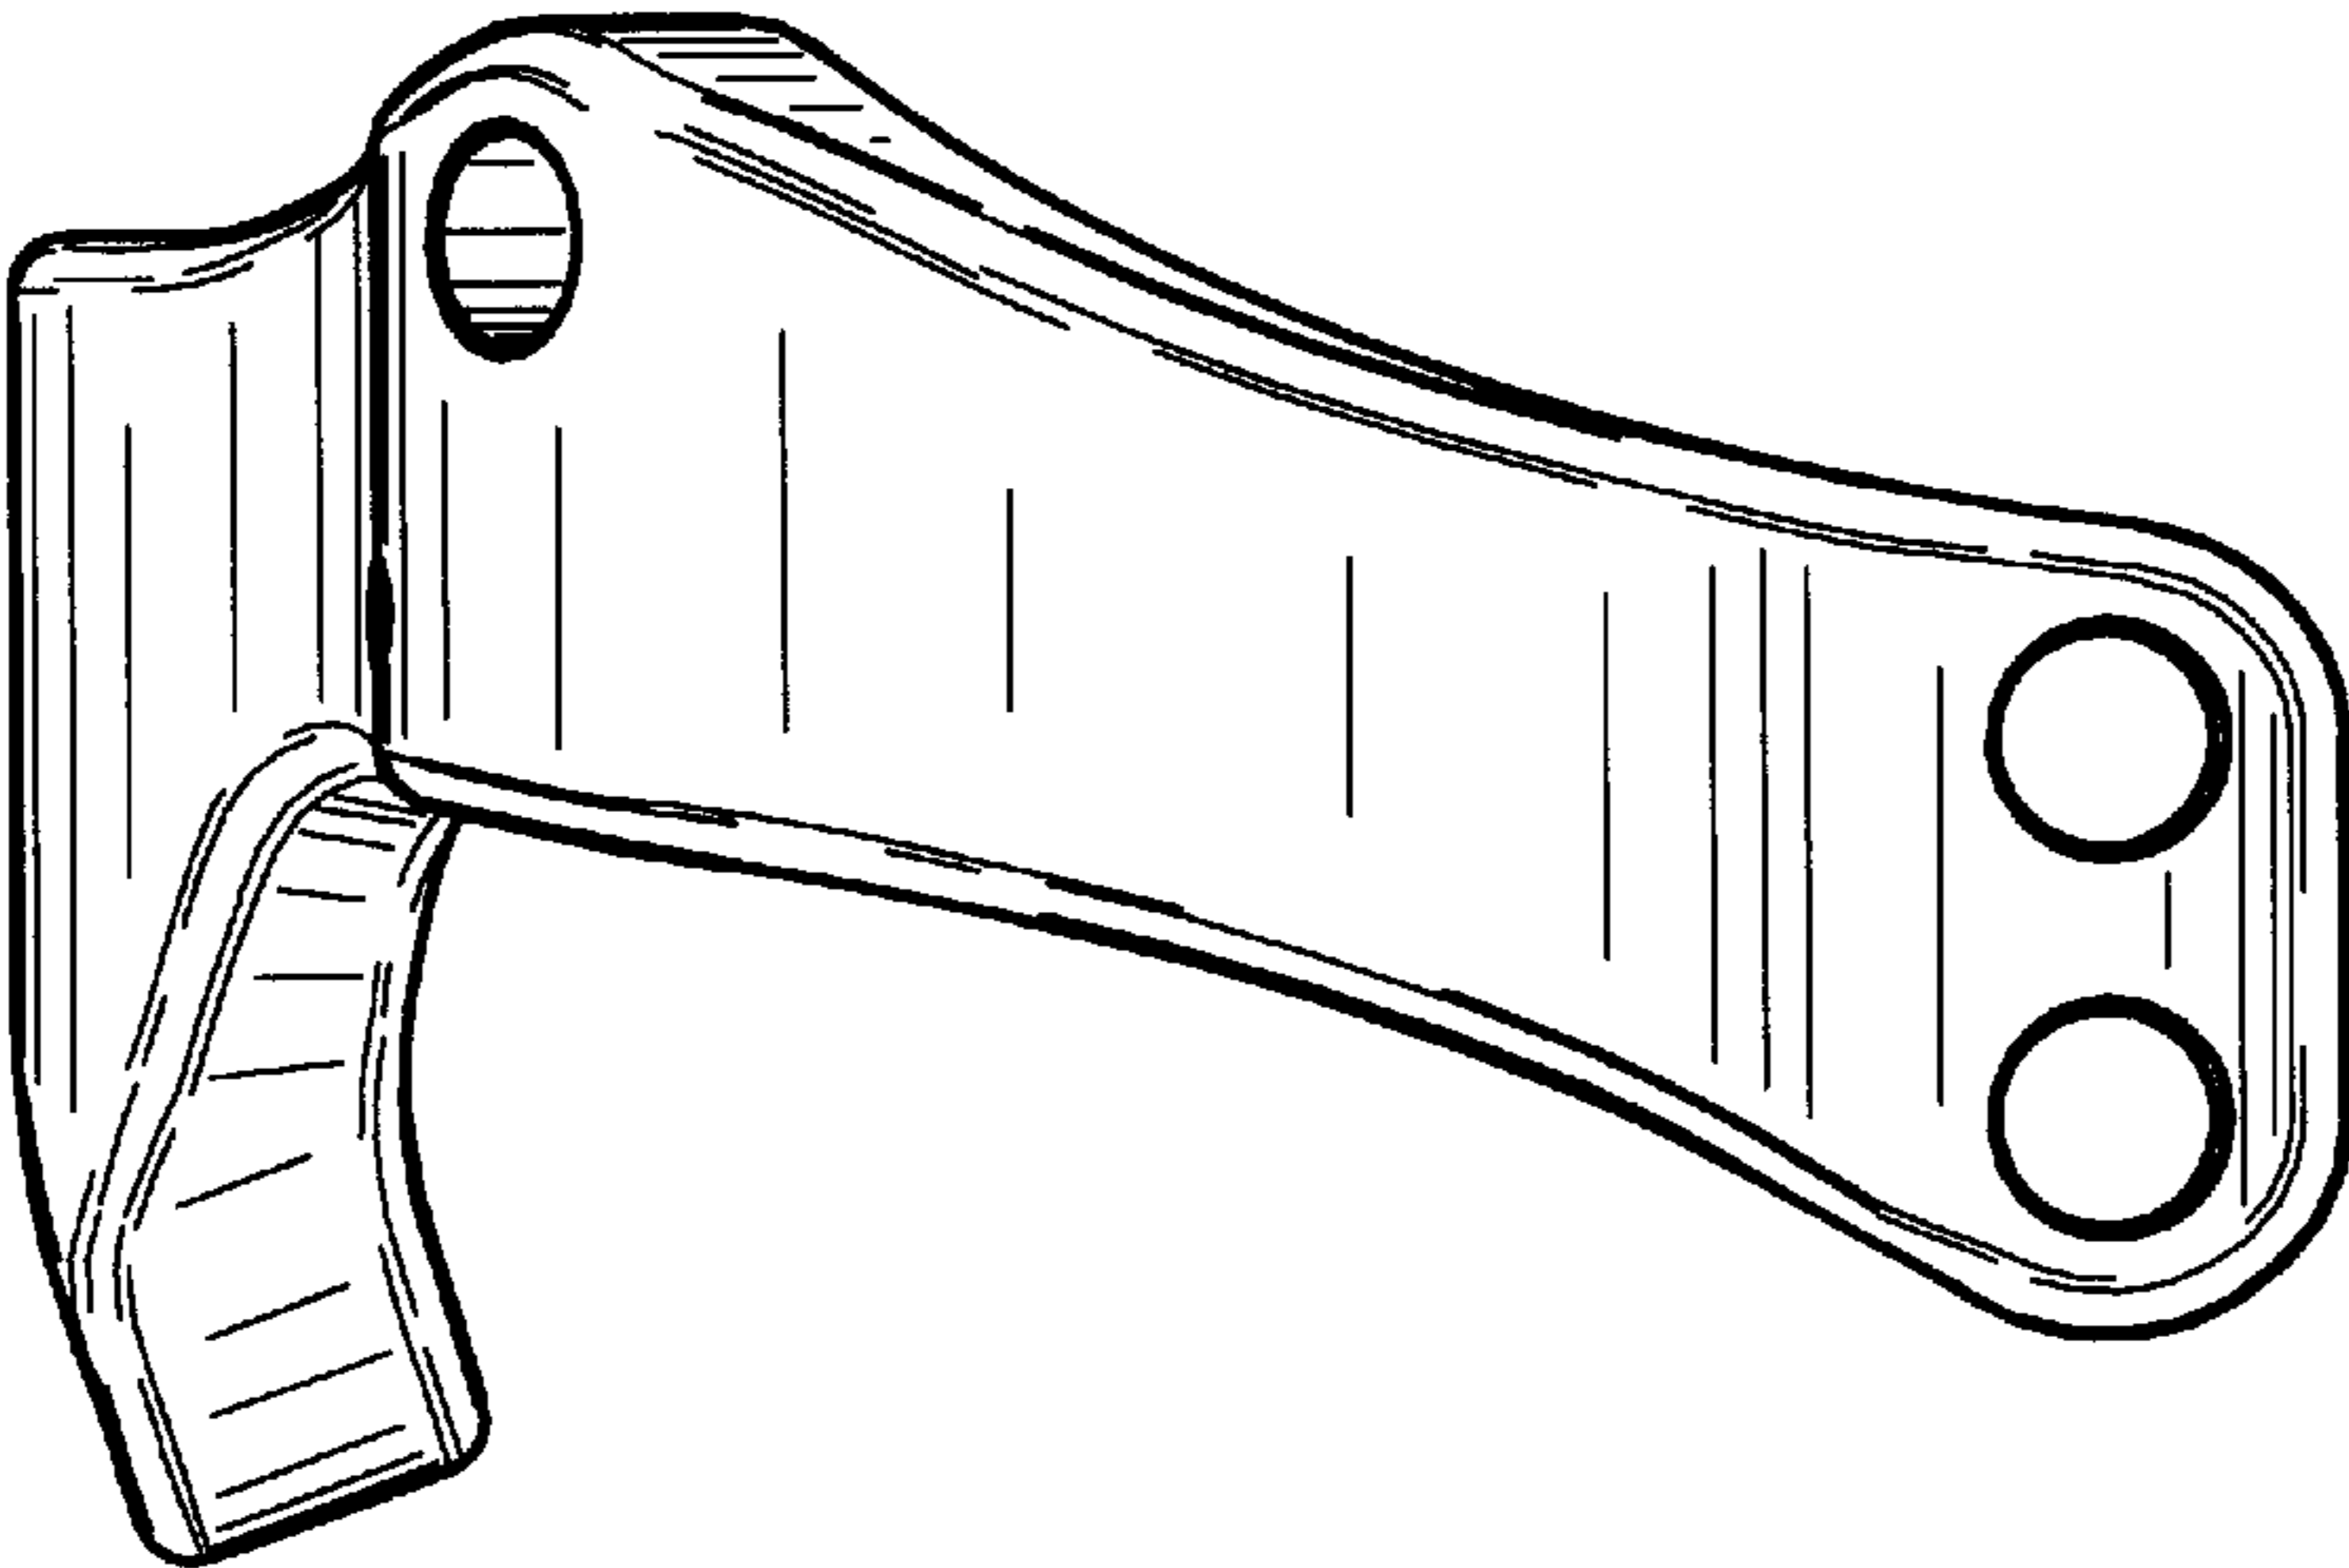


FIG. 3

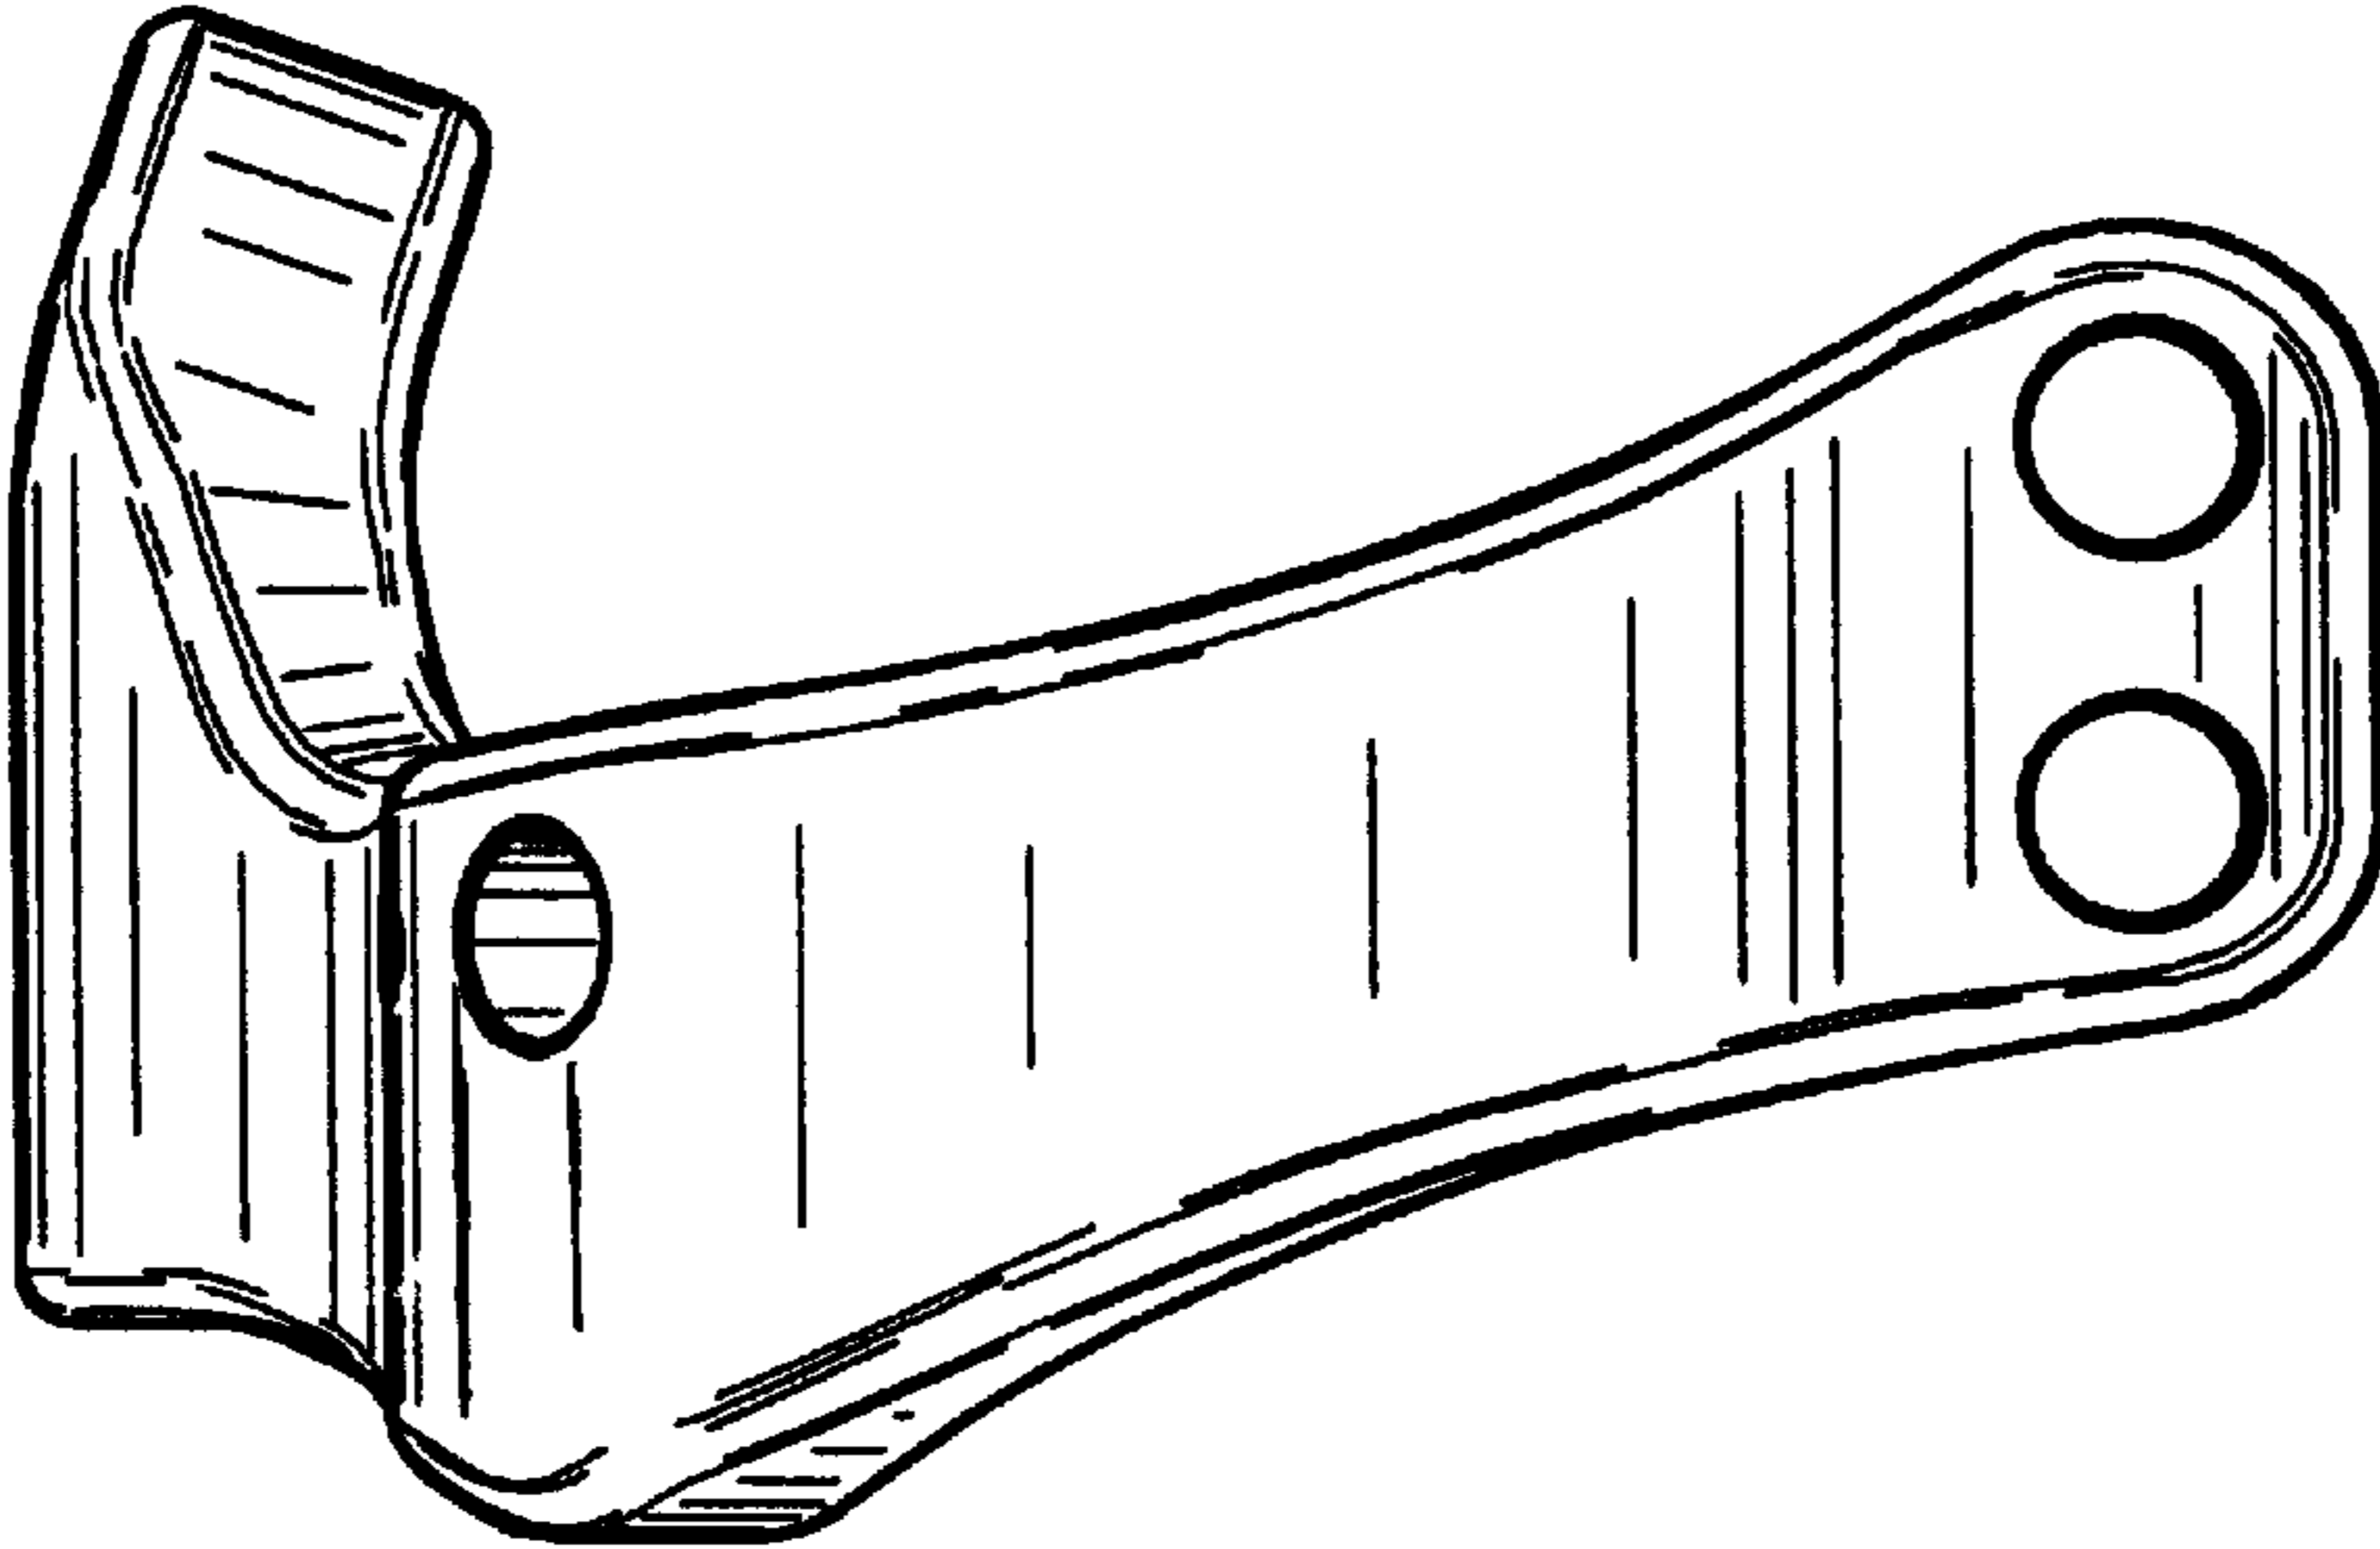


FIG. 4

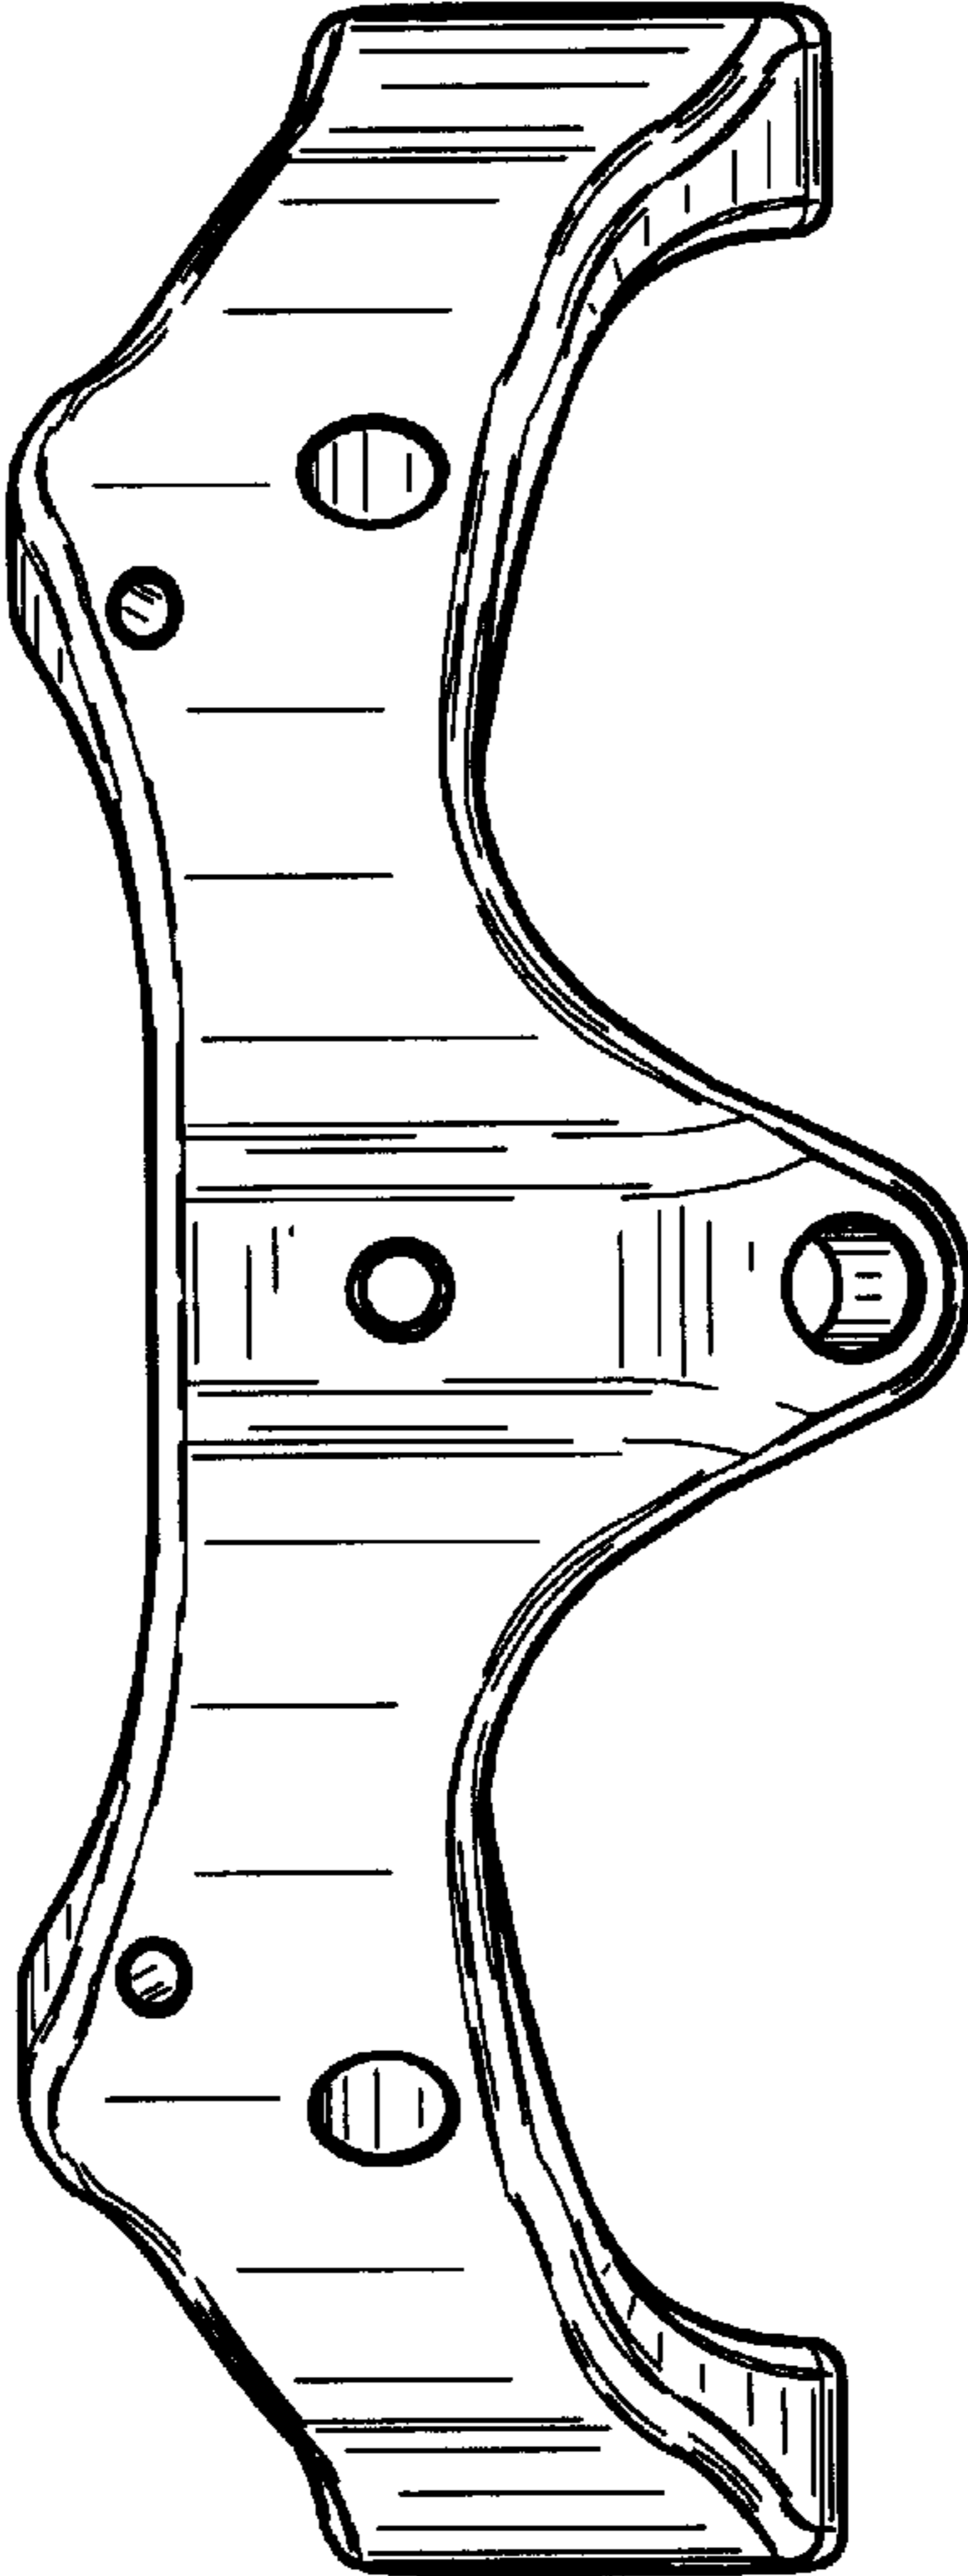


FIG. 5

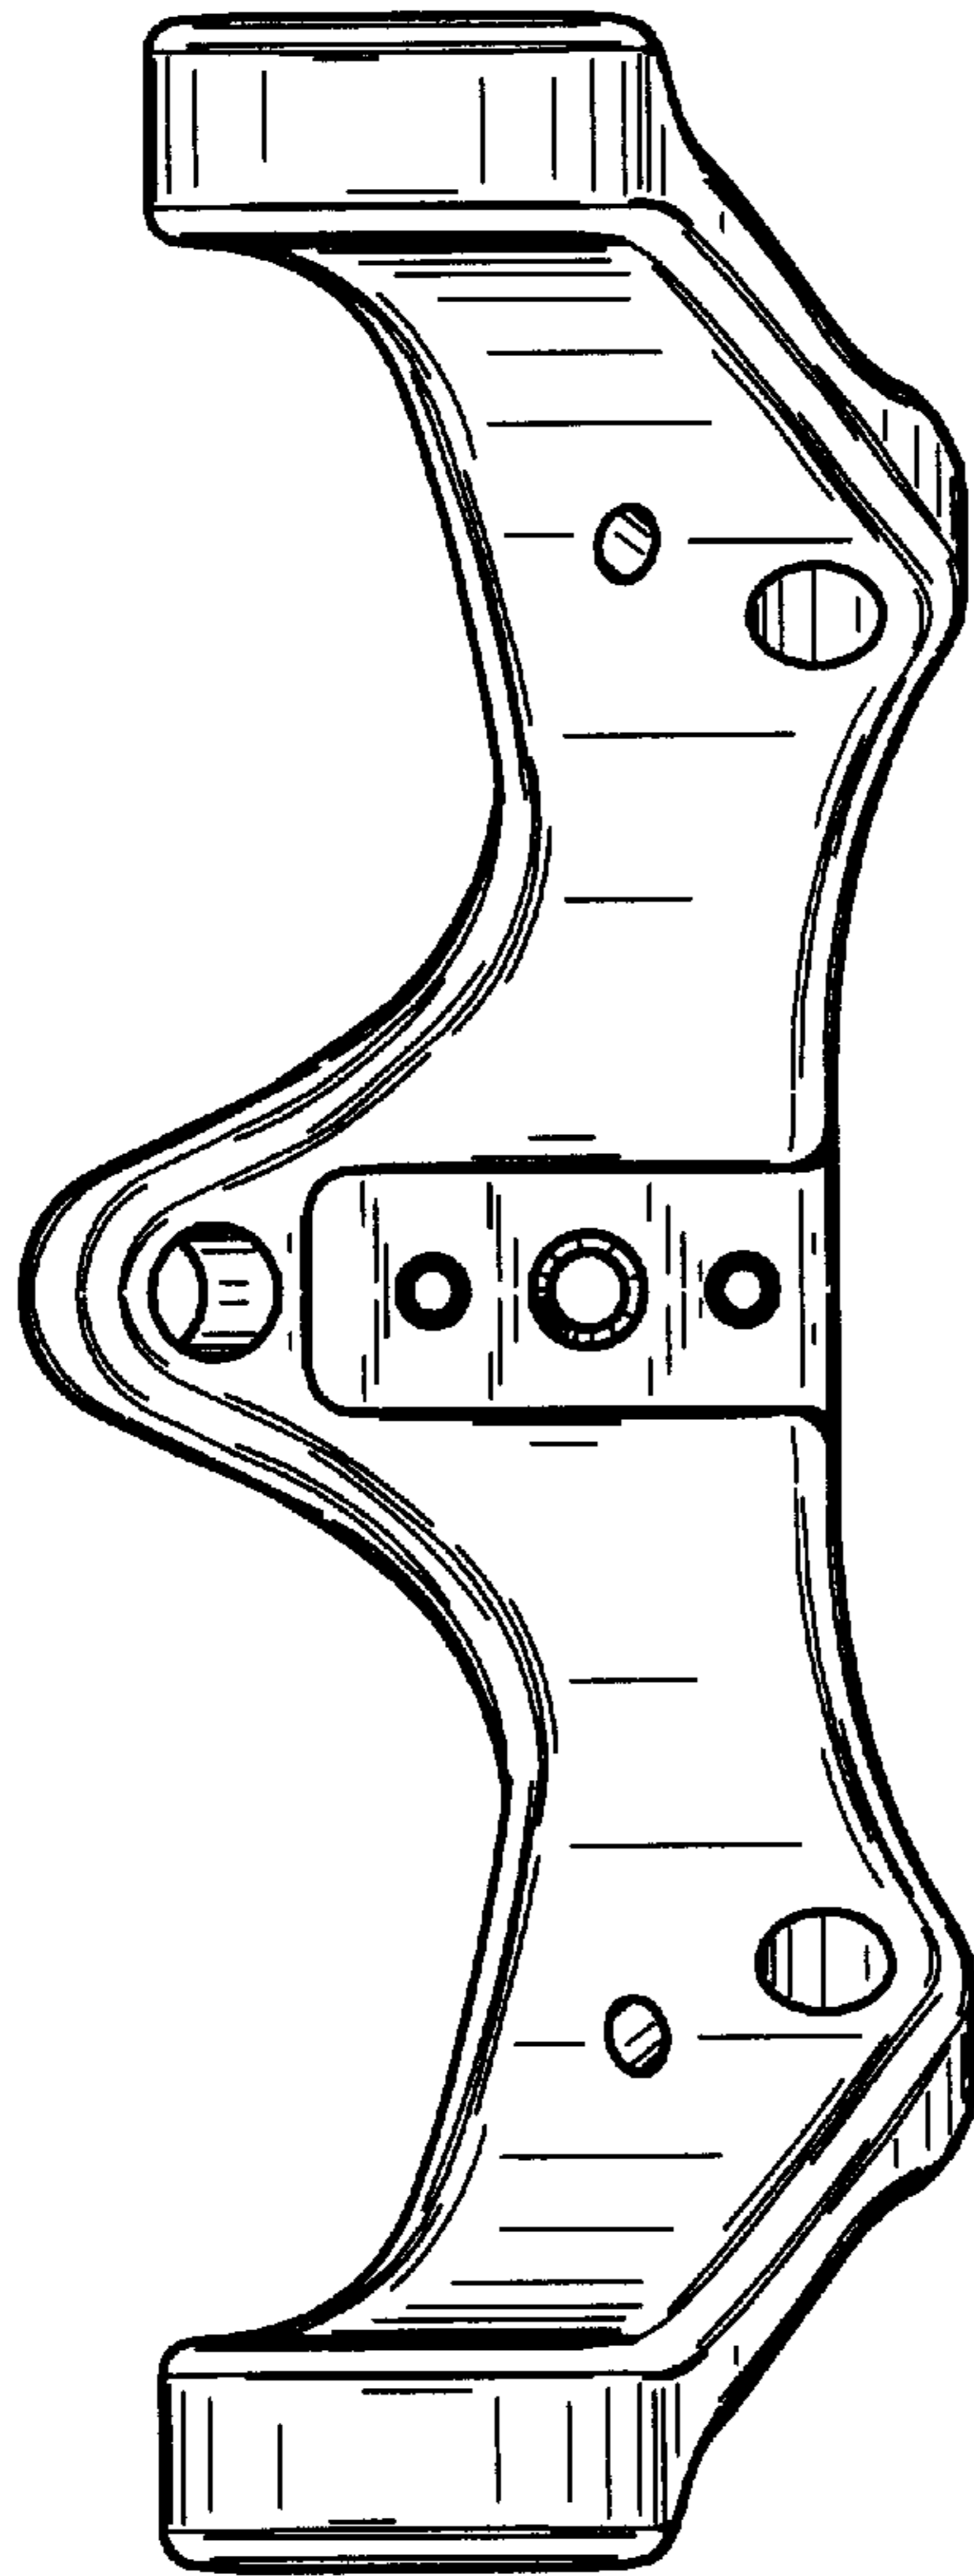


FIG. 6