



US00D536793S

(12) **United States Design Patent**
Assad et al.

(10) **Patent No.:** **US D536,793 S**
(45) **Date of Patent:** **** Feb. 13, 2007**

(54) **REMOTE PATIENT MANAGEMENT
COMMUNICATION DEVICE**

(75) Inventors: **Fareed Assad**, Minneapolis, MN (US);
Blair Erbstoesz, Kirkland, WA (US);
Benjamin L. Somberg, Shoreview, MN
(US); **Kimberly Gerst**, Eden Prairie,
MN (US); **Christian Richard Trifilio**,
St. Paul, MN (US)

(73) Assignee: **Cardiac Pacemakers, Inc.**, St. Paul,
MN (US)

(**) Term: **14 Years**

(21) Appl. No.: **29/220,252**

(22) Filed: **Dec. 28, 2004**

(51) **LOC (8) Cl.** **24-01**

(52) **U.S. Cl.** **D24/185**

(58) **Field of Classification Search** D24/185,
D24/186, 165; 600/502, 503, 499, 481, 484,
600/513, 485, 500, 480, 495, 479, 519, 528,
600/532, 538, 549, 300-301; D14/336

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D414,870 S * 10/1999 Saltzstein et al. D24/186
D427,315 S * 6/2000 Saltzstein et al. D24/186
D446,306 S * 8/2001 Ochi et al. D24/186
D459,813 S * 7/2002 Ramsey, III D24/186
D468,735 S * 1/2003 Landerholm et al. D14/336
6,575,904 B2 * 6/2003 Nagai et al. 600/301

D490,516 S * 5/2004 Takahashi et al. D24/186
6,771,172 B1 * 8/2004 Robinson et al. 600/301
D508,565 S * 8/2005 Nephin et al. D24/186
6,930,602 B2 * 8/2005 Villaseca et al. 600/301
D510,625 S * 10/2005 Widener et al. D24/186
6,985,869 B1 * 1/2006 Stoll et al. 600/301
D520,638 S * 5/2006 Zeindler D24/166

* cited by examiner

Primary Examiner—Louis S. Zarfes

Assistant Examiner—Daniel Yu

(74) *Attorney, Agent, or Firm*—Schwegman, Lundberg,
Woessner & Kluth, P.A.

(57) **CLAIM**

The ornamental design for a remote patient management
communication device, as shown and described.

DESCRIPTION

FIG. 1 is a perspective view of a remote patient management
communication device according to the present invention.

FIG. 2 is a front view of the remote patient management
communication device of FIG. 1.

FIG. 3 is a rear view of the remote patient management
communication device of FIG. 1.

FIG. 4 is a first side view of the remote patient management
communication device of FIG. 1.

FIG. 5 is a second side view of the remote patient manage-
ment communication device of FIG. 1.

FIG. 6 is a top view of the remote patient management
communication device of FIG. 1; and,

FIG. 7 is a bottom view of the remote patient management
communication device of FIG. 1.

1 Claim, 4 Drawing Sheets

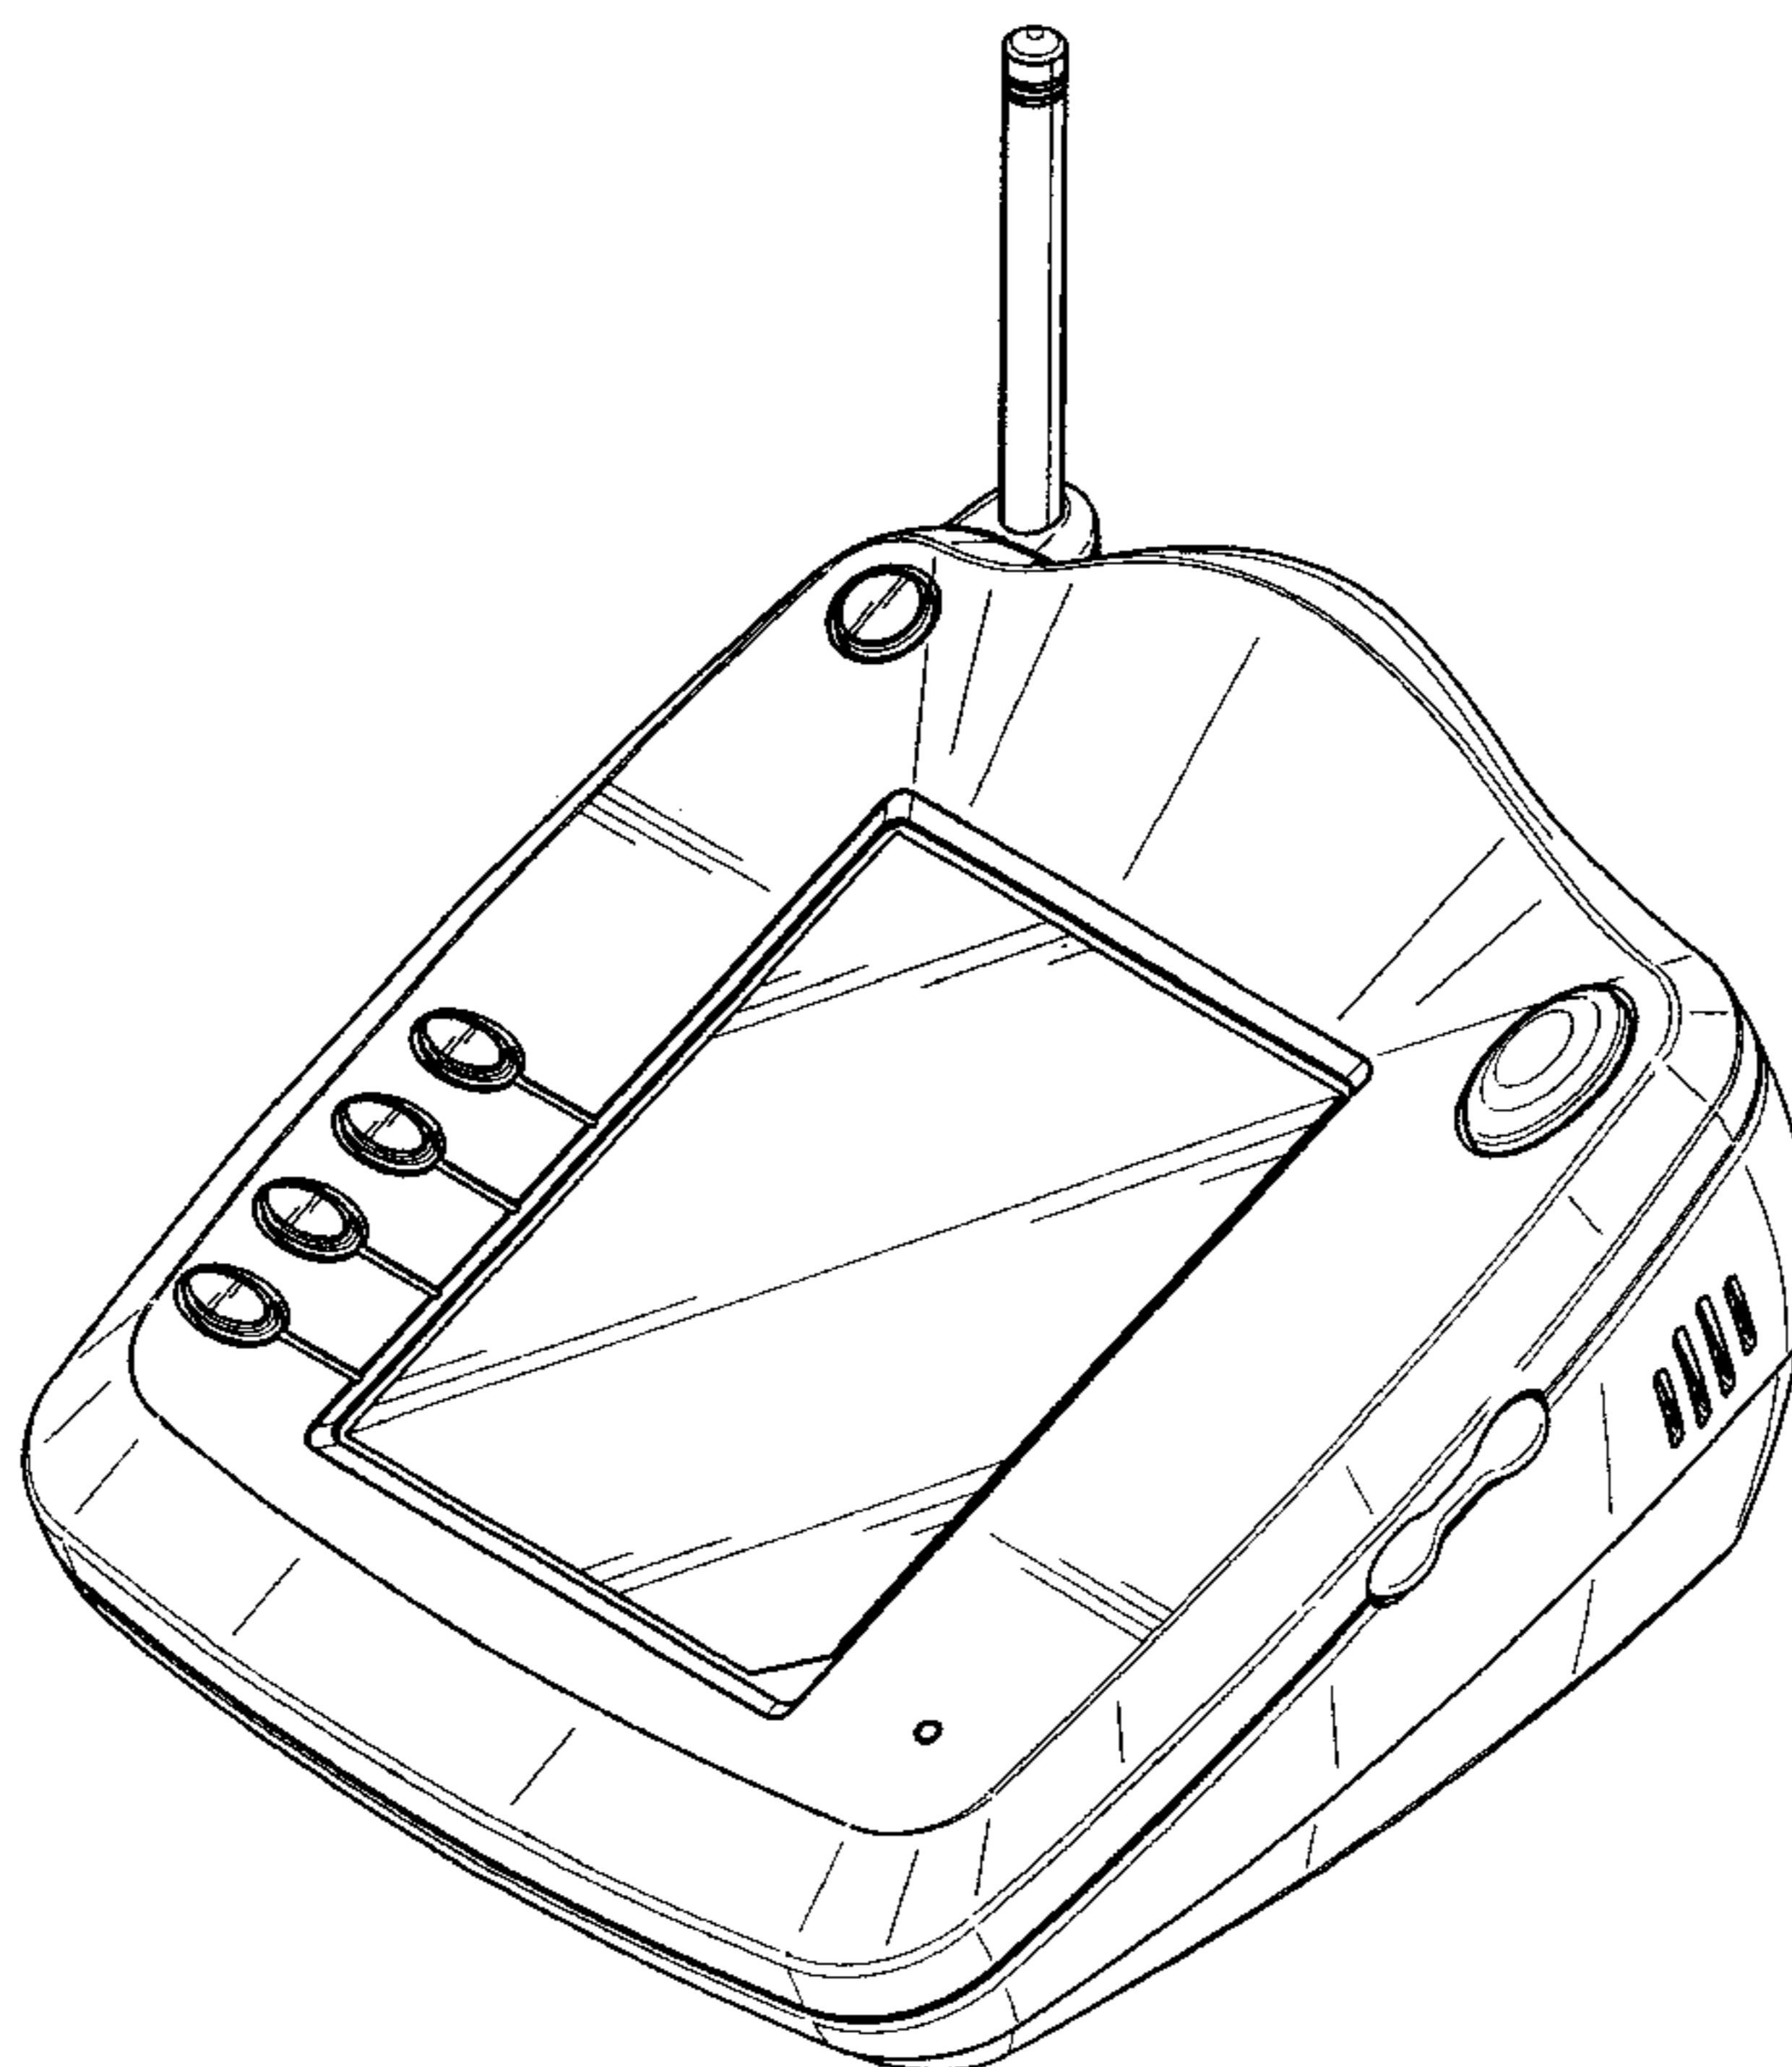


FIG. 1

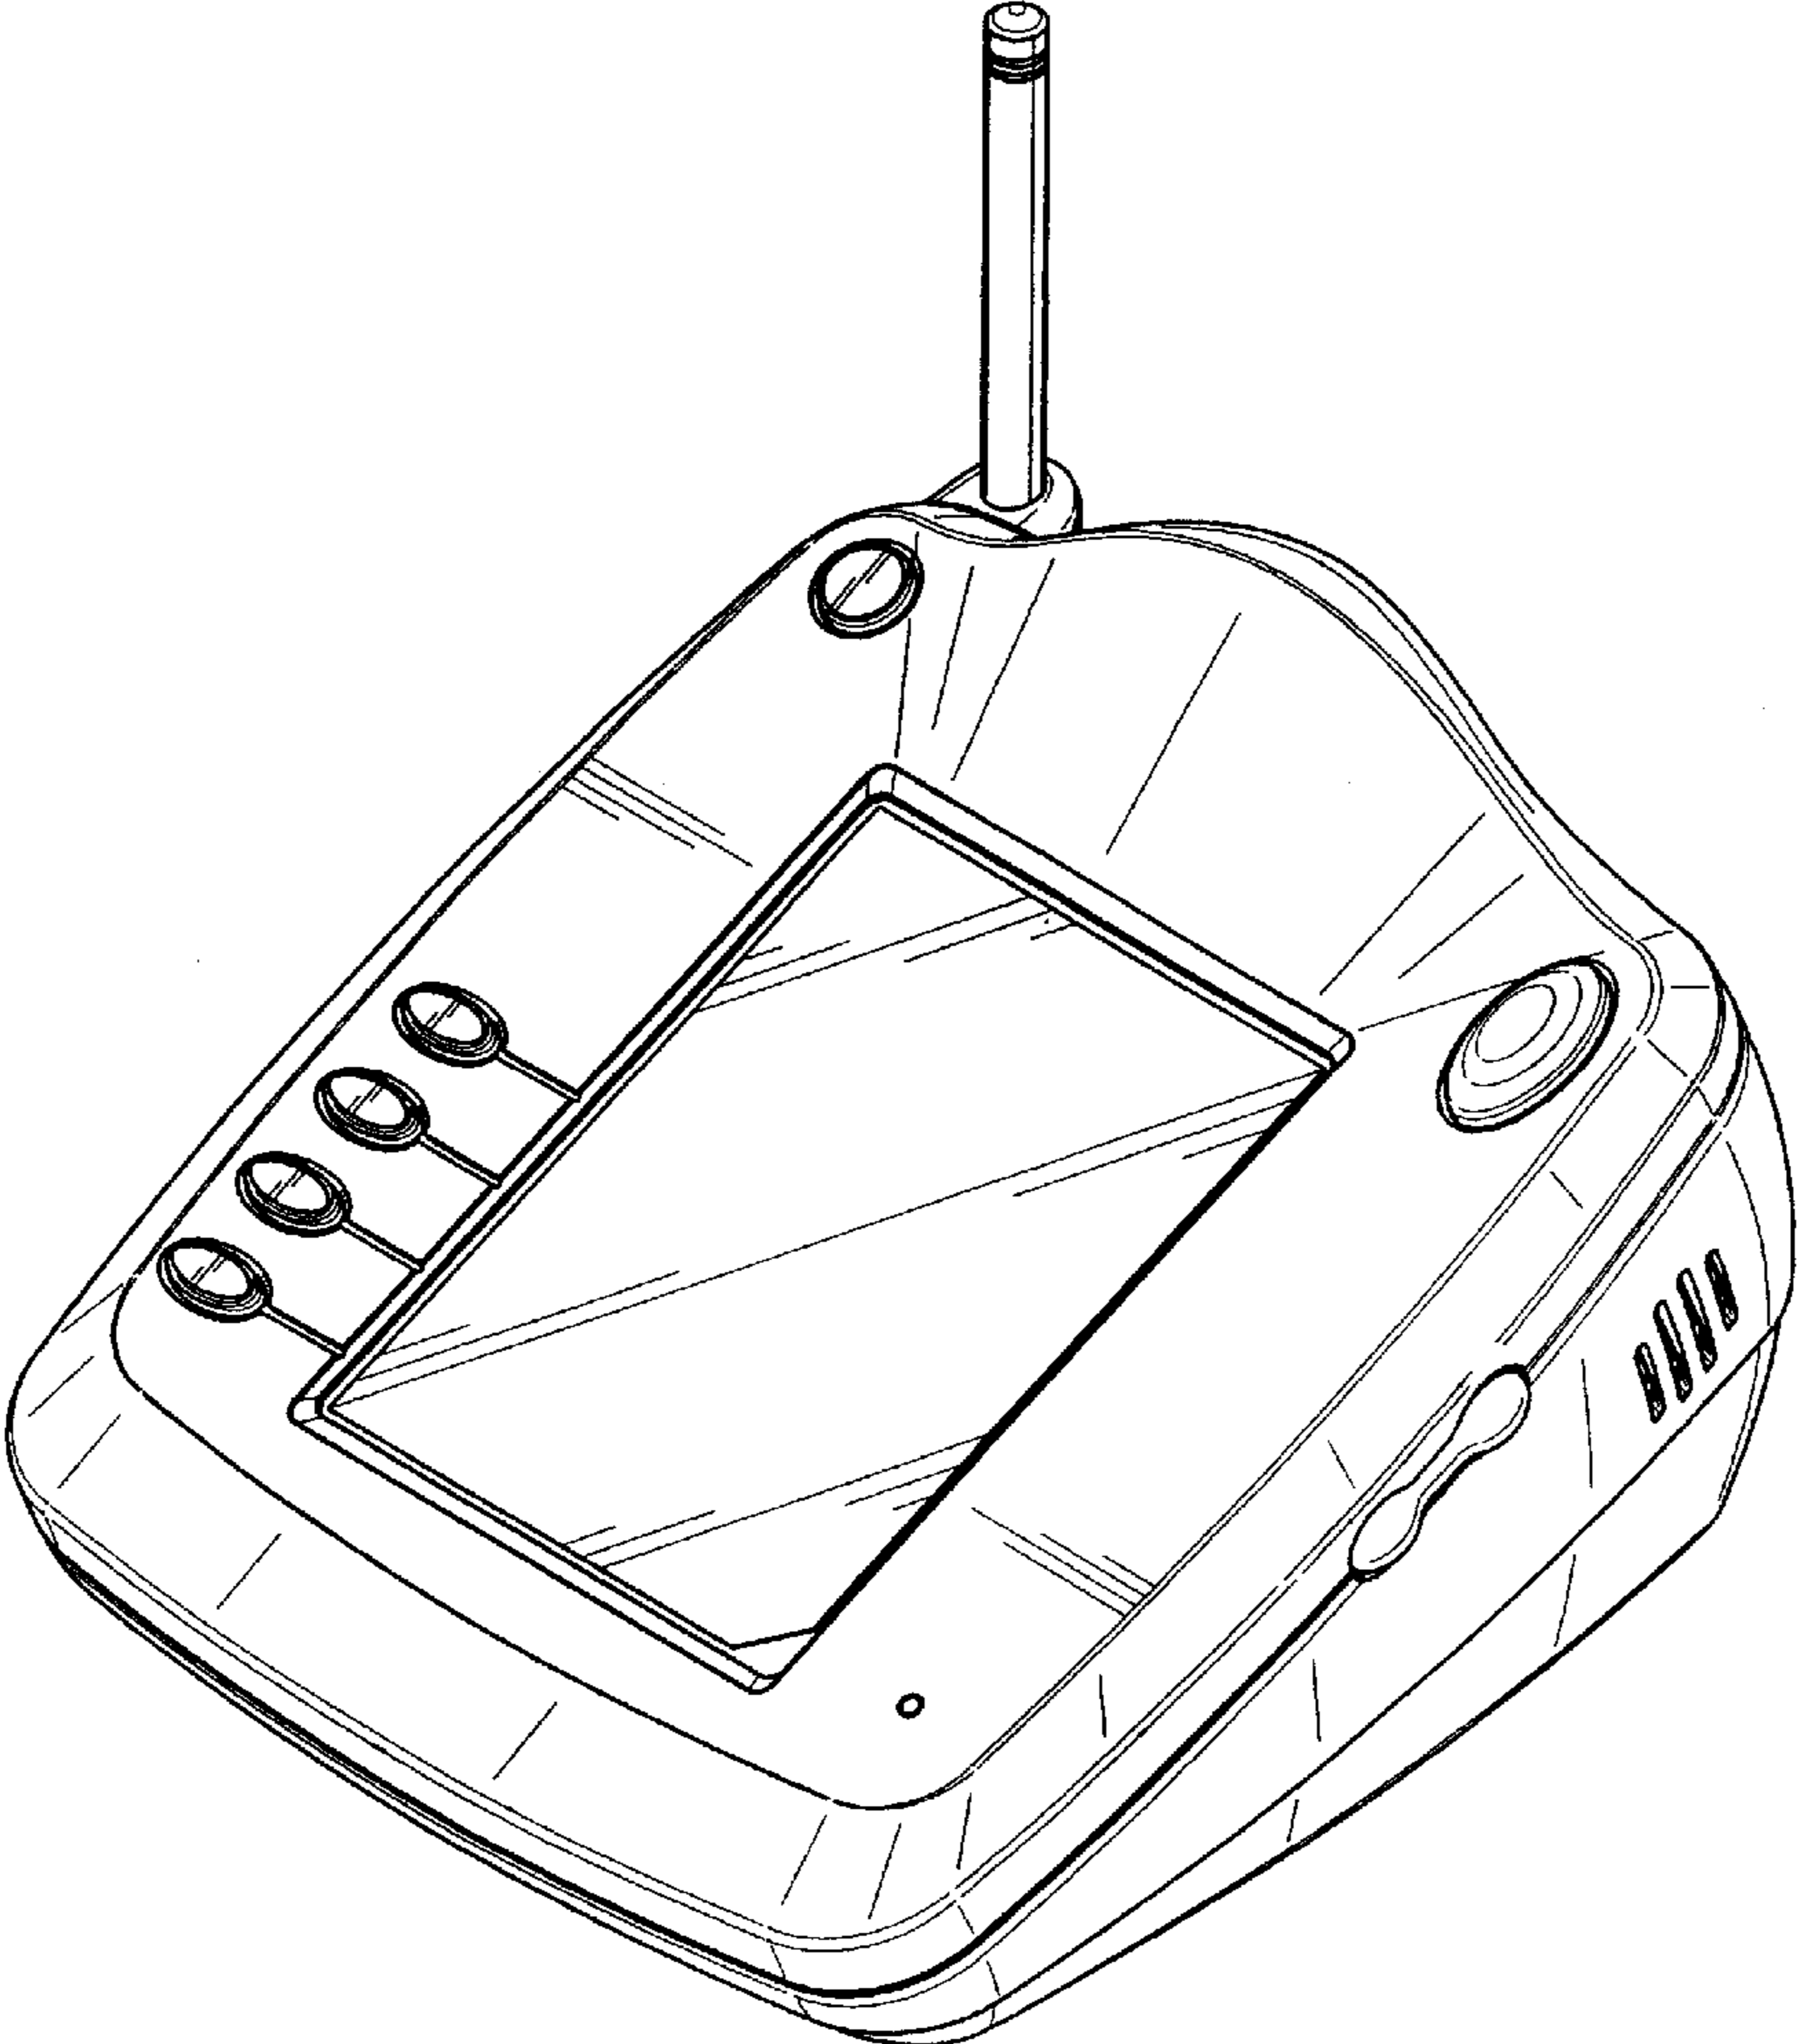


FIG. 2

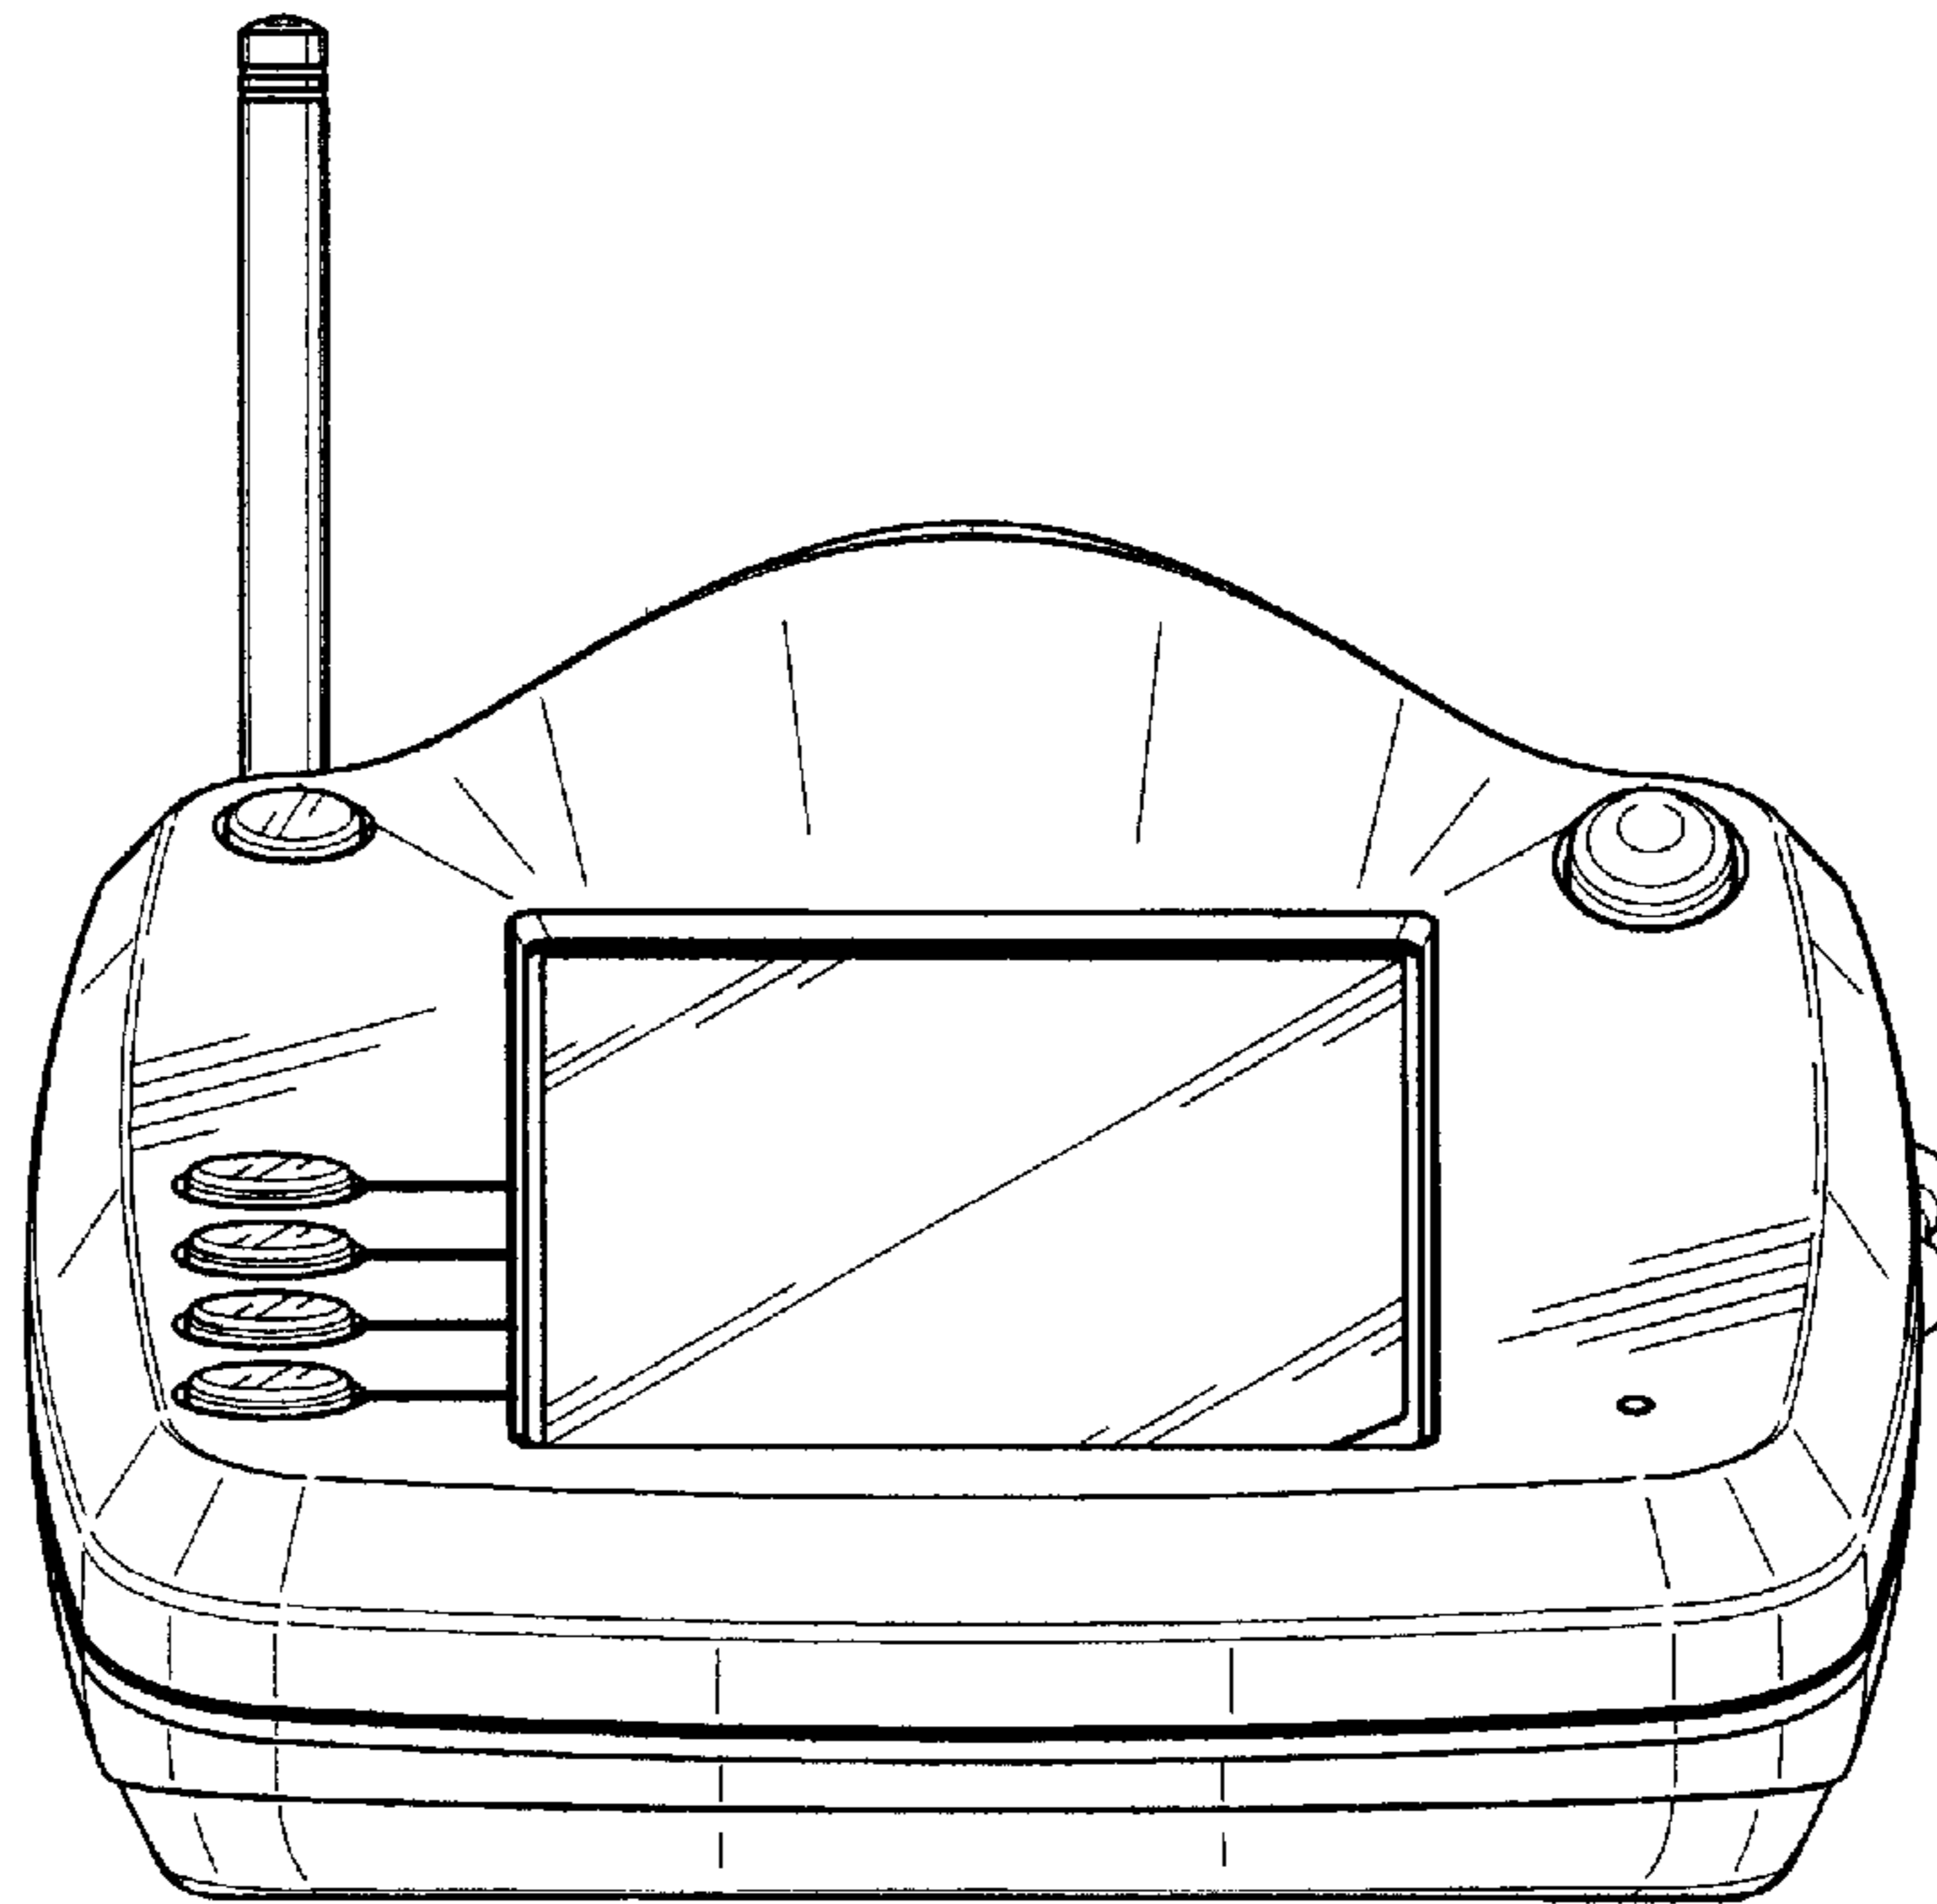


FIG. 3

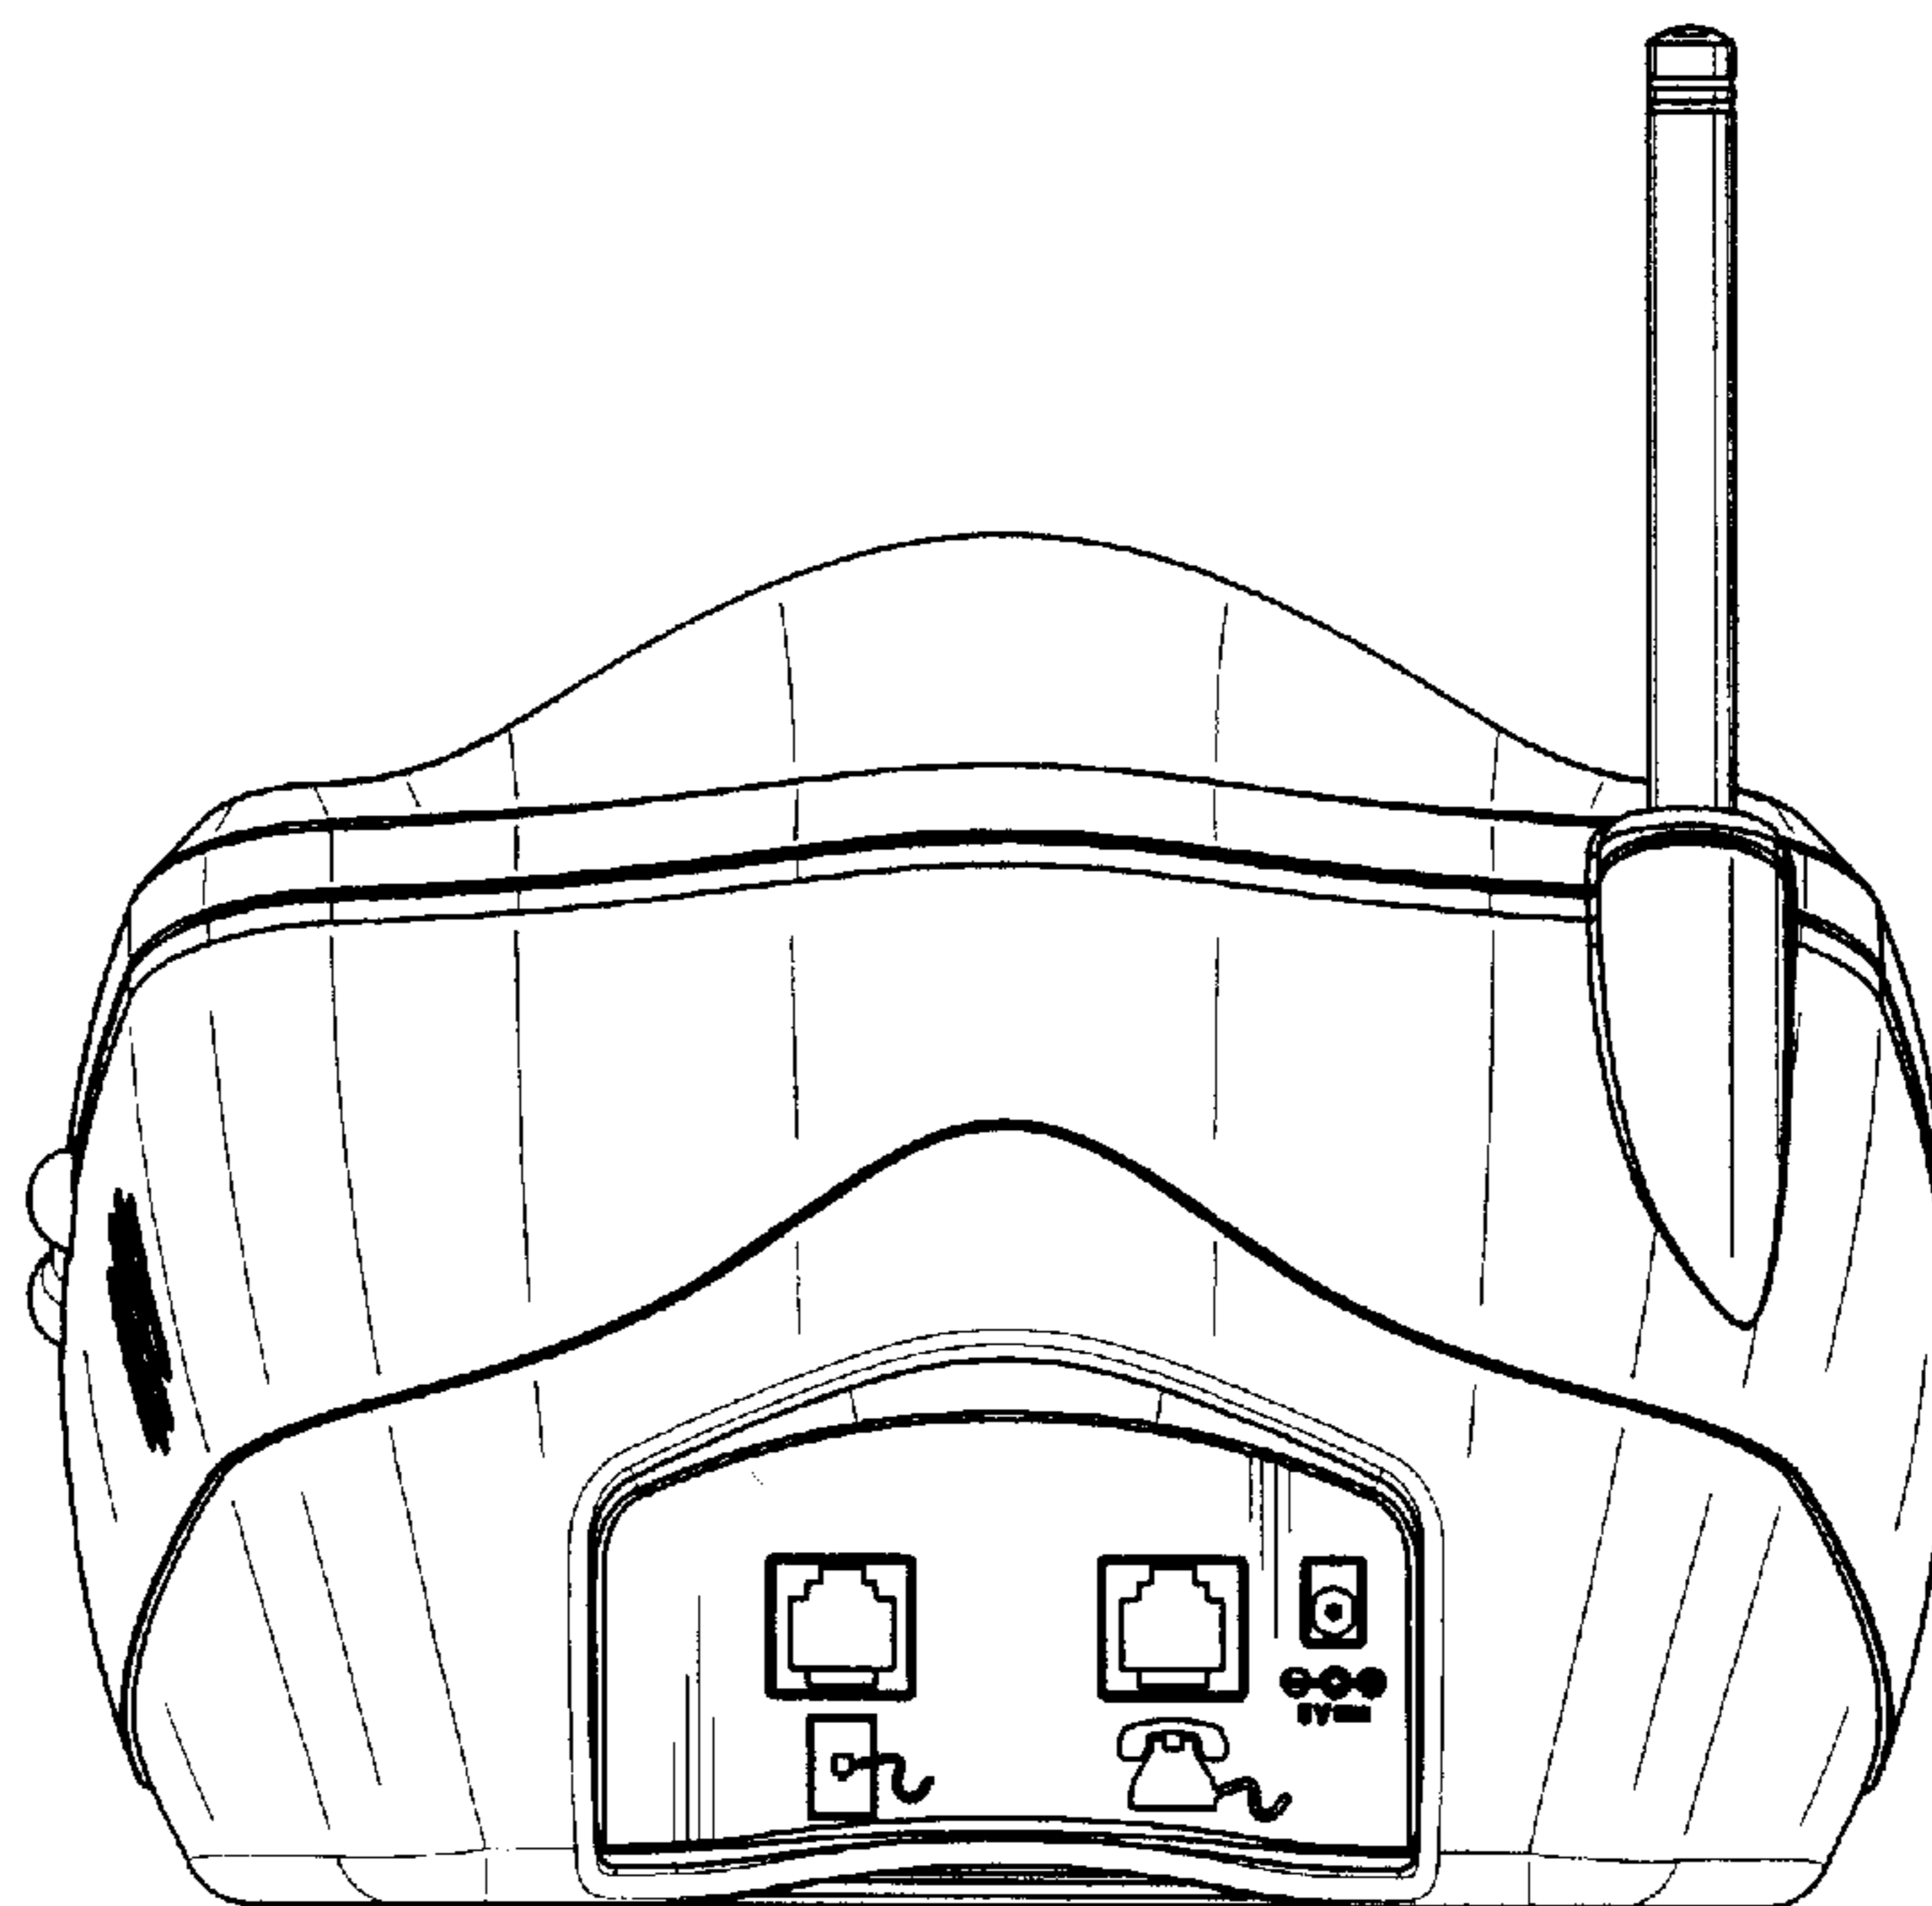


FIG. 4

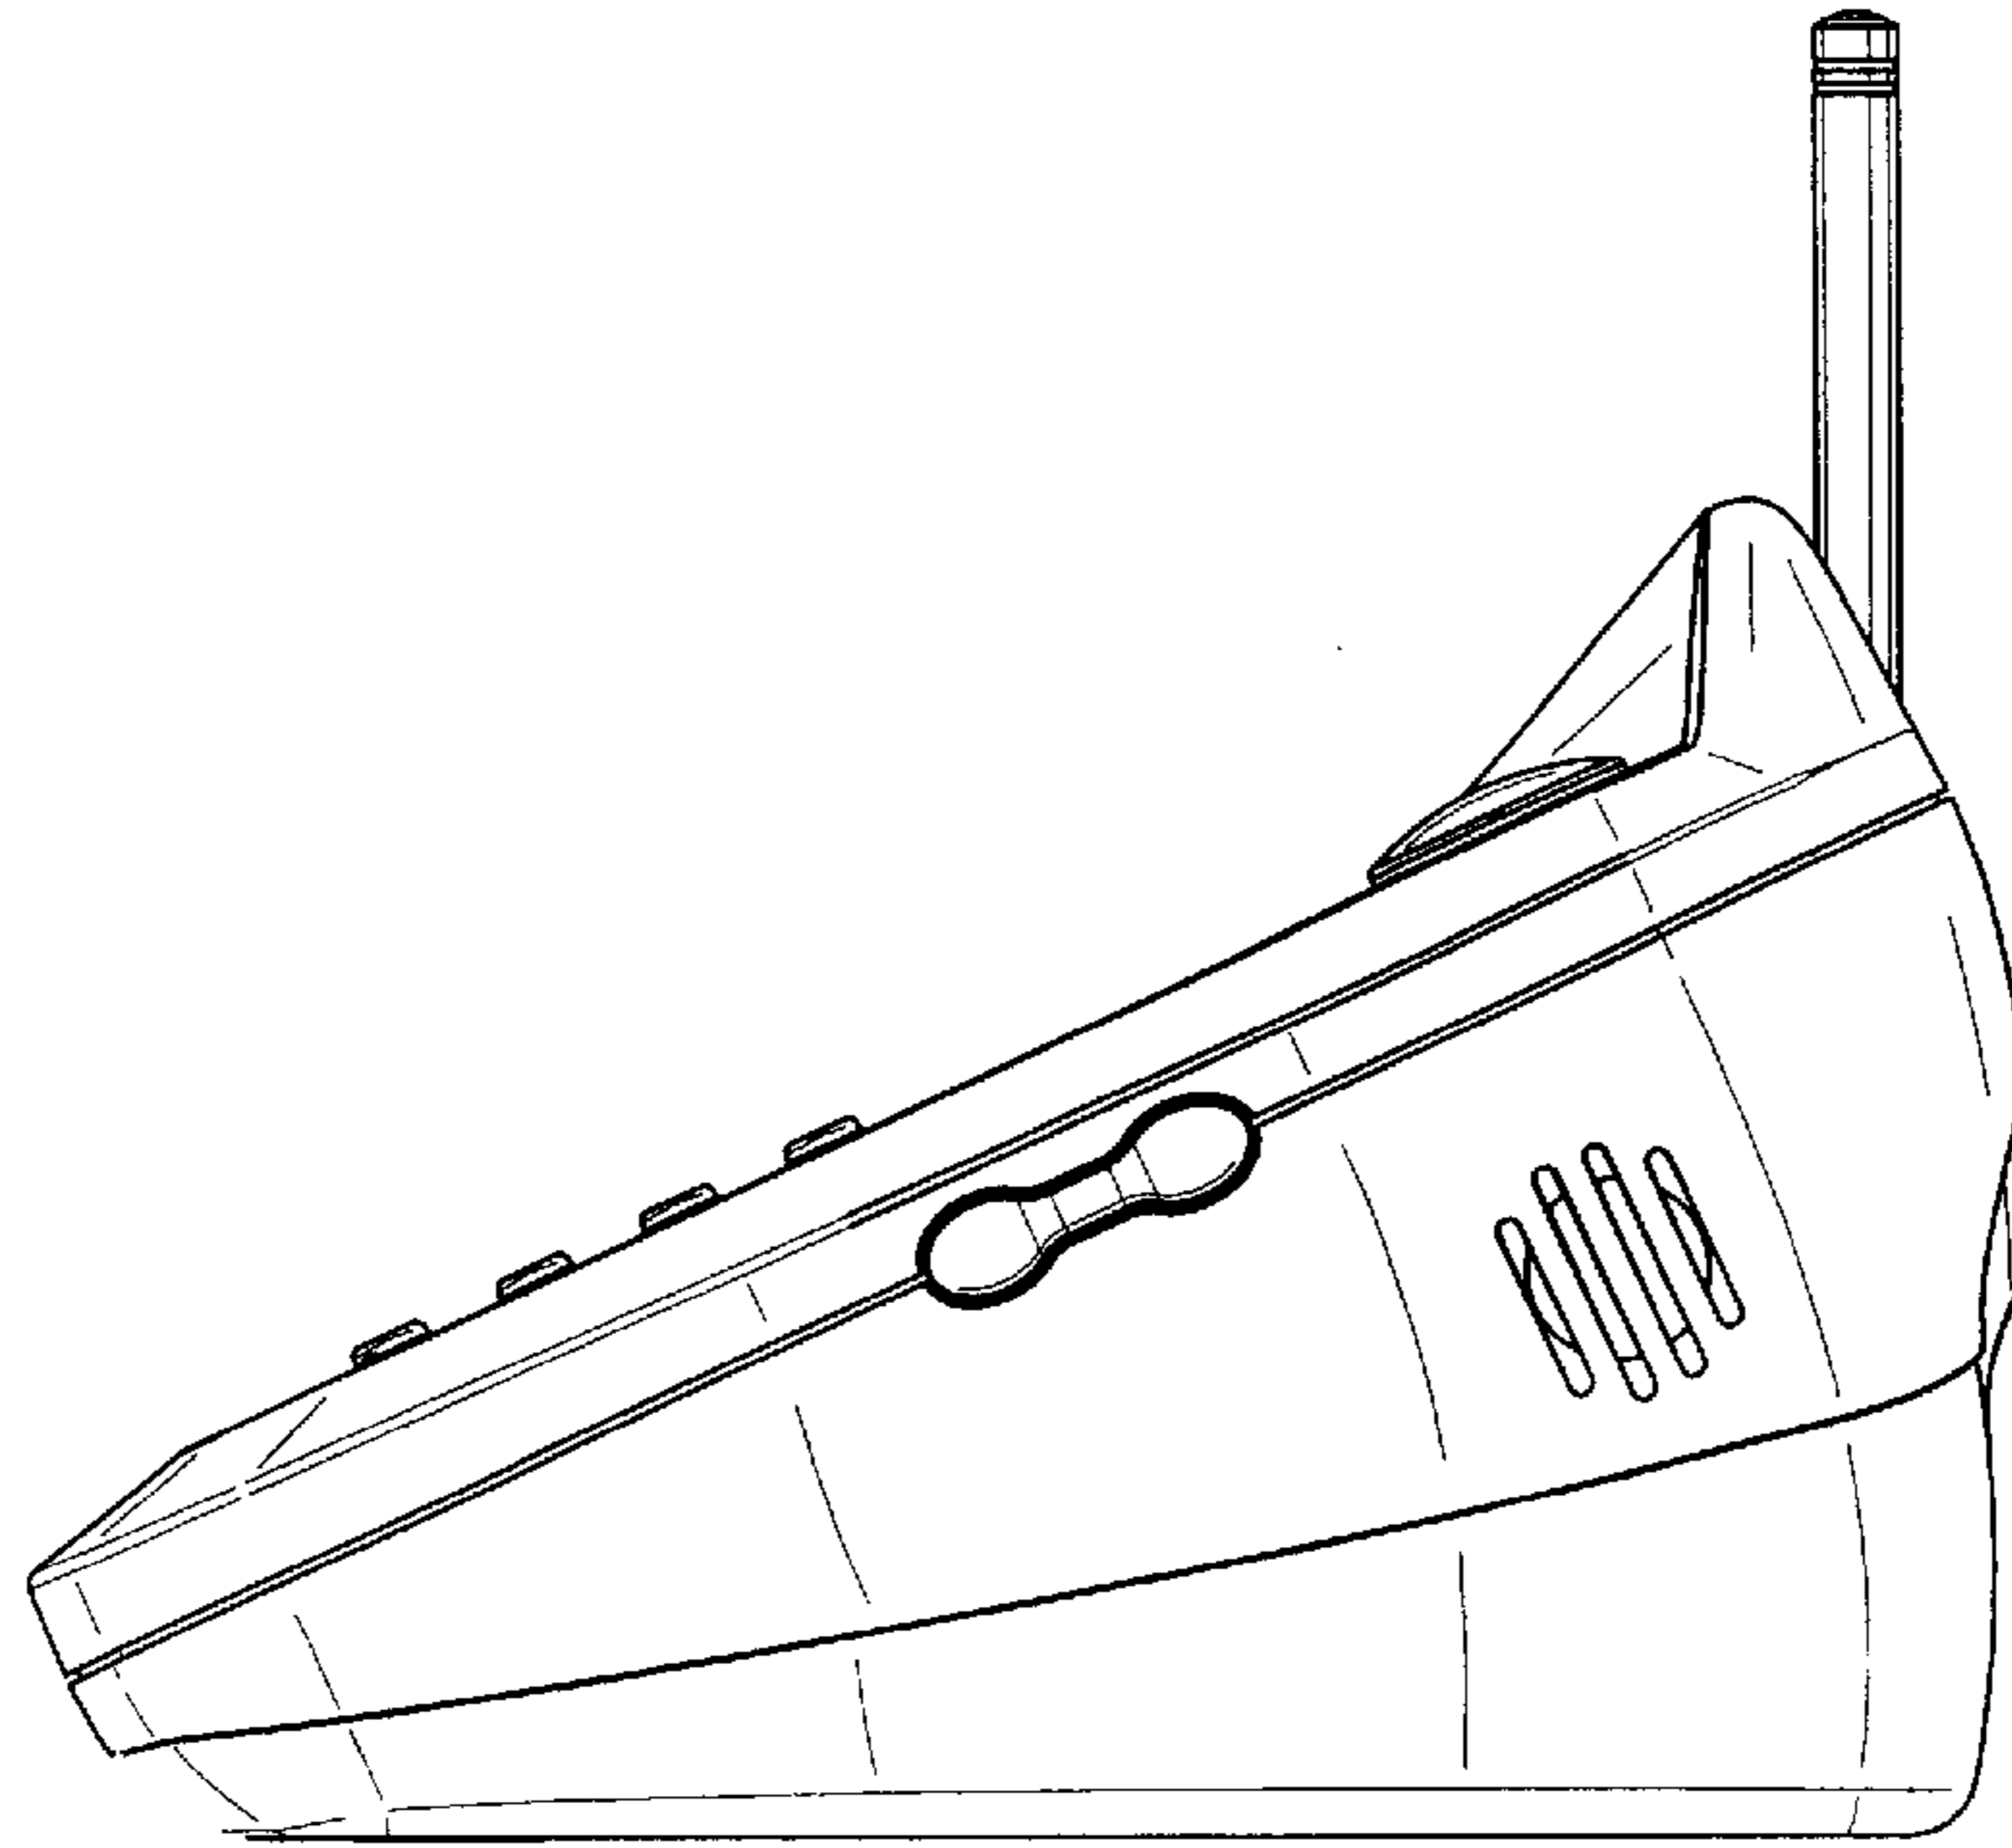


FIG. 5

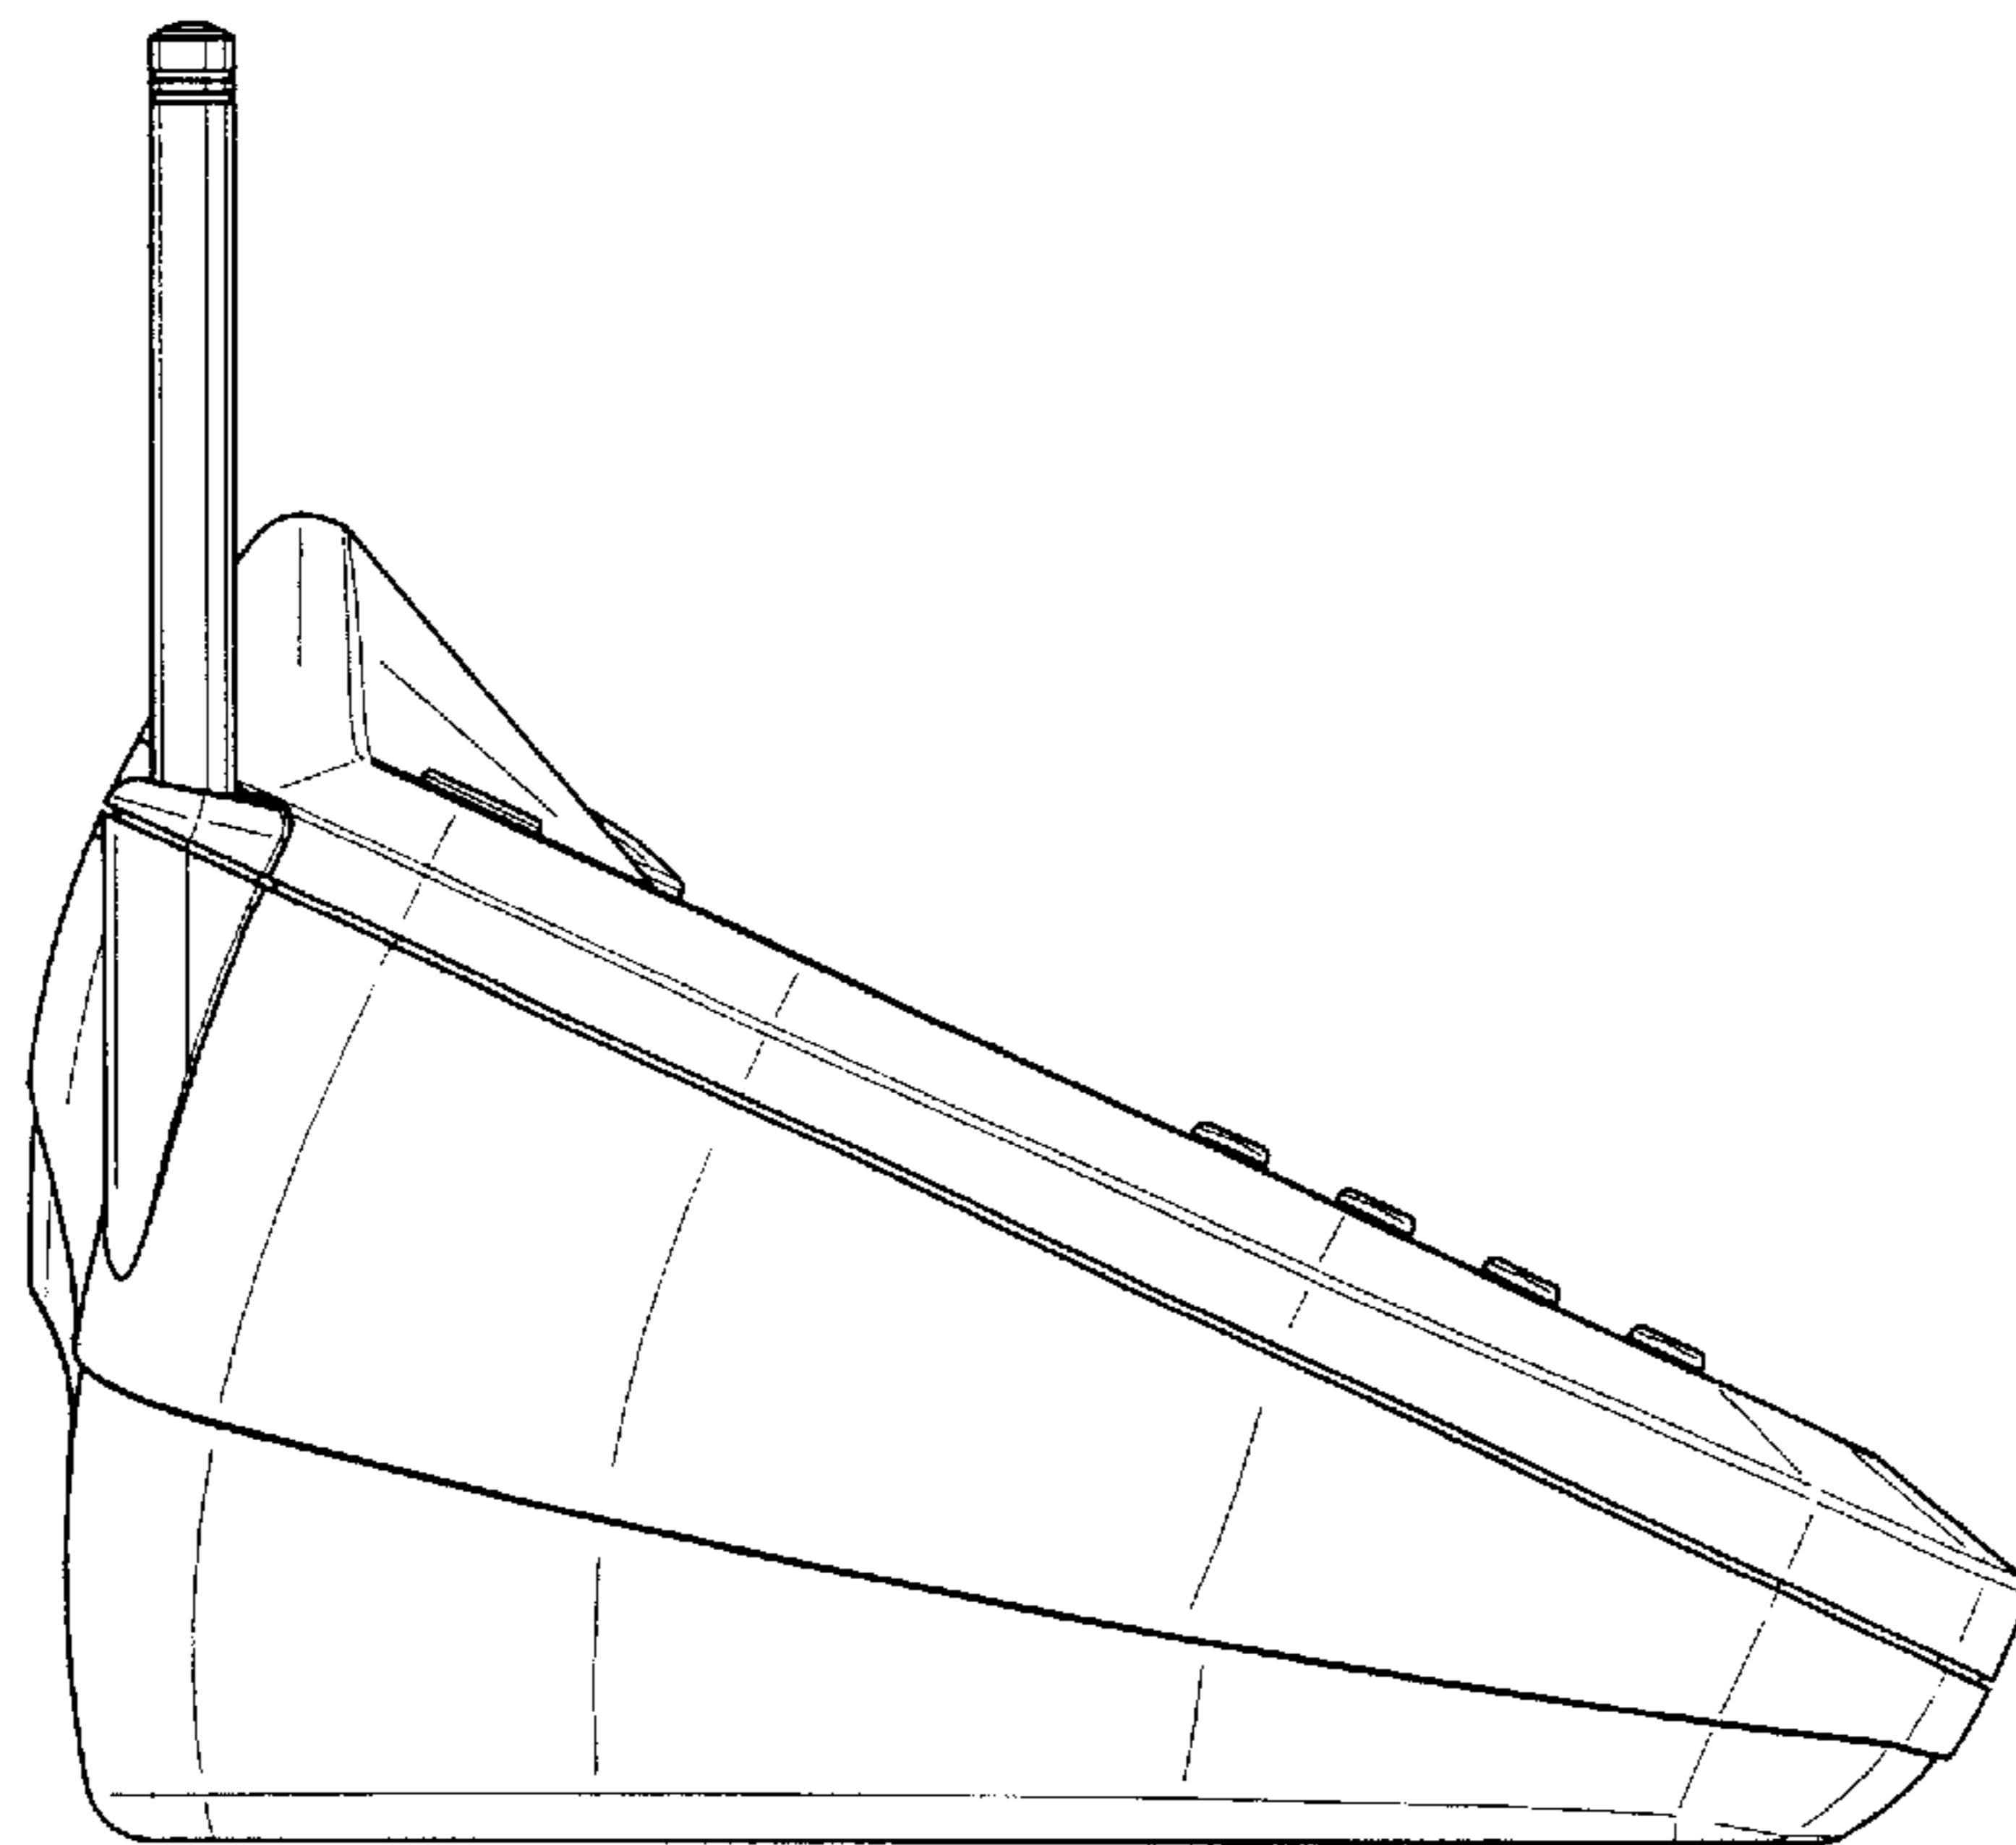


FIG. 6

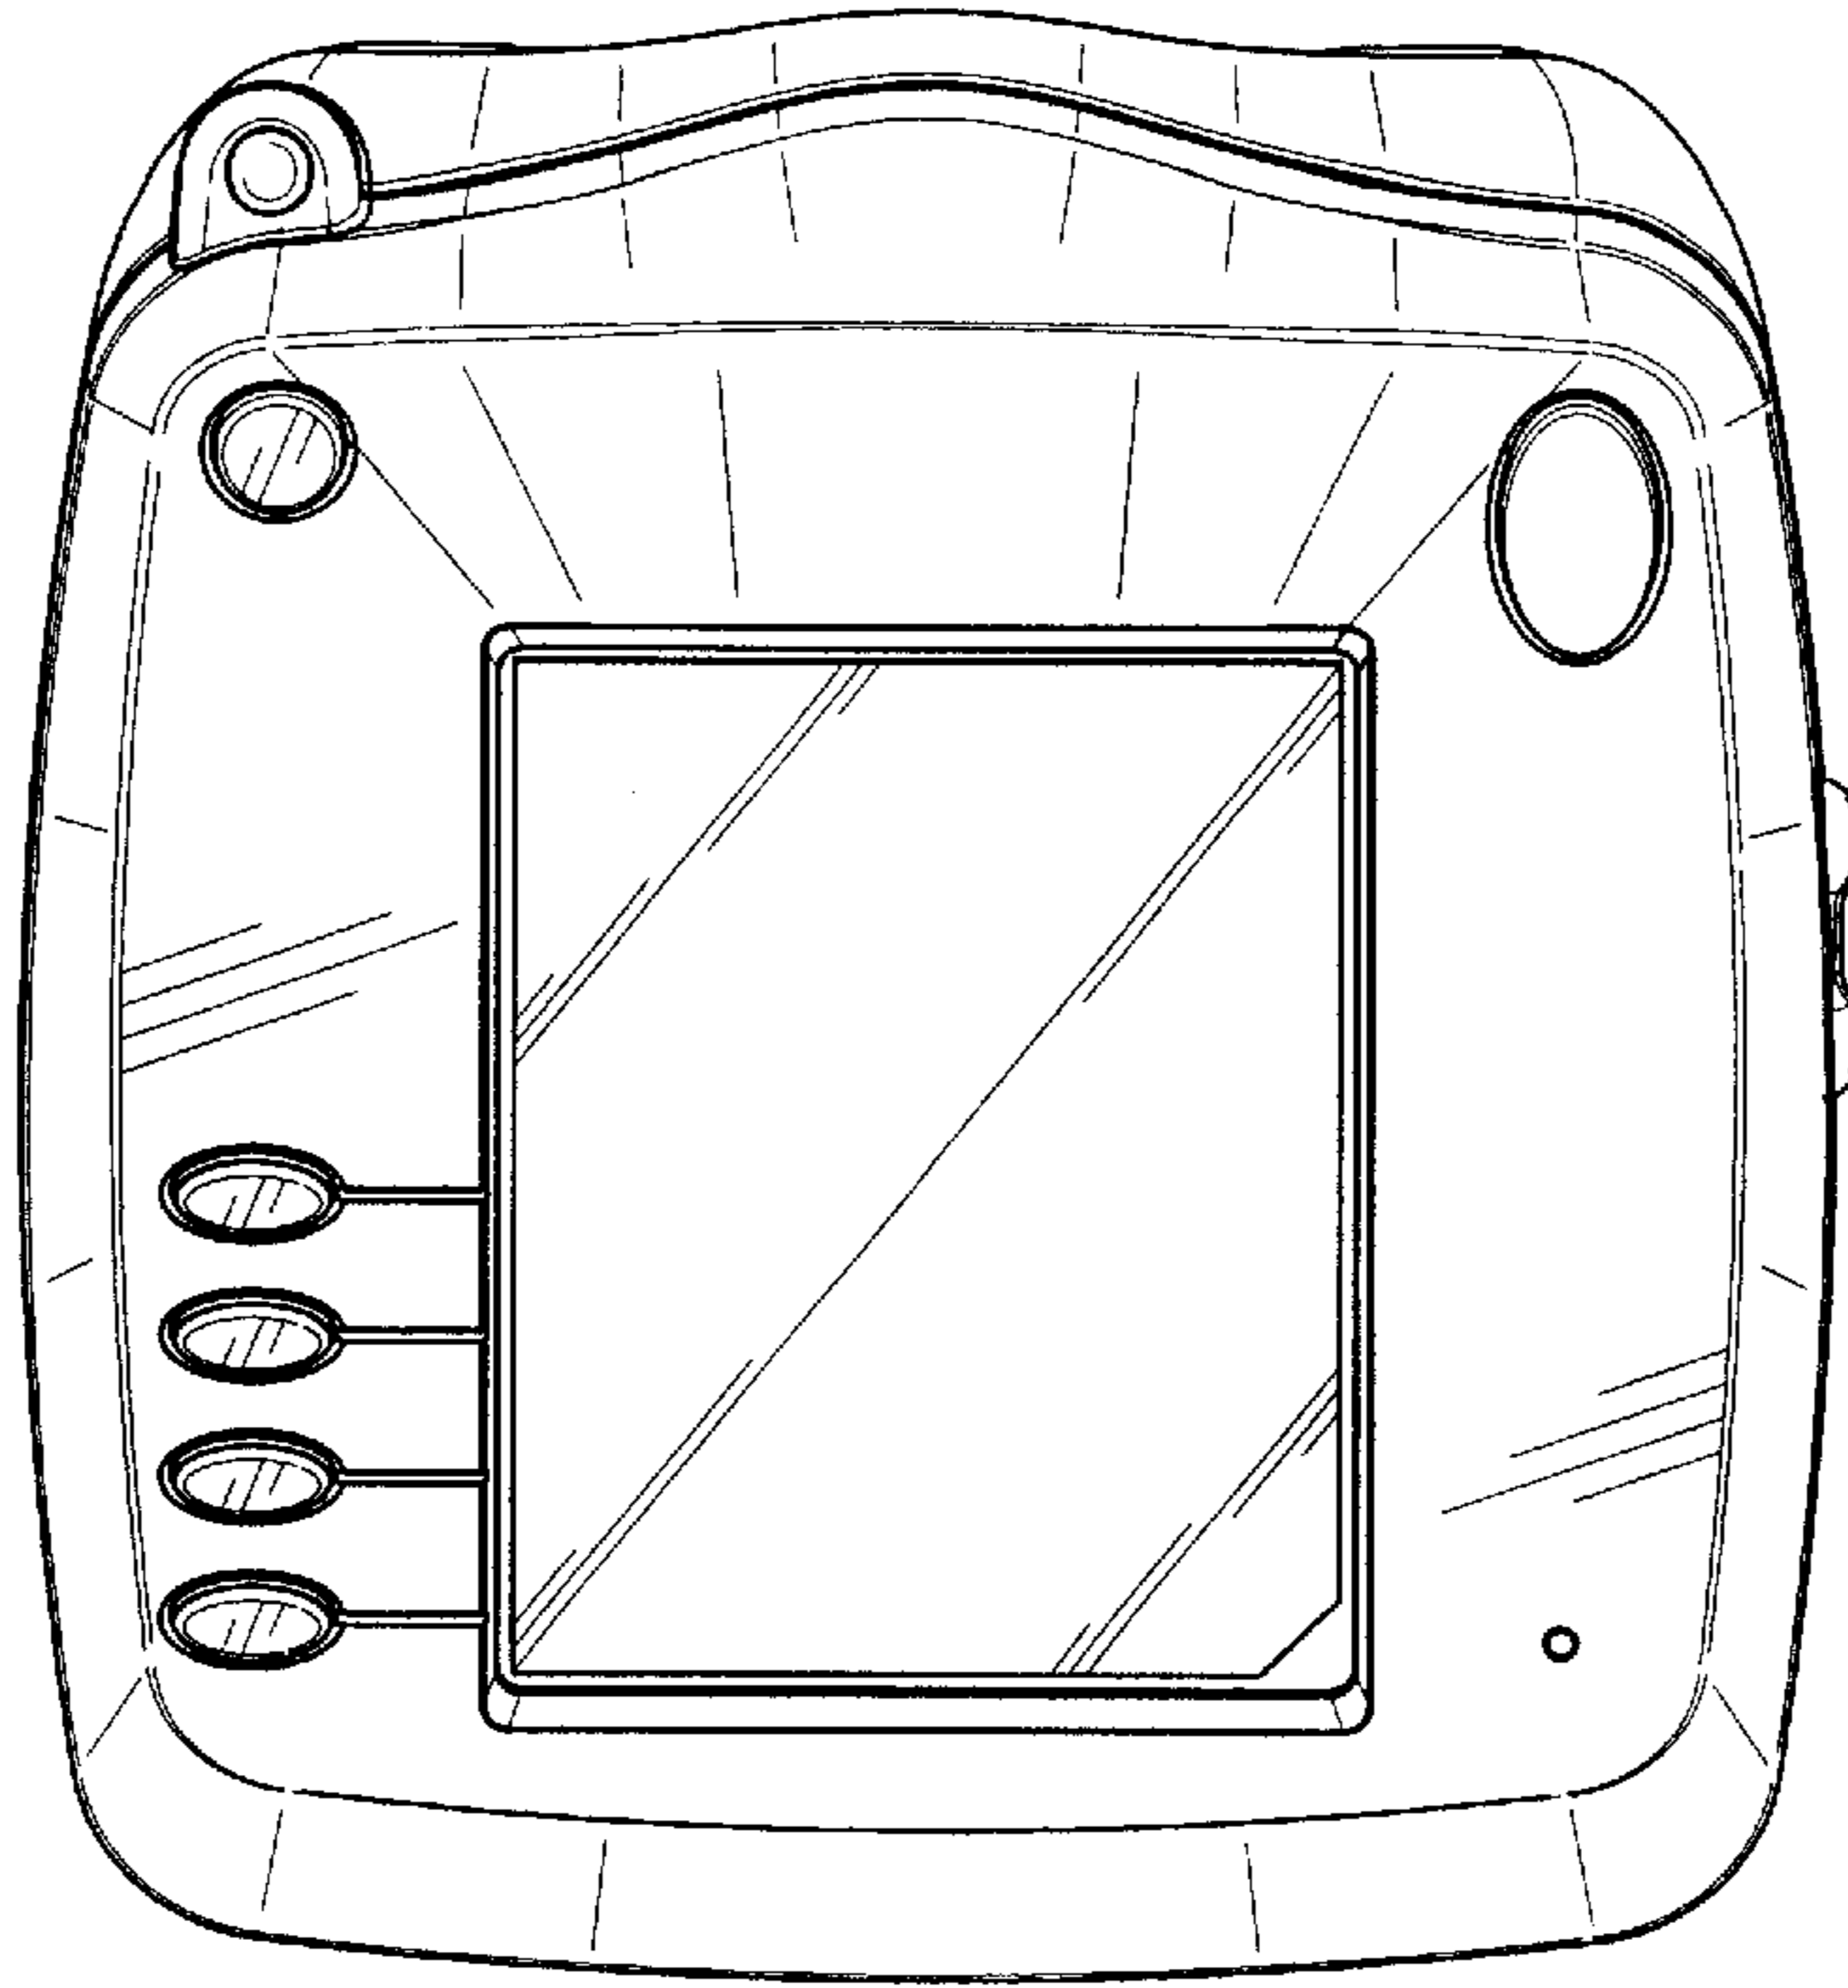


FIG. 7

