



US00D536794S

(12) **United States Design Patent** (10) **Patent No.:** **US D536,794 S**  
**Knieriem et al.** (45) **Date of Patent:** **\*\* Feb. 13, 2007**

(54) **VITAL SIGNS MONITOR**

(75) Inventors: **Alan S. Knieriem**, Baldwinsville, NY (US); **William R. Witkowski**, Marcellus, NY (US); **Ronald J. Kingston**, Syracuse, NY (US); **Scott W. Osiecki**, Skaneateles, NY (US)

(73) Assignee: **Welch Allyn, Inc.**, Skaneateles Falls, NY (US)

(\*\*) Term: **14 Years**

(21) Appl. No.: **29/221,032**

(22) Filed: **Jan. 10, 2005**

(51) **LOC (8) Cl.** ..... **24-01**

(52) **U.S. Cl.** ..... **D24/186**

(58) **Field of Classification Search** ..... D24/186, D24/165; 600/502, 503, 499, 481, 484, 513, 600/485, 500, 480, 495, 479, 519, 528, 532, 600/538, 549

See application file for complete search history.

(56) **References Cited**

**U.S. PATENT DOCUMENTS**

5,417,222 A 5/1995 Dempsey et al.  
5,579,001 A 11/1996 Dempsey et al.

(Continued)

**FOREIGN PATENT DOCUMENTS**

WO WO 95/07048 3/1995

**OTHER PUBLICATIONS**

David Malan et al., "CodeBlue: An Ad Hoc SensorNetwork Infrastructure for Emergency Medical Care," Apr. 2004, 4 pp.

"CodeBlue: Wireless Sensor Networks for Emergency Medical Care," <http://www.eecs.harvard.edu/~mdw/proj/vitaldust/>, 3 pp.

10Blade Inc. Cutting Edge Software ©2003 10Blade, Inc. 11 pp. <http://www.10blade.com>.

*Wireless Sensor Networks for Emergency Medical Care* by Matt Welsh, et al. © 2004 Matt Welsh—Harvard University 21 pp.

Online article from Business week entitled *Tech Wave 2: The Sensor Revolution—The Future of Tech—Road Map* dated Aug. 25, 2003 4 pp. [http://www.businessweek.com/magazine/content/03\\_34/b3846622.htm](http://www.businessweek.com/magazine/content/03_34/b3846622.htm).

Online article entitled "About Crossbow" dated May 5, 2004 2 pp. [http://www.xbow.com/General\\_Info/AboutCrossbow.htm](http://www.xbow.com/General_Info/AboutCrossbow.htm).

Online article from Crossbow Technology Inc. entitled *Moles, Smart Dust Sensors, Wireless Sensor Networks* © 2004 Crossbow Technology 2 pp. <http://www.xbow.com/Products/productsdetails.aspx?sid=3>.

(Continued)

*Primary Examiner*—Louis S. Zarfes

*Assistant Examiner*—Daniel Yu

(74) *Attorney, Agent, or Firm*—Wall Marjama & Bilinski LLP

(57) **CLAIM**

The ornamental design for a vital signs monitor, as shown and described.

**DESCRIPTION**

This vital signs monitor designed by Applicant Al Kneireim et al. is a device for making measurements of various vital signs of a human patient.

This application is related to co-pending U.S. utility patent application Ser. No. 11/032,625, entitled "A Portable Vital Signs Measurement Instrument and Method of Use Thereof", filed on even date herewith, which application is incorporated herein by reference in its entirety.

FIG. 1 is a perspective view of a vital signs monitor illustrating my new design;

FIG. 2 is a front elevation view thereof;

FIG. 3 is a left side elevation view thereof;


FIG. 4 is a right side elevation view thereof;

FIG. 5 is a top view thereof;

FIG. 6 is a bottom view thereof; and,

FIG. 7 is a rear perspective view thereof.

**1 Claim, 6 Drawing Sheets**

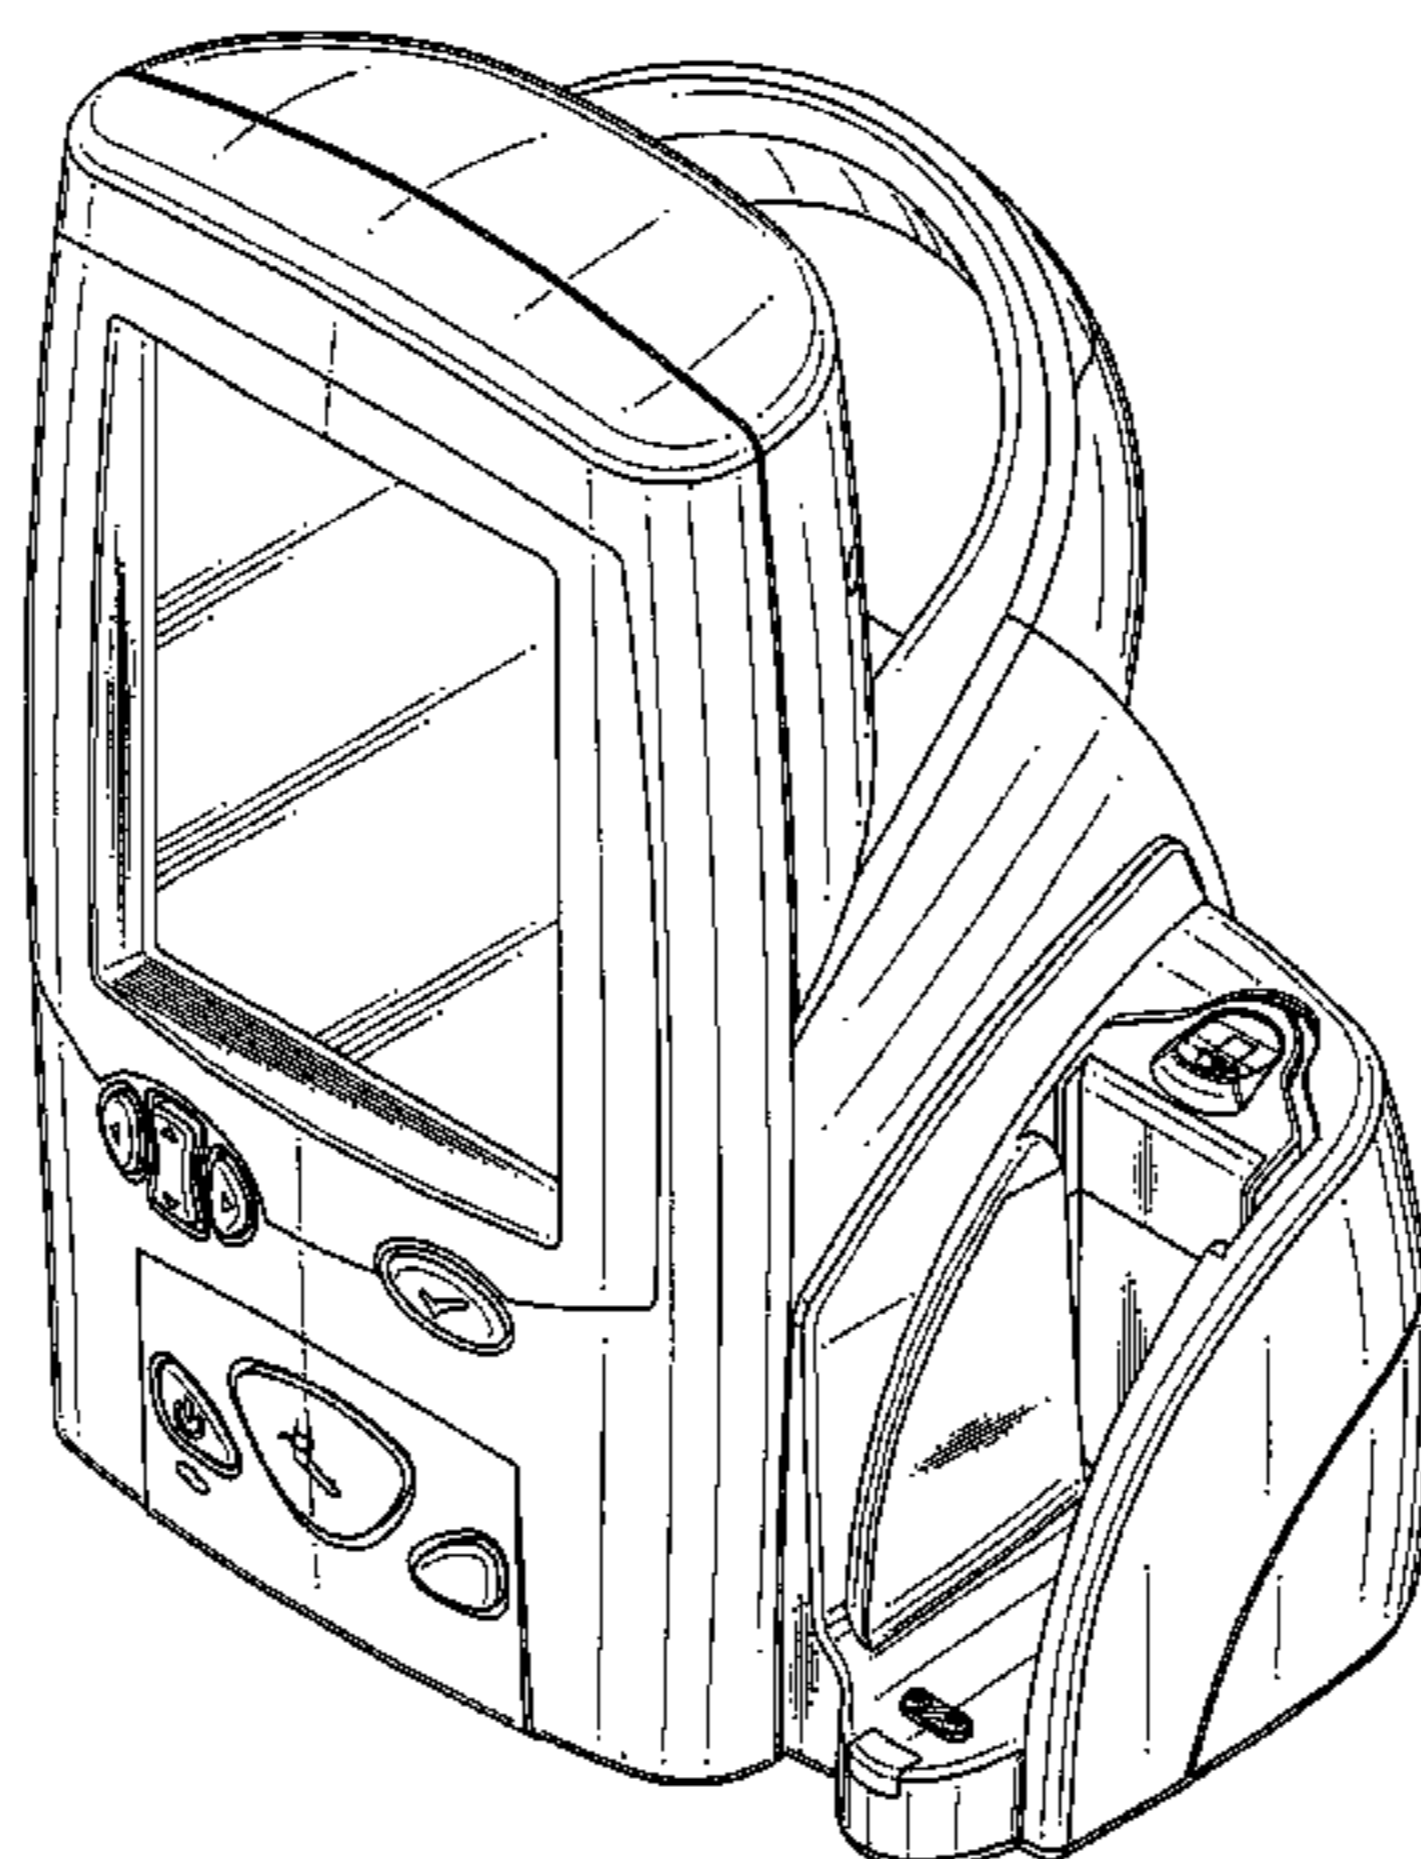

U.S. PATENT DOCUMENTS

5,579,775	A	12/1996	Dempsey et al.	
5,687,734	A	11/1997	Dempsey et al.	
5,748,103	A	5/1998	Flach et al.	
5,767,791	A	6/1998	Stoop et al.	
5,862,803	A	1/1999	Besson et al.	
5,944,659	A	8/1999	Flach et al.	
5,957,854	A	9/1999	Besson et al.	
6,057,758	A	5/2000	Dempsey et al.	
6,106,457	A	8/2000	Perkins et al.	
6,132,371	A	10/2000	Dempsey et al.	
6,213,942	B1	4/2001	Flach et al.	
6,289,238	B1	9/2001	Besson et al.	
6,393,431	B1	5/2002	Salvati et al.	
D460,559	S *	7/2002	Knieriem et al.	..... D24/186
6,544,173	B2	4/2003	West et al.	
6,544,174	B2	4/2003	West et al.	
D475,137	S *	5/2003	Manke et al.	..... D24/165
6,577,893	B1	6/2003	Besson et al.	
6,589,170	B1	7/2003	Flach et al.	
D512,151	S *	11/2005	Ward et al.	..... D24/186

OTHER PUBLICATIONS

Online article from Crossbow Technology Inc. entitled “Wireless Sensor Networks” dated May 5, 2004 2 pp [http://www.xbow.com/Products/Wireless\\_Sensor\\_Networks.htm](http://www.xbow.com/Products/Wireless_Sensor_Networks.htm).

Online article entitled “Vital sign device improves resuscitation monitoring”—American Heart Association meeting report—Co-authors Dan Myung, A.B. and Mark Gaynor, Ph.D. 2 pp [http://www.innovations-report.com/html/reports/information\\_technology/report-23177.html](http://www.innovations-report.com/html/reports/information_technology/report-23177.html).

Online article—Redding Medical—for Vital Signs Monitor 300 Series—Welch Allyn Vital Signs Monitor #300 Series 2 pp. [http://www.reddingmedical.com/1470\\_Welch\\_Allyn\\_Vital\\_Signs\\_Monitor\\_300\\_Sereis:cfm?l...](http://www.reddingmedical.com/1470_Welch_Allyn_Vital_Signs_Monitor_300_Sereis:cfm?l...)

Online article—Redding Medical—for Welch Allyn Vital Signs Monitor [http://www.reddingmedical.com/486\\_Welch\\_Allyn\\_Vital\\_Signs\\_Monitor.cfm?id=486&step=4...](http://www.reddingmedical.com/486_Welch_Allyn_Vital_Signs_Monitor.cfm?id=486&step=4...)

Online article—EMS House of DeFrance entitled “Vital Dust” device improves resuscitation monitoring 3 pp. [http://www.defrance.org/artman/publish/article\\_440.shtml](http://www.defrance.org/artman/publish/article_440.shtml).

Online article—thetelemedicineweblog—“Vital Dust Wireless Vital Sign Monitr Debuts at American Heart Association Conference” by Catherine Calacanis 3 pp. <http://telemedicine.weblogsinc.com/entry/5348124023511092/>.

Online article—“4100 Digital Pulse Oximeter”—North Medical Center—4100 Bluetooth Enabled Digital Pulse Oximeter 4 pp. <http://www.nonln.com/Products/4100.html>.

\* cited by examiner

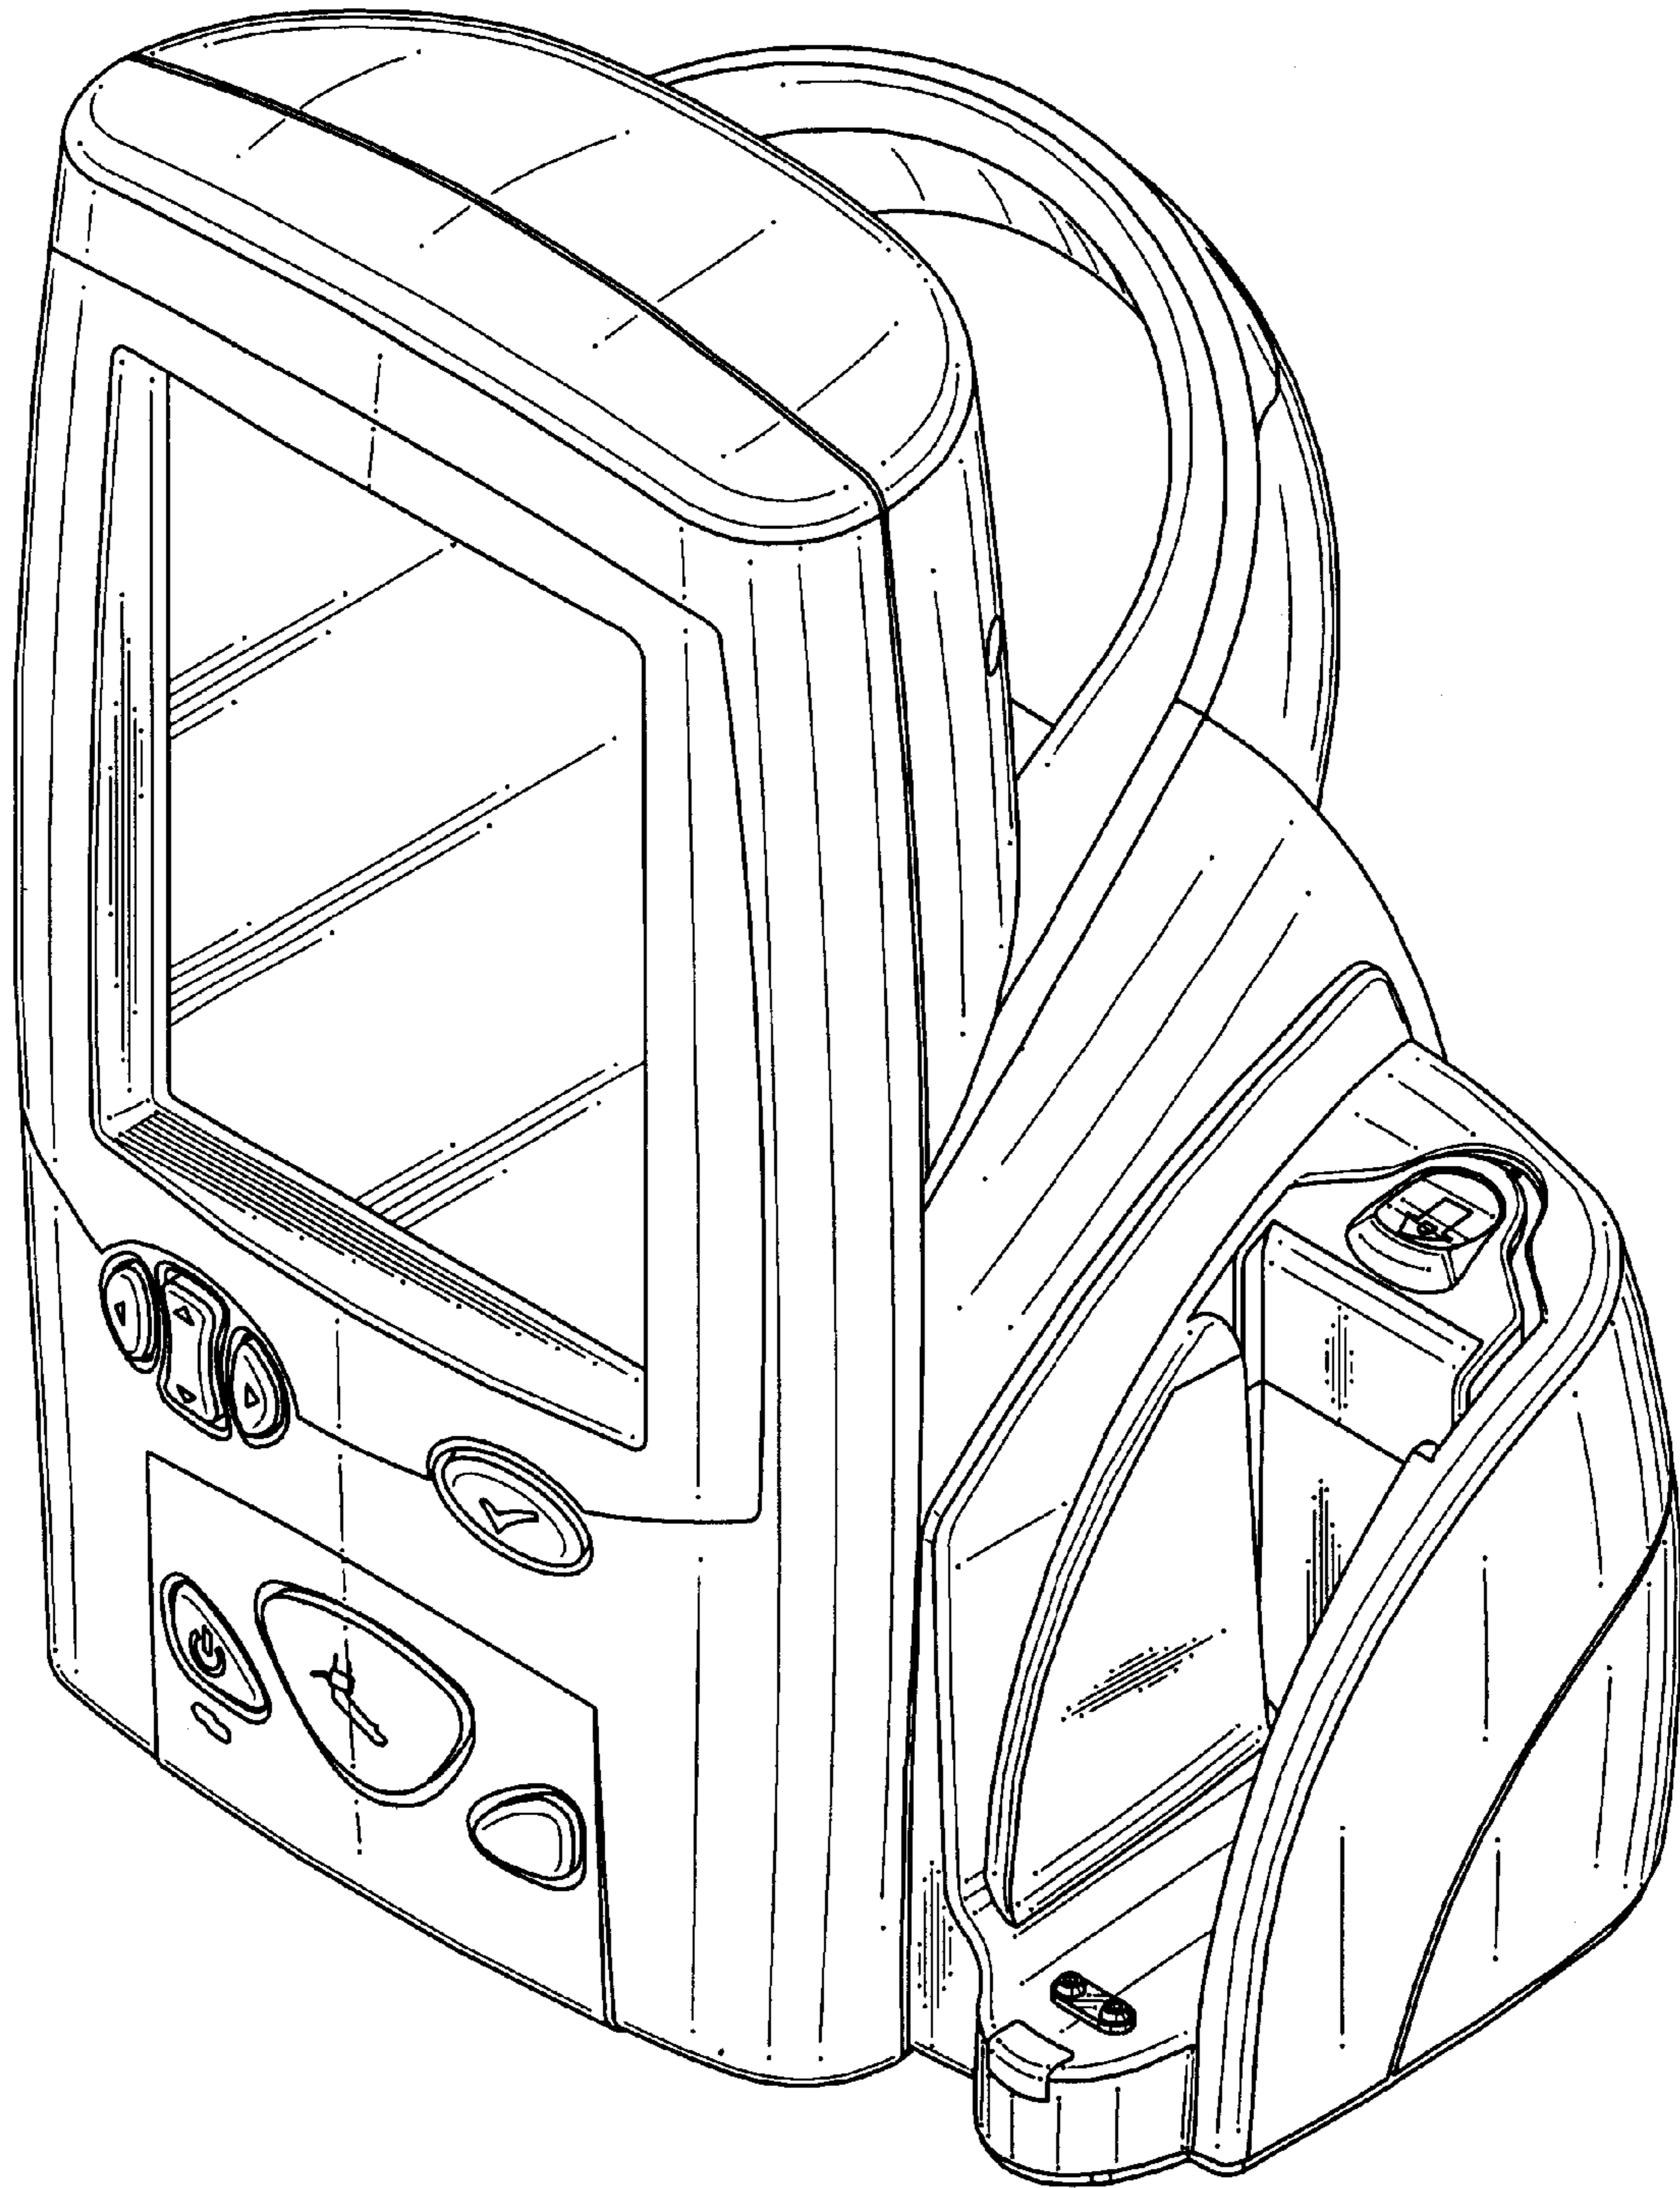


FIG. 1

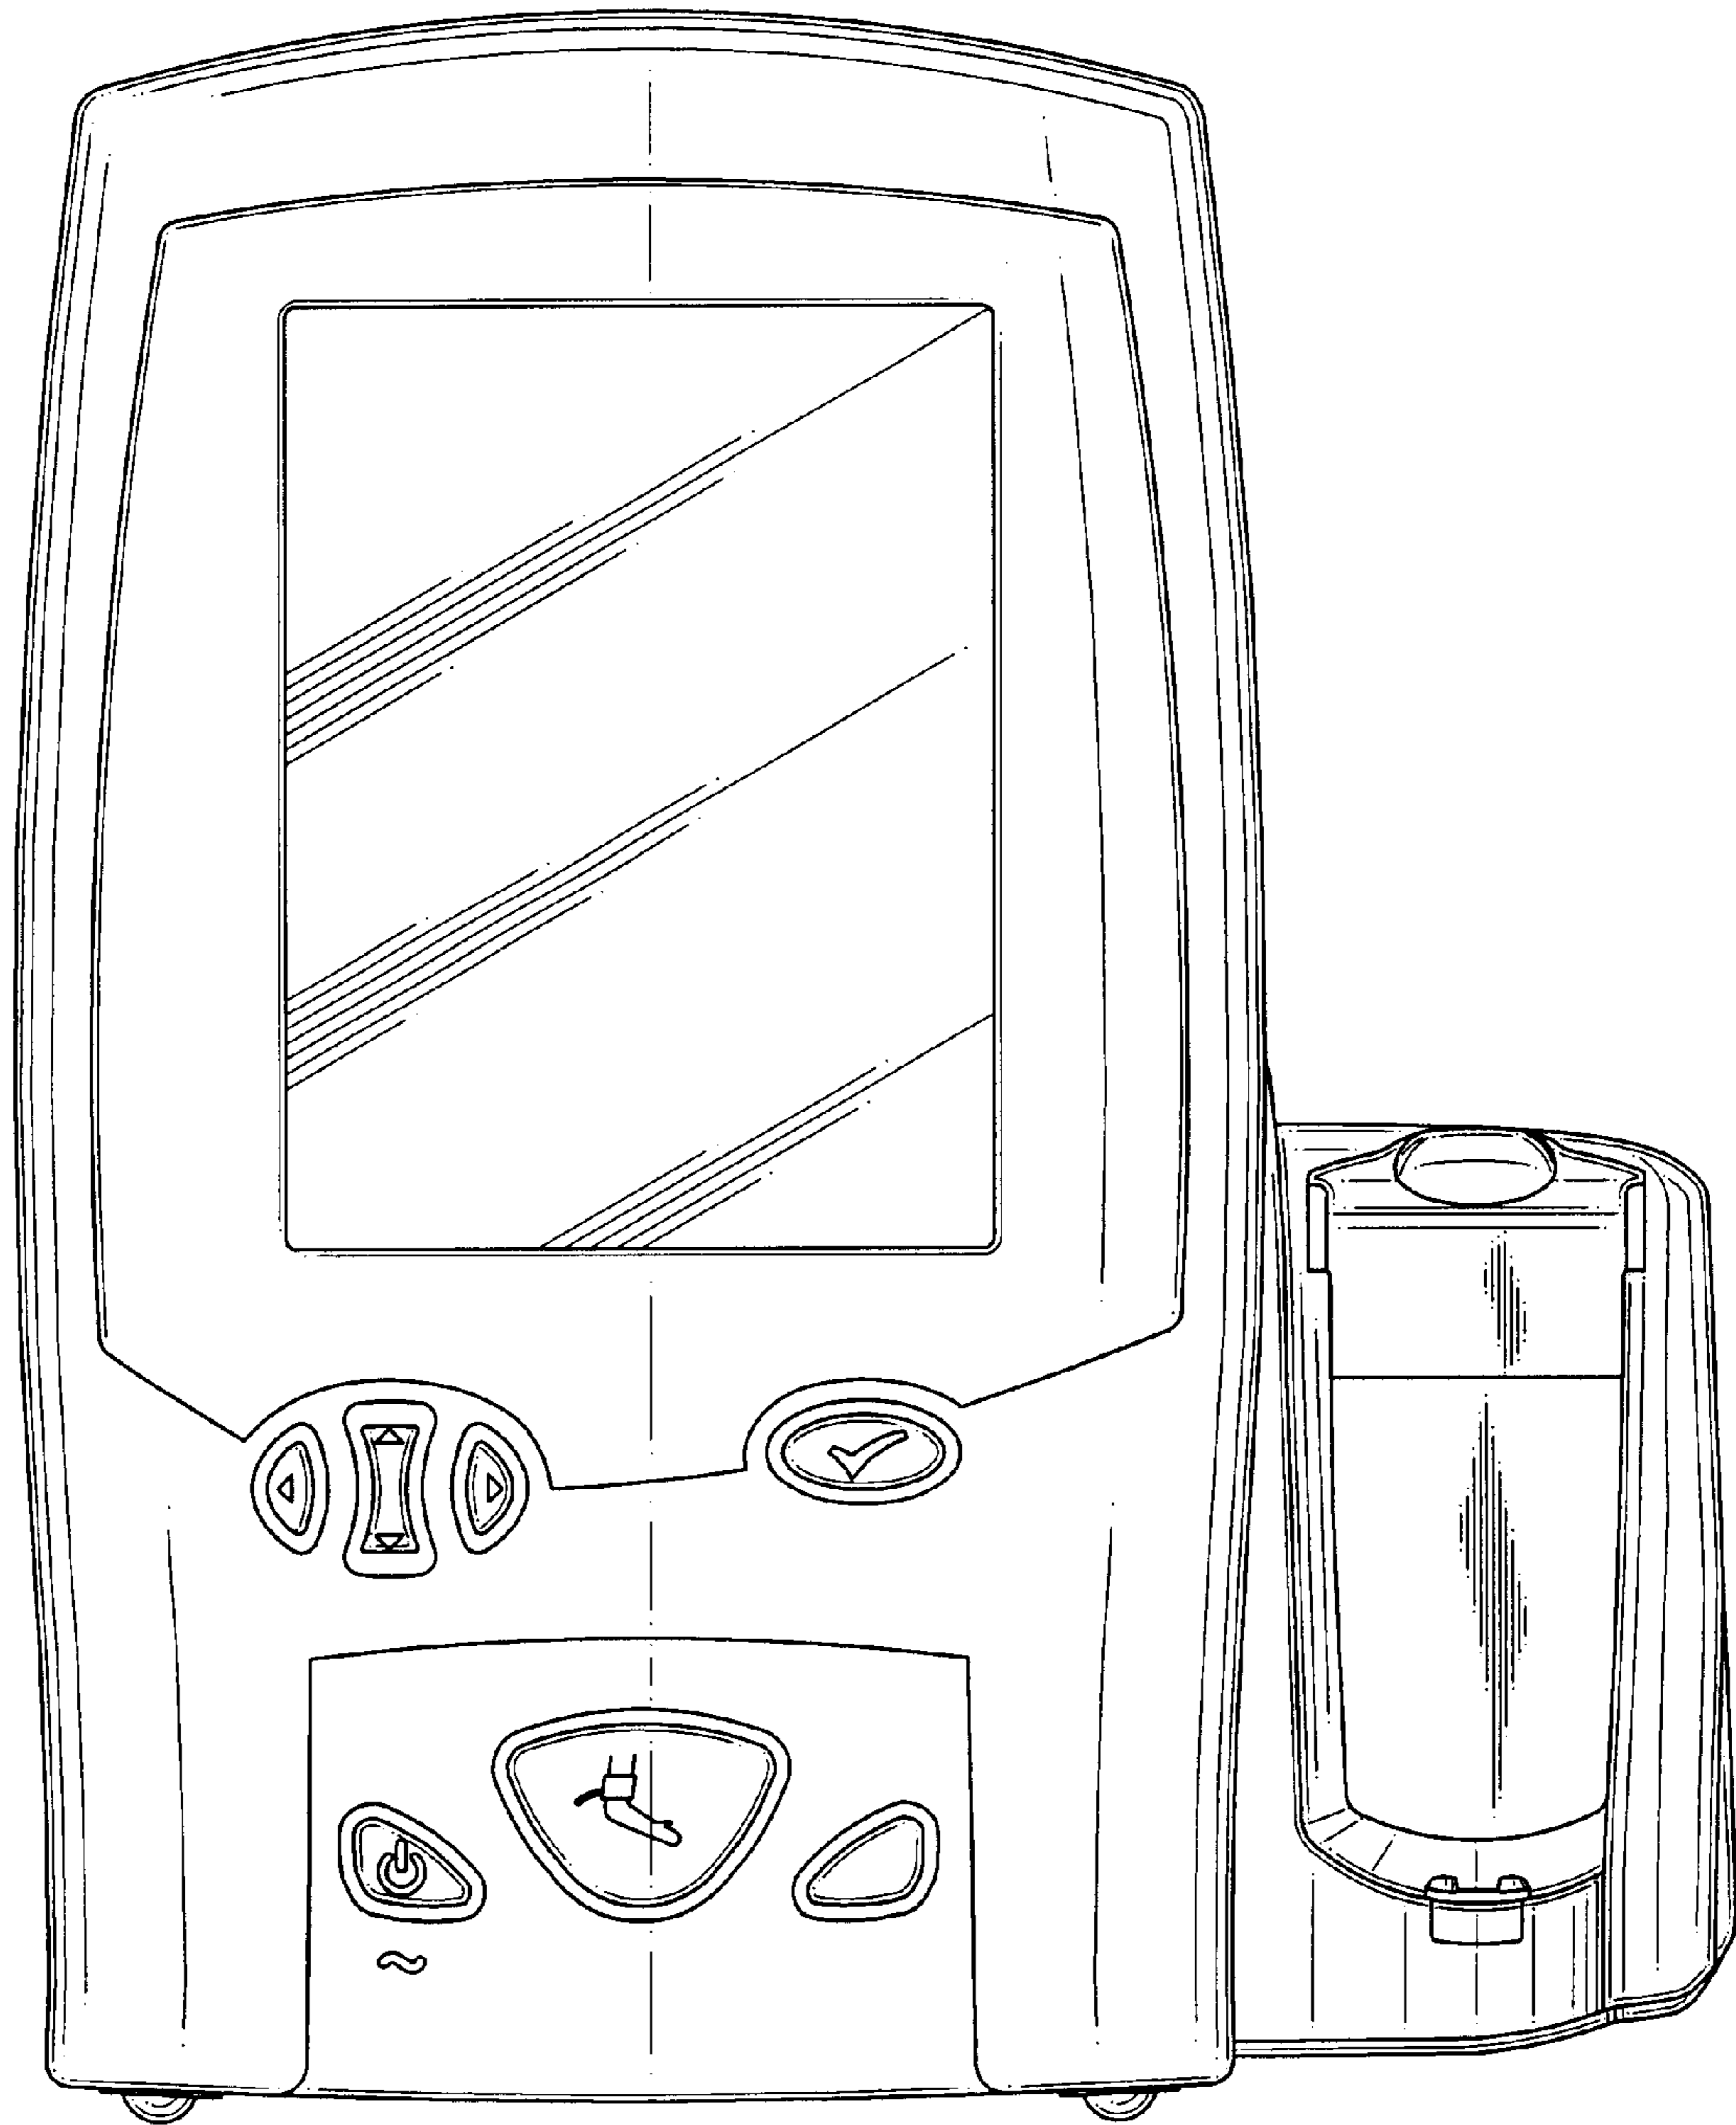


FIG.2

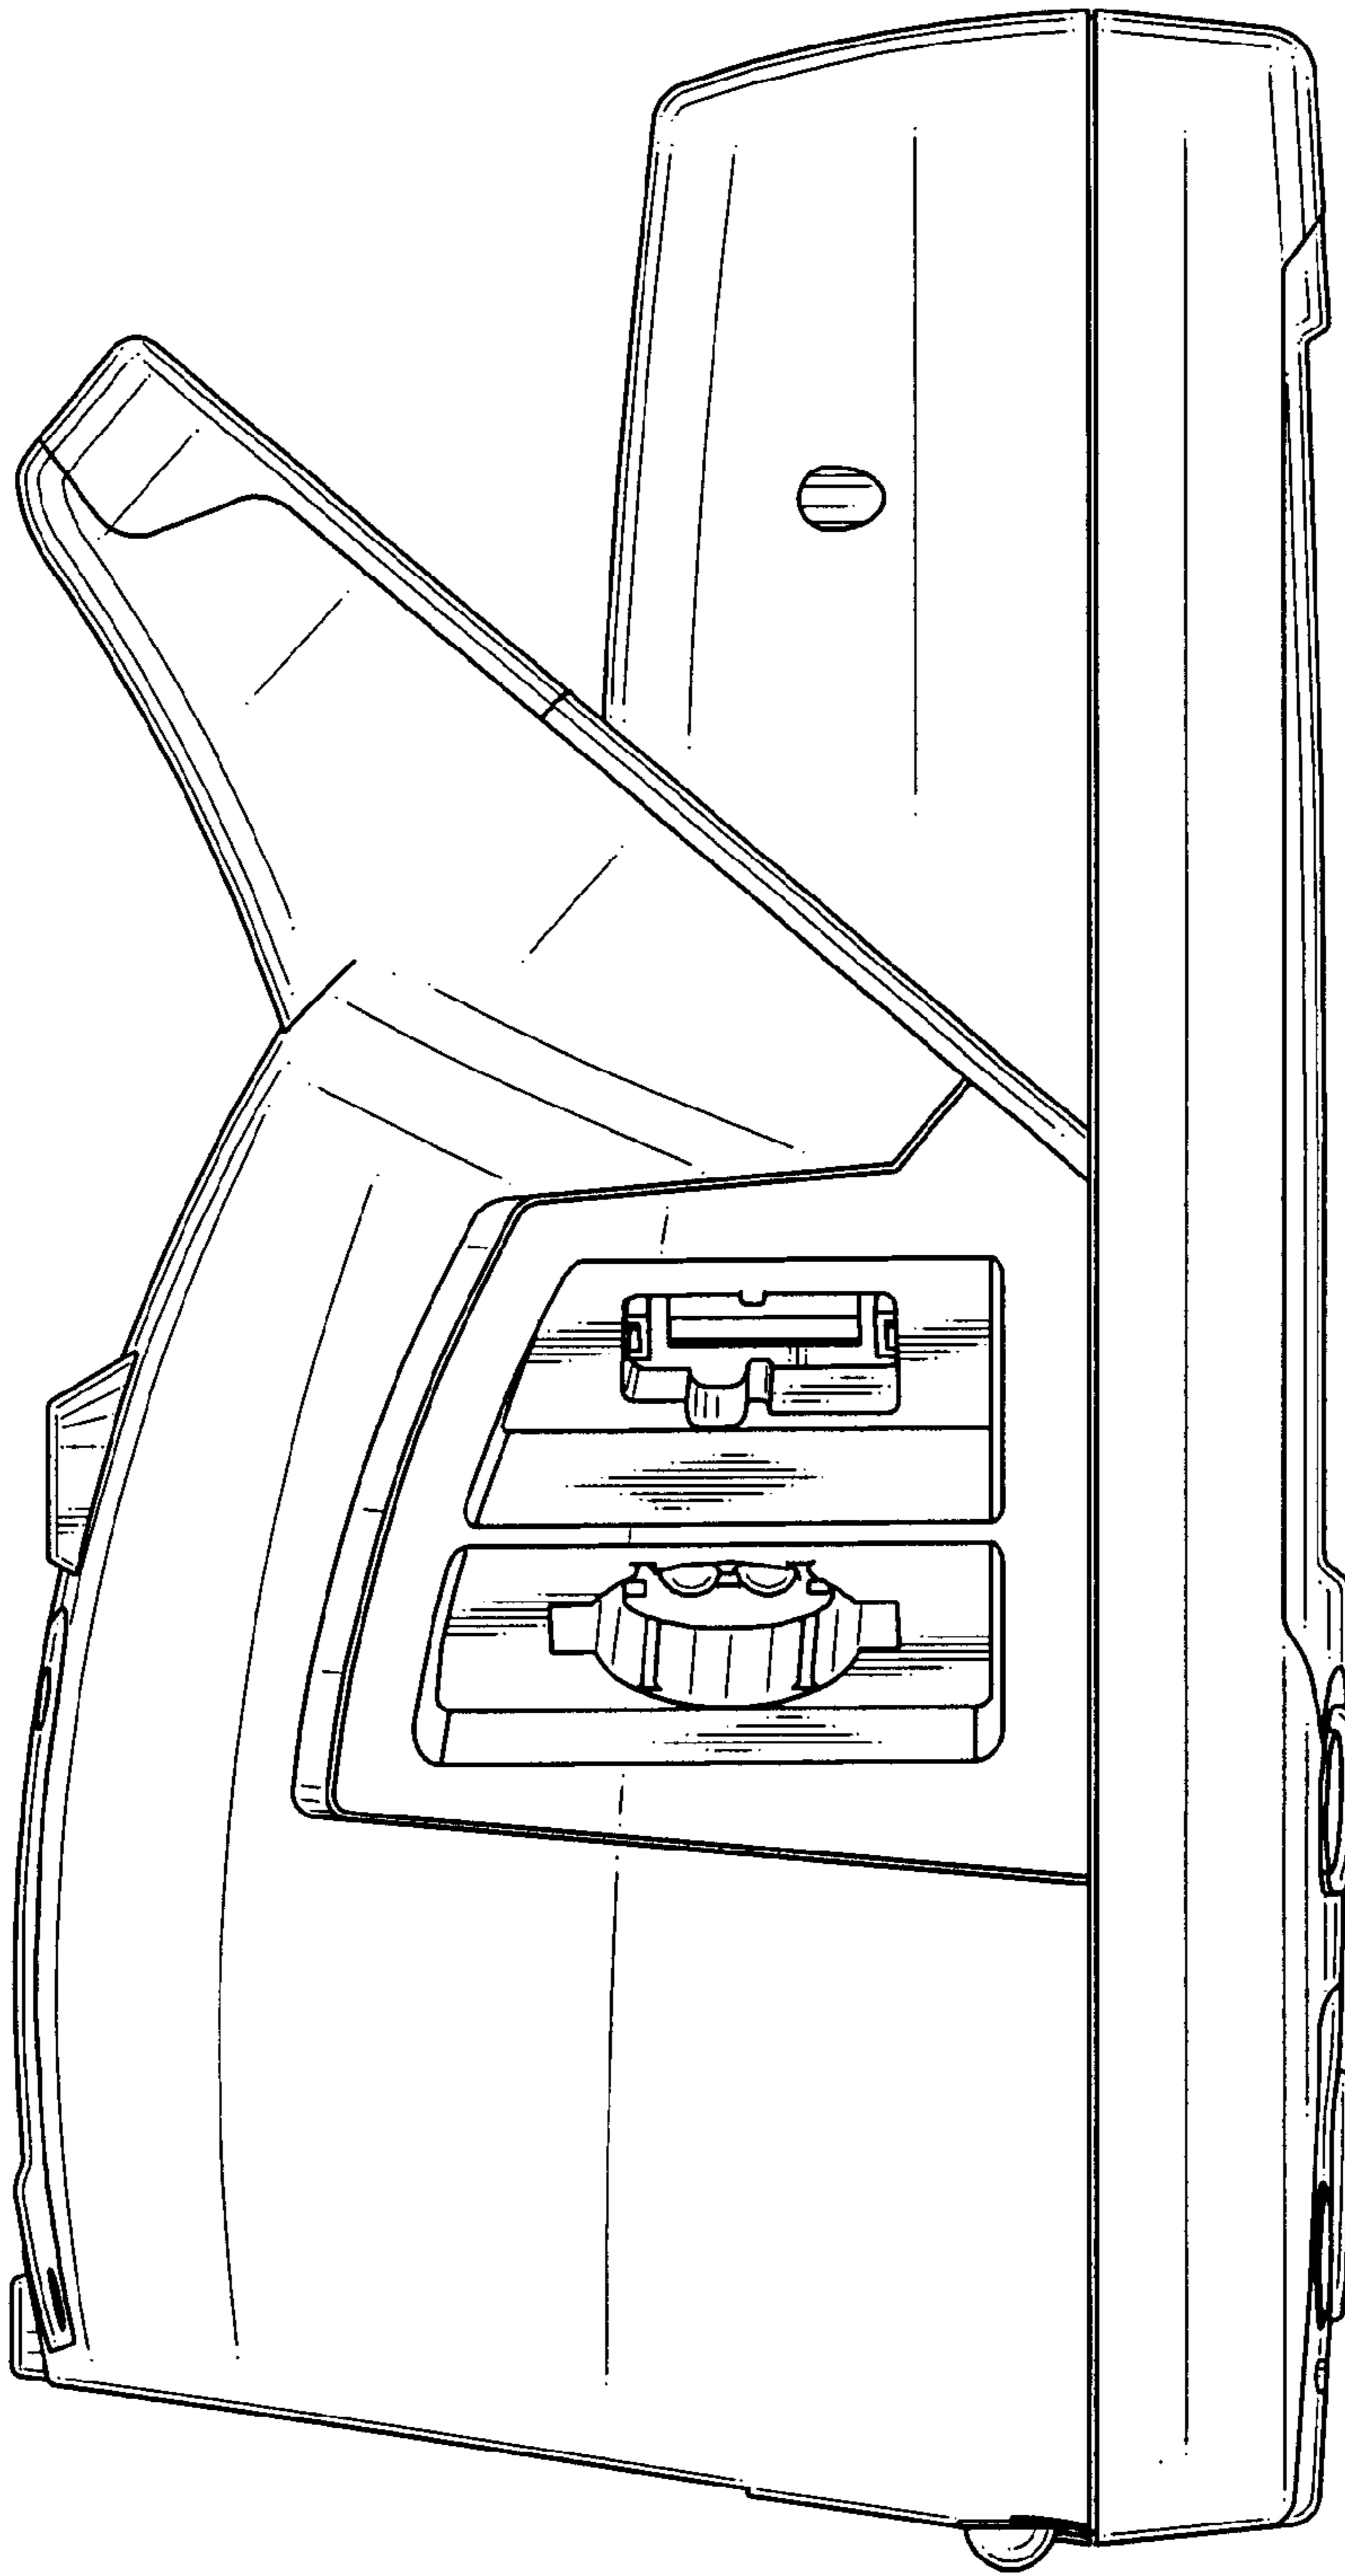


FIG.3

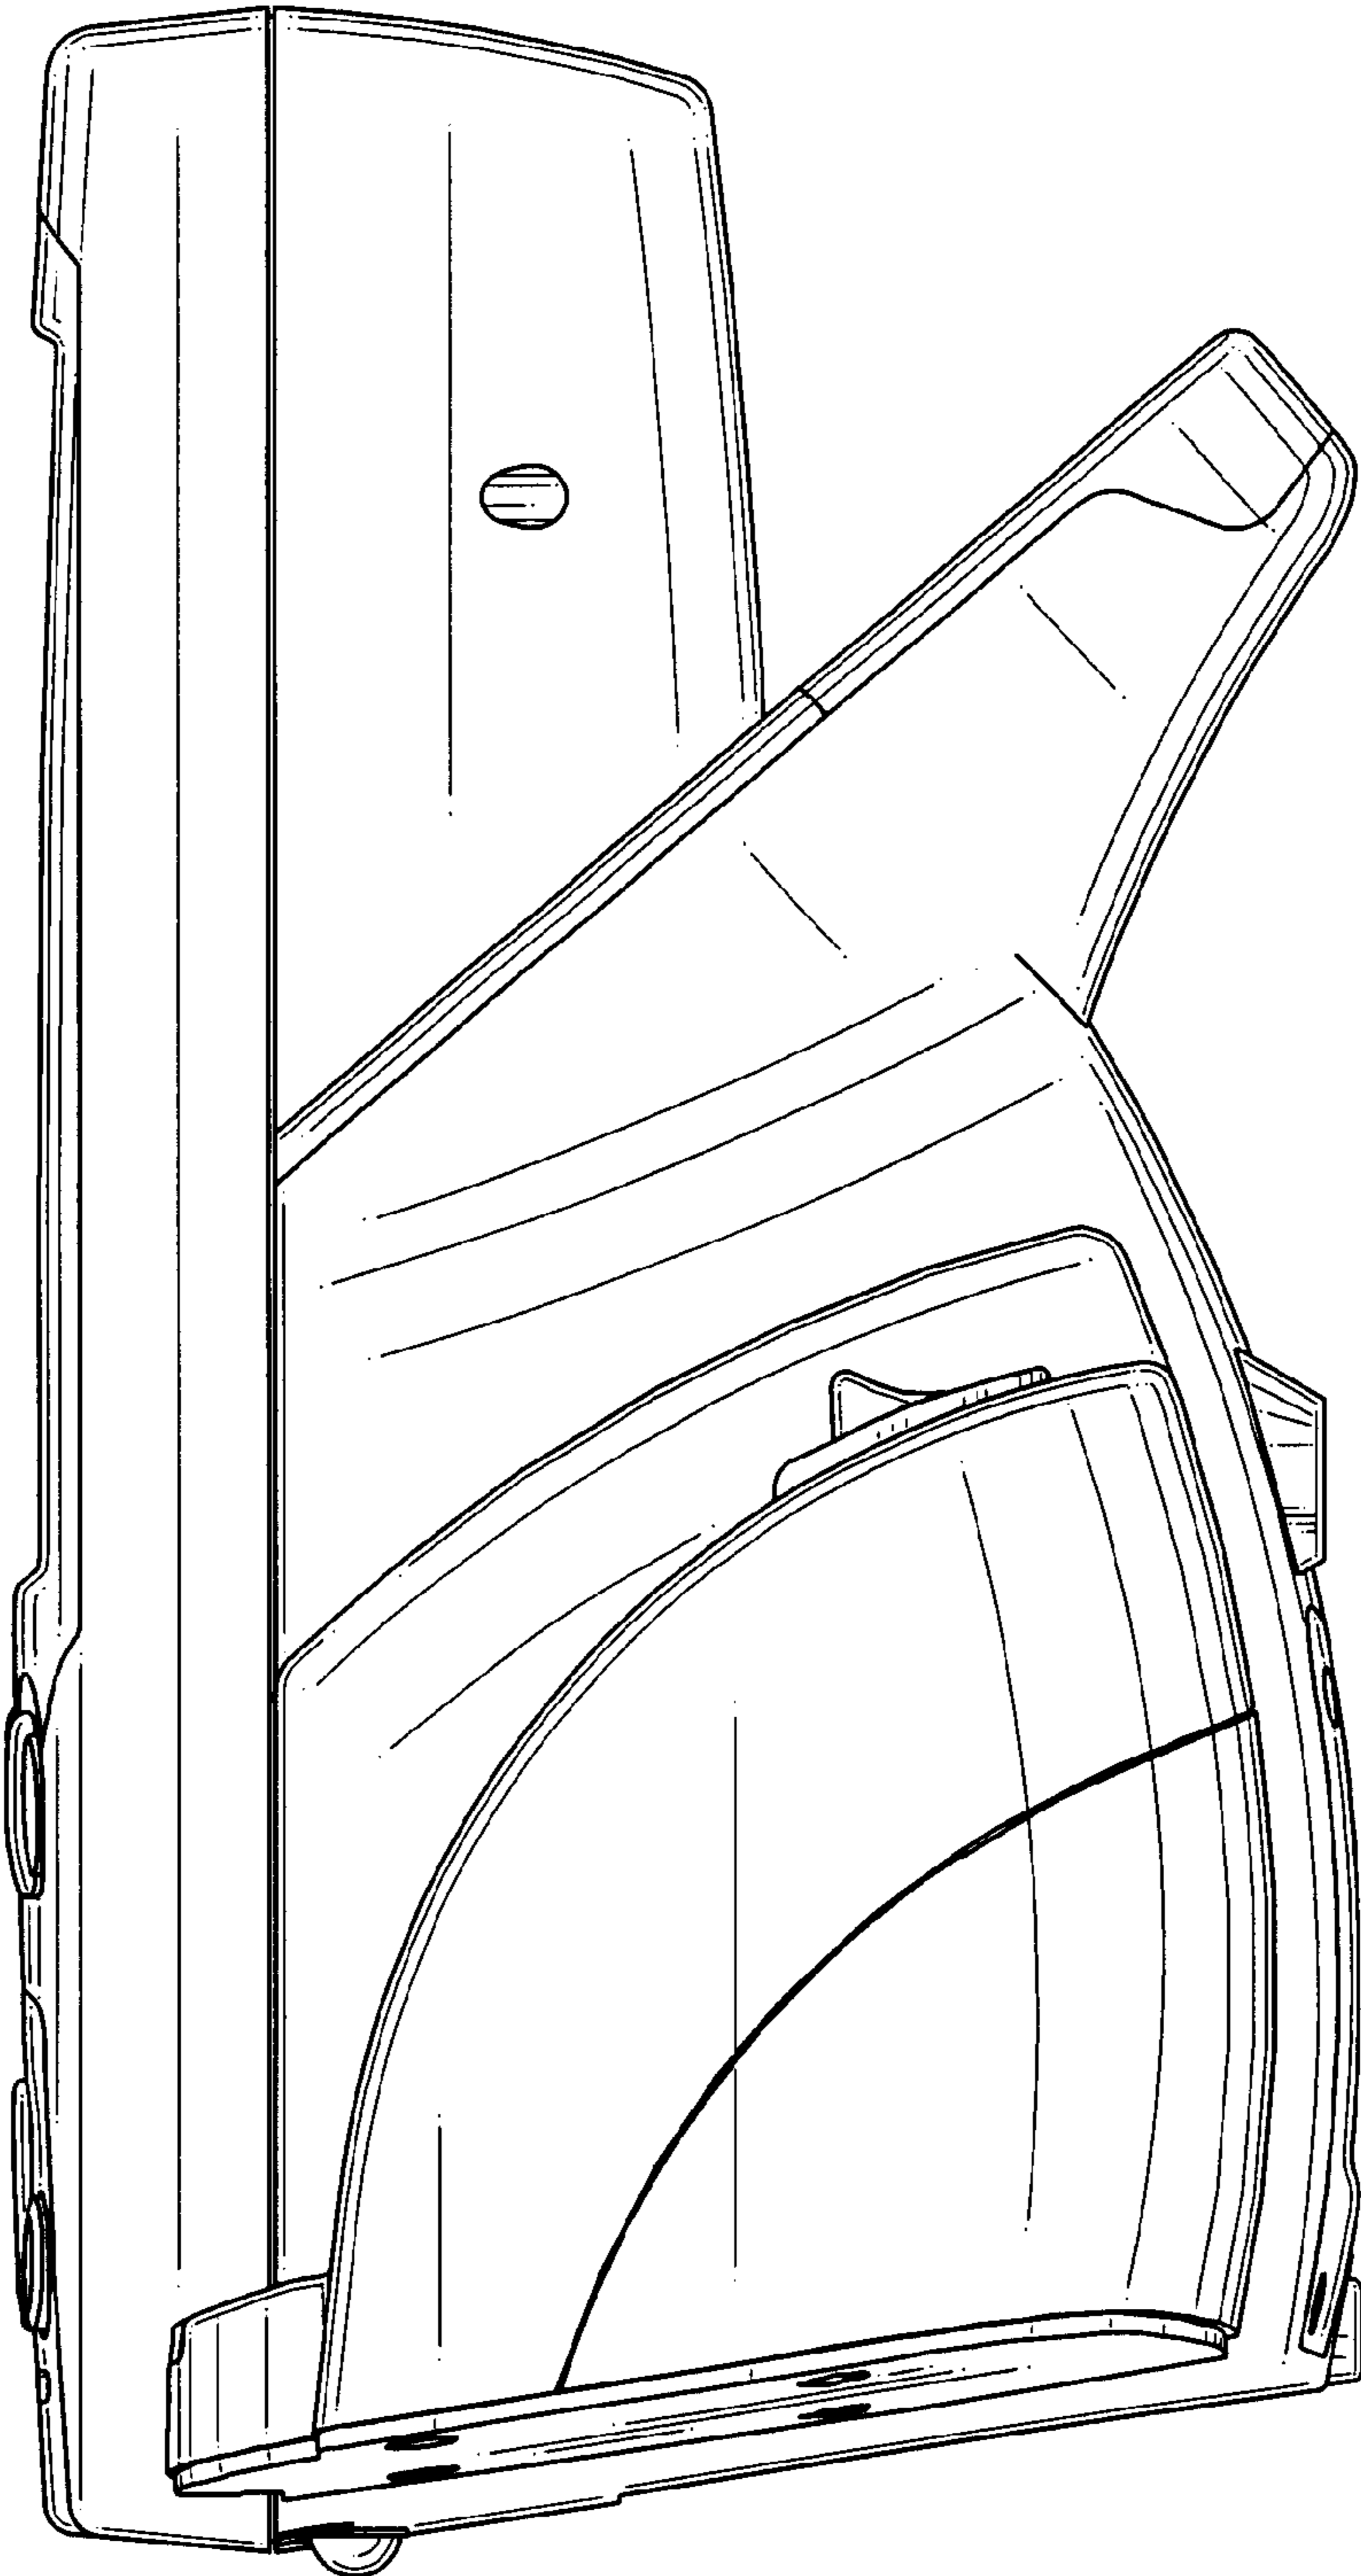


FIG. 4

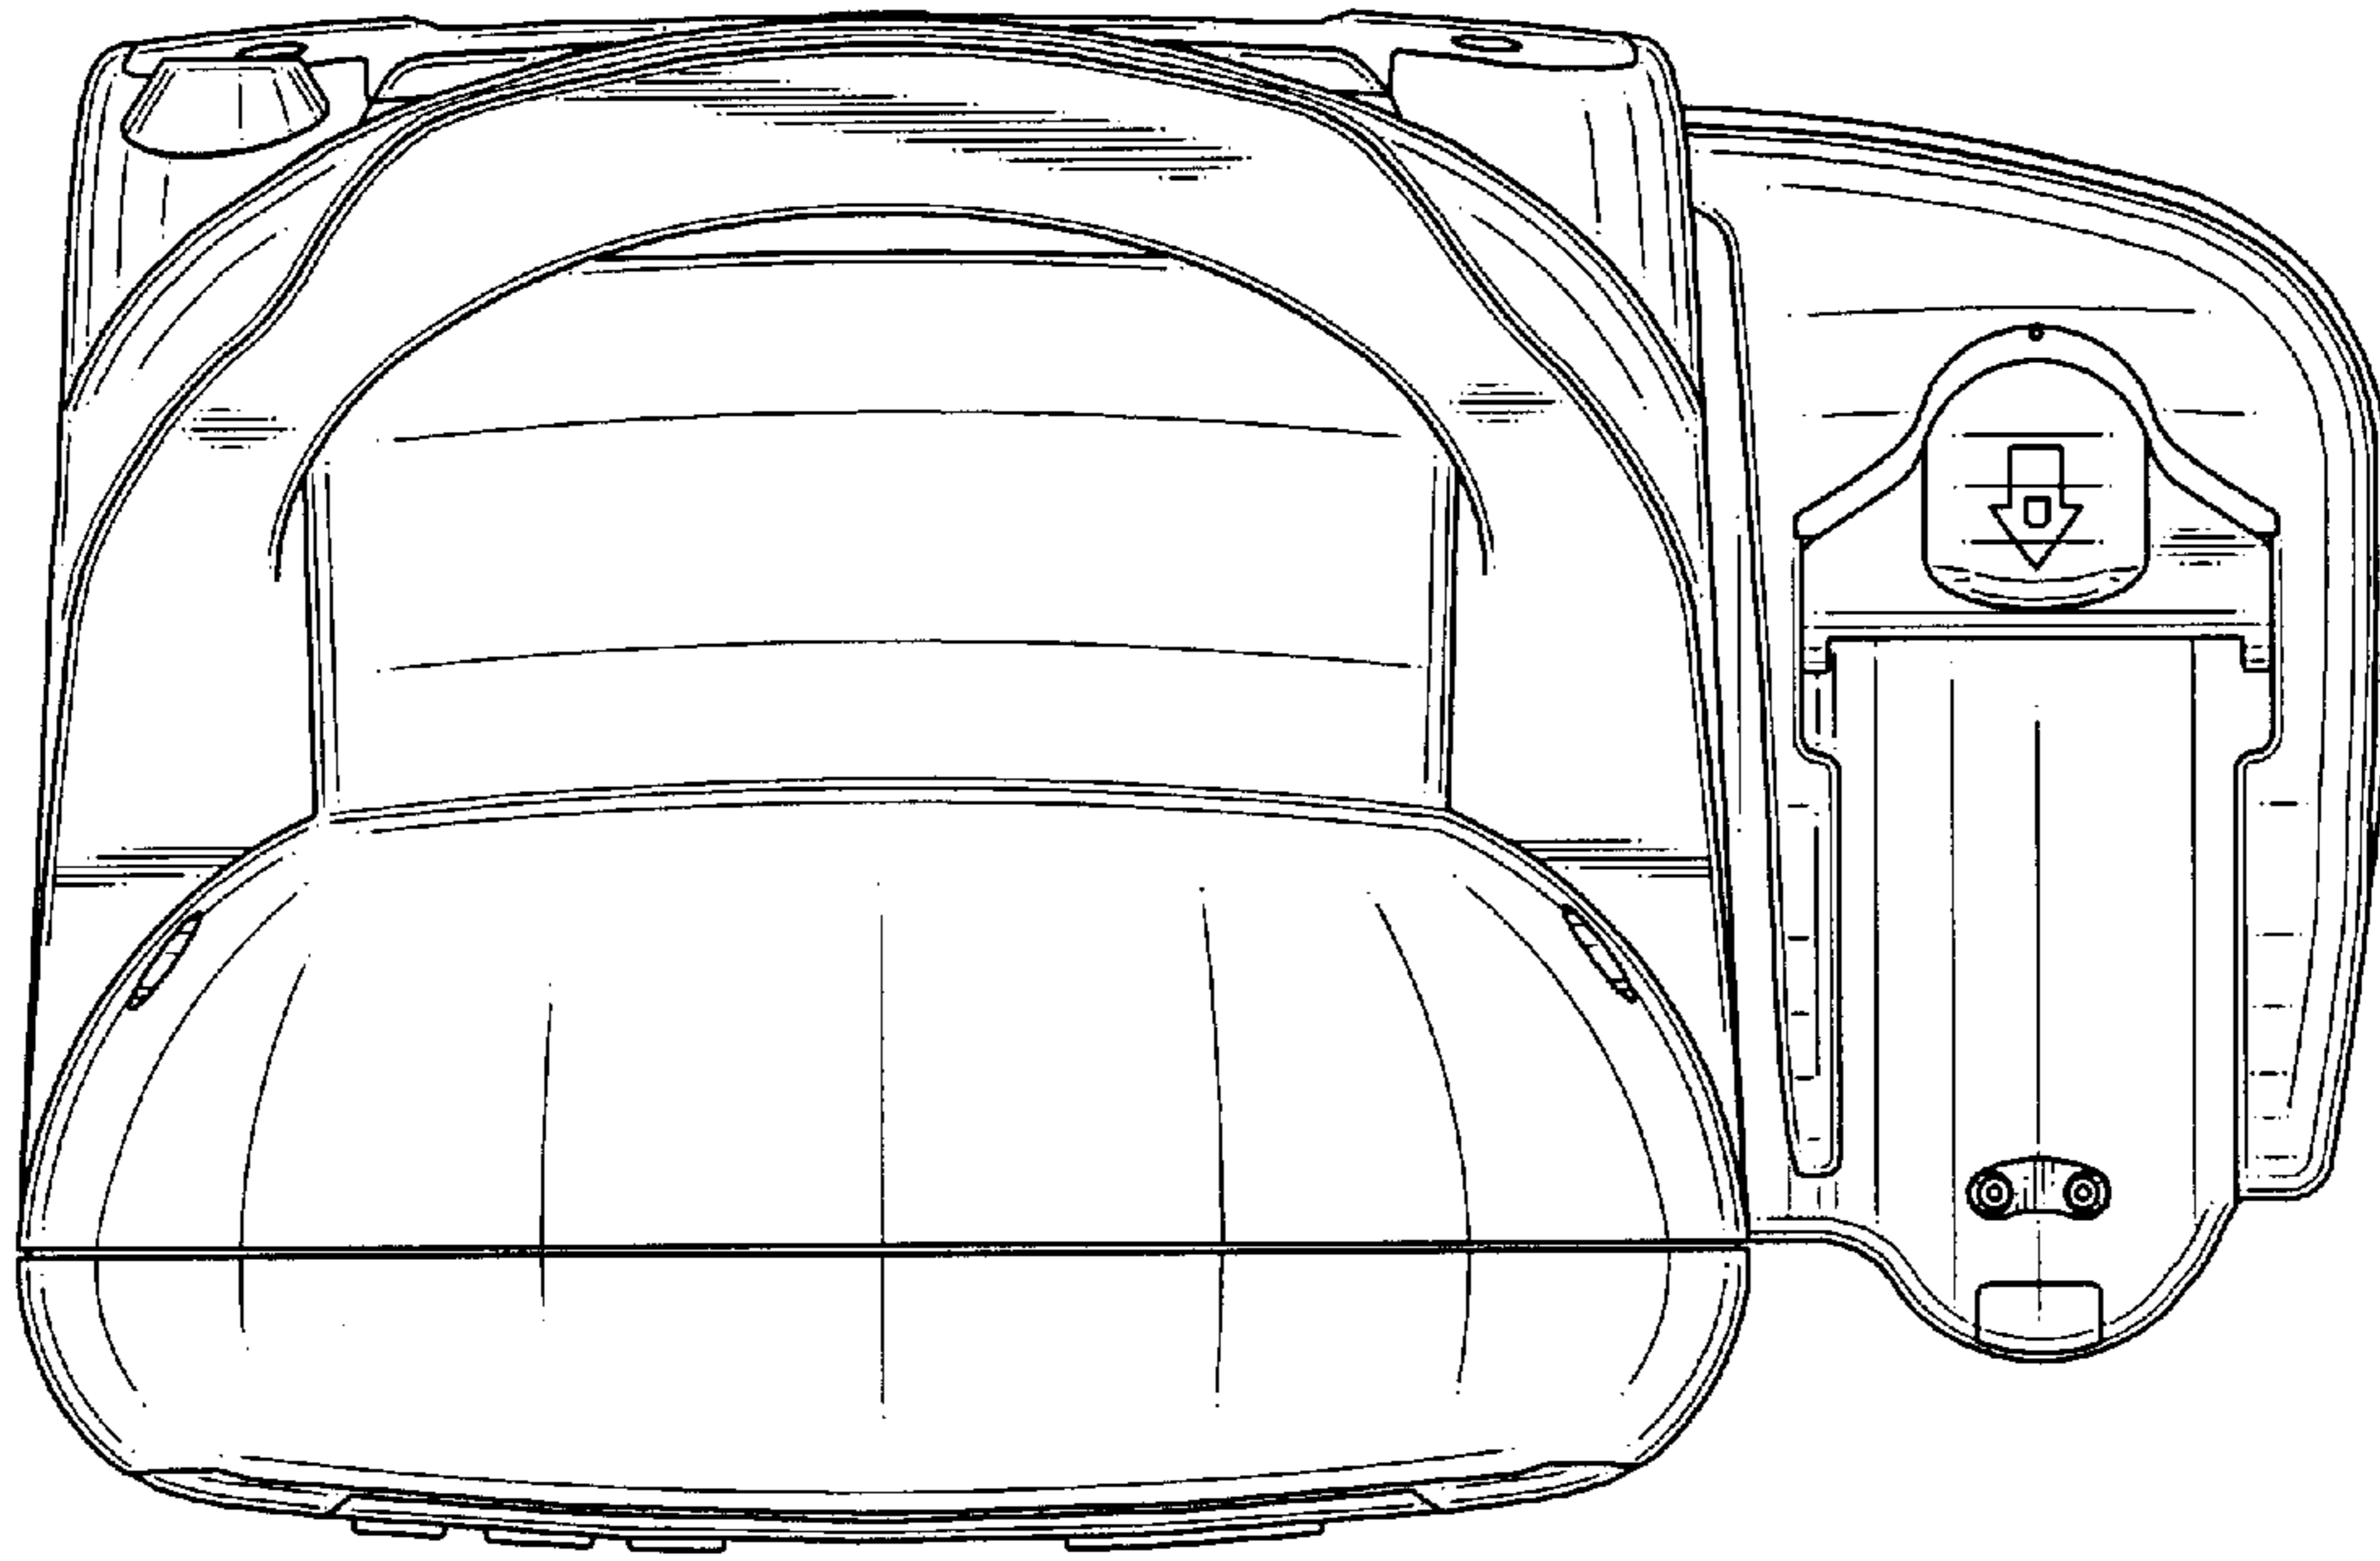


FIG. 5

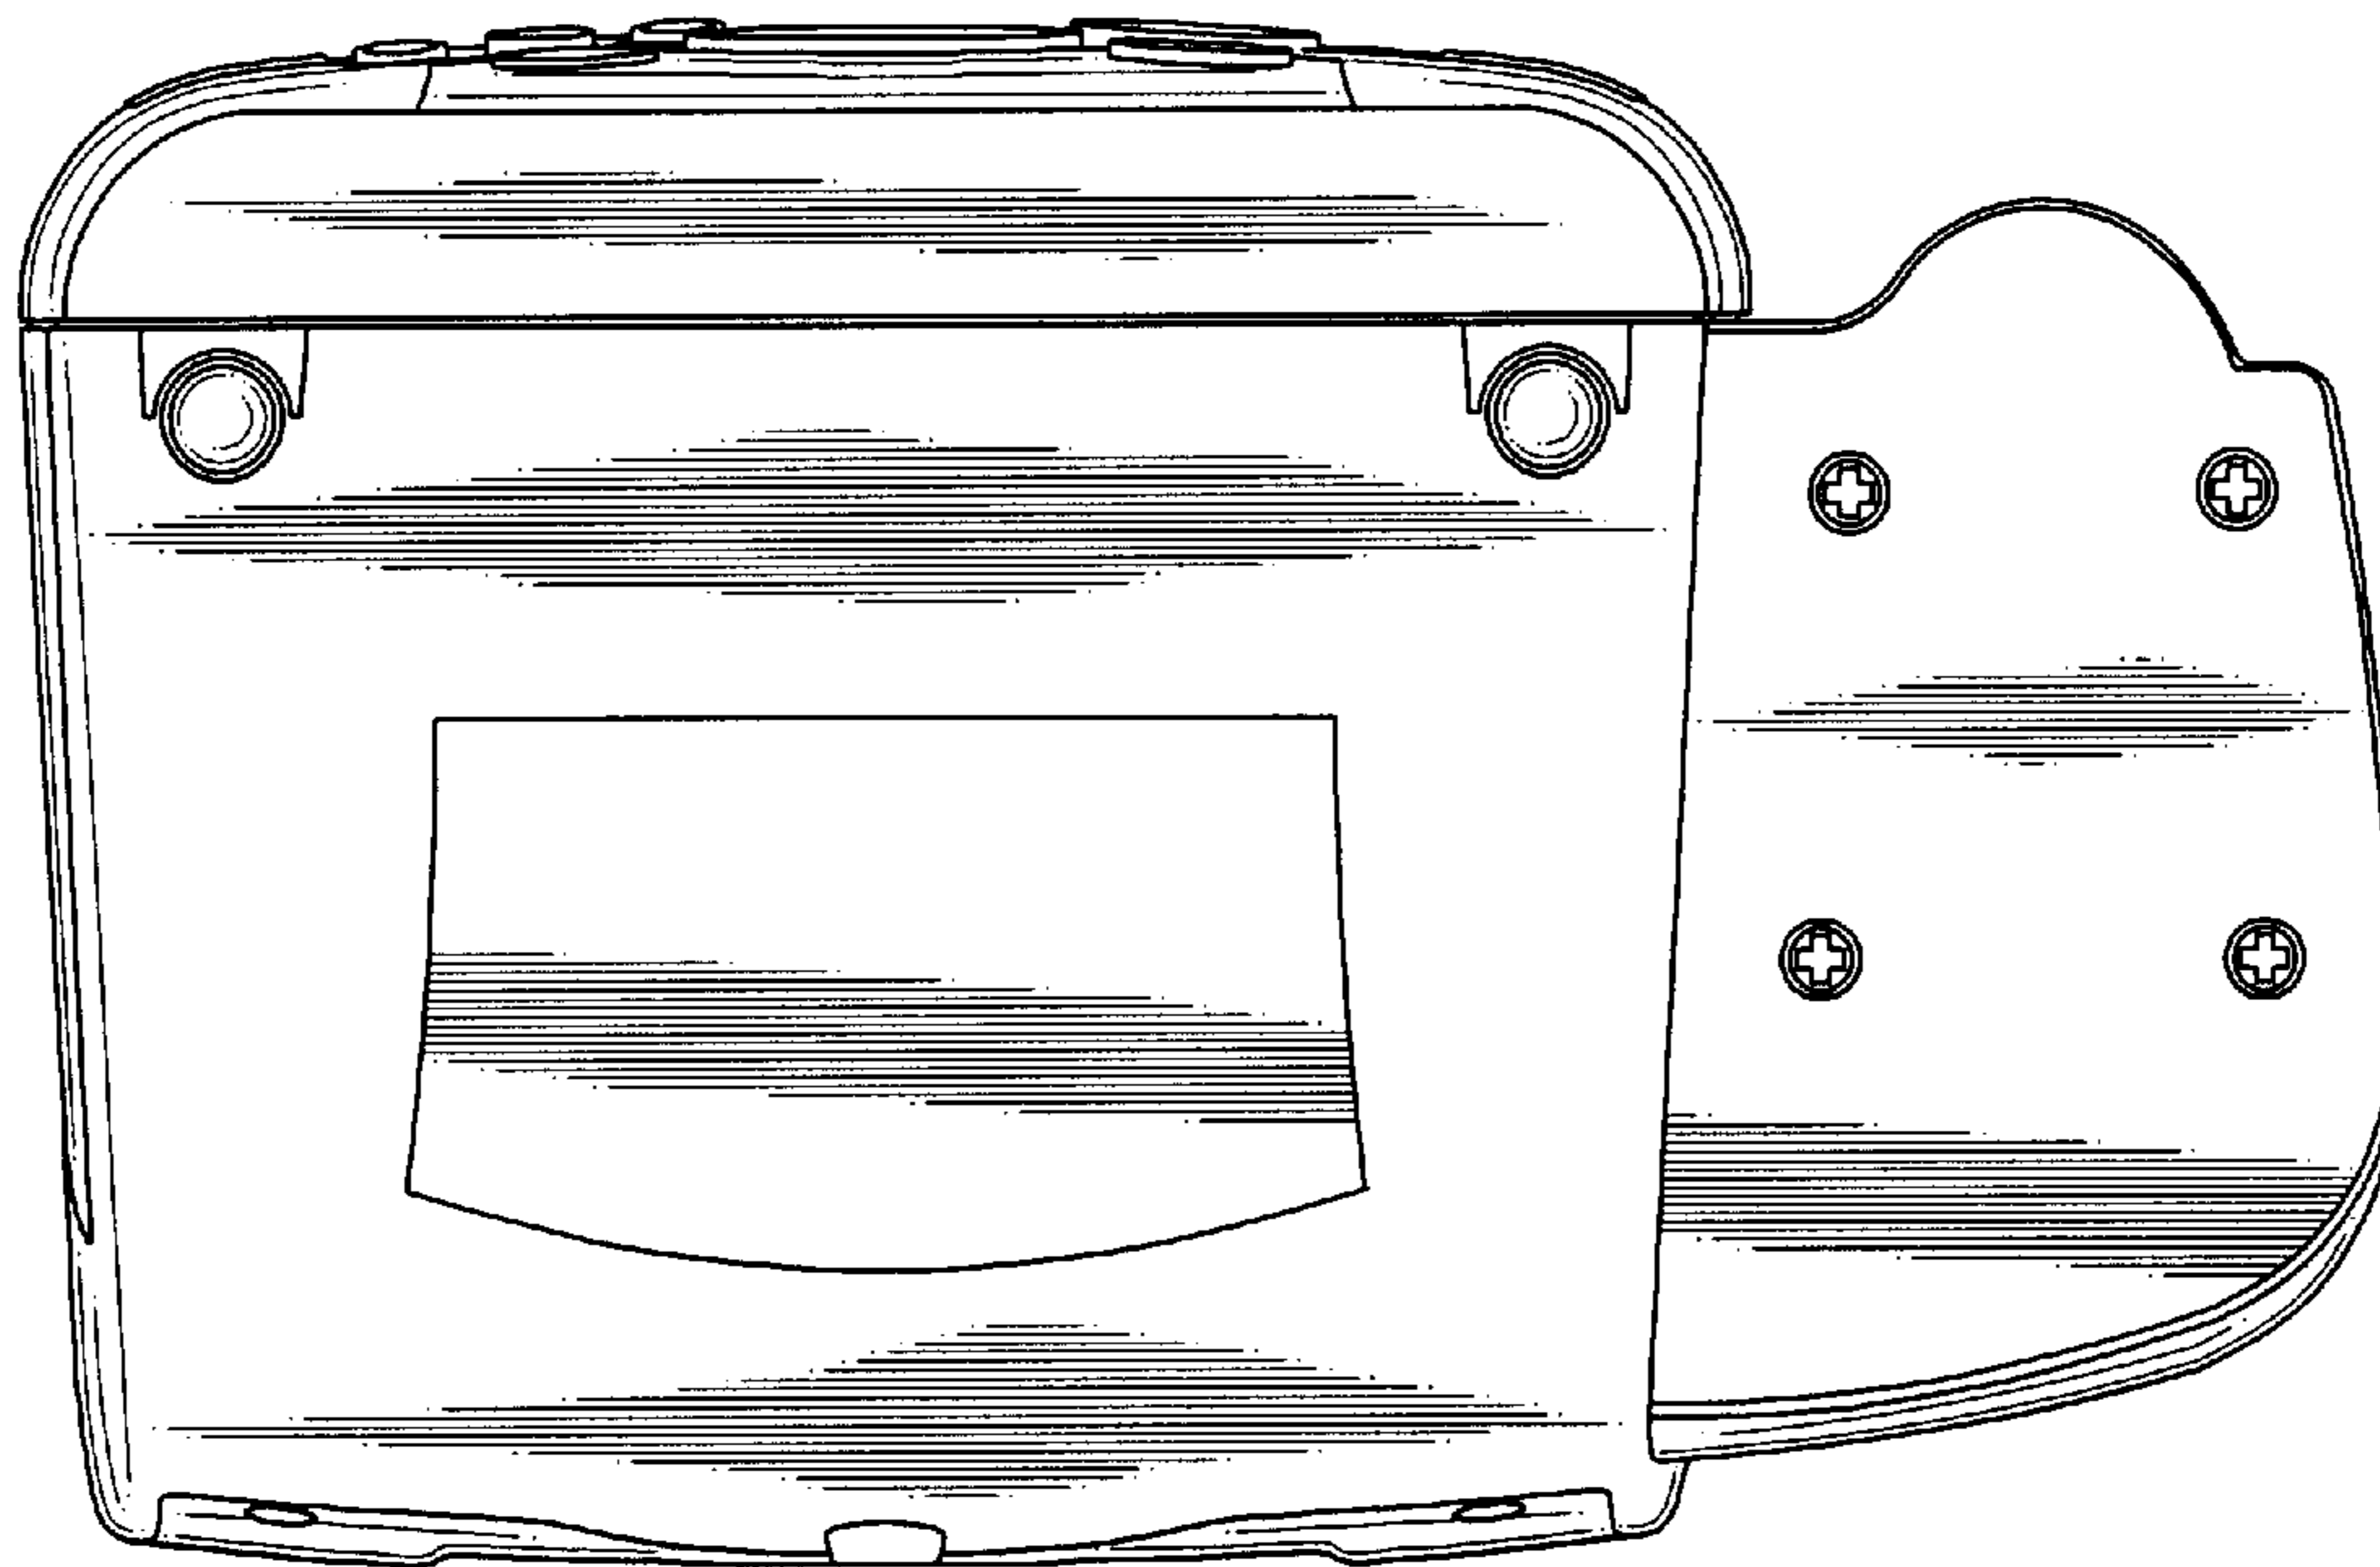


FIG. 6

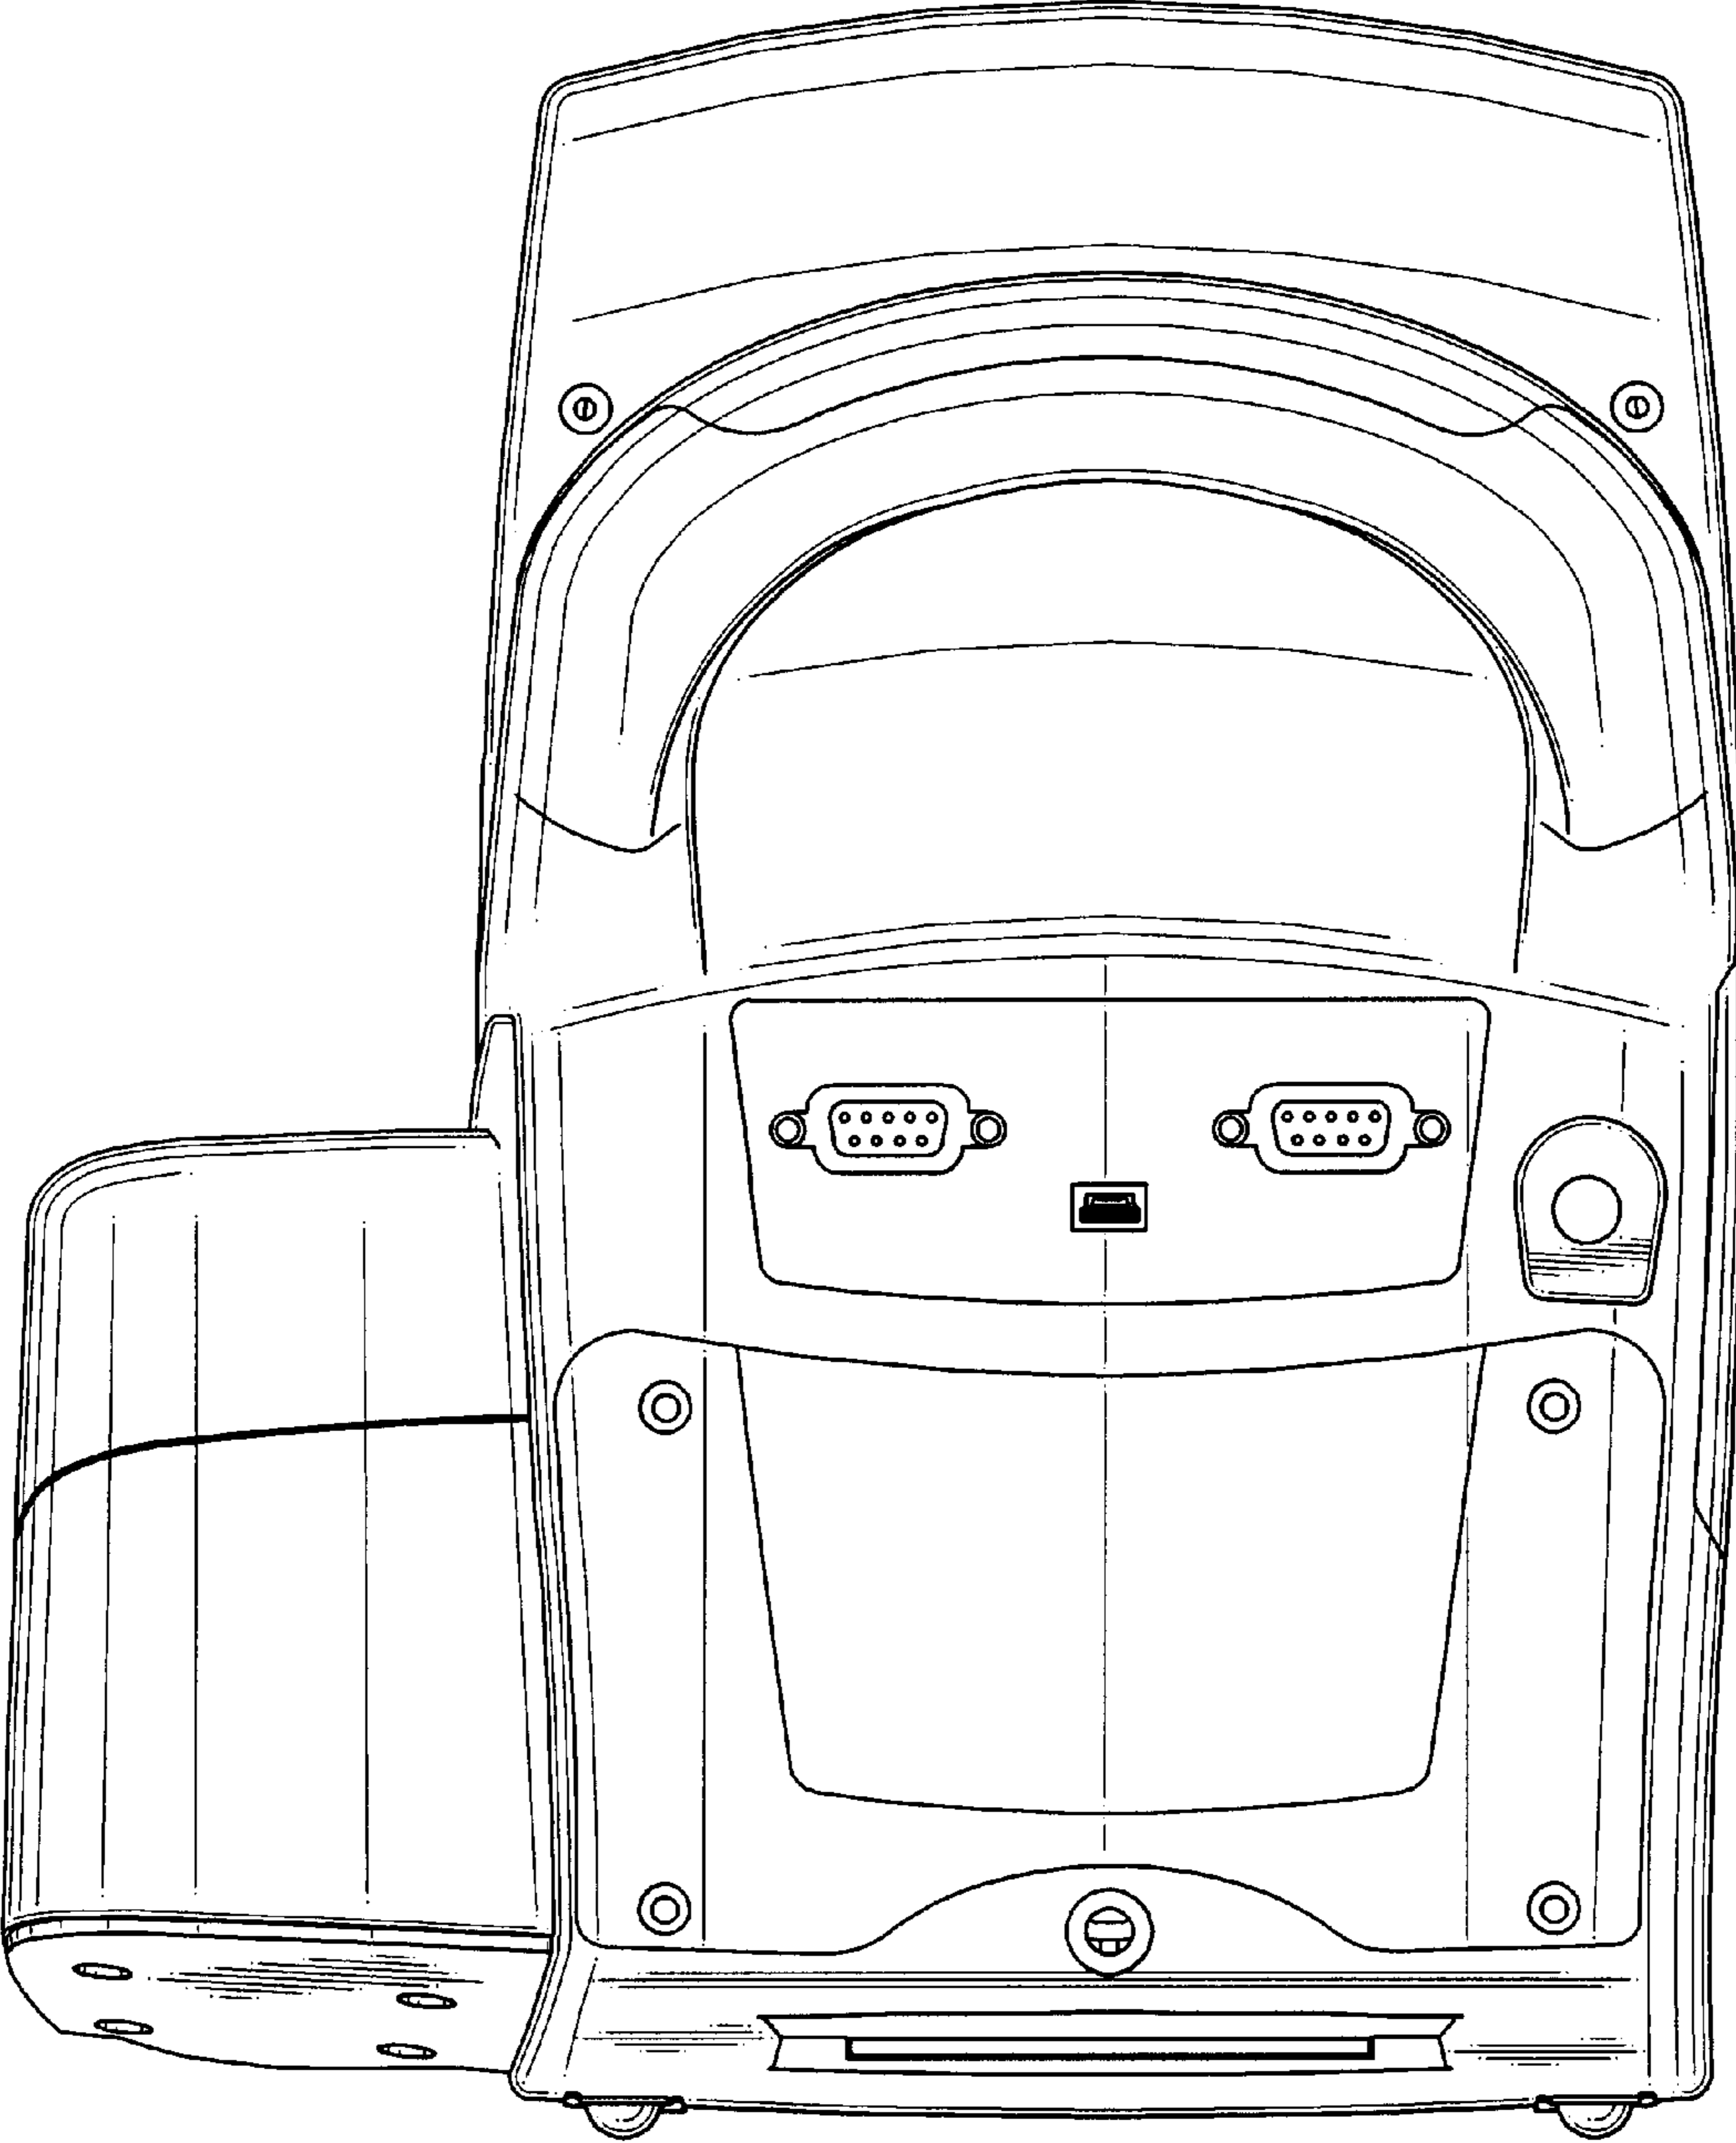


FIG.7