

US00D540945S

(12) **United States Design Patent**
Darnold et al.

(10) **Patent No.:** **US D540,945 S**

(45) **Date of Patent:** **** Apr. 17, 2007**

(54) **PERIODONTAL SCALING TIP FOR
ULTRASONIC DENTAL HANDPIECE**

(75) Inventors: **Leane Darnold**, Kirkwood, MO (US);
Doxey Phillips, Huntleigh, MO (US)

(73) Assignee: **Young OS, LC**, Fenton, MO (US)

(**) Term: **14 Years**

(21) Appl. No.: **29/199,700**

(22) Filed: **Feb. 18, 2004**

(51) **LOC (8) Cl.** **24-02**

(52) **U.S. Cl.** **D24/152; D24/133; D24/146;**
D24/147; D24/156

(58) **Field of Classification Search** D24/111,
D24/146, 156, 176, 217, 147, 144, 112; 451/165,
451/28, 910; 433/119, 165, 125, 29, 215,
433/141, 86

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

3,645,255	A	2/1972	Robinson	
4,283,175	A	8/1981	Nash	
D267,036	S *	11/1982	Podszus et al.	D24/146
D288,242	S *	2/1987	Govenius	D24/112
4,731,019	A	3/1988	Martin	
D297,054	S *	8/1988	Williams	D24/112
D321,400	S *	11/1991	Beckman et al.	D24/147
5,094,617	A	3/1992	Carr	
5,244,390	A	9/1993	Lazzara et al.	
D344,131	S *	2/1994	Hubbell	D24/112
D357,065	S *	4/1995	Castellini	D24/112
D359,118	S *	6/1995	Nates	D24/112
D359,119	S *	6/1995	Dragan et al.	D24/176
5,567,153	A	10/1996	Foulkes et al.	
5,704,787	A	1/1998	Hickok et al.	
5,733,119	A	3/1998	Carr	
5,785,521	A *	7/1998	Rizoiu et al.	433/29
5,836,765	A	11/1998	Hickok	
D437,937	S *	2/2001	Bottjer	D24/144
D438,954	S *	3/2001	Orsing	D24/112
6,663,386	B1 *	12/2003	Moelsgaard	433/29

6,722,882	B2	4/2004	Buchanan	
D509,588	S *	9/2005	Vercellotti et al.	D24/144
2002/0072035	A1	6/2002	Hickok	
2003/0096213	A1	5/2003	Hickok et al.	
2003/0157458	A1	8/2003	Buchanan	

OTHER PUBLICATIONS

Brochure of CPR Endodontic Instruments with Zirconium Nitride Coating/Spartan USA/2 pages.

(Continued)

Primary Examiner—Ian Simmons

Assistant Examiner—W. Laymon

(74) *Attorney, Agent, or Firm*—Polster, Lieder, Woodruff & Lucchesi, L.C.

(57) **CLAIM**

The ornamental design for a periodontal scaling tip for ultrasonic dental handpiece, as shown and described.

DESCRIPTION

FIG. 1 is a perspective view of a periodontal scaling tip for ultrasonic dental handpiece showing our new design;

FIG. 2 is a top plan view thereof;

FIG. 3 is a bottom plan view thereof;

FIG. 4 is a right elevational view thereof;

FIG. 5 is a left elevational view thereof;

FIG. 6 is a front elevational view thereof;

FIG. 7 is a rear elevational view thereof;

FIG. 8 is a perspective view of the second embodiment design of a periodontal scaling tip for ultrasonic dental handpiece showing our new design;

FIG. 9 is a bottom plan view thereof;

FIG. 10 is a top plan view thereof;

FIG. 11 is a right elevational view thereof;


FIG. 12 is a left elevational view thereof;

FIG. 13 is a front elevational view thereof; and,

FIG. 14 is a rear elevational view thereof.

The broken line showing of the periodontal probe is included for the purpose of illustrating environmental structure and forms no part of the claimed design.

1 Claim, 3 Drawing Sheets

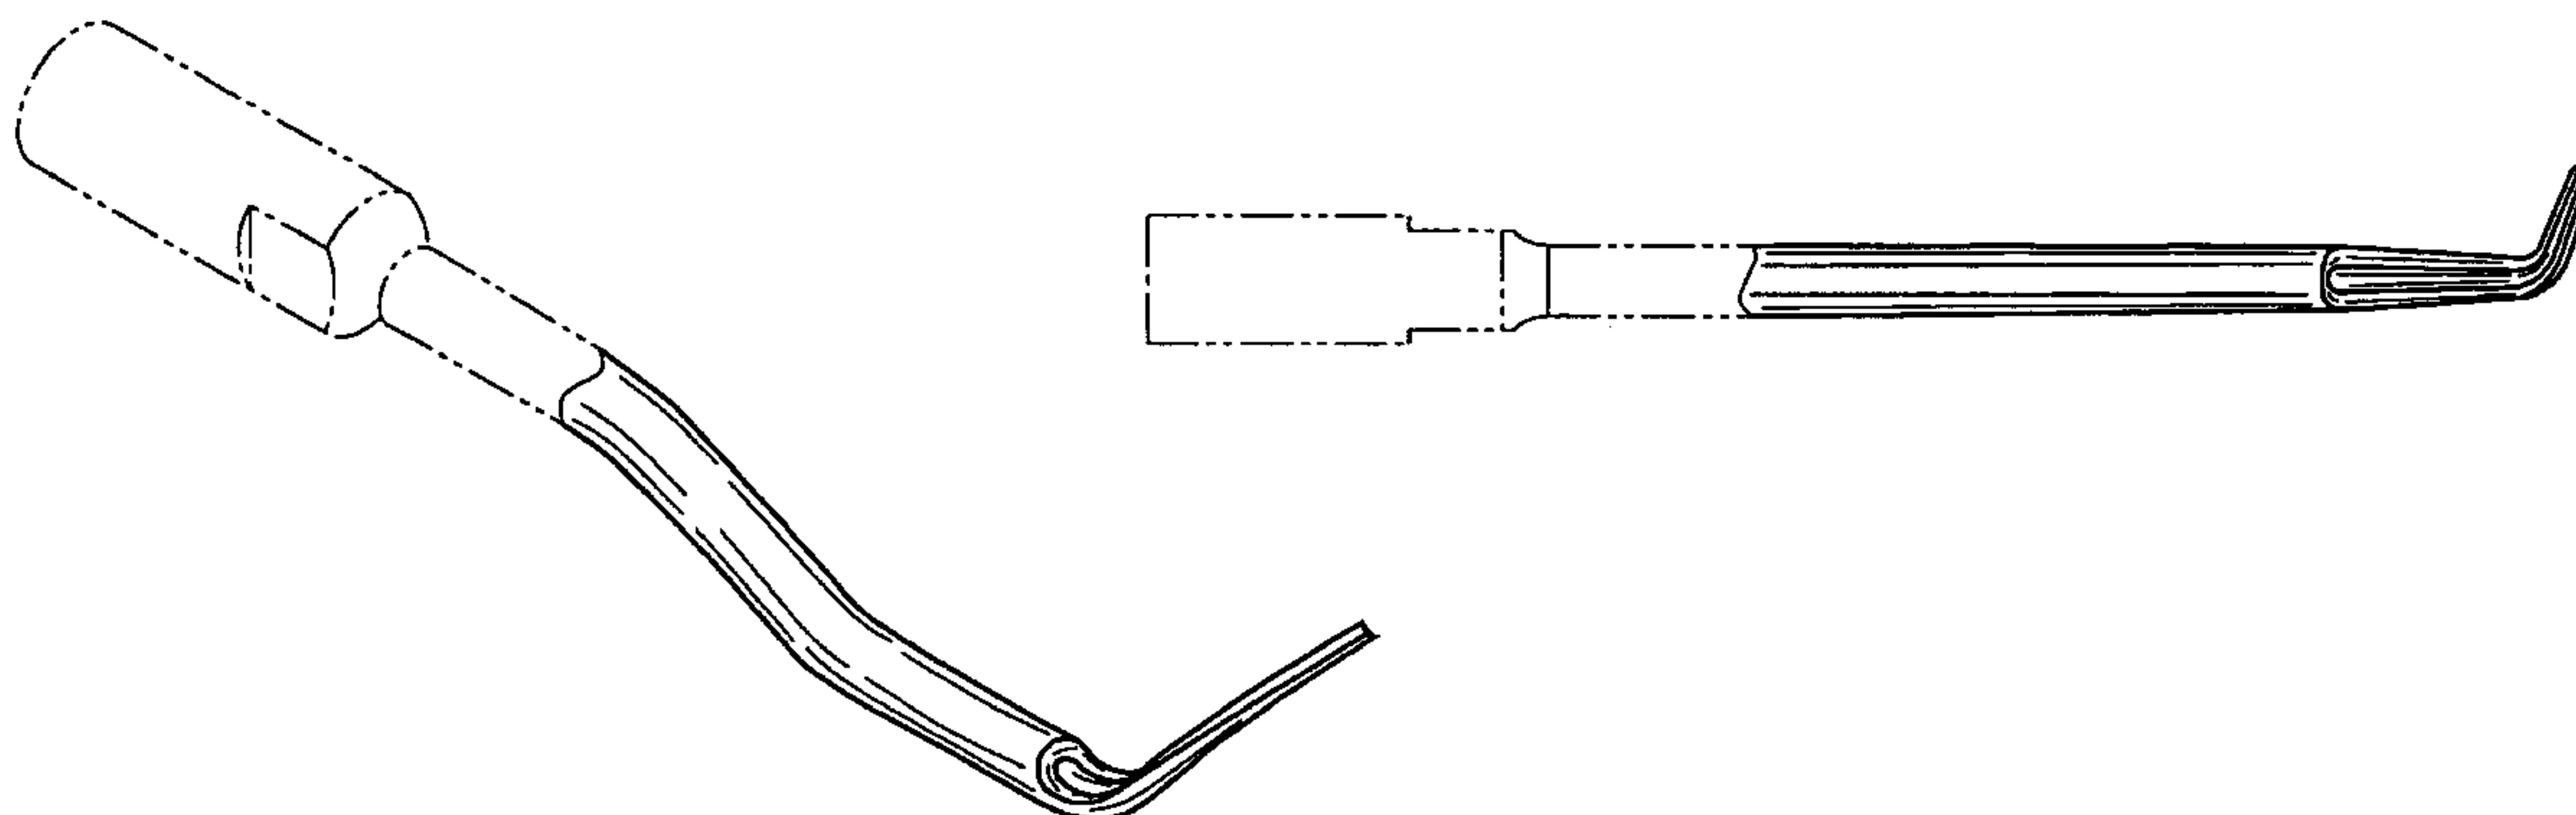

OTHER PUBLICATIONS

Brochure of CPR Endodontic Instruments/Titanium Series/
Spartan USA/2 pages.

1 page/CPR Diamonds/Obtura Spartan.

Image of UFT Tips—1 sheet/Obtura Spartan.

Image of CPR Tips—1 sheet/Obtura Spartan.

Comprehensive Endodontic Solutions brochure/eie Analytic
Technology/5 pages.

New KiS Diamonds brochure/Obtura Spartan/1 page.

BUC Access Refinement Tips brochure/Obtura Spartan/1
page.

ProUltra CPR and ProUltra KiS/Dentsply/1 two-sided bro-
chure.

KiS Microsurgical Ultrasonic Instruments brochure/Obtura
Spartan/1 page.

* cited by examiner

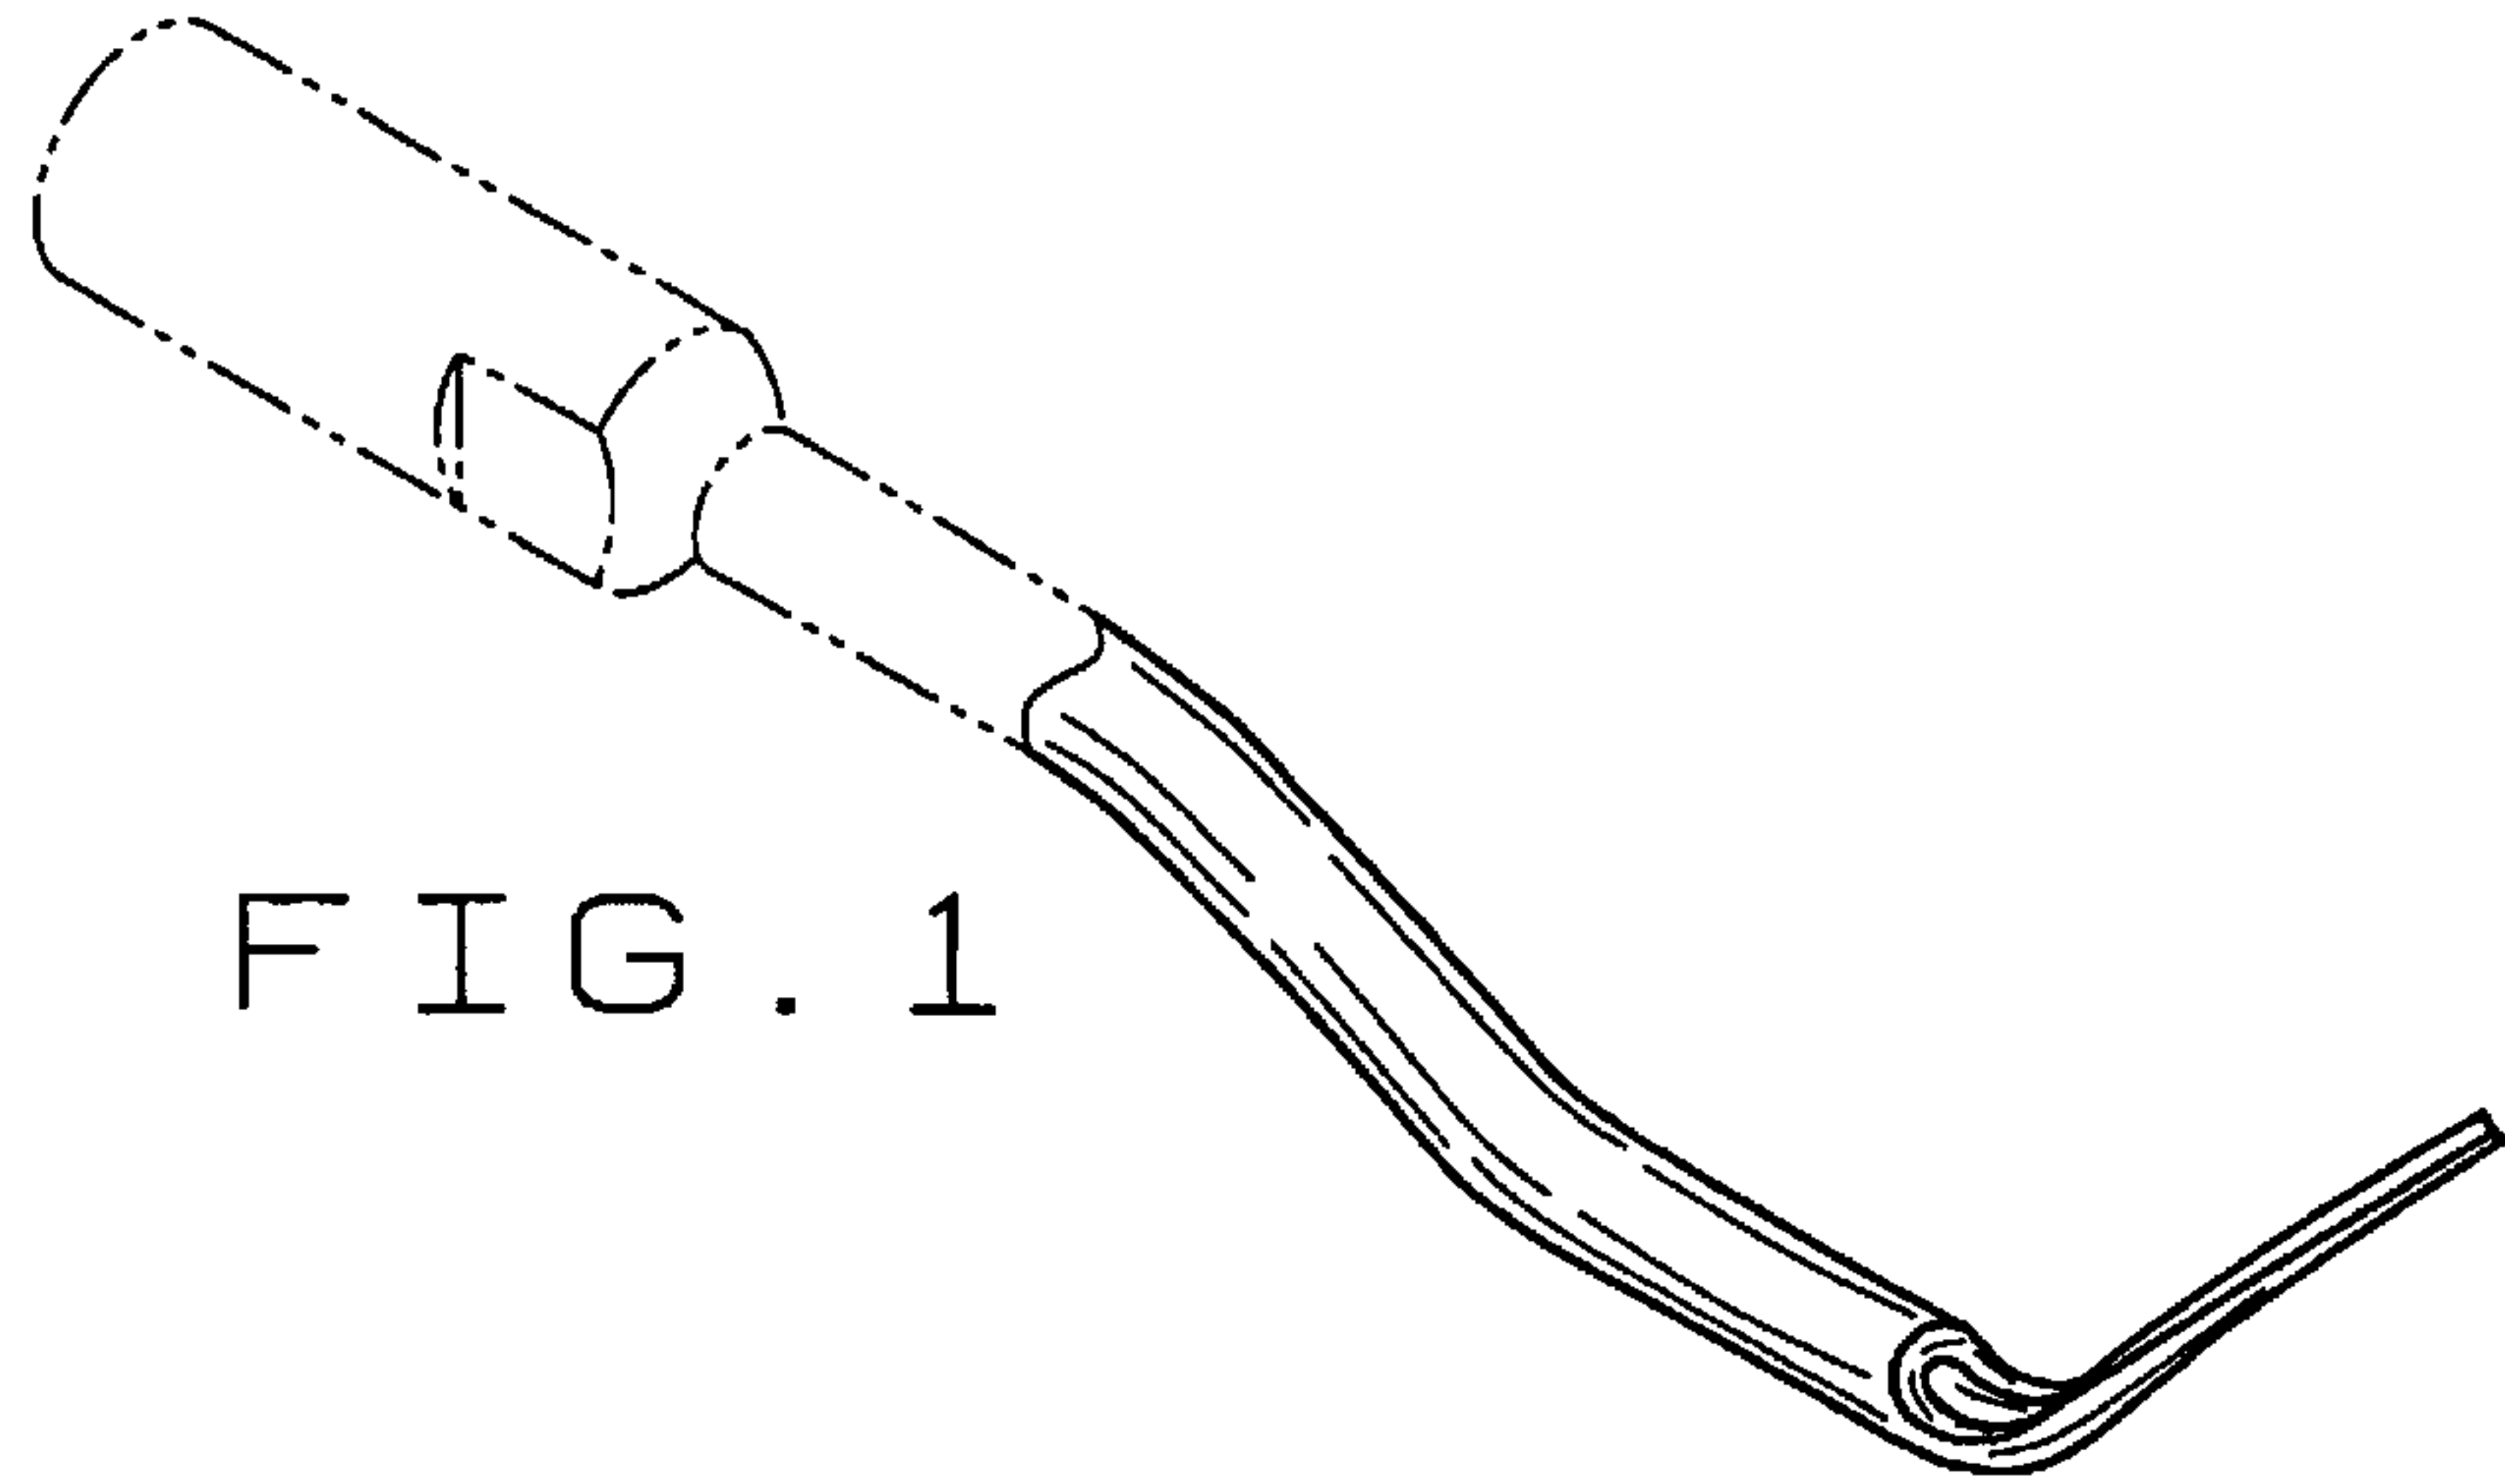


FIG. 1

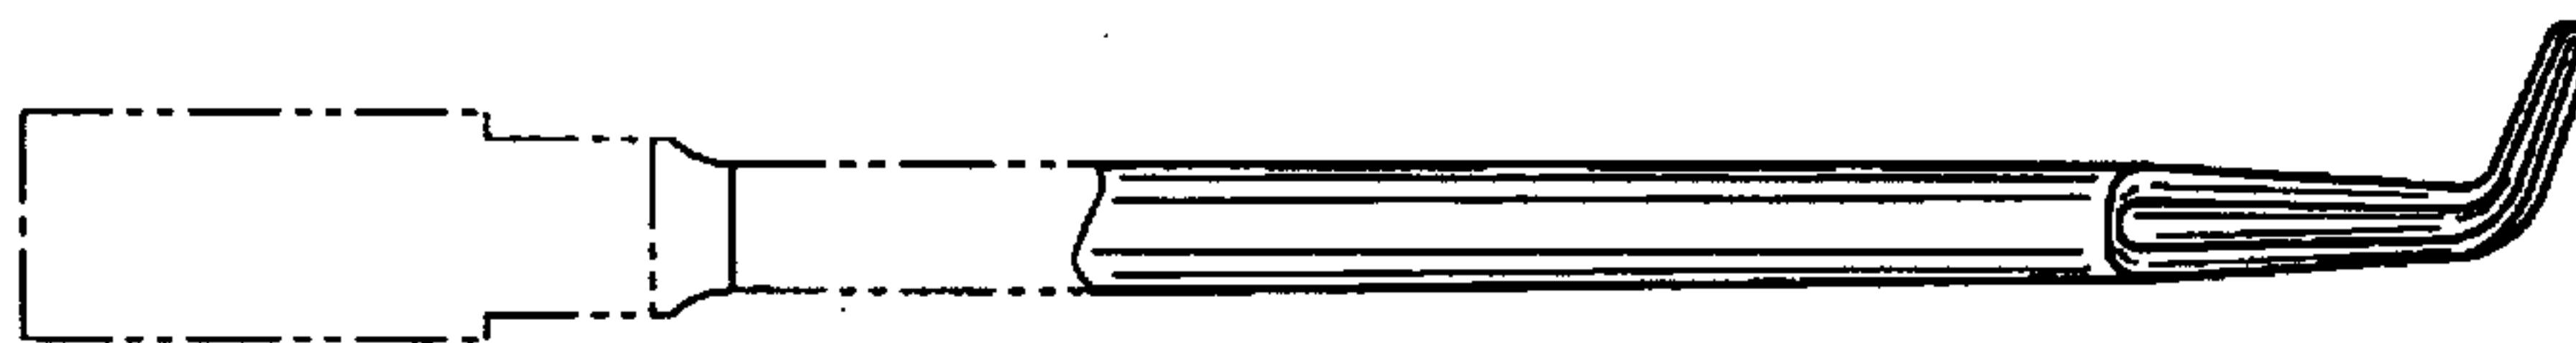


FIG. 2

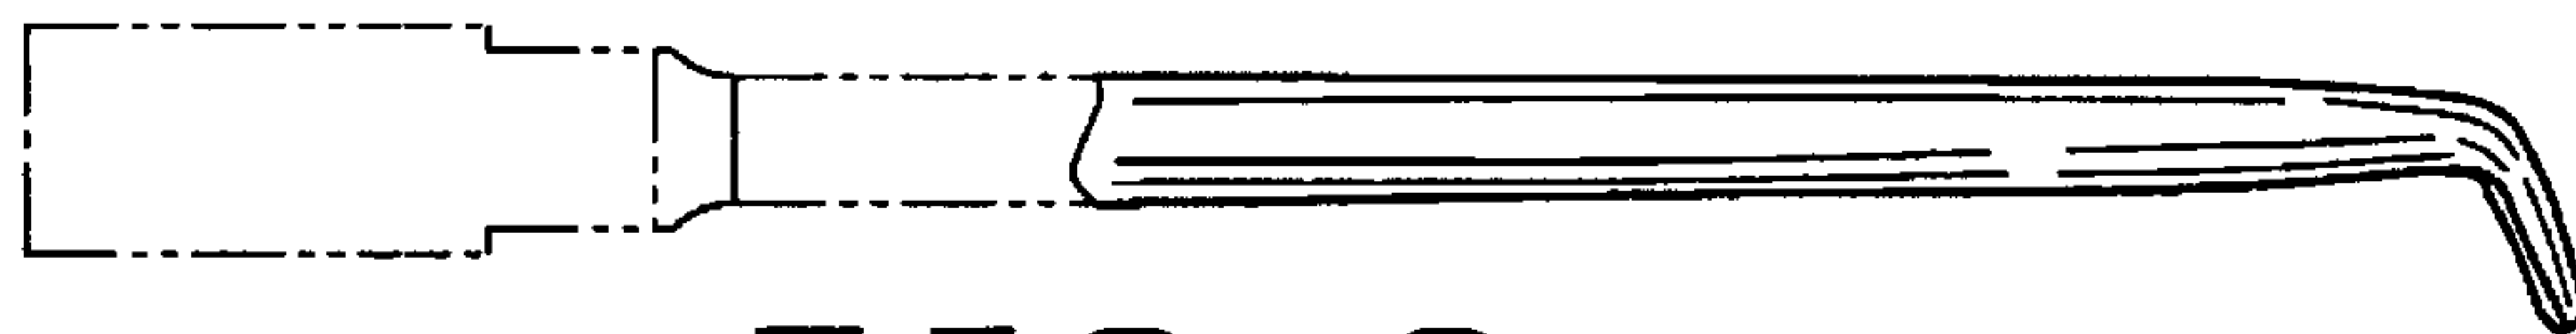


FIG. 3

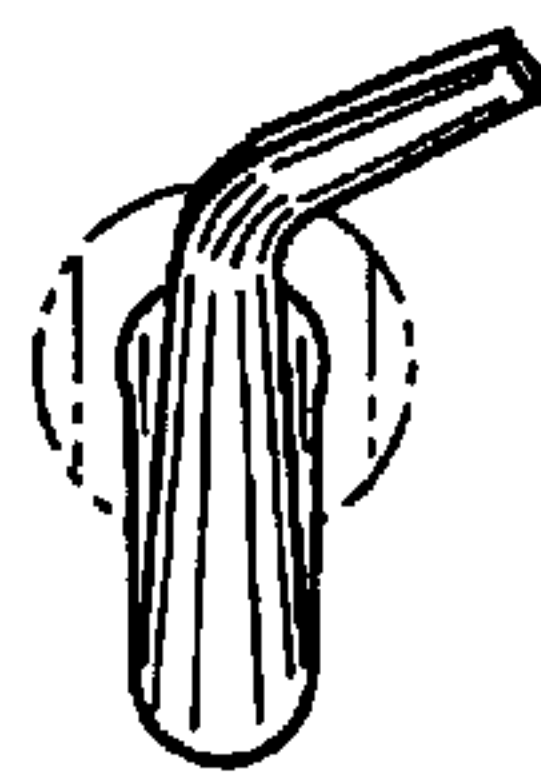


FIG. 4

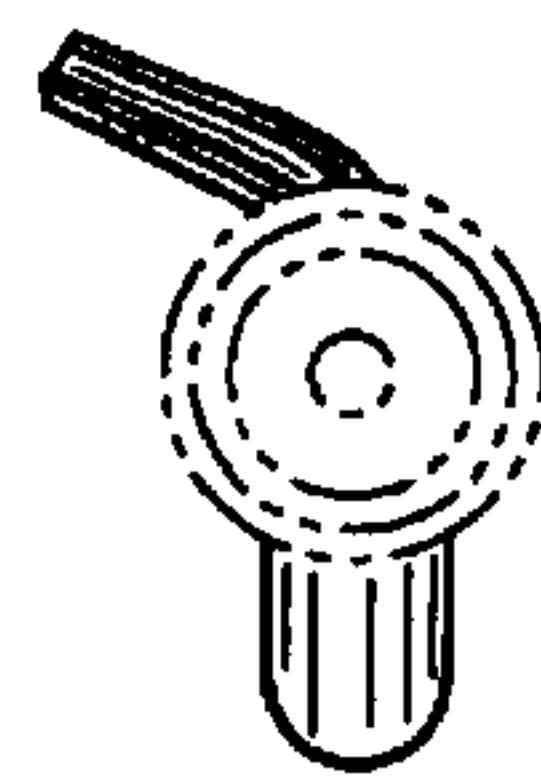


FIG. 5

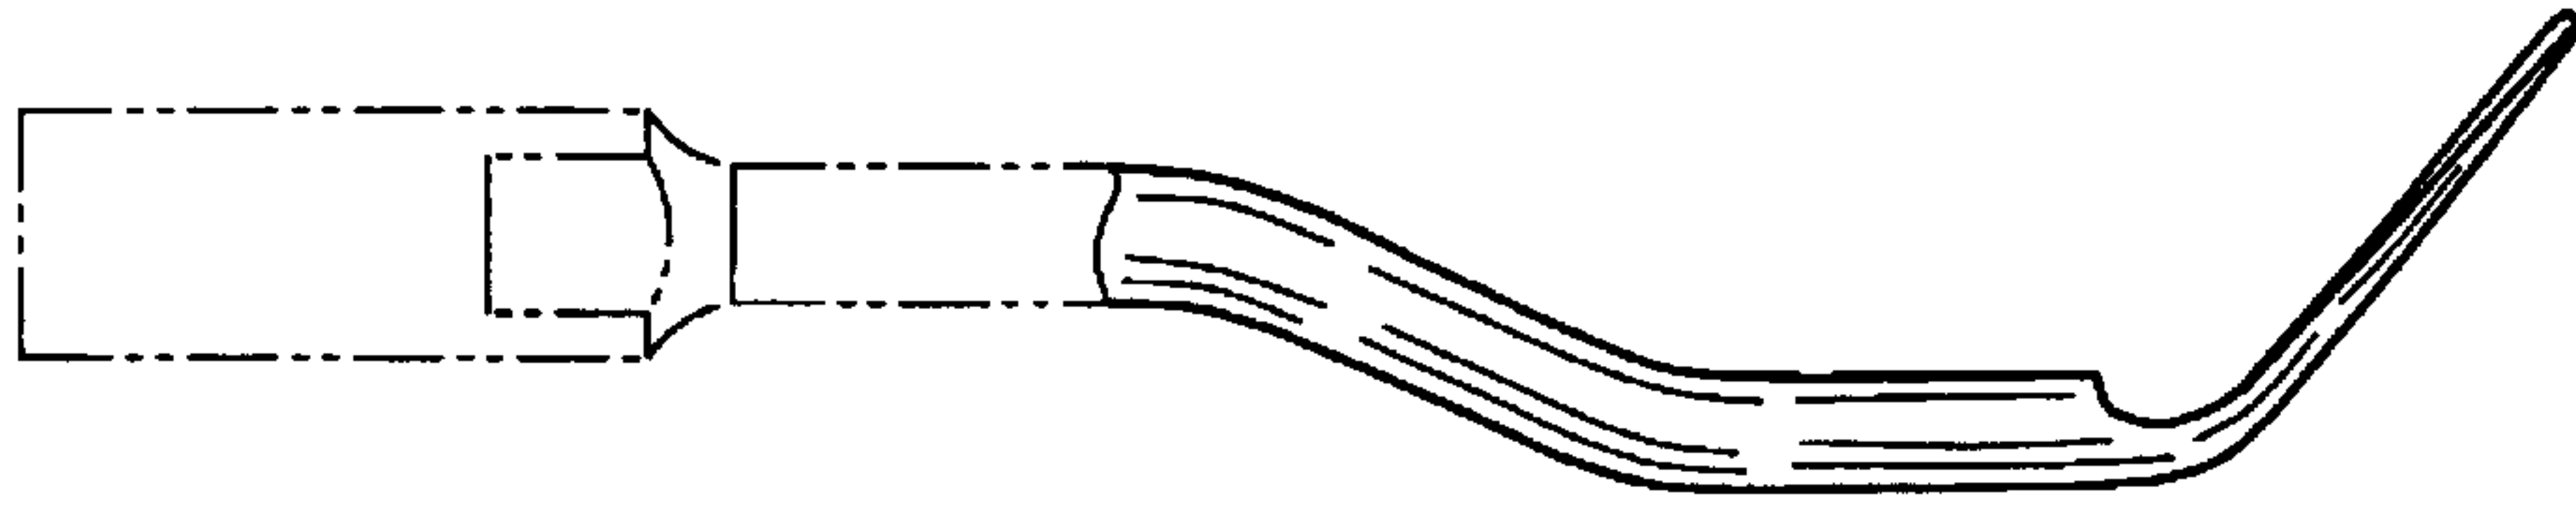


FIG. 6

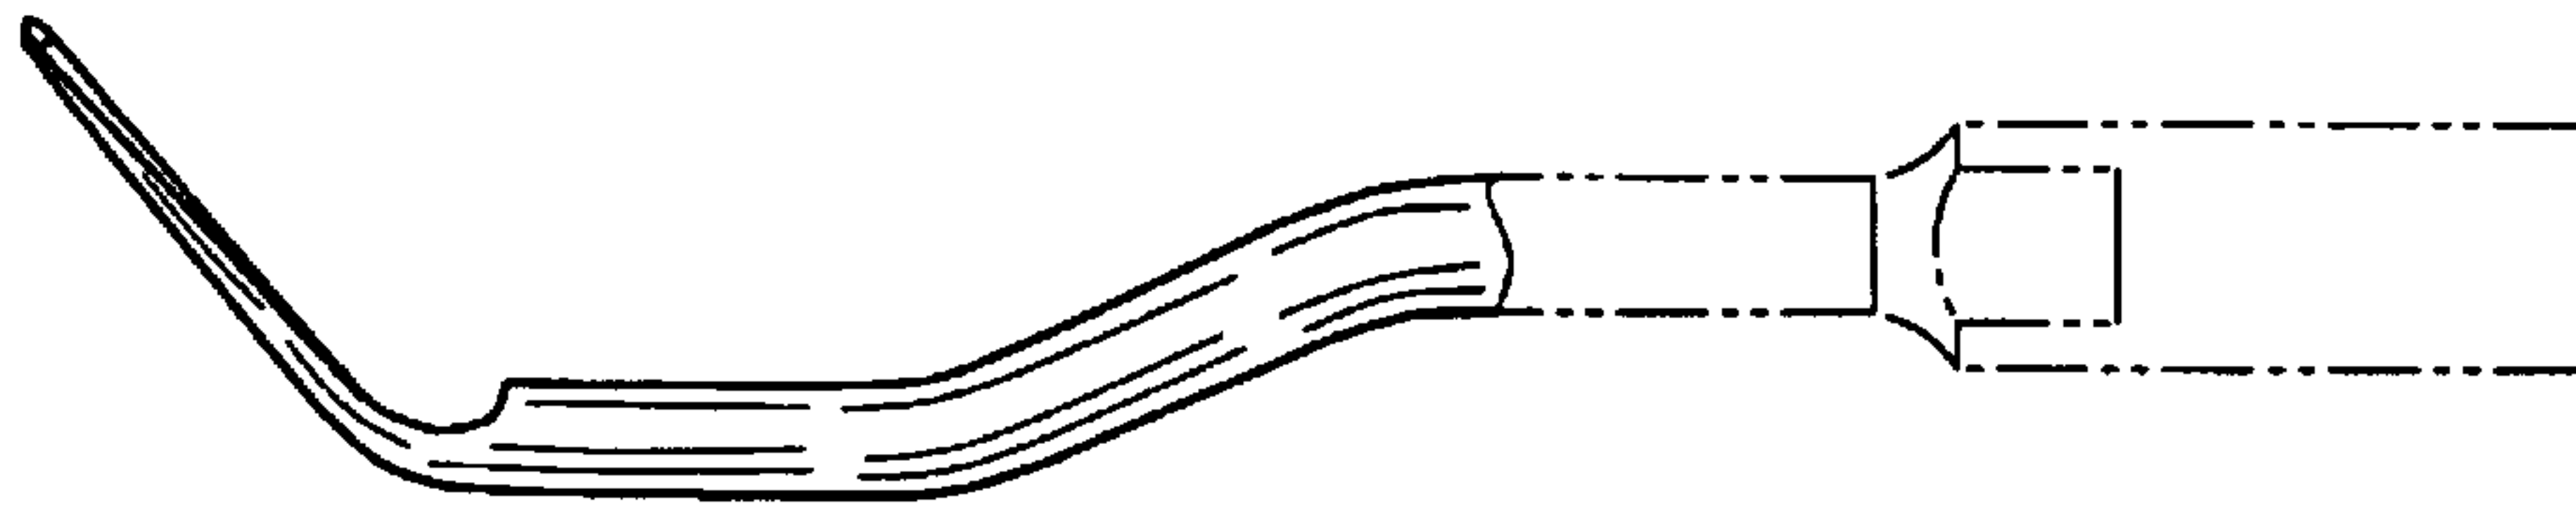


FIG. 7

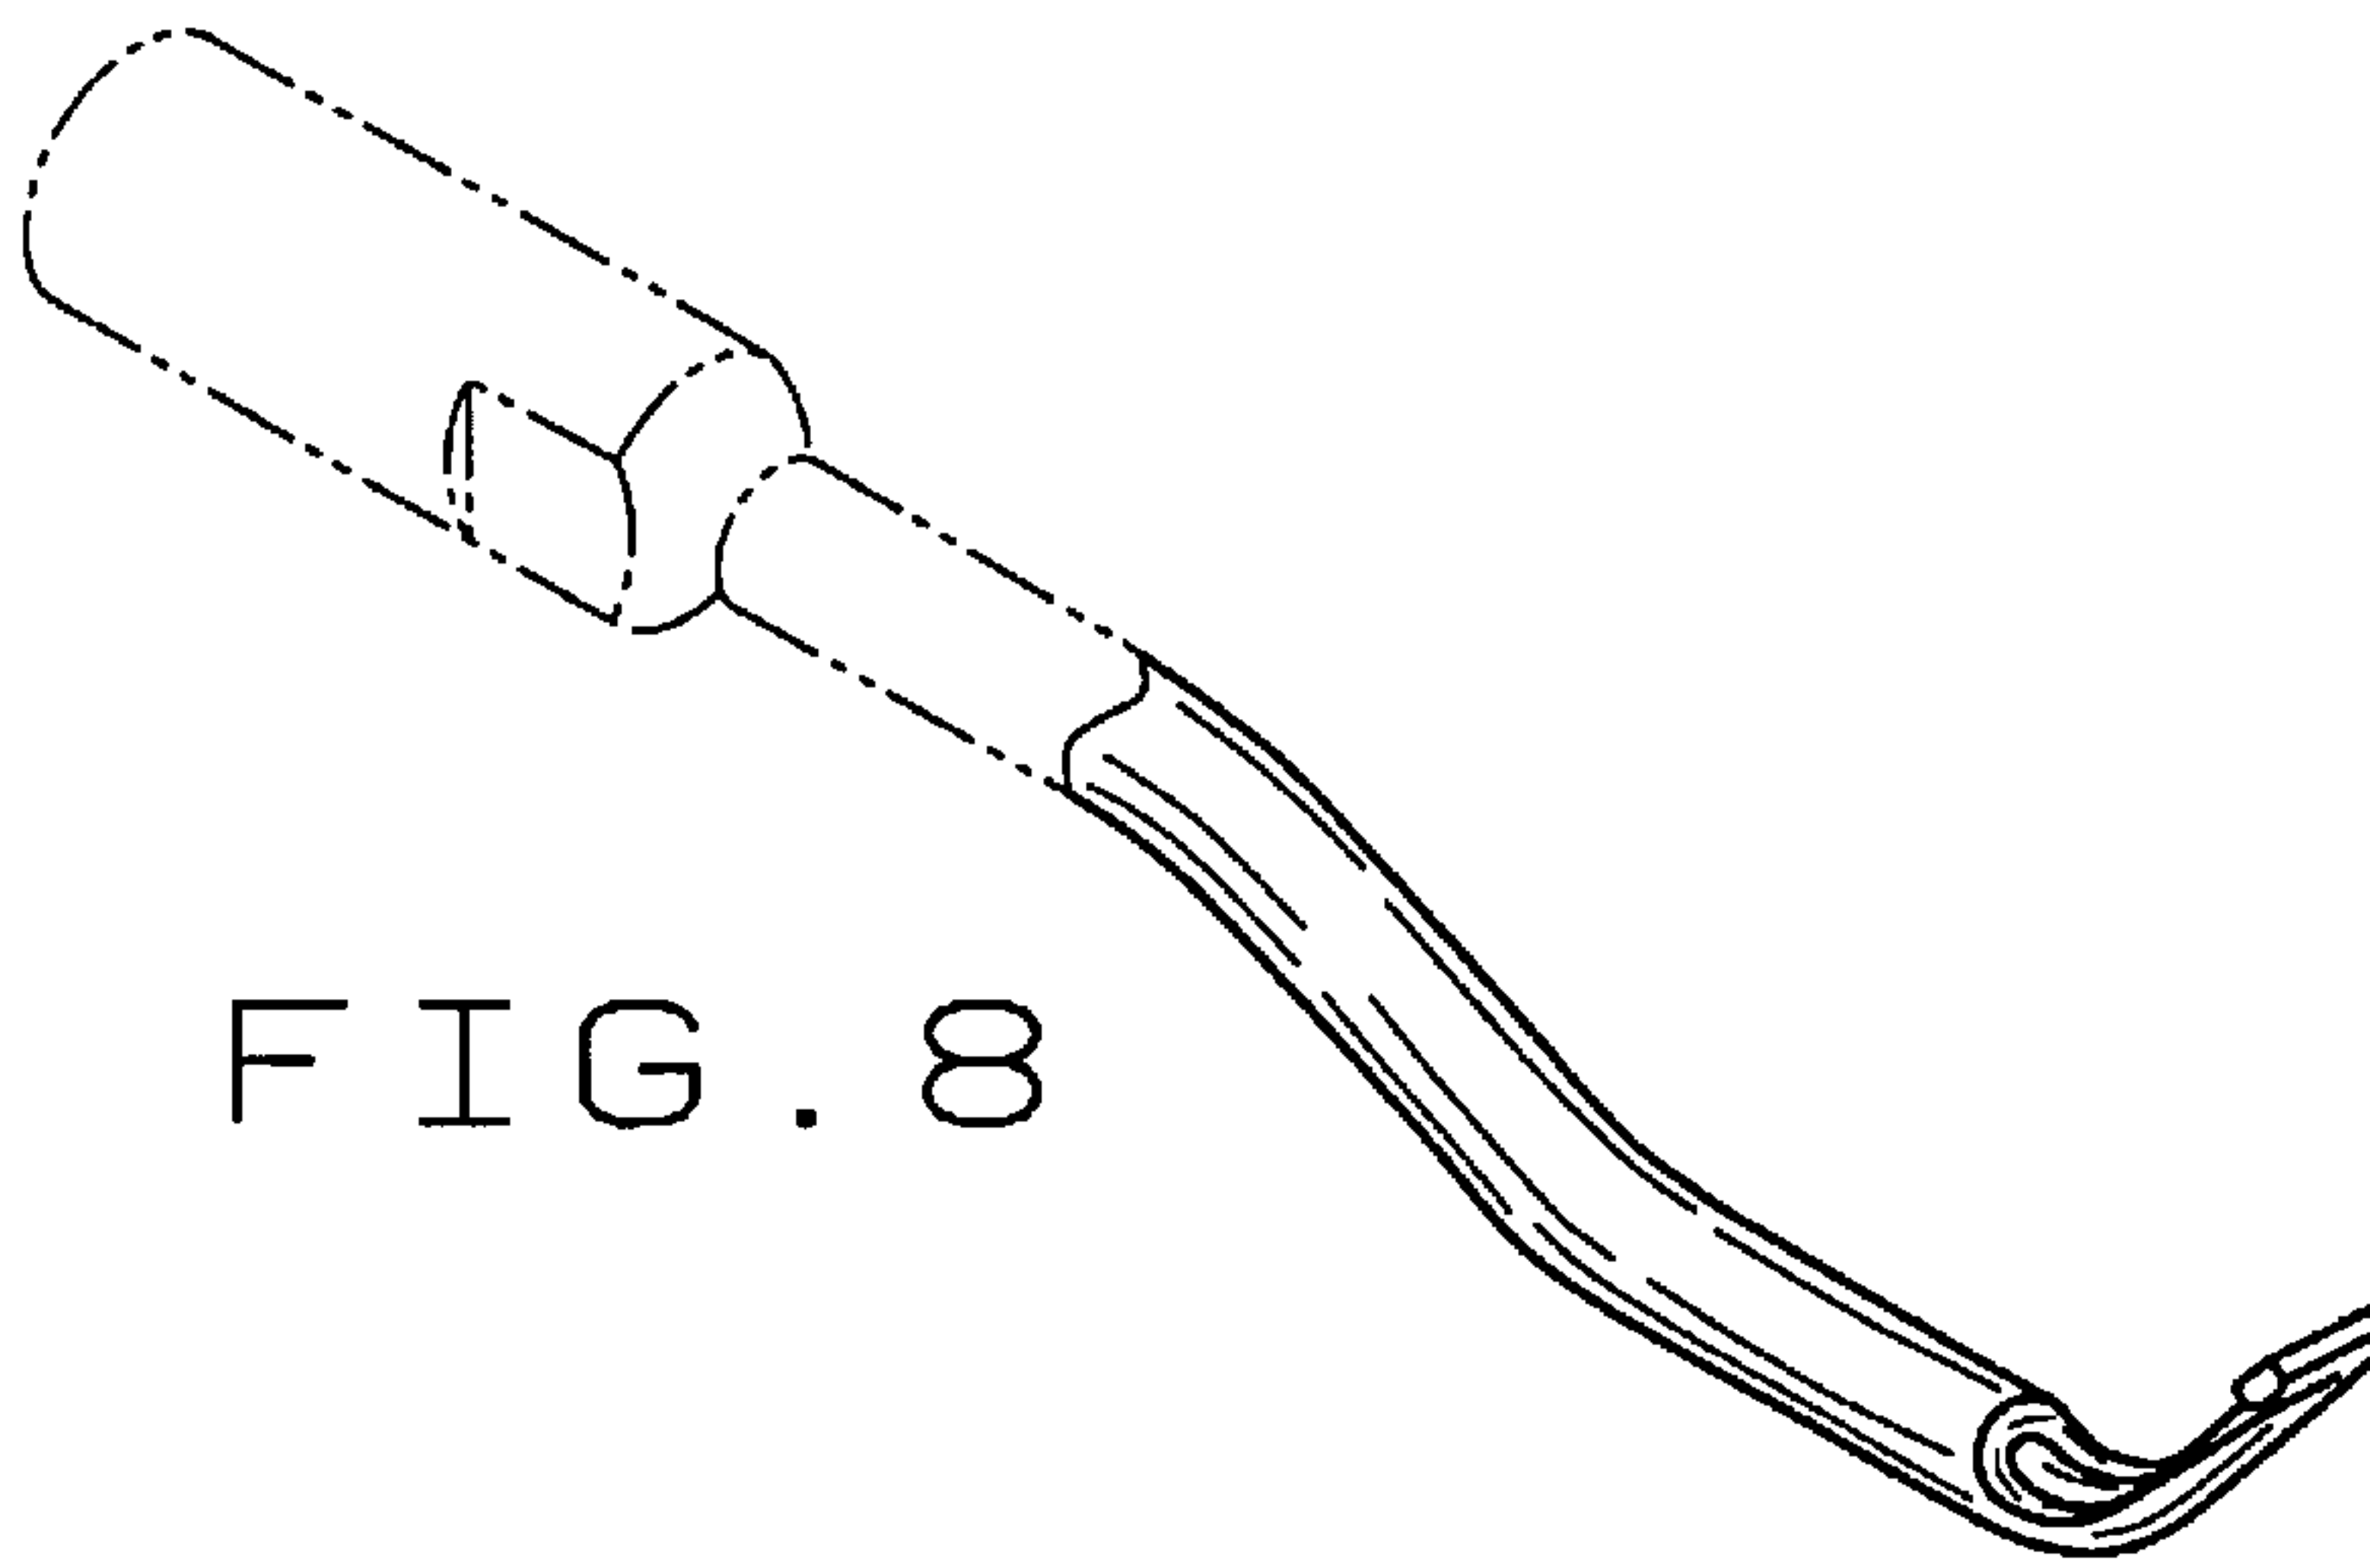


FIG. 8

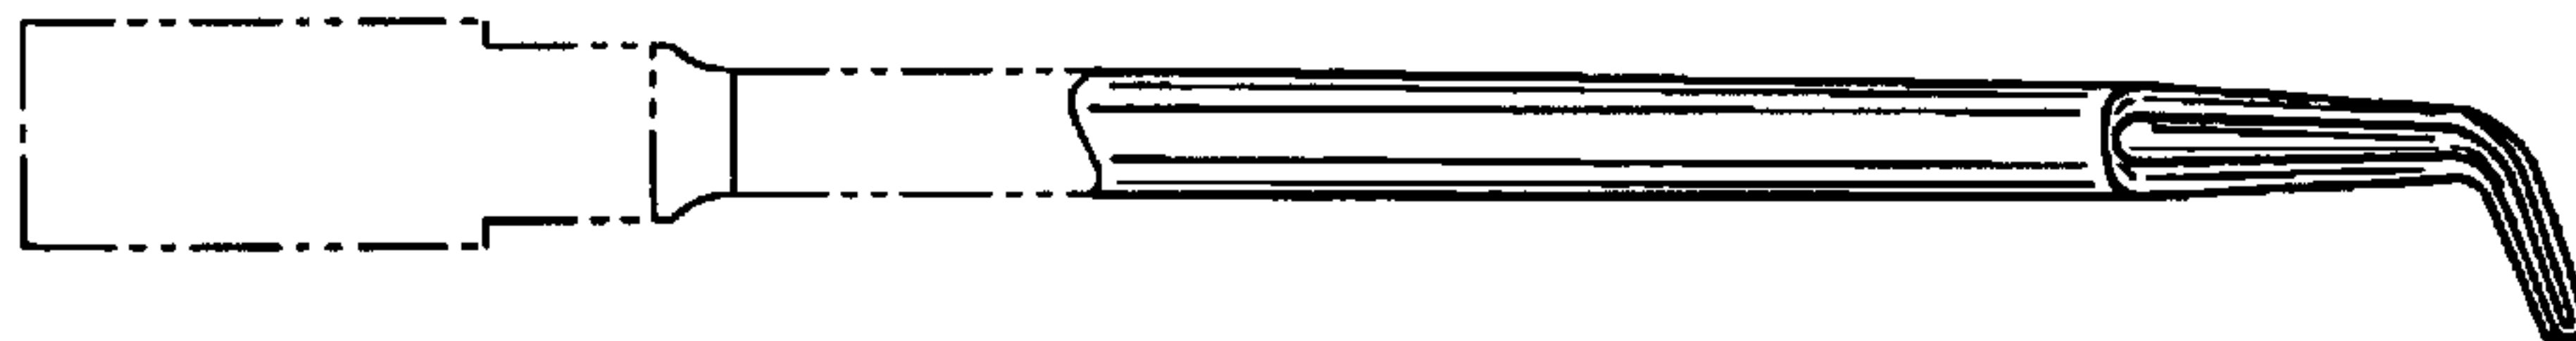


FIG. 9

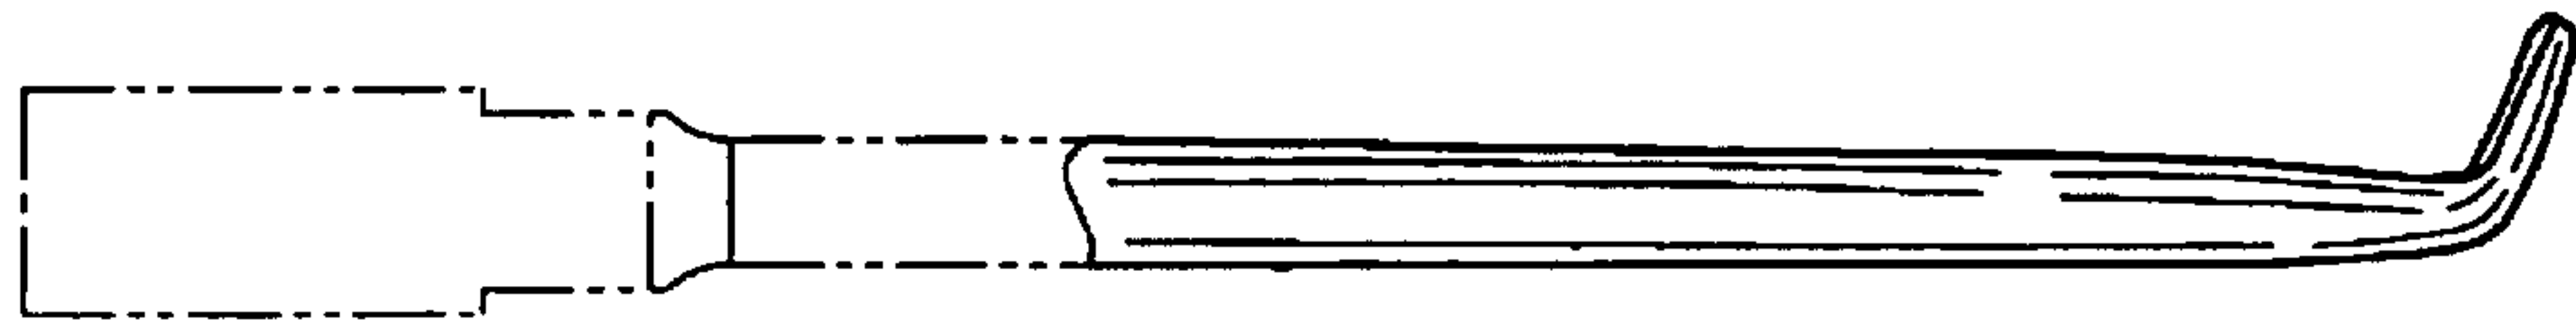


FIG. 10

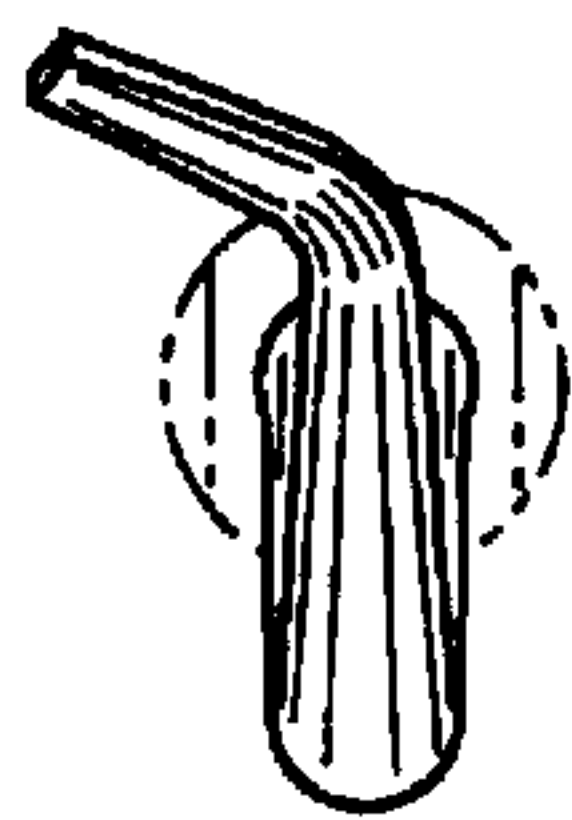


FIG. 11

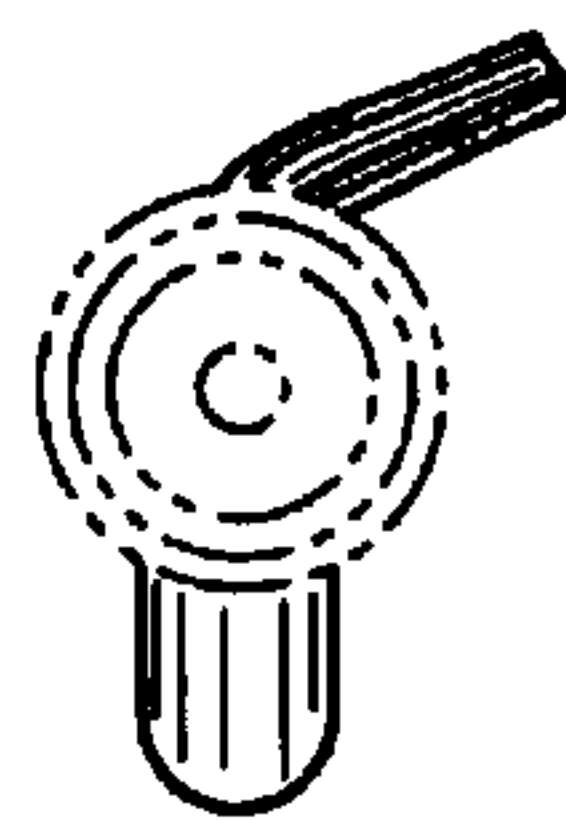


FIG. 12

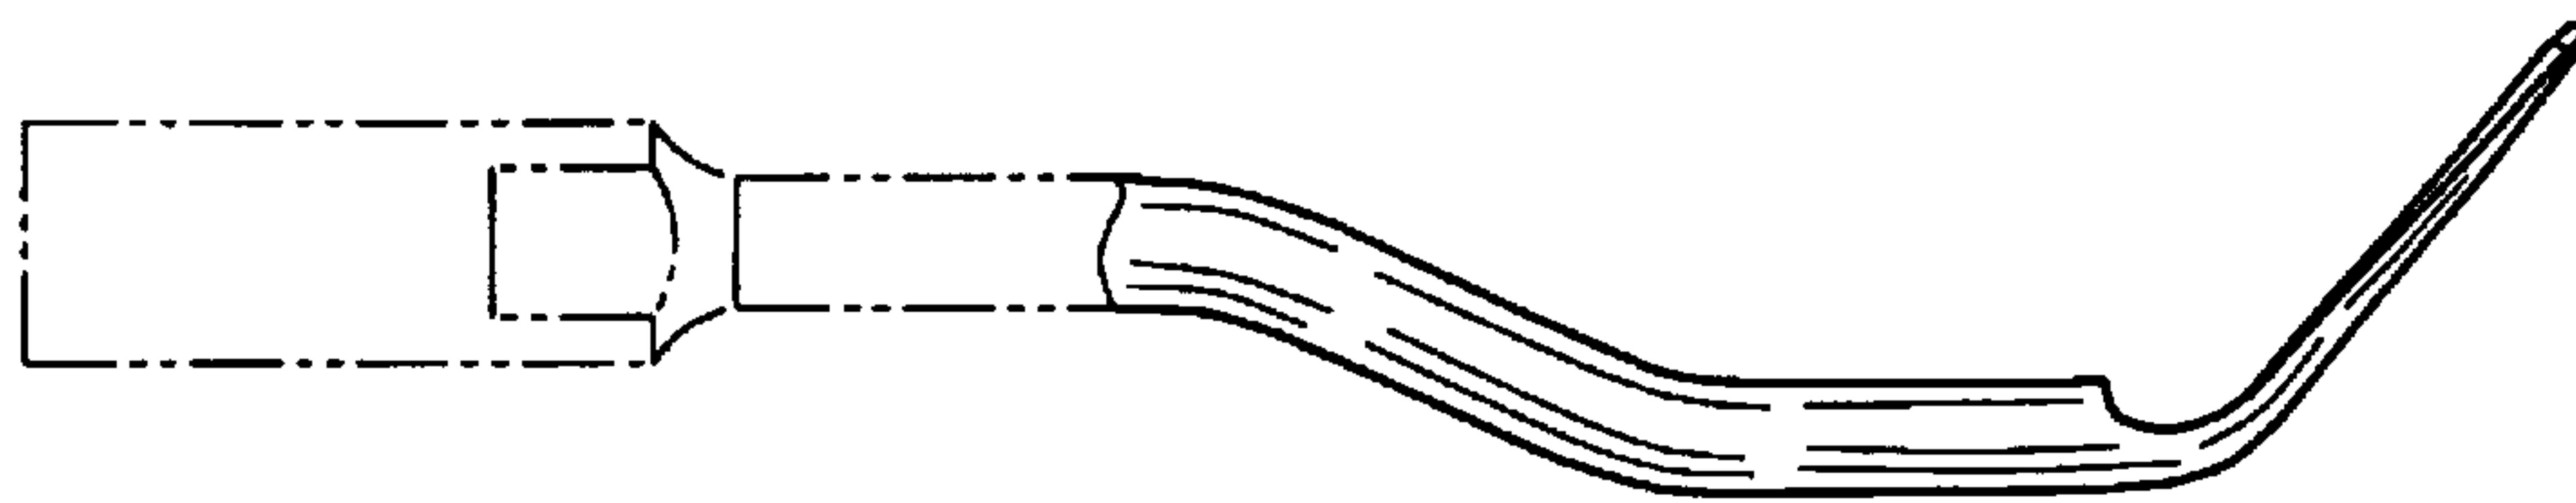


FIG. 13

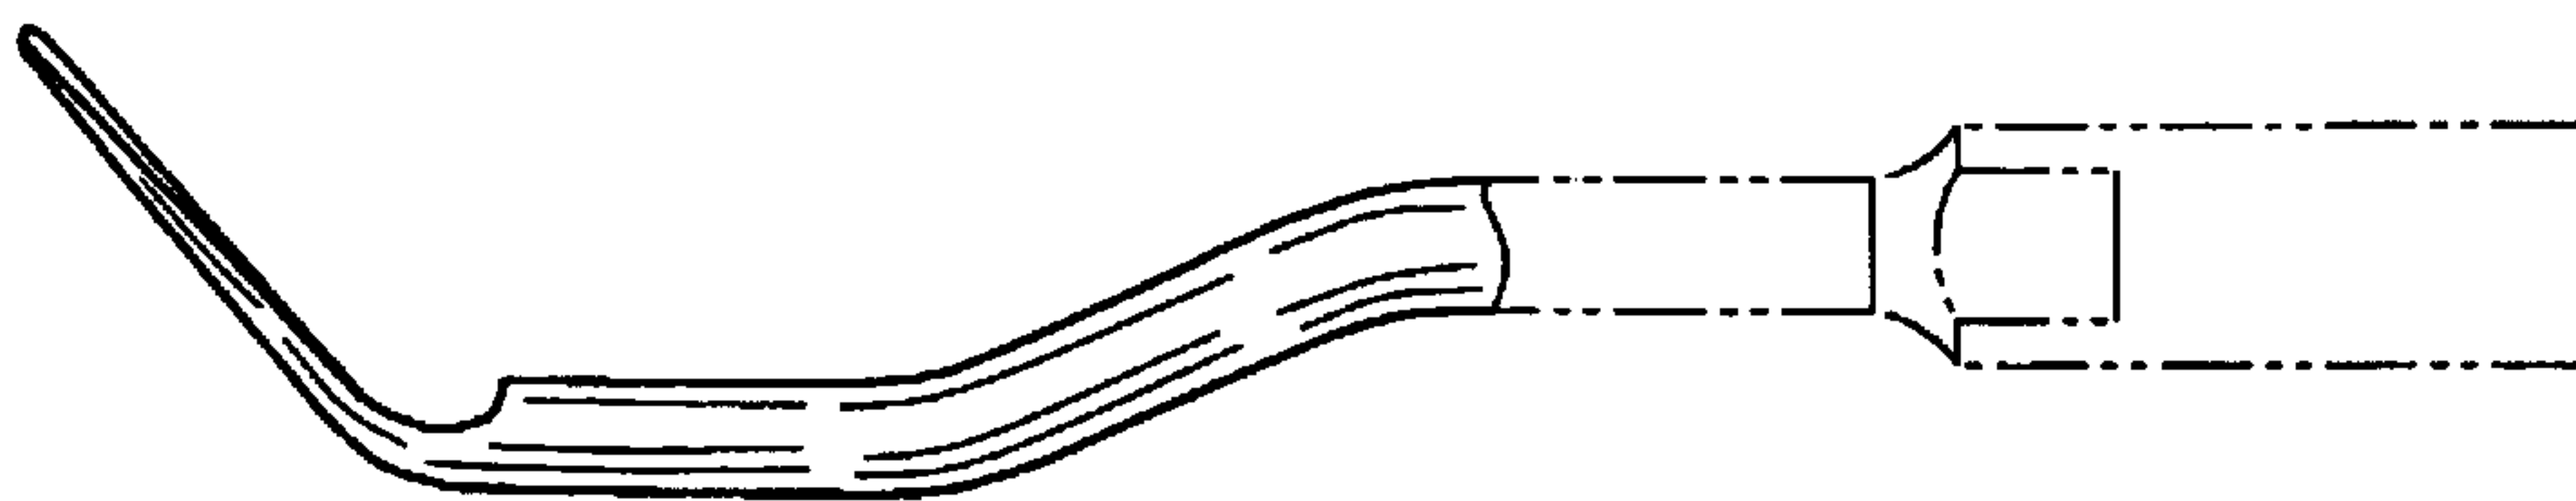


FIG. 14