

US00D547446S

(12) **United States Design Patent**
Racz et al.

(10) **Patent No.:** **US D547,446 S**

(45) **Date of Patent:** **** Jul. 24, 2007**

(54) **CATHETER CONNECTOR**

(75) Inventors: **N. Sandor Racz**, Irving, TX (US);
Gary Bullard, Saratoga Springs, NY (US)

(73) Assignee: **Custom Medical Applications, Inc.**,
Johnstown, NY (US)

(**) Term: **14 Years**

(21) Appl. No.: **29/224,810**

(22) Filed: **Mar. 7, 2005**

(51) **LOC (8) Cl.** **24-02**

(52) **U.S. Cl.** **D24/129**

(58) **Field of Classification Search** D24/105,
D24/108-109, 110.1, 112, 129-130; D26/2;
128/879, 912; 137/565.12; 604/164.11,
604/167.07, 533, 536, 905, 912
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

3,920,215 A	11/1975	Knauf	
D243,412 S *	2/1977	Krueger et al.	D24/164
4,327,723 A	5/1982	Frankhouser	
4,378,013 A	3/1983	LeFevre	
4,517,971 A *	5/1985	Sorbonne	128/879
4,613,329 A	9/1986	Bodicky	
4,834,719 A	5/1989	Arenas	
4,895,570 A	1/1990	Larkin	
4,929,236 A	5/1990	Sampson	
D323,713 S *	2/1992	Arioka et al.	D24/165
5,116,324 A *	5/1992	Brierley et al.	604/180
5,127,626 A	7/1992	Hilal et al.	
5,279,597 A	1/1994	Dassa et al.	
5,505,714 A	4/1996	Dassa et al.	
5,507,733 A	4/1996	Larkin et al.	
D408,530 S	4/1999	Eliassen et al.	
5,993,437 A	11/1999	Roaz	
D422,697 S *	4/2000	Bellhouse et al.	D24/112
6,099,519 A	8/2000	Olsen et al.	

6,123,690 A *	9/2000	Mejslov	604/533
D433,503 S	11/2000	Powers et al.	
6,190,372 B1	2/2001	Racz	
6,254,589 B1	7/2001	Roaz	

(Continued)

Primary Examiner—Louis S. Zarfes

Assistant Examiner—Eric L. Goodman

(74) *Attorney, Agent, or Firm*—TraskBritt

(57) **CLAIM**

The ornamental design for a catheter connector, as shown and described.

DESCRIPTION

FIG. 1 is a perspective view of a catheter connector showing my new design in situ;

FIG. 2 is another perspective view of the catheter connector shown in FIG. 1;

FIG. 3 is a front elevation view of the catheter connector shown in FIG. 1;

FIG. 4 is a rear elevation view of the catheter connector shown in FIG. 1;

FIG. 5 is a right elevation view of the catheter connector shown in FIG. 1;

FIG. 6 is a left elevation view of the catheter connector shown in FIG. 1;



FIG. 7 is a top plan view of the catheter connector shown in FIG. 1

FIG. 8 is a bottom plan view of the catheter connector shown in FIG. 1; and,

FIG. 9 is a modified perspective view showing the of the catheter connector shown in FIG. 1 in an opened position.

The broken line showing of the back, arms, tubes, and bandage in FIG. 1 and broken line showing of the latching system in FIGS. 1, 2, 3, 4, 5, 6, and 9 are for illustrative purposes only and form no part of the claimed design.

1 Claim, 4 Drawing Sheets

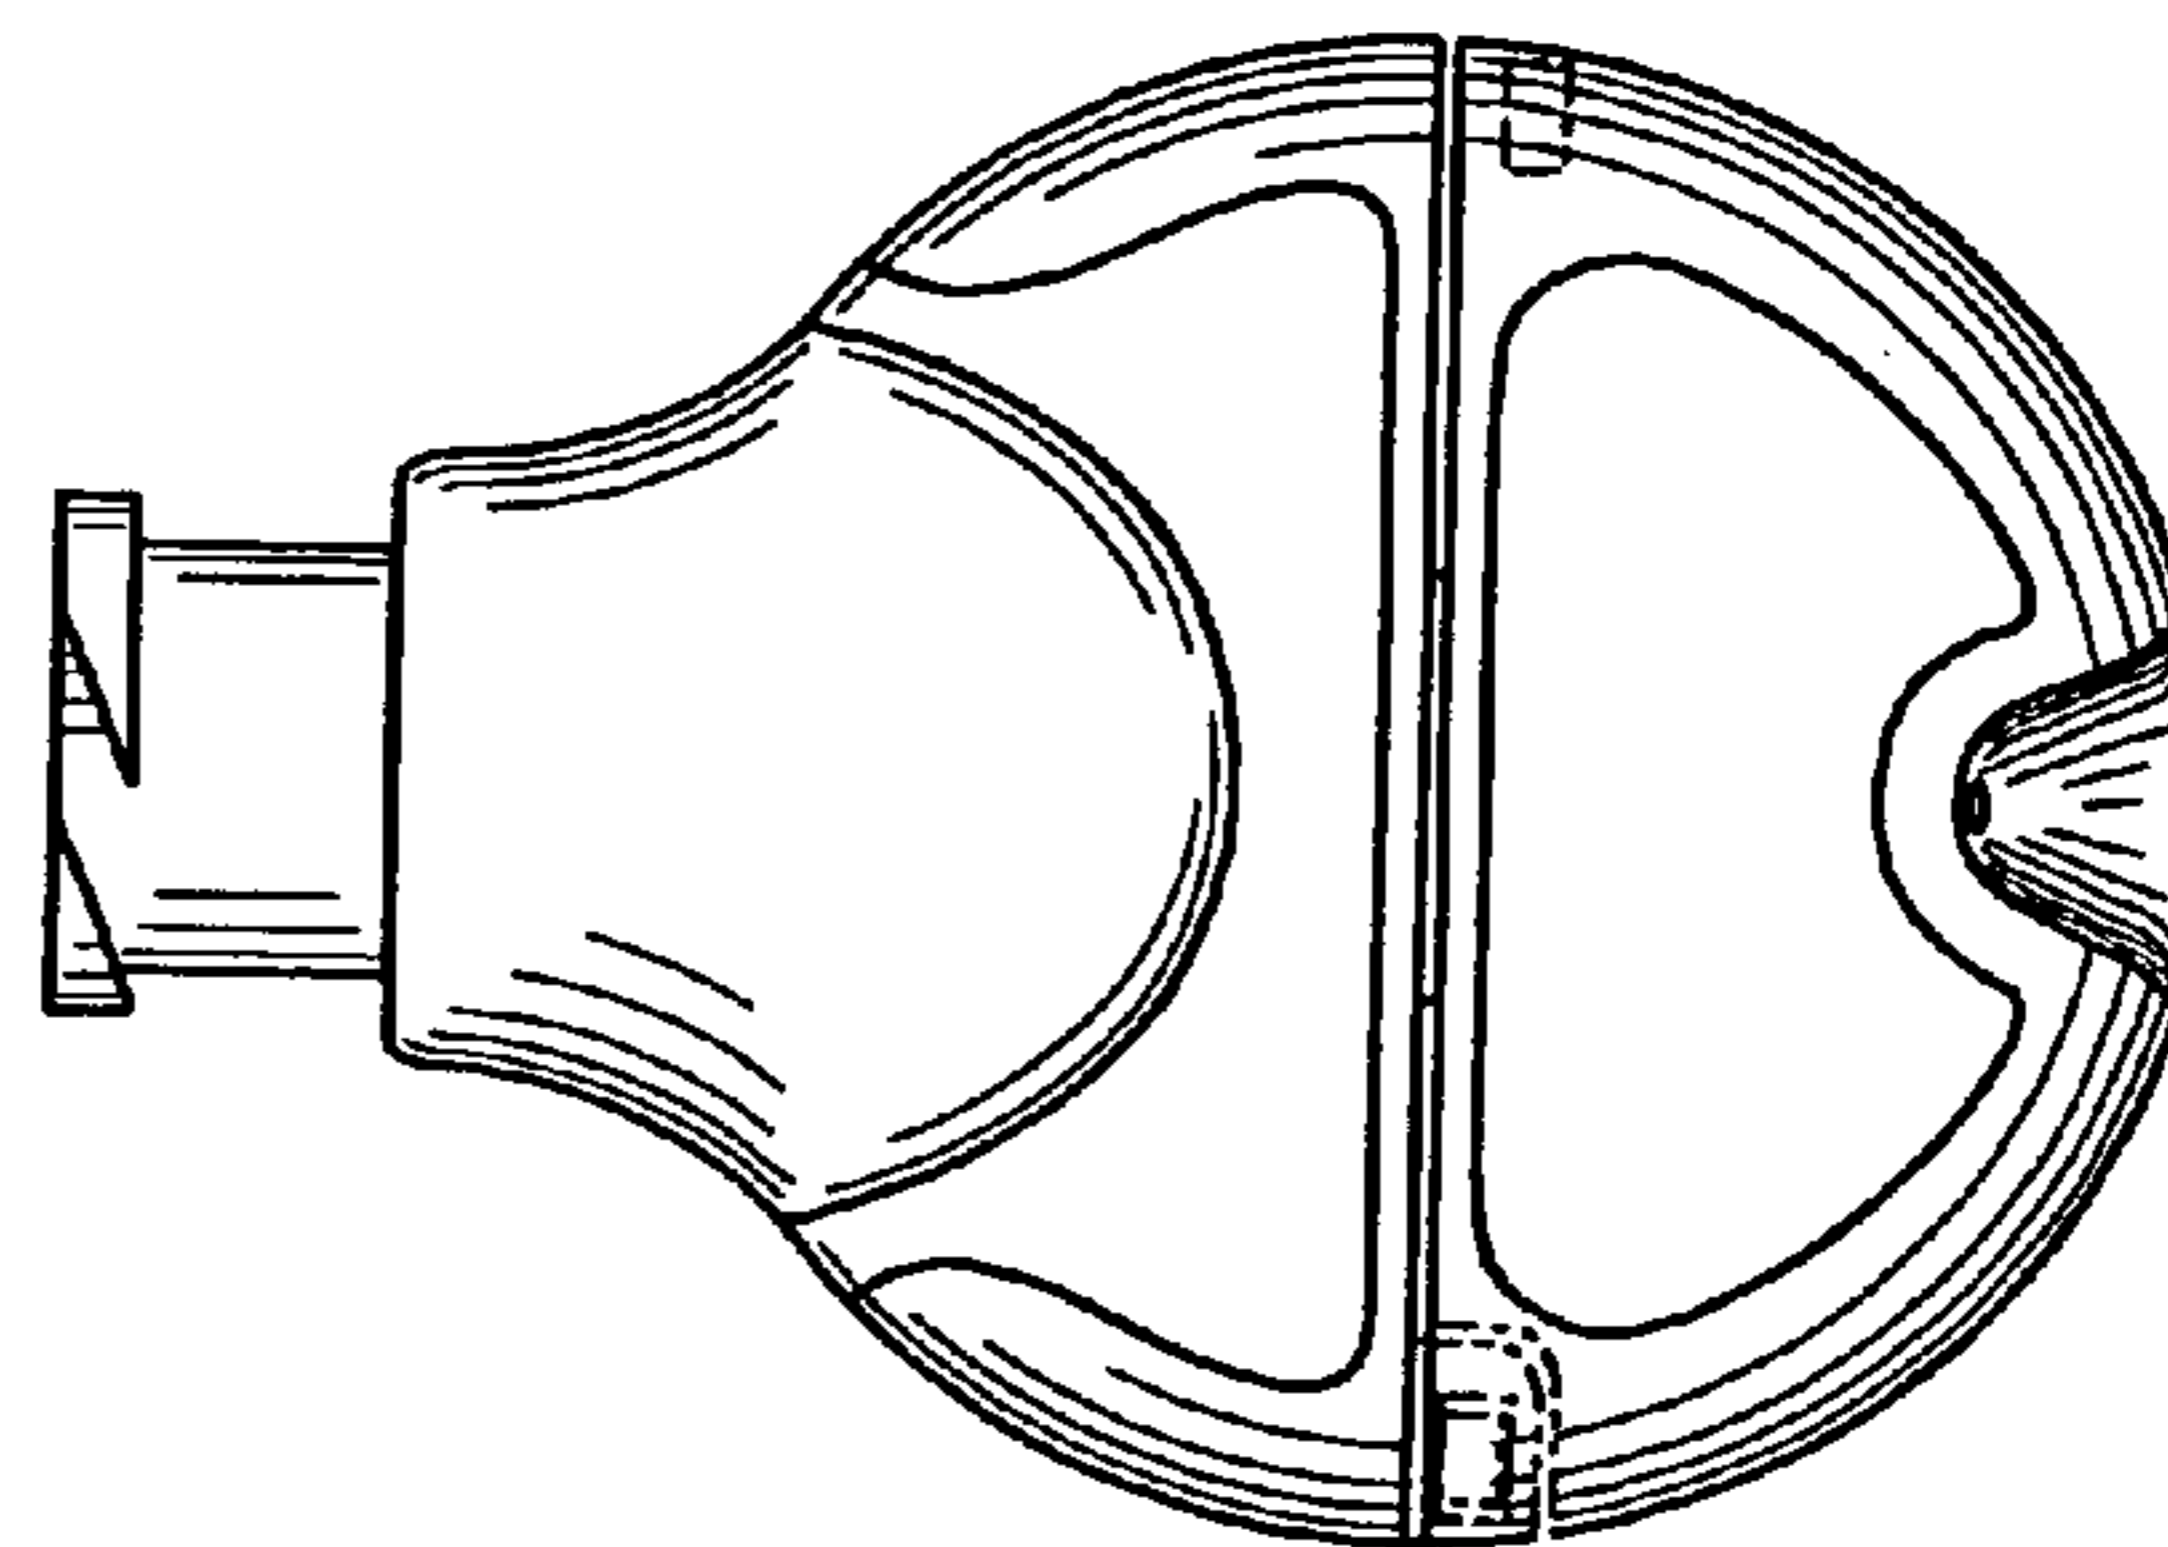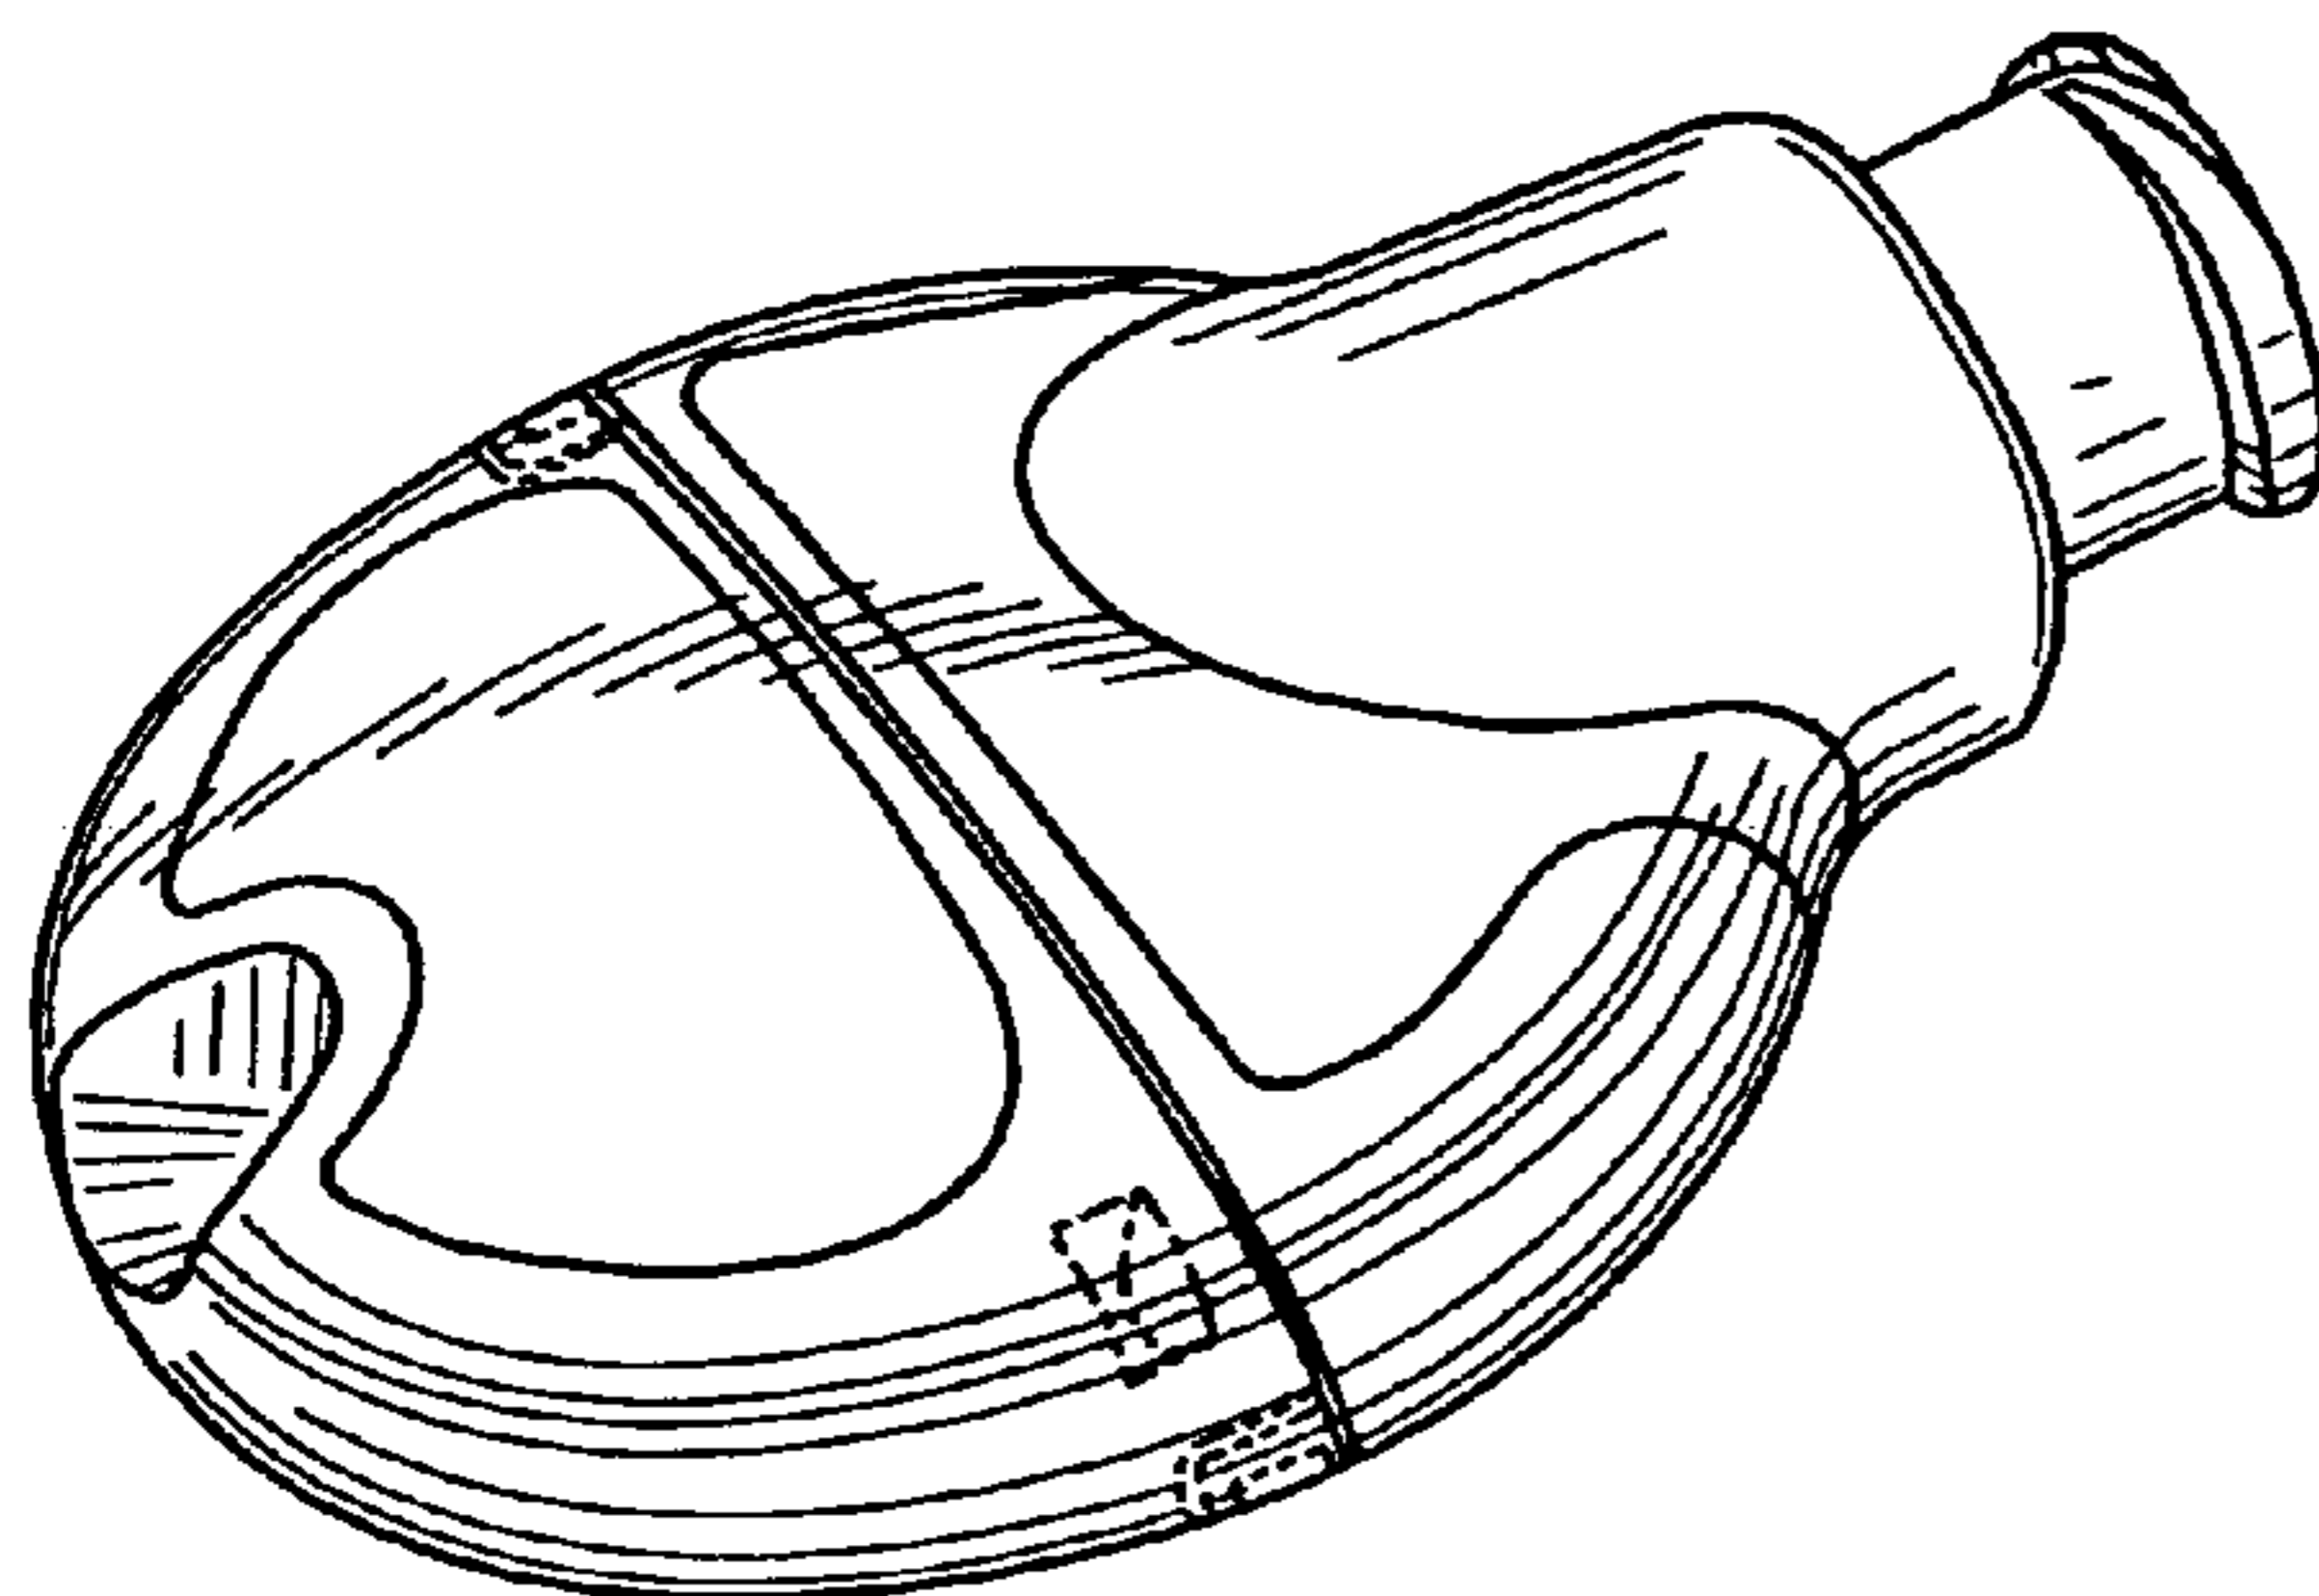

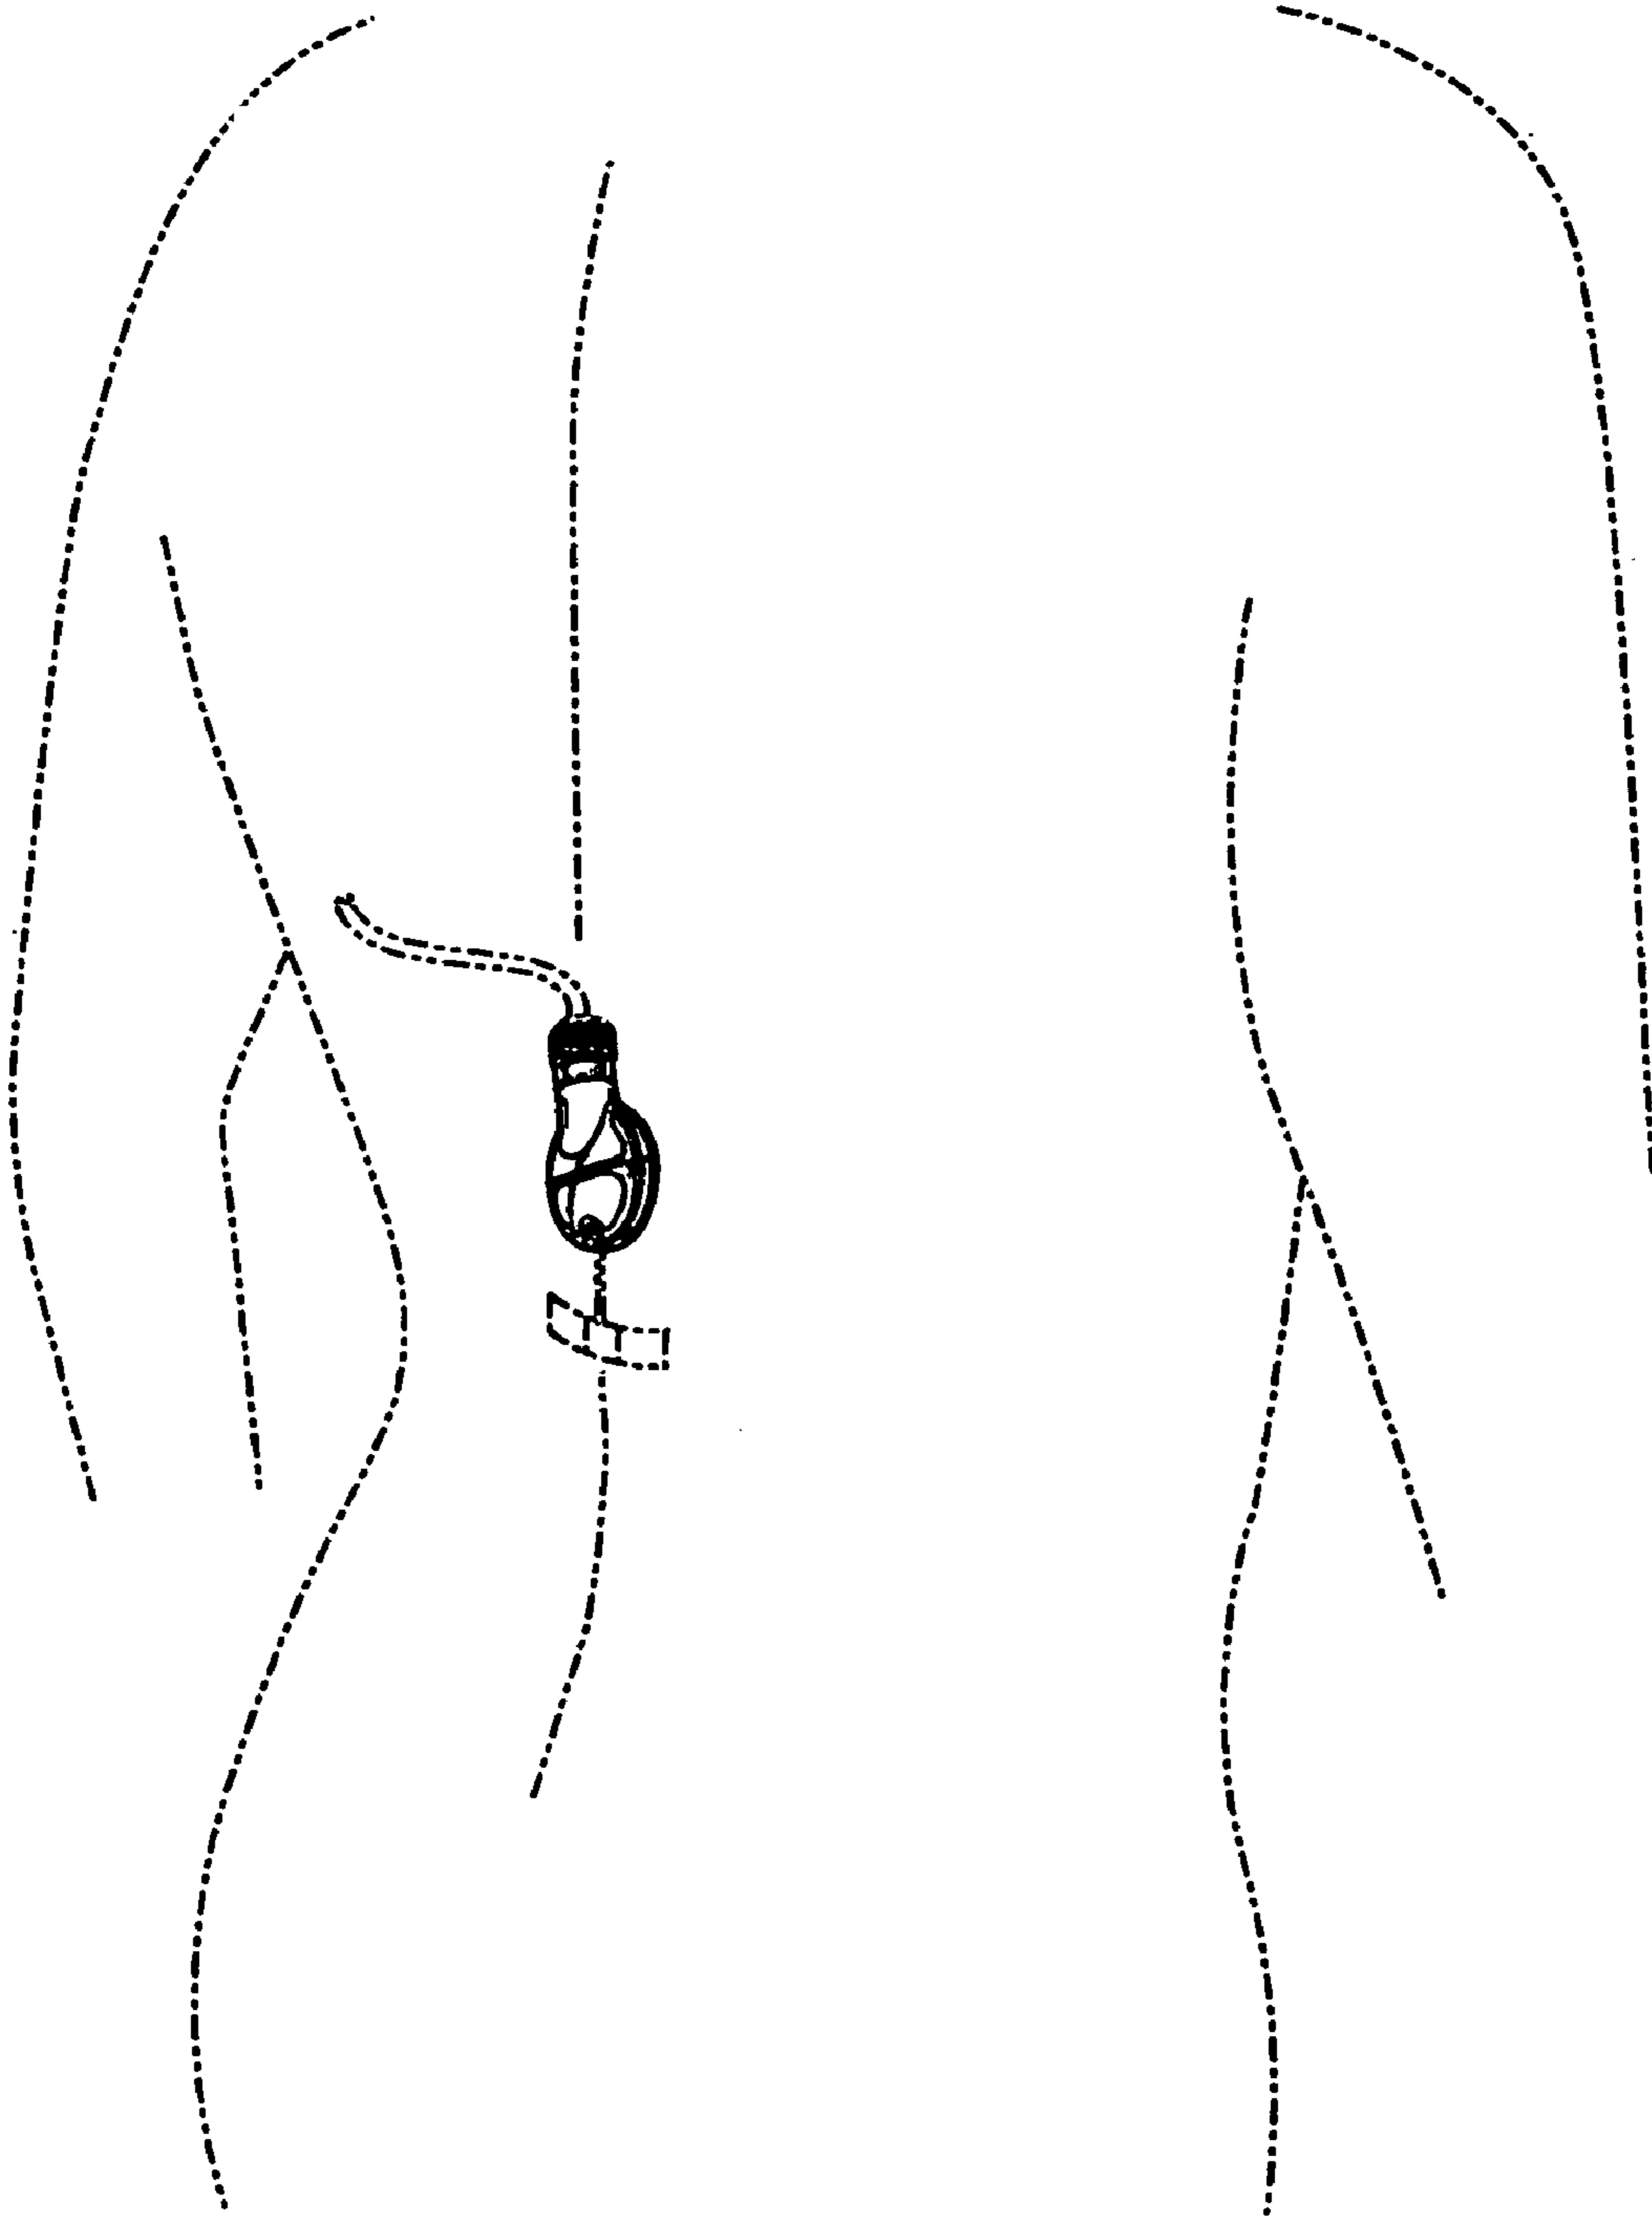


FIG. 1

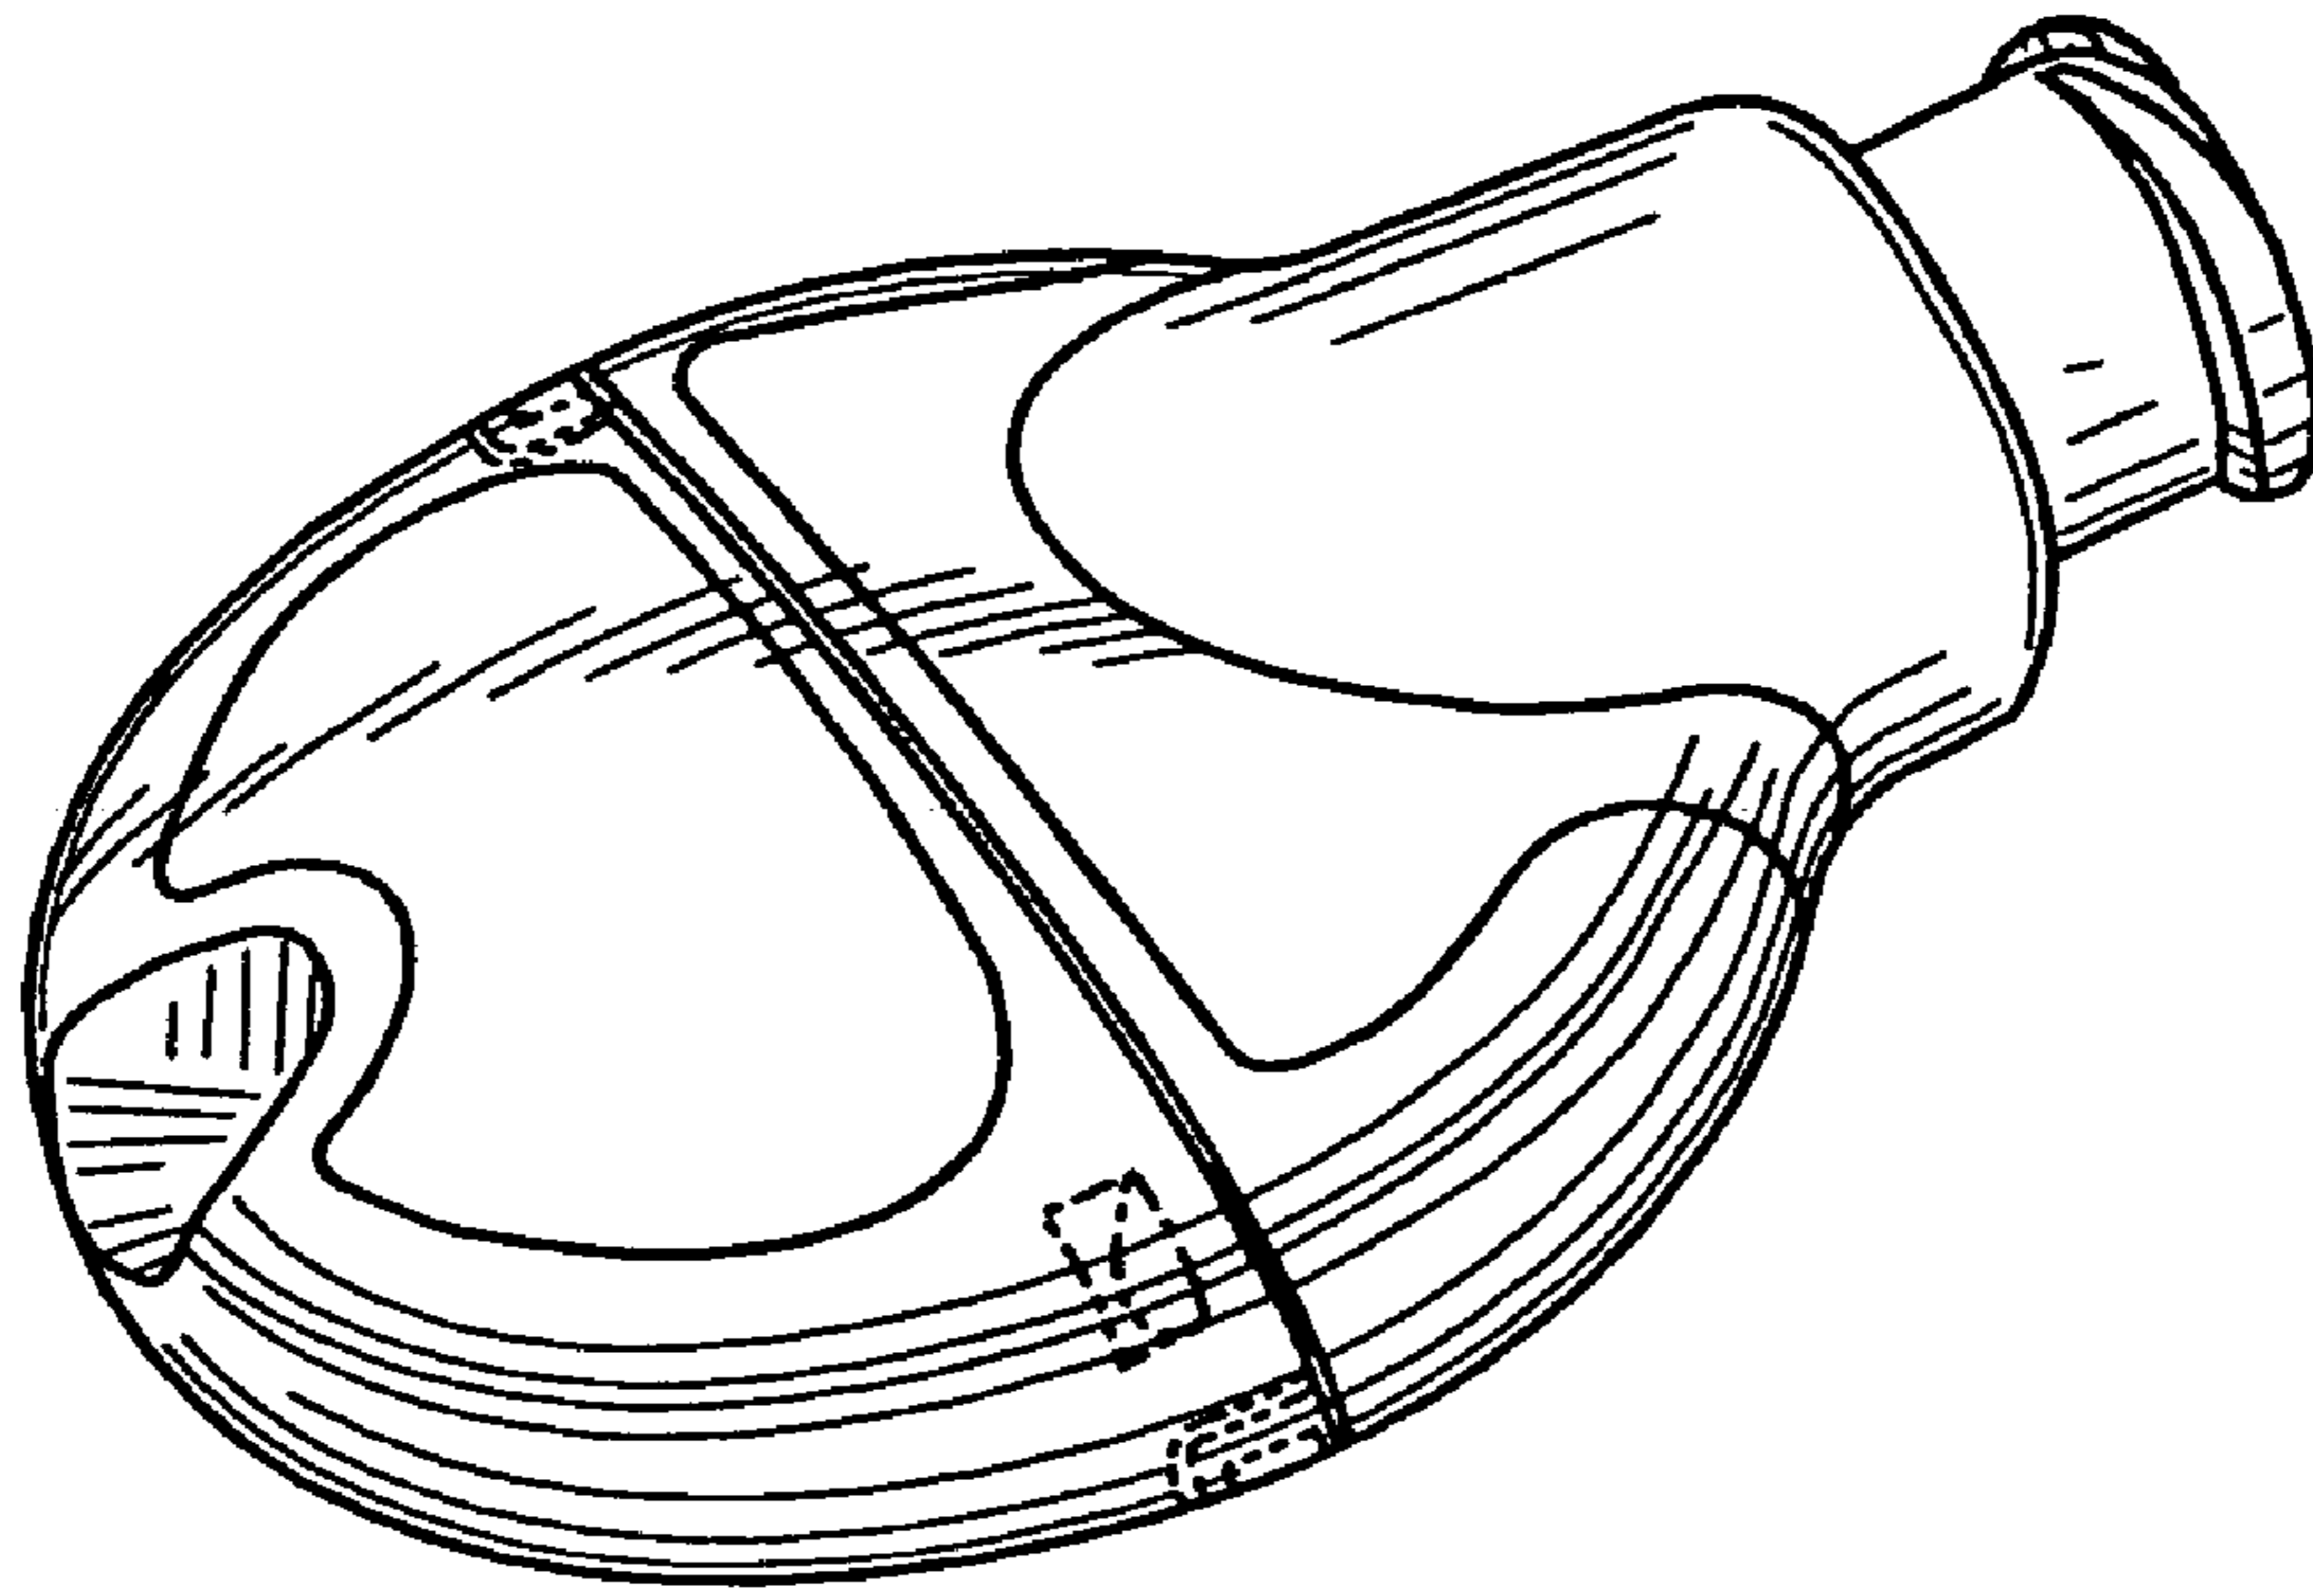


FIG. 2

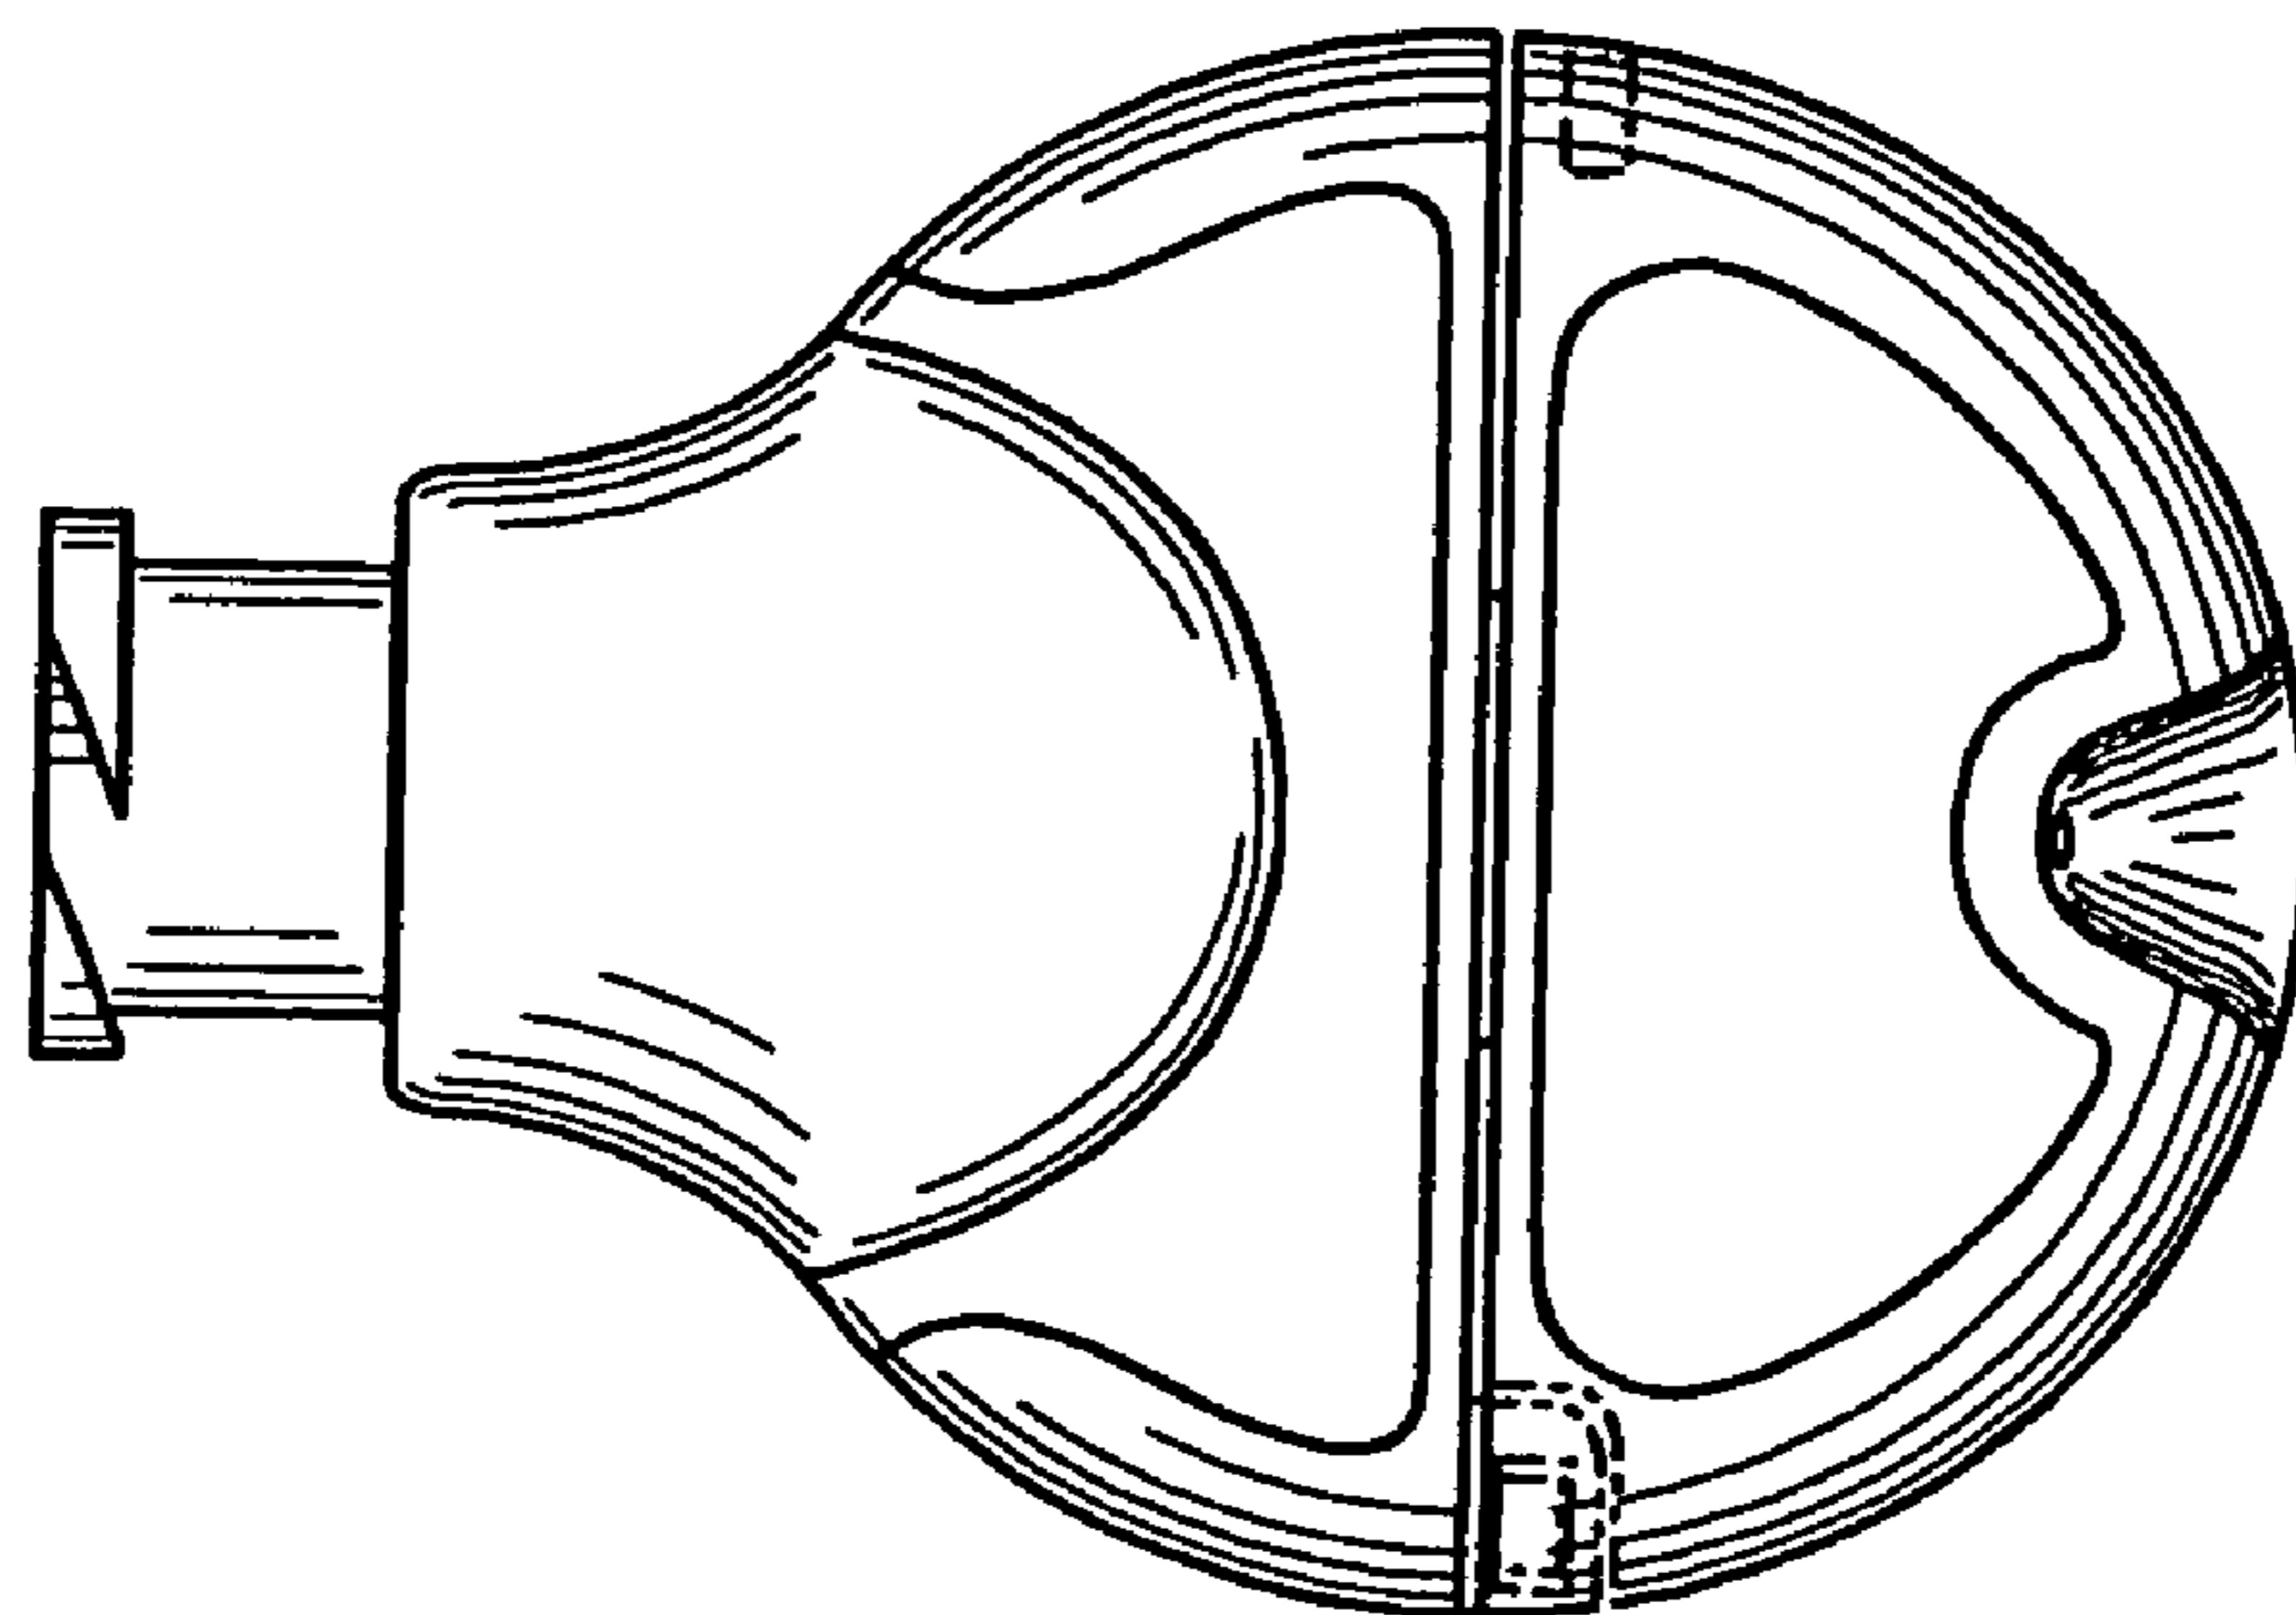


FIG. 3

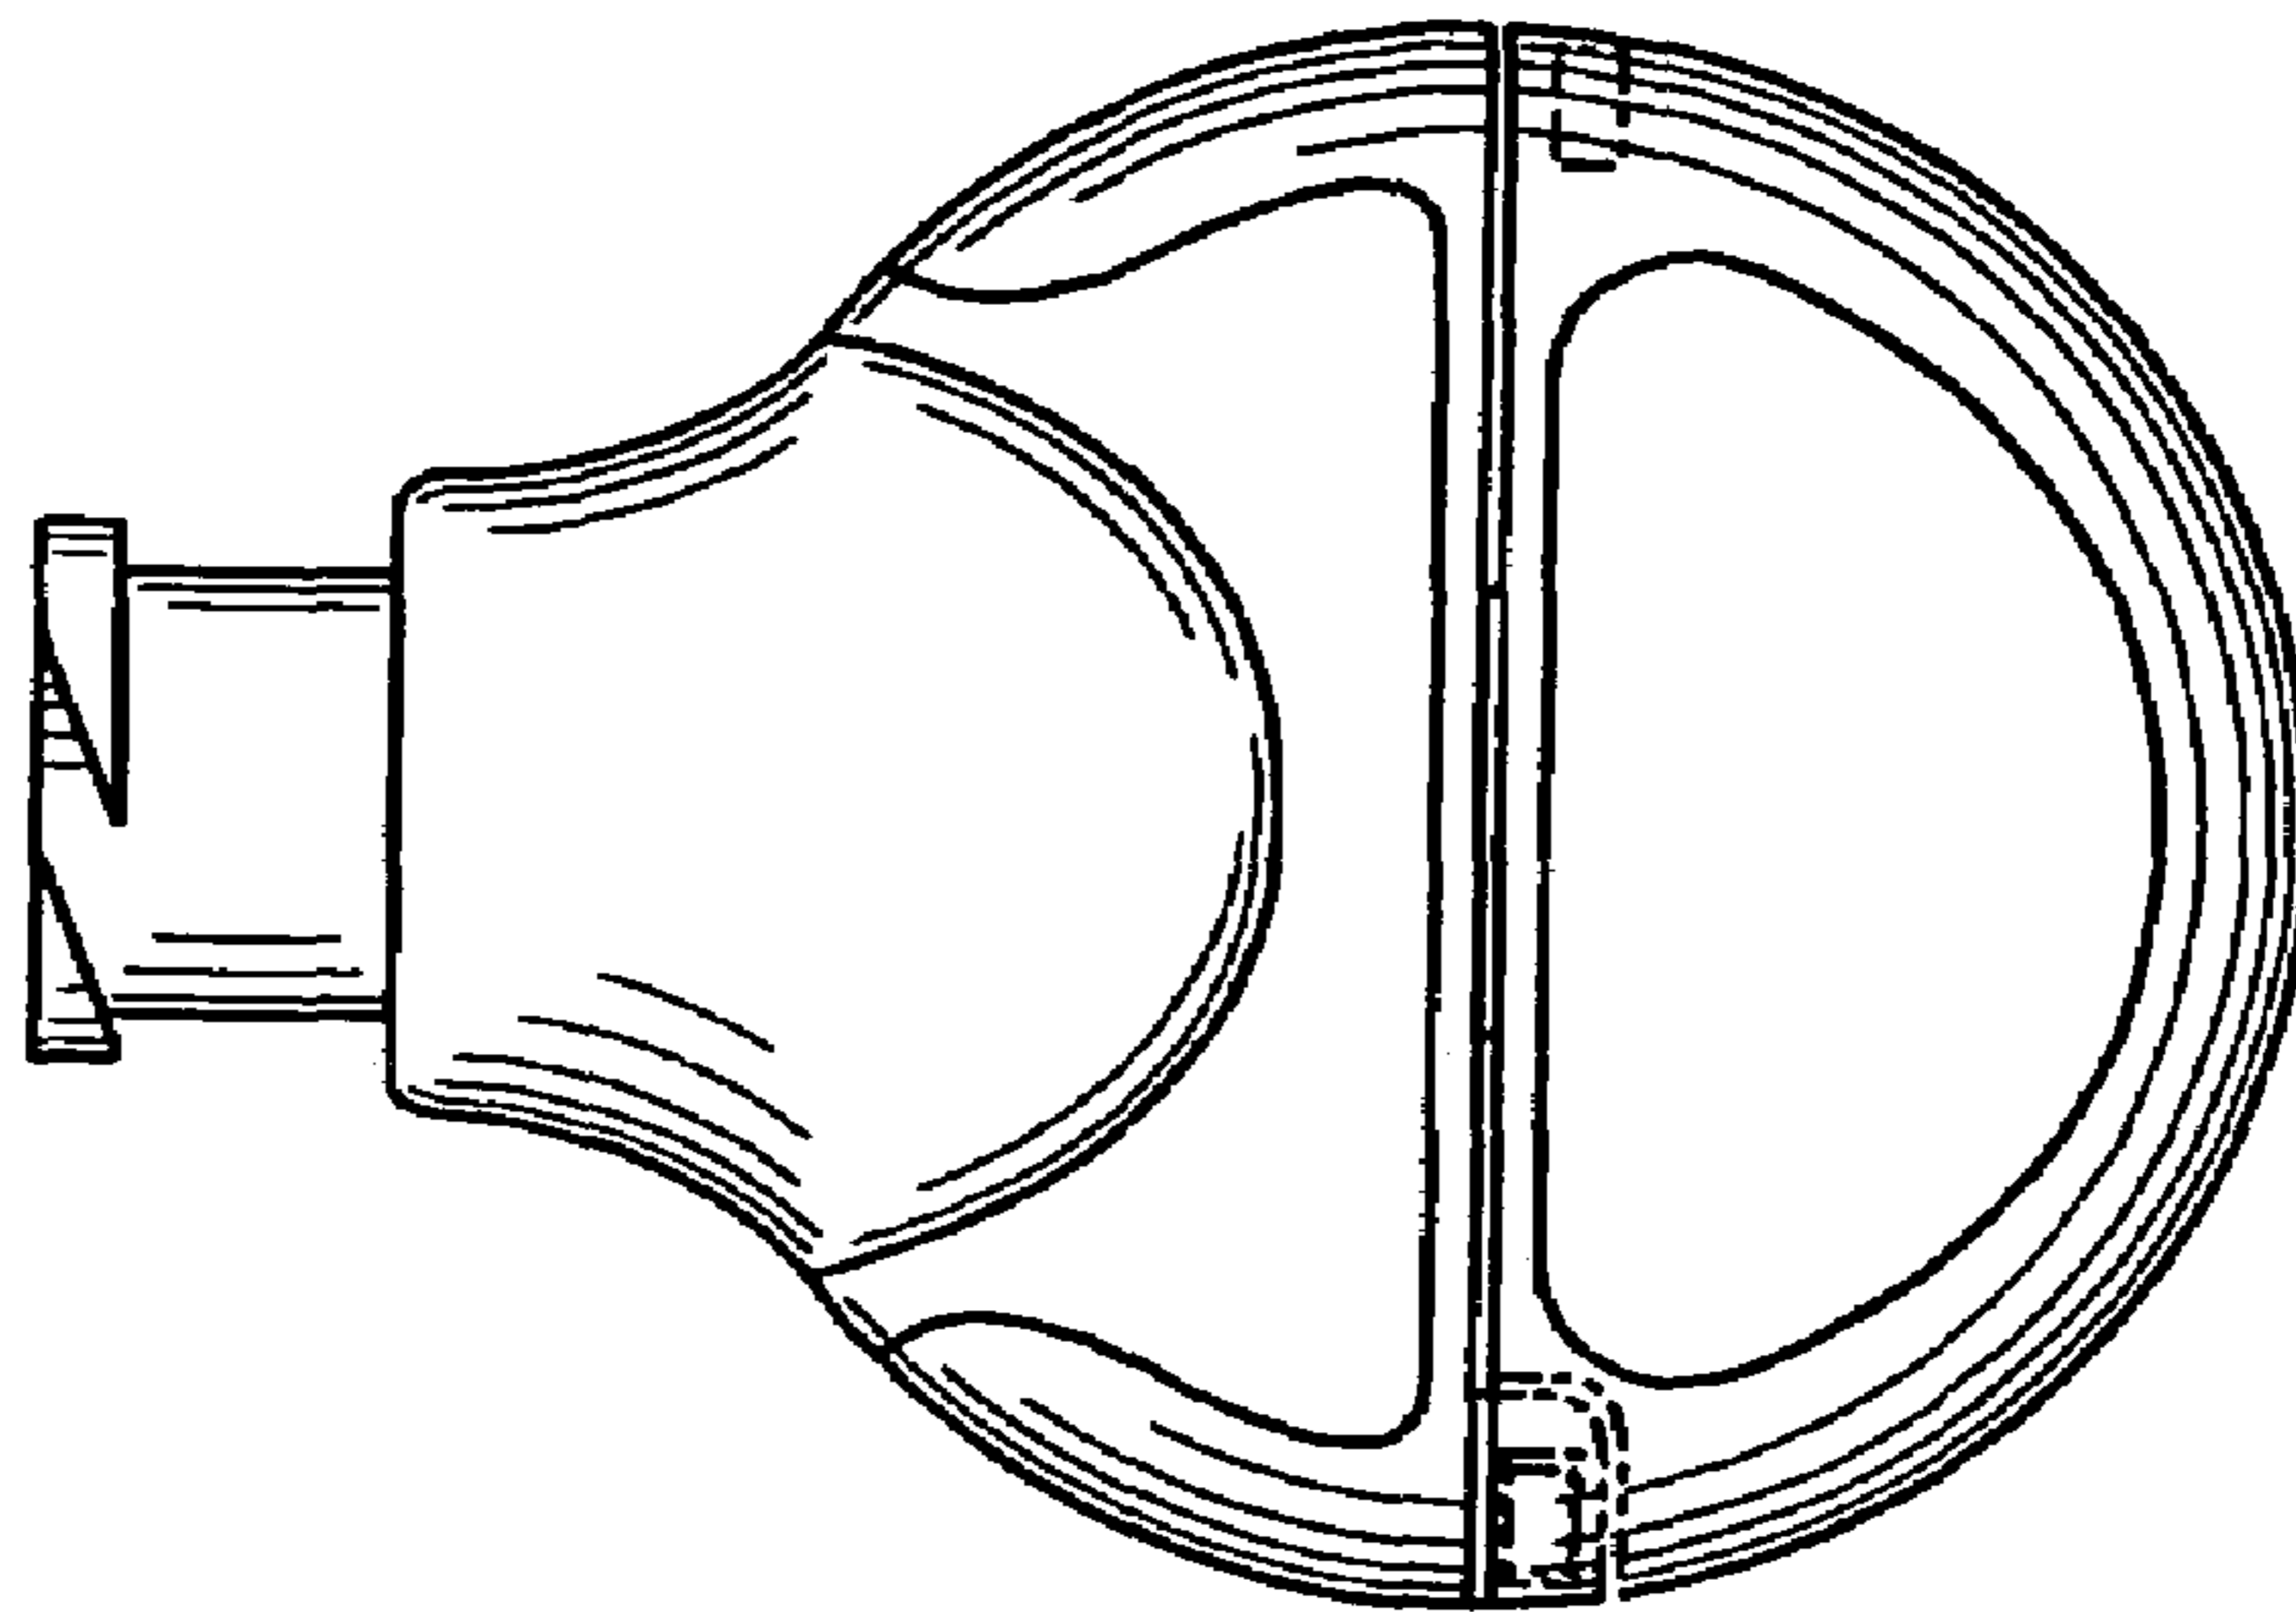


FIG. 4

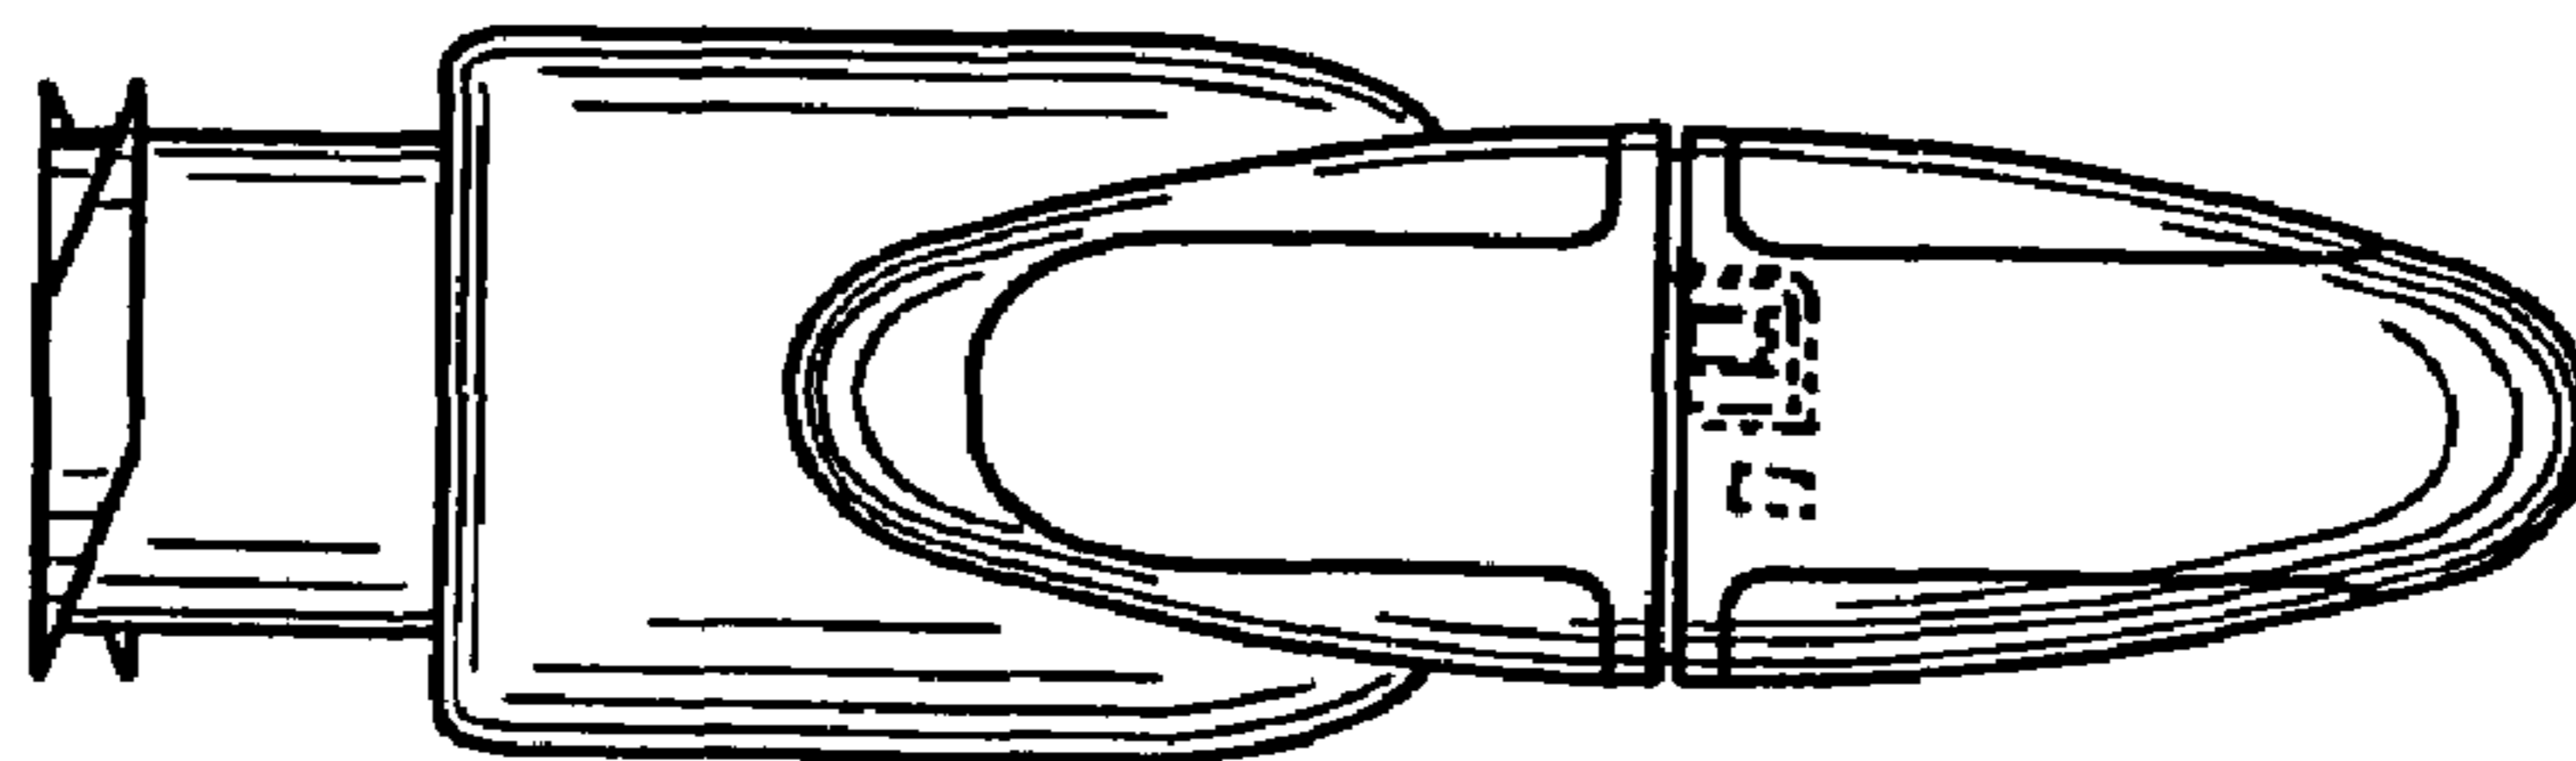


FIG. 5

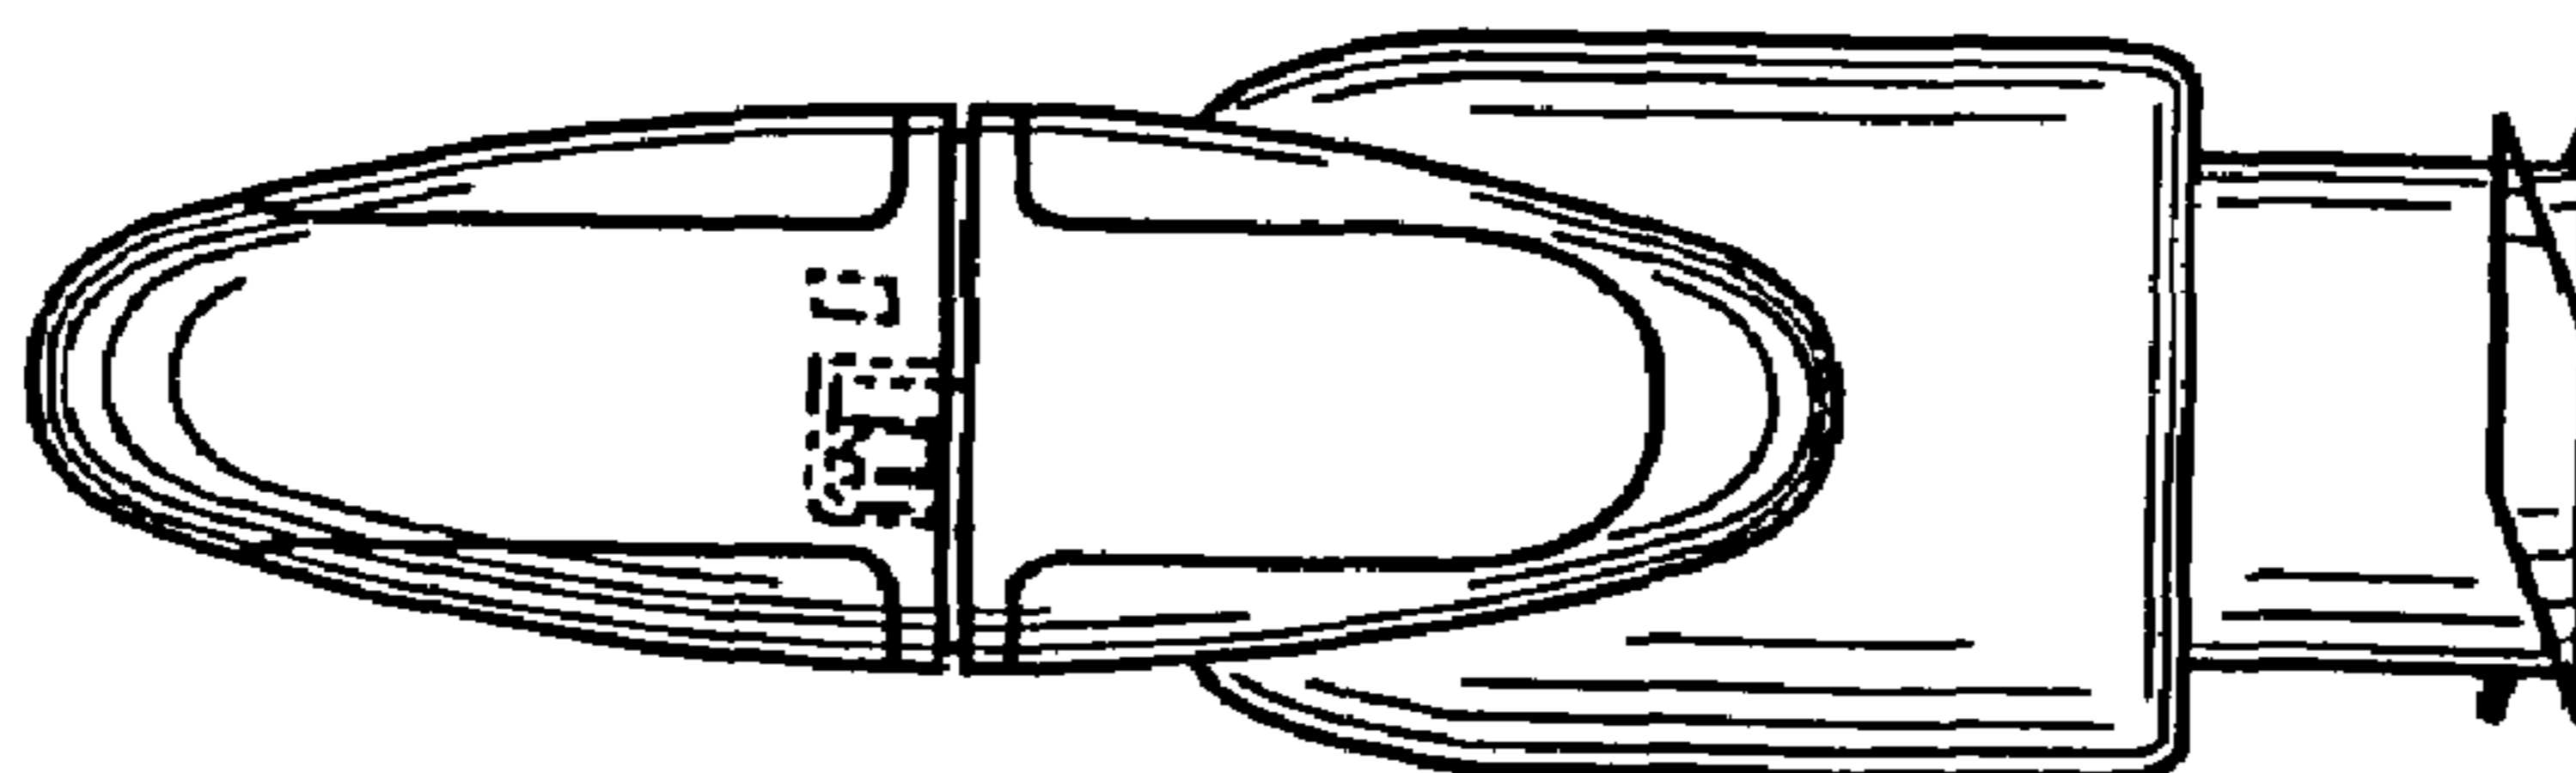


FIG. 6

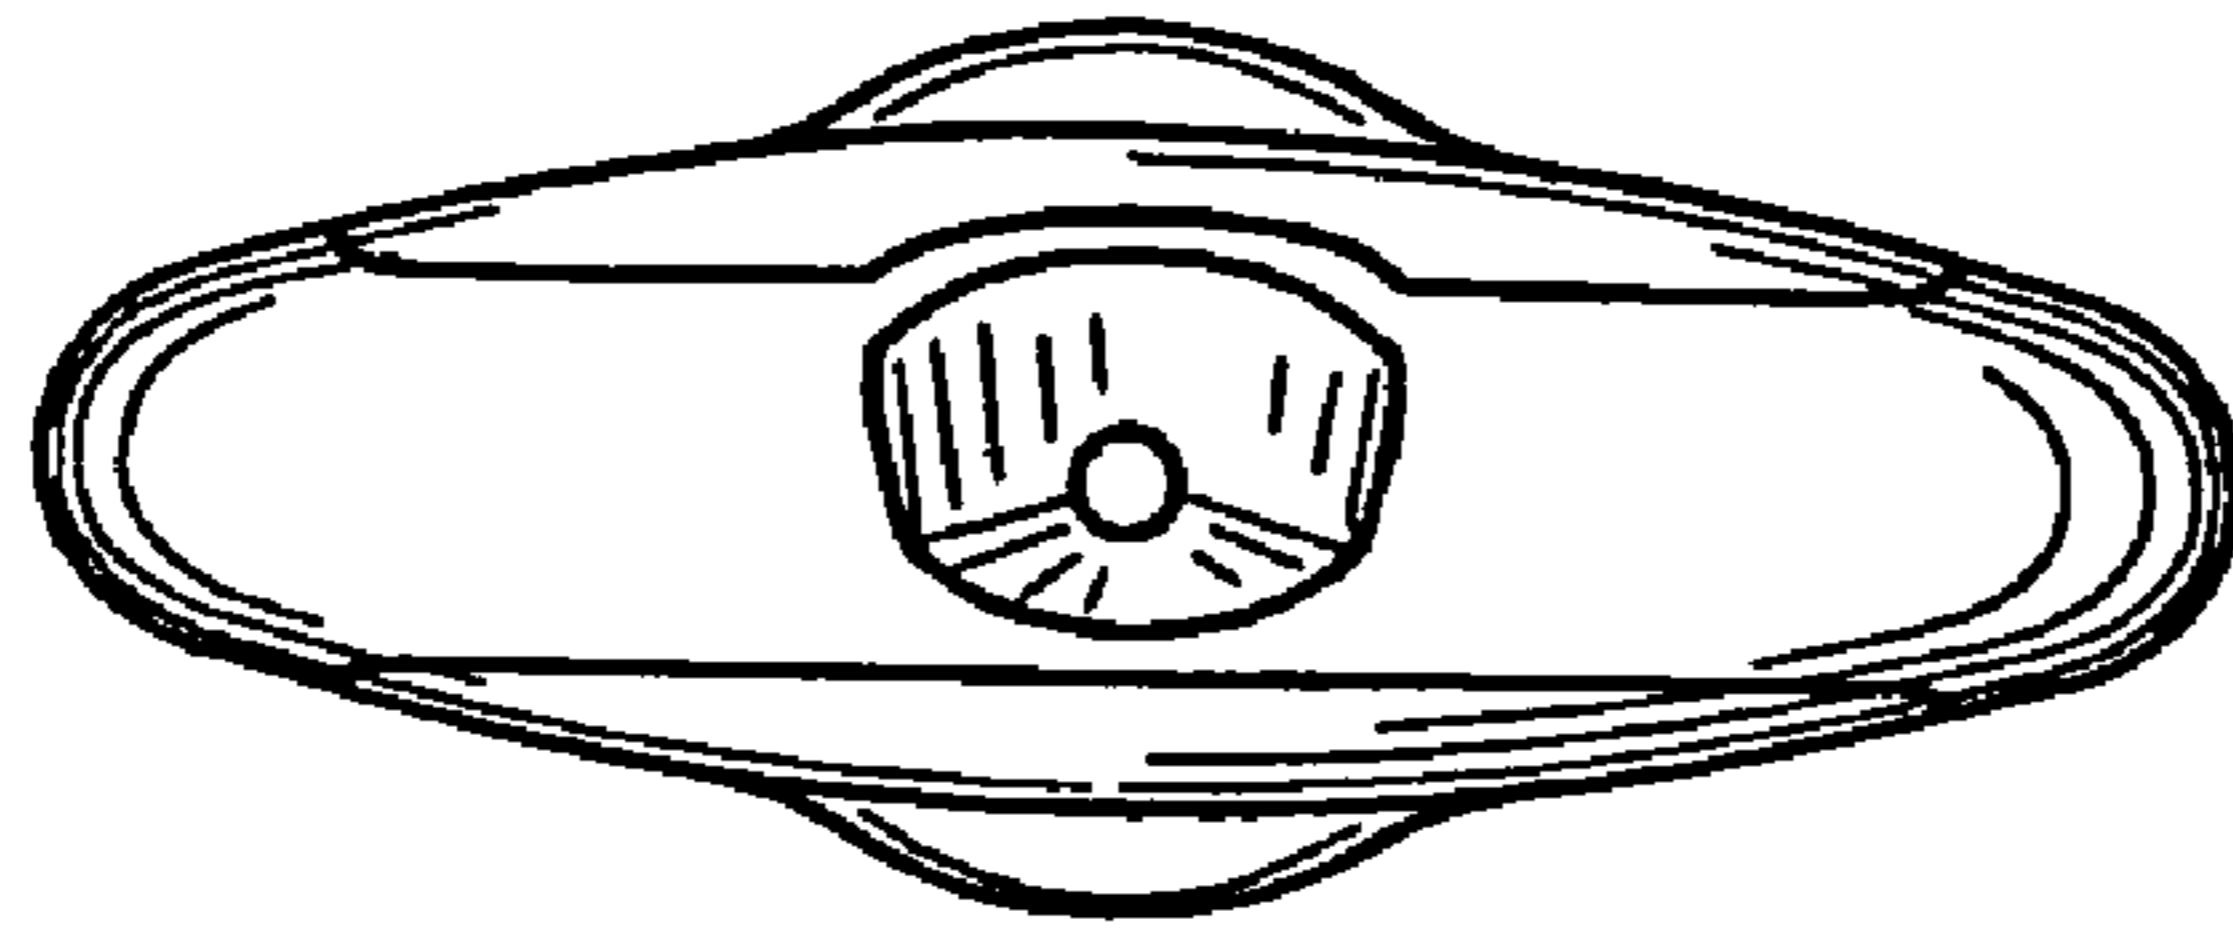


FIG. 7

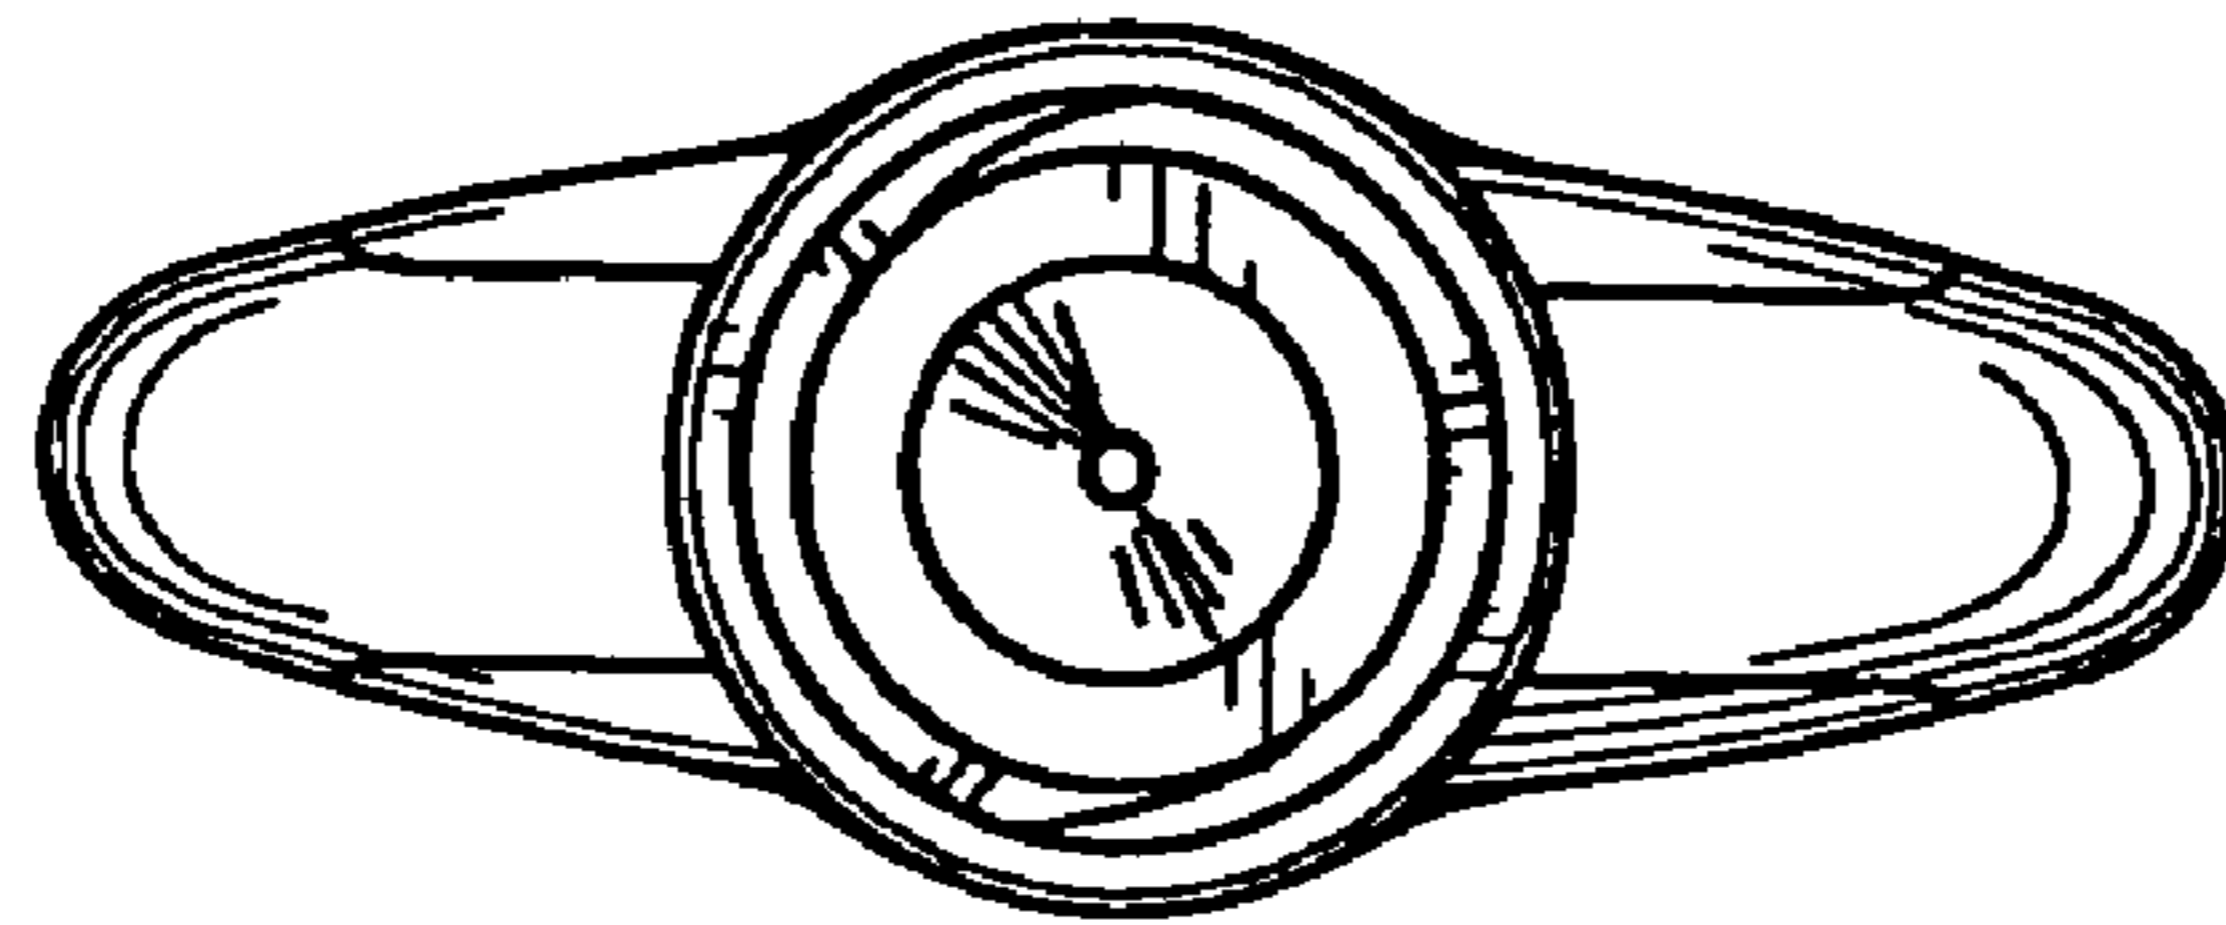


FIG. 8

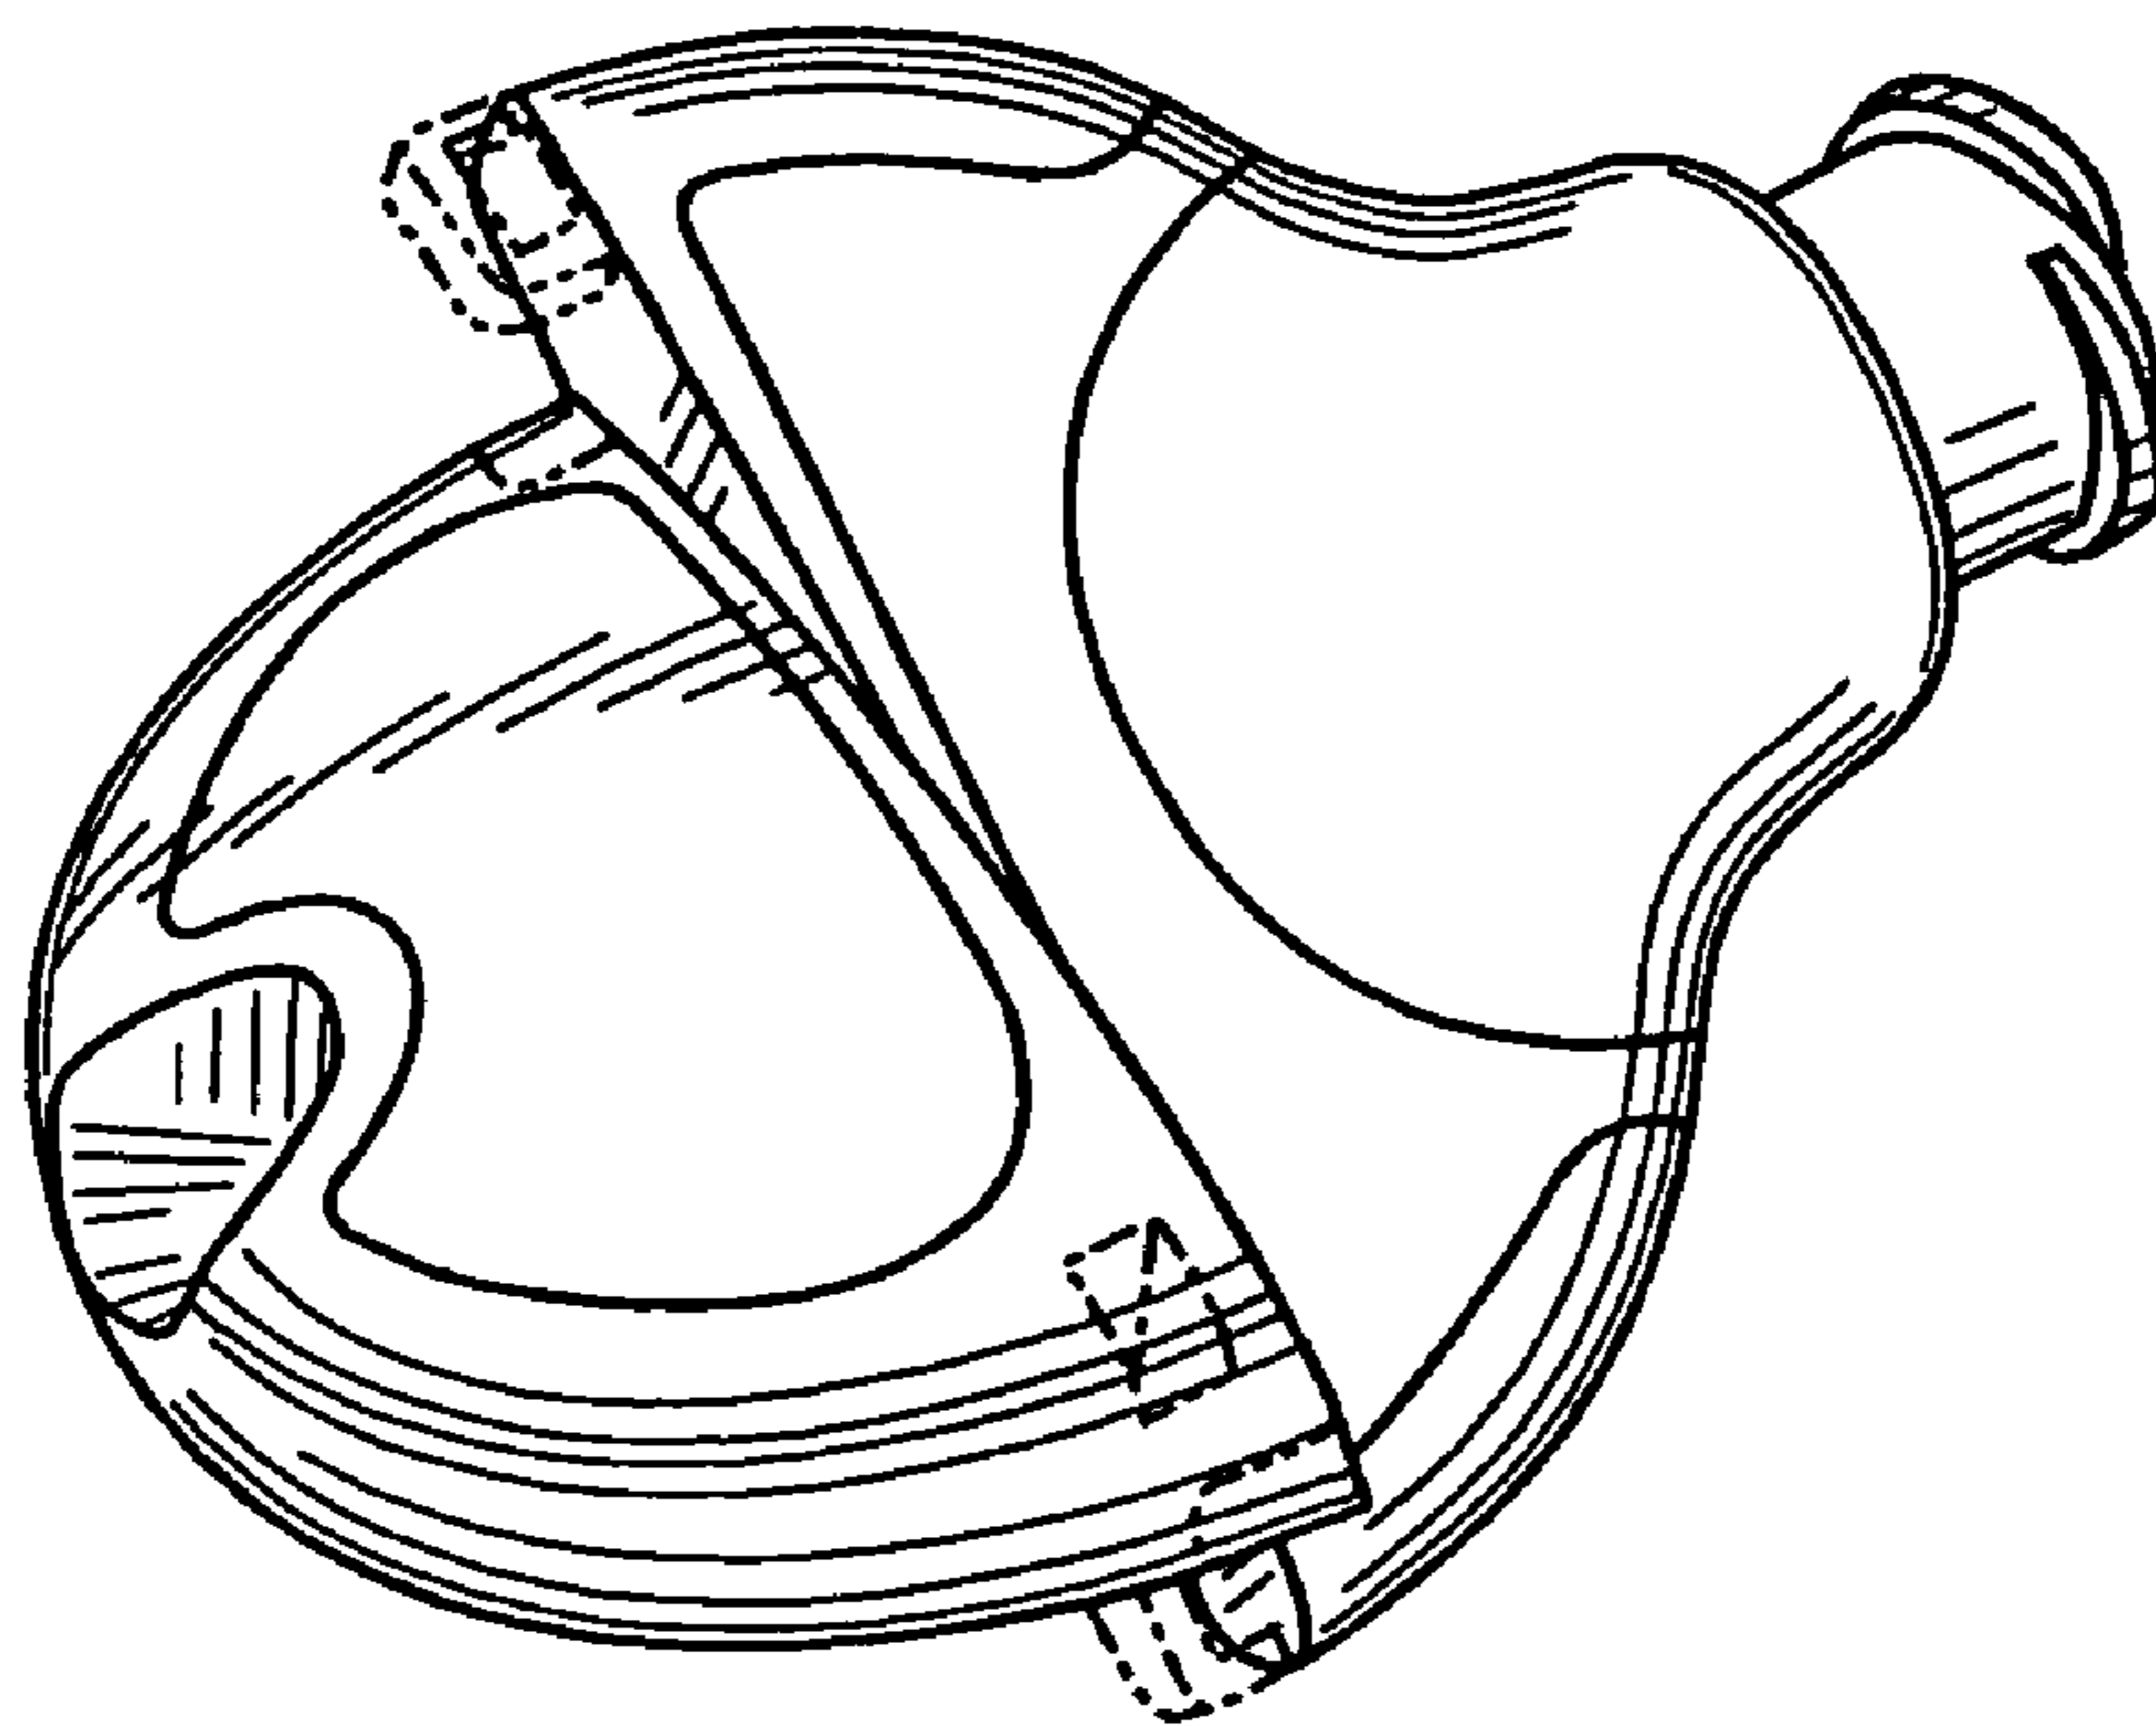


FIG. 9

UNITED STATES PATENT AND TRADEMARK OFFICE
CERTIFICATE OF CORRECTION

PATENT NO. : Des. 547,446 S
APPLICATION NO. : 29/224810
DATED : July 24, 2007
INVENTOR(S) : N. Sandor Racz and Gary Bullard

Page 1 of 1

It is certified that error appears in the above-identified patent and that said Letters Patent is hereby corrected as shown below:

On the title page:

In ITEM (56) **References Cited**
U.S. PATENT DOCUMENTS

1st column, 17th entry,

2nd column, 4th entry,

before the first entry "3,920,215 A 11/1975
Knauf" insert --3,254,671 A * 6/1966
Berliner ...137/565.12--
change "5,993,437 A 11/1999 Roaz" to
--5,993,437 A 11/1999 Racz--
change "6,254,589 B1 7/2001 Roaz" to --
6,254,589 B1 7/2001 Racz--

In DESCRIPTION

2nd column, 3rd line,

2nd column, 17th line,

change "my new design in situ;" to --our new
design in situ;--
change "FIG. 9 is a modified perspective view
showing the of the" to --FIG. 9 is a modified
perspective view showing the--

Signed and Sealed this

Sixth Day of May, 2008



JON W. DUDAS

Director of the United States Patent and Trademark Office