



US00D547862S

(12) **United States Design Patent**  
**Dikeman et al.**

(10) **Patent No.:** **US D547,862 S**  
(45) **Date of Patent:** **\*\* Jul. 31, 2007**

(54) **ADHESIVE PATIENT-CONTACT STRIP FOR INTRAVENOUS CATHETER ANCHORING DEVICES**

(75) Inventors: **W. Cary Dikeman**, Lenexa, KS (US); **Chris Winsor**, Olathe, KS (US); **Steve A. Cash**, Overland Park, KS (US); **Larry C. Smith**, Shawnee, KS (US)

(73) Assignee: **Nexus Medical, LLC**, Lenexa, KS (US)

(\*\*) Term: **14 Years**

(21) Appl. No.: **29/253,412**

(22) Filed: **Feb. 6, 2006**

(51) **LOC (8) Cl.** ..... **24-02**

(52) **U.S. Cl.** ..... **D24/128**

(58) **Field of Classification Search** ..... D24/128, D24/189; D30/133, 155; 128/DIG. 6, DIG. 26; 604/174, 178-180; 602/41-47, 50, 54-55, 602/57, 58-59

See application file for complete search history.

(56) **References Cited**

**U.S. PATENT DOCUMENTS**

4,711,636 A 12/1987 Bierman

(Continued)

**OTHER PUBLICATIONS**

Zefon International printout from [www.zefon.com/medical/griplok.htm](http://www.zefon.com/medical/griplok.htm) depicting prior art Grip-Lok Universal Tubing Securement Device (printed. Jun. 20, 2005).

(Continued)

*Primary Examiner*—Louis S. Zarfaz  
*Assistant Examiner*—Eric L Goodman

(74) *Attorney, Agent, or Firm*—Hovey Williams LLP

(57) **CLAIM**

The ornamental design for an adhesive patient-contact strip for intravenous catheter anchoring devices, as shown and described.

**DESCRIPTION**

FIG. 1 is a perspective view of an adhesive patient-contact strip for intravenous catheter anchoring devices embodying our design, with the strip being shown in use with an intravenous site securement device and catheter for environmental purposes only, and the device and catheter consequently being shown in broken lines and forming no part of the claimed design;

FIG. 2 is a perspective view of the adhesive patient-contact strip similar to FIG. 1, but with the site securement device and catheter being removed;



FIG. 3 is a top plan view of the adhesive patient-contact strip depicted in FIGS. 1 and 2;

FIG. 4 is a side elevation view of the adhesive patient-contact strip depicted in FIGS. 1-3, with the opposite side elevation being a mirror image thereof;

FIG. 5 is an end elevation view of the adhesive patient-contact strip depicted in FIGS. 1-4, with the opposite end elevation being a mirror image thereof; and,

FIG. 6 is a perspective view of the adhesive patient-contact strip similar to that of FIG. 1, but illustrating the strip in use with a catheter tubing collector, and the tubing collector consequently being shown in broken lines and forming no part of the claimed design.

**1 Claim, 1 Drawing Sheet**

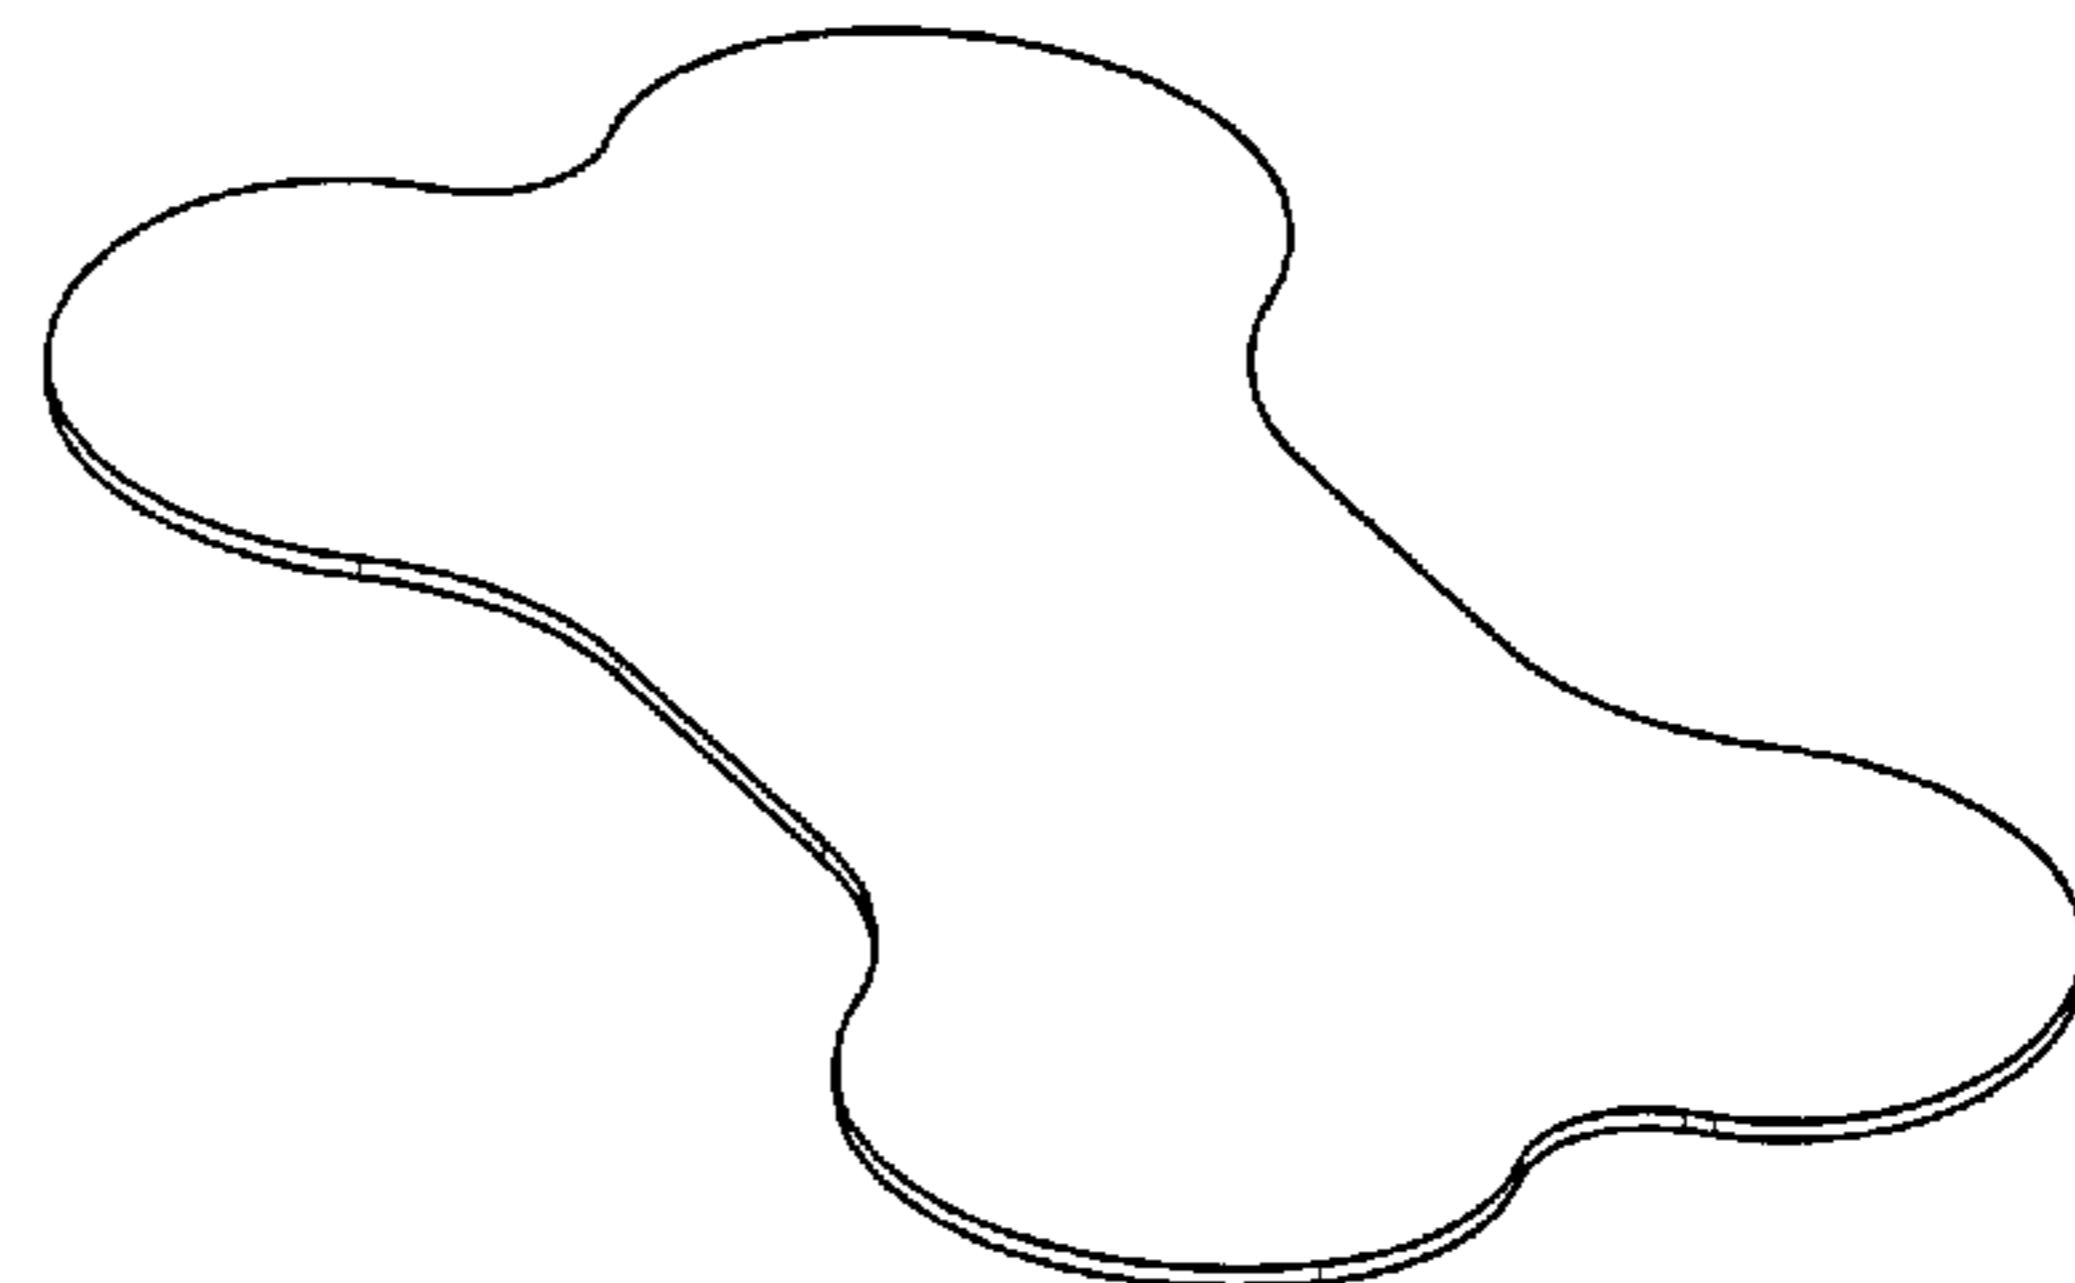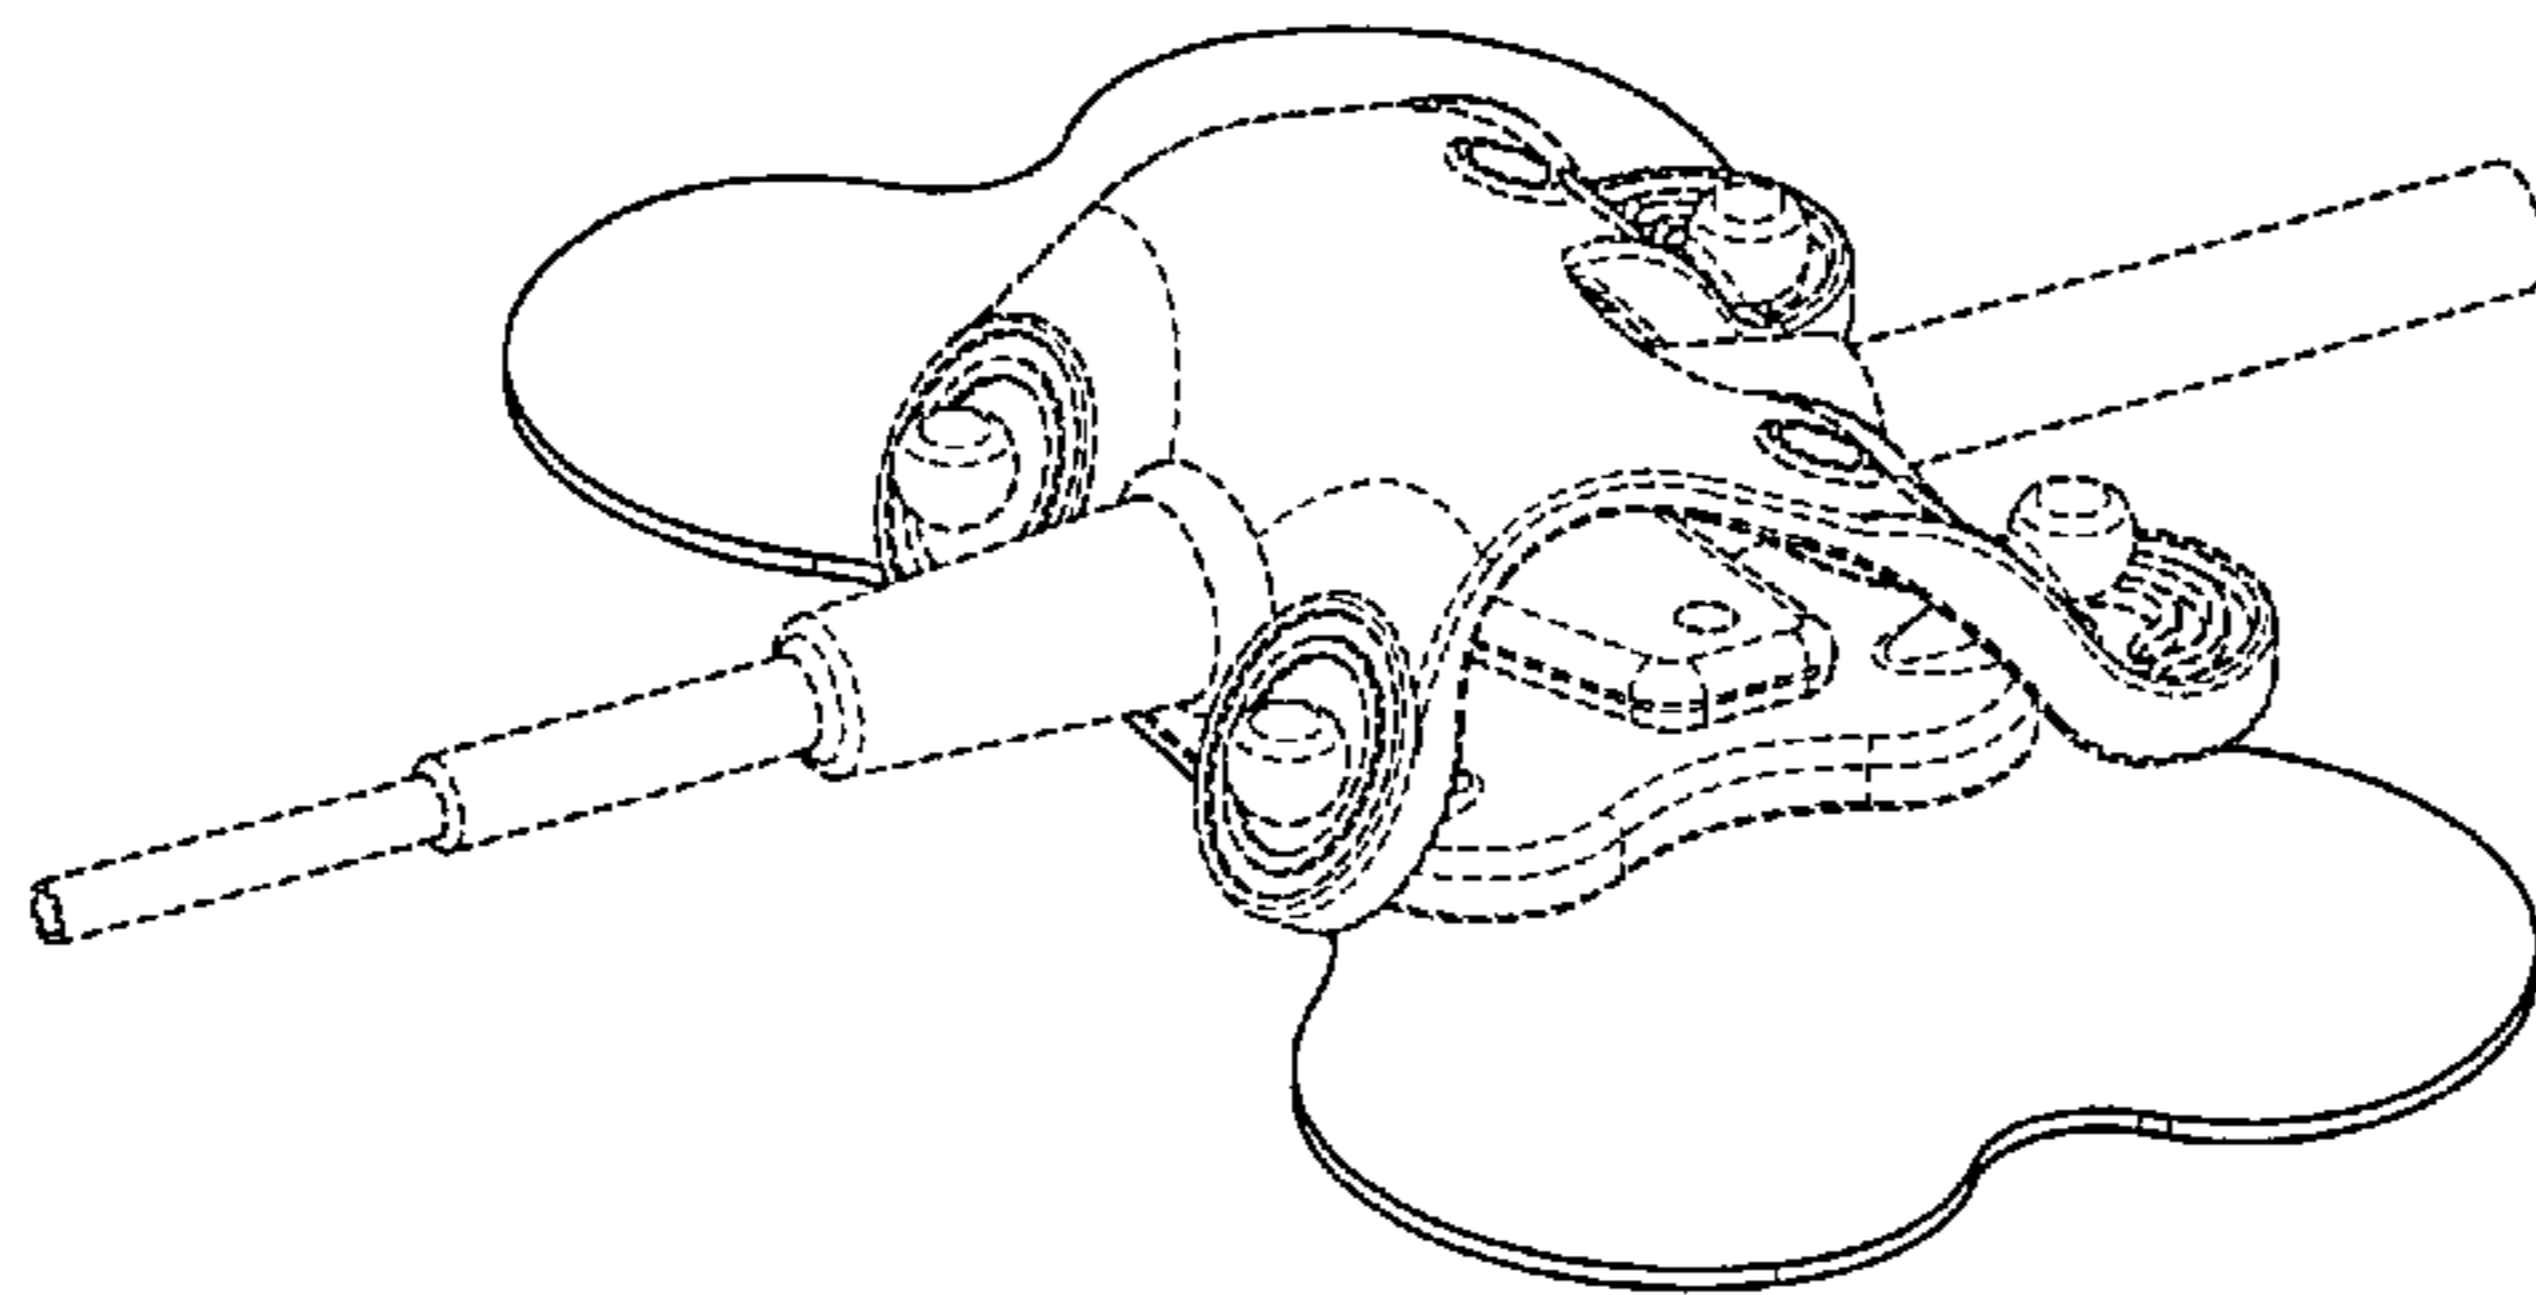

# US D547,862 S

## U.S. PATENT DOCUMENTS

5,192,273	A	3/1993	Bierman et al.	6,468,383	B2 *	10/2002	Kundel ..... 156/272.2
5,192,274	A	3/1993	Bierman	6,491,664	B2	12/2002	Bierman
5,290,248	A	3/1994	Bierman et al.	D470,936	S	2/2003	Bierman
D347,060	S	5/1994	Bierman	D471,631	S *	3/2003	Dunshee et al. .... D24/189
5,314,411	A	5/1994	Bierman et al.	6,551,285	B1	4/2003	Bierman
5,318,546	A	6/1994	Bierman	6,572,588	B1	6/2003	Bierman et al.
5,354,282	A	10/1994	Bierman	6,582,403	B1	6/2003	Bierman et al.
5,456,671	A	10/1995	Bierman	D492,411	S	6/2004	Bierman
D364,922	S	12/1995	Bierman	6,770,055	B2	8/2004	Bierman et al.
D375,355	S	11/1996	Bierman	6,786,892	B2	9/2004	Bierman
D375,356	S	11/1996	Bierman	6,796,310	B2	9/2004	Bierman
5,578,013	A	11/1996	Bierman	6,829,705	B2	12/2004	Smith
D377,831	S	2/1997	Bierman	6,837,875	B1	1/2005	Bierman
5,637,098	A	6/1997	Bierman	D503,977	S	4/2005	Bierman
5,693,032	A	12/1997	Bierman	D510,171	S *	10/2005	Lawrenson ..... D1/106
5,702,371	A	12/1997	Bierman	D513,323	S *	12/2005	Mueller et al. .... D24/189
D389,911	S	1/1998	Bierman	D521,690	S *	5/2006	Krcek et al. .... D30/133
5,722,959	A	3/1998	Bierman	2003/0150402	A1 *	8/2003	Muller ..... 119/856
D393,903	S	4/1998	Bierman	2006/0206047	A1 *	9/2006	Lampe et al. .... 602/42
5,800,402	A	9/1998	Bierman	2006/0229620	A1 *	10/2006	Rothman et al. .... 606/69
5,810,781	A	9/1998	Bierman	2006/0272588	A1 *	12/2006	Decroix ..... 119/61.5
D399,954	S	10/1998	Bierman				
5,827,230	A	10/1998	Bierman				
D401,329	S	11/1998	Bierman				
5,833,663	A	11/1998	Bierman et al.				
D404,815	S	1/1999	Bierman				
5,941,263	A	8/1999	Bierman				
D424,691	S *	5/2000	Yavitz ..... D24/128				
D425,619	S	5/2000	Bierman				
6,117,163	A	9/2000	Bierman				
D432,656	S *	10/2000	Nash et al. .... D24/189				
6,132,398	A	10/2000	Bierman				
6,213,979	B1	4/2001	Bierman				
6,224,571	B1	5/2001	Bierman				
6,283,945	B1	9/2001	Bierman				
6,290,676	B1	9/2001	Bierman				
6,361,523	B1	3/2002	Bierman				
6,413,240	B1 *	7/2002	Bierman et al. .... 604/174				
6,428,515	B1	8/2002	Bierman et al.				
6,458,104	B2	10/2002	Gautsche				

## OTHER PUBLICATIONS

Tri-State Hospital Supply Corporation, Centurion Healthcare Products brochure for LineGuard J-Loop Securement Device (Nov. 2, 2004).

Tri-State Hospital Supply Corporation, Centurion Healthcare Products brochure for SorbaView 2000 Window Dressing (Apr. 14, 2004).

Tri-State Hospital Supply Corporation, Centurion Healthcare Products brochure for IV Start Kits (Sep. 14, 2004).

Tri-State Hospital Supply Corporation, Centurion Healthcare Products brochure for HubGuard Catheter Securement (Mar. 3, 2004).

Tri-State Hospital Supply Corporation, Centurion Healthcare Products brochure for SorbaView Ultimate Window Dressing (May 7, 2004 and Jun. 22, 2004).

Tri-State Hospital Supply Corporation, Centurion Healthcare Products brochure for Port Access Trays (Apr. 24, 2003).

\* cited by examiner

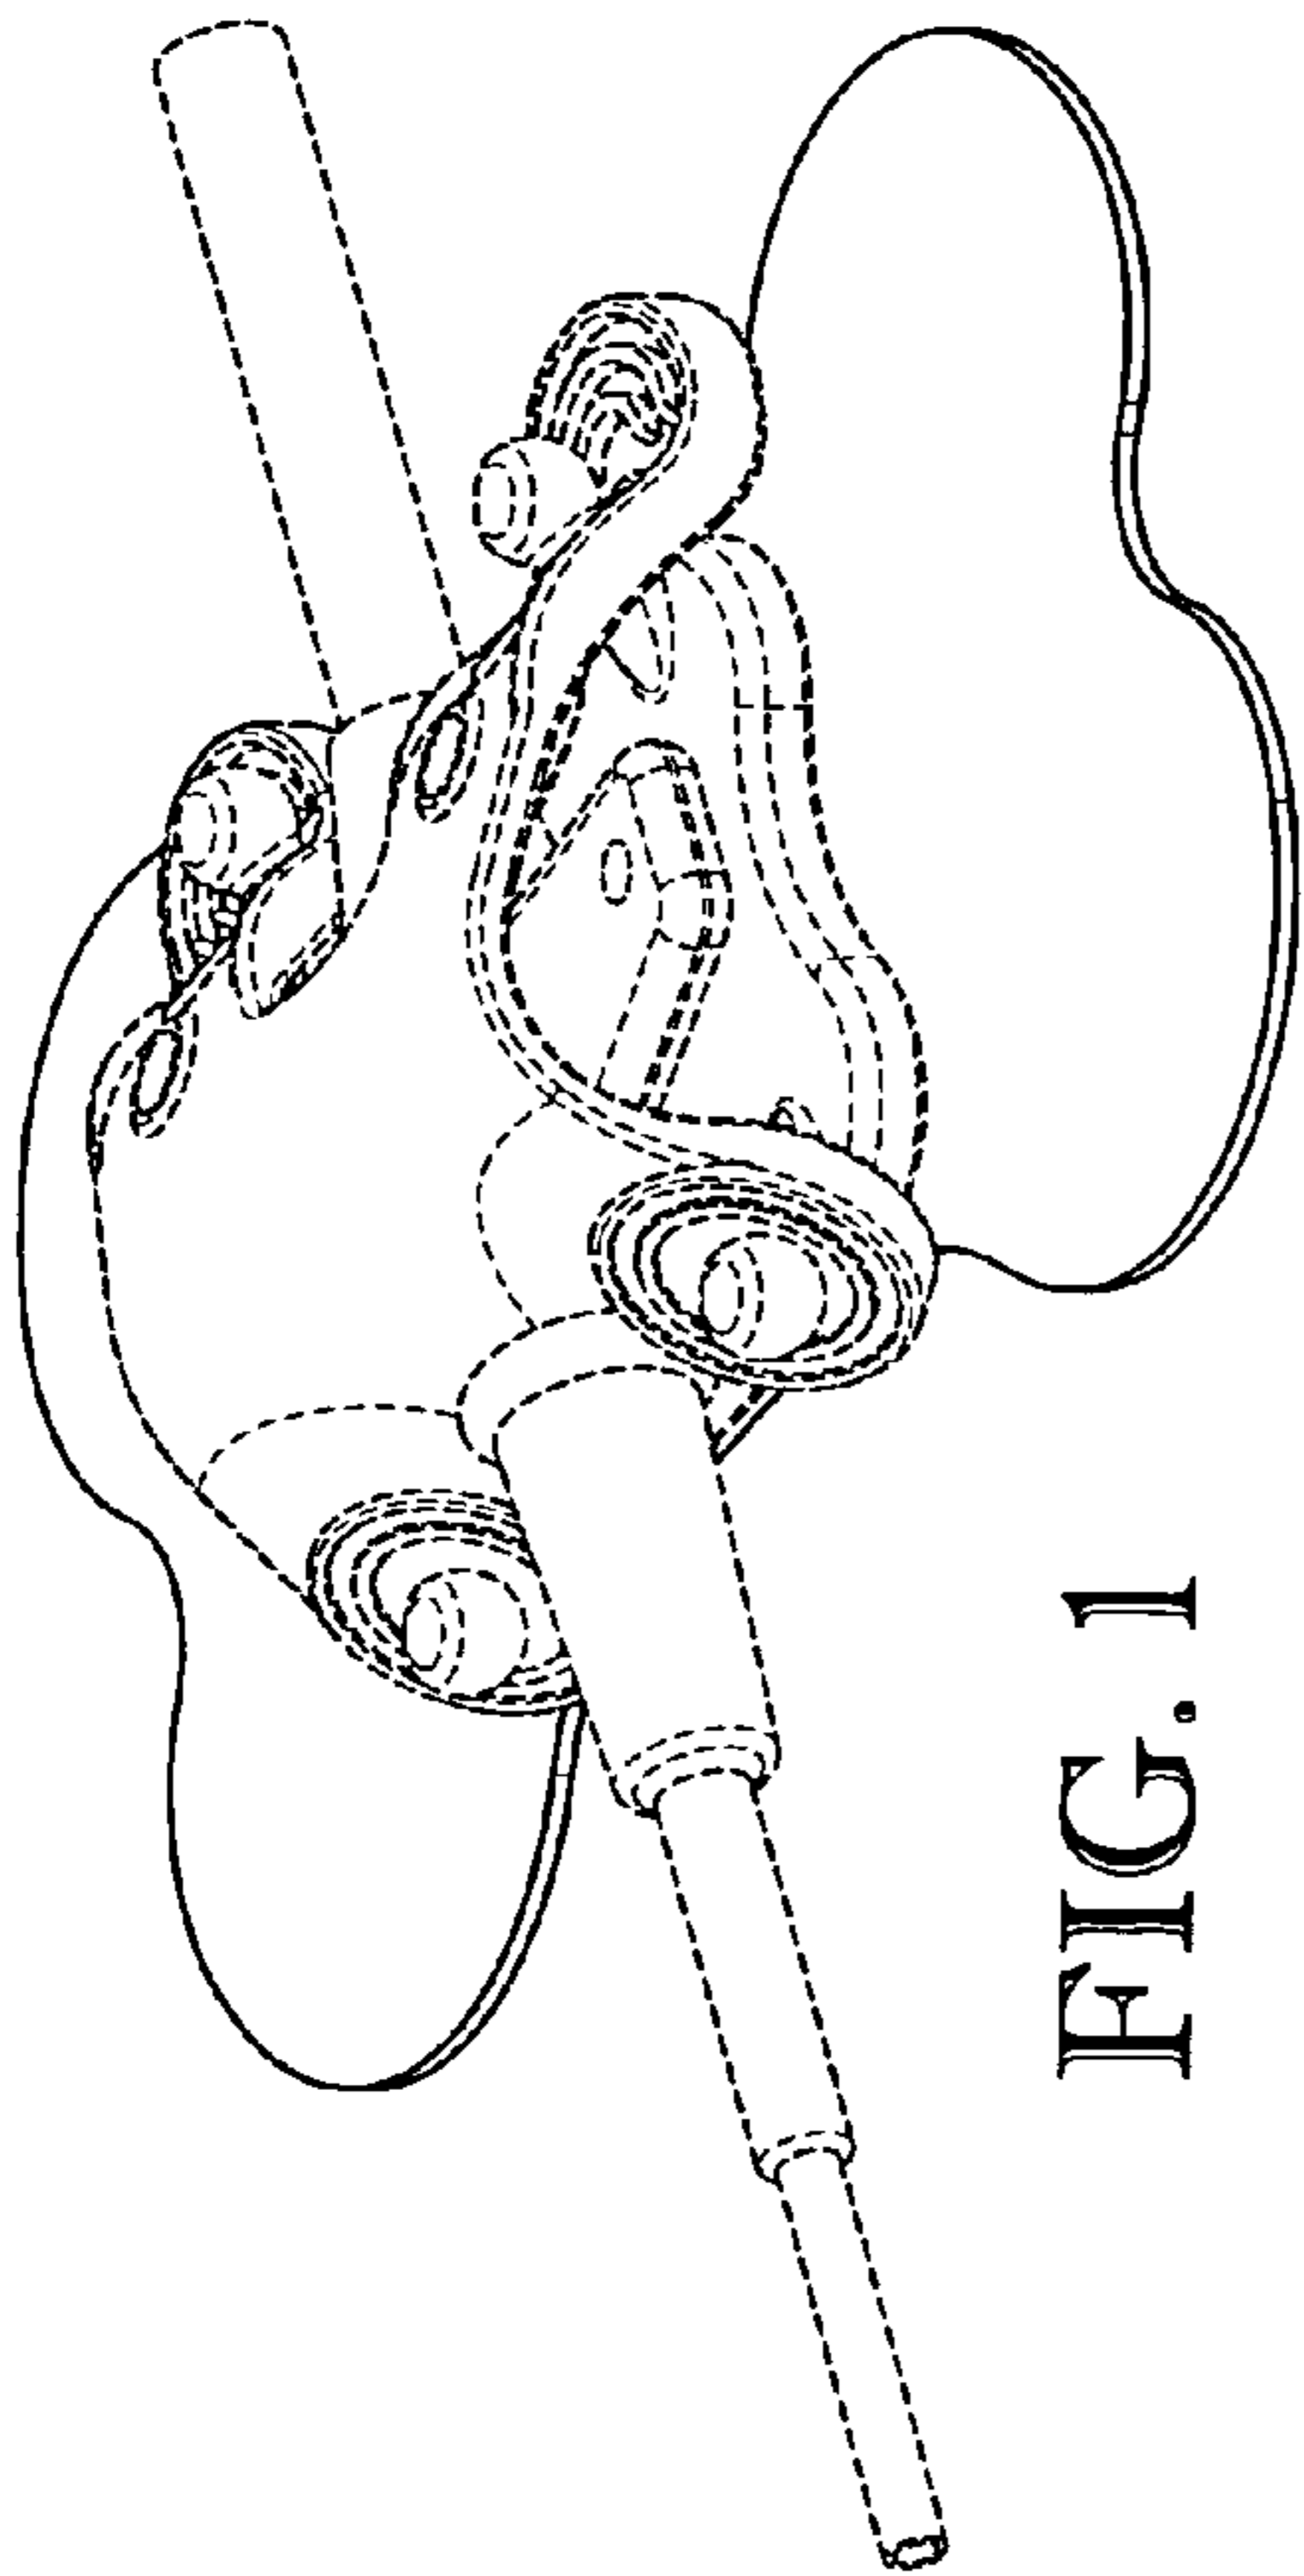


FIG. 1

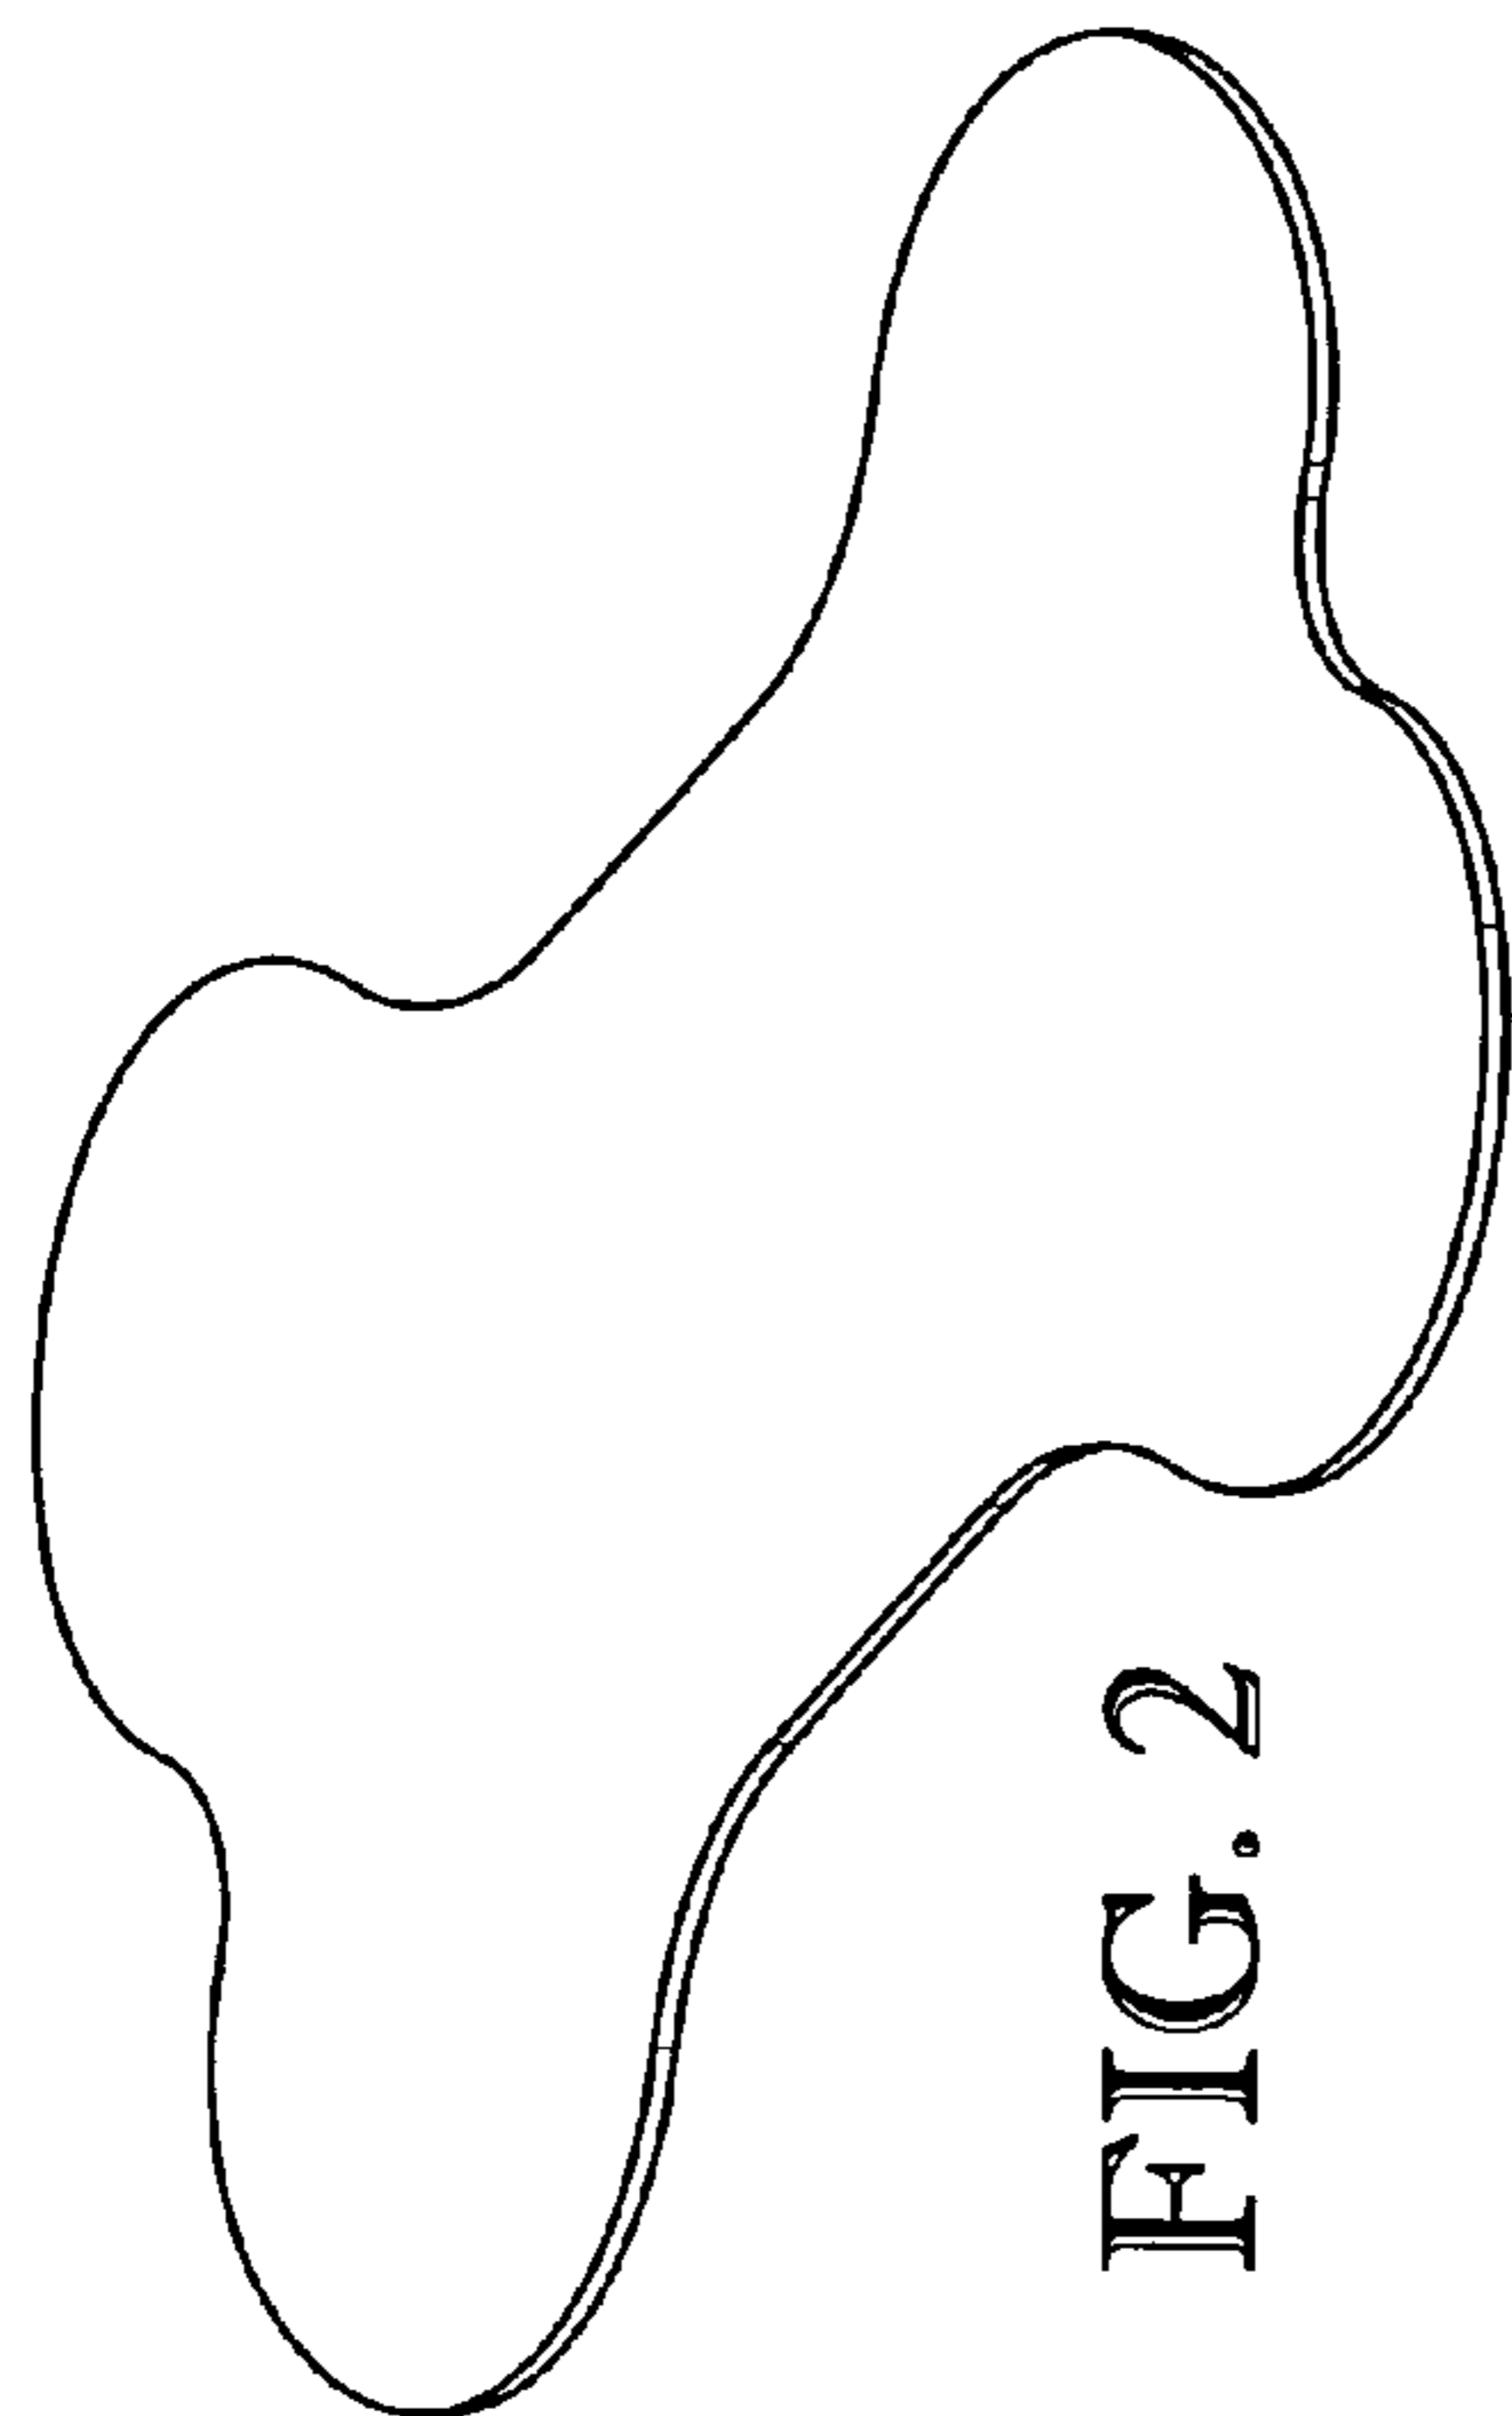


FIG. 2

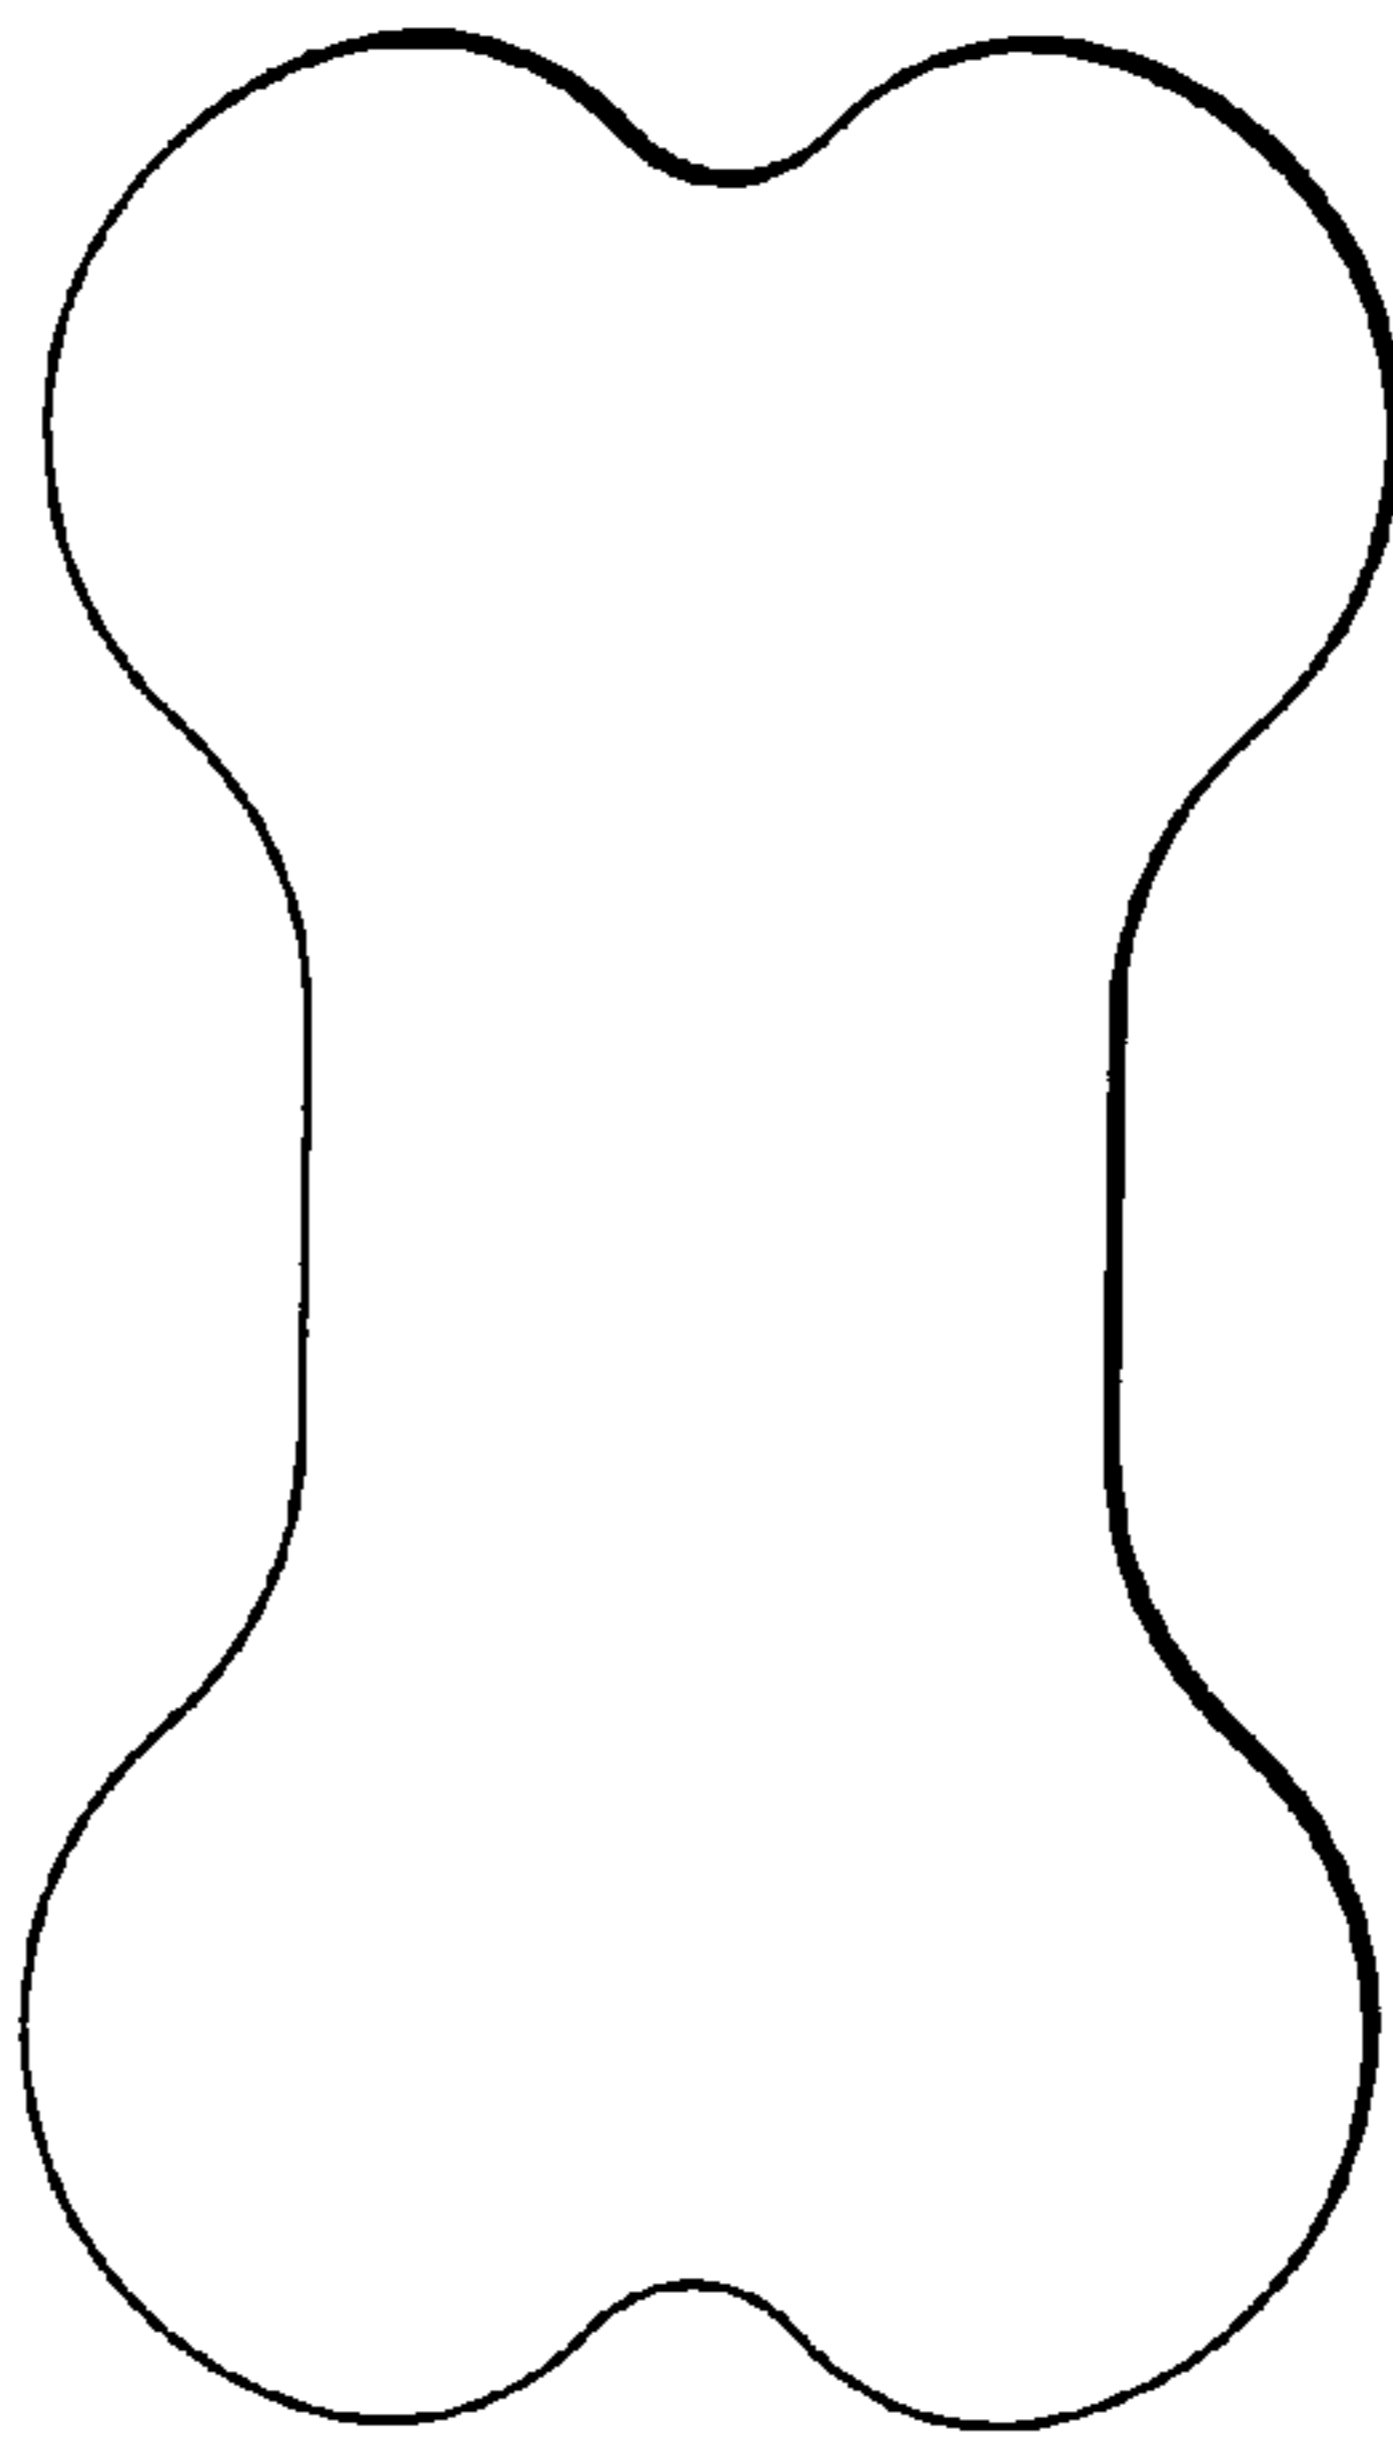


FIG. 3



FIG. 4

FIG. 5

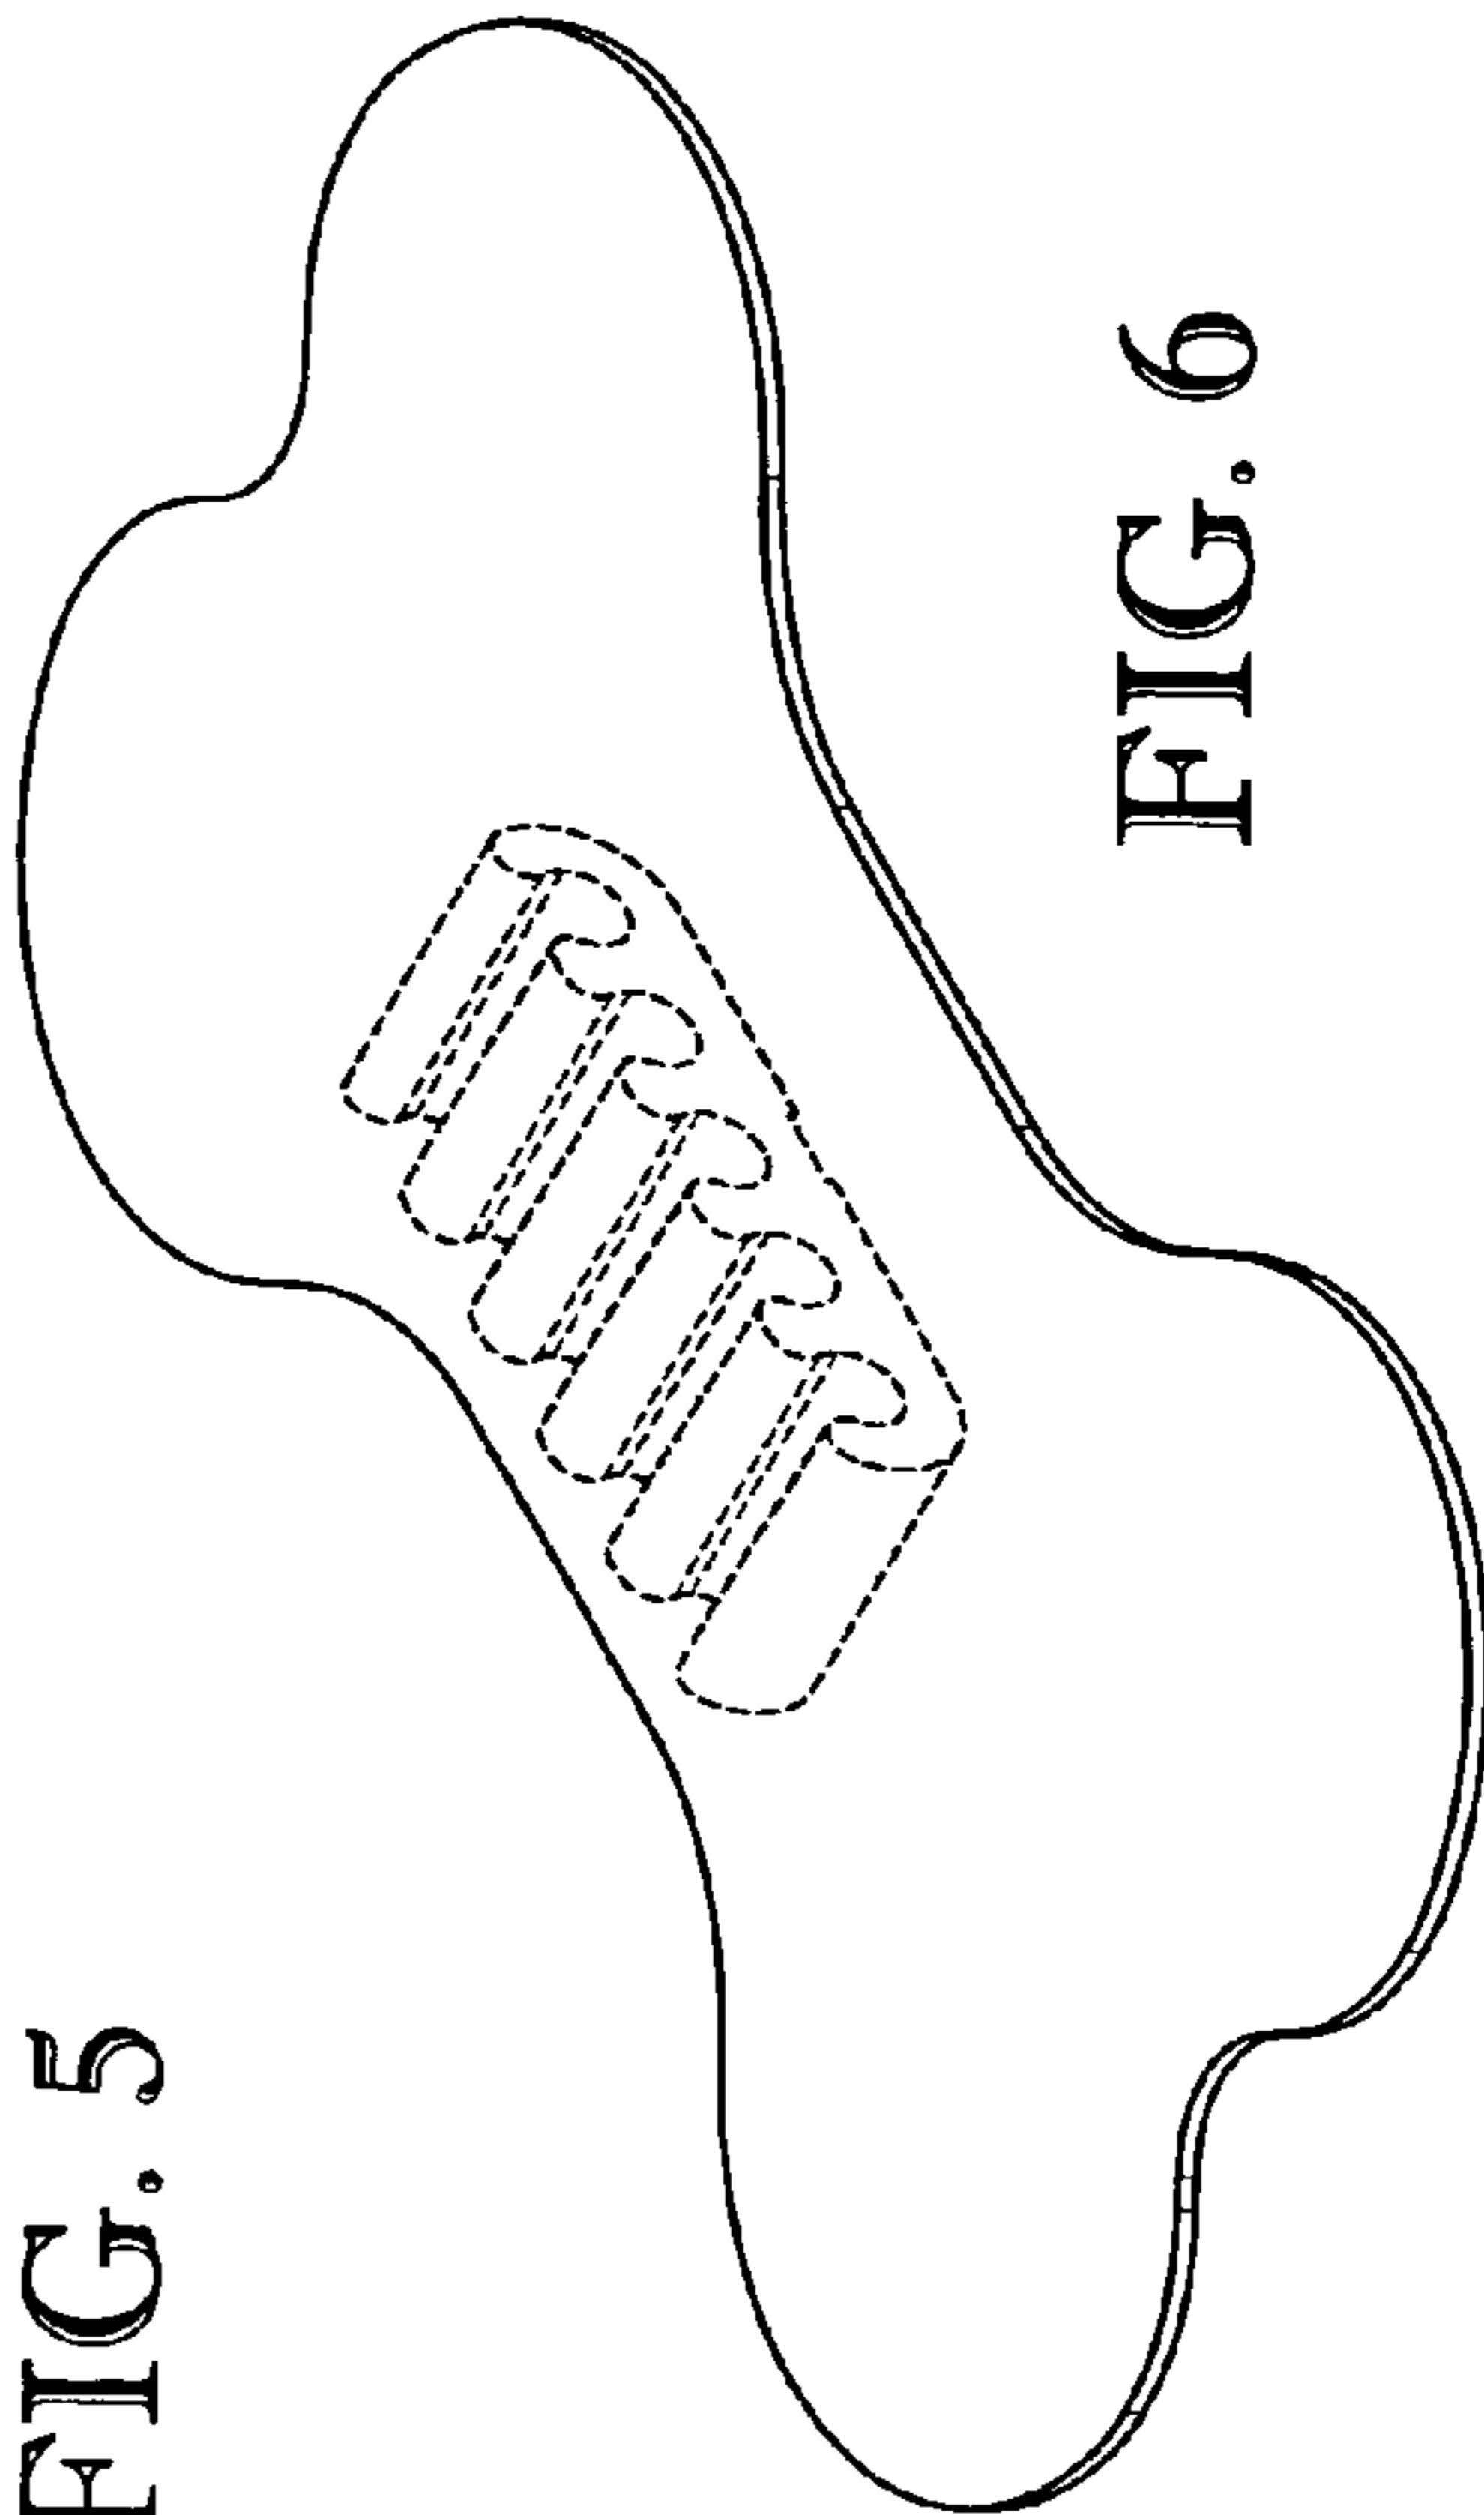


FIG. 6