



US00D549827S

(12) **United States Design Patent**  
**Maeno et al.**

(10) **Patent No.:** **US D549,827 S**

(45) **Date of Patent:** **\*\* Aug. 28, 2007**

(54) **BLOOD ANALYZER**

D496,732 S \* 9/2004 Nagai et al. .... D24/169  
D508,999 S \* 8/2005 Fanning et al. .... D24/216

(75) Inventors: **Akio Maeno**, Kyoto (JP); **Masaharu Matsumoto**, Kyoto (JP); **Yoshito Komada**, Kyoto (JP); **Hyosuke Yonezawa**, Kyoto (JP)

\* cited by examiner

*Primary Examiner*—Louis S. Zarfes

*Assistant Examiner*—Anhdao Doan

(73) Assignee: **Horiba, Ltd.**, Kyoto (JP)

(57) **CLAIM**

(\*\*) Term: **14 Years**

We claim the ornamental design for the blood analyzer, as shown and described.

(21) Appl. No.: **29/255,954**

(22) Filed: **Mar. 14, 2006**

**DESCRIPTION**

(30) **Foreign Application Priority Data**

Sep. 16, 2005 (JP) ..... D2005-026877

FIG. 1 is a front elevational view of the blood analyzer of the present invention;

FIG. 2 is a rear elevational view of the blood analyzer;

FIG. 3 is a top plan view of the blood analyzer;

FIG. 4 is a bottom plan view of the blood analyzer;

FIG. 5 is a right side elevational view of the blood analyzer;

FIG. 6 is a left side elevational view of the blood analyzer;

FIG. 7 is a cross sectional view of the blood analyzer taken along line 7—7 in FIG. 1 thereof;

FIG. 8 is a cross sectional view of the blood analyzer taken along line 8—8 in FIG. 1 thereof;

FIG. 9 is a cross sectional view of the blood analyzer taken along line 9—9 in FIG. 5 thereof;

FIG. 10 is a cross sectional view of the blood analyzer taken along line 10—10 in FIG. 5 thereof; and,

FIG. 11 is a top, front and right perspective view thereof.

(51) **LOC (8) Cl.** ..... **24-01**

(52) **U.S. Cl.** ..... **D24/169**

(58) **Field of Classification Search** ..... D24/169,  
D24/186, 232; D10/81; 600/301, 316, 322,  
600/324, 347, 365, 366, 368; 422/55, 61,  
422/68.1; 436/66—68


See application file for complete search history.

(56) **References Cited**

**U.S. PATENT DOCUMENTS**

- D339,639 S \* 9/1993 Ohnuma et al. .... D24/232
- D381,749 S \* 7/1997 Lawrence et al. .... D24/169
- D399,959 S \* 10/1998 Prokop et al. .... D24/169
- D402,369 S \* 12/1998 Prokop et al. .... D24/169
- D424,956 S \* 5/2000 von Buelow et al. .... D10/81
- D467,349 S \* 12/2002 Niedbala et al. .... D24/232
- D482,796 S \* 11/2003 Oyama et al. .... D24/232

**1 Claim, 11 Drawing Sheets**

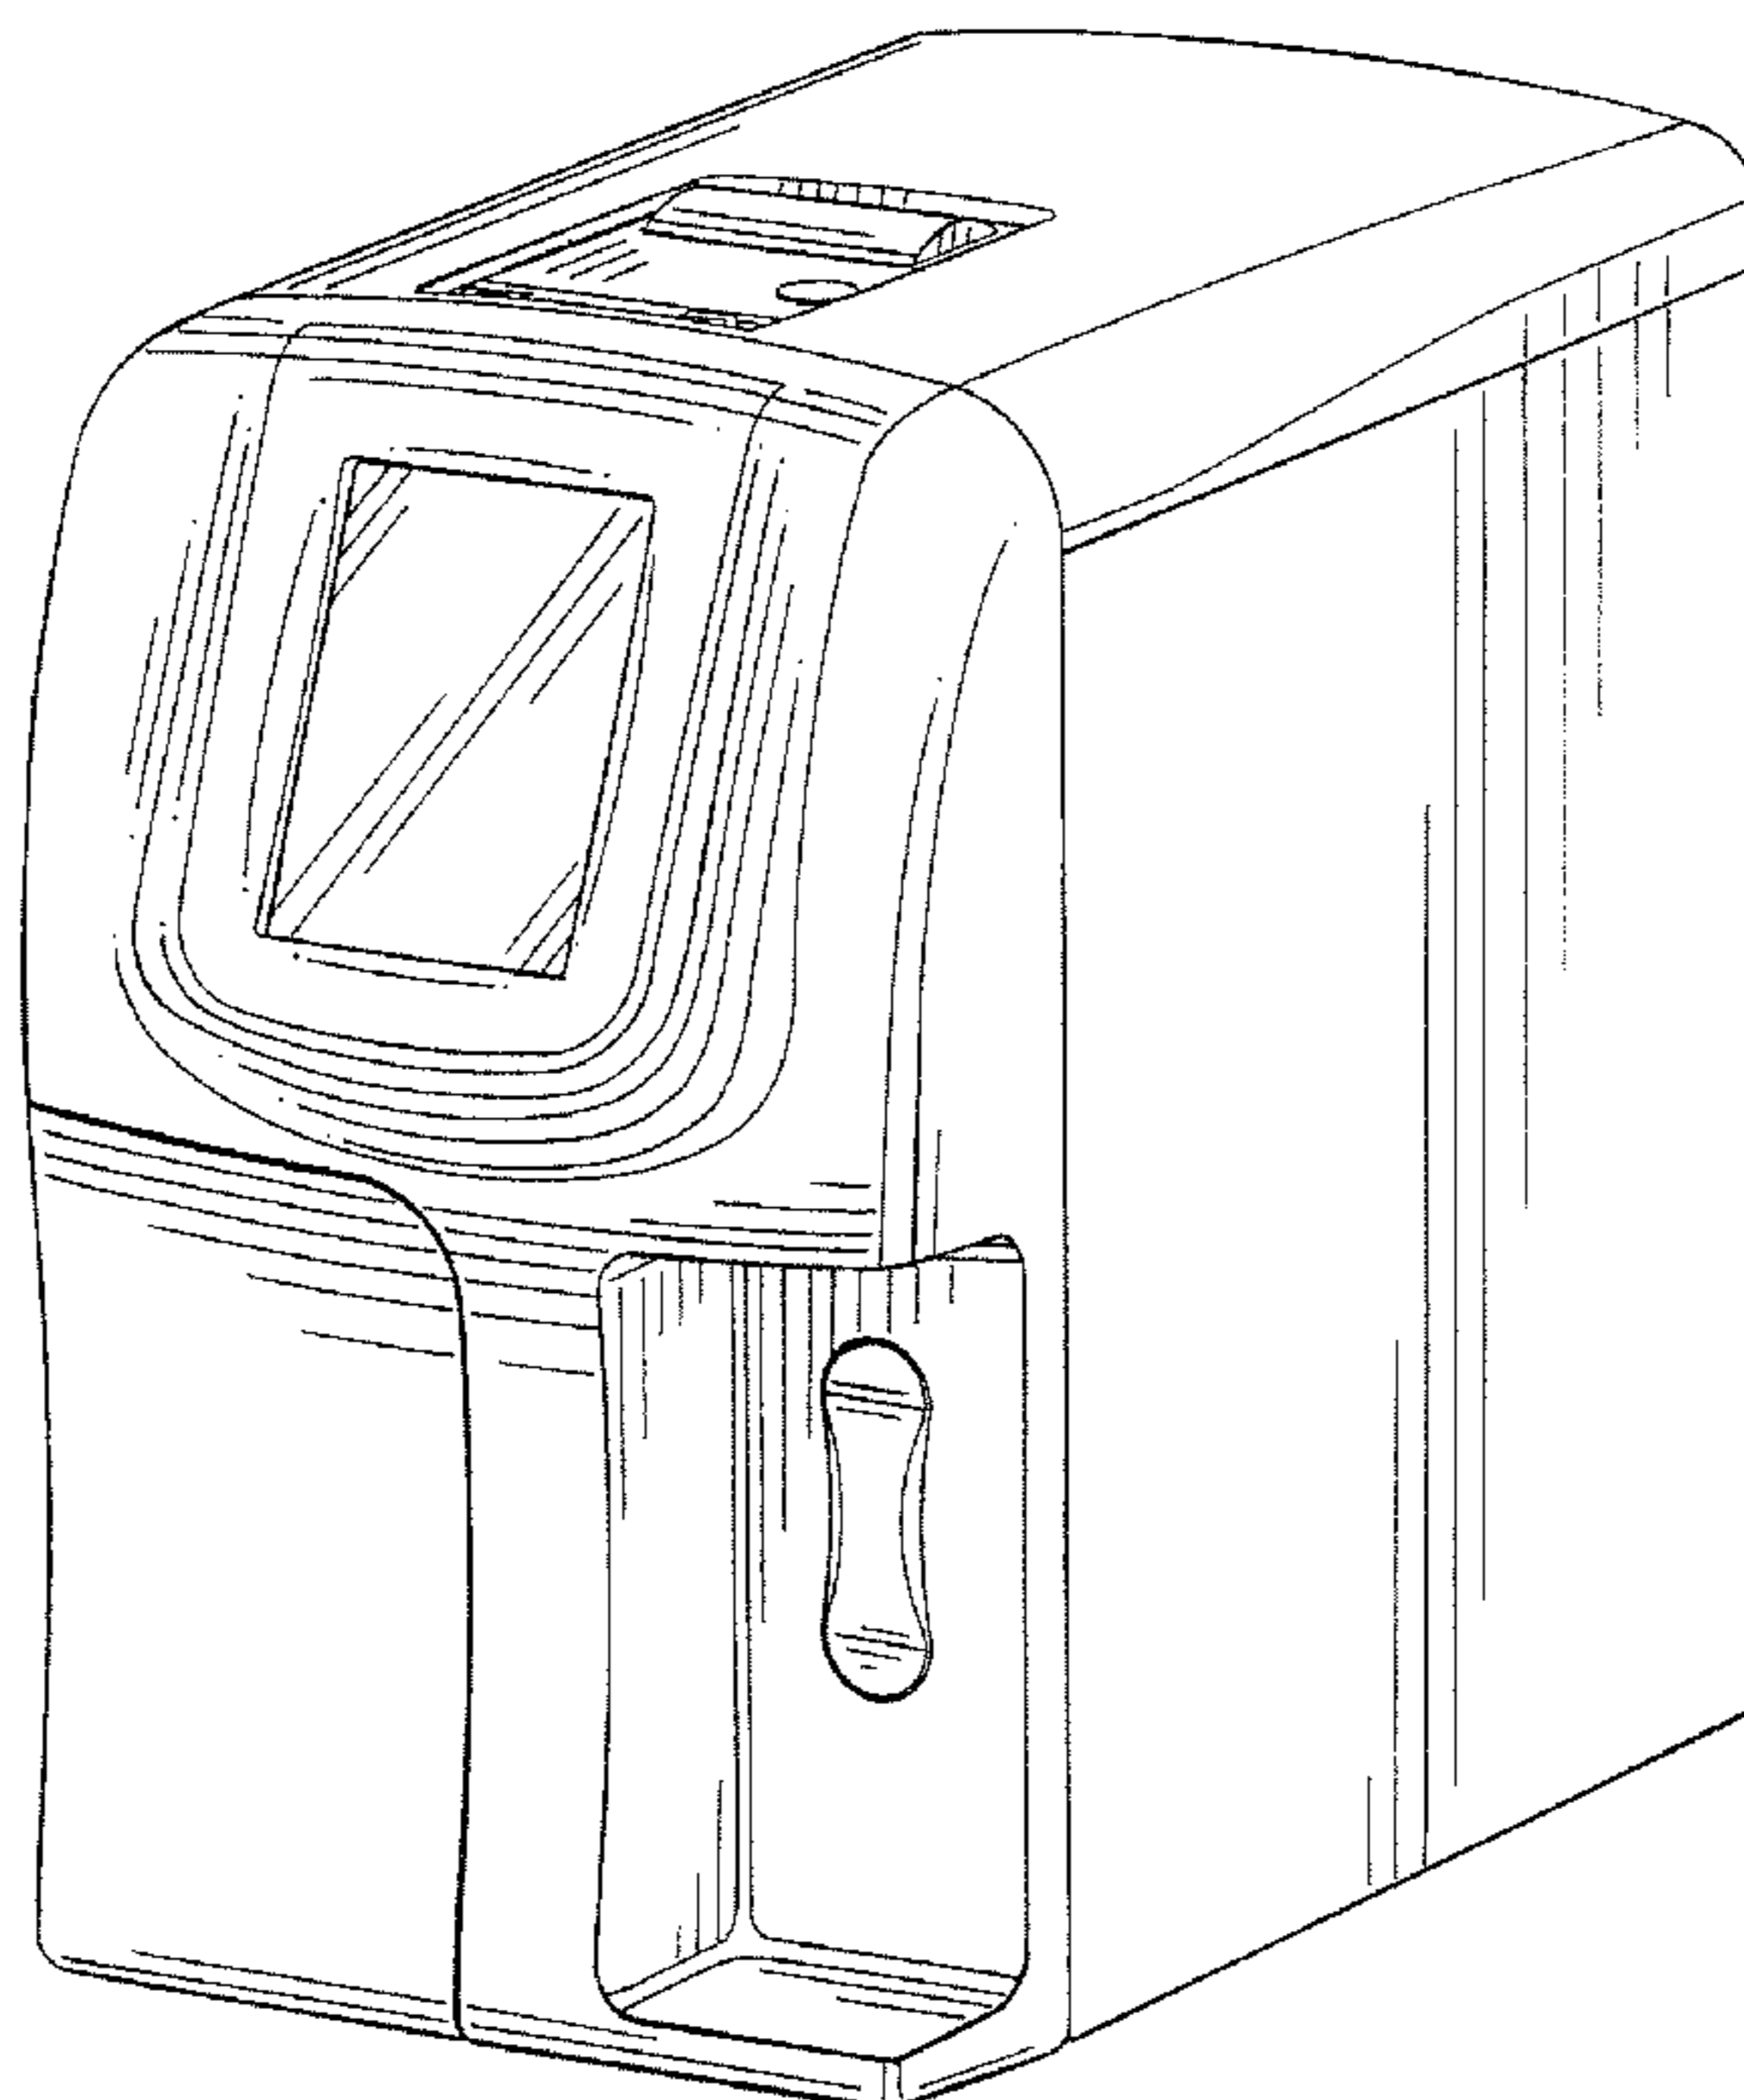



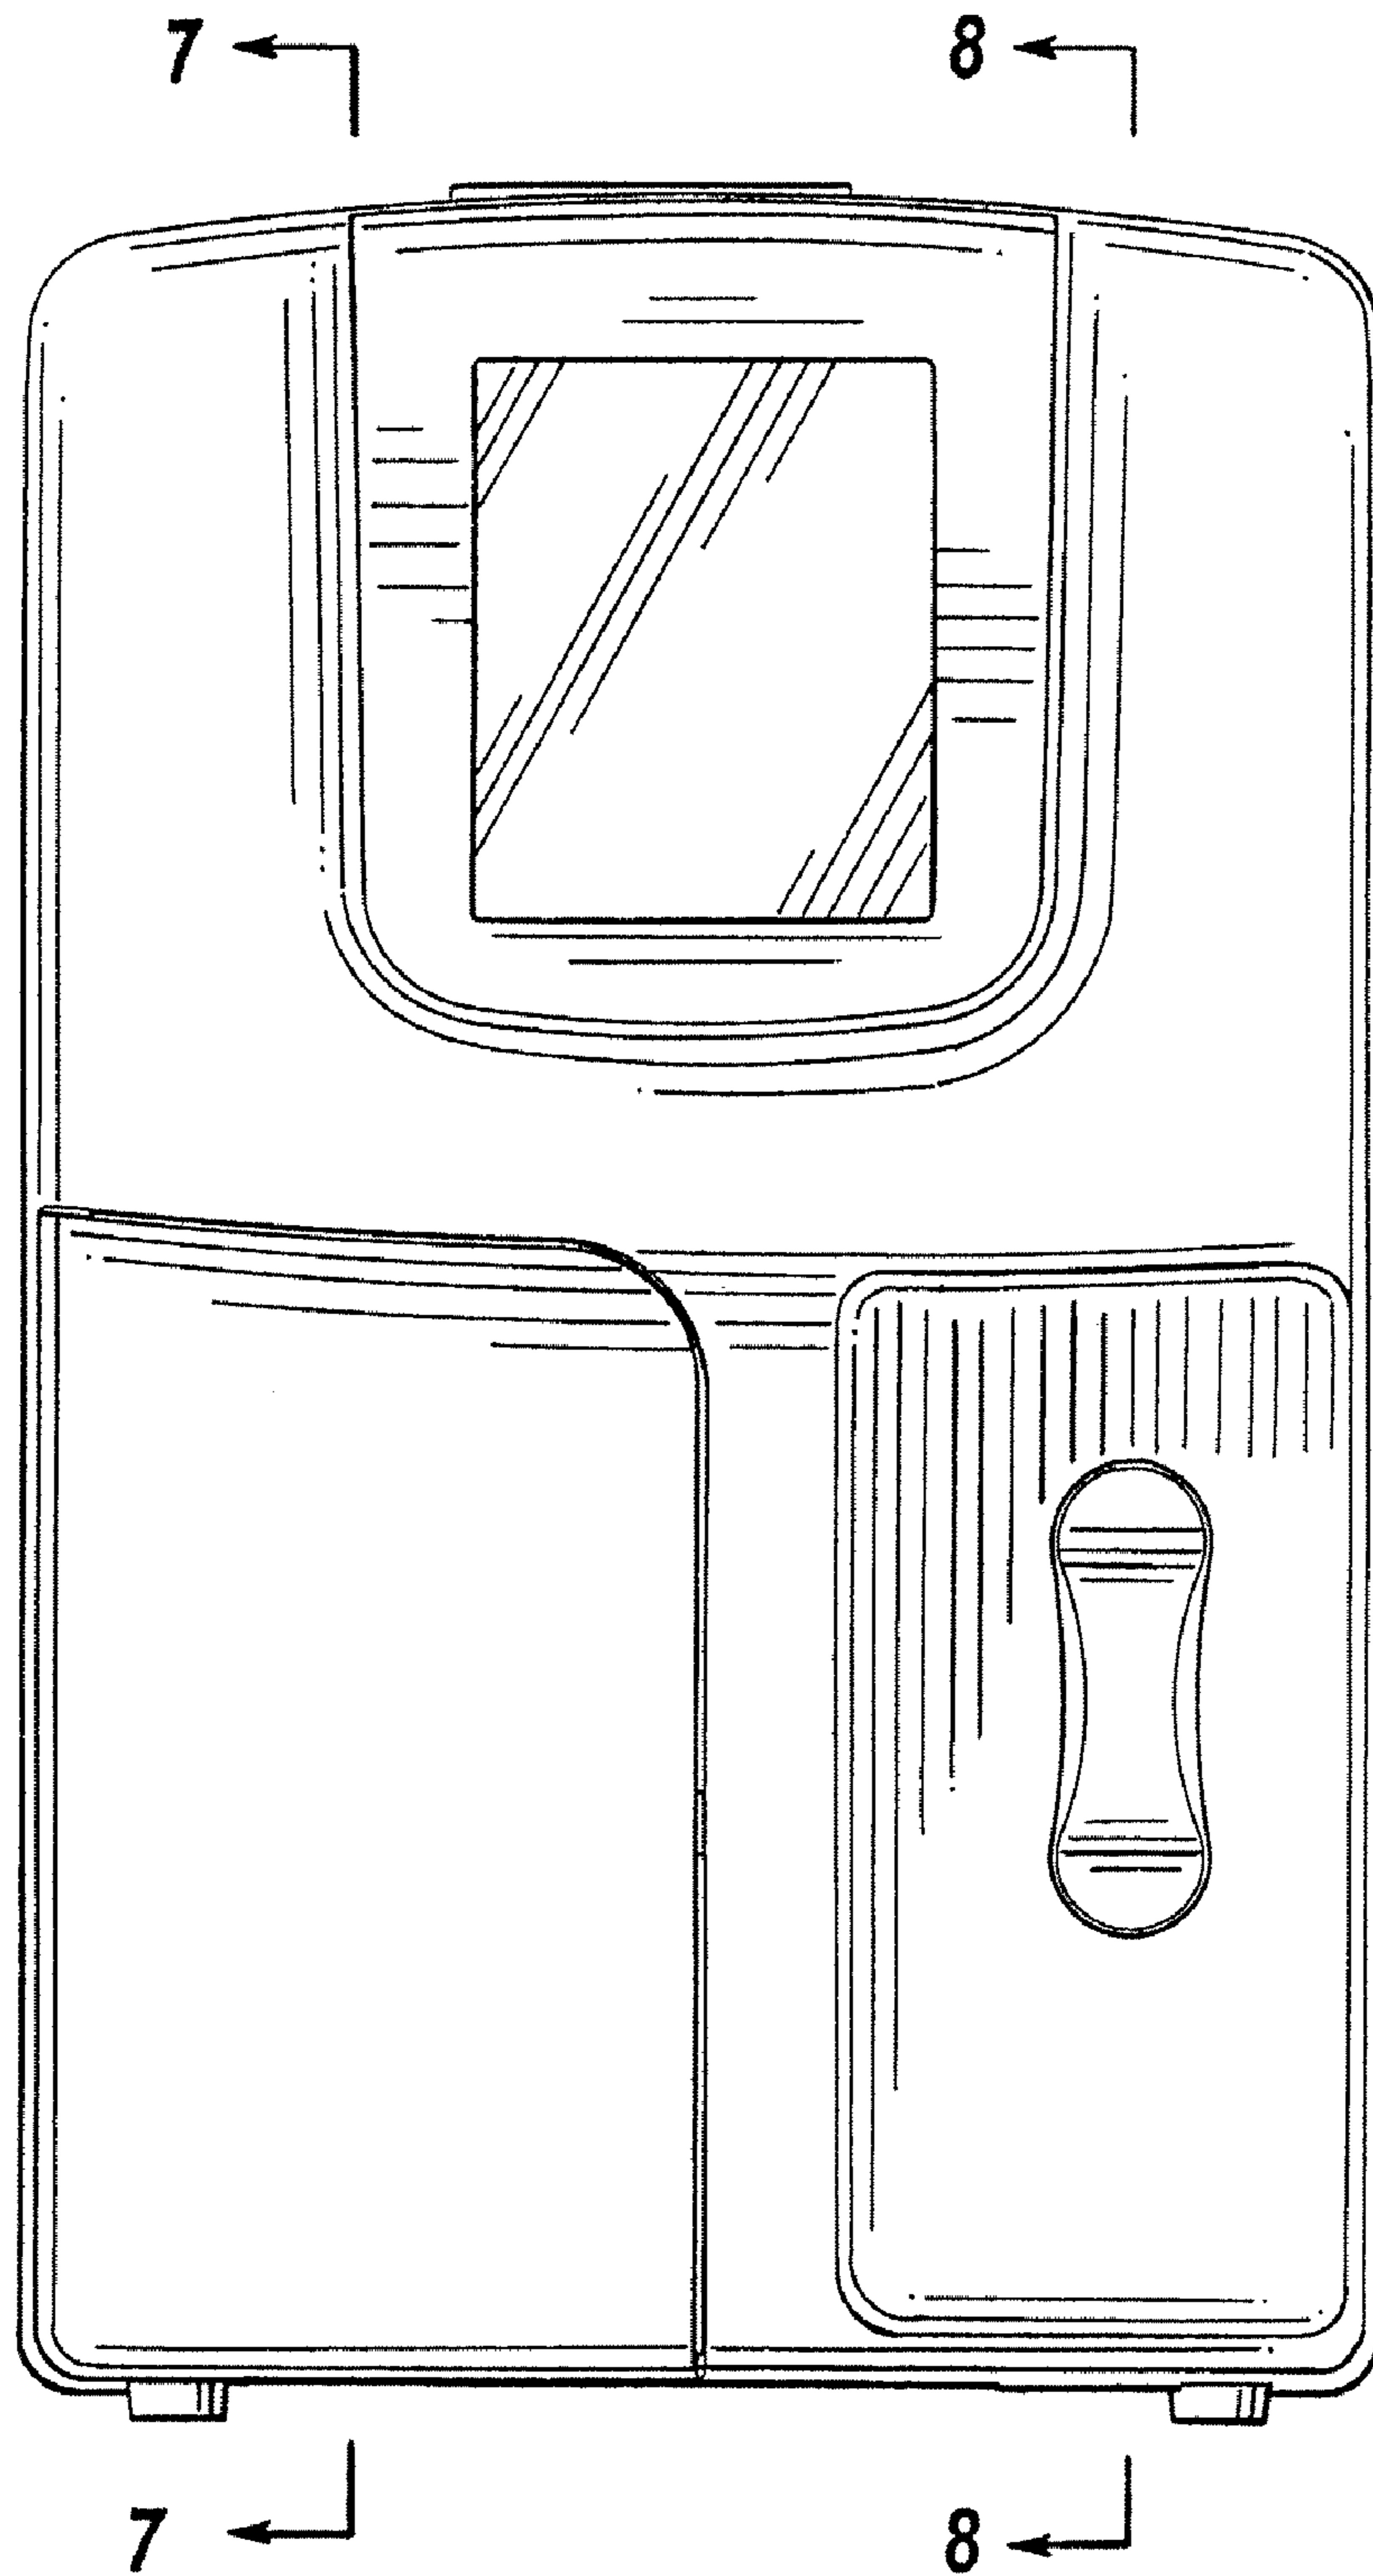



FIG. 1

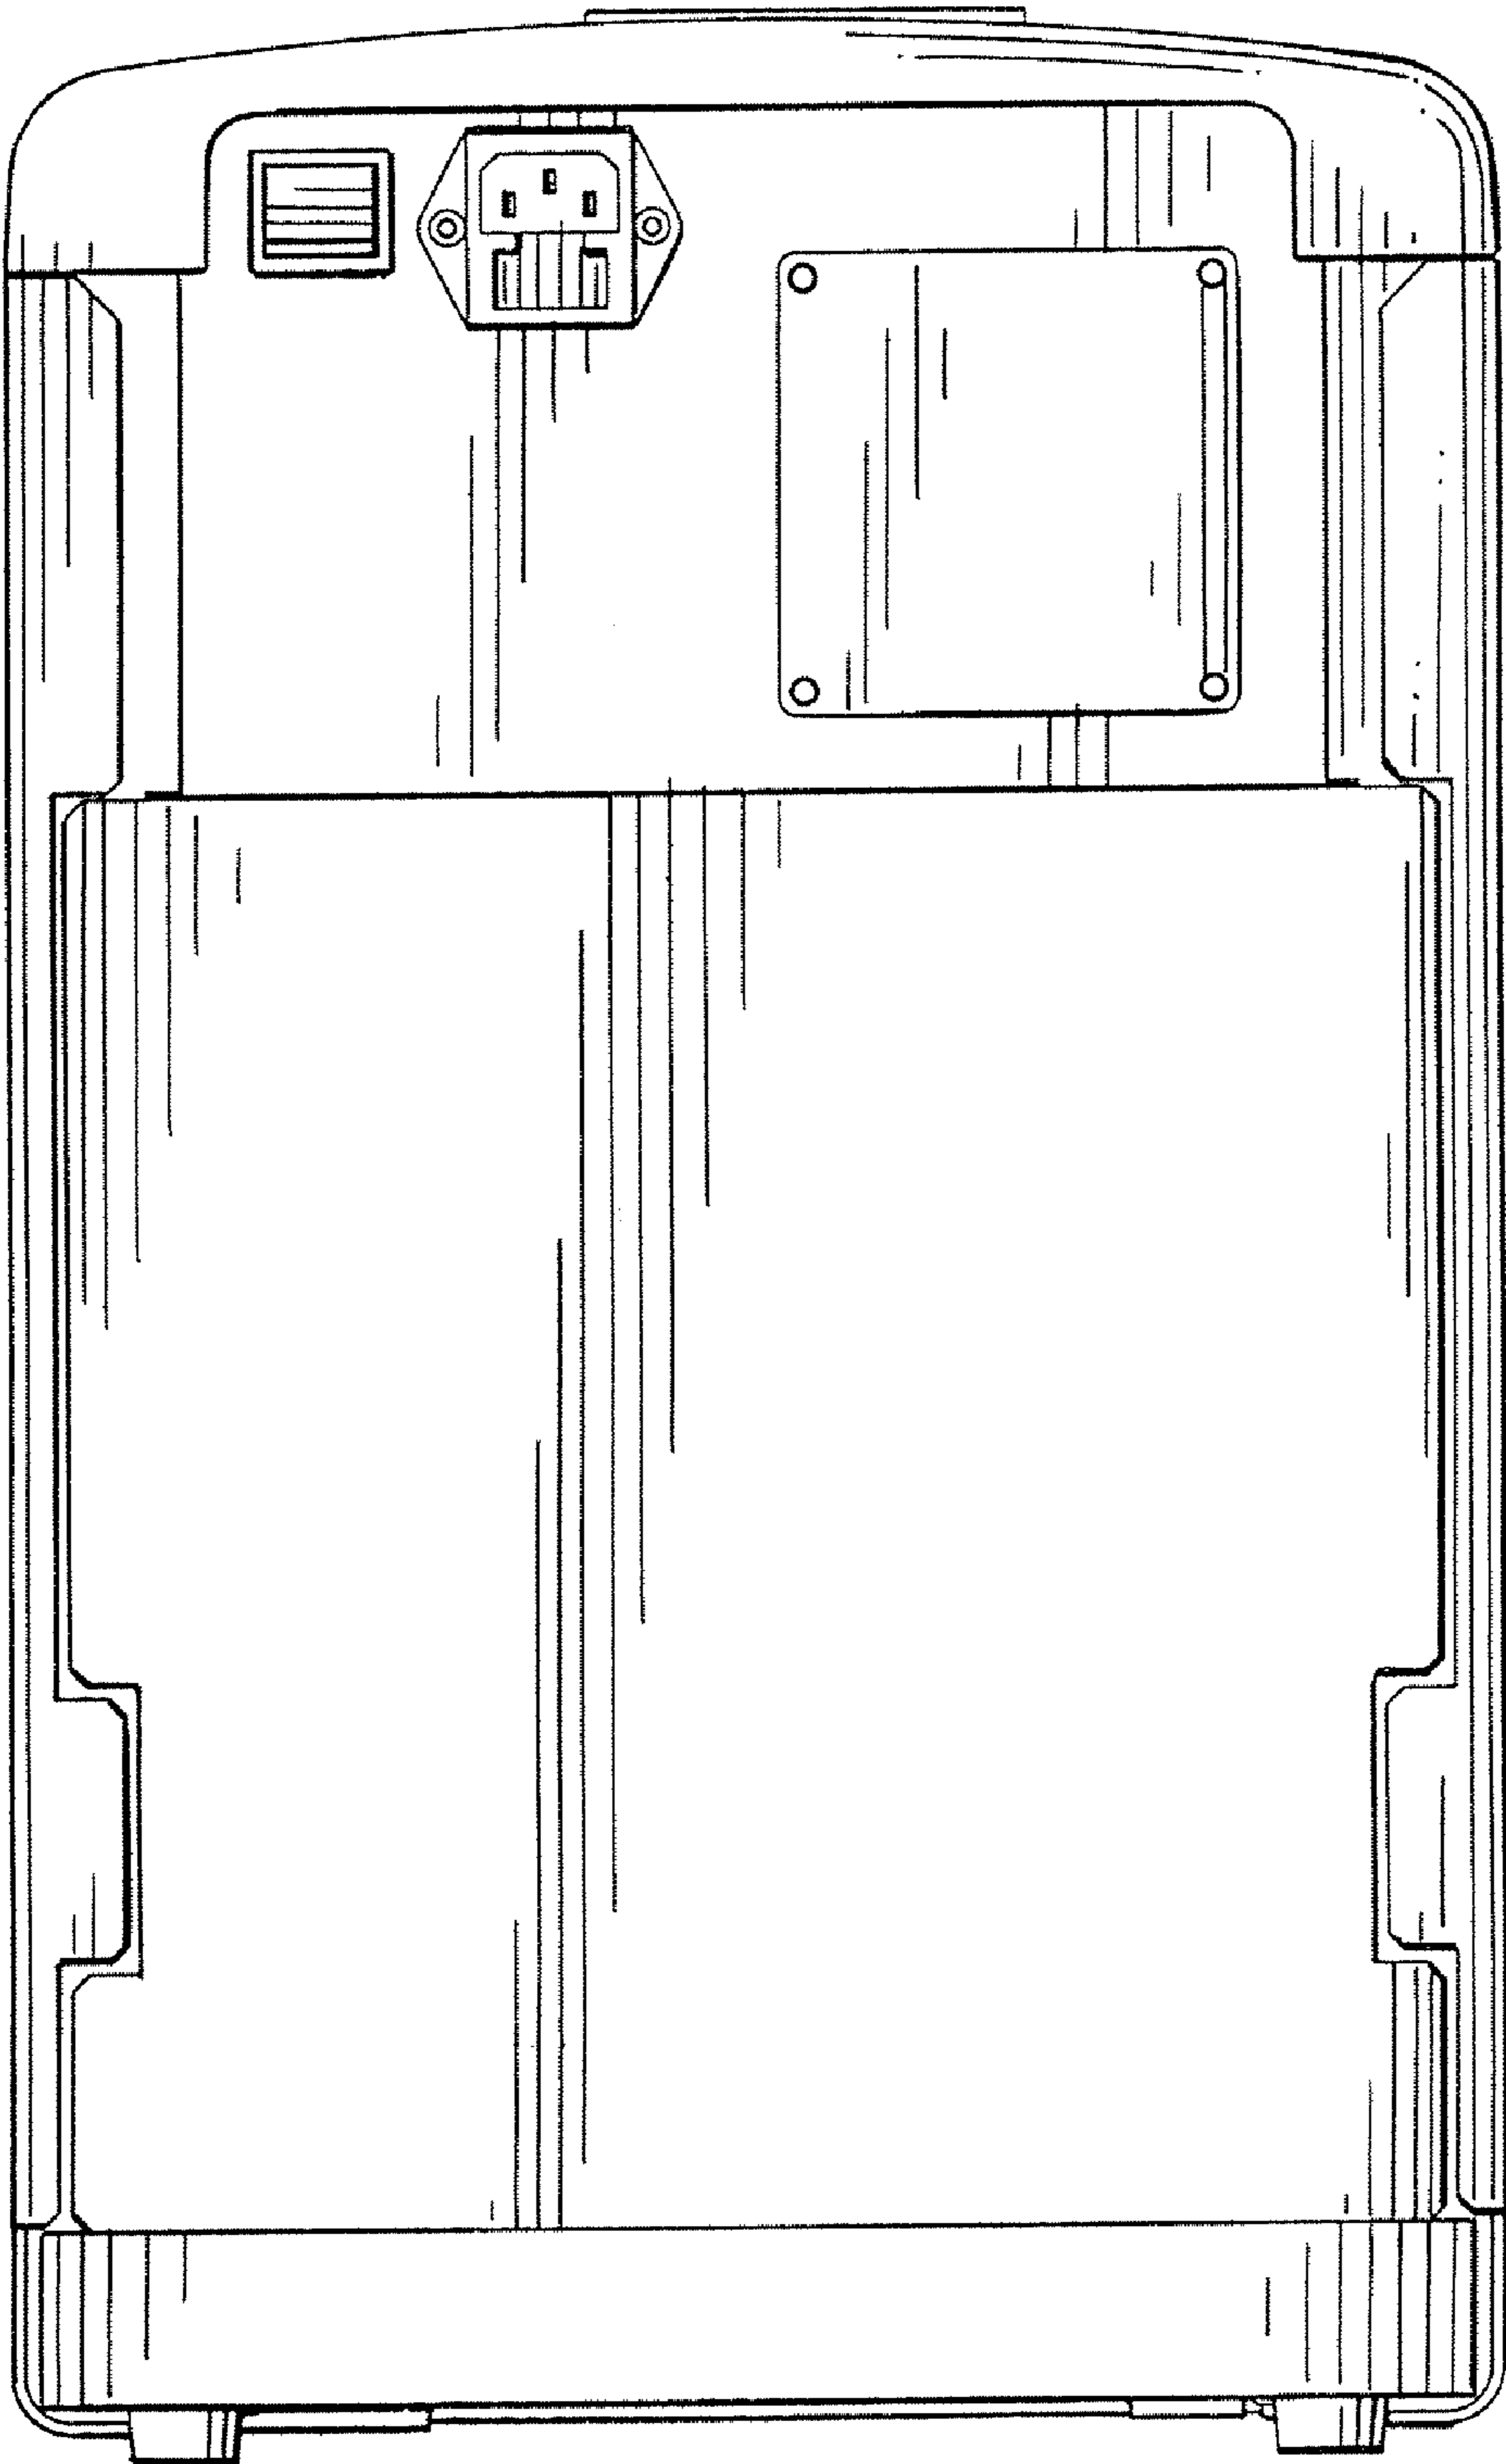

*FIG. 2*

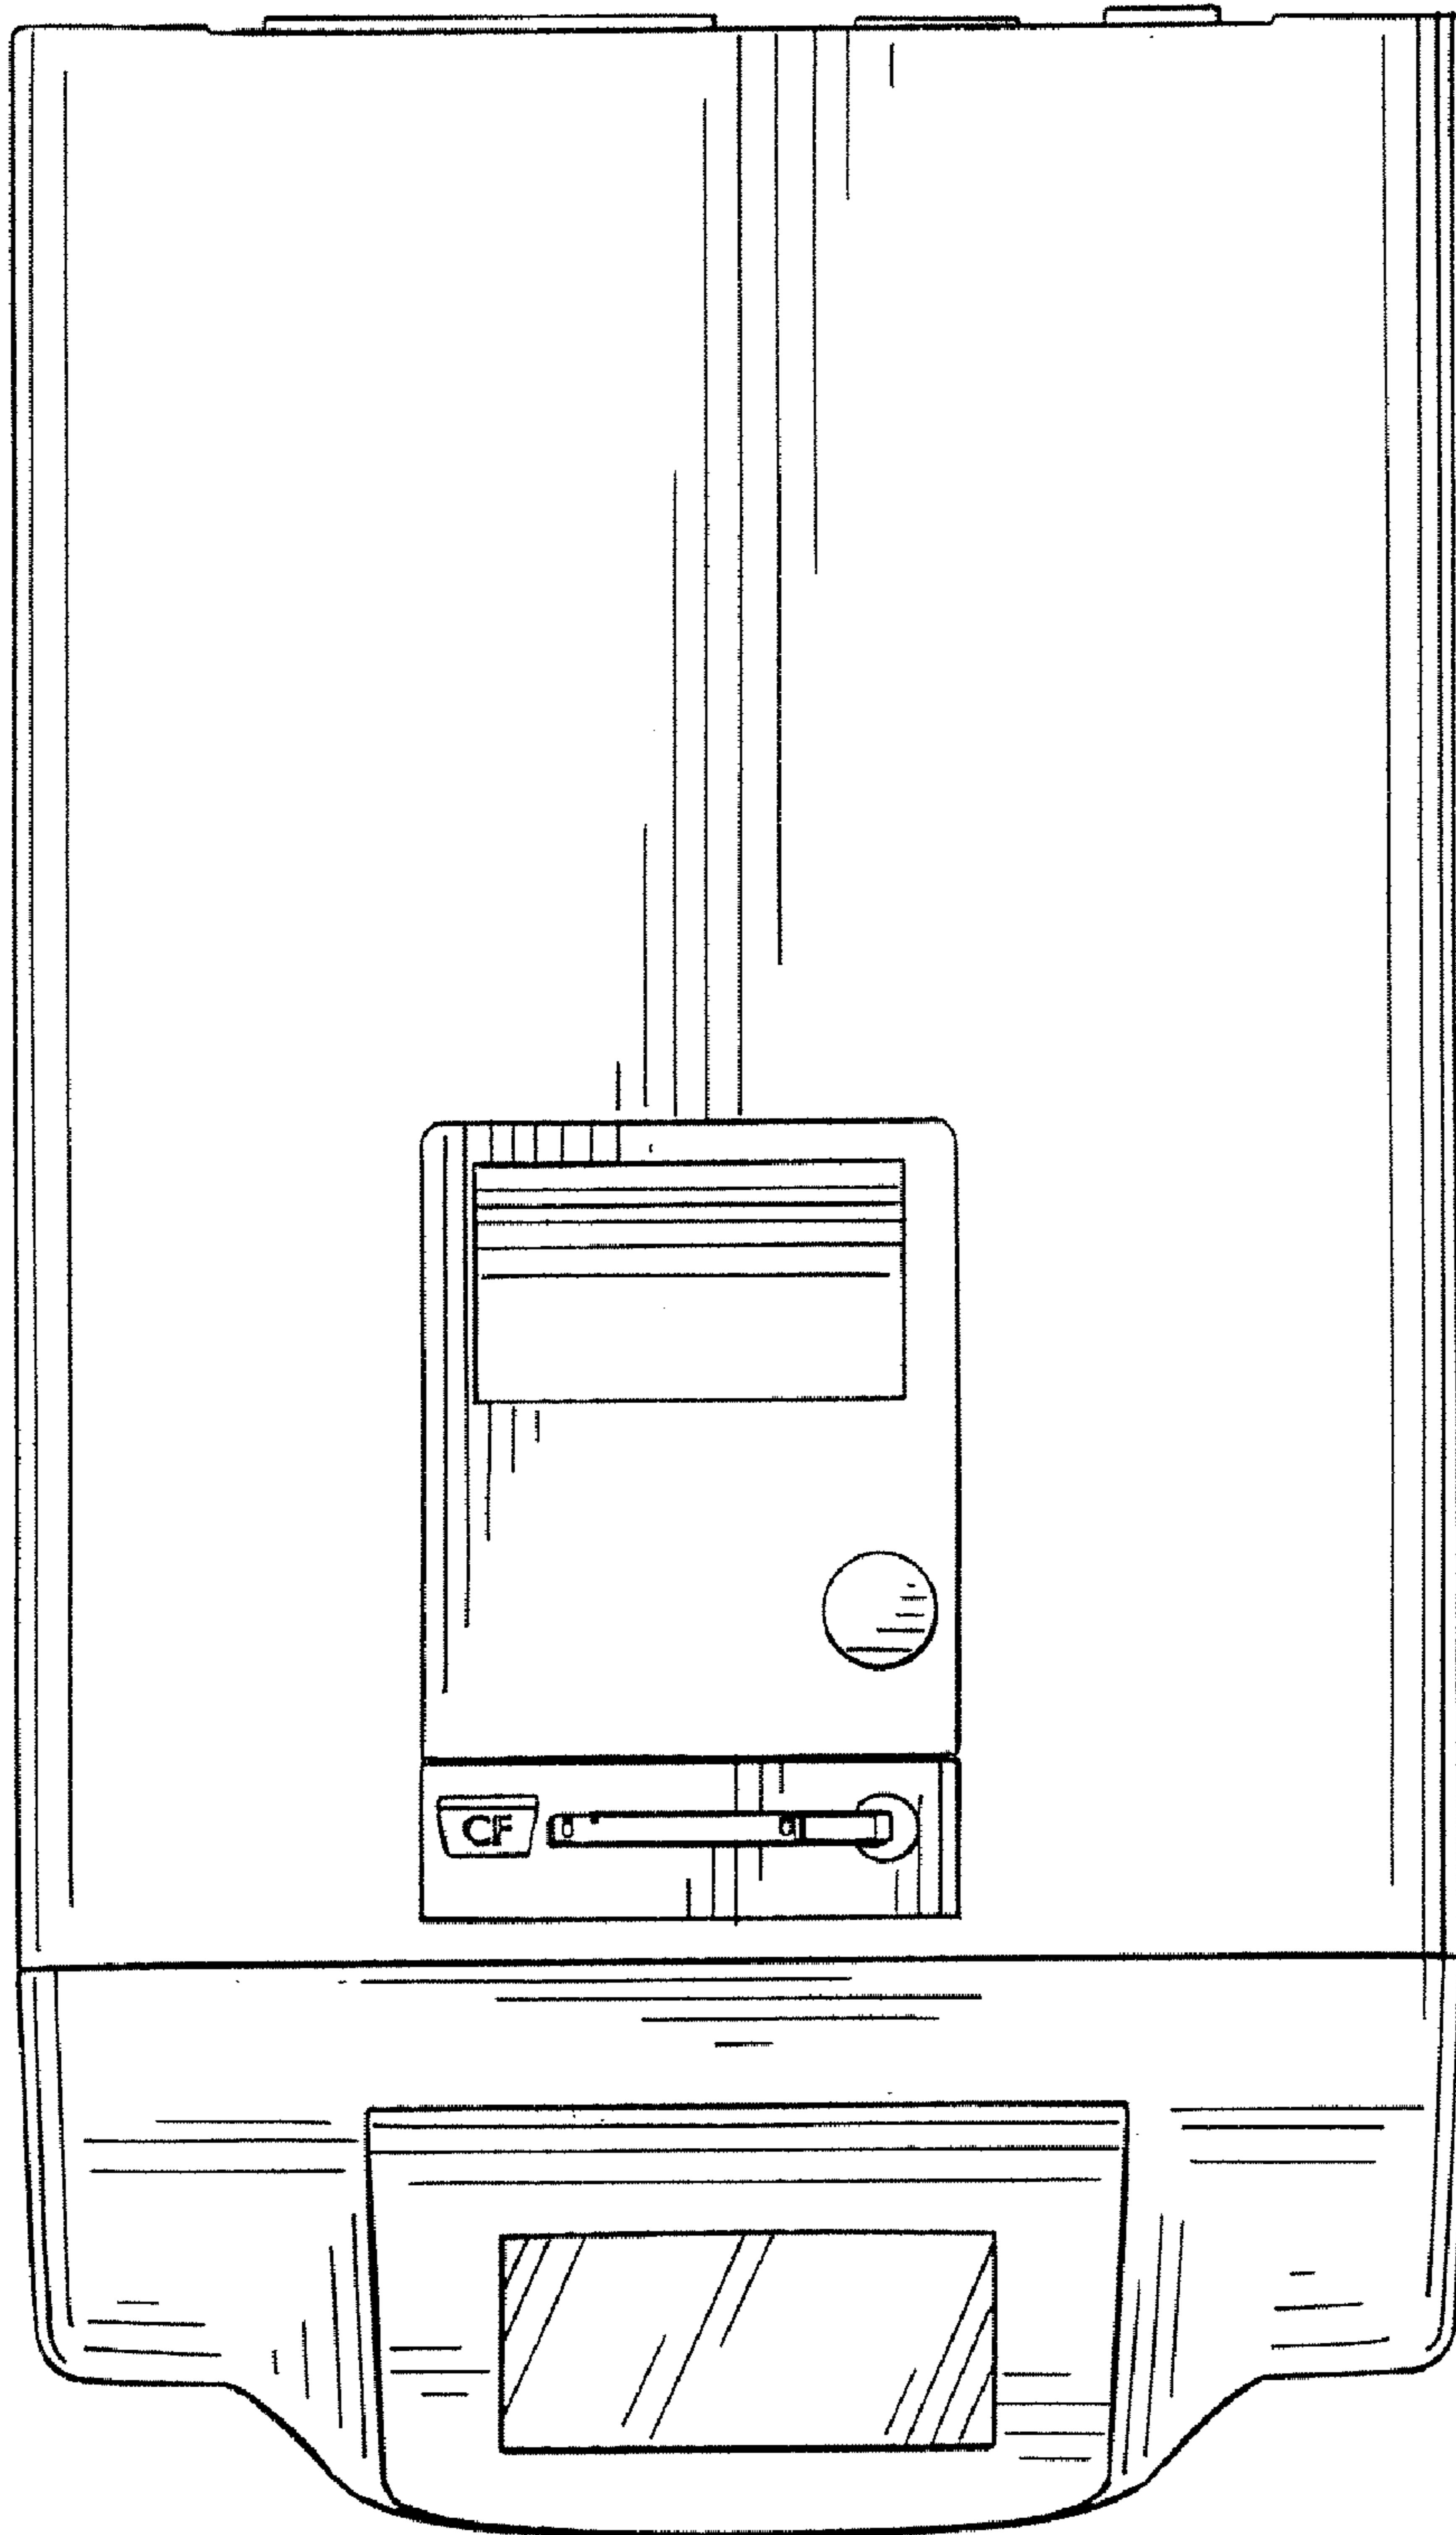

*FIG. 3*

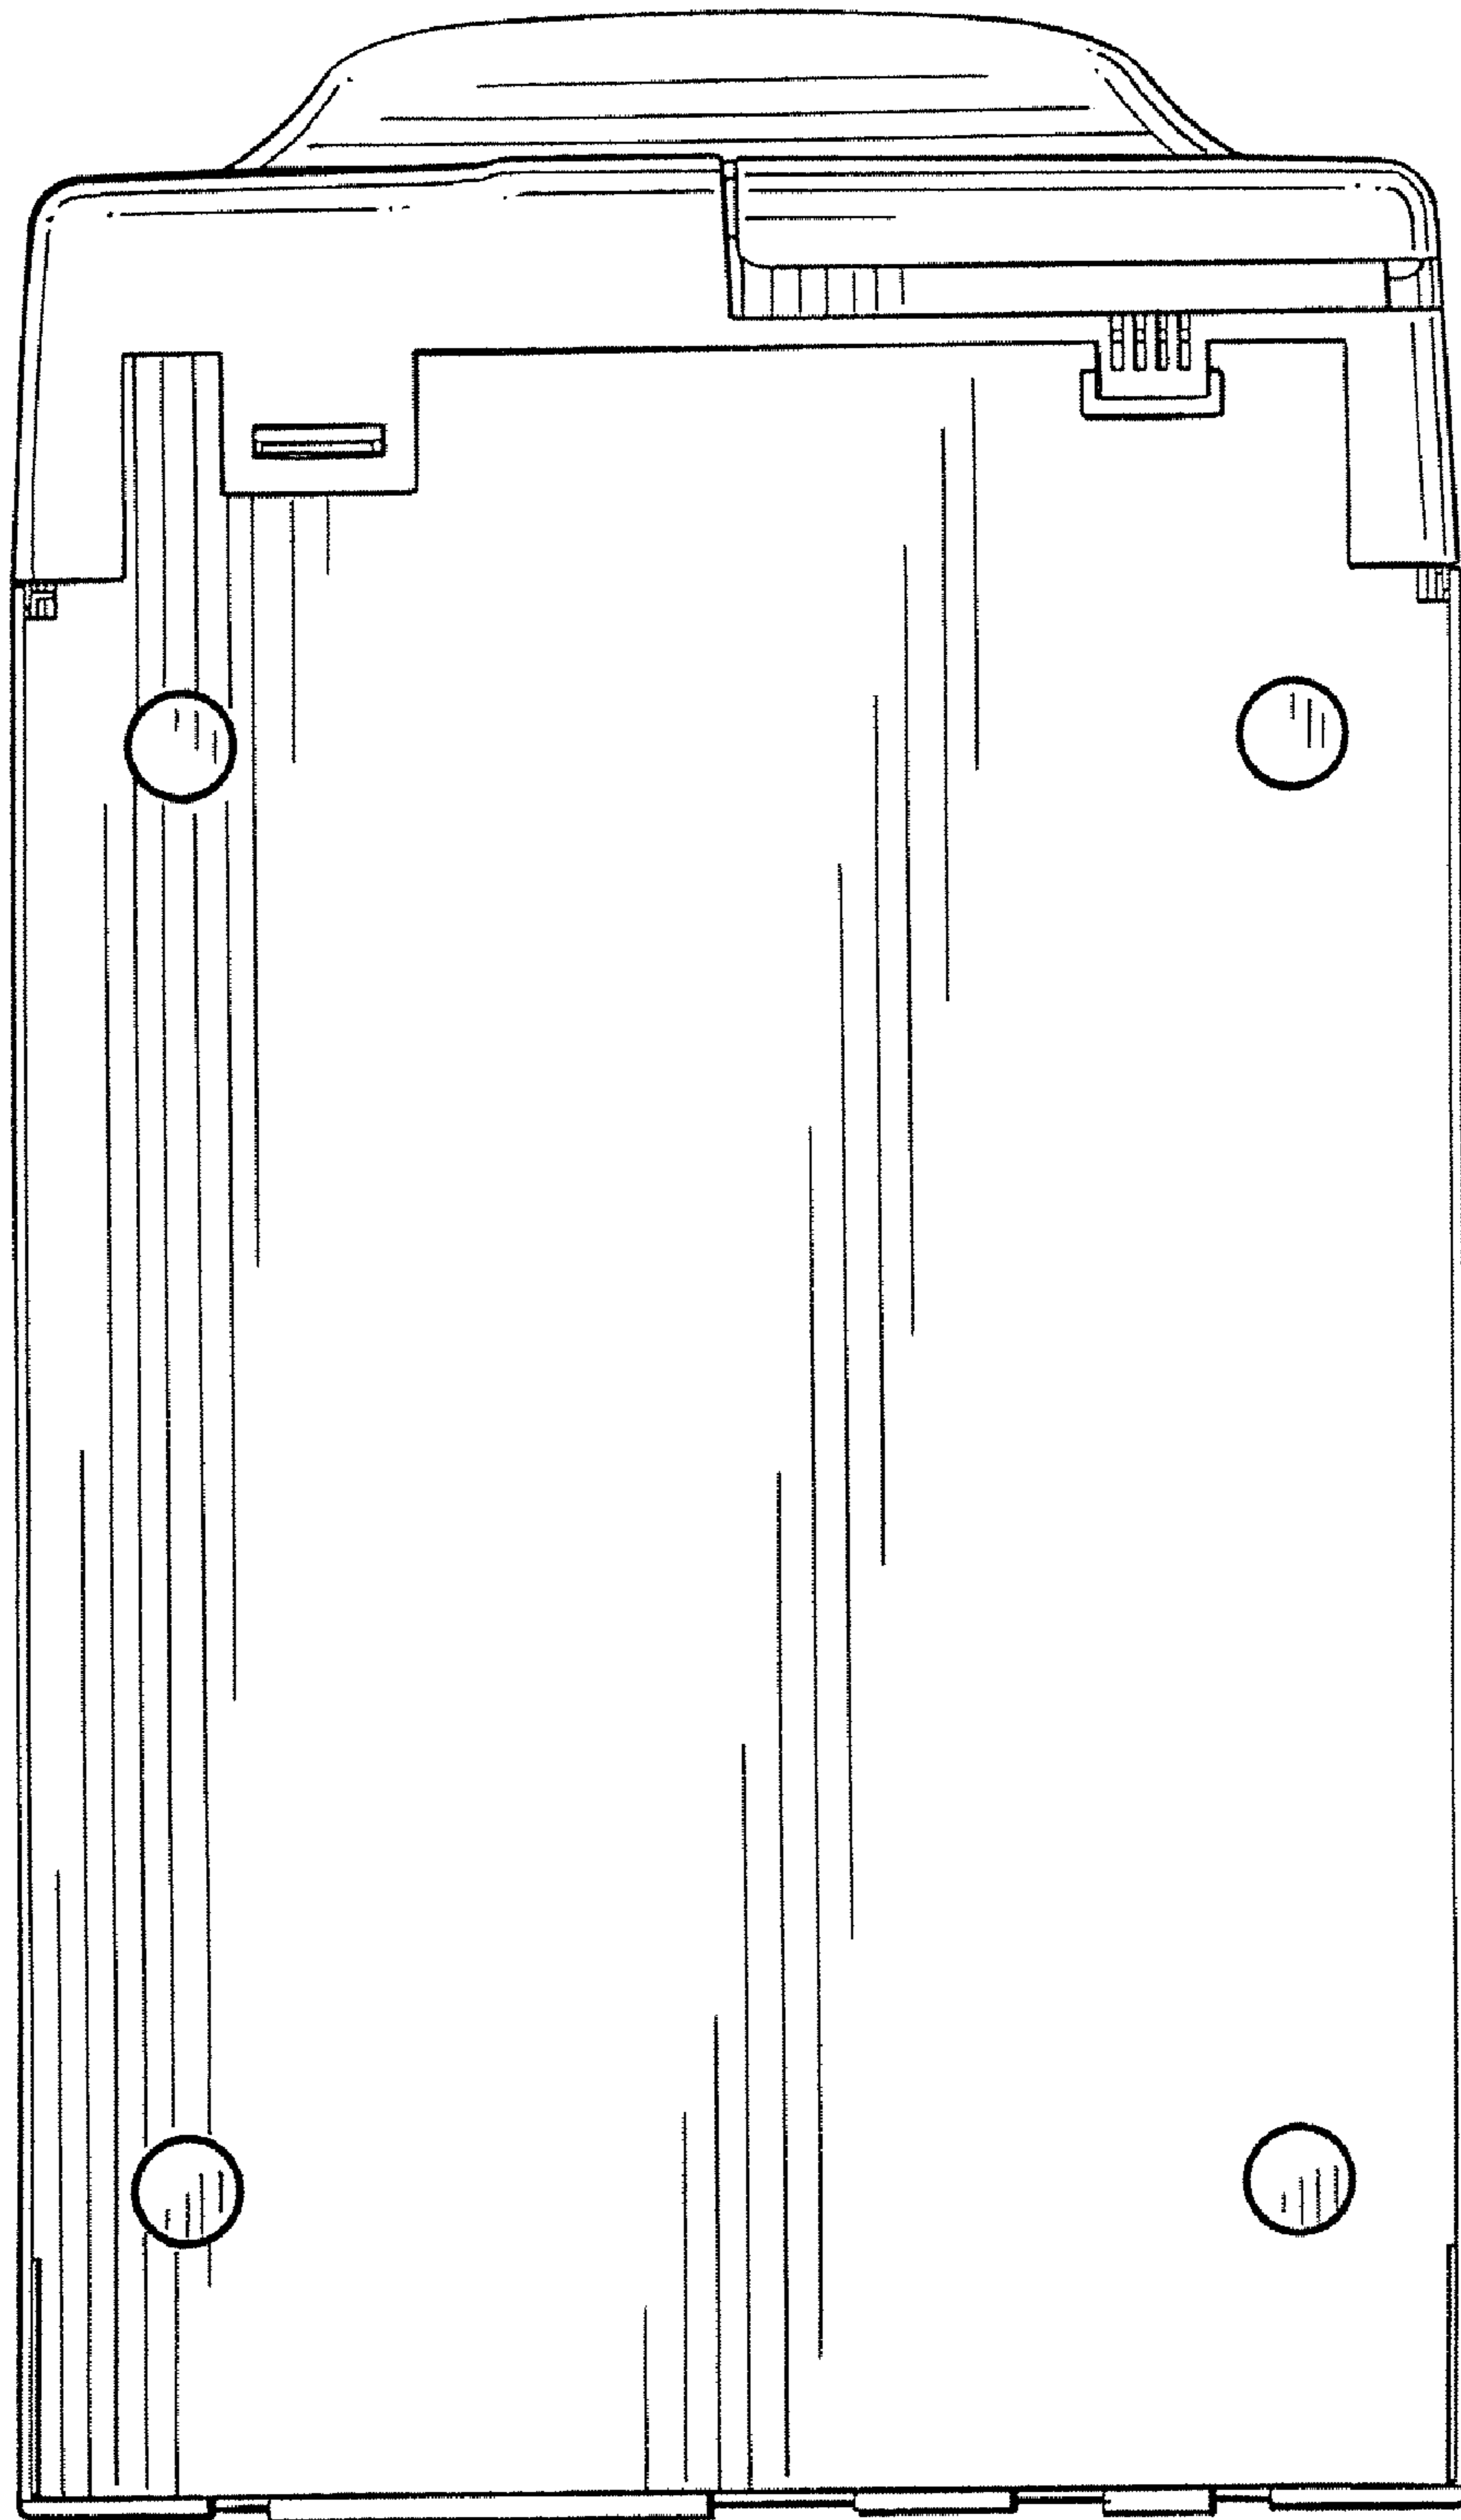

*FIG. 4*


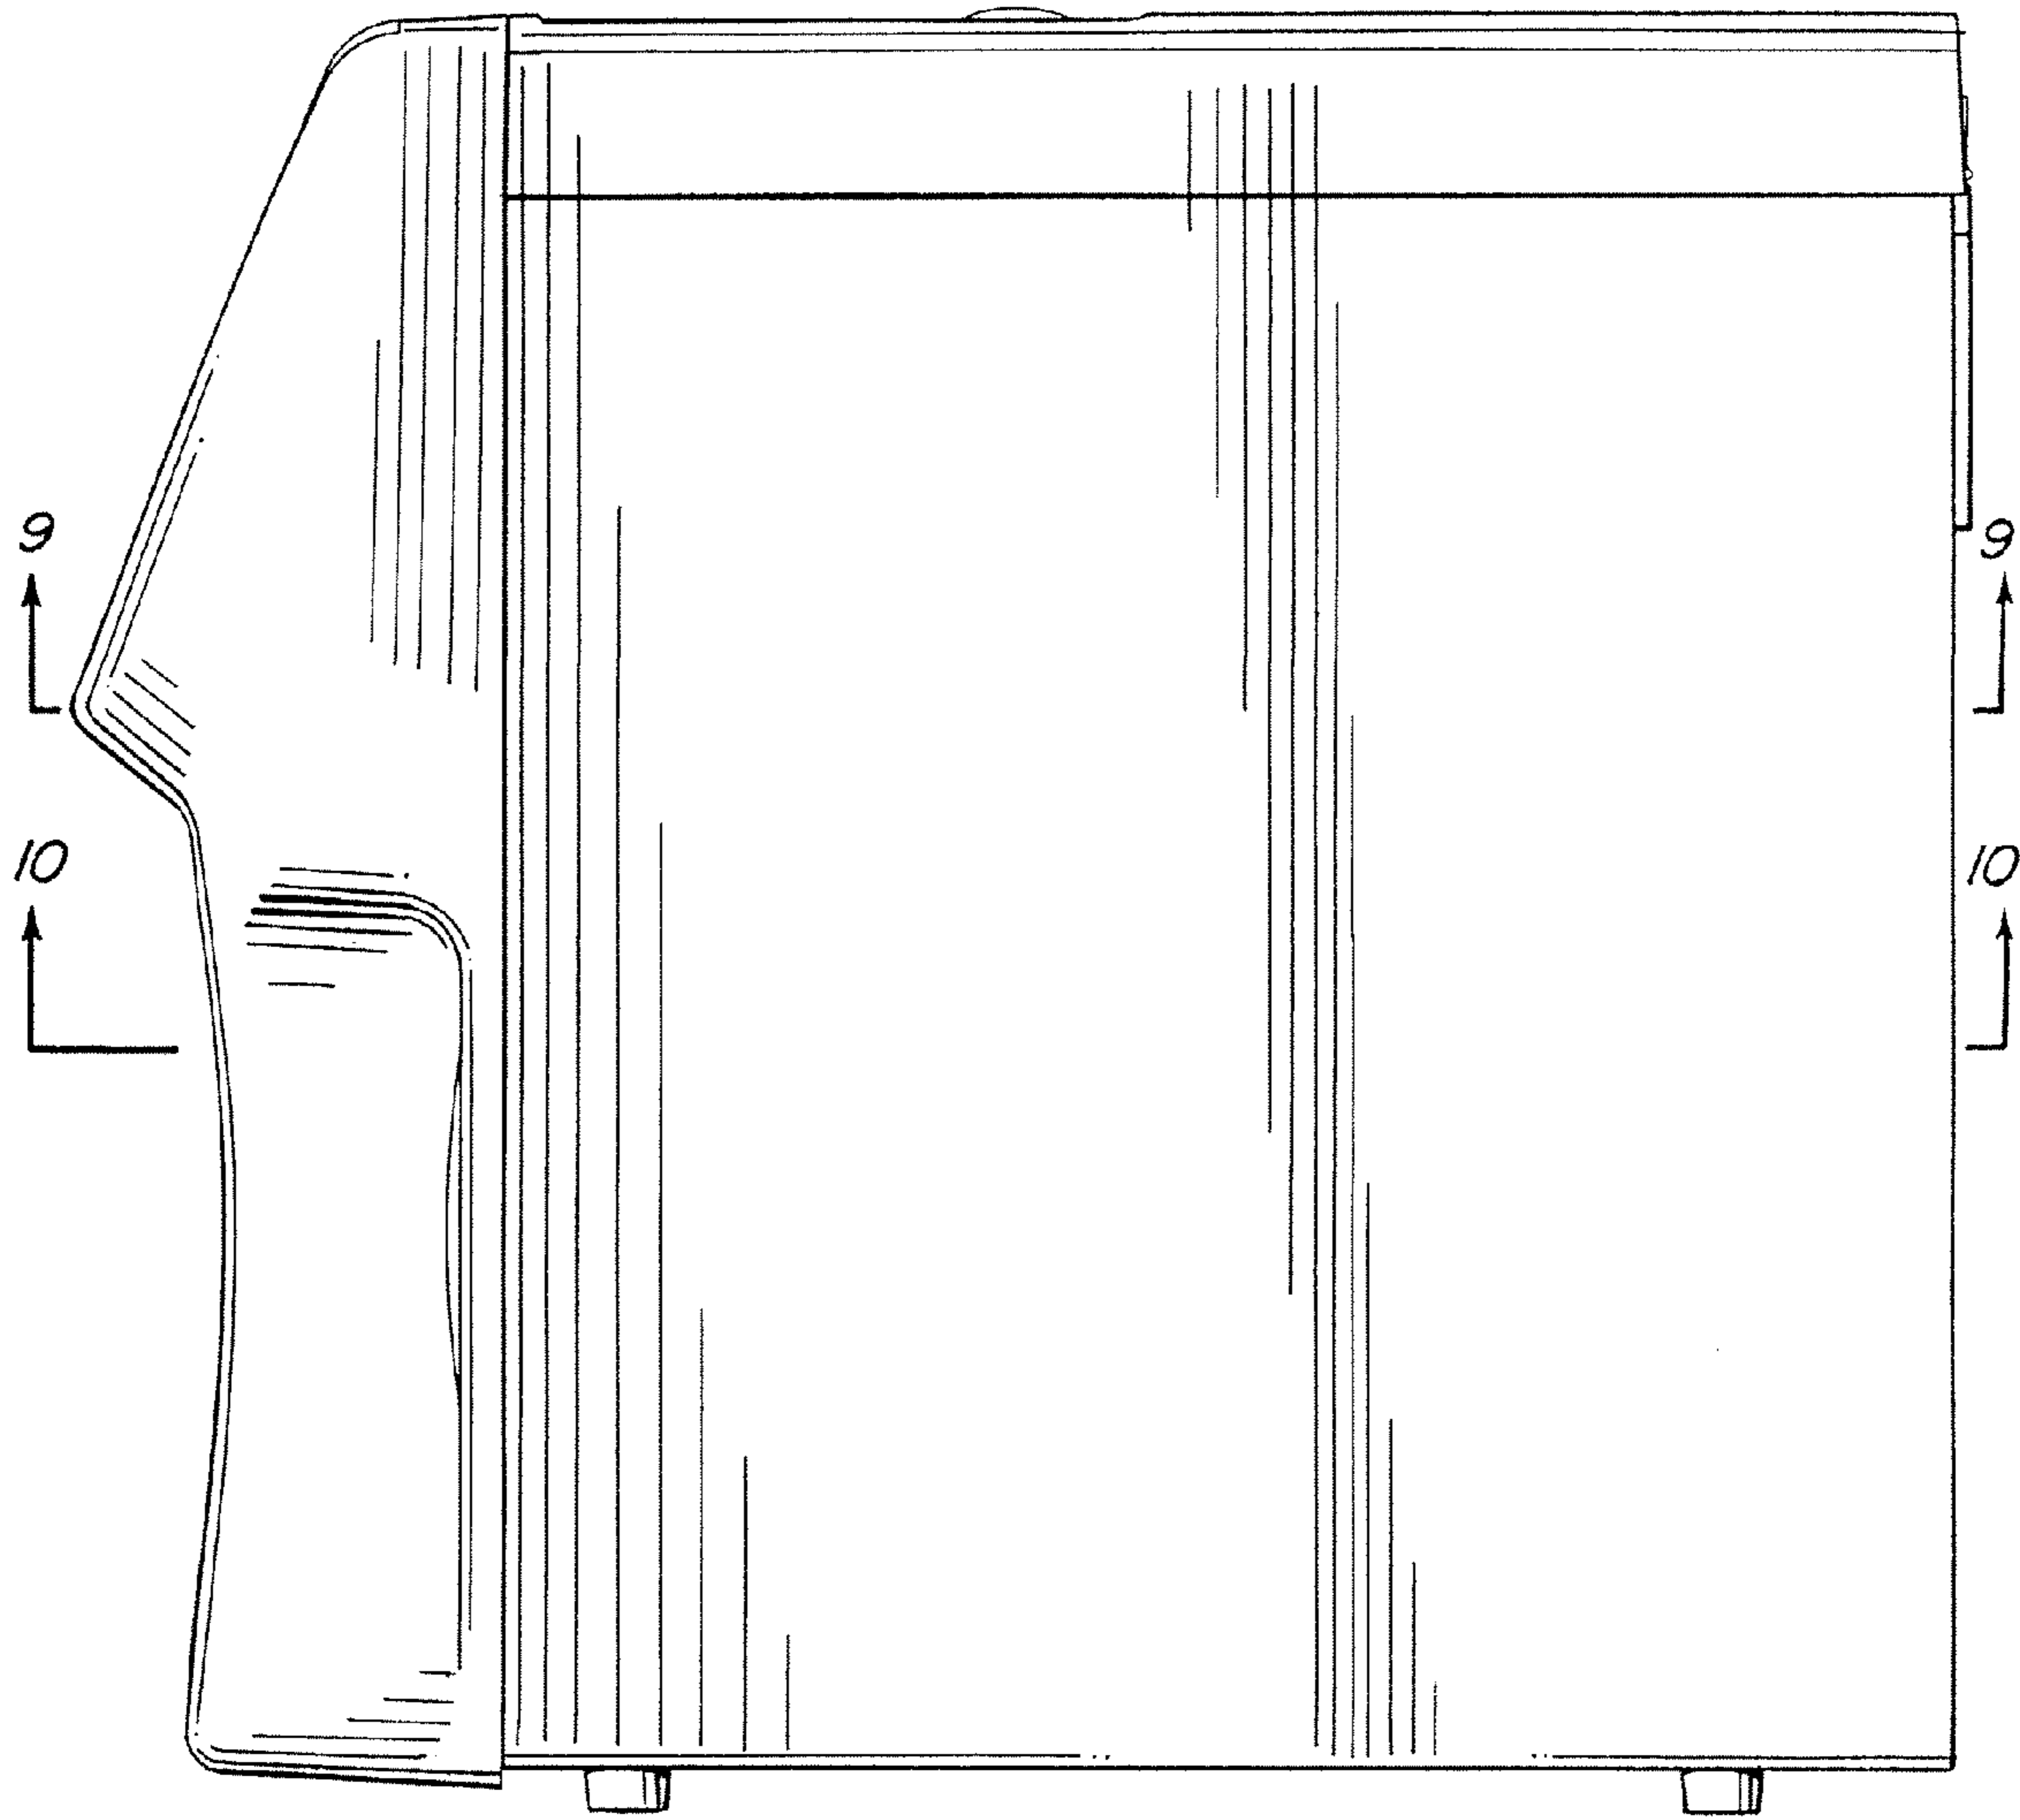


FIG. 5

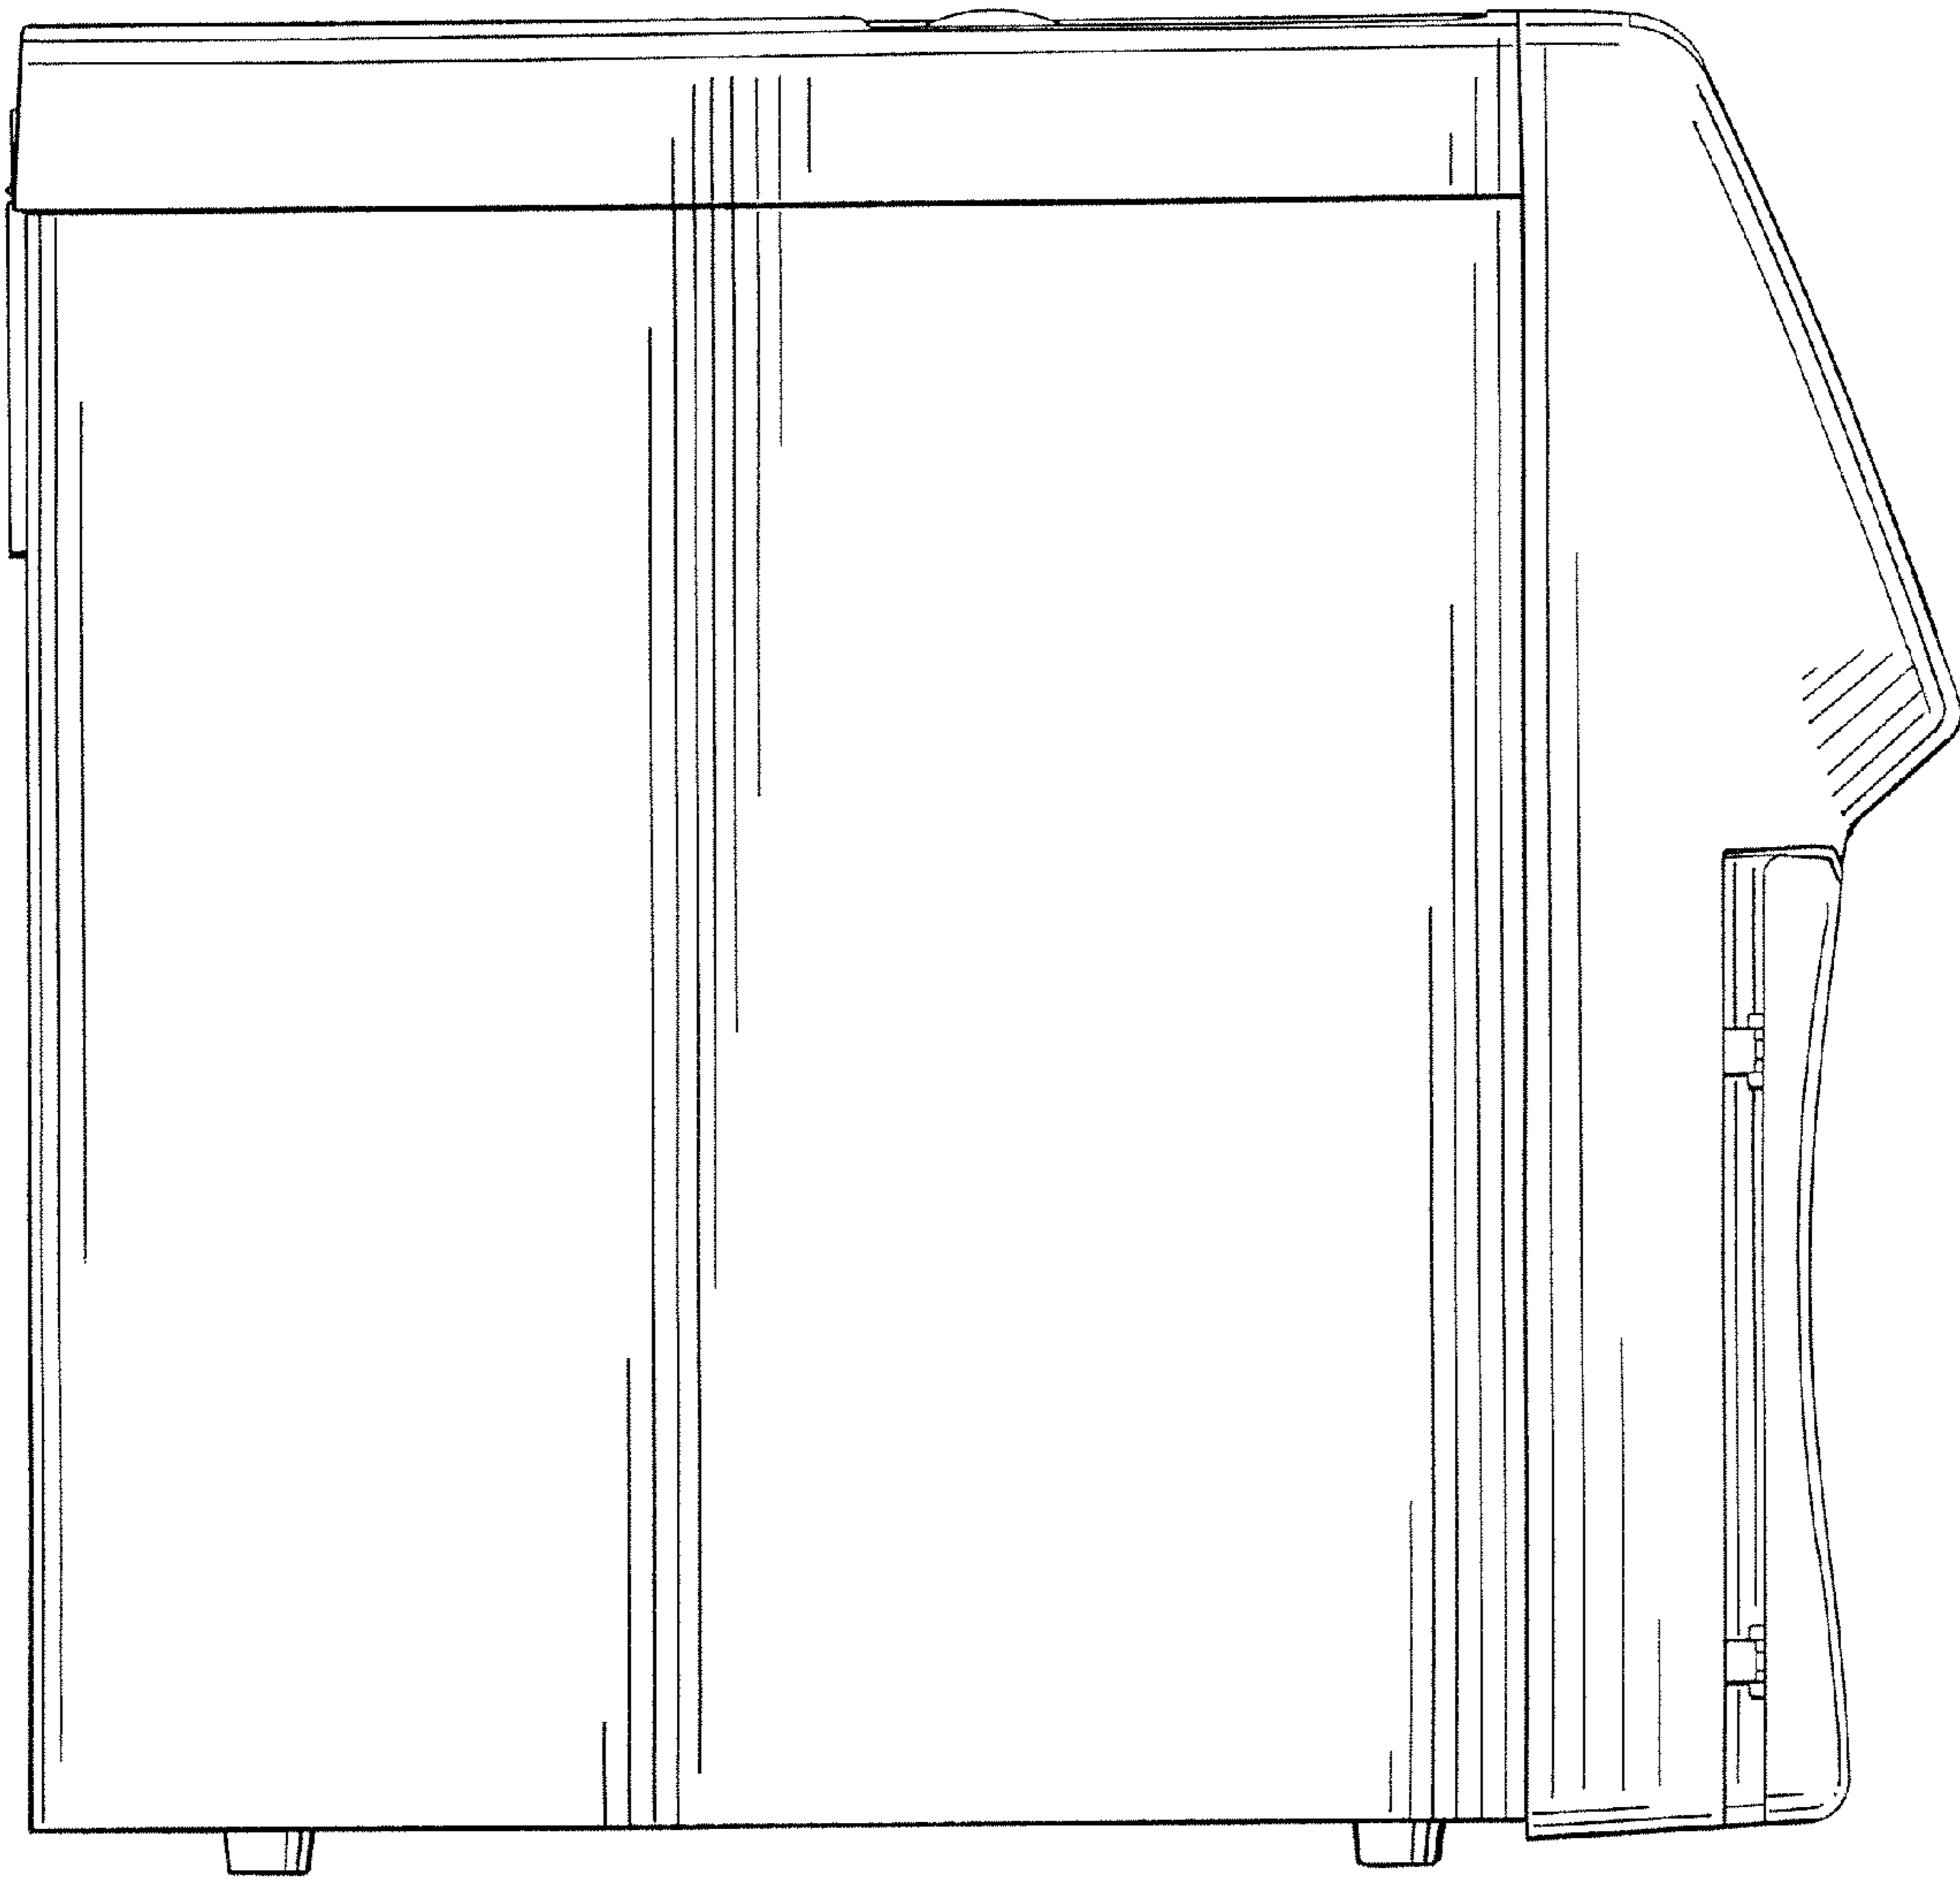

*FIG. 6*

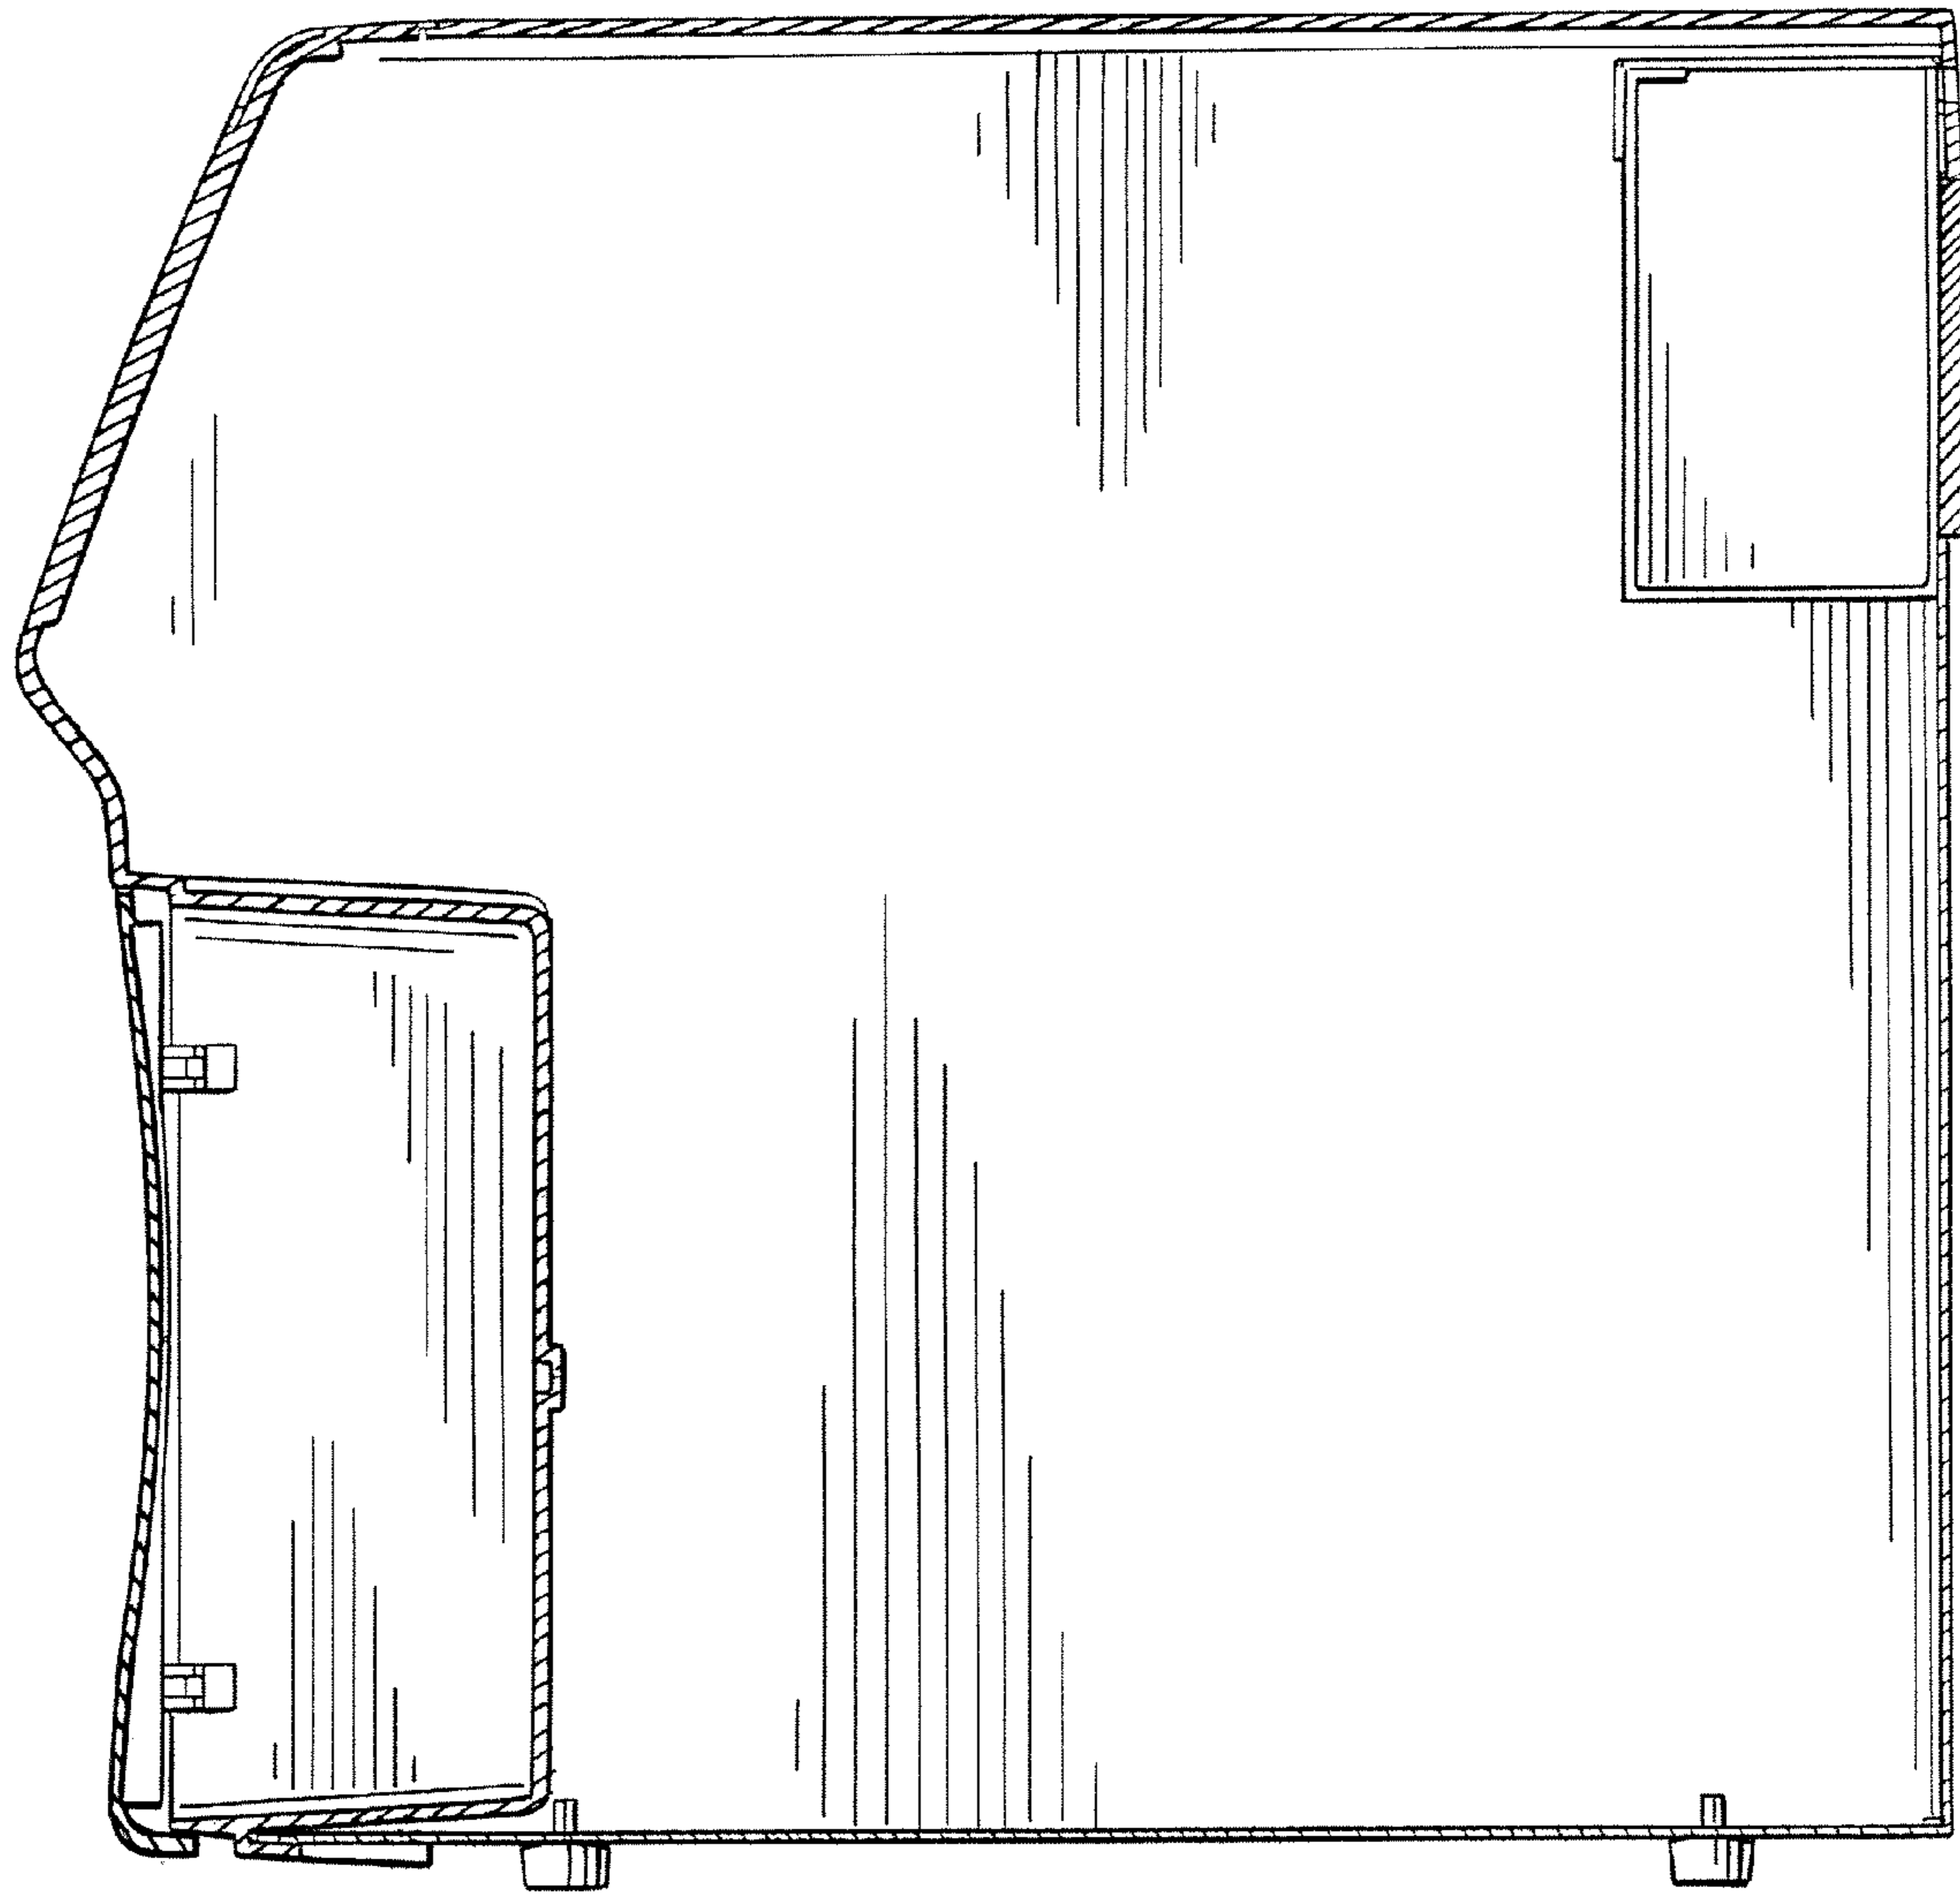


FIG. 7





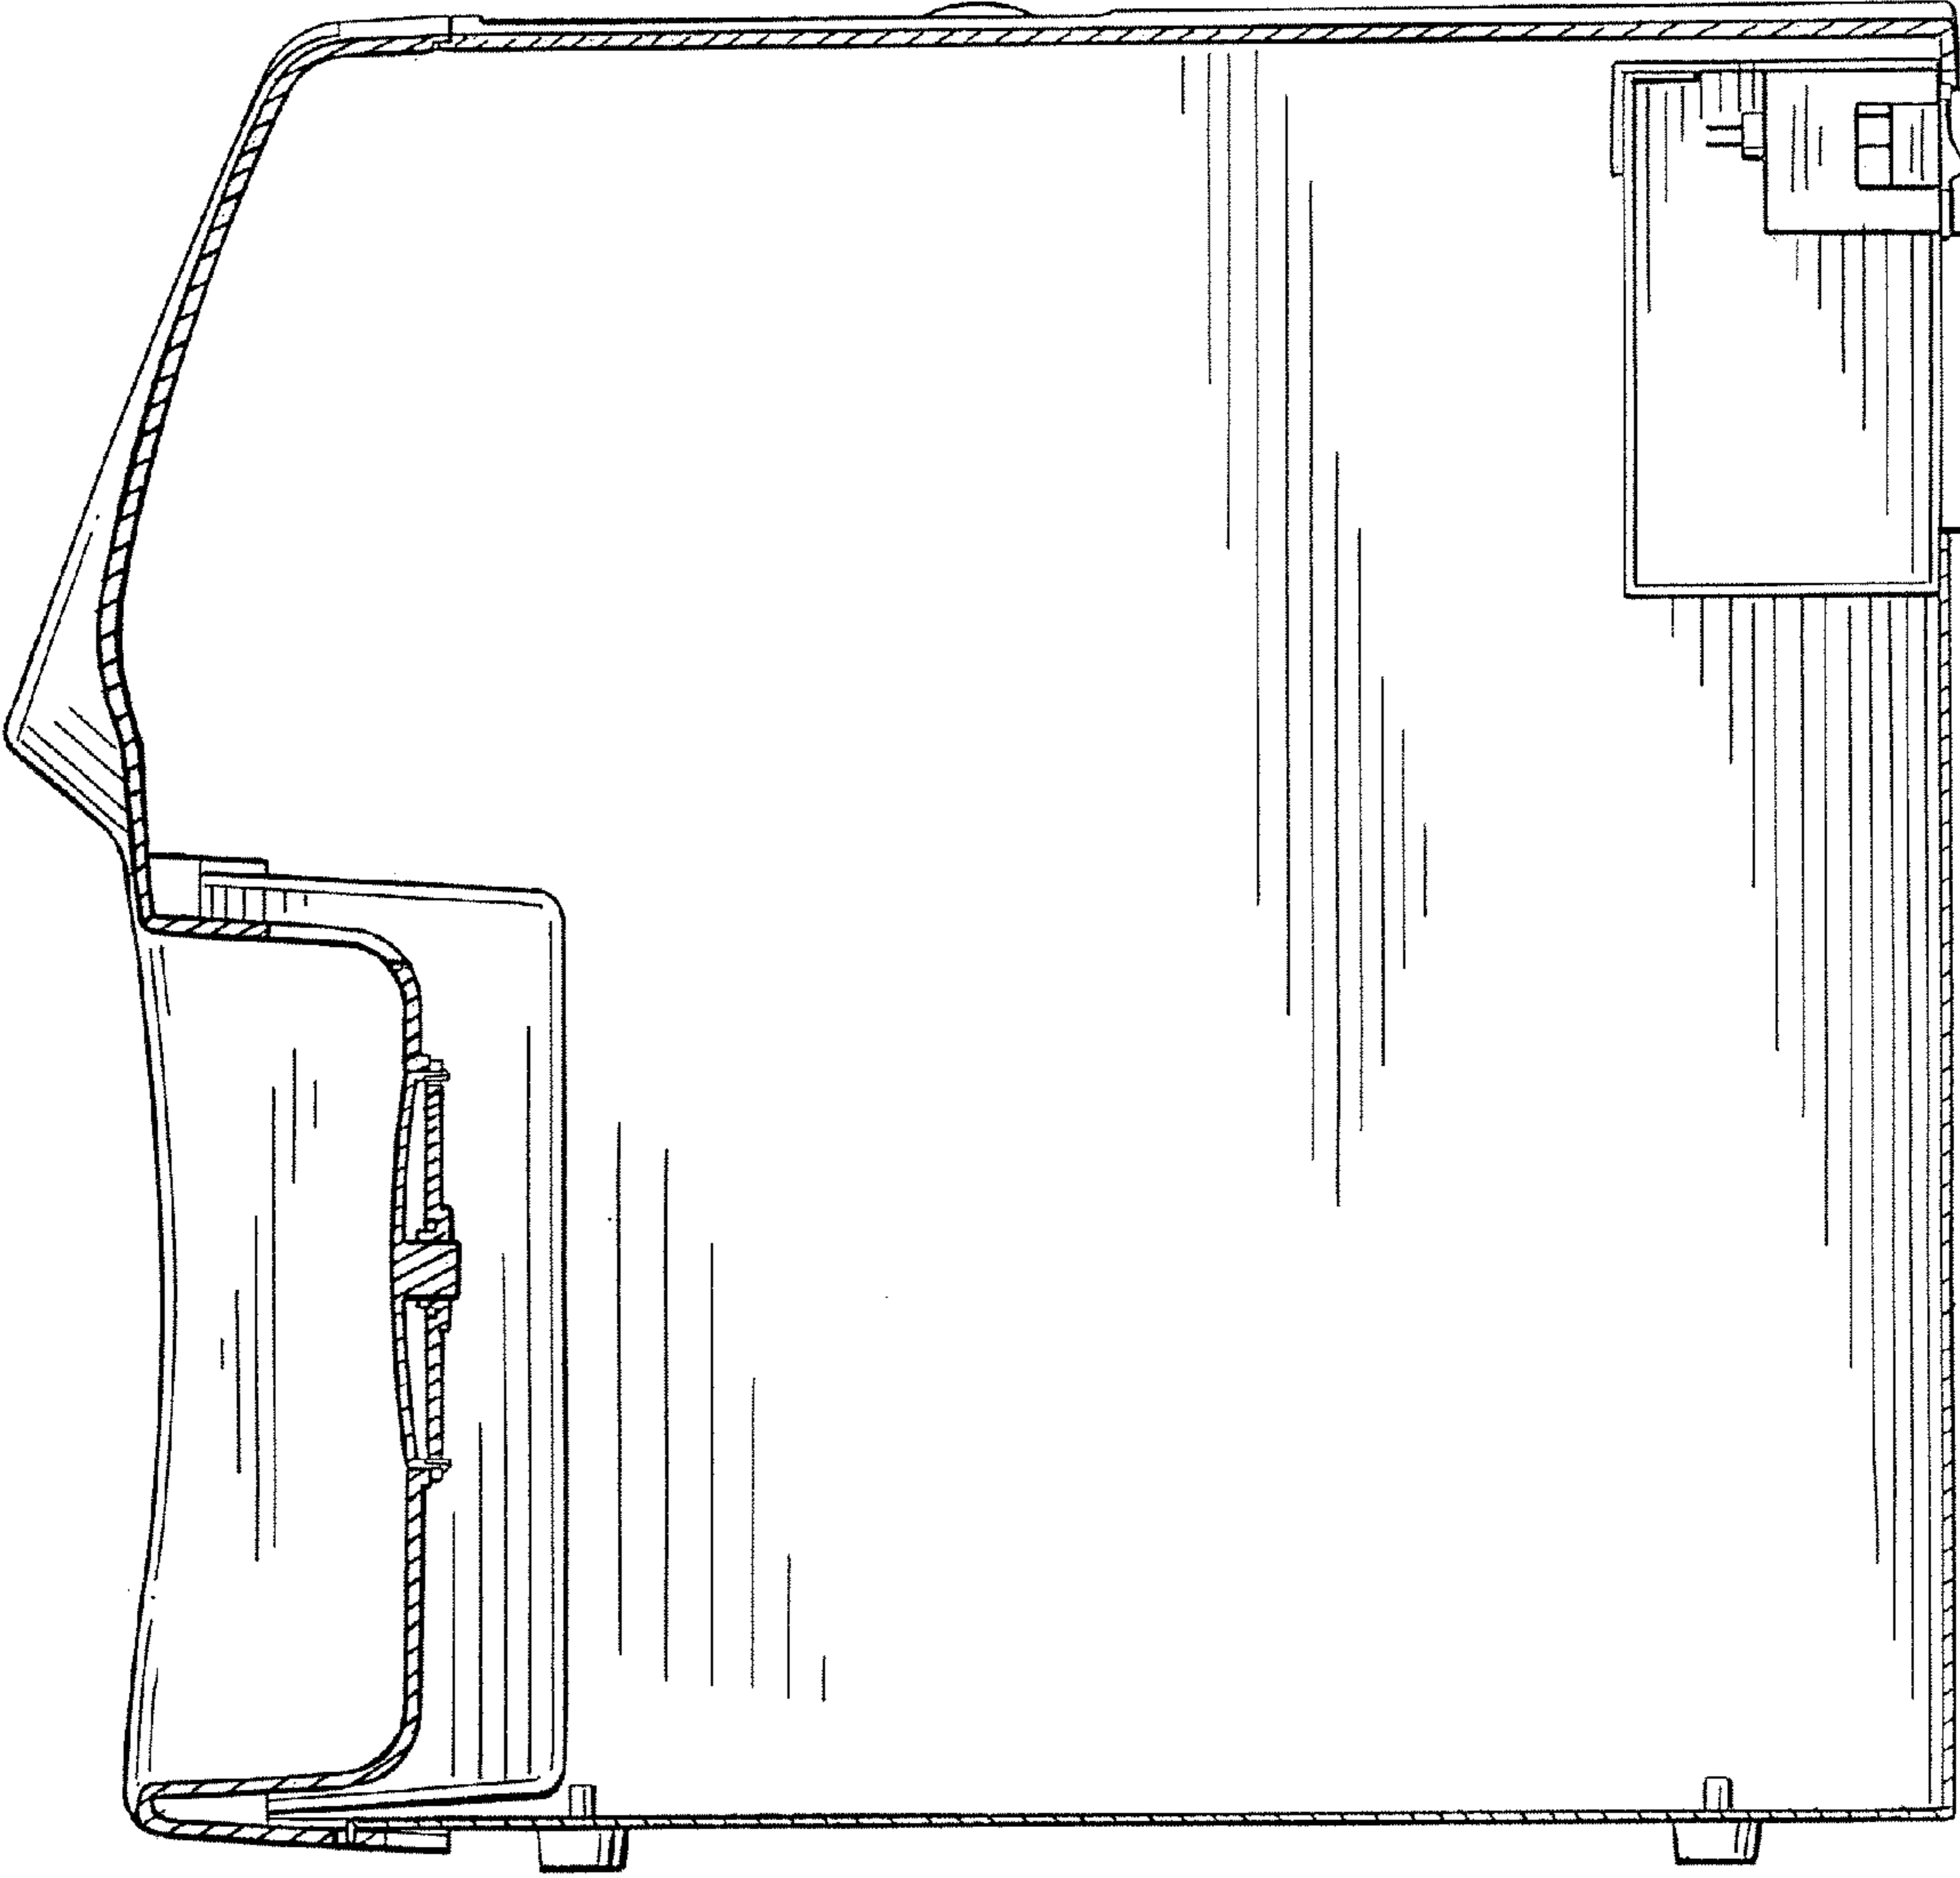



FIG. 8

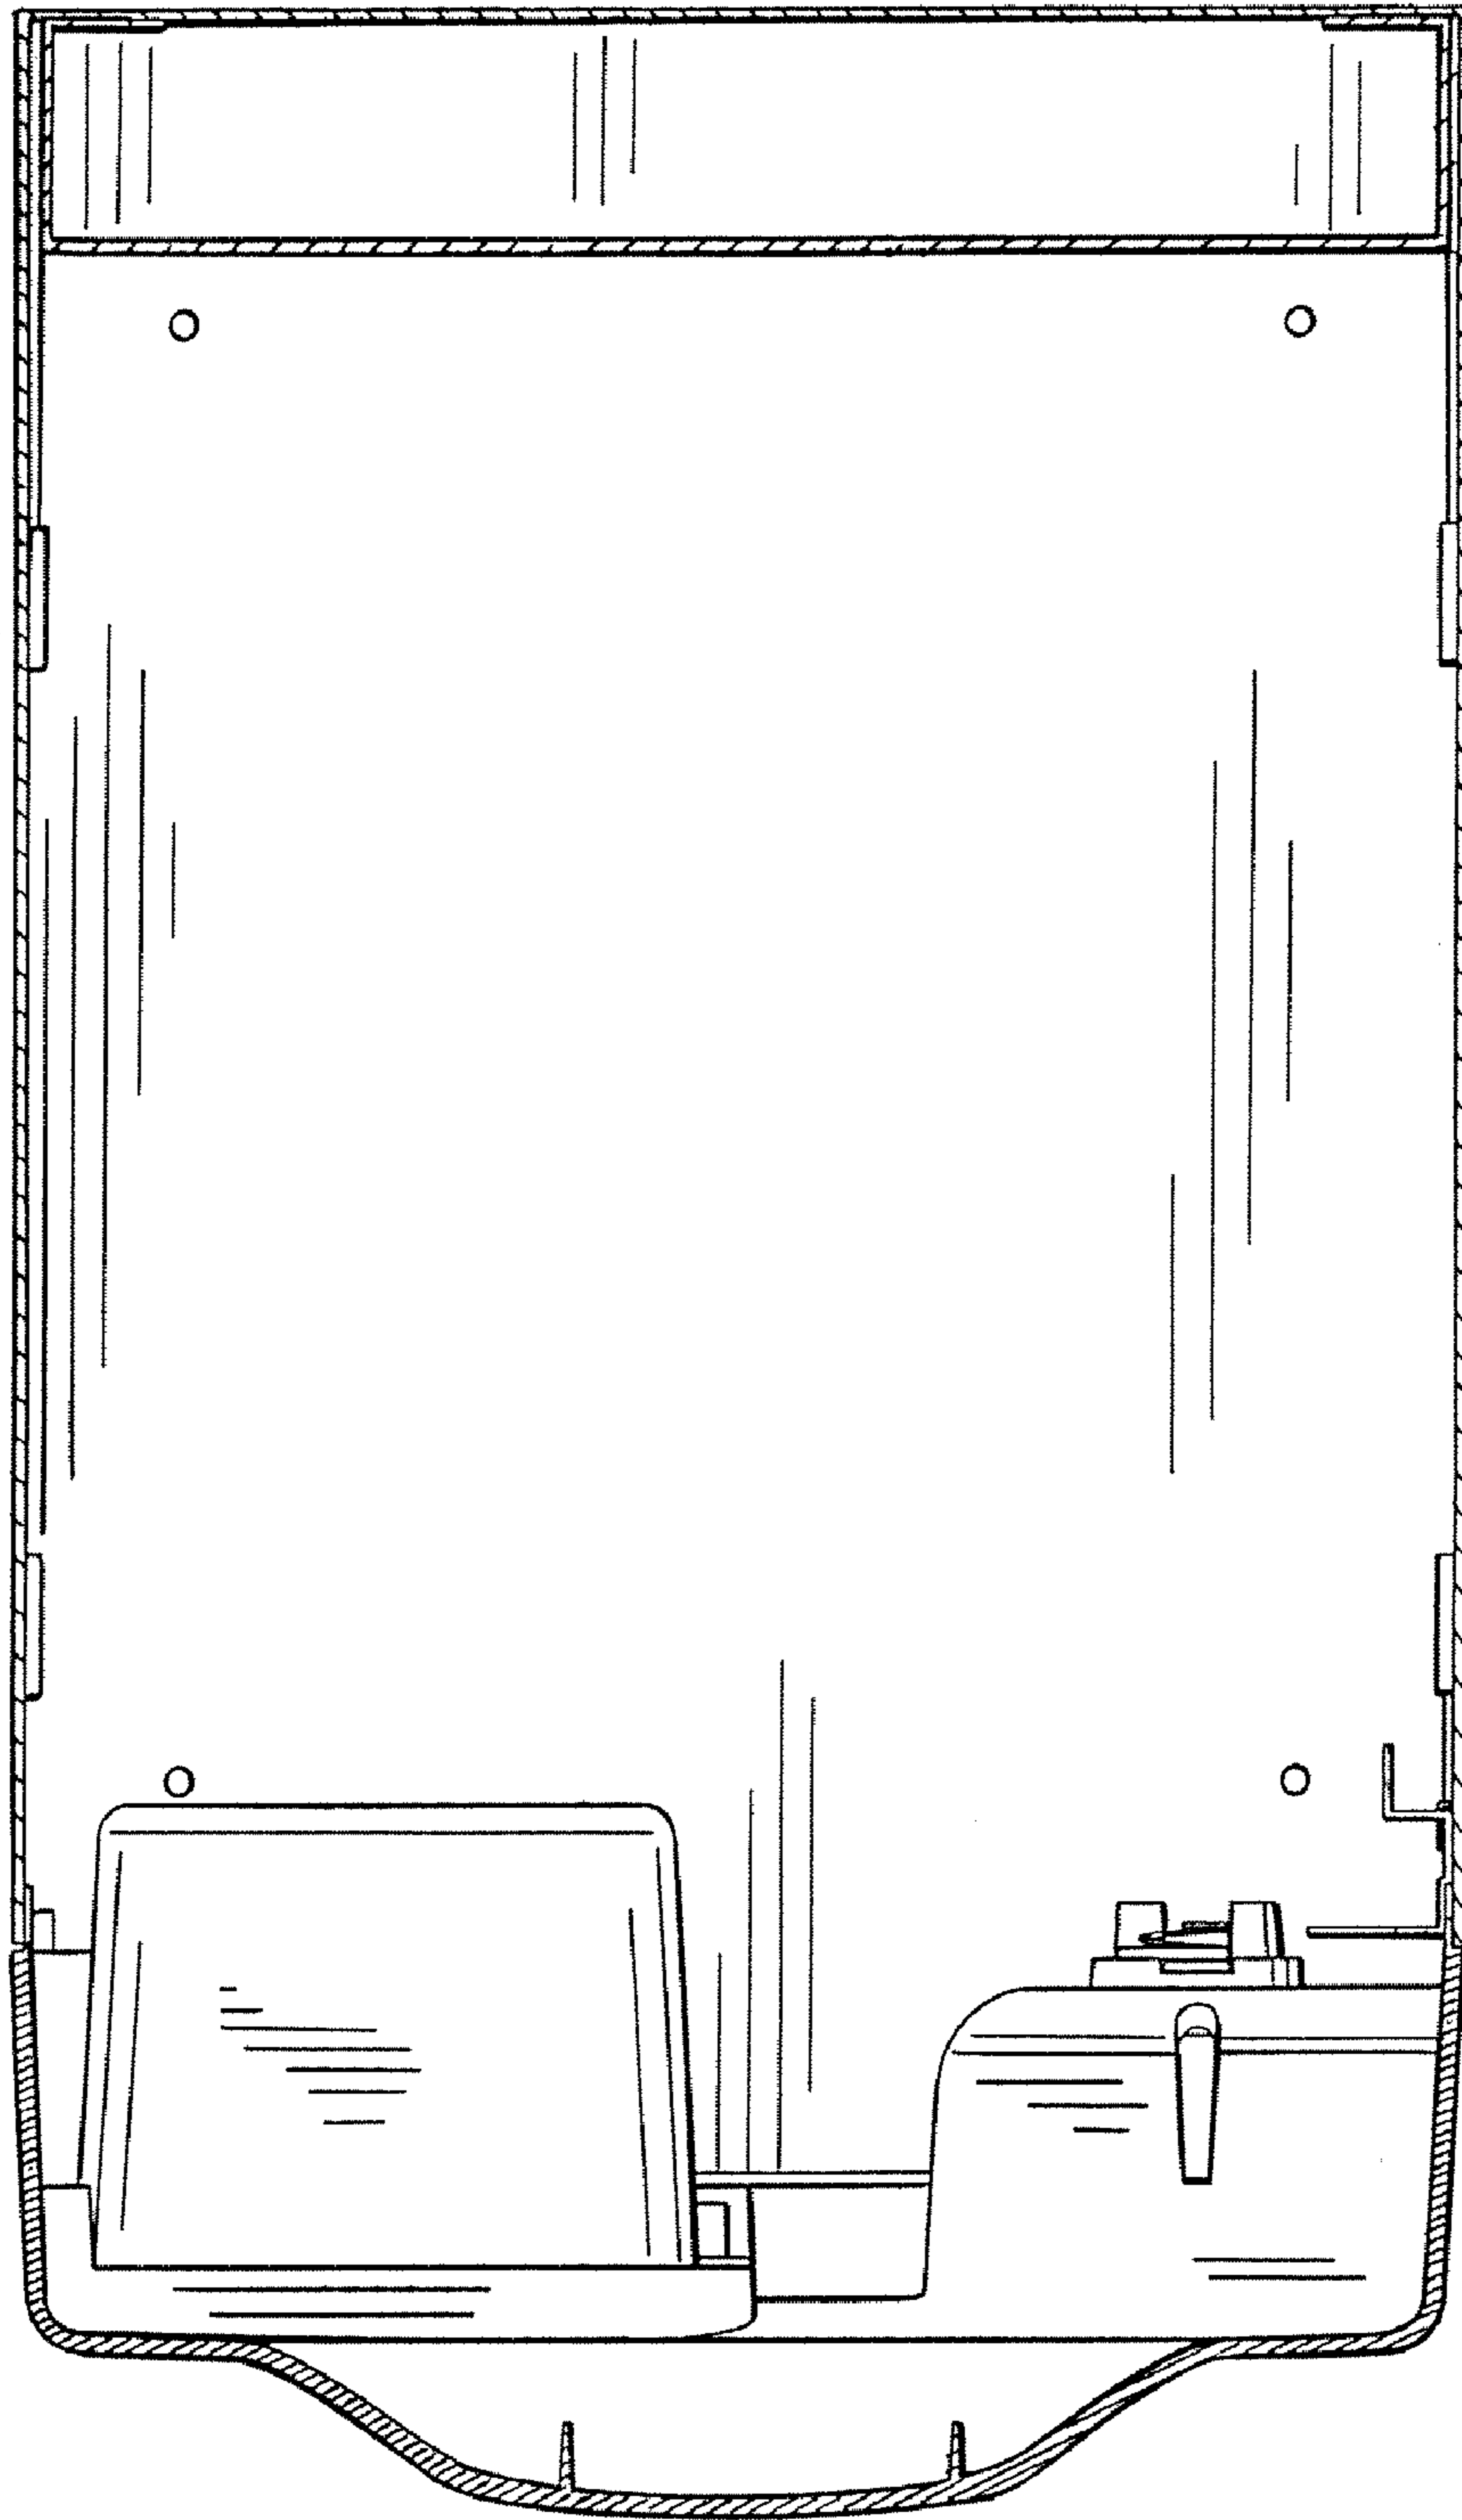

*FIG. 9*

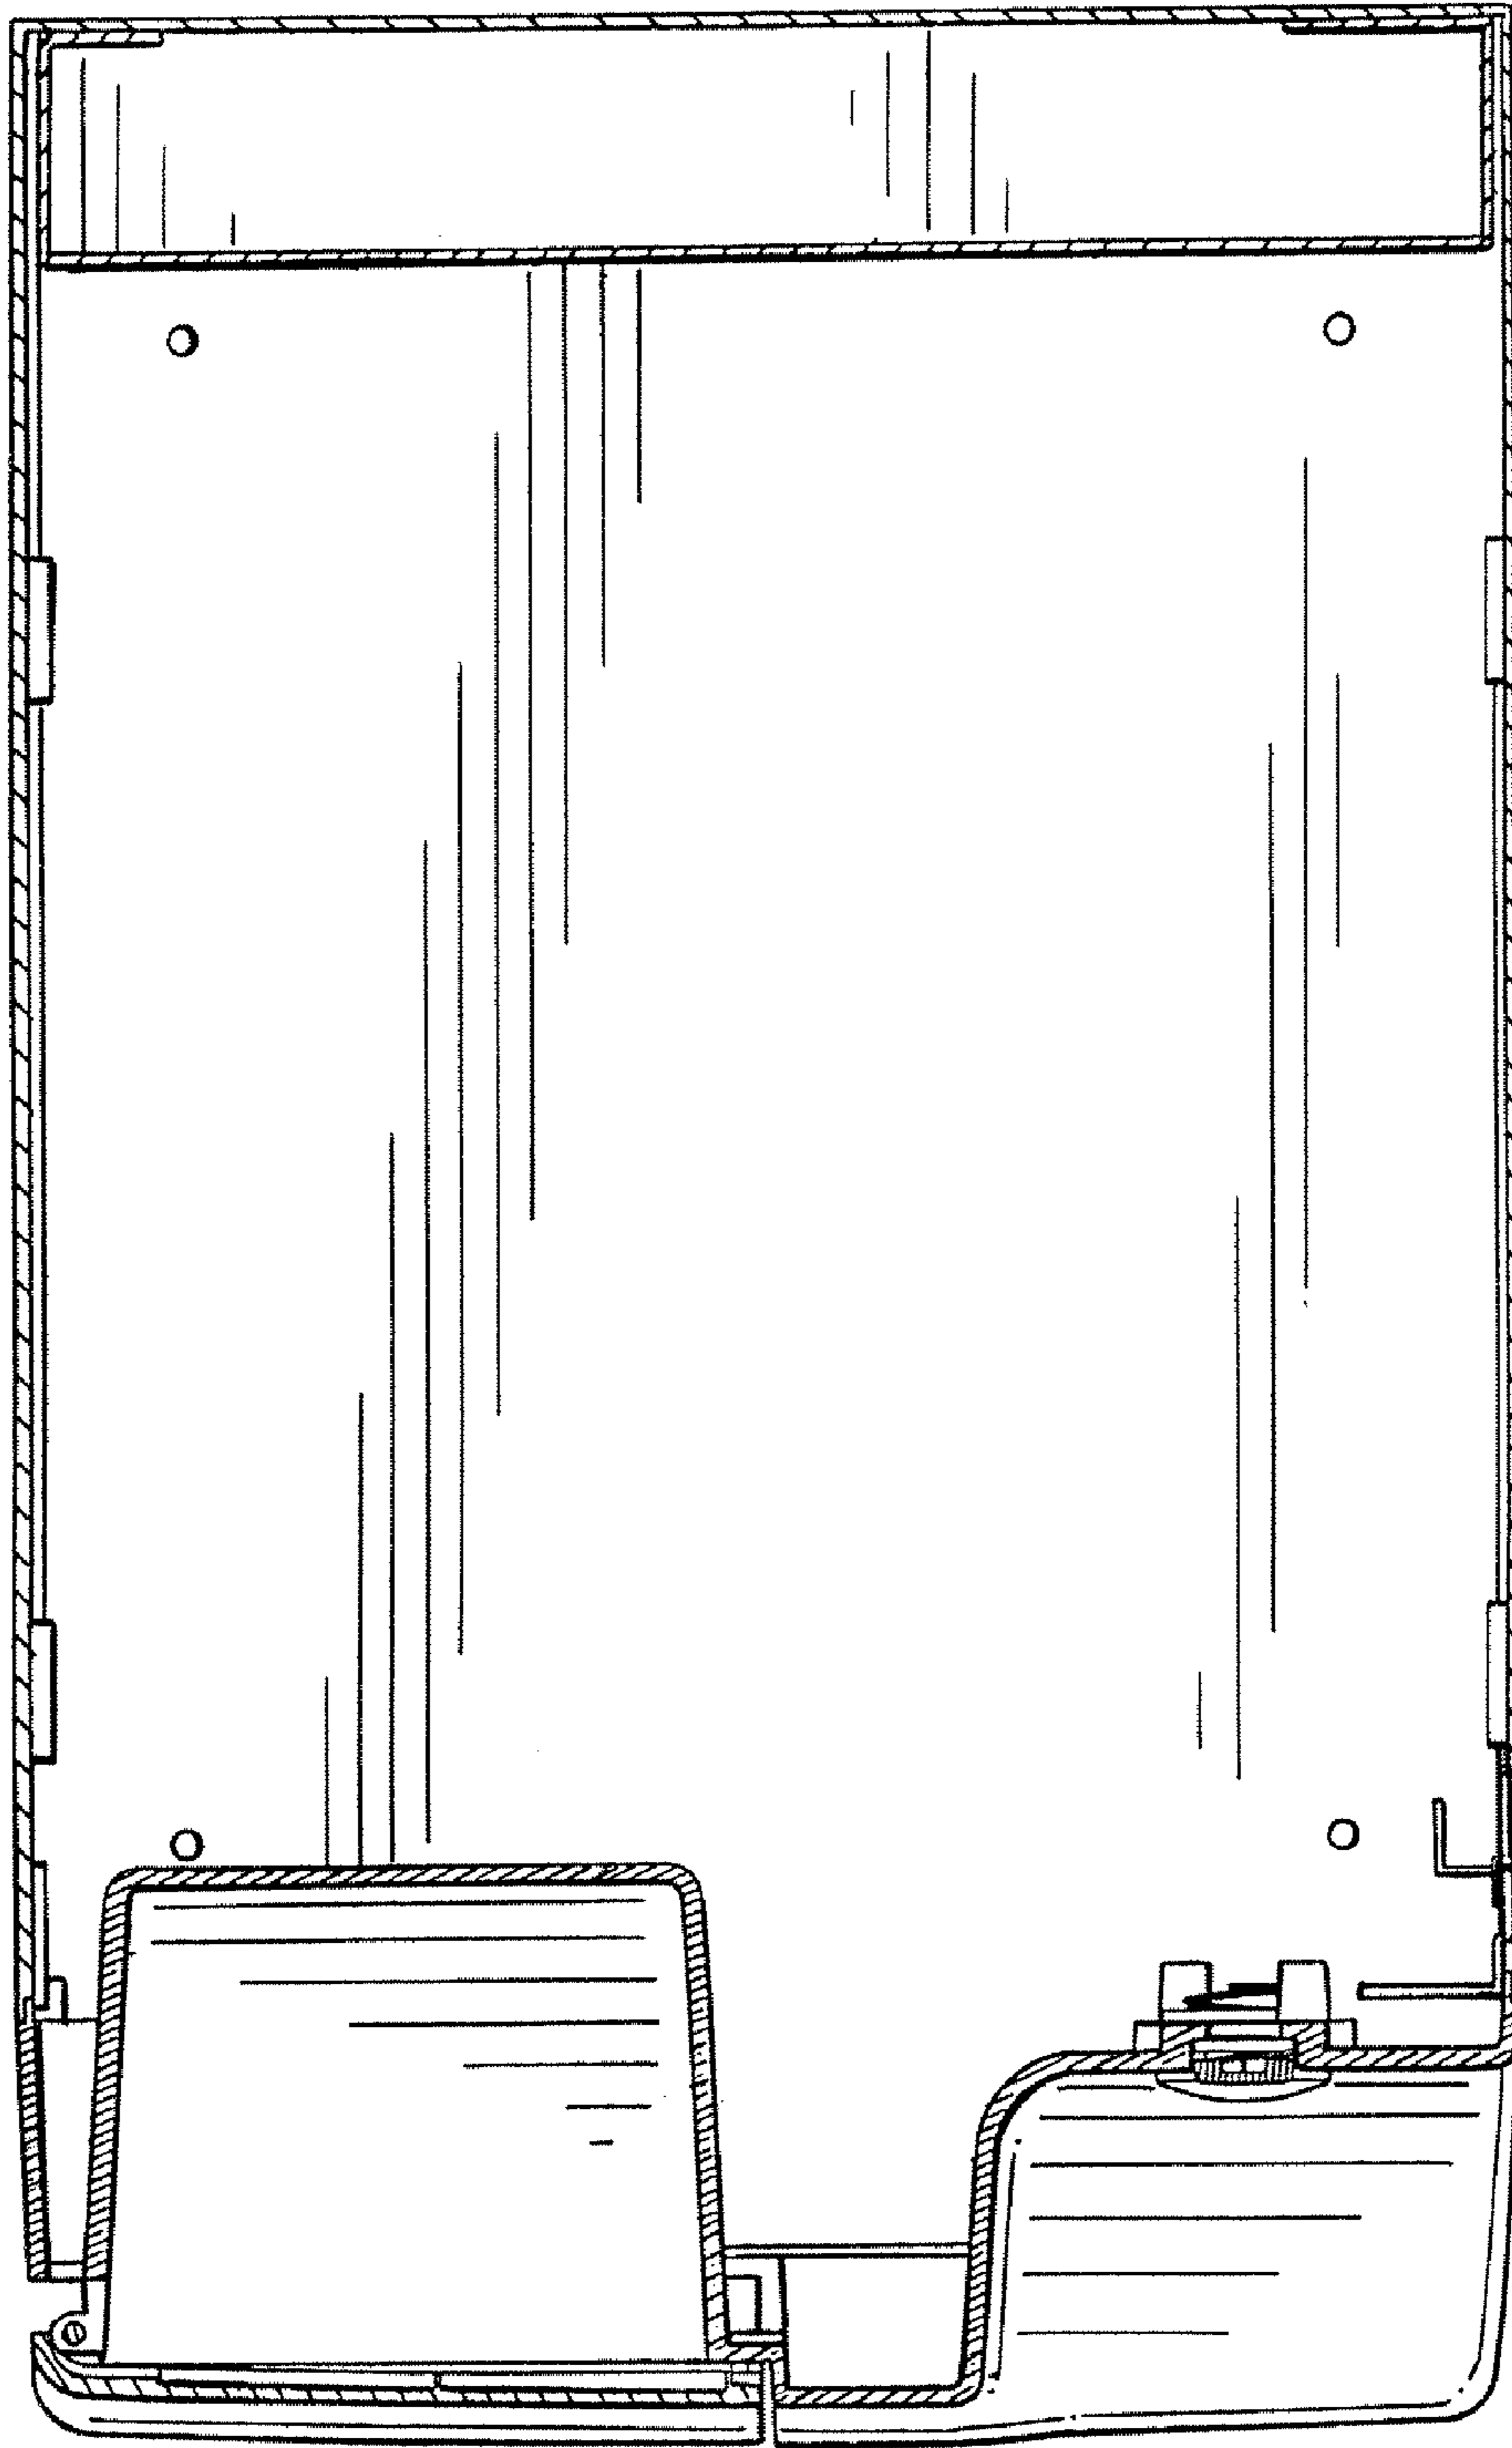

*FIG. 10*

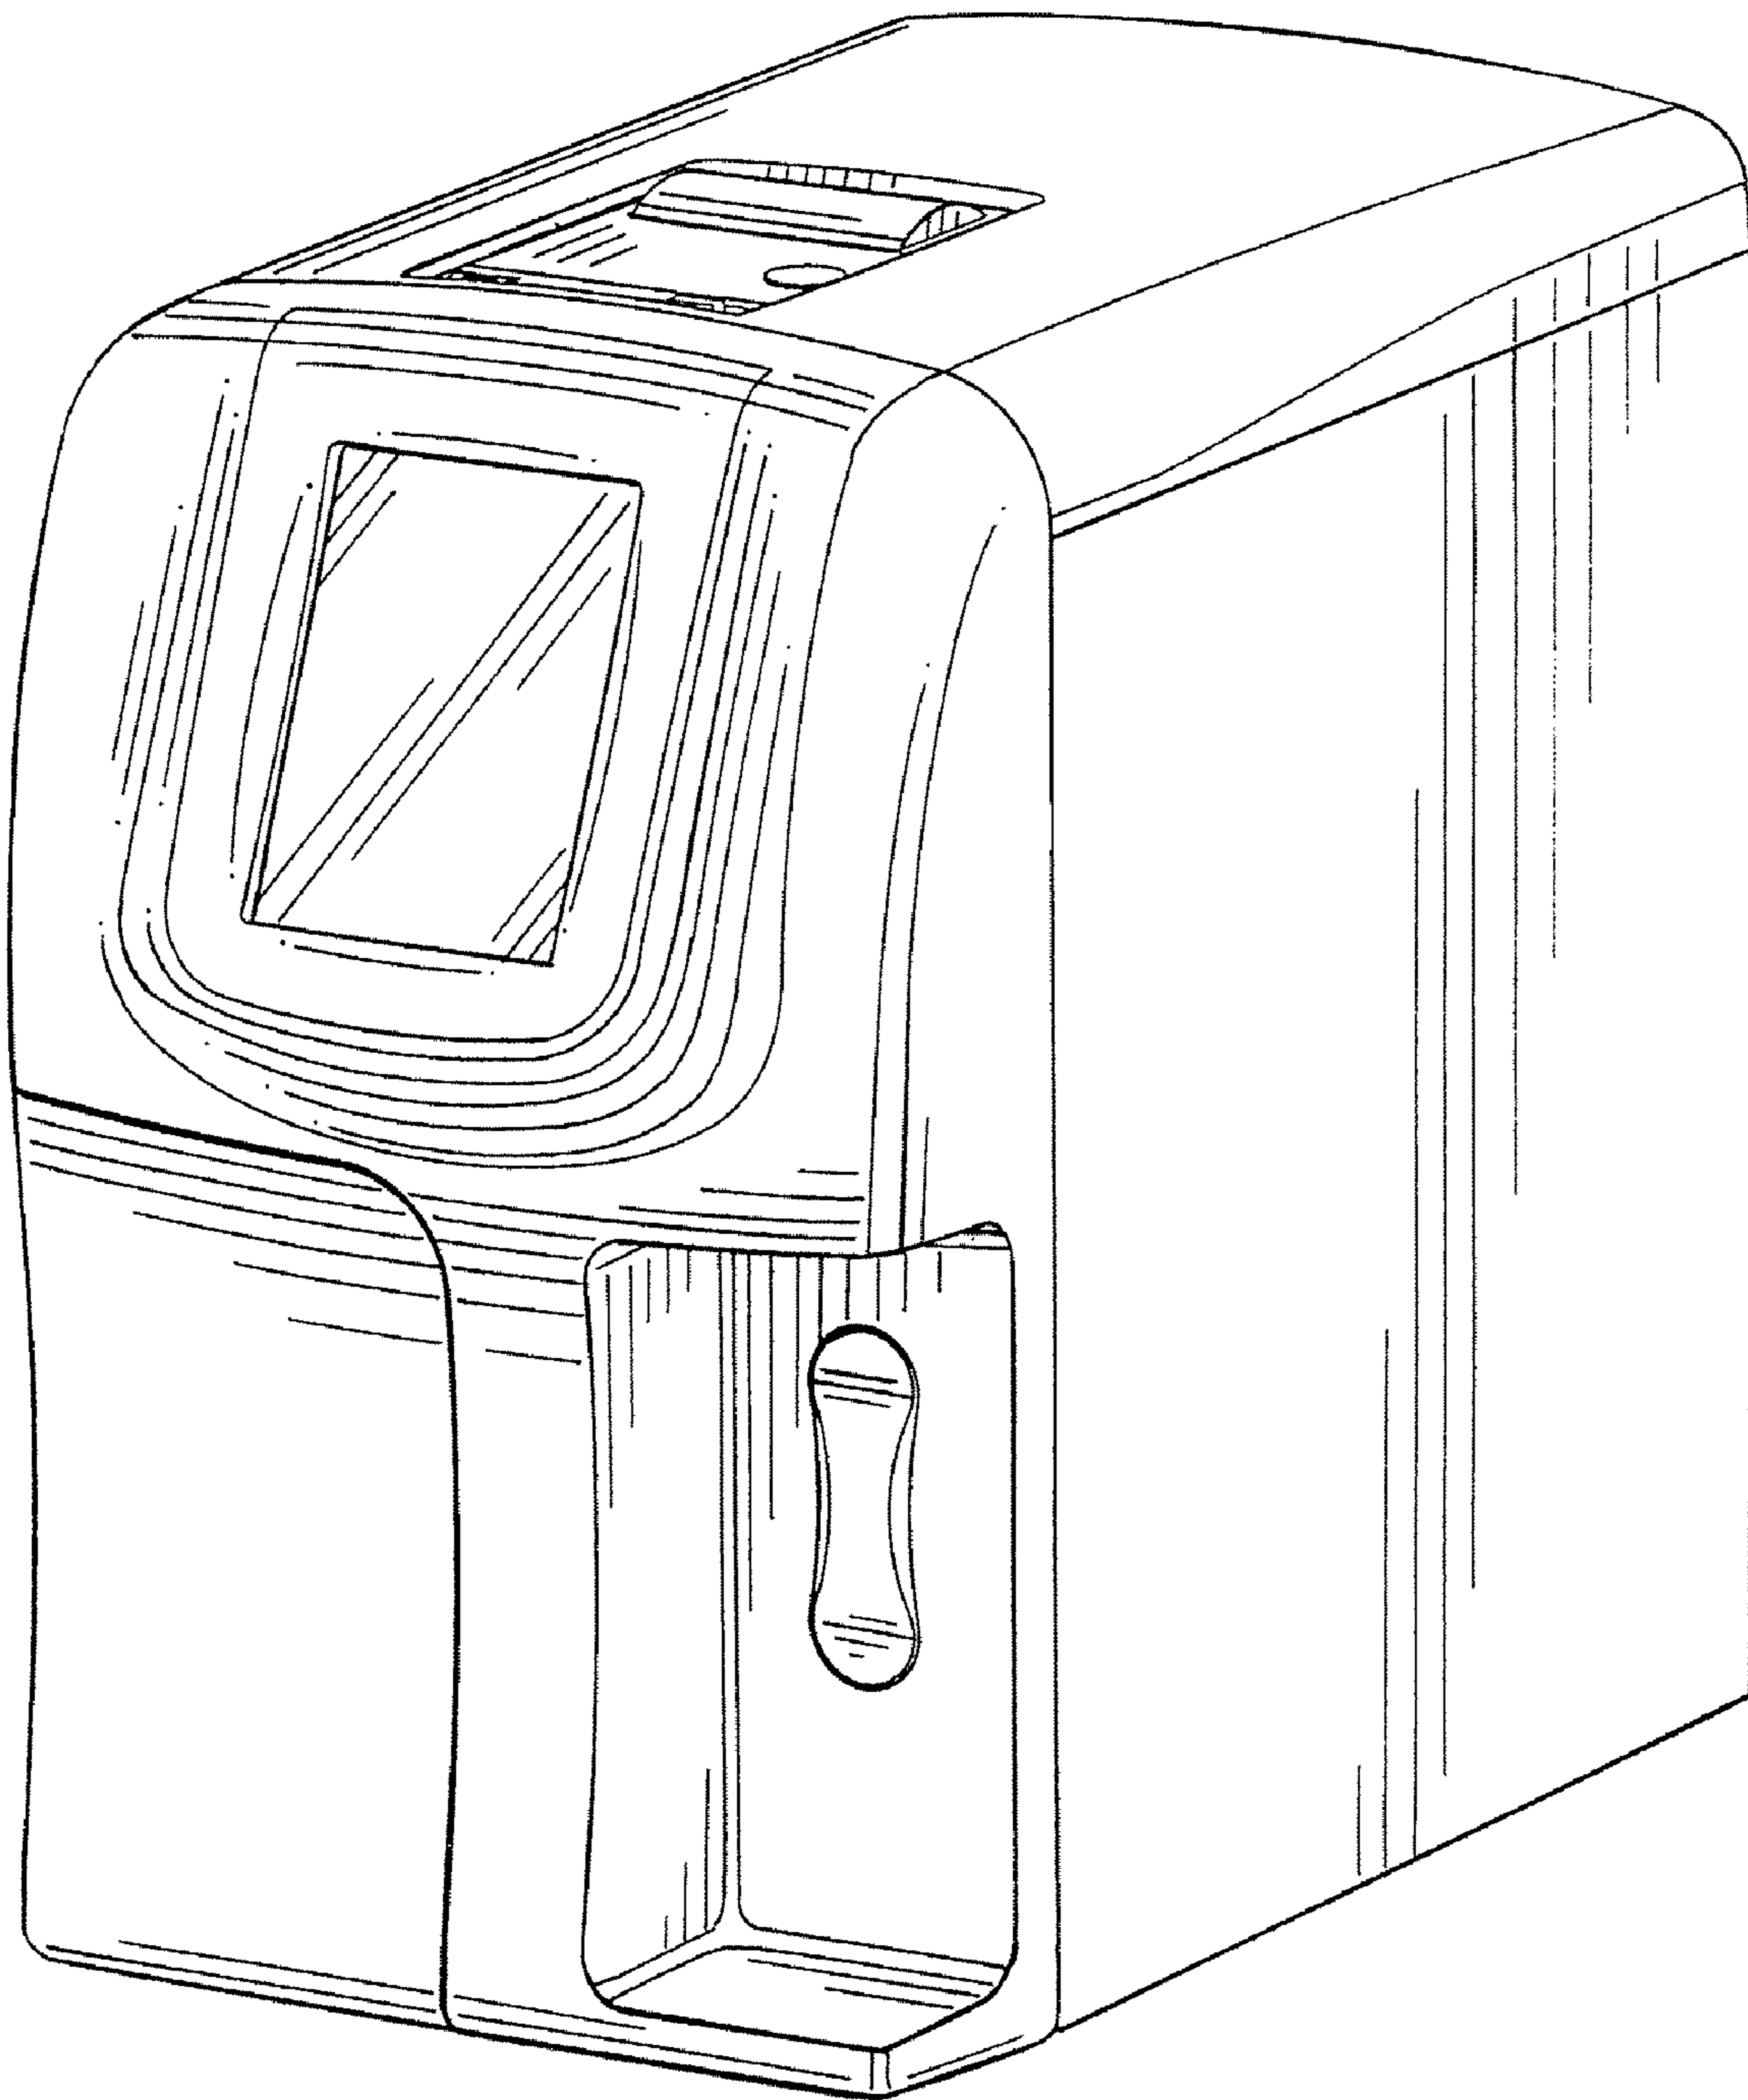

*FIG. 11*