



US00D552238S

(12) **United States Design Patent**
Zwart

(10) **Patent No.:** **US D552,238 S**

(45) **Date of Patent:** **** Oct. 2, 2007**

(54) **HEAD OF A BRUSH FOR TAKING A SMEAR SAMPLE**

5,370,128 A * 12/1994 Wainwright 600/569
5,462,063 A 10/1995 Kist et al. 600/569
6,193,674 B1 2/2001 Zwart 600/569

(75) Inventor: **Meindert Zwart**, Rosmalen (NL)

* cited by examiner

(73) Assignee: **Rovers Medical Devices B.V.** (NL)

Primary Examiner—Ian Simmons

Assistant Examiner—Christopher Lee

(**) Term: **14 Years**

(74) *Attorney, Agent, or Firm*—Steven M. Koehler;
Westman, Champlin & Kelly, P.A.

(21) Appl. No.: **29/232,219**

(22) Filed: **Jun. 16, 2005**

(57) **CLAIM**

(30) **Foreign Application Priority Data**

The ornamental design for a head of a brush for taking a smear sample, as shown and described.

Dec. 17, 2004 (EM) 000269097

DESCRIPTION

(51) **LOC (8) Cl.** **24-02**

FIG. 1 is a perspective view of a head of a brush for taking a smear sample of the present invention;

(52) **U.S. Cl.** **D24/146; D24/147**

FIG. 2 is a top plan view thereof;

(58) **Field of Classification Search** D24/146,
D24/147, 224, 119; D4/128, 104, 131, 133;
D28/7; 600/569, 570, 562; 15/207.2; 604/540
See application file for complete search history.

FIG. 3 is a bottom plan view thereof;

FIG. 4 is a left side view thereof;

FIG. 5 is a right side view thereof

(56) **References Cited**

FIG. 6 is a front elevational view thereof; and,


U.S. PATENT DOCUMENTS

FIG. 7 is a rear elevational view.

3,881,464 A 5/1975 Levene 128/2
4,127,113 A 11/1978 Nollan 128/2
4,700,713 A 10/1987 Kist 128/756
5,131,402 A * 7/1992 Van Dooren 600/570
5,191,899 A * 3/1993 Strickland et al. 600/569

The broken line showing is for illustrative purposes only and forms no part of the claimed design.

1 Claim, 5 Drawing Sheets

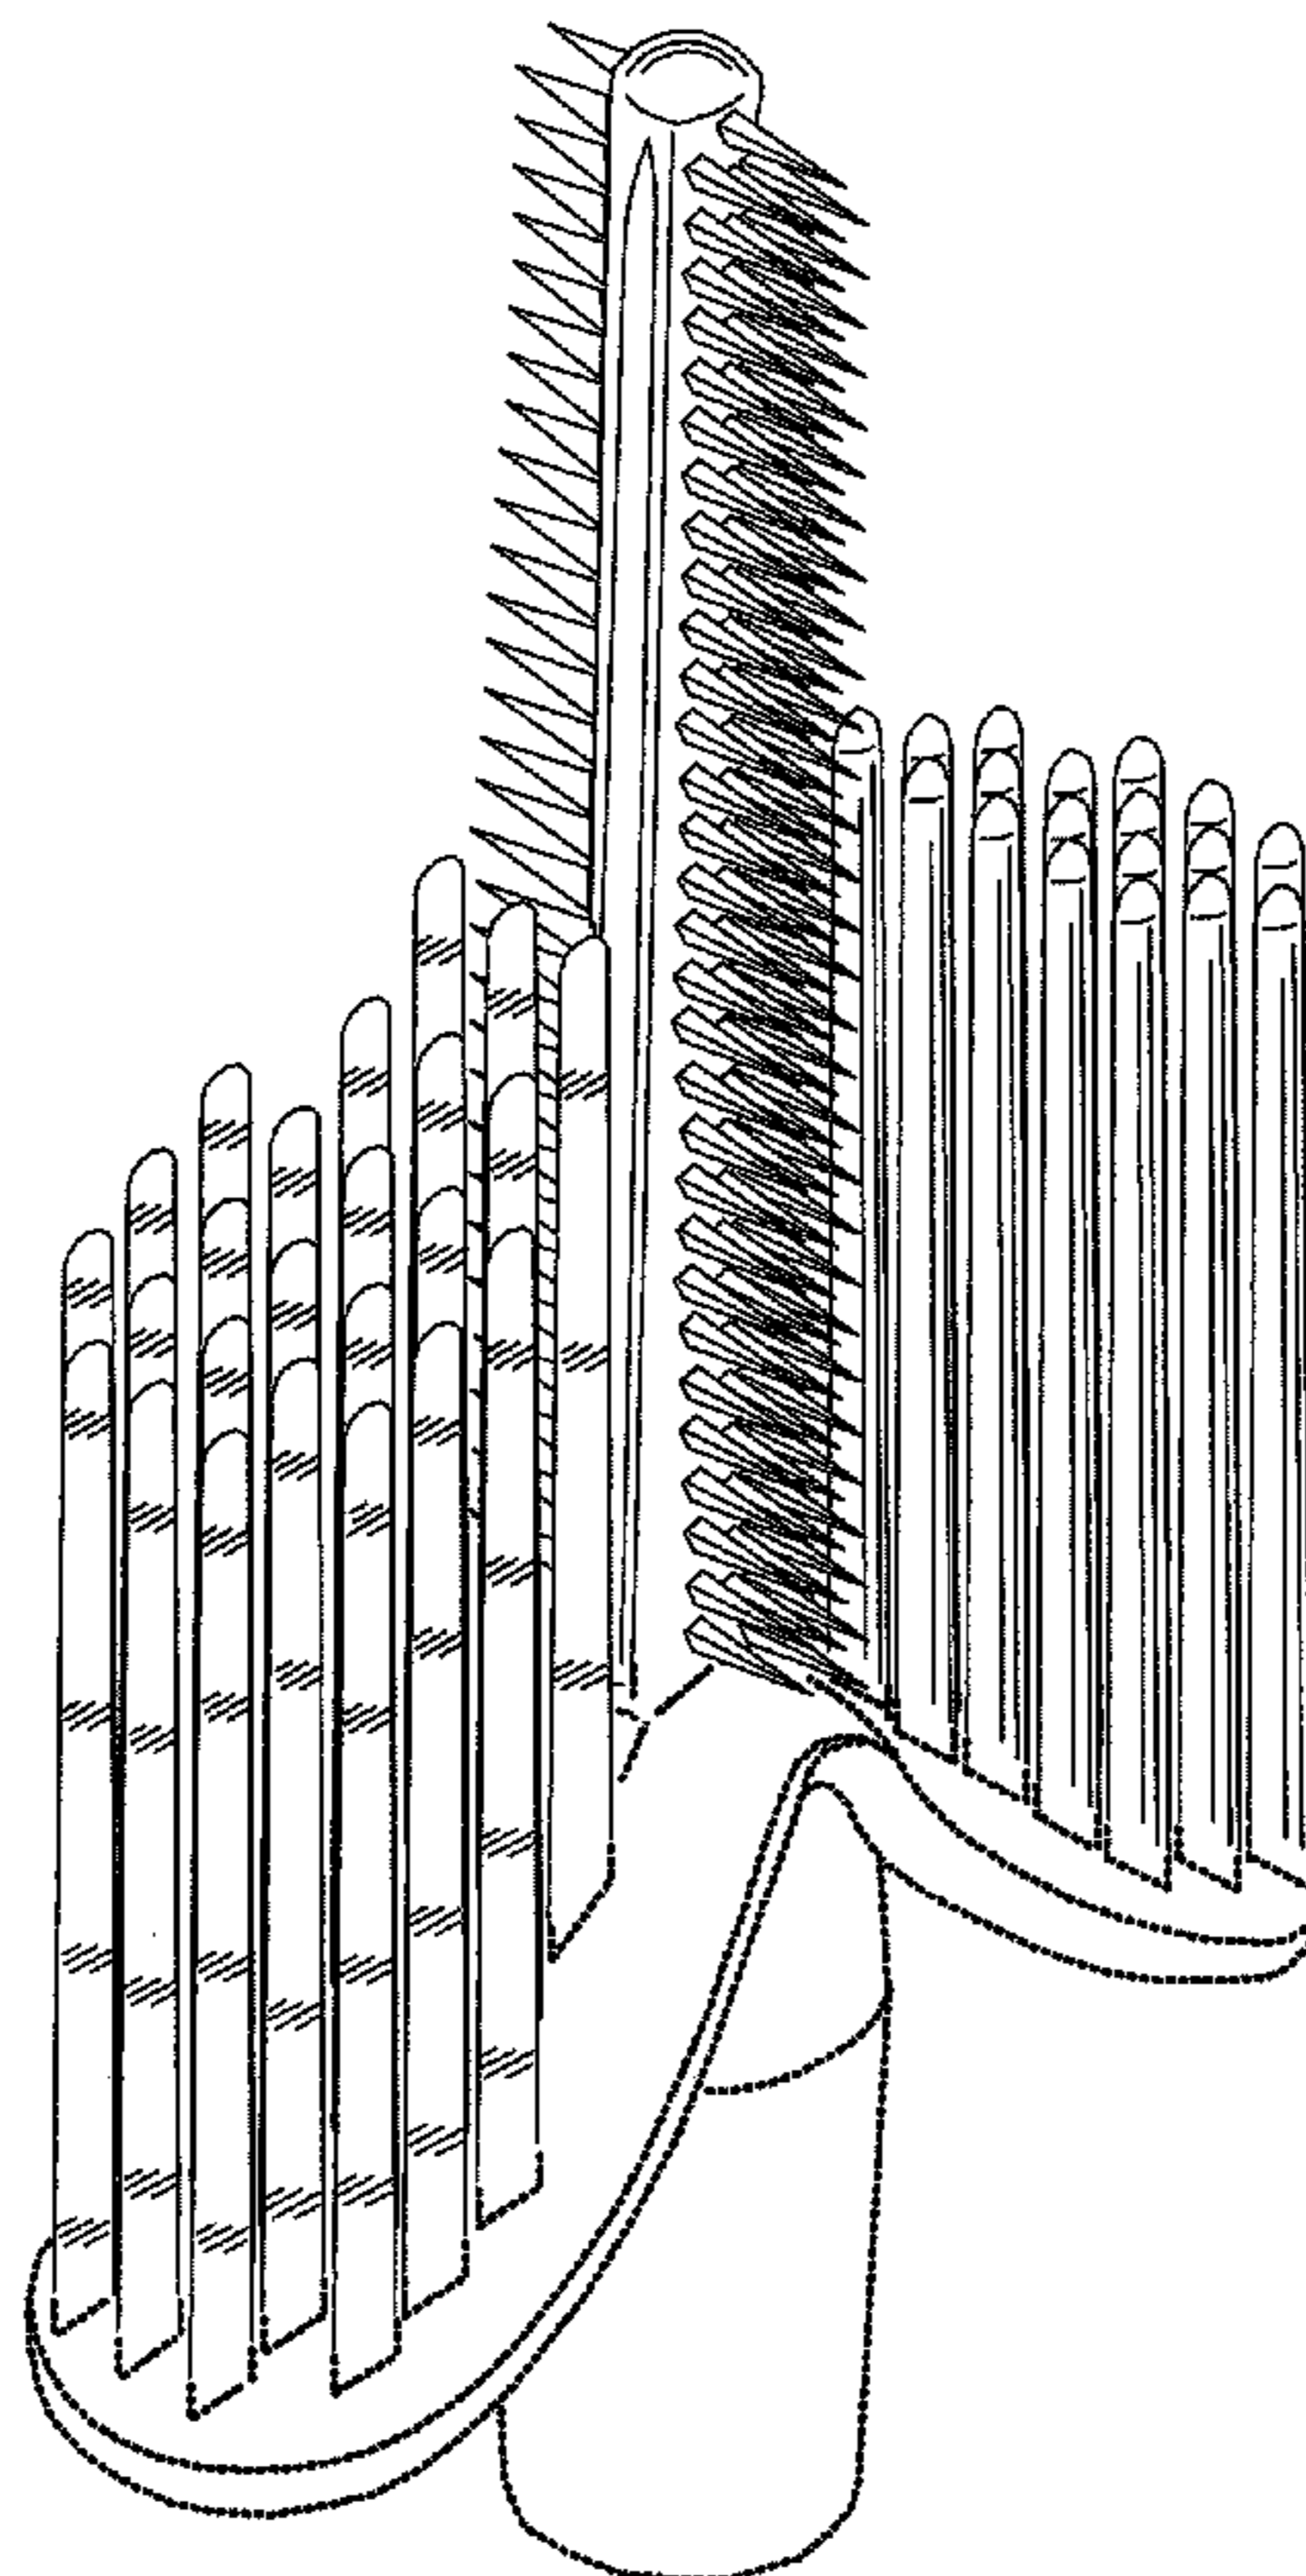

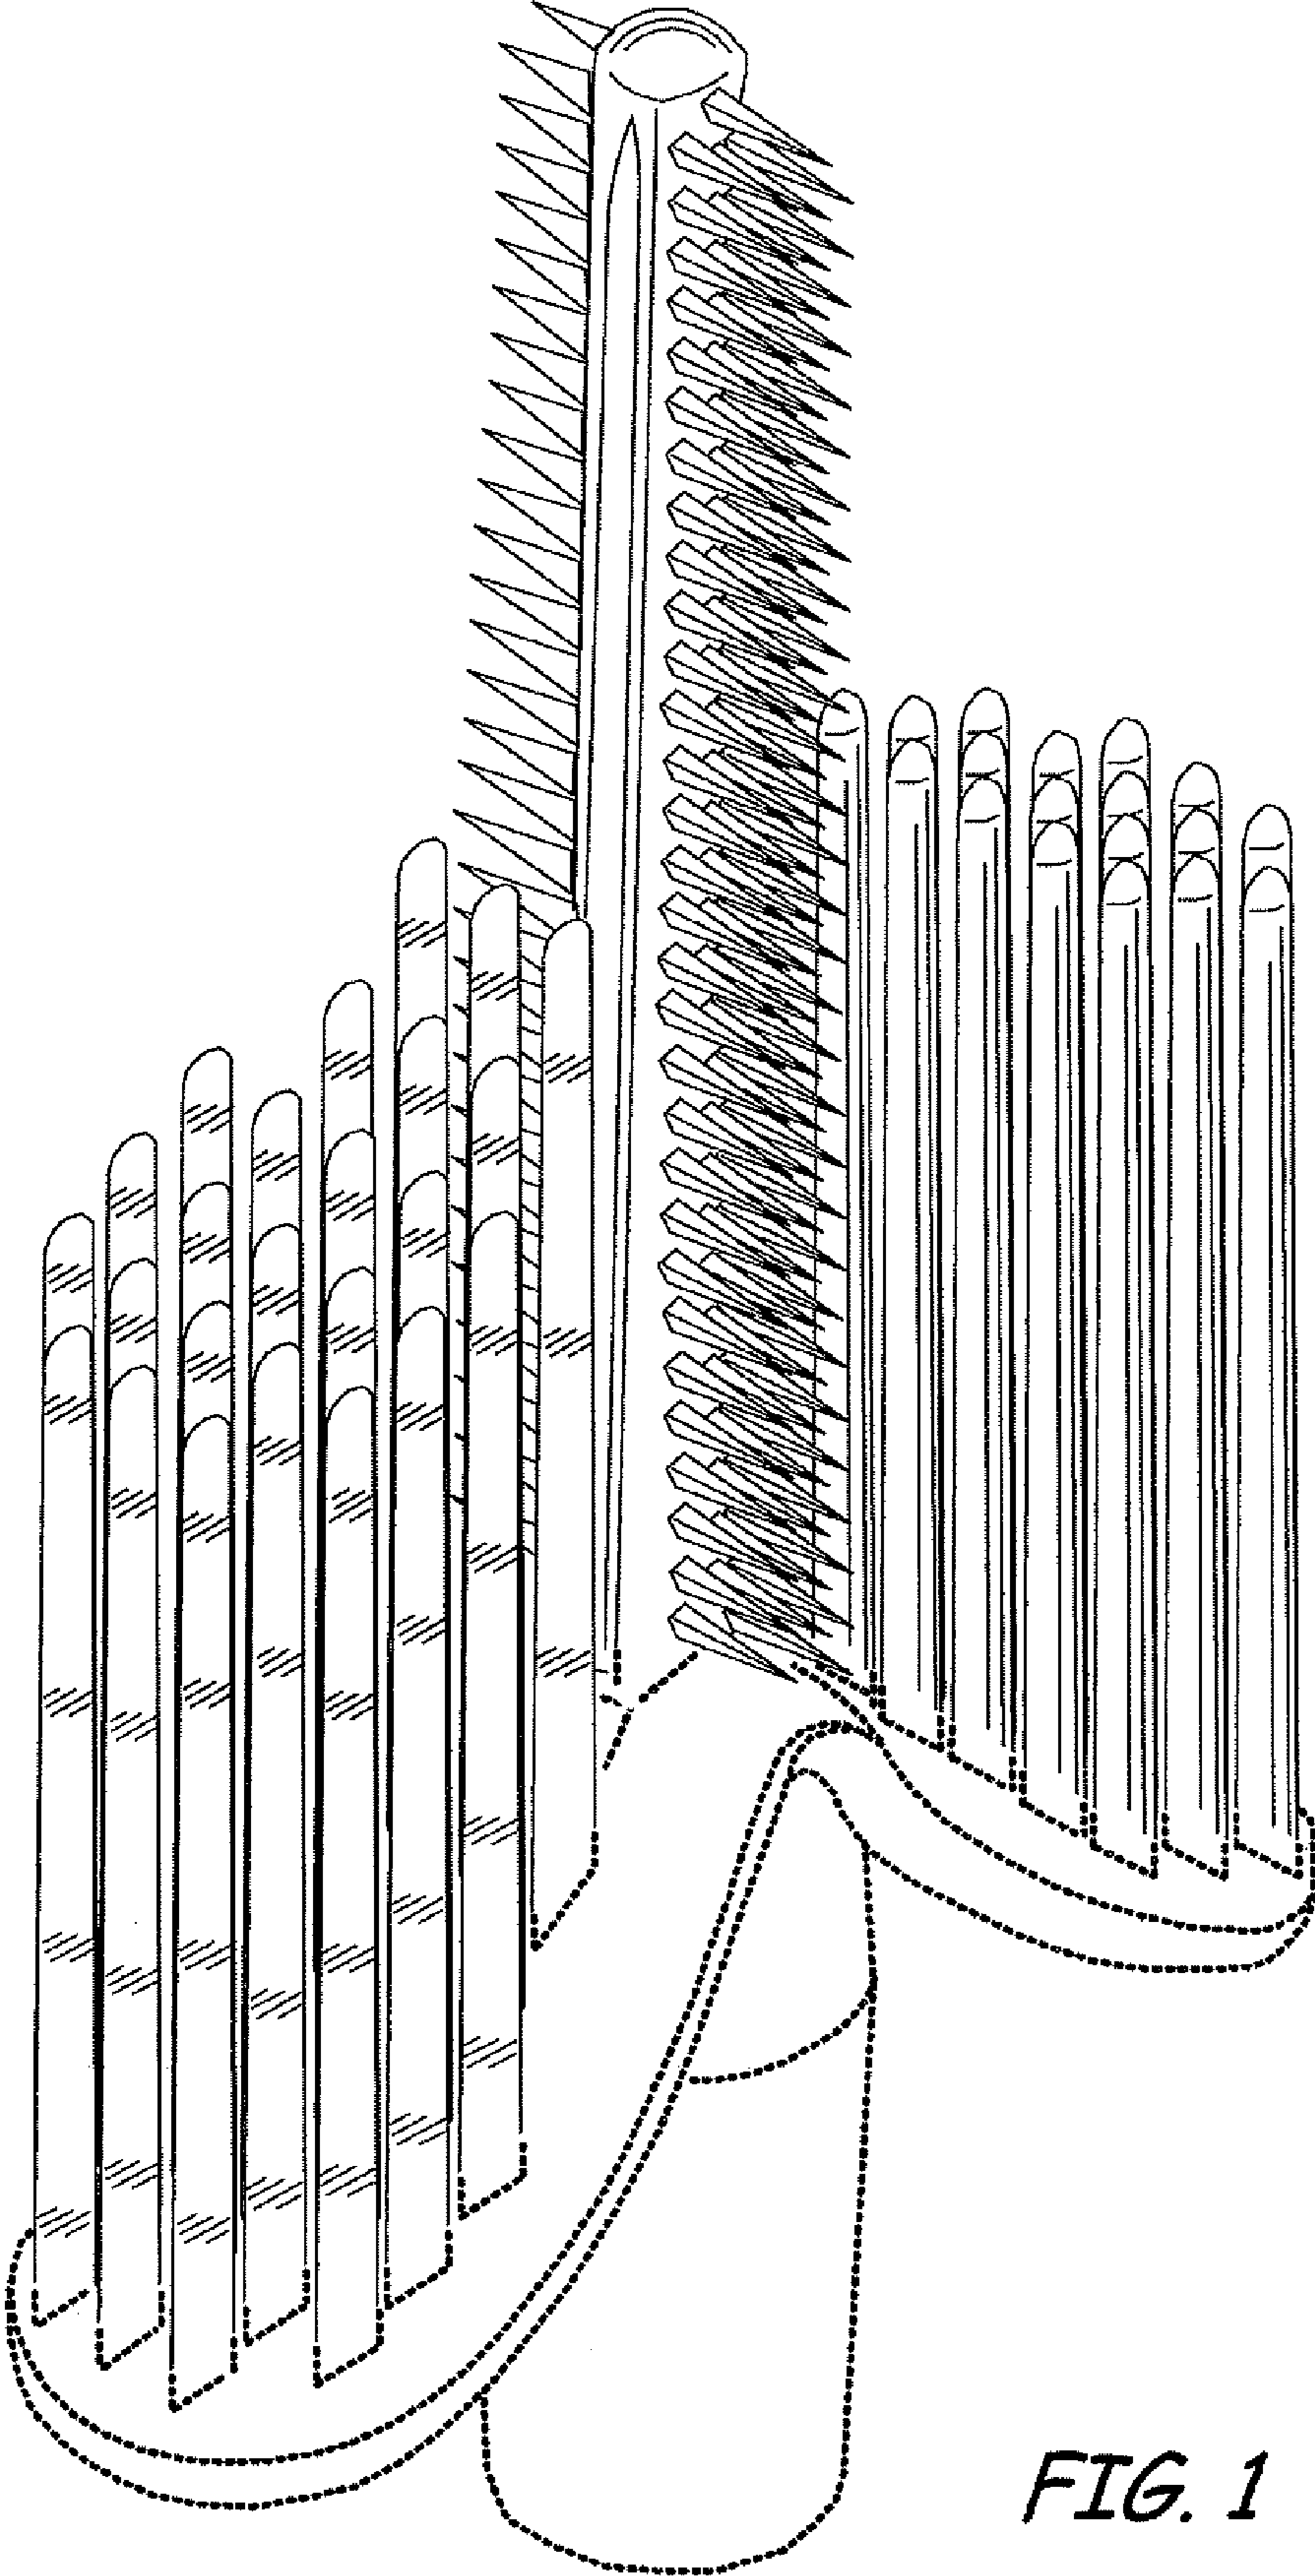


FIG. 1

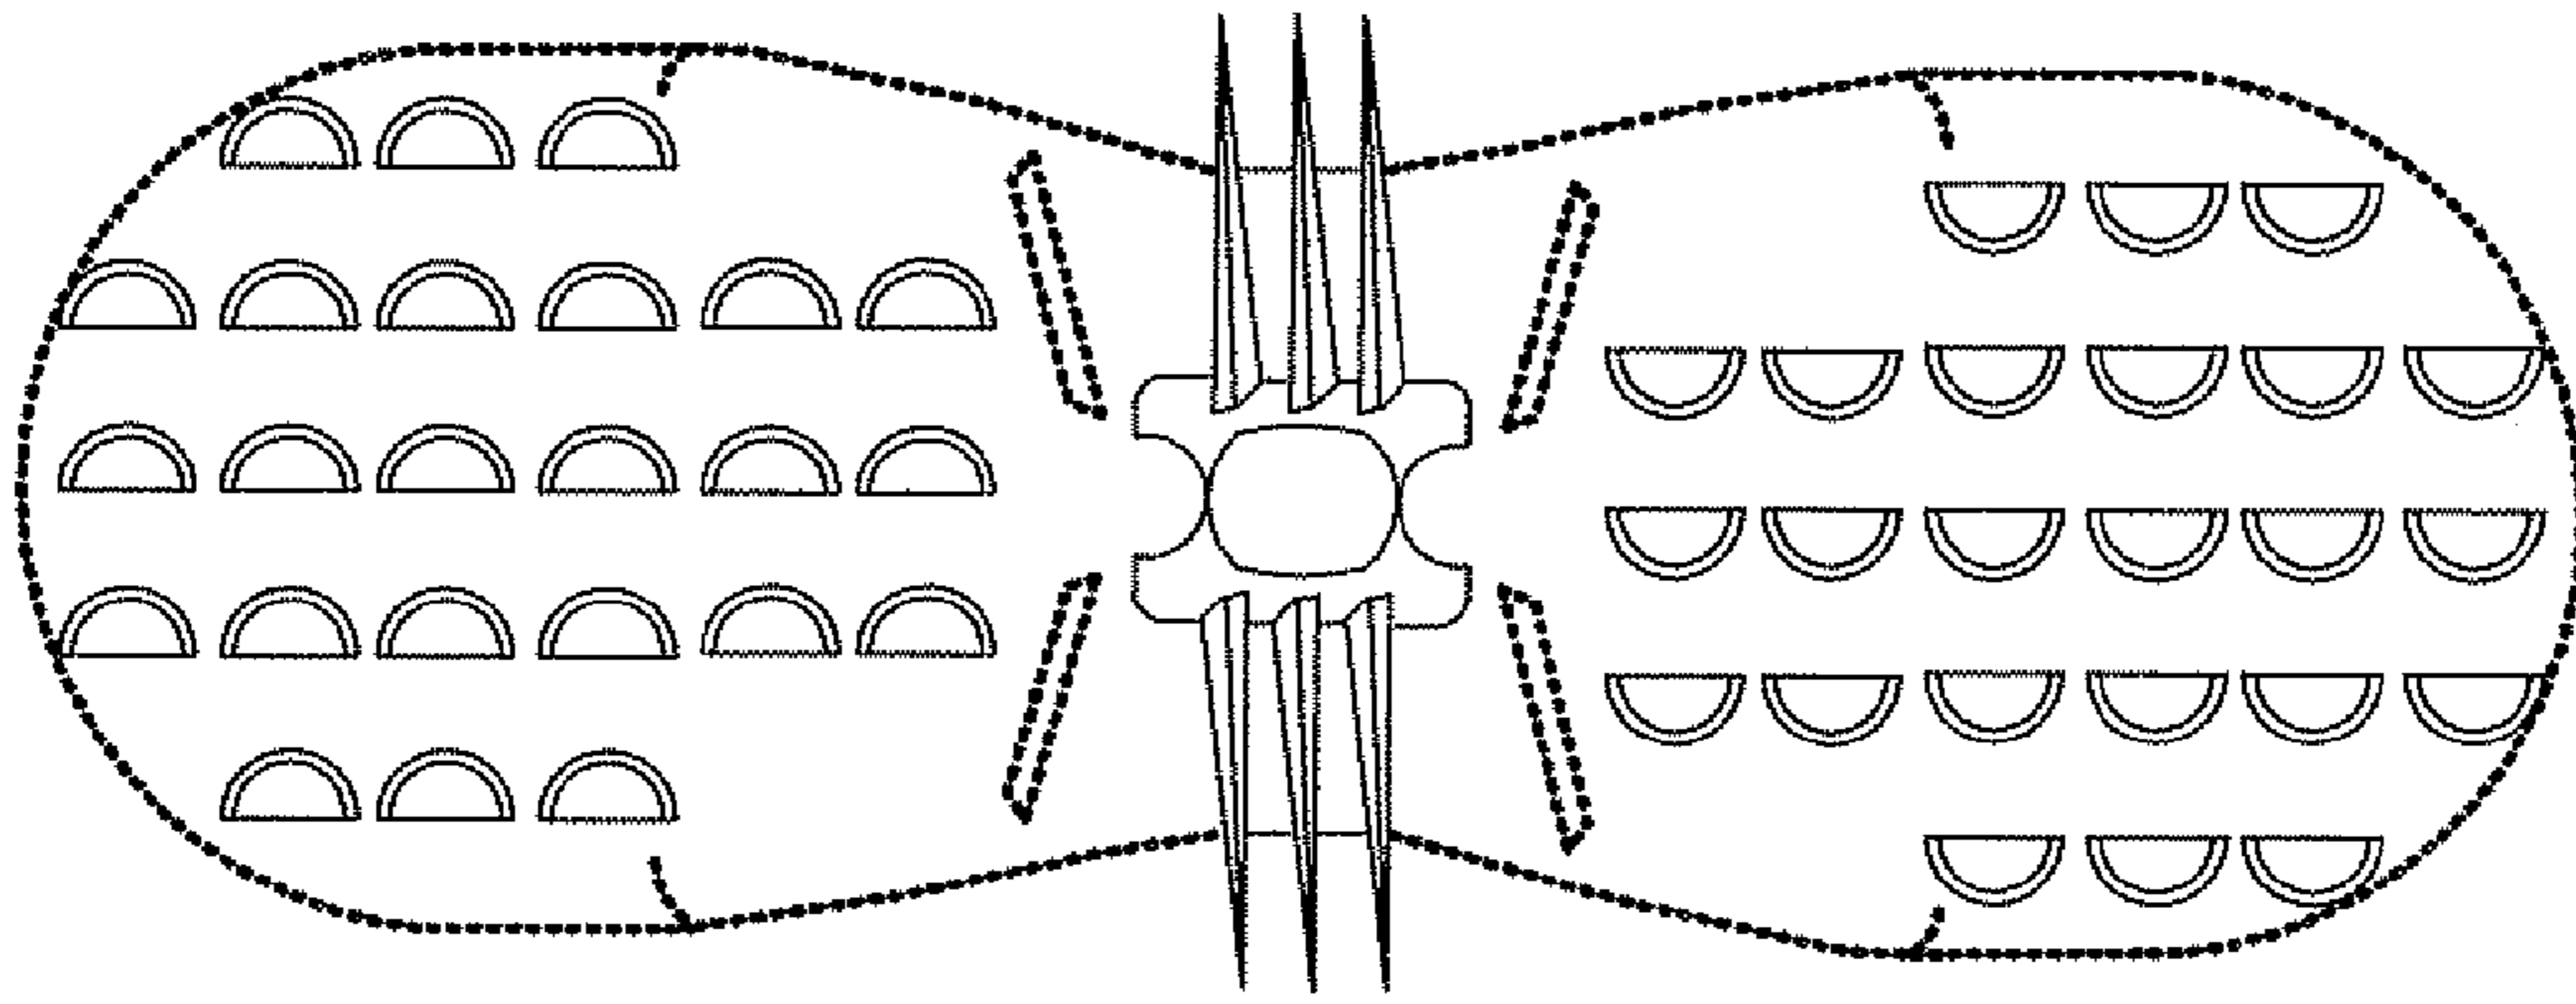


FIG. 2

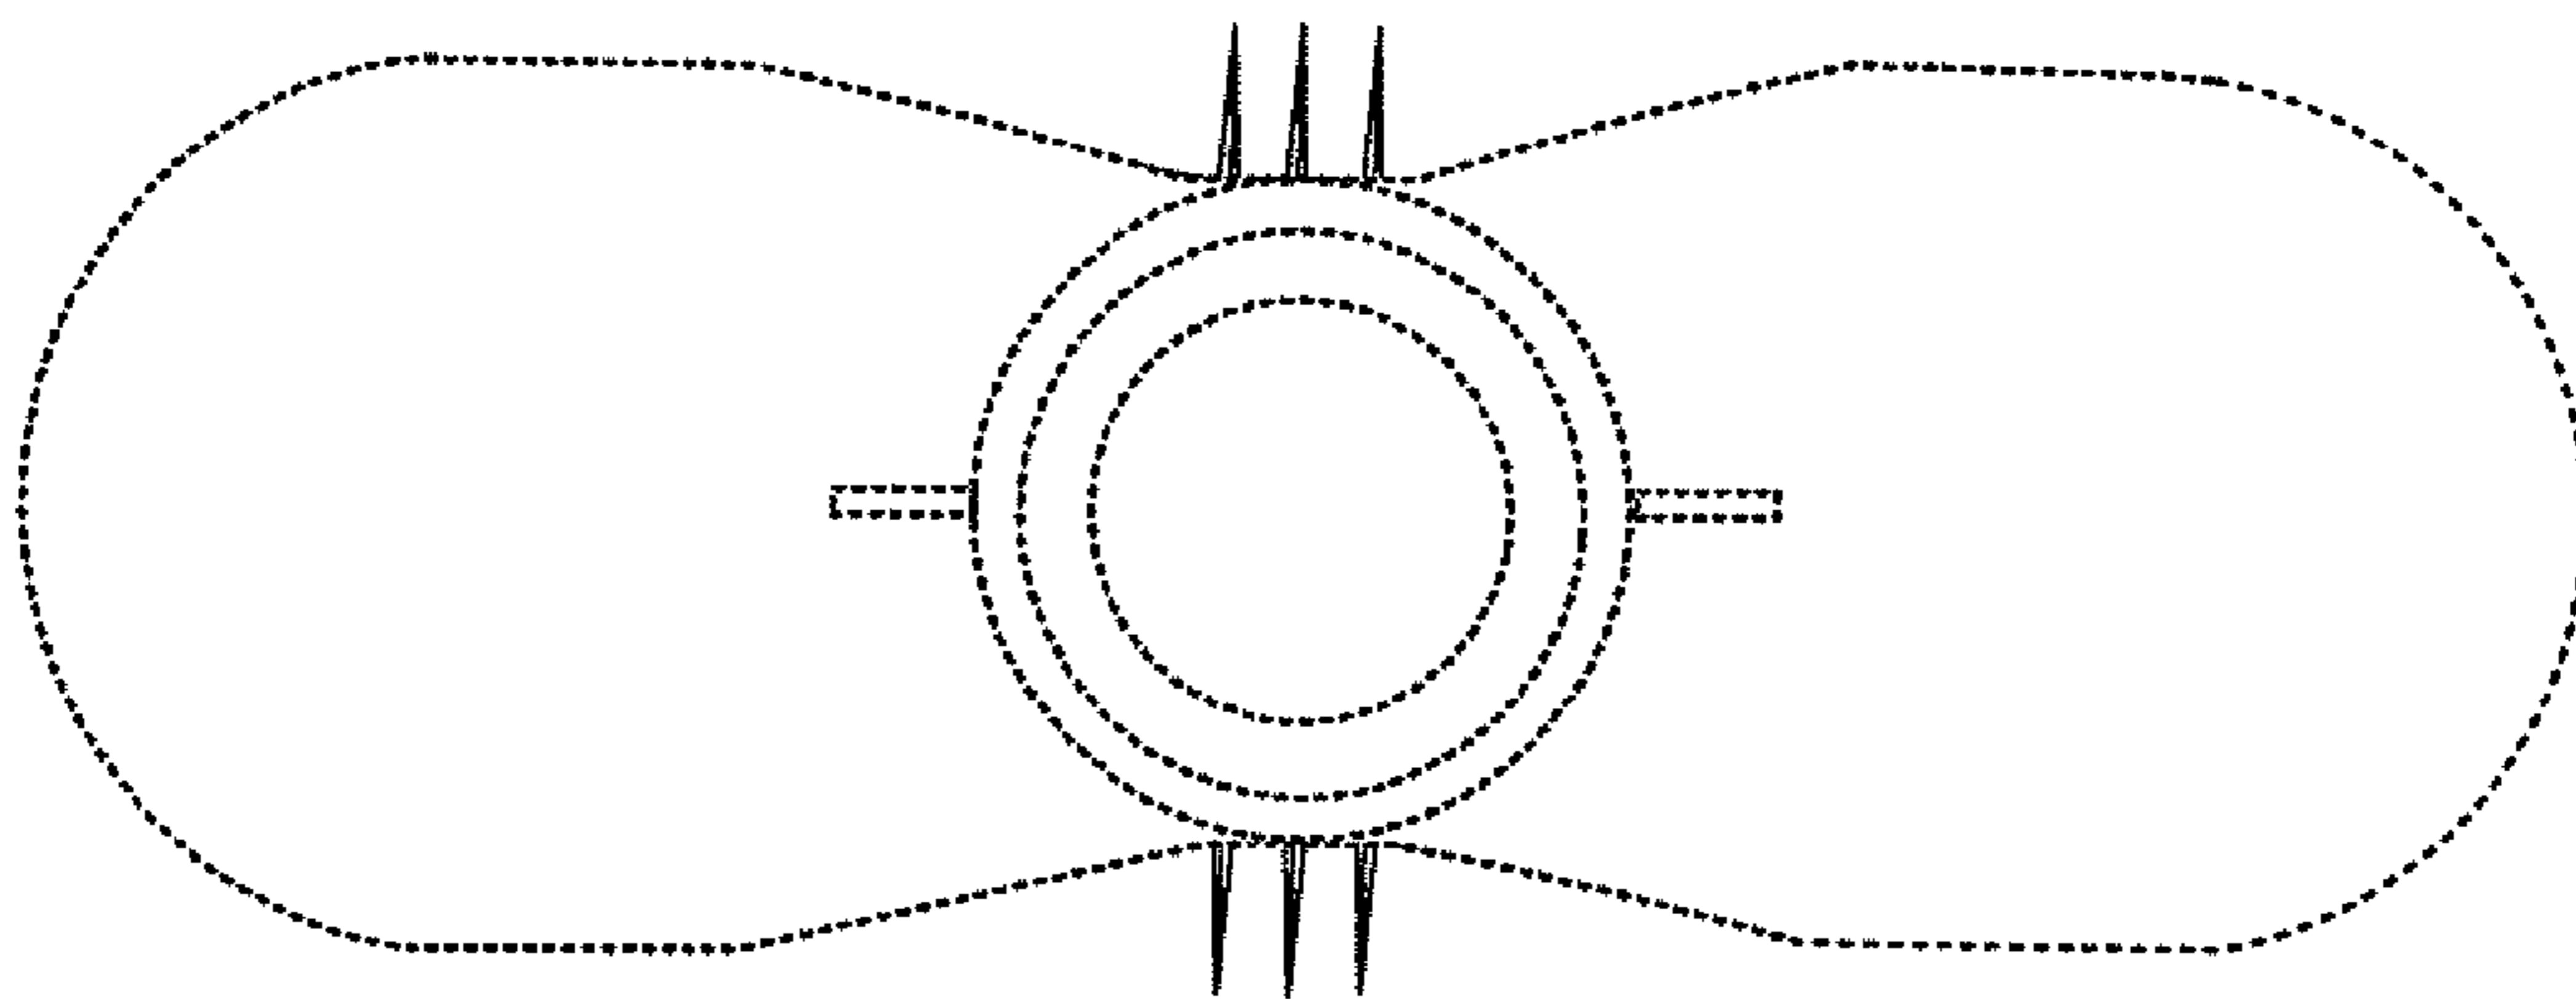


FIG. 3

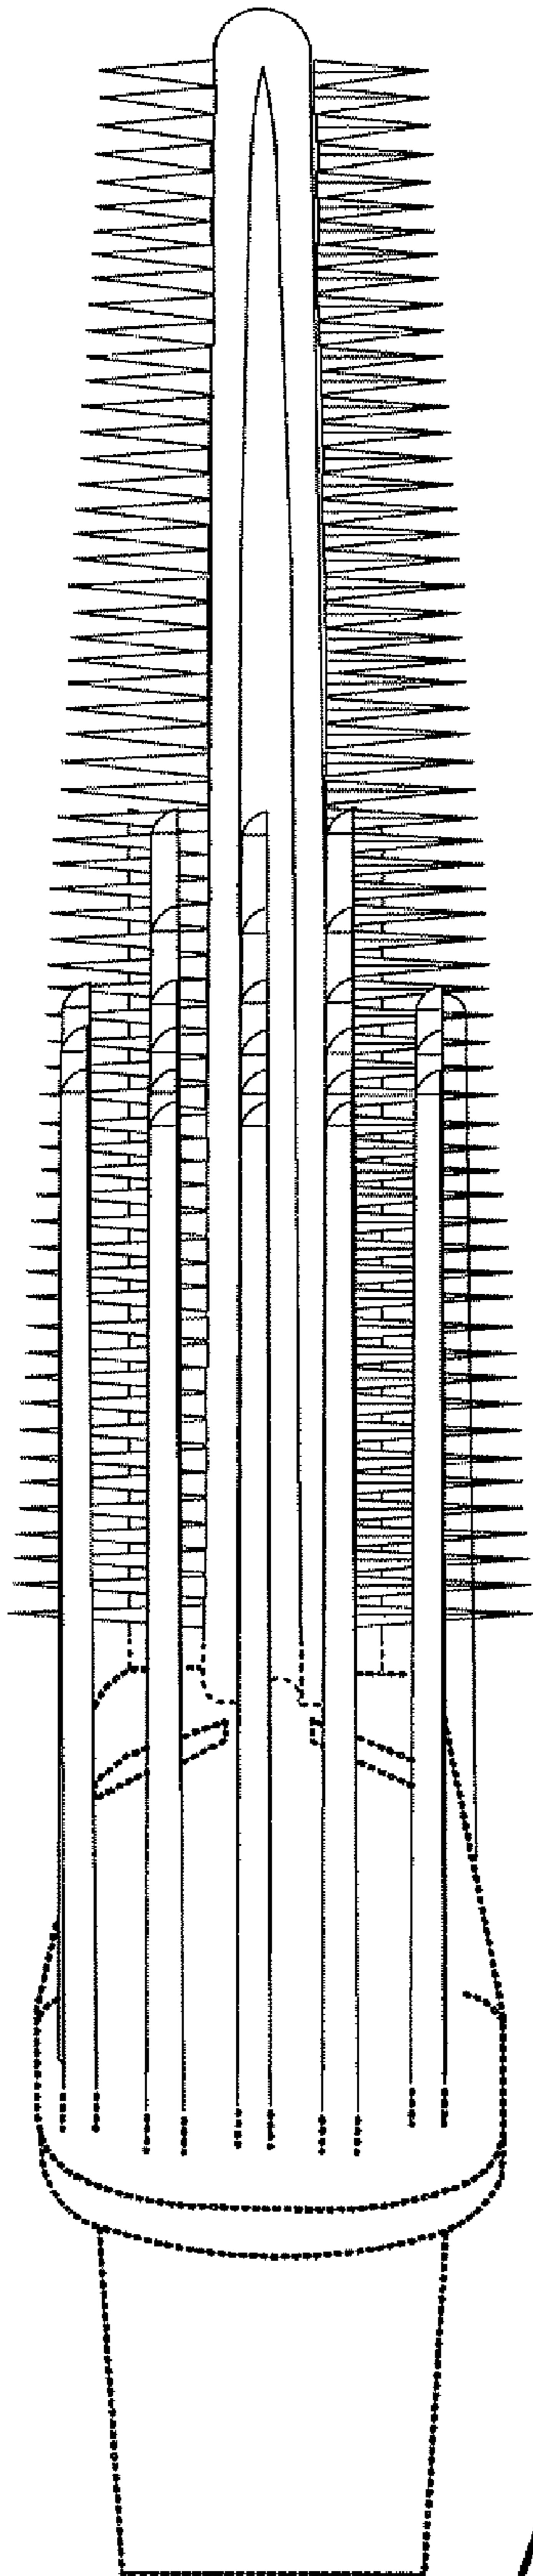


FIG. 4

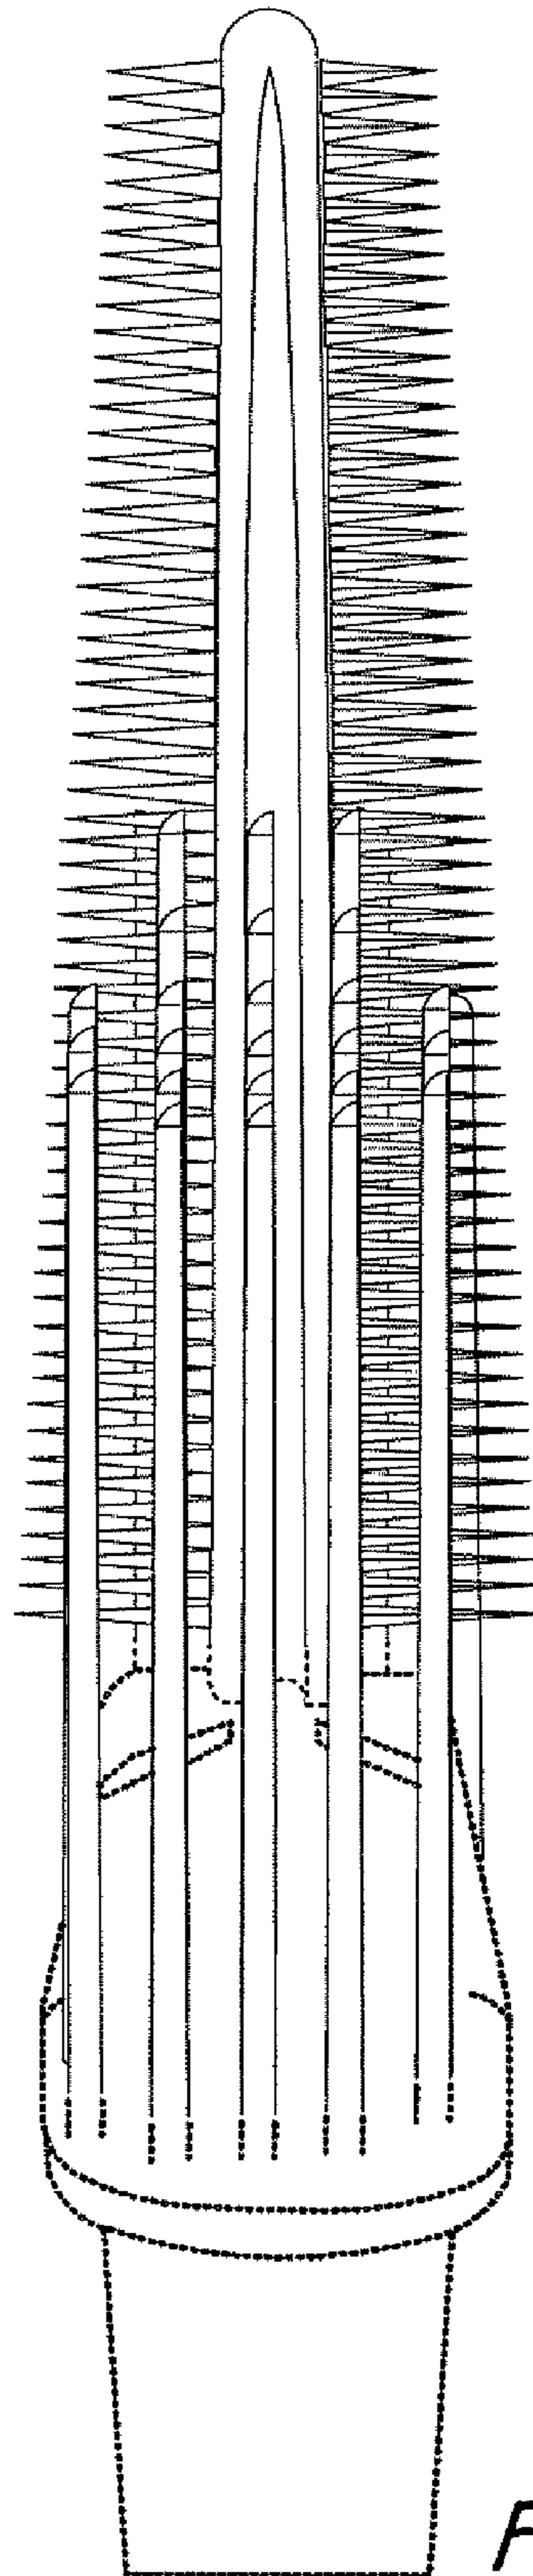


FIG. 5

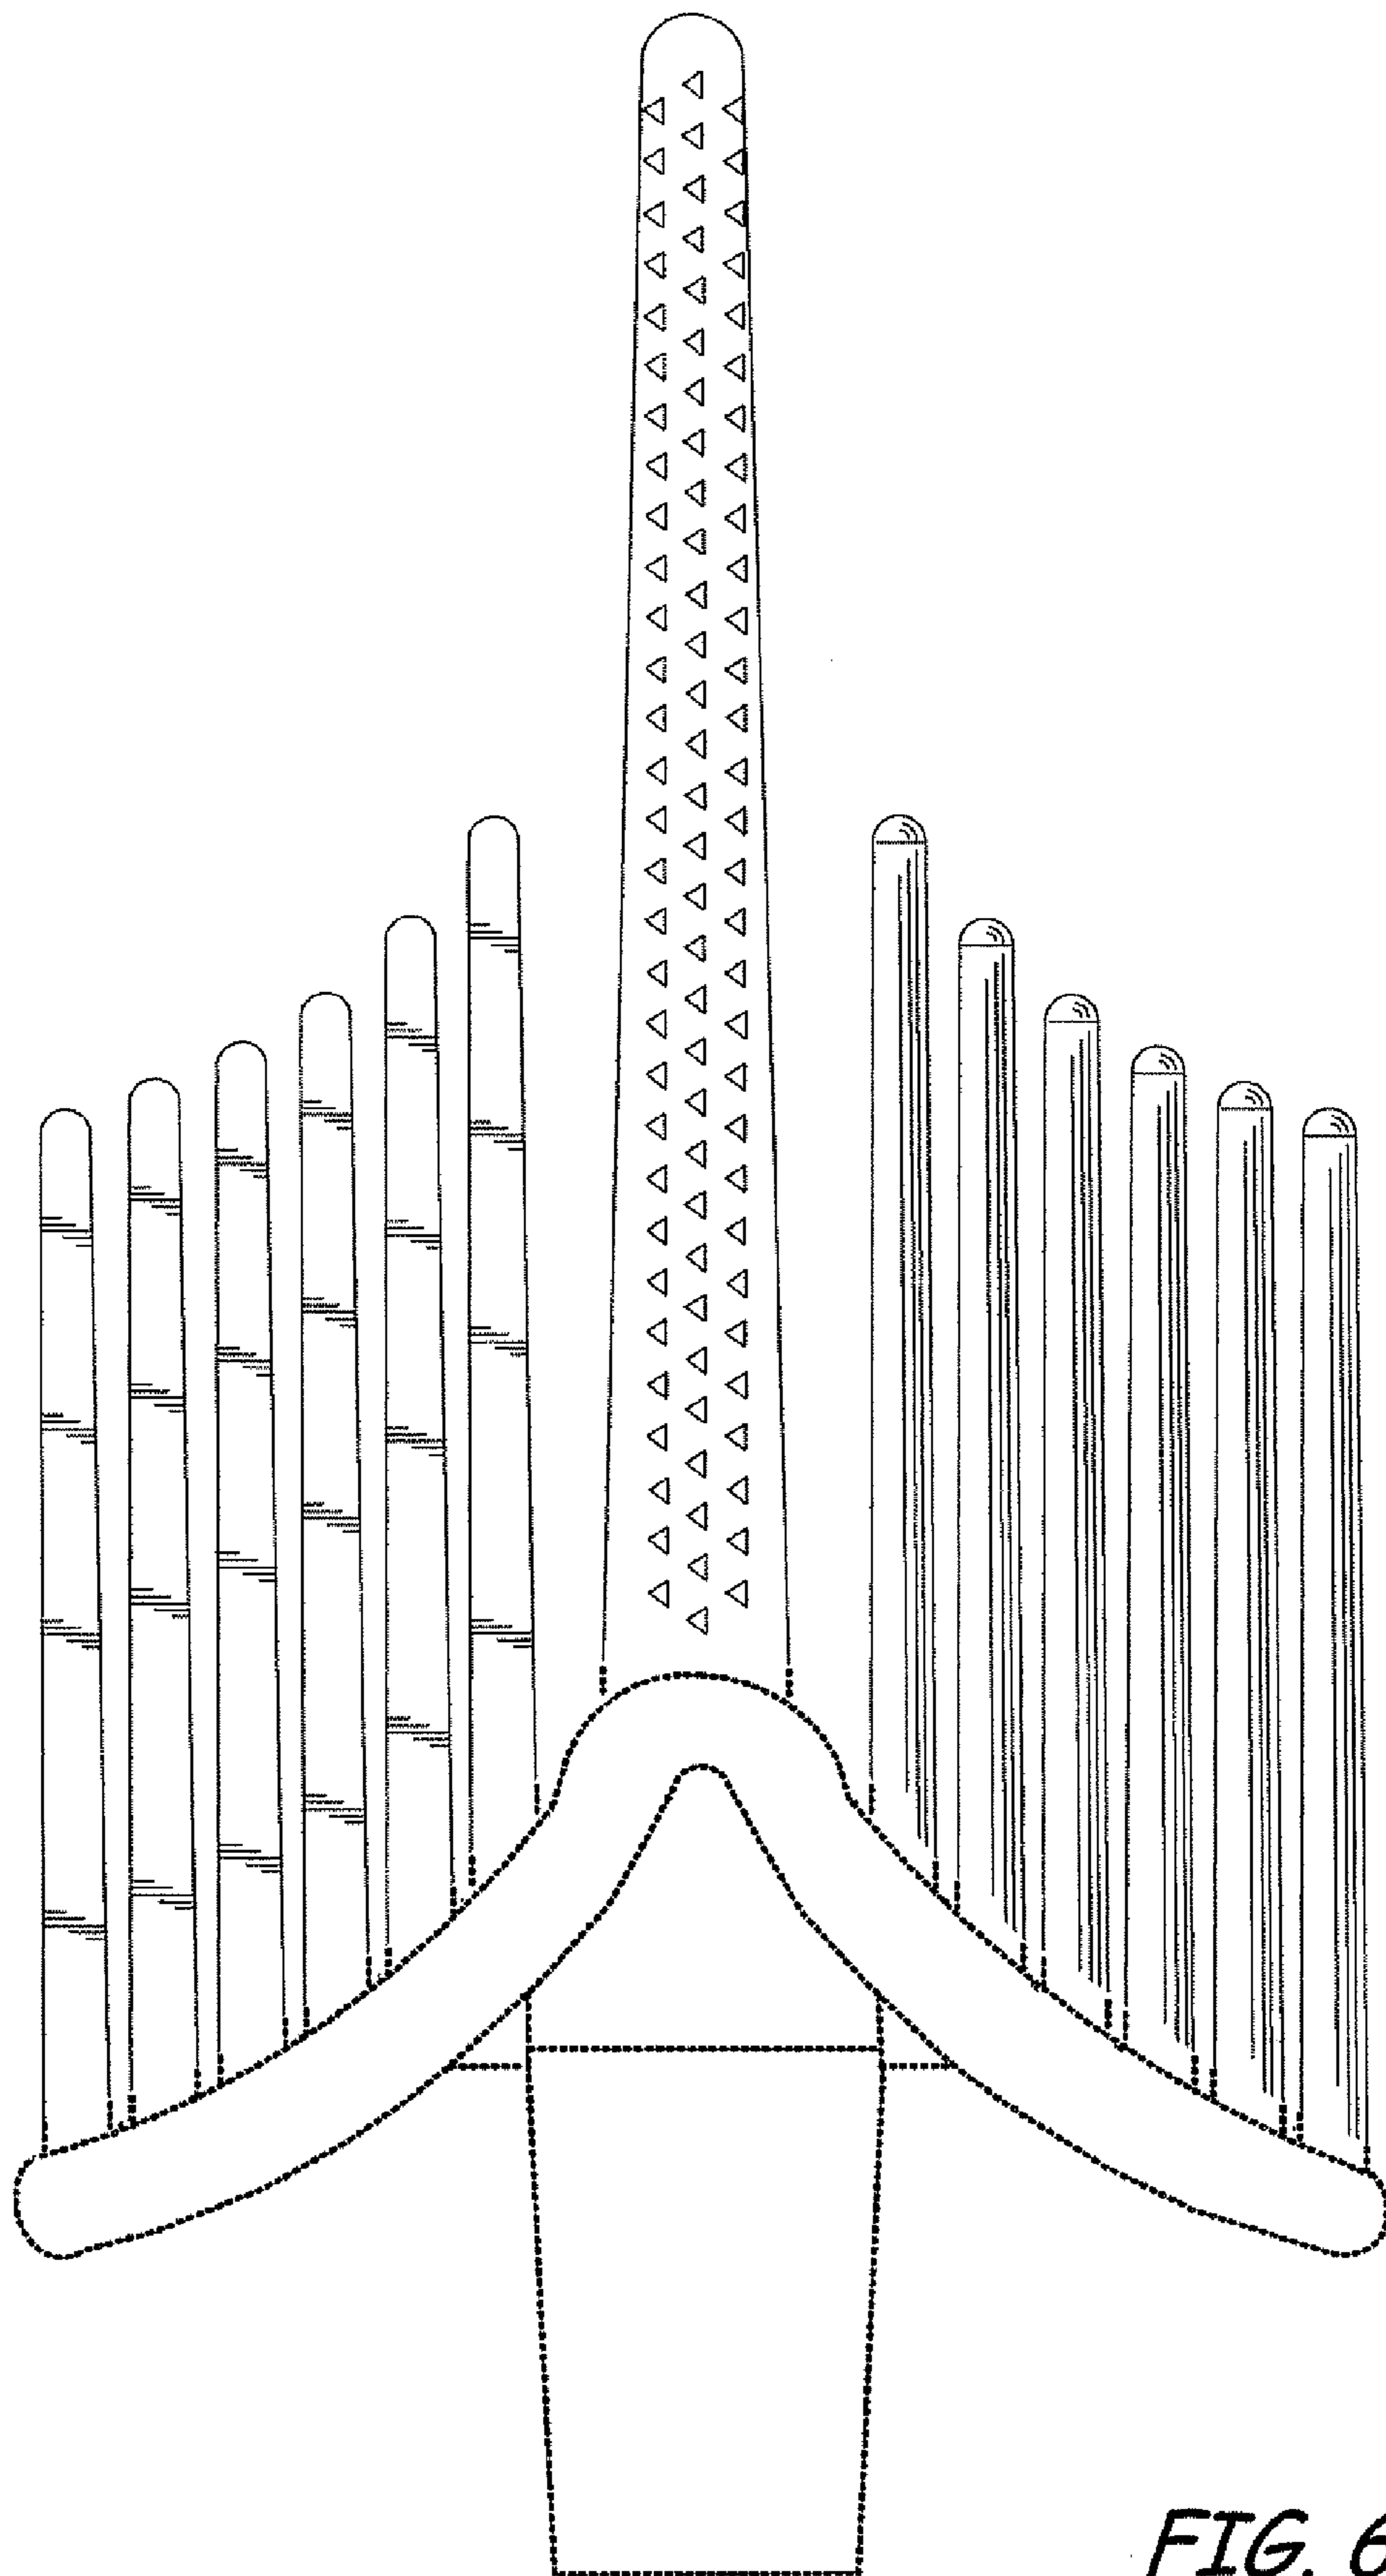


FIG. 6

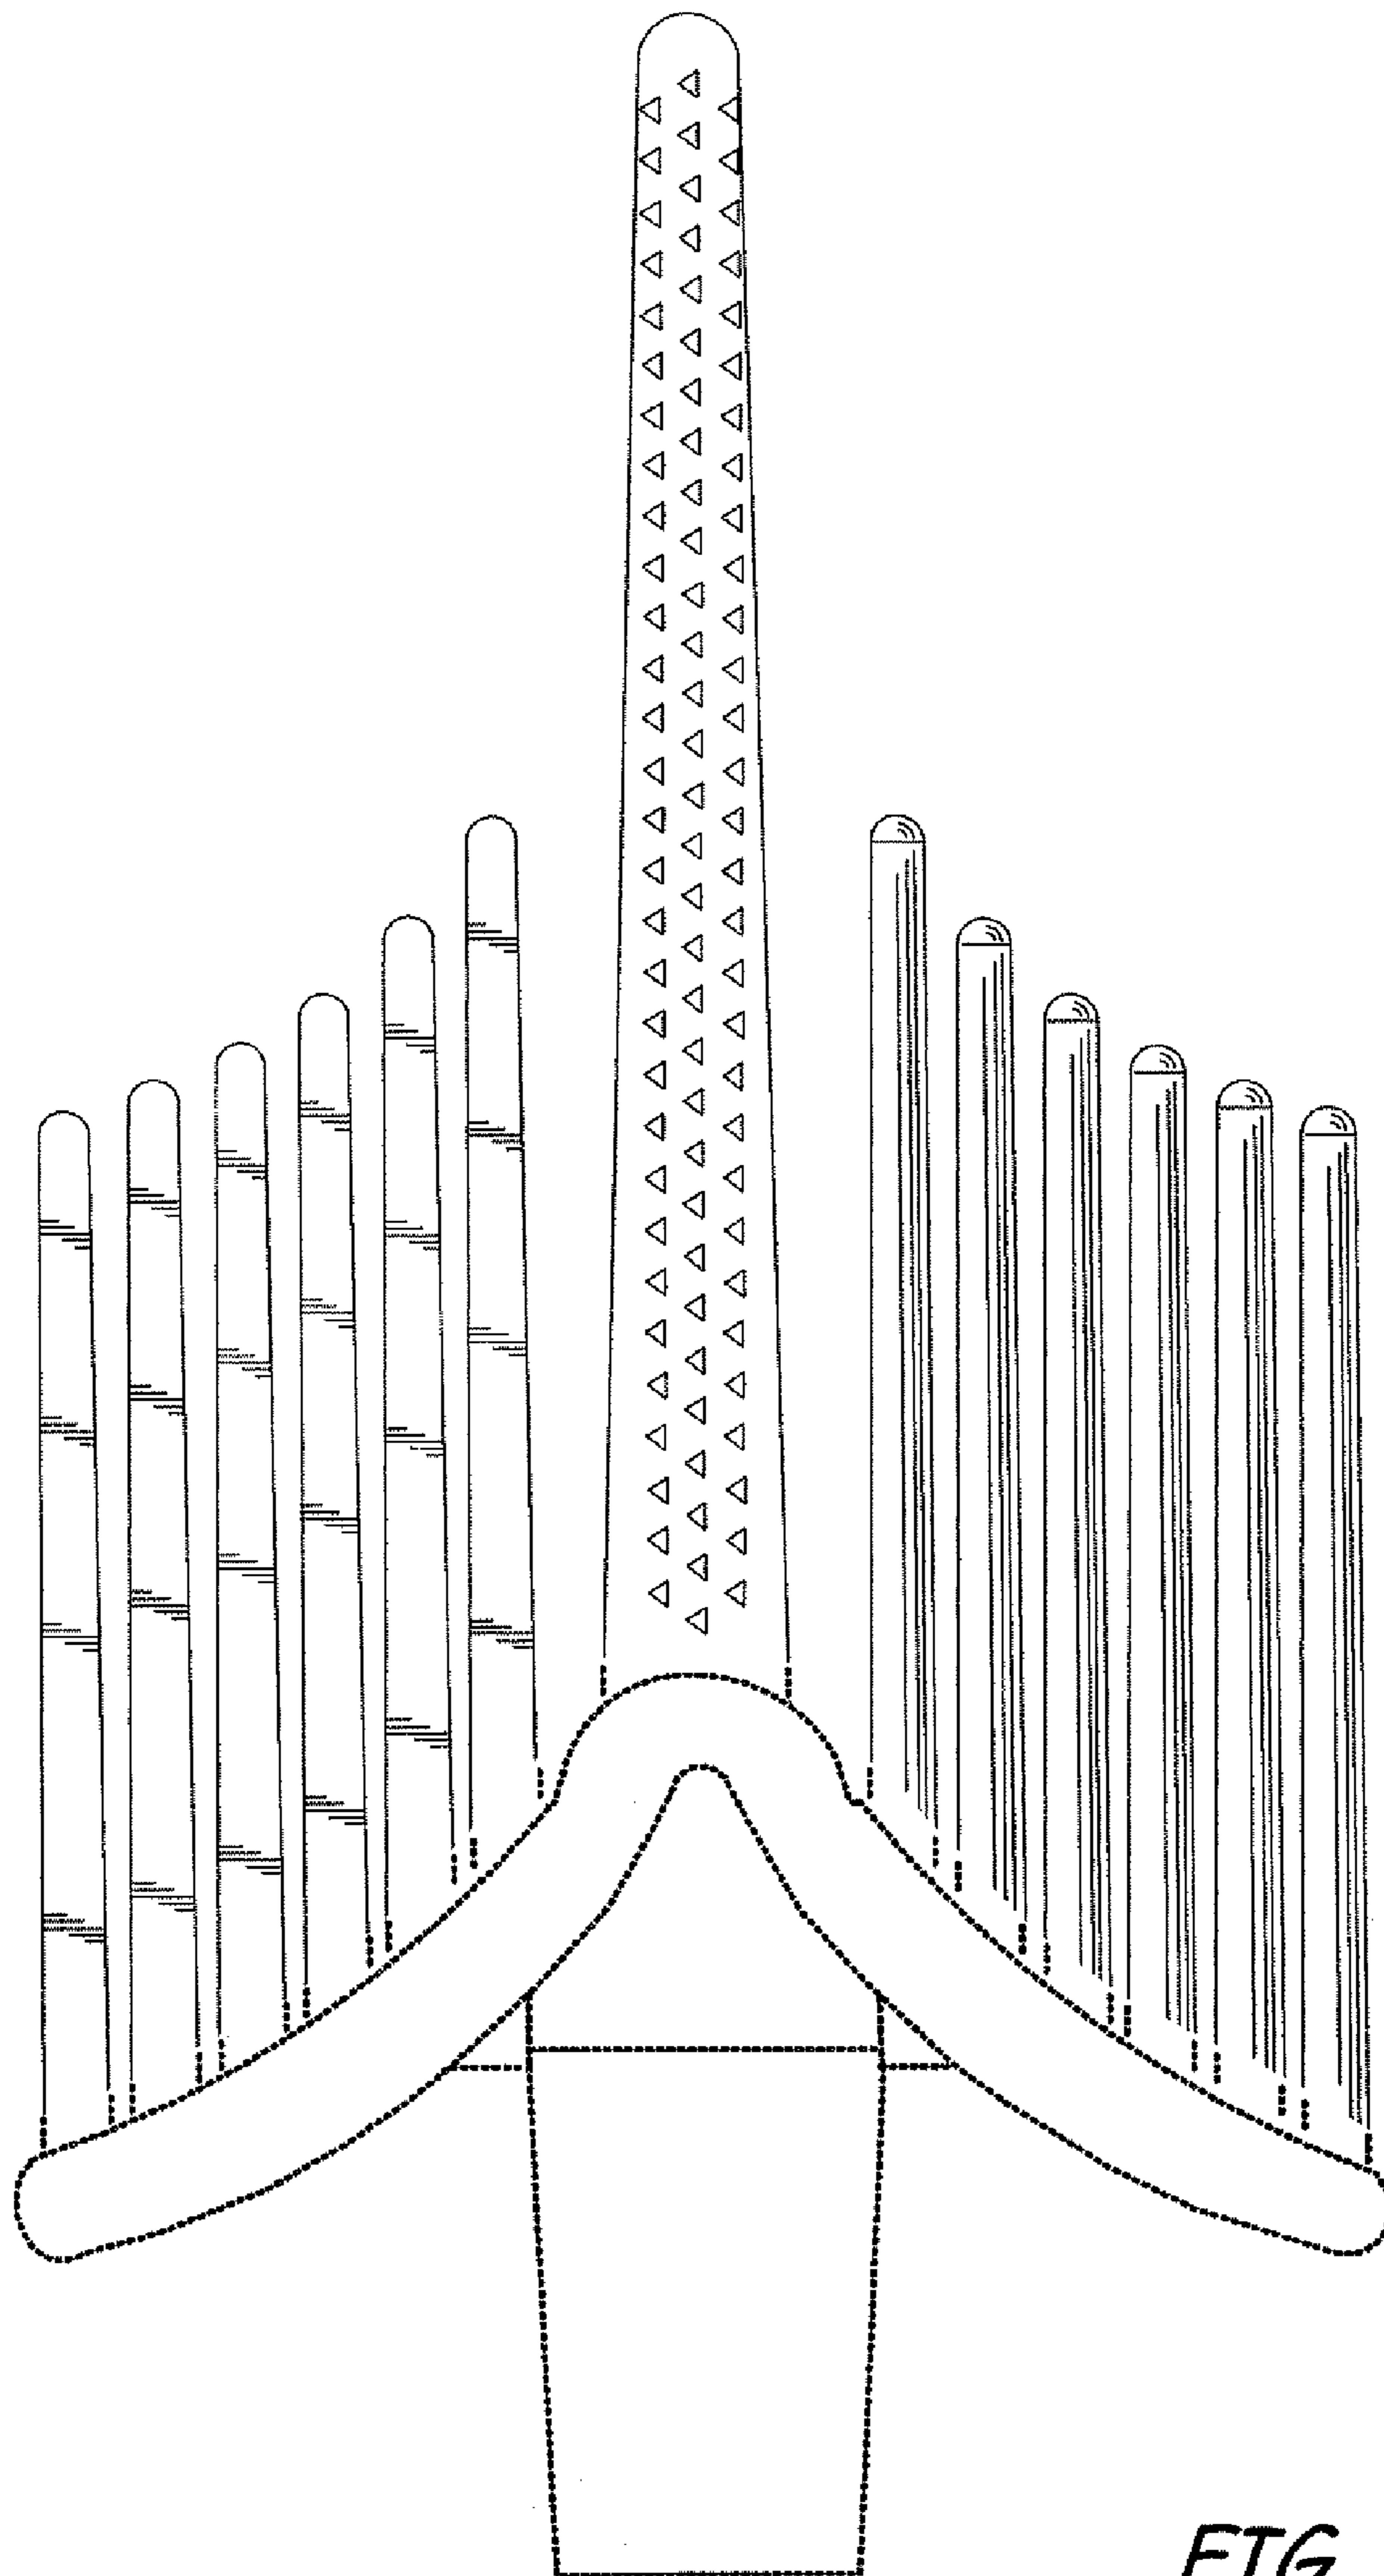


FIG. 7