



US00D560816S

(12) **United States Design Patent**  
**Talmer et al.**

(10) **Patent No.:** **US D560,816 S**  
(45) **Date of Patent:** **\*\* Jan. 29, 2008**

(54) **CUVETTE**

(75) Inventors: **Mark Talmer**, Pepperell, MA (US);  
**Paul C. Dahlstrom**, Hollis, NH (US)

(73) Assignee: **Biokit, S.A.**, Barcelona (ES)

(\*\*) Term: **14 Years**

(21) Appl. No.: **29/272,460**

(22) Filed: **Feb. 8, 2007**

(51) **LOC (8) Cl.** ..... **24-02**

(52) **U.S. Cl.** ..... **D24/224**

(58) **Field of Classification Search** ..... D24/117,  
D24/224; 422/61, 102, 104; 365/246; 435/296,  
435/299; 606/160

See application file for complete search history.

(56) **References Cited**

**U.S. PATENT DOCUMENTS**

D257,394 S *	10/1980	Reichler	.....	D24/117
D278,182 S *	3/1985	Aihara et al.	.....	D24/224
5,098,661 A *	3/1992	Froehlich et al.	.....	422/104
5,120,503 A *	6/1992	Hinckley et al.	.....	422/102
D330,428 S *	10/1992	Lewis et al.	.....	D24/224
D342,793 S *	12/1993	Balmer	.....	D24/224
D343,905 S *	2/1994	Nagata et al.	.....	D24/224
D344,138 S *	2/1994	Nagata	.....	D24/224
5,540,890 A	7/1996	Clark et al.		
5,571,479 A *	11/1996	Koch	.....	356/246
5,599,501 A	2/1997	Carey et al.		
D380,555 S *	7/1997	Kurosaki et al.	.....	D24/224
D401,700 S *	11/1998	Gray et al.	.....	D24/224
5,888,835 A	3/1999	Bushnell et al.		
5,985,671 A	11/1999	Leistner et al.		
D431,299 S *	9/2000	Lammie	.....	D24/224
6,149,872 A	11/2000	Mack et al.		

6,413,420 B1	7/2002	Foy et al.
6,562,239 B2	5/2003	Foy et al.
2003/0197799 A1	10/2003	Achter et al.
2005/0271550 A1	12/2005	Talmer et al.

**FOREIGN PATENT DOCUMENTS**

EP	0 712 000	9/1995
EP	0 806 665	5/1997
EP	0 889 328	1/1999
JP	1028561	1/1989
JP	8146001	6/1996
JP	10123136	5/1998
JP	2000111557	4/2000
JP	2001116752	4/2001
WO	WO98/18008	4/1998
WO	WO 03/086637	10/2003
WO	WO 05/124365	12/2005

\* cited by examiner

*Primary Examiner*—Robert A. Delehanty

*Assistant Examiner*—Mark Cavanna

(74) *Attorney, Agent, or Firm*—Kirkpatrick & Lockhart  
Preston Gates Ellis LLP

(57) **CLAIM**

The ornamental design for a cuvette, as shown and described.

**DESCRIPTION**

FIG. 1 is a side perspective view of the cuvette according to the invention;


FIG. 2 is a top plan view of the cuvette thereof;

FIG. 3 is a bottom plan view of the cuvette thereof;

FIG. 4 is a side plan view of the cuvette thereof; and,

FIG. 5 is a side plan view of the cuvette thereof.

**1 Claim, 2 Drawing Sheets**

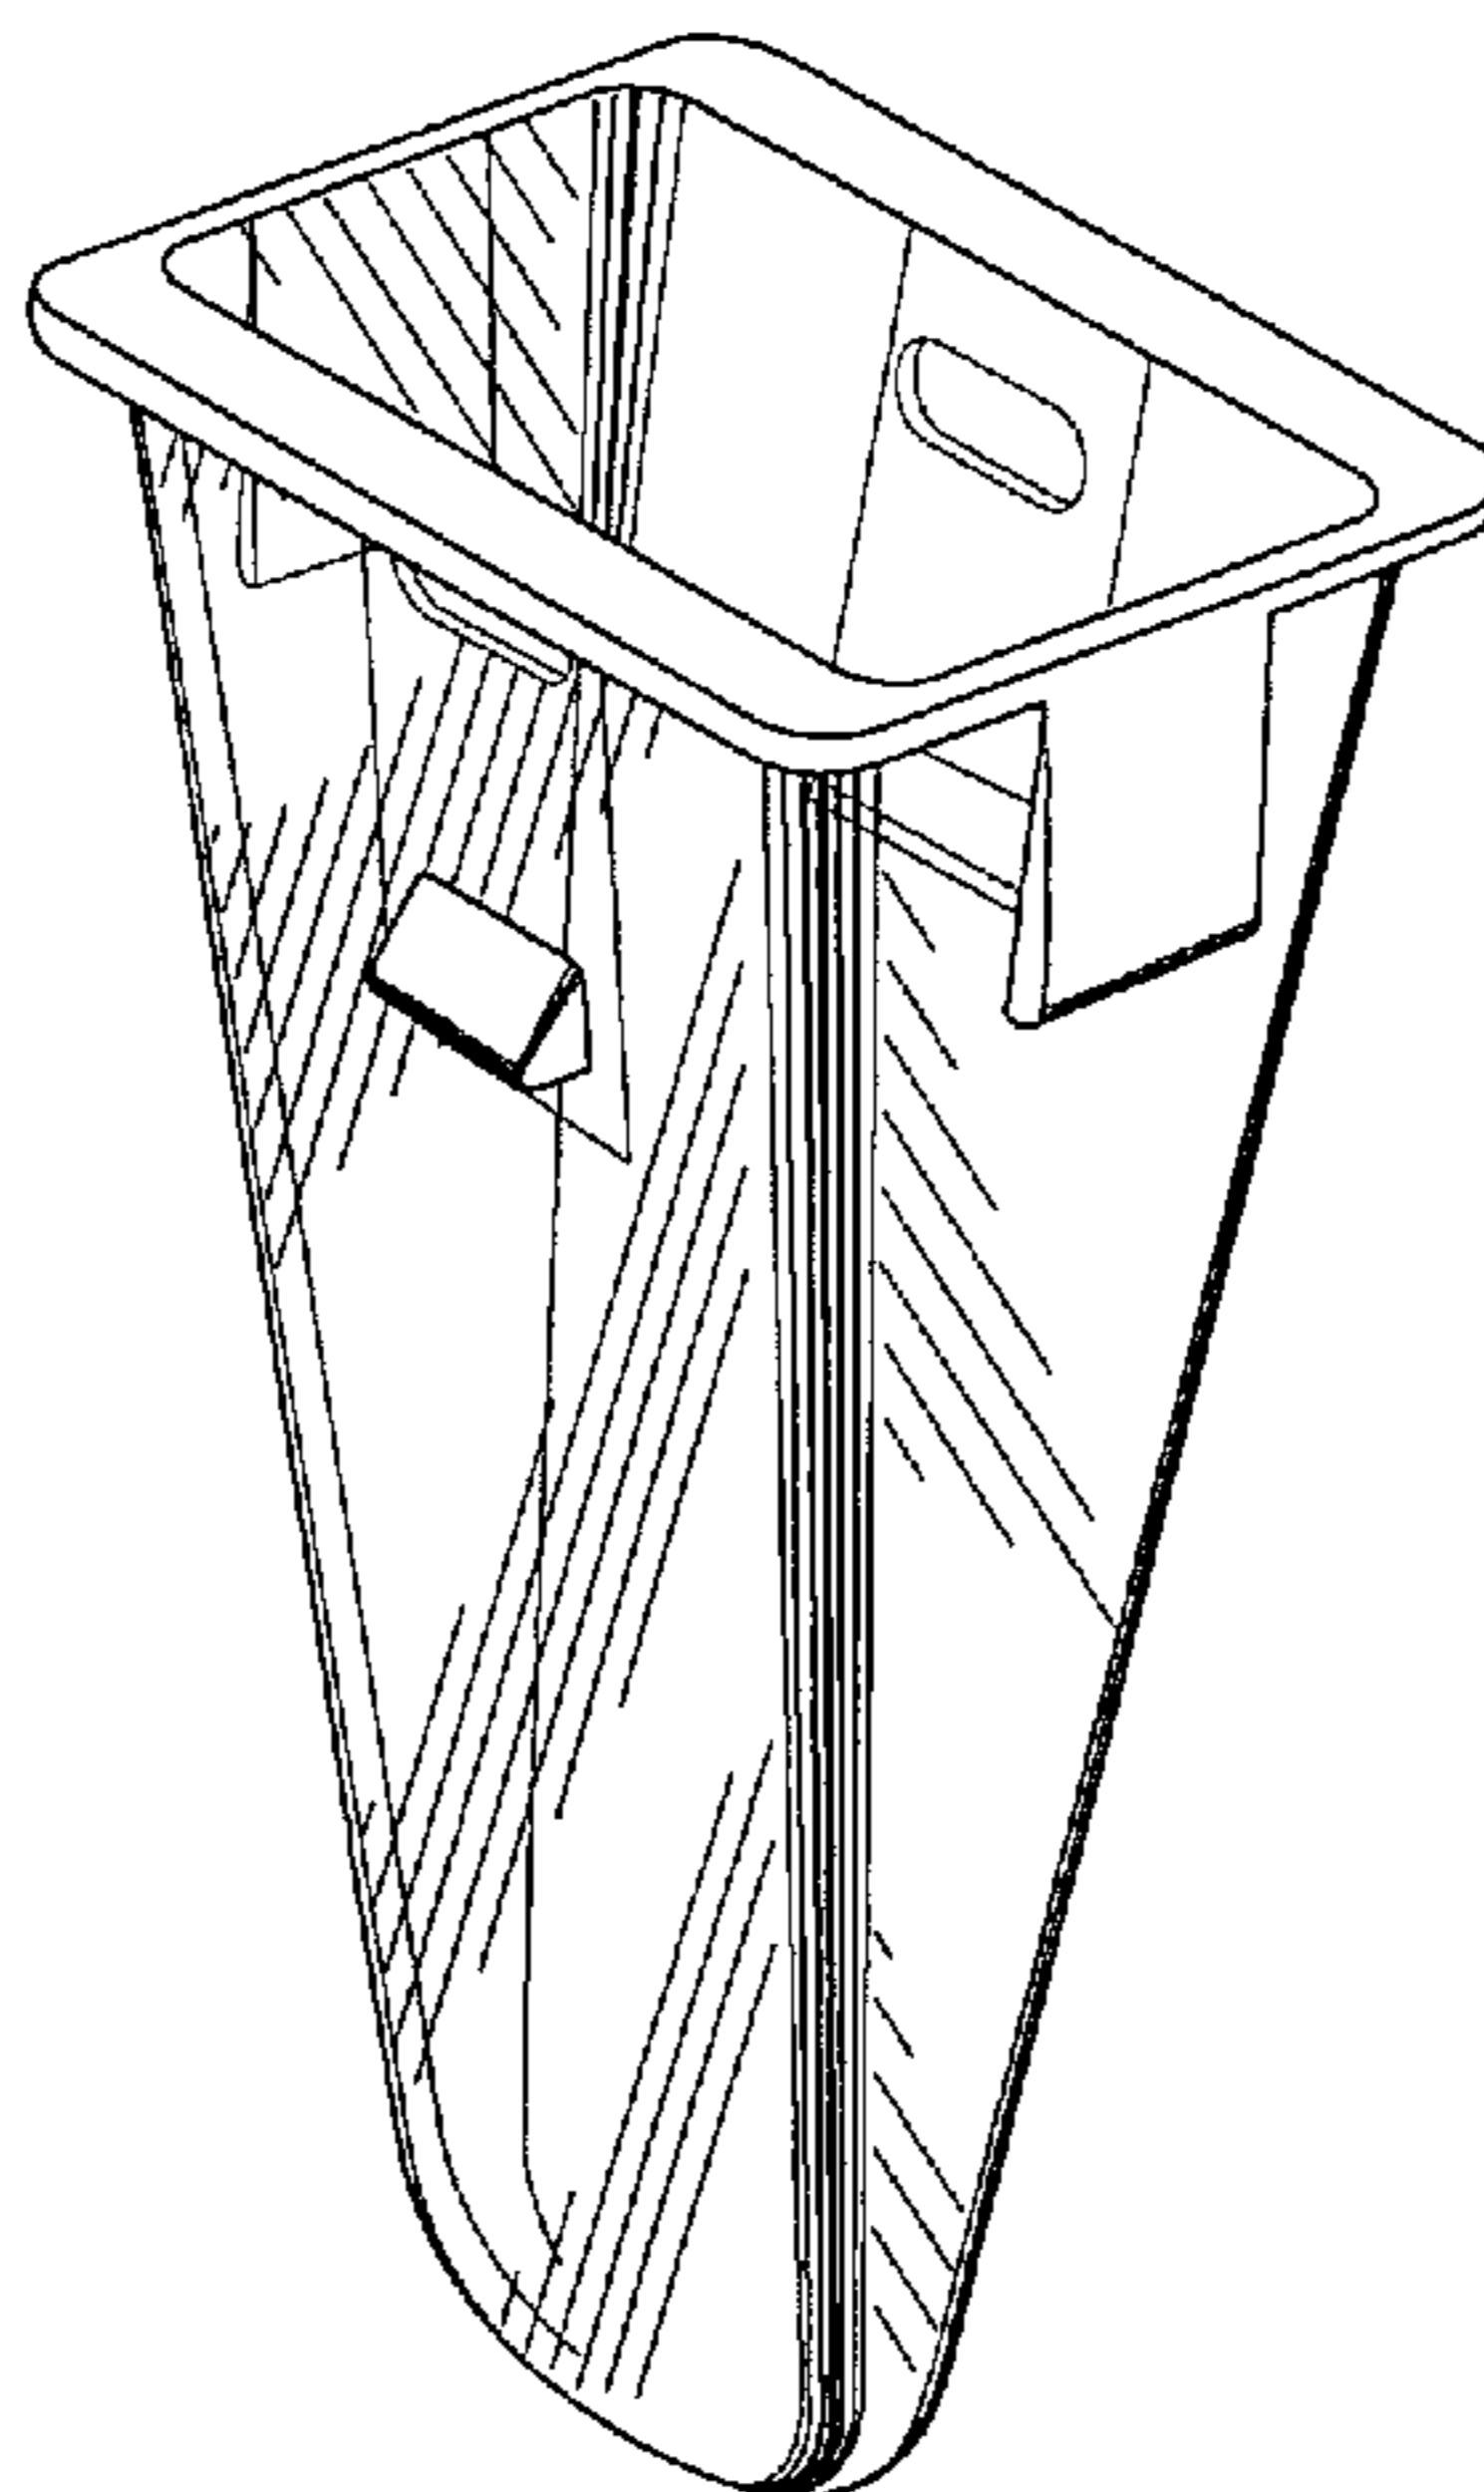

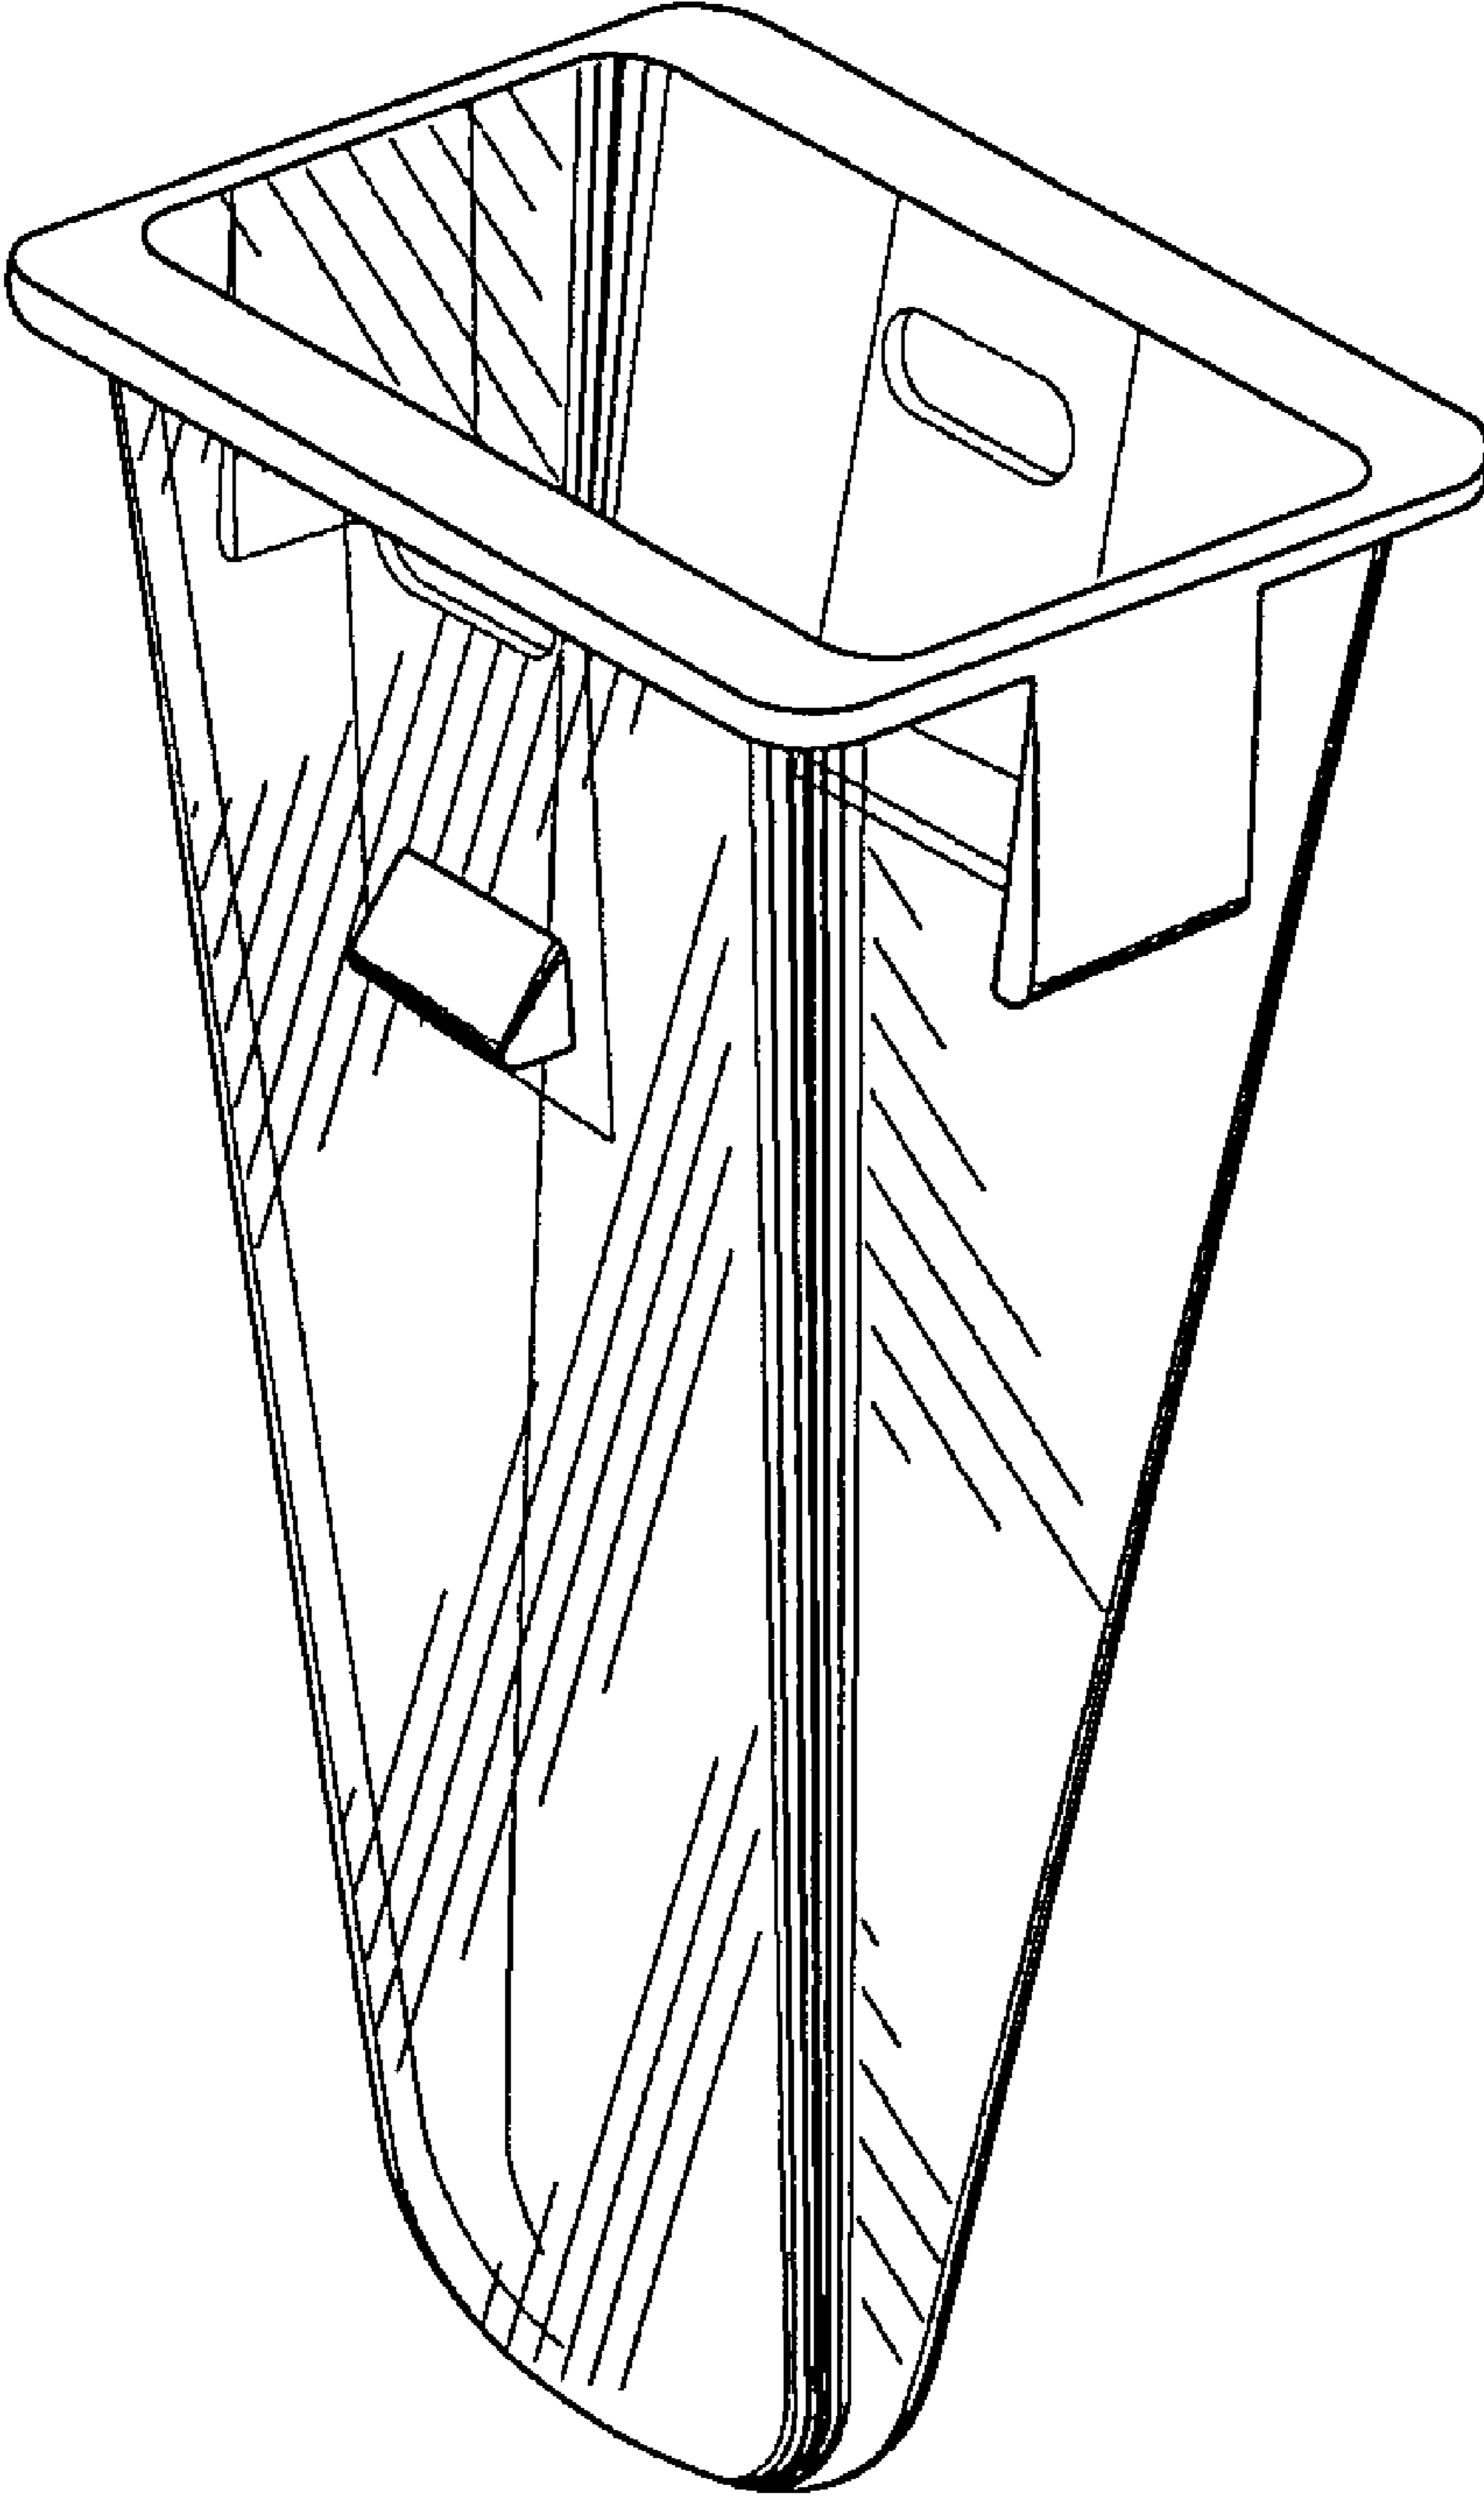


Fig. 1

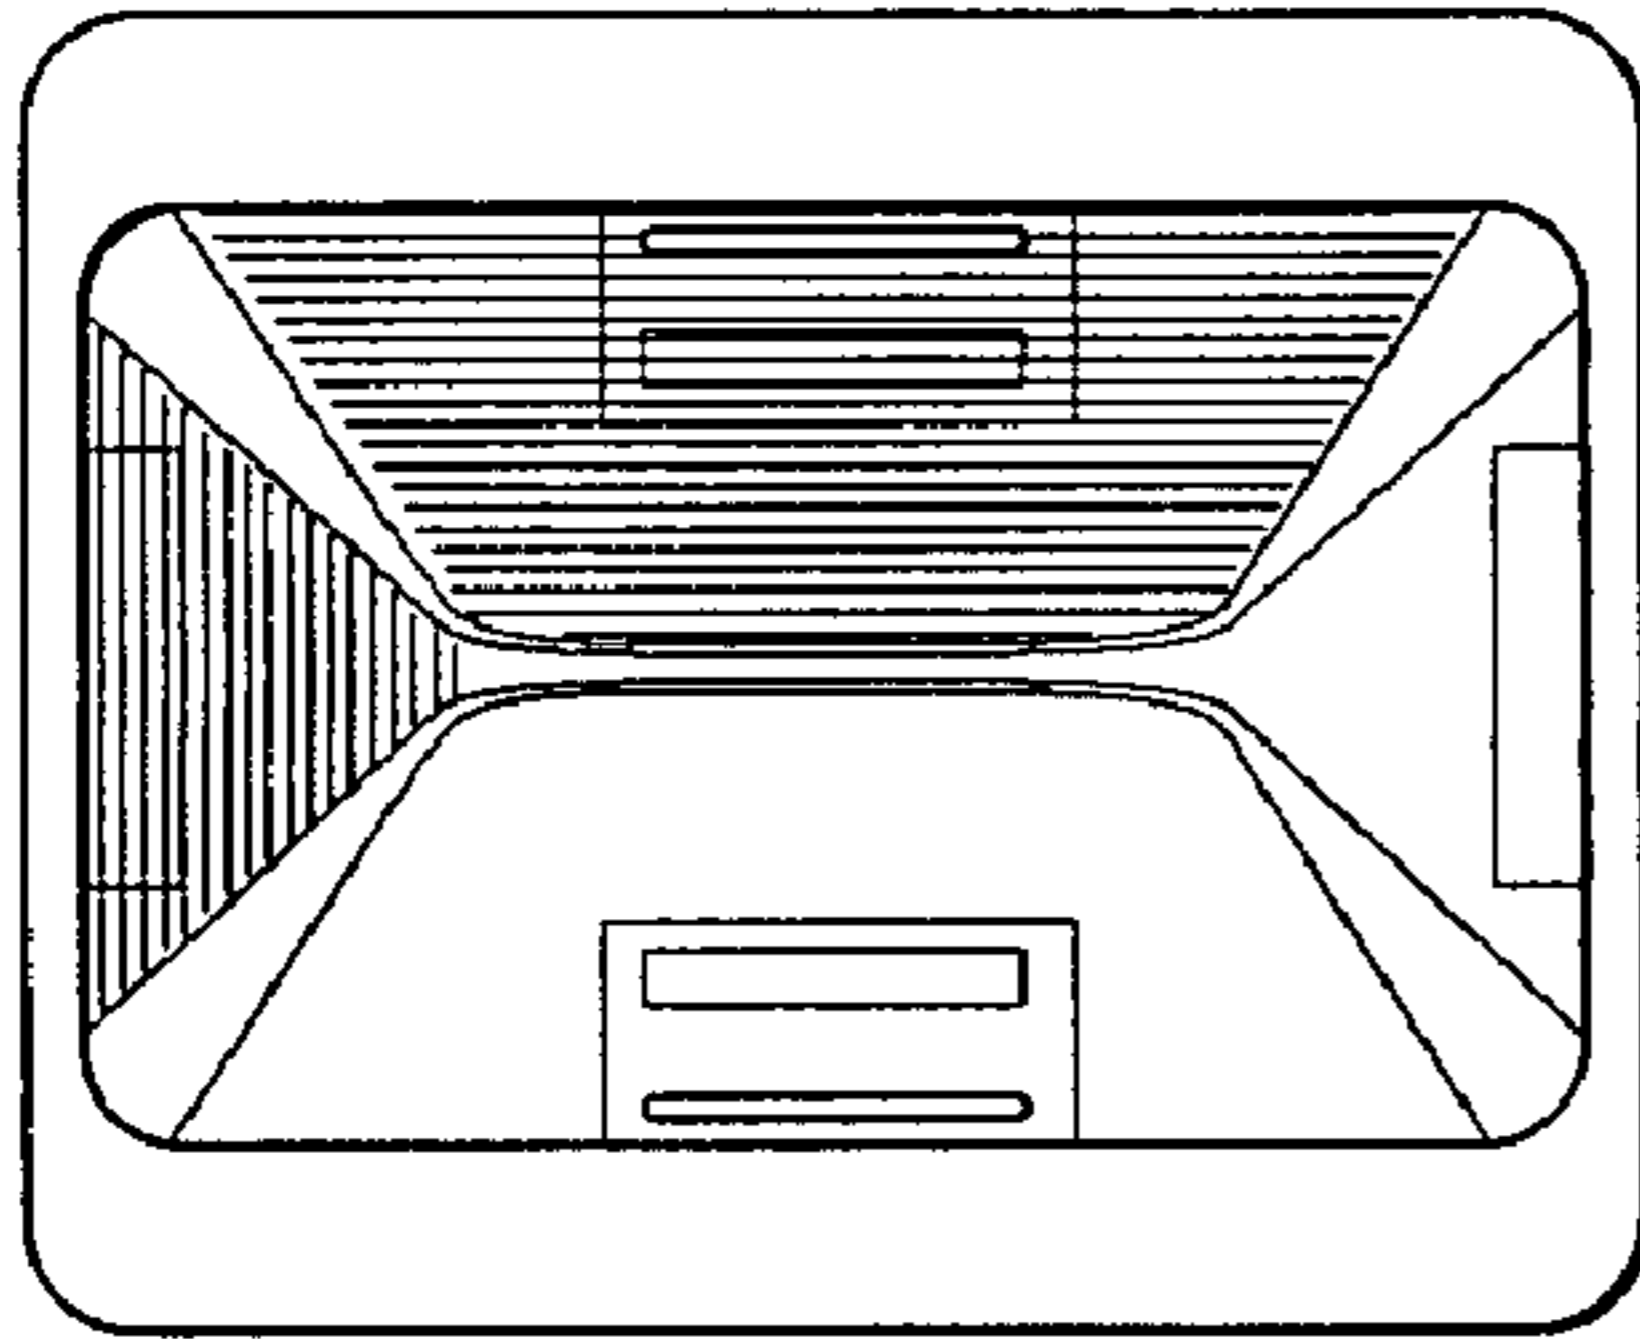


Fig. 2

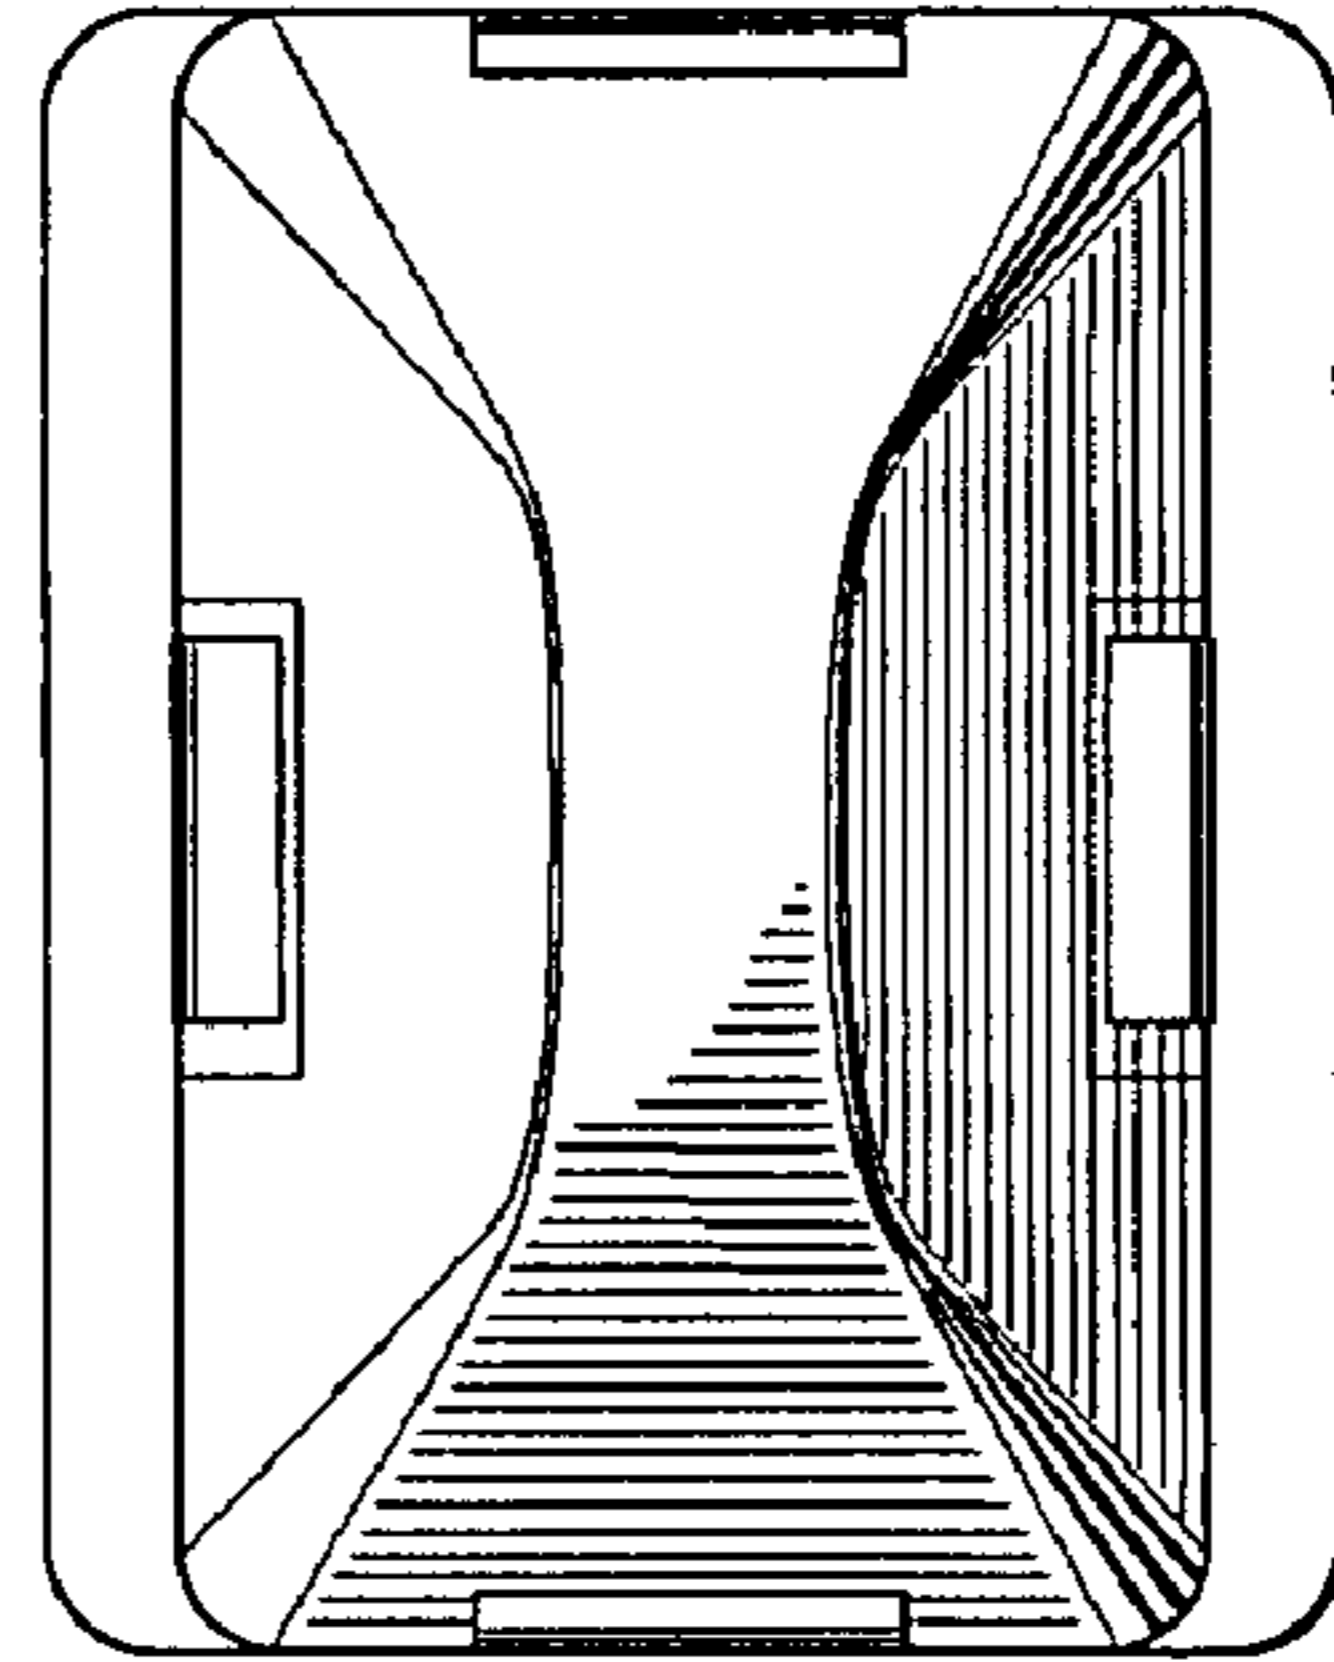


Fig. 3

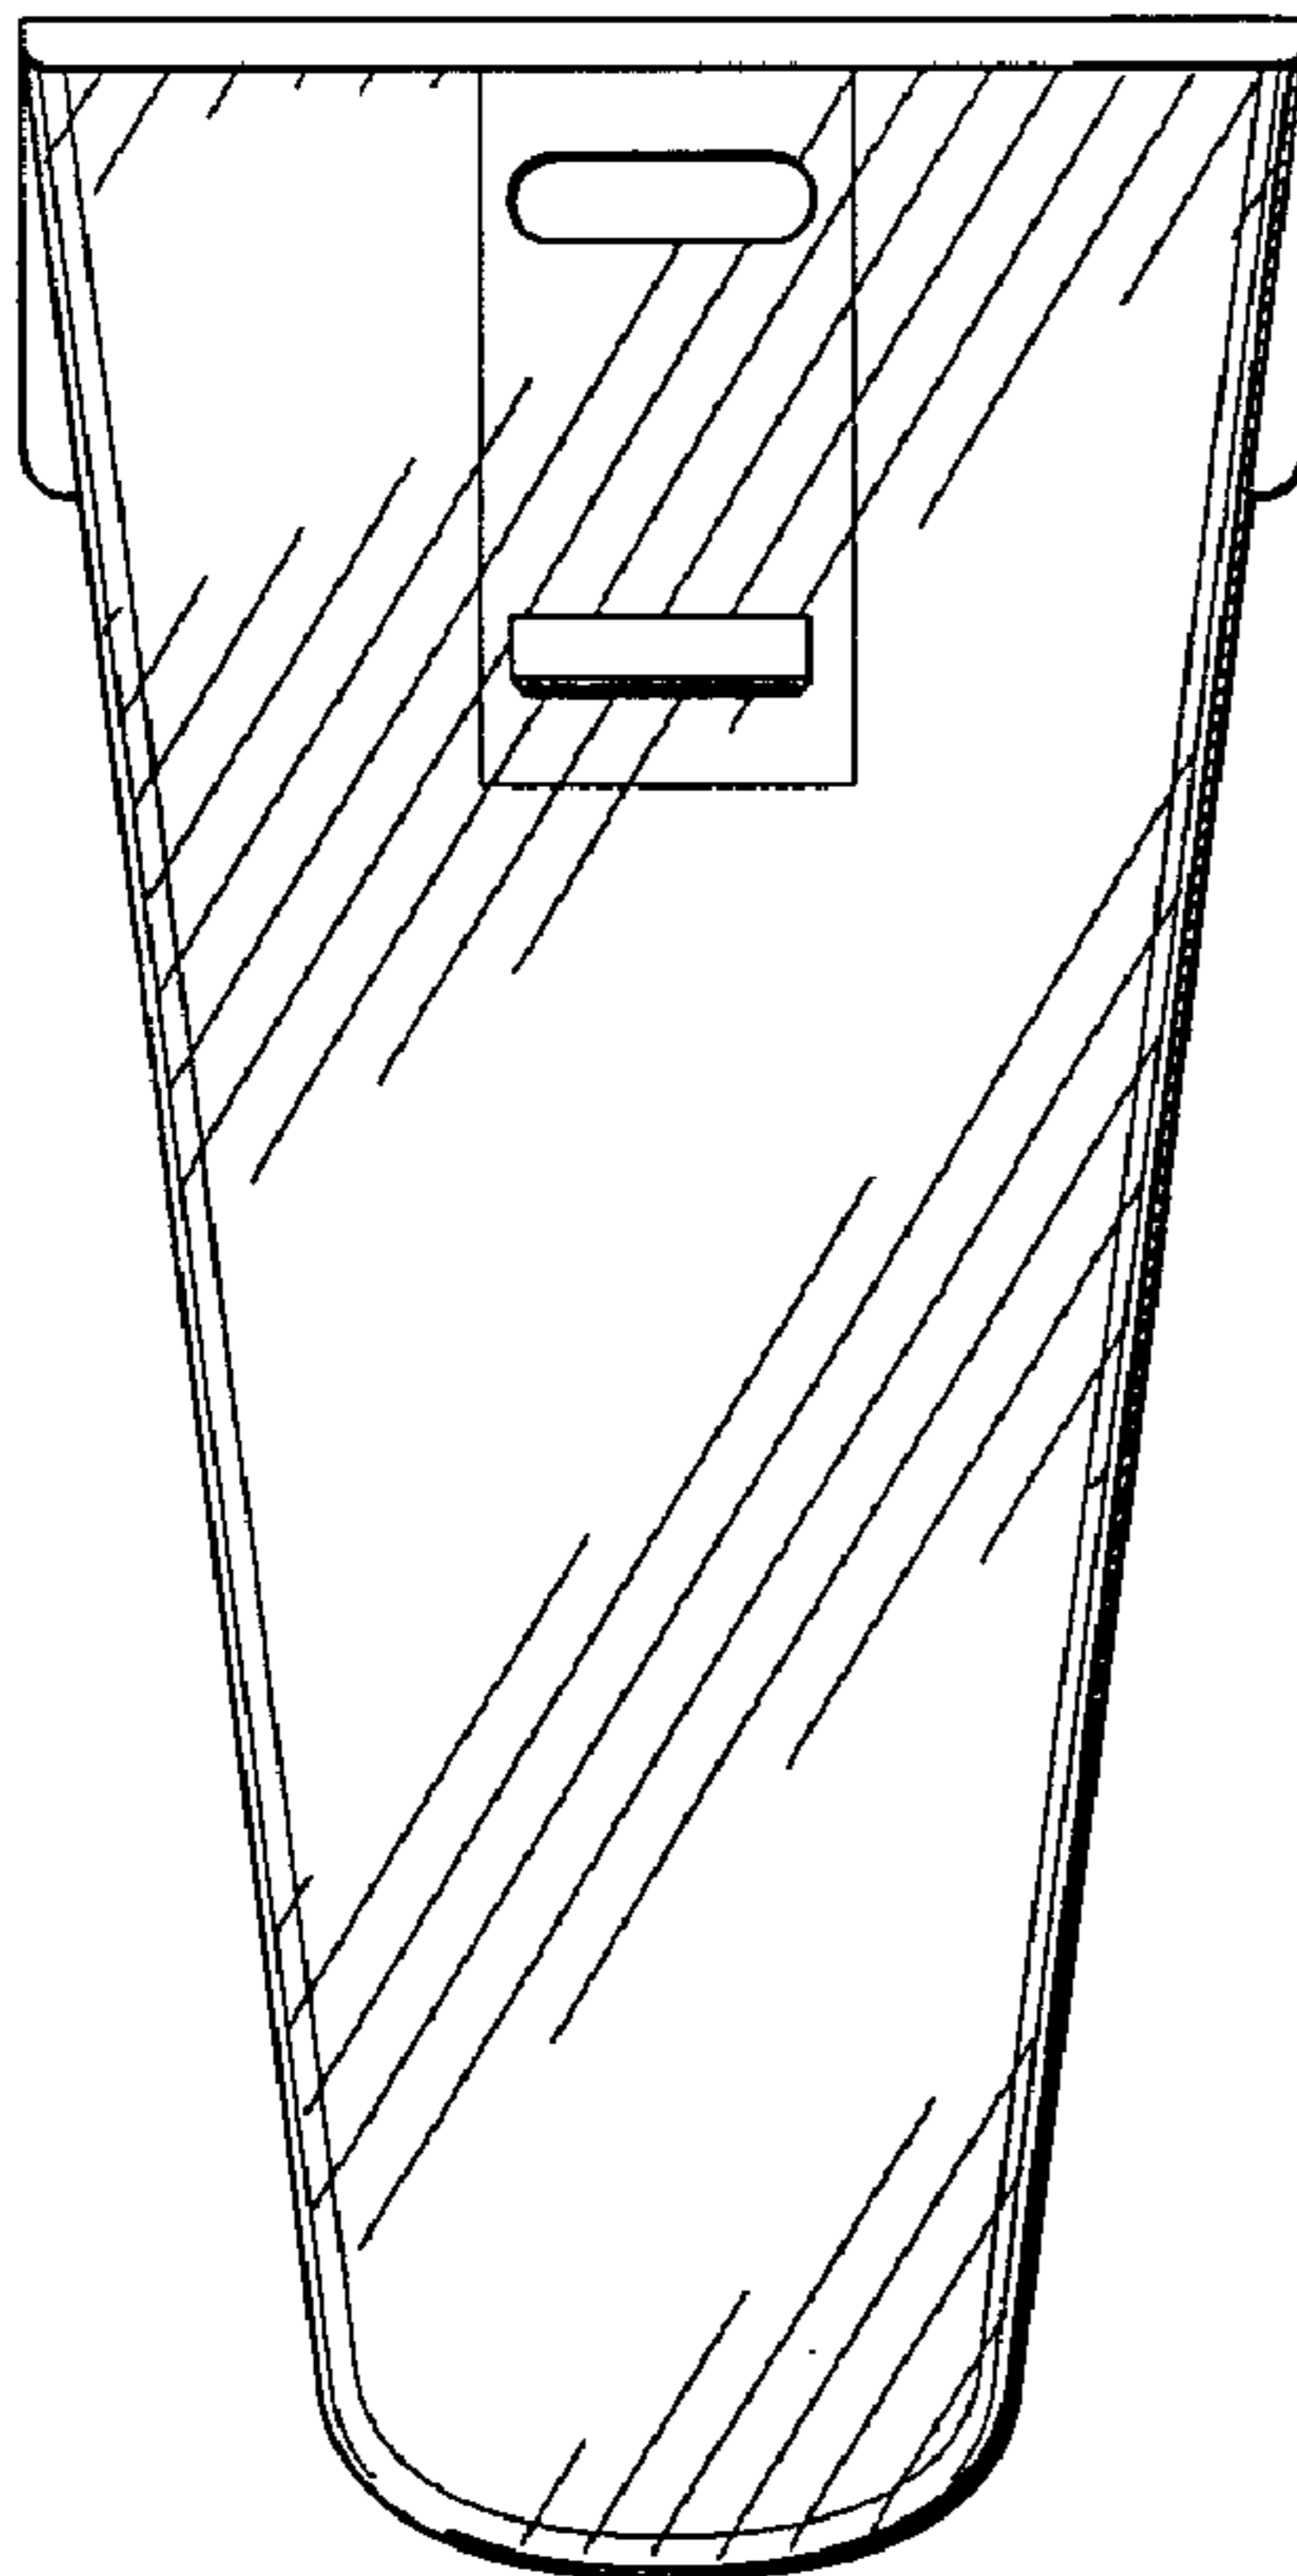


Fig. 4

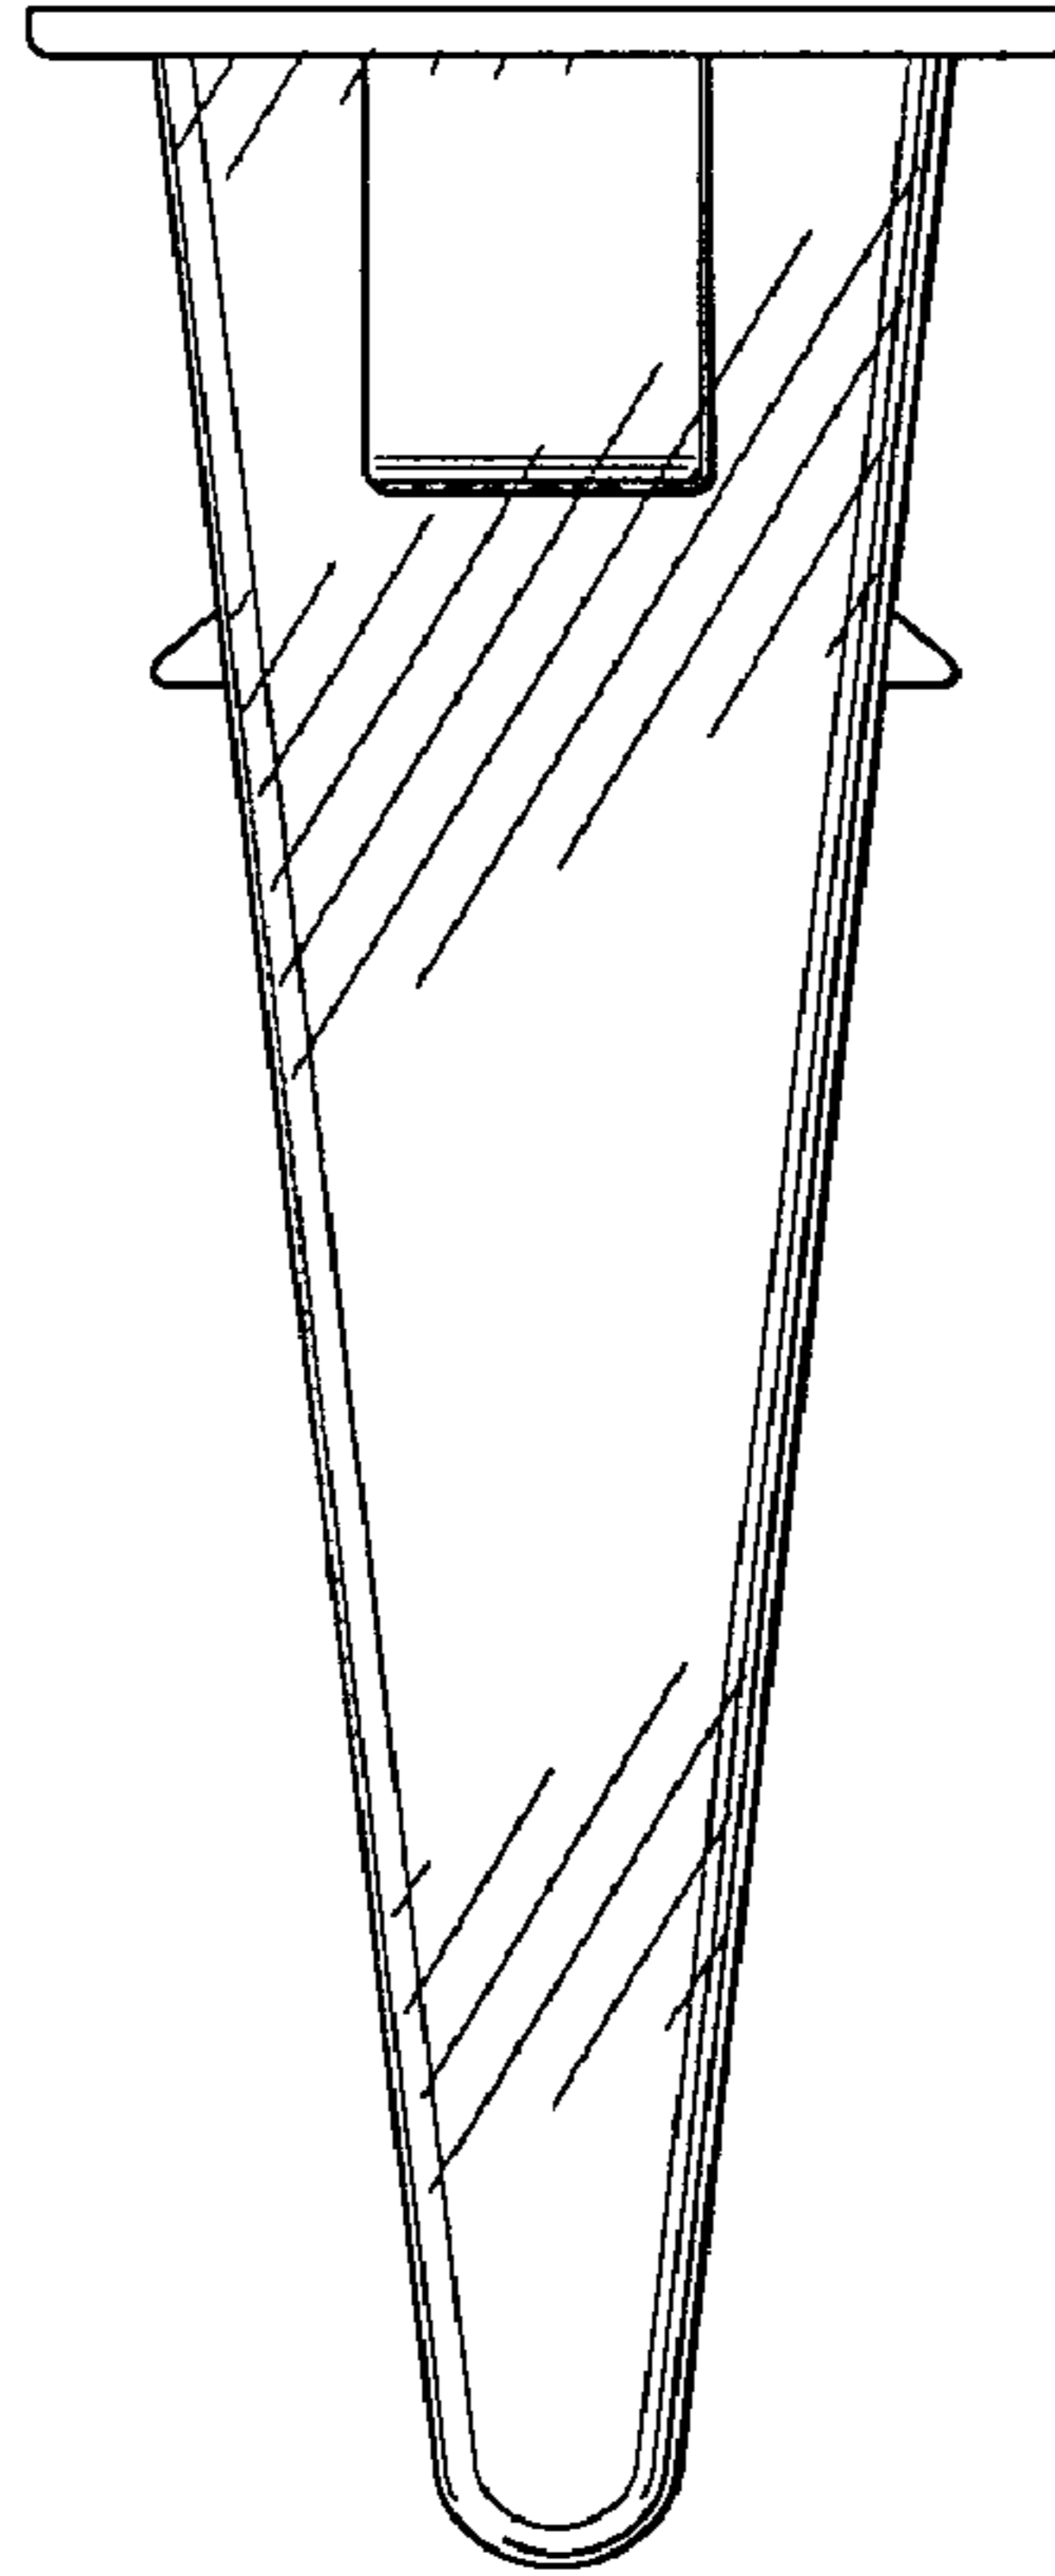


Fig. 5

UNITED STATES PATENT AND TRADEMARK OFFICE  
**CERTIFICATE OF CORRECTION**

PATENT NO. : Des. 560,816 S  
APPLICATION NO. : 29/272460  
DATED : January 29, 2008  
INVENTOR(S) : Talmer et al.

Page 1 of 1

It is certified that error appears in the above-identified patent and that said Letters Patent is hereby corrected as shown below:

**Page 1 of 1**

On the Title Page, under the heading Description, line 5, delete “and,” and replace it with --and--.

On the Title Page, under the heading References Cited, U.S. Patent Documents, delete “2003/0197799 A1” and replace it with --2003/0194799 A1--.

On the Title Page, after the heading References Cited, Foreign patent Documents, and \* cited by examiner, add:

--References Cited, Other Publications--

--Siemens Global website @

<http://diagnostics.siemens.com/webapp/wcs/stores/servlet/Product>, for ACS: 180<sup>®</sup> SE Automated Chemiluminescence System accessed June 13, 2007, © Siemens AG, 2007.--

Signed and Sealed this

First Day of July, 2008



JON W. DUDAS

*Director of the United States Patent and Trademark Office*