

US00D562985S

(12) **United States Design Patent**
Brefka et al.

(10) **Patent No.:** **US D562,985 S**
(45) **Date of Patent:** **** Feb. 26, 2008**

(54) **MEDICAL DEVICE WITH CABLE**

D537,164 S * 2/2007 Shigemori et al. D24/138

(75) Inventors: **Paul E. Brefka**, Southborough, MA (US); **John D'Arco**, Wilmington, MA (US); **Charles Fendrock**, Sudbury, MA (US); **Michael Williams**, Melrose, MA (US)

* cited by examiner

Primary Examiner—Robert A. Delehanty
Assistant Examiner—Mark Cavanna
(74) *Attorney, Agent, or Firm*—Pandiscio & Pandiscio

(73) Assignee: **Neurometrix, Inc.**, Waltham, MA (US)

(57) **CLAIM**

(**) Term: **14 Years**

The ornamental design for medical device with cable, as shown and described.

(21) Appl. No.: **29/261,021**

DESCRIPTION

(22) Filed: **Jun. 6, 2006**

A portion of the disclosure of this patent document contains material to which a claim for copyright is made. The copyright owner has no objection to the facsimile reproduction by anyone of the patent document or the patent disclosure, as it appears in the Patent and Trademark Office patent file or records, but reserves all other copyrights whatsoever.

(51) **LOC (8) Cl.** **24-01**

(52) **U.S. Cl.** **D24/186**

(58) **Field of Classification Search** D24/138,
D24/169, 186, 200, 215; D10/81; 600/41,
600/46, 48, 54–56, 58–65

FIG. 1 is a perspective view of a medical device with cable shown without the cable showing our new design;

See application file for complete search history.

FIG. 2 is a front elevational view thereof;

(56) **References Cited**

U.S. PATENT DOCUMENTS

- D323,561 S * 1/1992 Bartelt et al. D24/200
- D390,666 S * 2/1998 Lagerlof D24/186
- D414,870 S * 10/1999 Saltzstein et al. D24/186
- D437,058 S * 1/2001 Gozani D24/186
- D452,012 S * 12/2001 Phillips D24/186
- D495,800 S * 9/2004 Kaar et al. D24/169
- D502,655 S * 3/2005 Huang D10/81
- D503,641 S * 4/2005 Huang D10/81
- D504,953 S * 5/2005 Ryan D24/200
- D505,726 S * 5/2005 Ryan D24/200
- D510,625 S * 10/2005 Widener et al. D24/186
- D522,657 S * 6/2006 Murphy et al. D24/186

FIG. 3 is a rear elevational view thereof;

FIG. 4 is a right side elevational view thereof;

FIG. 5 is a left side elevational view thereof;


FIG. 6 is a top plan view thereof;

FIG. 7 is a bottom plan view thereof;

FIG. 8 is a front elevational view of a medical device with cable shown with the cable in condition of use; and,

FIG. 9 is a perspective view of a medical device with cable shown with the cable in condition of use.

1 Claim, 6 Drawing Sheets

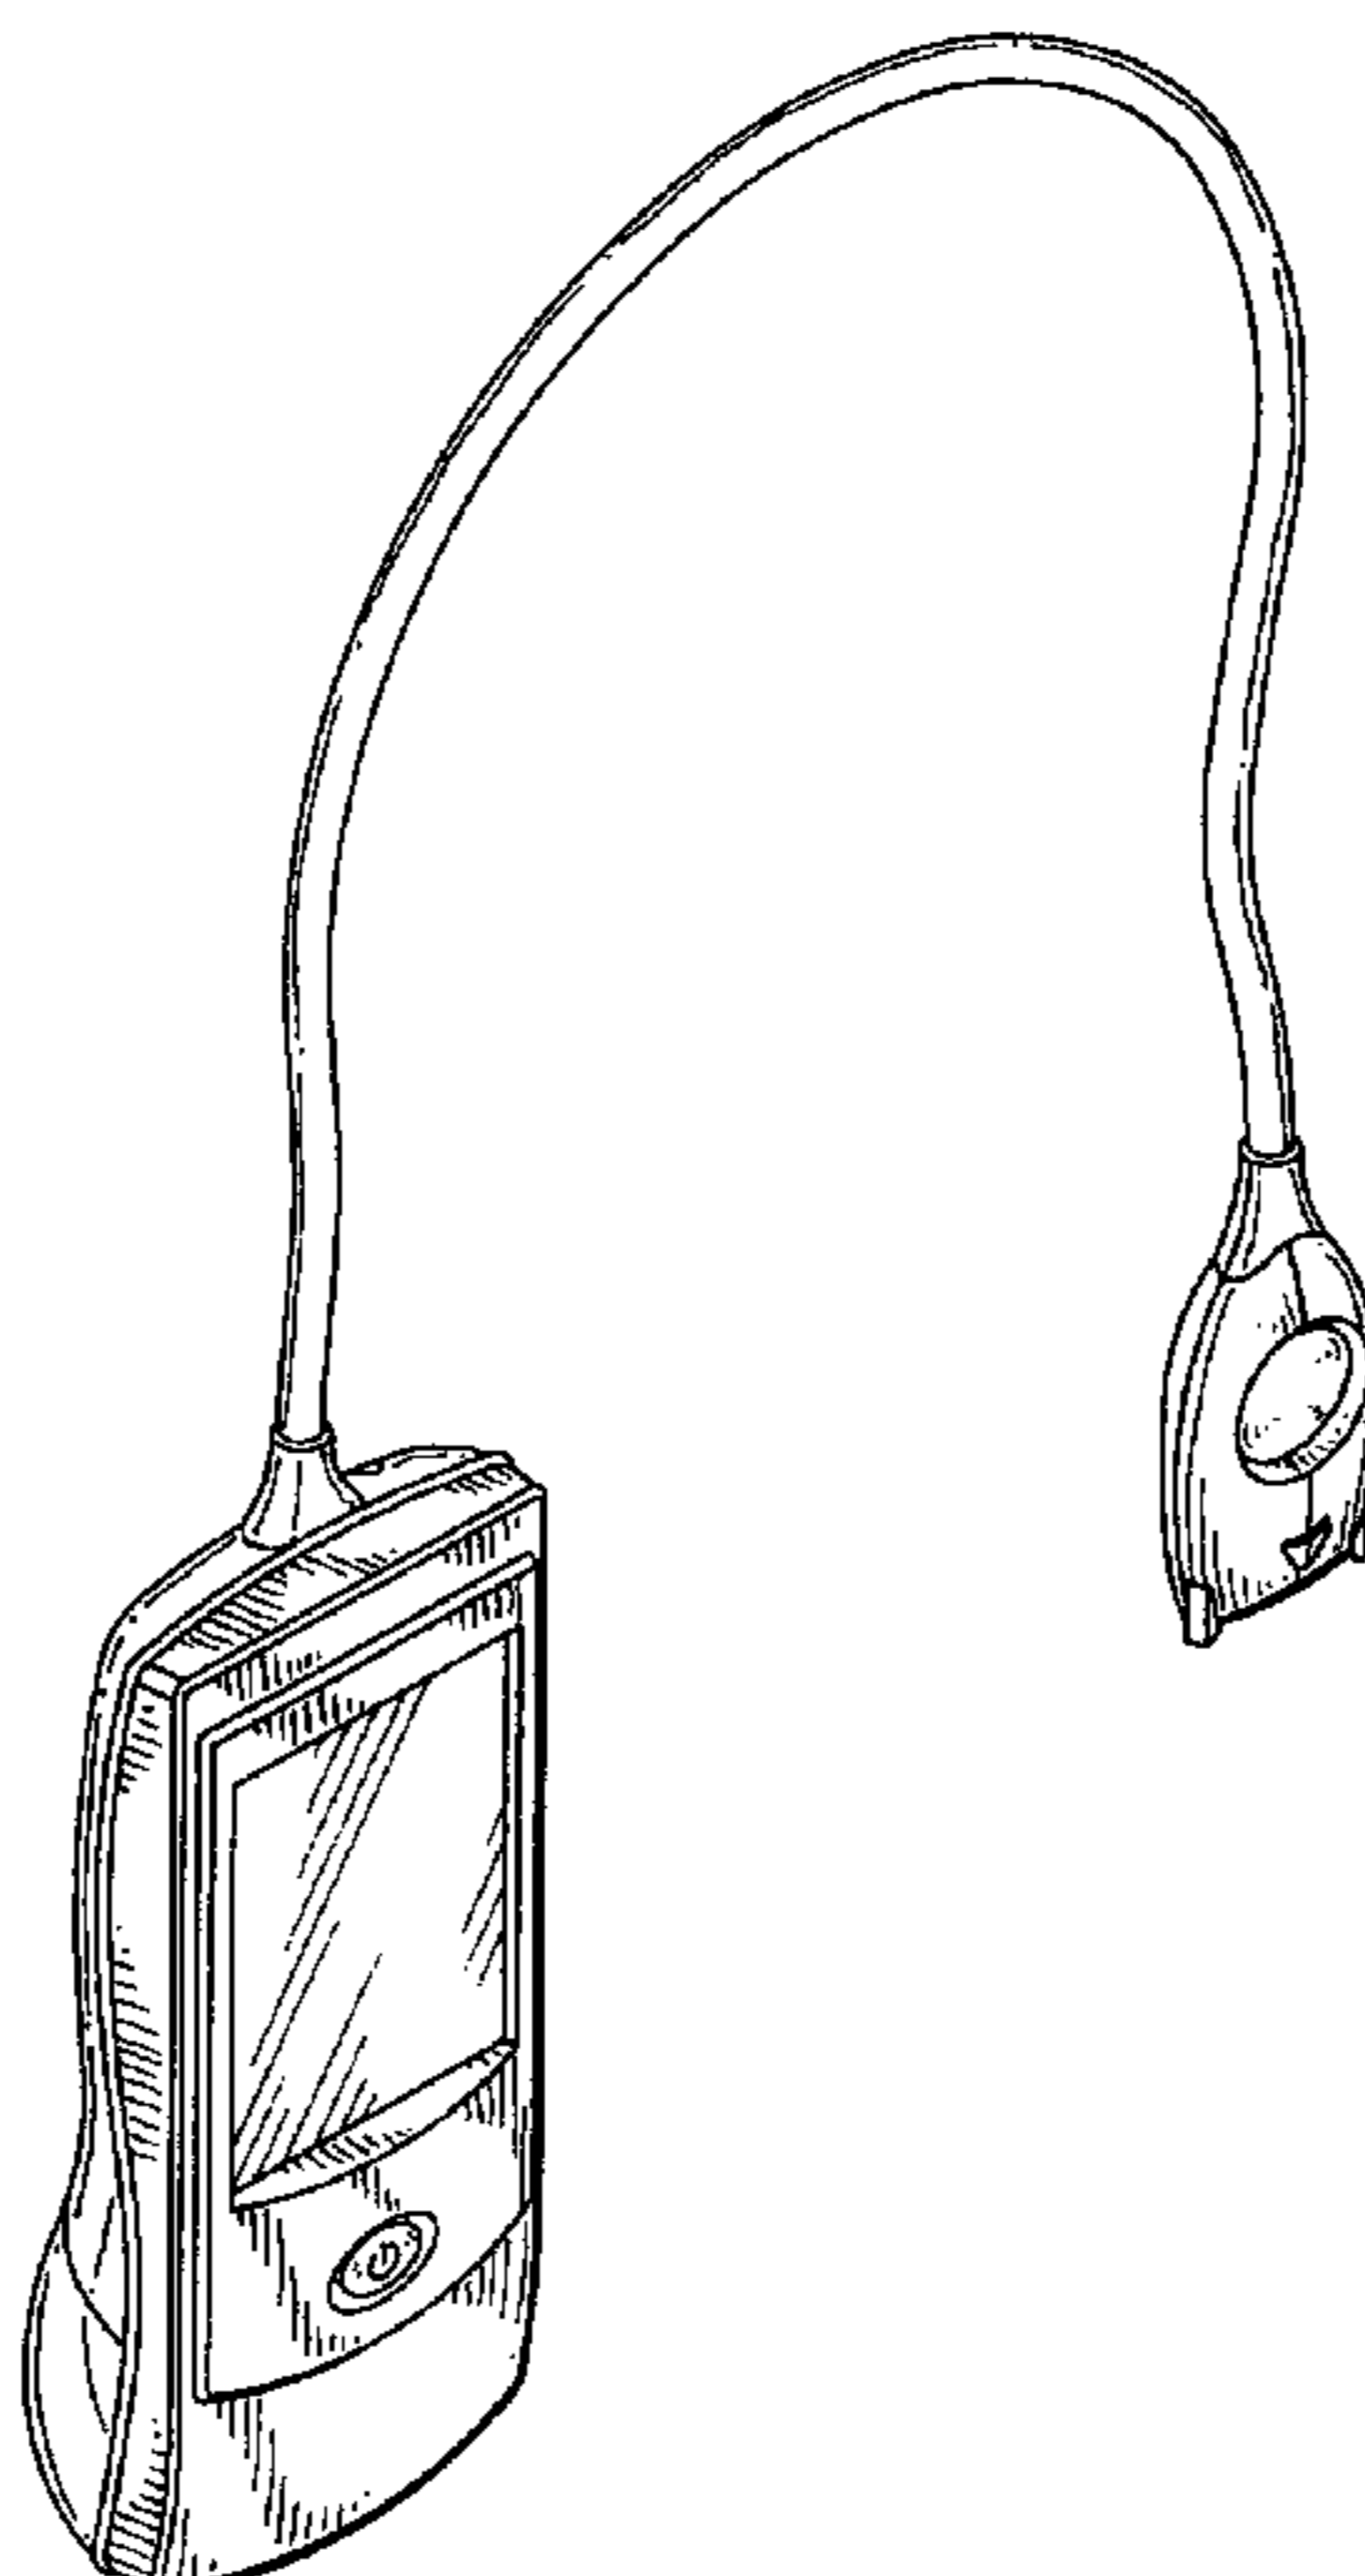

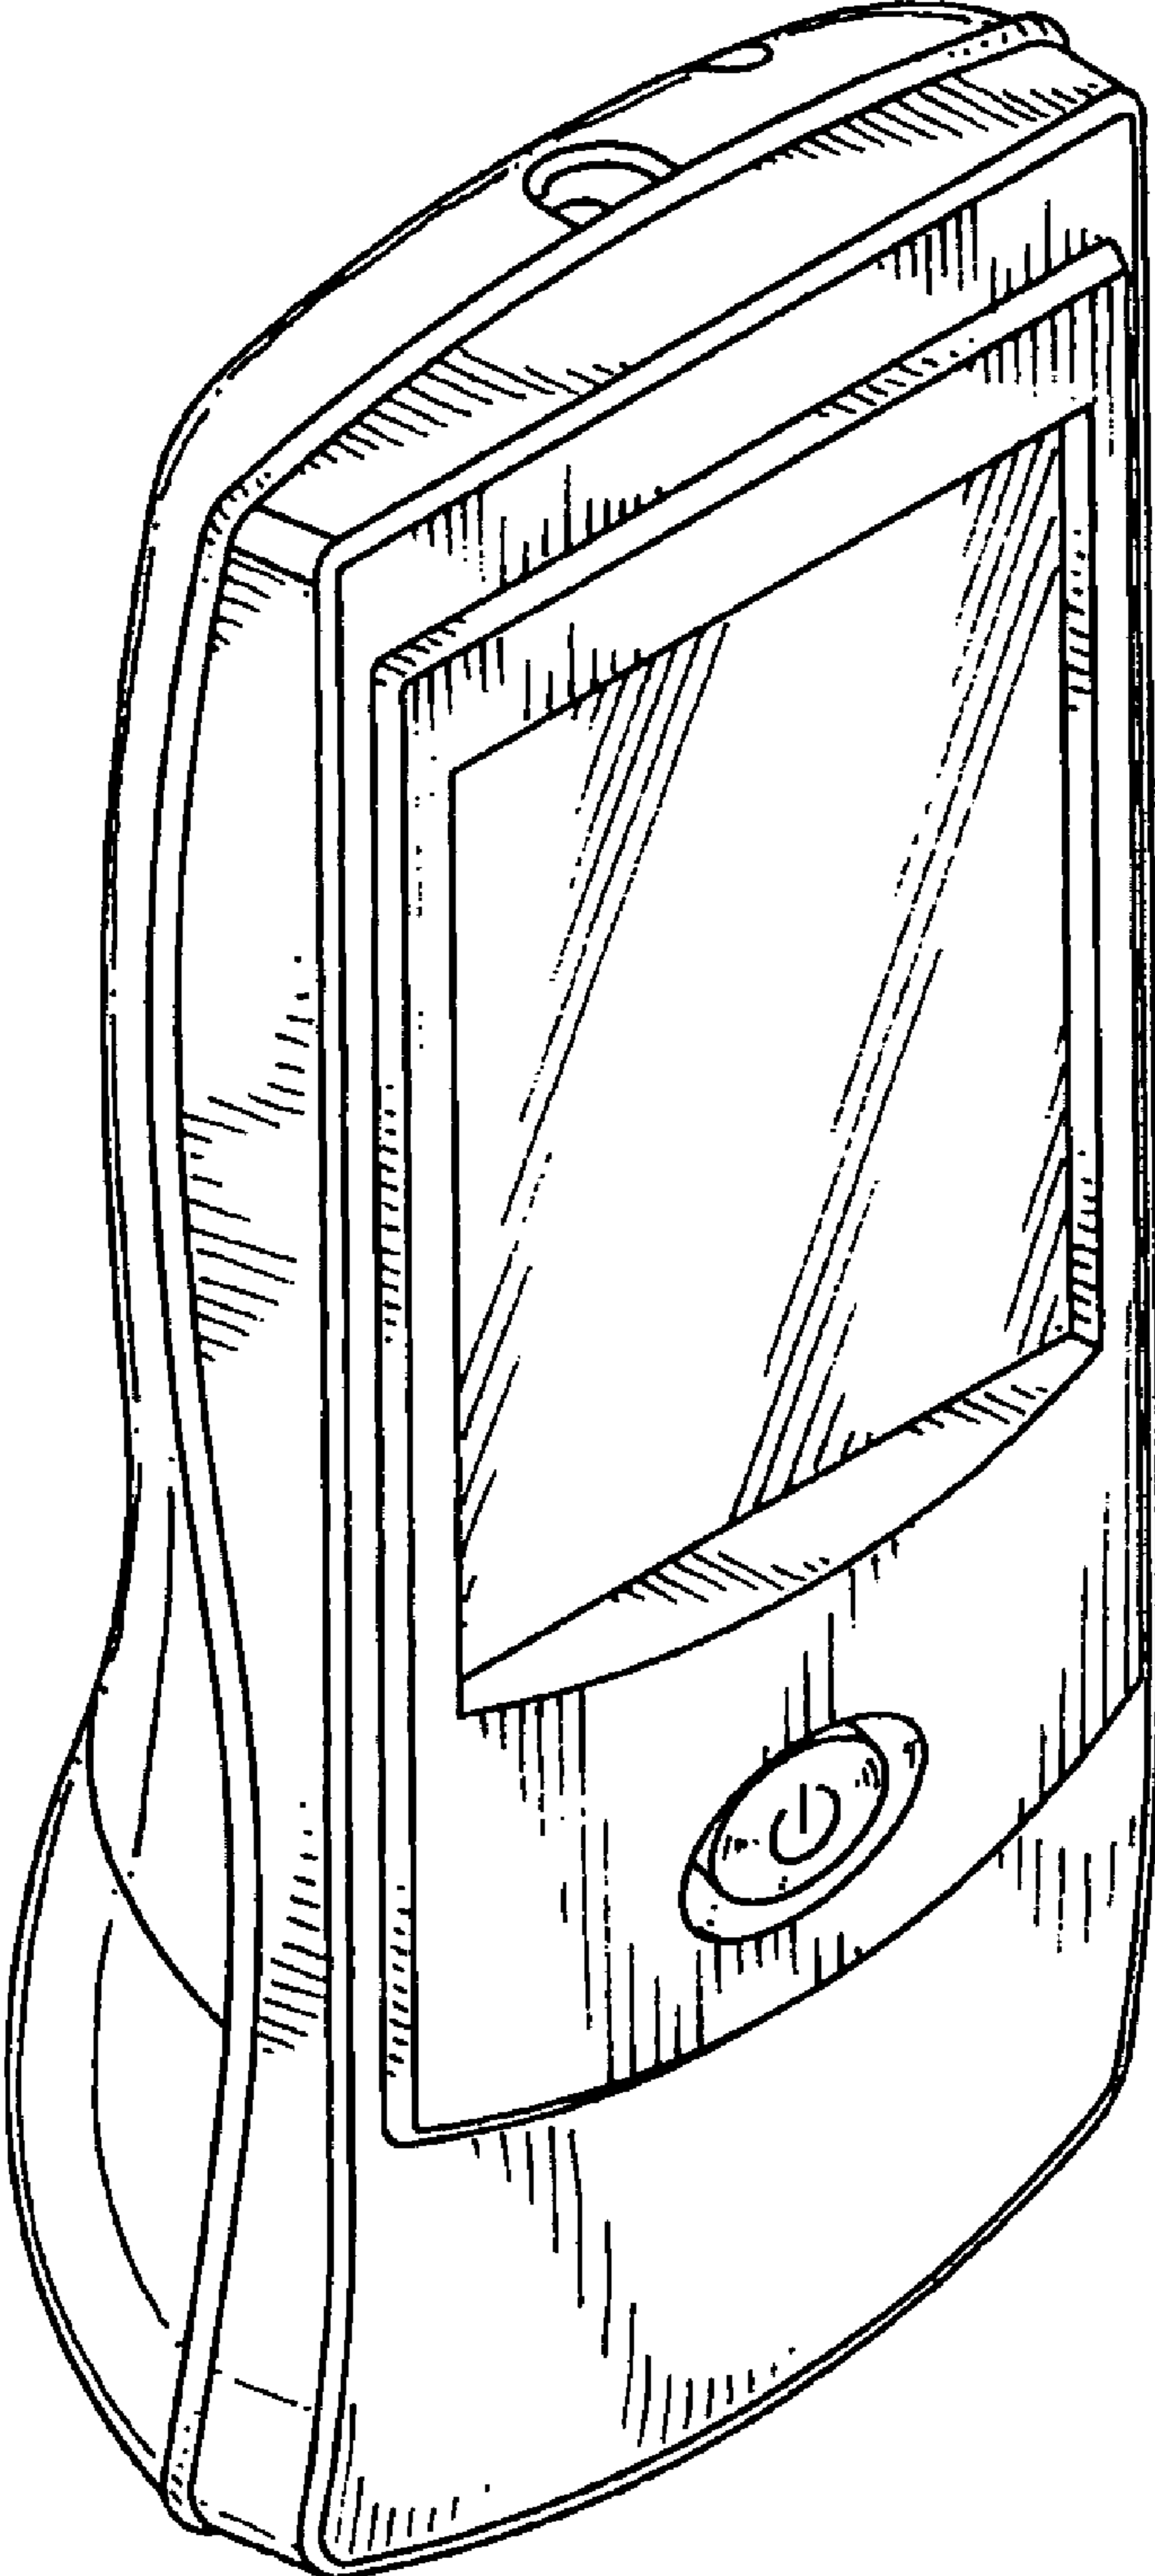


FIG. 1

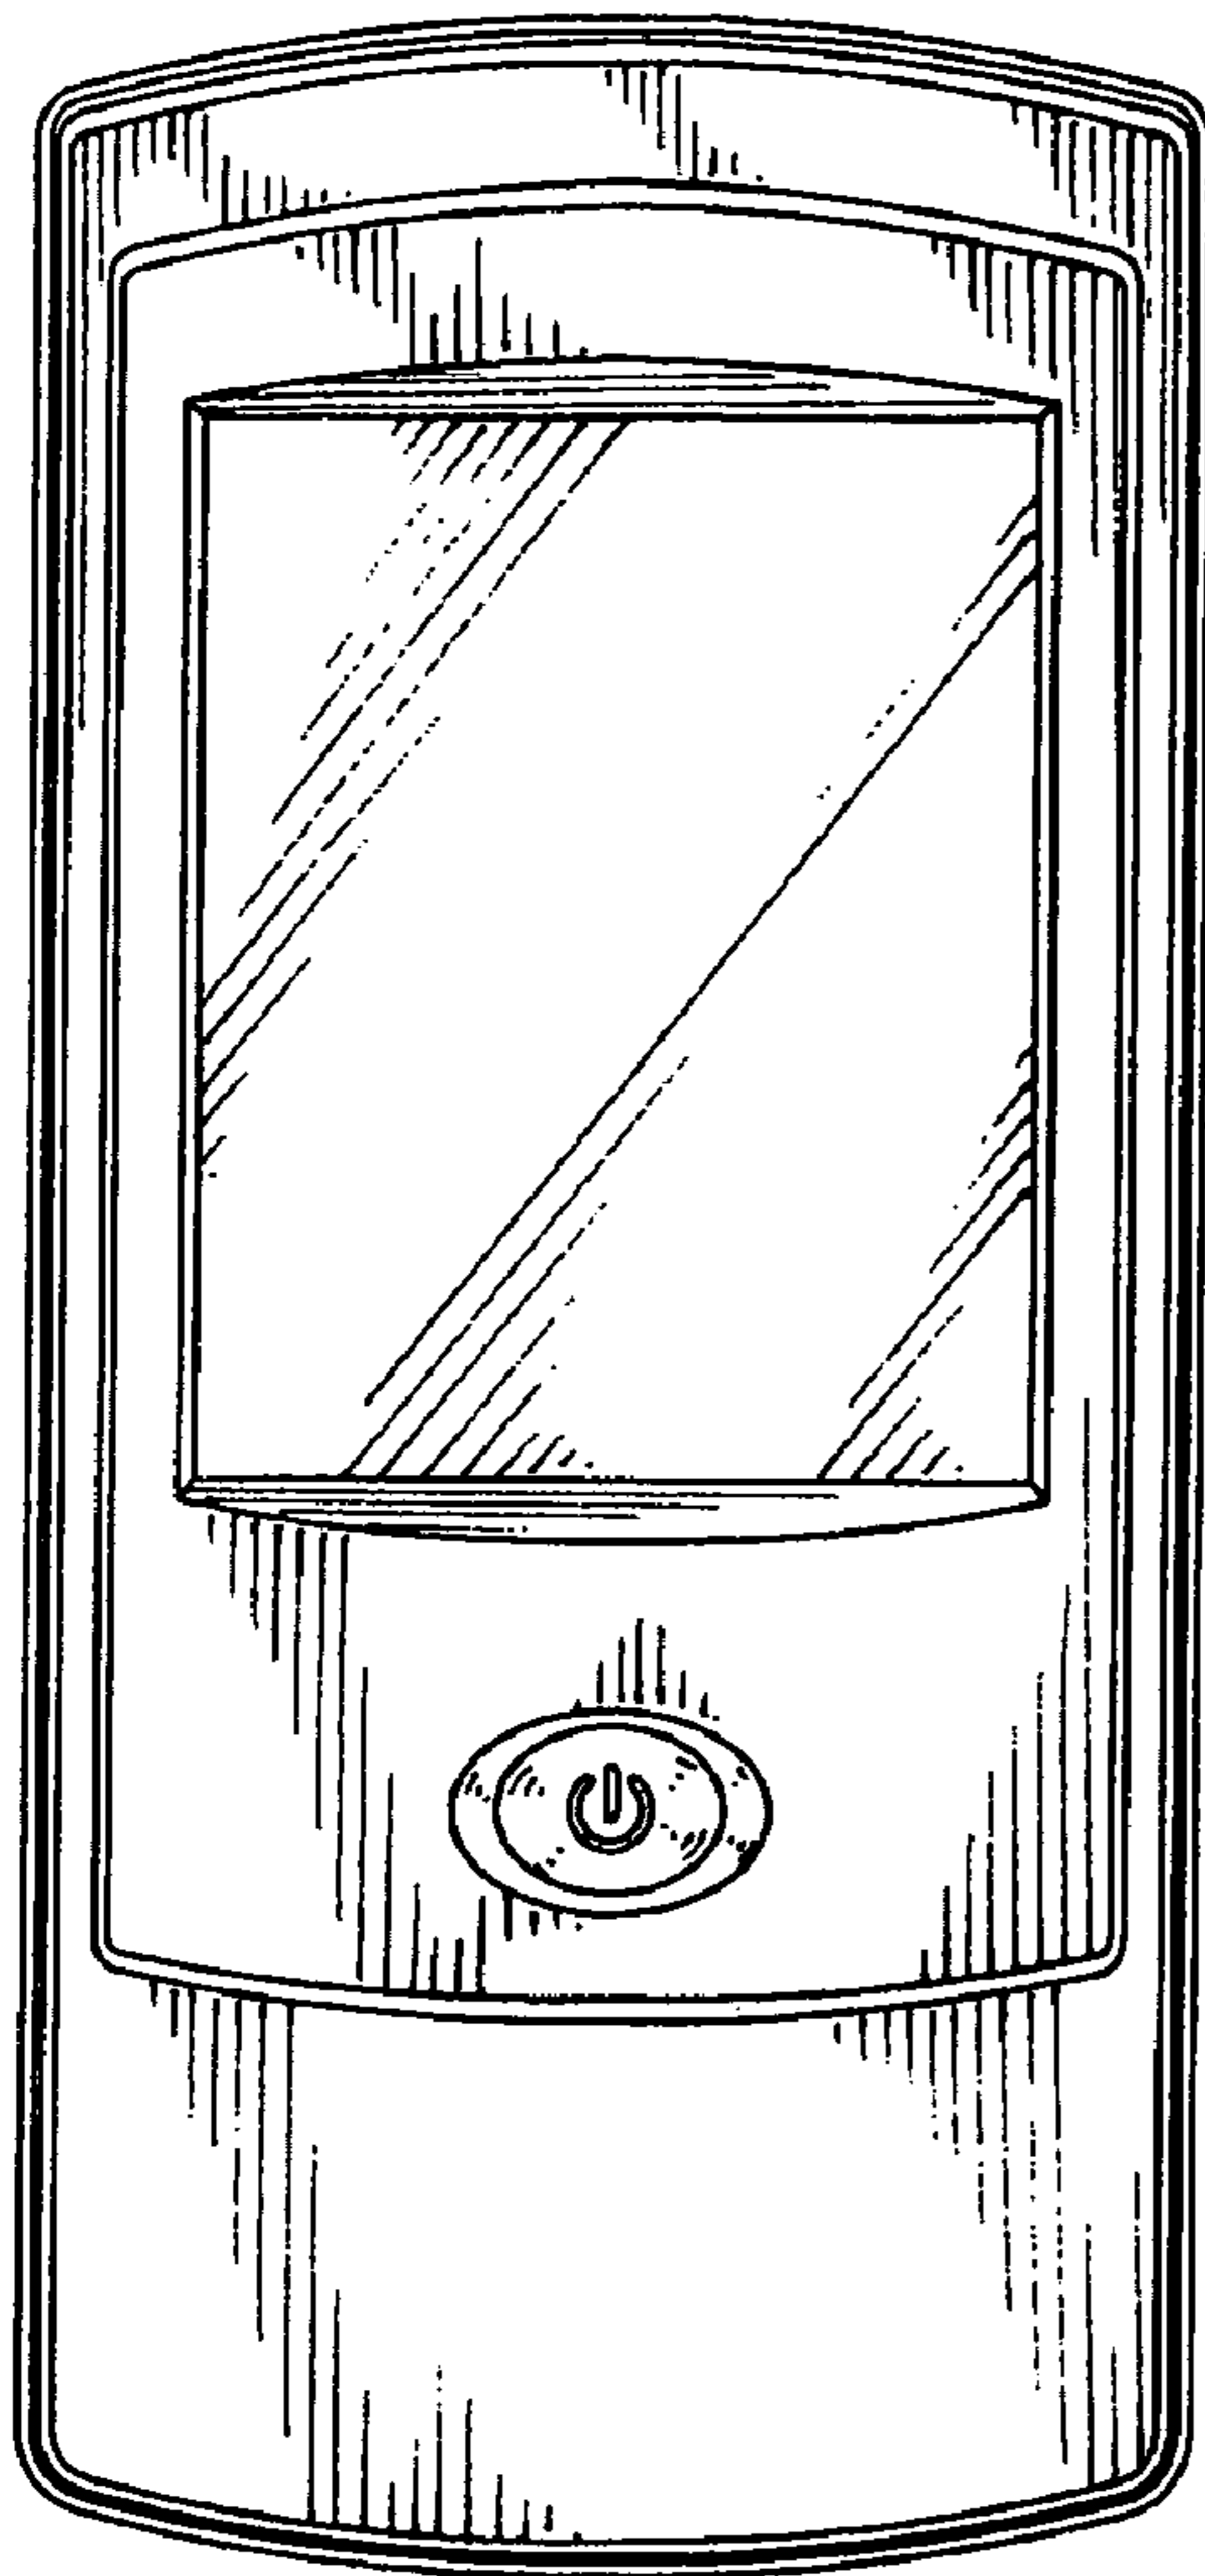


FIG. 2

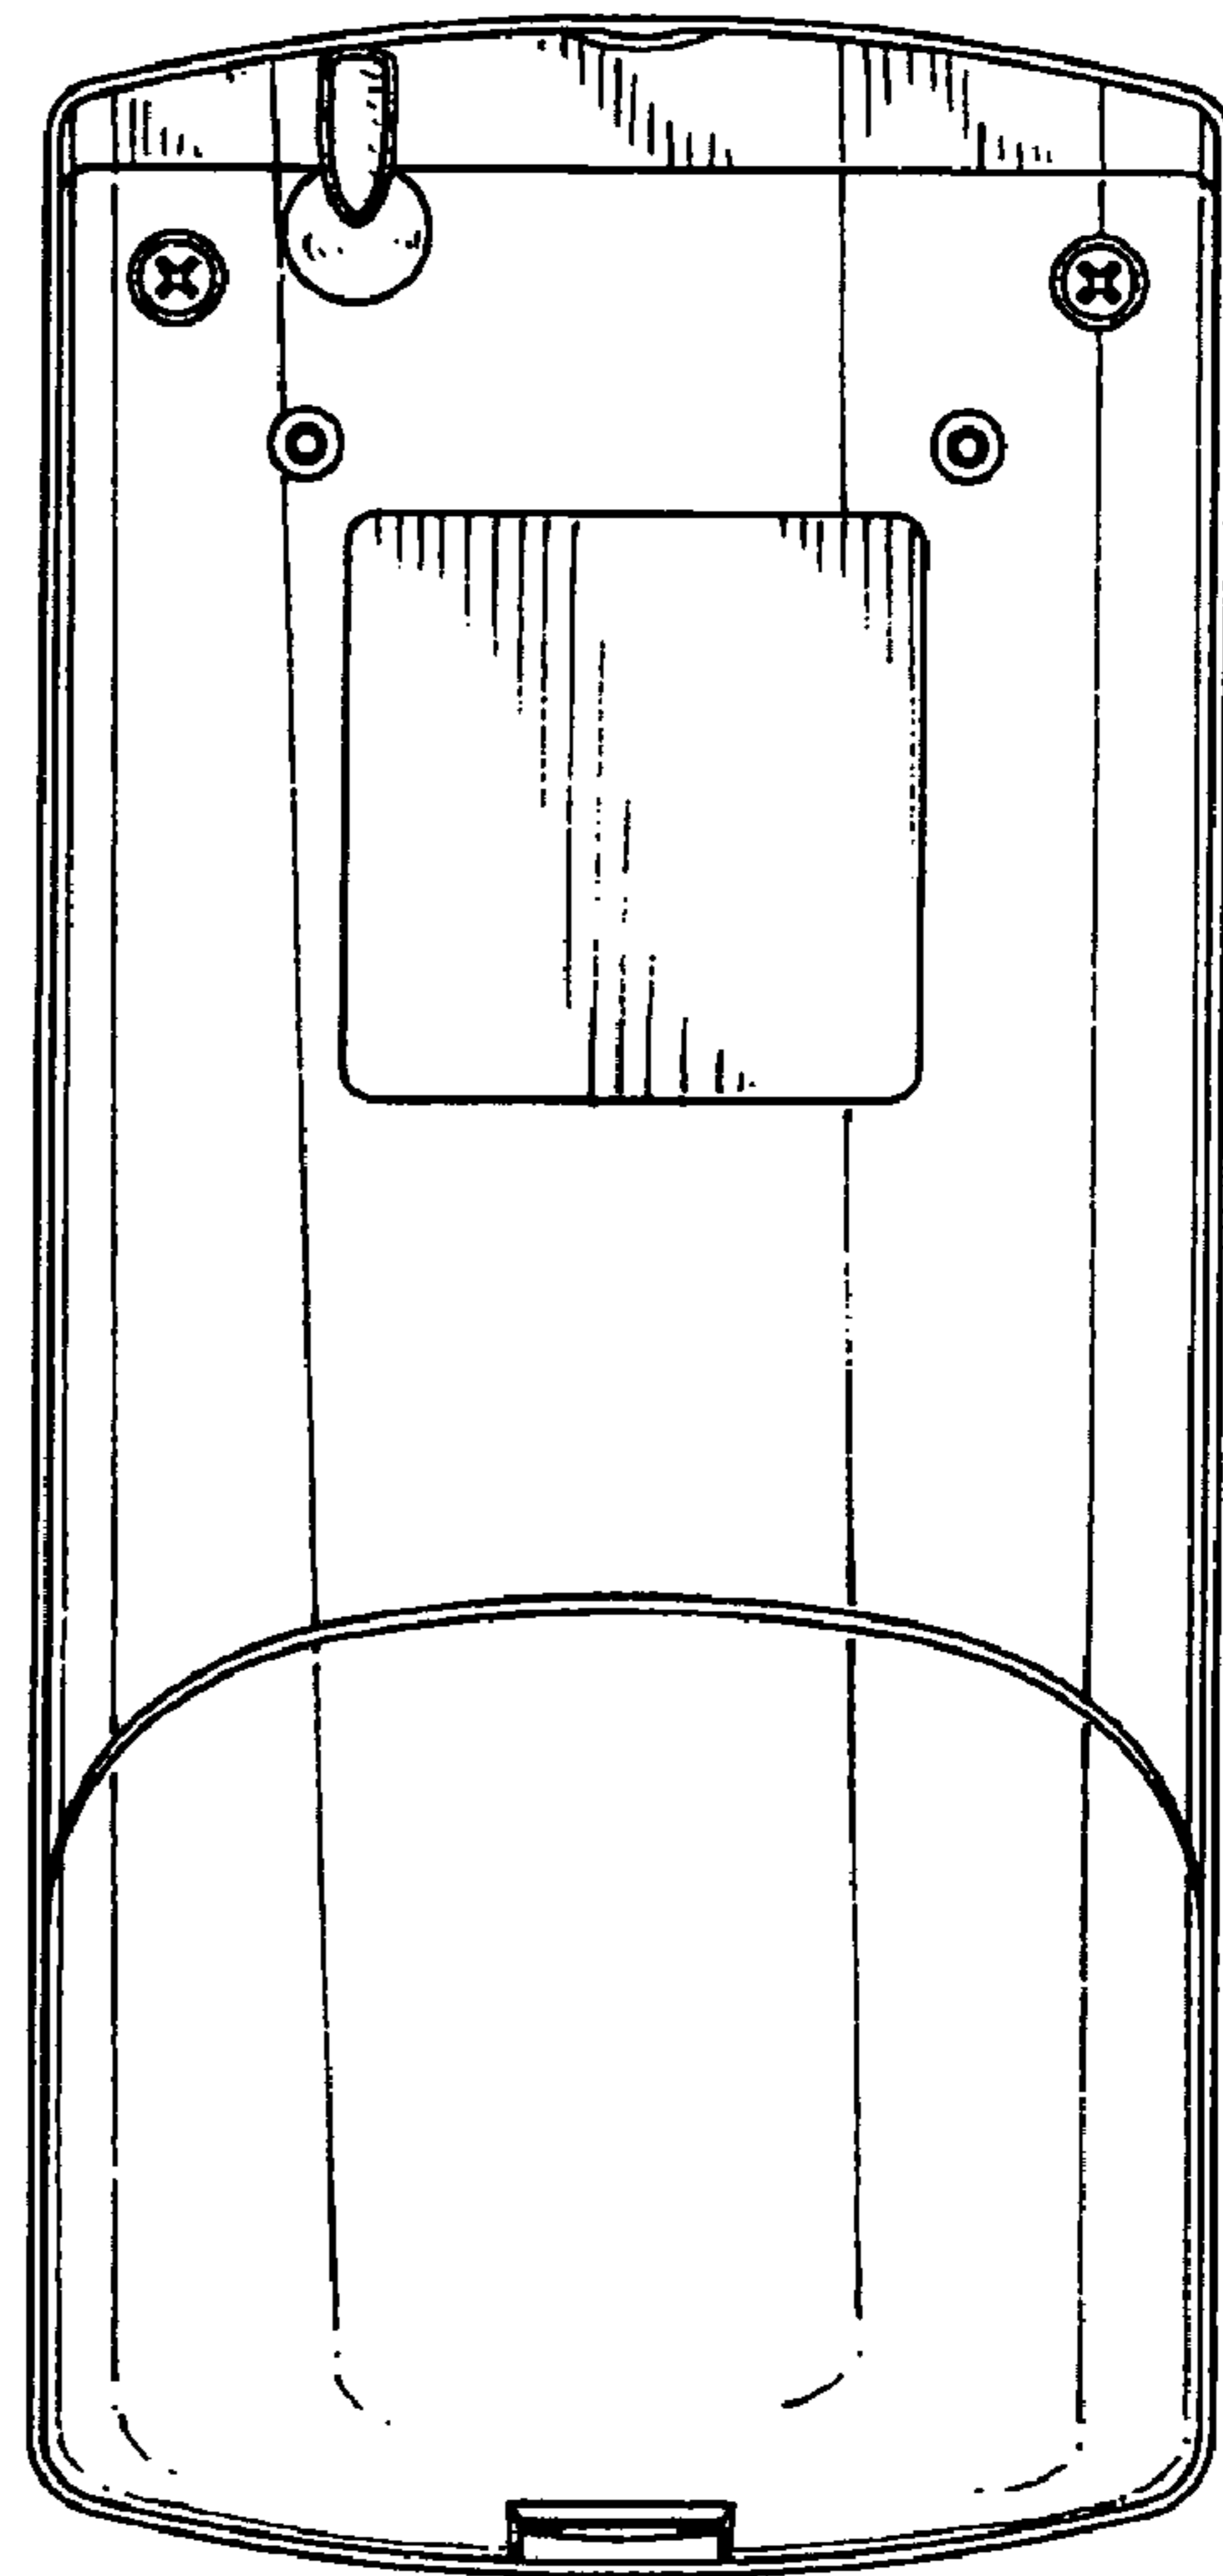


FIG. 3

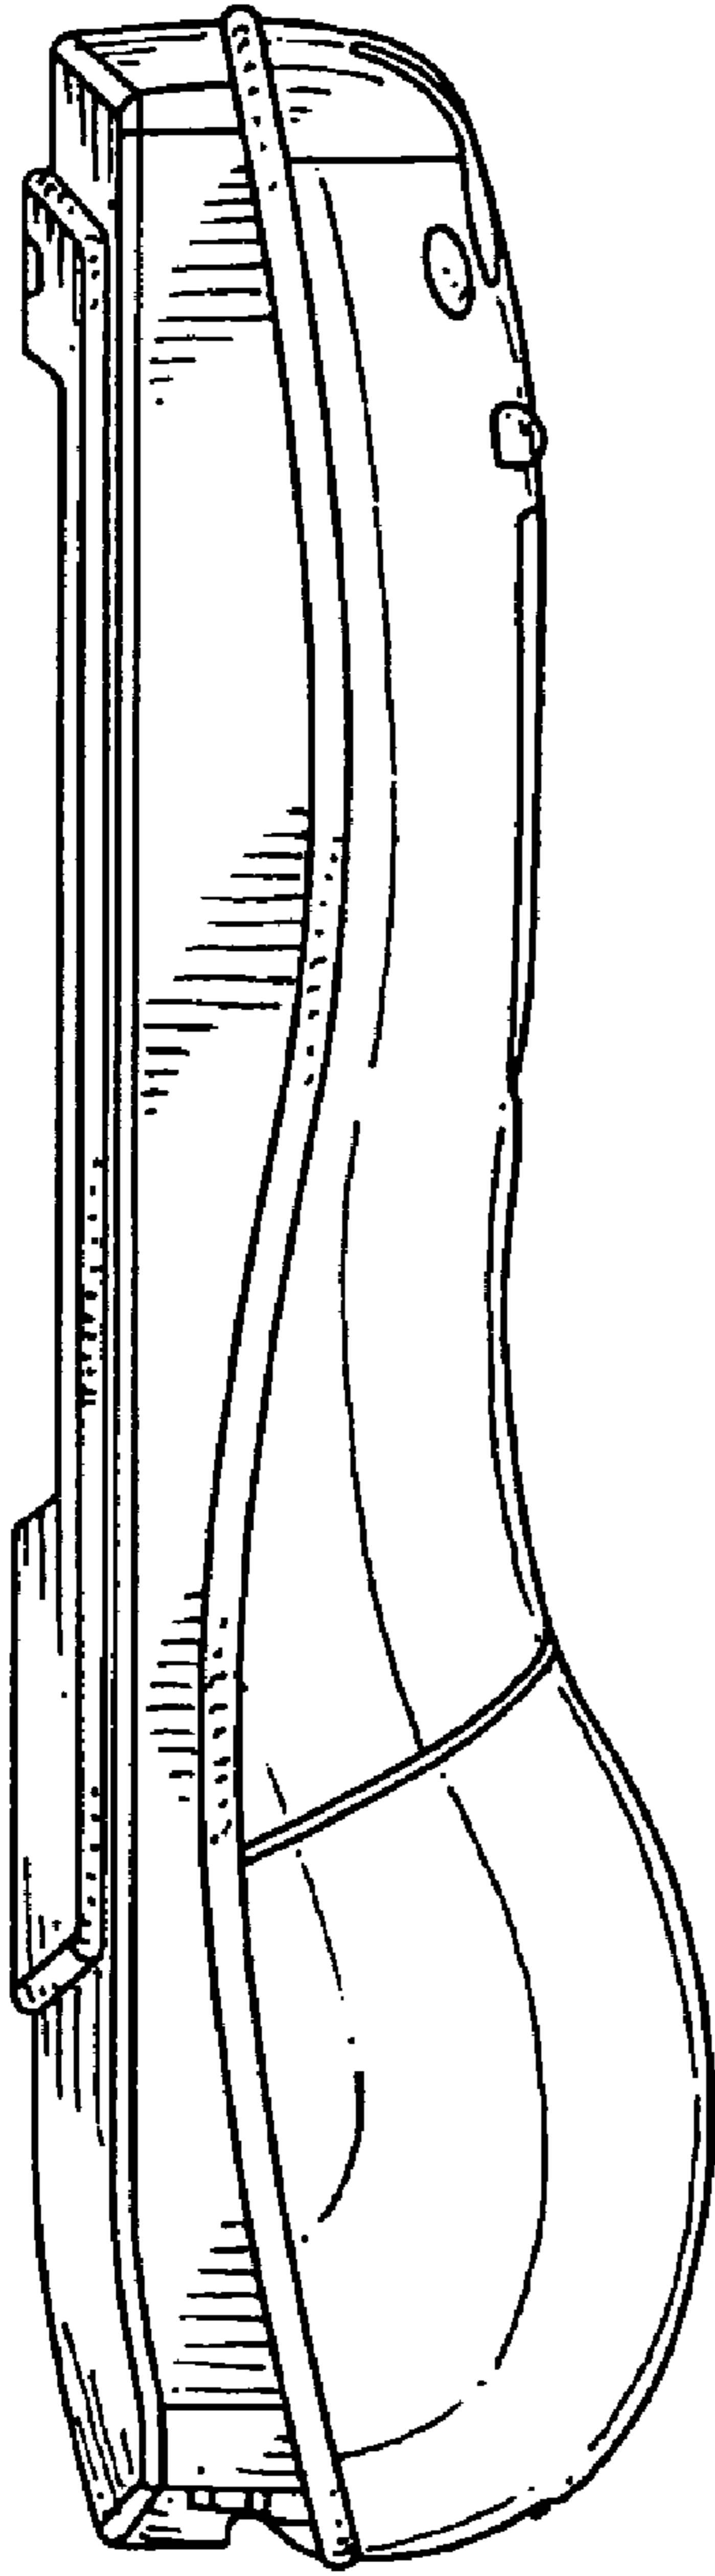


FIG. 4

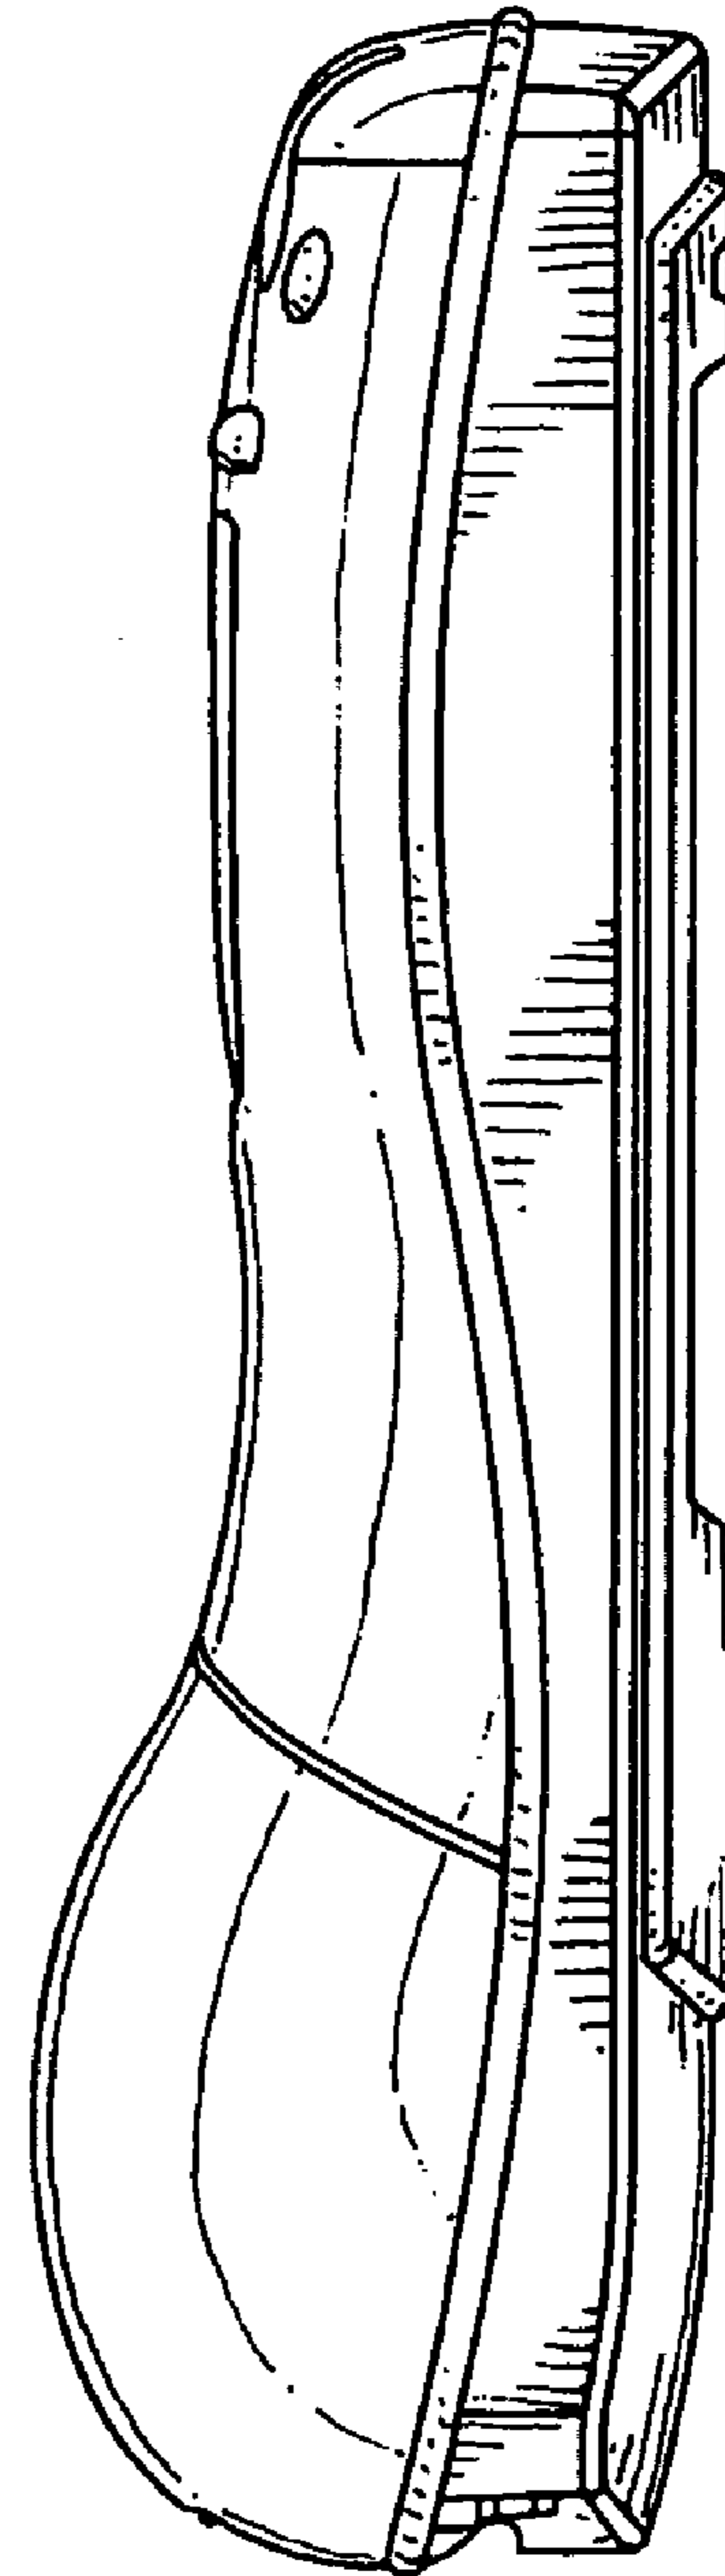


FIG. 5

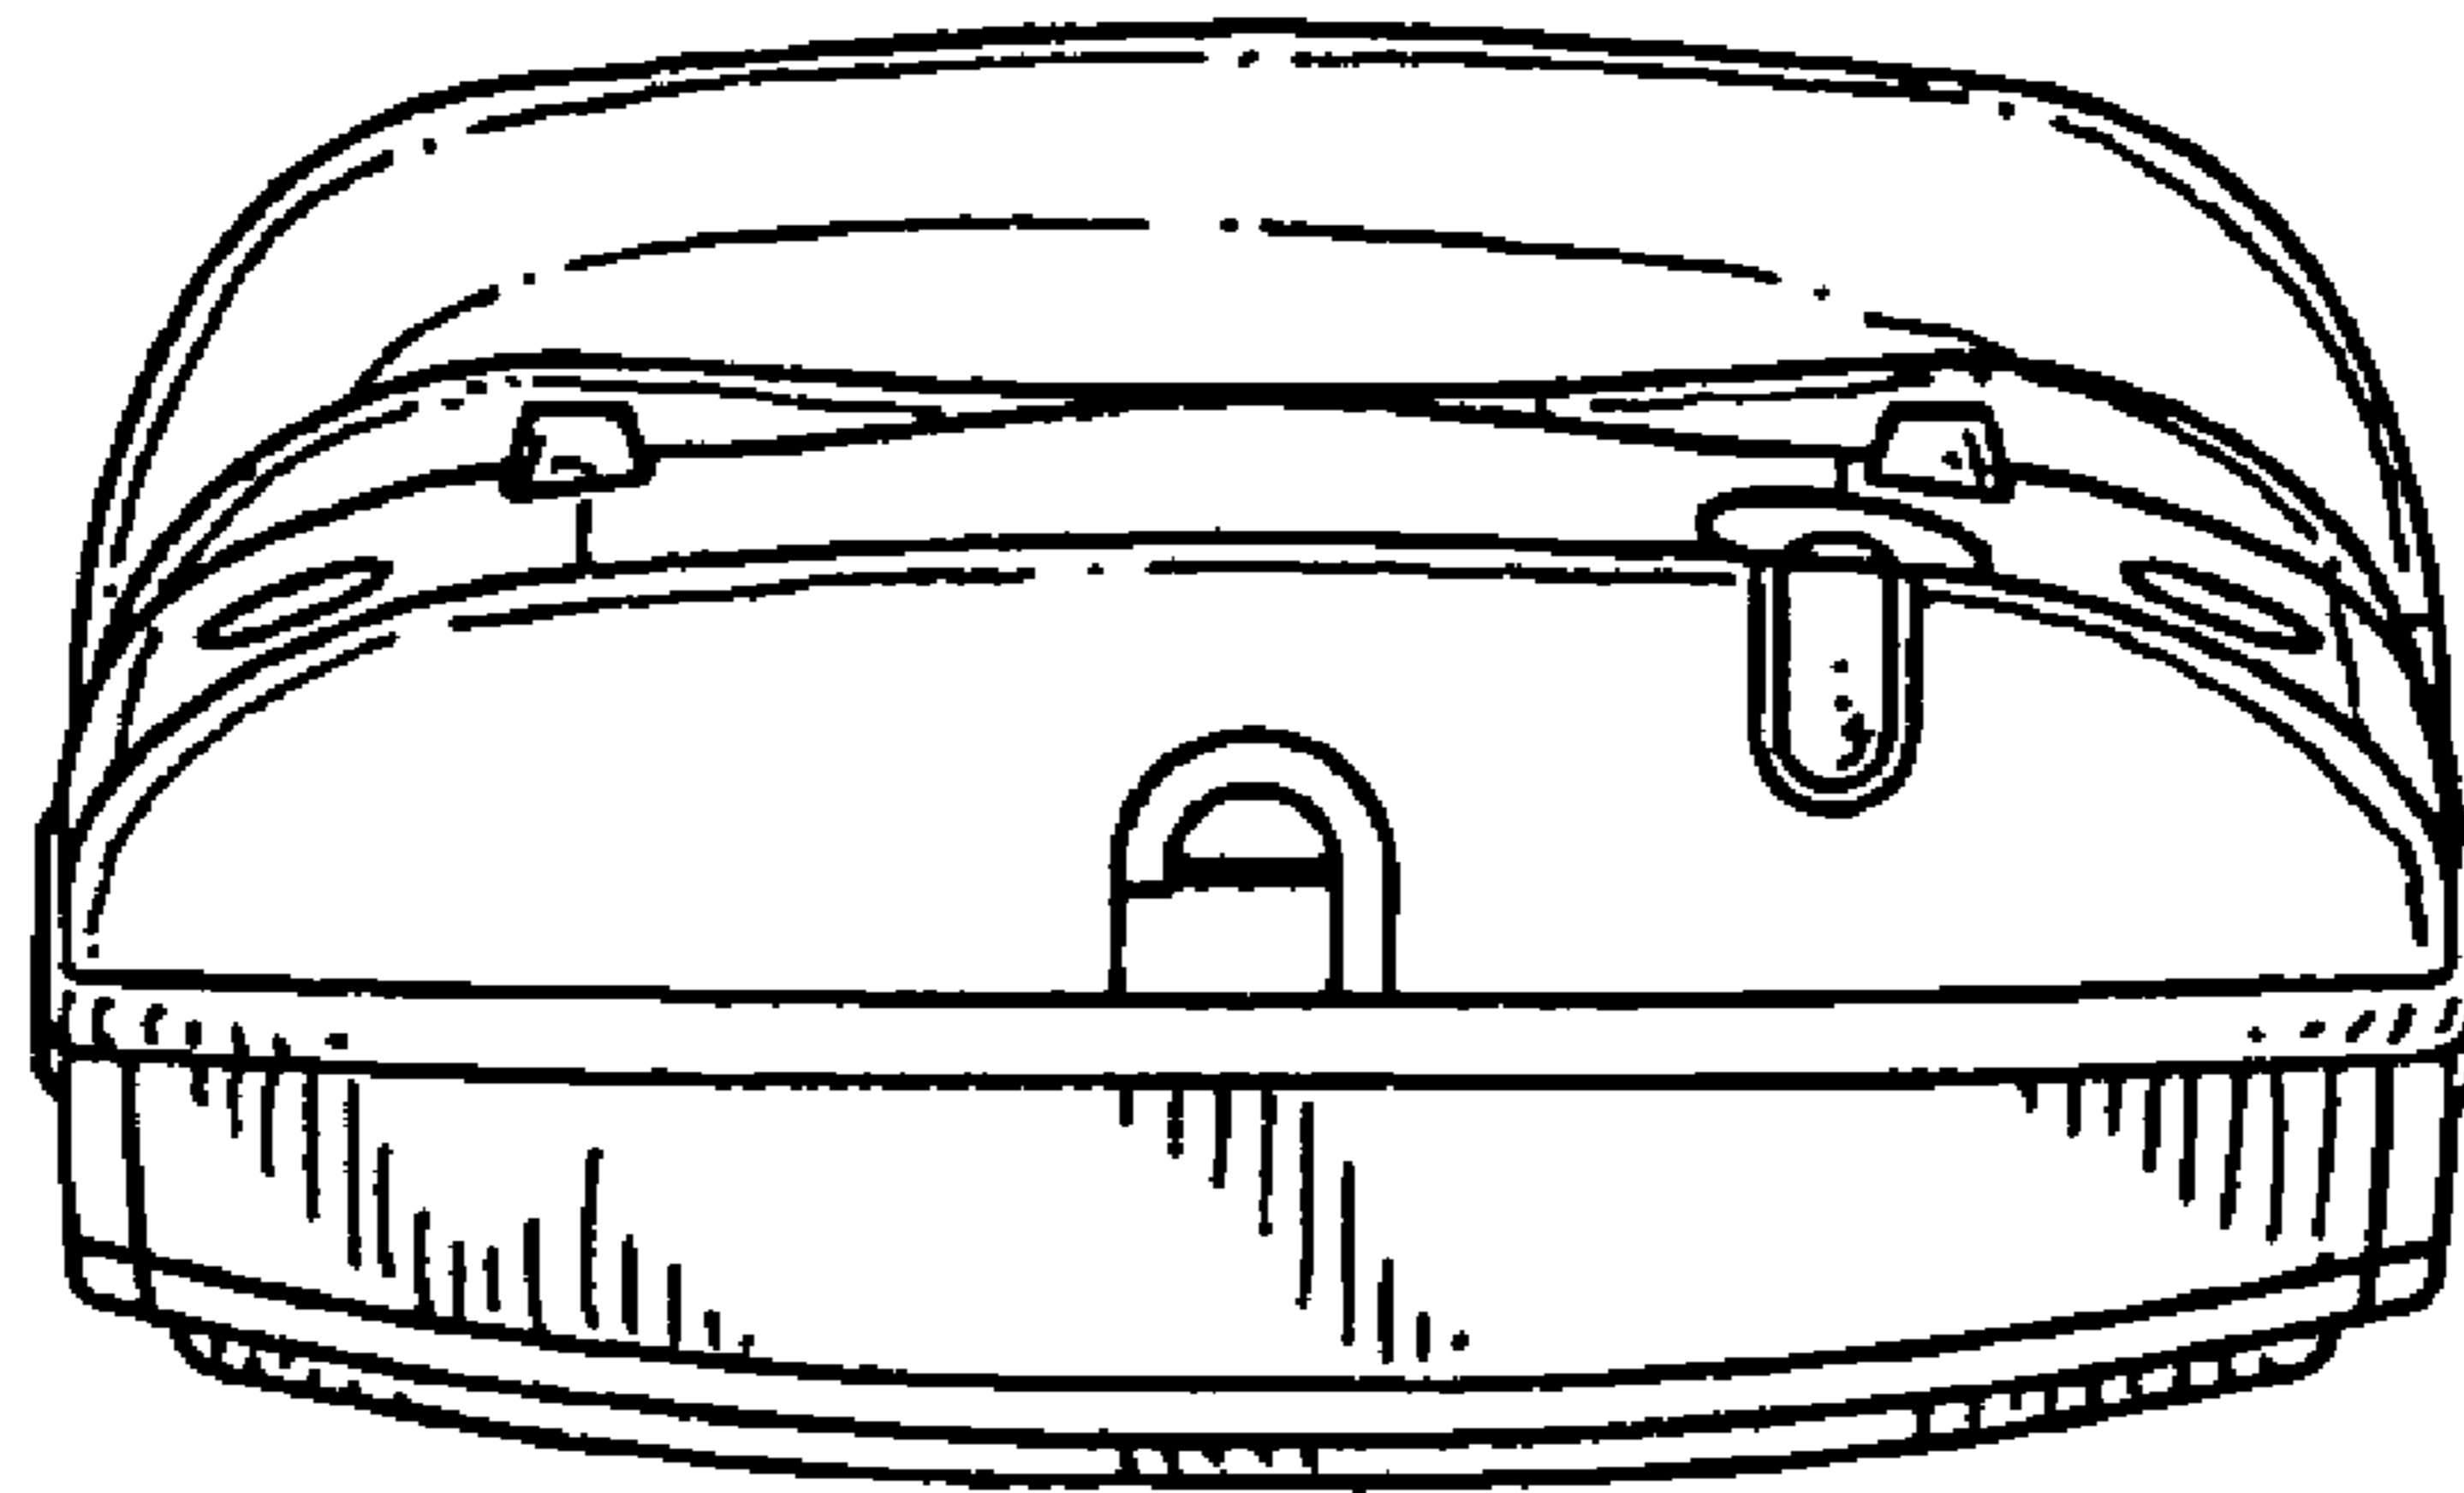


FIG. 6

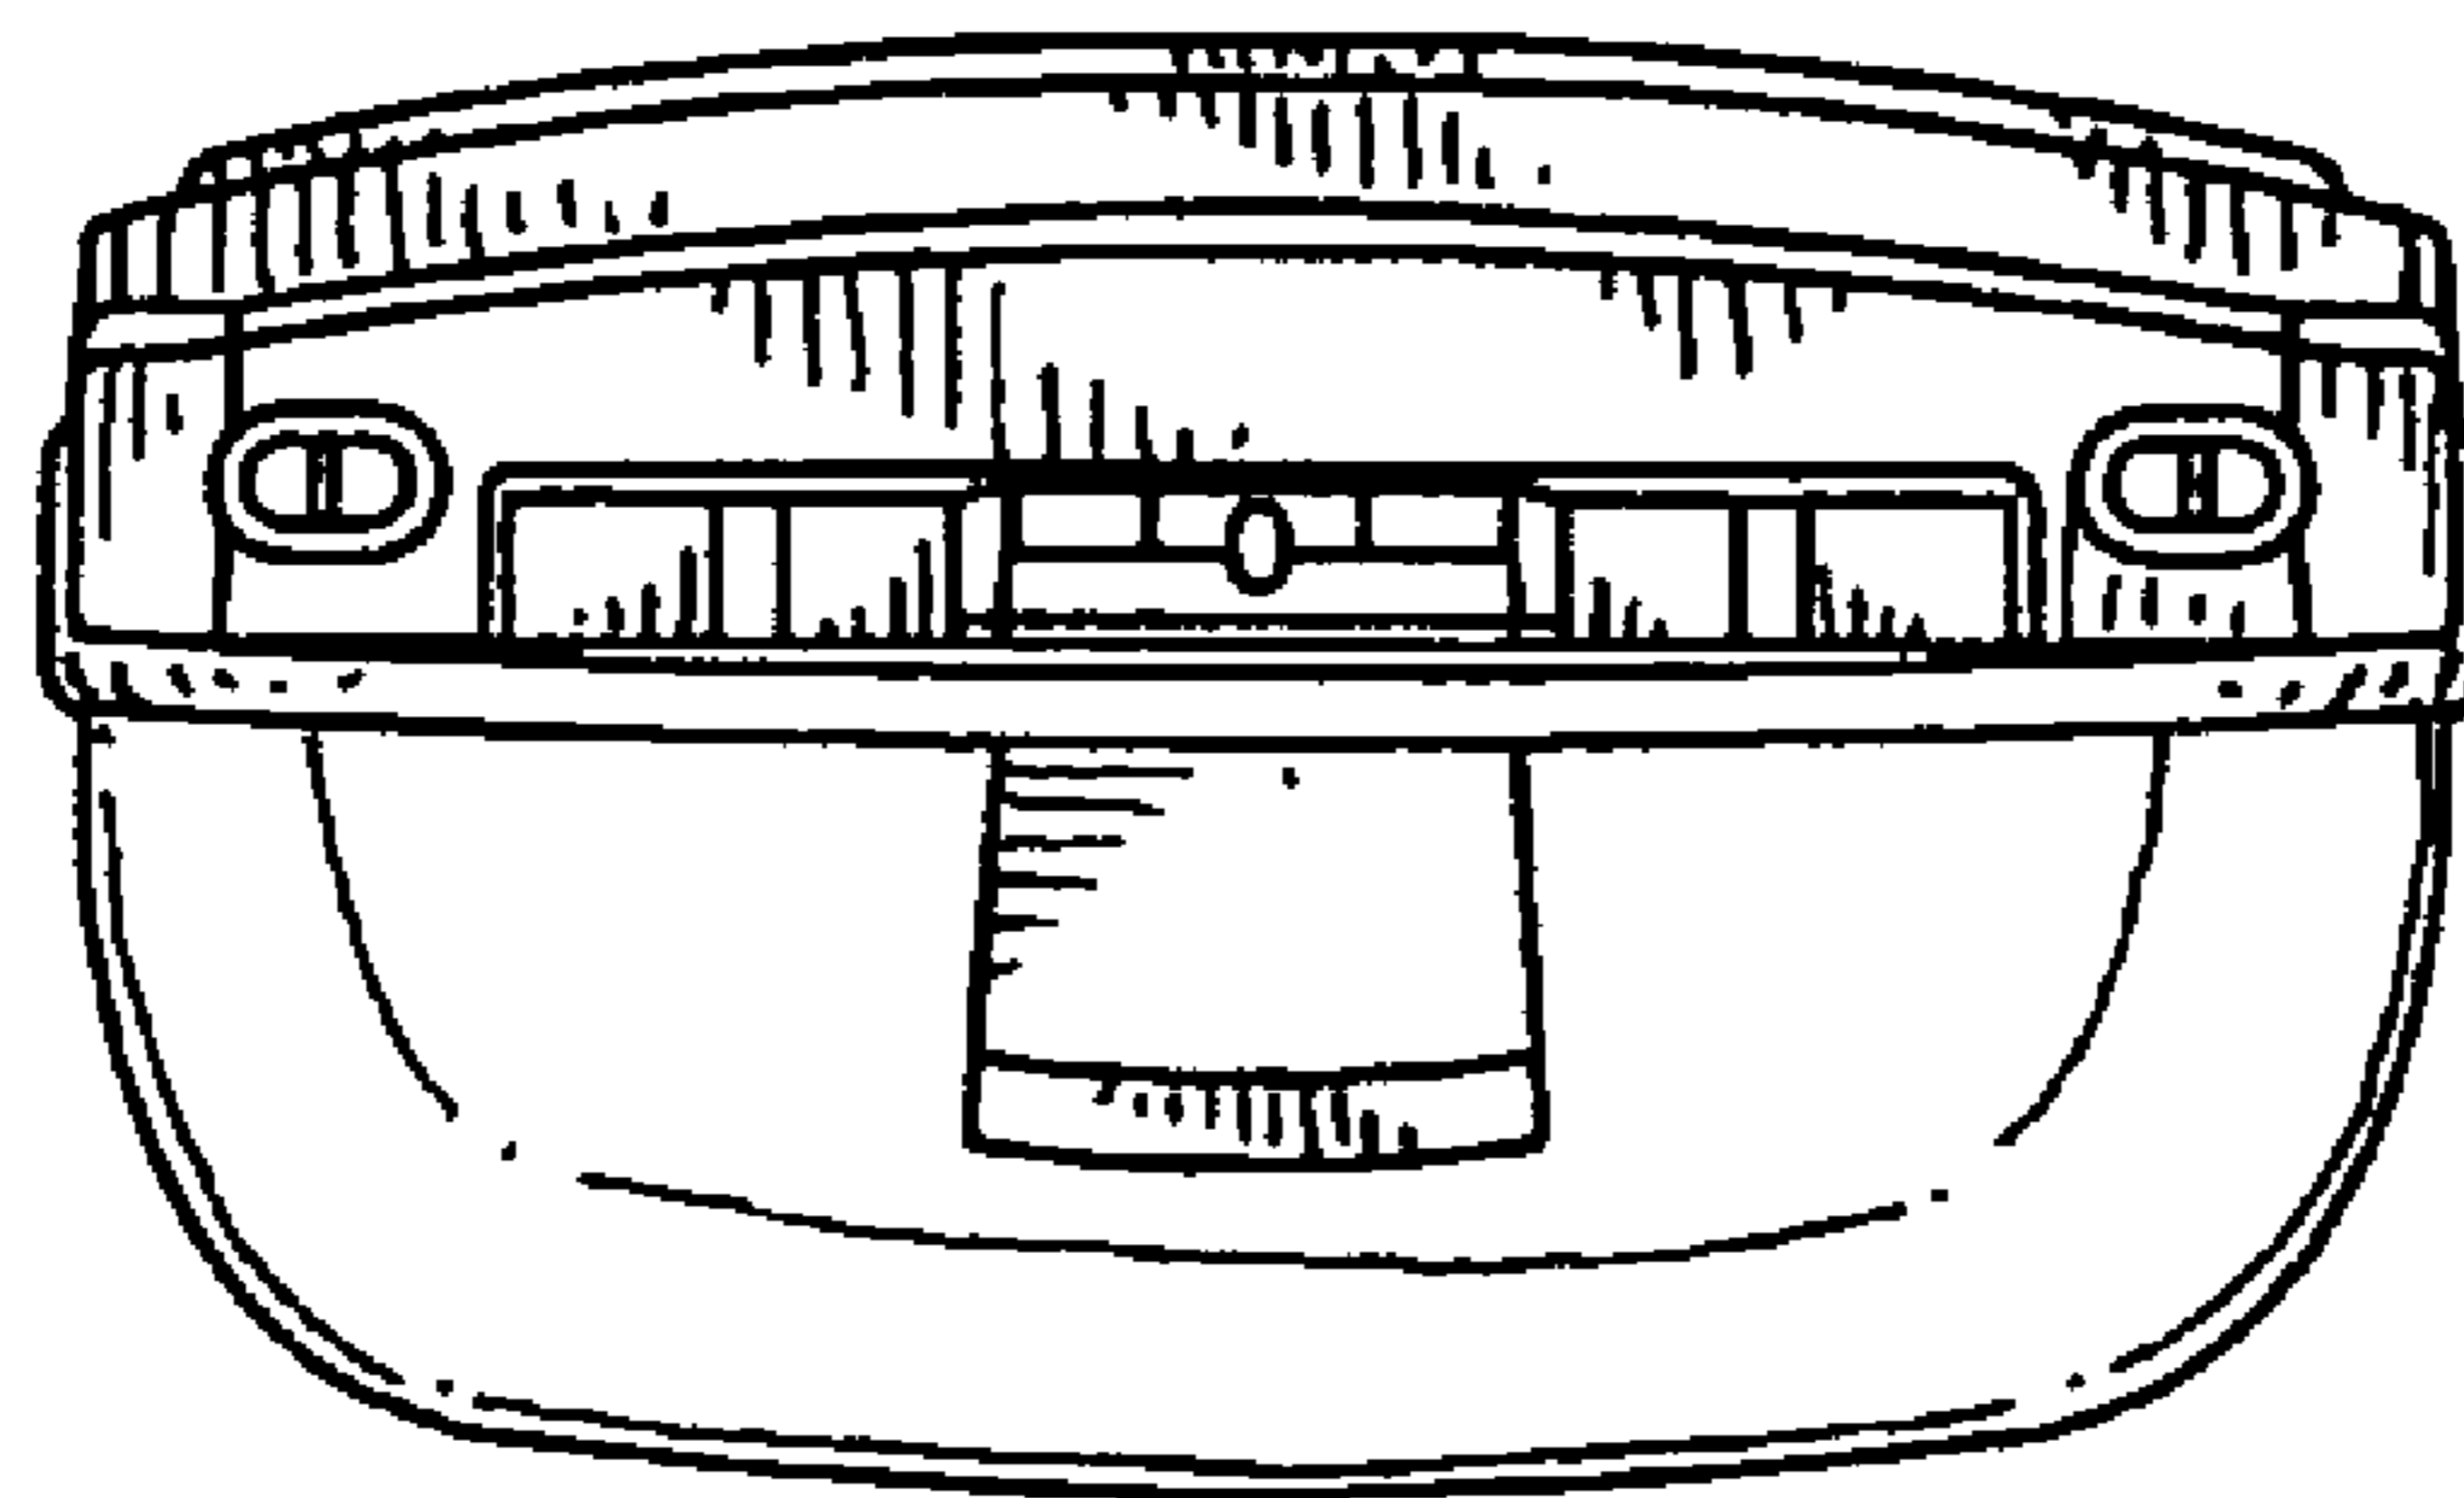


FIG. 7

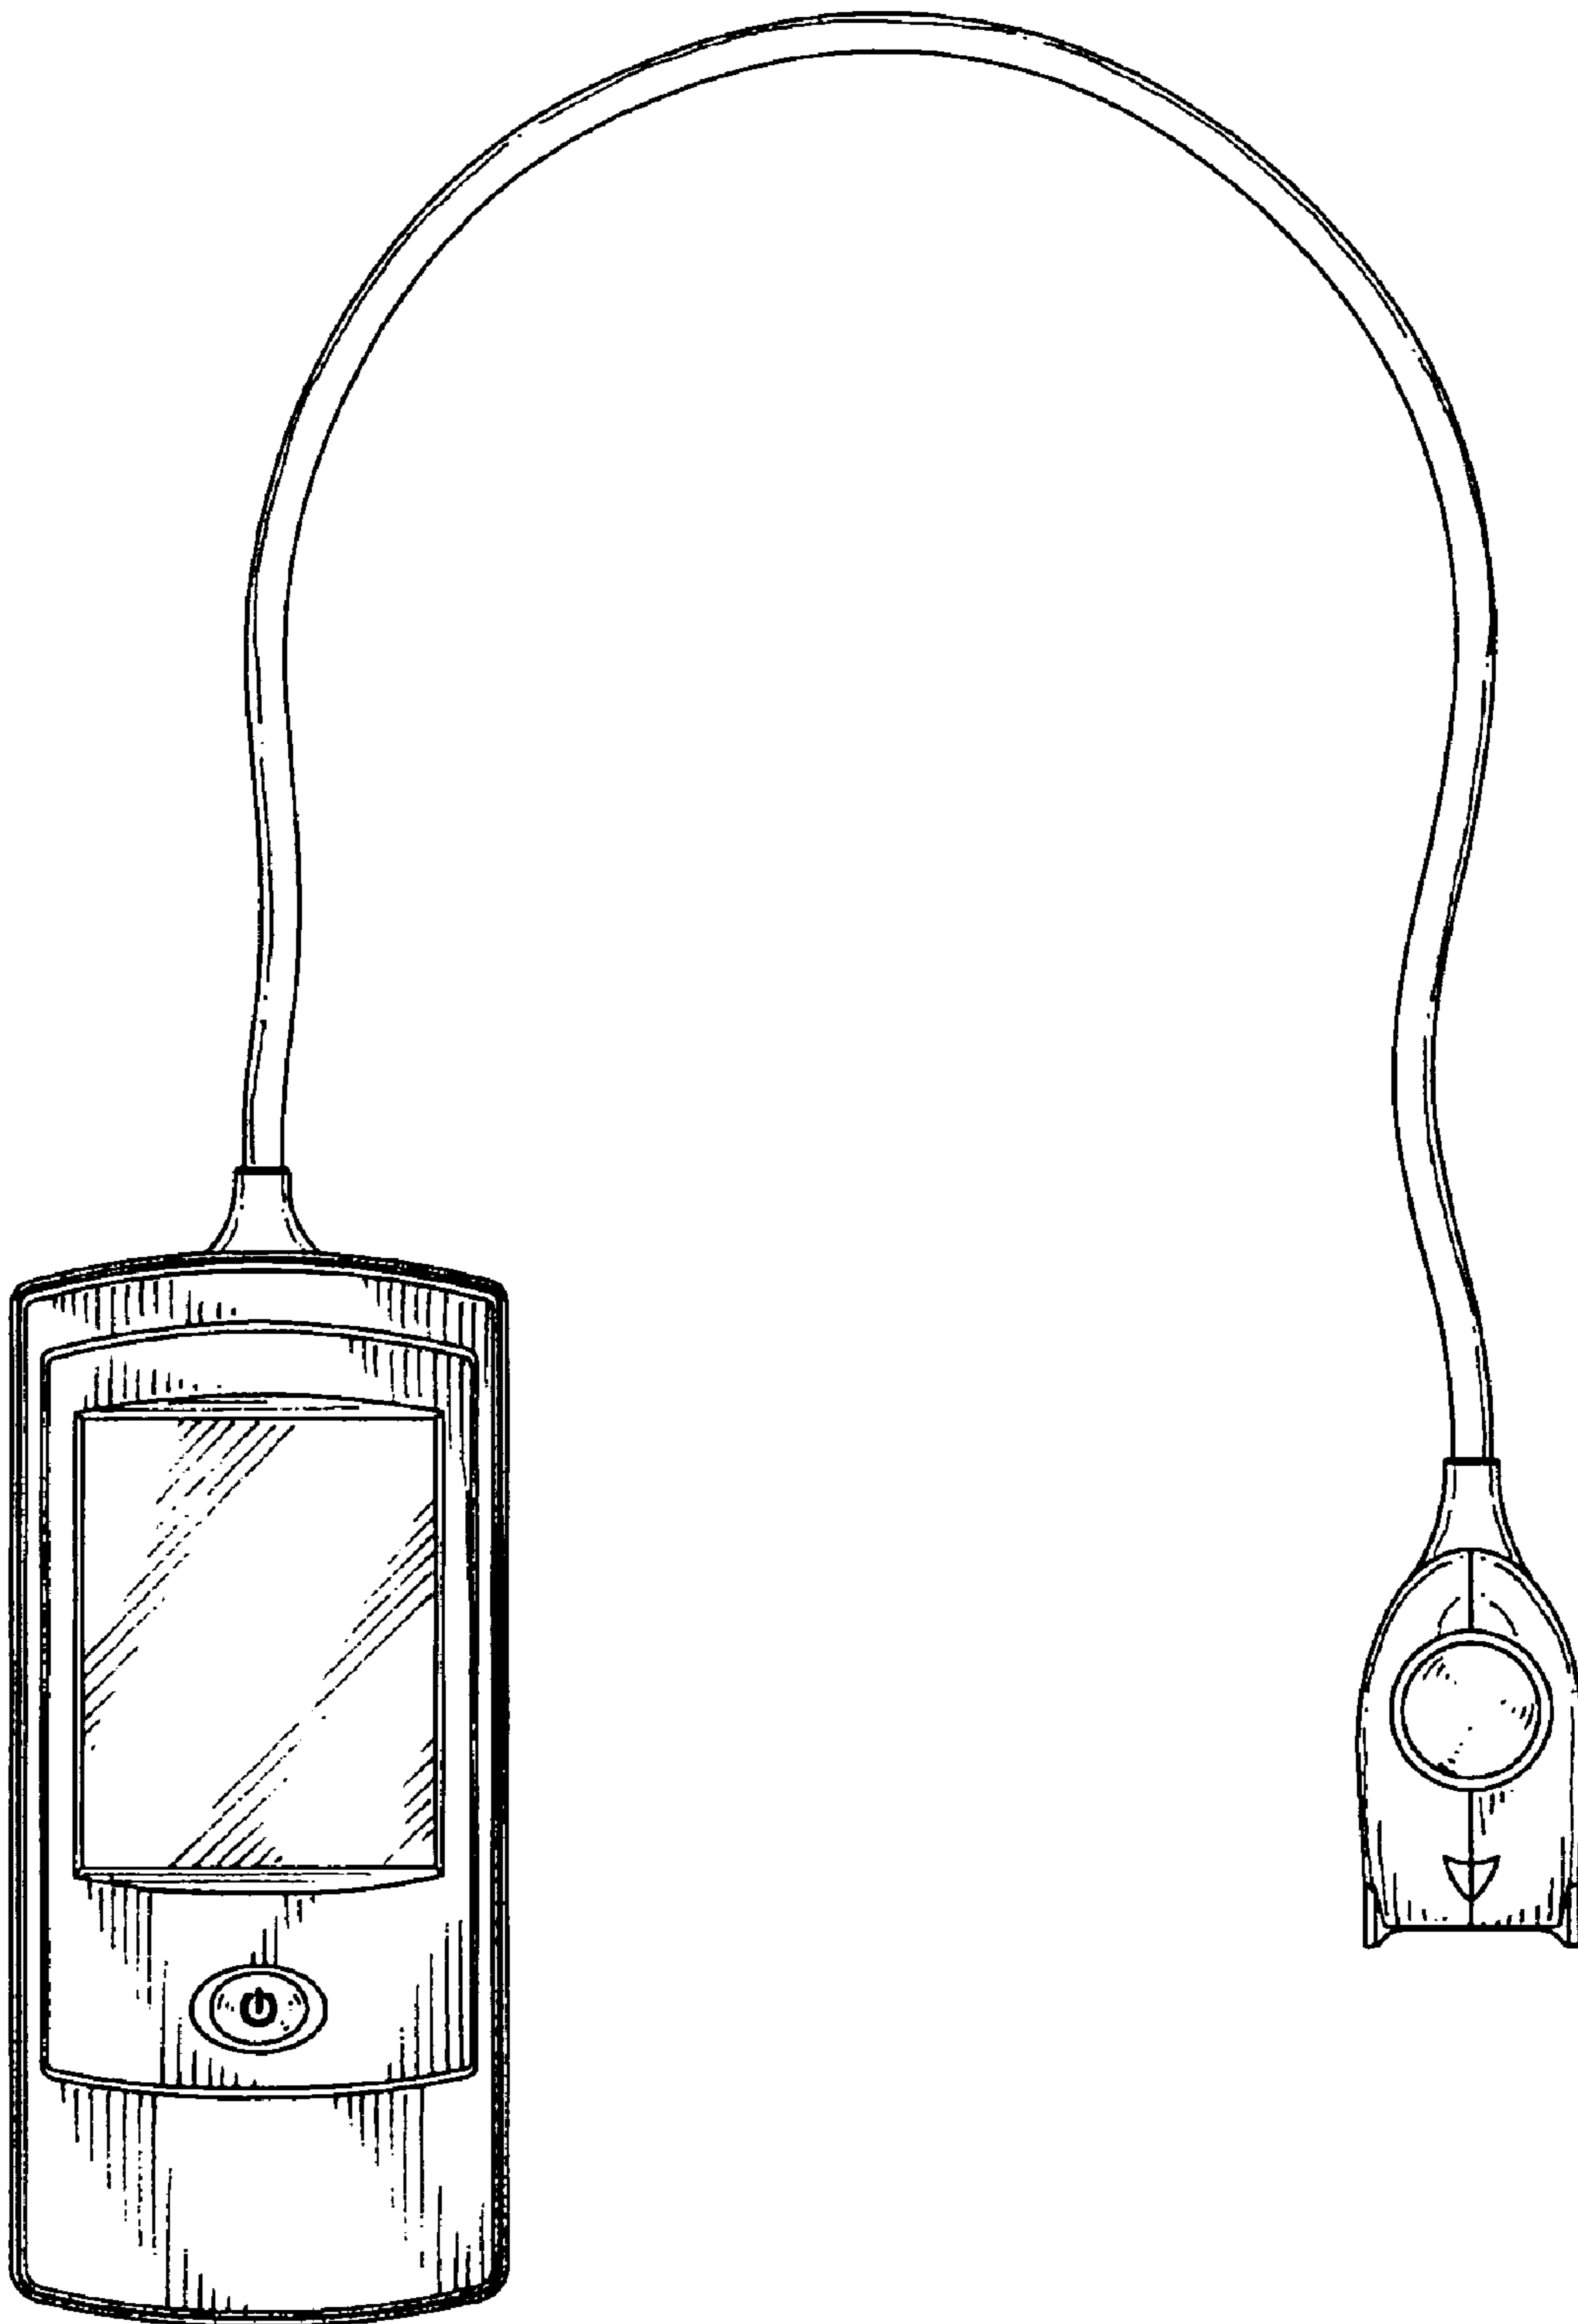


FIG. 8

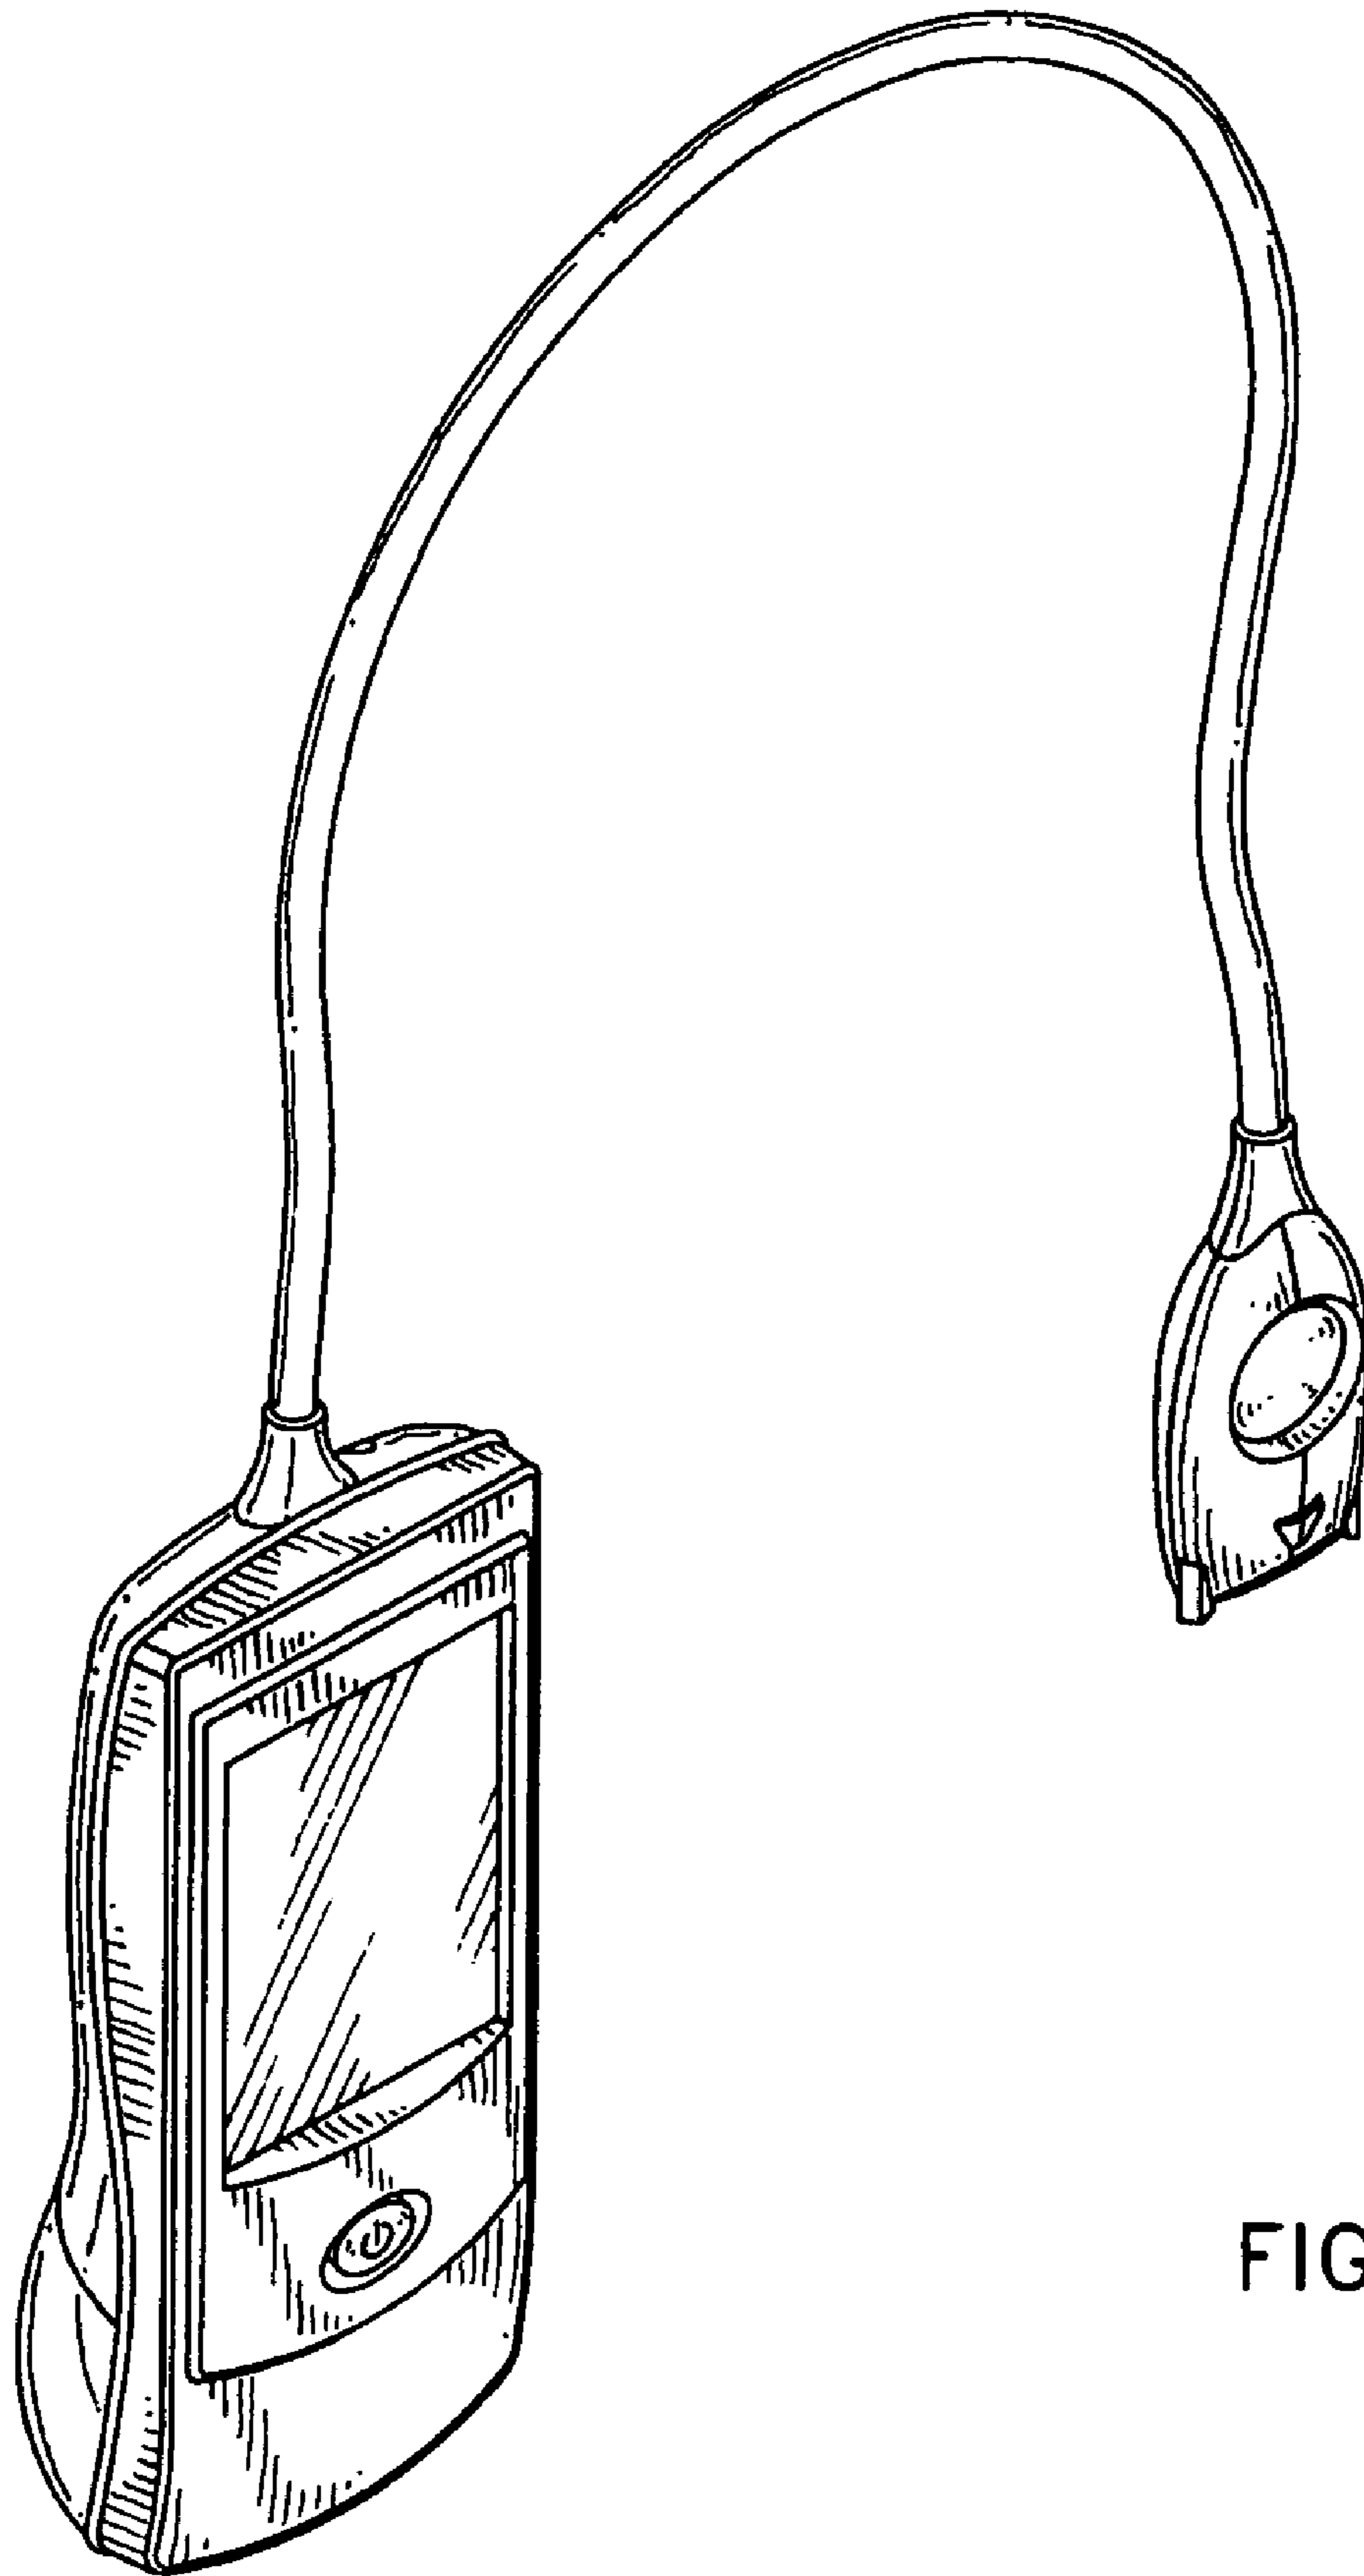


FIG. 9