



US00D566265S

(12) **United States Design Patent**  
**Hochman et al.**

(10) **Patent No.:** **US D566,265 S**

(45) **Date of Patent:** **\*\* Apr. 8, 2008**

(54) **DRIVE UNIT FOR ANESTHETIC**

D406,268 S \* 3/1999 Lamond et al. .... D15/7  
D423,665 S \* 4/2000 Herbst et al. .... D24/111  
D471,271 S \* 3/2003 Stromberg et al. .... D24/107

(75) Inventors: **Mark N. Hochman**, Great Neck, NY  
(US); **Donald Lamond**, Haworth, NJ  
(US)

\* cited by examiner

(73) Assignee: **Milestone Scientific Inc.**, Livingston,  
NJ (US)

*Primary Examiner*—Ian Simmons  
*Assistant Examiner*—Christopher Lee  
(74) *Attorney, Agent, or Firm*—Notaro & Michalos P.C.

(\*\*) Term: **14 Years**

(57) **CLAIM**

(21) Appl. No.: **29/276,307**

The ornamental design for a drive unit for anesthetic, as shown.

(22) Filed: **Jan. 22, 2007**

(51) **LOC (8) Cl.** ..... **24-01**

(52) **U.S. Cl.** ..... **D24/107**

(58) **Field of Classification Search** ..... D24/107,  
D24/111, 108, 156, 176, 221, 177; D15/7,  
D15/8, 9; 604/131, 151, 152, 232; 433/80  
See application file for complete search history.

**DESCRIPTION**


FIG. 1 is a front top right perspective of a drive unit for anesthetic showing our new design therefor;  
FIG. 2 is a right elevational view thereof;  
FIG. 3 is a left side elevational view thereof;  
FIG. 4 is a rear elevational view thereof;  
FIG. 5 is a front elevational view thereof; and,  
FIG. 6 is top plan view thereof.

(56) **References Cited**

**U.S. PATENT DOCUMENTS**

D312,307 S \* 11/1990 Leibson et al. .... D24/107

**1 Claim, 6 Drawing Sheets**

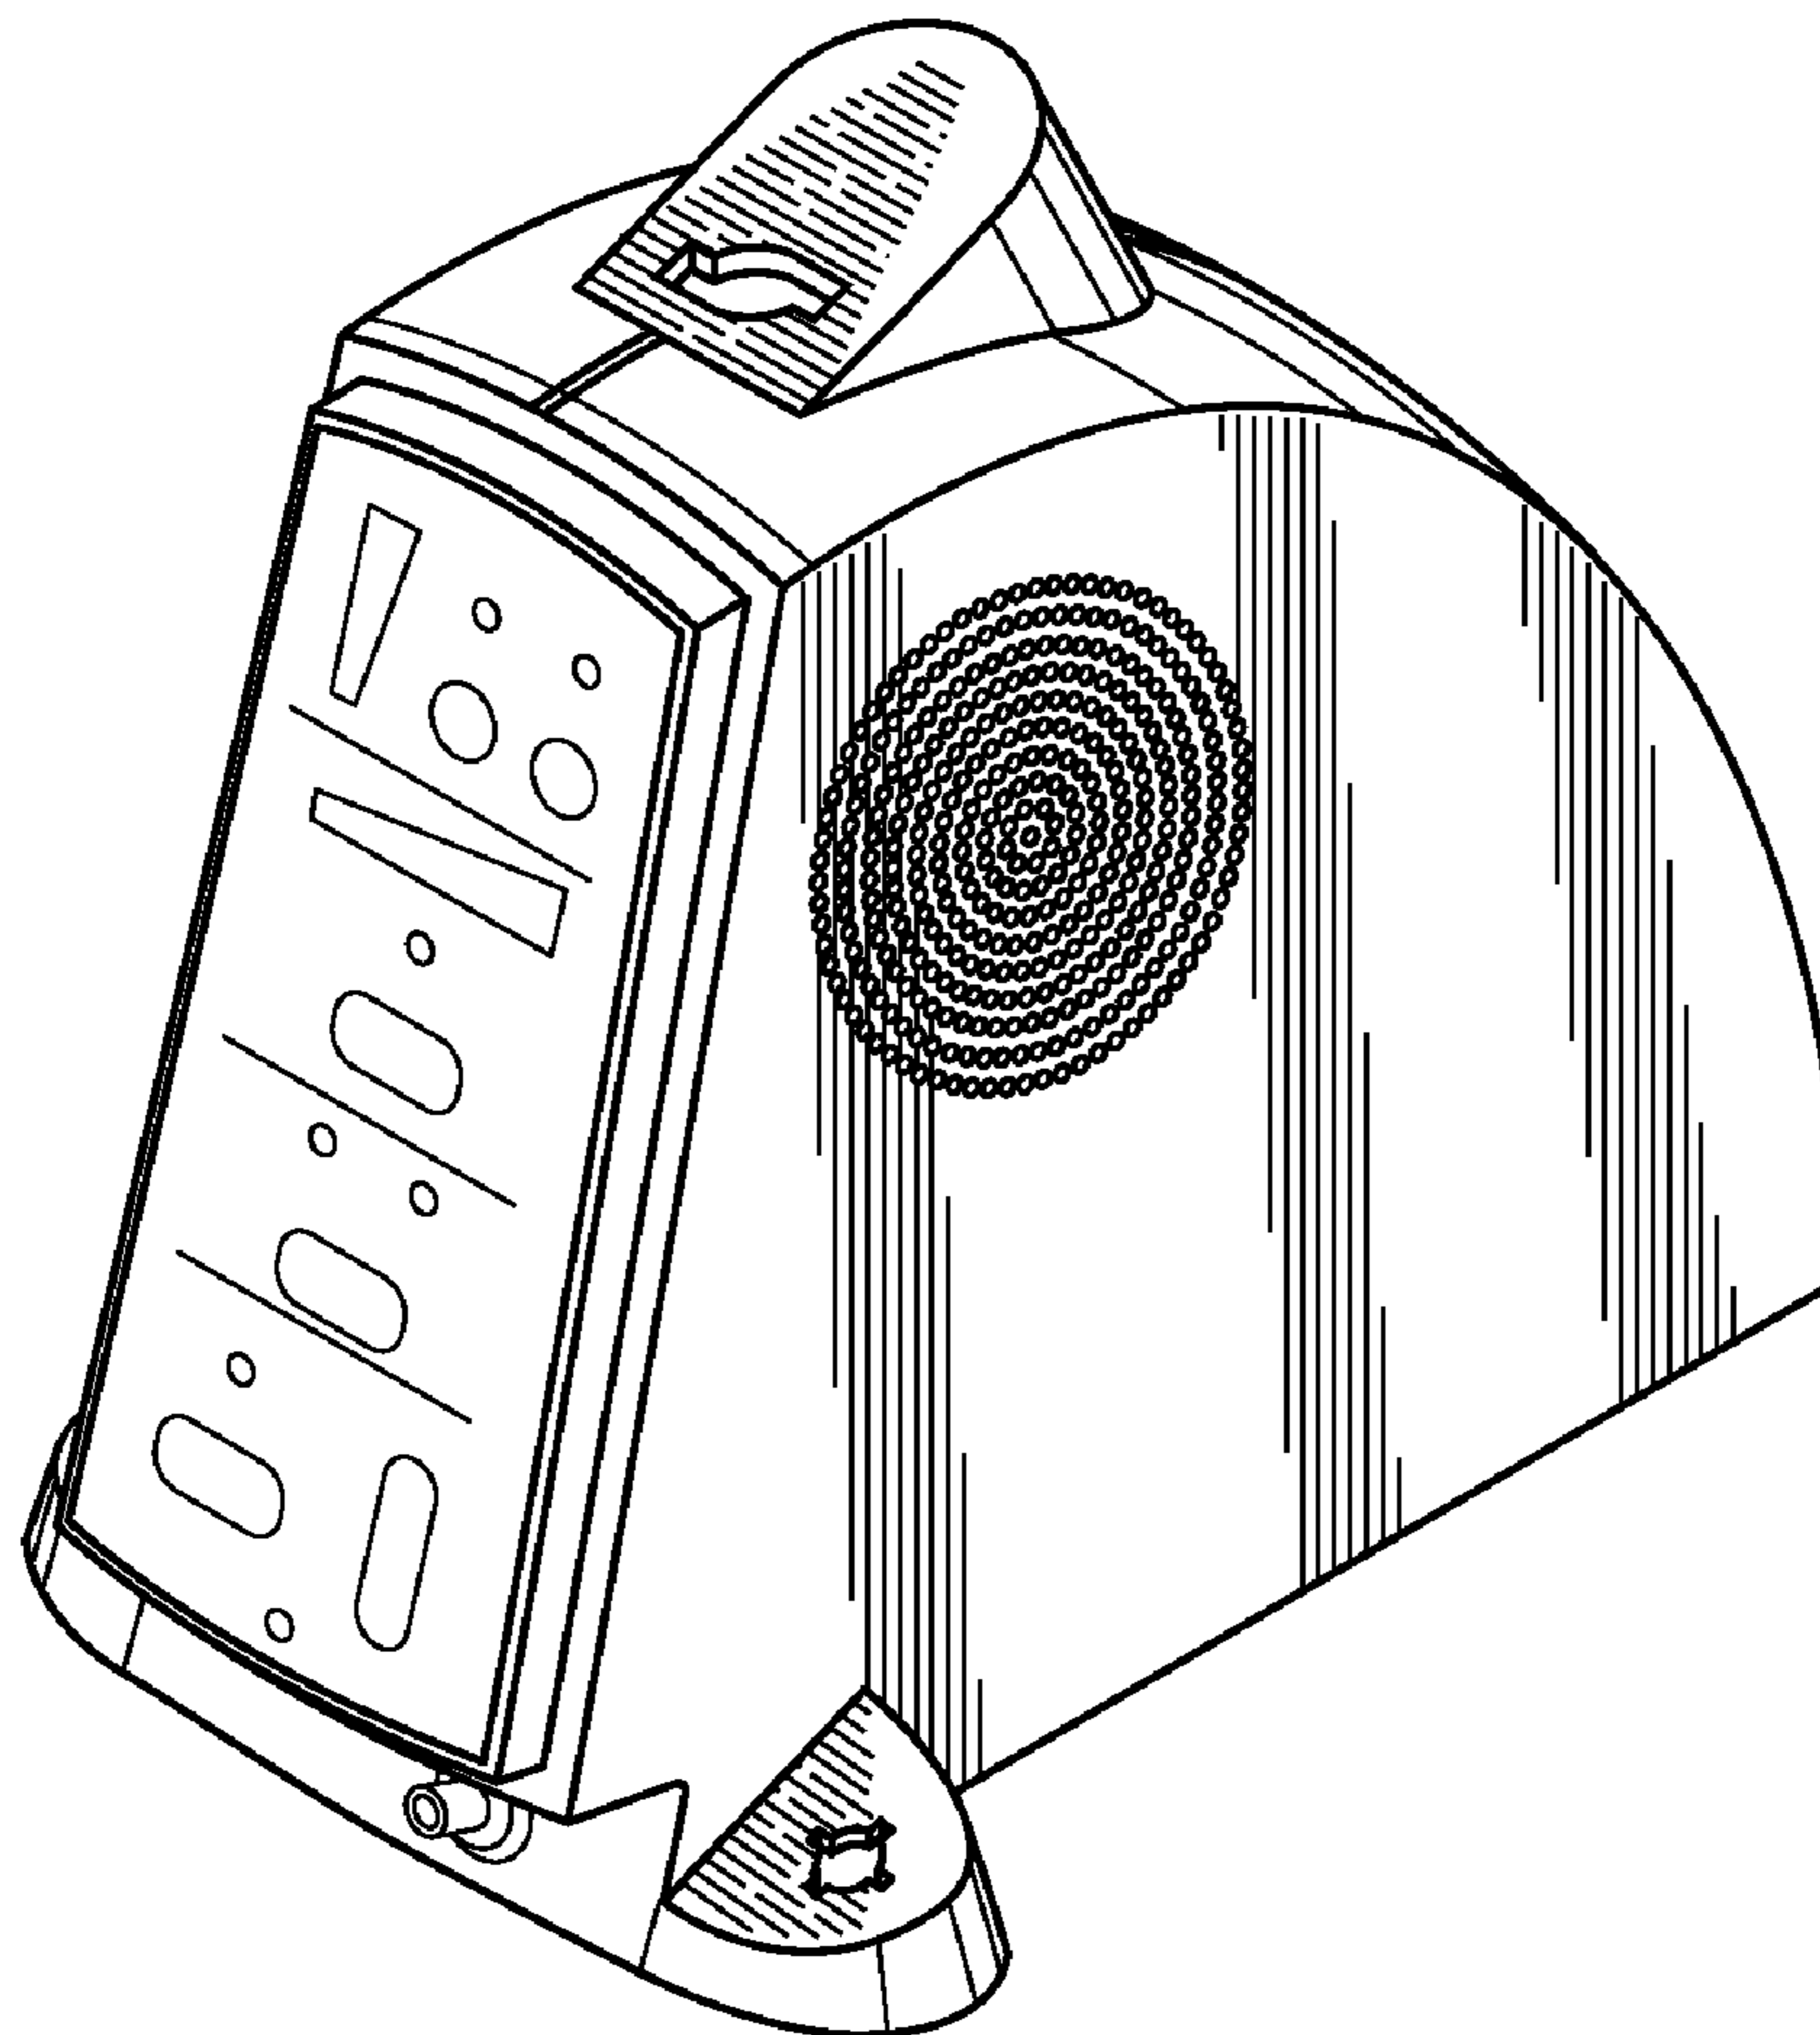

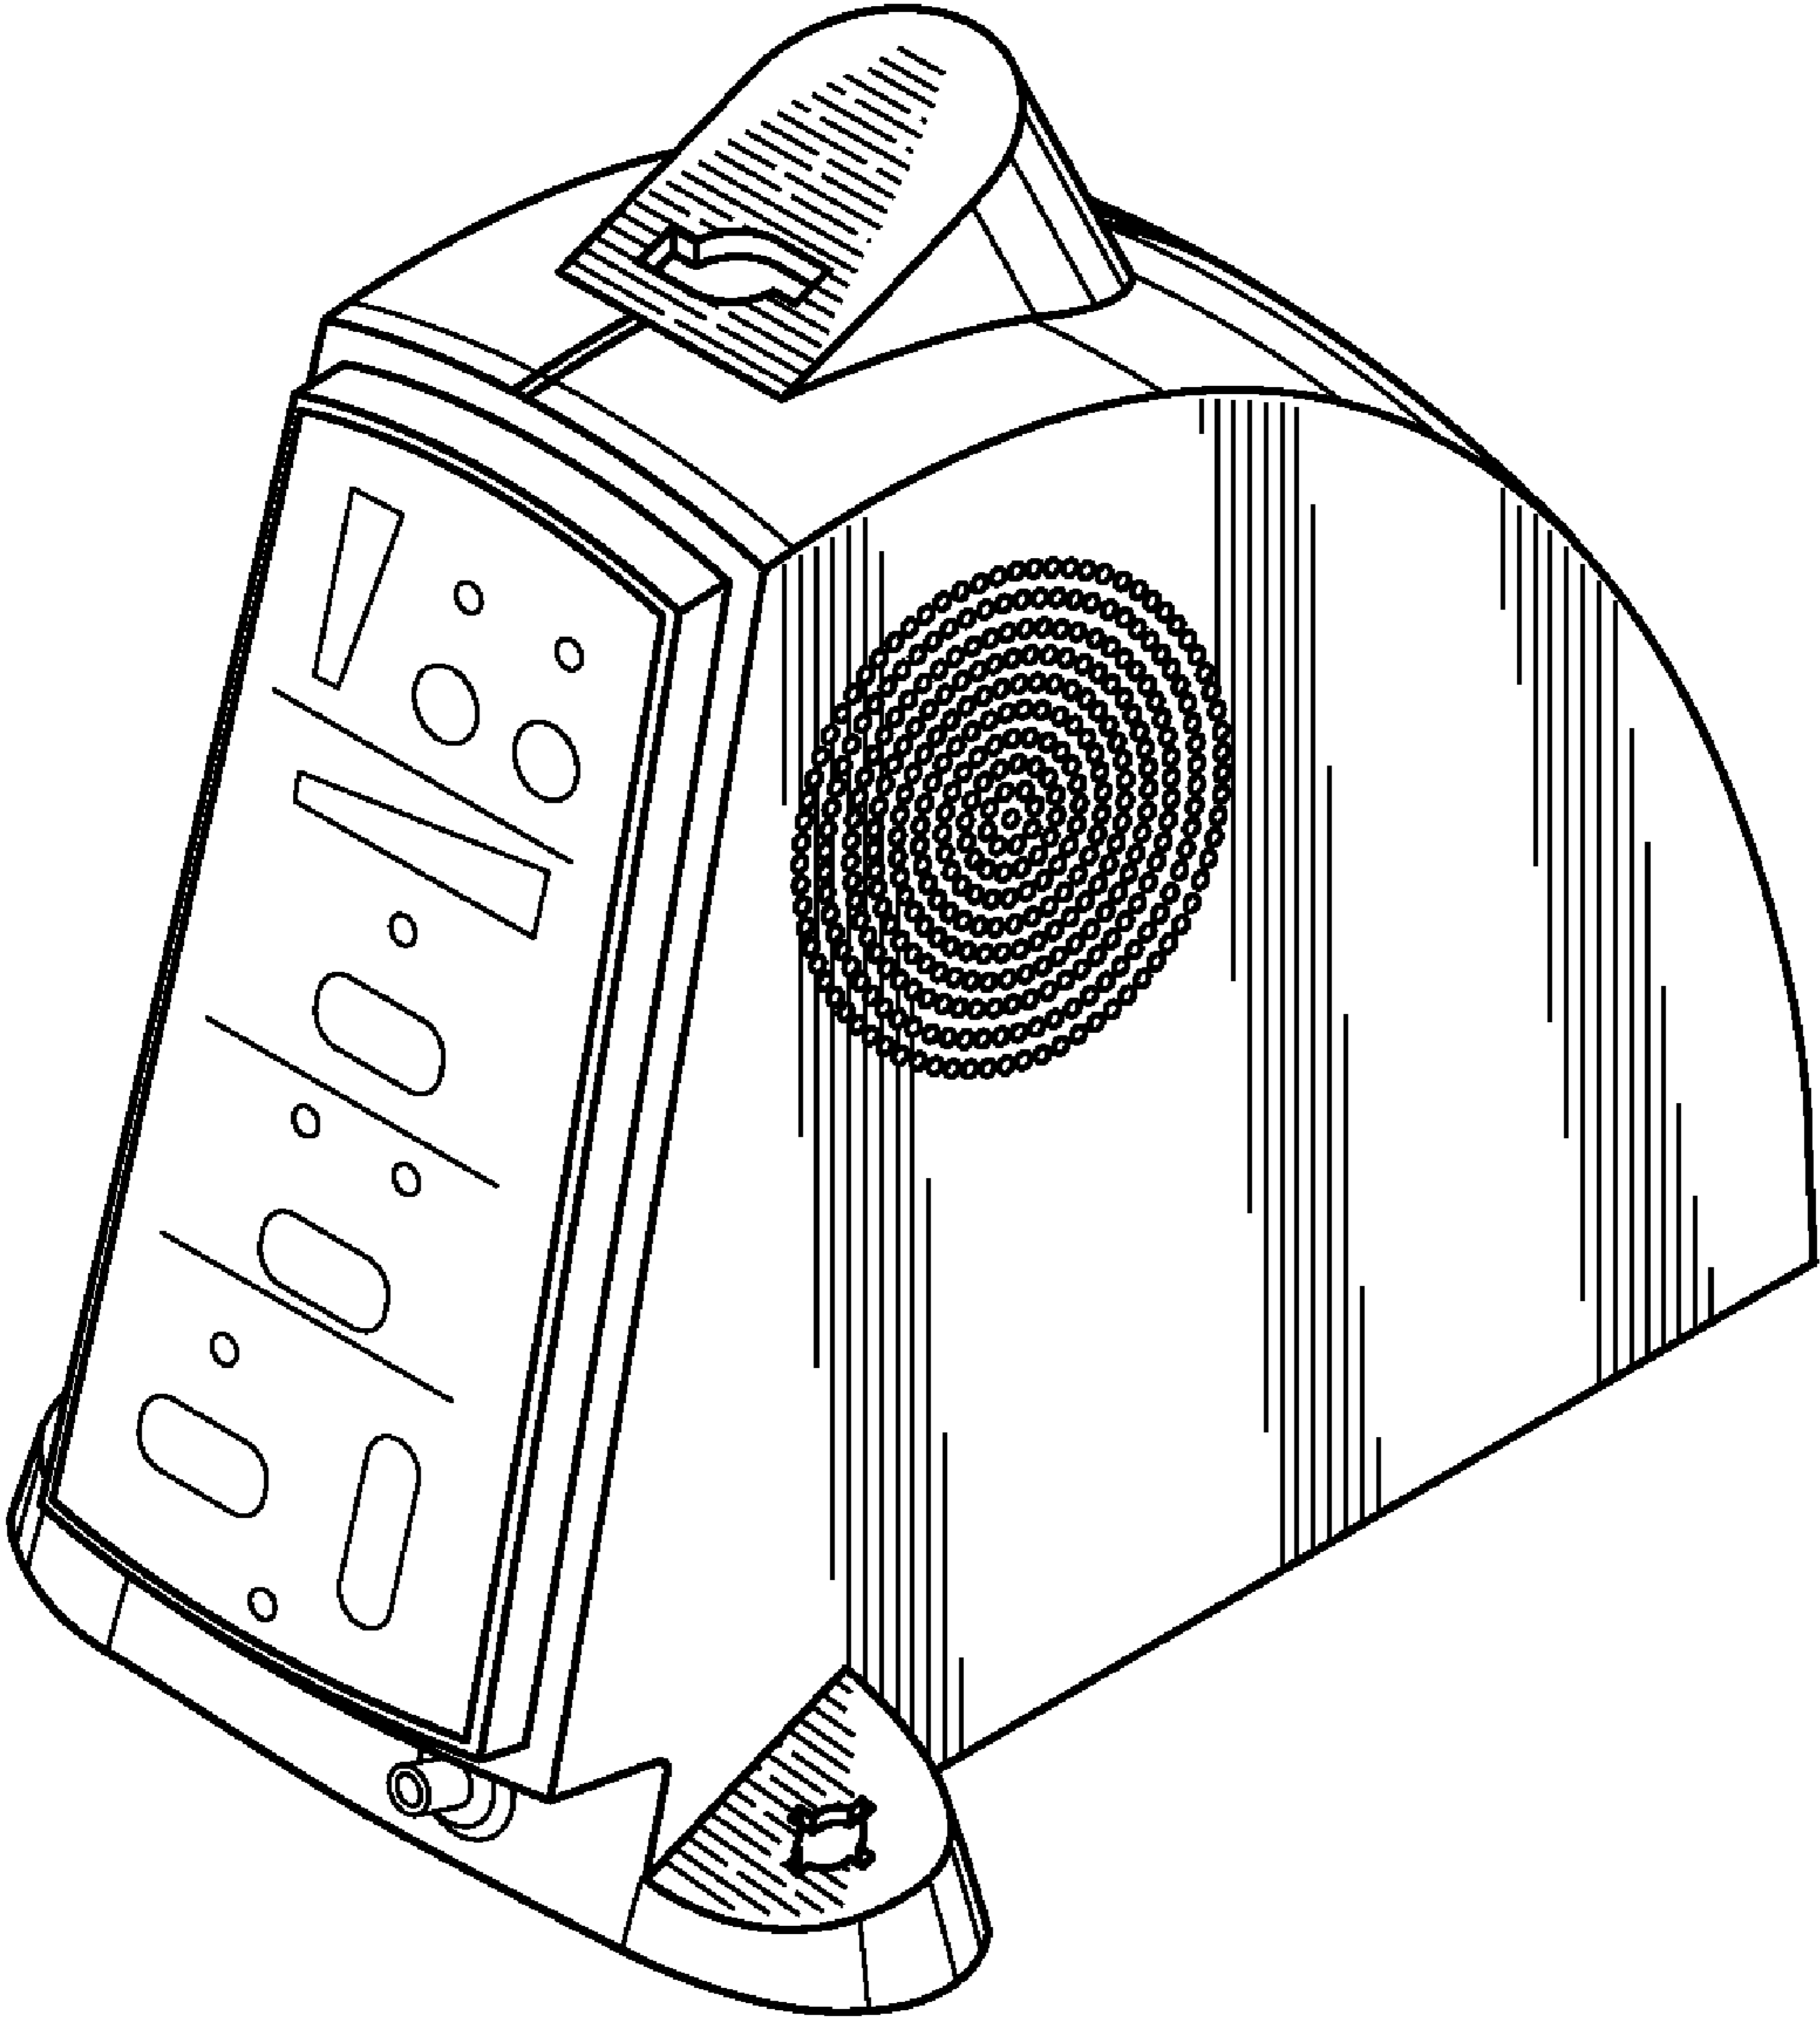


FIG. 1

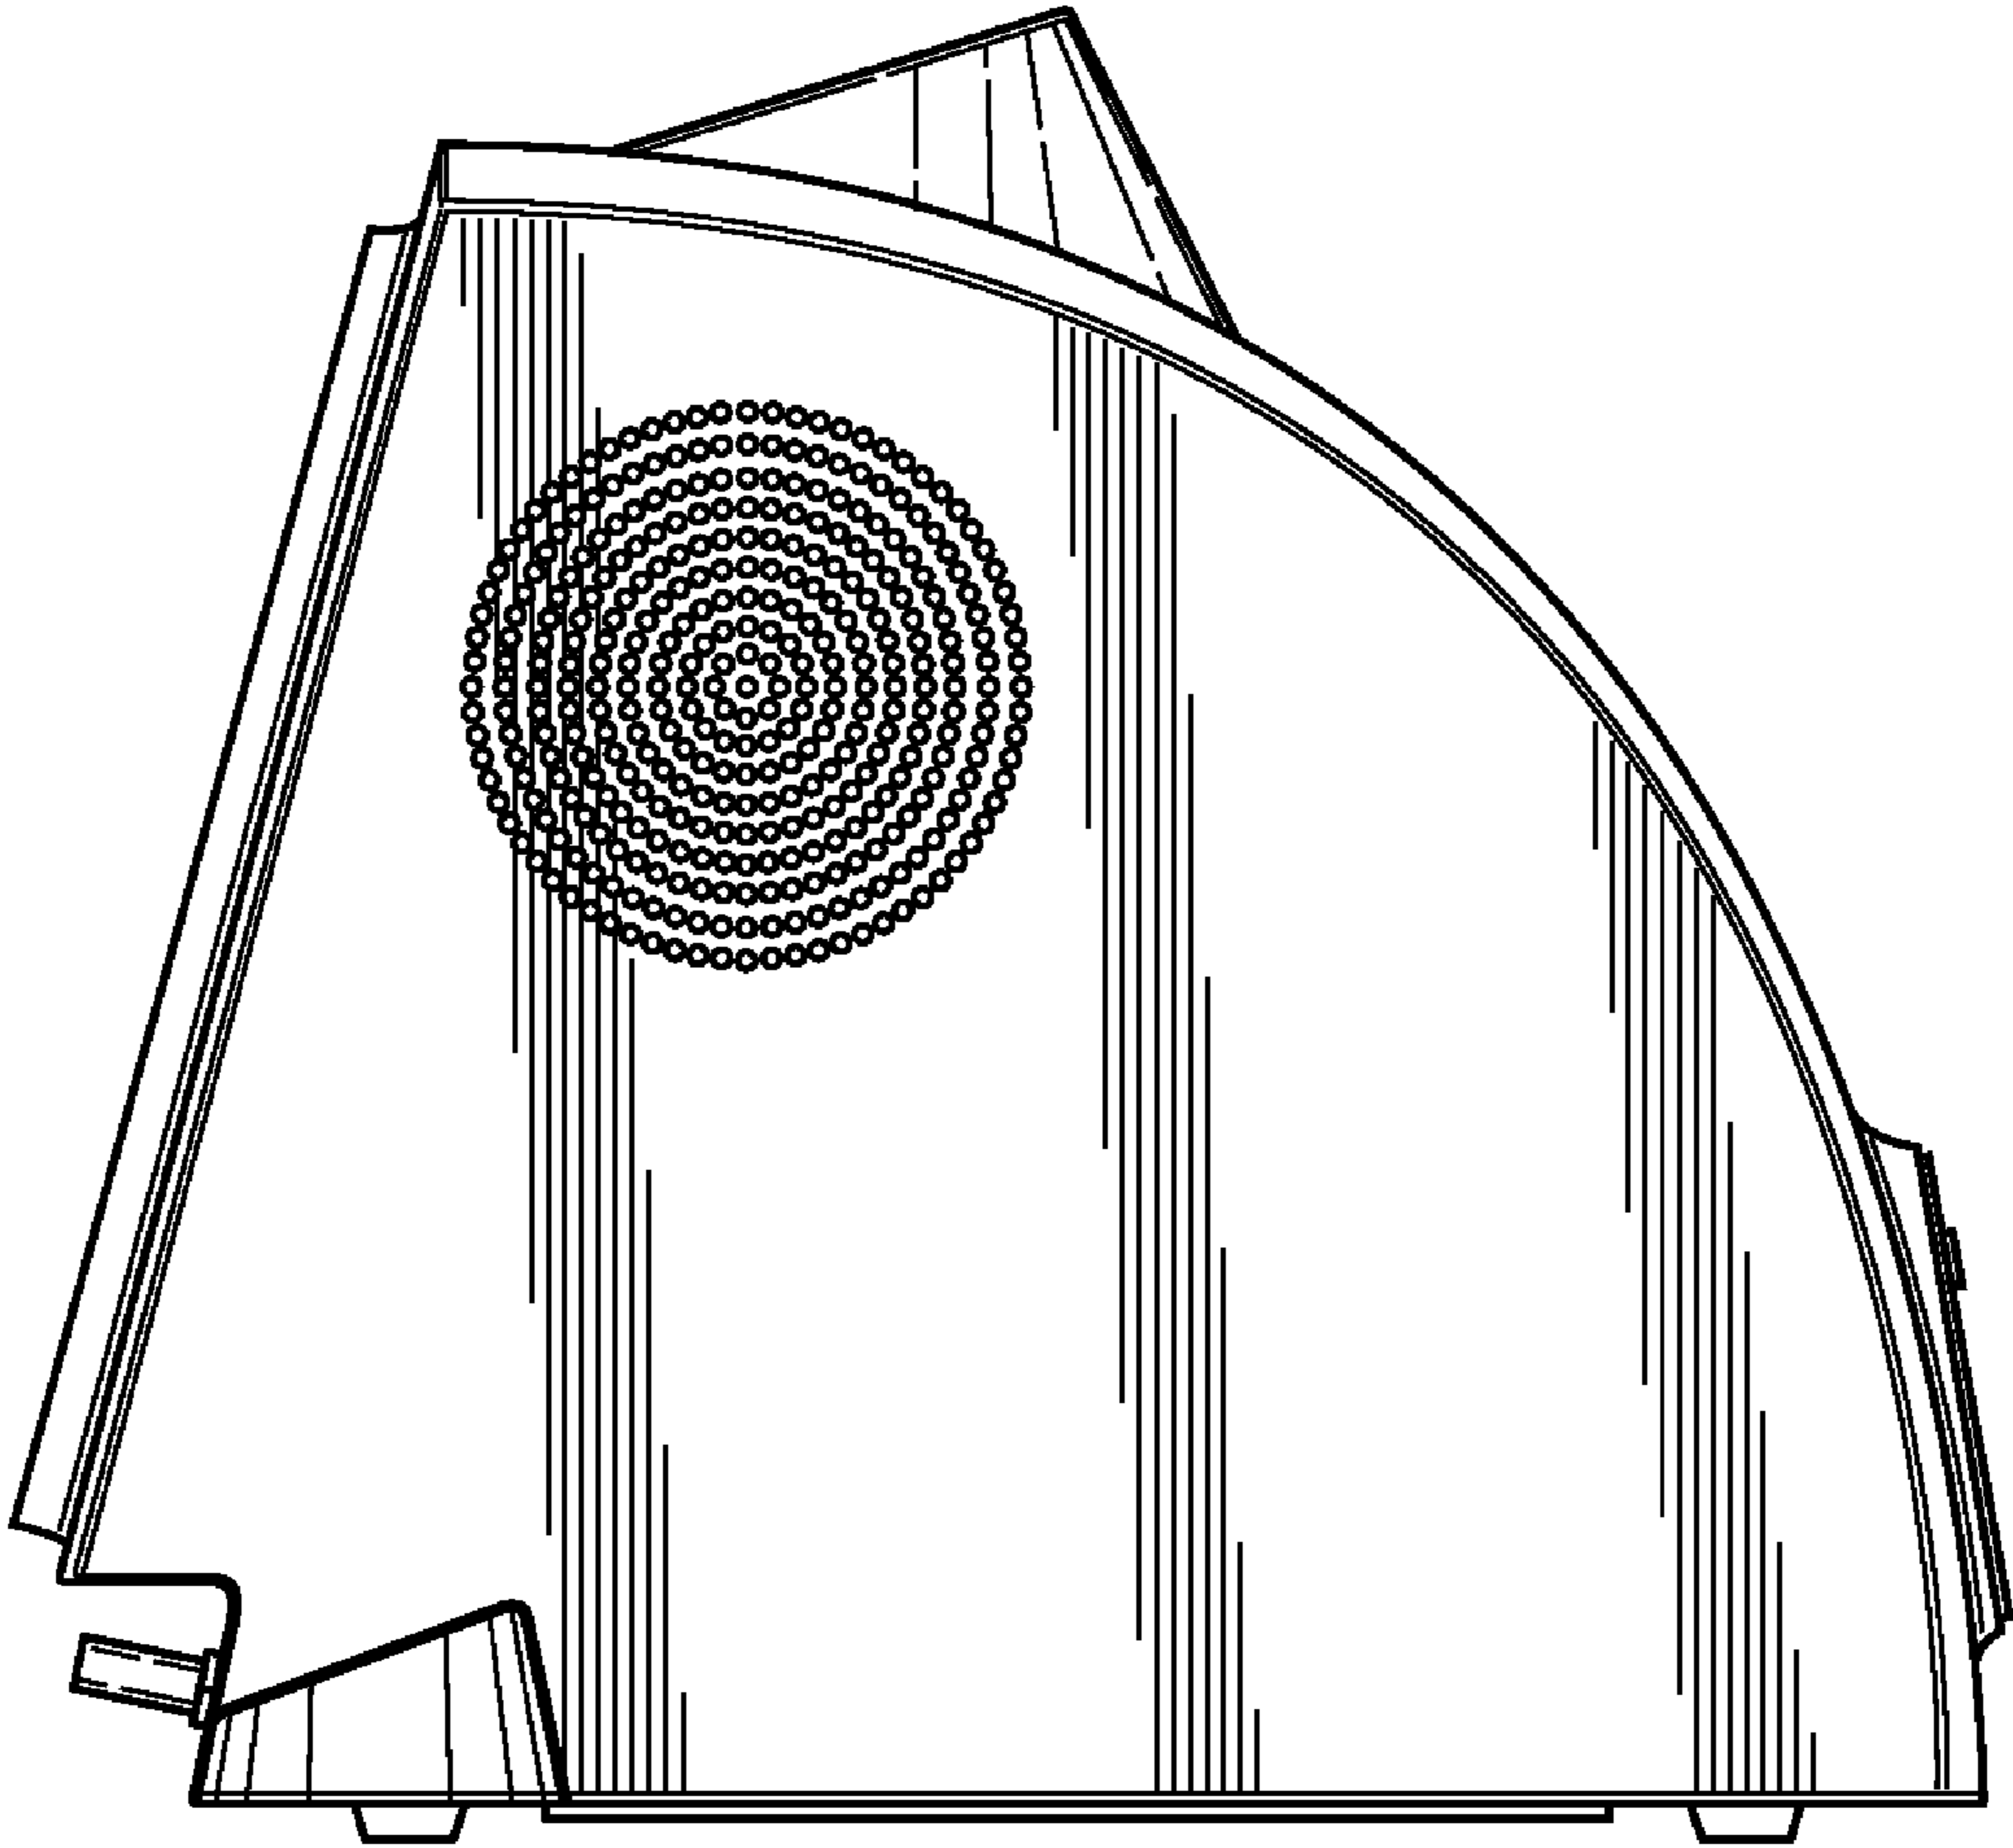


FIG. 2

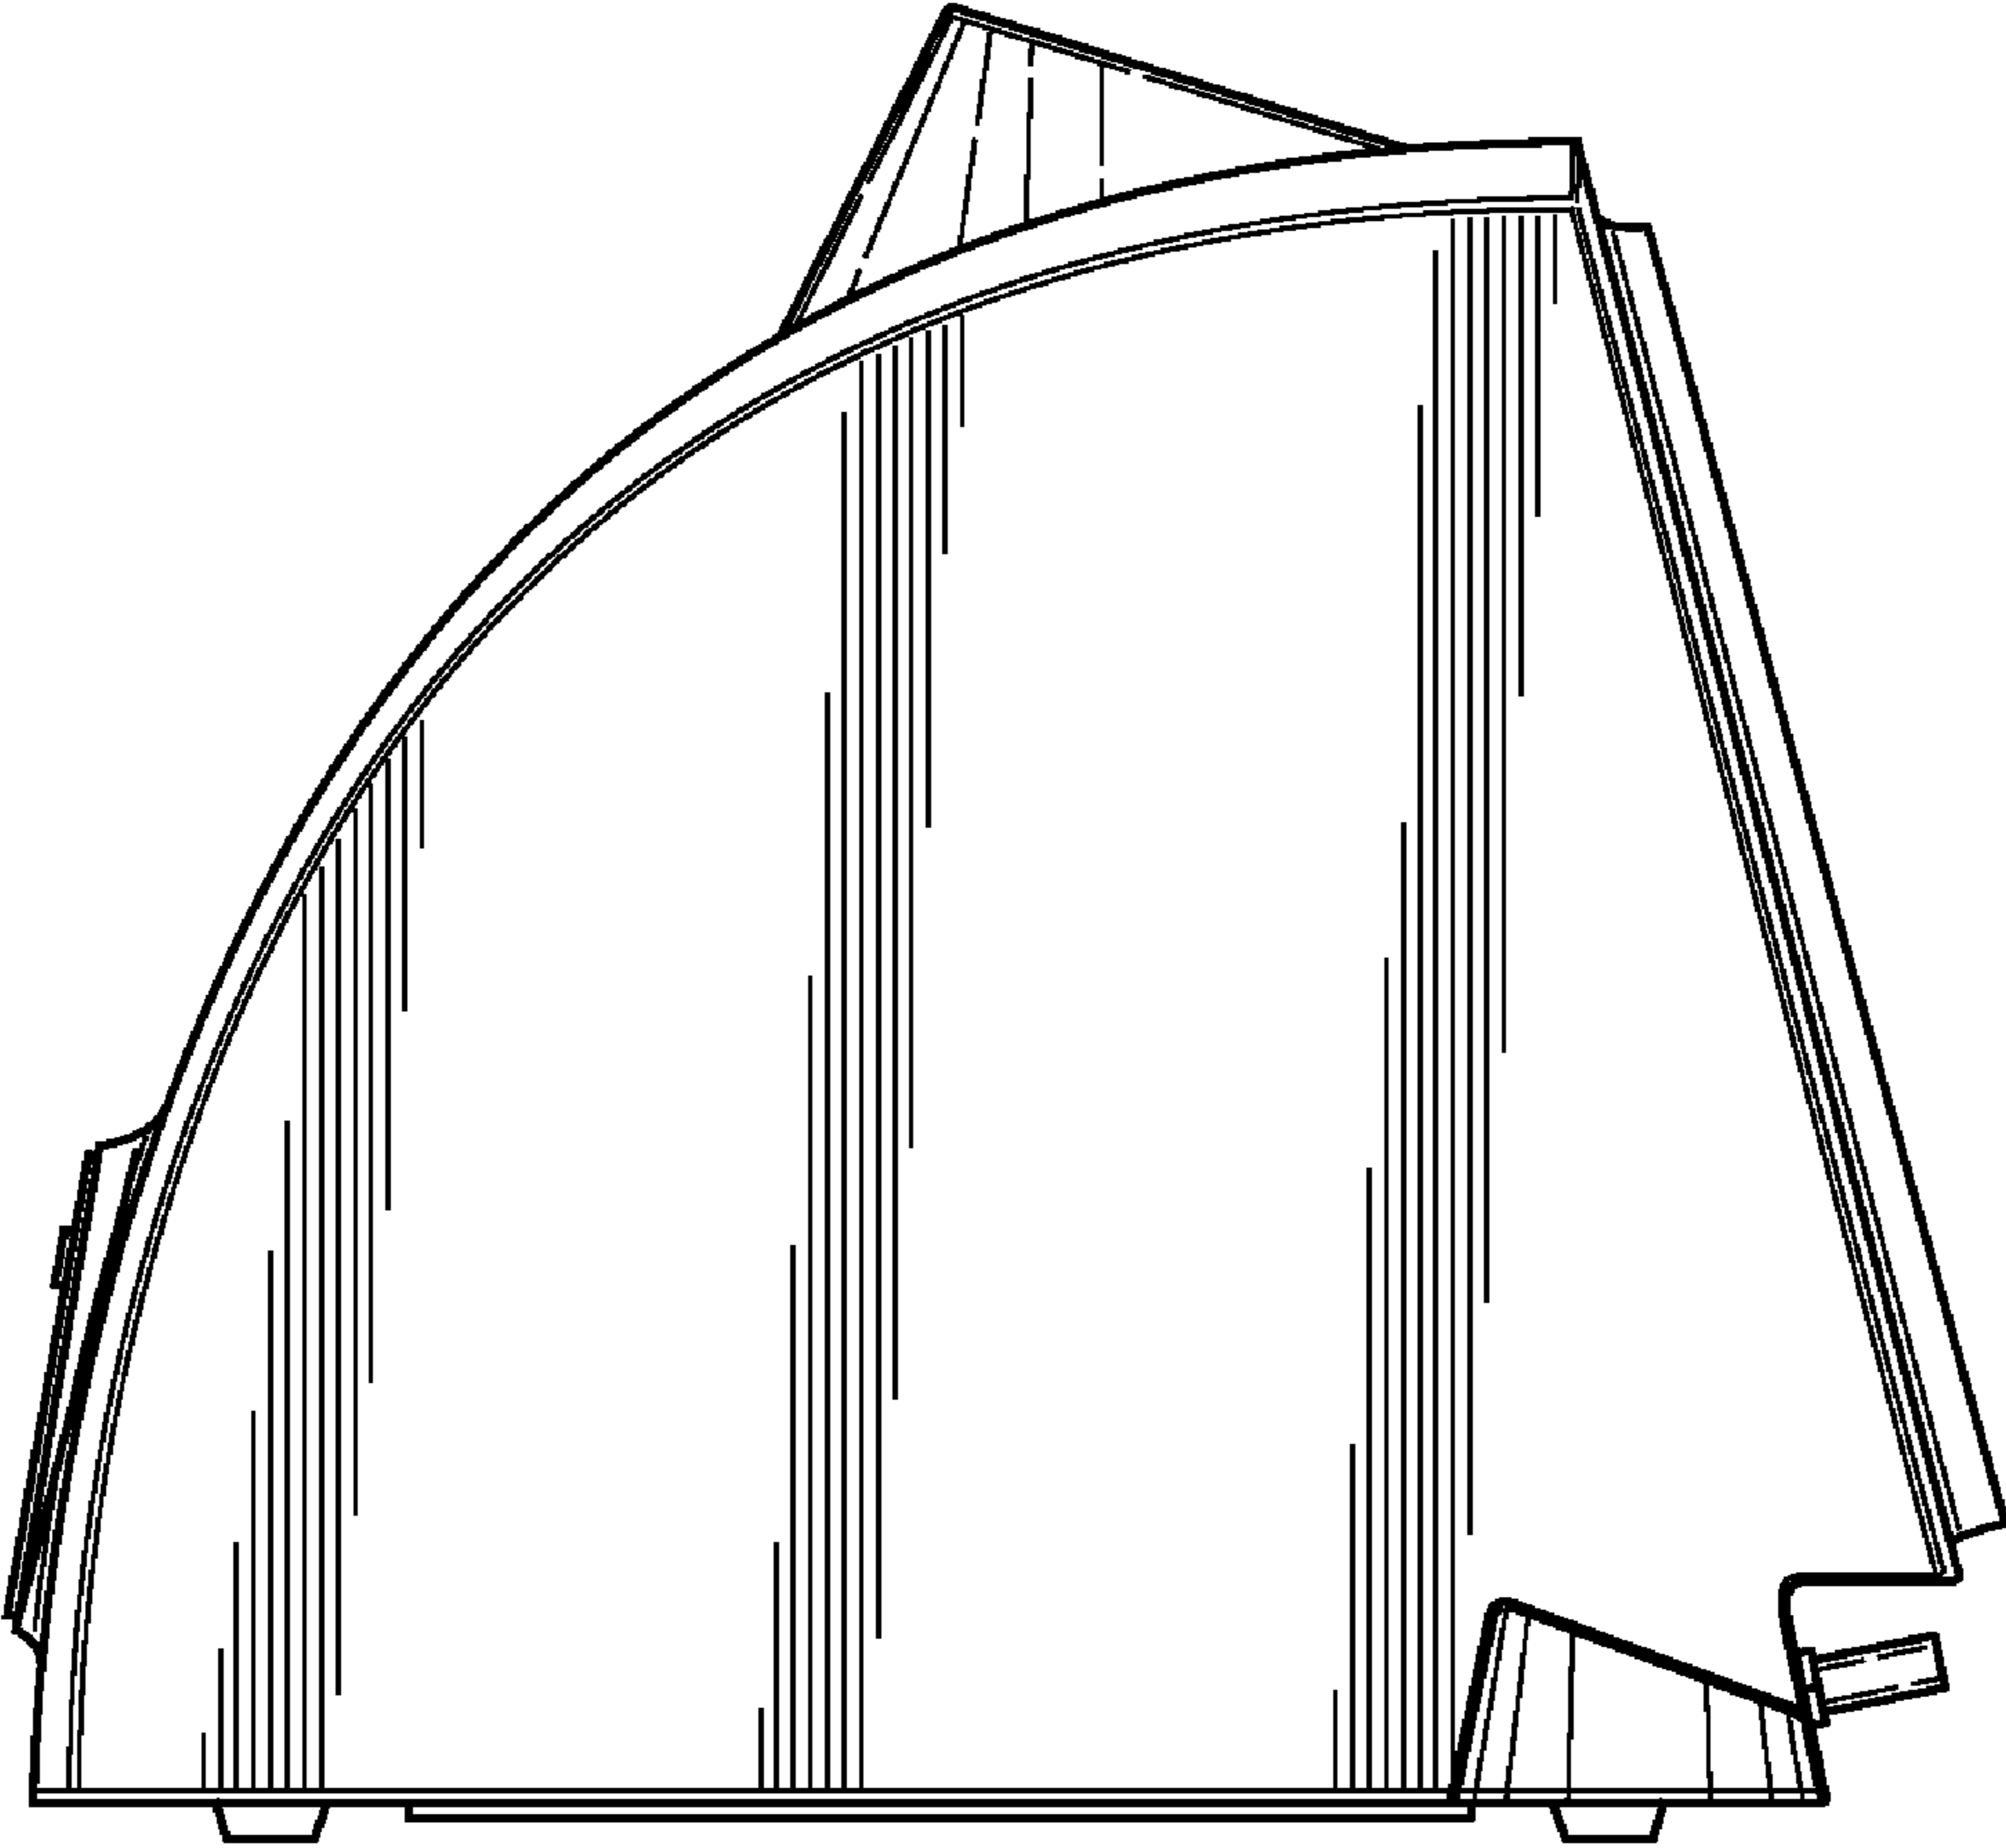


FIG. 3

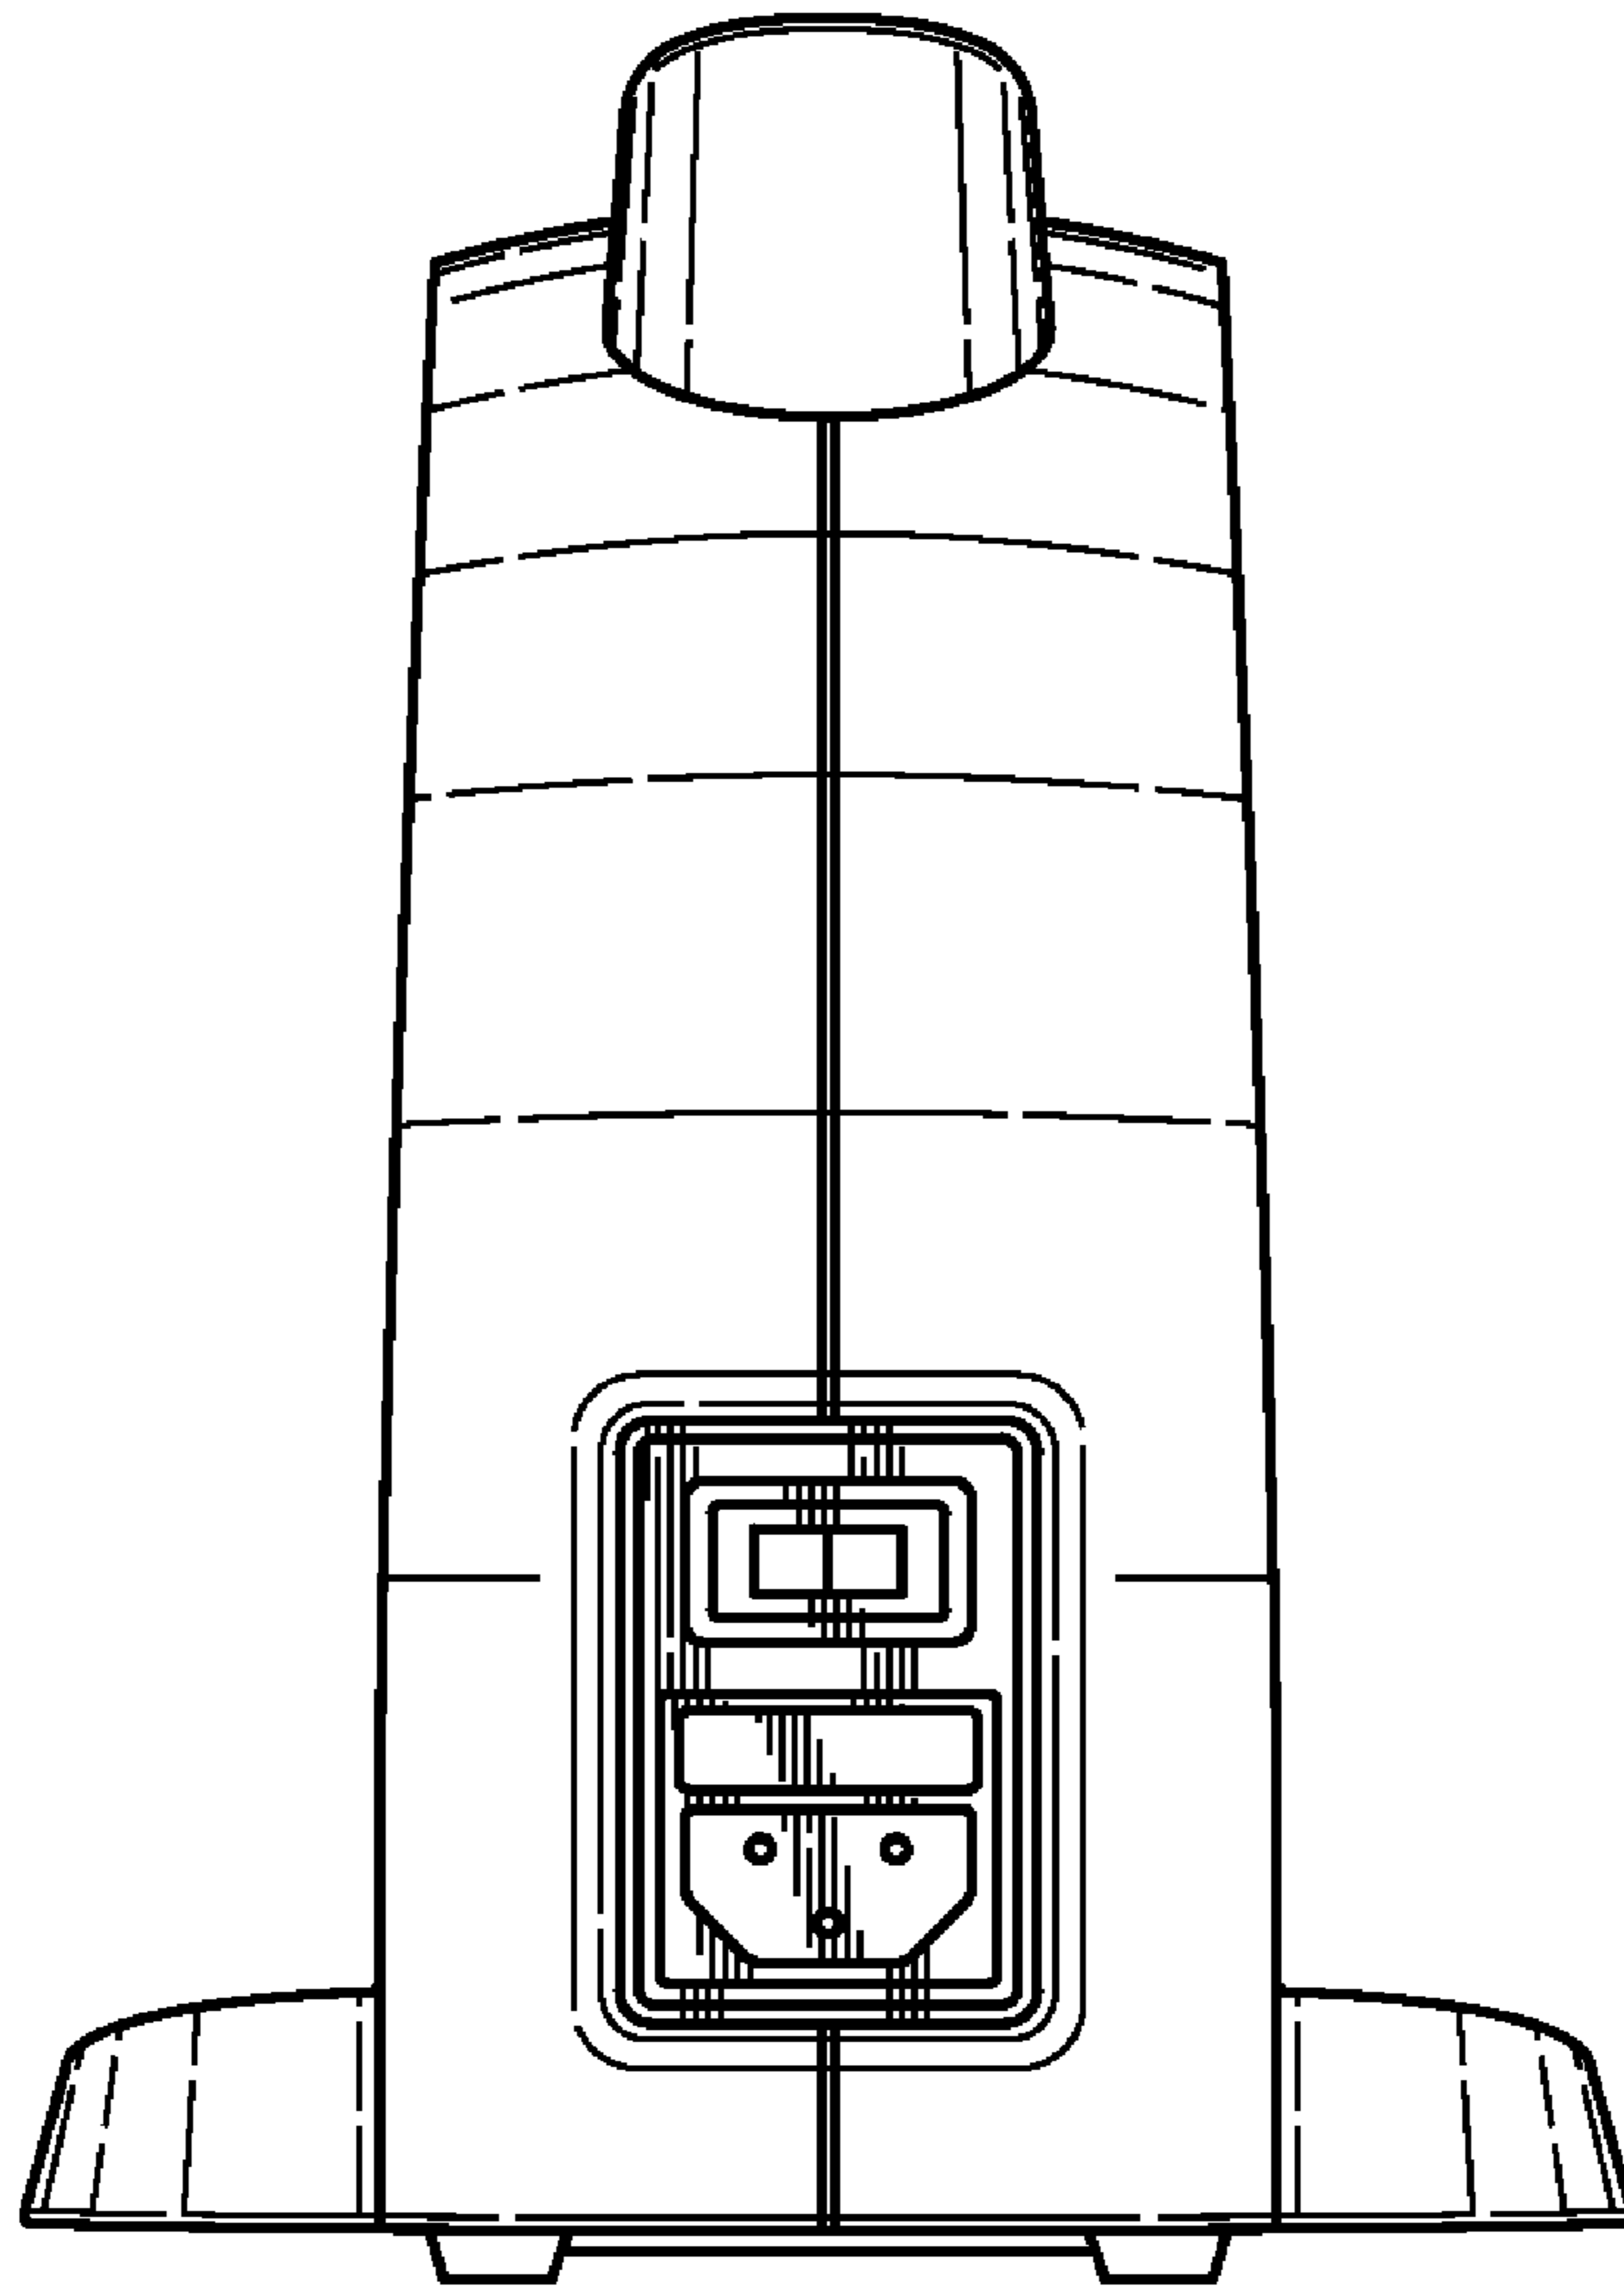


FIG. 4

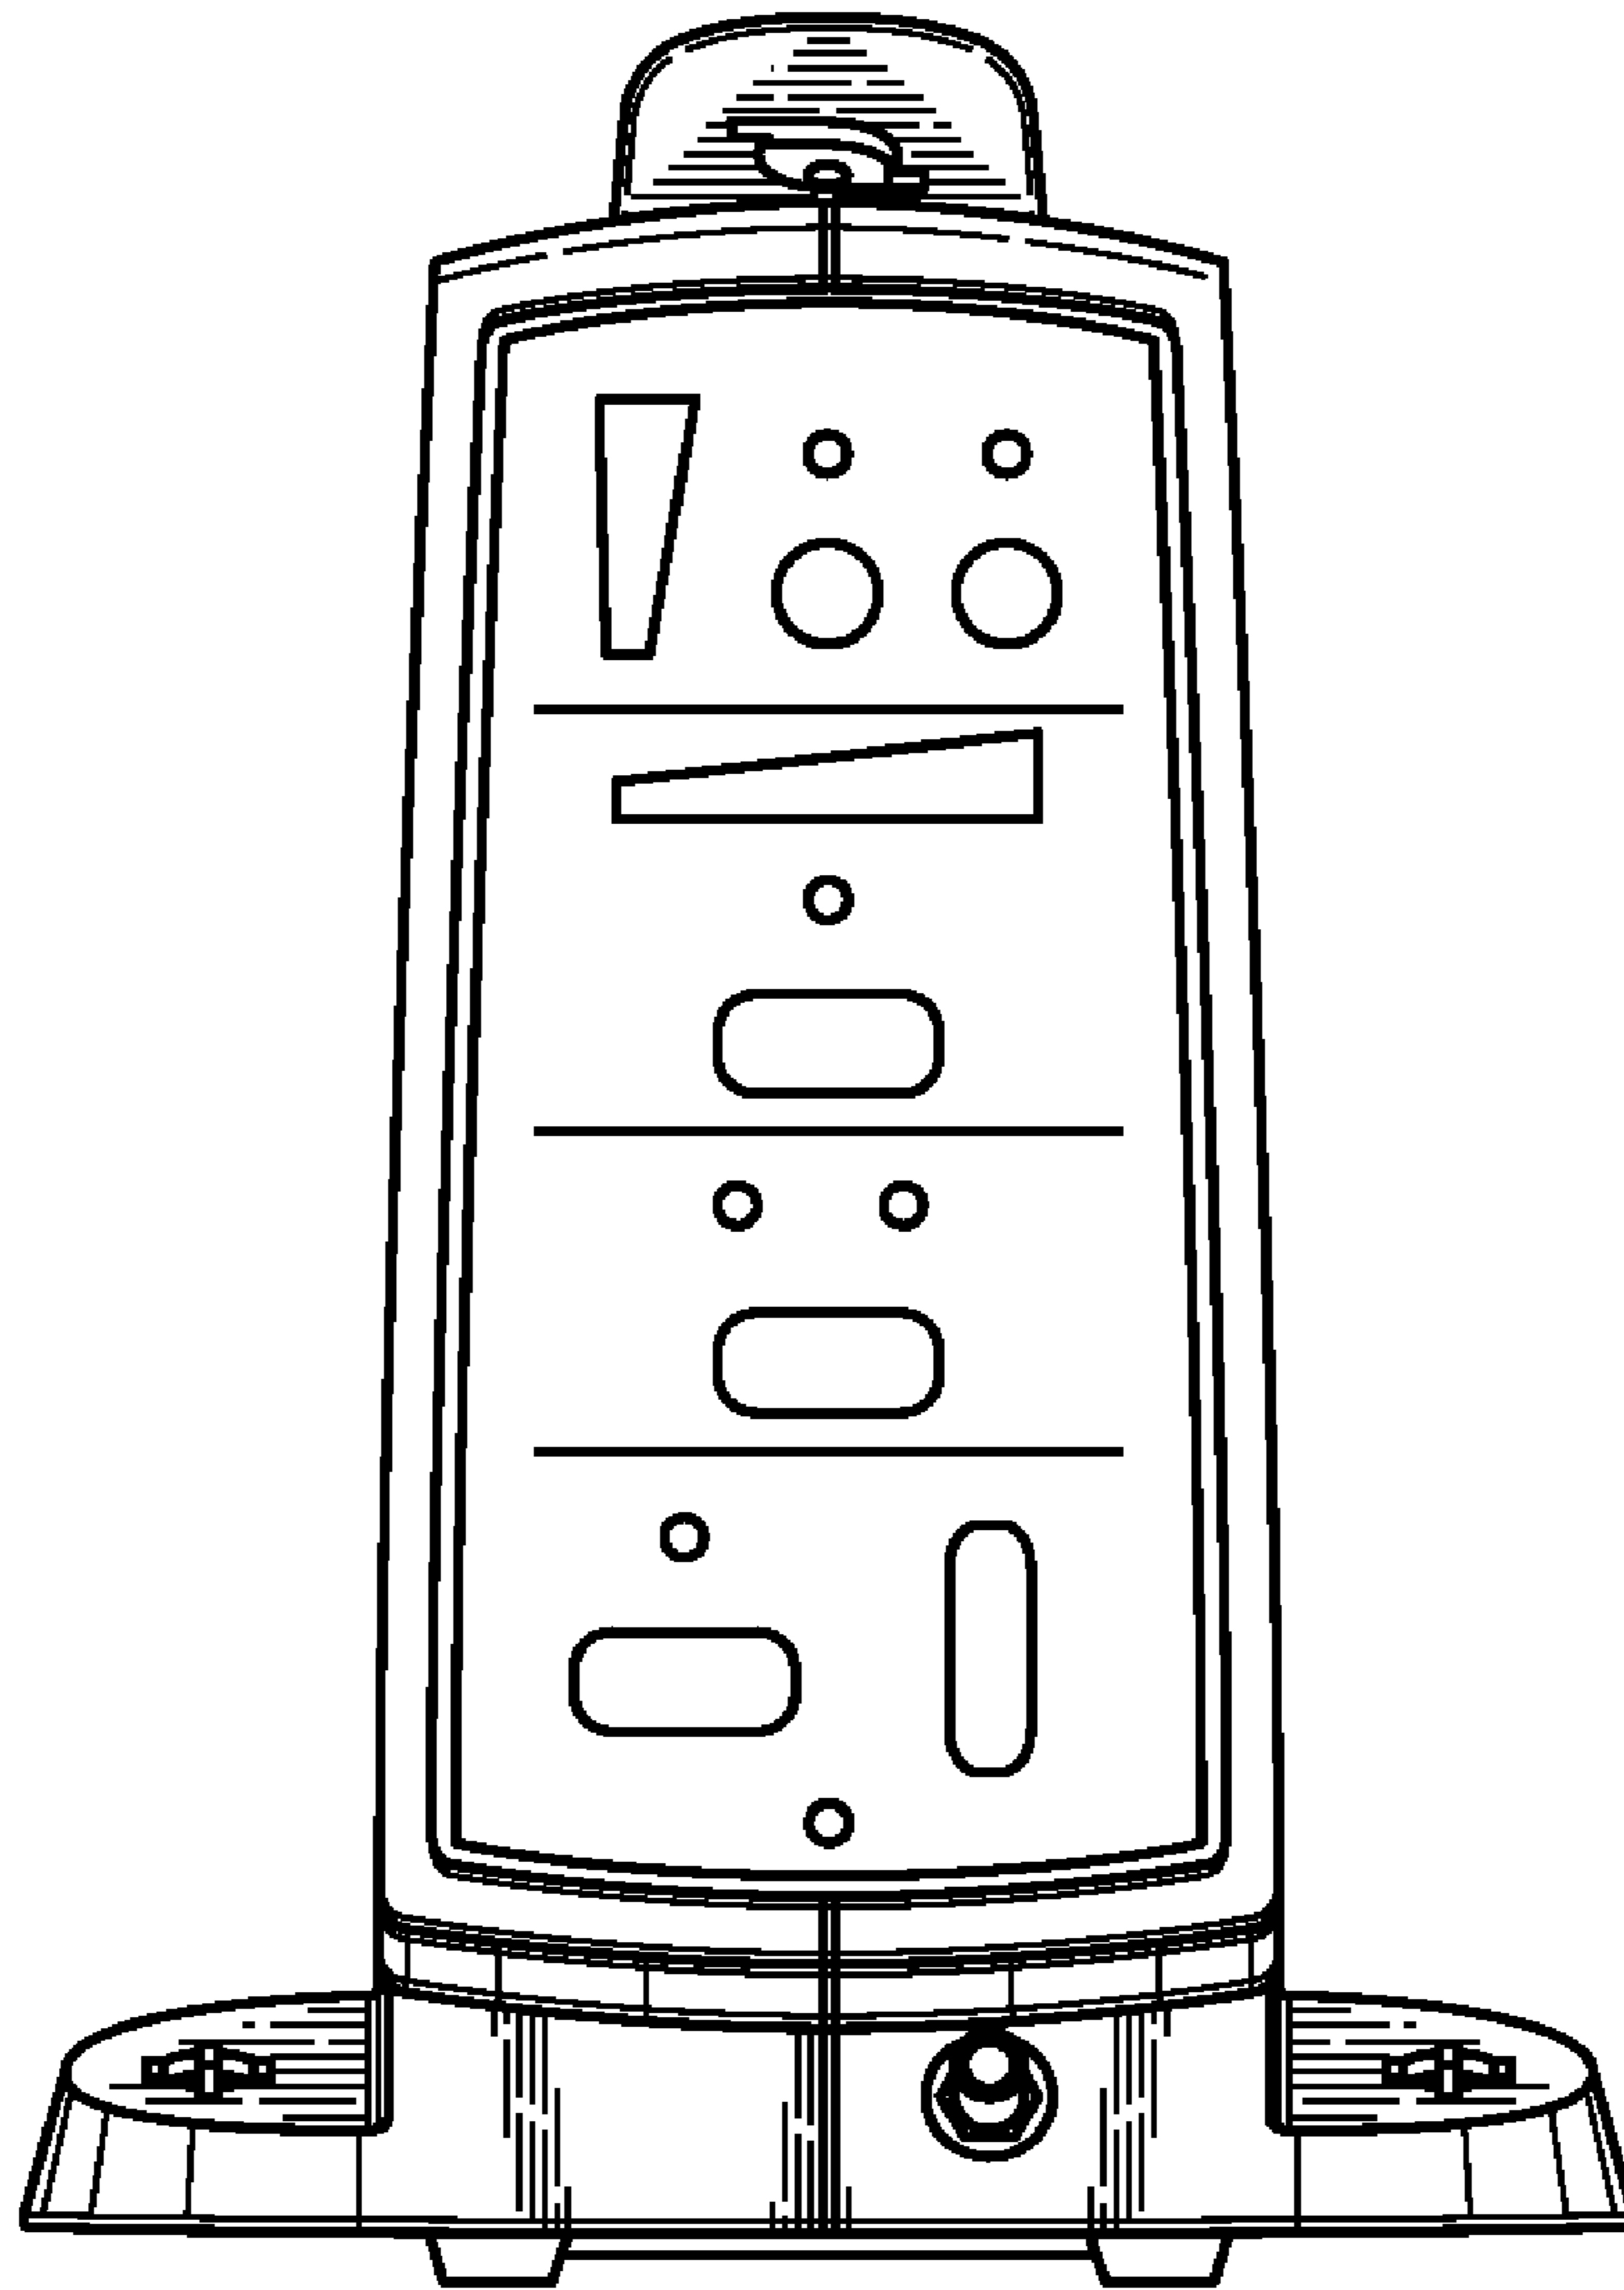


FIG. 5

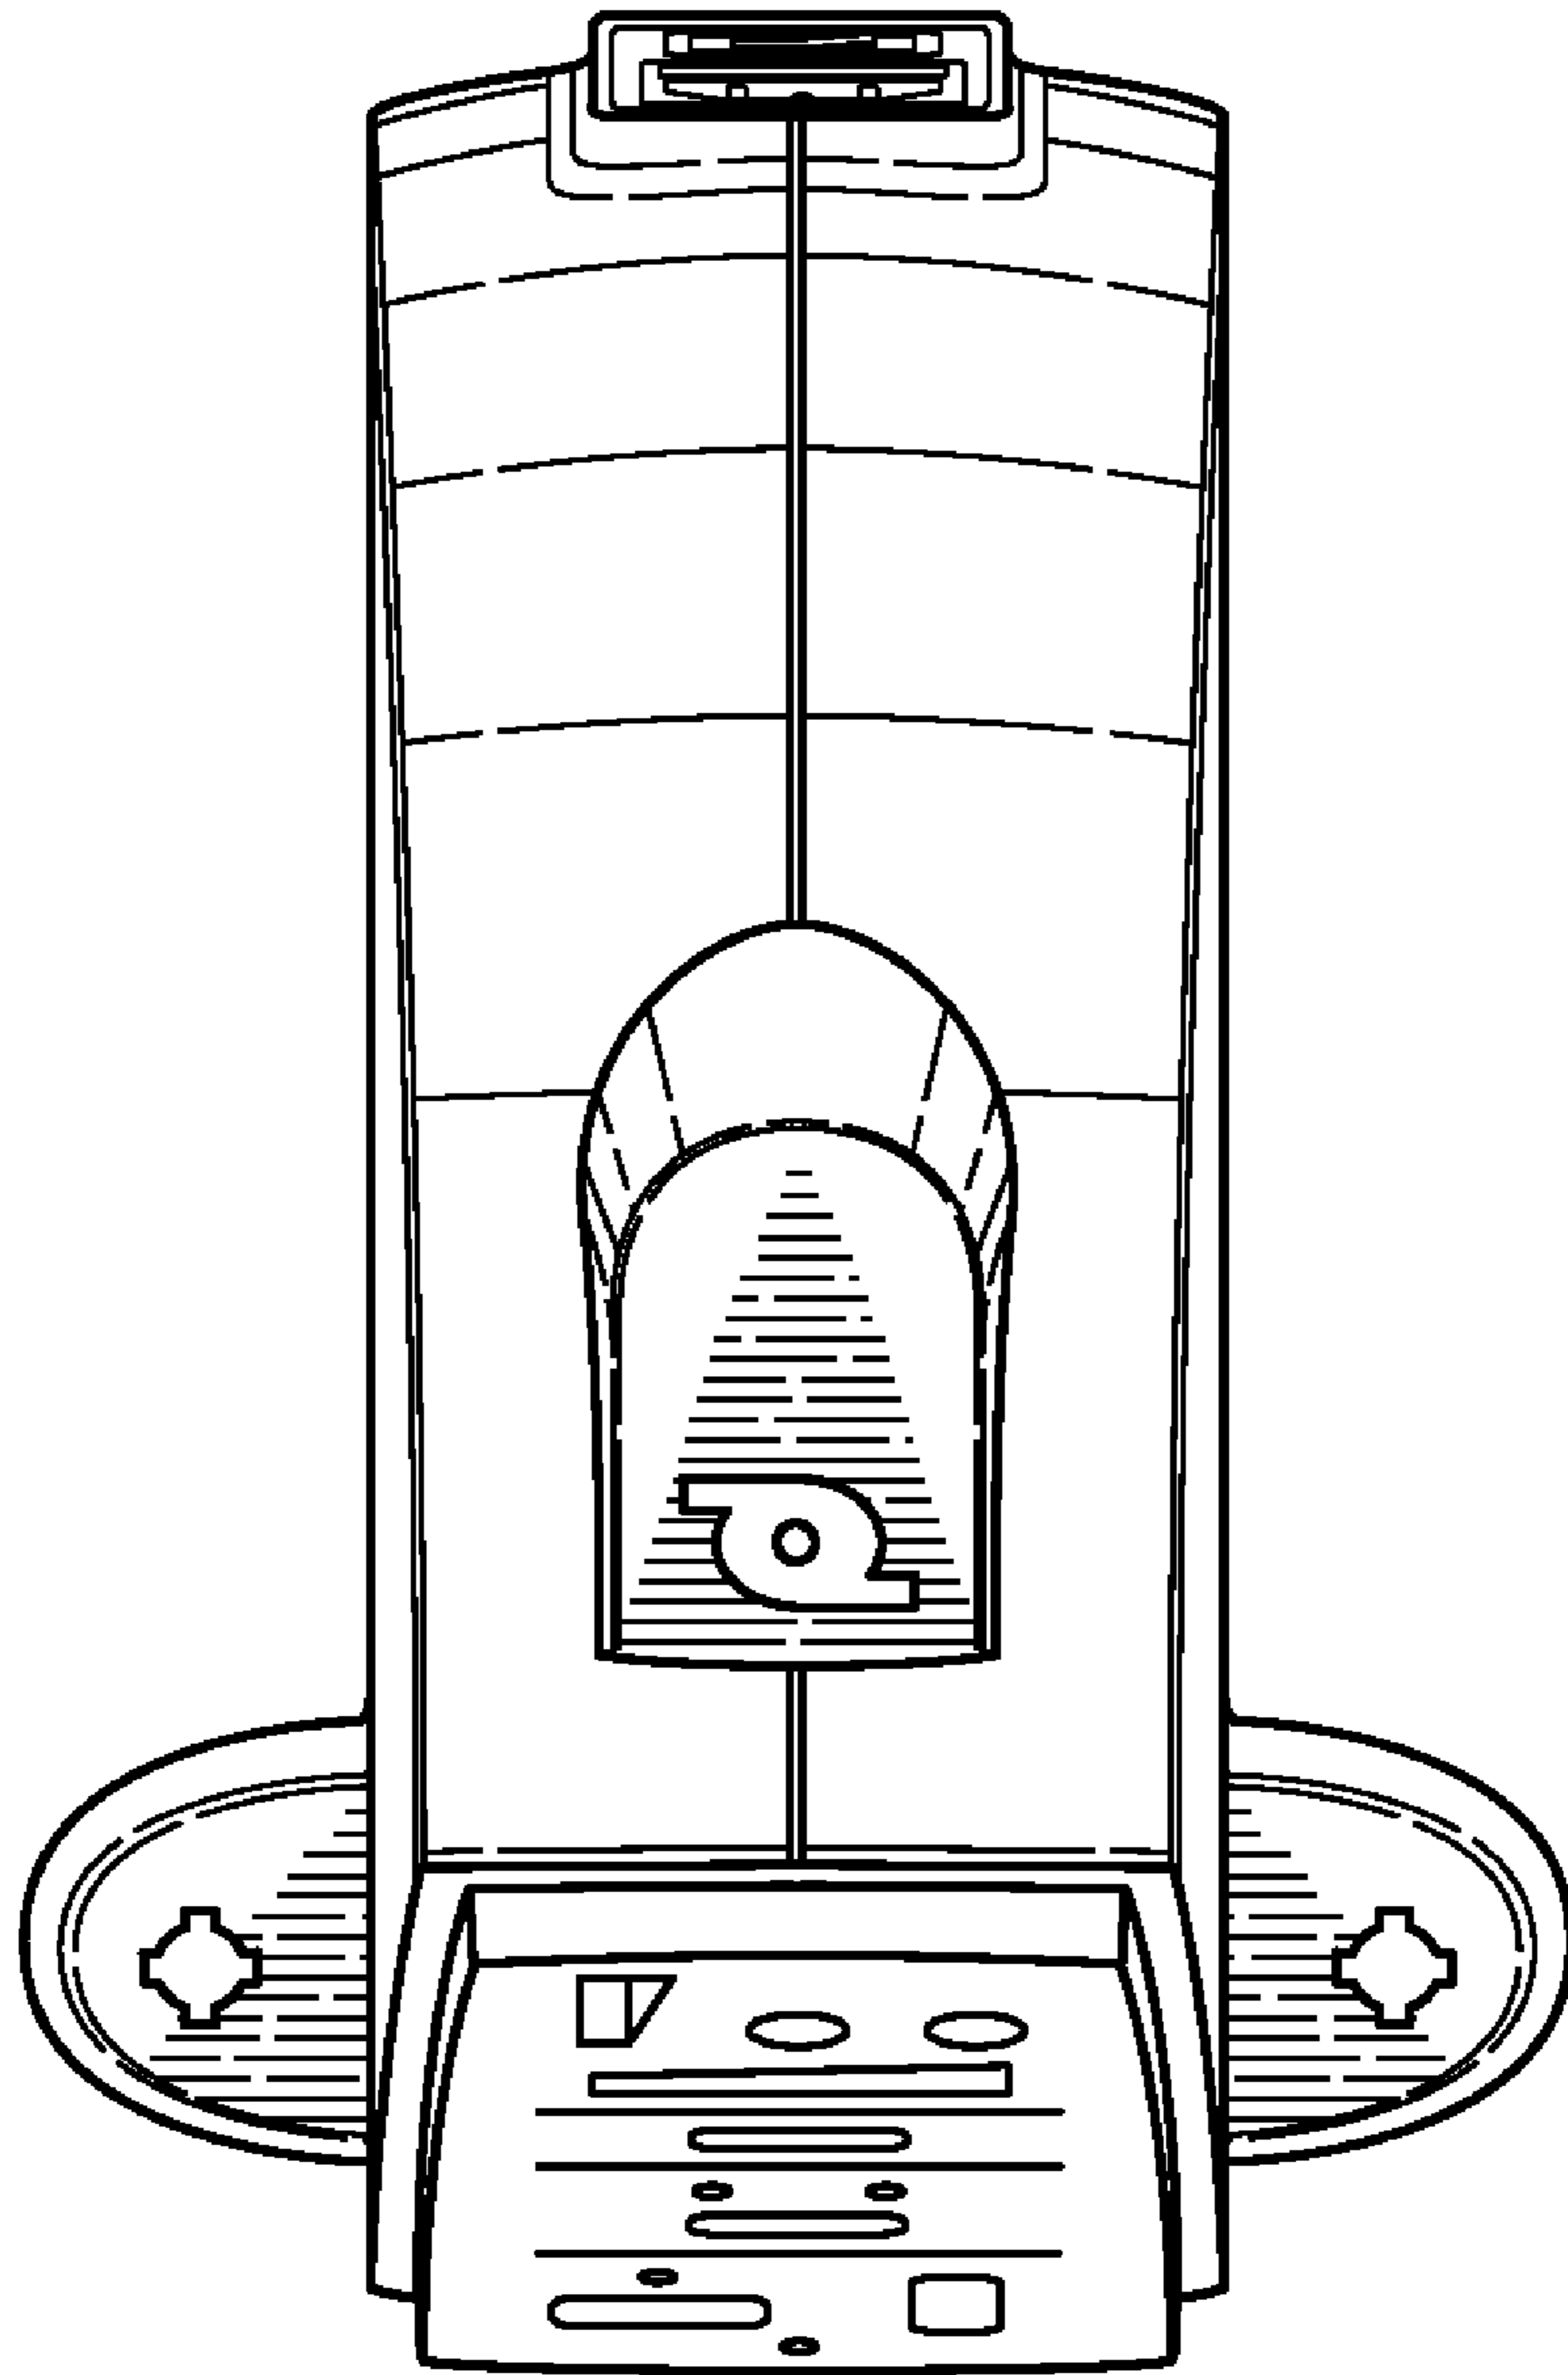


FIG. 6