



US00D566280S

(12) **United States Design Patent**
Baba et al.

(10) **Patent No.: US D566,280 S**

(45) **Date of Patent: ** Apr. 8, 2008**

(54) **ELECTROMAGNETIC WAVE DETECTOR
FOR A MAGNETIC RESONANCE
TOMOGRAPHY DIAGNOSIS APPARATUS**

2006/0289728 A1* 12/2006 Bois et al. 250/225
2007/0253660 A1* 11/2007 Wang et al. 385/5

(75) Inventors: **Noriaki Baba**, Tokyo (JP); **Yusei Mori**,
Sakura (JP); **Manabu Ishii**, Otawara
(JP); **Yutaka Kato**, Utsunomiya (JP);
Toshiharu Kumasaka, Nanyo (JP)

FOREIGN PATENT DOCUMENTS

JP 1265568 3/2006

(73) Assignees: **Kabushiki Kaisha Toshiba** (JP);
Toshiba Medical Systems Corporation
(JP)

* cited by examiner

Primary Examiner—Antoine D. Davis
(74) *Attorney, Agent, or Firm*—Banner & Witcoff, Ltd.

(**) Term: **14 Years**

(57) **CLAIM**

(21) Appl. No.: **29/280,296**

The ornamental design for an electromagnetic wave detector
for a magnetic resonance tomography diagnosis apparatus,
as shown and described.

(22) Filed: **May 23, 2007**

(30) **Foreign Application Priority Data**

Nov. 24, 2006 (JP) 2006-032217

DESCRIPTION

(51) **LOC (8) Cl.** **24-01**

(52) **U.S. Cl.** **D24/158; D10/46**

(58) **Field of Classification Search** D10/46,
D10/47; D24/158-161; 324/309, 318, 319,
324/321; 378/4, 19-21, 27, 146; 385/4,
385/5, 122; 250/225; 257/E31.033, E31.128
See application file for complete search history.


FIG. 1 is a front, top and left side perspective view of an
electromagnetic wave detector for a magnetic resonance
tomography diagnosis apparatus, showing our new design;
FIG. 2 is a front elevational view thereof;
FIG. 3 is a rear elevational view thereof;
FIG. 4 is a right side elevational view thereof; the opposite
side being a mirror image thereof;
FIG. 5 is a top plan view thereof; and,
FIG. 6 is a bottom plan view thereof.

(56) **References Cited**

U.S. PATENT DOCUMENTS

5,619,039 A * 4/1997 Montanari 250/352

1 Claim, 2 Drawing Sheets

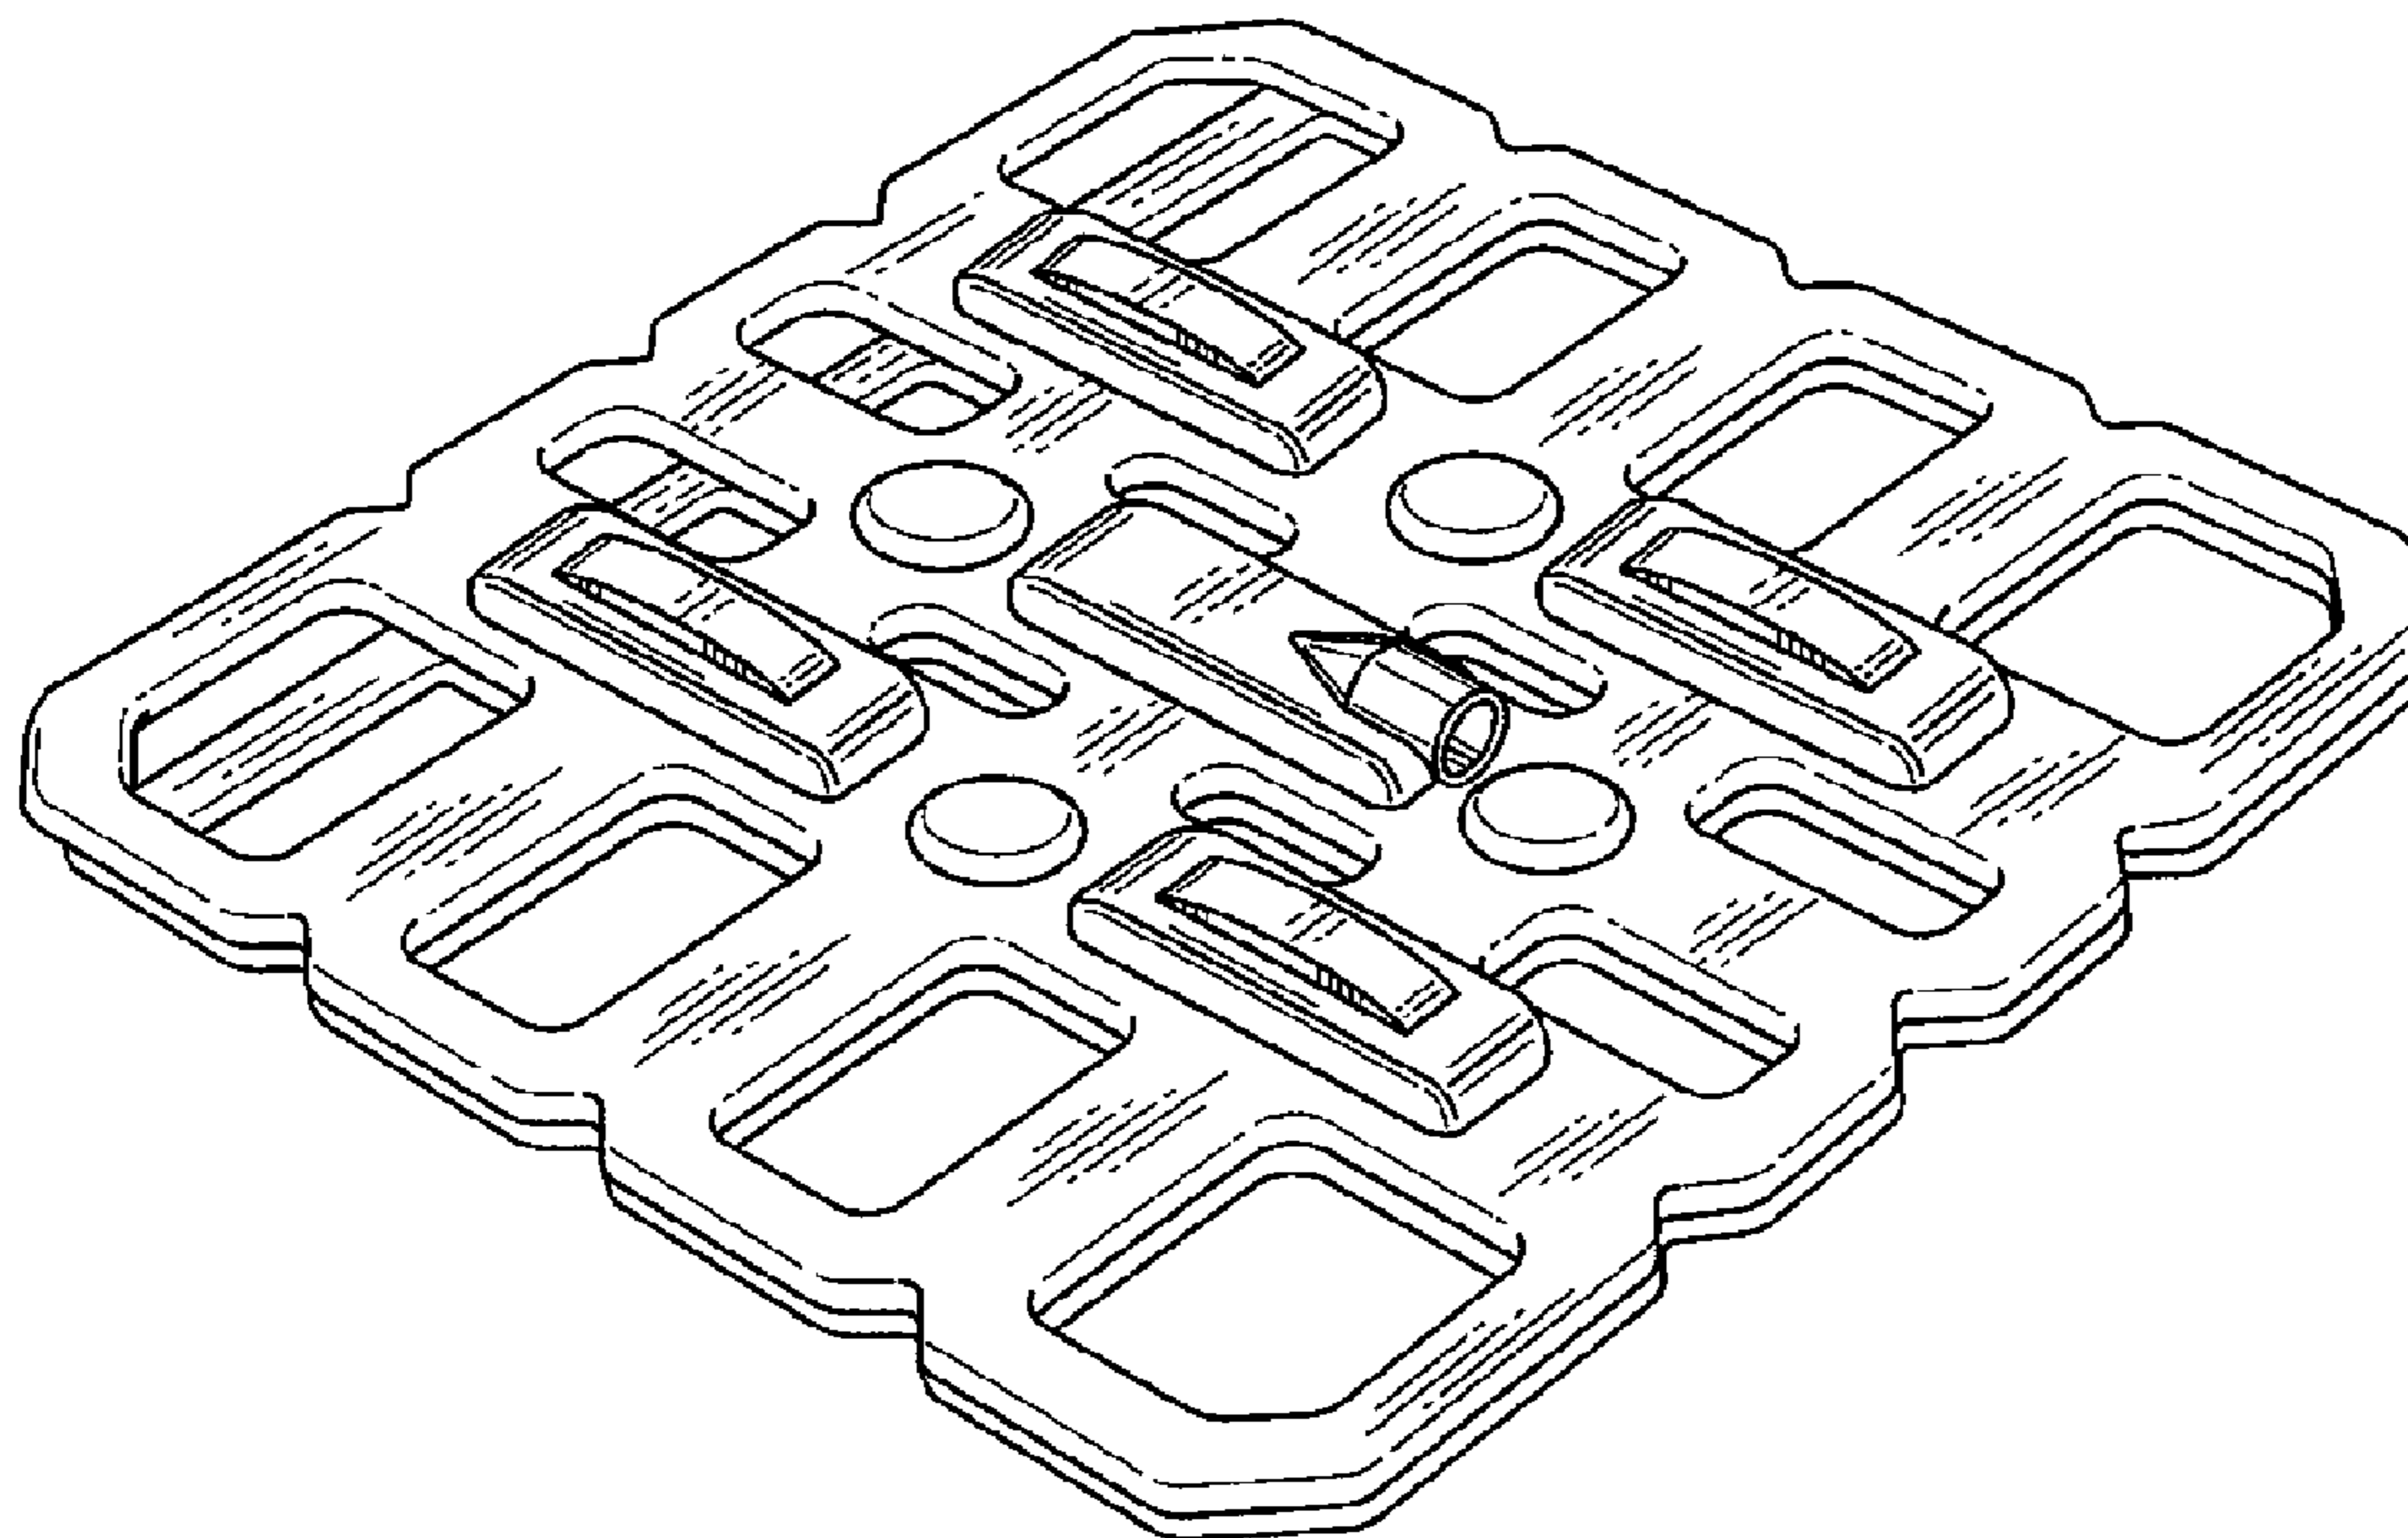

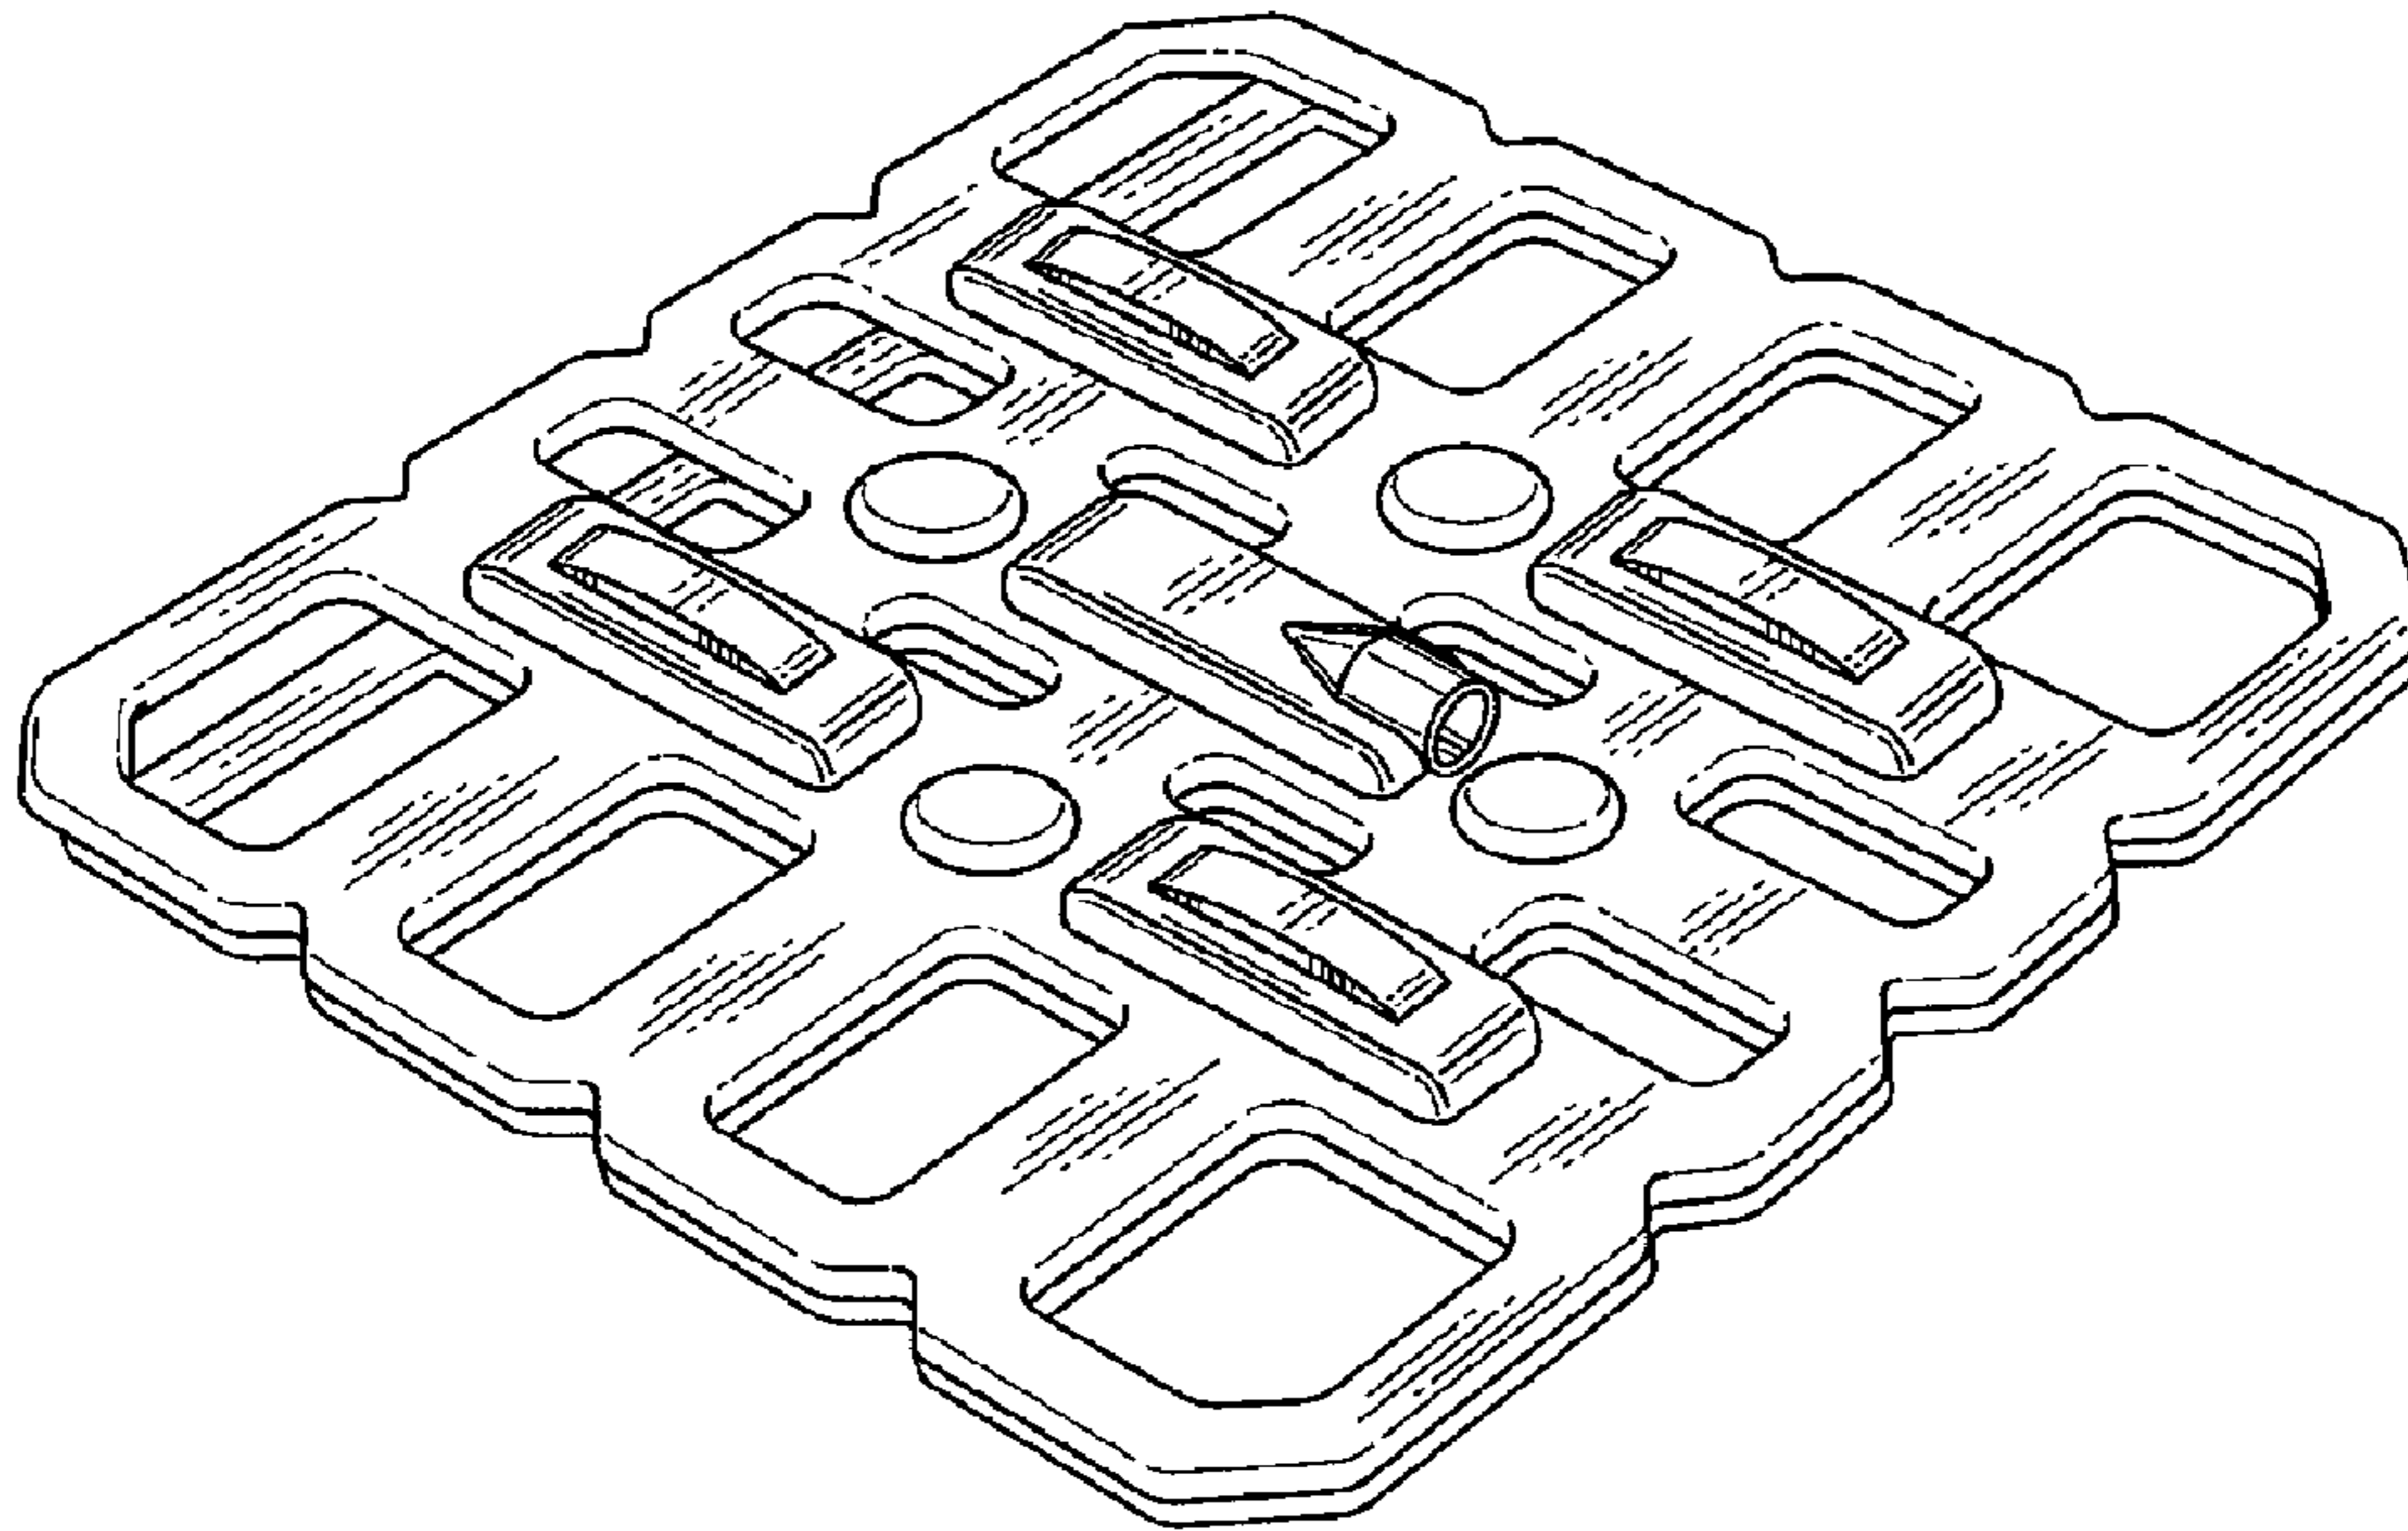


FIG. 1

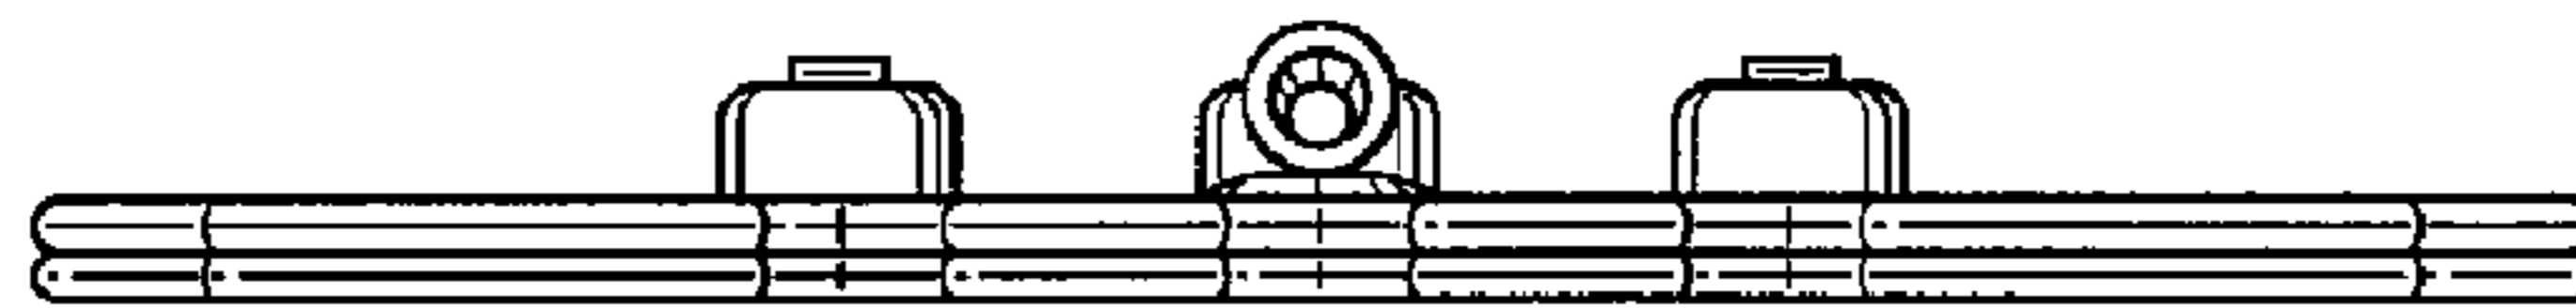


FIG. 2



FIG. 3



FIG. 4

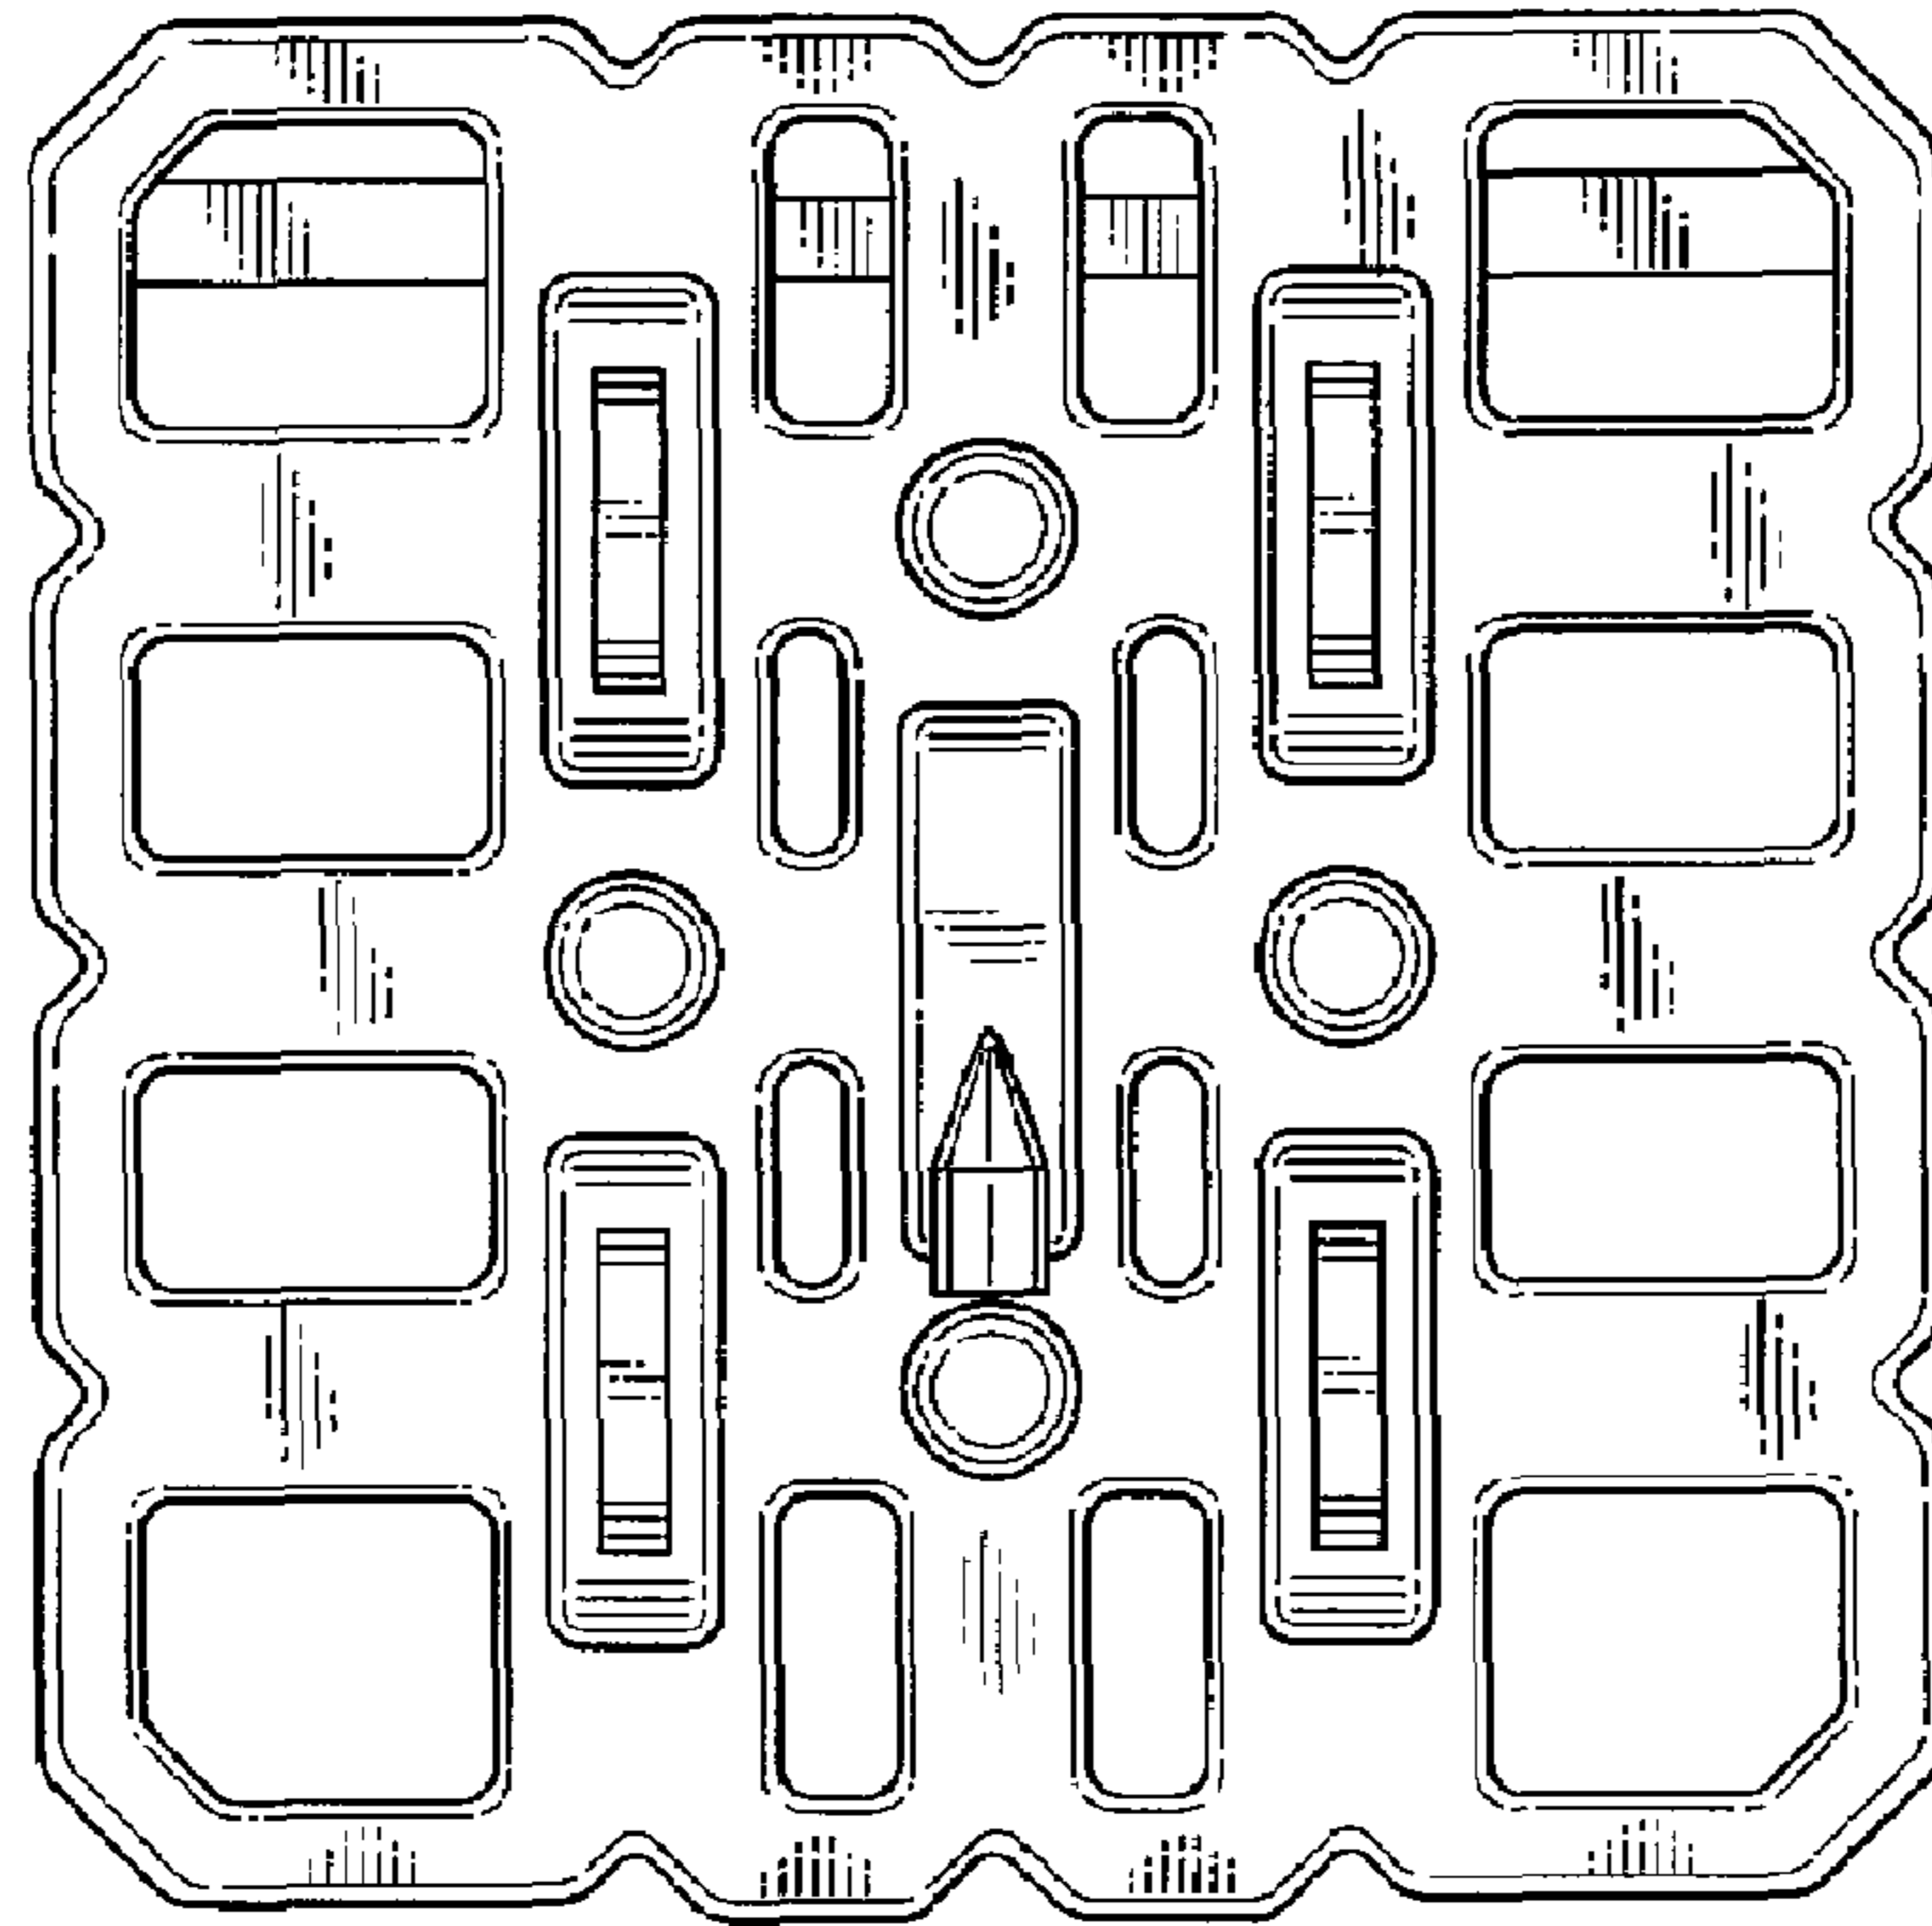


FIG. 5

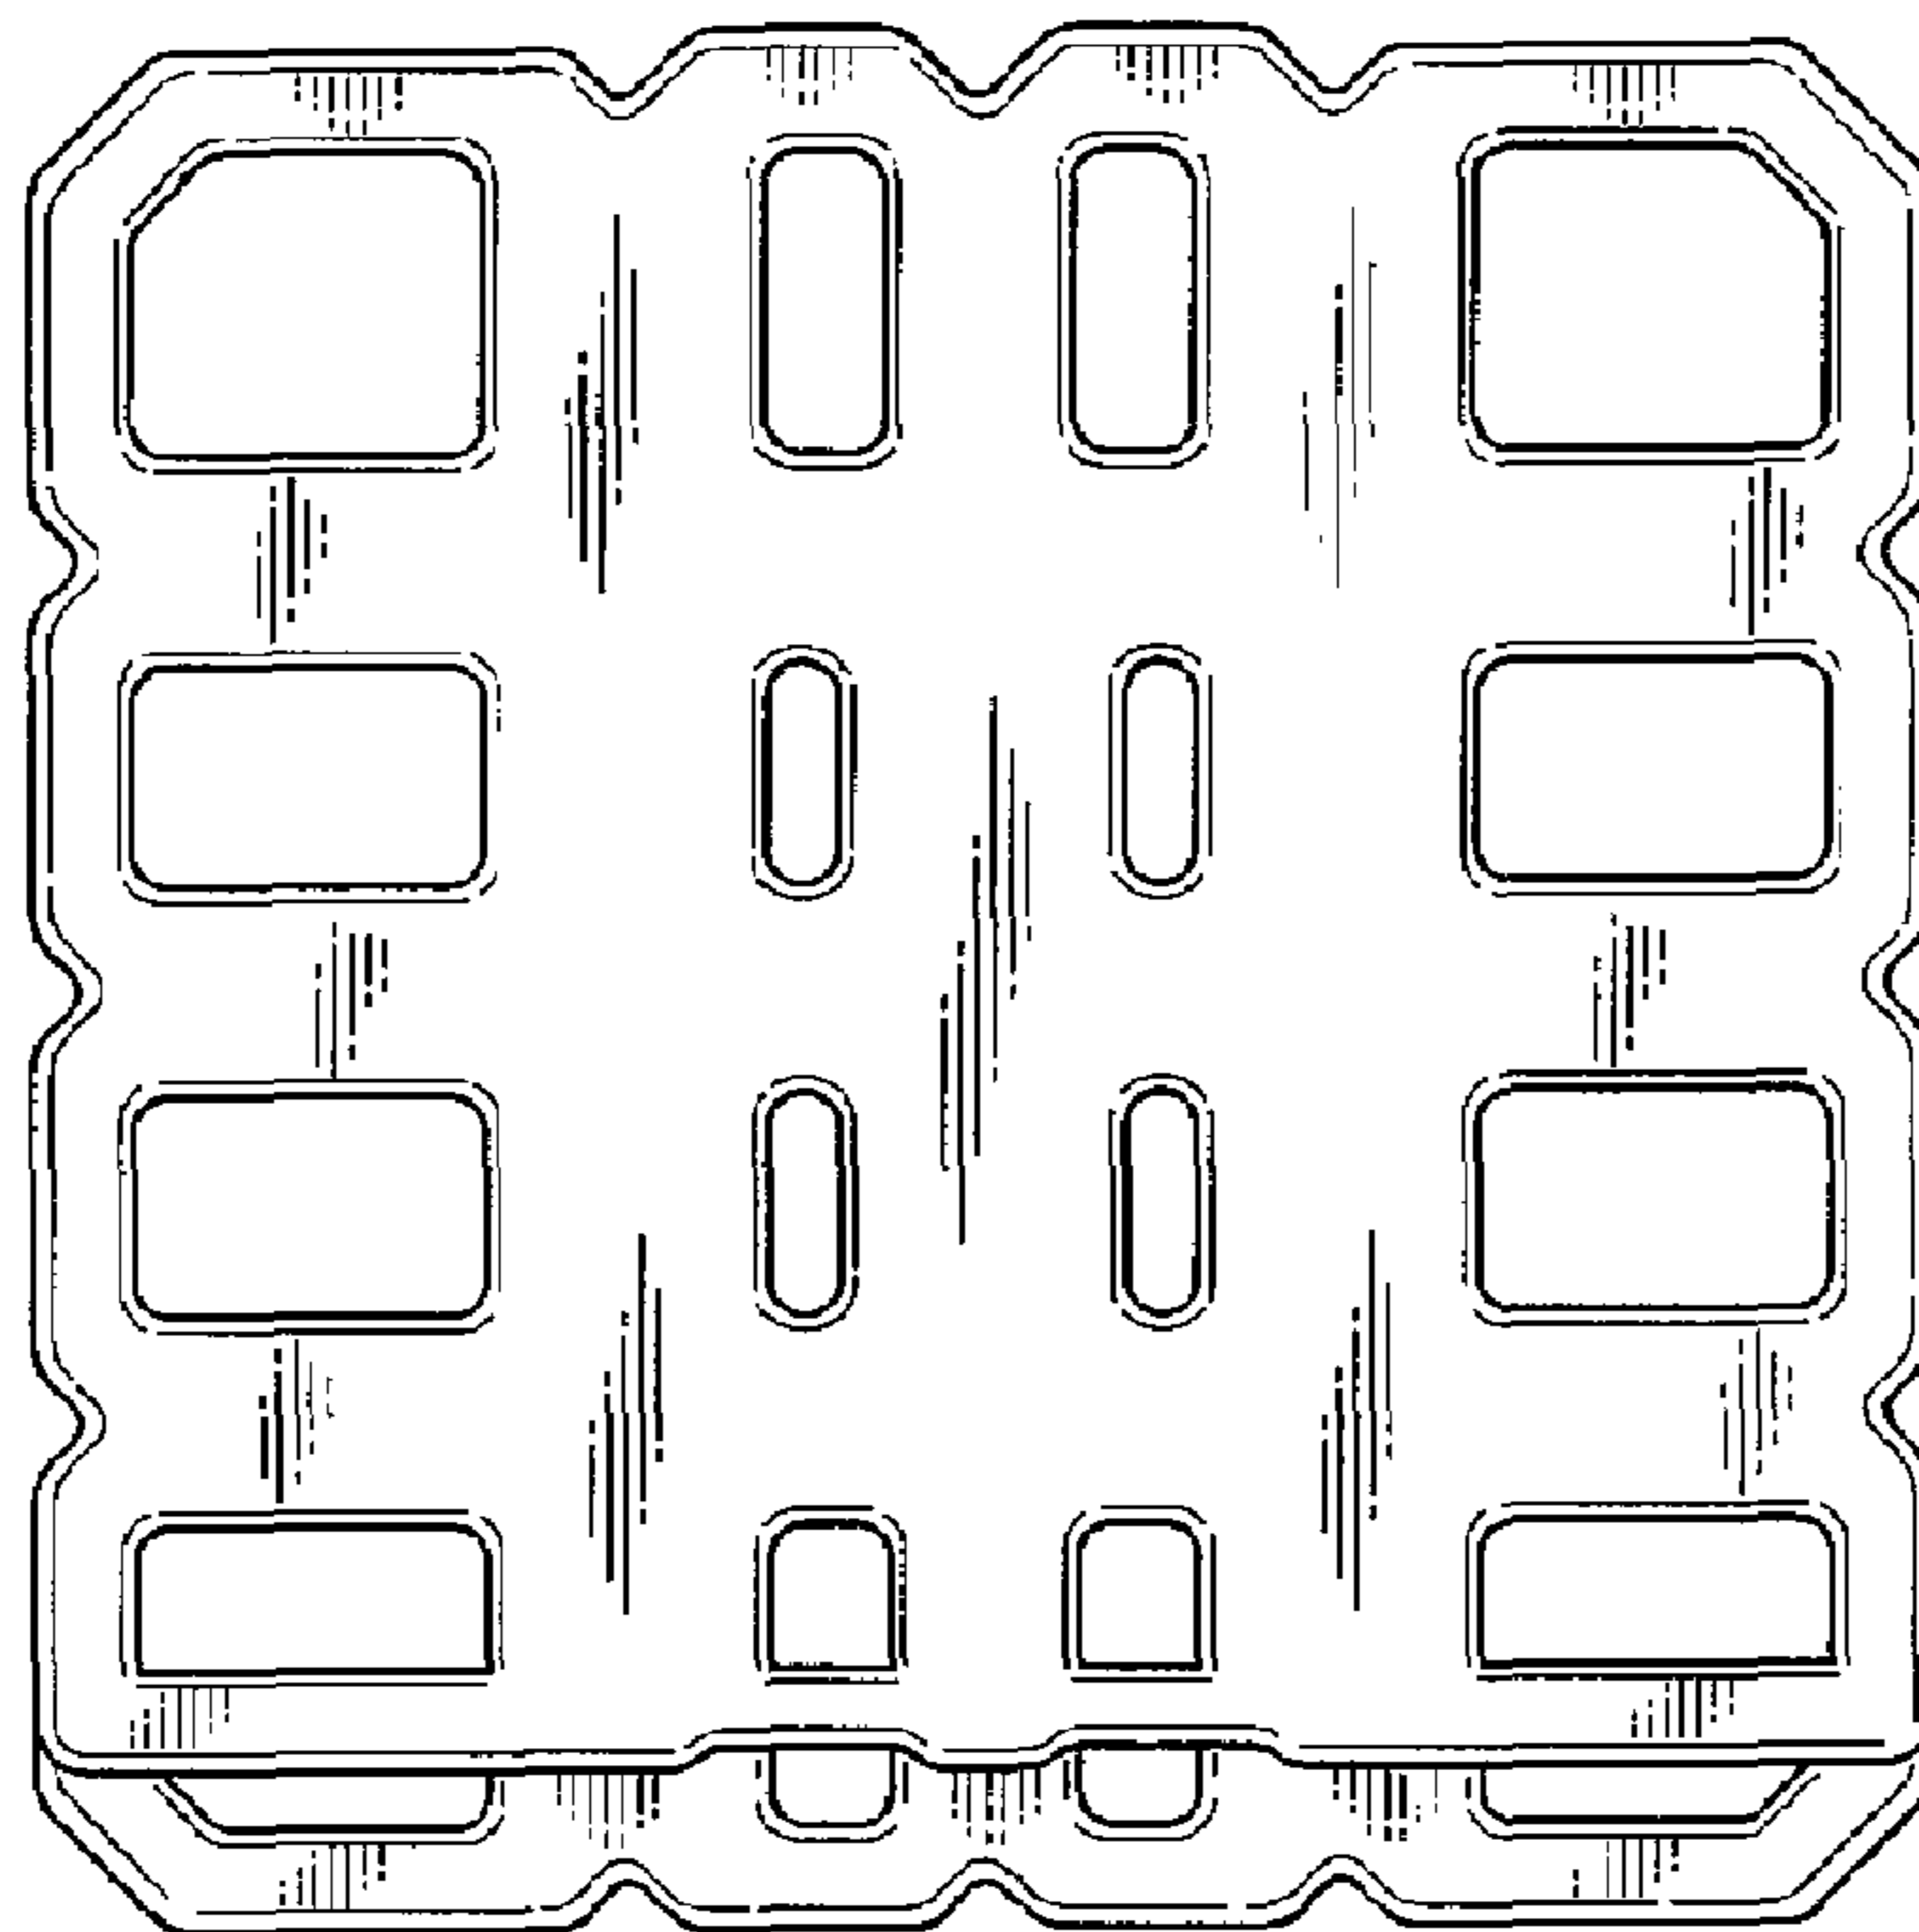


FIG. 6