



US00D567941S

(12) **United States Design Patent** (10) **Patent No.:** **US D567,941 S**
Dikeman et al. (45) **Date of Patent:** **** Apr. 29, 2008**

(54) **INTRAVENOUS SITE SECUREMENT DEVICE FOR CATHETERS**

2004/0167475 A1* 8/2004 Wright et al. 604/180

(75) Inventors: **W. Cary Dikeman**, Lenexa, KS (US);
Chris Winsor, Olathe, KS (US); **Steve A. Cash**, Overland Park, KS (US);
Larry C. Smith, Lenexa, KS (US)

(73) Assignee: **Nexus Medical, LLC**, Lenexa, KS (US)

(**) Term: **14 Years**

(21) Appl. No.: **29/276,851**

(22) Filed: **Feb. 7, 2007**

Related U.S. Application Data

(62) Division of application No. 29/245,311, filed on Dec. 21, 2005.

(51) **LOC (8) Cl.** **24-02**

(52) **U.S. Cl.** **D24/128**

(58) **Field of Classification Search** D24/128,
D24/189; D30/133, 155; 128/DIG. 6, DIG. 126;
604/174, 178–180; 602/41–47, 50, 54–55
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

| | | | | | |
|--------------|------|---------|----------------|-------|---------|
| 3,256,880 | A * | 6/1966 | Caypinar | | 128/877 |
| 4,114,626 | A * | 9/1978 | Beran | | 604/180 |
| 4,129,128 | A * | 12/1978 | McFarlane | | 604/180 |
| 4,392,857 | A * | 7/1983 | Beran | | 604/179 |
| D293,717 | S * | 1/1988 | Proulx et al. | | D24/189 |
| D401,329 | S * | 11/1998 | Bierman | | D24/128 |
| 6,024,761 | A * | 2/2000 | Barone et al. | | 607/108 |
| 6,572,588 | B1 * | 6/2003 | Bierman et al. | | 604/180 |
| D480,144 | S * | 9/2003 | Adams et al. | | D24/189 |
| 6,663,600 | B2 * | 12/2003 | Bierman et al. | | 604/174 |
| 2002/0026152 | A1 * | 2/2002 | Bierman | | 604/174 |

OTHER PUBLICATIONS

Complaint [dated Jan. 29, 2007] *Venetec Int.'l, Inc. v. Nexus Medical, LLC*, USDC D.Del., Case No. 1:07-CV-00057.

(Continued)

Primary Examiner—Louis S Zarfaz

Assistant Examiner—Eric L Goodman

(74) *Attorney, Agent, or Firm*—Hovey Williams LLP

(57) **CLAIM**

The ornamental design for an intravenous site securement device for catheters, as shown and described.

DESCRIPTION

FIG. 1 is a perspective view of an intravenous site securement device for catheters embodying our design, with the catheter, the adhesive strip for securing the device to the patient, the posts and frusto-spherical head ends of the platform connectors, and the retainer being shown in broken lines for illustrative purposes only and forming no part of the claimed design;

FIG. 2 is a perspective view of the device similar to FIG. 1, but with the catheter, adhesive strip, and retainer being removed so that only the platform is depicted;


FIG. 3 a top elevation view of the device as depicted in FIG. 2;

FIG. 4 is an end elevation view of the device as depicted in FIGS. 2 and 3, with the opposite end elevation view being a mirror image thereof;

FIG. 5 is a side elevation view of the device as depicted in FIGS. 2–4, with the opposite side elevation view being a mirror image thereof; and,

FIG. 6 is a bottom elevation view of the device as depicted in FIGS. 2–5, with the structure on the underside of the platform being shown in broken lines for illustrative purposes only and forming no part of the claimed design.

1 Claim, 1 Drawing Sheet

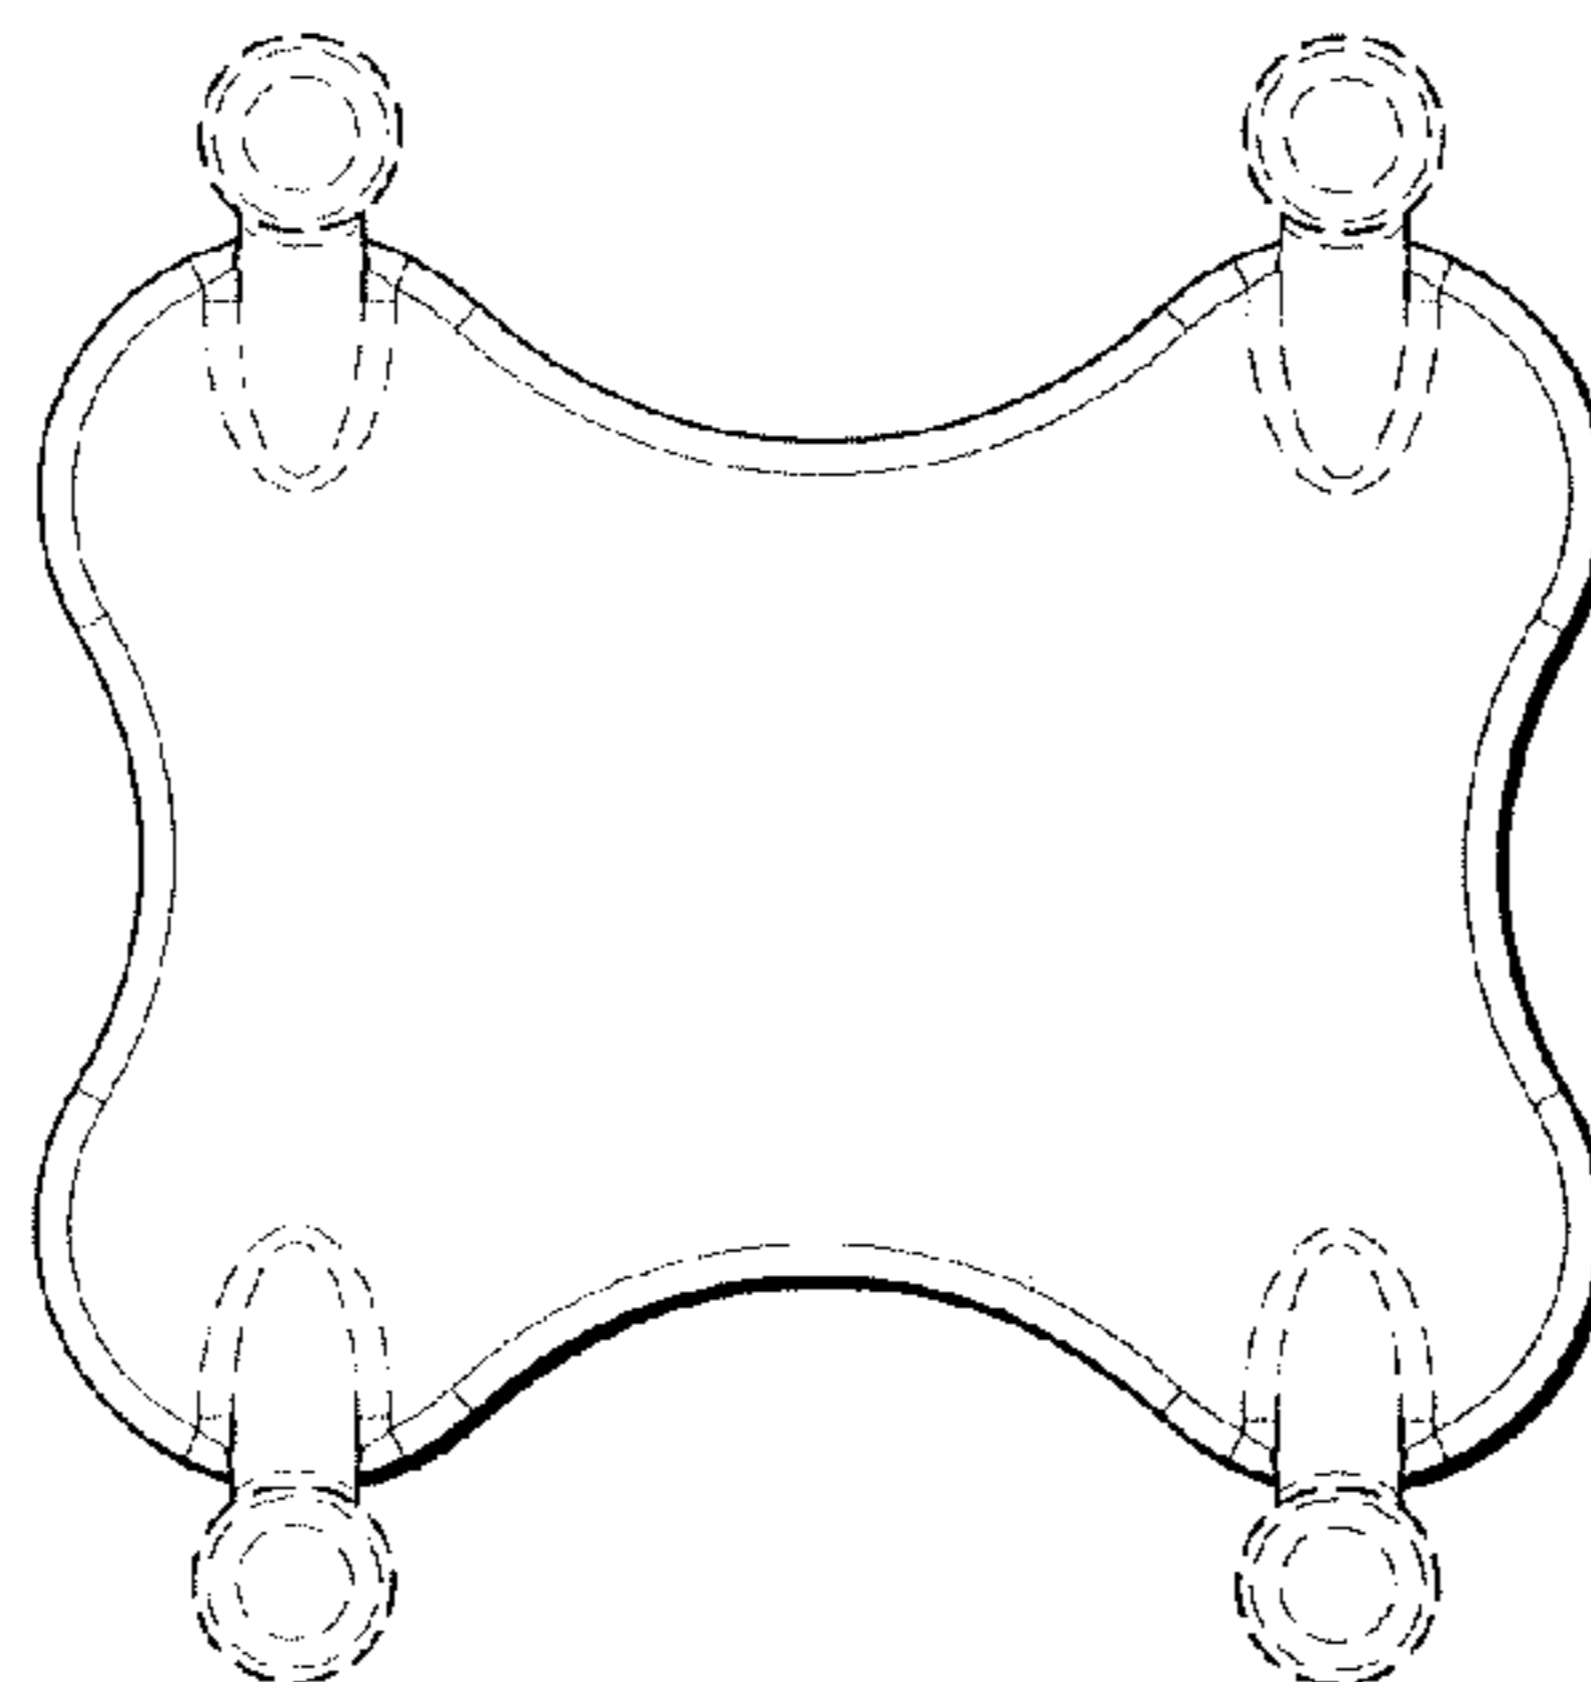

OTHER PUBLICATIONS

Nexus Medical, LLC's Answer to Venetec International, Inc.'s Complaint and Counterclaim [dated Mar. 22, 2007]. *Venetec Int'l, Inc. v. Nexus Medical, LLC*, USDC D.Del., Case No. 1:07-CV-00057.

Venetec International, Inc.'s Reply to Nexus Medical, LLC's Counterclaim [filed Apr. 11, 2007]. *Venetec Int'l, Inc. v. Nexus Medical, LLC*, USDC D.Del., Case No. 1:07-CV-00057.

First Supplemental Complaint [dated Jul. 24, 2007]. *Venetec Int'l, Inc. v. Nexus Medical, LLC*, USDC D.Del., Case No. 1:07-CV-00057.

Nexus Medical, LLC's Answer to Venetec International, Inc.'s First Supplemental Complaint and Counterclaim [dated Aug. 8, 2007]. *Venetec Int'l, Inc. v. Nexus Medical, LLC*, USDC D.Del., Case No. 1:07-CV-00057.

Venetec International, Inc.'s Reply to Nexus Medical, LLC's Counterclaim [filed Aug. 28, 2007]. *Venetec Int'l, Inc. v. Nexus Medical, LLC*, USDC D.Del., Case No. 1:07-CV-00057.

Second Supplemental Complaint [filed Sep. 5, 2007]. *Venetec Int'l, Inc. v. Nexus Medical, LLC*, USDC D.Del., Case No. 1:07-CV-00057.

Nexus Medical, LLC's Answer to Venetec International, Inc.'s Second Supplemental Complaint and Counterclaim [filed Sep. 19, 2007]. *Venetec Int'l, Inc. v. Nexus Medical, LLC*, USDC D.Del., Case No. 1:07-CV-00057.

Venetec International Inc.'s Reply to Nexus Medical, LLC's Counterclaim [filed Sep. 27, 2007]. *Venetec Int'l, Inc. v. Nexus Medical, LLC*, USDC D.Del., Case No. 1:07-CV-00057.

Request For Inter Partes Reexamination Under 37 C.F.R. 1.913 [filed Jun. 25, 2007]. In re Bierman, USPTO, Reexamination No. 95/000,271.

Civil Docket for Case No. 1:07-CV-00057 [printed Oct. 22, 2007].

* cited by examiner

FIG. 1

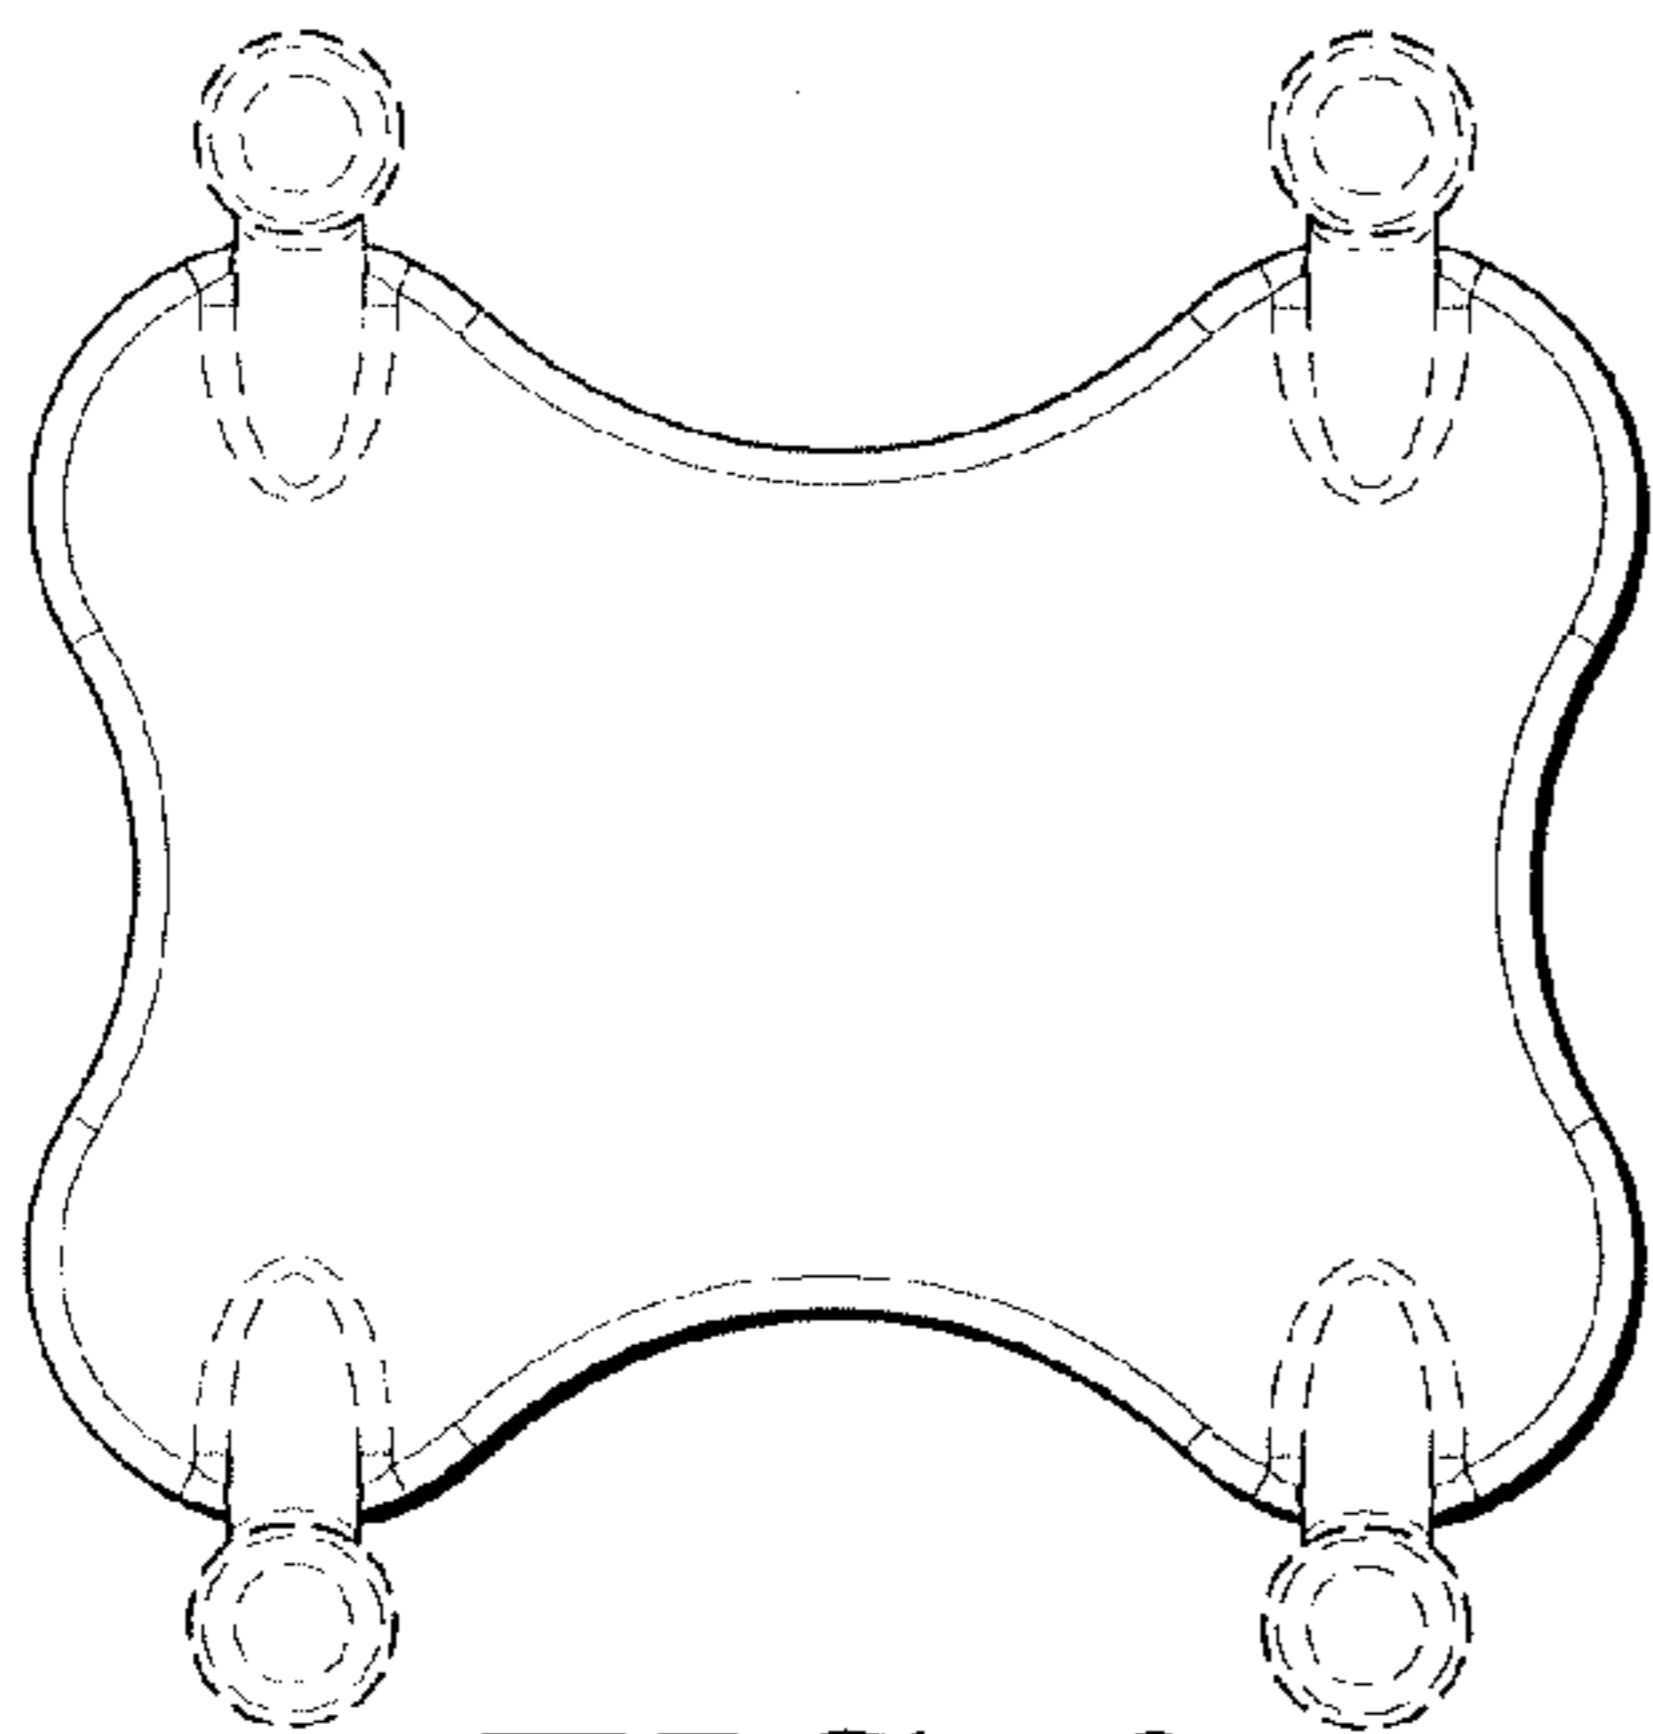
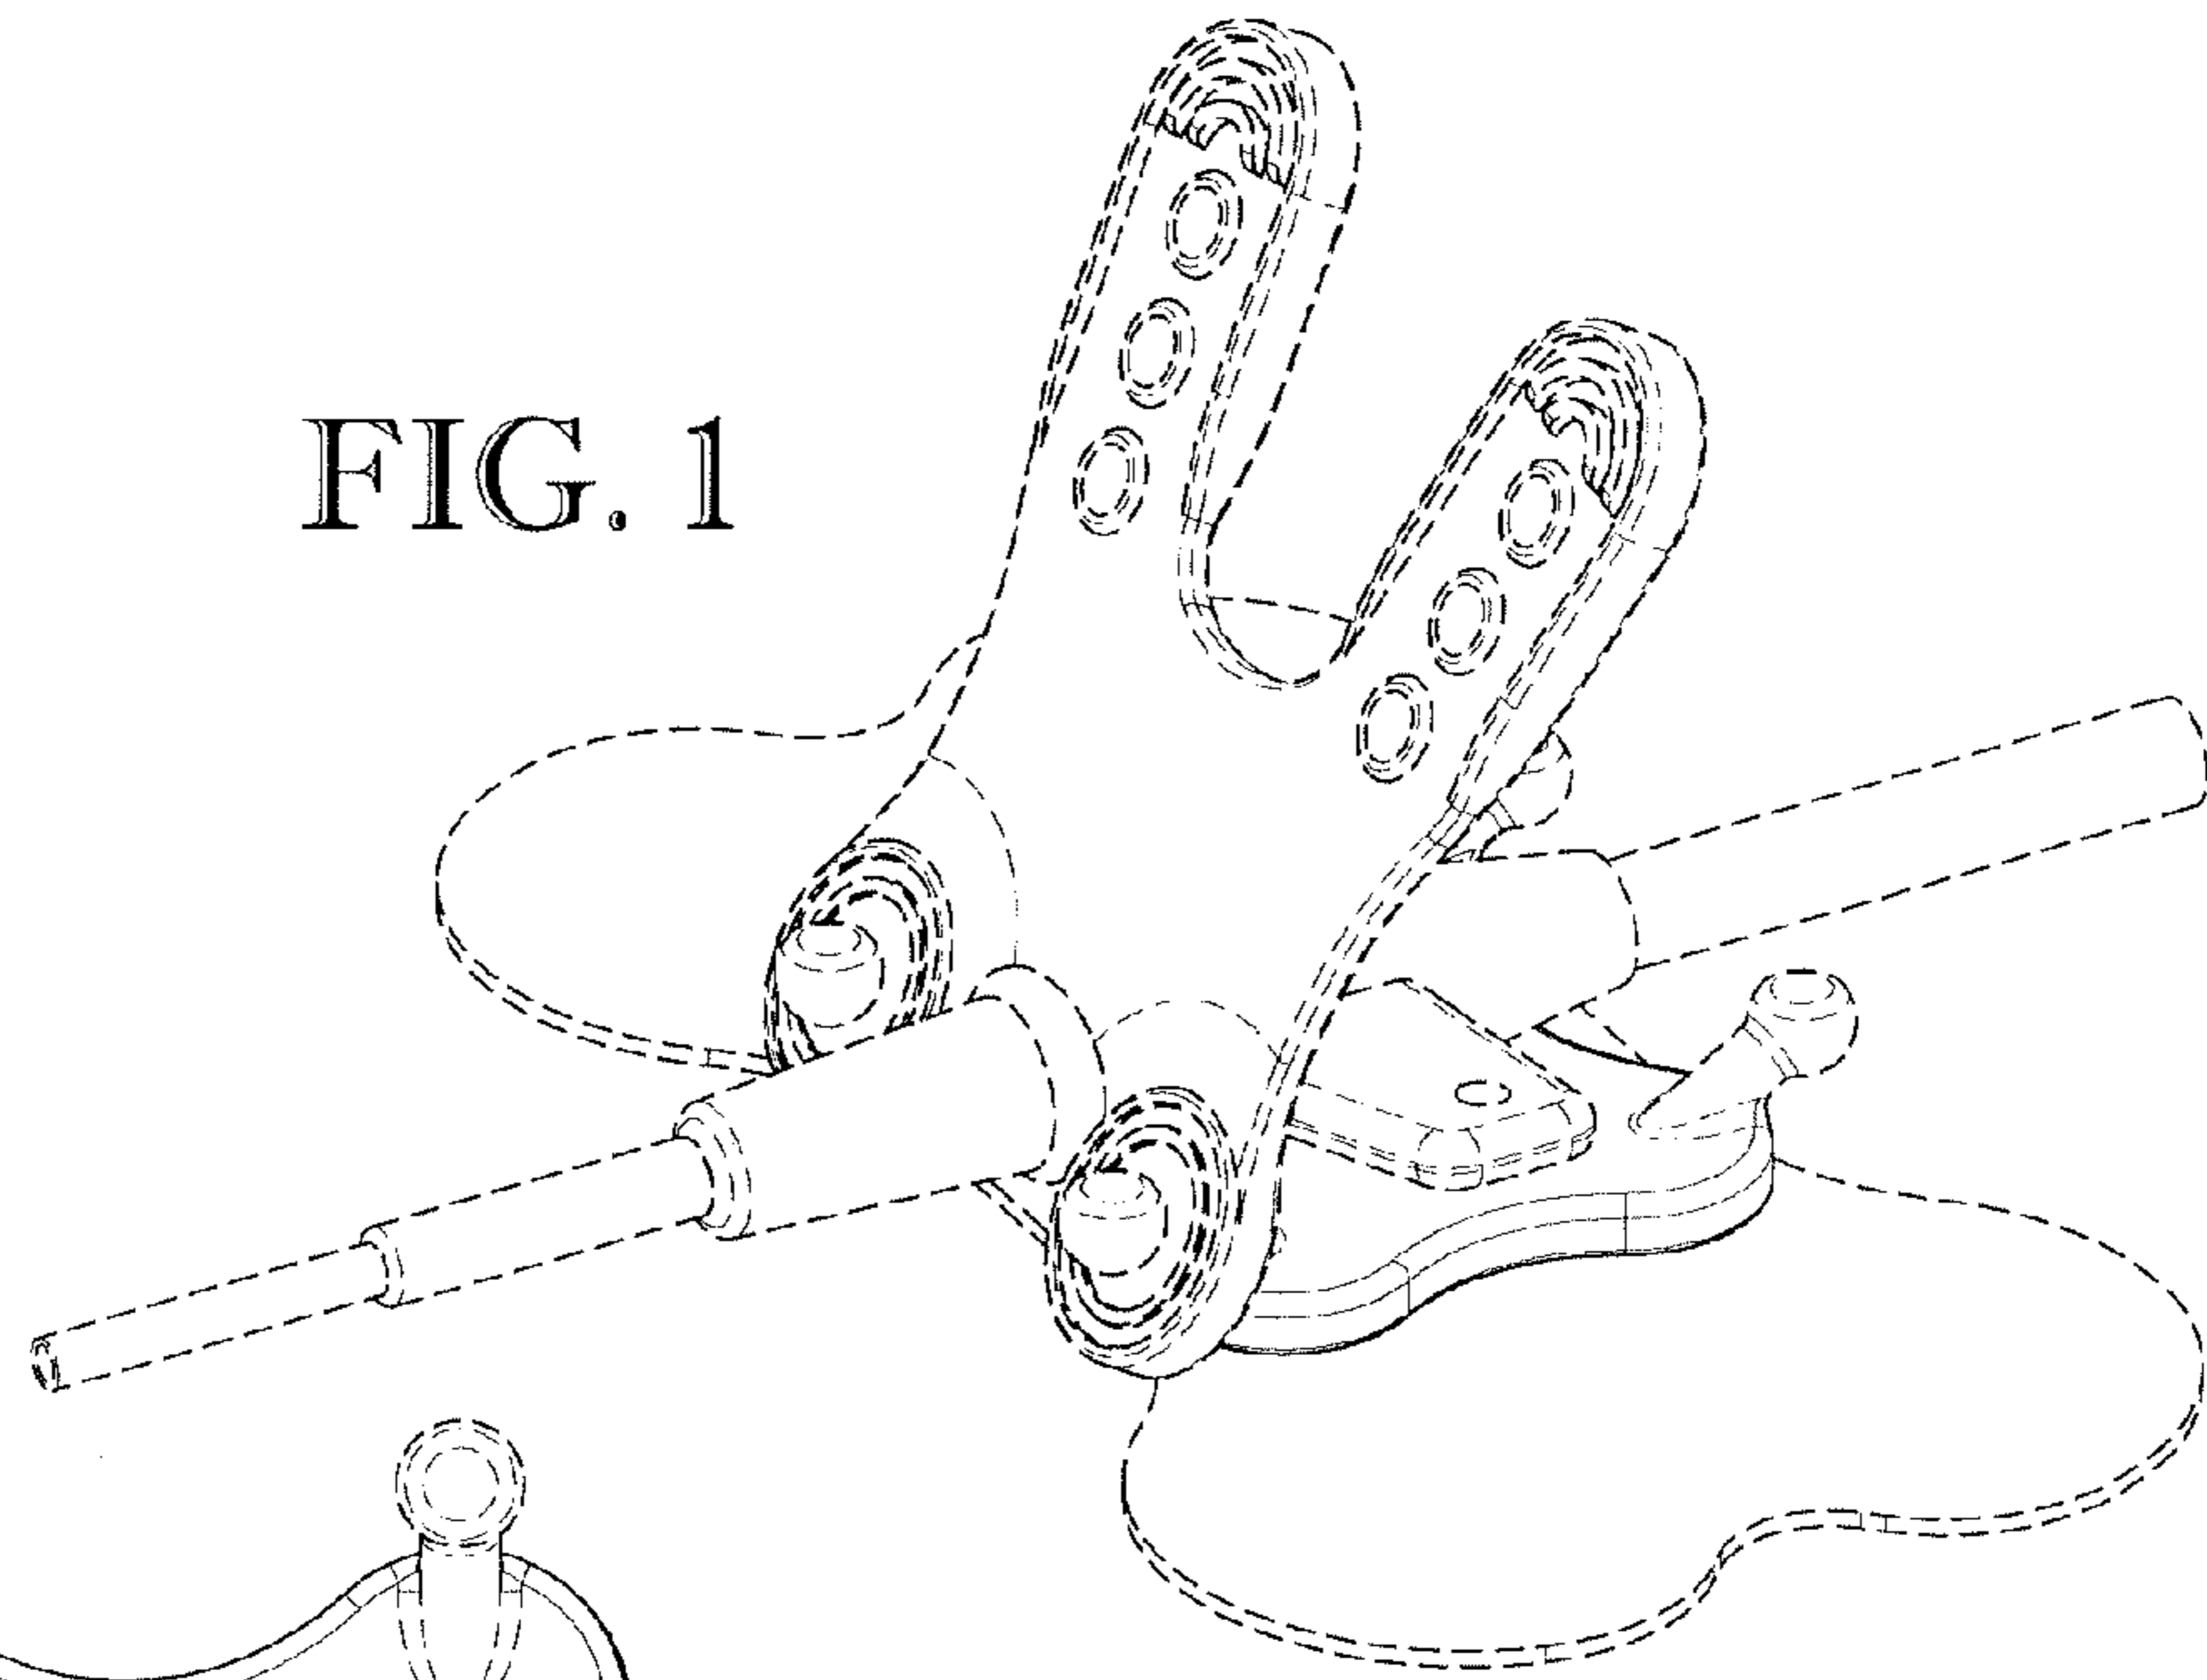


FIG. 3

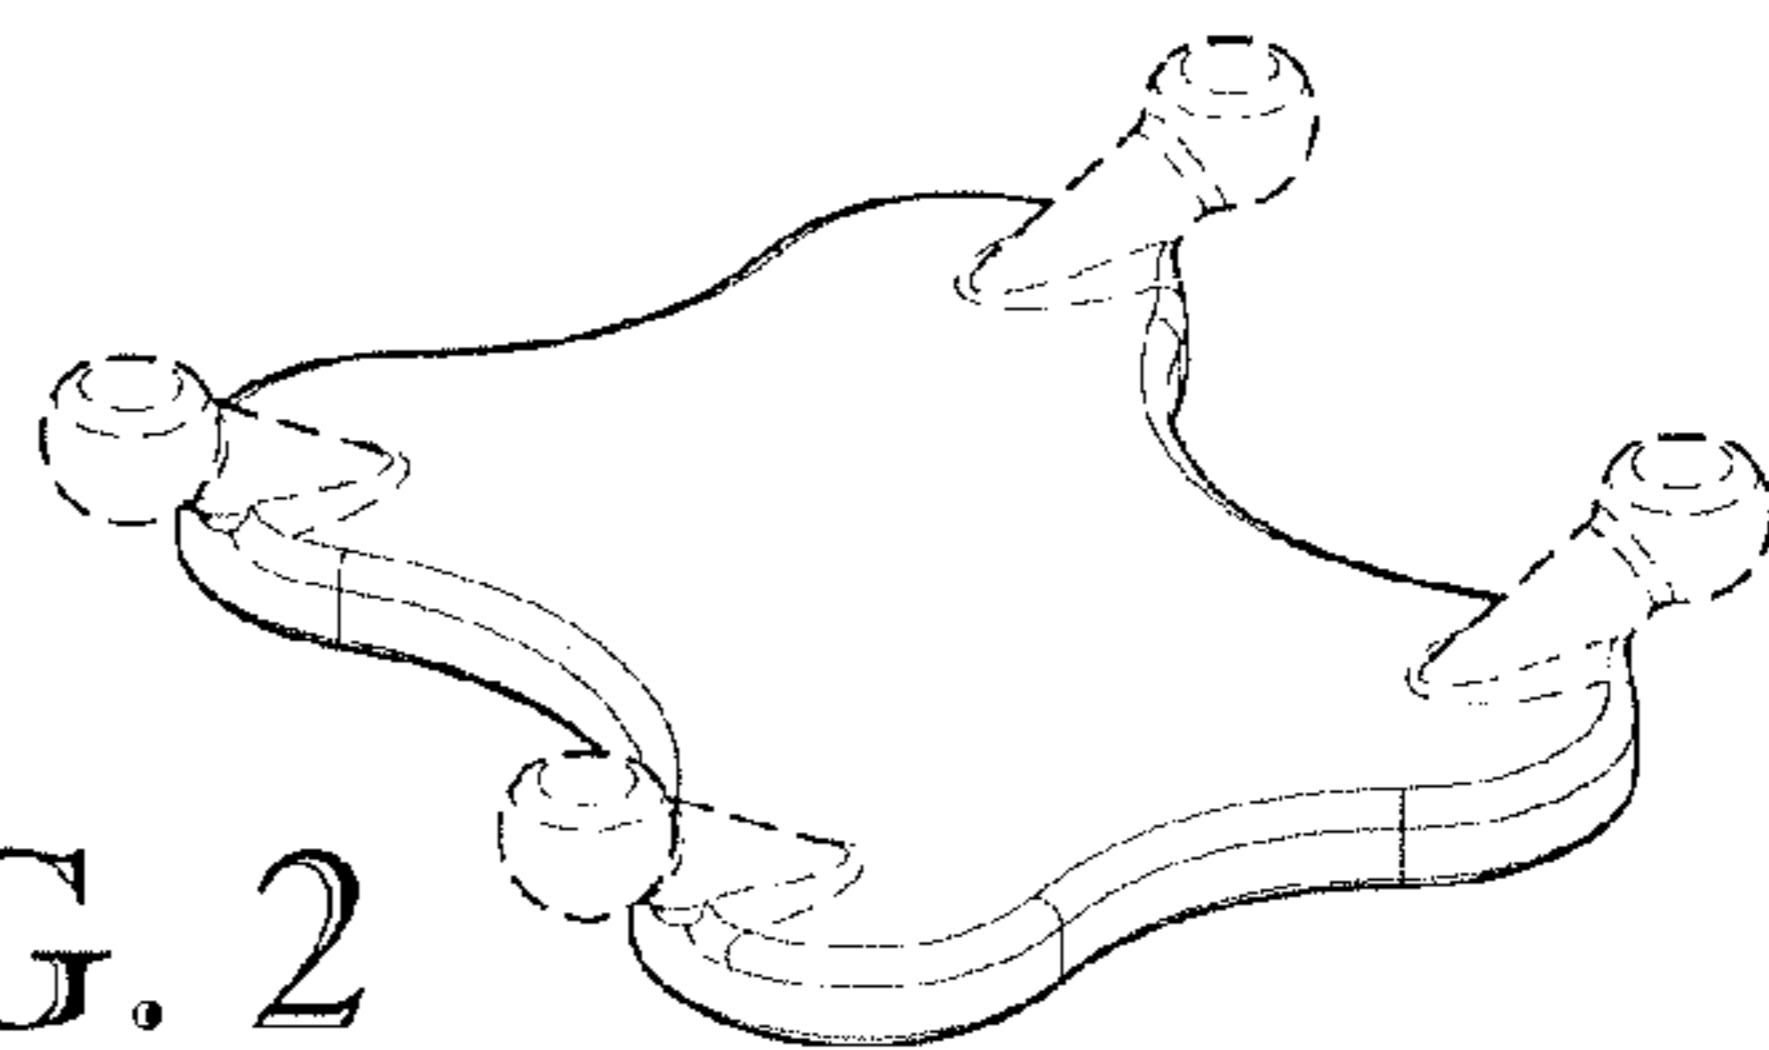


FIG. 2

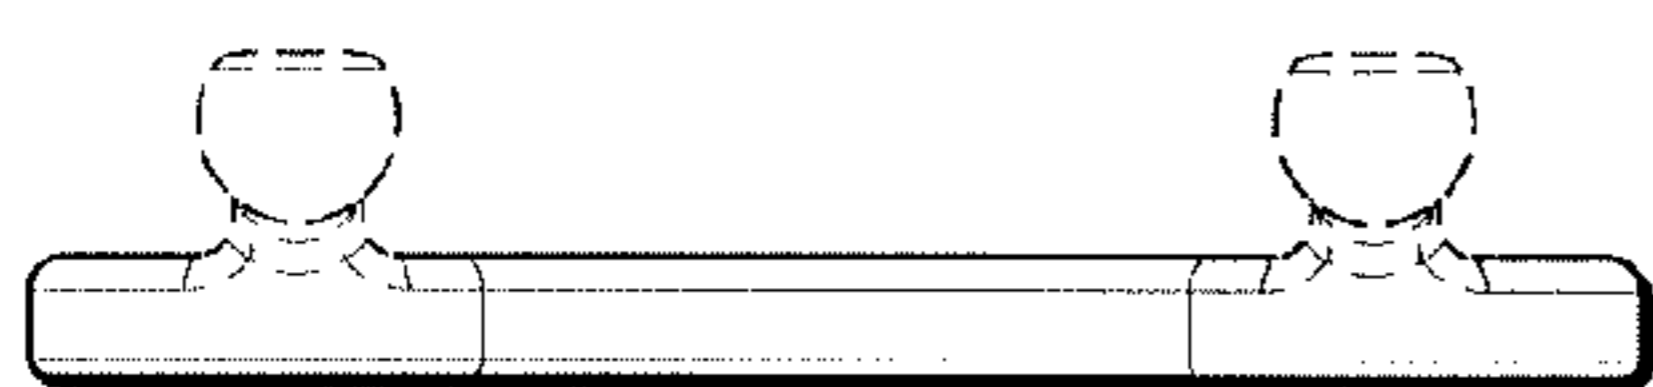


FIG. 4

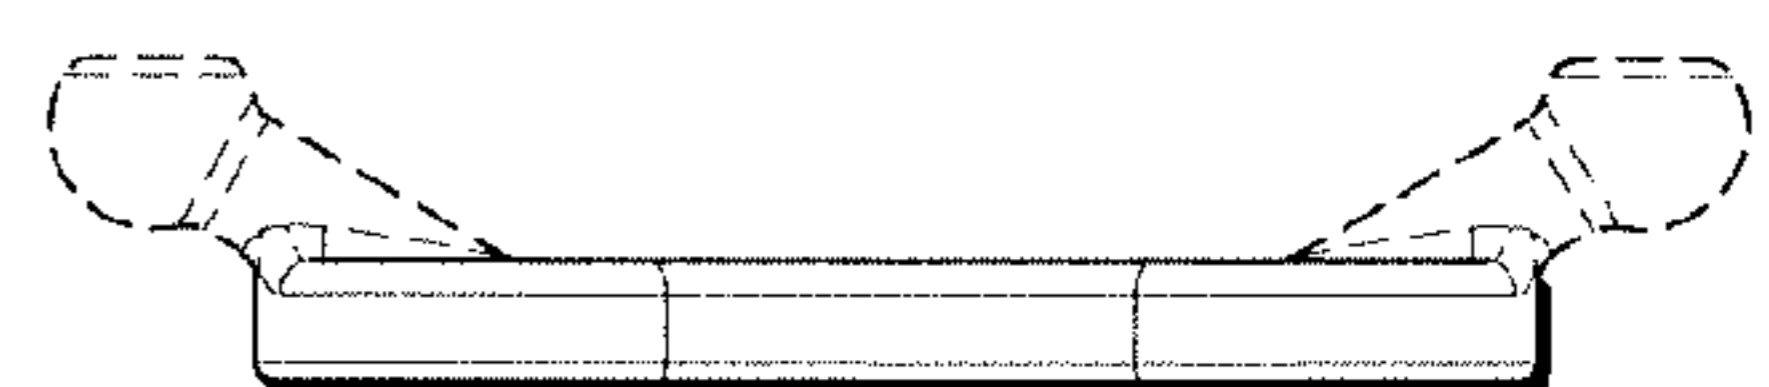


FIG. 5

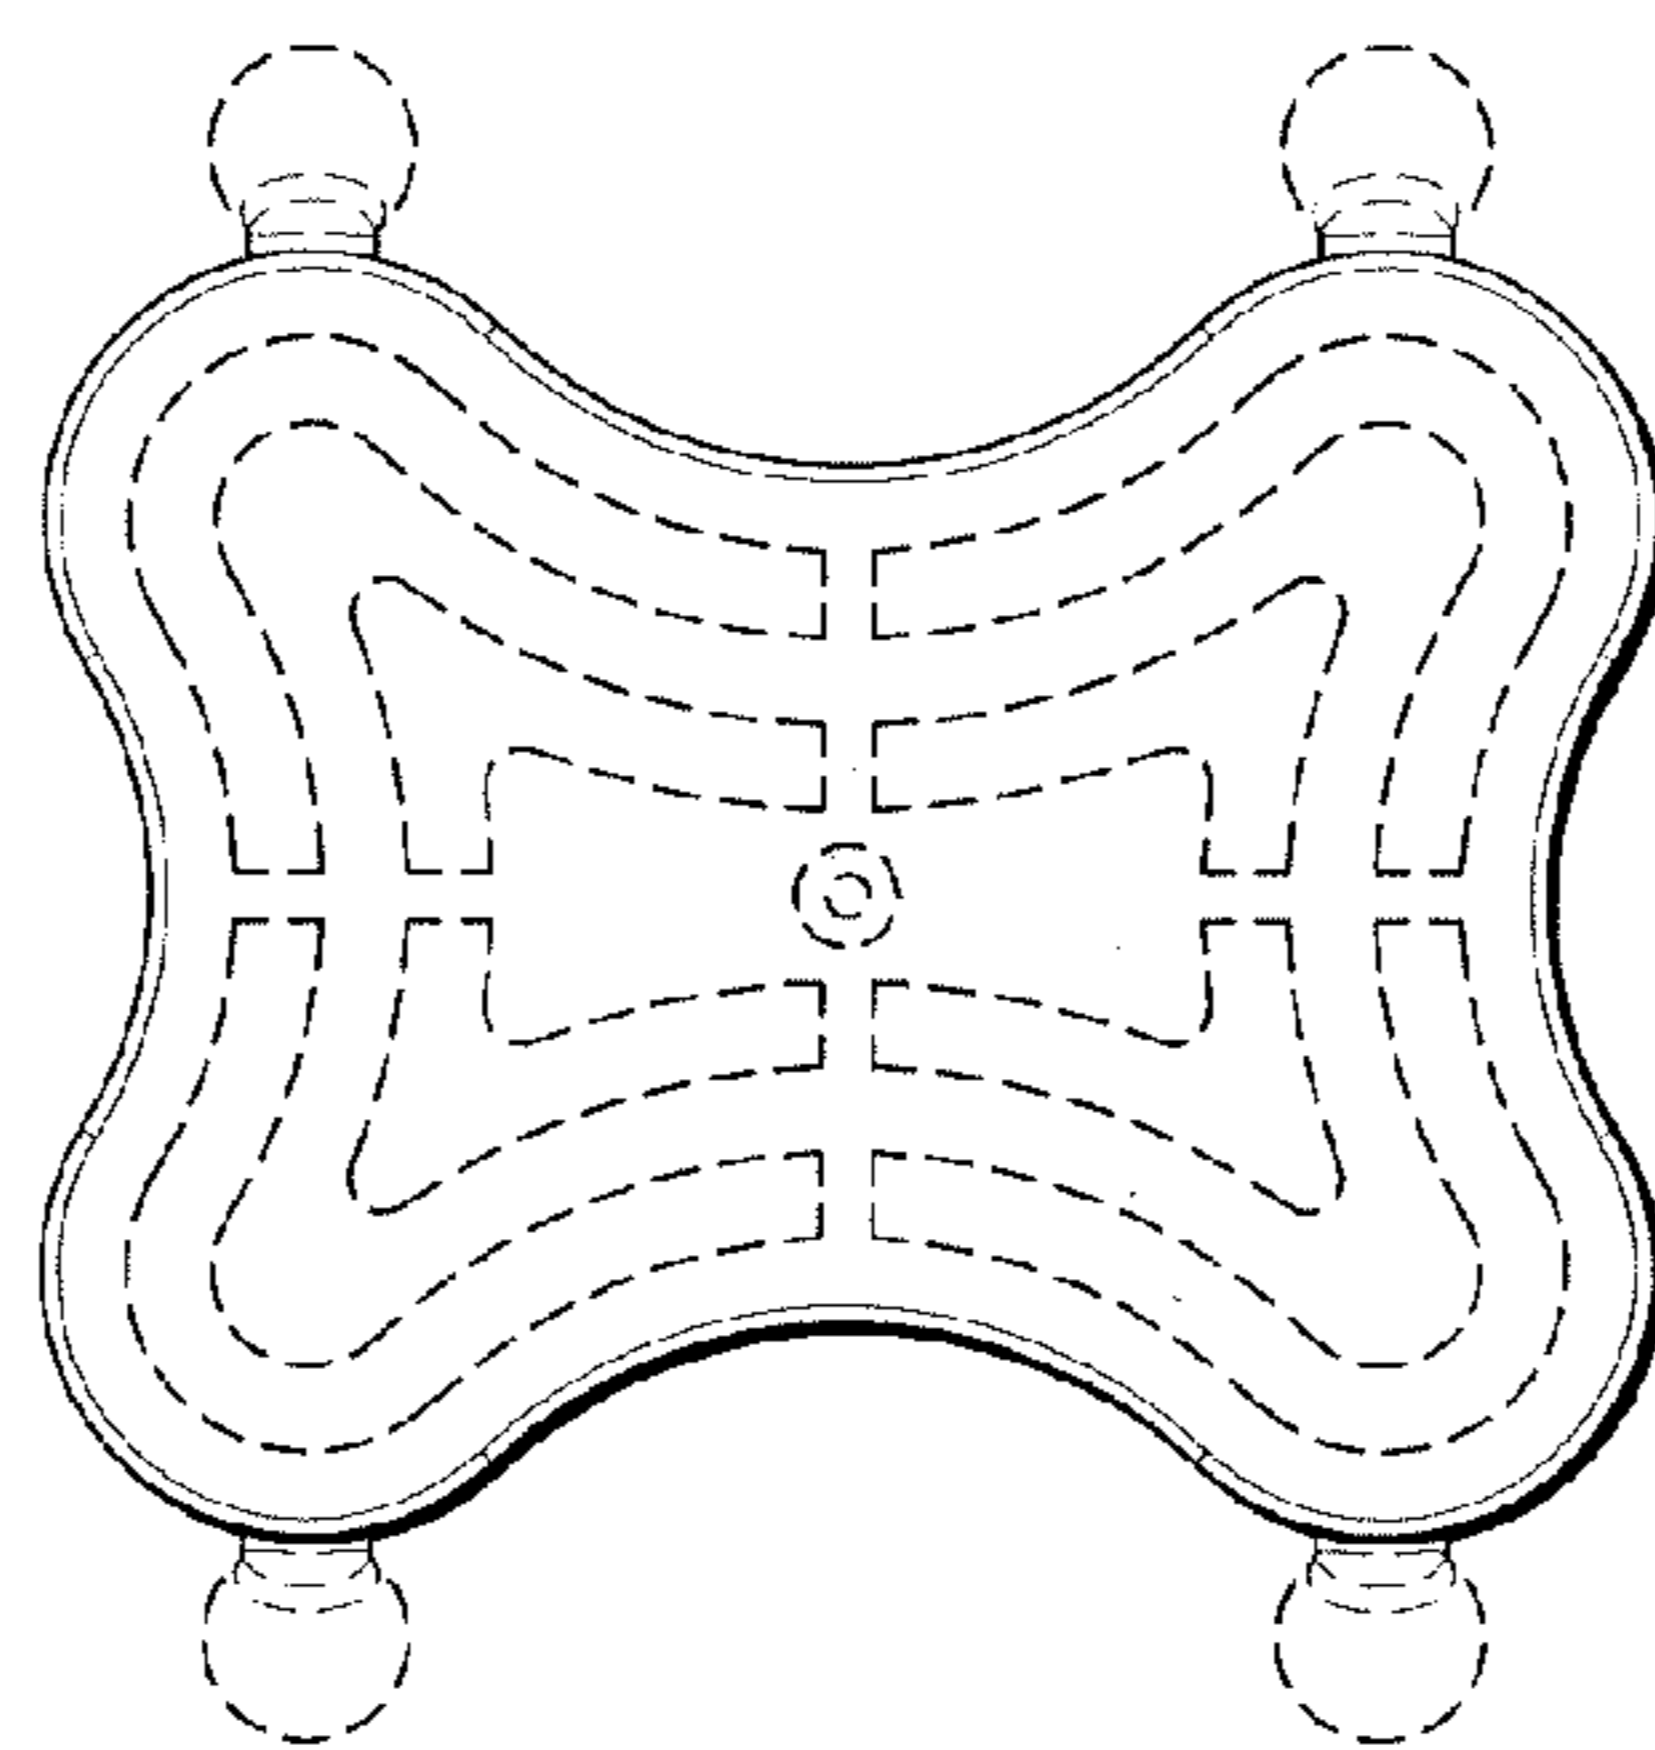


FIG. 6