

US00D571006S

(12) **United States Design Patent** (10) **Patent No.:** **US D571,006 S**
Baxter et al. (45) **Date of Patent:** **** Jun. 10, 2008**

(54) **OVAL TAPERING BLUNT CANNULA PROXIMAL PORTION**

5,201,717 A 4/1993 Wyatt et al.
5,356,396 A 10/1994 Wyatt et al.

(75) Inventors: **Charles S. Baxter**, Worthington, OH (US); **Theodore J. Mosler**, Raleigh, NC (US); **Charles R. Patzer**, Columbus, OH (US)

(Continued)

FOREIGN PATENT DOCUMENTS

(73) Assignee: **Smiths Medical ASD, Inc.**, Rockland, MA (US)

EP 0050459 B1 2/1985

(**) Term: **14 Years**

(Continued)

(21) Appl. No.: **29/278,291**

OTHER PUBLICATIONS

(22) Filed: **Mar. 23, 2007**

Photograph of SECURE sample site and shielded needle.

(51) **LOC (8) Cl.** **24-02**

(Continued)

(52) **U.S. Cl.** **D24/130**

Primary Examiner—Louis S Zarfaz

(58) **Field of Classification Search** D24/130, D24/112, 146, 147; 606/167, 170, 184, 185; 604/251, 264, 256, 168, 192, 198, 203, 411
See application file for complete search history.

Assistant Examiner—Eric L Goodman

(74) *Attorney, Agent, or Firm*—Wood, Harron & Evans, LLP

(56) **References Cited**

(57) **CLAIM**

U.S. PATENT DOCUMENTS

The ornamental design for an oval tapering blunt cannula proximal portion, as shown and described.

- 2,989,053 A 6/1961 Hamilton
- 3,352,531 A 11/1967 Kilmarx
- 4,058,121 A 11/1977 Choksi et al.
- 4,106,491 A 8/1978 Guerra
- 4,578,063 A 3/1986 Inman et al.
- 4,610,374 A 9/1986 Buehler
- 4,710,180 A 12/1987 Johnson
- 4,795,446 A 1/1989 Fecht
- 4,834,716 A 5/1989 Ogle, II
- 4,904,238 A 2/1990 Williams
- 4,983,160 A 1/1991 Steppe et al.
- 5,071,413 A 12/1991 Utterberg
- 5,098,407 A * 3/1992 Okamura 604/248
- 5,100,394 A 3/1992 Dudar et al.
- 5,112,318 A * 5/1992 Novacek et al. 604/240
- 5,114,400 A 5/1992 Lynn
- 5,135,489 A 8/1992 Jepson et al.
- 5,149,327 A 9/1992 Oshiyama
- 5,199,948 A 4/1993 McPhee

DESCRIPTION

FIG. 1 is a perspective view of an embodiment of our new, original and ornamental design;

FIG. 2 is a front elevational view thereof, the rear elevational view being a mirror image thereof;


FIG. 3 is a right side elevational view thereof, the left side elevational view being a mirror image thereof;

FIG. 4 is a bottom plan view thereof; and,

FIG. 5 is a top plan view thereof.

The structure shown in phantom is for illustrative purposes only and forms no part of the claimed design.

1 Claim, 2 Drawing Sheets

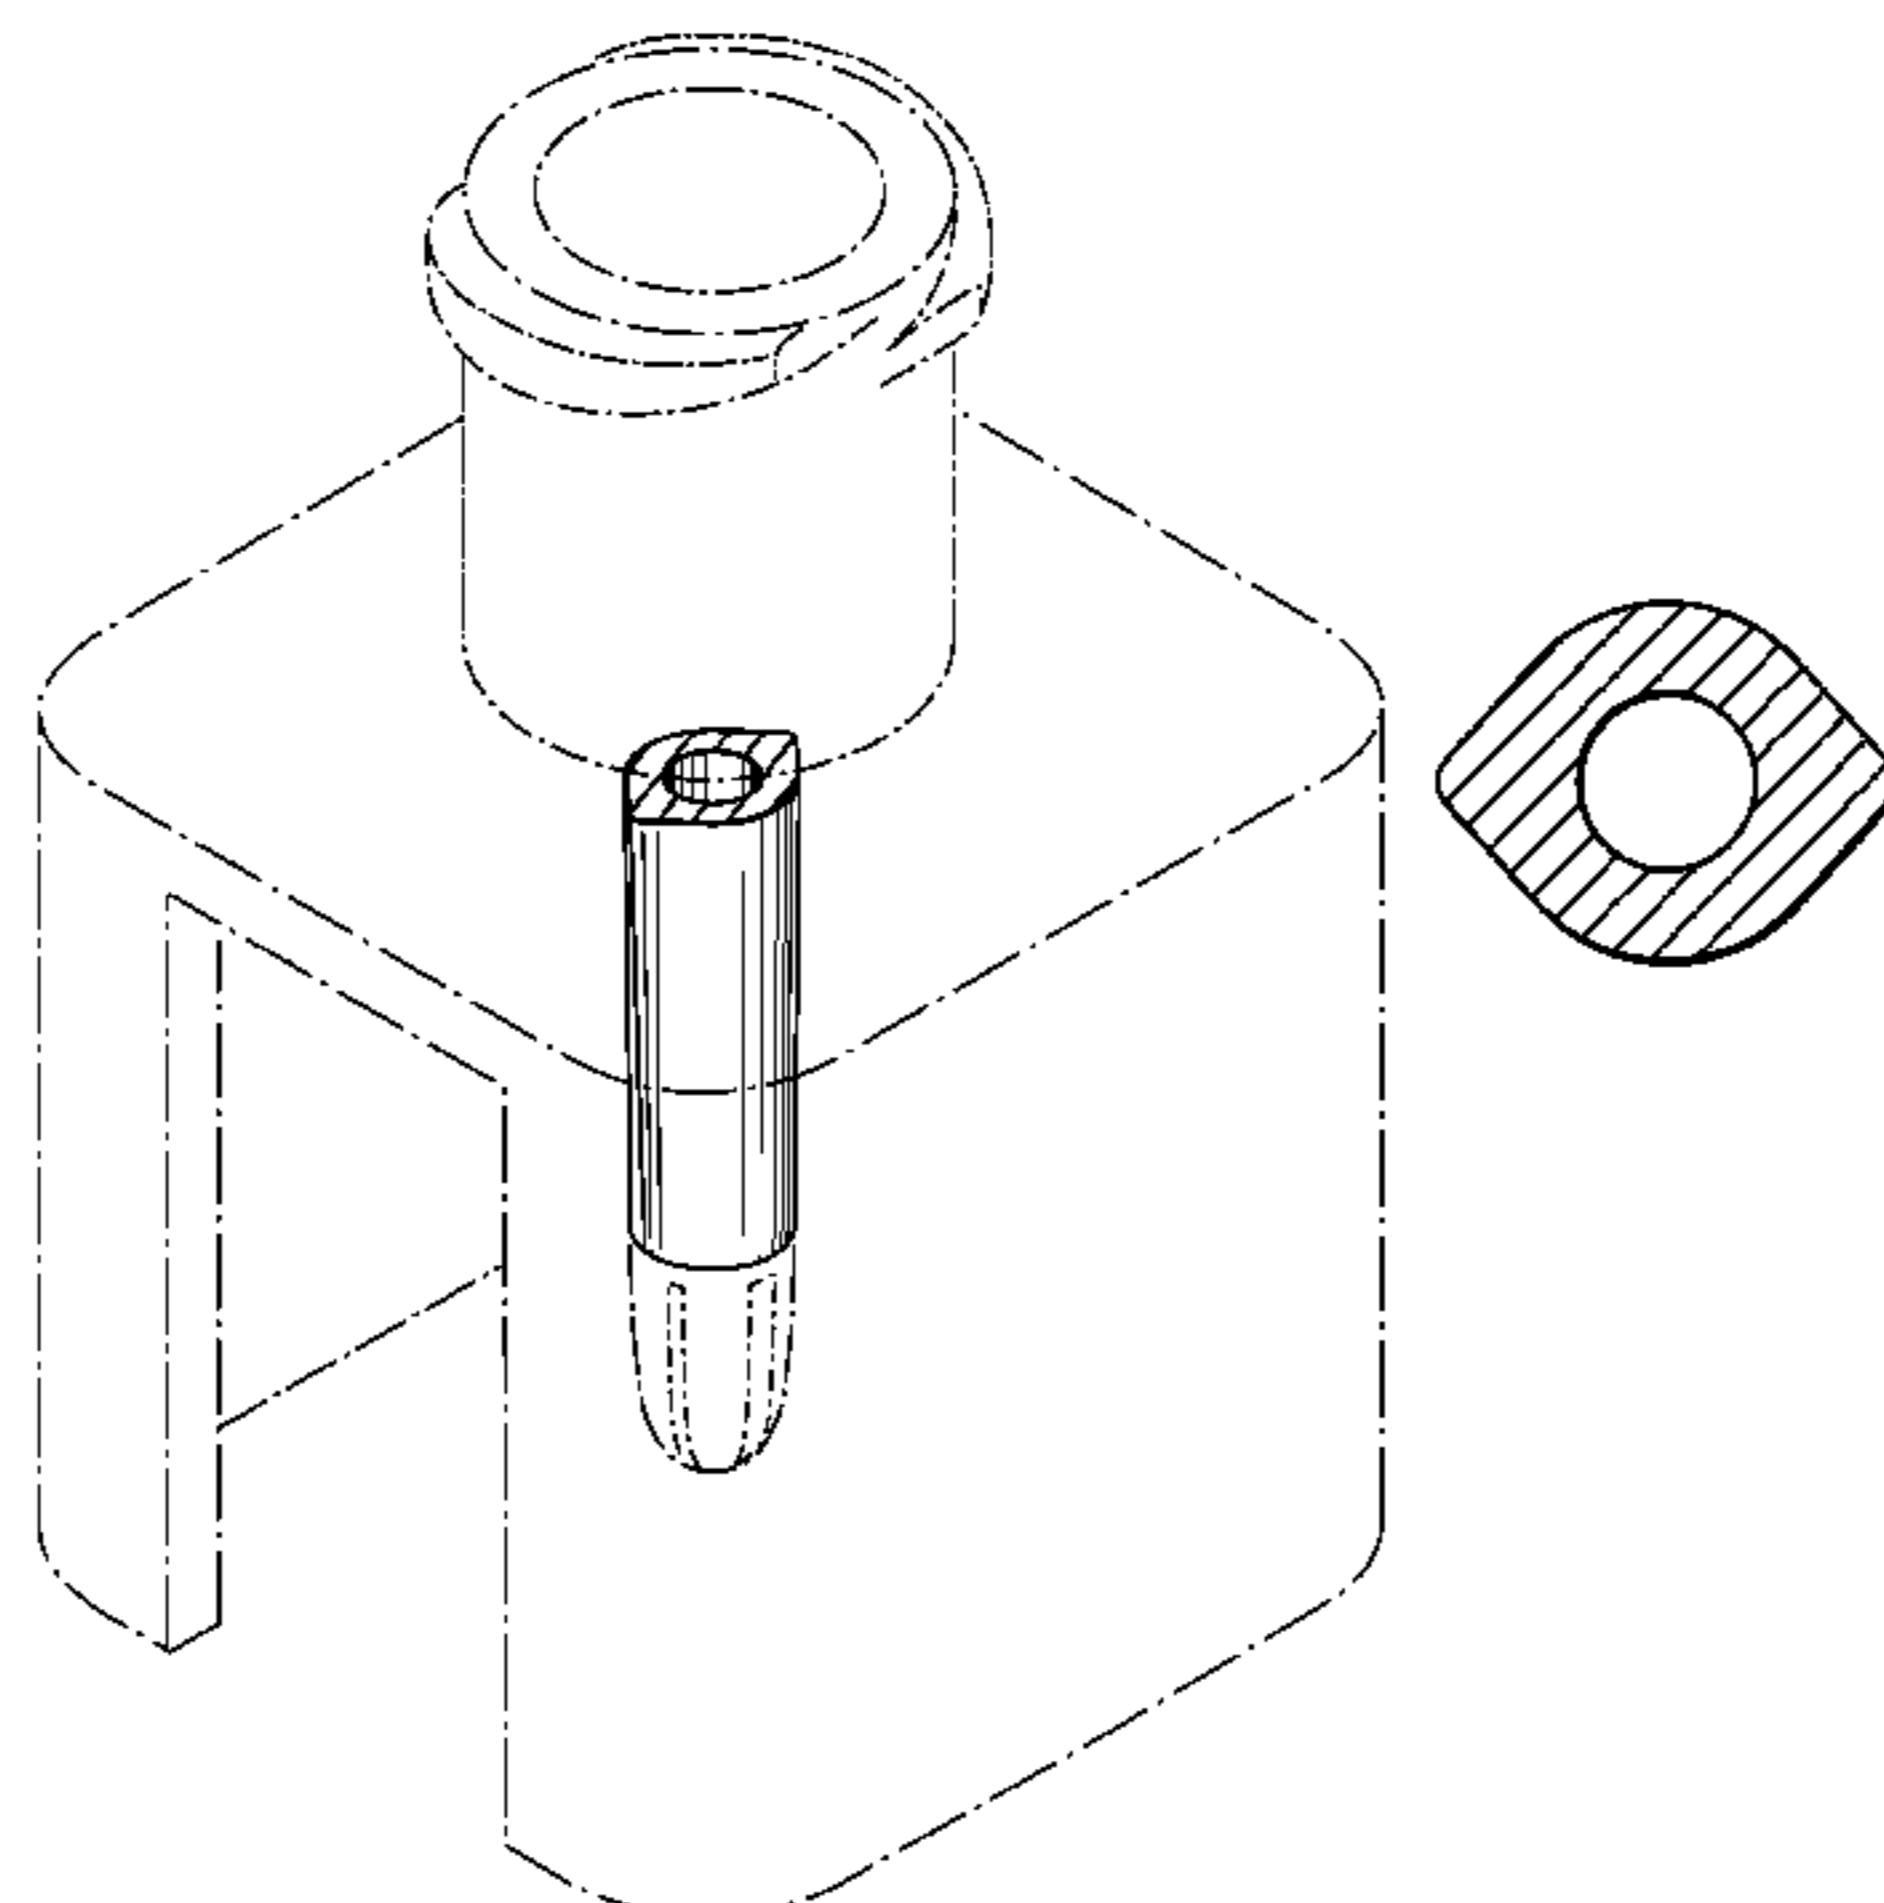

US D571,006 S

Page 2

U.S. PATENT DOCUMENTS

5,447,495 A 9/1995 Lynn et al.
5,453,089 A 9/1995 Brugger
5,466,219 A 11/1995 Lynn et al.
5,474,546 A 12/1995 Ambrisco et al.
5,501,676 A 3/1996 Niedospial et al.
5,632,735 A 5/1997 Wyatt et al.
D393,722 S * 4/1998 Fangrow et al. D24/112
5,776,125 A 7/1998 Dudar et al.
5,833,674 A 11/1998 Turnbull et al.
5,947,954 A * 9/1999 Bonaldo 604/533
D416,086 S * 11/1999 Parris et al. D24/112
5,976,115 A 11/1999 Parris et al.
6,029,946 A 2/2000 Doyle
6,050,978 A 4/2000 Orr et al.
6,387,086 B2 5/2002 Mathias et al.
6,569,125 B2 * 5/2003 Jepson et al. 604/201
7,056,308 B2 6/2006 Utterberg

7,140,592 B2 * 11/2006 Phillips 251/149.6
7,217,246 B1 * 5/2007 Stone 600/585
2002/0143298 A1 * 10/2002 Marsden 604/190
2003/0120221 A1 6/2003 Vaillancourt
2004/0002684 A1 * 1/2004 Lopez 604/240
2004/0227120 A1 * 11/2004 Raybuck 251/149.1
2005/0090805 A1 * 4/2005 Shaw et al. 604/523

FOREIGN PATENT DOCUMENTS

GB 2040379 A 8/1980
WO 9422524 10/1994
WO 9641649 12/1996

OTHER PUBLICATIONS

Photograph of VAMP sample site and blunt cannula/adaptor.
Photograph of SAFESSET sample site and blunt cannula/adaptor.

* cited by examiner

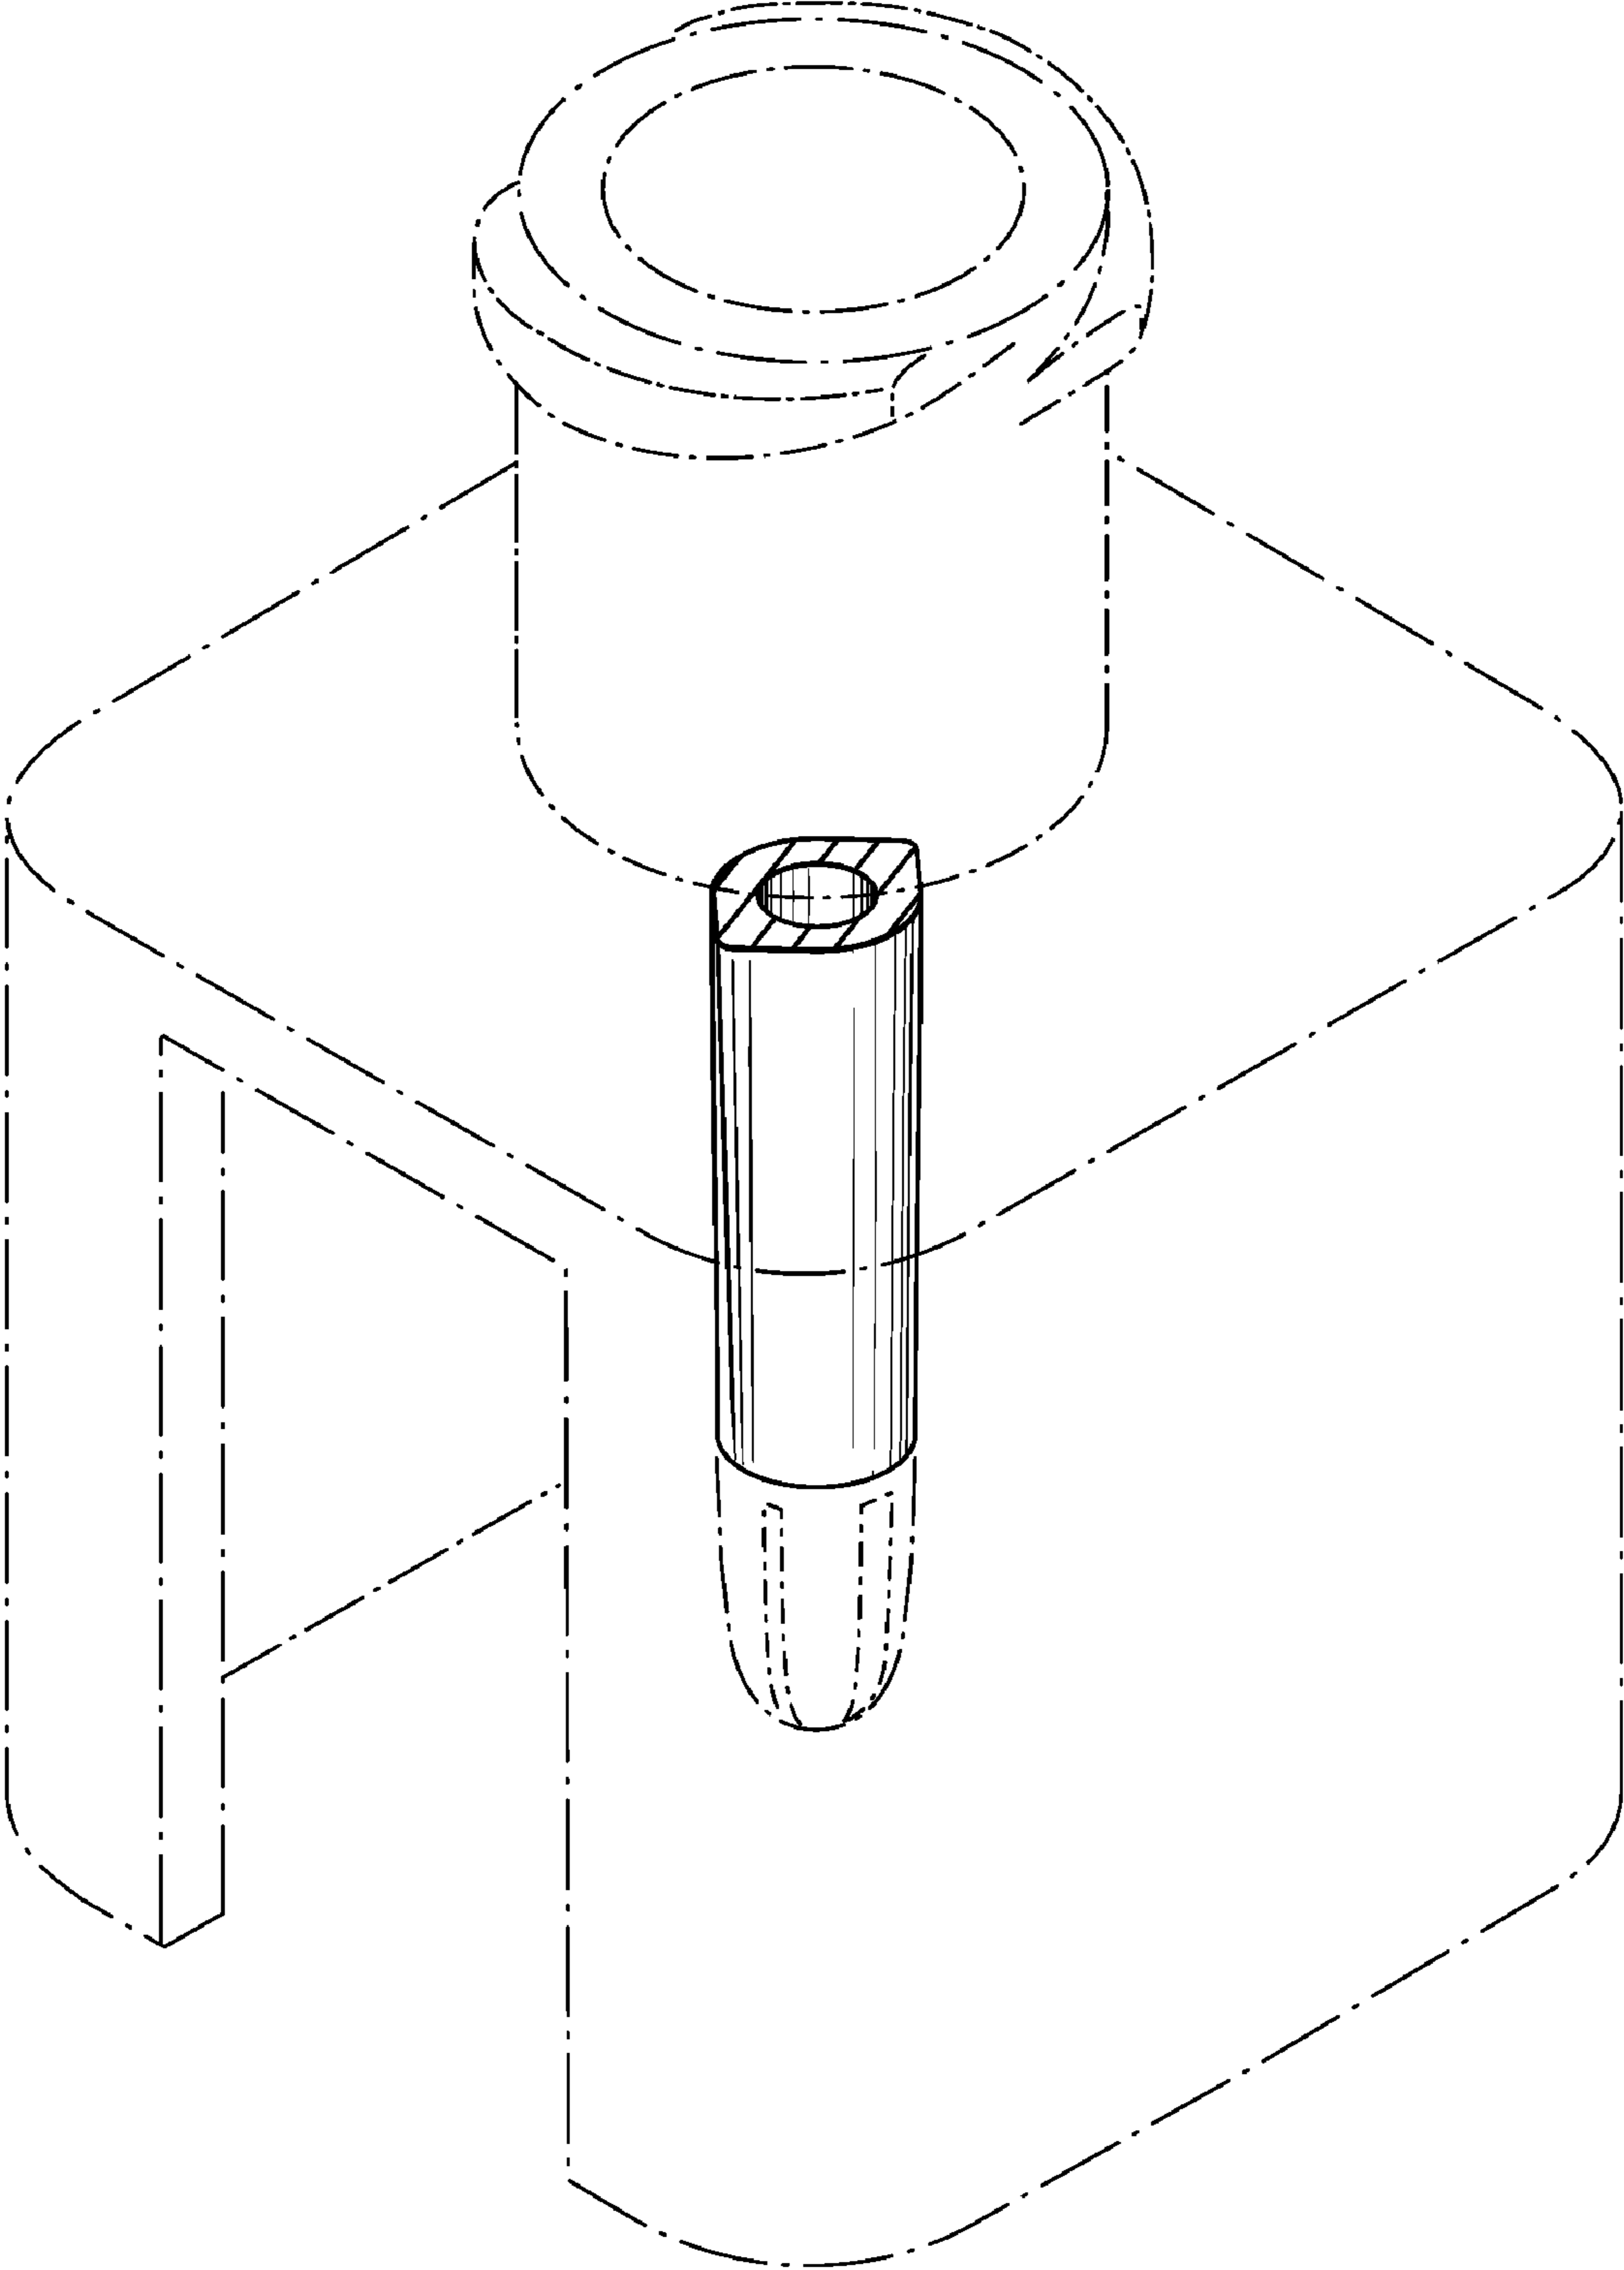


FIG. 1

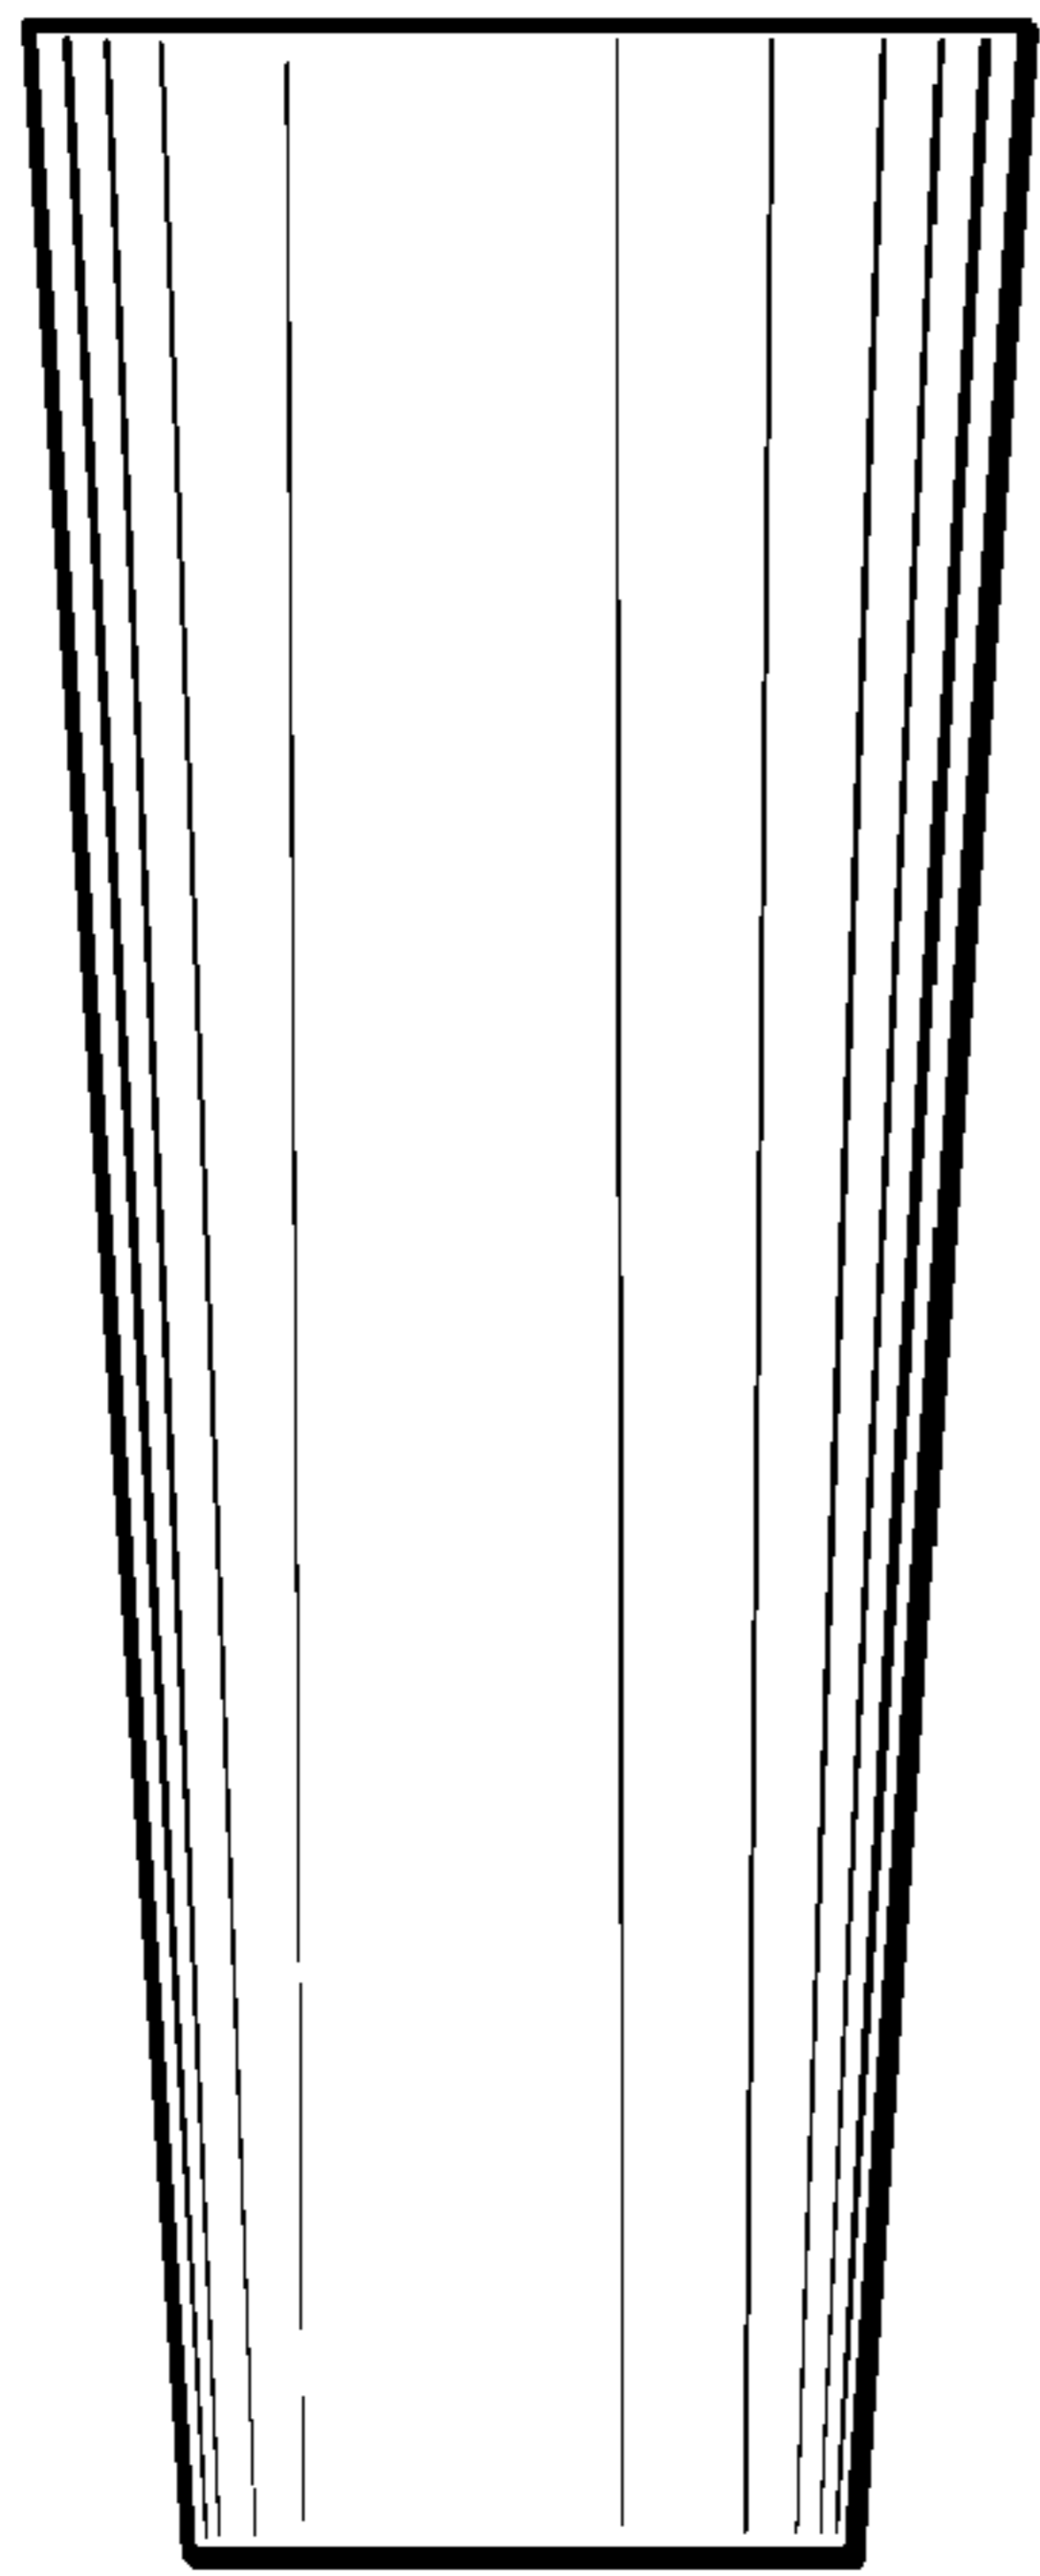


FIG. 2

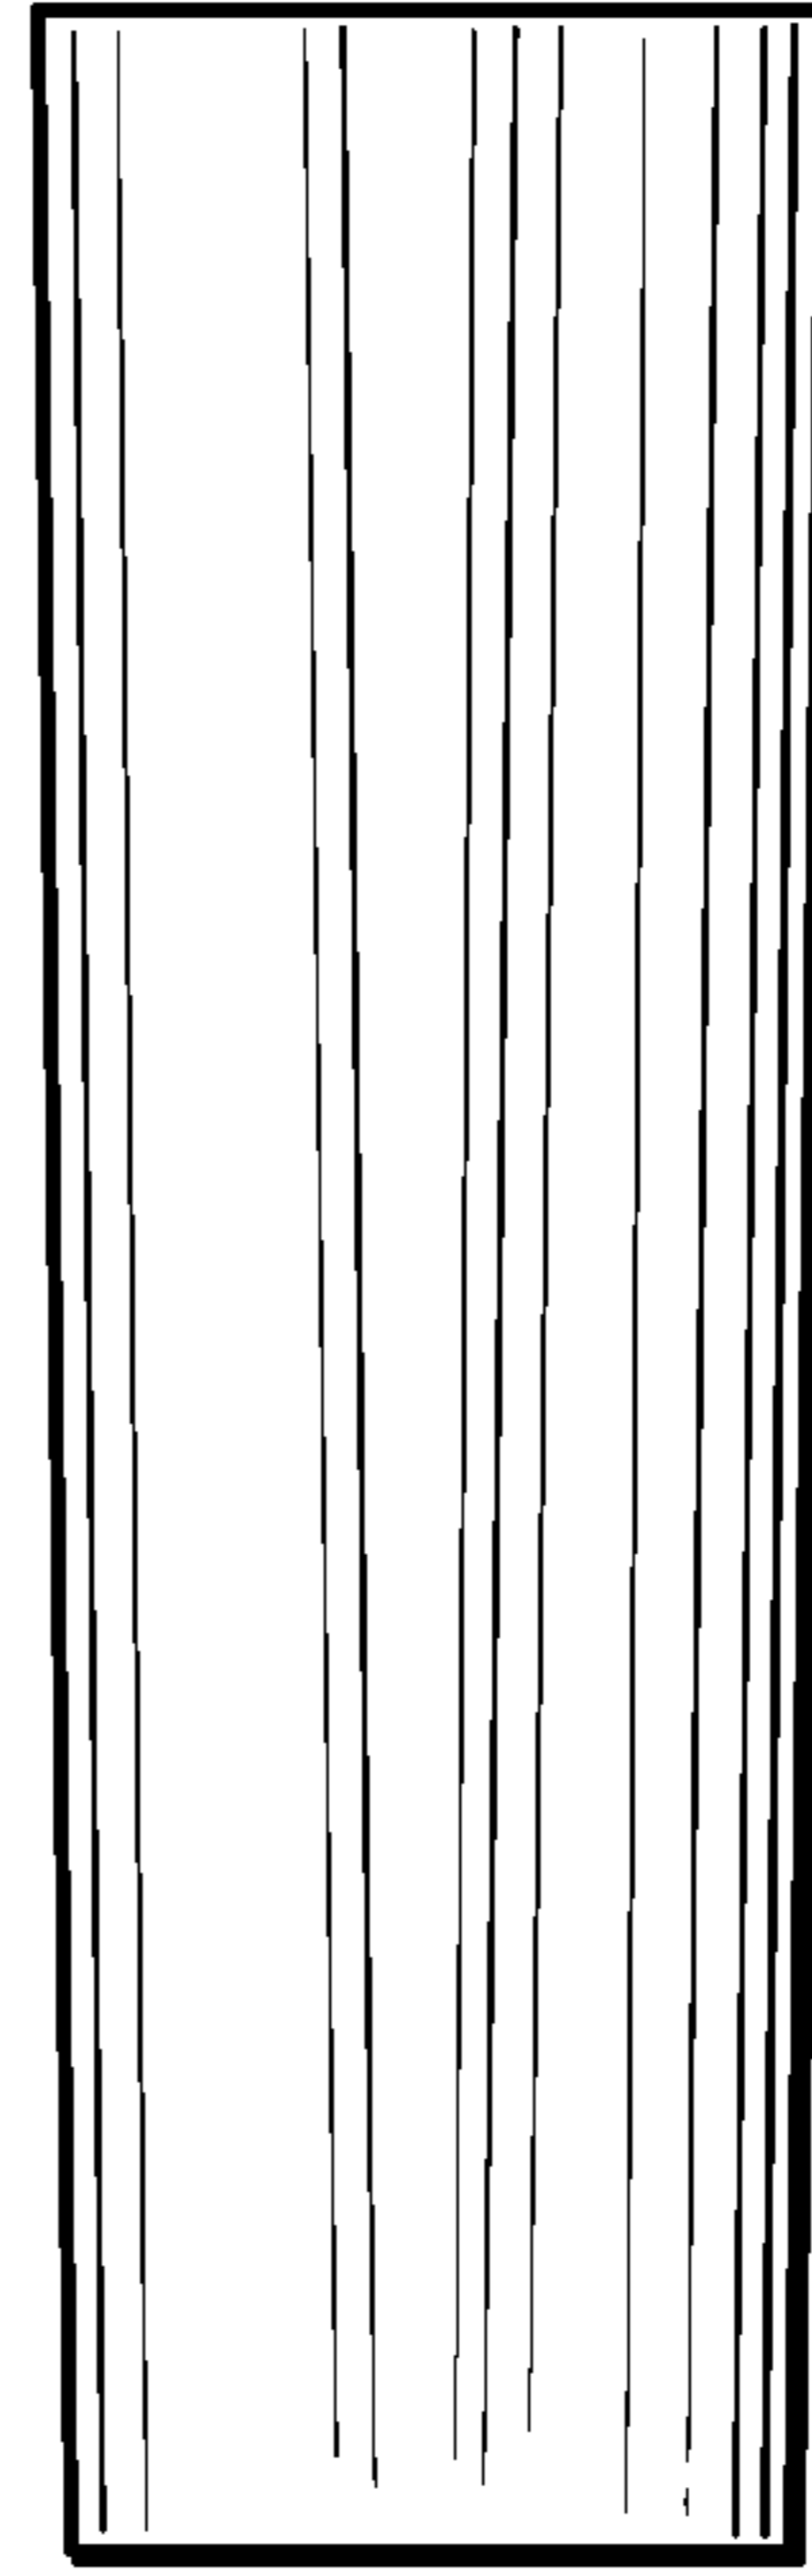


FIG. 3

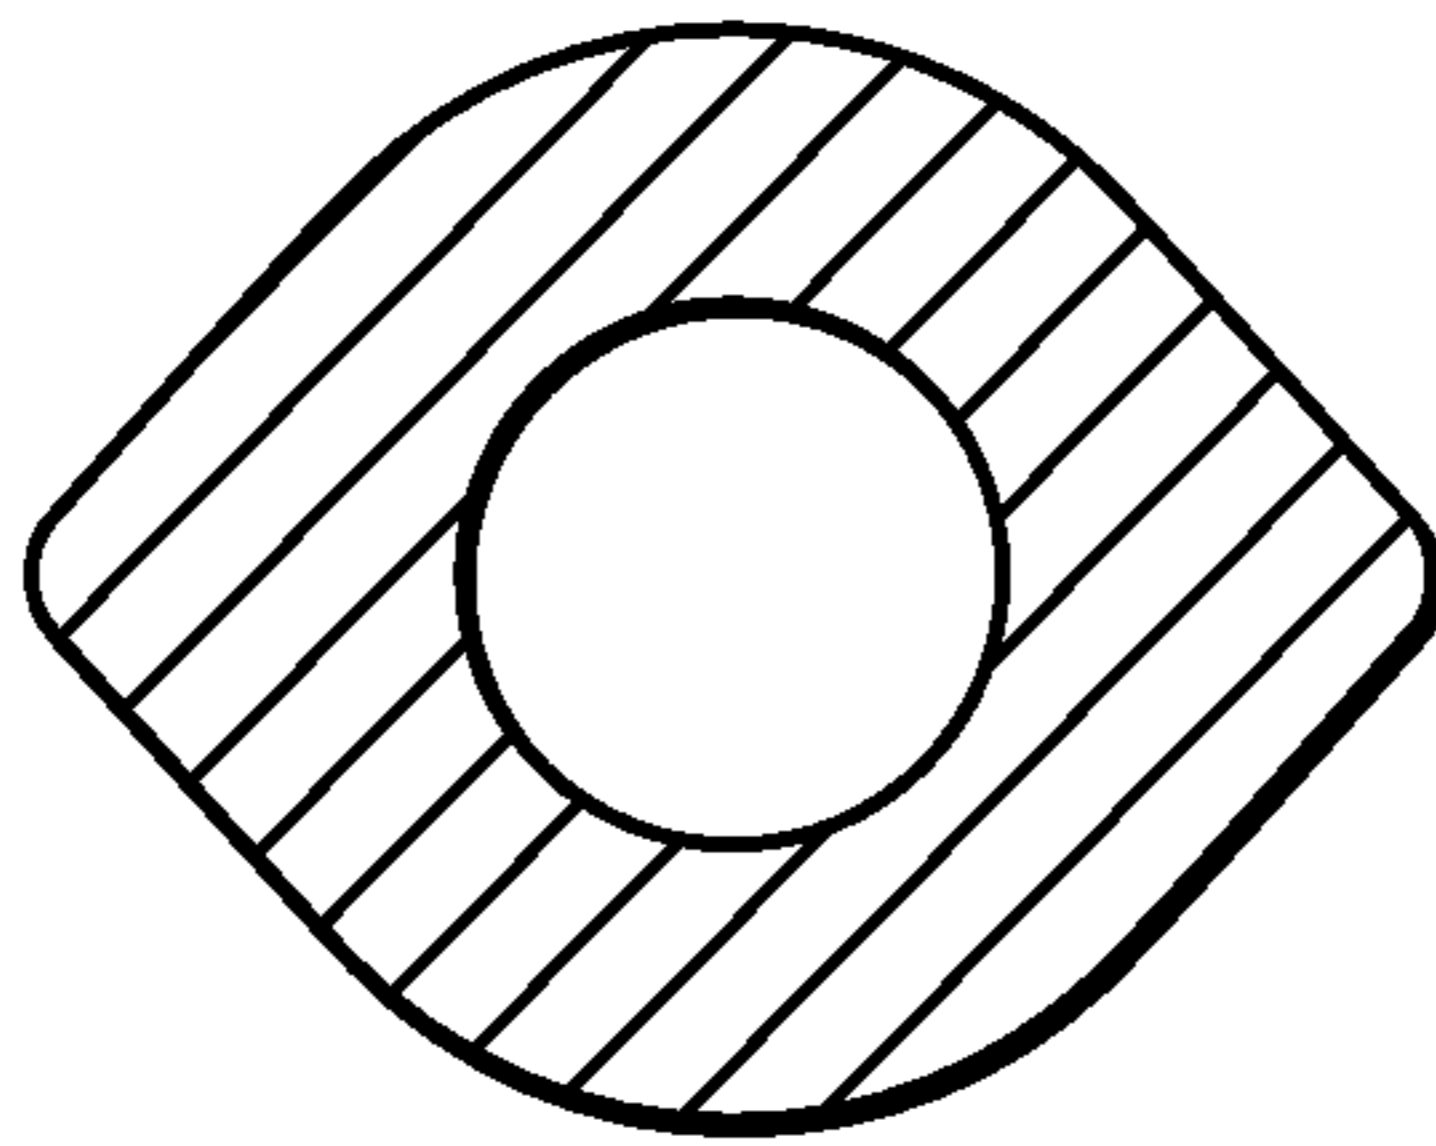


FIG. 4

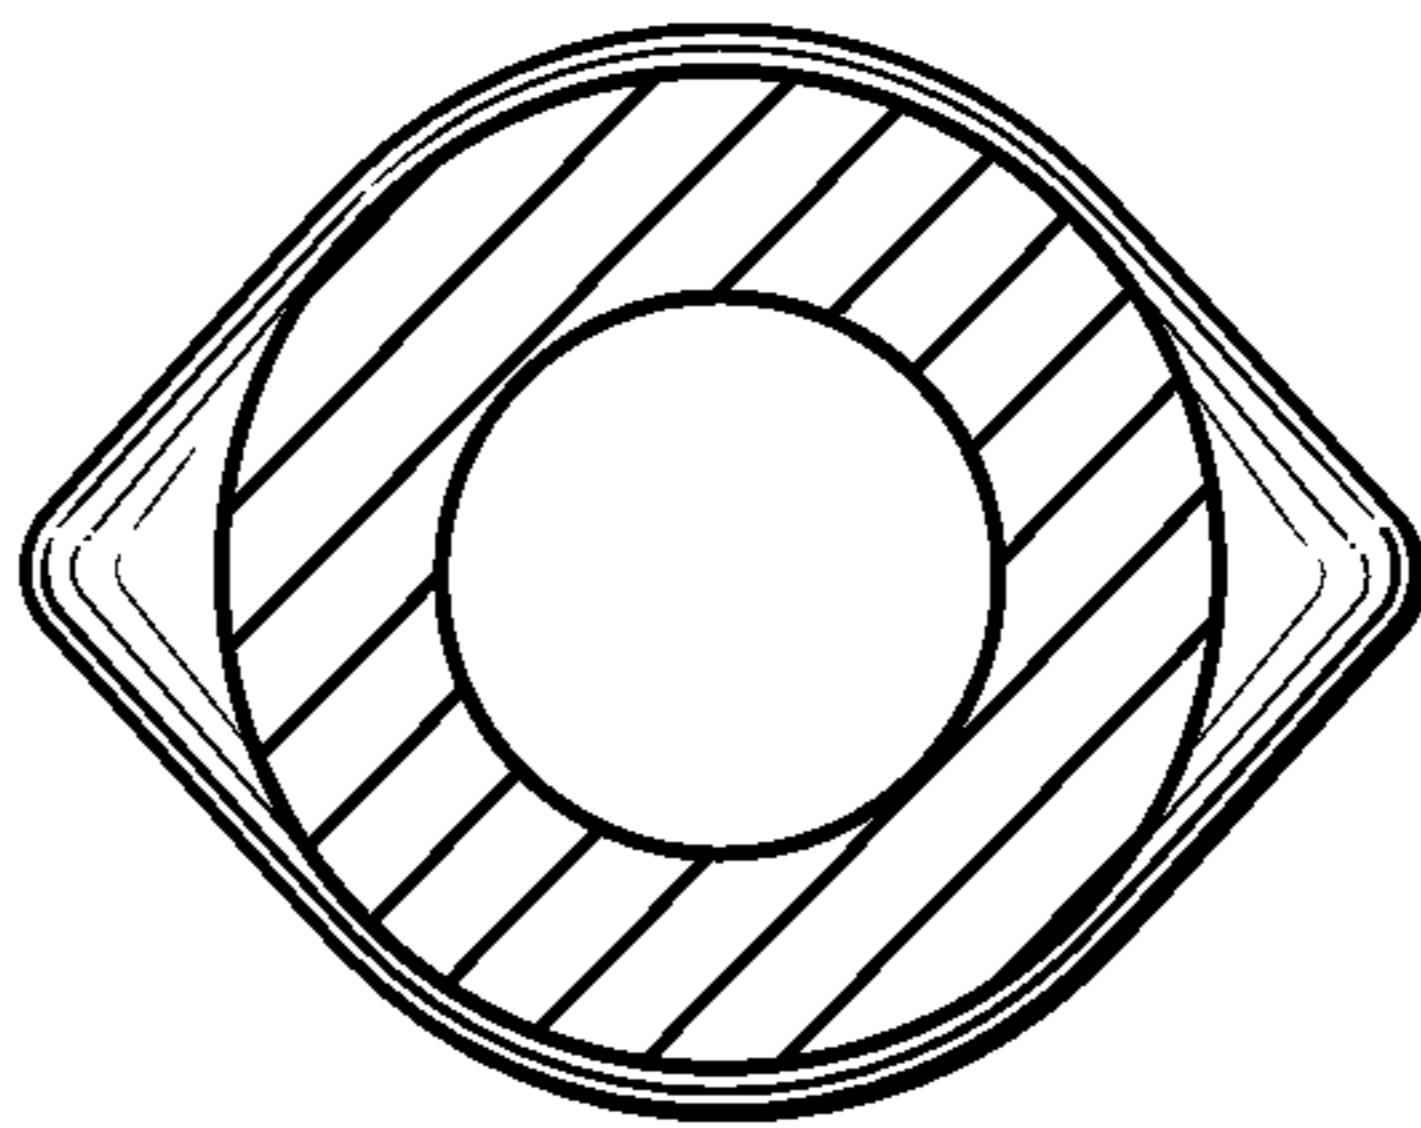


FIG. 5