



US00D573496S

(12) **United States Design Patent**  
**Wakamatsu et al.**

(10) **Patent No.:** **US D573,496 S**  
(45) **Date of Patent:** **\*\* Jul. 22, 2008**

(54) **MEASURING DEVICE FOR BIO-SENSOR**  
(75) Inventors: **Shunichi Wakamatsu**, Saitama (JP);  
**Hiroyuki Kukita**, Saitama (JP);  
**Takayuki Isikawa**, Saitama (JP); **Masao Yamaguchi**, Saitama (JP)

(73) Assignee: **Nihon Dempa Kogyo Co., Ltd.**, Tokyo (JP)

(\*\*) Term: **14 Years**

(21) Appl. No.: **29/291,359**

(22) Filed: **Aug. 24, 2007**

(30) **Foreign Application Priority Data**  
Apr. 25, 2007 (JP) ..... 2007-011092

(51) **LOC (8) Cl.** ..... **10-04**

(52) **U.S. Cl.** ..... **D10/81**

(58) **Field of Classification Search** ..... D10/81;  
D24/186, 232, 233, 234; 73/864.01, 864.12;  
134/21, 22.11, 24, 26-27, 139 R; 422/62-64,  
422/100; 436/47, 49, 179, 180

See application file for complete search history.

(56) **References Cited**  
U.S. PATENT DOCUMENTS  
D296,823 S \* 7/1988 Kuwa et al. .... D10/81  
\* cited by examiner  
*Primary Examiner*—Antoine D Davis  
(74) *Attorney, Agent, or Firm*—Scott D. Wofsy; Edwards Angell Palmer & Dodge LLP

(57) **CLAIM**  
The ornamental design for a measuring device for bio-sensor, as shown and described.

**DESCRIPTION**  
FIG. 1 is a front view of a measuring device for bio-sensor of a new design;  
FIG. 2 is a back view thereof;  
FIG. 3 is a left side view thereof;  
FIG. 4 is a right side view thereof;  
FIG. 5 is a plan view thereof; and,  
FIG. 6 is a bottom plan view thereof.

**1 Claim, 3 Drawing Sheets**

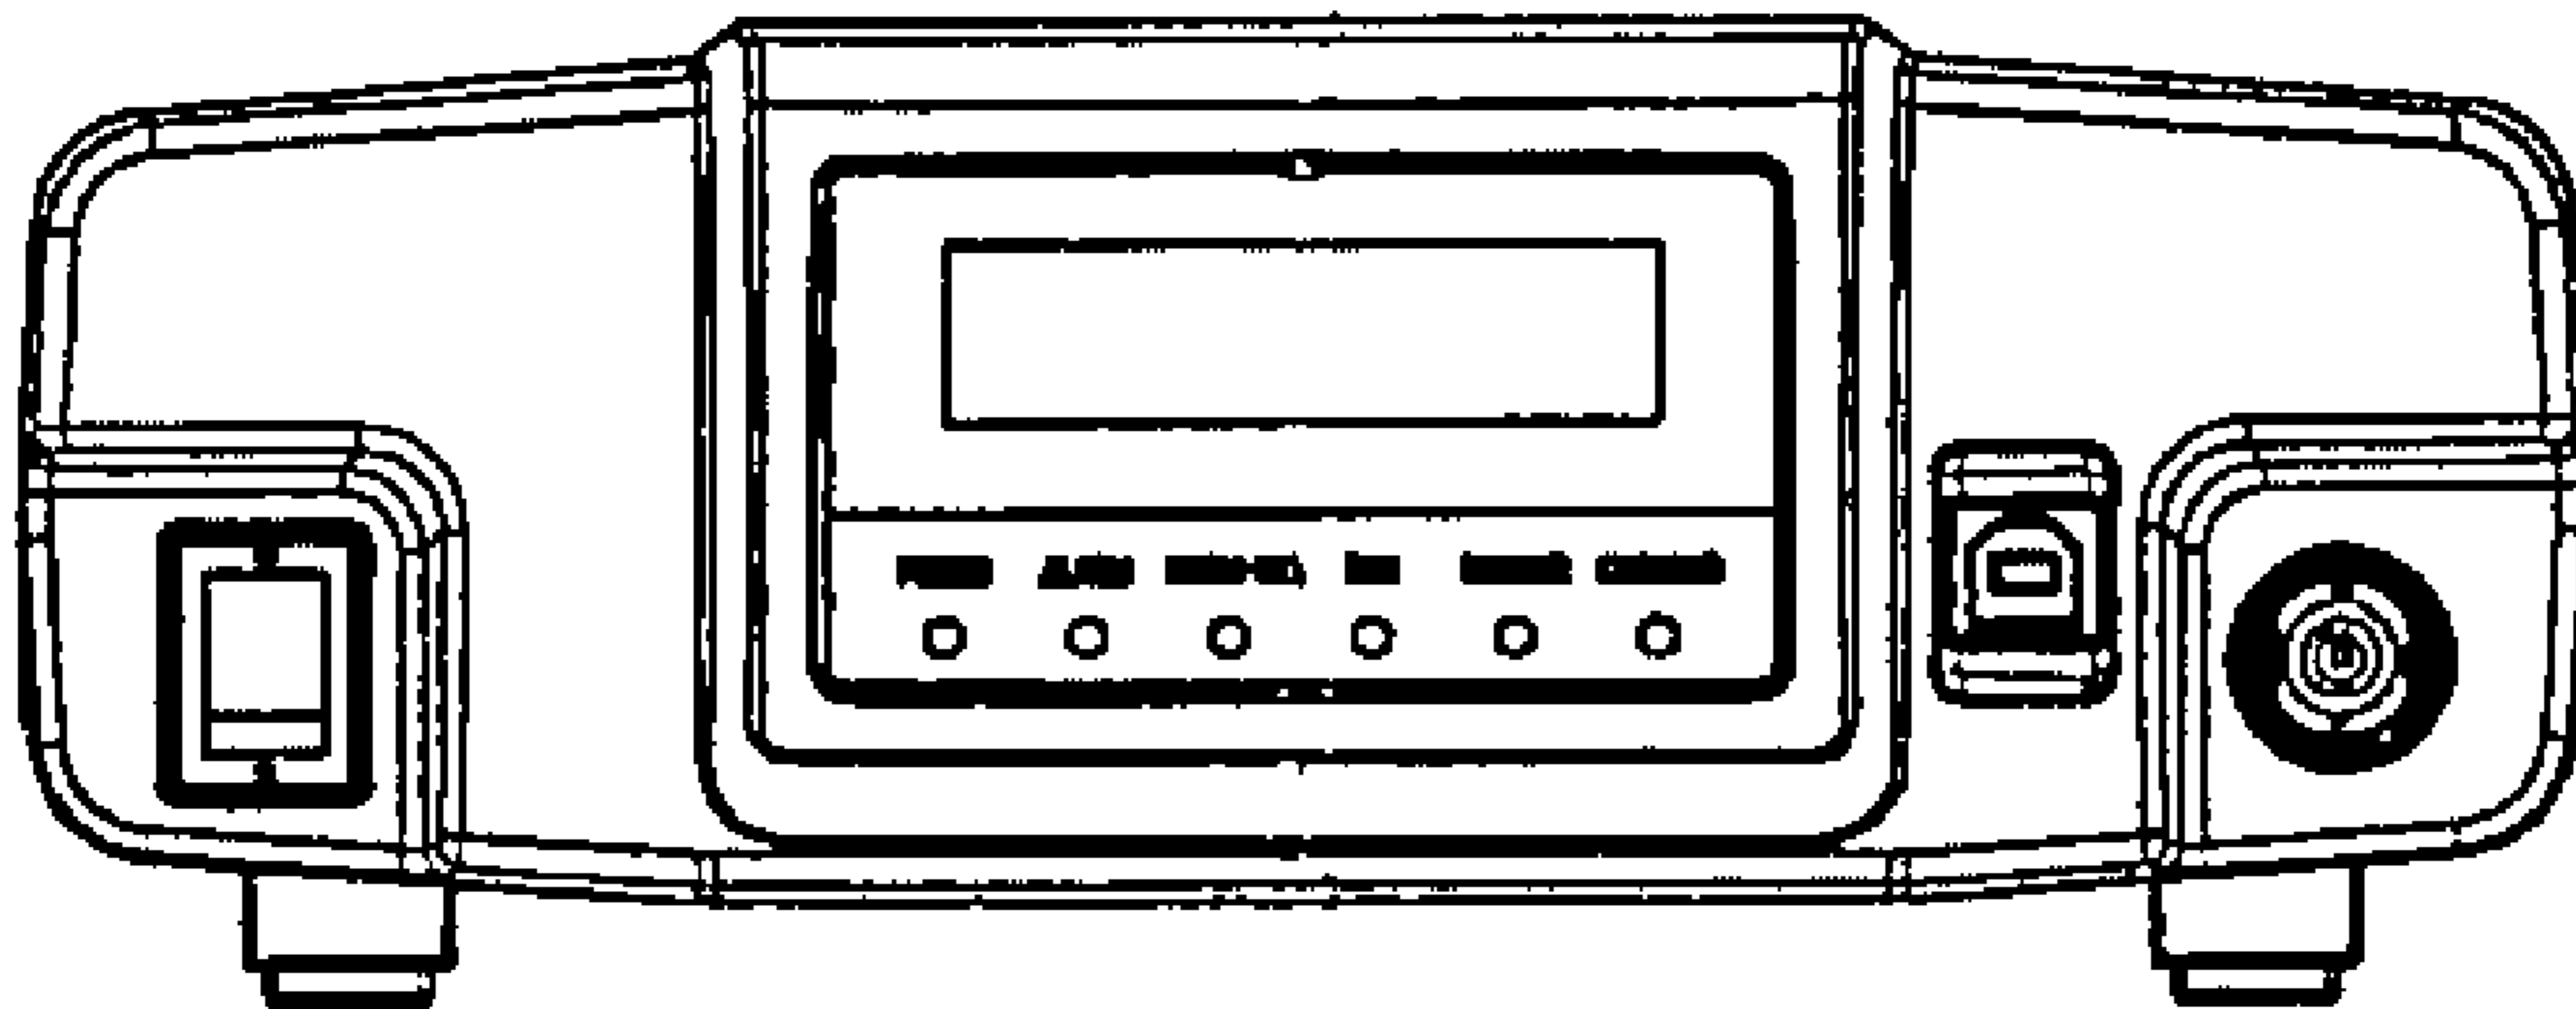


FIG. 1

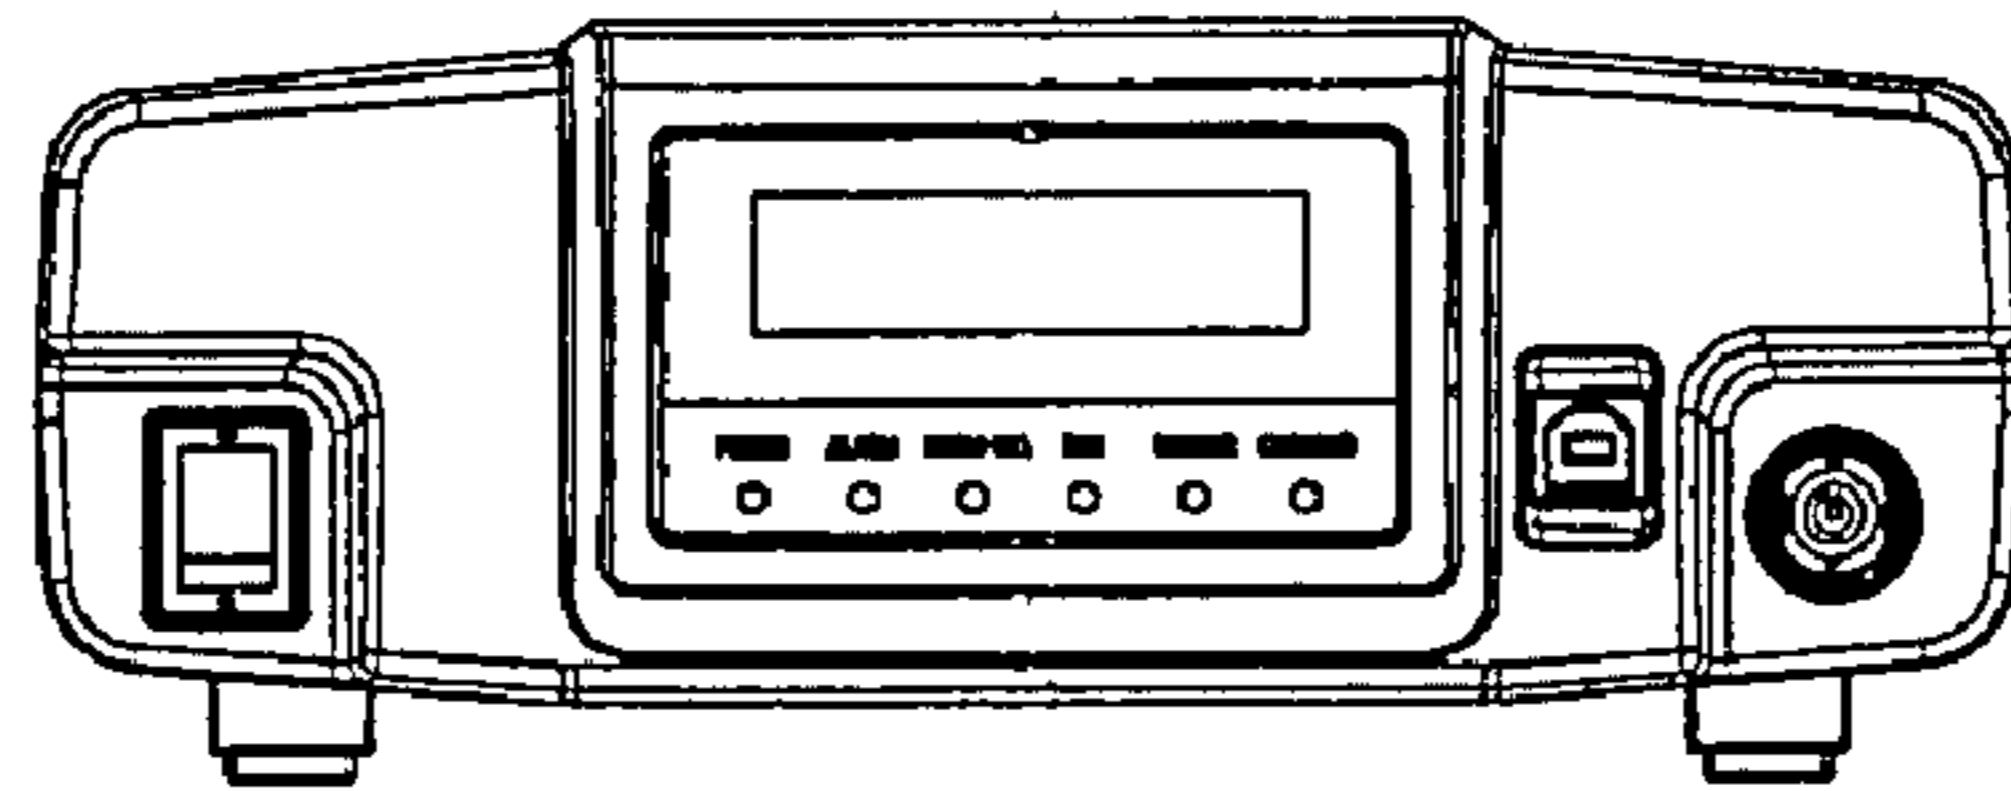


FIG. 2



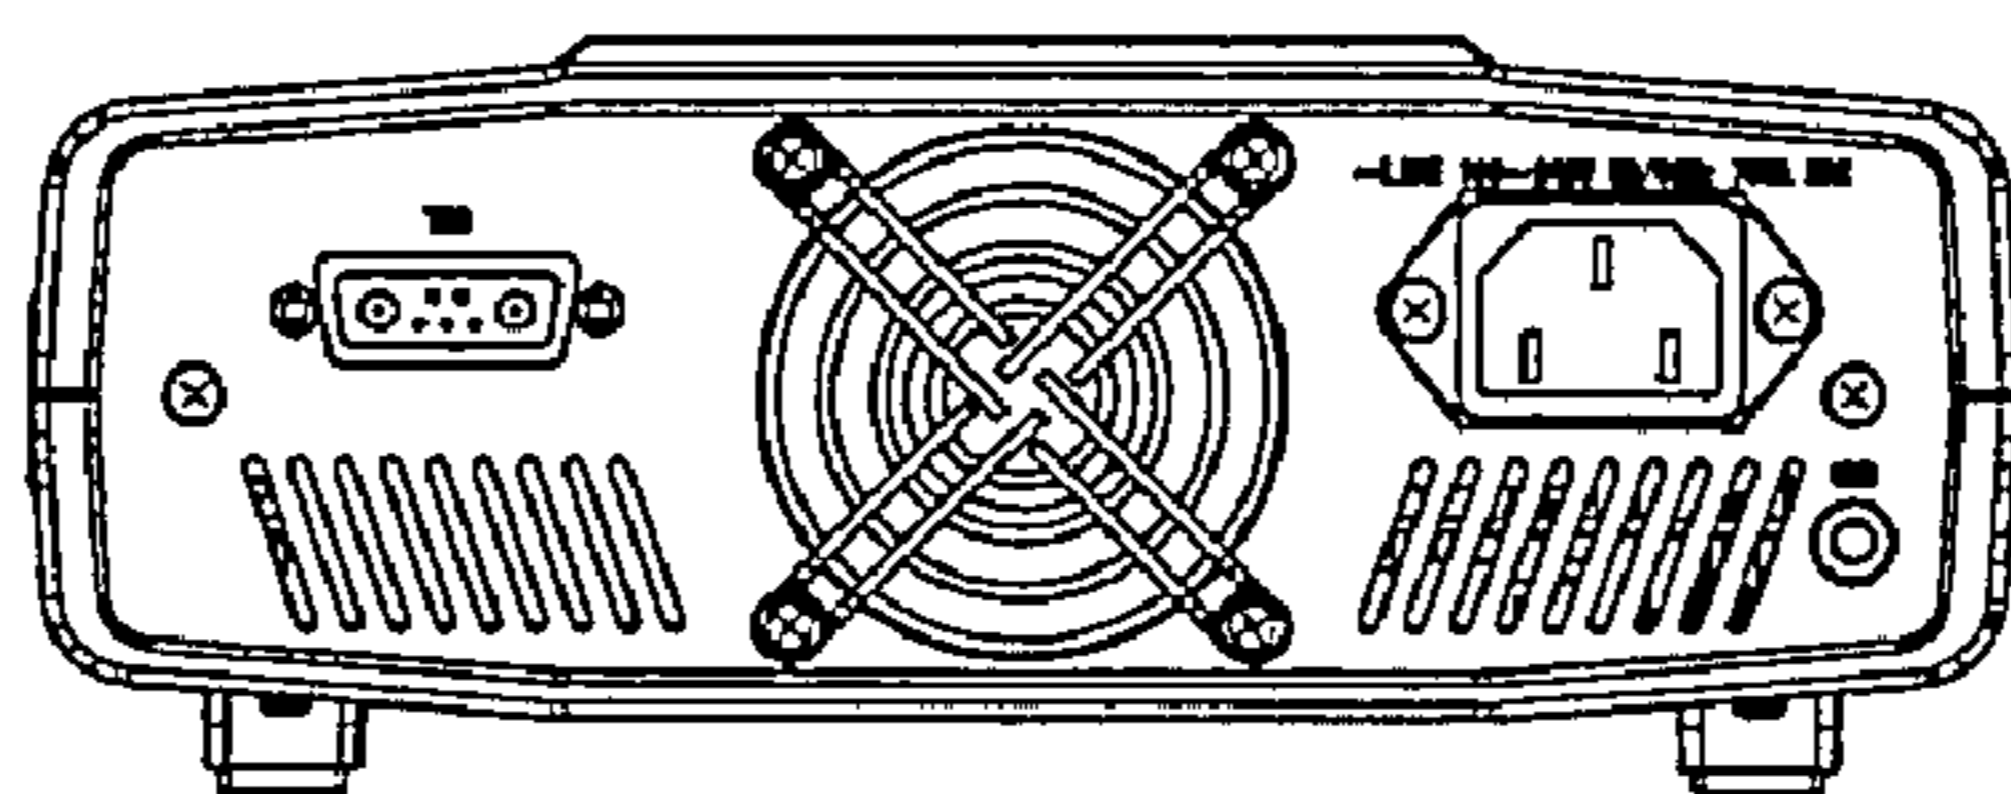



FIG. 3

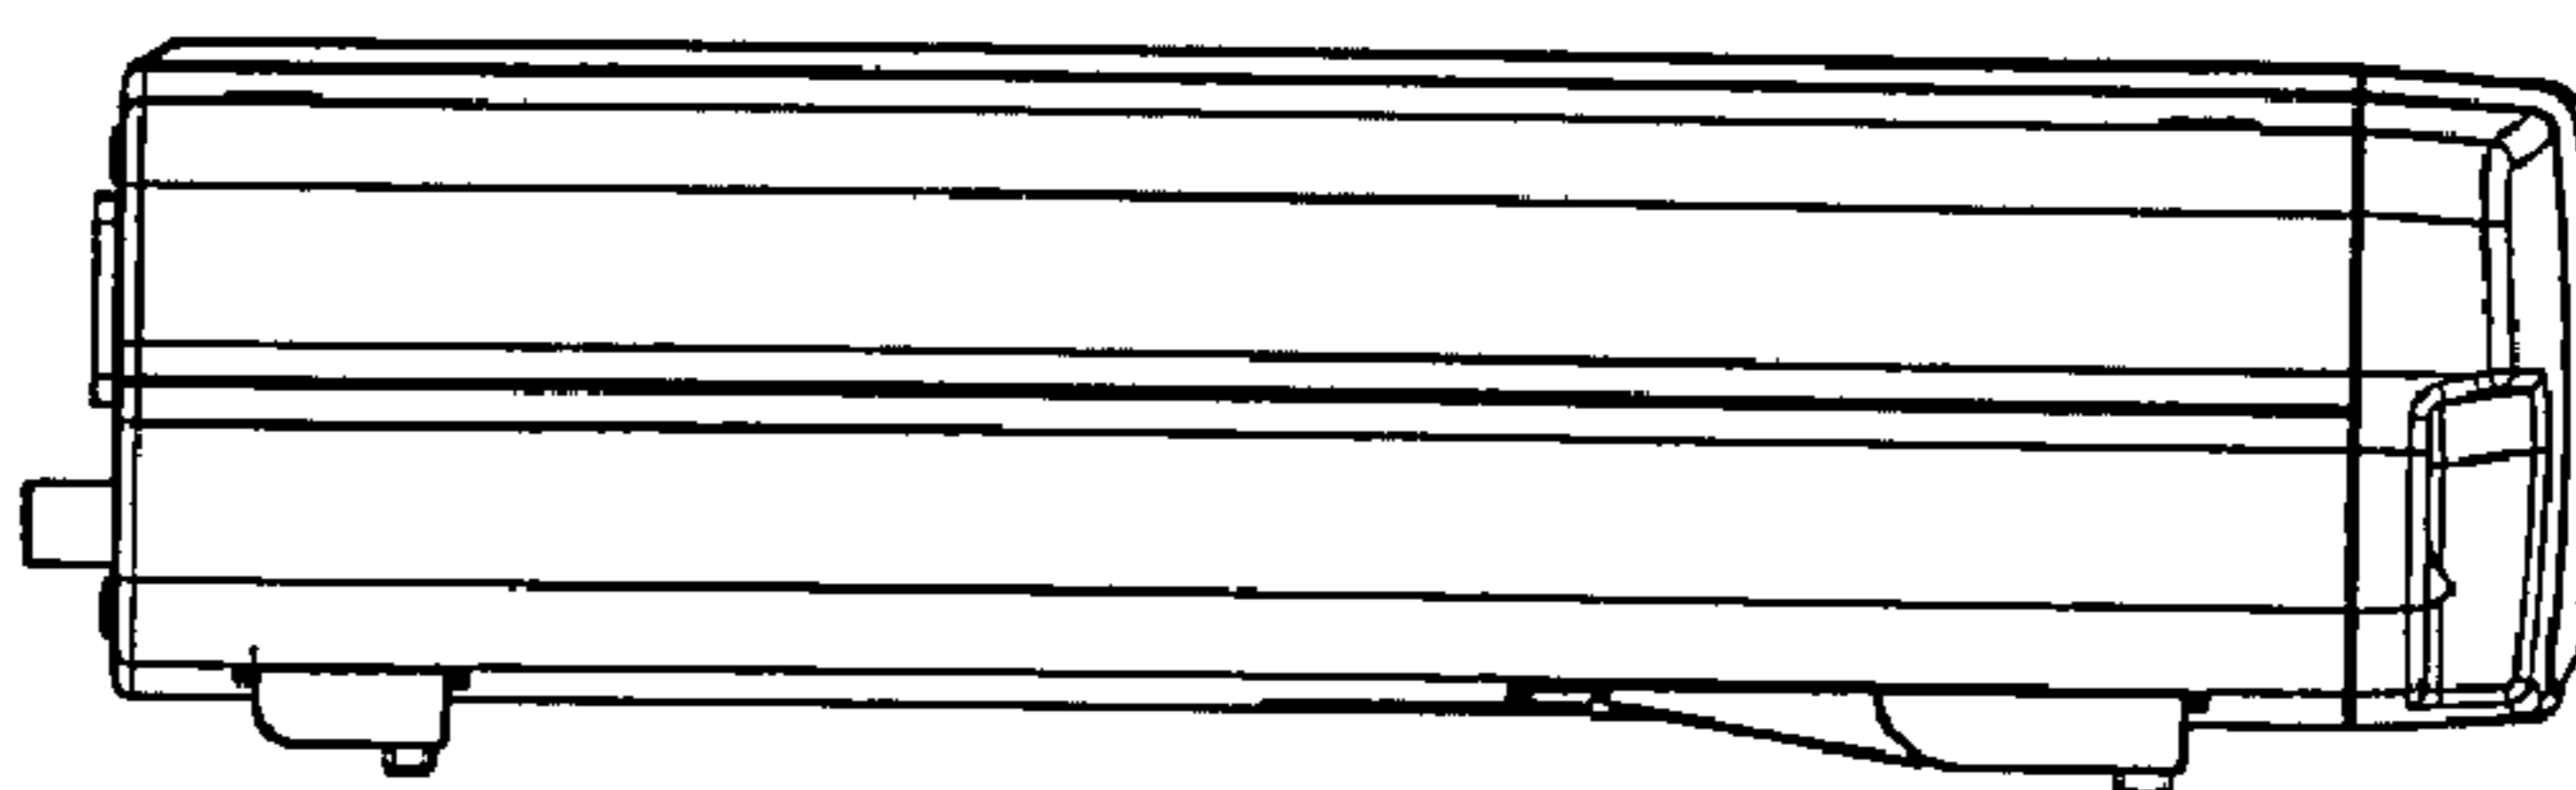

**FIG. 4**

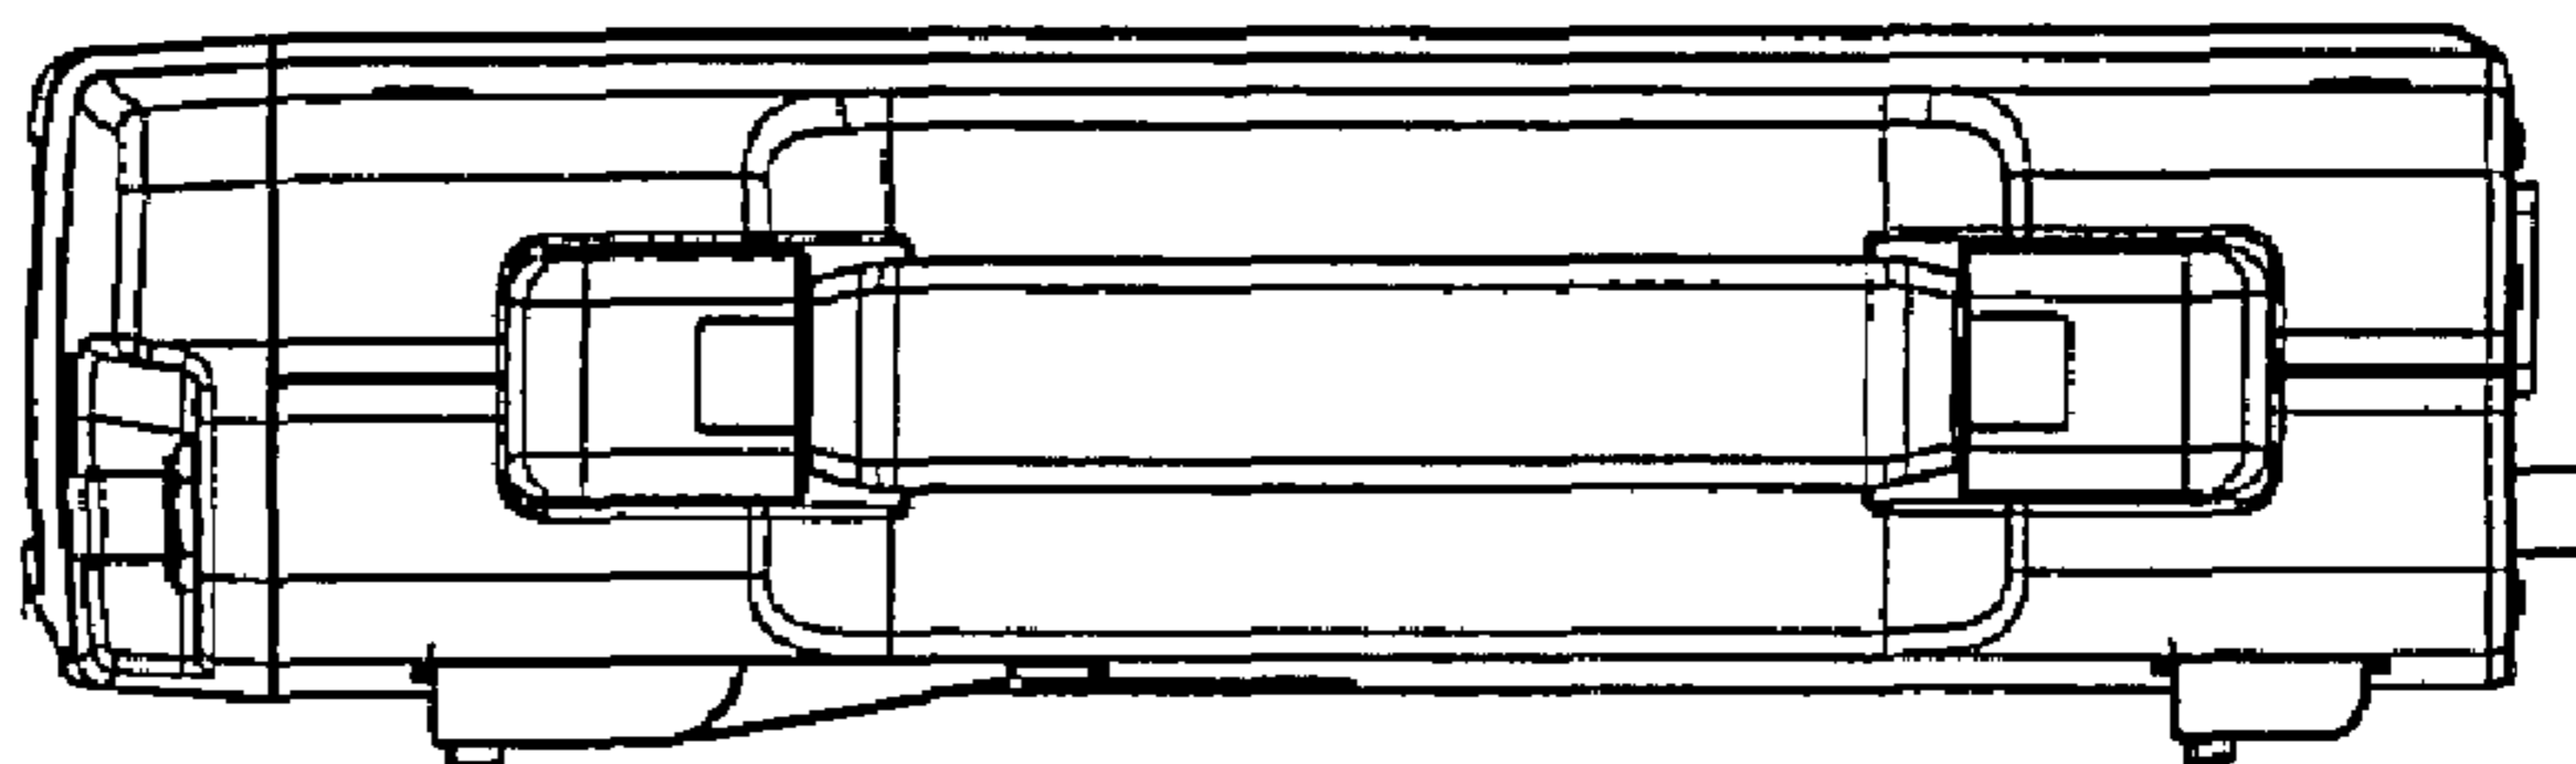

**FIG. 5**

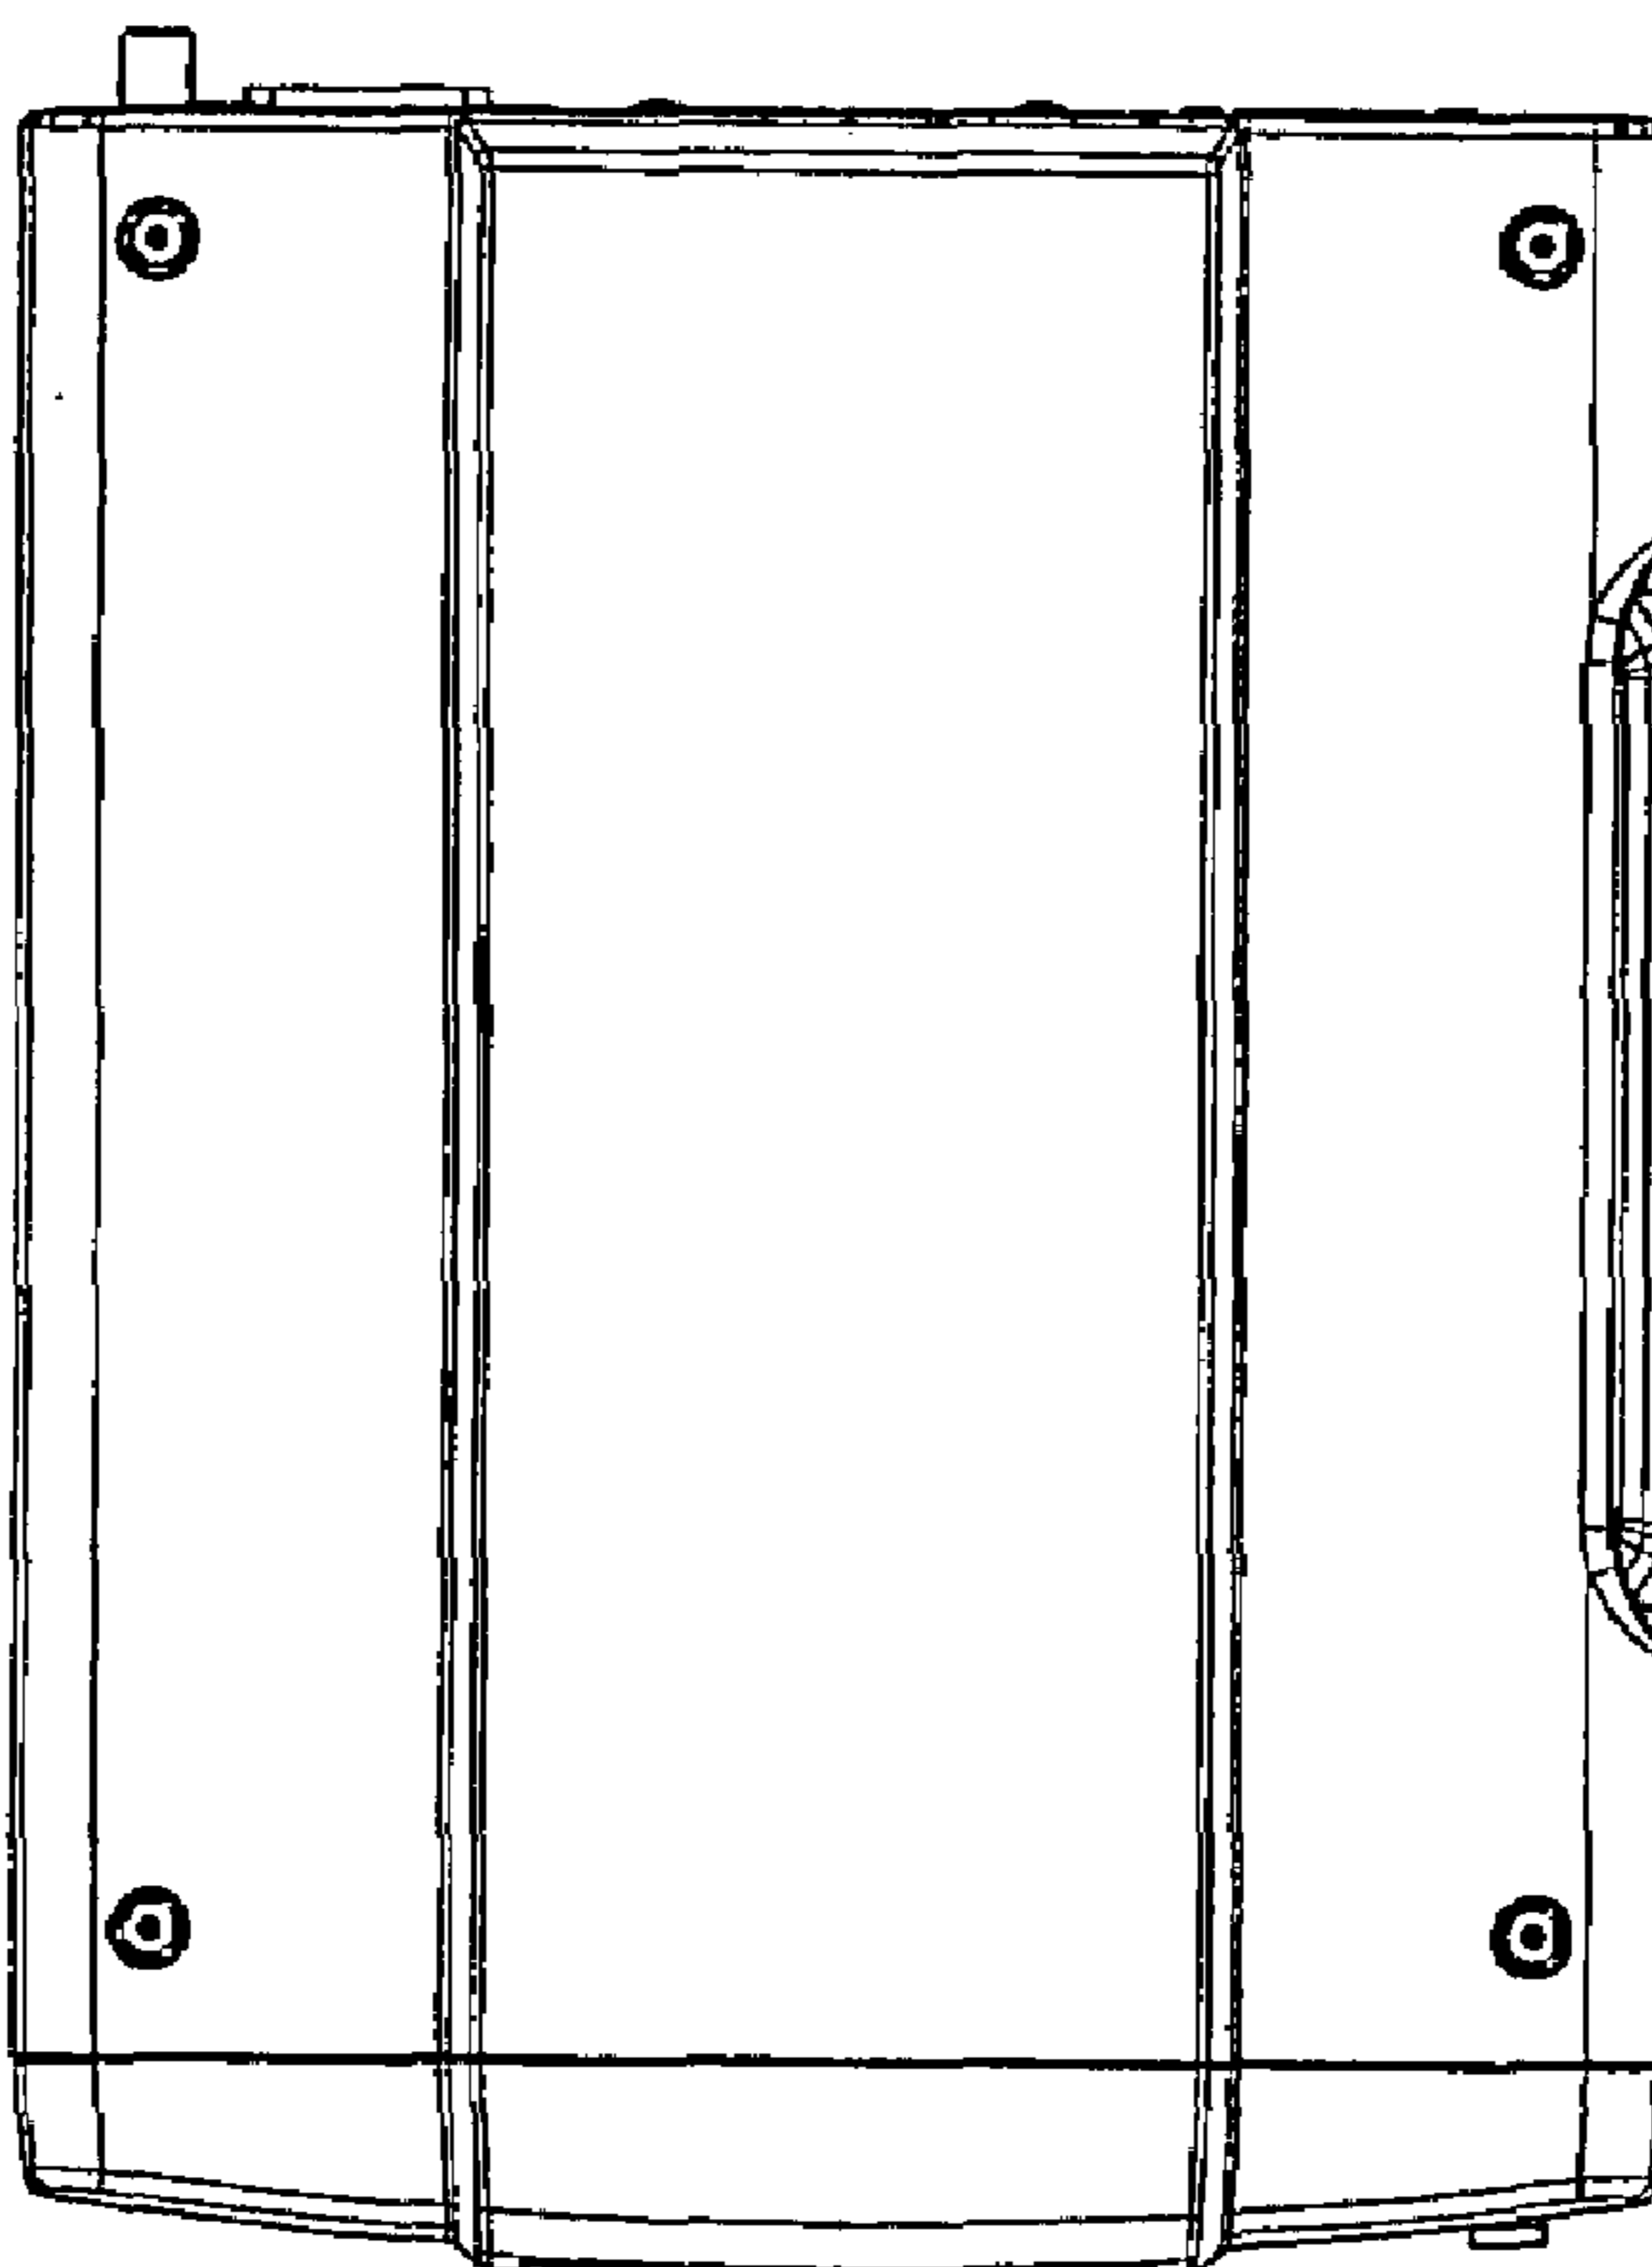

**FIG. 6**

