



US00D578535S

(12) **United States Design Patent**
Schmitz

(10) **Patent No.:** **US D578,535 S**
(45) **Date of Patent:** **** Oct. 14, 2008**

(54) **SCANNER**

(75) Inventor: **Rainer Schmitz**, Steinfurt (DE)

(73) Assignee: **3M Innovative Properties Company**,
St. Paul, MN (US)

(**) Term: **14 Years**

(21) Appl. No.: **29/278,394**

(22) Filed: **Mar. 28, 2007**

(51) **LOC (8) Cl.** **14-02**

(52) **U.S. Cl.** **D14/421**

(58) **Field of Classification Search** D14/420-424,
D14/383-386, 341, 129, 336, 409, 374; D18/4.1,
D18/4.4-4.6; D21/329; D26/371, 45, 50;
235/375, 378, 385, 454, 462.02, 486, 380,
235/382, 382.5; 382/312-315, 318-321;
250/203.1, 216; 399/7, 211; 358/497, 473,
358/474, 471, 494

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D229,781 S *	1/1974	Laughon	D16/225
D255,455 S *	6/1980	Gensike et al.	D16/225
D280,103 S *	8/1985	Bonnefoy	D16/225
D303,376 S *	9/1989	Nishida	D14/385
D310,359 S *	9/1990	Inukai	D14/374
D323,894 S *	2/1992	Rosati et al.	D24/186
D325,196 S *	4/1992	Stanger et al.	D14/384
D348,260 S *	6/1994	Allgeier	D14/430
D386,489 S *	11/1997	Goldman et al.	D14/420
D420,657 S *	2/2000	Keen et al.	D14/428
D447,140 S *	8/2001	Mittler	D14/383
D454,879 S *	3/2002	Lin et al.	D14/420
D464,969 S *	10/2002	Byun et al.	D14/420
D480,397 S *	10/2003	Forsythe et al.	D14/383
6,788,285 B2 *	9/2004	Paolucci et al.	345/156

OTHER PUBLICATIONS

Product Photo: "Speedscan 5AX," BEGO, Germany, Launch date 2006, pp. 1.

Product Photo: "Pro50," Cynovad, Canada, Launch date 2000, pp. 1.

Product Photo: "Preciscan," DCS/Bien Air, Launch date 1999, pp. 1.

Product Photo: "Cercon Eye," Degudent, Germany, Launch date 2006, pp. 1.

Product Photo: "ED1," Etkon/Straumann, Germany, Launch date 2001, pp. 1.

Product Photo: "hiScanu," Hint-Els, Germany, Launch date 2005, pp. 1.

Product Photo: "Everest (BaseCamp) scan (eco)," KaVo Dental GmbH, Bismarckring 39, 88400 Biberach, Germany, Launch date 2002, pp. 1.

Product Photo: "Everest Scan Pro," KaVo Dental GmbH, Bismarckring 39, 88400 Biberach, Germany, Launch date 2002, pp. 1.

Product Photo: "TopDent TMS-220," Polytec GmbH, Polytec Platz 1-7, 76337 Waldbronn, Germany, Launch date 2005, pp. 1.

Product Photo: "inEOS," Sirona Dental Systems, Fabrikstr. 31 64625 Bensheim, Germany, Launch date 2005, pp. 1.

(Continued)

Primary Examiner—Melanie Tung

Assistant Examiner—Susan Moon Lee

(74) *Attorney, Agent, or Firm*—Sean J. Edman

(57) **CLAIM**

The ornamental design for a scanner, as shown and described.

DESCRIPTION

FIG. 1 is a perspective view of a scanner showing the new design;

FIG. 2 is a front view thereof;

FIG. 3 is a side view thereof;

FIG. 4 is a rear view thereof;


FIG. 5 is a side view thereof;

FIG. 6 is a top view thereof; and,

FIG. 7 is a bottom view thereof.

The portions shown in broken line are for illustrative purposes only and form no part of the claimed design.

1 Claim, 3 Drawing Sheets

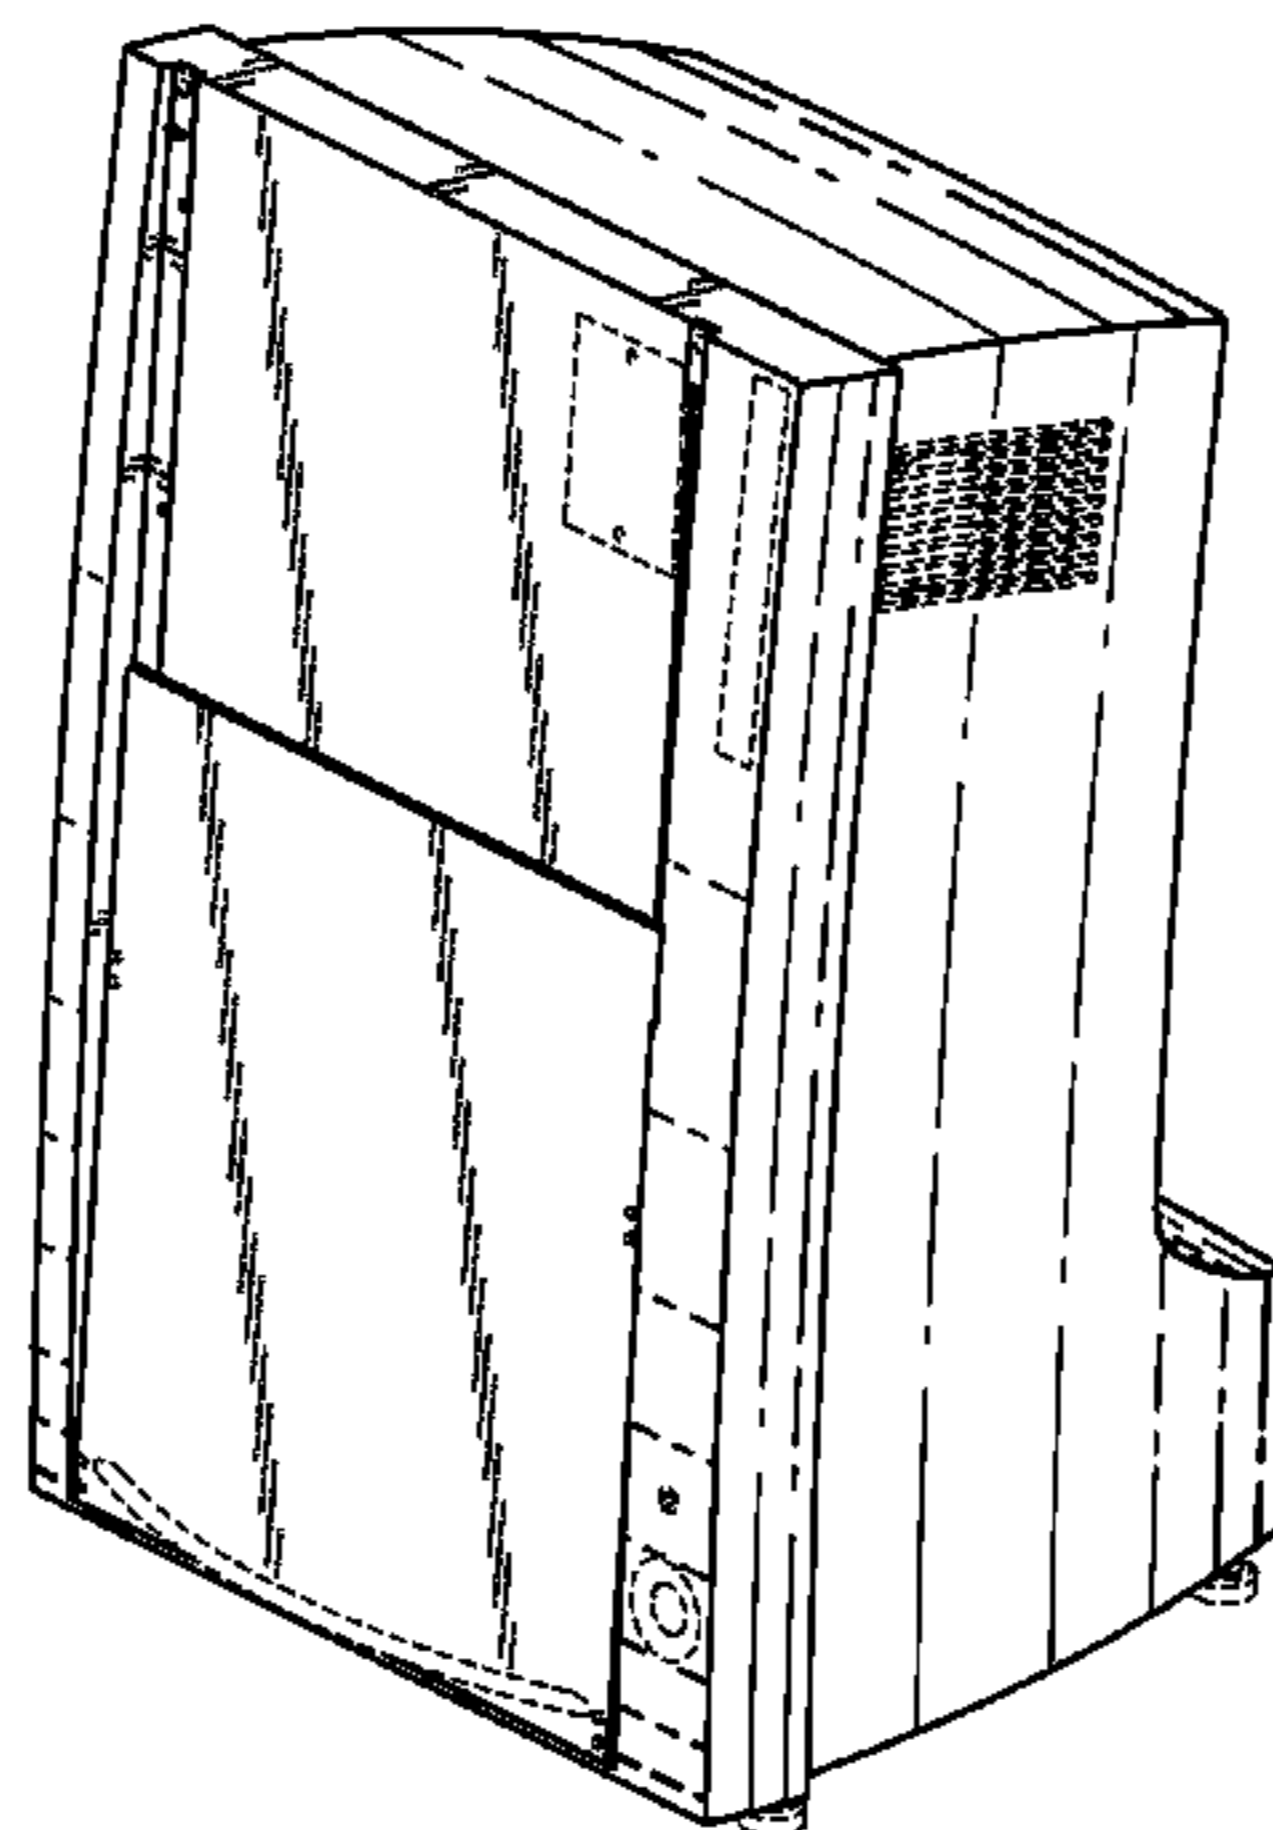

OTHER PUBLICATIONS

Product Photo: "Activity 101," Smart optics Sensortechnik GmbH, Sinterstrasse 8a, 44795 Bochum, Germany, Launch date 2006, pp. 1.

Product Photo: "Procera Forte," Nobel Biocare AB, PO Box 5190 SE-402 26 Göteborg Schweden Stolbergerstr. 200, 50933 Köln, Germany, Launch date 2004, pp. 1.

Product Photo: "Procera Piccolo," Nobel Biocare AB, PO Box 5190 SE-402 26 Göteborg Schweden Stolbergerstr. 200, 50933 Köln, Germany, Launch date 2003, pp. 1.

Product Photo: "3shape D250," Wieland Dental + Technik GmbH & Co. KG, Launch 2005, pp. 1.

* cited by examiner

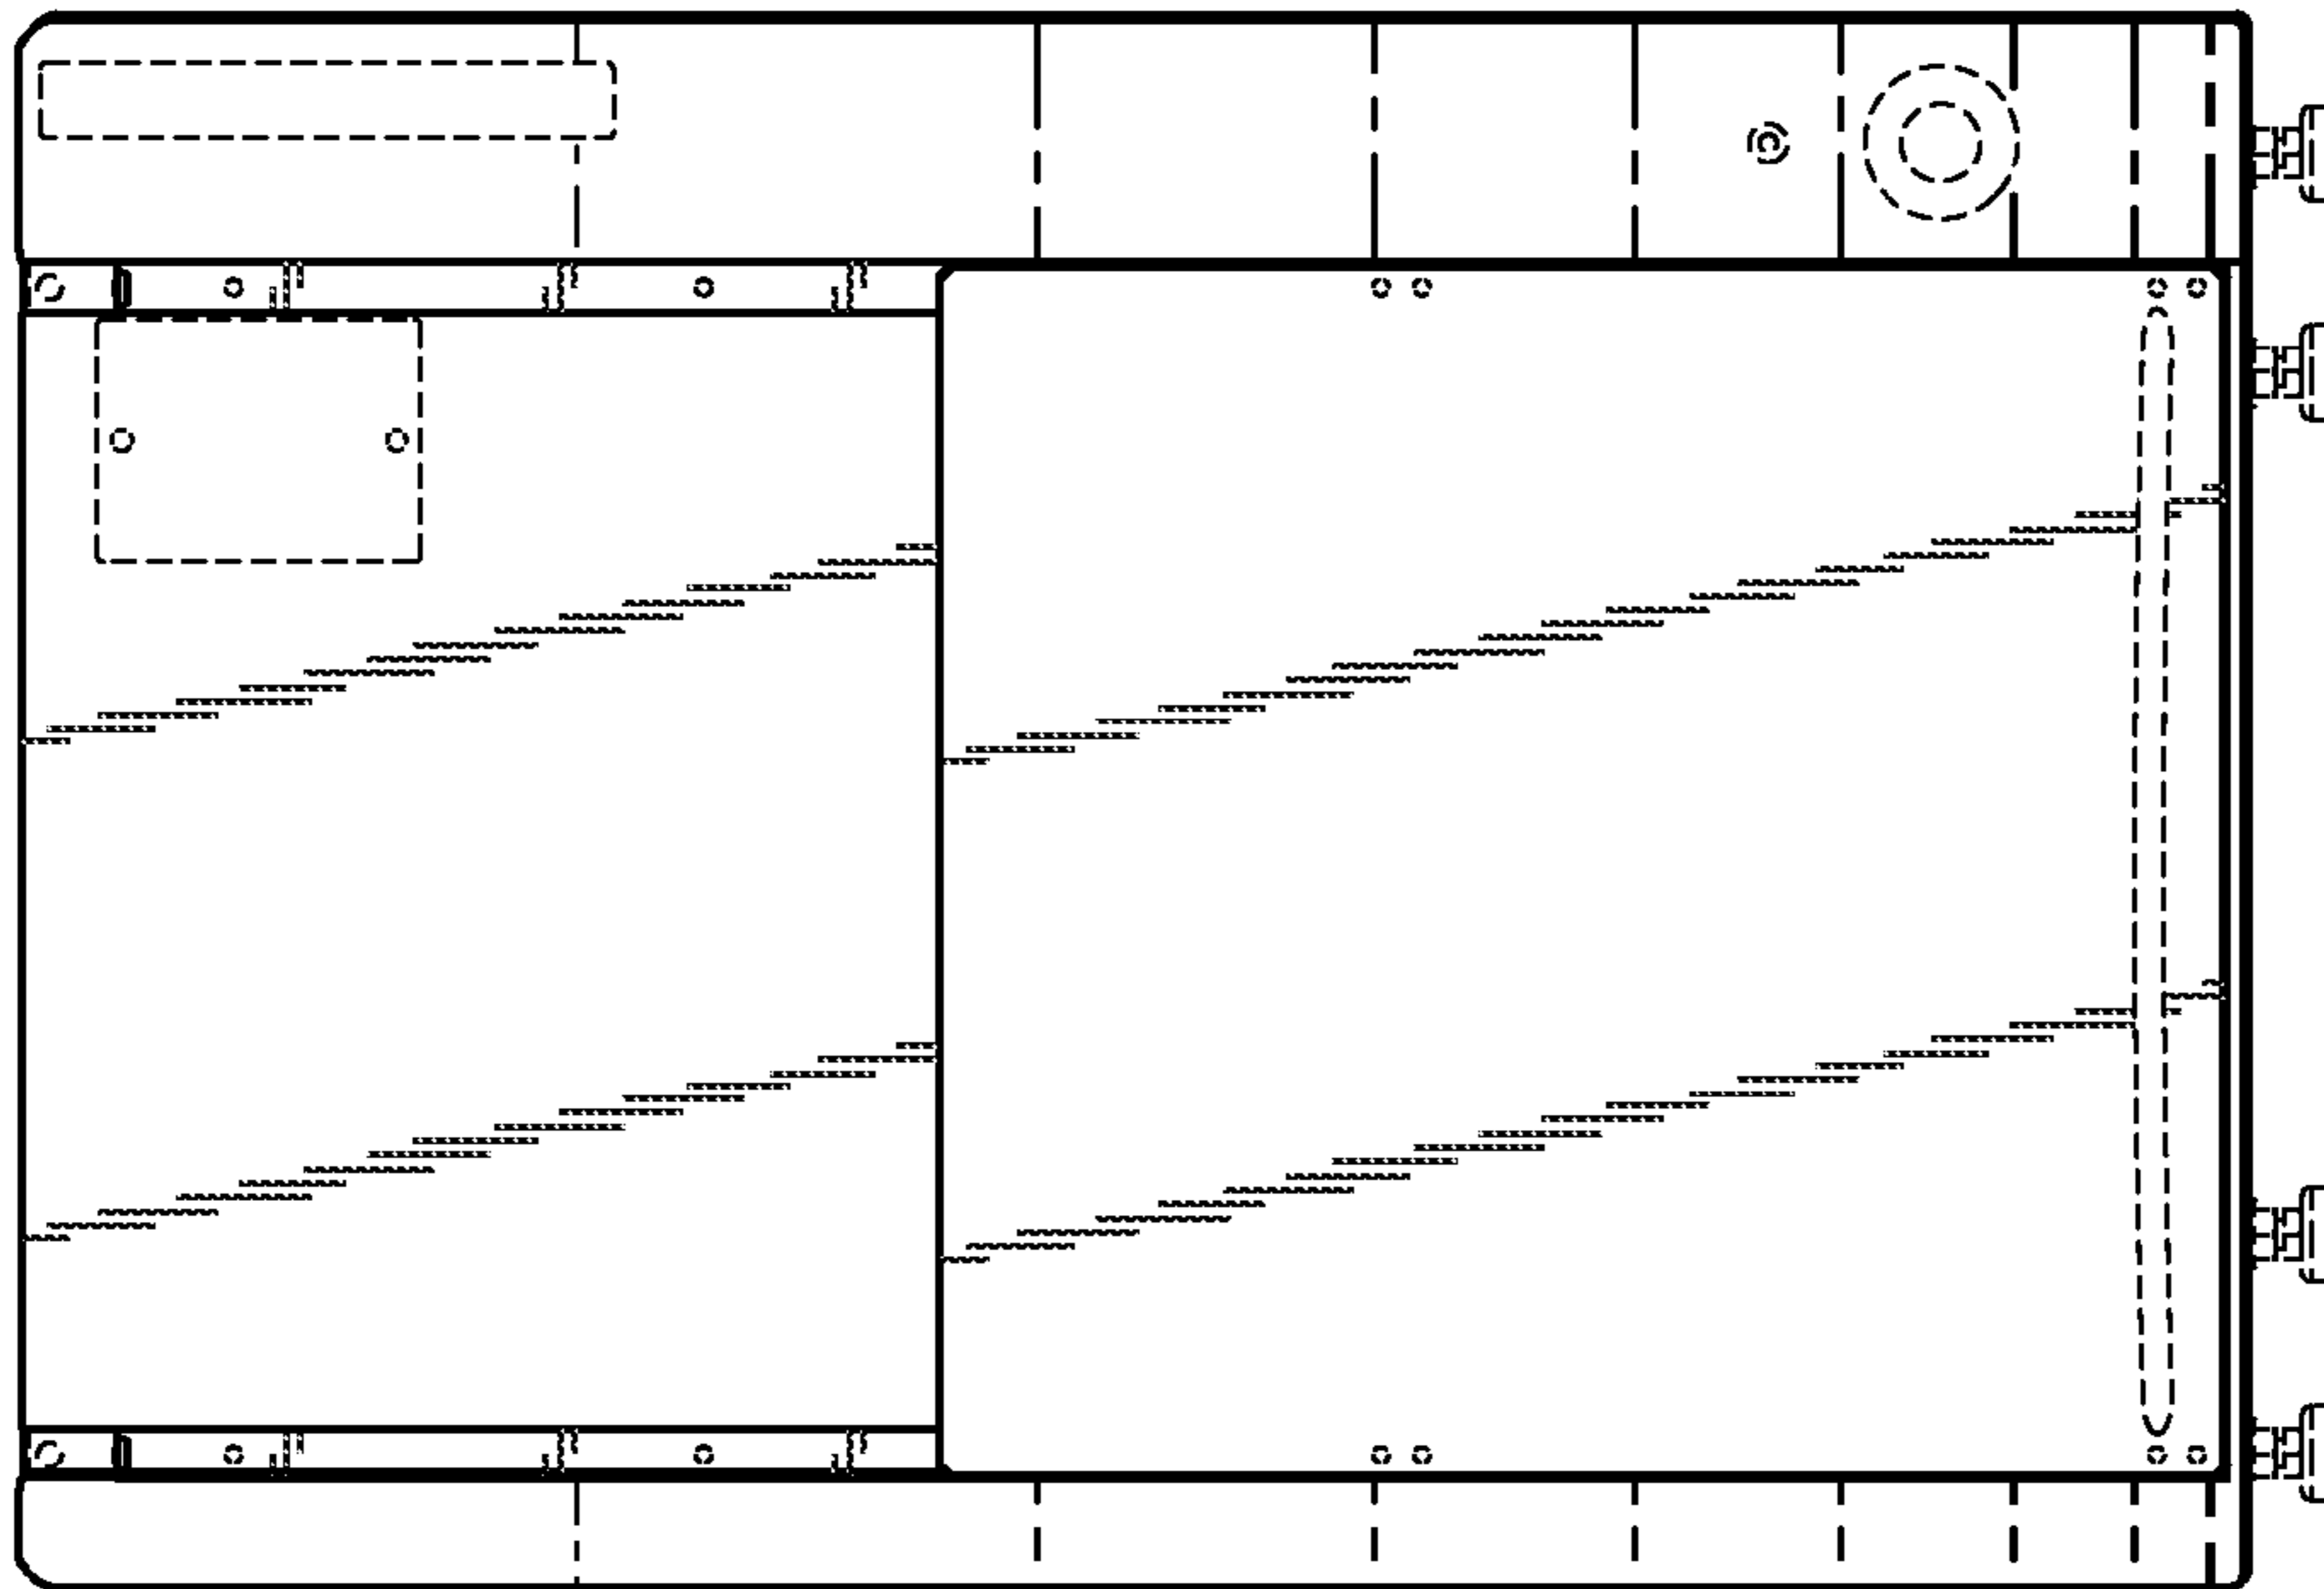


FIG. 2

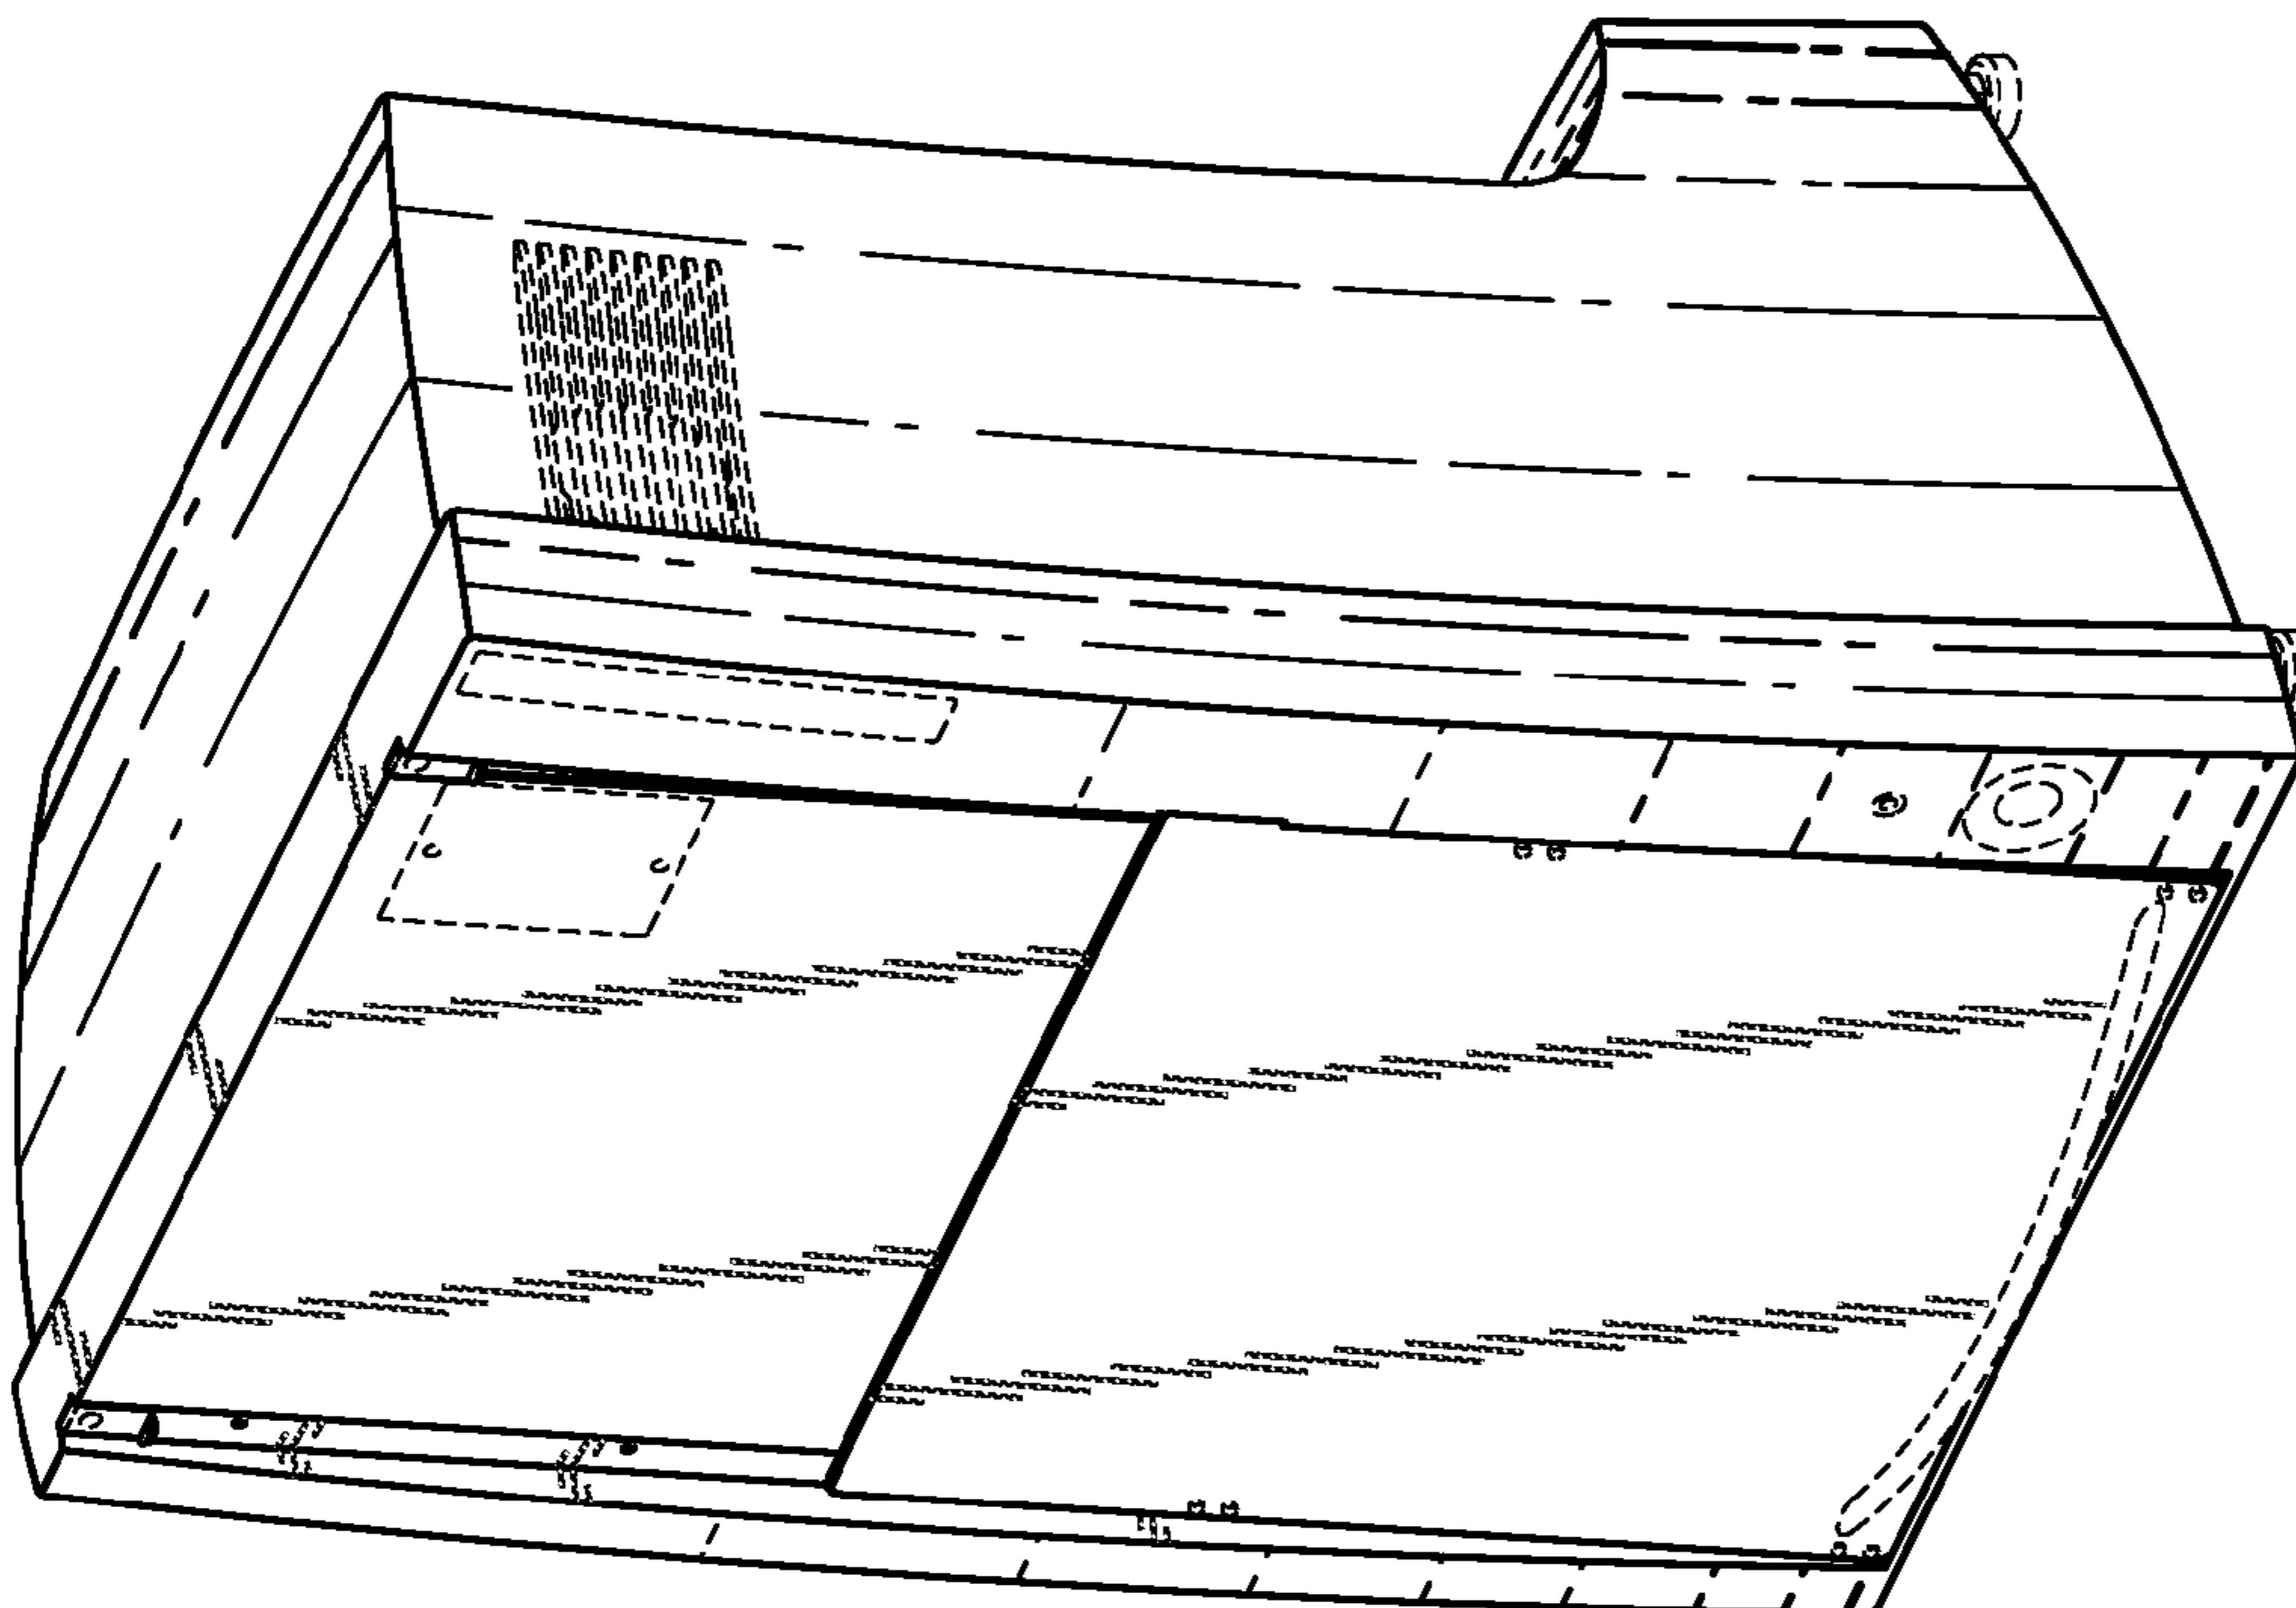


FIG. 1

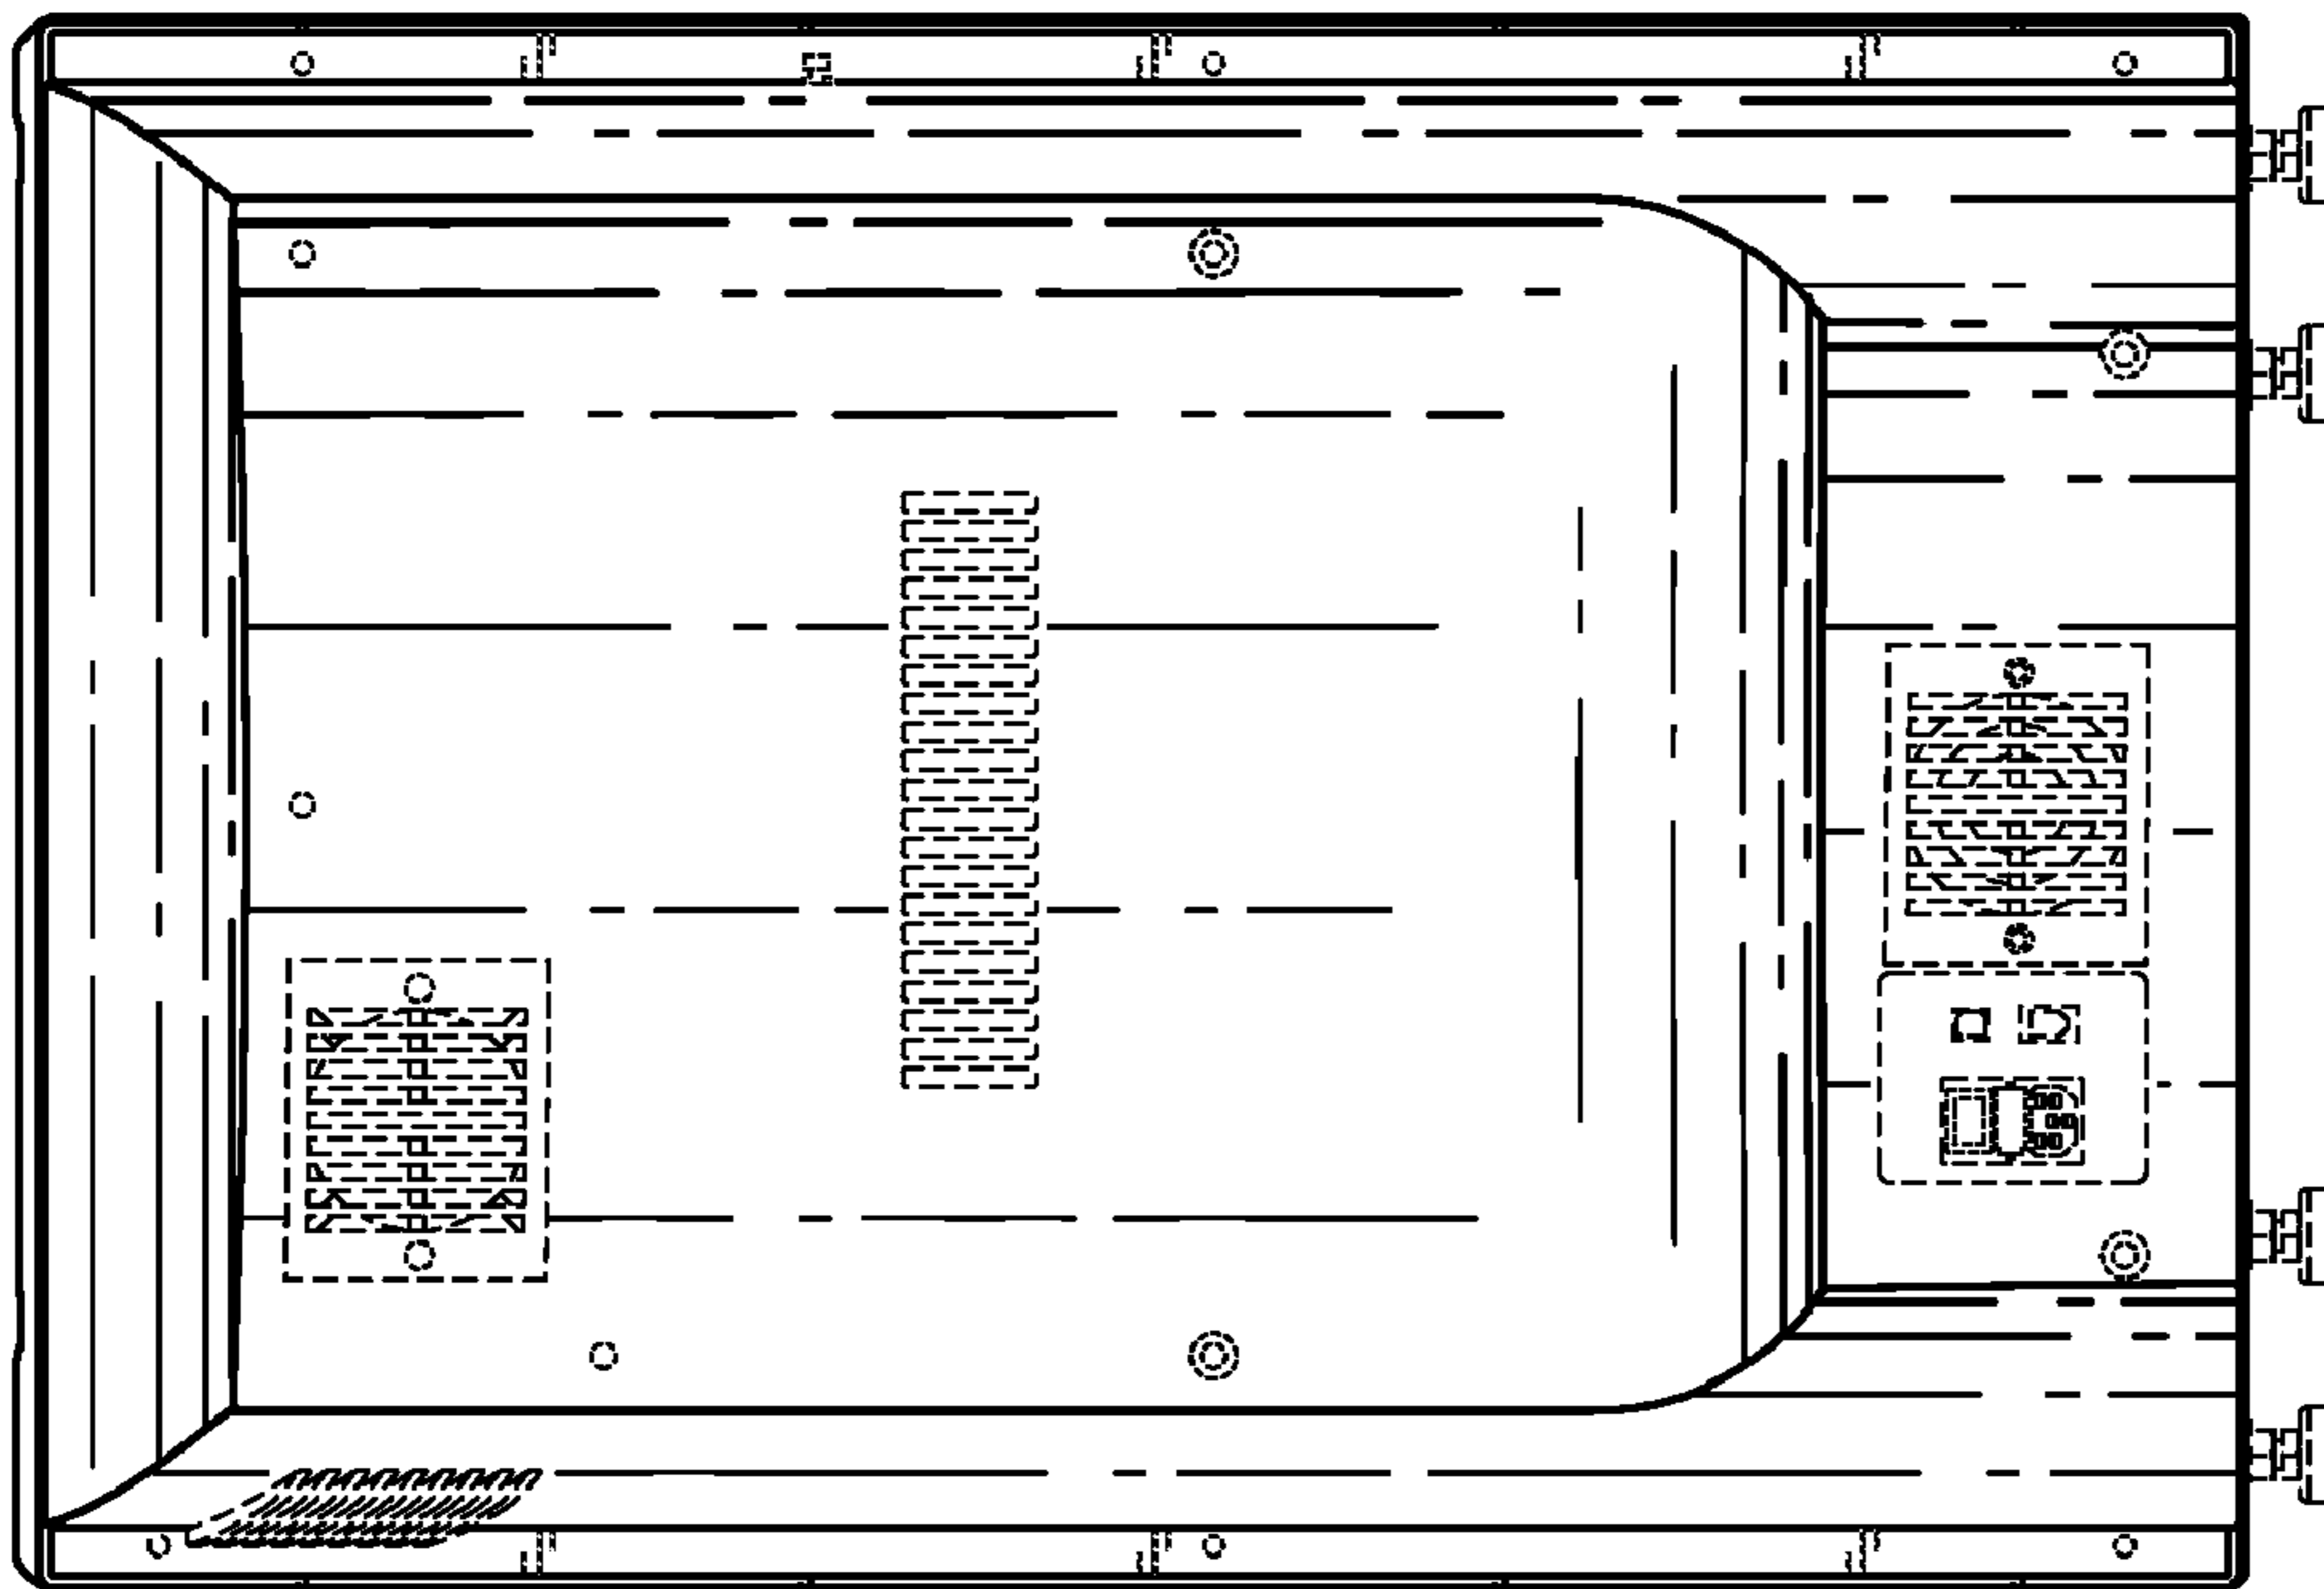


FIG. 4

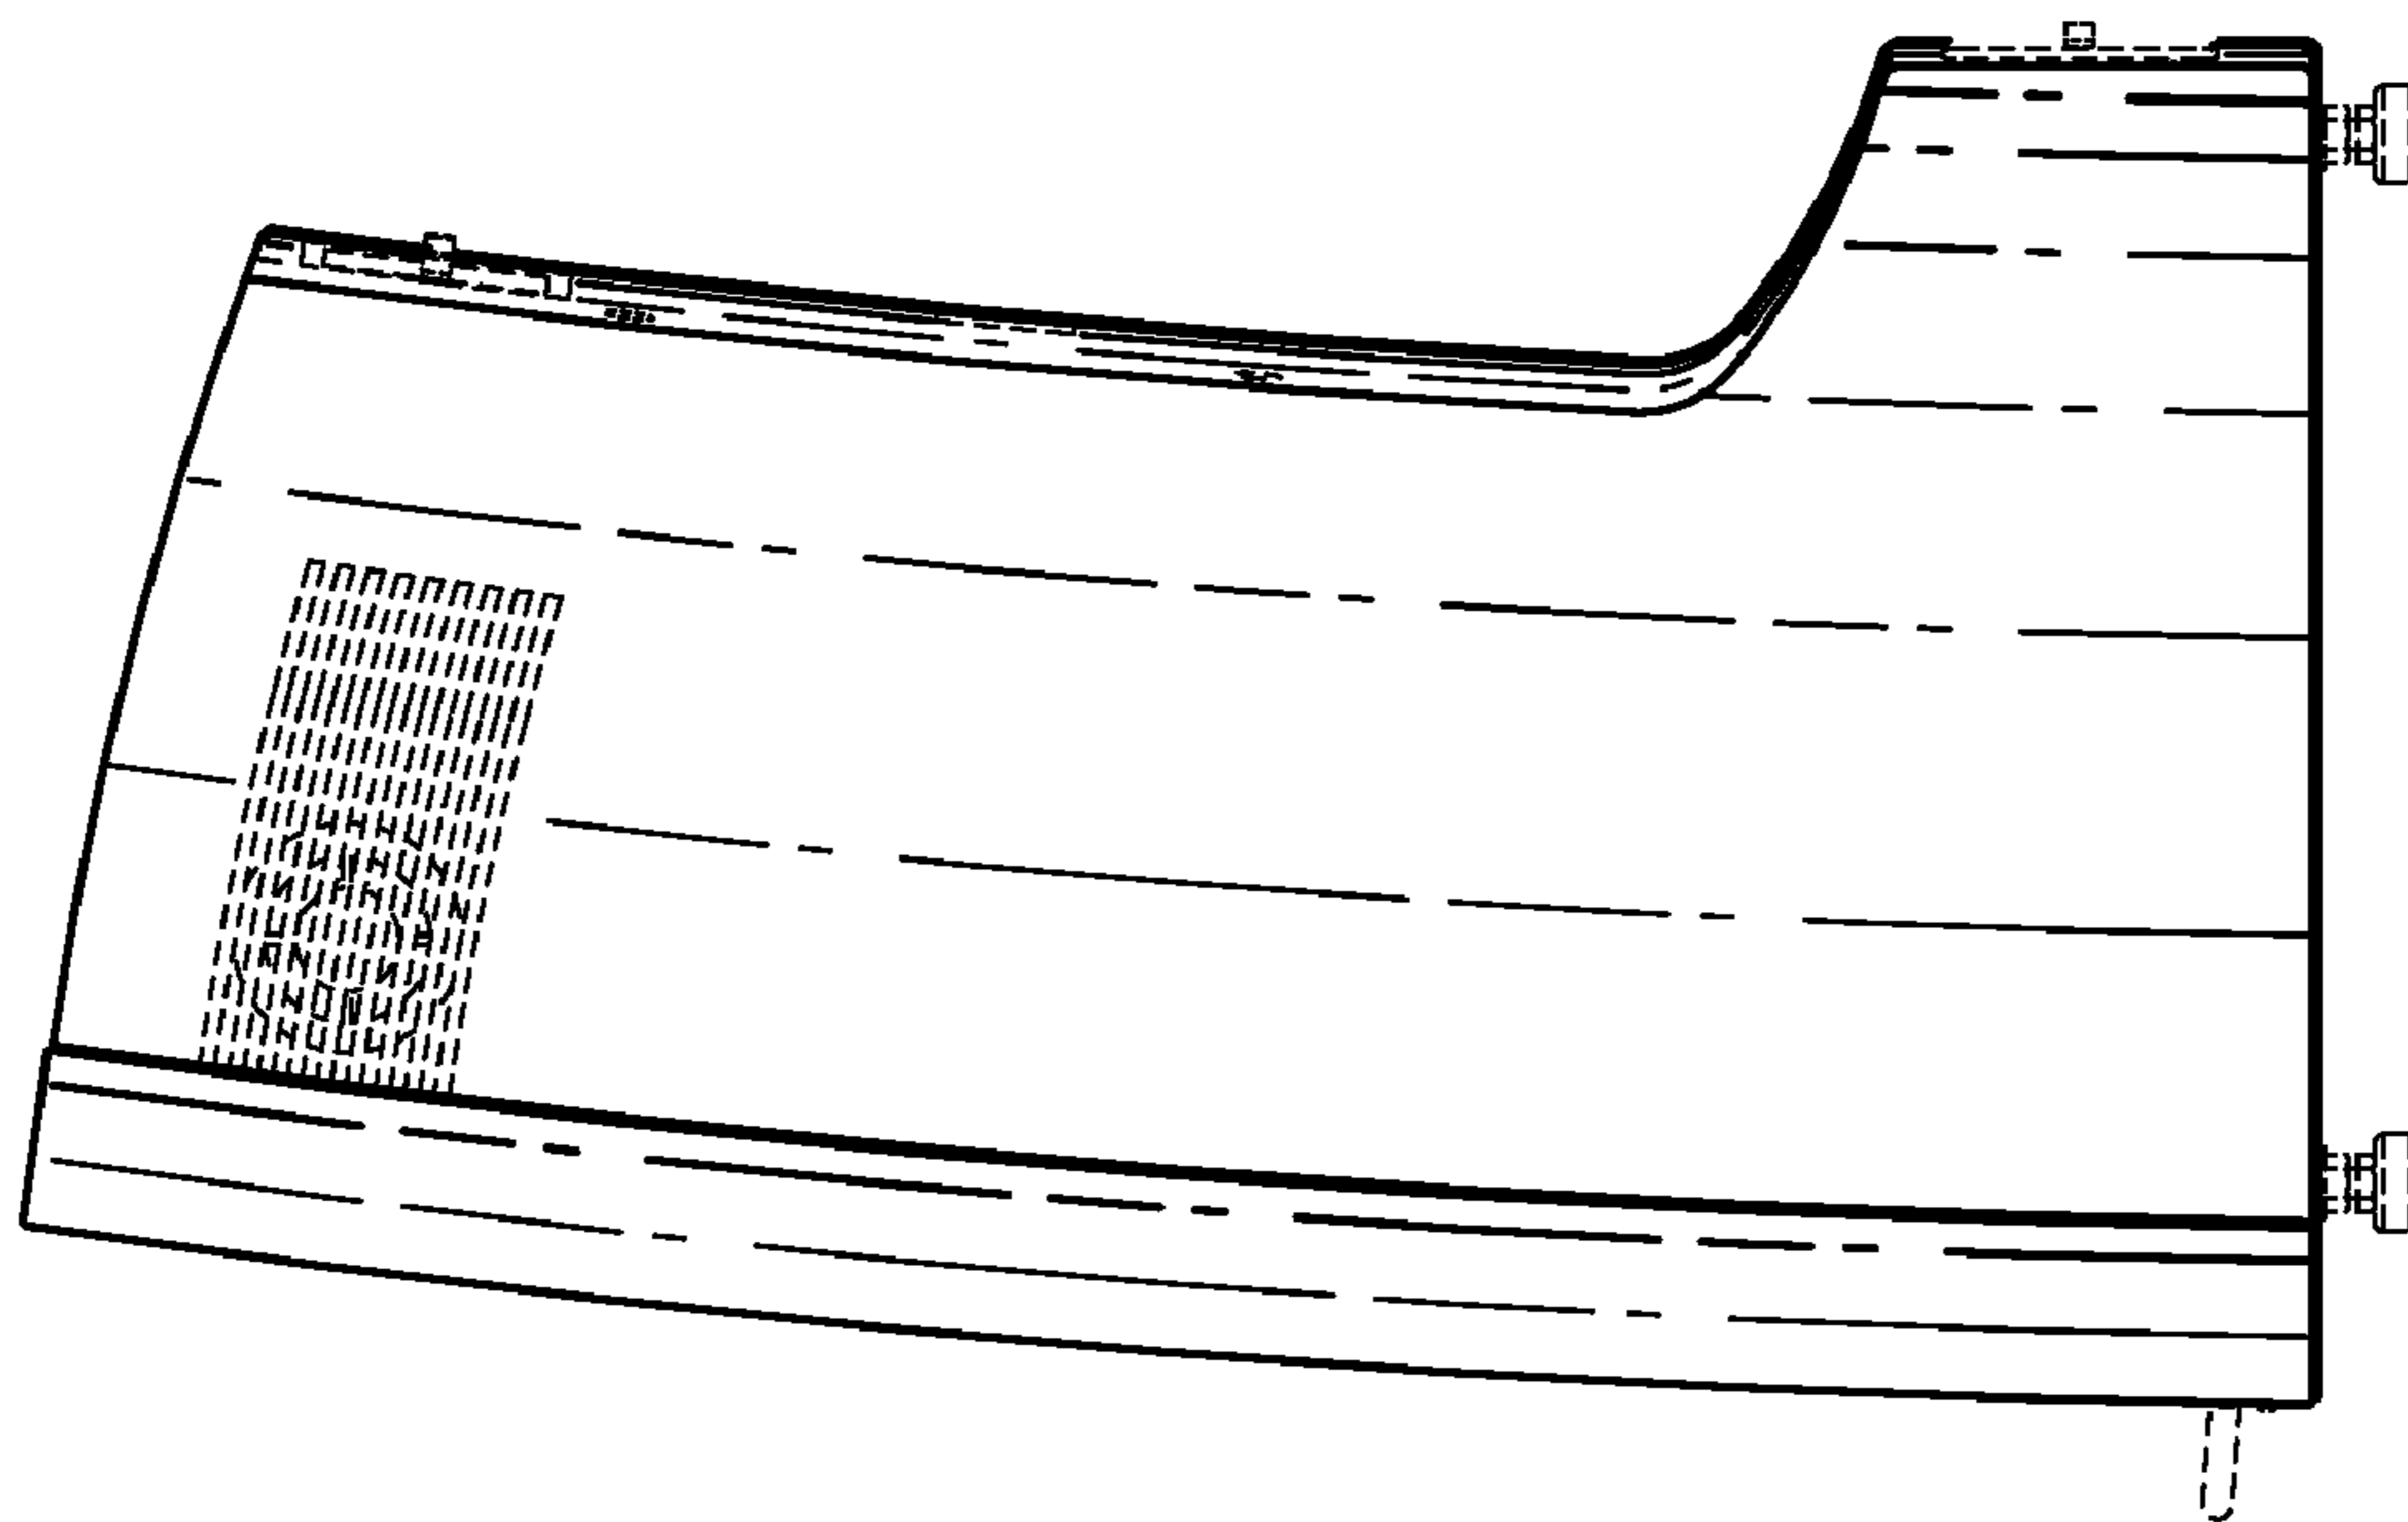


FIG. 3

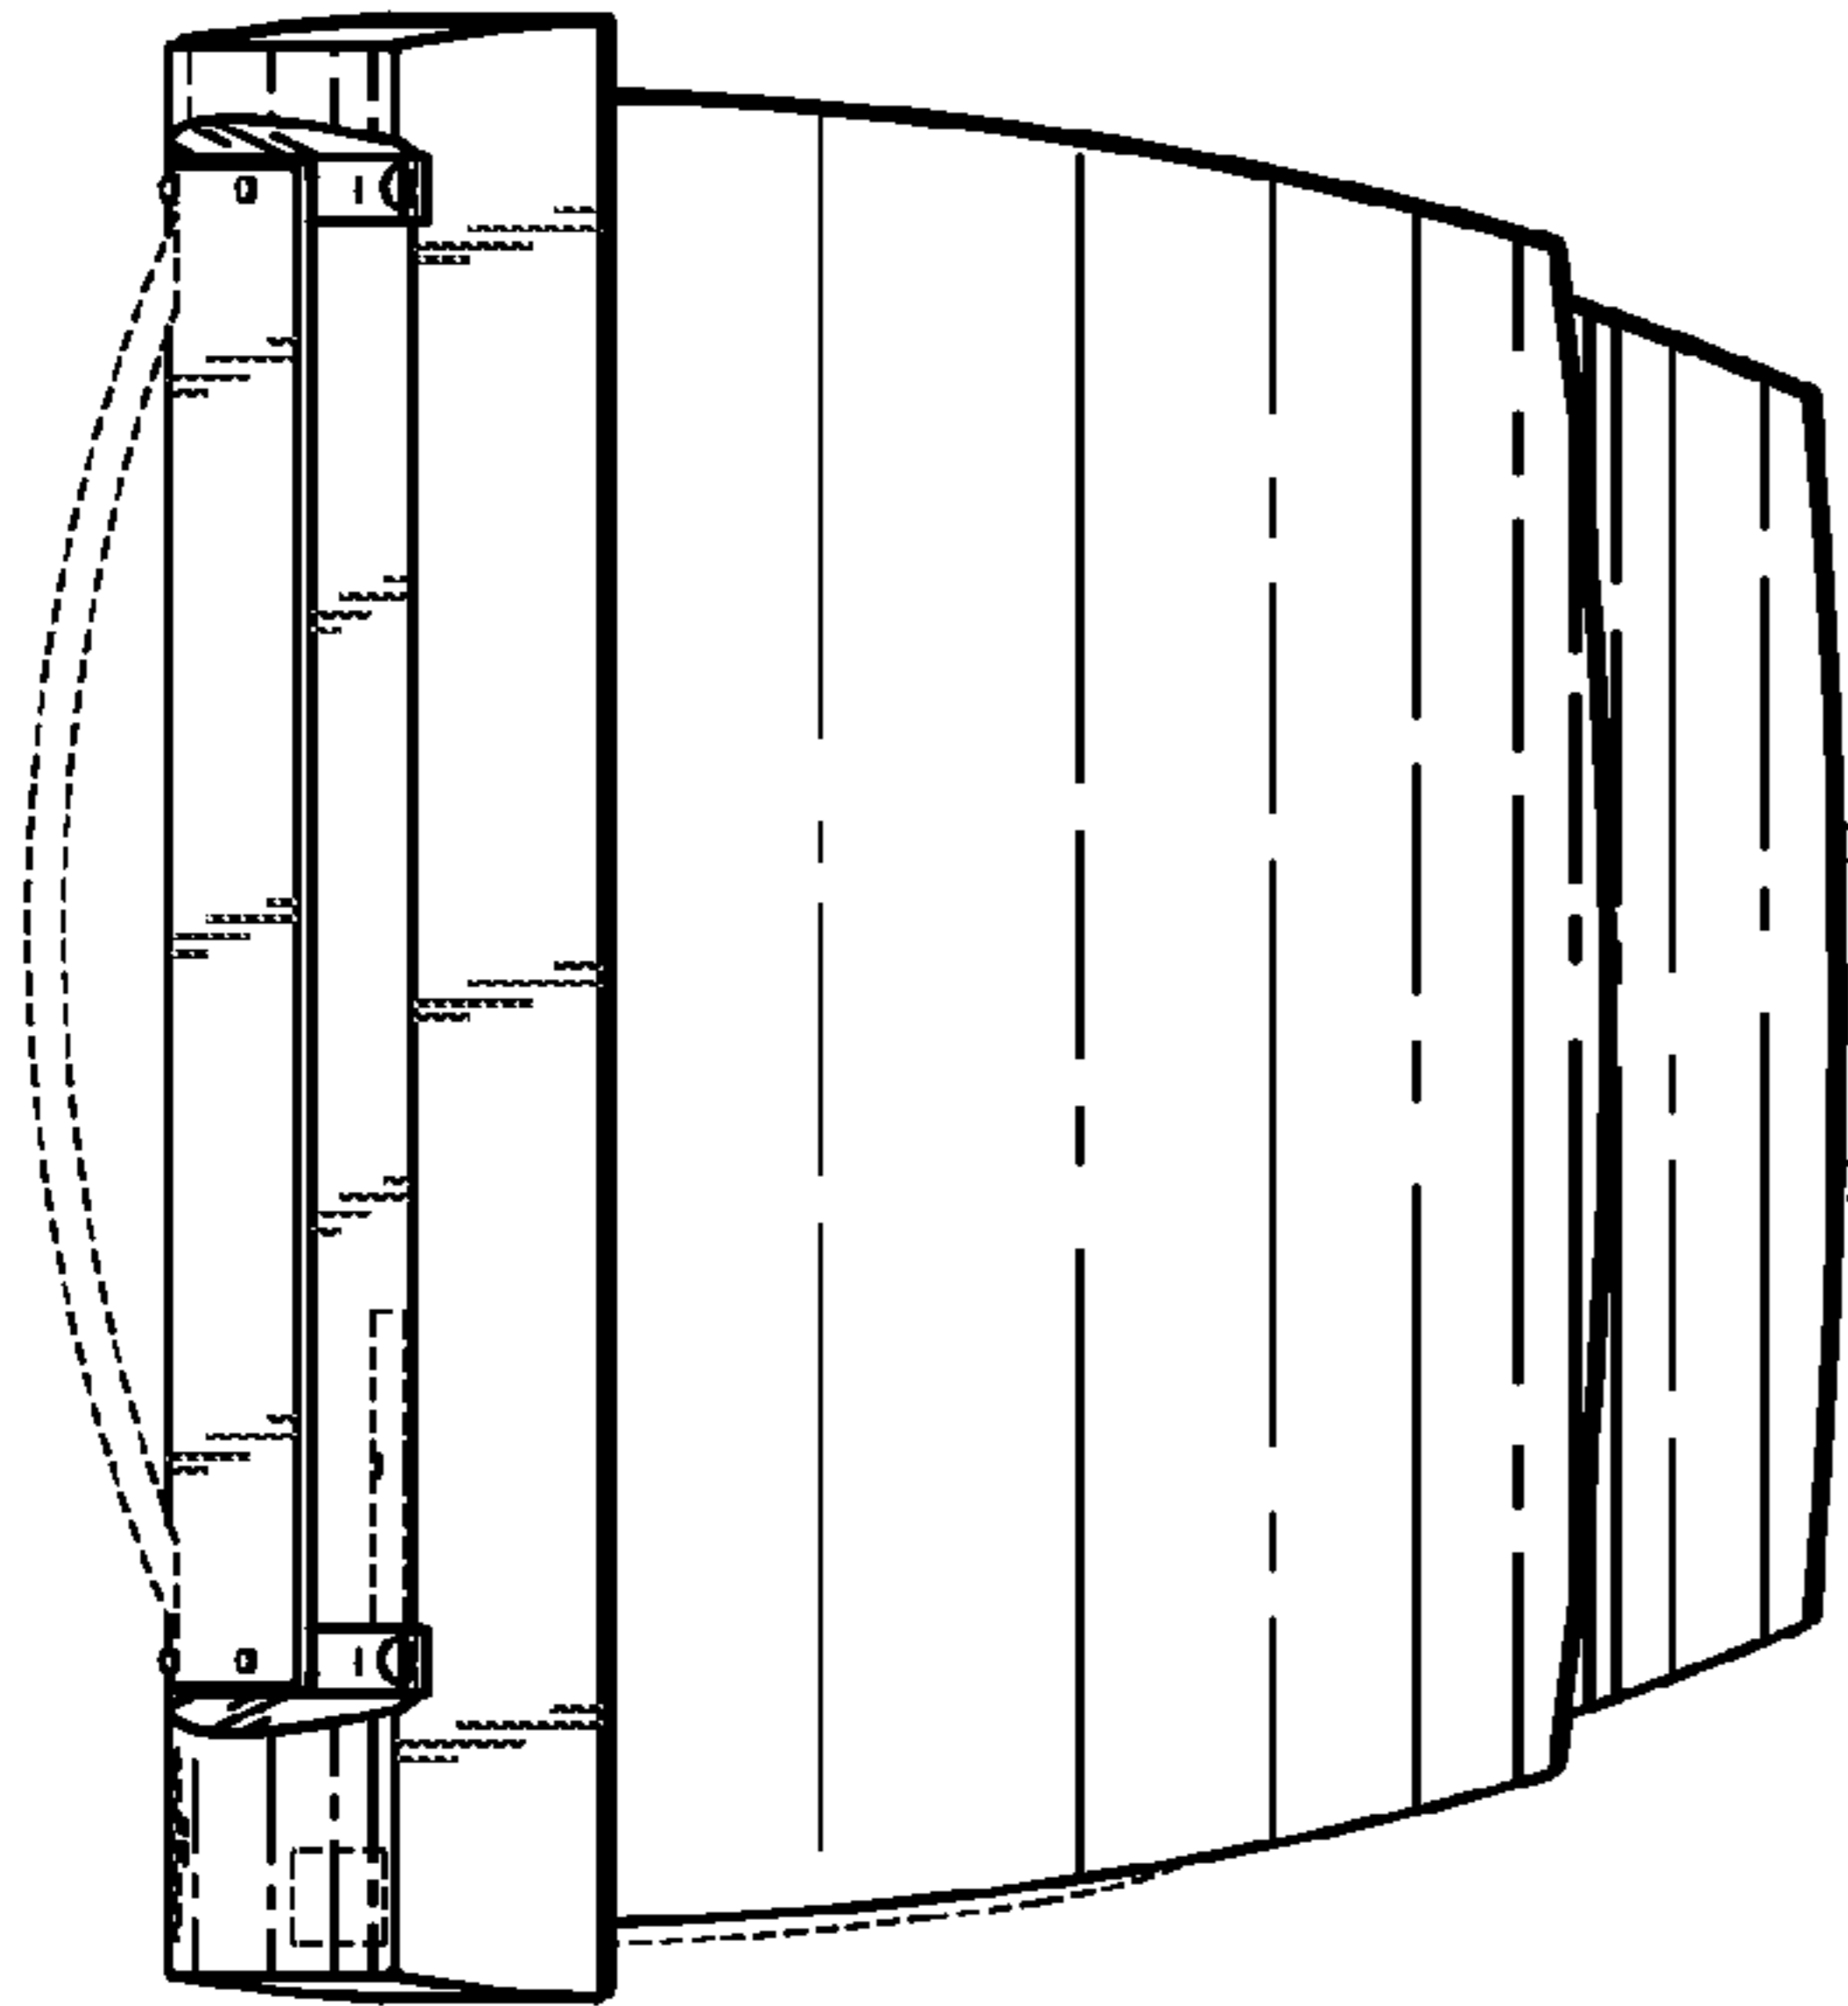


FIG. 6

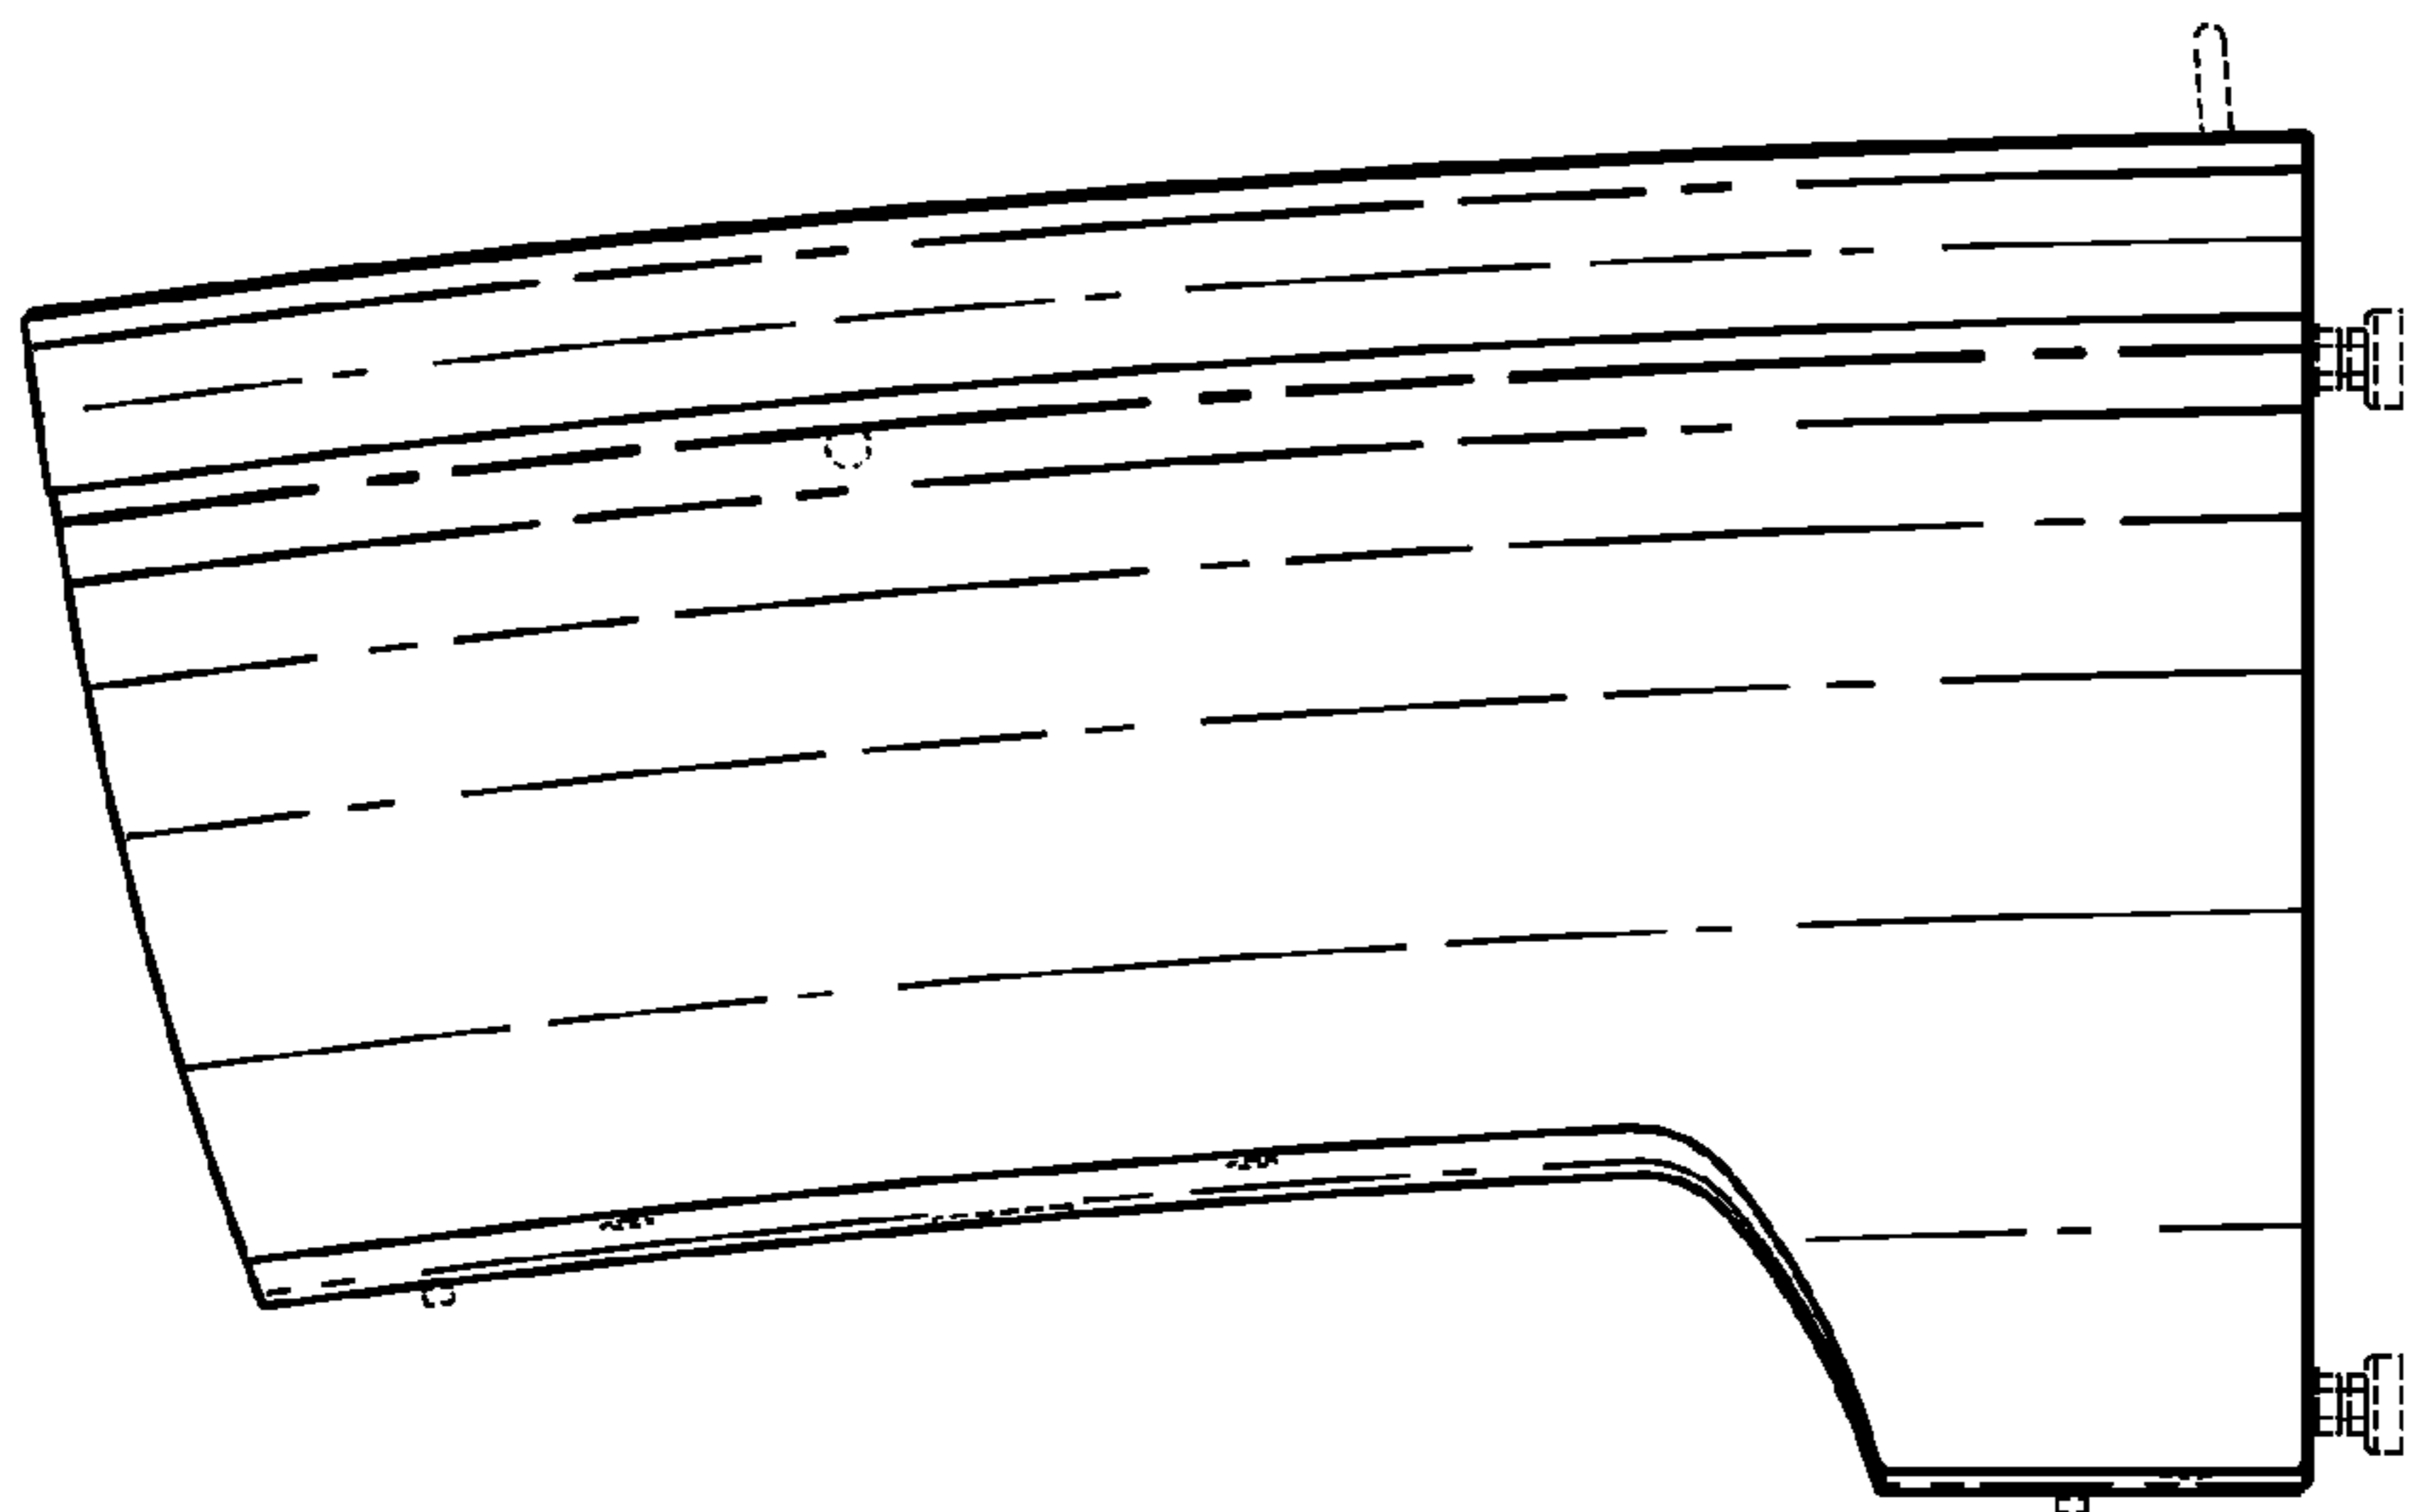


FIG. 5

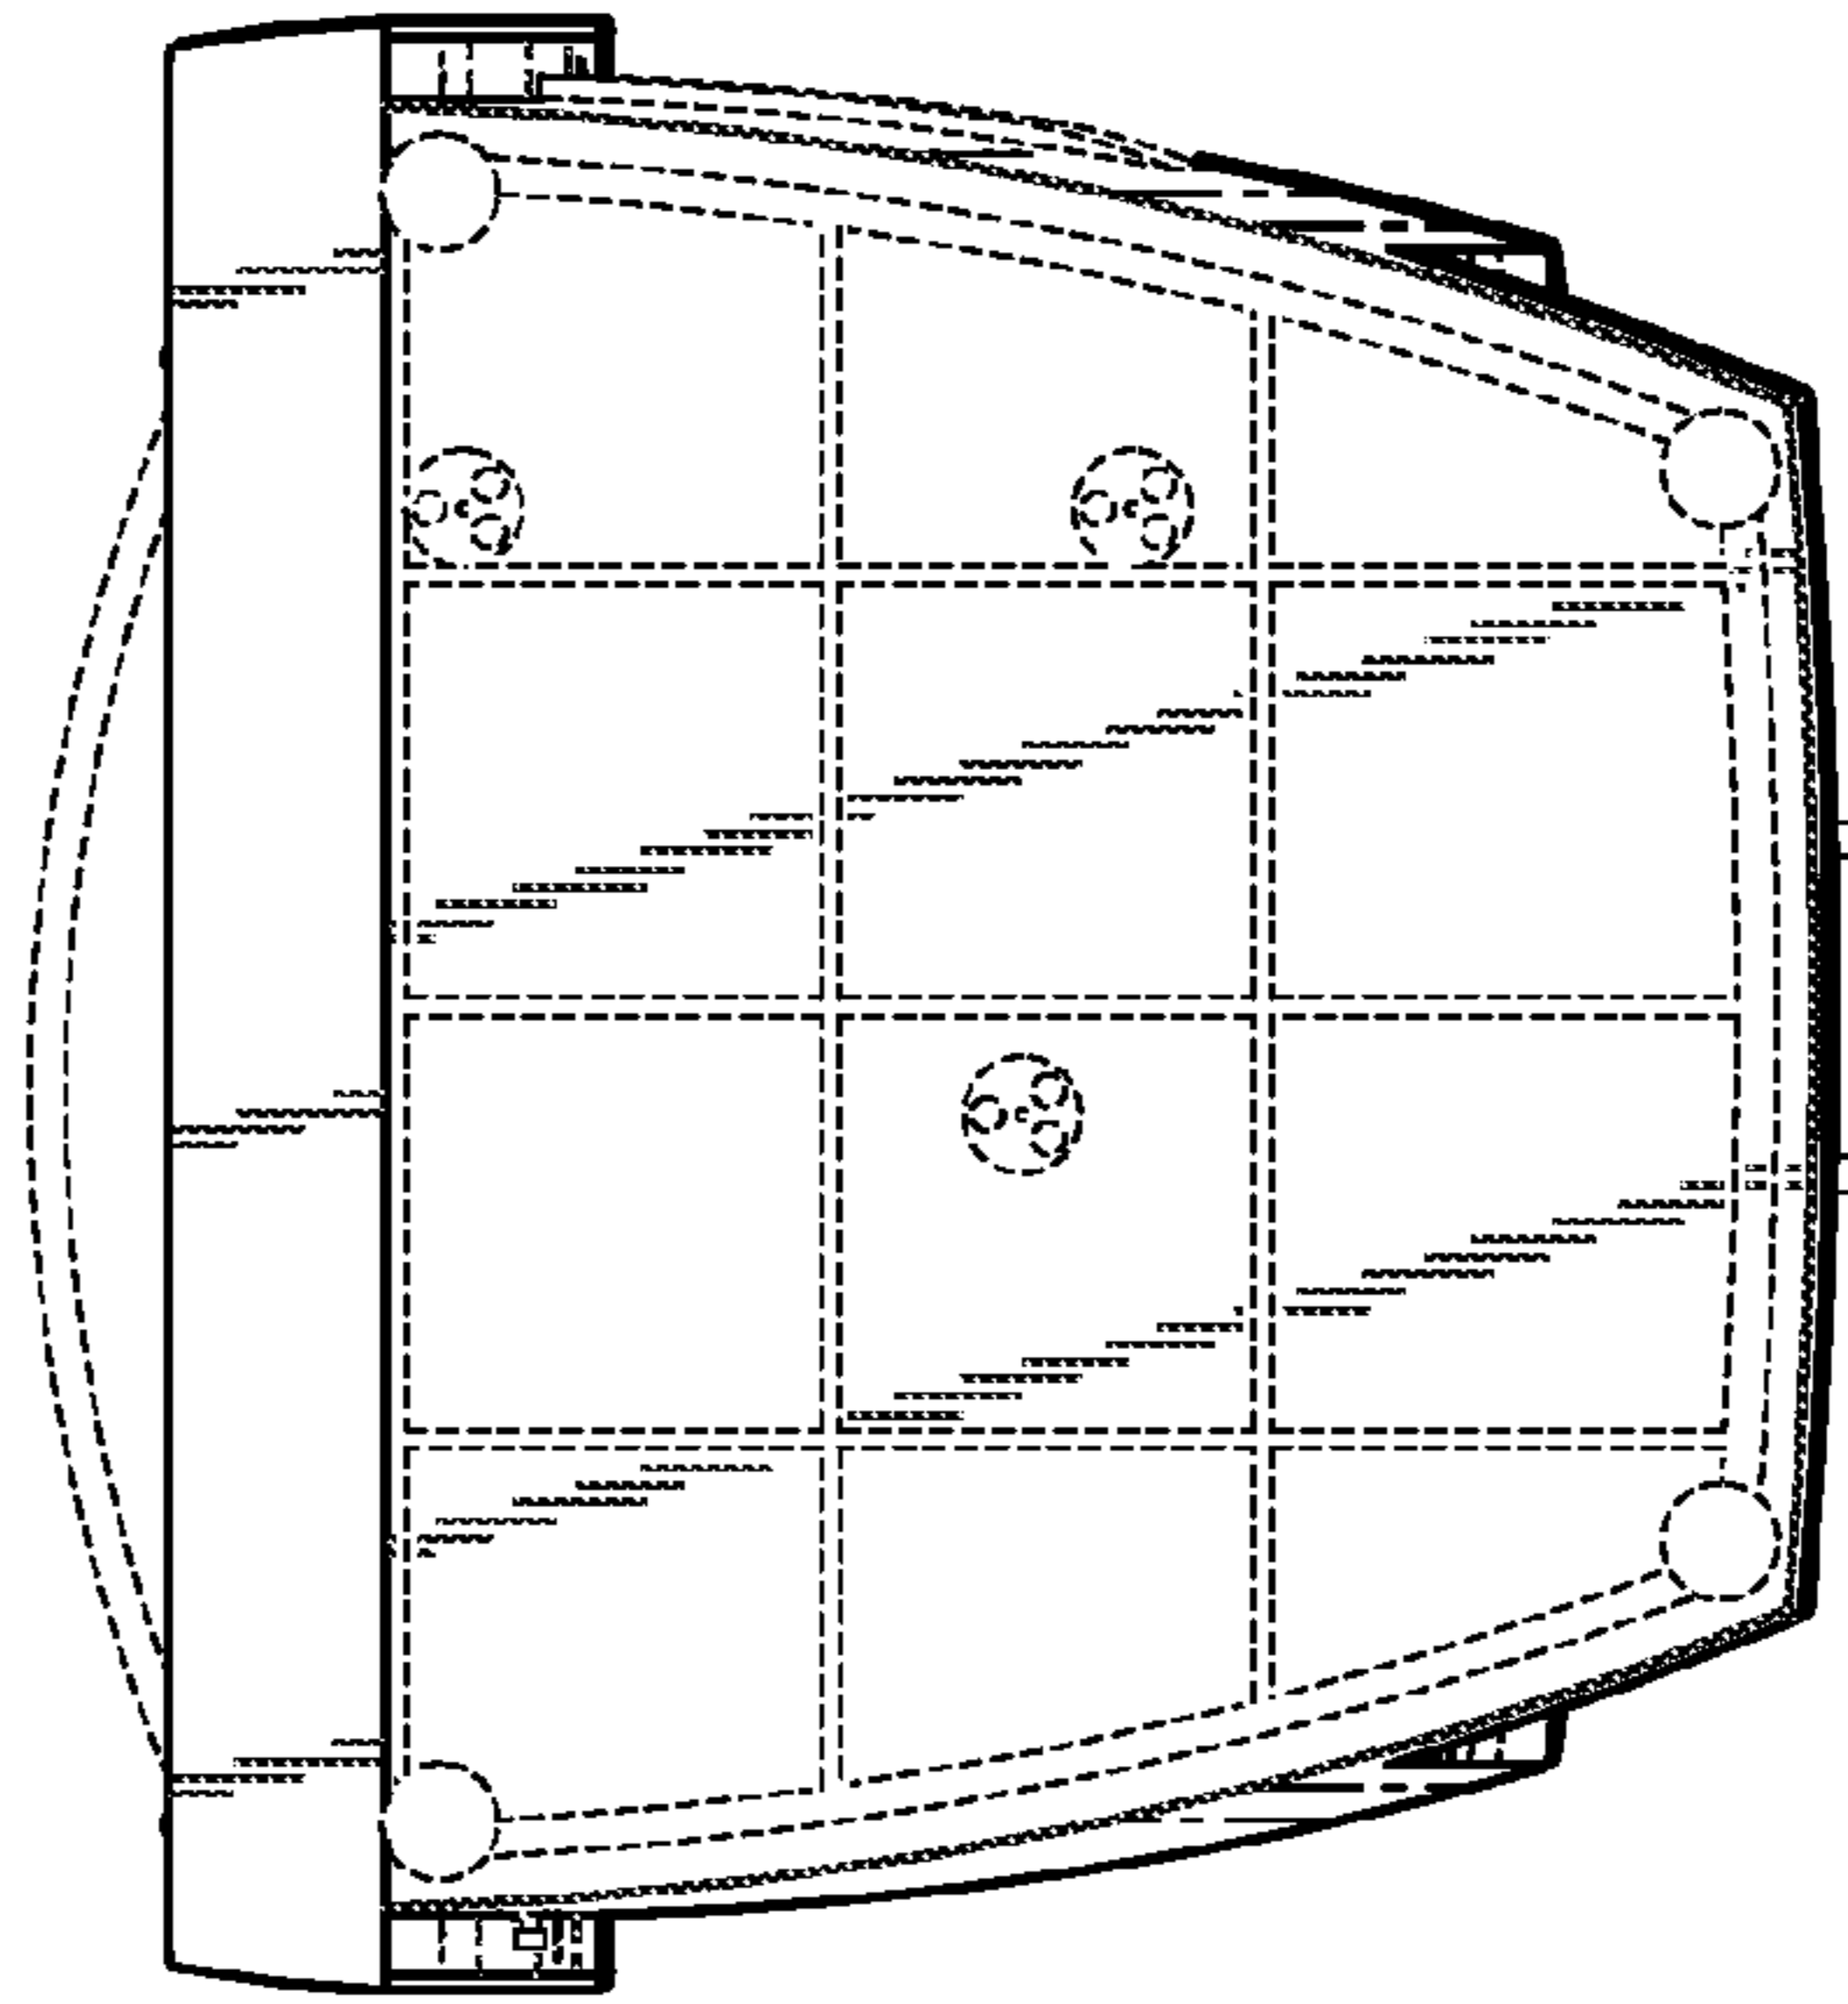


FIG. 7

UNITED STATES PATENT AND TRADEMARK OFFICE
CERTIFICATE OF CORRECTION

PATENT NO. : Des. 578,535 S
APPLICATION NO. : 29/278394
DATED : October 14, 2008
INVENTOR(S) : Rainer Schmitz

Page 1 of 1

It is certified that error appears in the above-identified patent and that said Letters Patent is hereby corrected as shown below:


Title page.

On the title page, insert item -- [30] Priority European Application No. is given as: 596127-1/2, filed Sep. 28, 2006 whereas the same has not been incorporated in the Issued Patent. --.

Item [56], **References Cited**, OTHER PUBLICATIONS, Delete ““ED1,”” and insert -- “ES1,” -- therefor.

Signed and Sealed this

Twenty-ninth Day of September, 2009

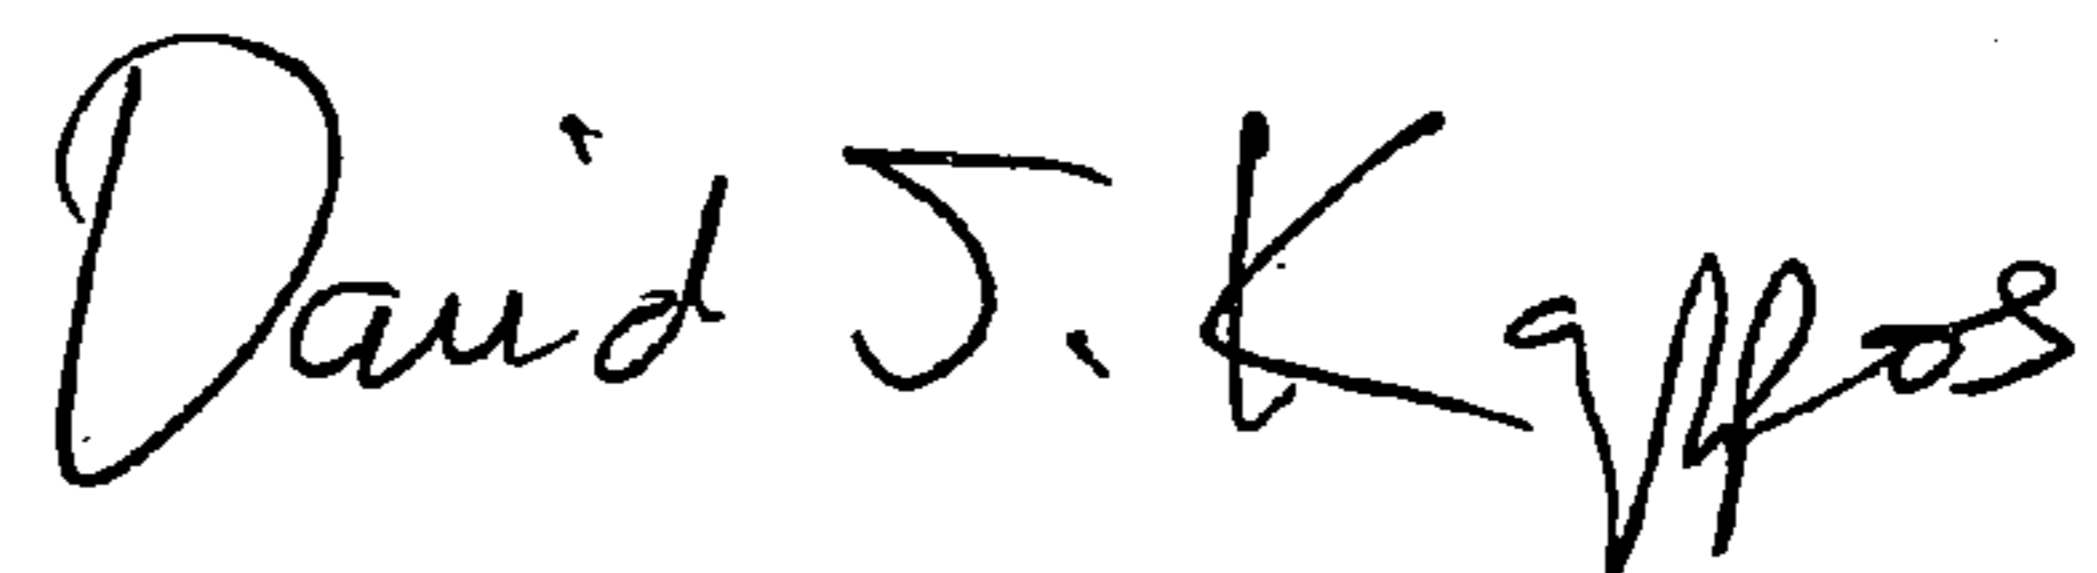

David J. Kappos
Director of the United States Patent and Trademark Office